
Peak Find - Explora_001 PDA_1,8600.JWS

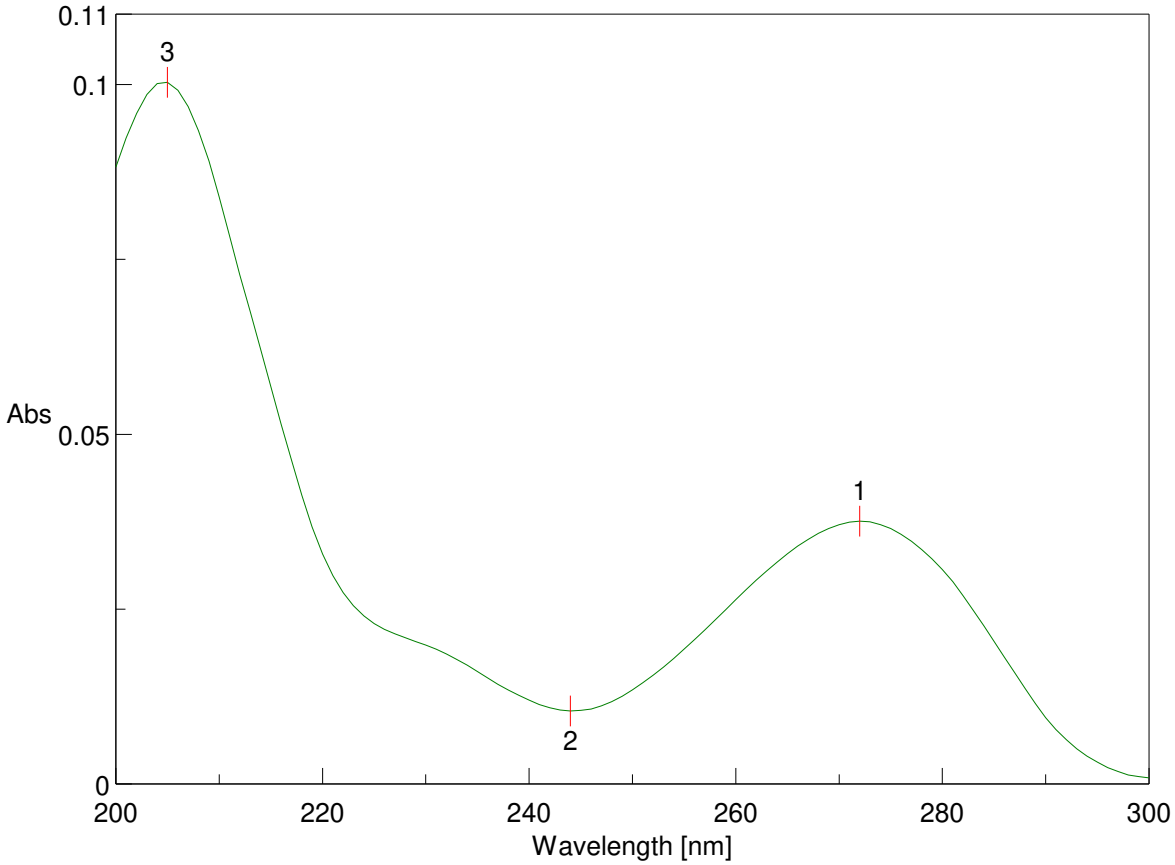

[Comments]

User	Administrator
Division	---
Company	Valer
Creation date	11/08/2020 11:20

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A000661665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.037569	2	244	0.010446
3	205	0.100249			

Chromatogram

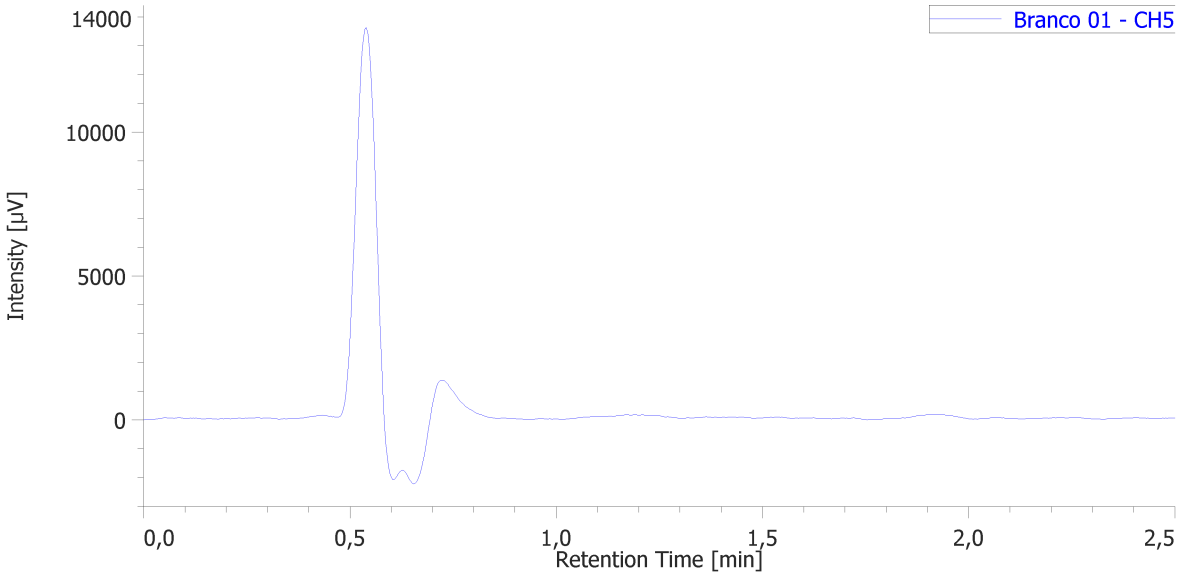


Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:34:32
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:32:00
Volume	10,00 [µL]
Sample #	71
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	Branco 01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

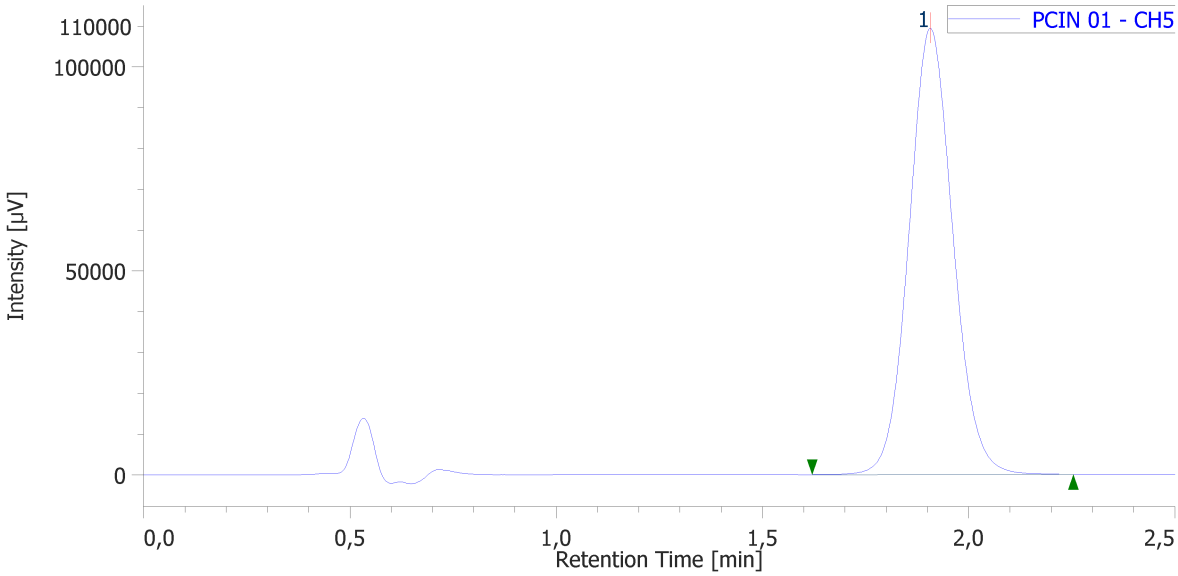

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:37:50
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:35:18
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	PCIN 01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,907	812300	109399	100,000	100,000	N/A	1568	N/A	1,073	

Creator Administrator
Reviewer
Approver

Chromatogram

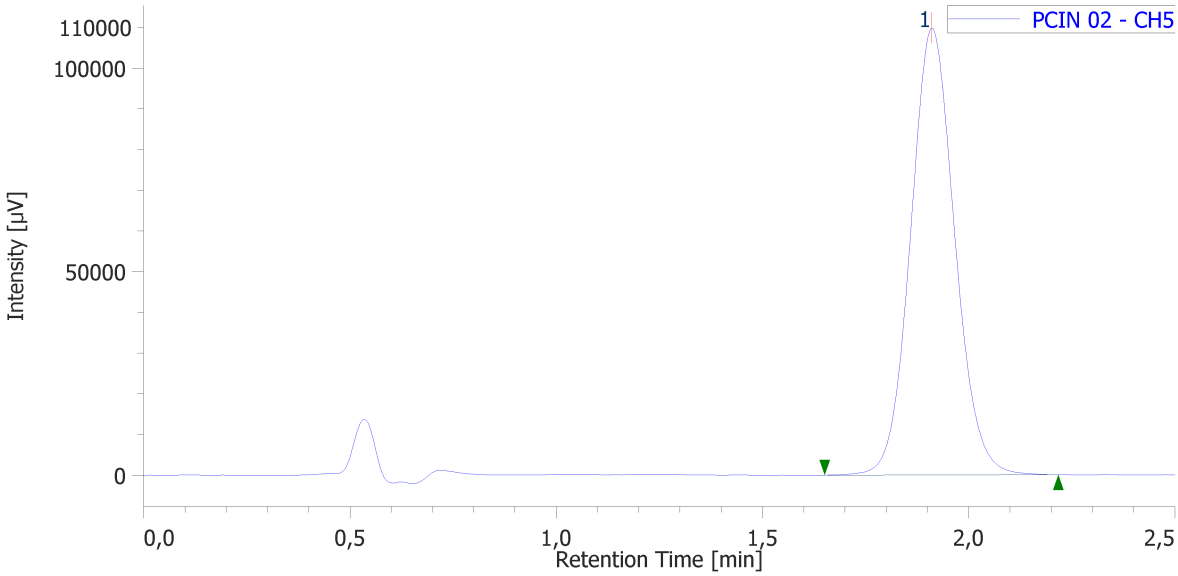

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:41:10
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:38:37
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	PCIN 02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,910	815491	109683	100,000	100,000	N/A	1565	N/A	1,082	

Creator Administrator
Reviewer
Approver

Chromatogram

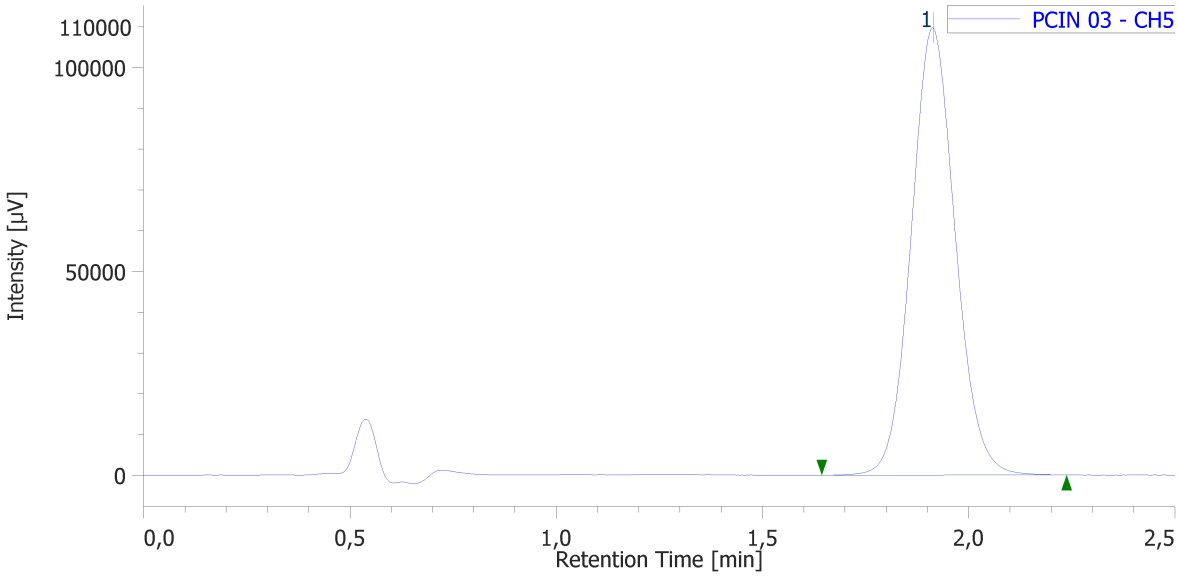

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:44:30
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:41:58
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	PCIN 03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,913	814837	109618	100,000	100,000	N/A	1574	N/A	1,067	

Creator Administrator
Reviewer
Approver

Chromatogram

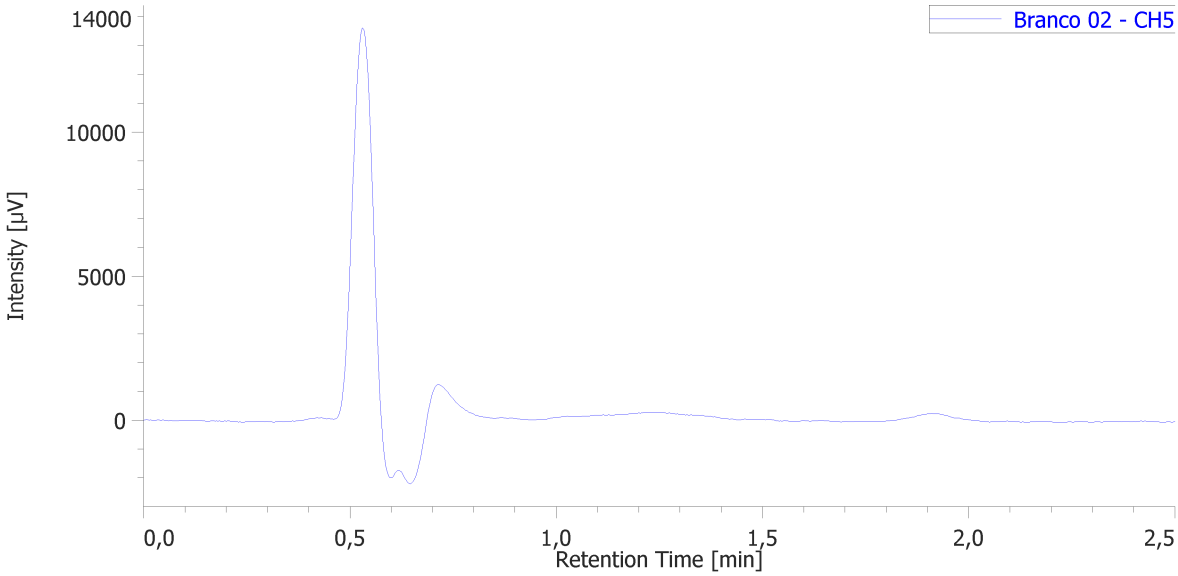


Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:47:50
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:45:18
Volume	10,00 [µL]
Sample #	71
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	Branco 02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

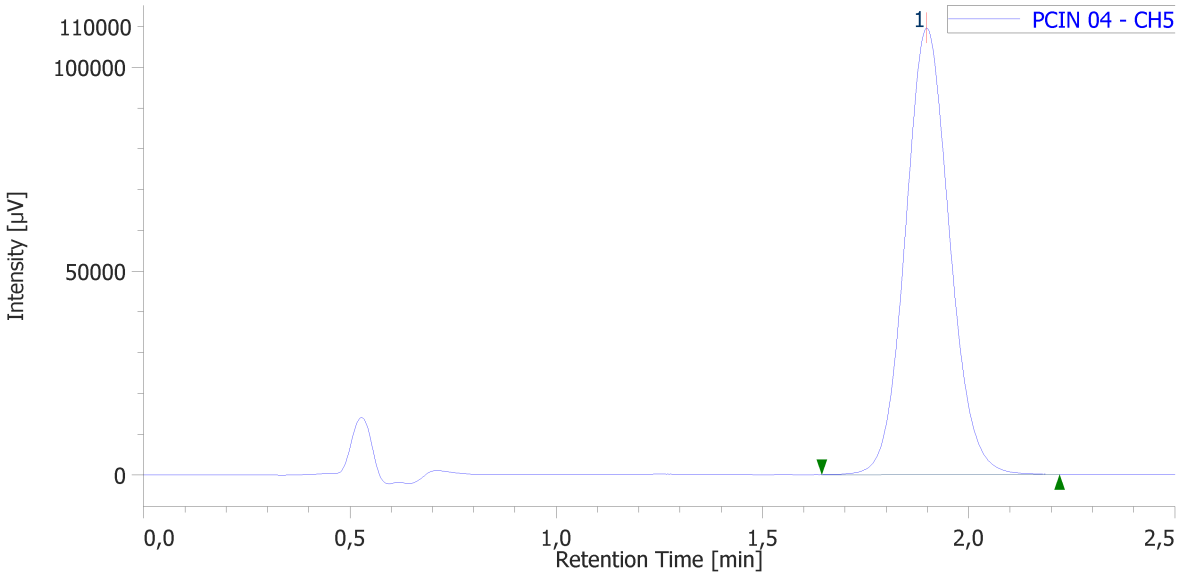

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:51:10
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:48:37
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	PCIN 04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,897	815495	109482	100,000	100,000	N/A	1537	N/A	1,090	

Creator Administrator
Reviewer
Approver

Chromatogram

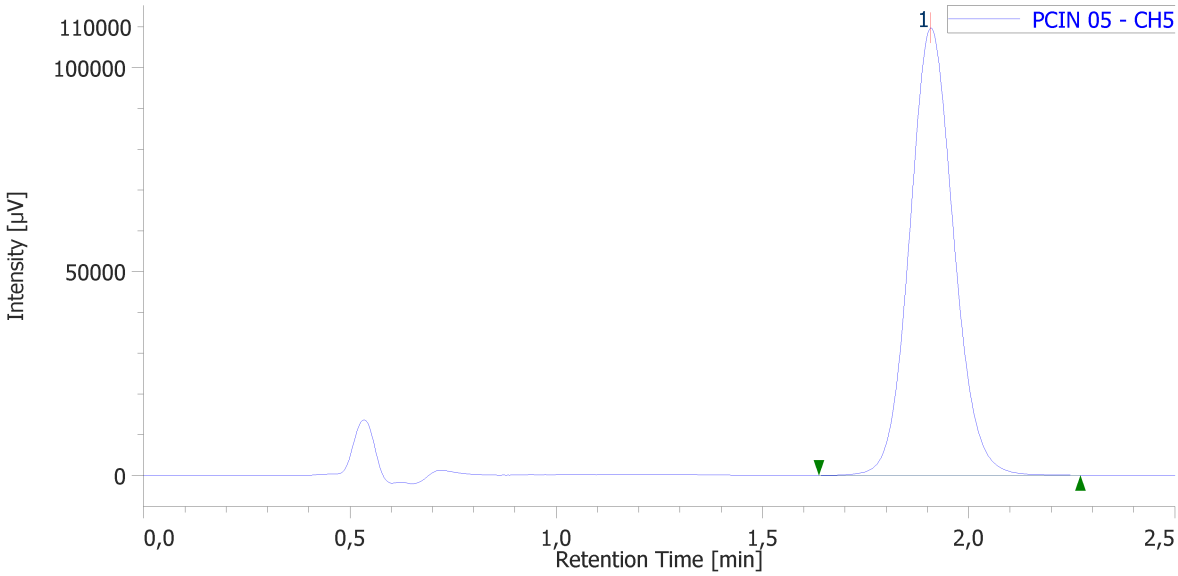

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:54:28
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:51:55
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	PCIN 05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,907	814119	109678	100,000	100,000	N/A	1570	N/A	1,093	

Creator Administrator
Reviewer
Approver

Chromatogram

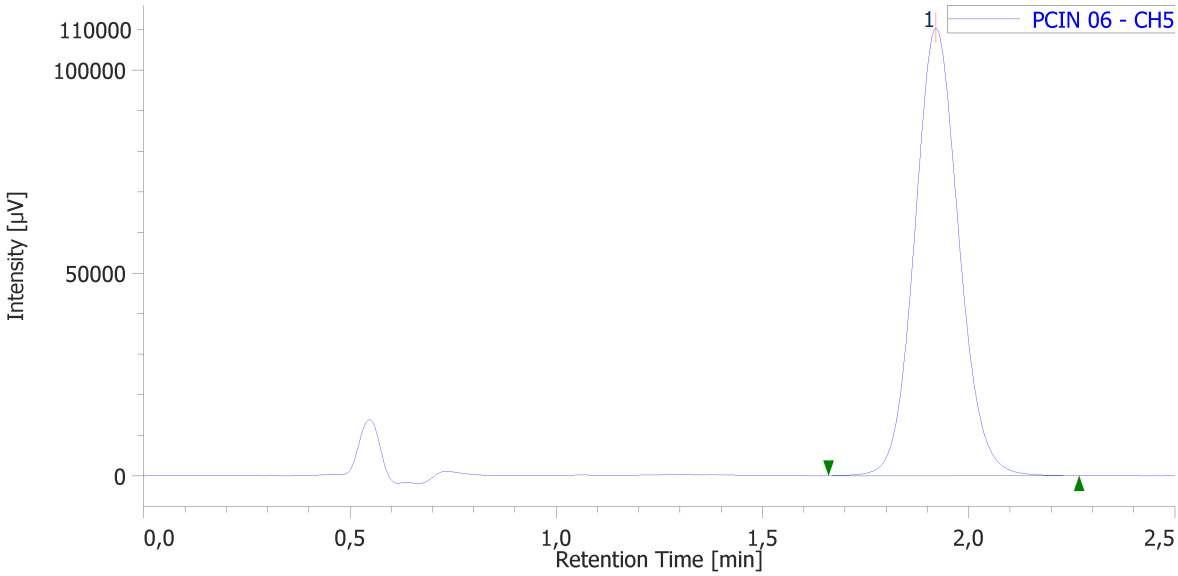

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 11:57:45
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:55:14
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	PCIN 06
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,920	821419	110327	100,000	100,000	N/A	1581	N/A	1,085	

Creator Administrator
Reviewer
Approver

Chromatogram

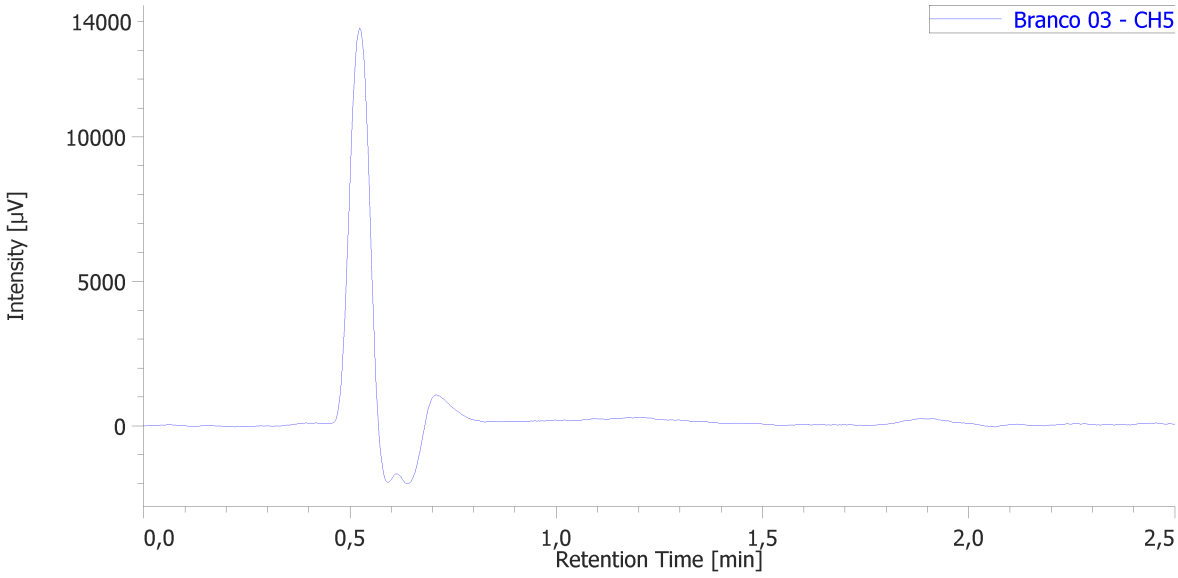


Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 12:01:05
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 11:58:35
Volume	10,00 [µL]
Sample #	71
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	Branco 03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

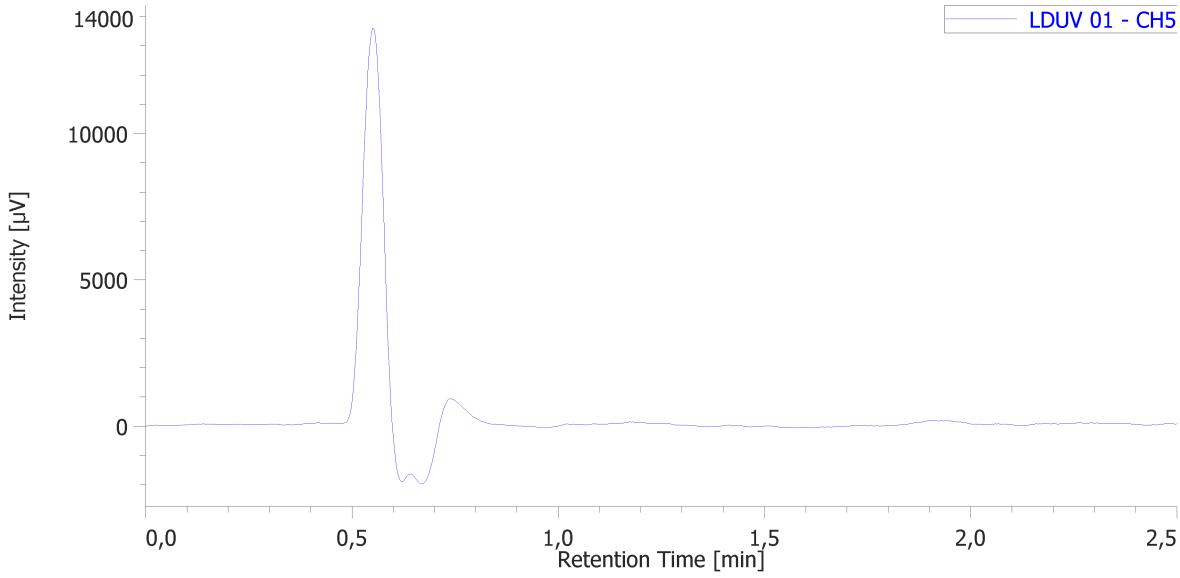


Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:12:11
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:09:38
Volume	10,00 [µL]
Sample #	71
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	LDUV 01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

Creator	Administrator
Reviewer	
Approver	

Chromatogram

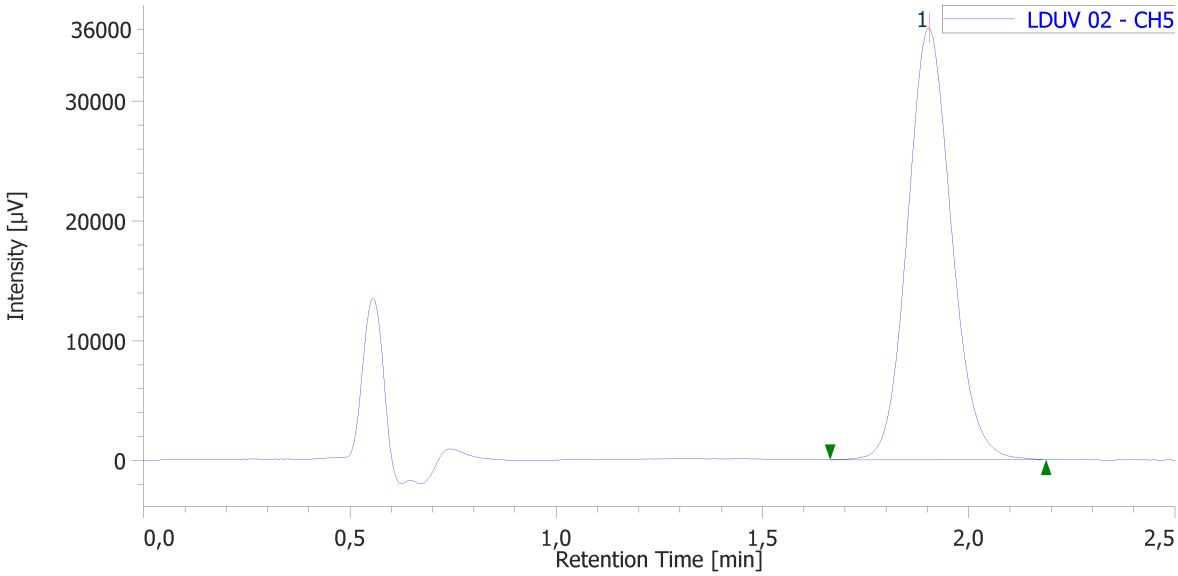

Chromatogram Information

User Name	Administrator
Date Modified	11/08/2020 13:15:29
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:12:57
Volume	10,00 [µL]
Sample #	72
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	LDUV 02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,903	266841	36015	100,000	100,000	N/A	1568	N/A	1,093	

Creator Administrator
Reviewer
Approver

Chromatogram

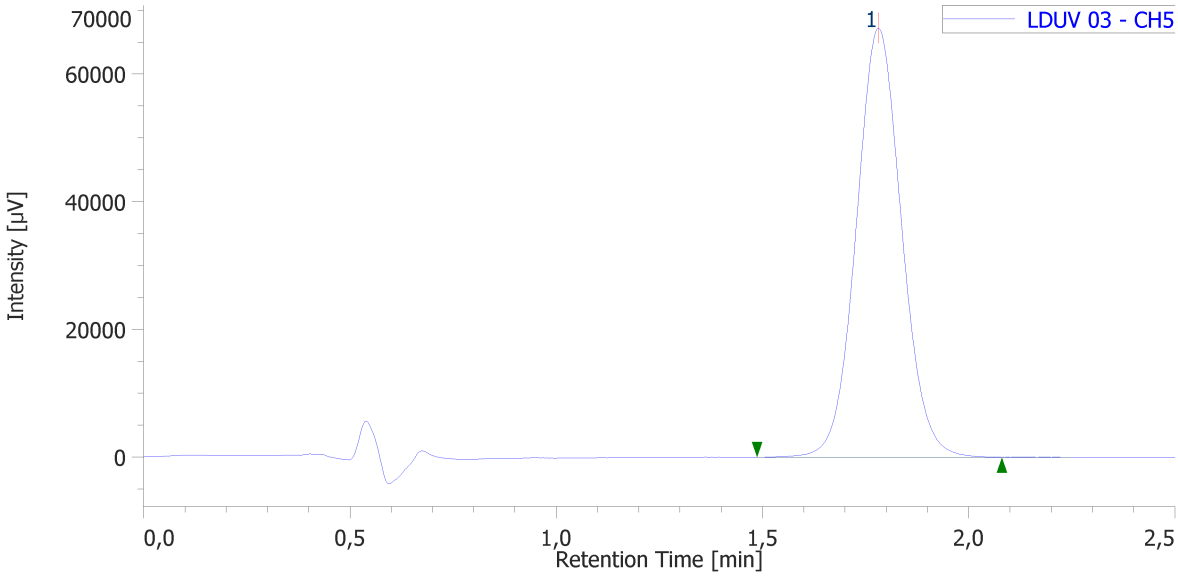

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:18:49
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:16:18
Volume	10,00 [µL]
Sample #	73
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	LDUV 03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,780	514971	67241	100,000	100,000	N/A	1284	N/A	1,065	

Creator Administrator
Reviewer
Approver

Chromatogram

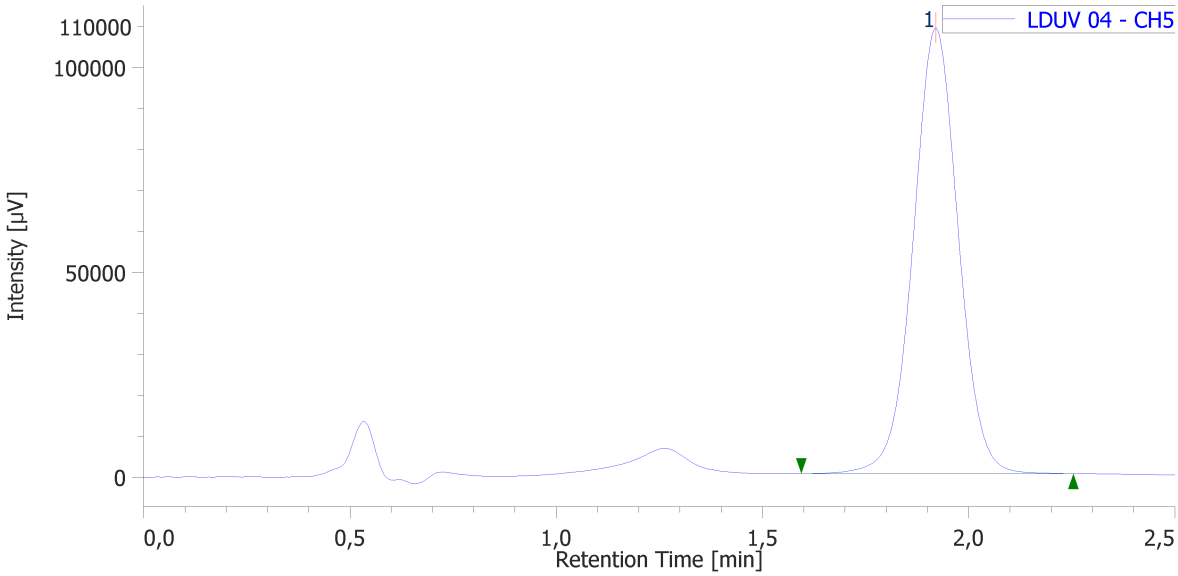

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:44:25
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:19:36
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	LDUV 04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,920	826149	108753	100,000	100,000	N/A	1534	N/A	1,005	

Creator Administrator
Reviewer
Approver

Chromatogram

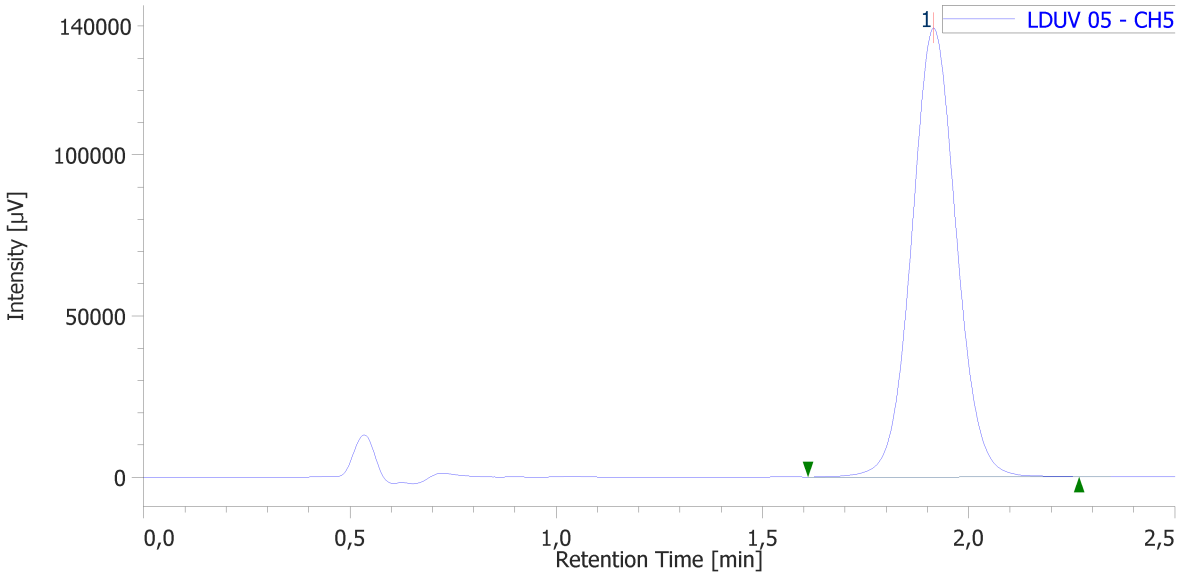

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:49:21
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:22:55
Volume	10,00 [µL]
Sample #	75
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	LDUV 05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,913	1050393	139245	100,000	100,000	N/A	1536	N/A	1,054	

Creator Administrator
Reviewer
Approver

Chromatogram

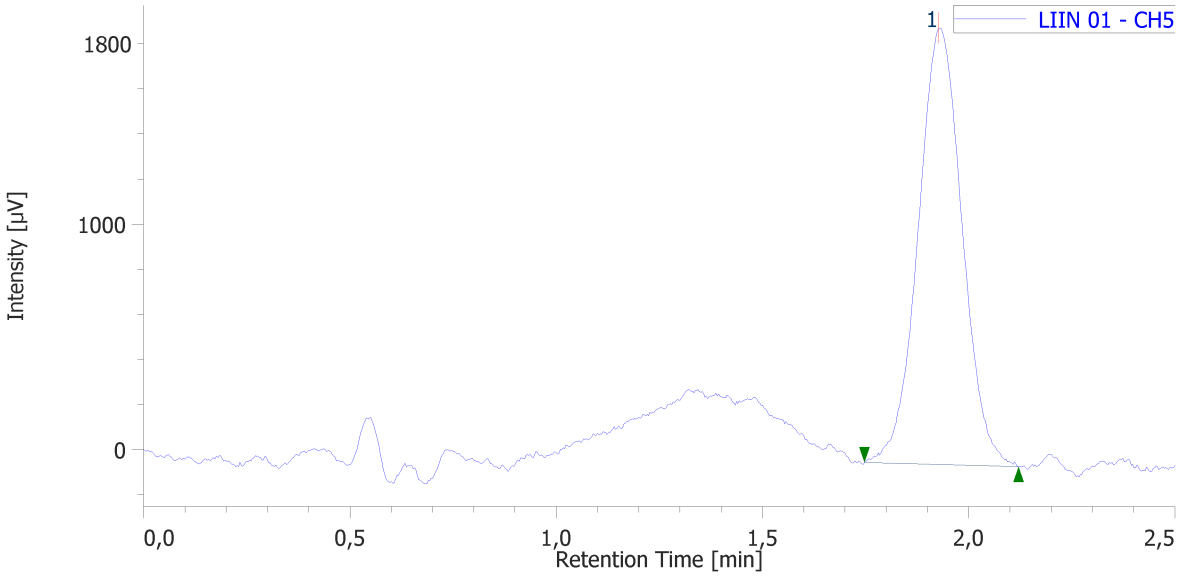

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:50:57
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:48:25
Volume	0,10 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	LIIN 01
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,927	14353	1934	100,000	100,000	N/A	1596	N/A	1,048	

Creator Administrator
Reviewer
Approver

Chromatogram

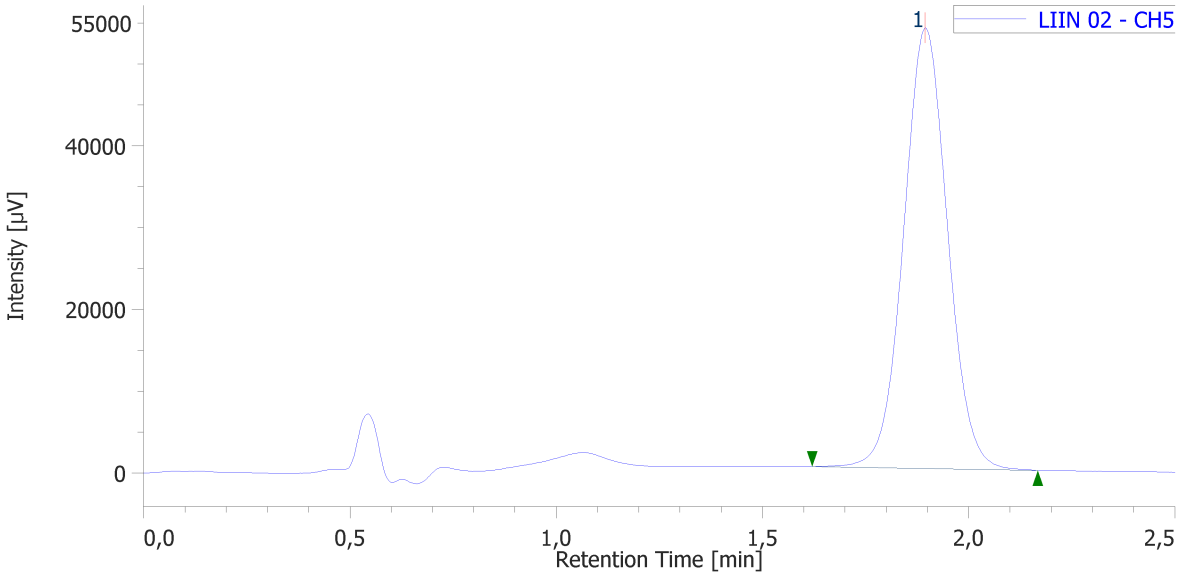

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:54:13
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:51:41
Volume	5,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	LIIN 02
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	398985	53784	100,000	100,000	N/A	1545	N/A	1,044	

Creator Administrator
Reviewer
Approver

Chromatogram

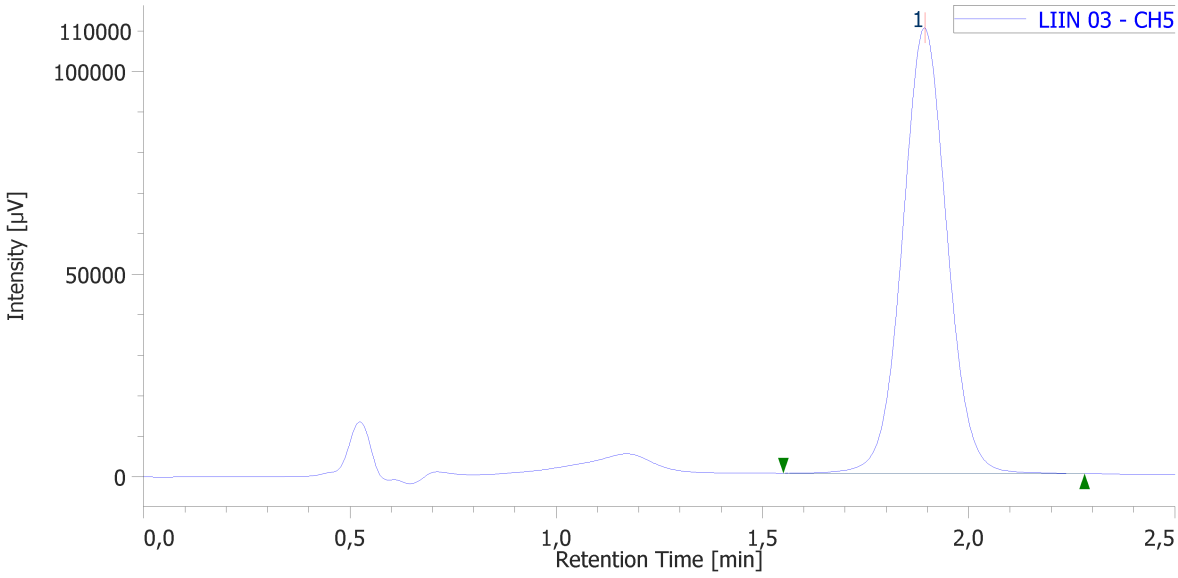

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 13:57:33
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:55:00
Volume	10,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	LIIN 03
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,893	826449	109827	100,000	100,000	N/A	1521	N/A	1,024	

Creator Administrator
Reviewer
Approver

Chromatogram

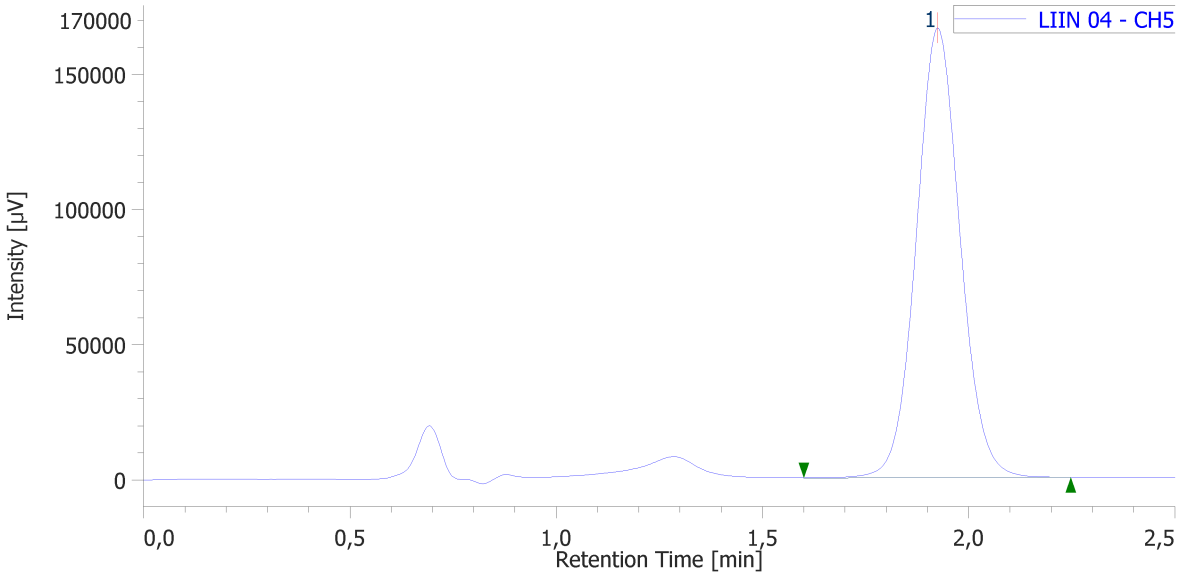

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 14:00:53
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 13:58:21
Volume	15,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	LIIN 04
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,923	1227258	166182	100,000	100,000	N/A	1619	N/A	1,068	

Creator Administrator
Reviewer
Approver

Chromatogram

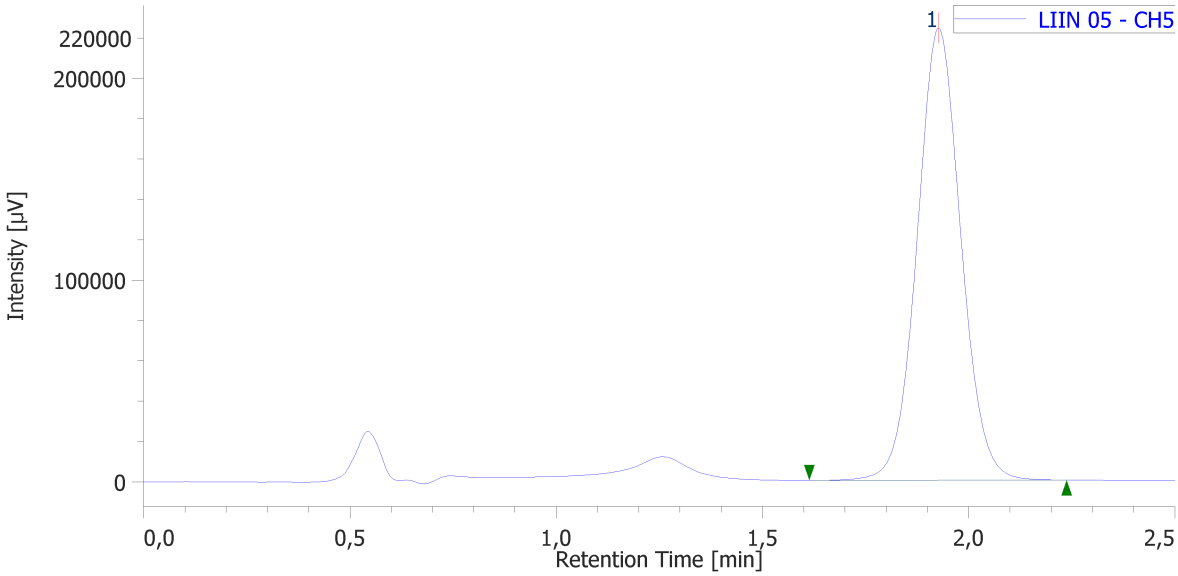

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 14:04:19
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 14:01:46
Volume	20,00 [µL]
Sample #	74
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	LIIN 05
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,927	1655134	224071	100,000	100,000	N/A	1624	N/A	1,047	

Creator Administrator
Reviewer
Approver

Chromatogram

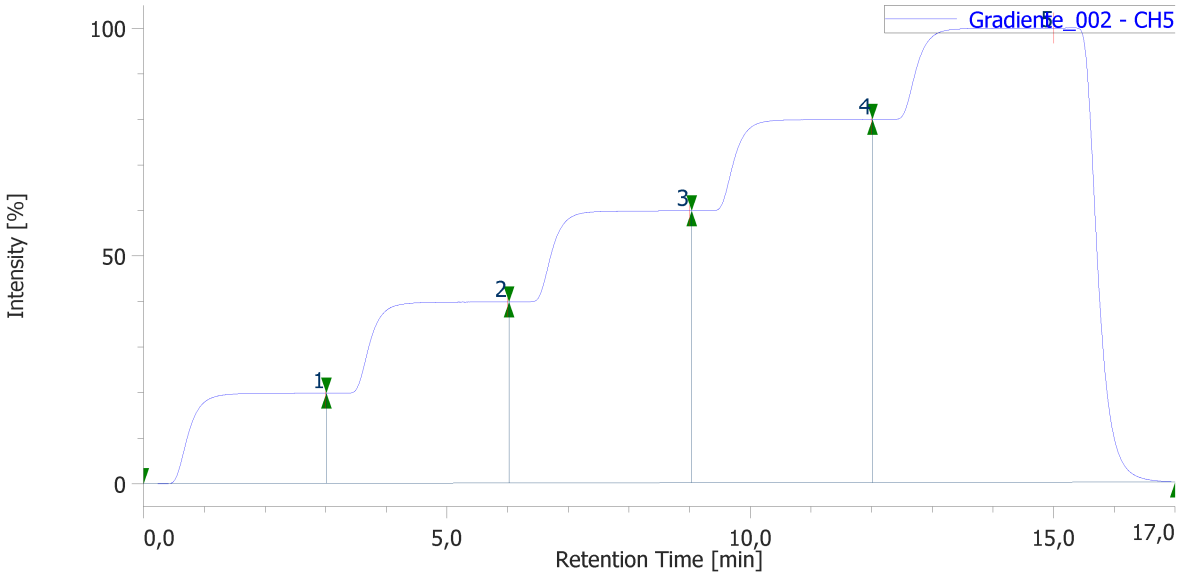

Chromatogram Information	
User Name	Administrator
Date Modified	11/08/2020 15:12:32
Description	
HPLC System Name	HPL 09
Injection Date	11/08/2020 14:55:30
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	17,0 [min]
Acquisition Sequence	
Control Method	Gradiente
Peak ID Table	Grad
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,000	13414654	99138	4,981	6,627	N/A	N/A	N/A	N/A	
2	40%	5	6,000	31548653	199209	11,714	13,317	N/A	N/A	N/A	N/A	
3	60%	5	9,000	49672441	299064	18,444	19,992	N/A	N/A	N/A	N/A	
4	80%	5	12,000	67079937	399201	24,908	26,685	N/A	N/A	N/A	N/A	
5	100%	5	15,000	107600063	499339	39,953	33,379	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver