
Chromatogram

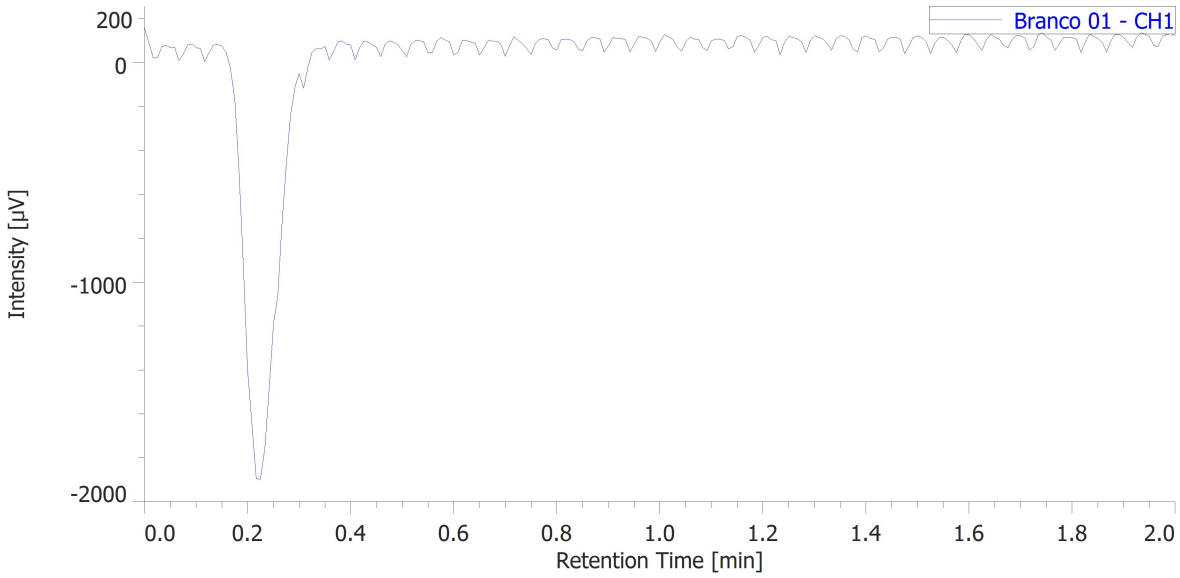


Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 2:53:58 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 2:51:56 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator
Reviewer
Approver

Chromatogram

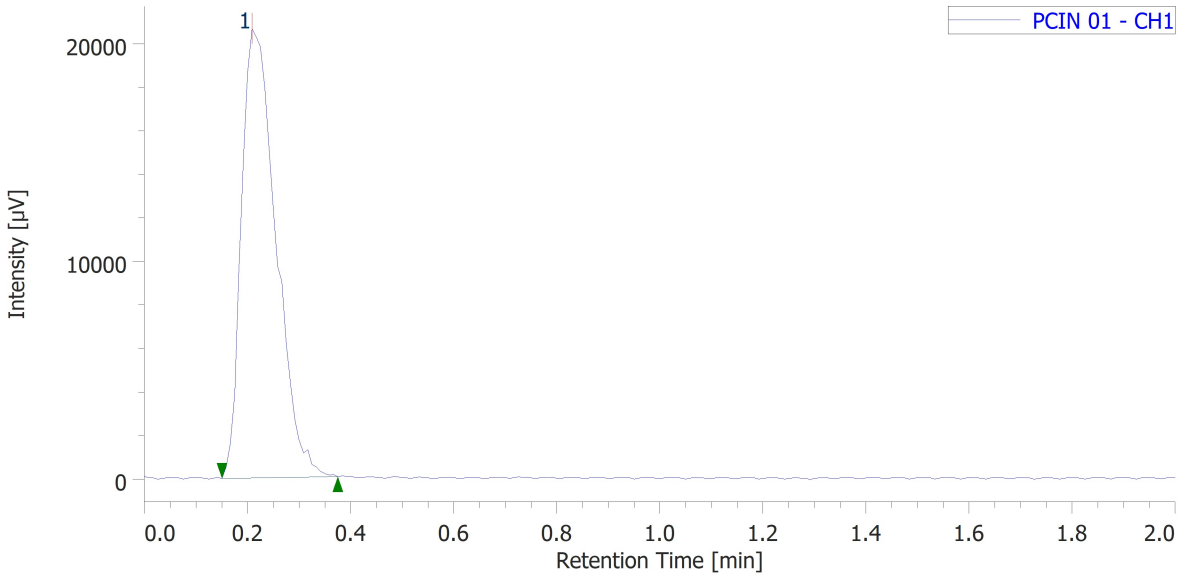

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 2:56:14 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 2:54:12 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.208	96068	20626	100.000	100.000	N/A	47	N/A	1.706	

Creator
Reviewer
Approver

Chromatogram

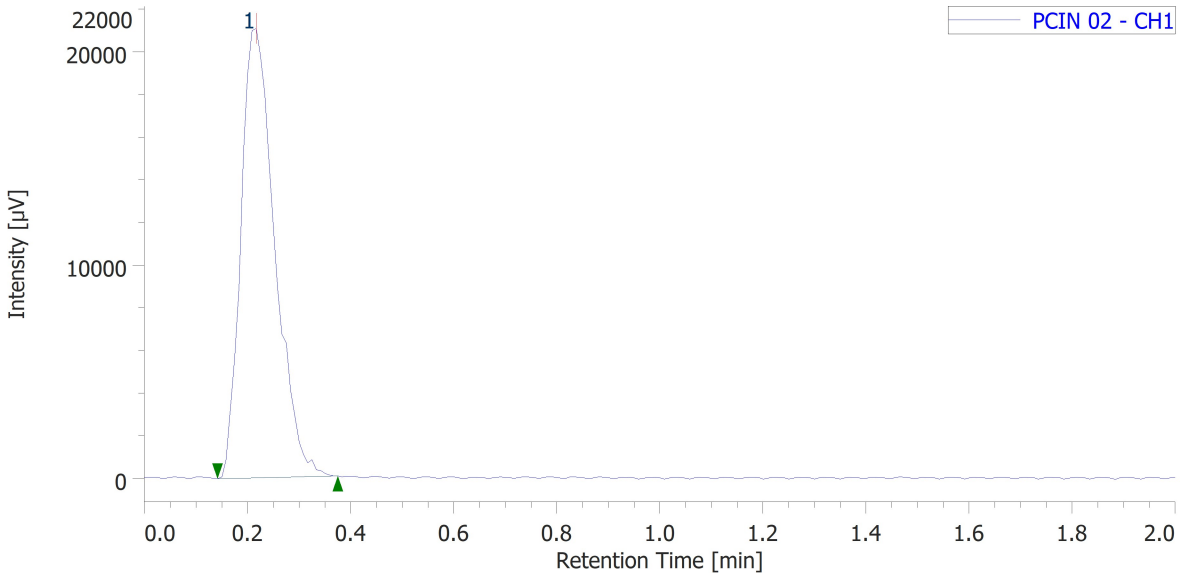

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 2:58:30 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 2:56:29 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	96324	21039	100.000	100.000	N/A	57	N/A	1.289	

Creator
Reviewer
Approver

Chromatogram

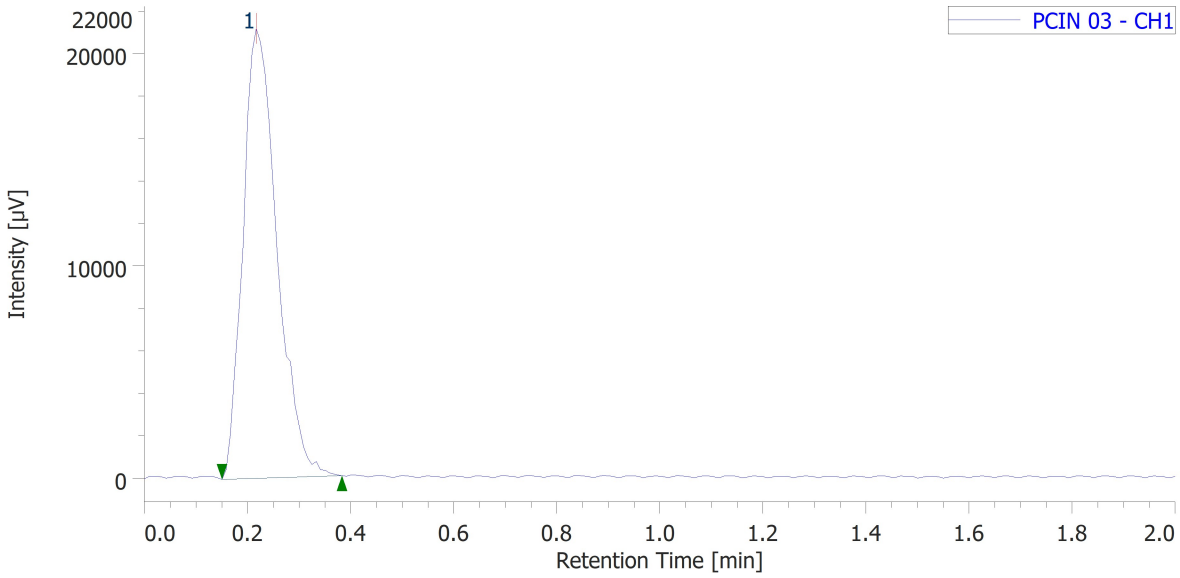

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:00:46 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 2:58:45 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	97009	21158	100.000	100.000	N/A	57	N/A	1.379	

Creator
Reviewer
Approver

Chromatogram

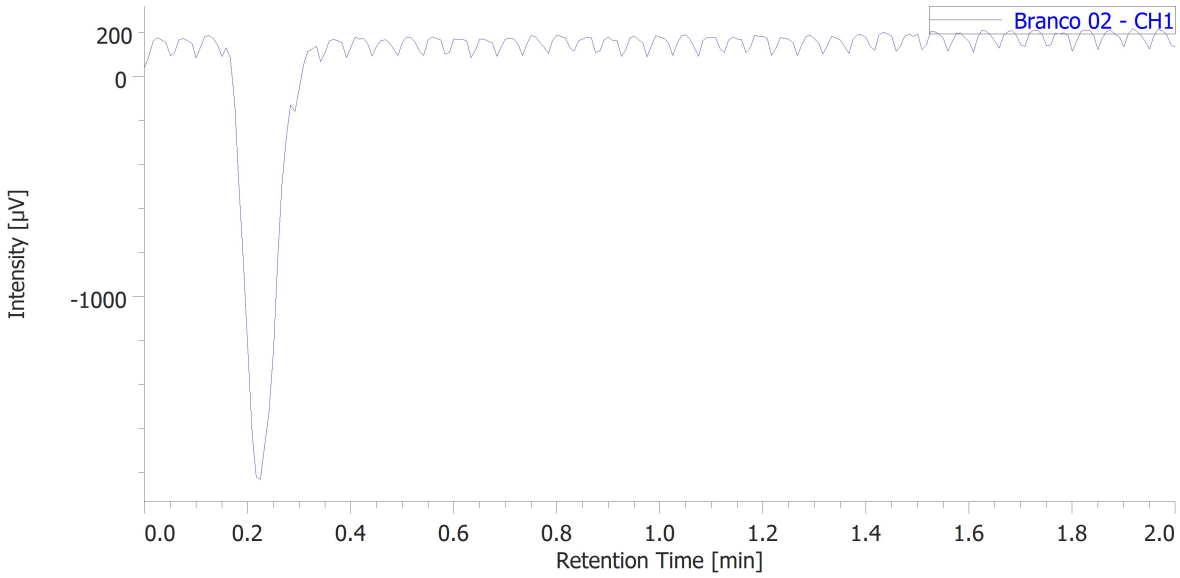


Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:03:04 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:01:02 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação (Manual)

Creator
Reviewer
Approver

Chromatogram

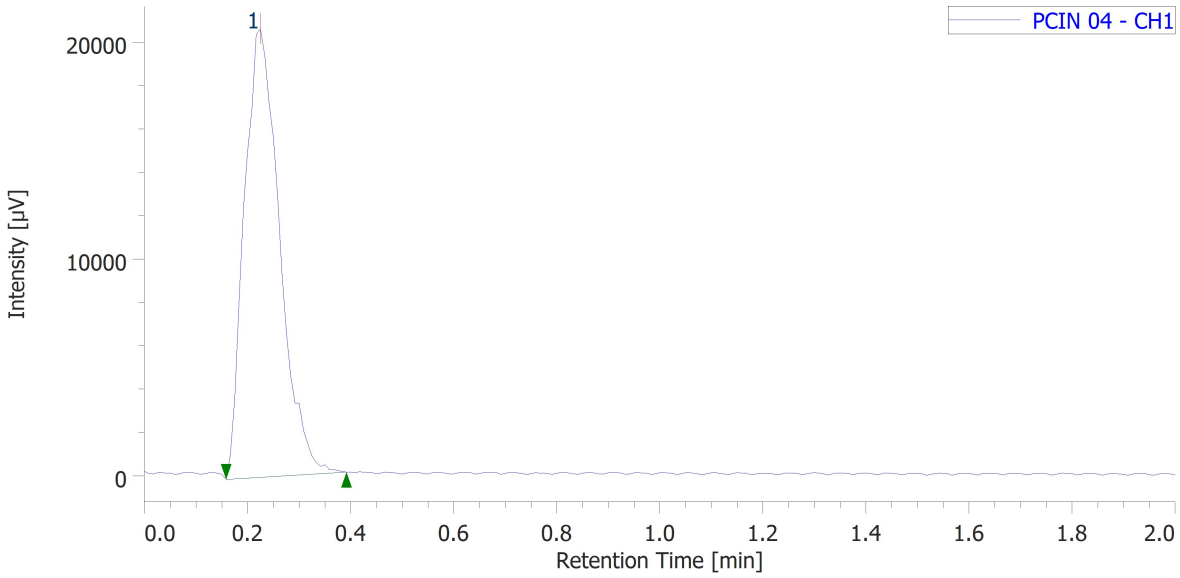

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:05:20 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:03:19 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.225	98516	20680	100.000	100.000	N/A	48	N/A	1.325	

Creator
Reviewer
Approver

Chromatogram

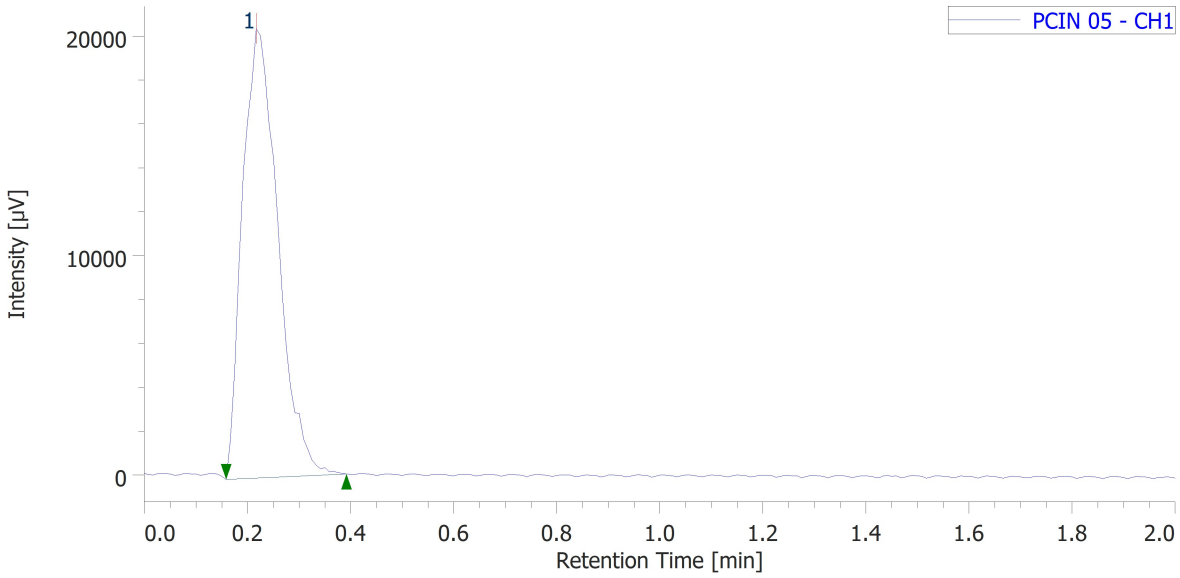

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:07:36 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:05:35 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	97794	20458	100.000	100.000	N/A	43	N/A	1.464	

Creator
Reviewer
Approver

Chromatogram

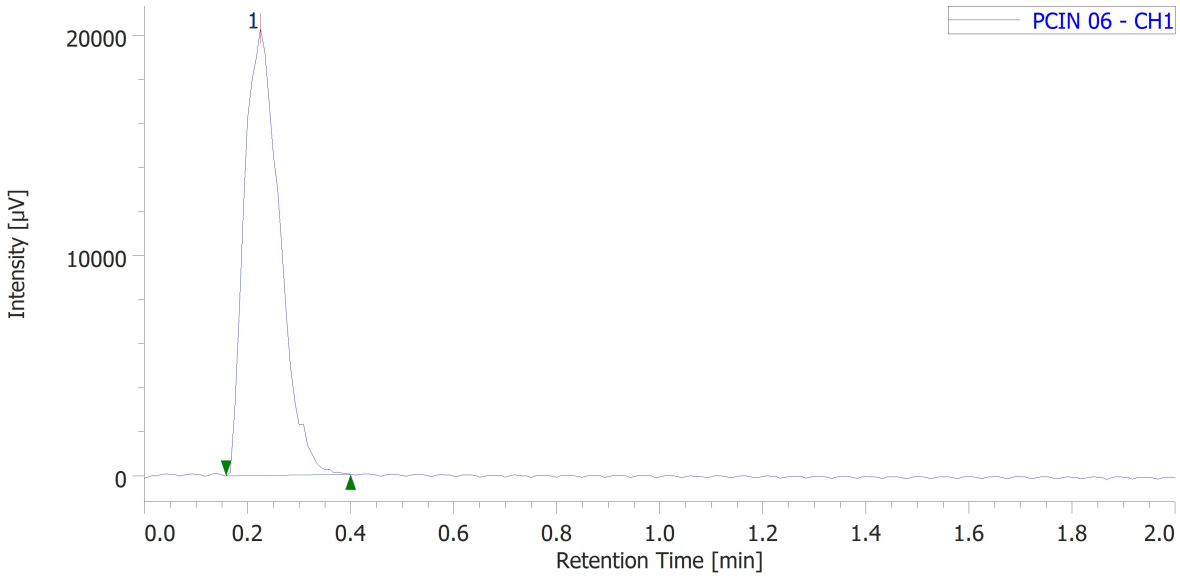

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:09:54 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:07:52 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.225	96813	20267	100.000	100.000	N/A	45	N/A	1.384	

Creator
Reviewer
Approver

Chromatogram

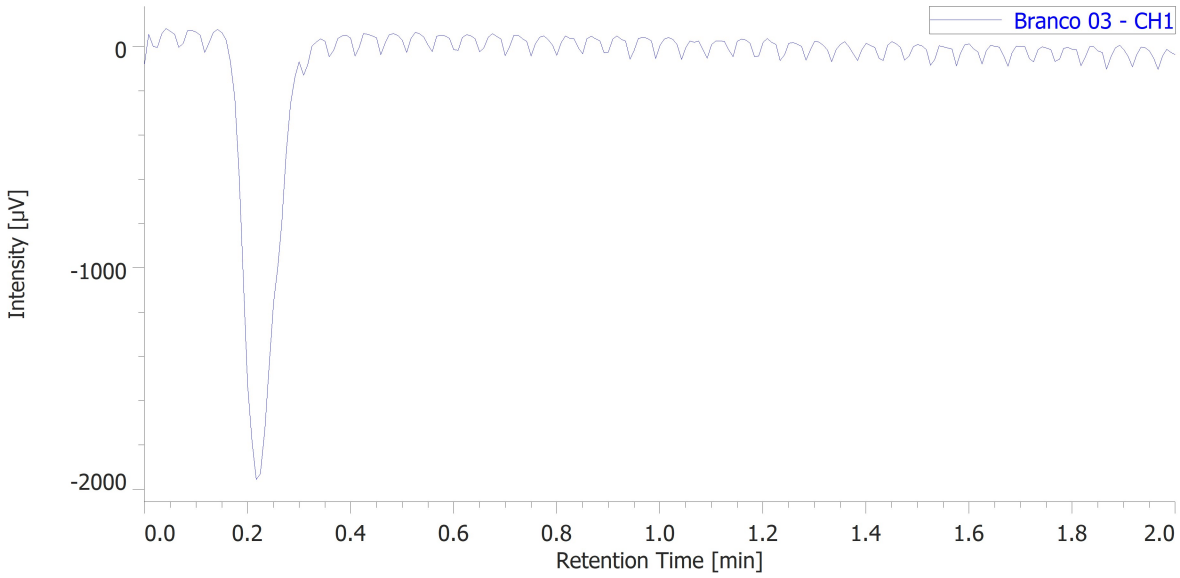


Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:12:10 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:10:09 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator
Reviewer
Approver

Chromatogram

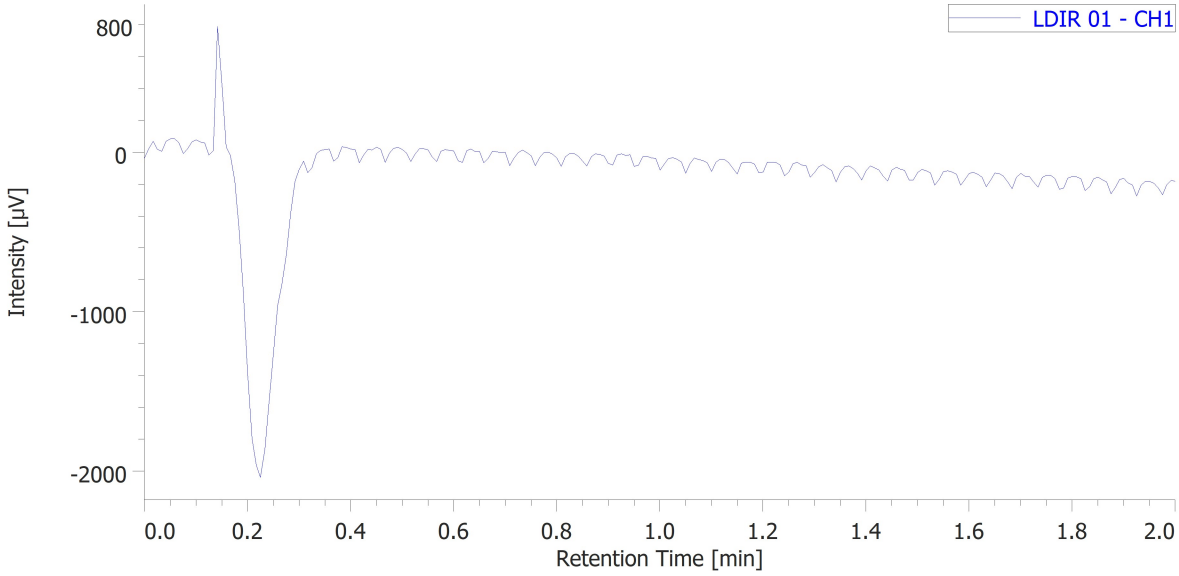


Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:50:11 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:12:25 PM
Volume	2.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

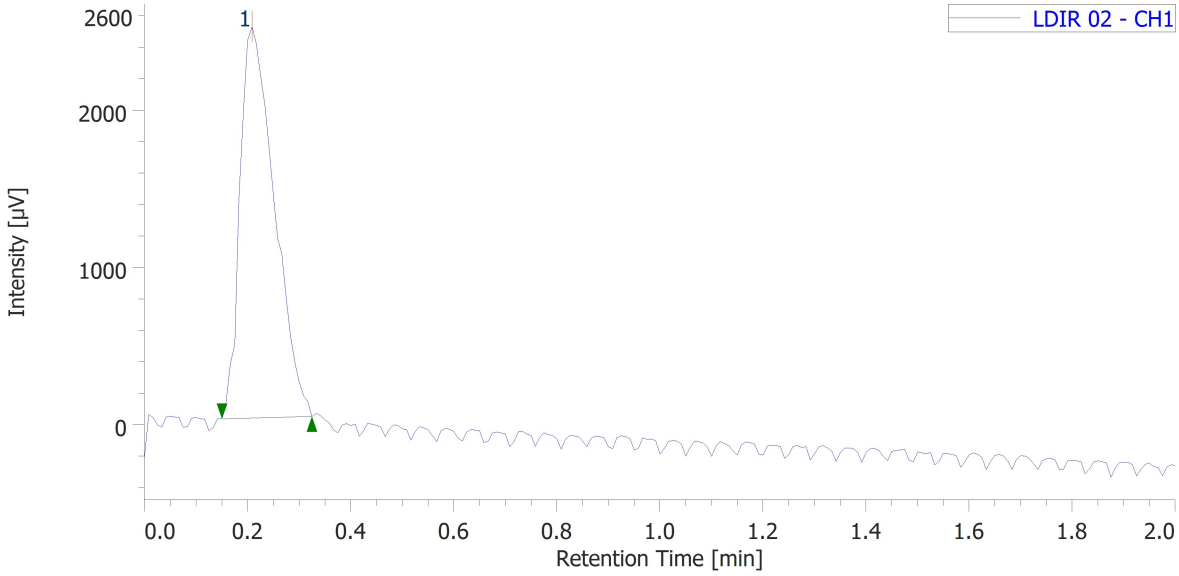

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:50:12 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:14:42 PM
Volume	2.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.208	11532	2487	100.000	100.000	N/A	45	N/A	1.526	

Creator QPackSA
Reviewer
Approver

Chromatogram

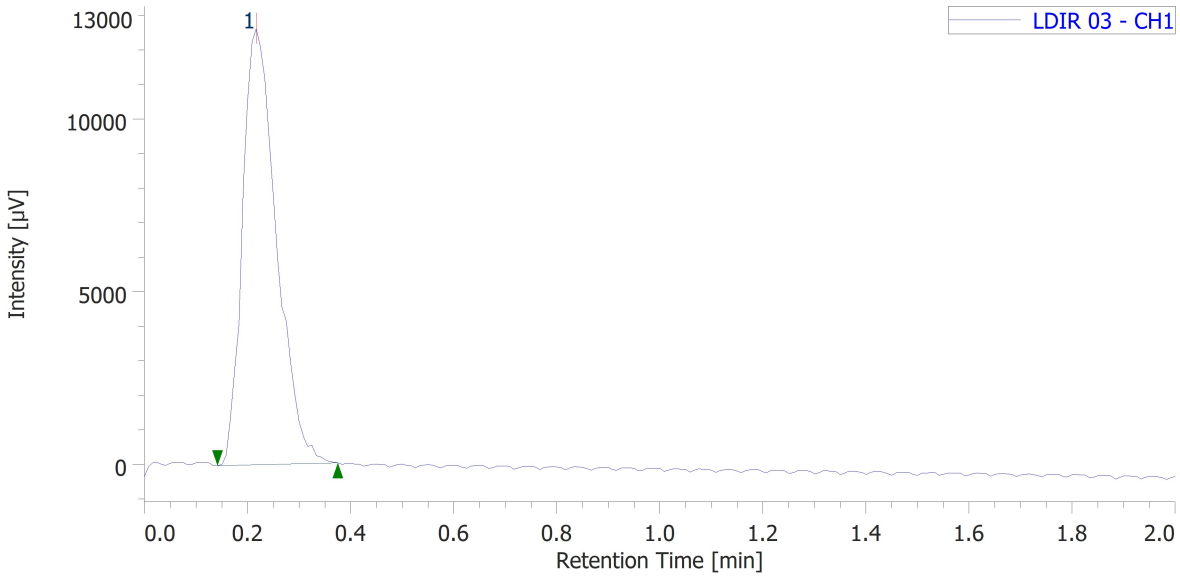

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:50:12 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:16:59 PM
Volume	2.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	57807	12619	100.000	100.000	N/A	55	N/A	1.362	

Creator QPackSA
Reviewer
Approver

Chromatogram

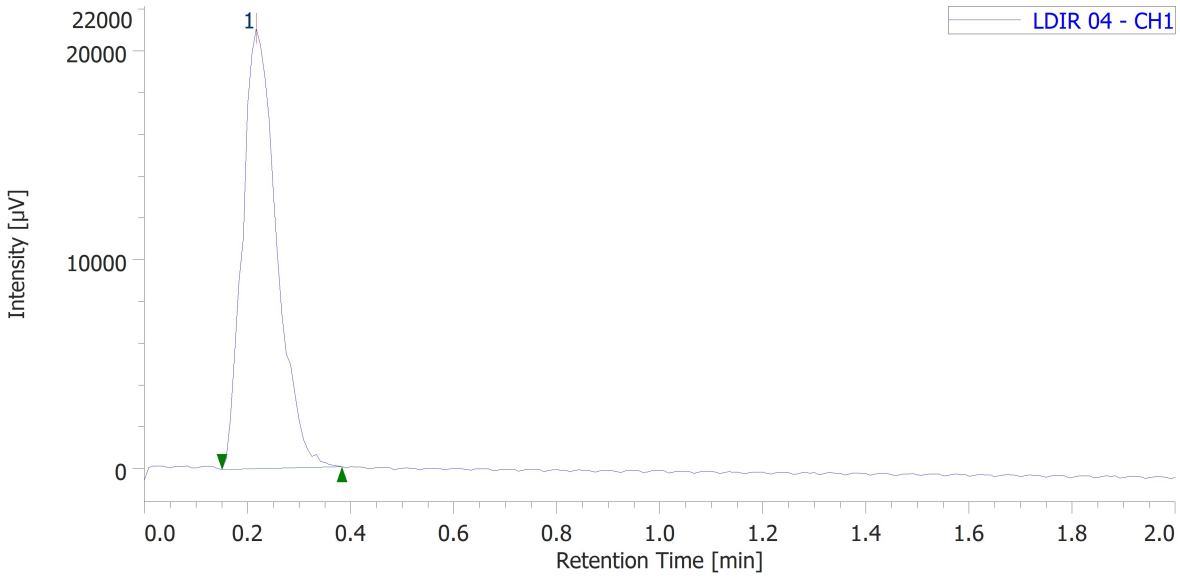

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:50:12 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:19:15 PM
Volume	2.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	96748	21059	100.000	100.000	N/A	57	N/A	1.363	

Creator QPackSA
Reviewer
Approver

Chromatogram

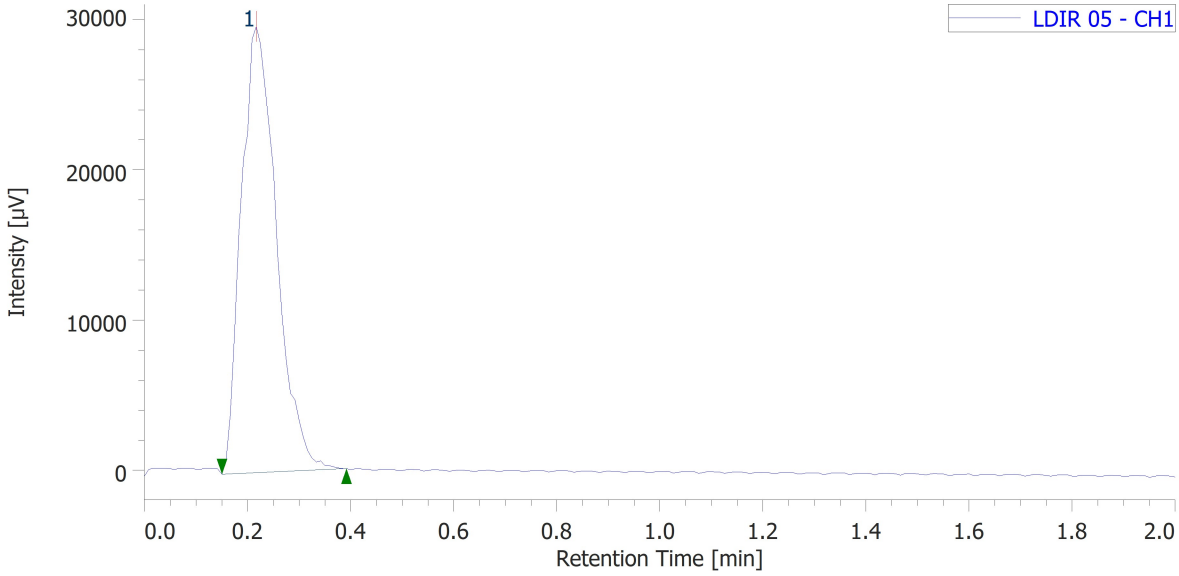

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:50:12 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:21:32 PM
Volume	2.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	140860	29690	100.000	100.000	N/A	45	N/A	1.363	

Creator QPackSA
Reviewer
Approver

Chromatogram

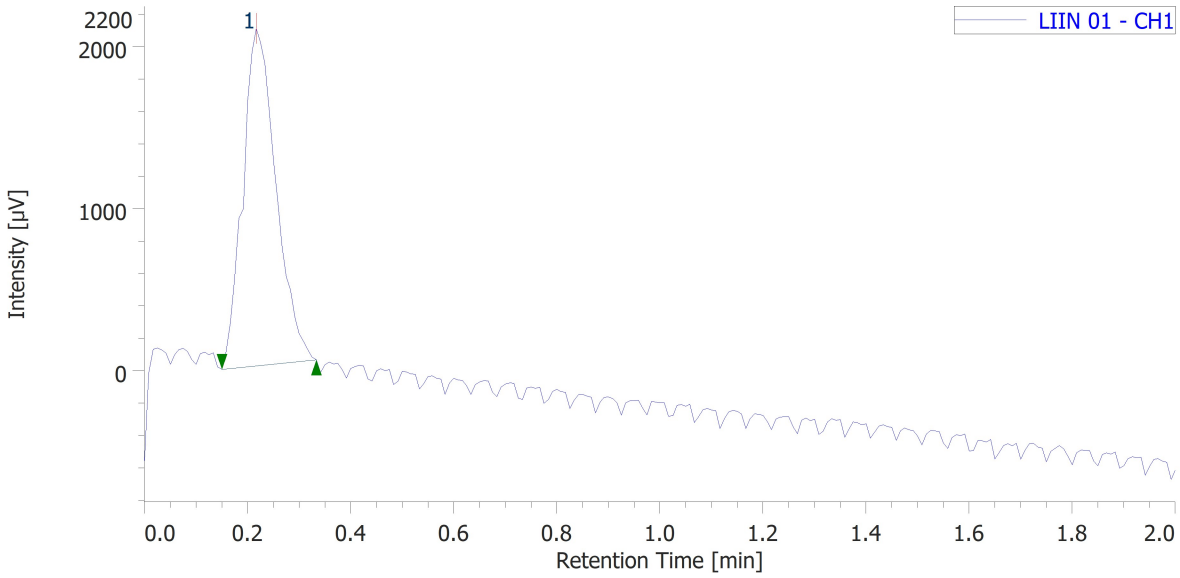

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:57:49 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:23:46 PM
Volume	0.1 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	9290	2080	100.000	100.000	N/A	62	N/A	1.303	

Creator QPackSA
Reviewer
Approver

Chromatogram

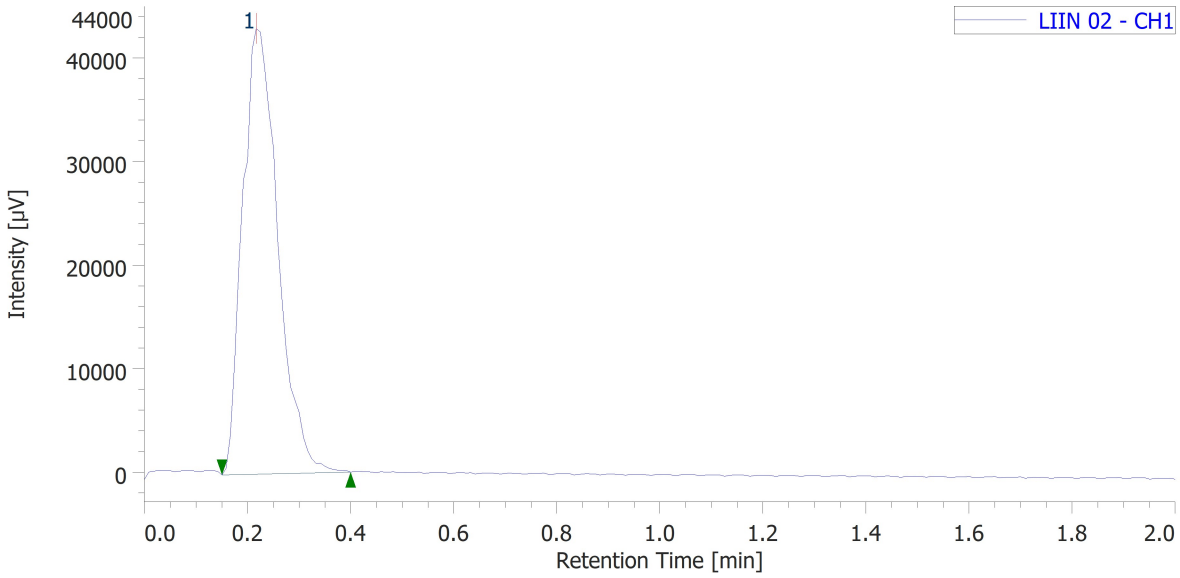

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:57:49 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:26:03 PM
Volume	2.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	204759	42989	100.000	100.000	N/A	46	N/A	1.420	

Creator QPackSA
Reviewer
Approver

Chromatogram

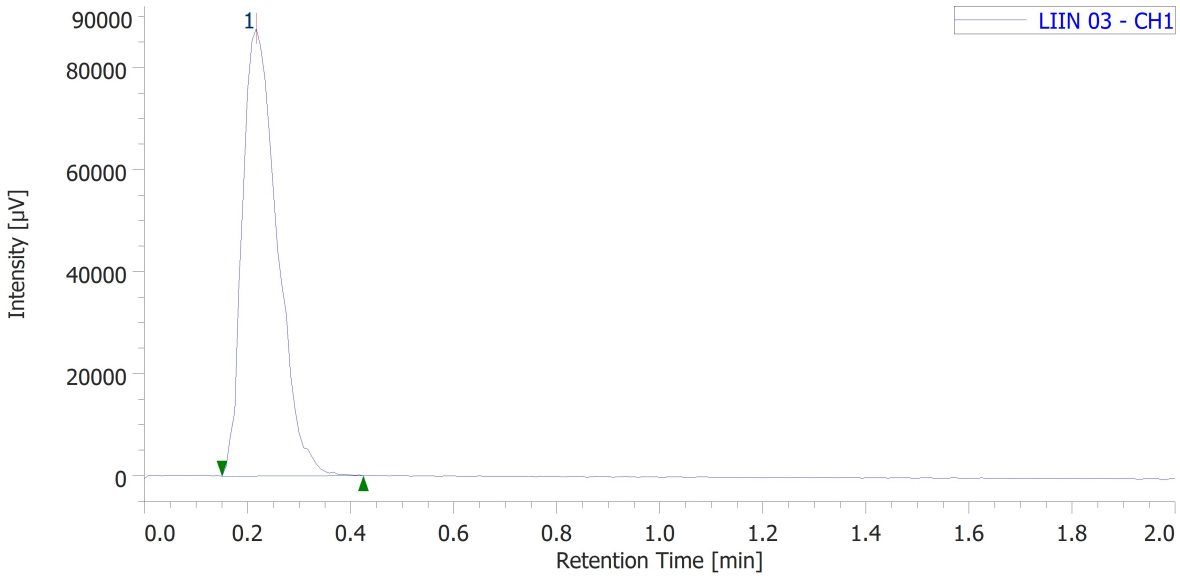

Chromatogram Information

User Name	QPackSA
Date Modified	4/4/2025 3:57:49 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:28:21 PM
Volume	4.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.217	413482	87662	100.000	100.000	N/A	49	N/A	1.456	

Creator QPackSA
Reviewer
Approver

Chromatogram

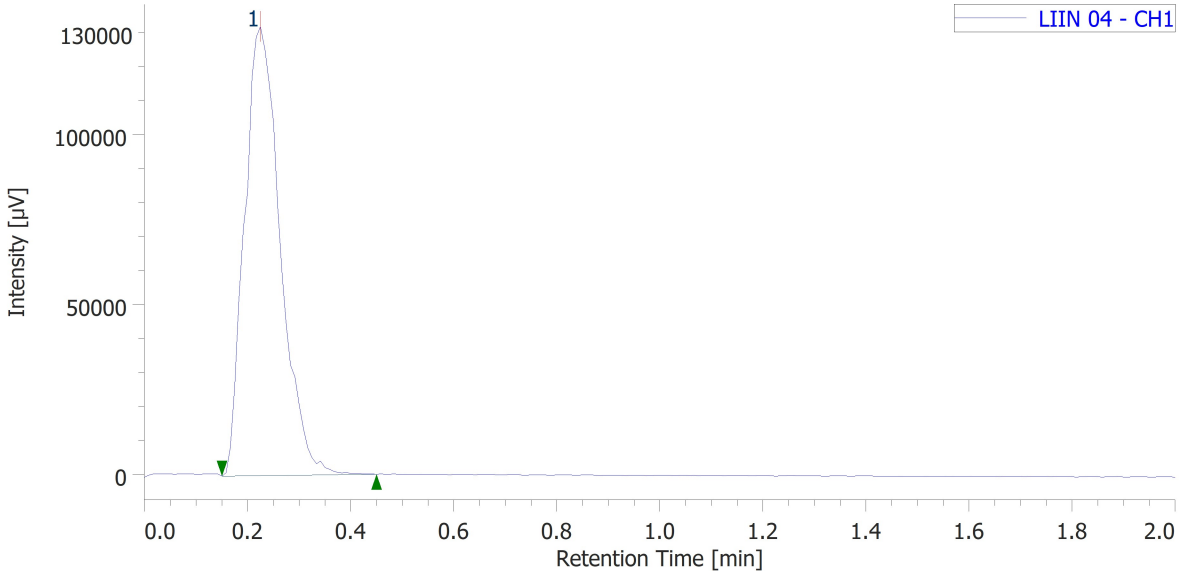

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:57:49 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:30:40 PM
Volume	6.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.225	638467	132104	100.000	100.000	N/A	49	N/A	1.295	

Creator QPackSA
Reviewer
Approver

Chromatogram

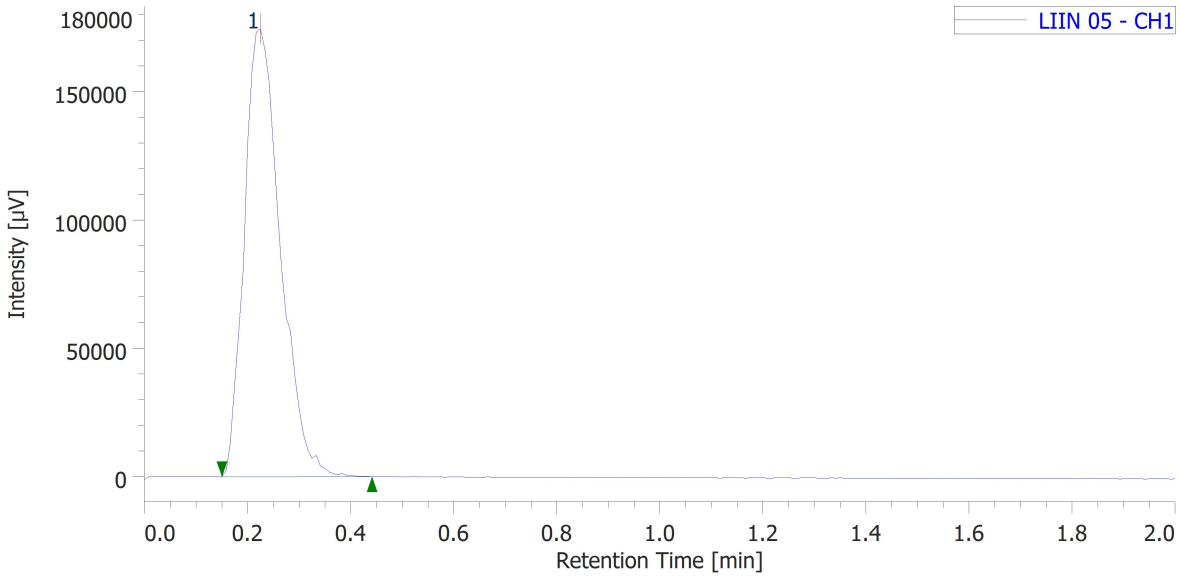

Chromatogram Information	
User Name	QPackSA
Date Modified	4/4/2025 3:57:49 PM
Description	
HPLC System Name	HPLC 02
Injection Date	4/4/2025 3:33:00 PM
Volume	8.0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação Injetor
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicerol	1	0.225	849528	174489	100.000	100.000	N/A	55	N/A	1.277	

Creator QPackSA
Reviewer
Approver