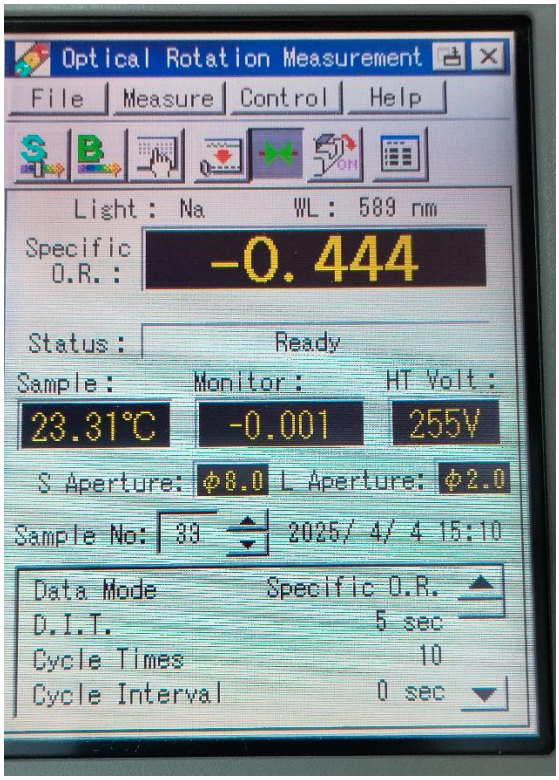
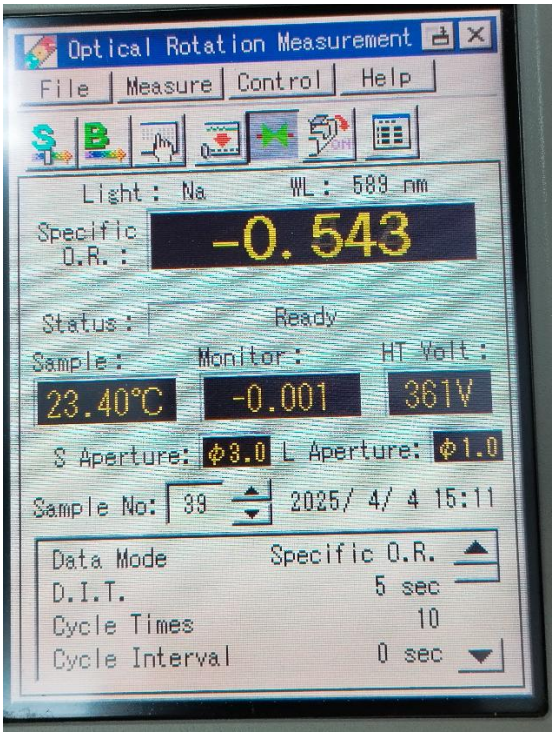
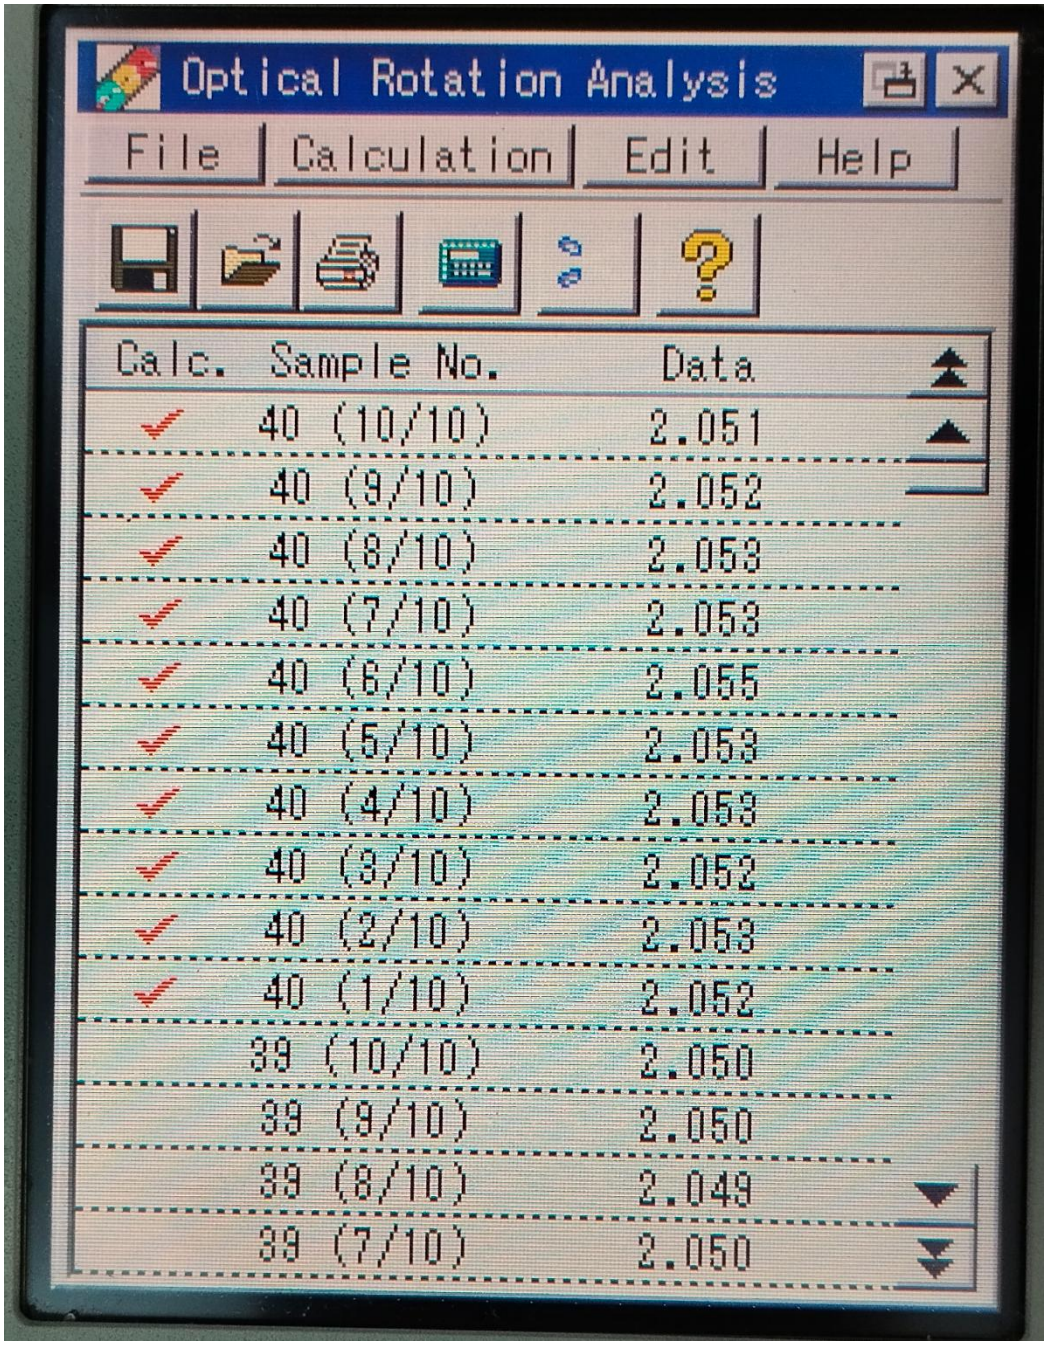
19.1 – NÍVEL DE ENERGIA DO SISTEMA

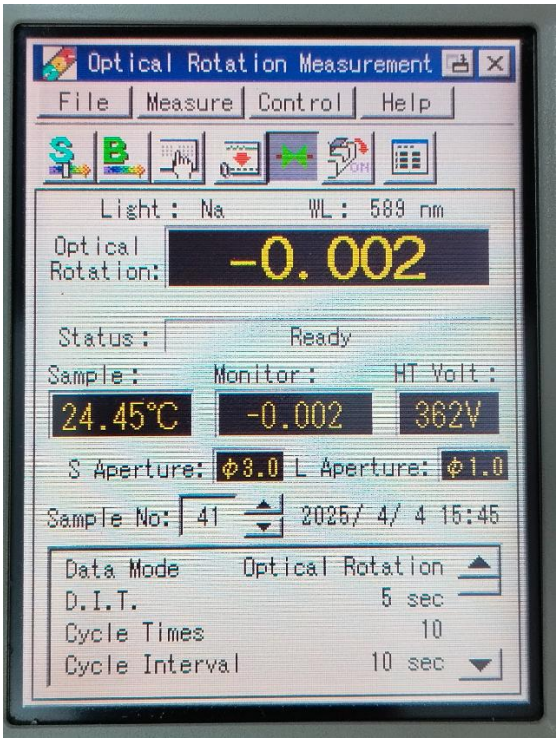


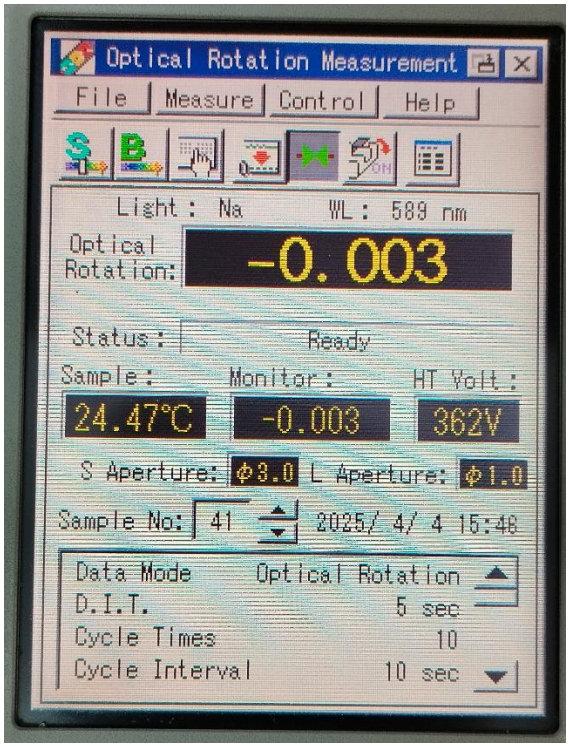


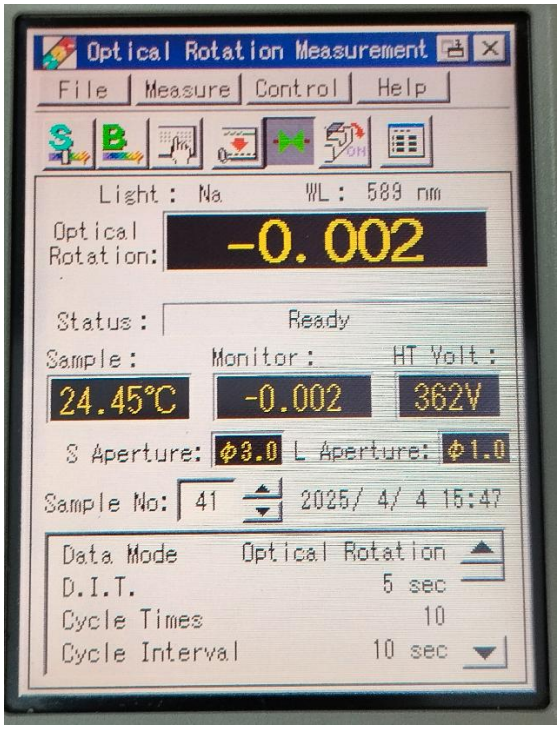
19.2 – EXATIDÃO E PRECISÃO DAS LEITURAS

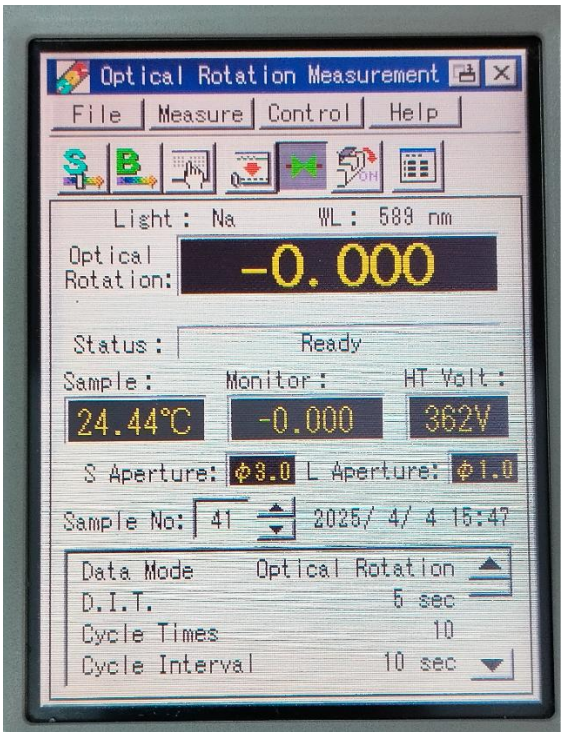


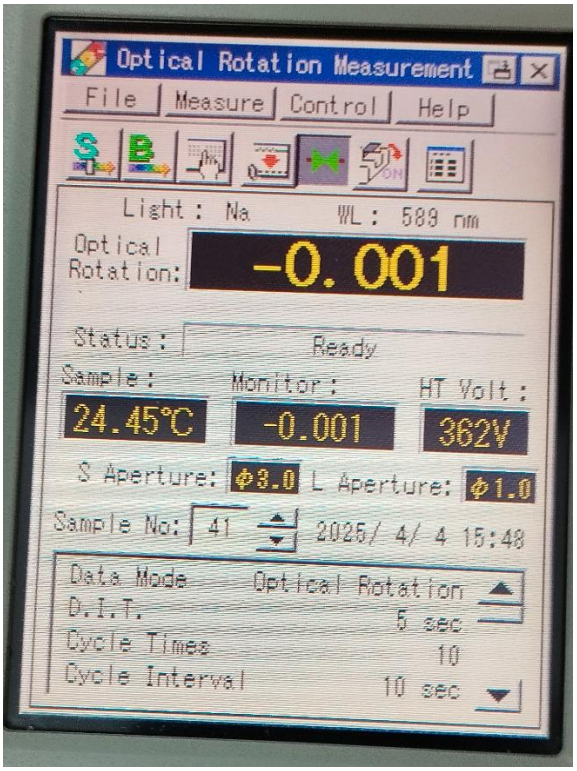
19.3 – REPETIBILIDADE DO ZERO

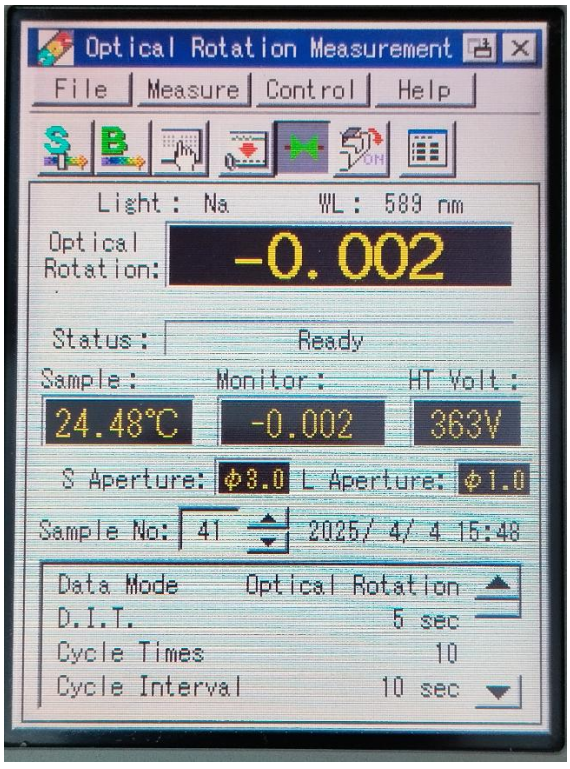


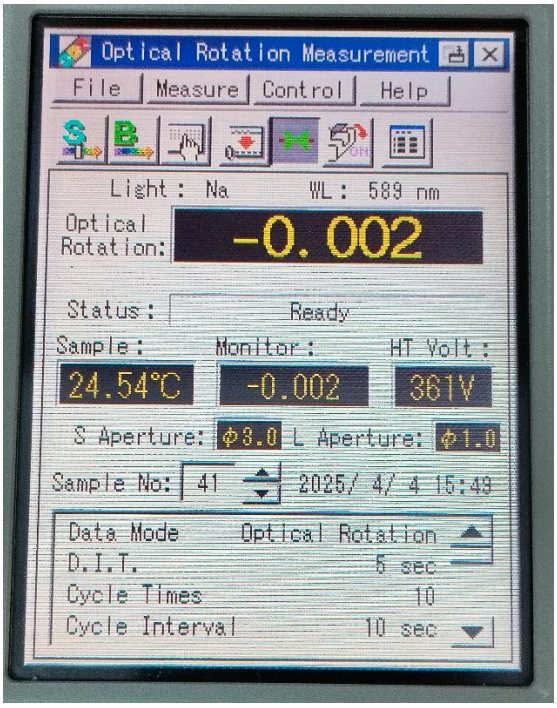


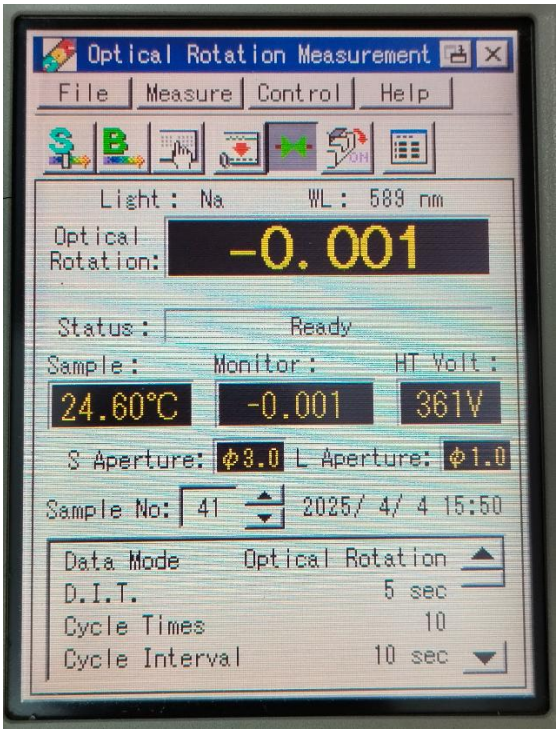

Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.002
Status :
Ready
Sample :
Monitor :
HT Volt :
24.45℃
-0.002
362V
S Aperture:
φ3.0
L Aperture:
φ1.0
Sample No:
41
2025/ 4/ 4 15:47
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec

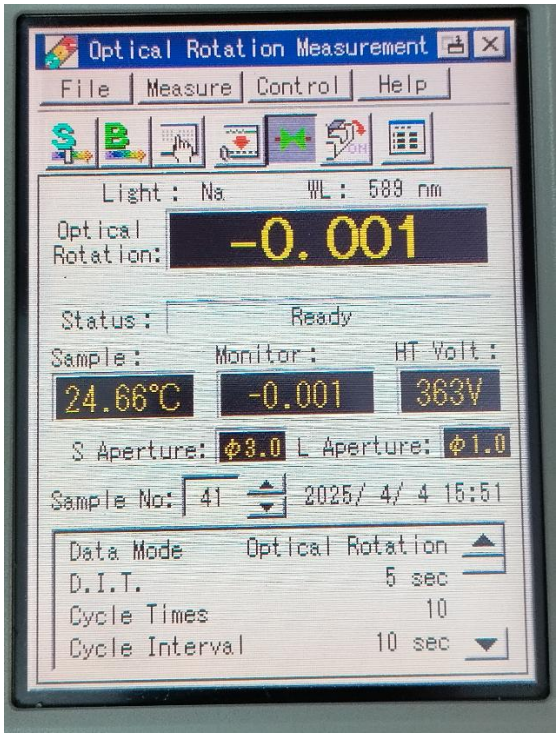

Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.000
Status :
Ready
Sample :
Monitor :
HT Volt :
24.44℃
-0.000
362V
S Aperture:
φ3.0
L Aperture:
φ1.0
Sample No:
41
2025/ 4/ 4 15:47
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec

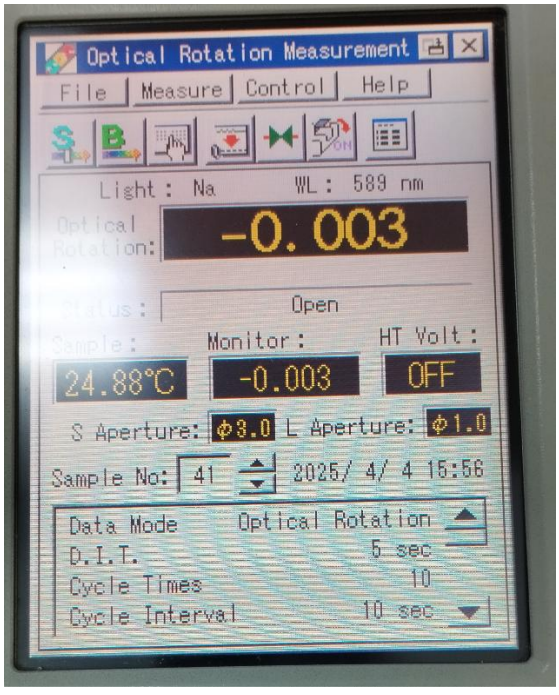

Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.001
Status :
Ready
Sample :
Monitor :
HT Volt :
24.45°C
-0.001
362V
S Aperture: φ3.0
L Aperture: φ1.0
Sample No: 41
2025/ 4/ 4 15:48
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec


Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.002
Status :
Ready
Sample :
Monitor :
HT Volt :
24.48°C
-0.002
363V
S Aperture: φ3.0
L Aperture: φ1.0
Sample No: 41
2025/ 4/ 4 15:48
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec


Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.002
Status :
Ready
Sample :
Monitor :
HT Volt :
24.54℃
-0.002
361V
S Aperture: φ3.0
L Aperture: φ1.0
Sample No: 41
2025/ 4/ 4 15:49
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec


Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.001
Status :
Ready
Sample :
Monitor :
HT Volt :
24.60℃
-0.001
361V
S Aperture: φ3.0
L Aperture: φ1.0
Sample No: 41
2025/ 4/ 4 15:50
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec


Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.001
Status :
Ready
Sample :
Monitor :
HT Volt :
24.66°C
-0.001
363V
S Aperture:
φ3.0
L Aperture:
φ1.0
Sample No:
41
2025/ 4/ 4 15:51
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec


Optical Rotation Measurement
File
Measure
Control
Help
Light : Na
WL : 589 nm
Optical Rotation:
-0.003
Status :
Open
Sample :
Monitor :
HT Volt :
24.88°C
-0.003
OFF
S Aperture:
φ3.0
L Aperture:
φ1.0
Sample No:
41
2025/ 4/ 4 15:56
Data Mode
Optical Rotation
D.I.T.
5 sec
Cycle Times
10
Cycle Interval
10 sec

19.4 – PRECISÃO DA TEMPERATURA

