
Peak Find - 01 Exatidão do Comprimento de Onda 2023.jws

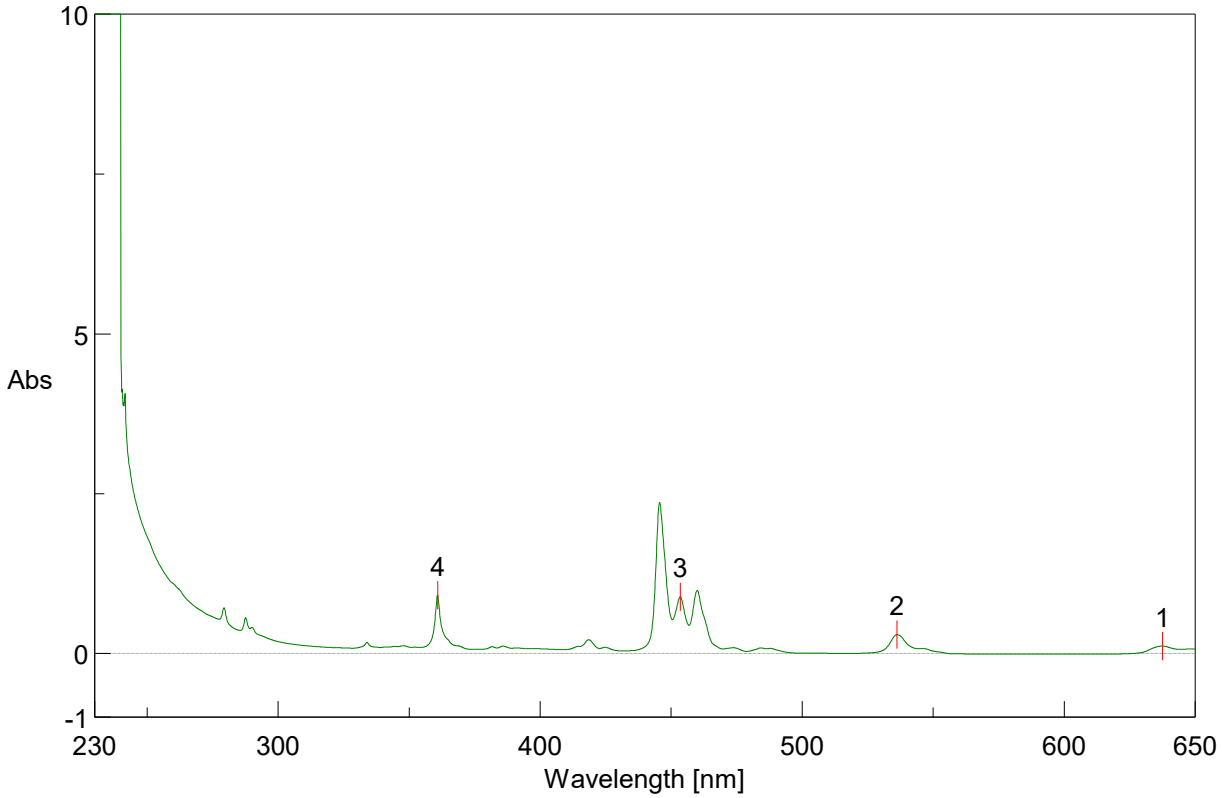

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	10/04/2023 11:52
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Measurement date	10/04/2023 11:50
Parameter file	C:\Jasco\Exatidão do Comprimento de Onda.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	637.5	0.111292	2	536.2	0.289532
3	453.5	0.882948	4	360.9	0.90821

Peak Find - 02 REP01 Comprimento de Onda 2023.jws

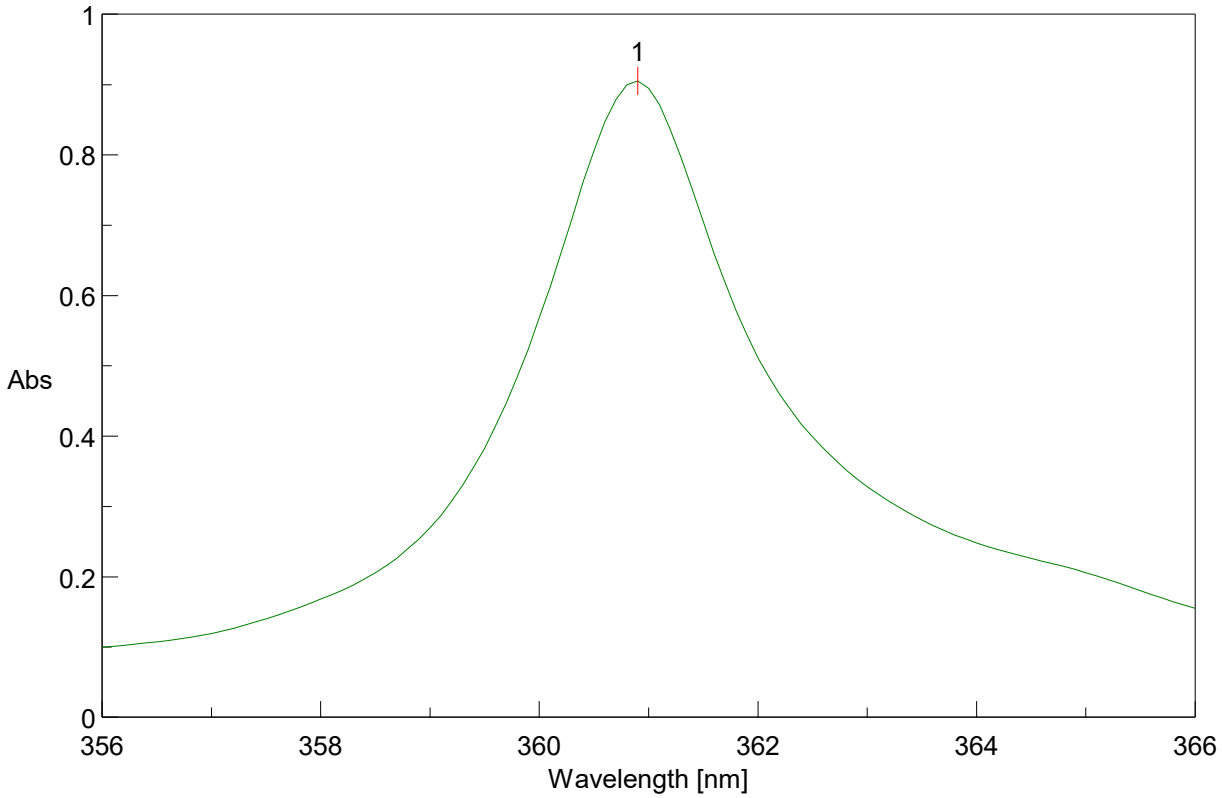

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco
Division Assistência Técnica
Company VicPharma

[Detailed Information]
Creation date 10/04/2023 11:56

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 366 nm
End 356 nm
Data interval 0.1 nm
Data points 101

[Measurement Information]
Instrument name V-730
Model name V-730
Serial No. D334661798

Measurement date 10/04/2023 11:54


Parameter file C:\Jasco\Repetibilidade do Comprimento de Onda.uvsp
Photometric mode Abs
Measurement range 366 - 356 nm
Data interval 0.1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 40 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction None
No. of cycles 1

Creation QPackSA
Review
Approval

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.904926			

Peak Find - 02 REP02 Comprimento de Onda 2023.jws

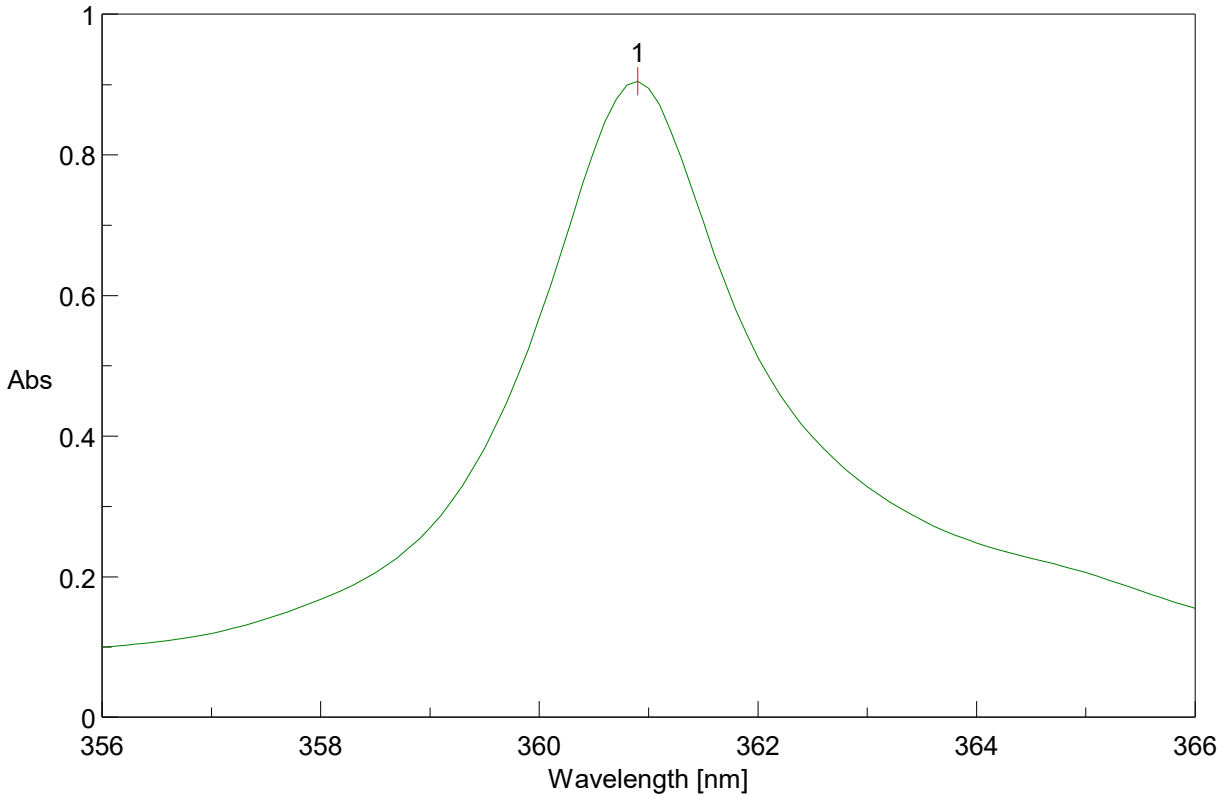

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco
Division Assistência Técnica
Company VicPharma

[Detailed Information]
Creation date 10/04/2023 11:57

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 366 nm
End 356 nm
Data interval 0.1 nm
Data points 101

[Measurement Information]
Instrument name V-730
Model name V-730
Serial No. D334661798

Measurement date 10/04/2023 11:55


Parameter file C:\Jasco\Repetibilidade do Comprimento de Onda.uvsp
Photometric mode Abs
Measurement range 366 - 356 nm
Data interval 0.1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 40 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction None
No. of cycles 1

Creation QPackSA
Review
Approval

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.904489			

Peak Find - 02 REP03 Comprimento de Onda 2023.jws

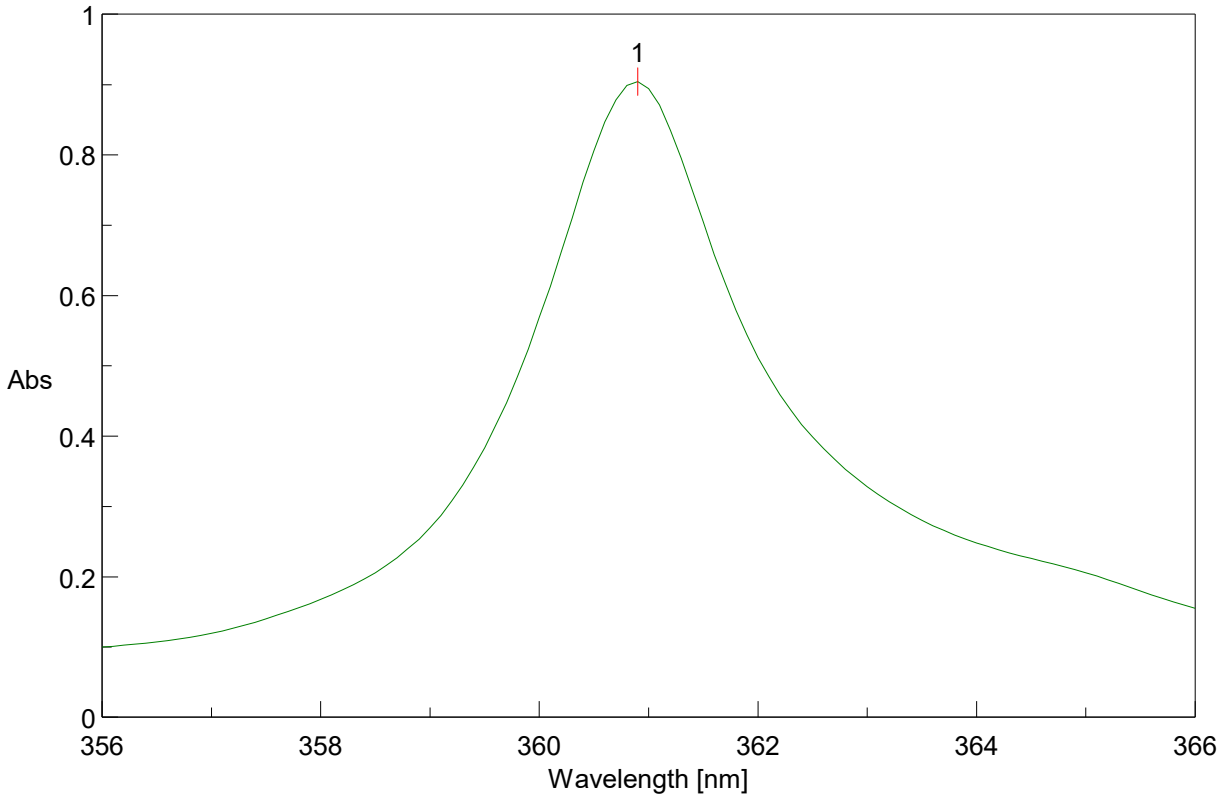

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco
Division Assistência Técnica
Company VicPharma

[Detailed Information]
Creation date 10/04/2023 11:57

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 366 nm
End 356 nm
Data interval 0.1 nm
Data points 101

[Measurement Information]
Instrument name V-730
Model name V-730
Serial No. D334661798

Measurement date 10/04/2023 11:55


Parameter file C:\Jasco\Repetibilidade do Comprimento de Onda.uvsp
Photometric mode Abs
Measurement range 366 - 356 nm
Data interval 0.1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 40 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction None
No. of cycles 1

Creation QPackSA
Review
Approval

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	0.904019			

Full Width at Half Maximum - 03 Resolução 2023.jws

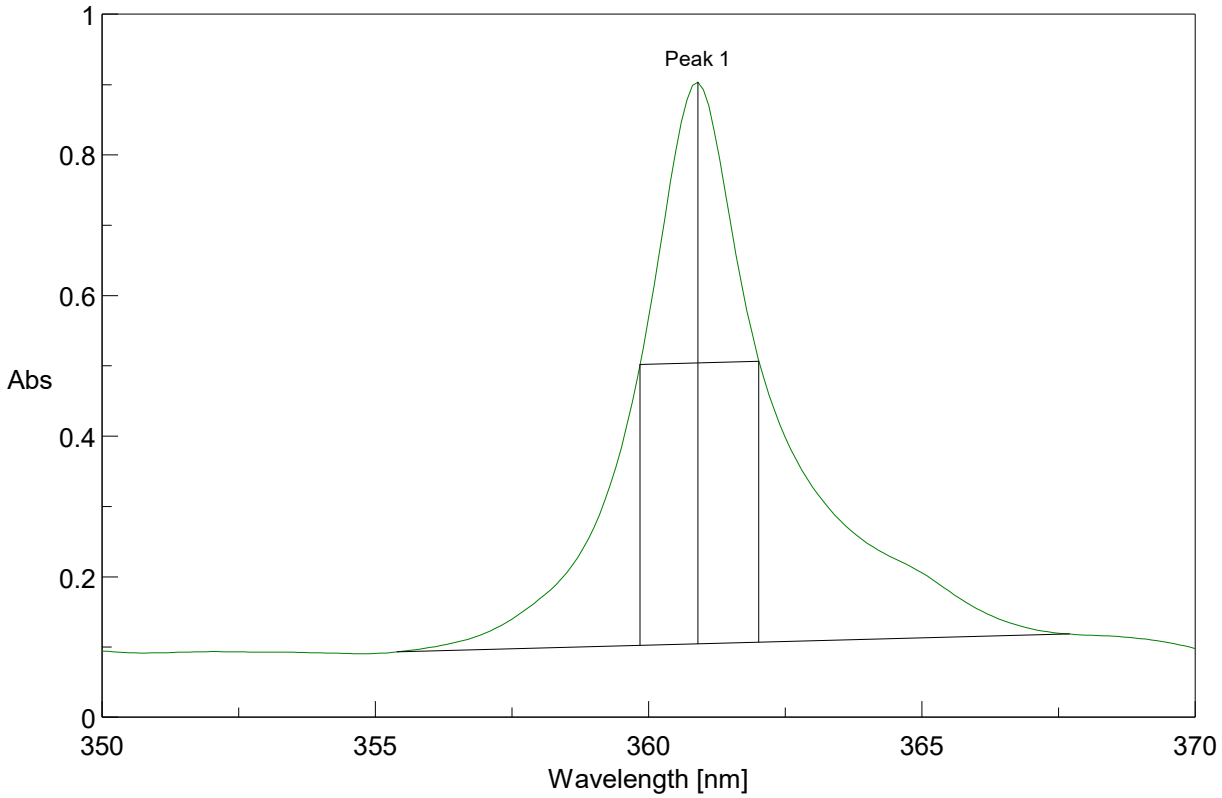

[Result of FWHM Calculation]

Base 1	Base 2	Peak	Height	FWHM
355.4	367.7	360.9	0.798998	2.17447

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	10/04/2023 11:59
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	370 nm
End	350 nm
Data interval	0.1 nm
Data points	201

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Measurement date	10/04/2023 11:56
Parameter file	C:\Jasco\Resolução.uvsp
Photometric mode	Abs
Measurement range	370 - 350 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

04 Exatidão Fotométrica 2023.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	10/04/2023 12:02
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Parameter file	C:\Jasco\Exatidão Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	On/Measured
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Blank-1			0.0000
Sample-1	F2		0.2741
Sample-2	F3		0.5302
Sample-3	F4		1.1027

Creation	QPackSA
Review	
Approval	


05 Repetibilidade Fotométrica 2023.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	10/04/2023 12:06
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Parameter file	C:\Jasco\Repetibilidade Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	361.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	On/Measured
No. of cycles	3
Cycle interval	0 sec

Mode	Sample Name	Comment	361.0 nm
Blank-1			0.0001
ample-1-			0.9206
ample-1-2			0.9203
ample-1-3			0.9204
mple-1-Av			0.9204
mple-1-S.			0.0001
mple-1-C			0.0139

Creation	QPackSA
Review	
Approval	

Peak Find - 06 Estabilidade da Linha de Base 2023.jws

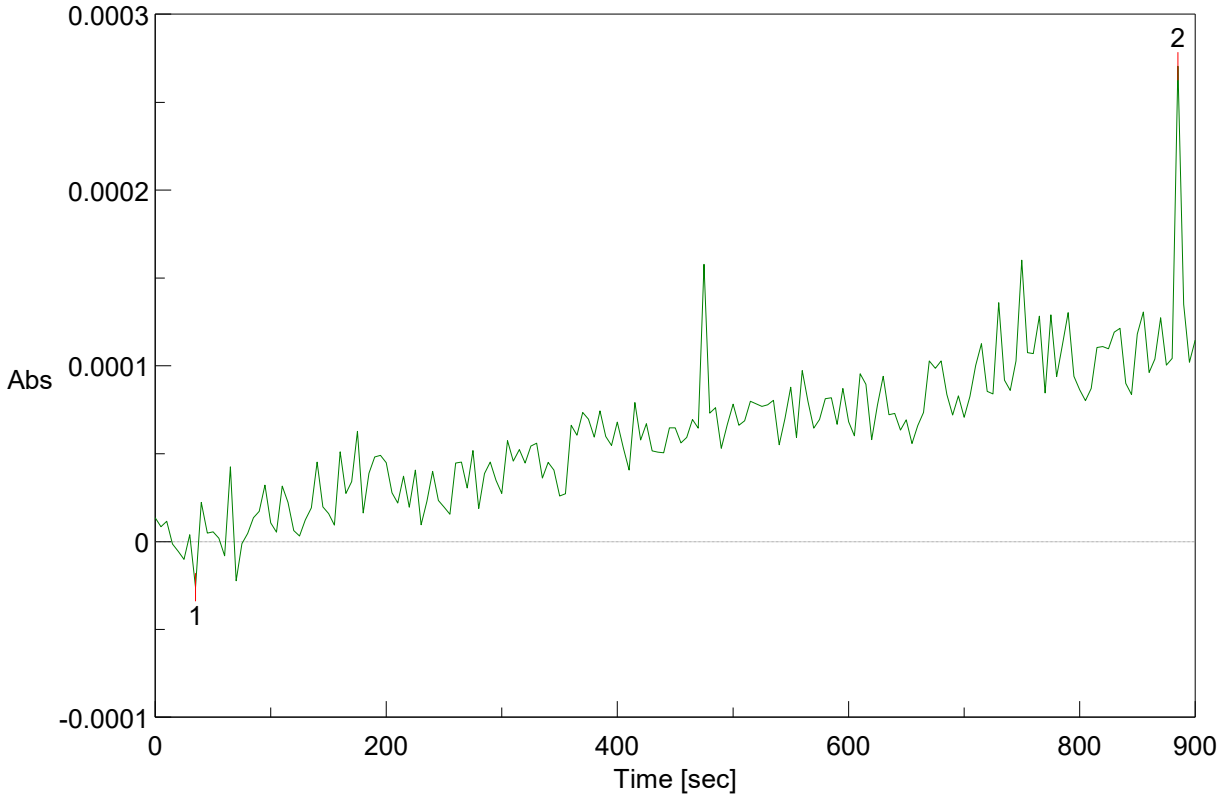

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	10/04/2023 12:26
Data array type	Linear data array
Horizontal axis	Time [sec]
Vertical axis	Abs
Start	0 sec
End	900 sec
Data interval	5 sec
Data points	181


[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Measurement date	10/04/2023 12:25
Parameter file	C:\Jasco\Estabilidade da Linha de Base.uvtm
Photometric mode	Abs
Measurement range	0 - 900 sec
Data interval	5 sec
UV/Vis bandwidth	1.0 nm
Response	3.84 sec
Monitor wavelength	250 nm
Change source at	340 nm
Light source	D2/WI
Correction	Blank

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	35	-2.60863E-005	2	885	0.000270235

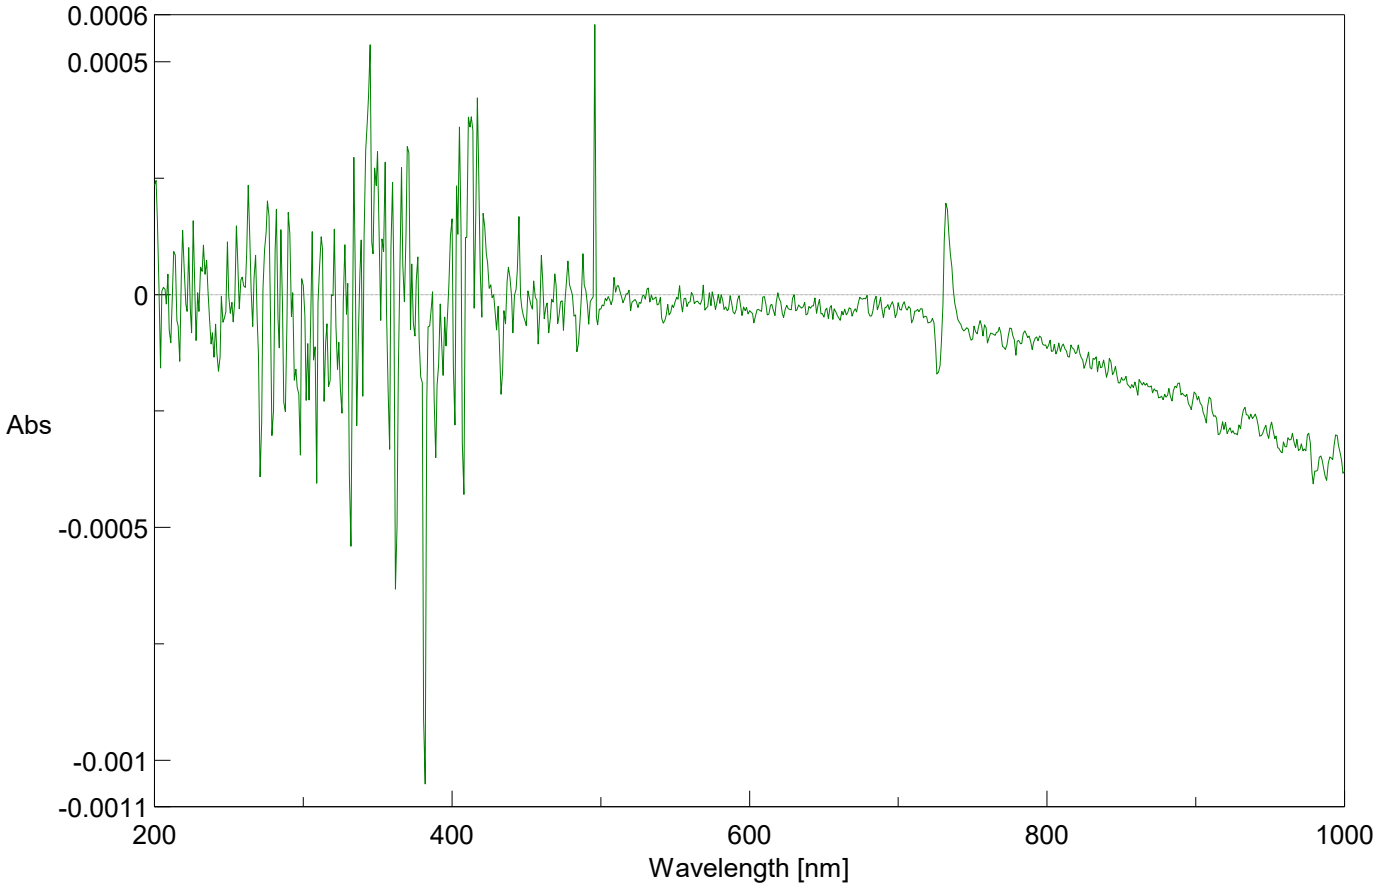

07 Uniformidade da Linha de Base 2023.jws

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco
Division Assistência Técnica
Company VicPharma

[Detailed Information]
Creation date 10/04/2023 12:35

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 1000 nm
End 200 nm
Data interval 1 nm
Data points 801

[Measurement Information]
Instrument name V-730
Model name V-730
Serial No. D334661798

Measurement date 10/04/2023 12:34

Parameter file C:\Jasco\Uniformidade da Linha de Base.uvsp
Photometric mode Abs
Measurement range 1000 - 200 nm
Data interval 1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 400 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction Baseline
No. of cycles 1

Creation QPackSA
Review
Approval