
Peak Find - Explo 01 UV_tR1,81 D.jws

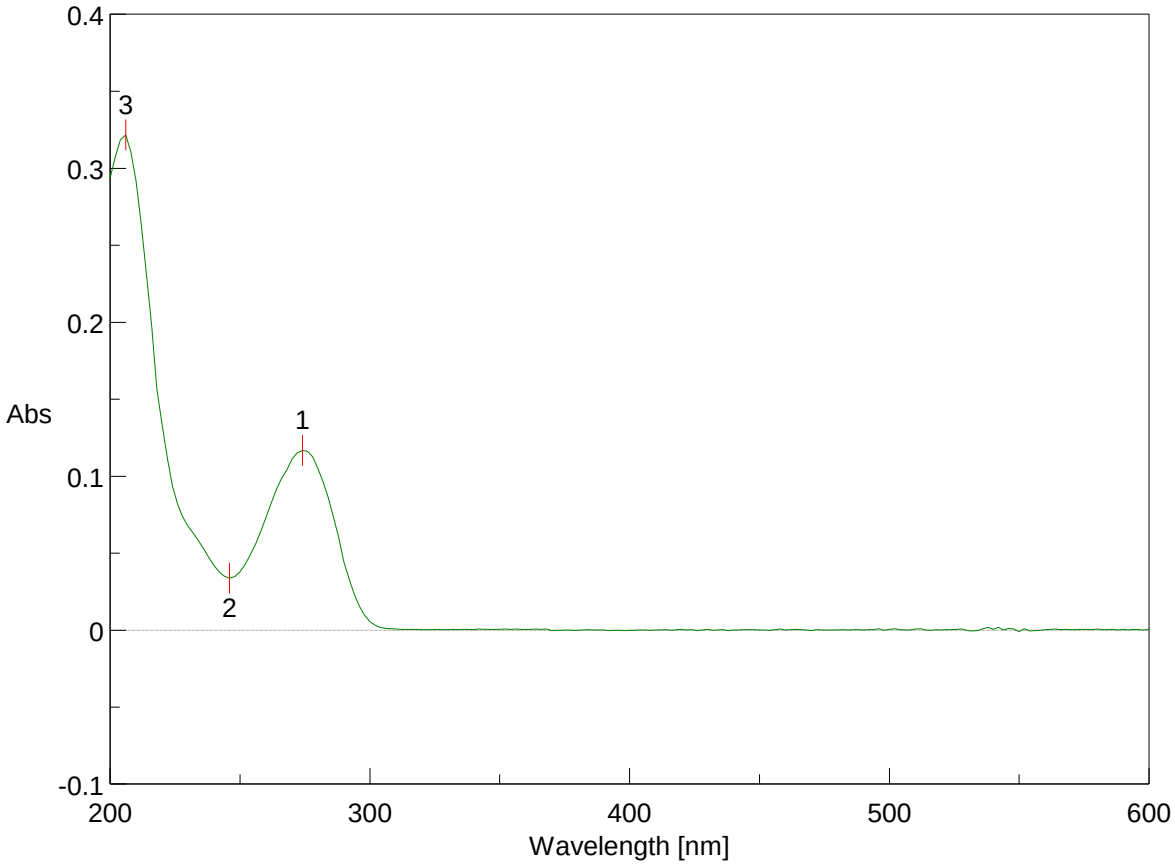

[Comments]

User	Administrator
Division	---
Company	Jasco do Brasil
Creation date	29/03/2016 09:24

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	201


[Measurement Information]

Instrument Name	UV-1575
Model Name	UV-1575
Serial No.	XXXXX
ROM version	V1.16

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.116622	2	246	0.0337688
3	206	0.321647			

Chromatogram

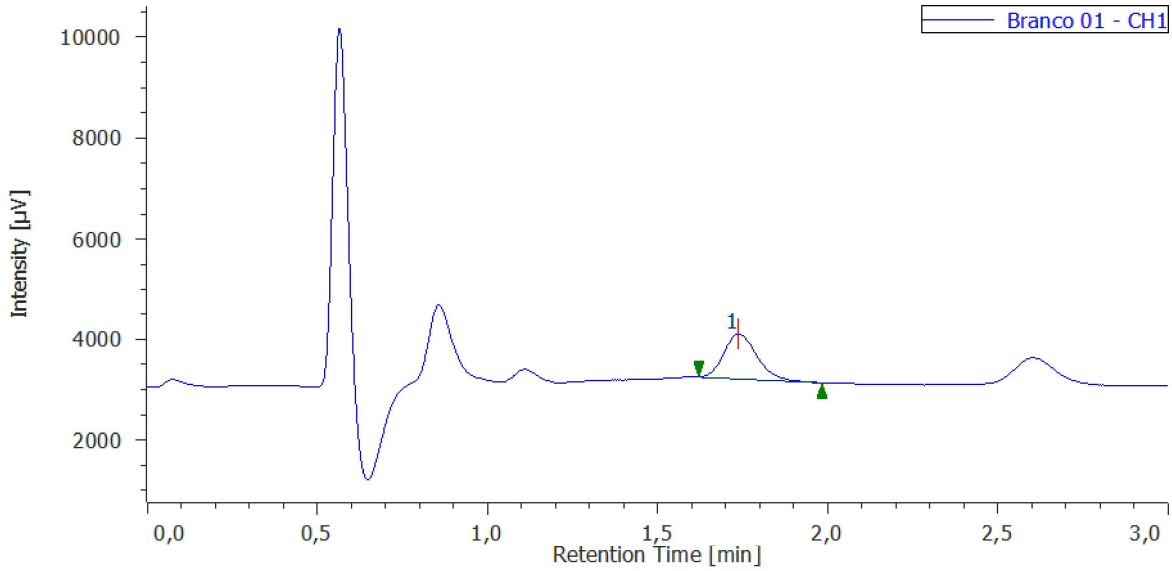


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:04:49
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:40:45
Volume	10,00 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,737	6097	901	100,000	100,000	N/A	1573	N/A	1,238	

Chromatogram

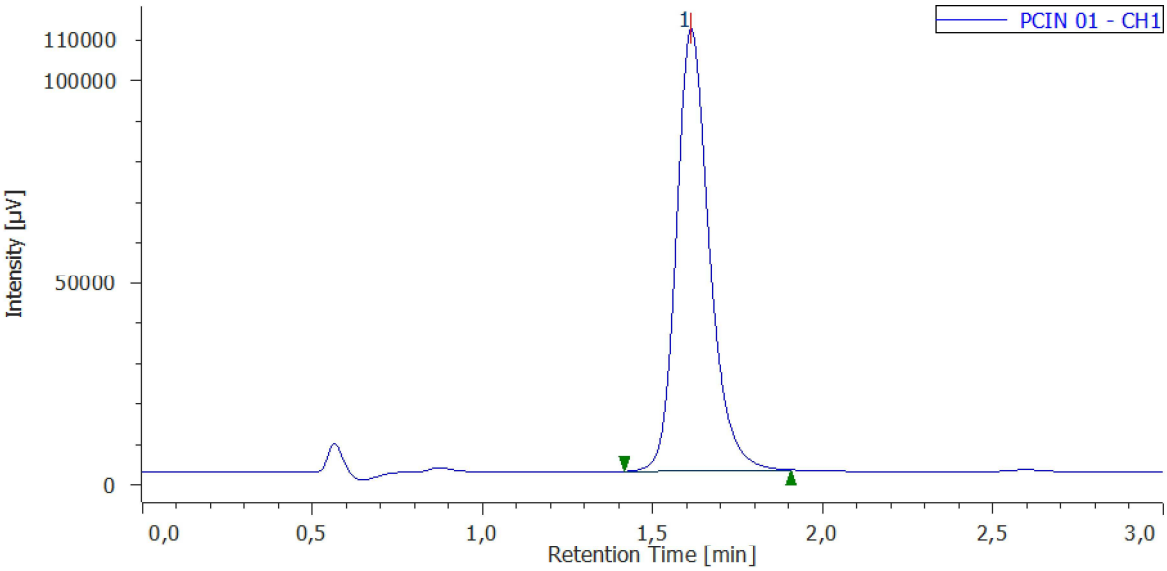


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 09:48:46
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:44:22
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,613	740128	109456	100,000	100,000	N/A	1422	N/A	1,225	

Chromatogram

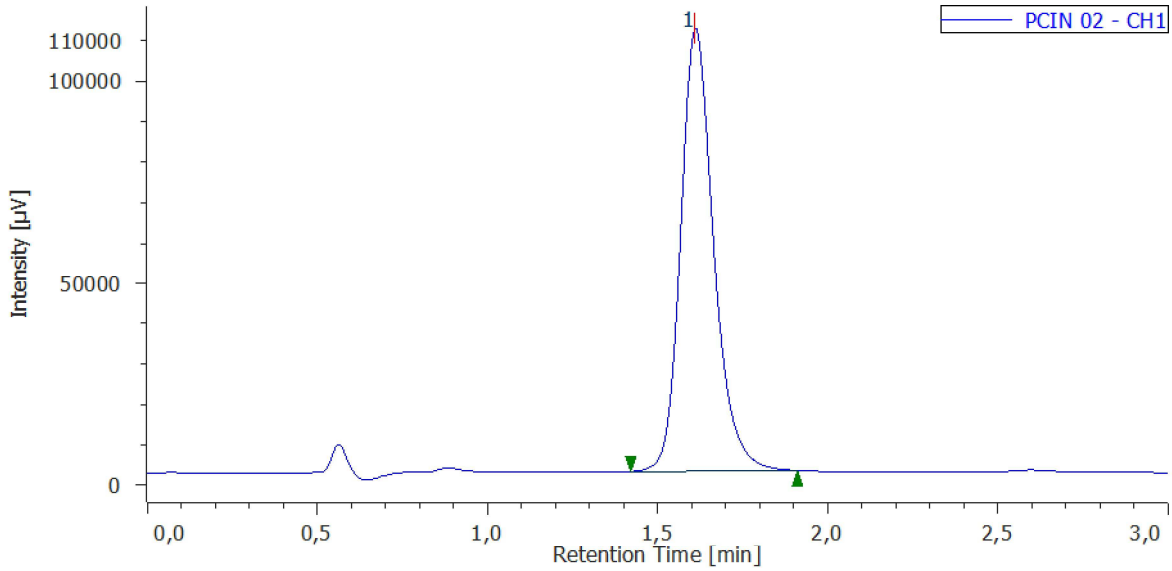


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 09:51:02
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:47:59
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,610	741049	109477	100,000	100,000	N/A	1410	N/A	1,244	

Chromatogram

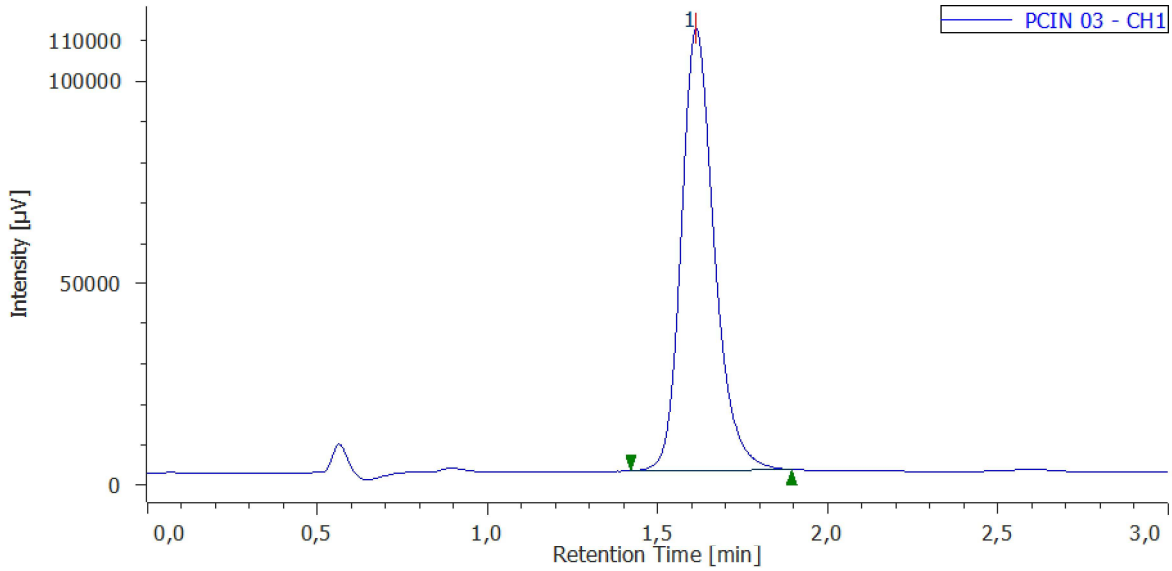


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 09:54:40
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:51:36
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,613	739459	109314	100,000	100,000	N/A	1415	N/A	1,225	

Chromatogram

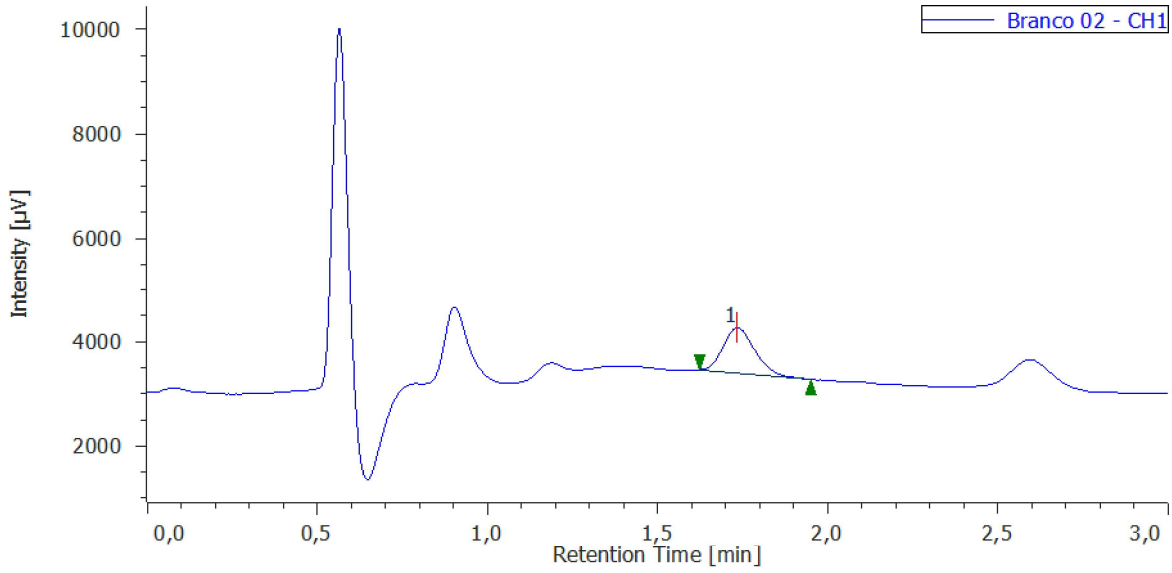


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:05:30
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:55:13
Volume	10,00 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,733	5685	877	100,000	100,000	N/A	1635	N/A	1,216	

Chromatogram

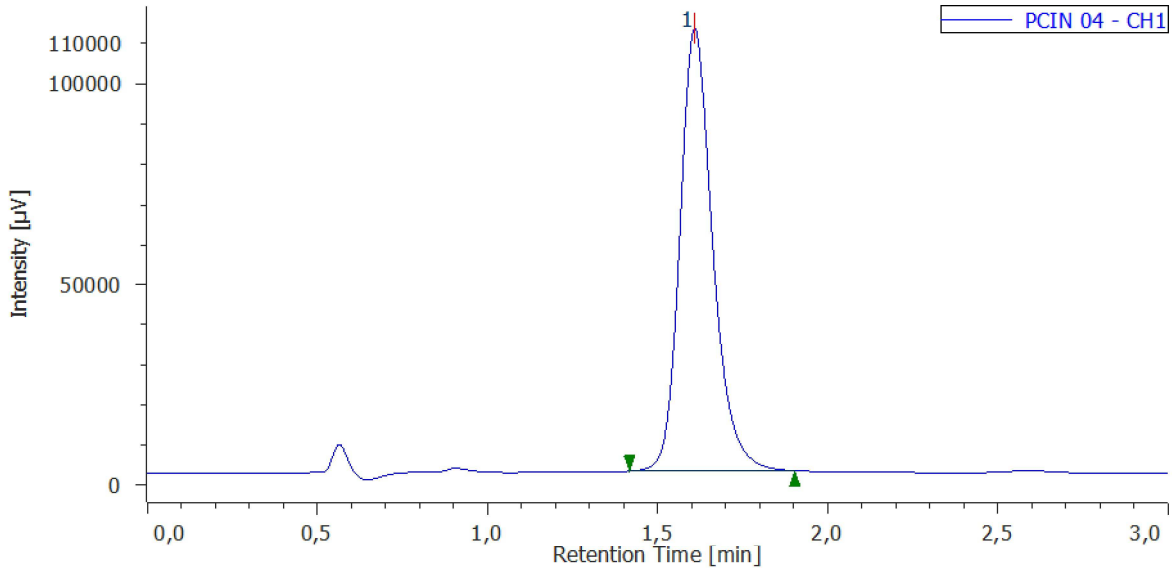


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:01:52
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 09:58:49
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,607	742736	110194	100,000	100,000	N/A	1416	N/A	1,256	

Chromatogram

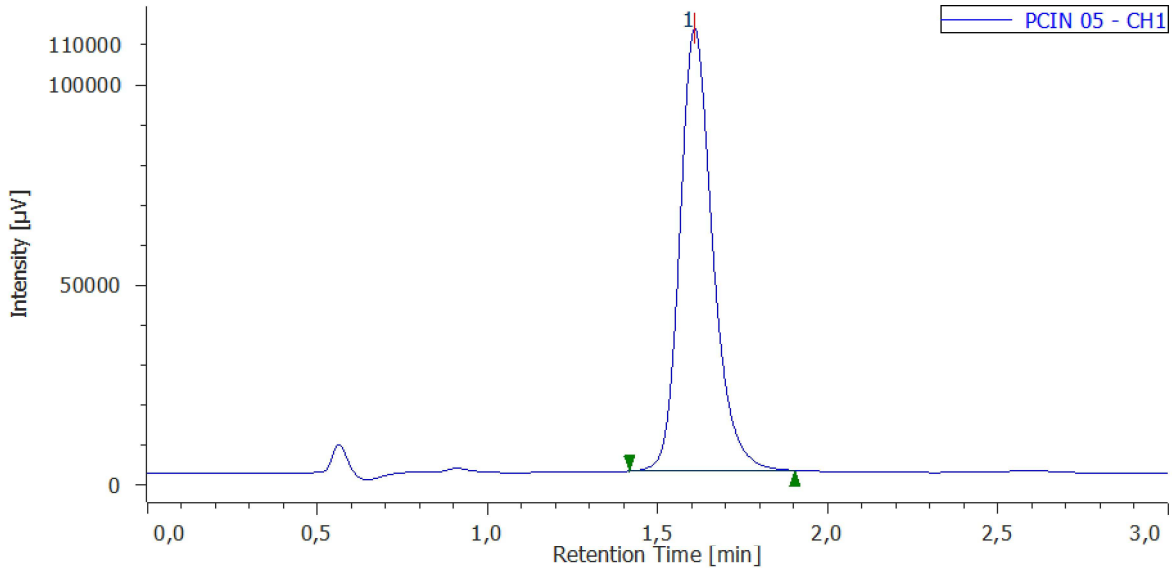


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:05:30
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:02:26
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,610	745446	110502	100,000	100,000	N/A	1418	N/A	1,212	

Chromatogram

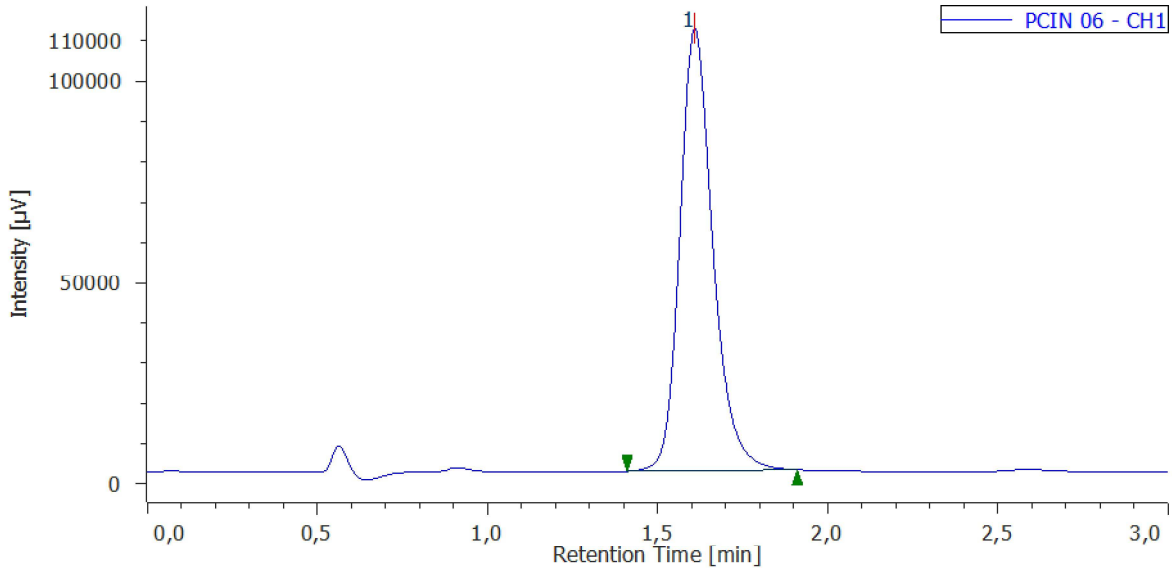


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:21:35
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:18:32
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,610	744297	109823	100,000	100,000	N/A	1416	N/A	1,219	

Chromatogram

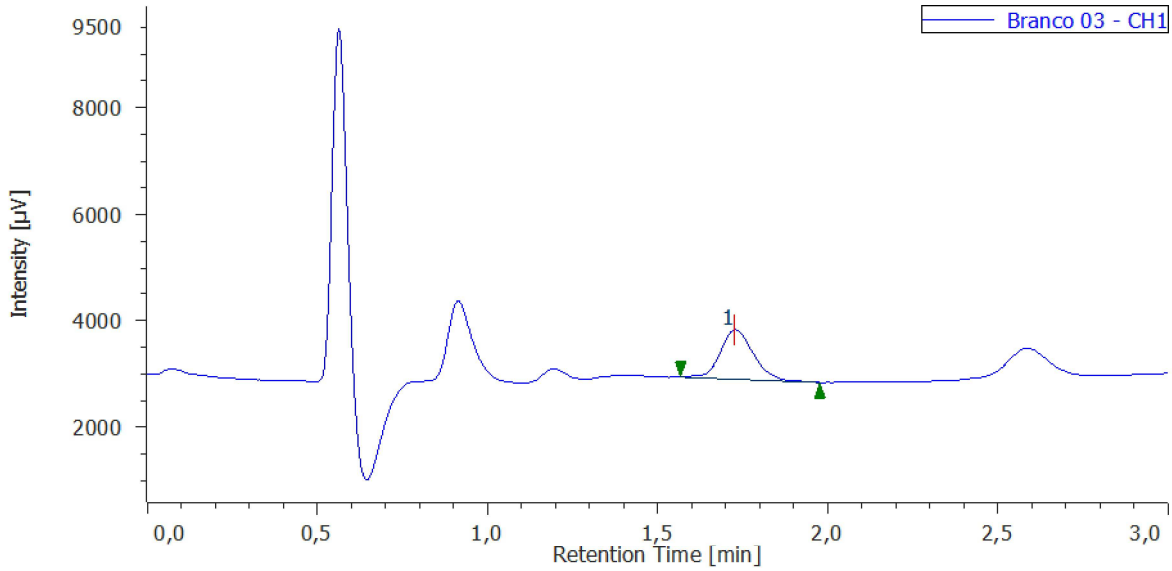


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:30:34
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:22:09
Volume	10,00 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,727	6302	929	100,000	100,000	N/A	1578	N/A	1,144	

Chromatogram

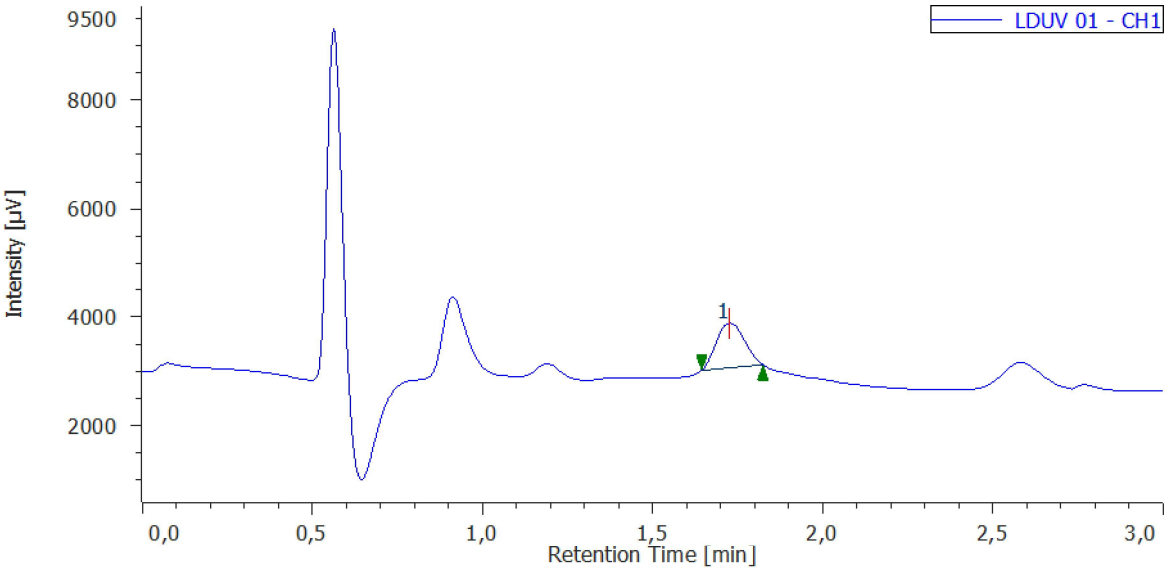


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 11:17:15
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:28:51
Volume	10,00 [µL]
Sample #	41
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,727	4709	819	100,000	100,000	N/A	1834	N/A	1,092	

Chromatogram

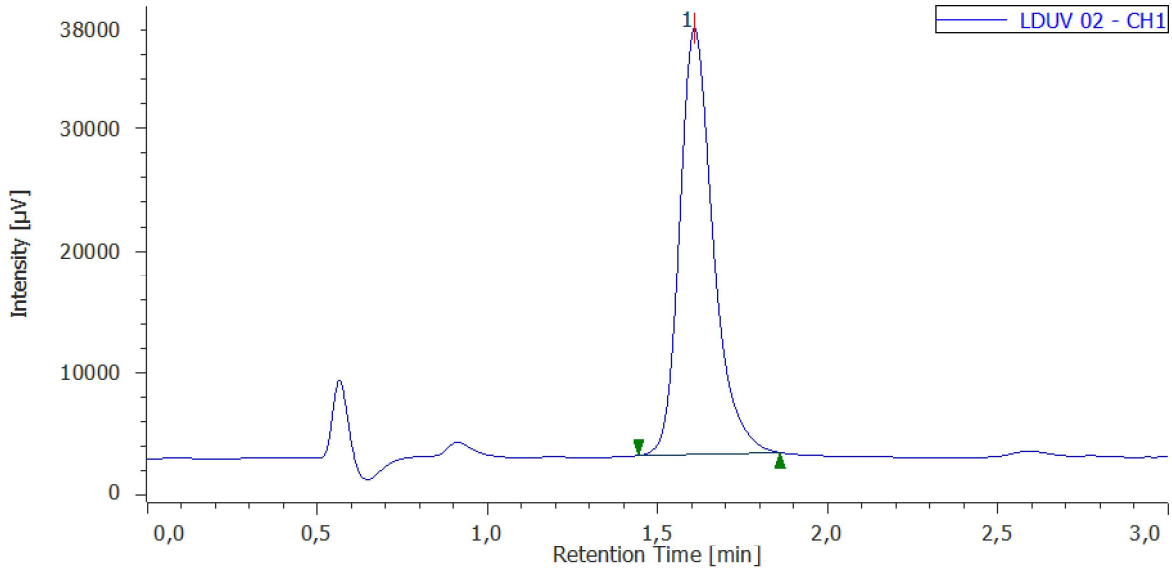


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:35:07
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:32:04
Volume	10,00 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,607	238906	34788	100,000	100,000	N/A	1378	N/A	1,314	

Chromatogram

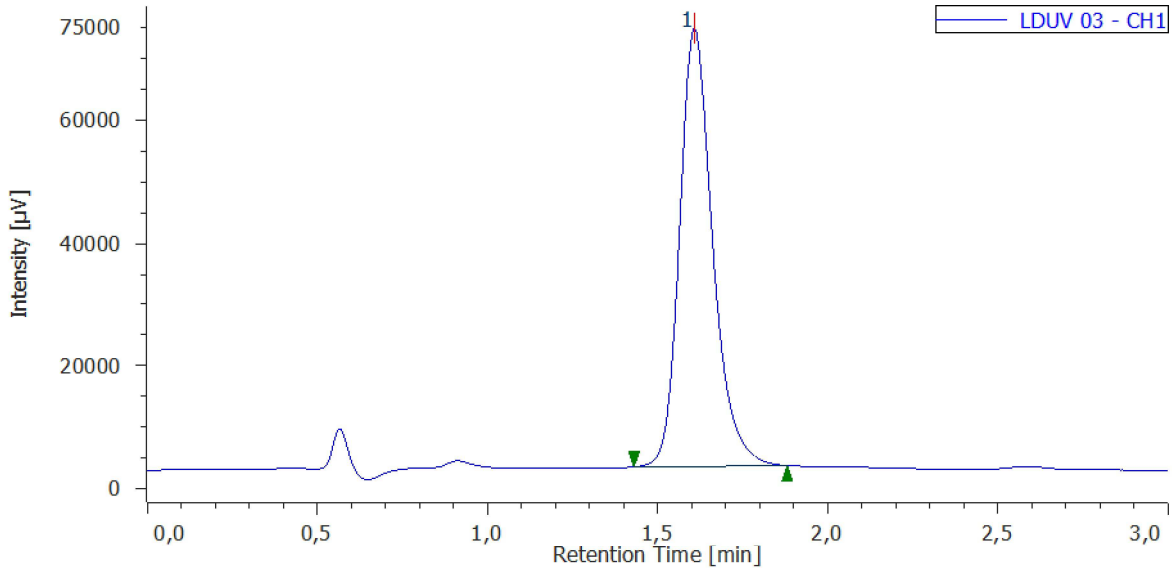


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:38:19
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:35:17
Volume	10,00 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,607	483097	71210	100,000	100,000	N/A	1388	N/A	1,264	

Chromatogram

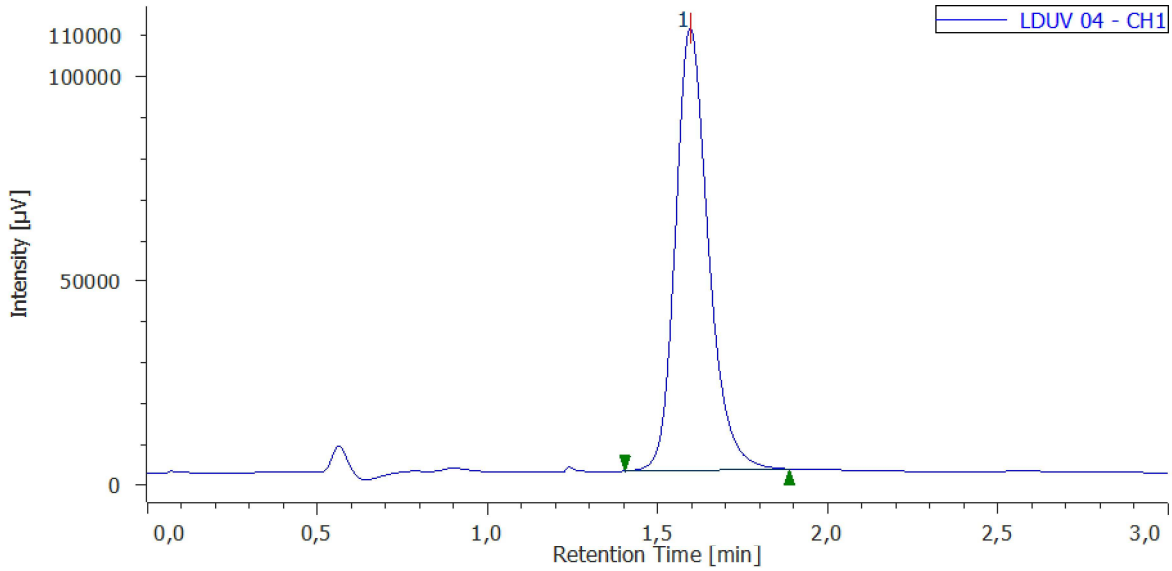


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:41:33
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:38:30
Volume	10,00 [µL]
Sample #	44
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,597	731583	108162	100,000	100,000	N/A	1378	N/A	1,215	

Chromatogram

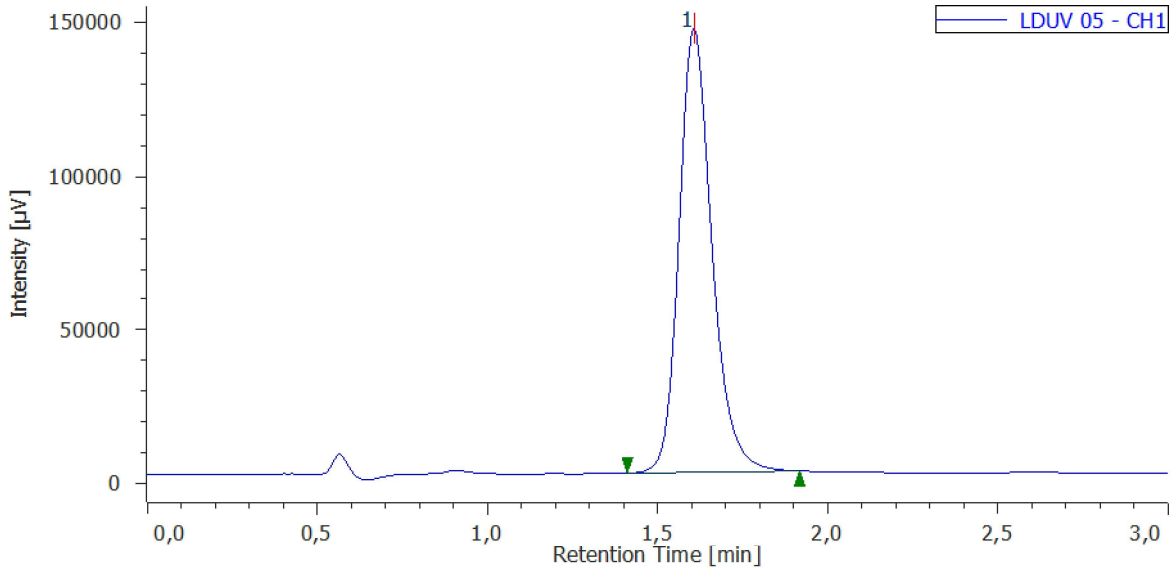


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:44:45
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:41:43
Volume	10,00 [µL]
Sample #	45
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,607	974190	144366	100,000	100,000	N/A	1409	N/A	1,223	

Chromatogram

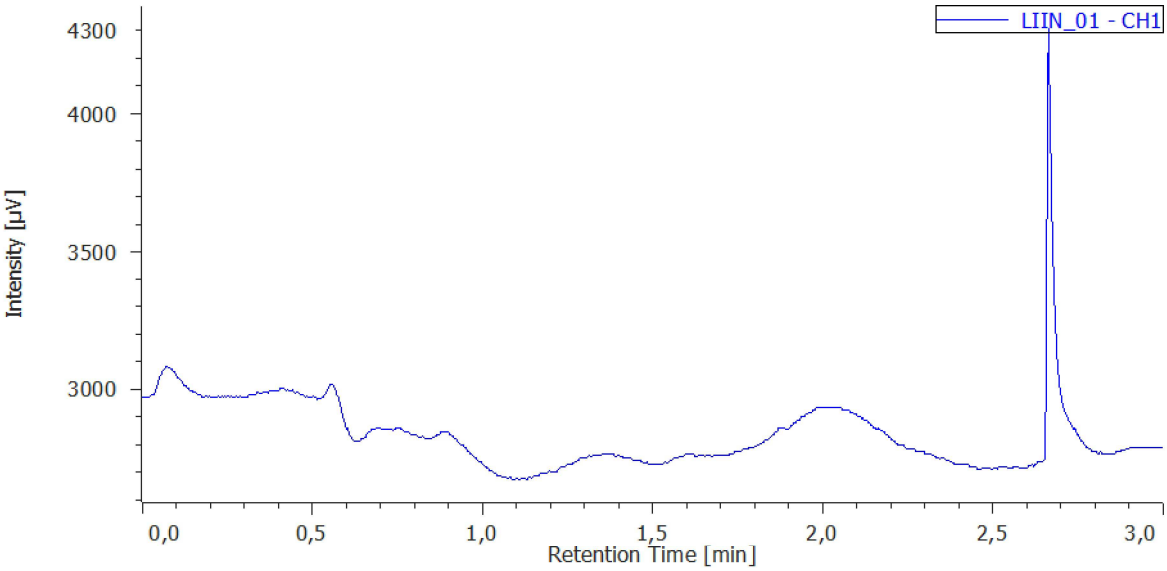


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:47:59
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:44:56
Volume	0,10 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

Chromatogram

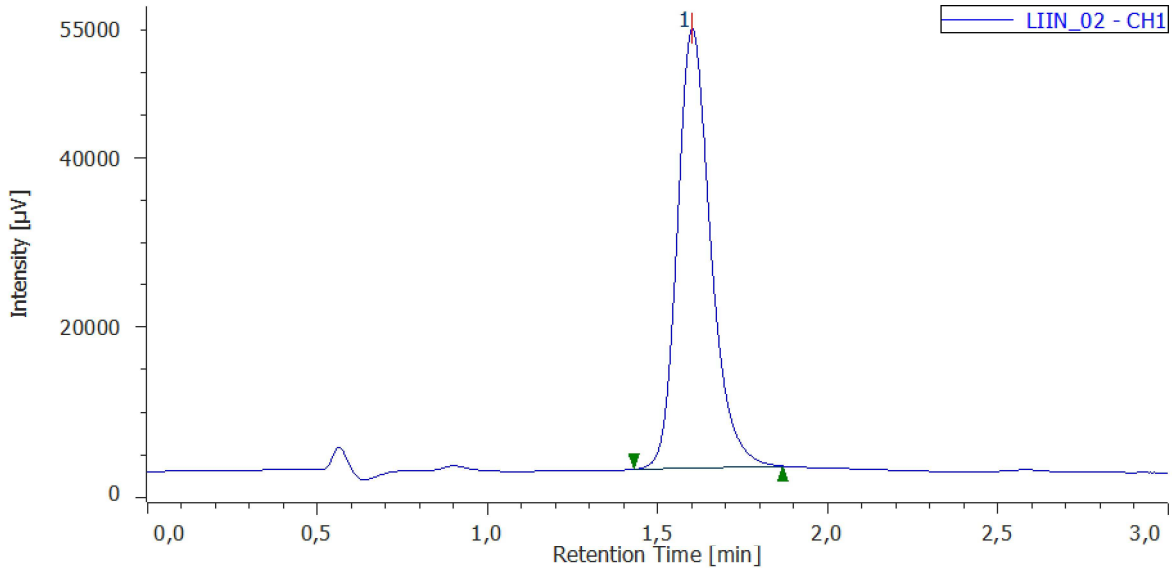


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:51:11
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:48:09
Volume	5,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,600	353929	51713	100,000	100,000	N/A	1351	N/A	1,262	

Chromatogram

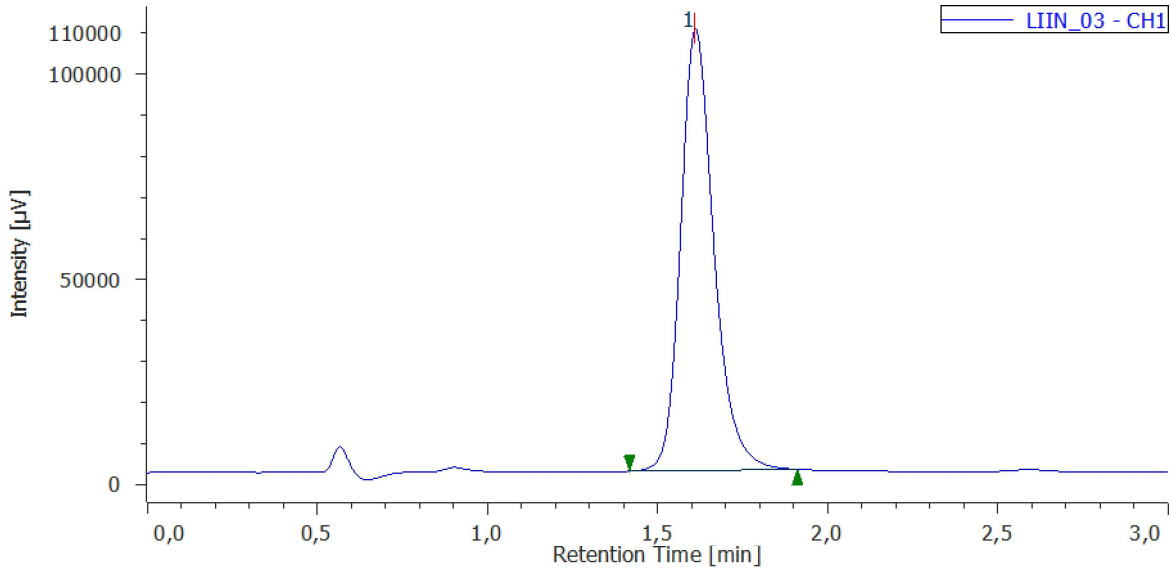


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:54:25
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:51:21
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,610	732789	107672	100,000	100,000	N/A	1391	N/A	1,257	

Chromatogram

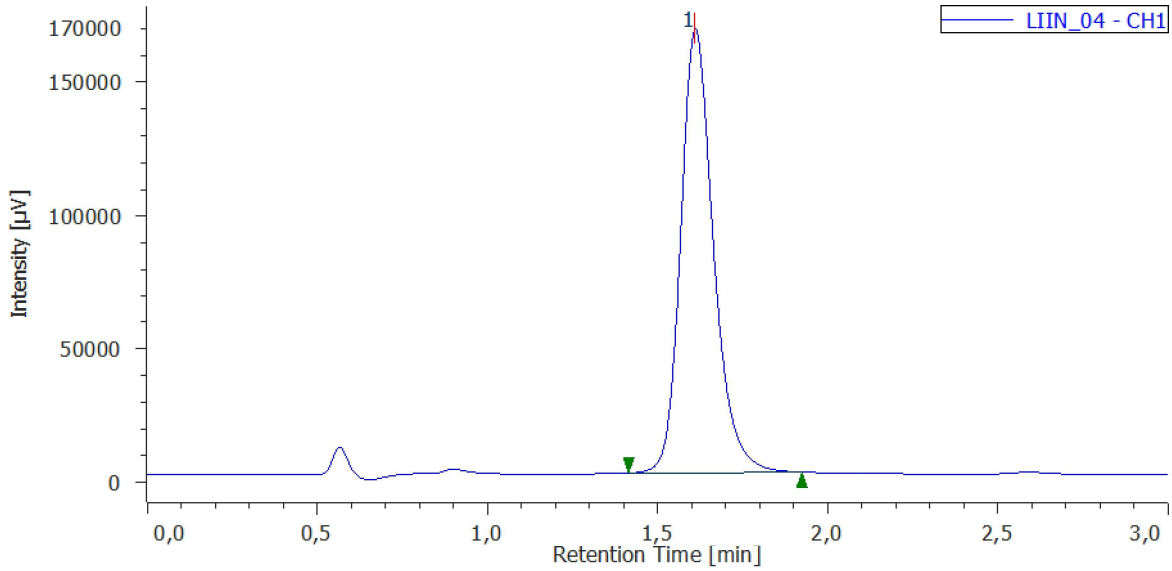


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 10:57:37
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:54:34
Volume	15,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,610	1119126	166387	100,000	100,000	N/A	1431	N/A	1,249	

Chromatogram

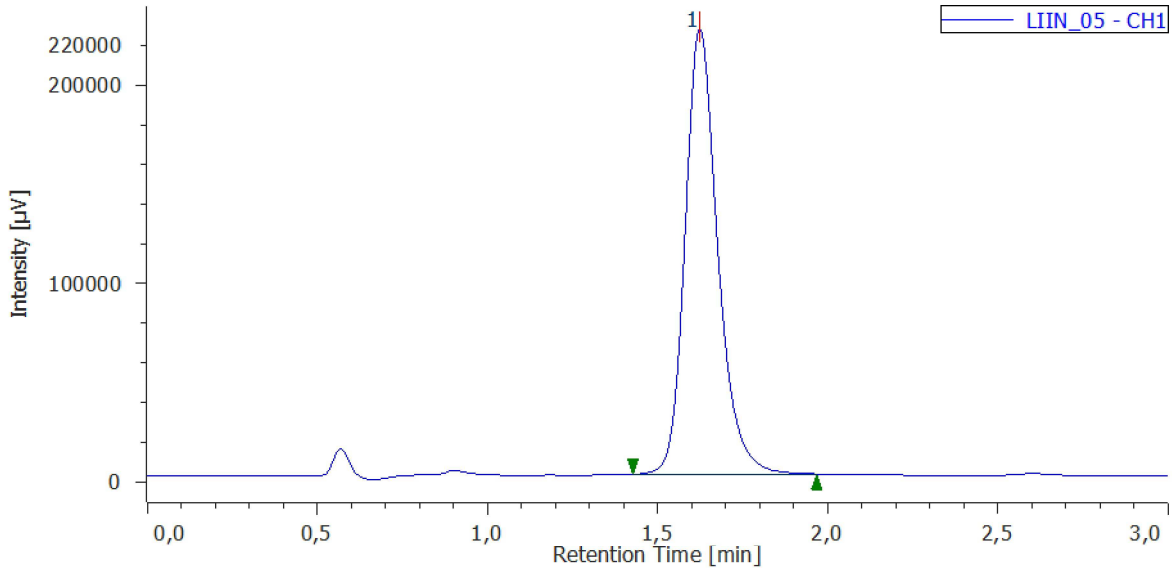


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 11:00:51
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 10:57:47
Volume	20,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDUV
Control Method	Qualificação Pd Cafeina
Peak ID Table	Identificação Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Integração Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	1	1,623	1503742	224568	100,000	100,000	N/A	1468	N/A	1,235	

Peak Find - Explo Pd Quinina_003 FPEm_tR0,44 D.jws

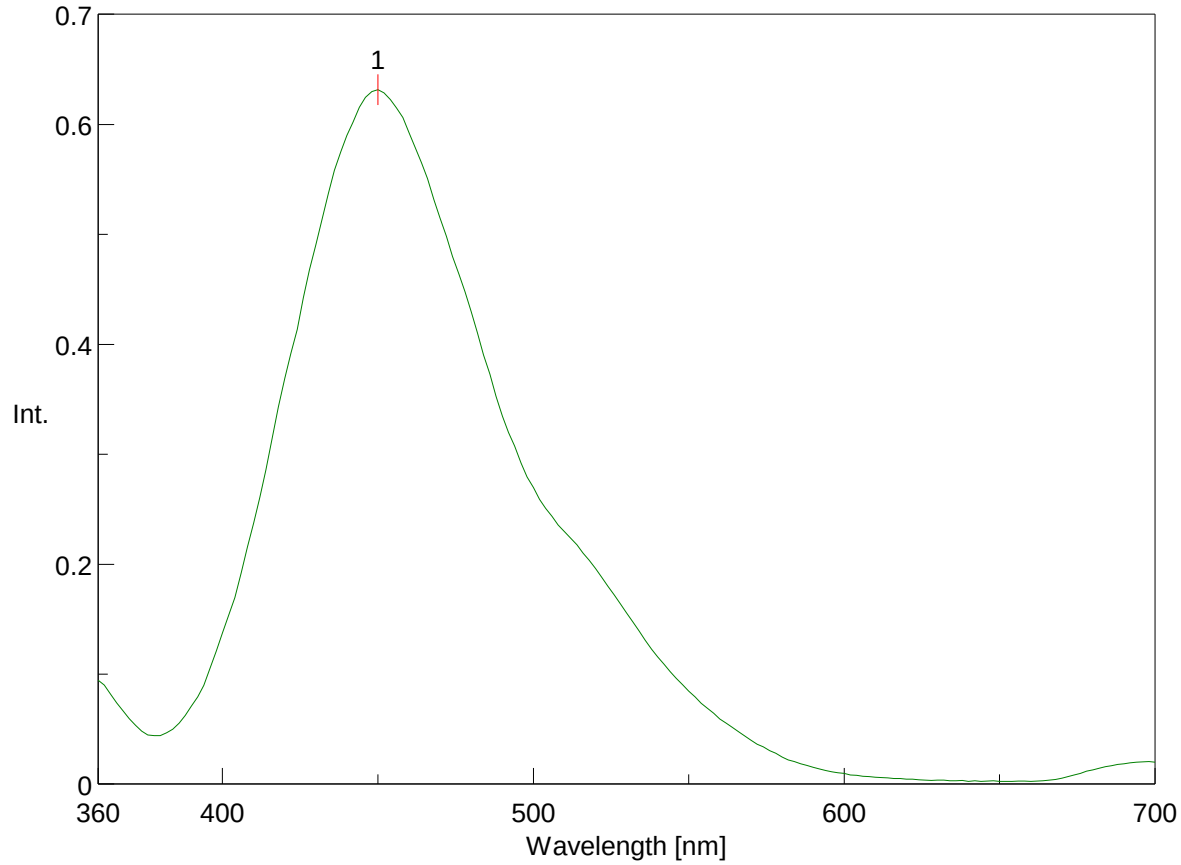

[Comments]

User	Administrator
Division	---
Company	Jasco do Brasil
Creation date	29/03/2016 13:29

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171


[Measurement Information]

Instrument Name	FP-1520
Model Name	FP-1520
Serial No.	869
ROM version	V1.35
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	0.631241			

Chromatogram

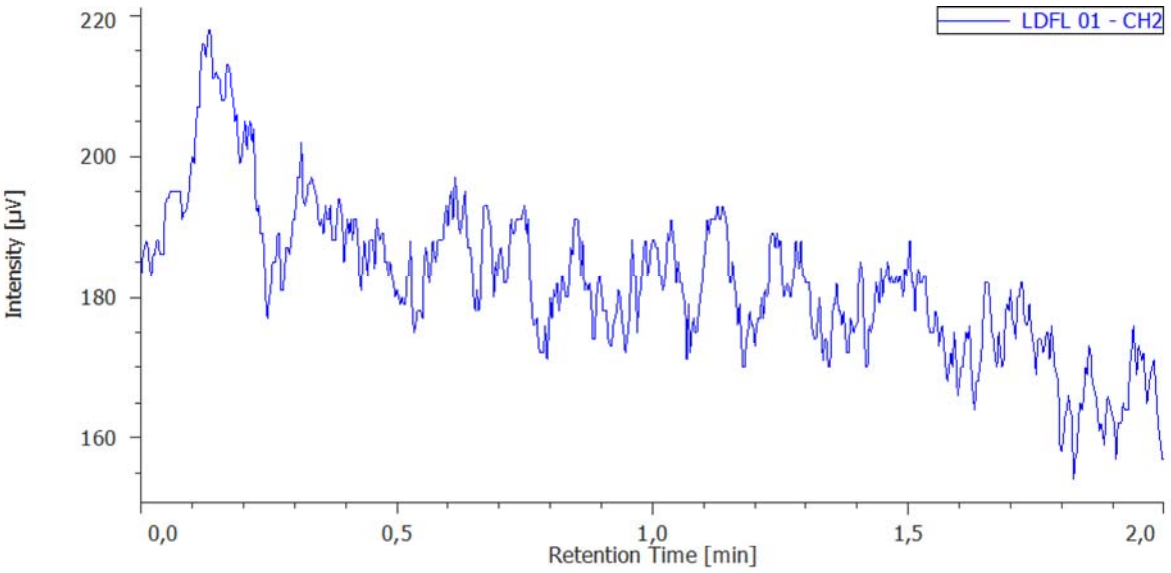


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 15:14:51
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 14:41:08
Volume	10,00 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDFL
Control Method	Qualificação Pd Quinina
Peak ID Table	Identificação Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 01-CH2
Sample Name	
Channel Name	FL
Sampling Interval	200 [msec]
Peak Method	Integração Quinina

Chromatogram

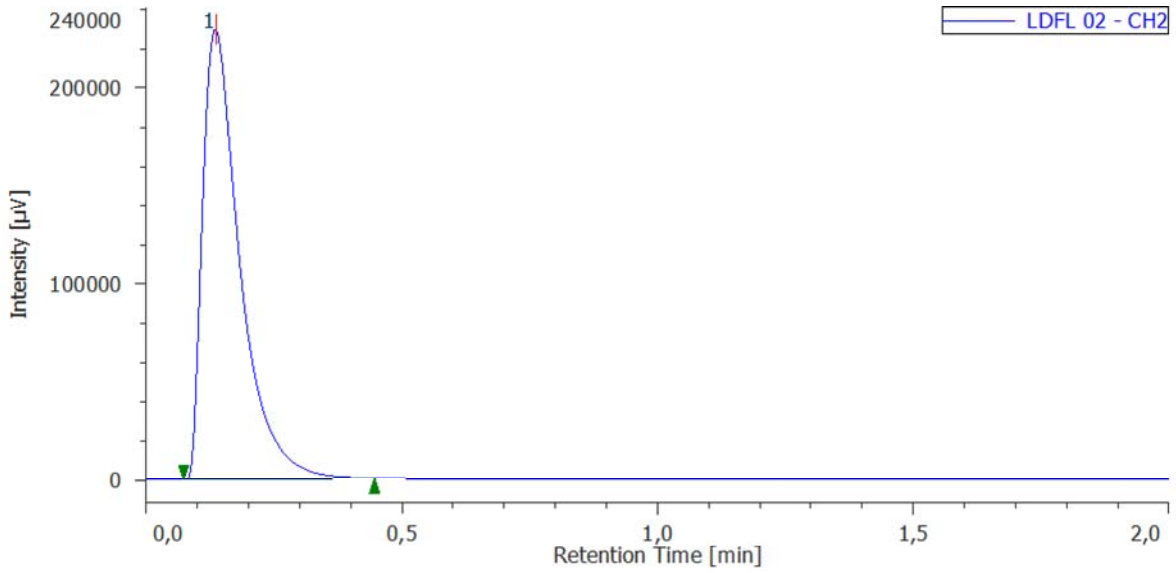


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 15:14:51
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 14:43:27
Volume	10,00 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 – LDFL
Control Method	Qualificação Pd Quinina
Peak ID Table	Identificação Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 02-CH2
Sample Name	
Channel Name	FL
Sampling Interval	200 [msec]
Peak Method	Integração Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Pd Quinina	2	0,137	1164054	229460	100,000	100,000	N/A	19	N/A	1,977	

Chromatogram

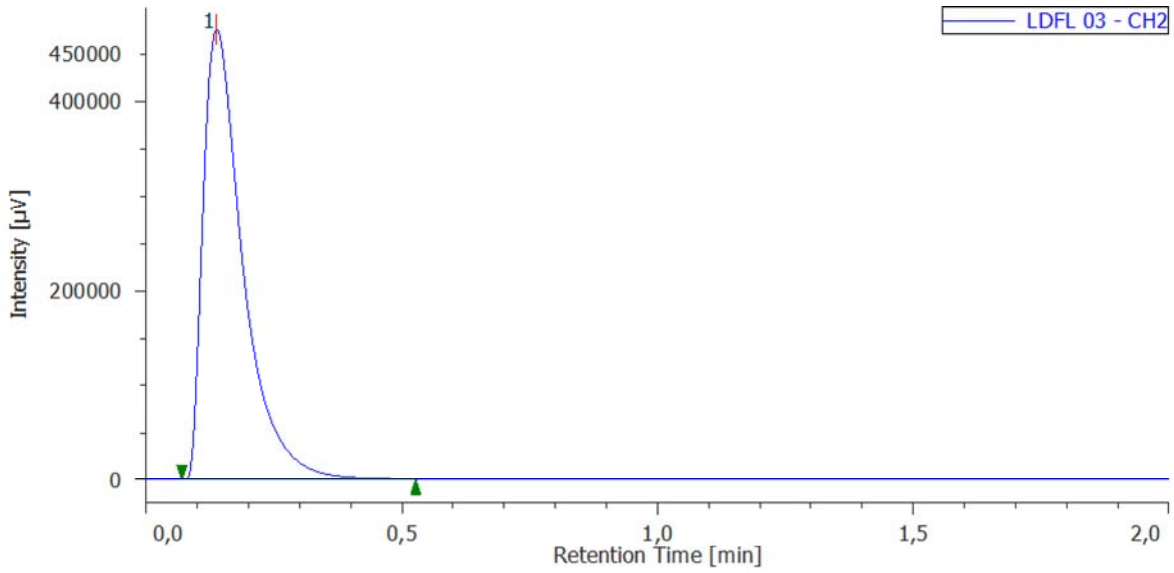


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 15:14:51
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 14:45:49
Volume	10,00 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 - LDFL
Control Method	Qualificação Pd Quinina
Peak ID Table	Identificação Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 03-CH2
Sample Name	
Channel Name	FL
Sampling Interval	200 [msec]
Peak Method	Integração Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Pd Quinina	2	0,137	2576186	475413	100,000	100,000	N/A	17	N/A	2,085	

Chromatogram

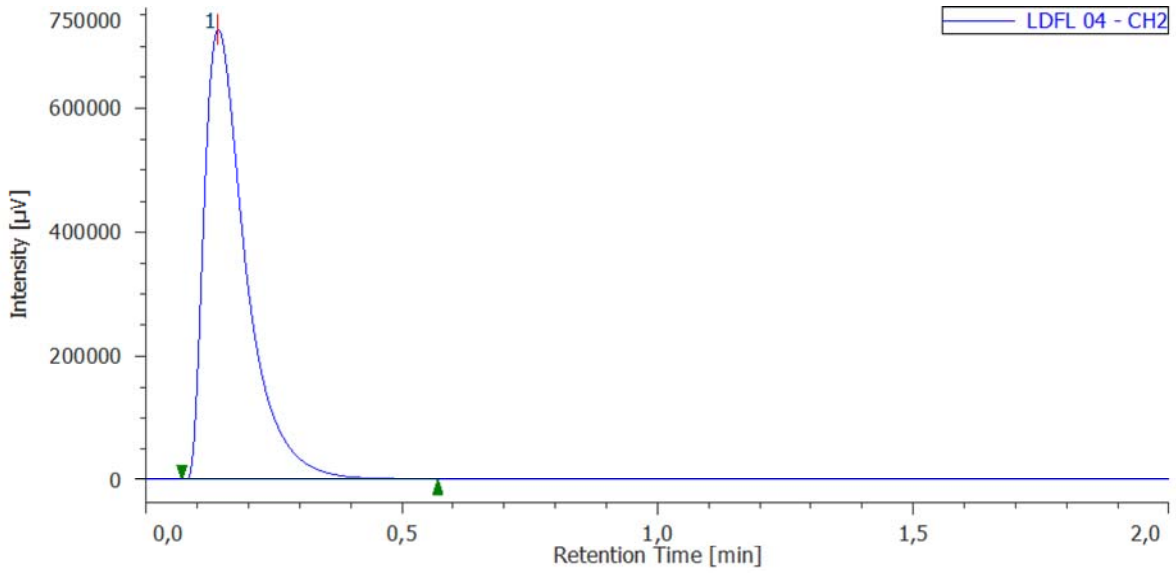


Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 15:14:51
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 14:48:12
Volume	10,00 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 - LDFL
Control Method	Qualificação Pd Quinina
Peak ID Table	Identificação Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 04-CH2
Sample Name	
Channel Name	FL
Sampling Interval	200 [msec]
Peak Method	Integração Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Pd Quinina	2	0,140	4110769	726286	100,000	100,000	N/A	16	N/A	2,085	

Chromatogram

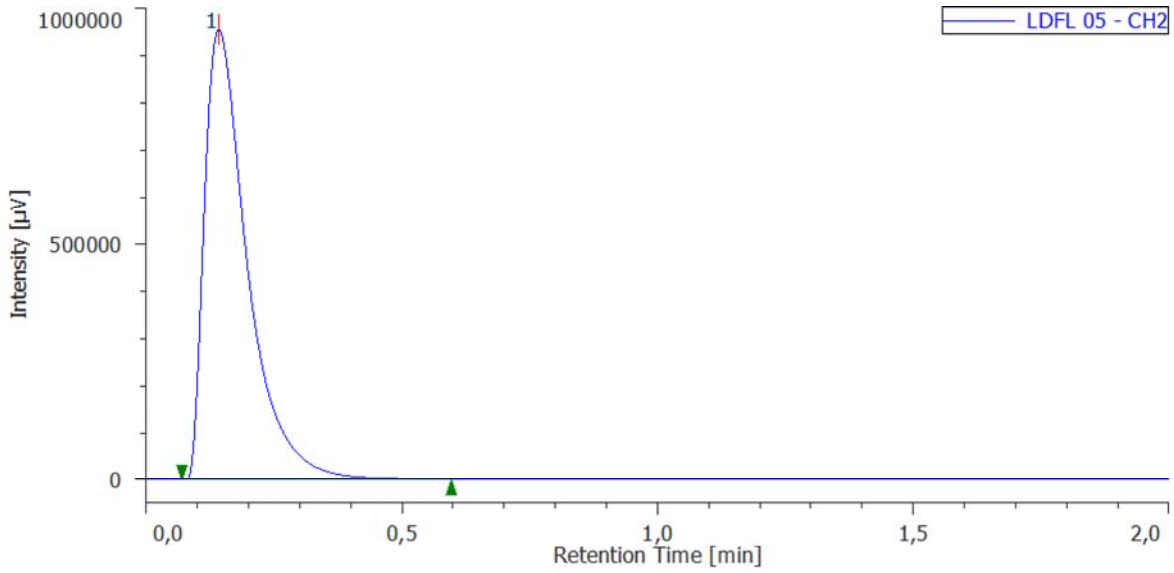

Chromatogram Information	
User Name	Administrator
Date Modified	29/03/2016 15:14:52
Description	
HPLC System Name	HPLC
Injection Date	29/03/2016 14:50:37
Volume	10,00 [µL]
Sample #	50
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 5CQ1HP 01 - LDFL
Control Method	Qualificação Pd Quinina
Peak ID Table	Identificação Quinina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDFL 05-CH2
Sample Name	
Channel Name	FL
Sampling Interval	200 [msec]
Peak Method	Integração Quinina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Pd Quinina	2	0,143	5582292	955608	100,000	100,000	N/A	16	N/A	2,016	