
Peak Find - EDUV.jws

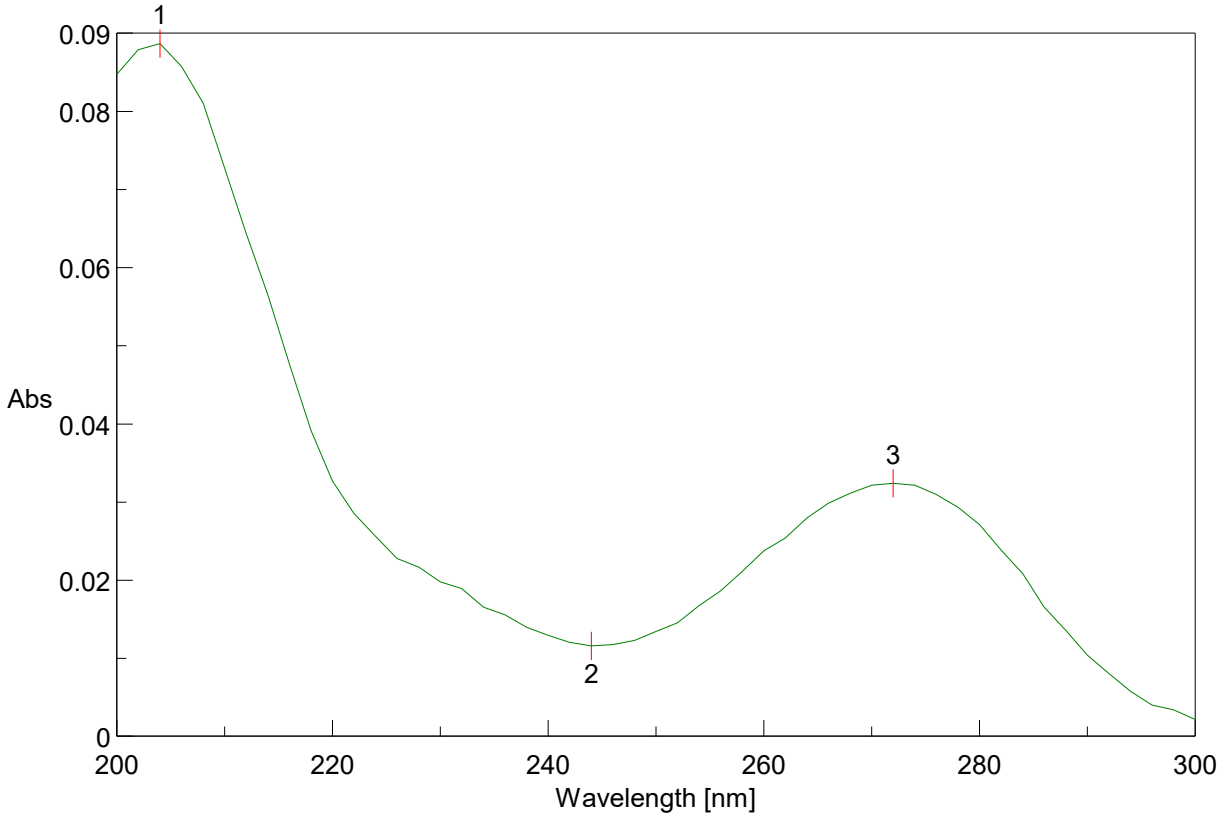

[Comments]

User	QPackSA
Division	---
Company	MULTICARE
Creation date	25/05/2022 14:07

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	85


[Measurement Information]

Instrument Name	UV-2070
Model Name	UV-2070
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	204	0.088639	2	244	0.0115415
3	272	0.032362			

Chromatogram

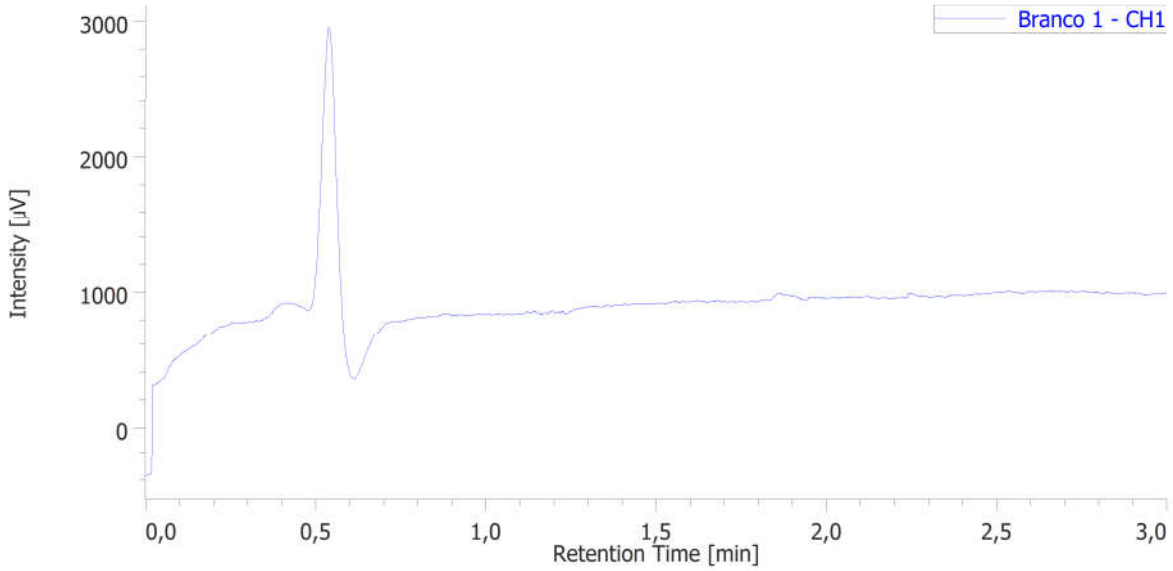


Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:21
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:21:49
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

Chromatogram

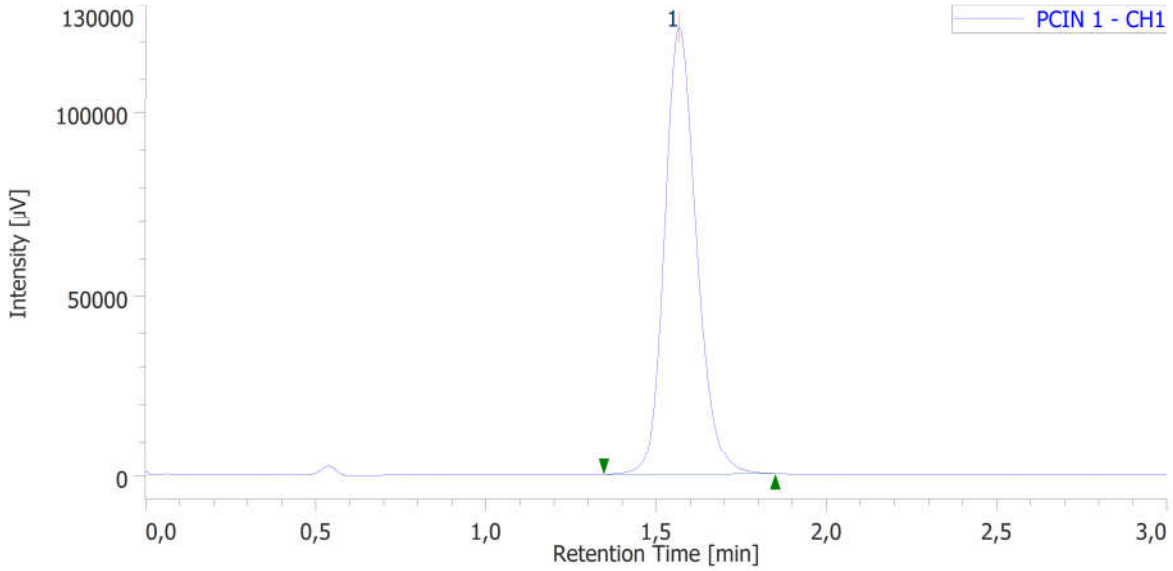

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:23
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:25:01
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,568	806917	123321	100,000	100,000	N/A	1395	N/A	1,181	

Creator QPackSA

Chromatogram

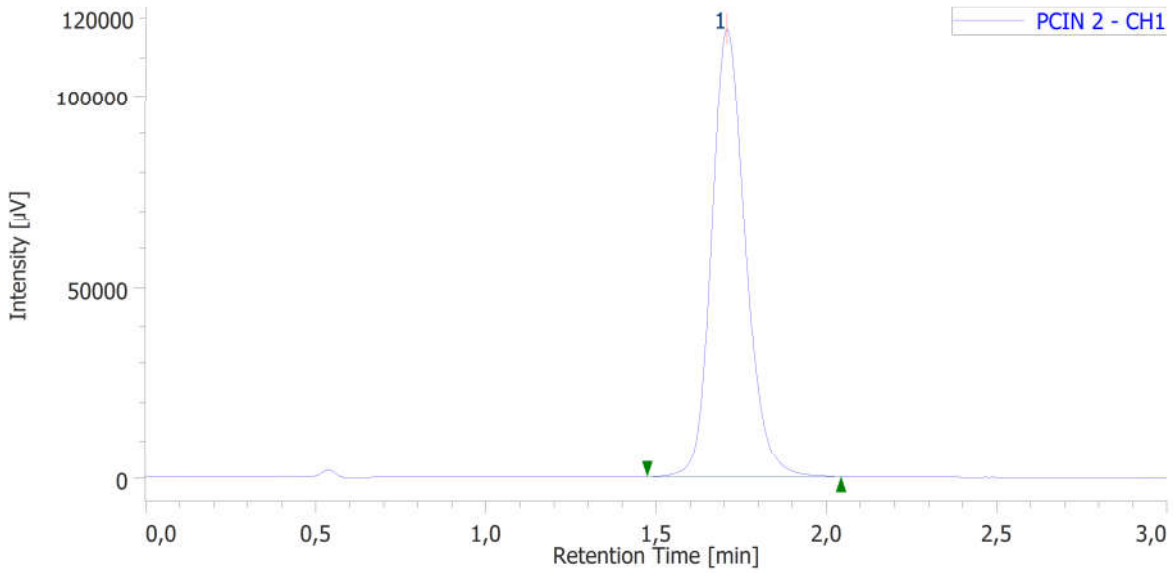

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:23
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:28:14
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,708	809217	116893	100,000	100,000	N/A	1492	N/A	1,187	

Creator QPackSA

Chromatogram

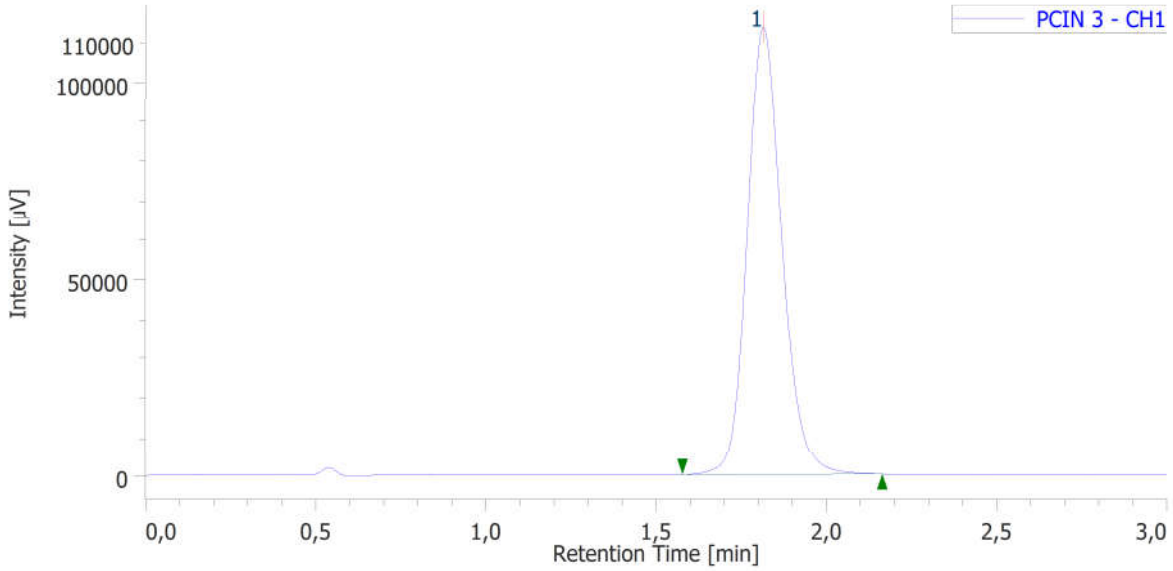

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:23
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:31:26
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,815	809043	113485	100,000	100,000	N/A	1590	N/A	1,167	

Creator QPackSA

Chromatogram

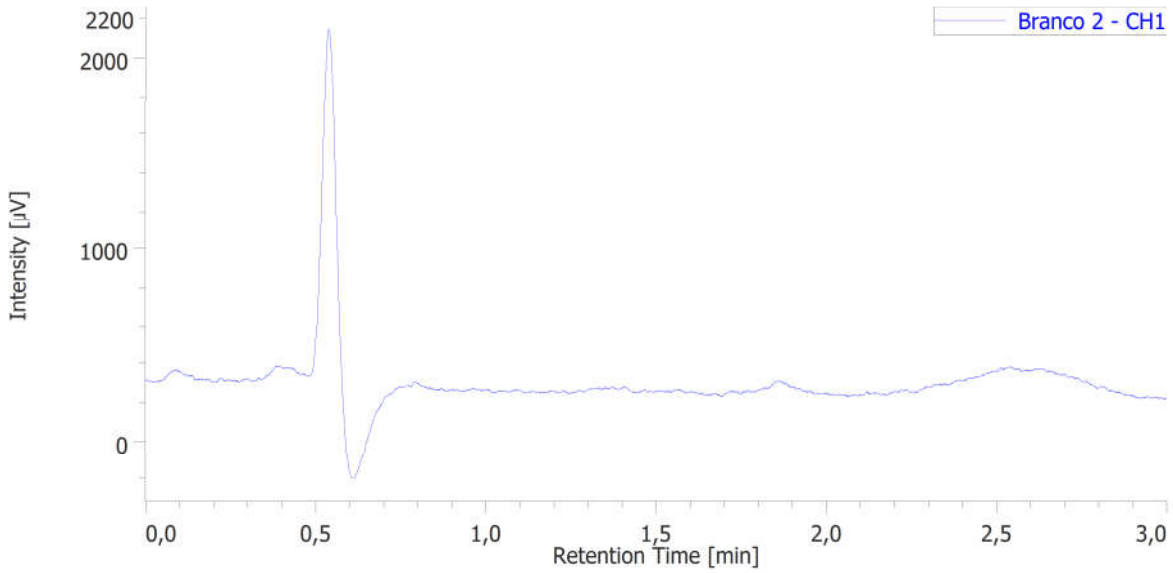


Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:24
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:34:39
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

Creator QPackSA

Chromatogram

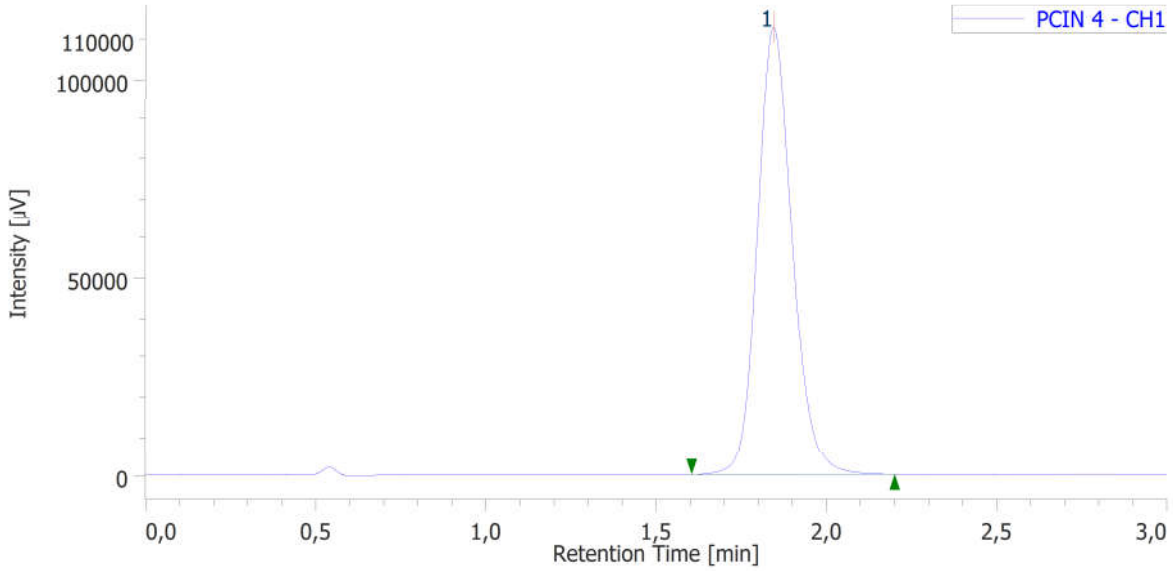

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:24
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:37:51
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,845	803976	112604	100,000	100,000	N/A	1629	N/A	1,168	

Creator QPackSA

Chromatogram

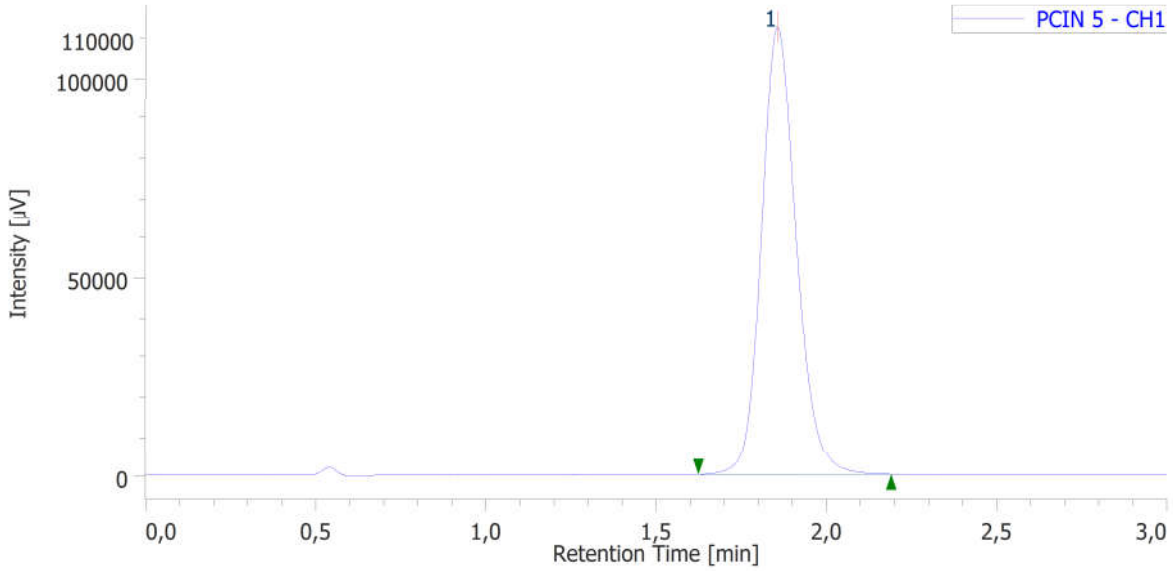

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:25
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:41:04
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,857	802371	112253	100,000	100,000	N/A	1654	N/A	1,165	

Creator QPackSA

Chromatogram

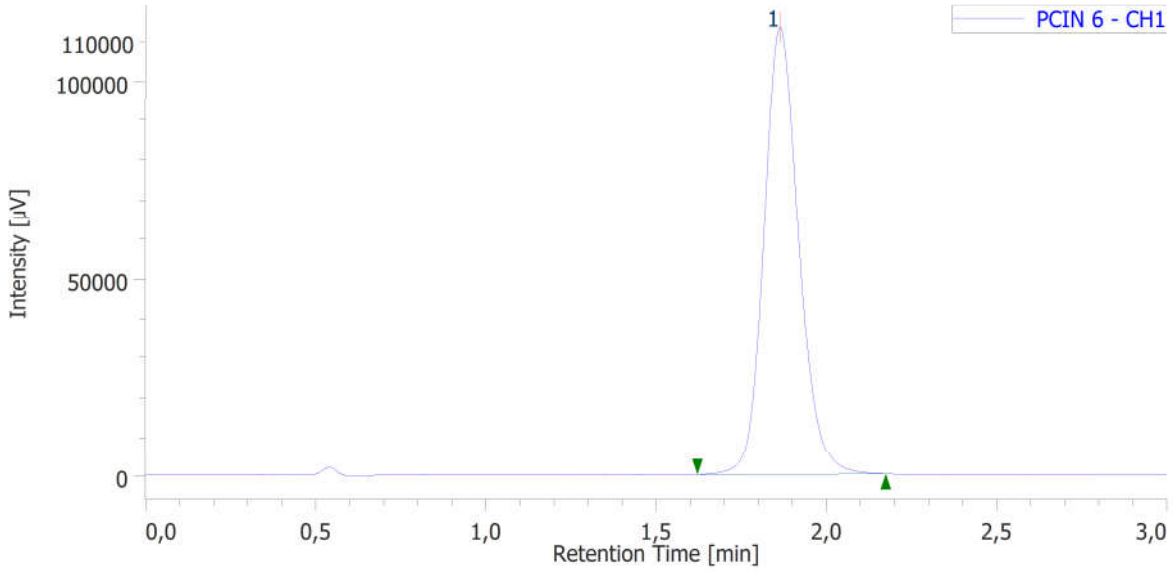

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:25
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:44:16
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,864	806679	112992	100,000	100,000	N/A	1671	N/A	1,162	

Creator QPackSA

Chromatogram

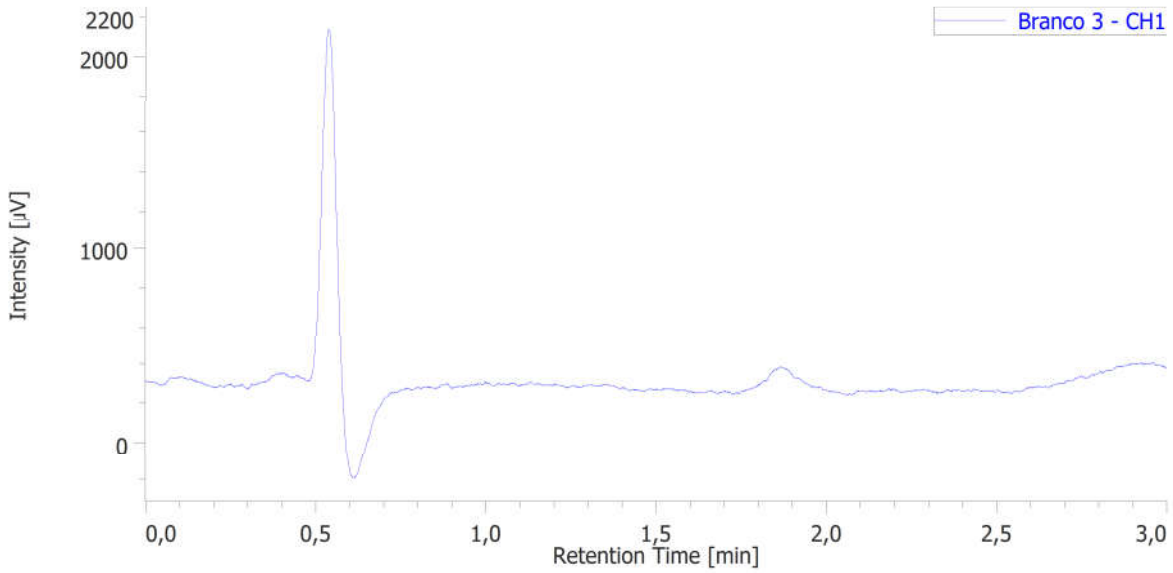


Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 14:56:26
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 14:47:29
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

Creator QPackSA

Chromatogram

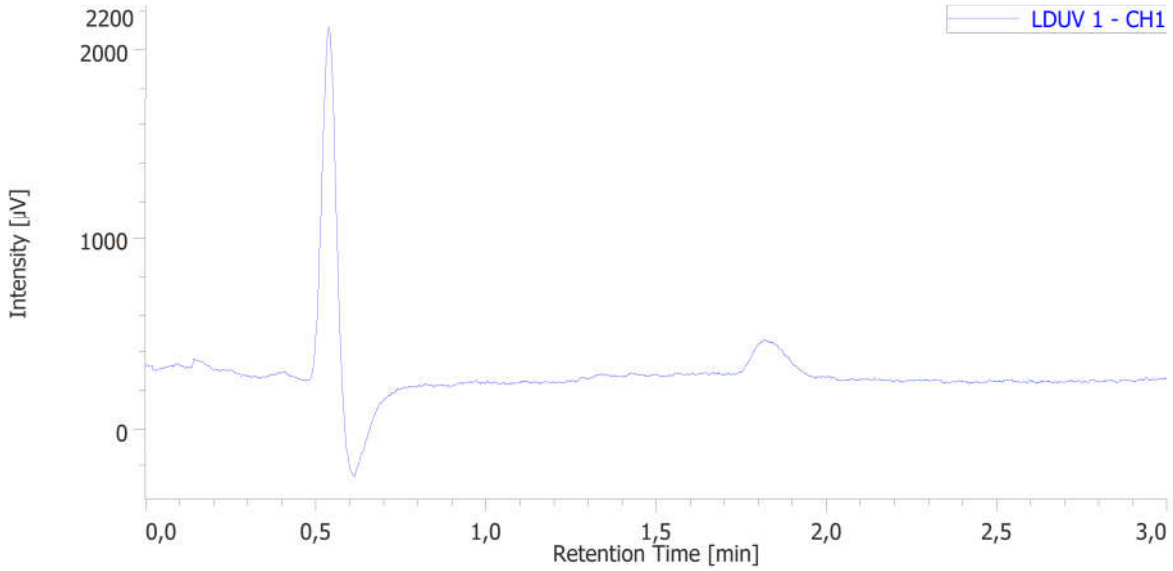


Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:18:08
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:15:05
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

Creator QPackSA

Chromatogram

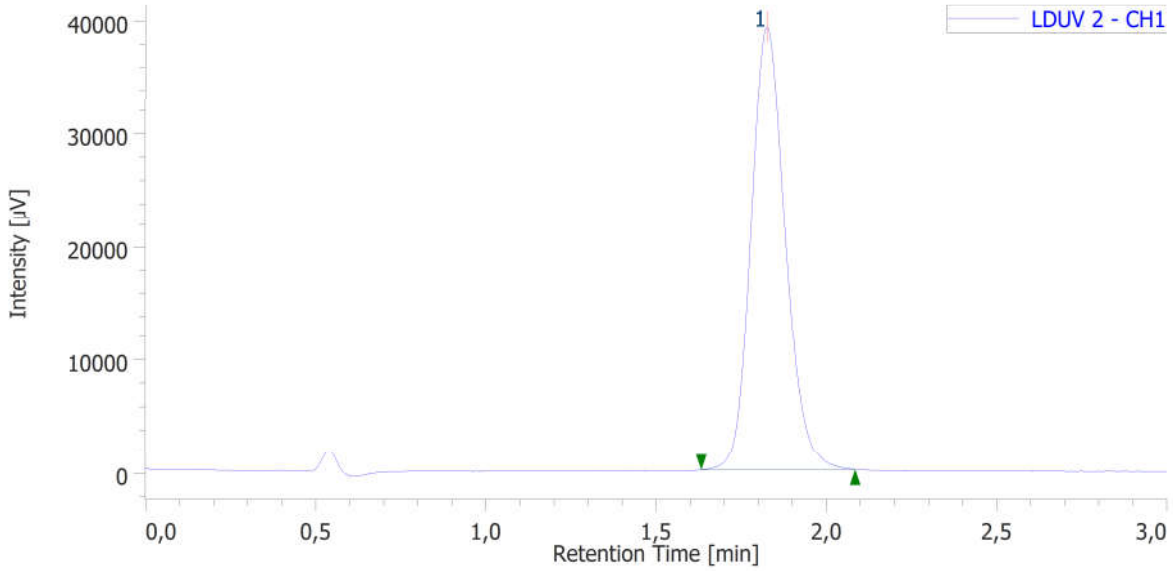

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:21:20
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:18:17
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,825	275358	39176	100,000	100,000	N/A	1618	N/A	1,166	

Creator QPackSA

Chromatogram

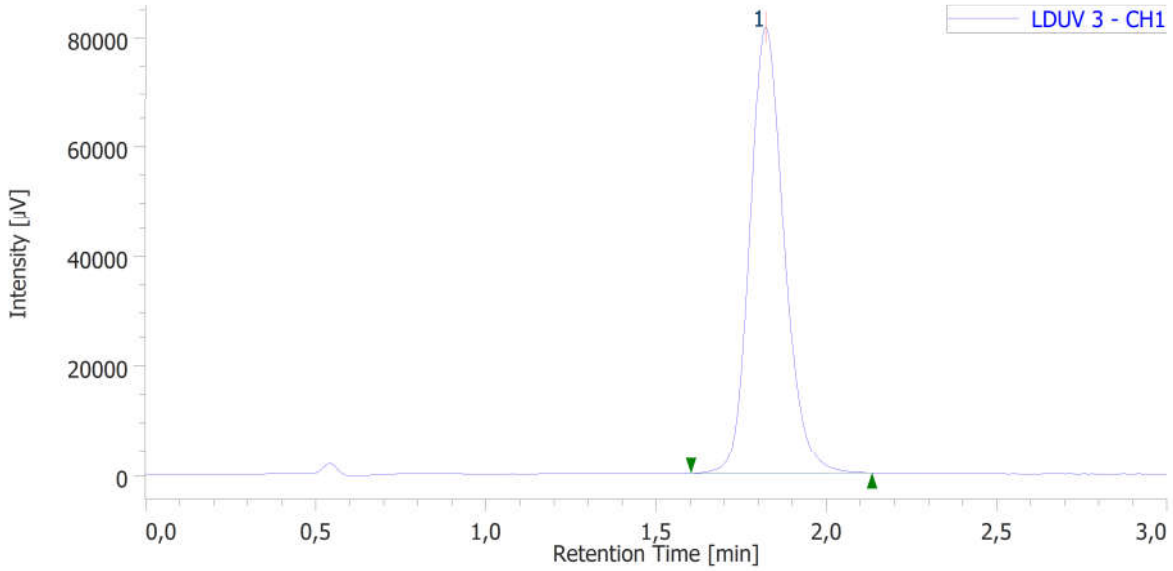

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:24:32
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:21:30
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,822	572409	81433	100,000	100,000	N/A	1634	N/A	1,169	

Creator QPackSA

Chromatogram

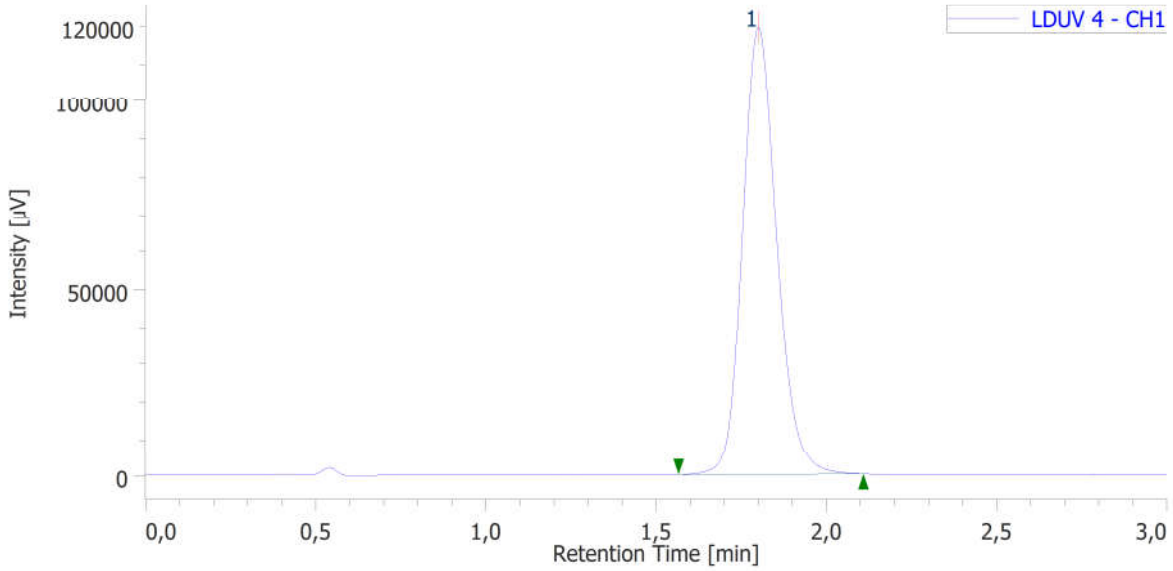

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:27:44
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:24:43
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,800	836807	119340	100,000	100,000	N/A	1604	N/A	1,177	

Creator QPackSA

Chromatogram

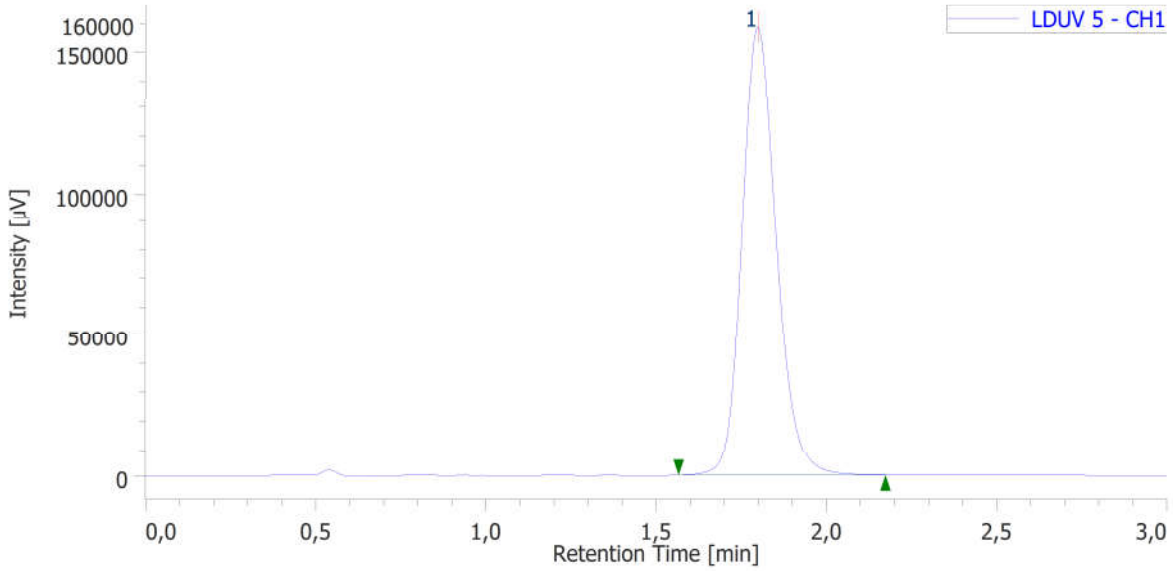

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:30:58
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:27:55
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,799	1113362	158155	100,000	100,000	N/A	1594	N/A	1,174	

Creator QPackSA

Chromatogram

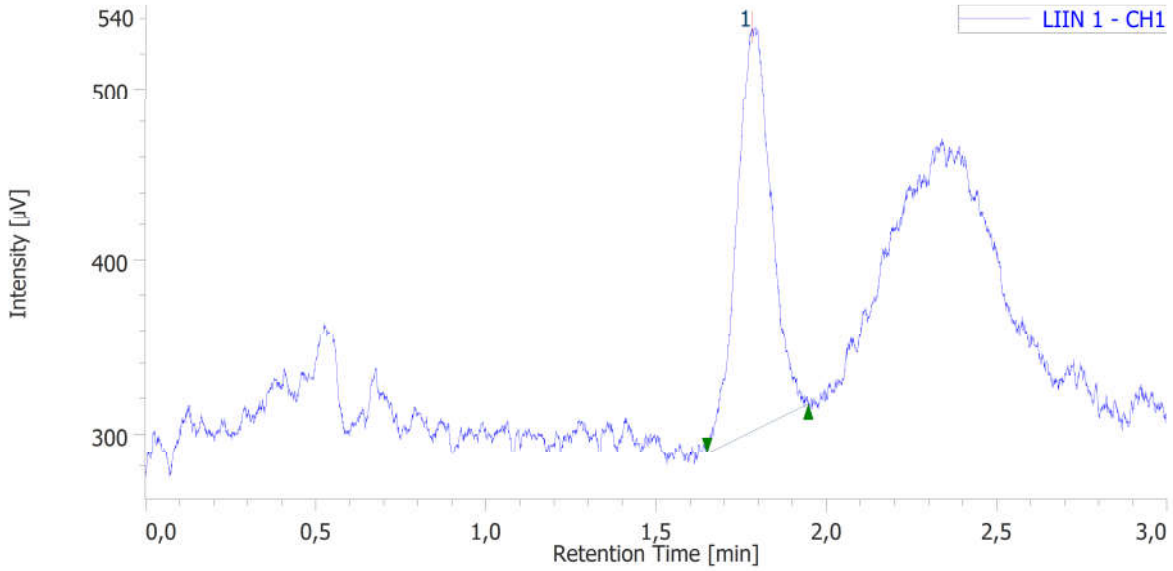

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:37:28
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:34:26
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,782	1639	234	100,000	100,000	N/A	1470	N/A	1,069	

Creator

Chromatogram

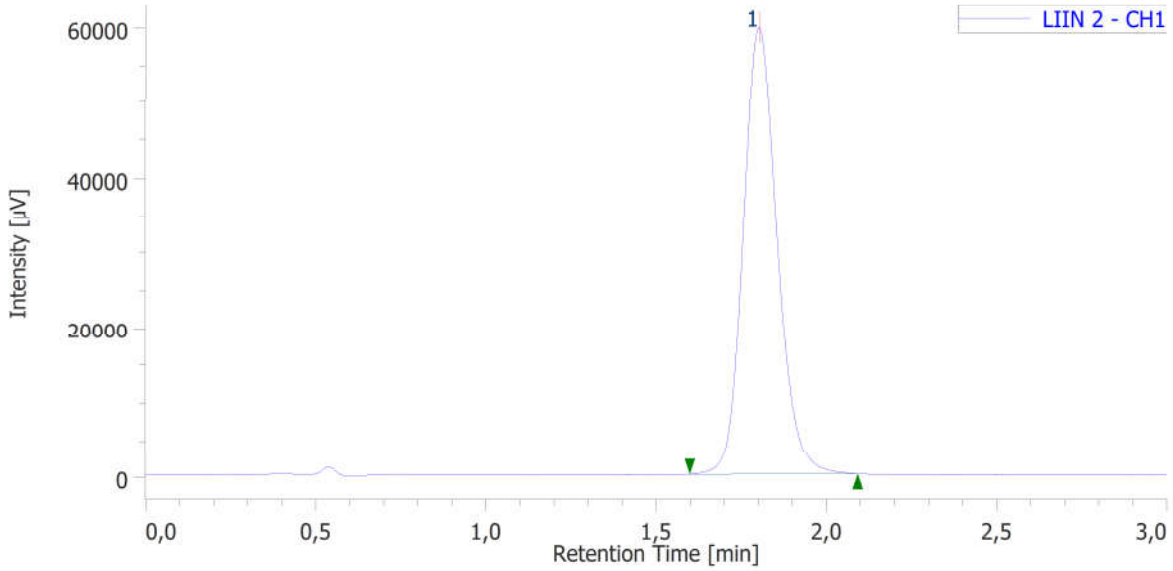

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:40:40
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:37:38
Volume	5,00 [μL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,803	413814	59638	100,000	100,000	N/A	1634	N/A	1,155	

Creator QPackSA

Chromatogram

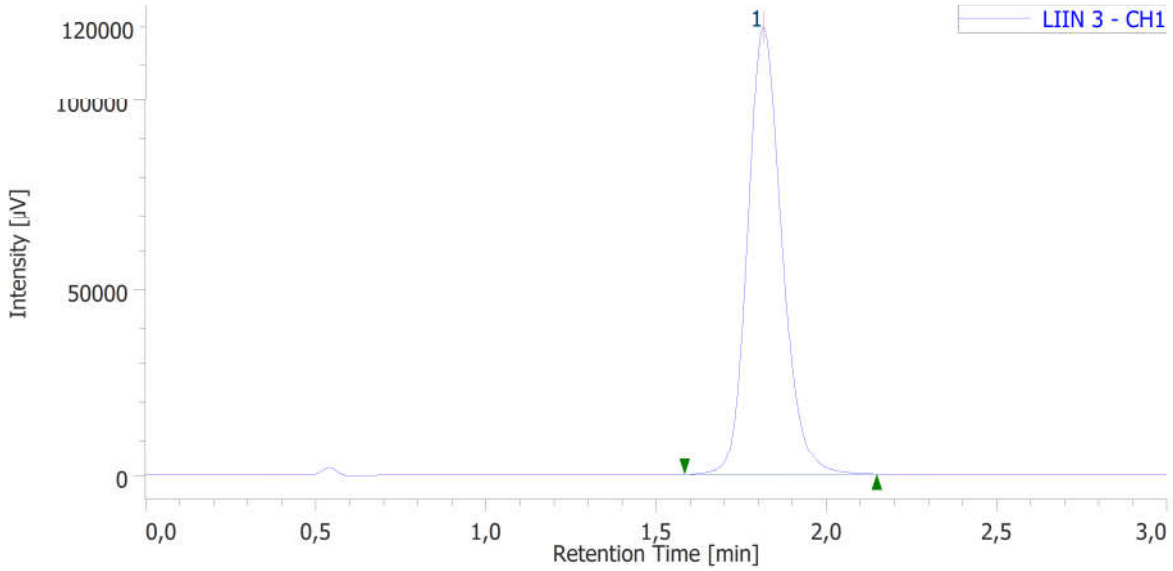

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:43:52
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:40:51
Volume	10,00 [μL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,815	837938	119487	100,000	100,000	N/A	1633	N/A	1,174	

Creator QPackSA

Chromatogram

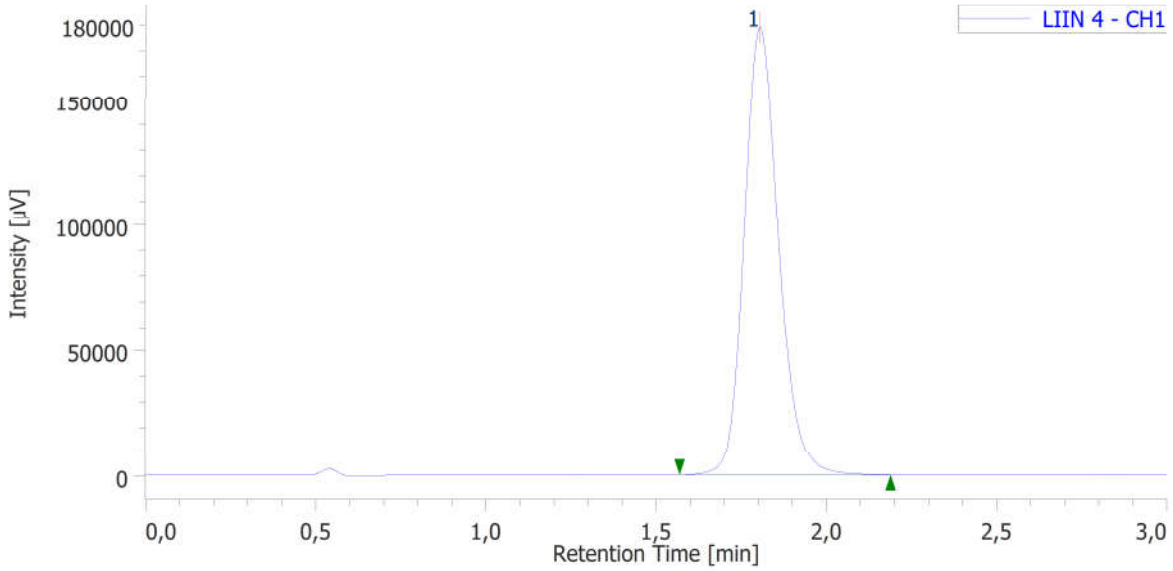

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:47:06
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:44:03
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,805	1259068	178658	100,000	100,000	N/A	1602	N/A	1,183	

Creator QPackSA

Chromatogram

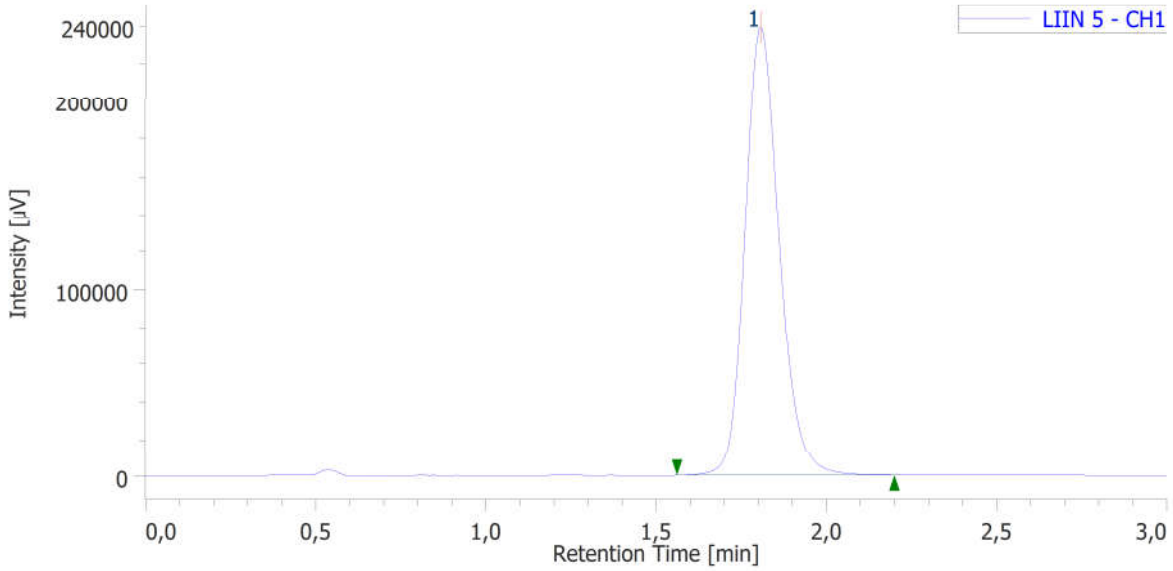

Chromatogram Information	
User Name	QPackSA
Date Modified	25/05/2022 15:50:18
Description	
HPLC System Name	Multicare
Injection Date	25/05/2022 15:47:16
Volume	20,00 [μL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,807	1679886	238788	100,000	100,000	N/A	1613	N/A	1,197	

Creator QPackSA

Chromatogram

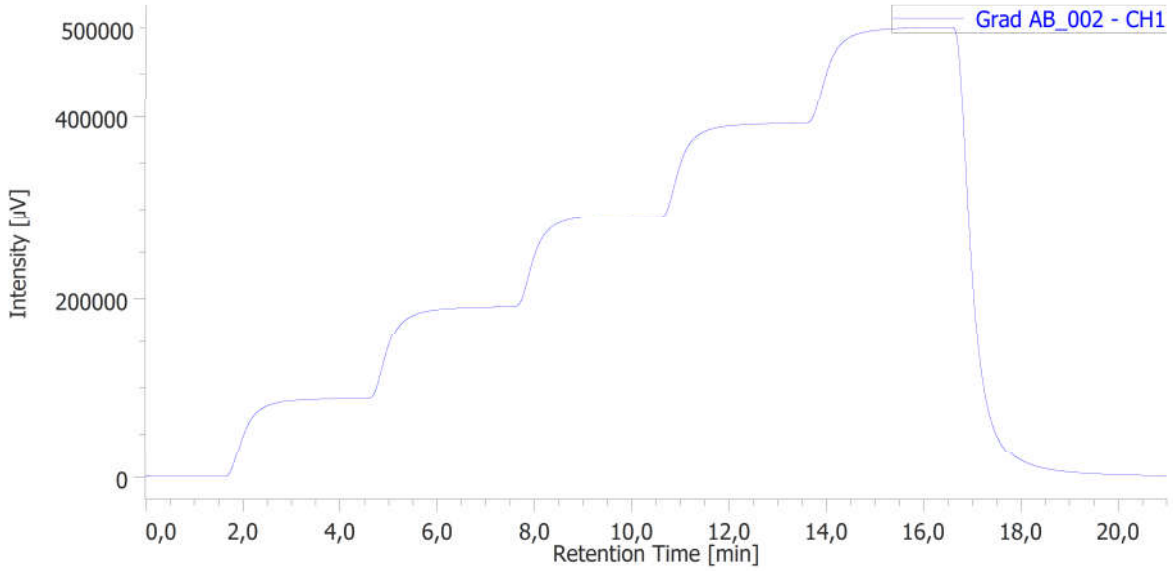


Chromatogram Information	
User Name	QPackSA
Date Modified	26/05/2022 09:19:54
Description	
HPLC System Name	Multicare
Injection Date	26/05/2022 08:58:52
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AB_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Creator QPackSA

Chromatogram

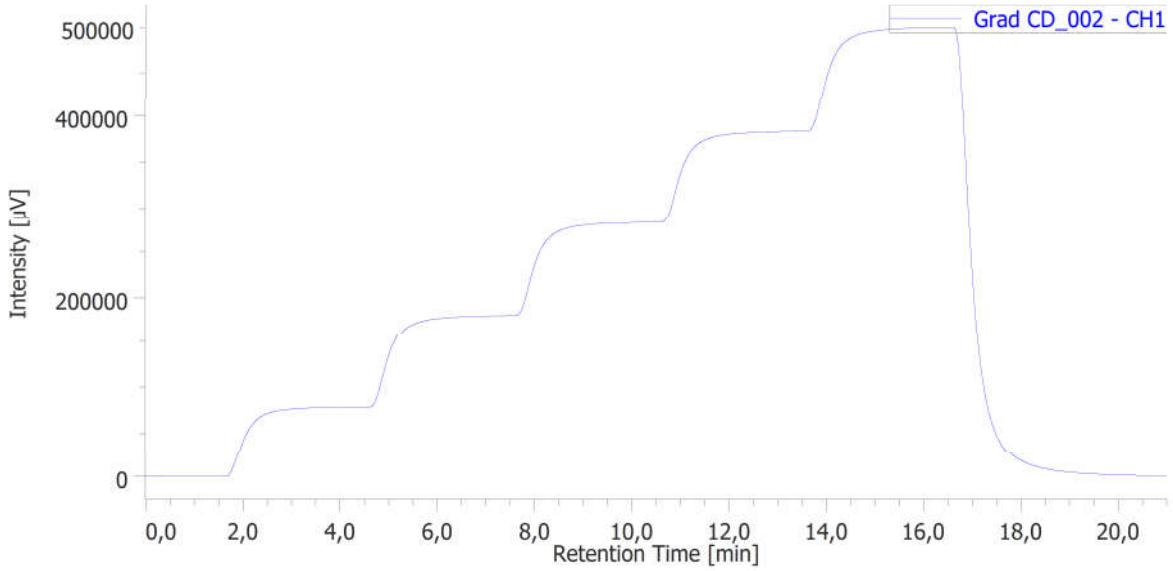

Chromatogram Information	
User Name	QPackSA
Date Modified	26/05/2022 10:06:50
Description	
HPLC System Name	Multicare
Injection Date	26/05/2022 09:45:48
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Creator QPackSA