HPLC - Agilent Lab Advisor


Service & Diagnostics

Scan

al Scan - 1260 VWD [DEACX00141]

mp On | Blank Scan

e Scan | from 200 | to 300 | step 1

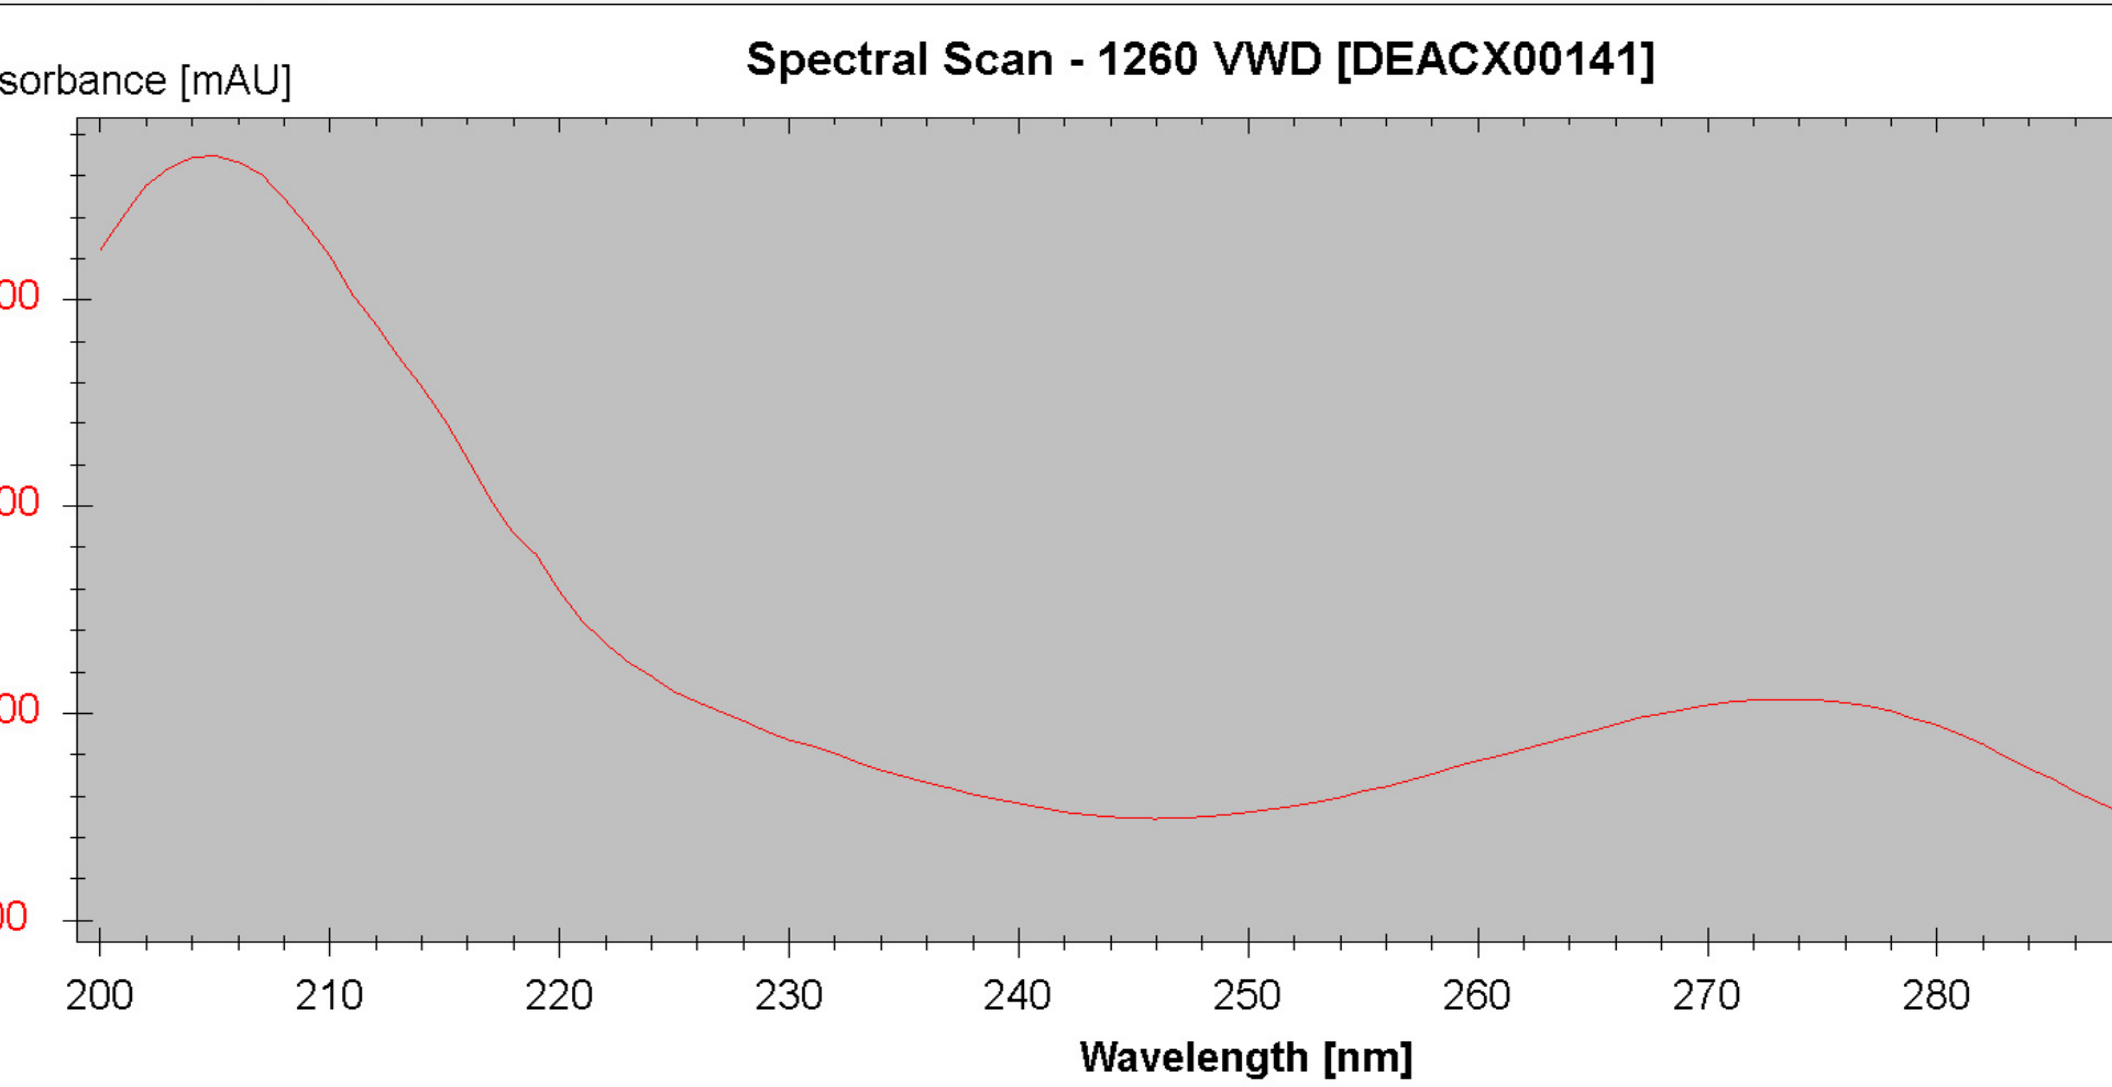

Activate
Go to PC se
more

HPLC - Agilent Lab Advisor


Service & Diagnostics

Scan

al Scan - 1260 VWD [DEACX00141]

mp On | Blank Scan

e Scan | from 200 | to 300 | step 1

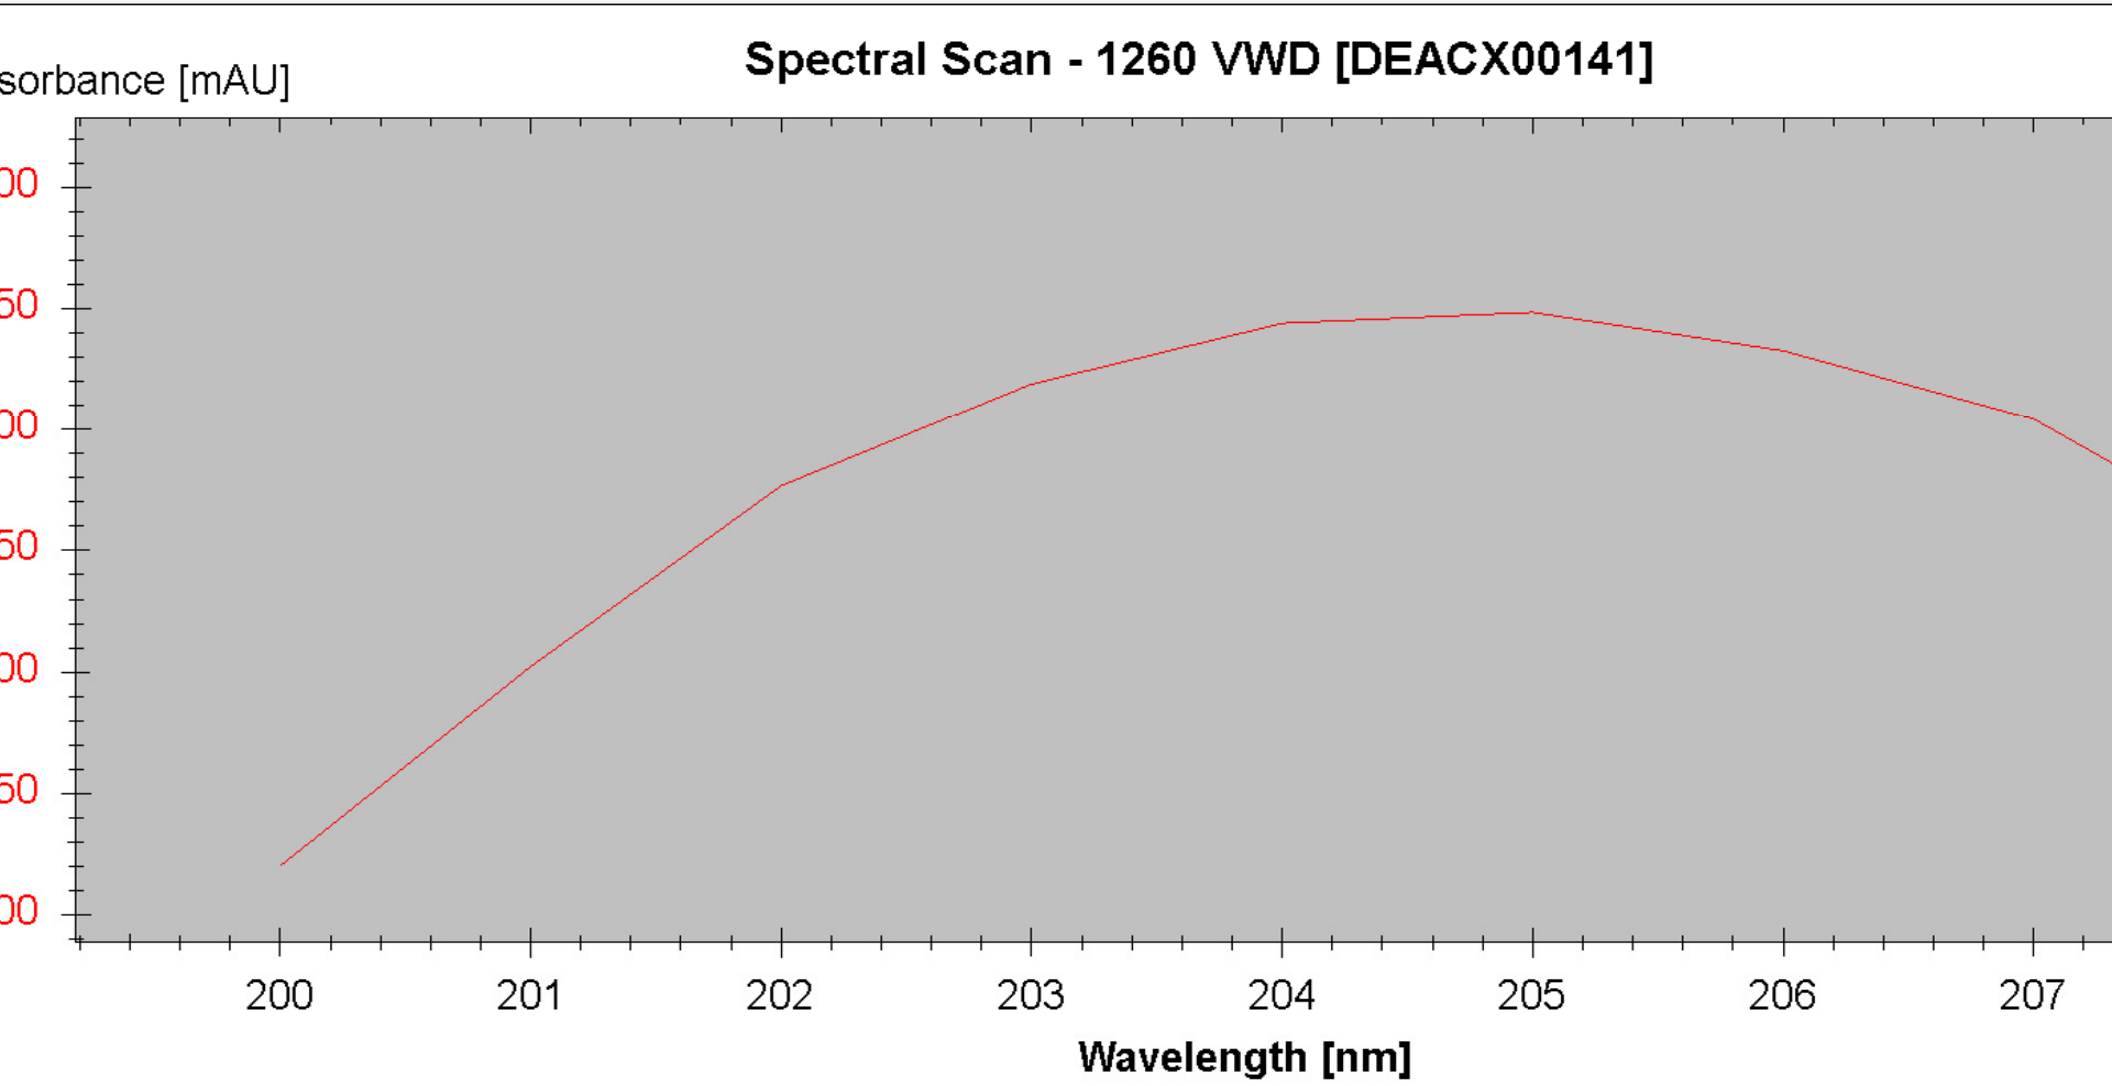

Activate
Go to PC se
more.

HPLC - Agilent Lab Advisor


Service & Diagnostics

Scan

al Scan - 1260 VWD [DEACX00141]

mp On | Blank Scan

e Scan | from 200 | to 300 | step 1

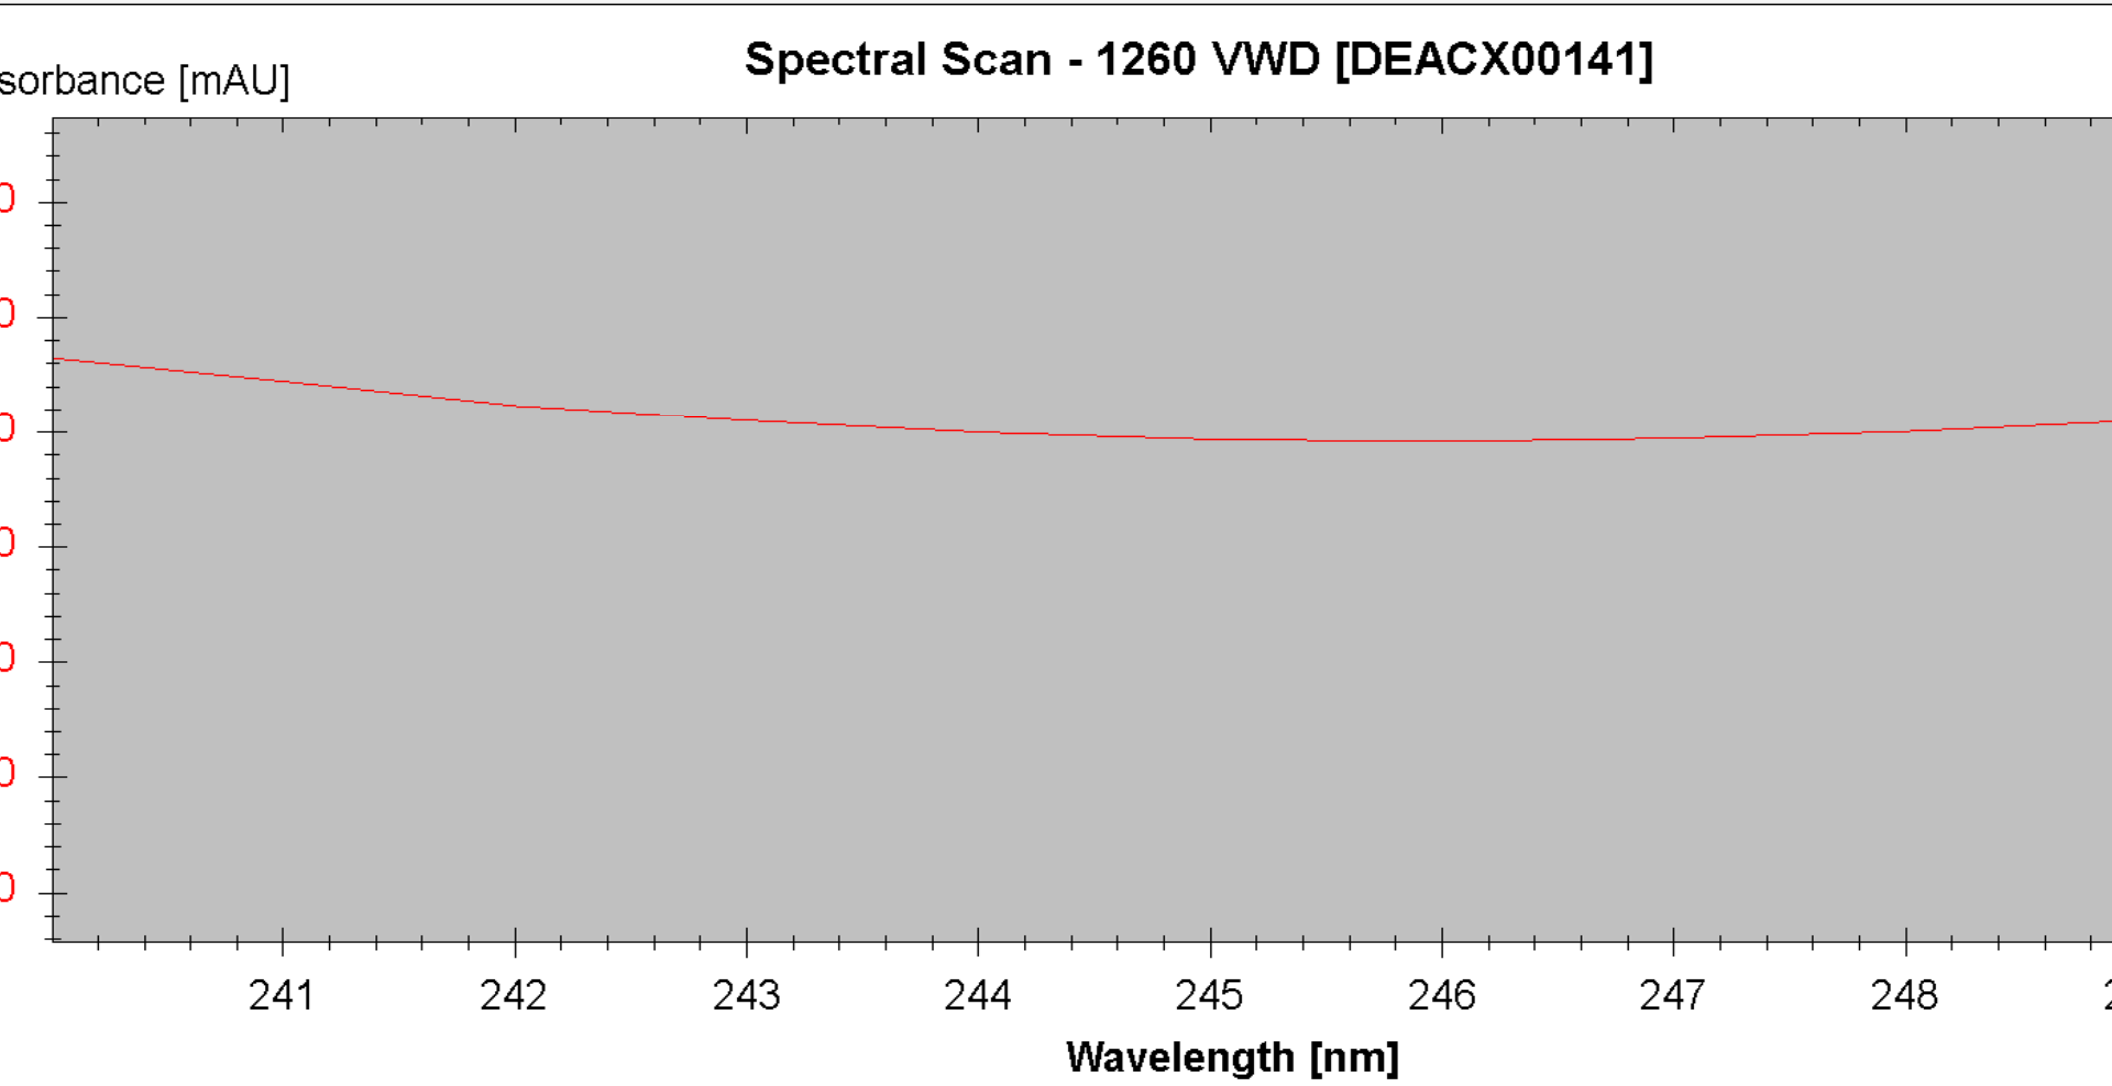

Activate
Go to PC se
more.

HPLC - Agilent Lab Advisor


Service & Diagnostics

Scan

al Scan - 1260 VWD [DEACX00141]

mp On | Blank Scan


e Scan | from 200 | to 300 | step 1

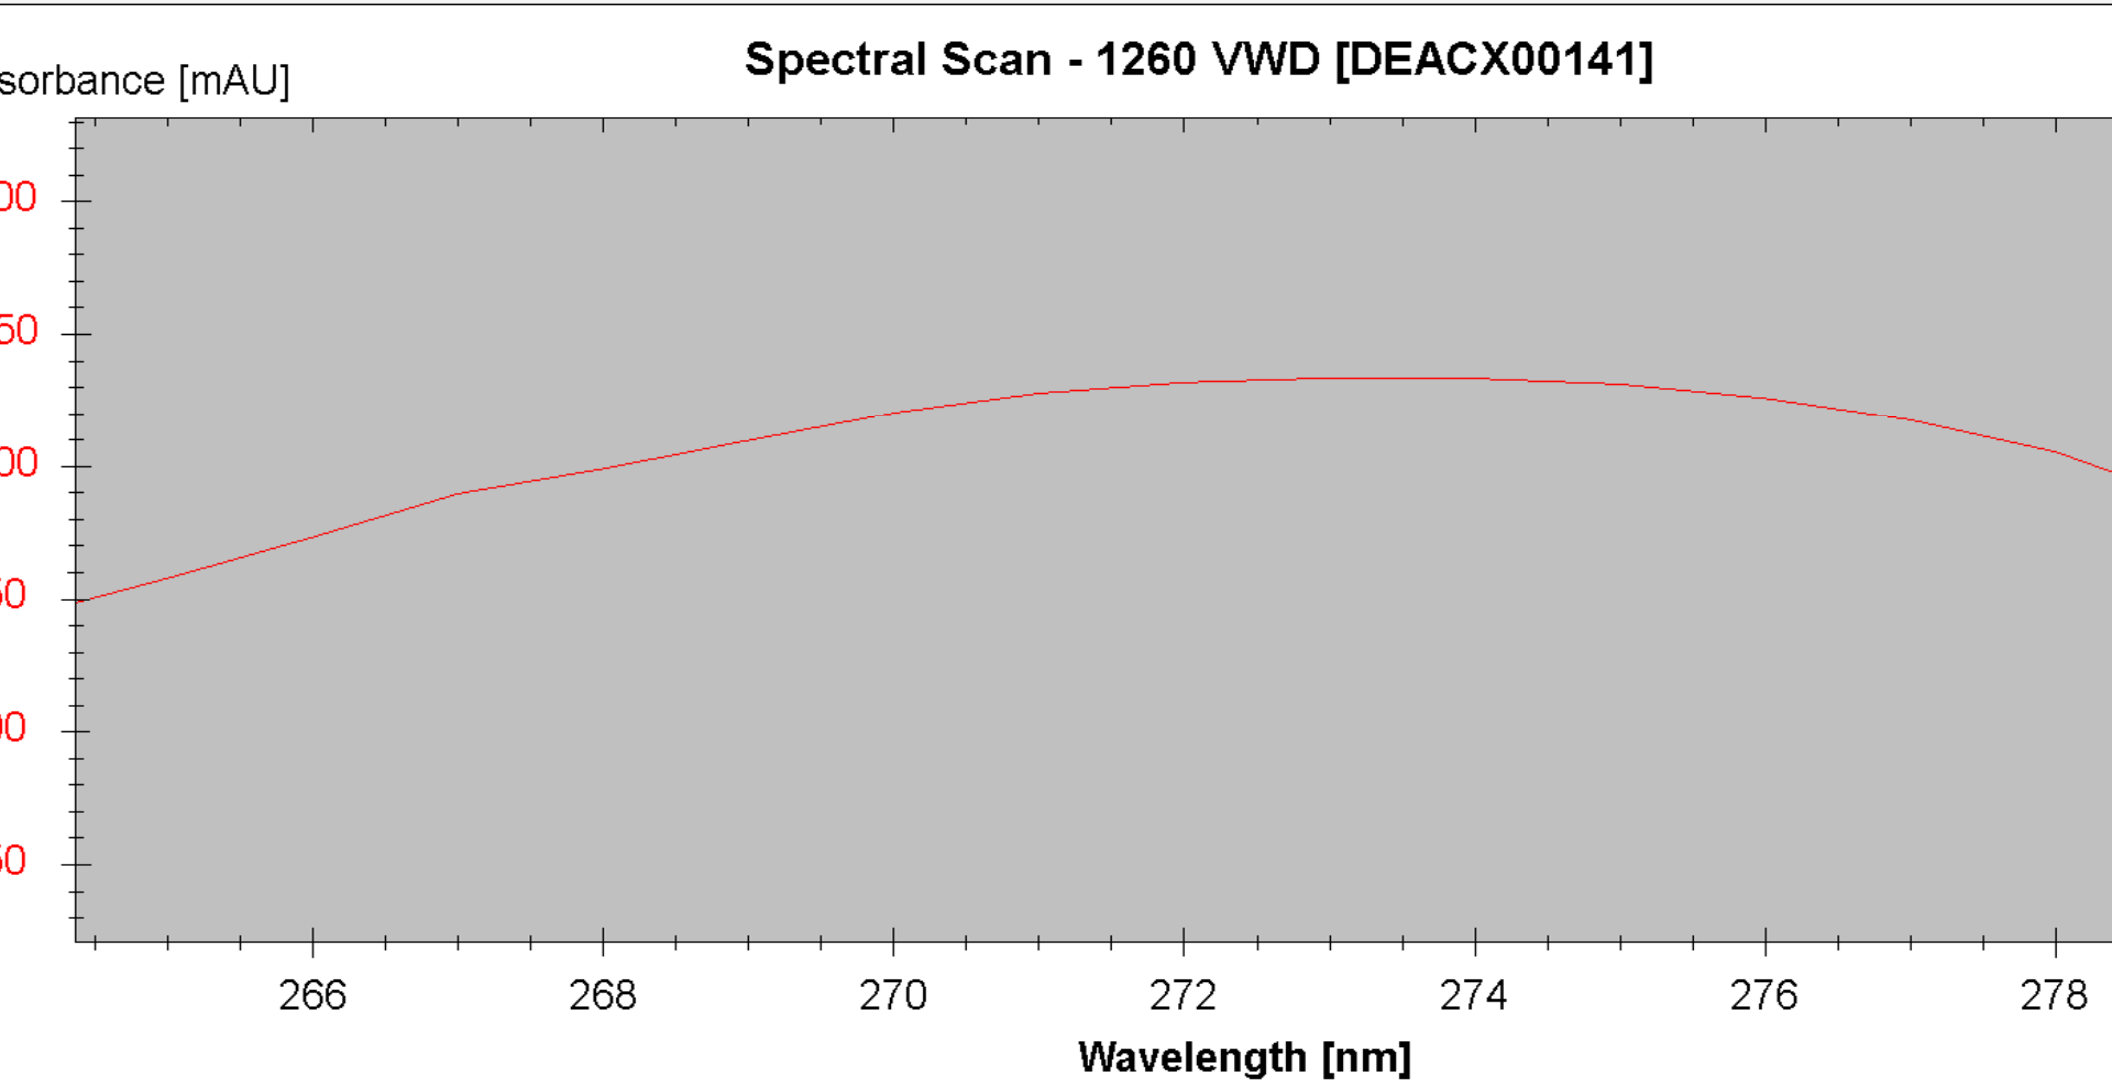

Activate
Go to PC se
more.

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\001-P1-A1-Branco PCIN 001.D
Sample Name: Branco PCIN 001

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Acq. Instrument : HPLC 2                          Location :   P1-A1
Injection Date  : 4/18/2023 2:18:56 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

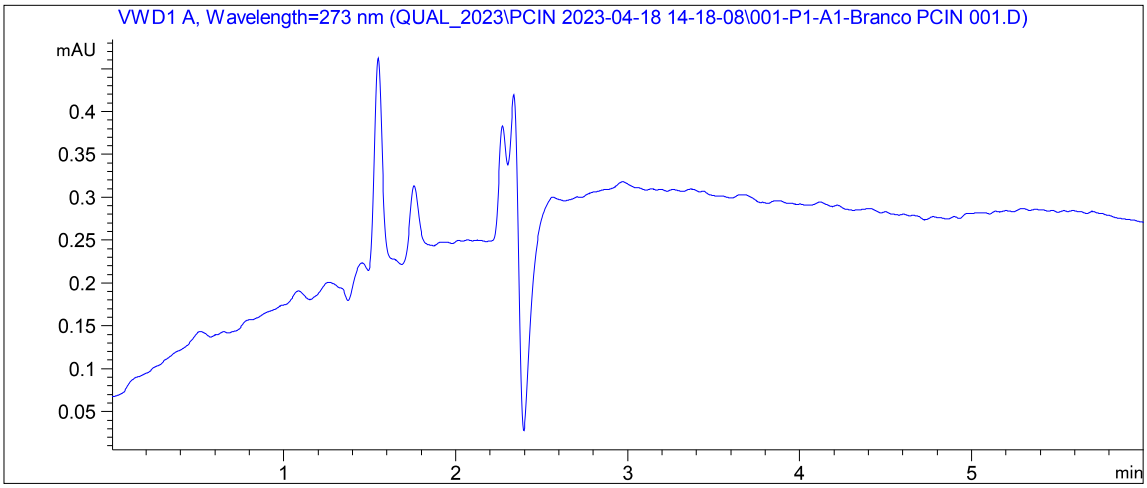


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.630         0.0000    0.00000   0.0000 Cafeina

Totals :                       0.00000



1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\002-P1-A2-PCIN 001.D
Sample Name: PCIN 001

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   2
Acq. Instrument : HPLC 2                          Location :   P1-A2
Injection Date  : 4/18/2023 2:26:07 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

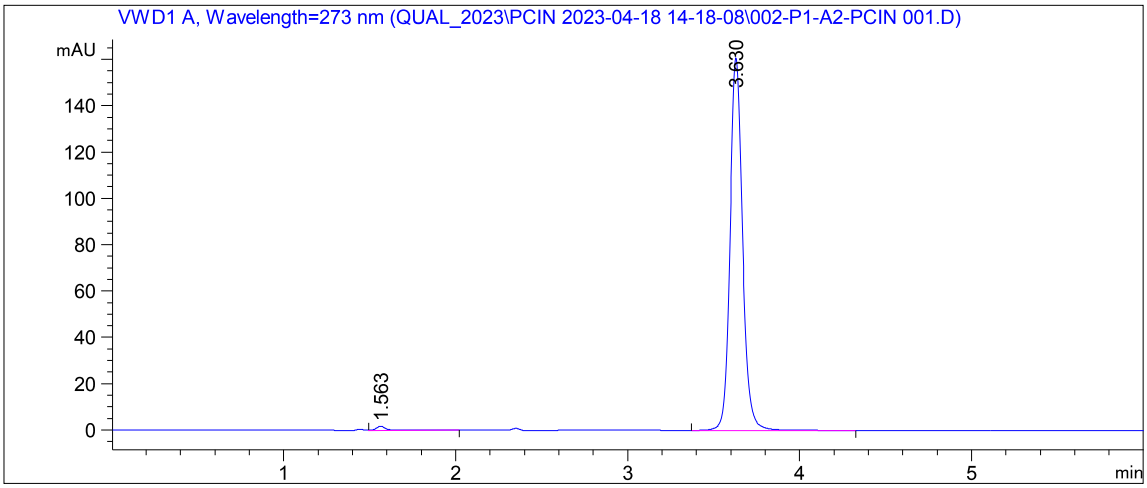


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.563 VV R    0.0793   10.92359   1.3293 ?
   2   3.630 BB      0.0778  810.82312  98.6707 Cafeina

Totals :                    821.74671


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\003-P1-A2-PCIN 002.D
Sample Name: PCIN 002

```
======================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   3
Acq. Instrument : HPLC 2                          Location :   P1-A2
Injection Date  : 4/18/2023 2:33:06 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

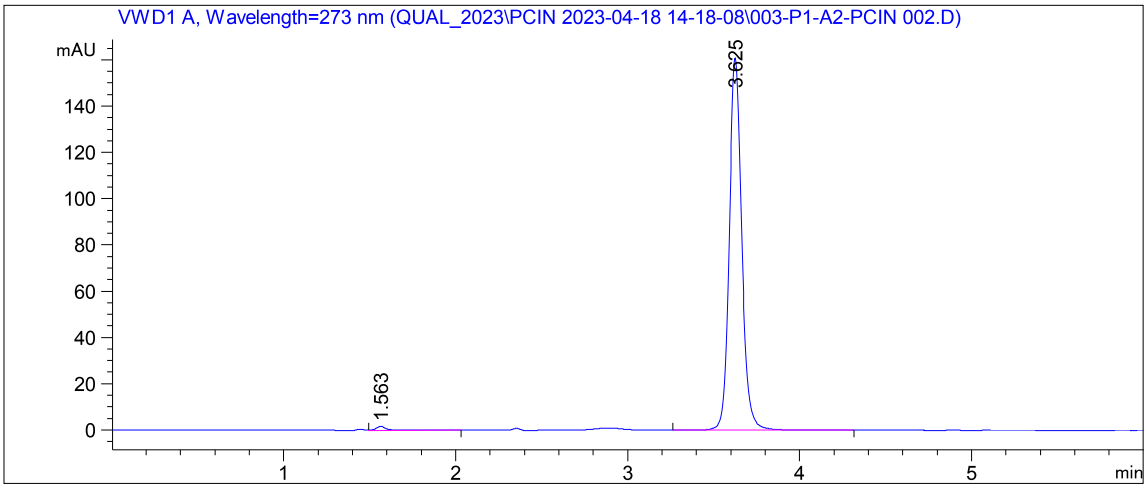


```
======================================================================
                        Area Percent Report
======================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.563 VV R    0.0830   11.35491   1.3803 ?
   2   3.625 BB      0.0768  811.30420  98.6197 Cafeina

Totals :                    822.65910


======================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\004-P1-A2-PCIN 003.D
Sample Name: PCIN 003

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   4
Acq. Instrument : HPLC 2                          Location :   P1-A2
Injection Date  : 4/18/2023 2:40:08 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

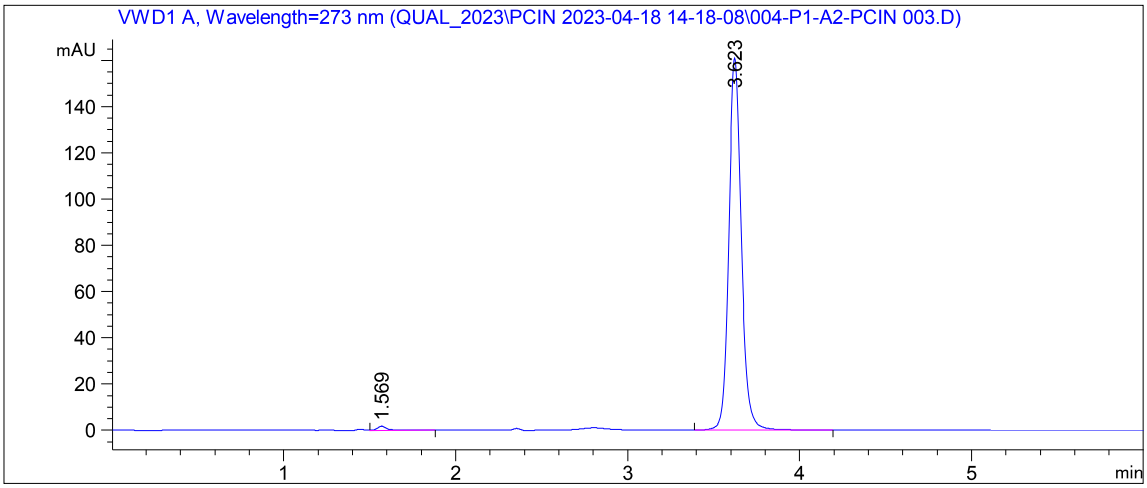


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.569 VV R    0.0695    9.56204   1.1666 ?
   2   3.623 BB      0.0777  810.09985  98.8334 Cafeina

Totals :                    819.66190


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\005-P1-A1-Branco PCIN 002.D
Sample Name: Branco PCIN 002

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   5
Acq. Instrument : HPLC 2                          Location :   P1-A1
Injection Date  : 4/18/2023 2:47:07 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

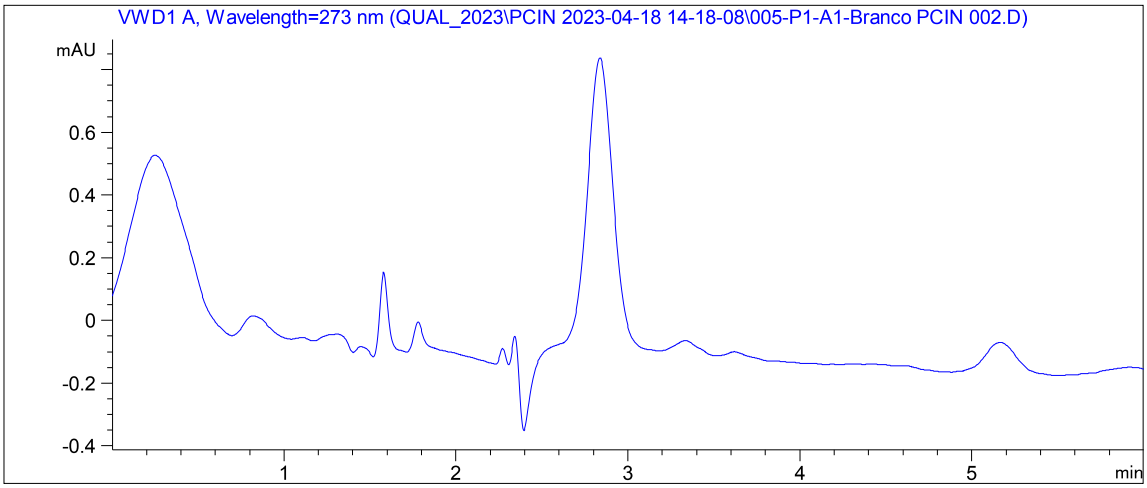


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.630         0.0000    0.00000   0.0000 Cafeina

Totals :                       0.00000



1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\006-P1-A2-PCIN 004.D
Sample Name: PCIN 004

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   6
Acq. Instrument : HPLC 2                          Location :   P1-A2
Injection Date  : 4/18/2023 2:54:08 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

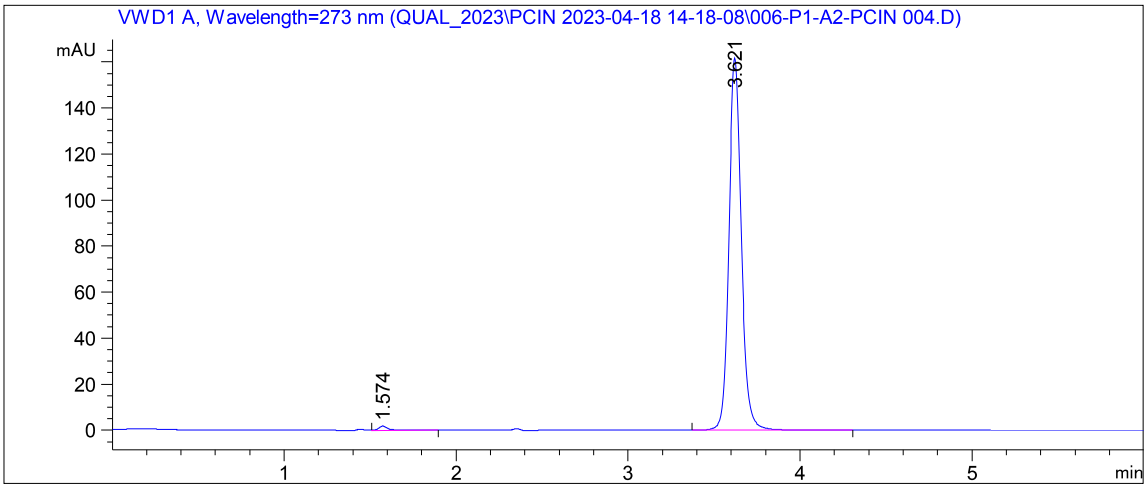


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.574 VV R    0.0678    9.65365   1.1773 ?
   2   3.621 BB      0.0774  810.32904  98.8227 Cafeina

Totals :                    819.98269


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\007-P1-A2-PCIN 005.D
Sample Name: PCIN 005

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   7
Acq. Instrument : HPLC 2                           Location :   P1-A2
Injection Date  : 4/18/2023 3:01:09 PM                  Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

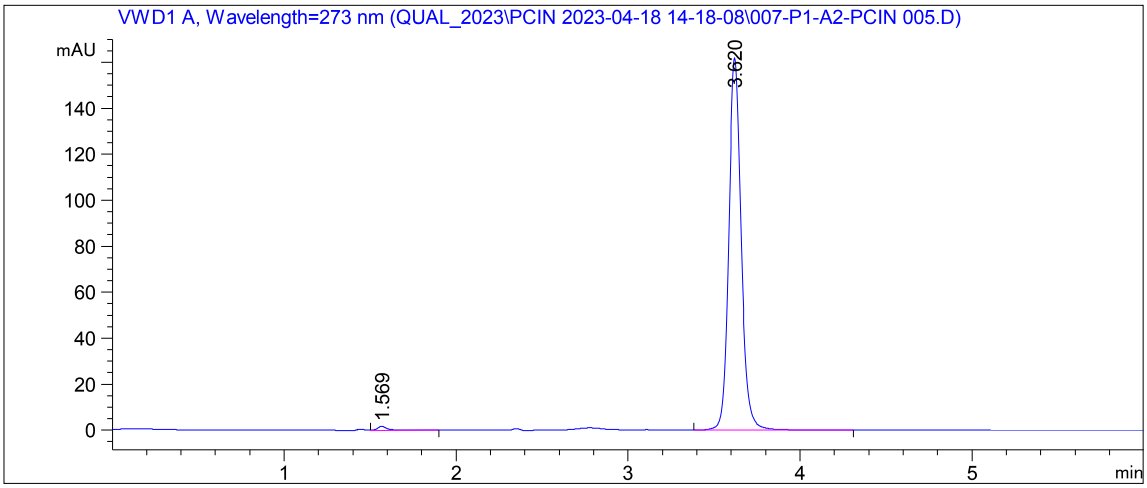


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.569 VV R    0.0708    9.71583   1.1874 ?
   2   3.620 BB      0.0763  808.54352  98.8126 Cafeina

Totals :                    818.25935


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\008-P1-A2-PCIN 006.D
Sample Name: PCIN 006

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   8
Acq. Instrument : HPLC 2                          Location :   P1-A2
Injection Date  : 4/18/2023 3:08:08 PM                 Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

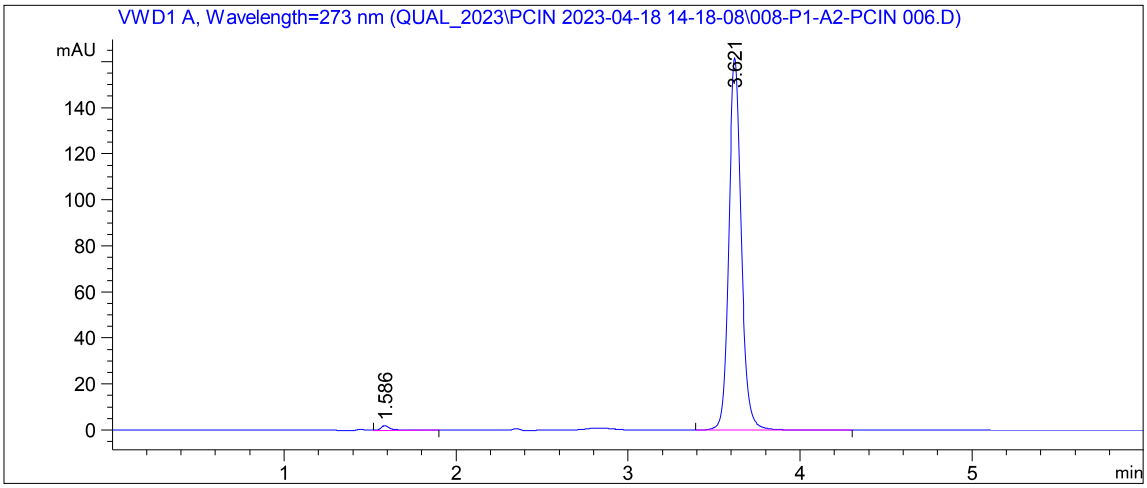


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   1.586 VV R    0.0651   10.19455   1.2434 ?
   2   3.621 BB      0.0774  809.72607  98.7566 Cafeina

Totals :                     819.92062


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\009-P1-A1-Branco PCIN 003.D
Sample Name: Branco PCIN 003

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   9
Acq. Instrument : HPLC 2                         Location :   P1-A1
Injection Date  : 4/18/2023 3:15:07 PM                Inj :   1
                                                Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M
Last changed    : 4/18/2023 2:18:08 PM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\PCIN 2023-04-18 14-18-08\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/18/2023 3:26:36 PM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

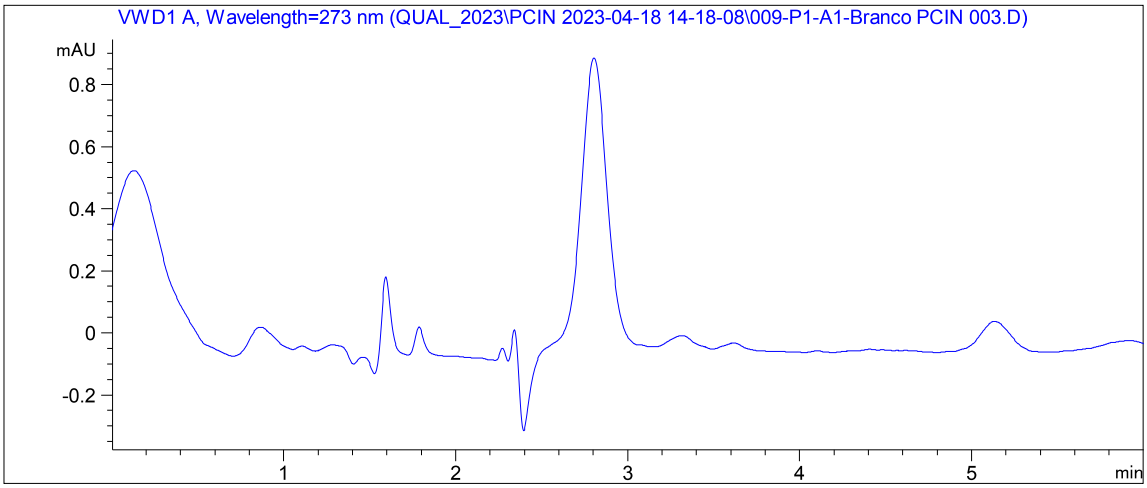


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      4/18/2023 3:26:36 PM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.630         0.0000    0.00000   0.0000 Cafeina

Totals :                       0.00000



1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\001-P1-A3-LDUV 001.D
Sample Name: LDUV 001

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Acq. Instrument : HPLC 2                          Location :   P1-A3
Injection Date  : 4/19/2023 8:48:00 AM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M
Last changed    : 4/19/2023 8:47:11 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 9:30:25 AM by SYSTEM
Method Info     : Qualificacao
```

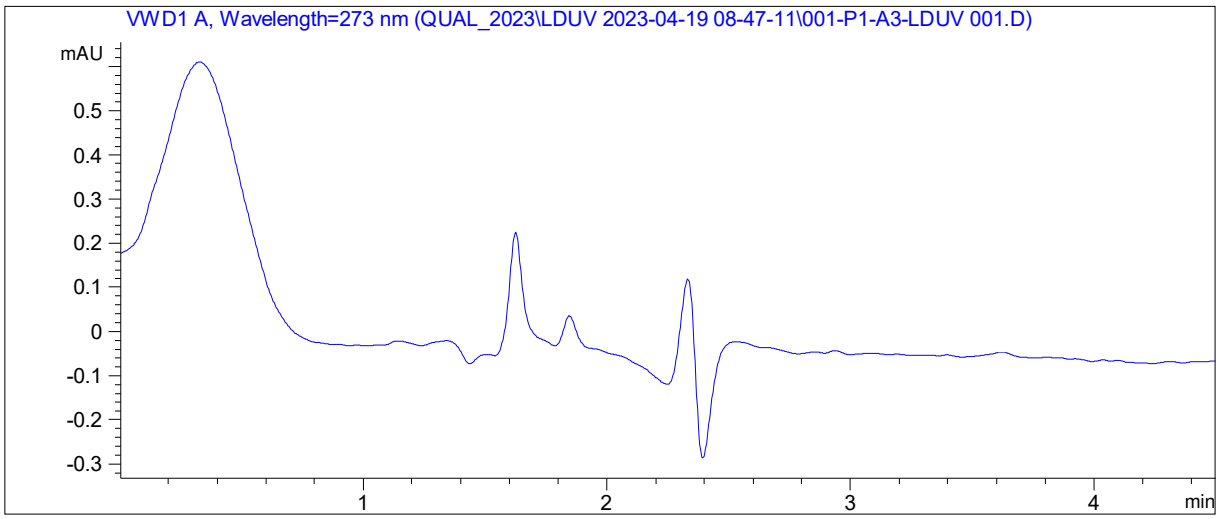


```
==========================================================================
                          Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\002-P1-A4-LDUV 002.D
Sample Name: LDUV 002

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   2
Acq. Instrument : HPLC 2                           Location :   P1-A4
Injection Date  : 4/19/2023 8:53:49 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M
Last changed    : 4/19/2023 8:47:11 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 9:30:25 AM by SYSTEM
Method Info     : Qualificacao
```

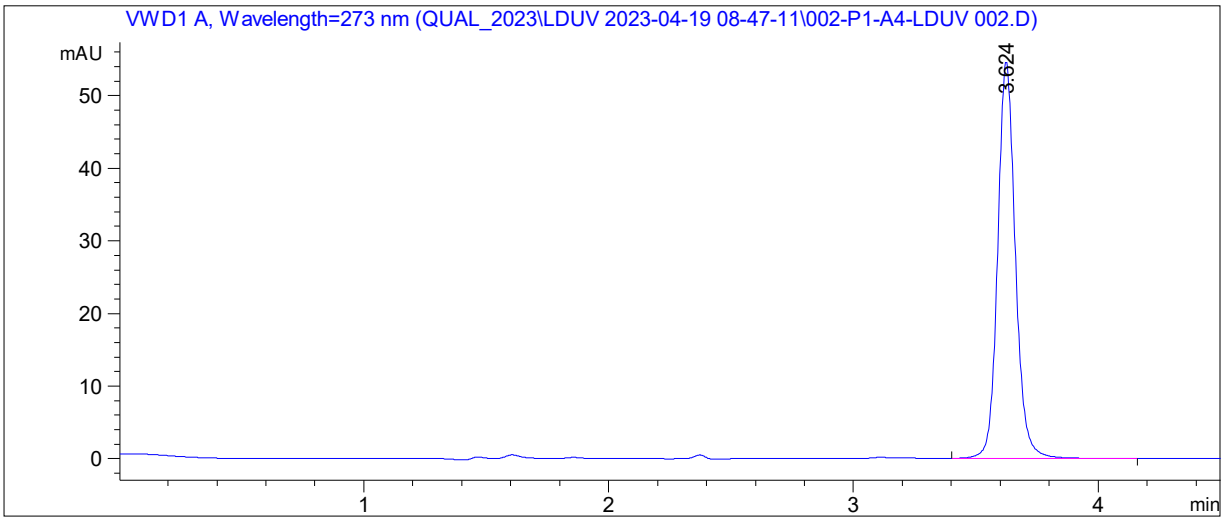


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   3.624 BB    0.0767  275.03961   54.69863 100.0000

Totals :                   275.03961   54.69863

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\003-P1-A5-LDUV 003.D
Sample Name: LDUV 003

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Acq. Instrument : HPLC 2                           Location :   P1-A5
Injection Date  : 4/19/2023 8:59:19 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M
Last changed    : 4/19/2023 8:47:11 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 9:30:25 AM by SYSTEM
Method Info     : Qualificacao
```

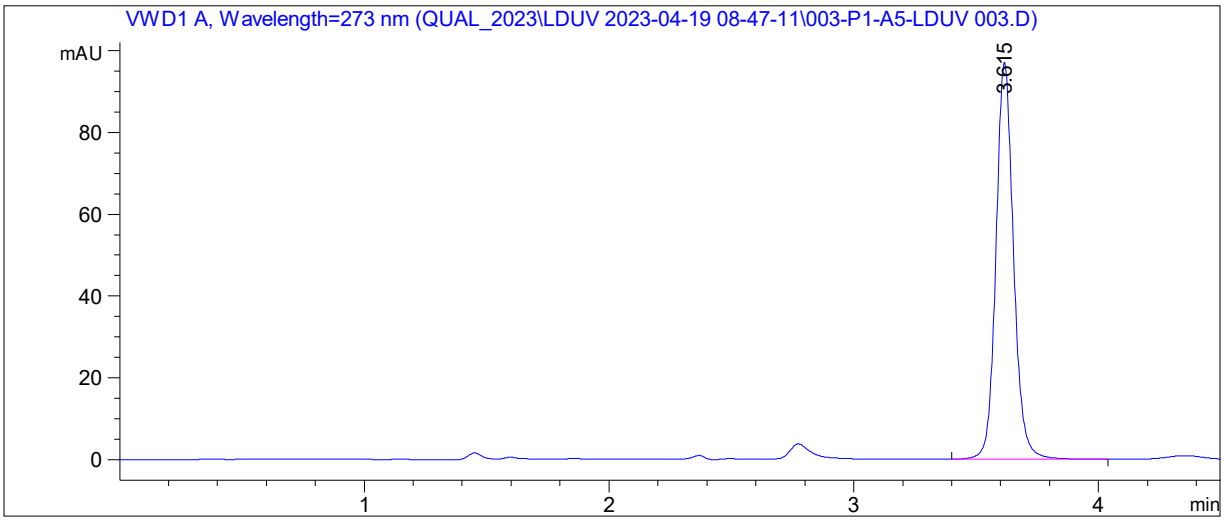


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   3.615 BB    0.0762  485.46329   97.25912 100.0000

Totals :                   485.46329   97.25912


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\004-P1-A6-LDUV 004.D
Sample Name: LDUV 004

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   4
Acq. Instrument : HPLC 2                           Location :   P1-A6
Injection Date  : 4/19/2023 9:04:47 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M
Last changed    : 4/19/2023 8:47:11 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LDUV 2023-04-19 08-47-11\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 9:30:25 AM by SYSTEM
Method Info     : Qualificacao
```

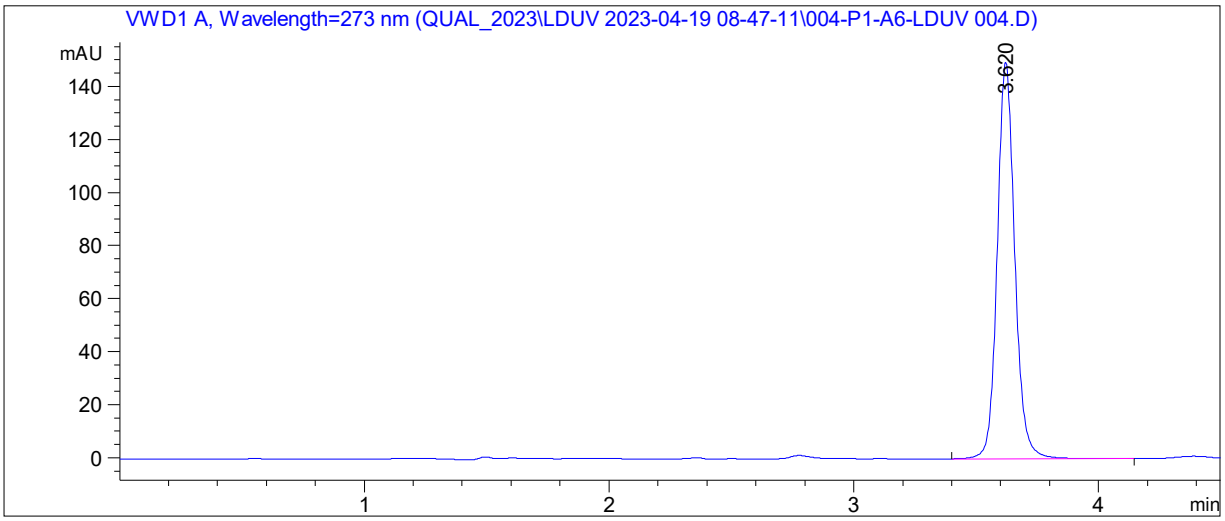


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   3.620 BB    0.0761  745.29370  149.63889 100.0000

Totals :                   745.29370  149.63889


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LDUV_05 2023-04-19 09-24-34.D
Sample Name: LDUV_05

```
==========================================================================
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : HPLC 2                          Location :   P1-A7
Injection Date  : 4/19/2023 9:25:15 AM
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Methods\Qualificacao.M
Last changed    : 4/19/2023 8:47:08 AM by SYSTEM
Analysis Method : C:\CHEM32\3\METHODS\GRAD AB.M
Last changed    : 4/19/2023 9:37:23 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao Gradiente AB
```

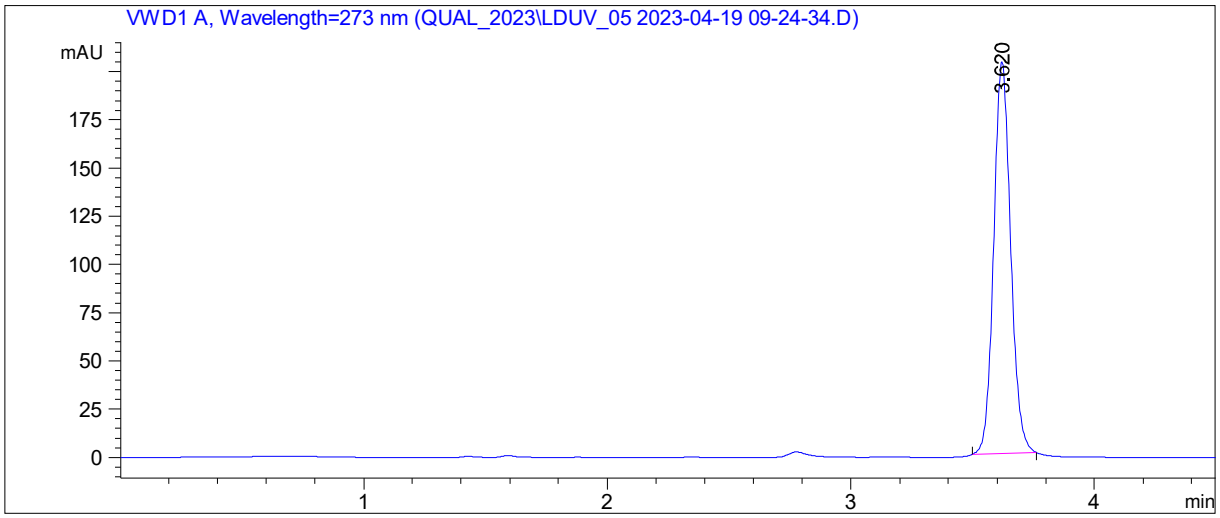


```
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :     10.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   3.620 BBA   0.0740  974.64917  203.04539 100.0000

Totals :                   974.64917  203.04539


==========================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\001-P1-A8-LIIN 001.D
Sample Name: LIIN 001

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Acq. Instrument : HPLC 2                           Location :   P1-A8
Injection Date  : 4/19/2023 9:39:10 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M
Last changed    : 4/19/2023 9:38:25 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 10:09:22 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

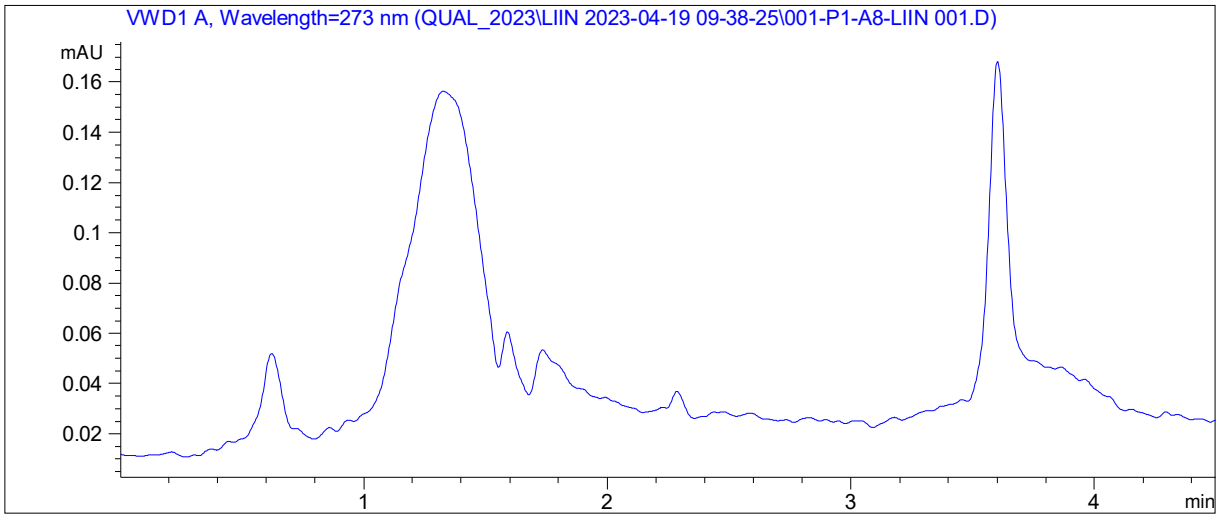


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 2023 10:08:16 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|----------------------
   1   3.609         0.0000    0.00000   0.0000 Cafeina

Totals :                       0.00000



1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\002-P1-A8-LIIN 002.D
Sample Name: LIIN 002

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   2
Acq. Instrument : HPLC 2                          Location :   P1-A8
Injection Date  : 4/19/2023 9:44:34 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 5.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M
Last changed    : 4/19/2023 9:38:25 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 10:09:22 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

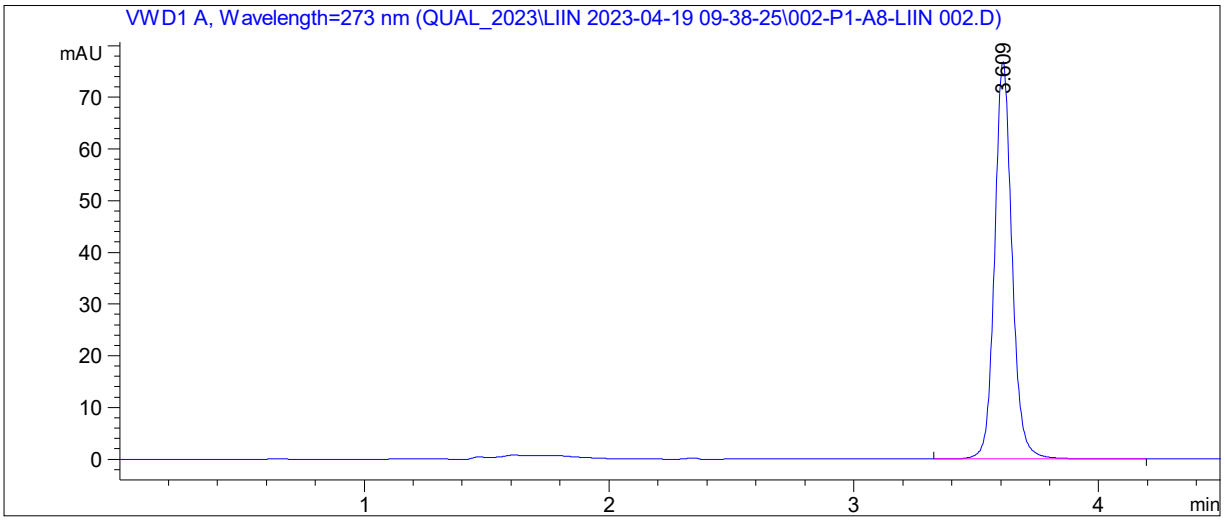


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 2023 10:08:16 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.609 BB      0.0758  381.42444 100.0000 Cafeina

Totals :                    381.42444


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\003-P1-A8-LIIN 003.D
Sample Name: LIIN 003

```
==========================================================================
Acq. Operator    : SYSTEM                          Seq. Line :   3
Acq. Instrument : HPLC 2                           Location :   P1-A8
Injection Date   : 4/19/2023 9:50:07 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method      : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M
Last changed     : 4/19/2023 9:38:25 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M (
                  Sequence Method)
Last changed     : 4/19/2023 10:09:22 AM by SYSTEM
                   (modified after loading)
Method Info      : Qualificacao
```

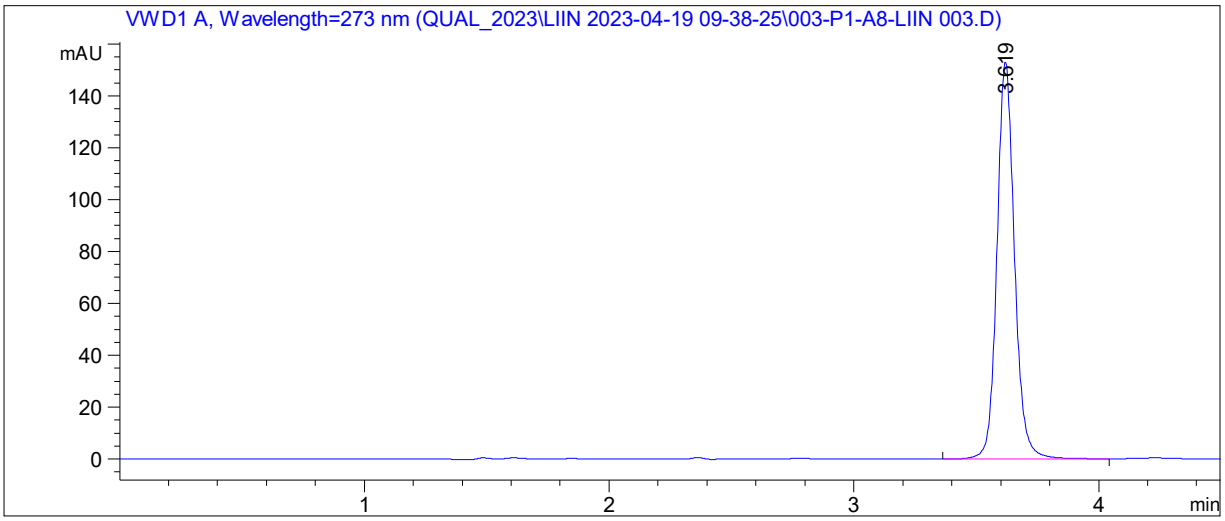


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 2023 10:08:16 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type    Width     Area      Area     Name
  #   [min]           [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.619 BB      0.0759  761.40924 100.0000 Cafeina

Totals :                     761.40924


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\004-P1-A8-LIIN 004.D
Sample Name: LIIN 004

```
==========================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   4
Acq. Instrument : HPLC 2                          Location :   P1-A8
Injection Date  : 4/19/2023 9:55:39 AM                Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M
Last changed    : 4/19/2023 9:38:25 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 10:09:22 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

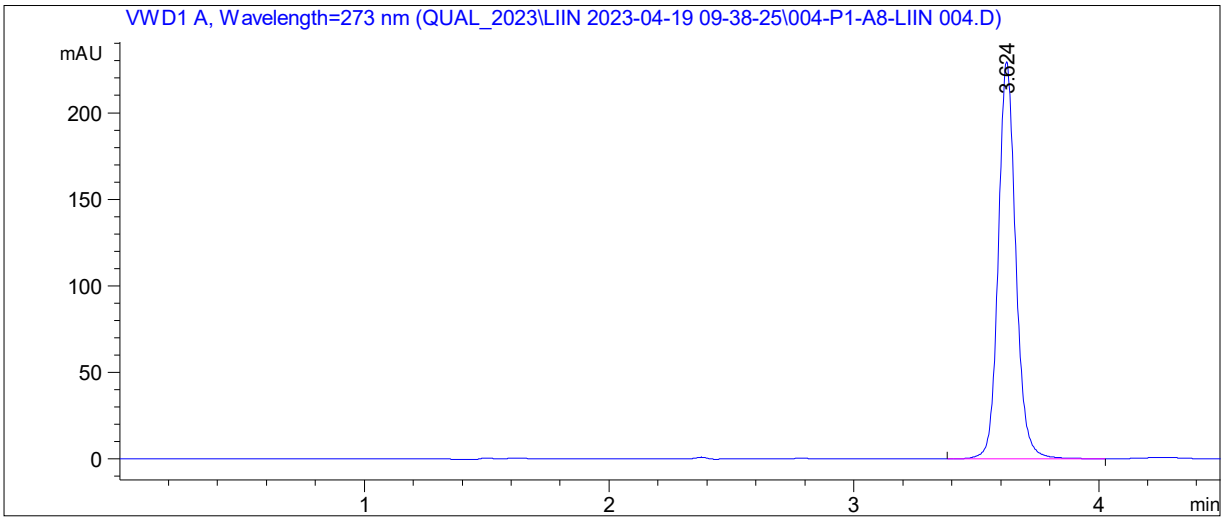


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 2023 10:08:16 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|--------------------
   1   3.624 BB      0.0759 1139.98083 100.0000 Cafeina

Totals :                   1139.98083


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\005-P1-A8-LIIN 005.D
Sample Name: LIIN 005

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   5
Acq. Instrument : HPLC 2                           Location :   P1-A8
Injection Date  : 4/19/2023 10:01:17 AM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M
Last changed    : 4/19/2023 9:38:25 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\LIIN 2023-04-19 09-38-25\Qualificacao.M (
                  Sequence Method)
Last changed    : 4/19/2023 10:09:22 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

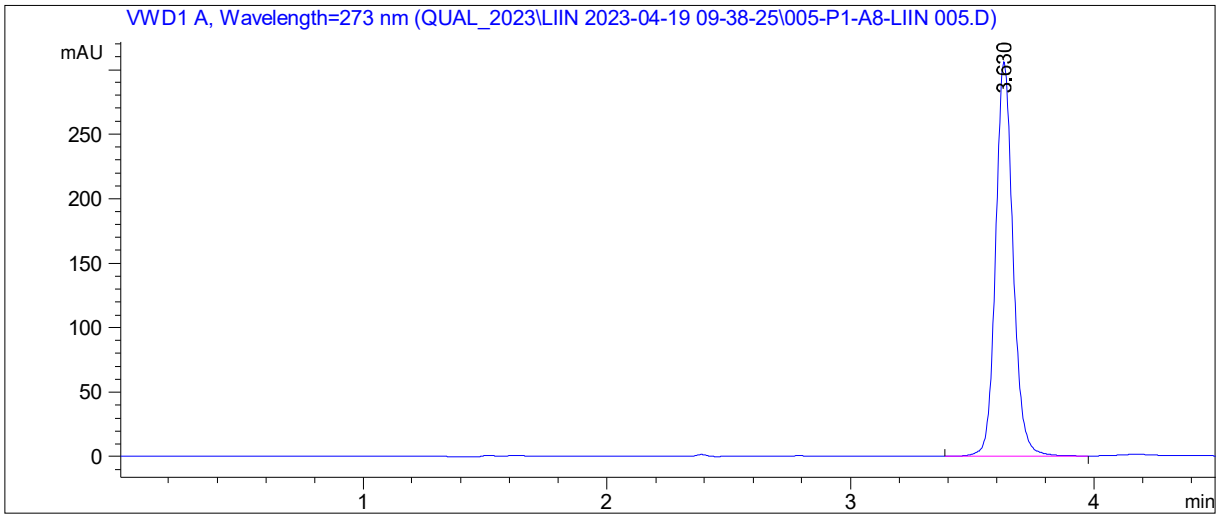


```
=====================================================================
                        Area Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 2023 10:08:16 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm


Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [mAU*s]       %
----|-------|------|-------|----------|--------|----------------------
   1   3.630 BB      0.0758 1517.46057 100.0000 Cafeina

Totals :                   1517.46057


=====================================================================
                        *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\RELB 2023-04-19 10-07-15\001-P1-A9-RELB_001.D
Sample Name: RELB_001

```
=====================================================================
Acq. Operator   : SYSTEM                          Seq. Line :   1
Acq. Instrument : HPLC 2                           Location :   P1-A9
Injection Date  : 4/19/2023 10:08:10 AM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Acq. Method     : C:\Chem32\3\Data\QUAL_2023\RELB 2023-04-19 10-07-15\RELB.M
Last changed    : 4/19/2023 10:07:16 AM by SYSTEM
Analysis Method : C:\Chem32\3\Data\QUAL_2023\RELB 2023-04-19 10-07-15\RELB.M (Sequence Method
                  )
Last changed    : 4/19/2023 10:27:05 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao
```

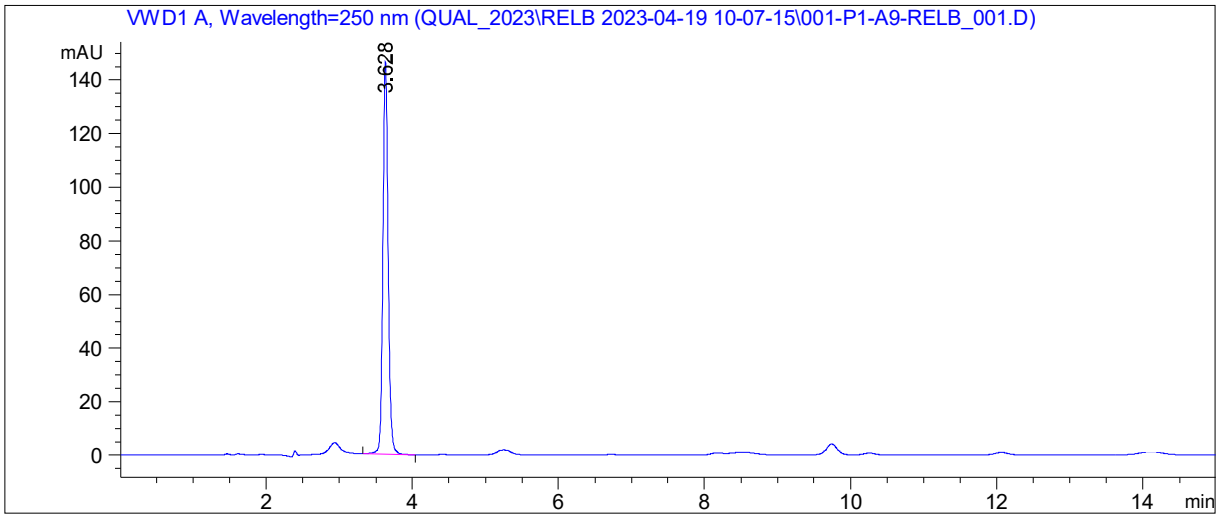


```
=====================================================================
                        Height Percent Report
=====================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, April 19, 202310:27:05 AM
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=250 nm

Peak RetTime  Type   Width    Height    Height   Name
  #   [min]          [min]    [mAU]        %
----|-------|------|-------|----------|--------|----------------------
   1   3.628 BB      0.0758  146.72116 100.0000 Cafeina


Totals :                     146.72116


=====================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\GRAD AB 2023-04-19 11-24-30.D
Sample Name: GRAD AB

```
==========================================================================
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : HPLC 2                          Location :     -
Injection Date  : 4/19/2023 11:24:37 AM
                                                  Inj Volume : No inj
Acq. Method     : C:\CHEM32\3\METHODS\GRAD AB.M
Last changed    : 4/19/2023 11:23:54 AM by SYSTEM
Analysis Method : C:\CHEM32\3\METHODS\GRAD AB.M
Last changed    : 4/19/2023 11:48:25 AM by SYSTEM
                  (modified after loading)
Method Info     : Qualificacao Gradiente AB

Additional Info : Peak(s) manually integrated
```

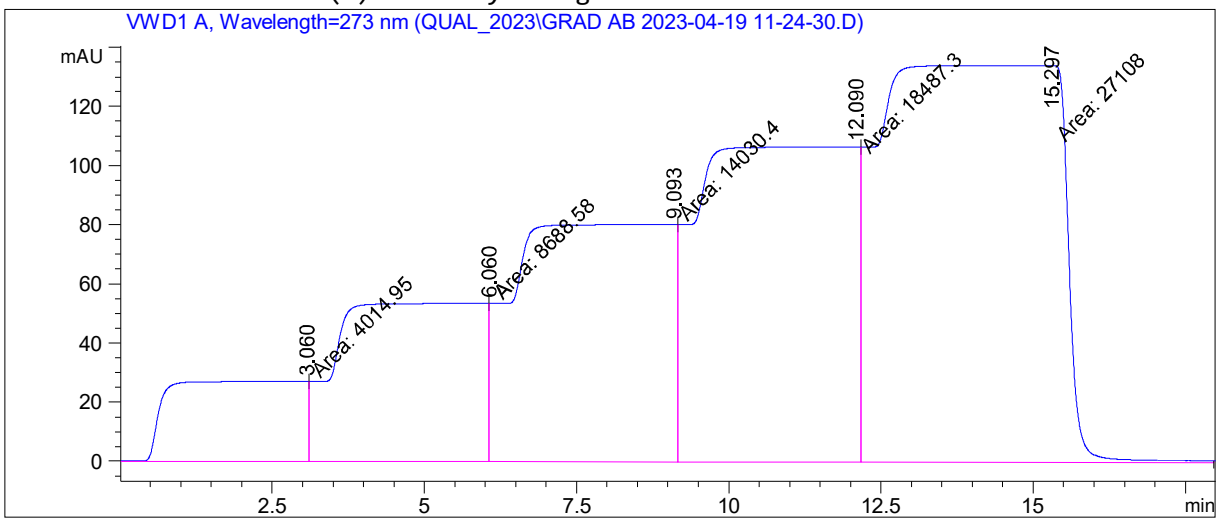


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :     10.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: VWD1 A, Wavelength=273 nm

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   3.060 MF    2.4727 4014.94775   27.06196   5.5509
   2   6.060 FM    2.7005 8688.57617   53.62307  12.0125
   3   9.093 FM    2.9154 1.40304e4    80.20760  19.3979
   4  12.090 FM    2.8916 1.84873e4   106.55786  25.5599
   5  15.297 FM    3.3639 2.71080e4   134.30742  37.4787

Totals :                  7.23292e4   401.75791



==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\QUAL_2023\GRAD CD 2023-04-19 12-05-20.D
Sample Name: GRAD CD

==========

Acq. Operator : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : HPLC 2 Location : -
Injection Date : 4/19/2023 12:05:26 PM
Inj Volume : No inj
Method : C:\CHEM32\3\METHODS\GRAD CD.M
Last changed : 4/19/2023 11:47:17 AM by SYSTEM
Method Info : Qualificacao Gradiente CD

Additional Info : Peak(s) manually integrated

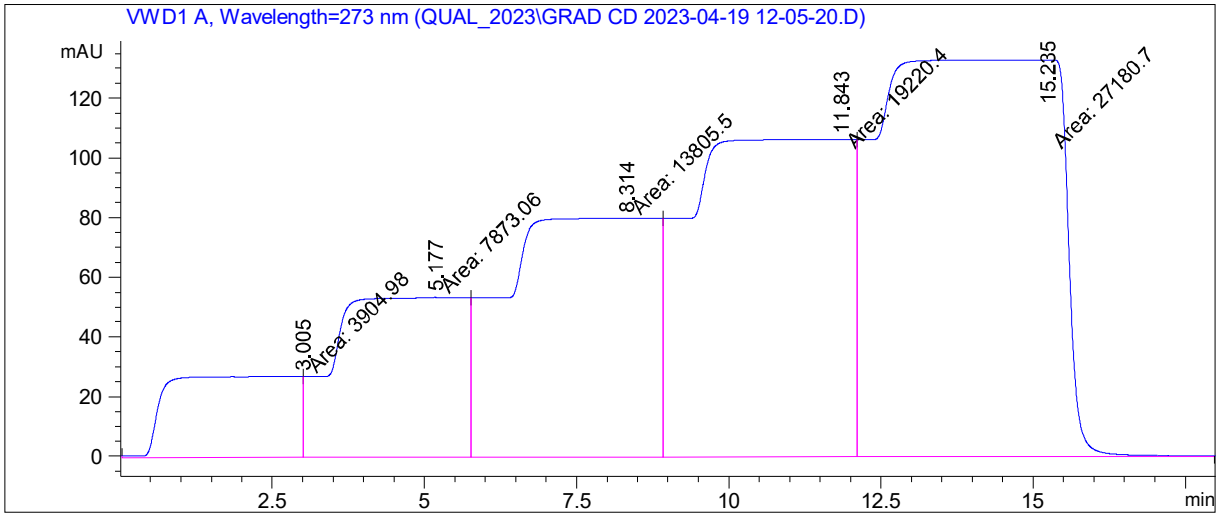

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 10.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	3.005	MF	2.3992	3904.98047	27.12700	5.4247
2	5.177	FM	2.4406	7873.05762	53.76453	10.9371
3	8.314	FM	2.8786	1.38055e4	79.93290	19.1784
4	11.843	FM	3.0129	1.92204e4	106.32458	26.7007
5	15.235	FM	3.4108	2.71807e4	132.81866	37.7590
Totals :				7.19847e4	399.96767	

==========

*** End of Report ***