


DAD1, 1.442 (478 mAU, -) of 002-0101.D
mAU
400
300
200
100
0
EDUV => nm = 205 mAU = 482.638836
EDUV => nm = 273 mAU = 176.88942
EDUV => nm = 245 mAU = 47.297955
200
210
220
230
240
250
260
270
280
290
nm

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\001-0101.D
Sample Name: Branco 1

==========

Acq. Operator : Seq. Line : 1
Acq. Instrument : CR LAIN 05 Location : 1
Injection Date : 31-Oct-17 11:05:03 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M
Last changed : 31-Oct-17 11:04:08 AM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (Sequence Method)
Last changed : 31-Oct-17 11:10:43 AM

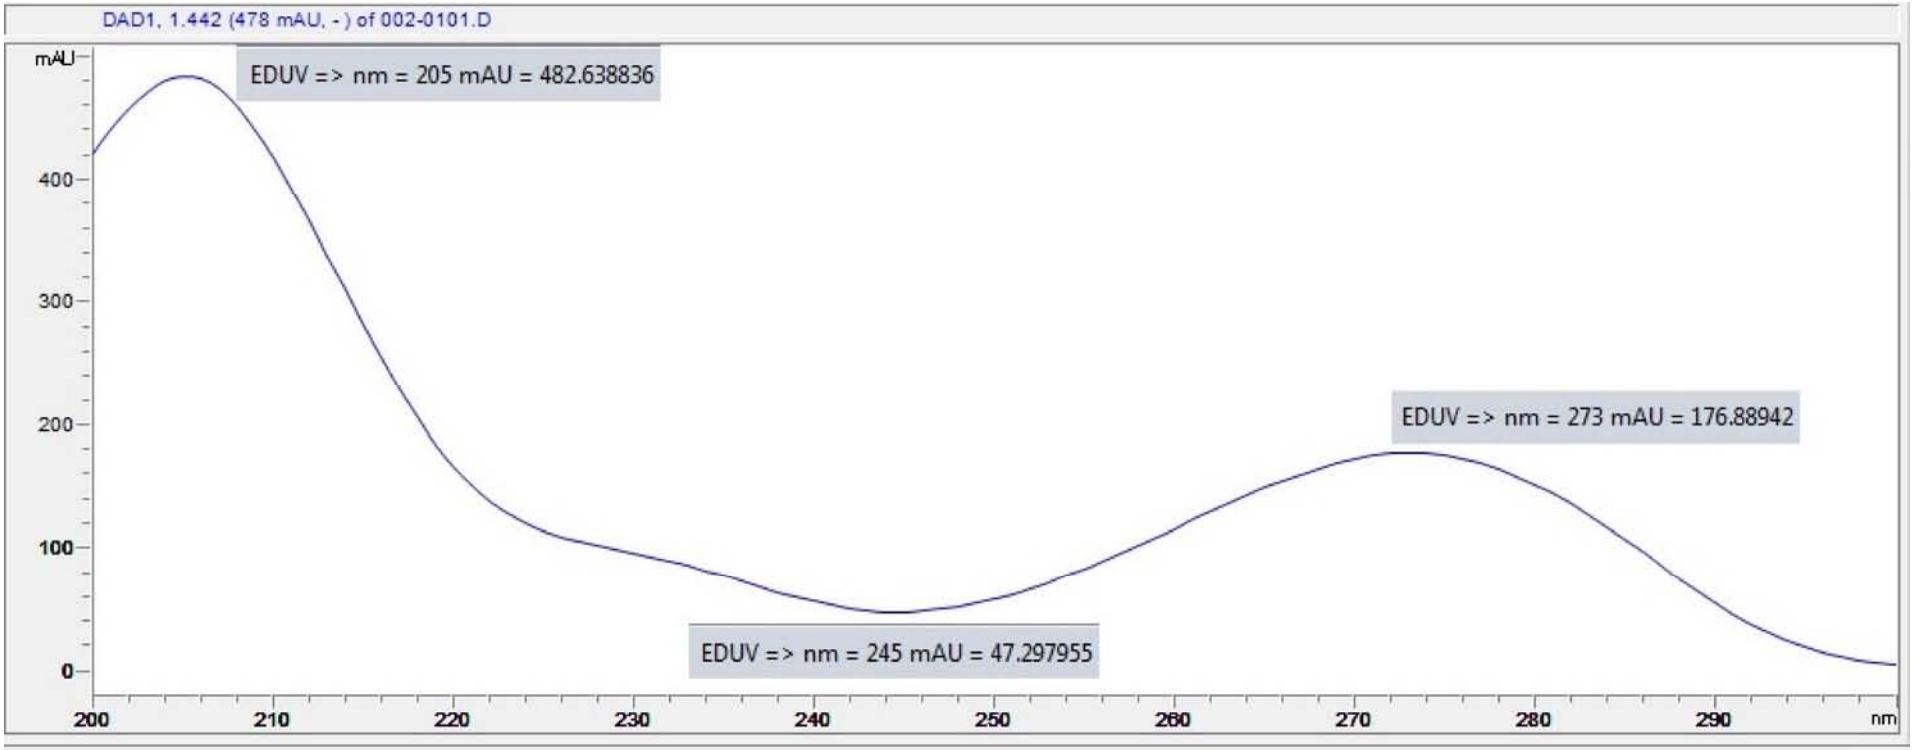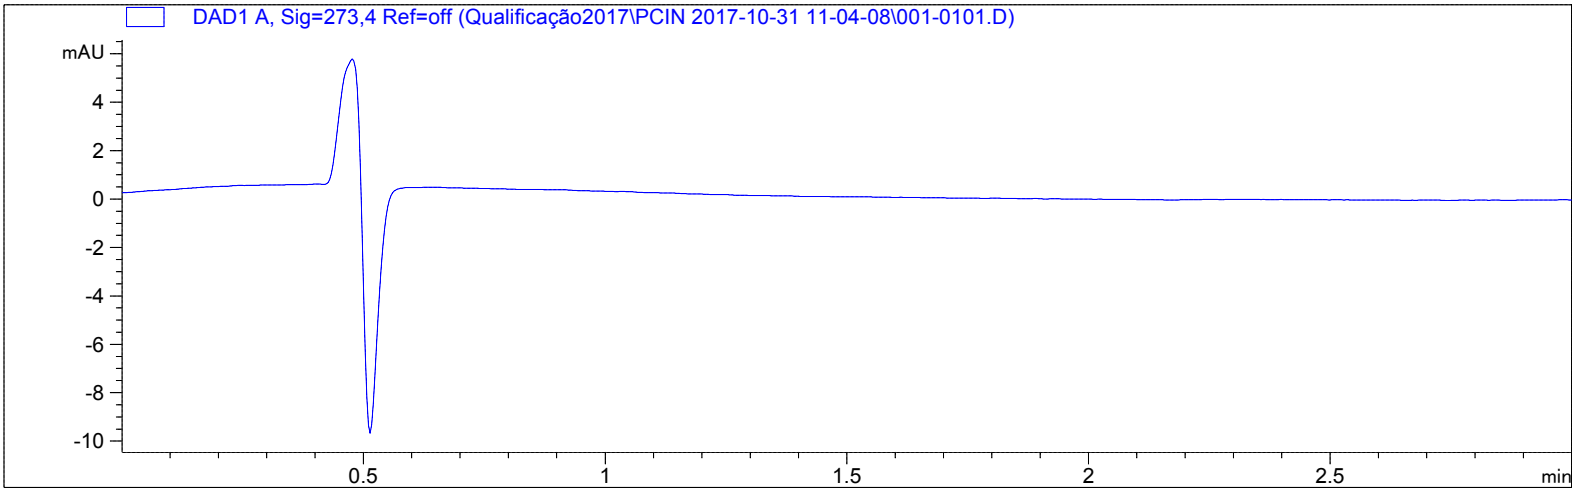

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0201.D
Sample Name: PCIN 1

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   2
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 11:08:57 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M
Last changed    : 31-Oct-17 11:04:08 AM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

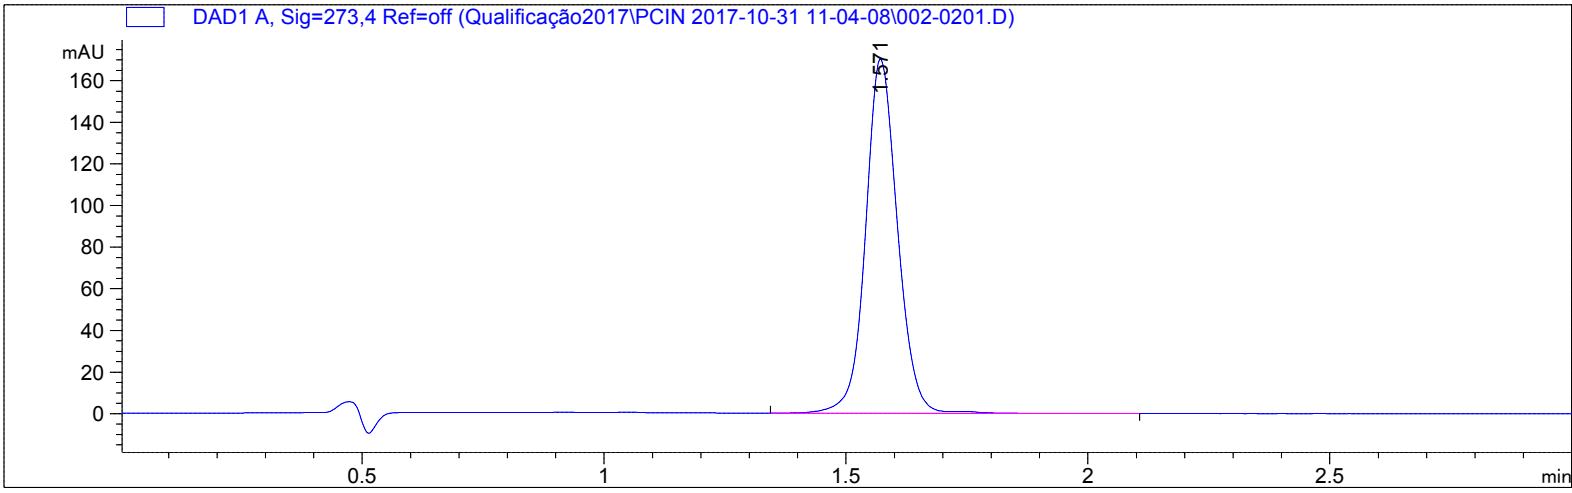


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.571 BB    0.0695  781.09424  170.43628 100.0000

Totals :                   781.09424  170.43628


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0301.D
Sample Name: PCIN 2

```
================================================================================
Acq. Operator   :                                   Seq. Line :   3
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 11:12:51 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

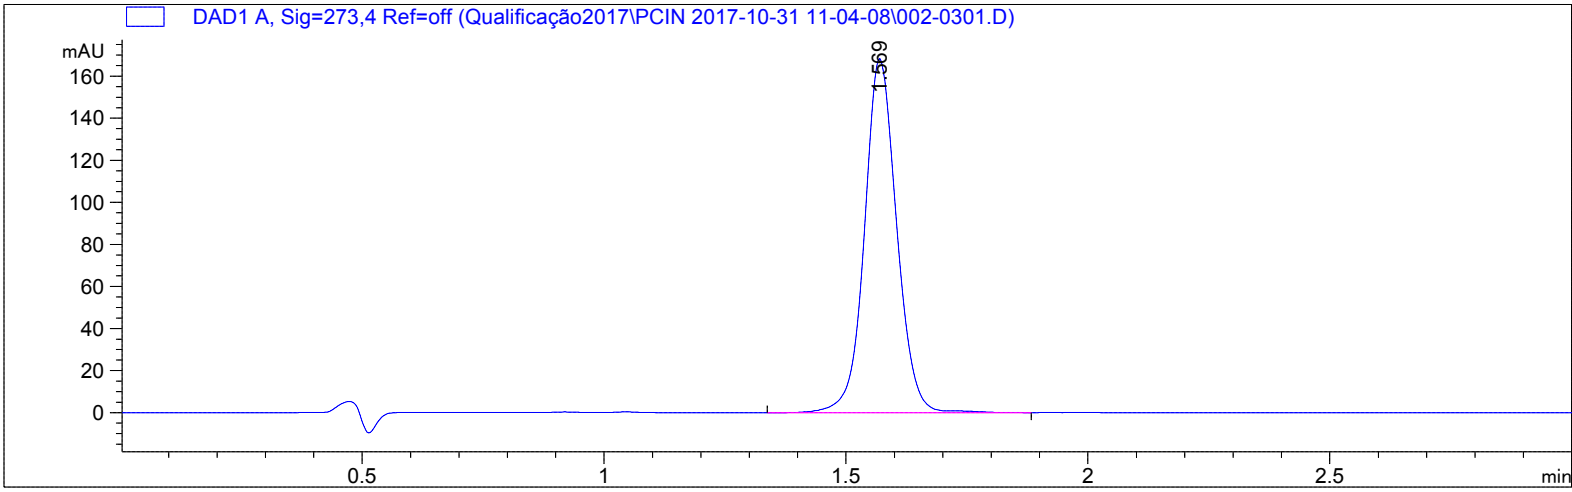


```
================================================================================
                        External Standard Report
================================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
================================================================================
================================================================================
                           Area Percent Report
================================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.569 BB    0.0710  779.76306  168.41364 100.0000

Totals :                   779.76306  168.41364


================================================================================
                           *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0401.D
Sample Name: PCIN 3

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   4
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 11:16:44 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

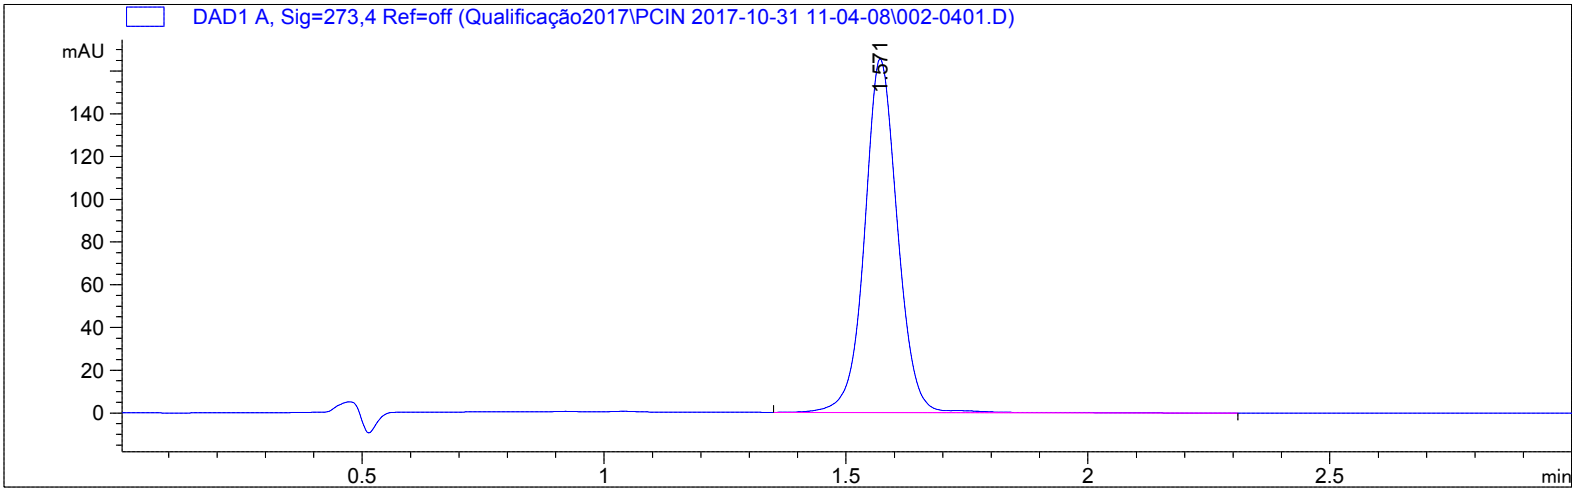


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.571 BB    0.0711  783.23352  165.70146 100.0000


Totals :                   783.23352  165.70146


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\001-0501.D
Sample Name: Branco 2

==========

Acq. Operator	:	Seq. Line :	5
Acq. Instrument	: CR LAIN 05	Location :	1
Injection Date	: 31-Oct-17 11:20:41 AM	Inj :	1
		Inj Volume :	10.000 µl
Method	: C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (Sequence Method)		
Last changed	: 31-Oct-17 11:10:43 AM		

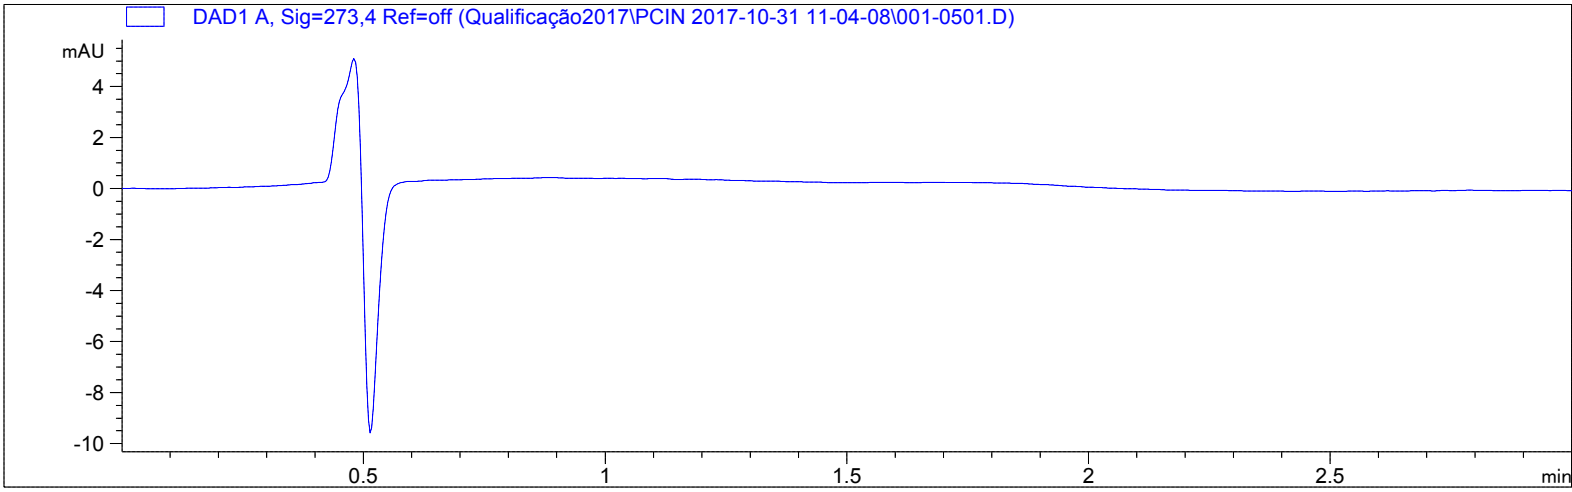

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0601.D
Sample Name: PCIN 4

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   6
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 11:24:35 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

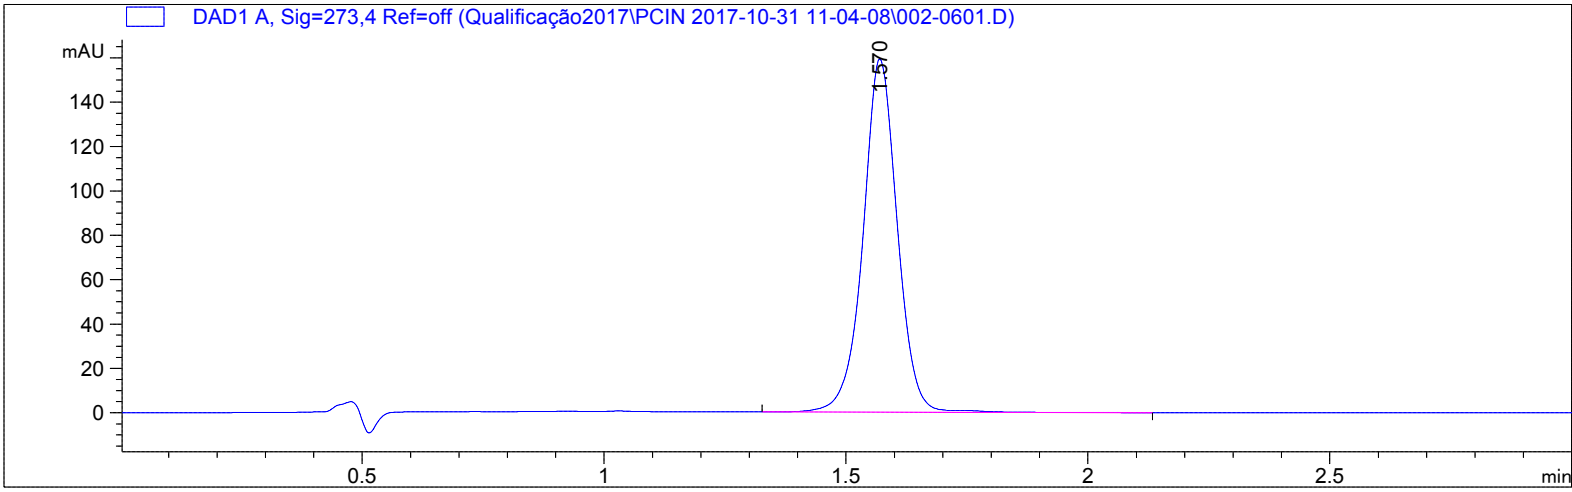


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.570 BB    0.0744  783.70203  159.40085 100.0000

Totals :                   783.70203  159.40085


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0701.D
Sample Name: PCIN 5

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   7
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 11:28:29 AM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

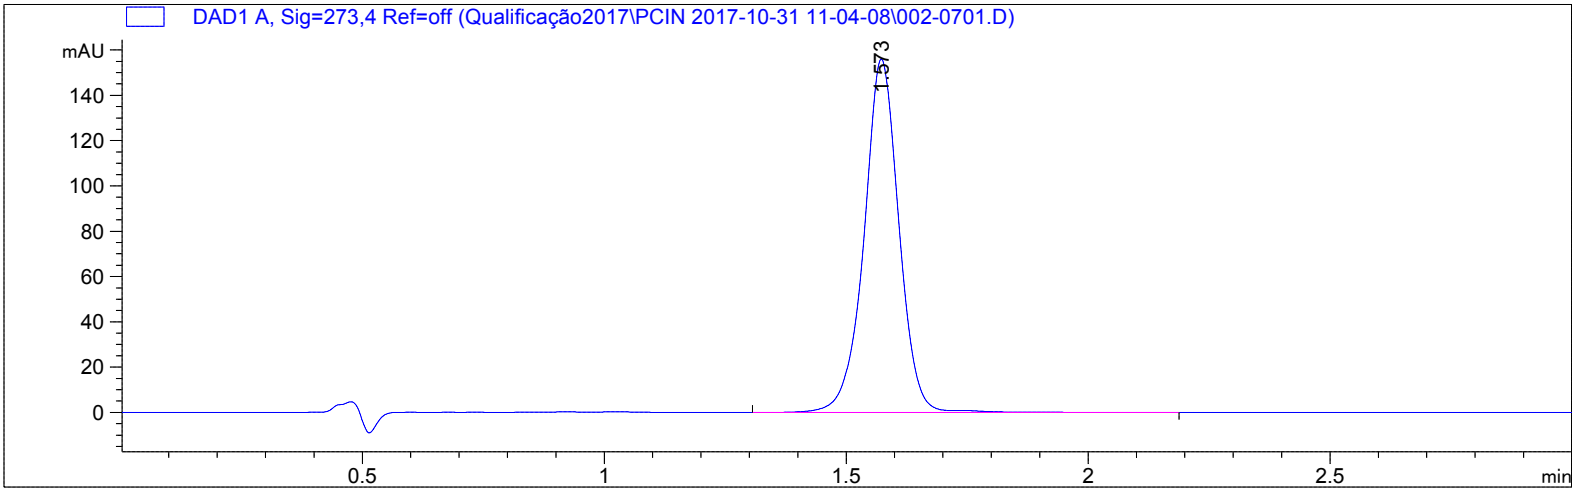


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.573 BB    0.0754  782.41632  156.23517 100.0000

Totals :                   782.41632  156.23517


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\002-0801.D
Sample Name: PCIN 6

```
==========================================================================
Acq. Operator   :                                  Seq. Line :   8
Acq. Instrument : CR LAIN 05                        Location :   2
Injection Date  : 31-Oct-17 11:32:23 AM                Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 11:10:43 AM
```

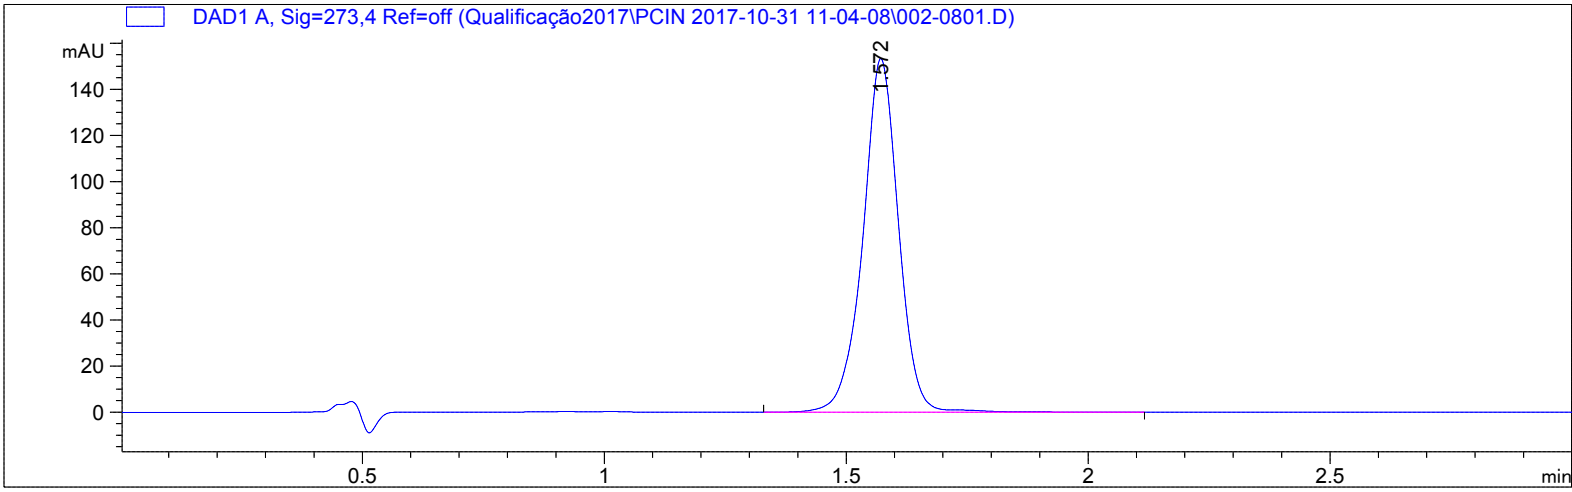


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.572 BB    0.0767  785.11377  153.53421 100.0000


Totals :                   785.11377  153.53421


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\001-0901.D
Sample Name: Branco 3

==========

Acq. Operator	:	Seq. Line :	9
Acq. Instrument	: CR LAIN 05	Location :	1
Injection Date	: 31-Oct-17 11:36:18 AM	Inj :	1
		Inj Volume :	10.000 µl
Method	: C:\Chem32\1\Data\Qualificação2017\PCIN 2017-10-31 11-04-08\Qualificação.M (Sequence Method)		
Last changed	: 31-Oct-17 11:10:43 AM		

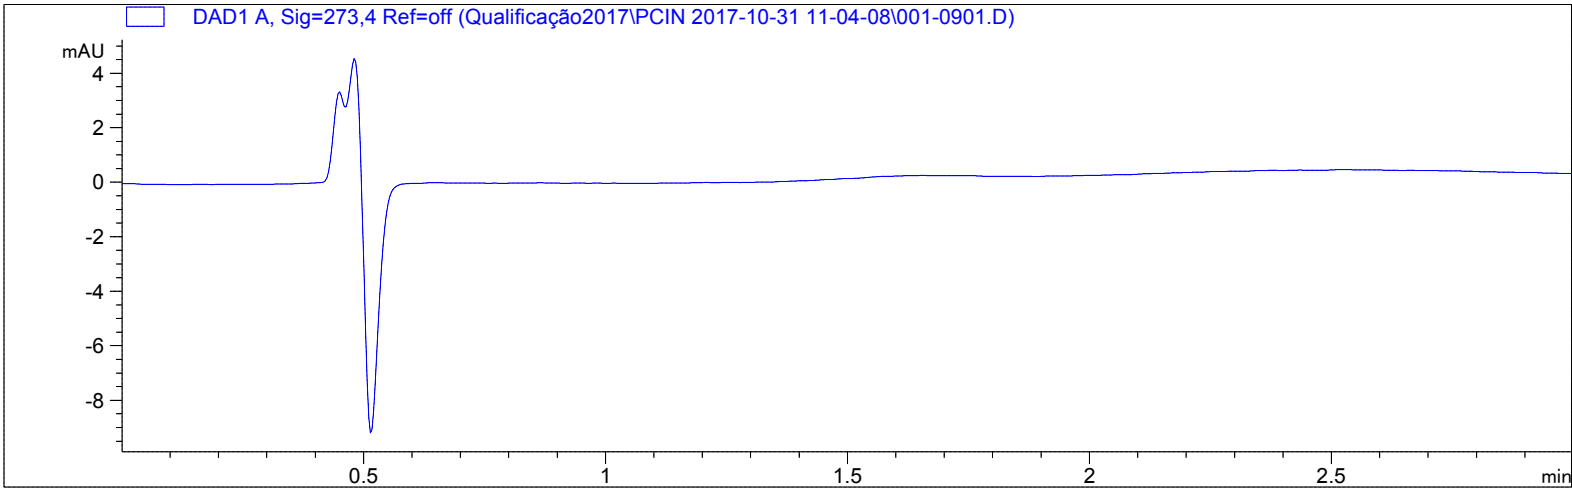

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========


*** End of Report ***

Data File C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\001-0101.D
Sample Name: LDUV 1

==========

Acq. Operator	:	Seq. Line	: 1
Acq. Instrument	: CR LAIN 05	Location	: 1
Injection Date	: 31-Oct-17 12:13:49 PM	Inj	: 1
		Inj Volume	: 10.000 µl

Acq. Method : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M
Last changed : 31-Oct-17 12:12:55 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M (Sequence Method)
Last changed : 31-Oct-17 12:23:16 PM

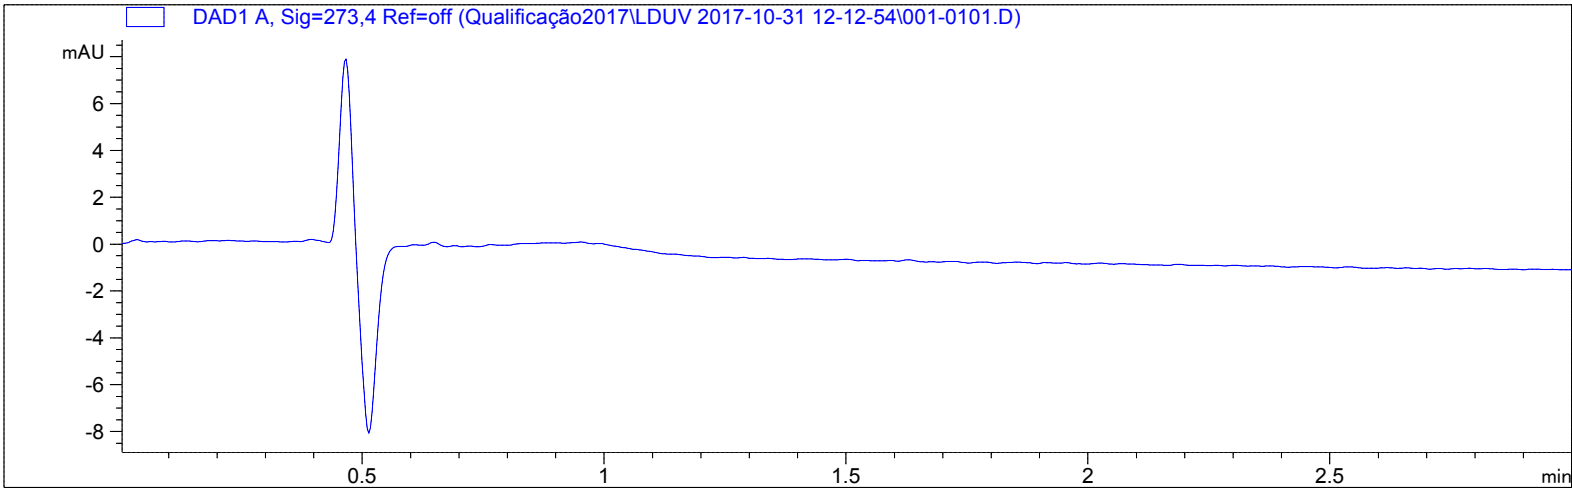

==========

External Standard Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs


No peaks found

==========

*** End of Report ***

Data File C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\002-0201.D
Sample Name: LDUV 2

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   2
Acq. Instrument : CR LAIN 05                         Location :   2
Injection Date  : 31-Oct-17 12:17:44 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M
Last changed    : 31-Oct-17 12:12:55 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:23:16 PM
```

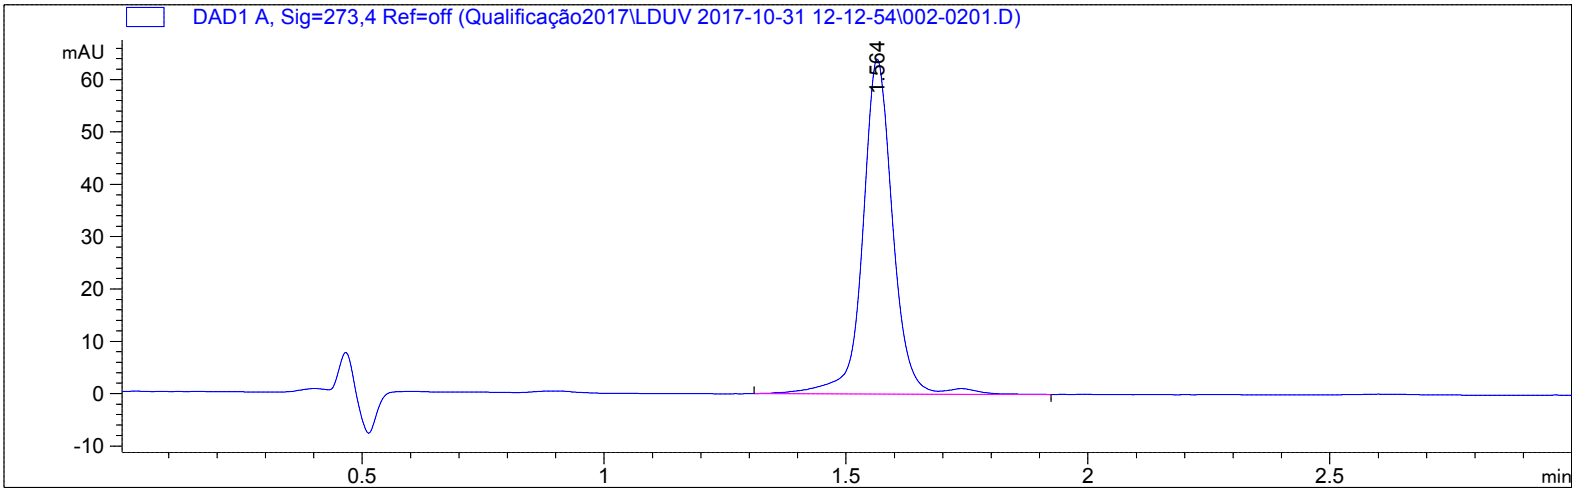


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.564 BV R  0.0655  277.56009   64.09793 100.0000

Totals :                   277.56009   64.09793


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\003-0301.D
Sample Name: LDUV 3

```
==========================================================================
Acq. Operator   :                                  Seq. Line :   3
Acq. Instrument : CR LAIN 05                        Location :   3
Injection Date  : 31-Oct-17 12:21:38 PM                Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M
Last changed    : 31-Oct-17 12:12:55 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:23:16 PM
```

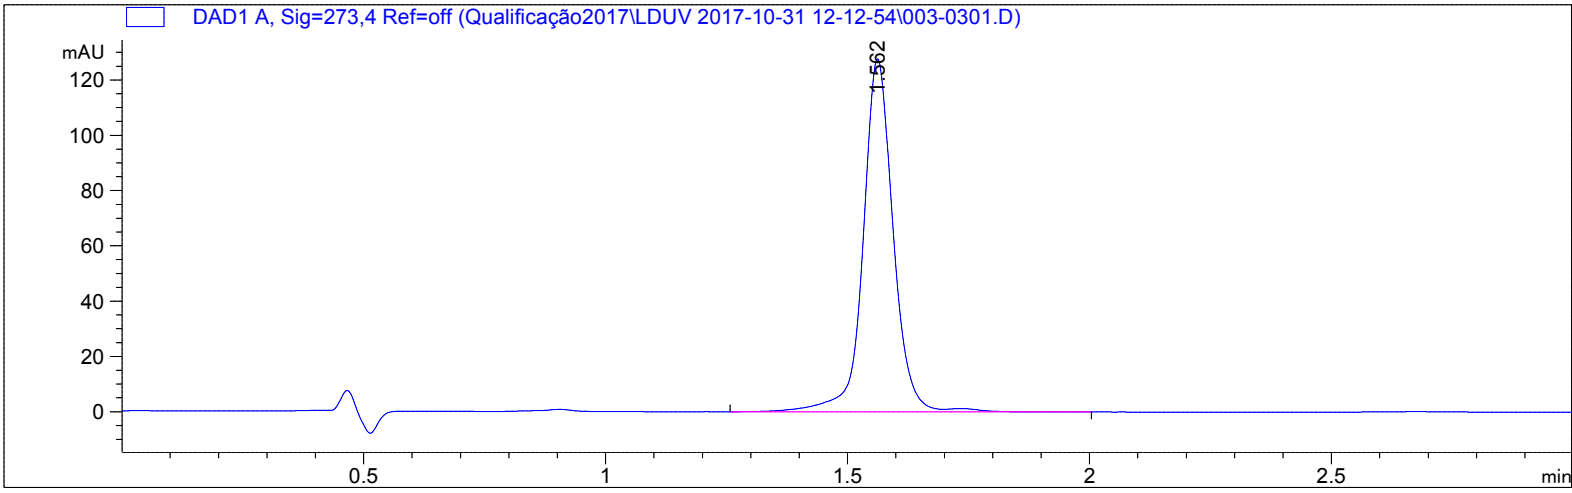


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.562 BV R  0.0647  555.81323  127.86372 100.0000

Totals :                   555.81323  127.86372


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\004-0401.D
Sample Name: LDUV 4

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   4
Acq. Instrument : CR LAIN 05                         Location :   4
Injection Date  : 31-Oct-17 12:25:33 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:23:16 PM
```

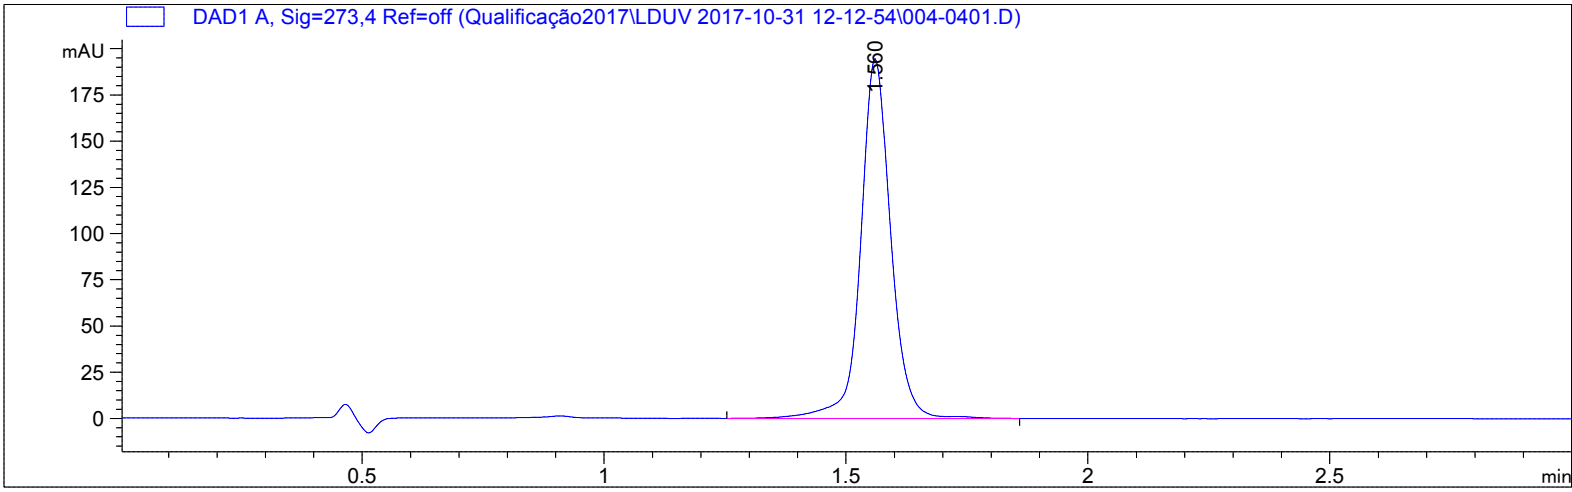


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.560 BB    0.0655  842.56238  194.68935 100.0000

Totals :                   842.56238  194.68935


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\005-0501.D
Sample Name: LDUV 5

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   5
Acq. Instrument : CR LAIN 05                         Location :   5
Injection Date  : 31-Oct-17 12:29:27 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\LDUV 2017-10-31 12-12-54\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:23:16 PM
```

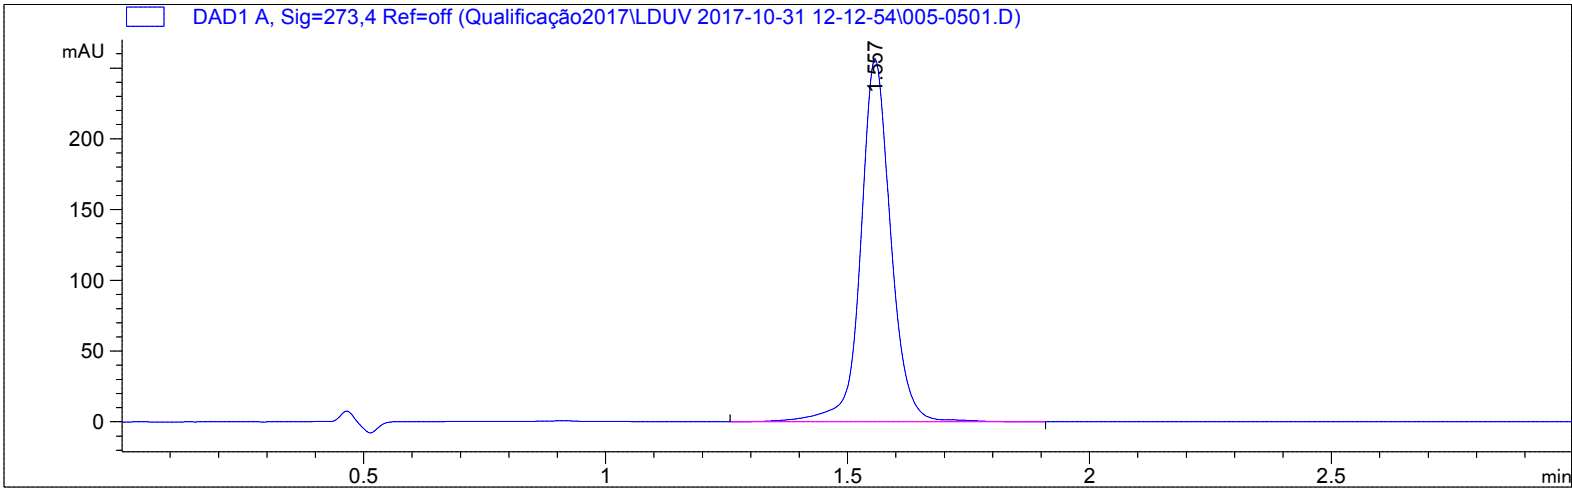


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.557 BB    0.0656 1112.66528  256.63071 100.0000

Totals :                  1112.66528  256.63071


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\001-0101.D
Sample Name: LIIN 1

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   1
Acq. Instrument : CR LAIN 05                         Location :   1
Injection Date  : 31-Oct-17 12:42:35 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.100 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M
Last changed    : 31-Oct-17 12:41:42 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:50:02 PM
```

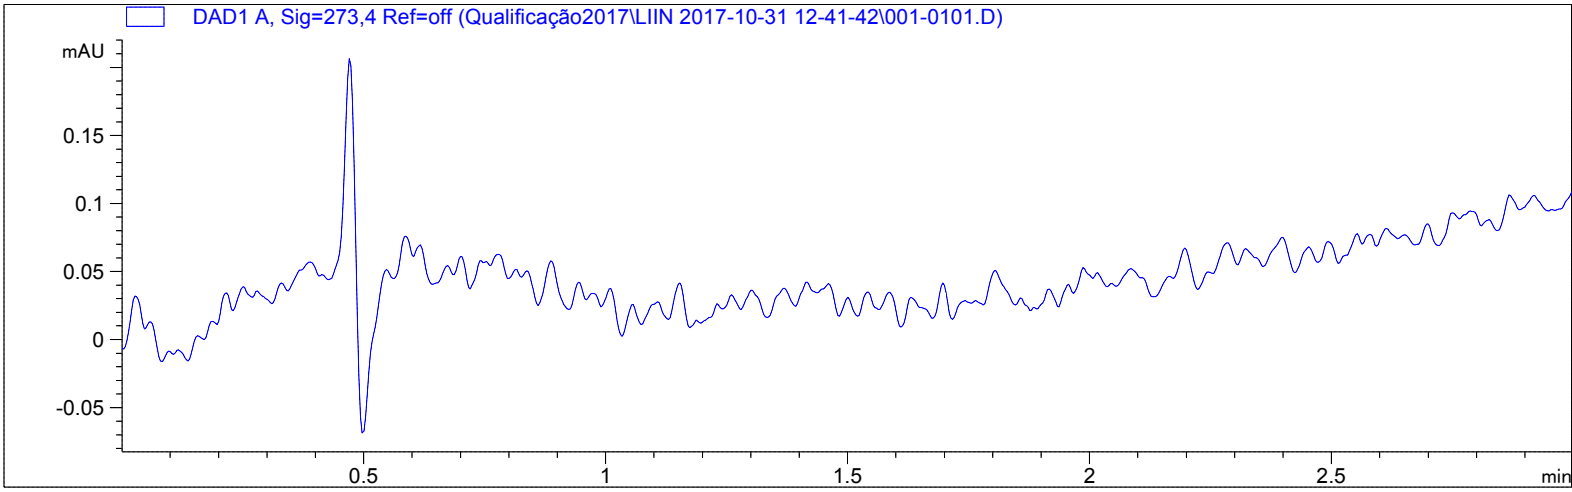


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\001-0201.D
Sample Name: LIIN 2

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   2
Acq. Instrument : CR LAIN 05                         Location :   1
Injection Date  : 31-Oct-17 12:46:27 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 5.000 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M
Last changed    : 31-Oct-17 12:41:42 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:50:02 PM
```

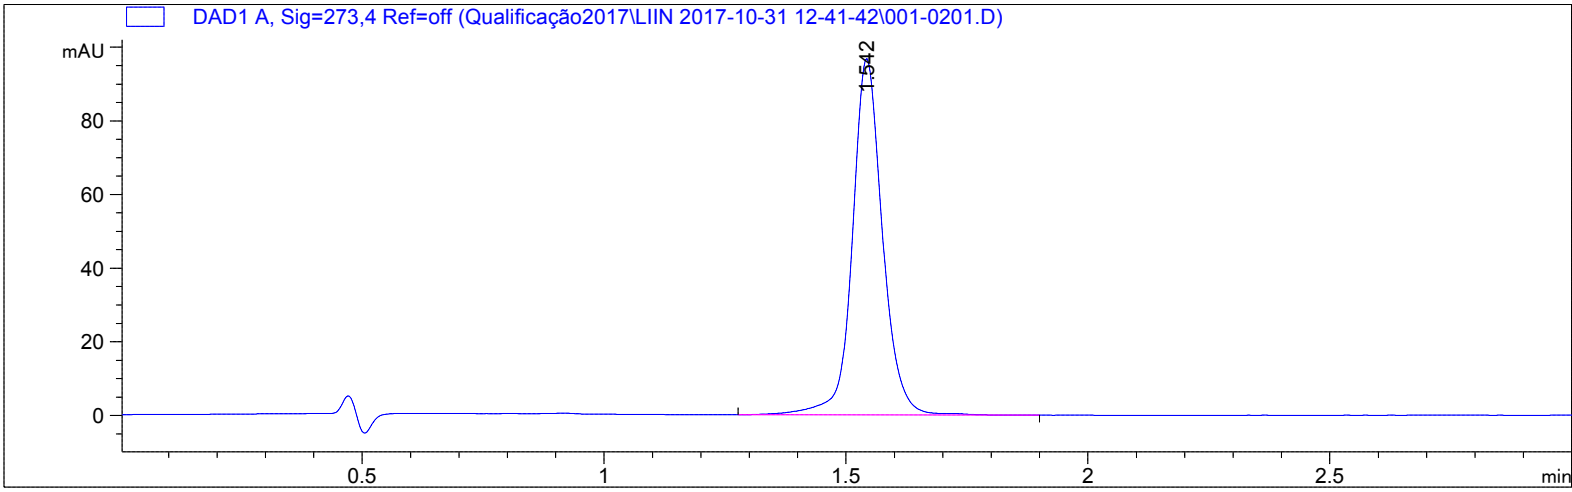


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                        Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.542 BB    0.0658  421.45129   96.81933 100.0000

Totals :                   421.45129   96.81933


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\001-0301.D
Sample Name: LIIN 3

```
==========================================================================
Acq. Operator   :                                  Seq. Line :   3
Acq. Instrument : CR LAIN 05                        Location :   1
Injection Date  : 31-Oct-17 12:50:21 PM                 Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M
Last changed    : 31-Oct-17 12:41:42 PM
Analysis Method : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:50:02 PM
```

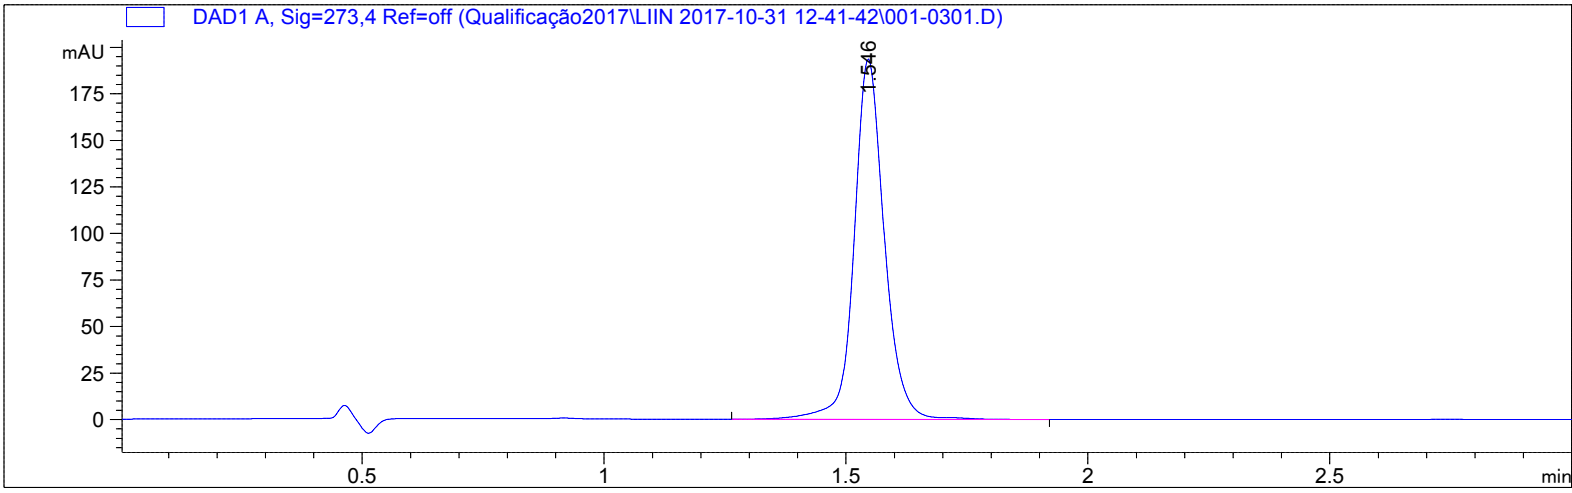


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.546 BB    0.0657  841.73480  193.65720 100.0000

Totals :                   841.73480  193.65720


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\001-0401.D
Sample Name: LIIN 4

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   4
Acq. Instrument : CR LAIN 05                         Location :   1
Injection Date  : 31-Oct-17 12:54:16 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 15.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:50:02 PM
```

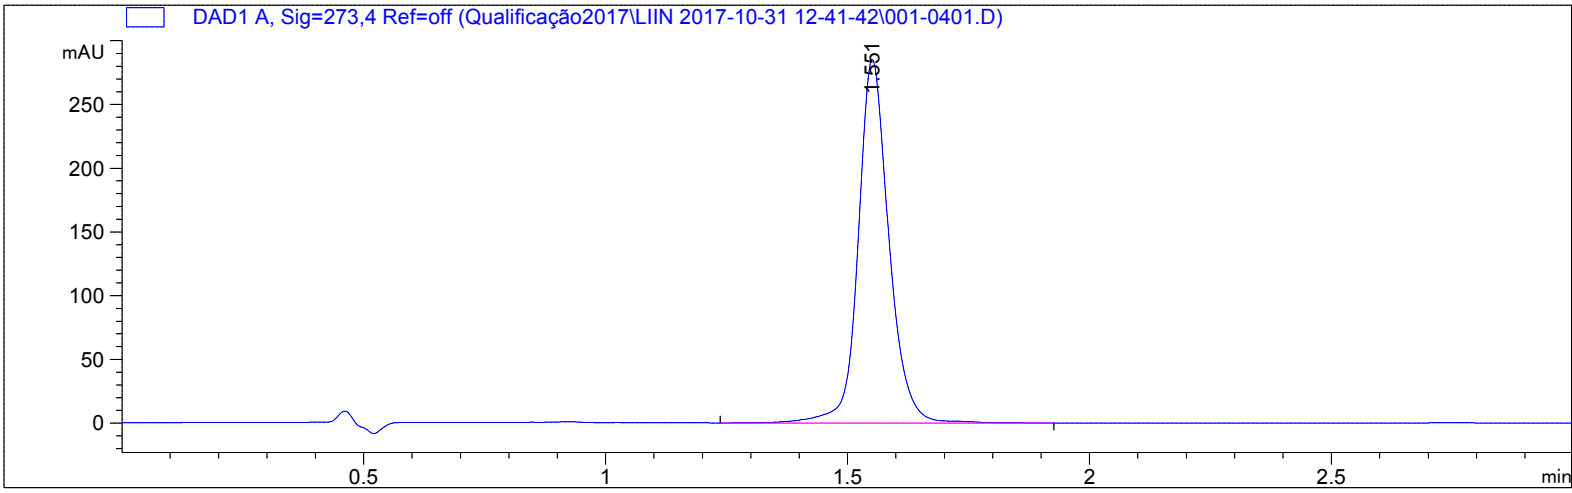


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.551 BB    0.0666 1263.31177  285.52338 100.0000

Totals :                  1263.31177  285.52338


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\001-0501.D
Sample Name: LIIN 5

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   5
Acq. Instrument : CR LAIN 05                         Location :   1
Injection Date  : 31-Oct-17 12:58:14 PM                  Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 20.000 µl
Method          : C:\Chem32\1\Data\Qualificação2017\LIIN 2017-10-31 12-41-42\Qualificação.M (
                  Sequence Method)
Last changed    : 31-Oct-17 12:50:02 PM
```

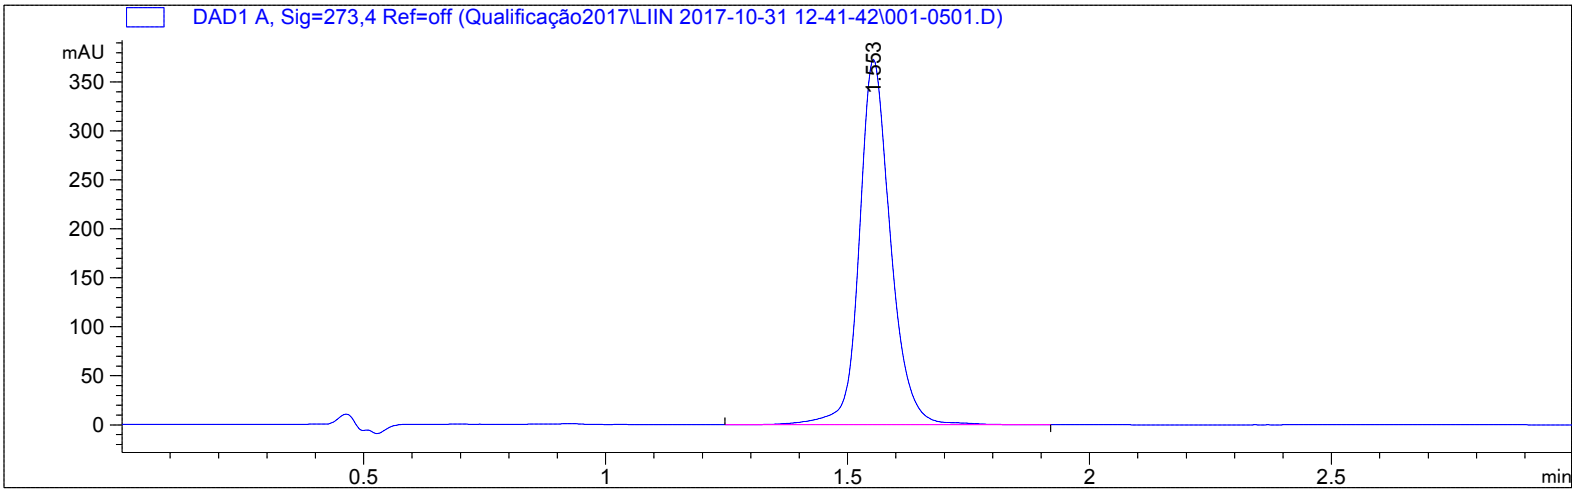


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=273,4 Ref=off


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]   [mAU*s]     [mAU]       %
----|-------|----|-------|----------|----------|--------|
   1   1.553 BB    0.0676 1682.91858  373.24753 100.0000

Totals :                  1682.91858  373.24753


==========================================================================
                         *** End of Report ***
```

Data File C:\Chem32\1\Data\Qualificação2017\Grad AB 2017-10-31 13-24-37\001-0101.D
Sample Name: Grad AB

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   1
Acq. Instrument : CR LAIN 05                         Location :   1
Injection Date  : 31-Oct-17 1:25:32 PM                    Inj :   1
                                                  Inj Volume : 10.000 µl
Different Inj Volume from Sample Entry!  Actual Inj Volume : 0.100 µl
Method          : C:\Chem32\1\Data\Qualificação2017\Grad AB 2017-10-31 13-24-37\Grad AB.M (
                  Sequence Method)
Last changed    : 31-Oct-17 1:24:37 PM
```

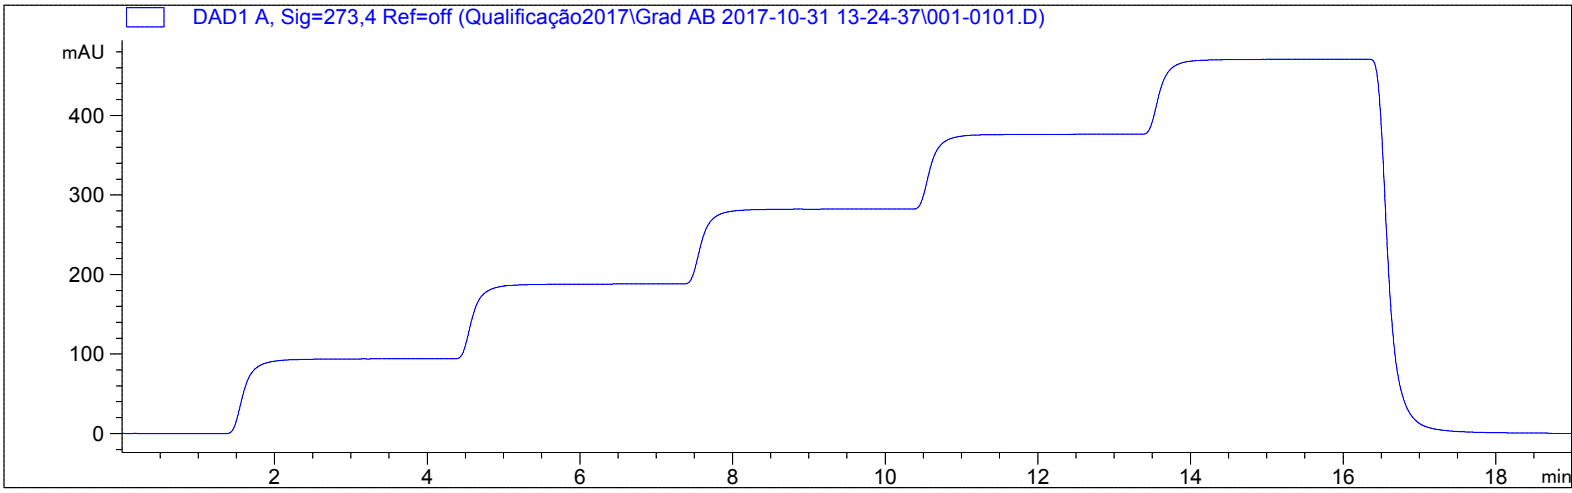


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
==========================================================================
==========================================================================
                         Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\001-0101.D
Sample Name: LDRI 1

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   1
Acq. Instrument : CR LAIN 05 RID                     Location :   1
Injection Date  : 01-Nov-17 8:07:08 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
Last changed    : 01-Nov-17 8:06:05 AM
Analysis Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
                  (Sequence Method)
Last changed    : 01-Nov-17 8:20:12 AM
Additional Info : Peak(s) manually integrated
```

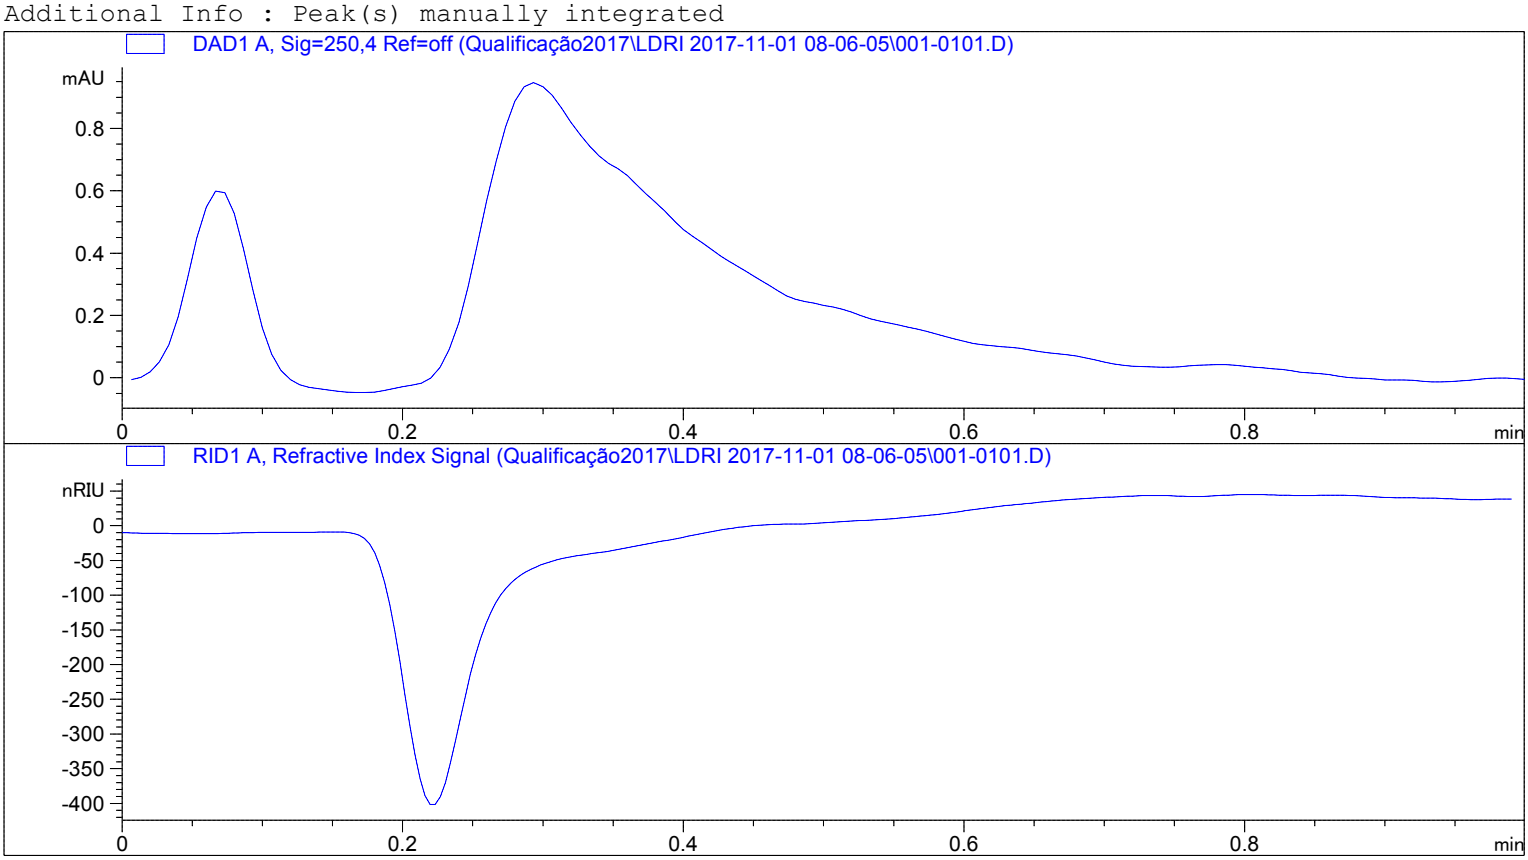


```
==========================================================================
                          Area Percent Report
==========================================================================


Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs

No peaks found

==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\002-0201.D
Sample Name: LDRI 2

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   2
Acq. Instrument : CR LAIN 05 RID                     Location :   2
Injection Date  : 01-Nov-17 8:09:09 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
Last changed    : 01-Nov-17 8:06:05 AM
Analysis Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
                  (Sequence Method)
Last changed    : 01-Nov-17 8:20:12 AM
```

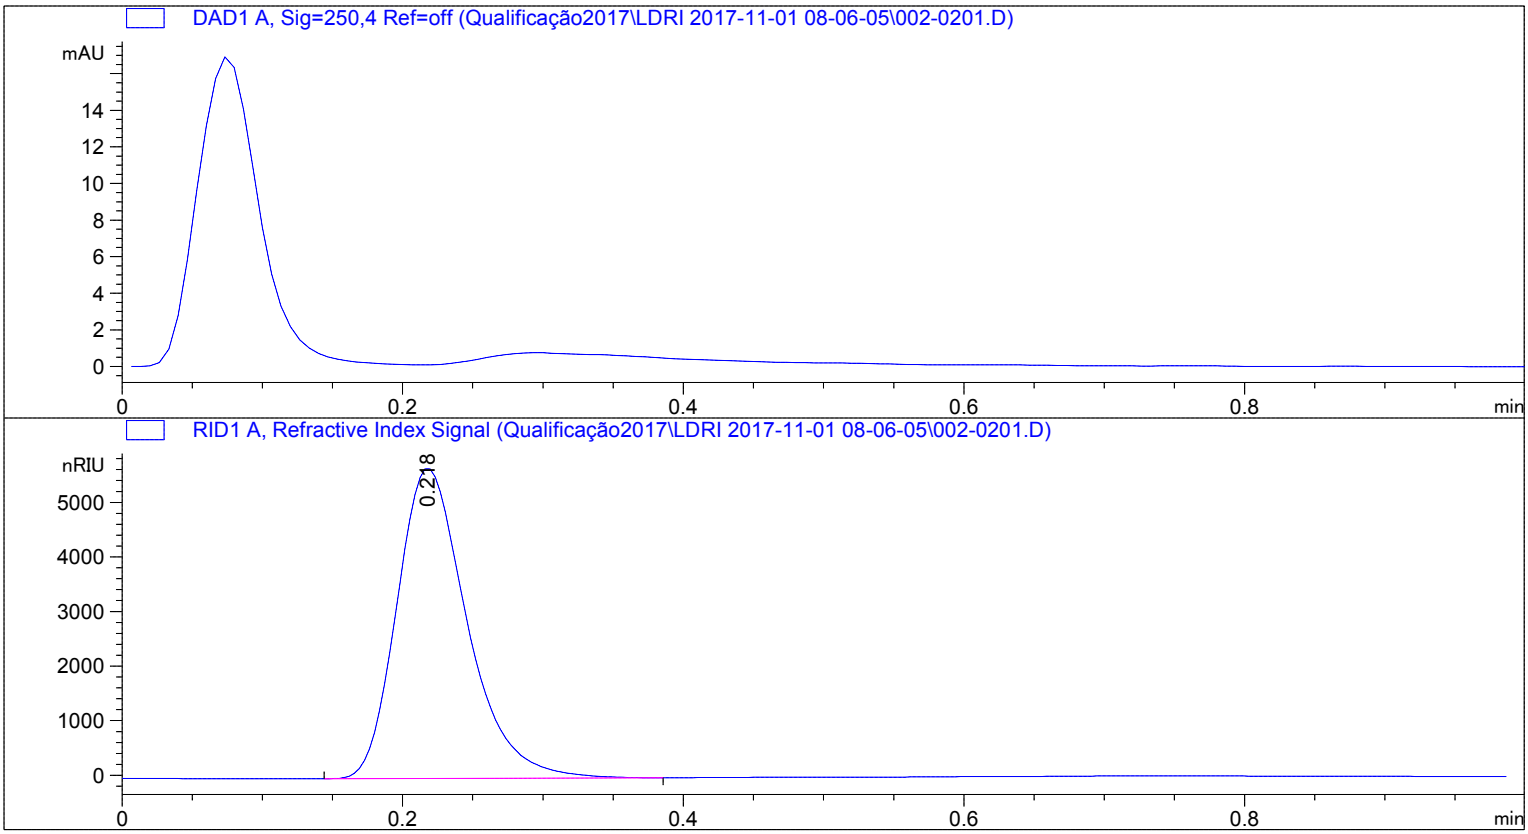


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=250,4 Ref=off


Signal 2: RID1 A, Refractive Index Signal

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]  [nRIU*s]    [nRIU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.218 BB    0.0534 1.97201e4  5692.79541 100.0000


Totals :                  1.97201e4  5692.79541


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\003-0301.D
Sample Name: LDRI 3

==========

Acq. Operator : Seq. Line : 3
Acq. Instrument : CR LAIN 05 RID Location : 3
Injection Date : 01-Nov-17 8:11:09 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
Last changed : 01-Nov-17 8:06:05 AM
Analysis Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
(Sequence Method)
Last changed : 01-Nov-17 8:20:12 AM

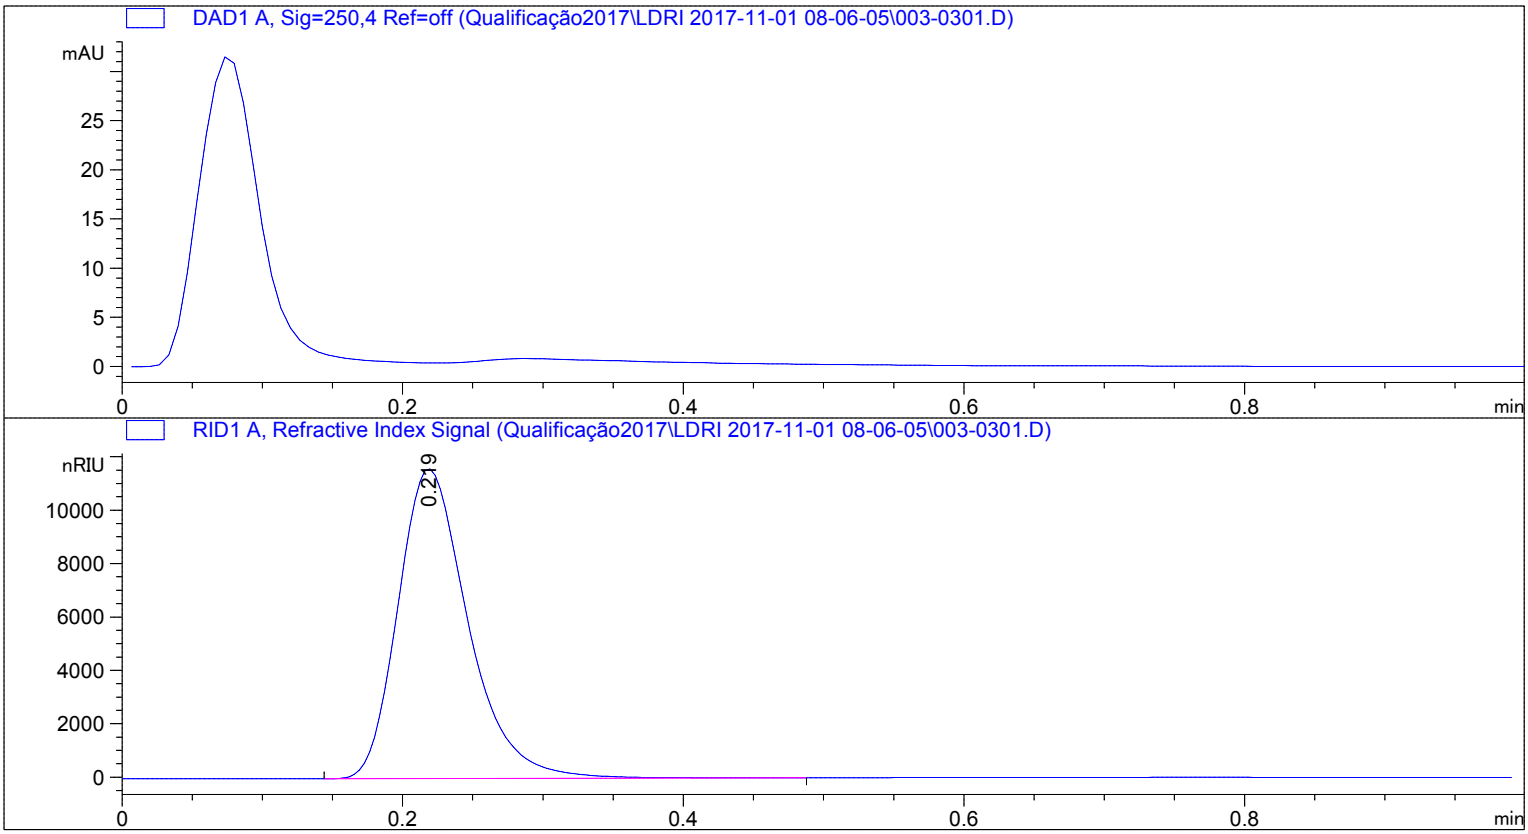

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=250,4 Ref=off

Signal 2: RID1 A, Refractive Index Signal


Peak #	RetTime [min]	Type	Width [min]	Area [nRIU*s]	Height [nRIU]	Area %
1	0.219	BV R	0.0534	4.02481e4	1.16129e4	100.0000
Totals :				4.02481e4	1.16129e4	

==========

*** End of Report ***

Data File C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\004-0401.D
Sample Name: LDRI 4

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   4
Acq. Instrument : CR LAIN 05 RID                     Location :   4
Injection Date  : 01-Nov-17 8:13:09 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
Last changed    : 01-Nov-17 8:06:05 AM
Analysis Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
                  (Sequence Method)
Last changed    : 01-Nov-17 8:20:12 AM
```

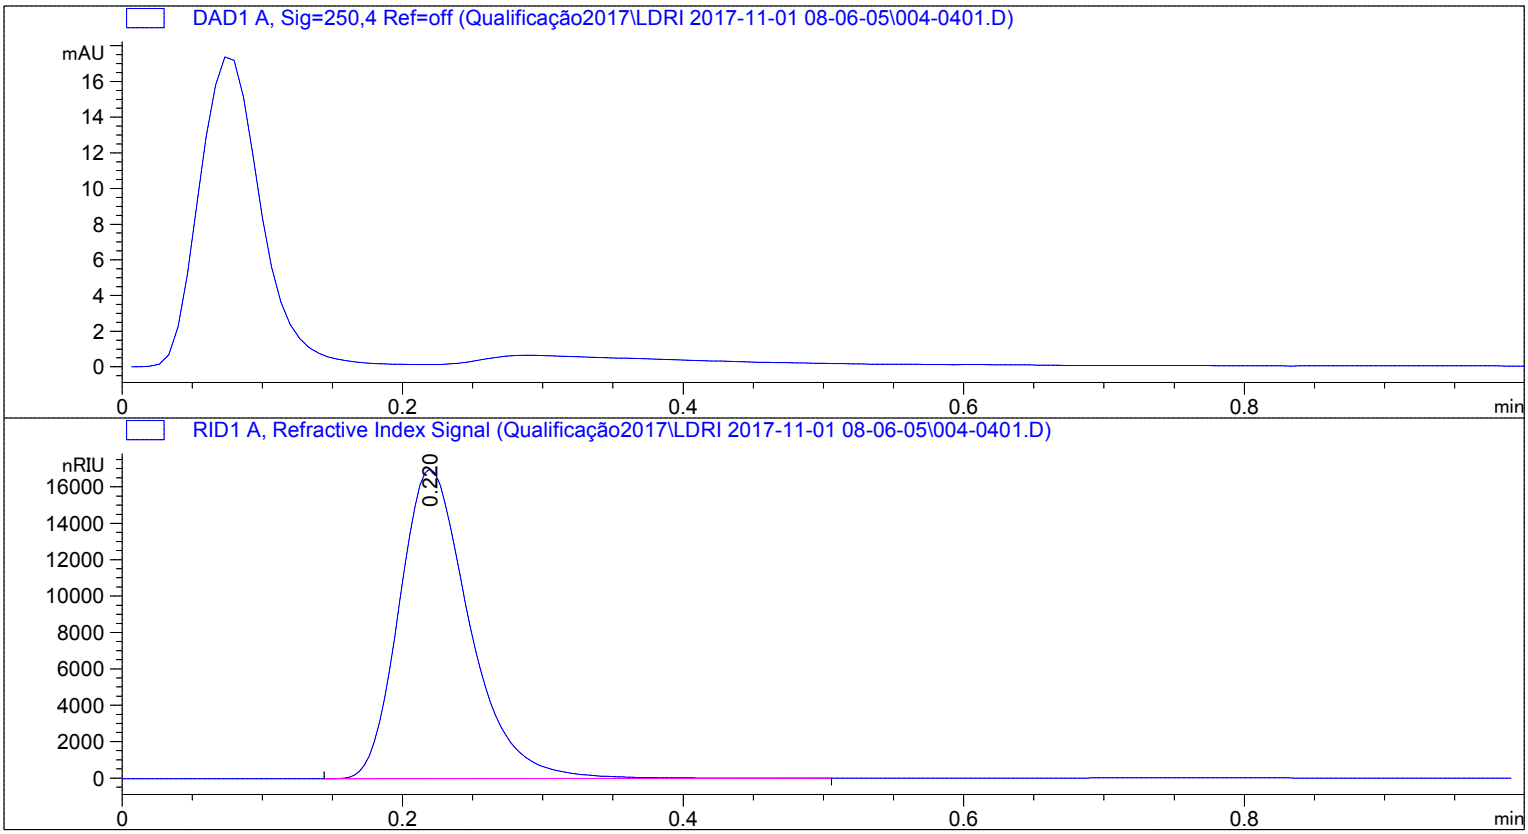


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=250,4 Ref=off


Signal 2: RID1 A, Refractive Index Signal


Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]  [nRIU*s]    [nRIU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.220 BB    0.0535 5.91236e4  1.70288e4  100.0000

Totals :                  5.91236e4  1.70288e4


==========================================================================
                          *** End of Report ***
```

Data File C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\005-0501.D
Sample Name: LDRI 5

```
==========================================================================
Acq. Operator   :                                   Seq. Line :   5
Acq. Instrument : CR LAIN 05 RID                     Location :   5
Injection Date  : 01-Nov-17 8:15:10 AM                   Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
Last changed    : 01-Nov-17 8:14:02 AM
Analysis Method : C:\Chem32\3\Data\Qualificação2017\LDRI 2017-11-01 08-06-05\QualificaçãoRI.M
                  (Sequence Method)
Last changed    : 01-Nov-17 8:20:12 AM
```

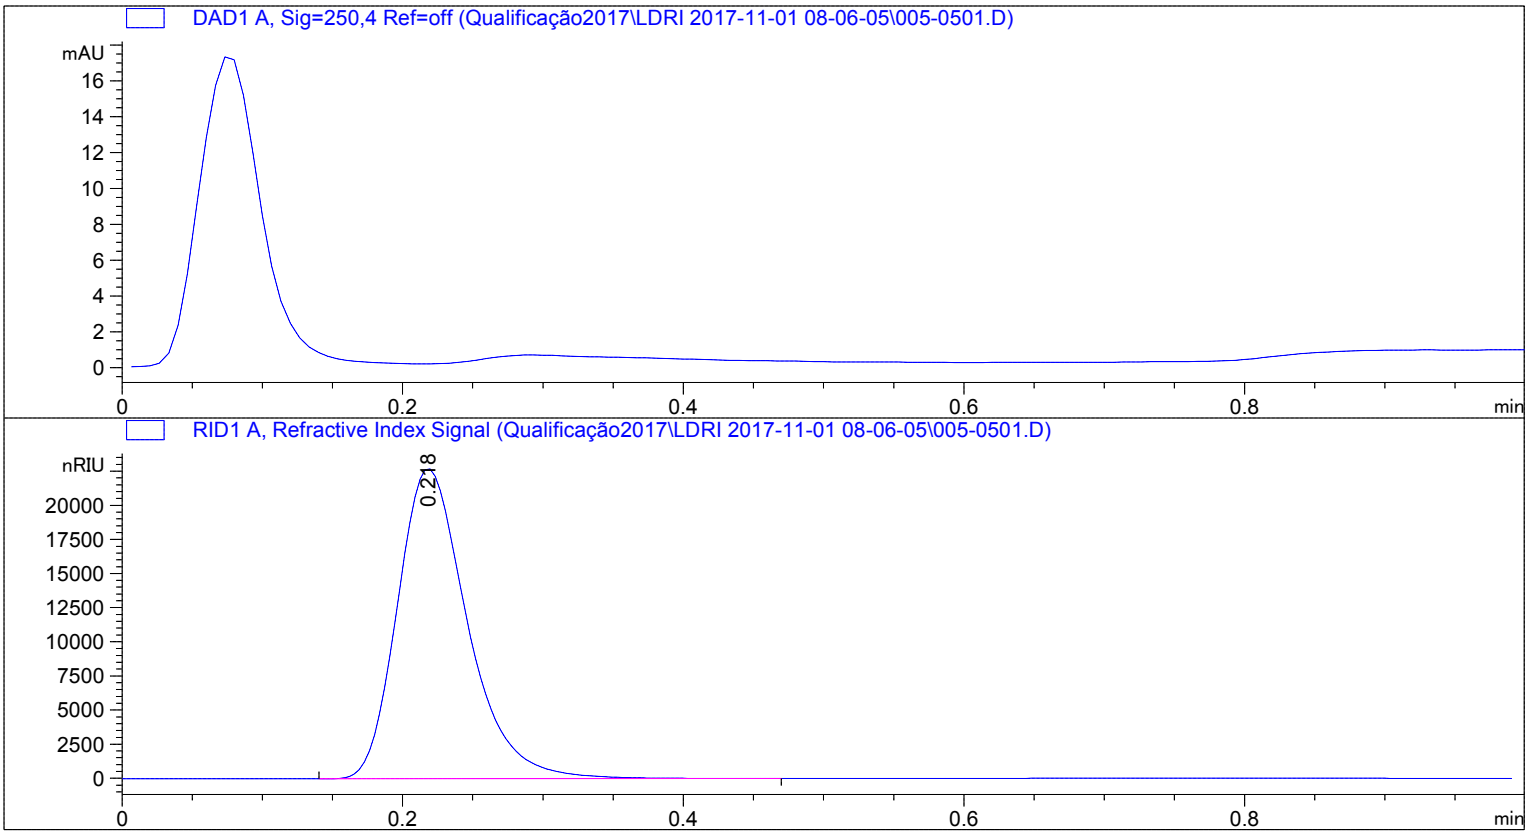


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: DAD1 A, Sig=250,4 Ref=off


Signal 2: RID1 A, Refractive Index Signal

Peak RetTime Type  Width     Area      Height     Area
  #   [min]        [min]  [nRIU*s]    [nRIU]       %
----|-------|----|-------|----------|----------|--------|
   1   0.218 BB    0.0533 7.86548e4  2.27464e4  100.0000

Totals :                  7.86548e4  2.27464e4


==========================================================================
                          *** End of Report ***
```