
Peak Find - EDUV.jws

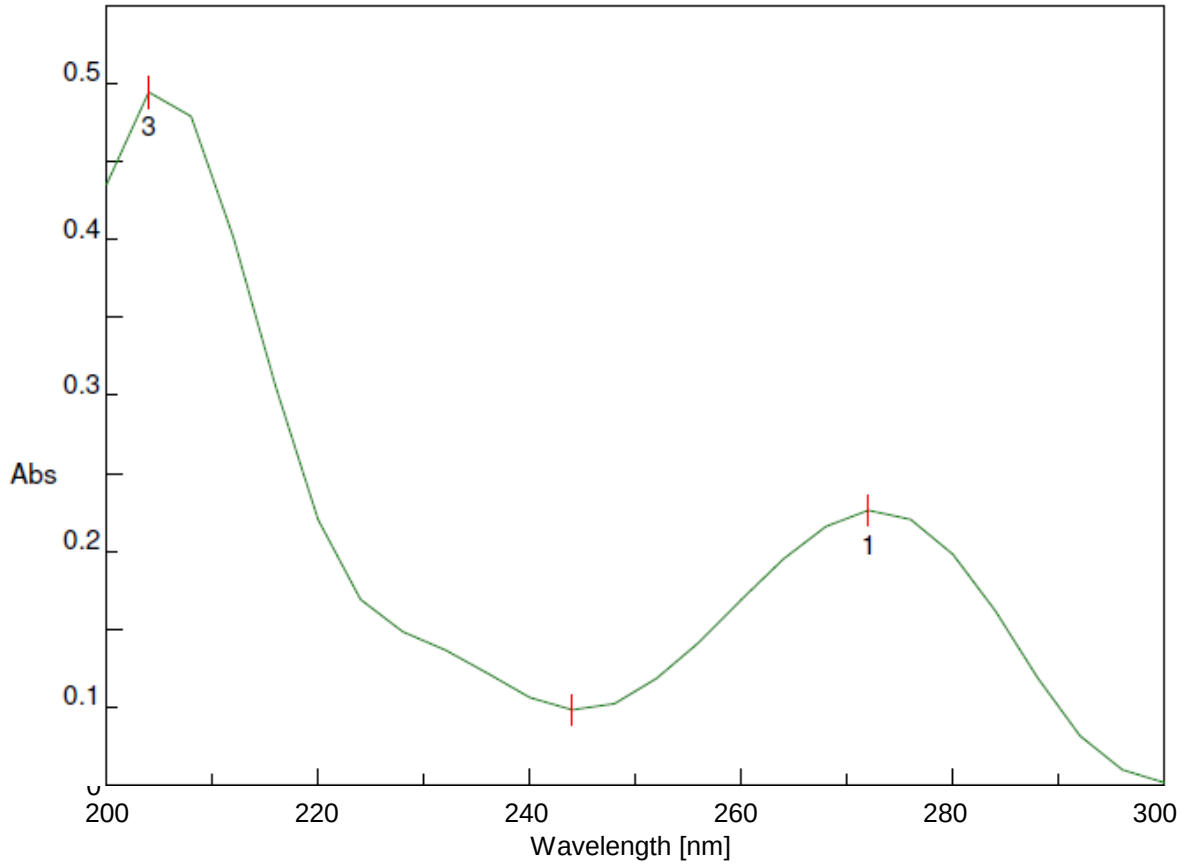

[Comments]

User	QPackSA
Division	---
Company	ALC
Creation date	25/04/2023 10:59
Date modified	25/04/2023 11:00

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	201

[Measurement Information]


Instrument Name	UV-1575
Model Name	UV-1575
Serial No.	XXXXX
ROM version	V1.20

[Result of Peak Picking]


No.	Position	Intensity	No.	Position	Intensity
1	272	0.170623	2	244	0.043017
3	204	0.4450144			

Relatório SRELB

Detector UV – UV-1575 – N/S A114560681	Data: 25/04/2023
Ruído:	
Valor máximo: -1930.9 mAU	**Diferença: 17.50 mAU**
Valor mínimo: -1913.4 mAU	

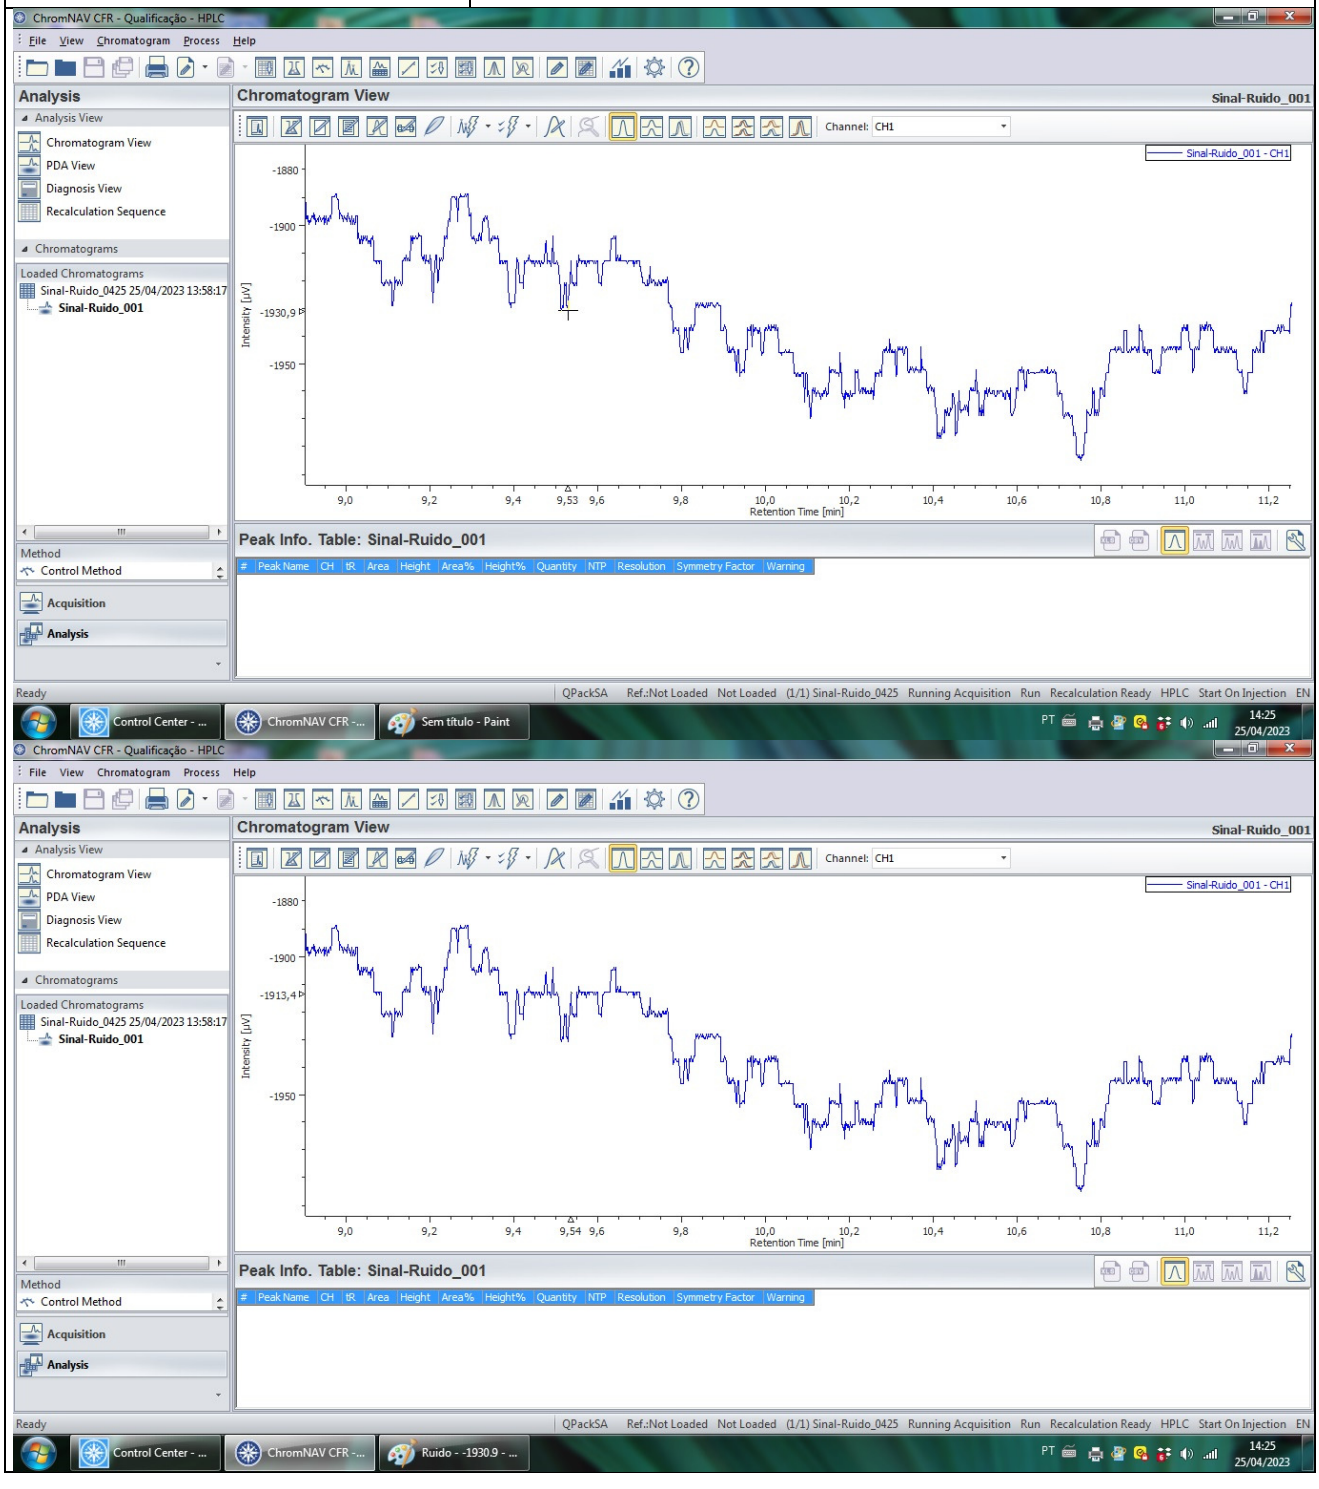


Estabilidade da Linha de Base:	
Valor máximo: -2008.3 mAU	**Diferença (em 20 minutos): 156.0 mAU**
Valor mínimo: -1852.3 mAU	**Diferença (em 60 minutos): 156.0 x 3 = 468 mAU**

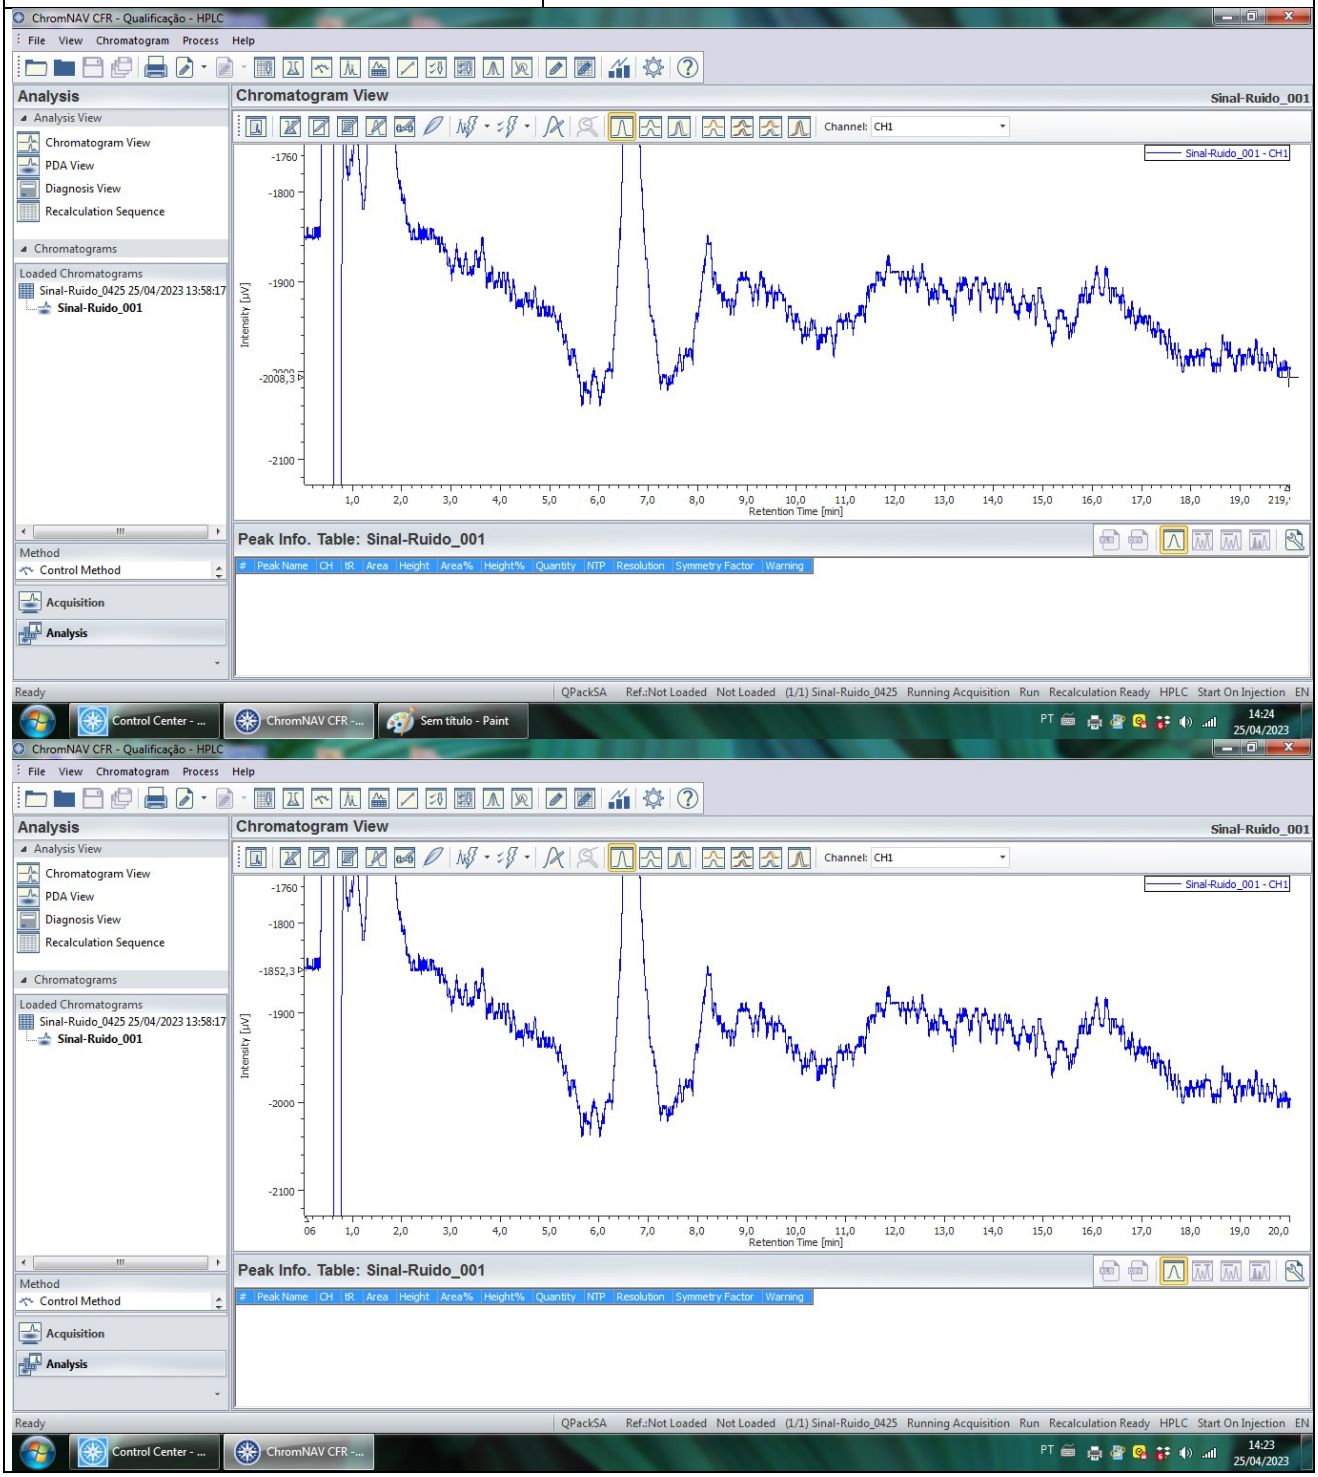


Altura do Pico:

Valor: 120388.4 mAU

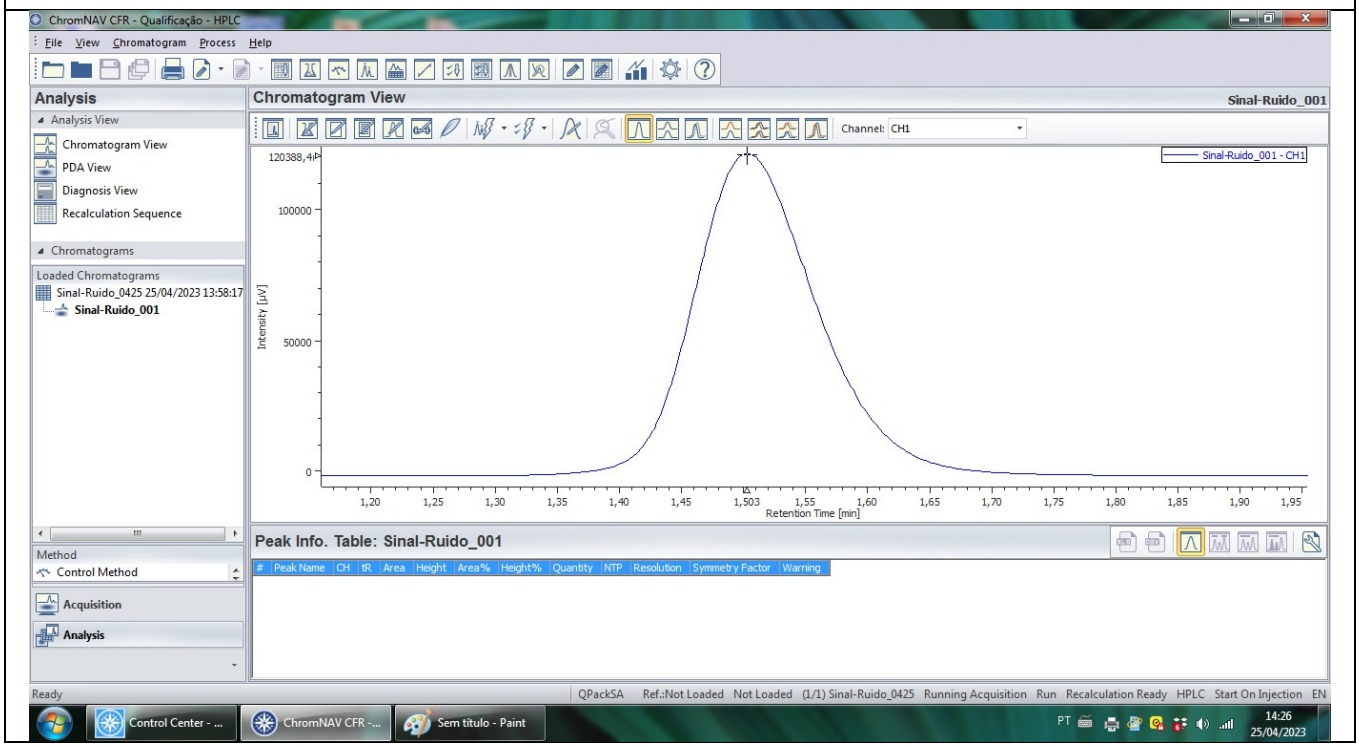

Chromatogram

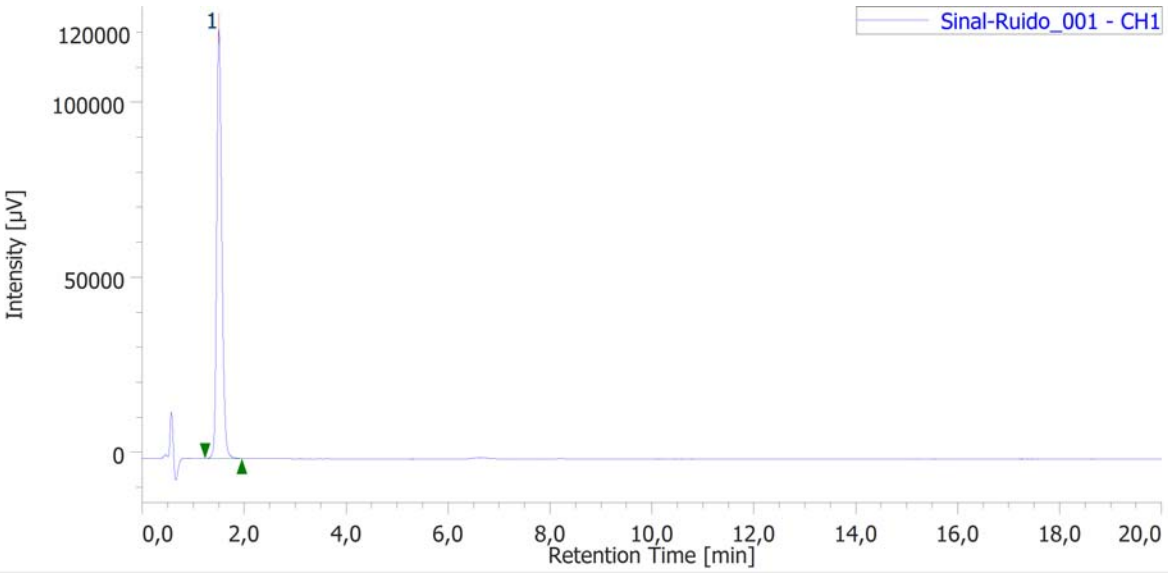

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 14:28:36
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 14:00:53
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal-Ruido_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,503	854041	122628	100,000	100,000	N/A	1131	N/A	1,233	

Creator QPackSA
Reviewer
Approver

Chromatogram

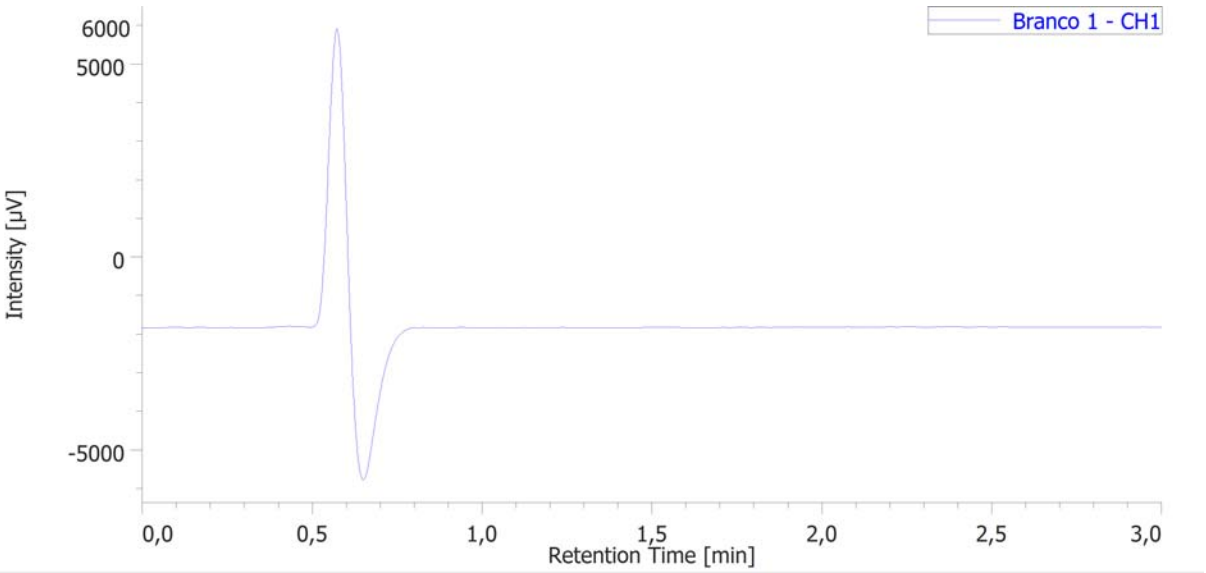


Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:02:05
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:31:19
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

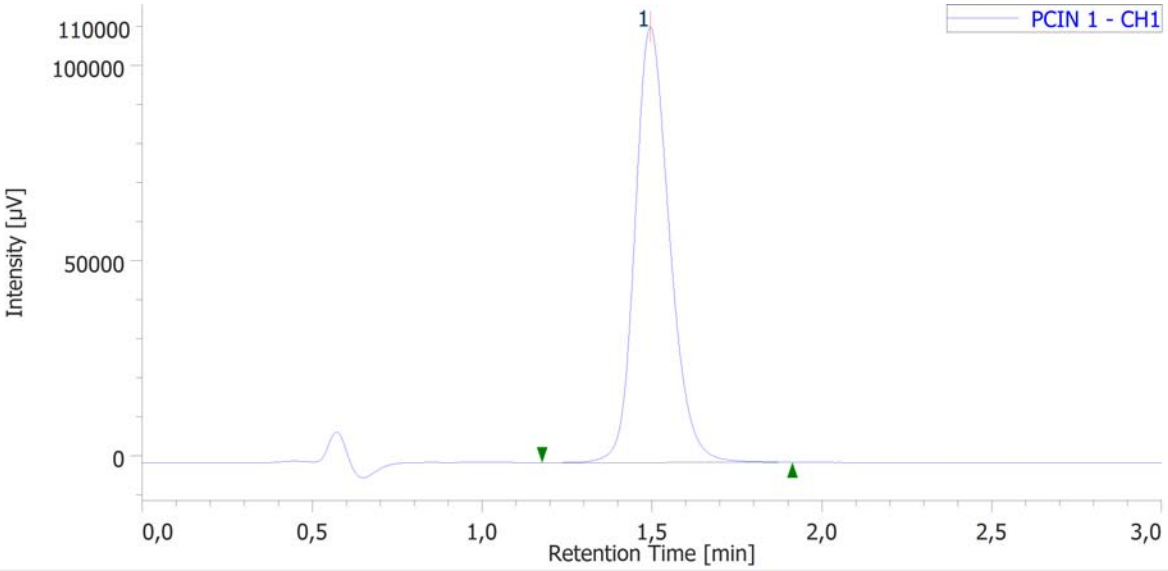

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:02:07
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:35:10
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,495	788593	111587	100,000	100,000	N/A	1086	N/A	1,205	

Creator QPackSA
Reviewer
Approver

Chromatogram

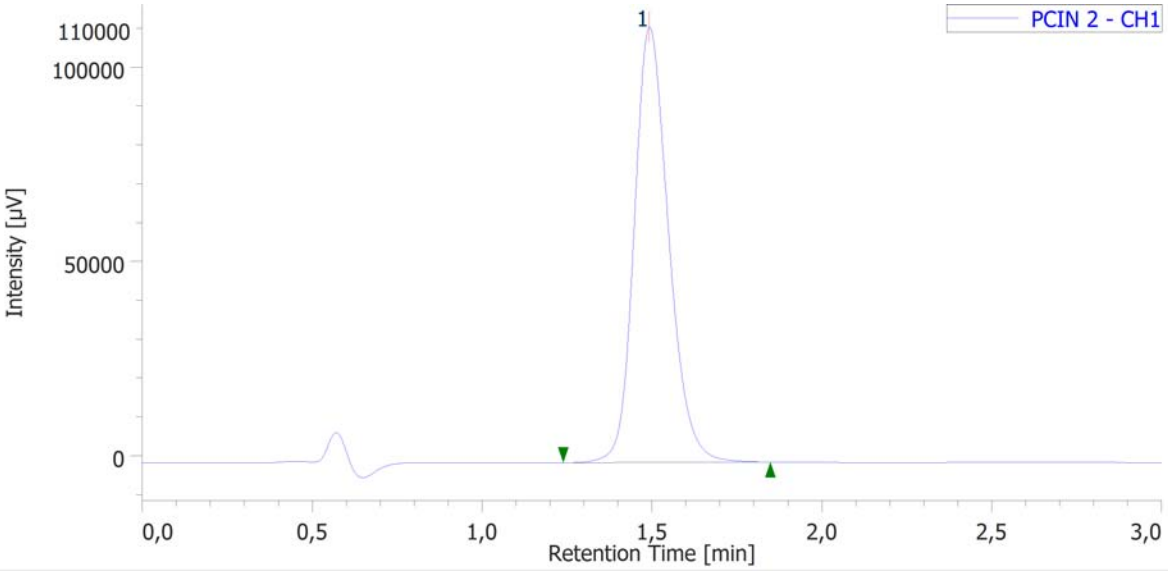

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:02:07
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:39:01
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,492	789013	112009	100,000	100,000	N/A	1085	N/A	1,218	

Creator QPackSA
Reviewer
Approver

Chromatogram

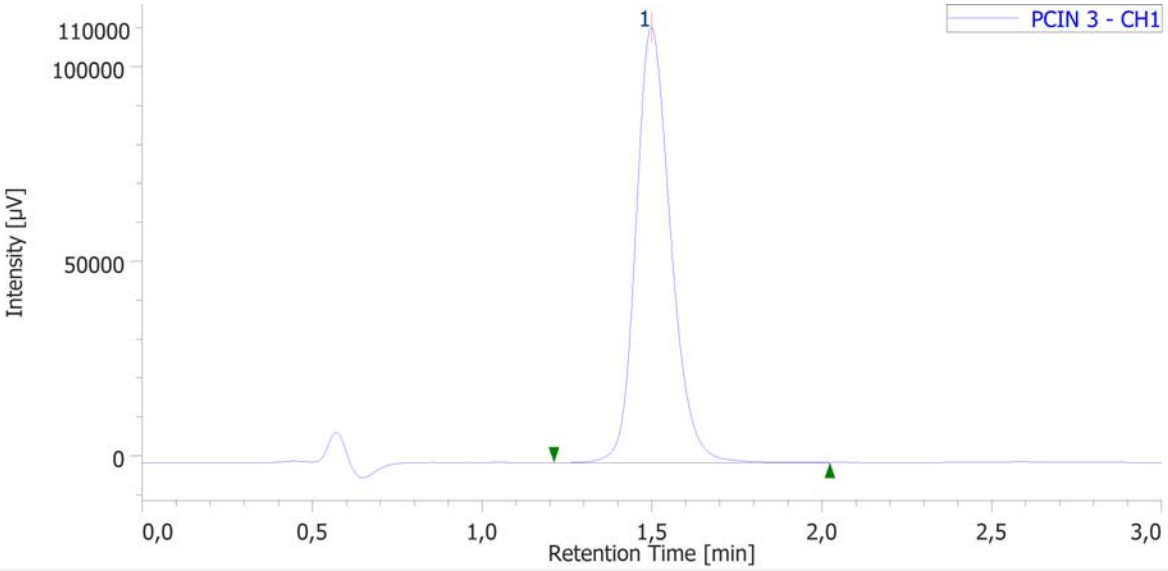

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:02:08
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:42:52
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,498	794609	111912	100,000	100,000	N/A	1077	N/A	1,203	

Creator QPackSA
Reviewer
Approver

Chromatogram

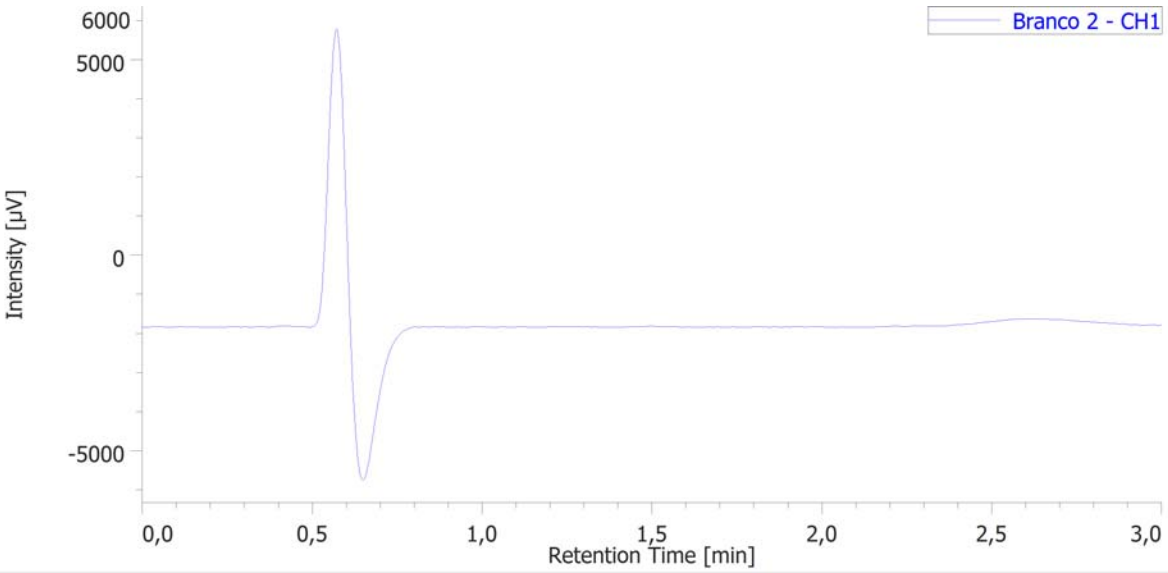


Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:02:08
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:46:43
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

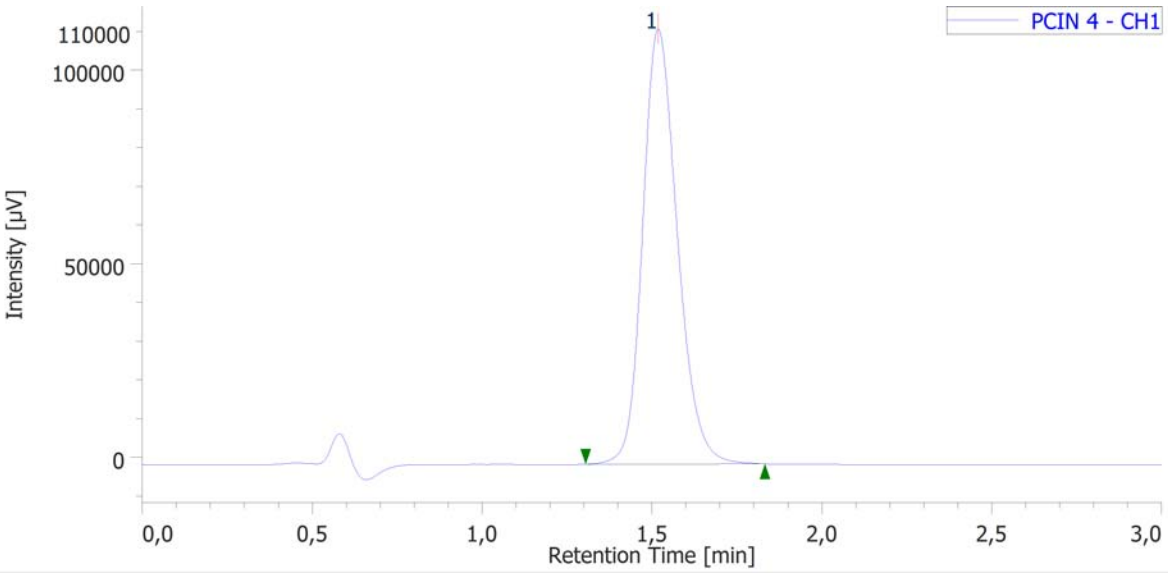

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:06:30
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:50:34
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,518	797472	112263	100,000	100,000	N/A	1105	N/A	1,203	

Creator QPackSA
Reviewer
Approver

Chromatogram

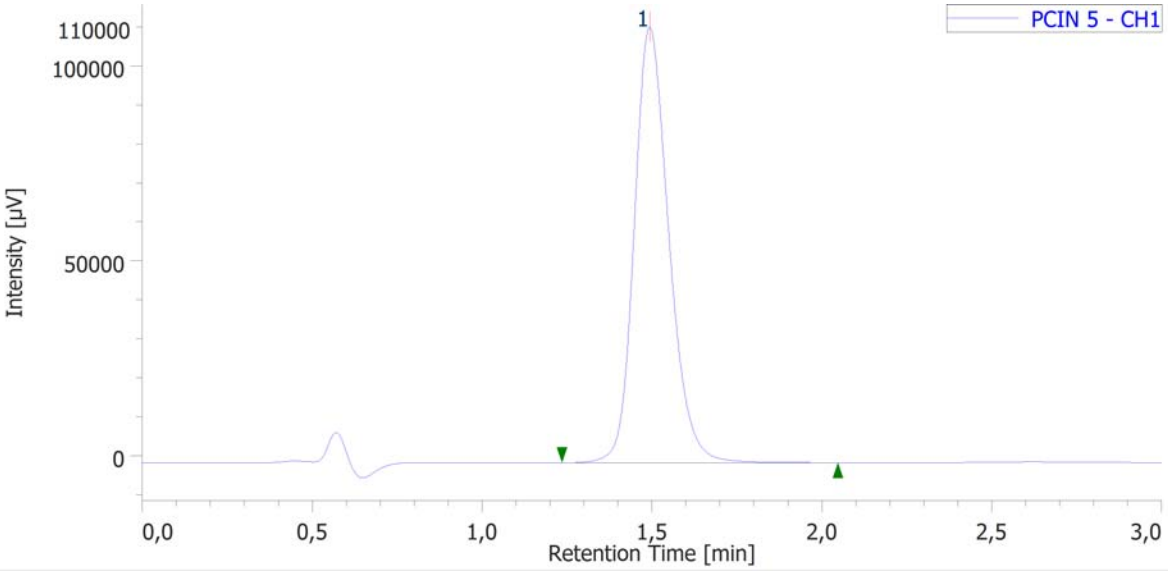

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:07:41
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:54:26
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,493	789946	111743	100,000	100,000	N/A	1084	N/A	1,206	

Creator QPackSA
Reviewer
Approver

Chromatogram

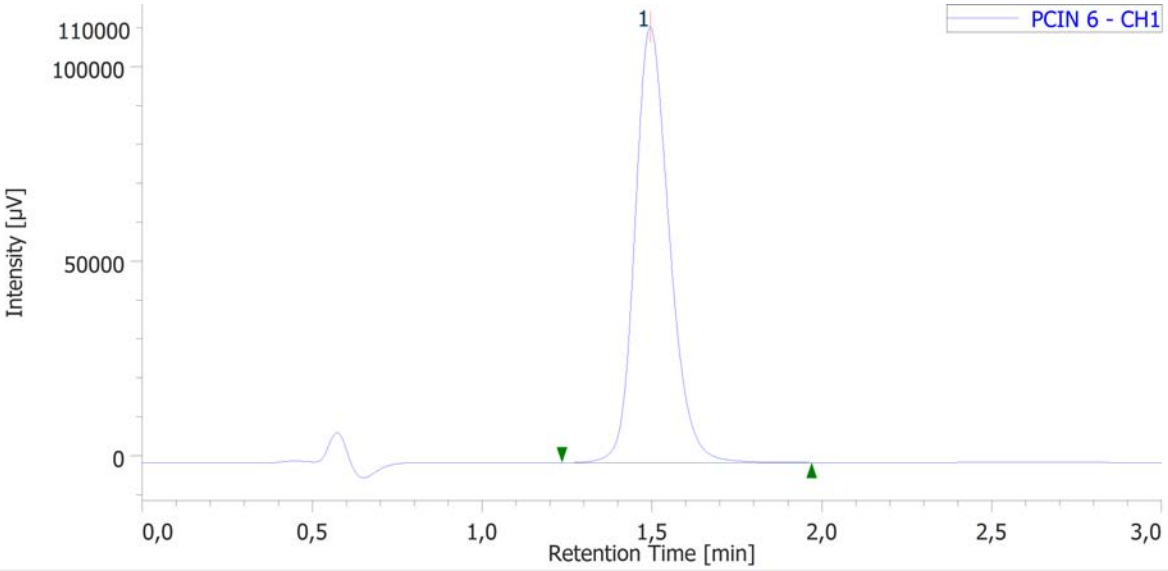

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:08:09
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 12:58:17
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,495	786895	111877	100,000	100,000	N/A	1085	N/A	1,208	

Creator QPackSA
Reviewer
Approver

Chromatogram

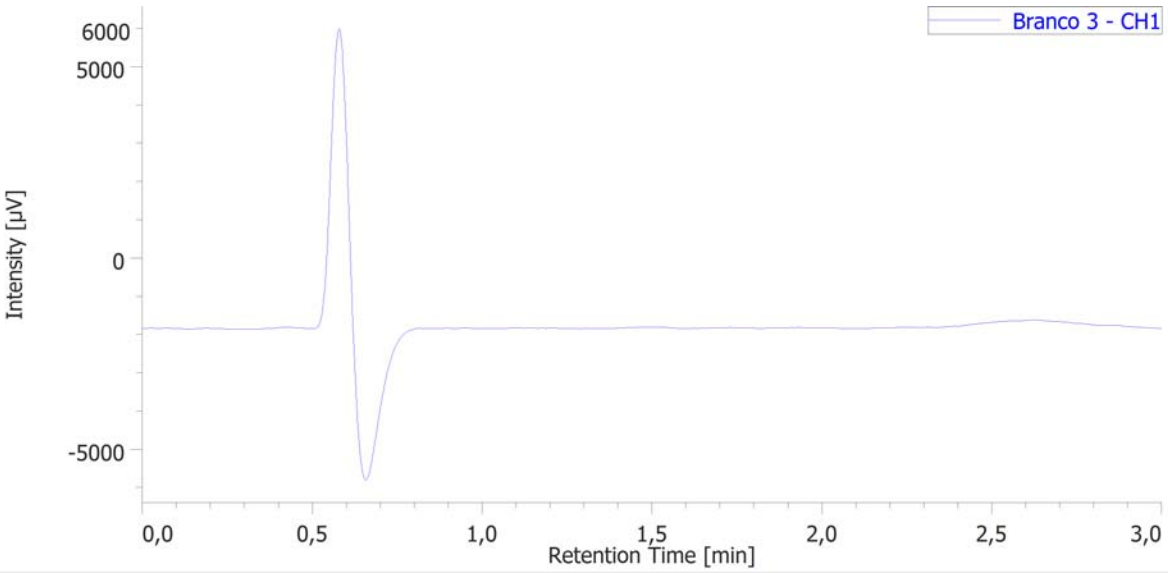


Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:08:43
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:02:08
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

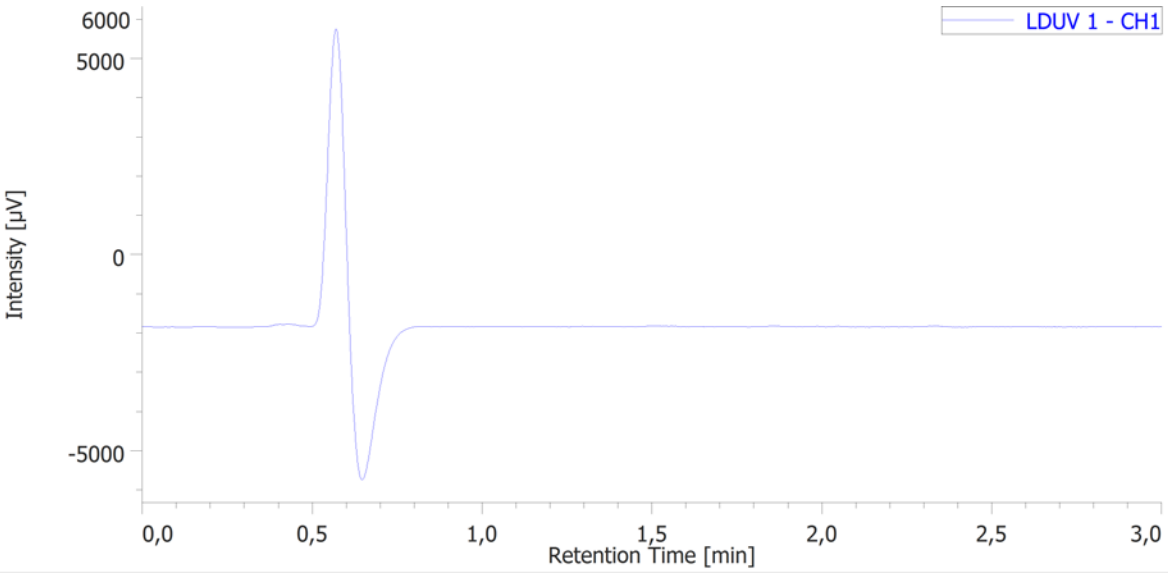


Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:34:33
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:13:22
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

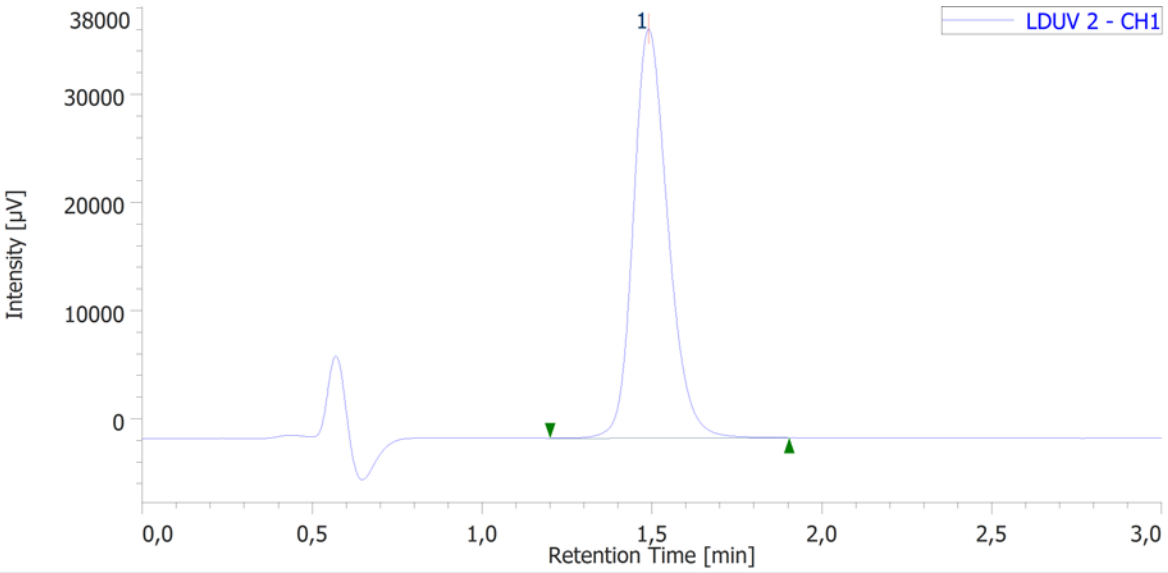

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:34:35
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:17:13
Volume	10,00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,490	267359	37789	100,000	100,000	N/A	1072	N/A	1,218	

Creator QPackSA
Reviewer
Approver

Chromatogram

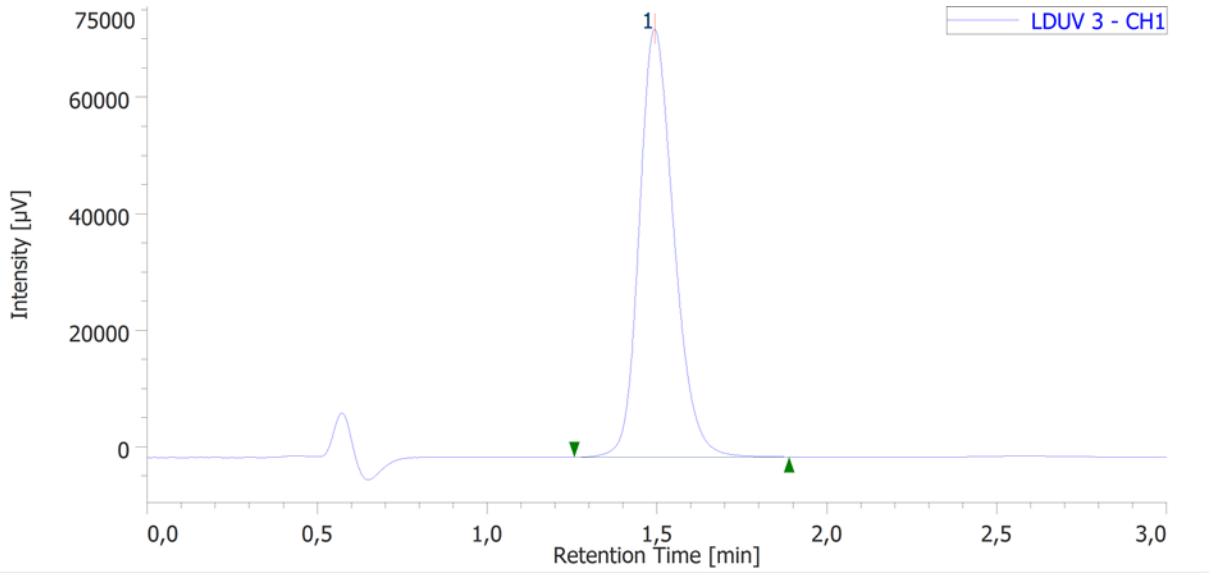

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:34:35
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:21:04
Volume	10,00 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,493	519806	73425	100,000	100,000	N/A	1070	N/A	1,209	

Creator QPackSA
Reviewer
Approver

Chromatogram

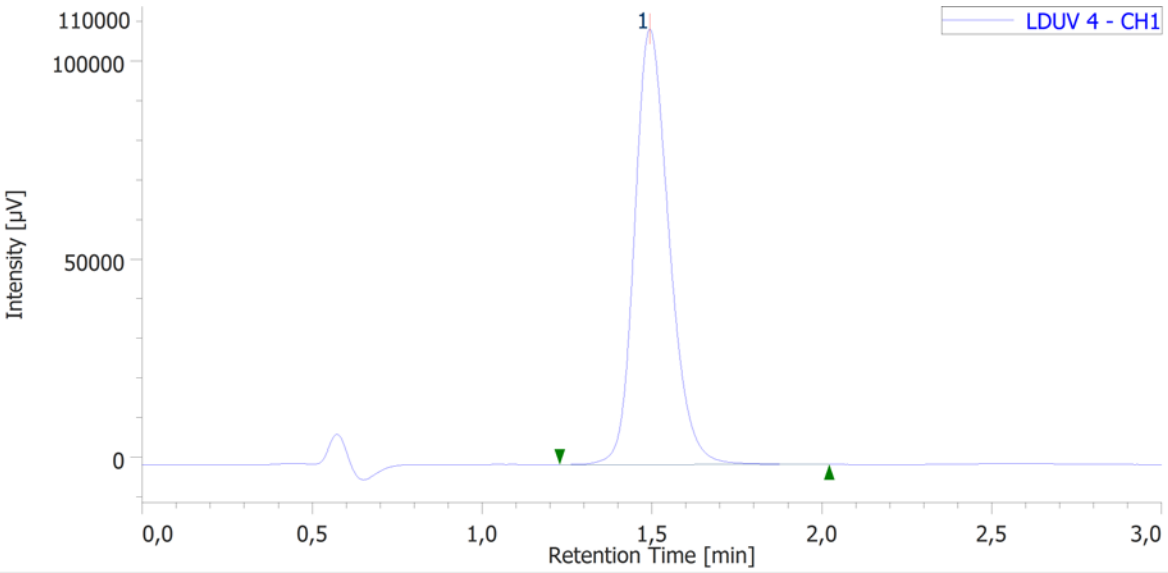

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:34:36
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:24:55
Volume	10,00 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,493	777006	109802	100,000	100,000	N/A	1078	N/A	1,222	

Creator QPackSA
Reviewer
Approver

Chromatogram

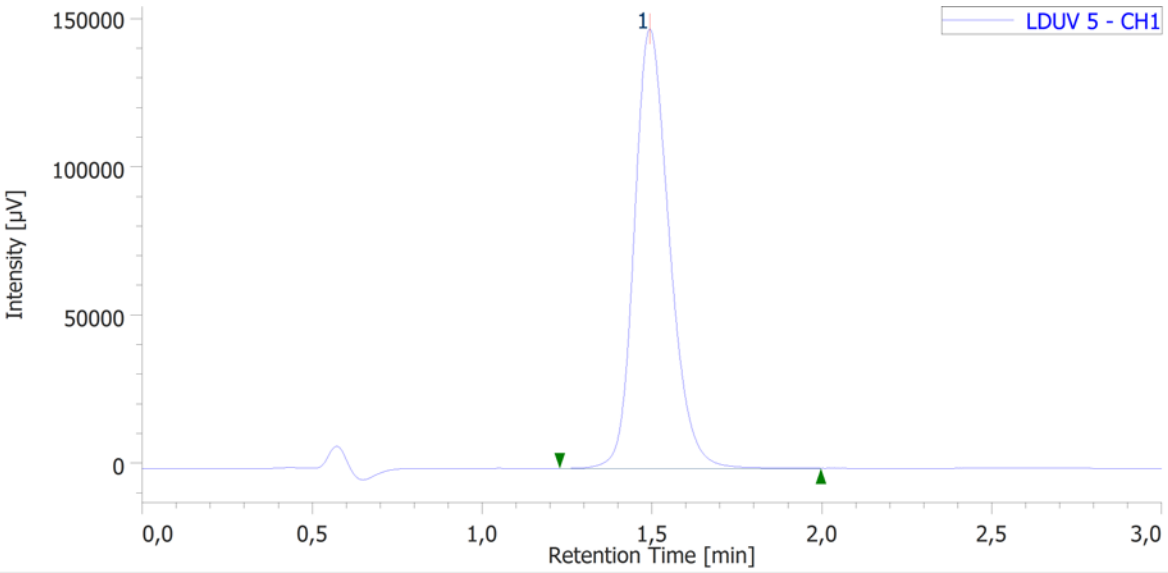

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:34:36
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:28:46
Volume	10,00 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,493	1062862	148192	100,000	100,000	N/A	1046	N/A	1,220	

Creator QPackSA
Reviewer
Approver

Chromatogram

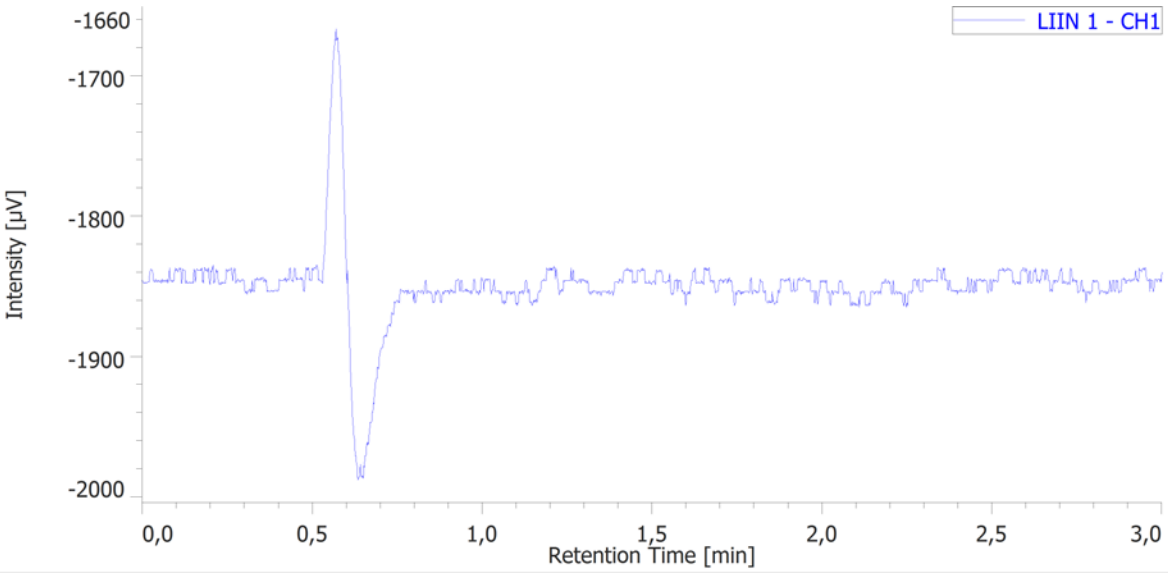


Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:59:10
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:36:13
Volume	0,10 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

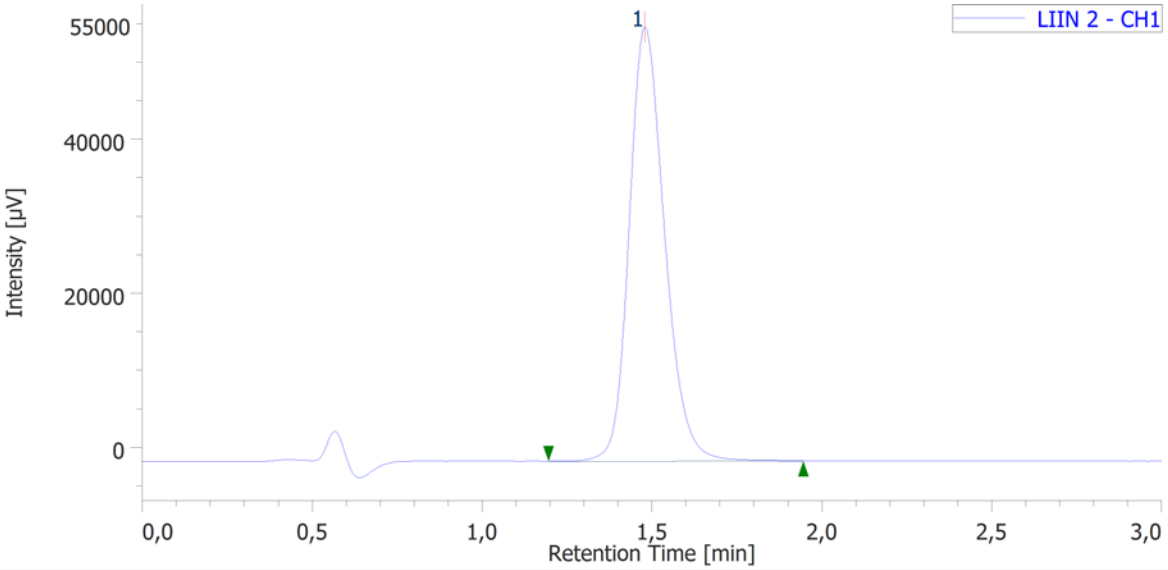

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:59:10
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:40:00
Volume	5,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,478	407861	56323	100,000	100,000	N/A	1008	N/A	1,221	

Creator QPackSA
Reviewer
Approver

Chromatogram

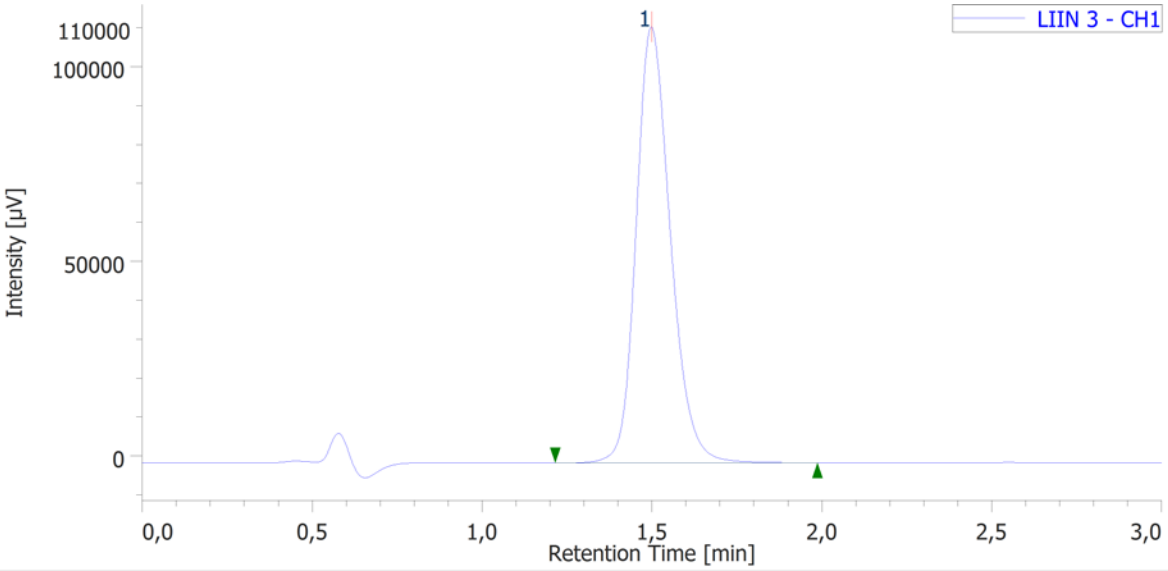

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:59:11
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:43:51
Volume	10,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,498	784765	111900	100,000	100,000	N/A	1108	N/A	1,210	

Creator QPackSA
Reviewer
Approver

Chromatogram

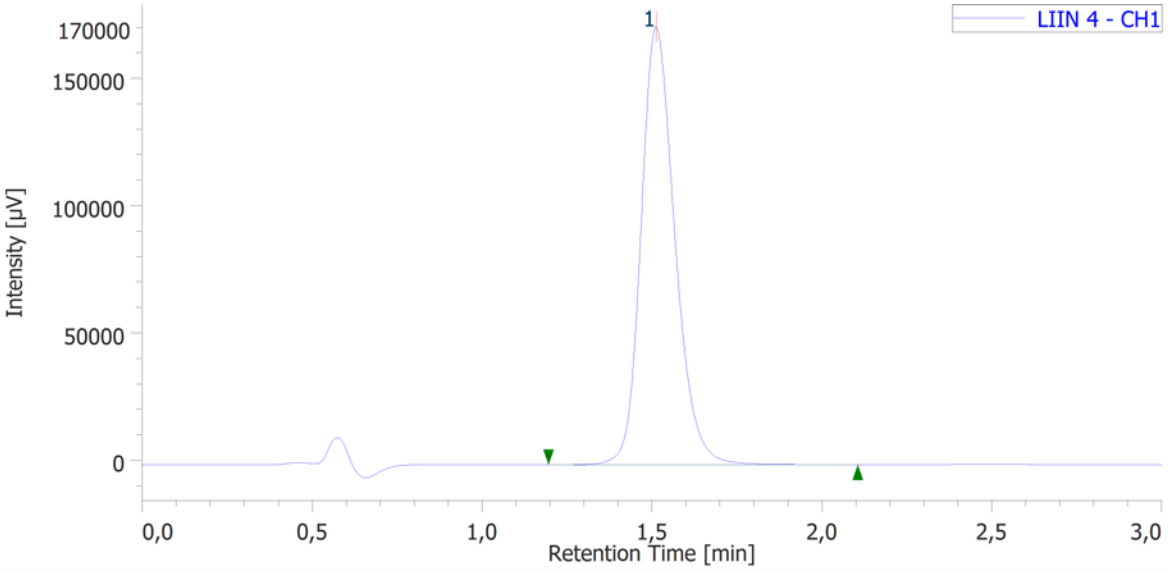

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:59:11
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:47:47
Volume	15,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,512	1191242	171819	100,000	100,000	N/A	1162	N/A	1,218	

Creator QPackSA
Reviewer
Approver

Chromatogram

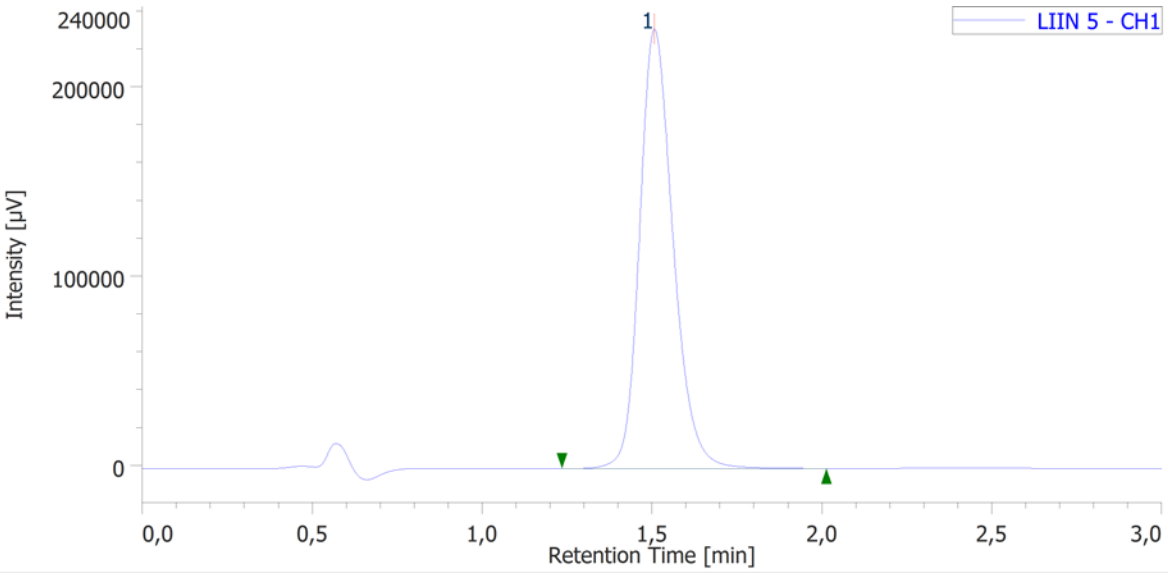

Chromatogram Information	
User Name	QPackSA
Date Modified	25/04/2023 13:59:12
Description	
HPLC System Name	HPLC
Injection Date	25/04/2023 13:51:50
Volume	20,00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,507	1589895	231940	100,000	100,000	N/A	1192	N/A	1,229	

Creator QPackSA
Reviewer
Approver