
Chromatogram

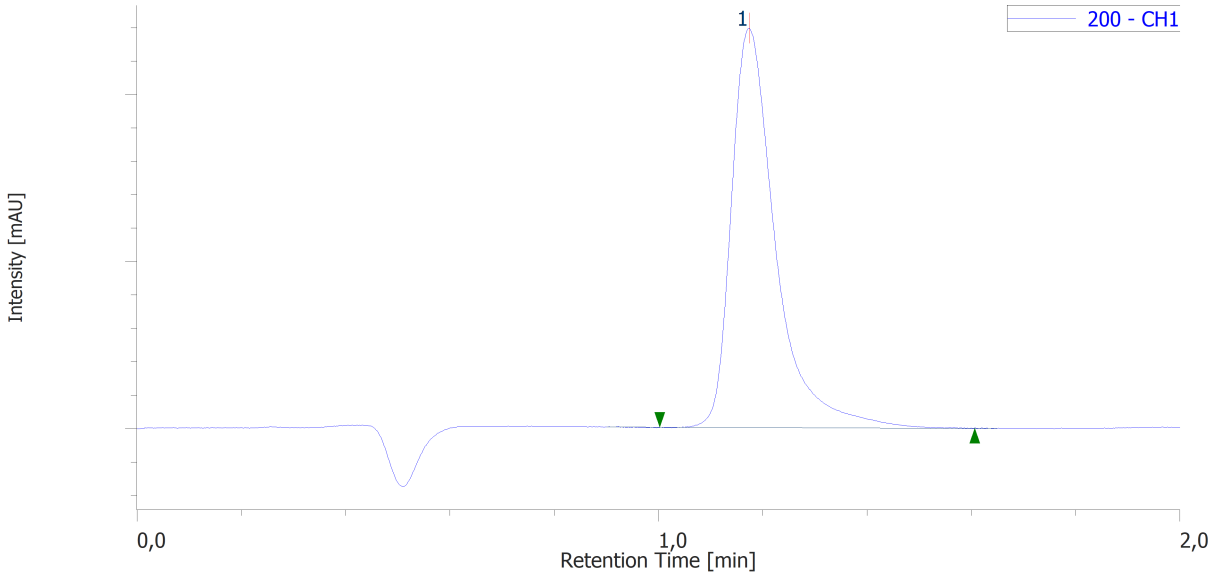

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:29:59
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:27:55
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	200
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	200-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	704231,1	119458,9	100	100	N/A	1085	N/A	1,636	

Creator
Reviewer
Approver

Chromatogram

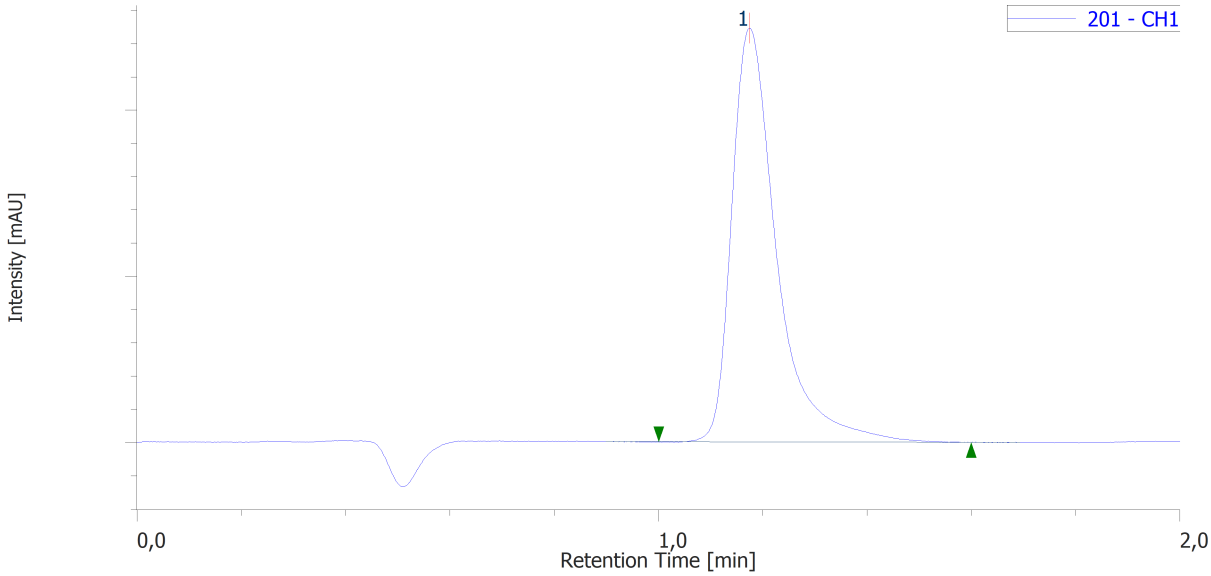

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:32:10
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:30:08
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	201
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	201-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	743743,4	124443,6	100	100	N/A	1058	N/A	1,643	

Creator
Reviewer
Approver

Chromatogram

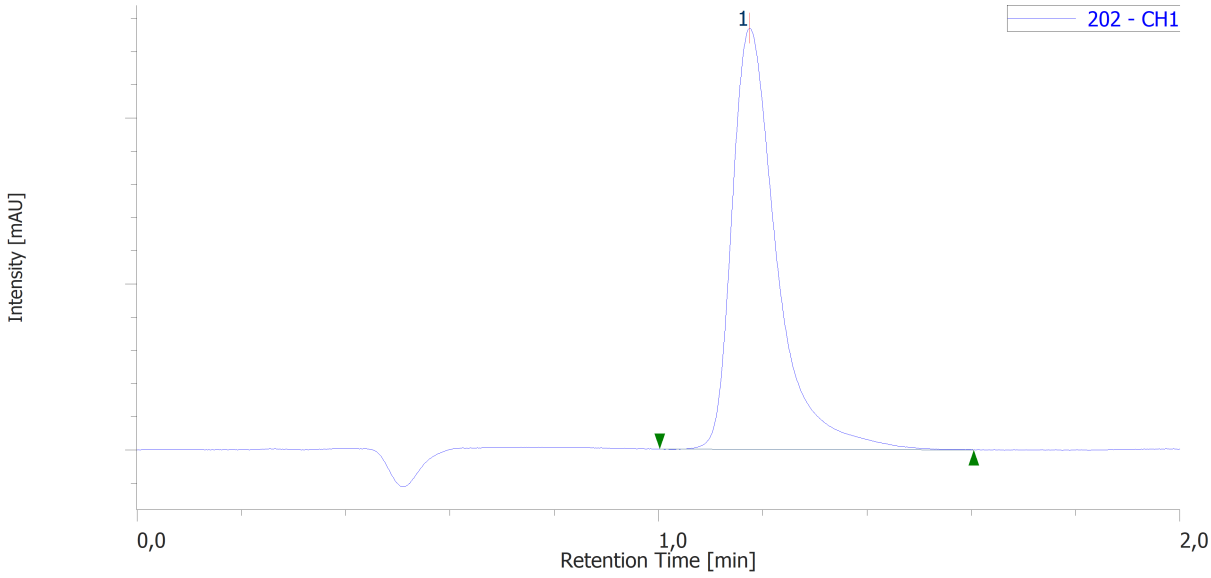

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:34:28
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:32:21
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	202
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	202-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	755860,8	126844,2	100	100	N/A	1060	N/A	1,658	

Creator
Reviewer
Approver

Chromatogram

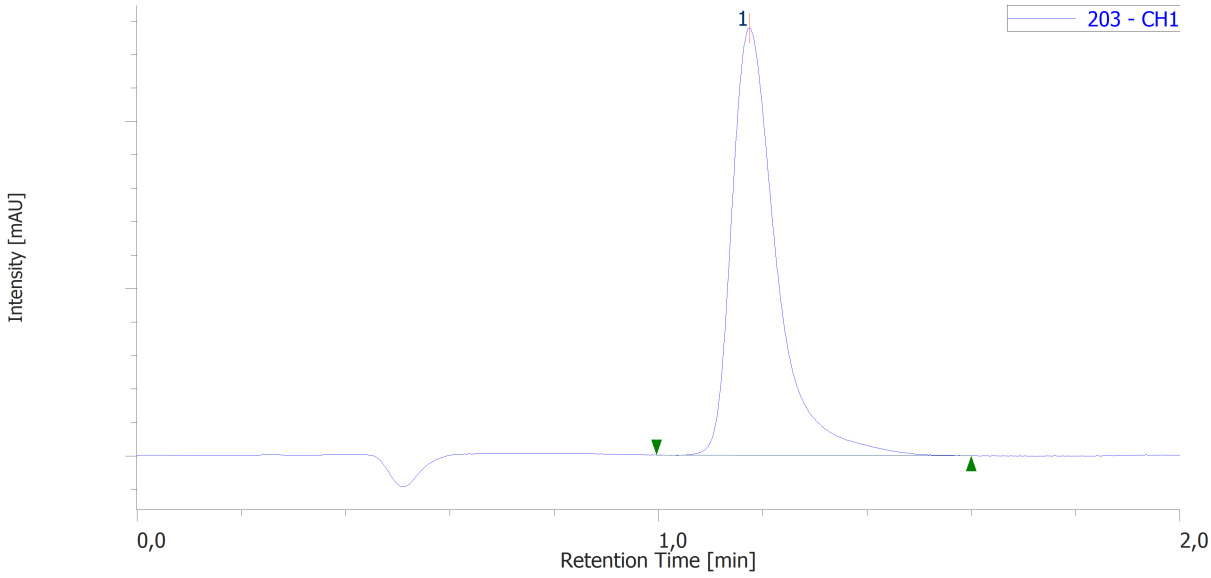

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:36:35
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:34:33
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	203
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	203-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	759203,5	127614,8	100	100	N/A	1060	N/A	1,667	

Creator
Reviewer
Approver

Chromatogram

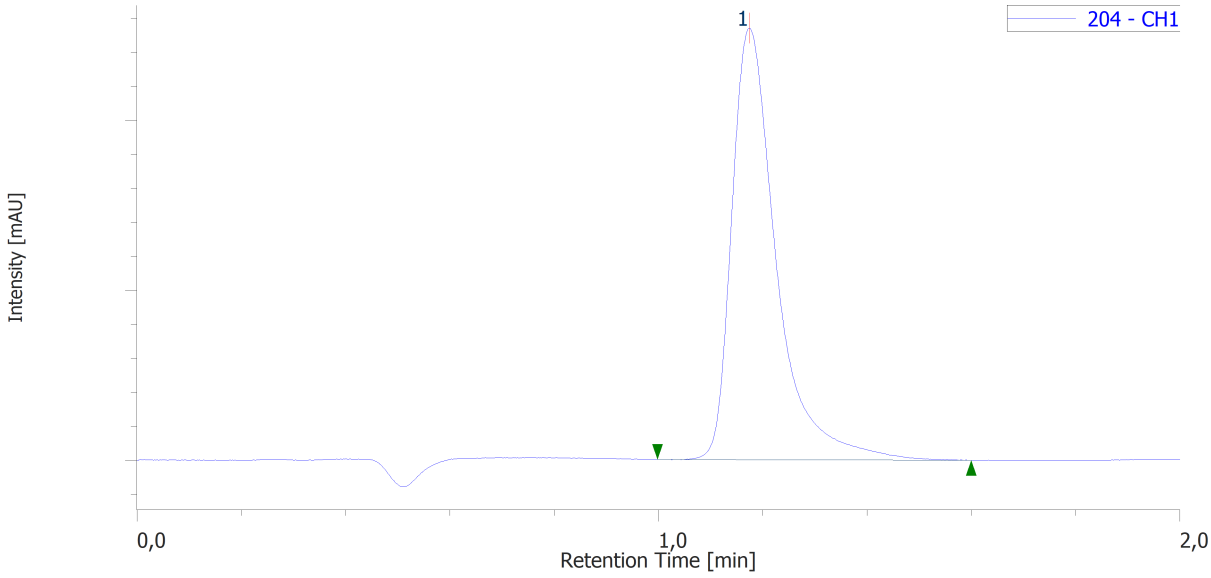

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:38:48
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:36:46
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	204
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	204-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	755557,0	126902,4	100	100	N/A	1059	N/A	1,668	

Creator
Reviewer
Approver

Chromatogram

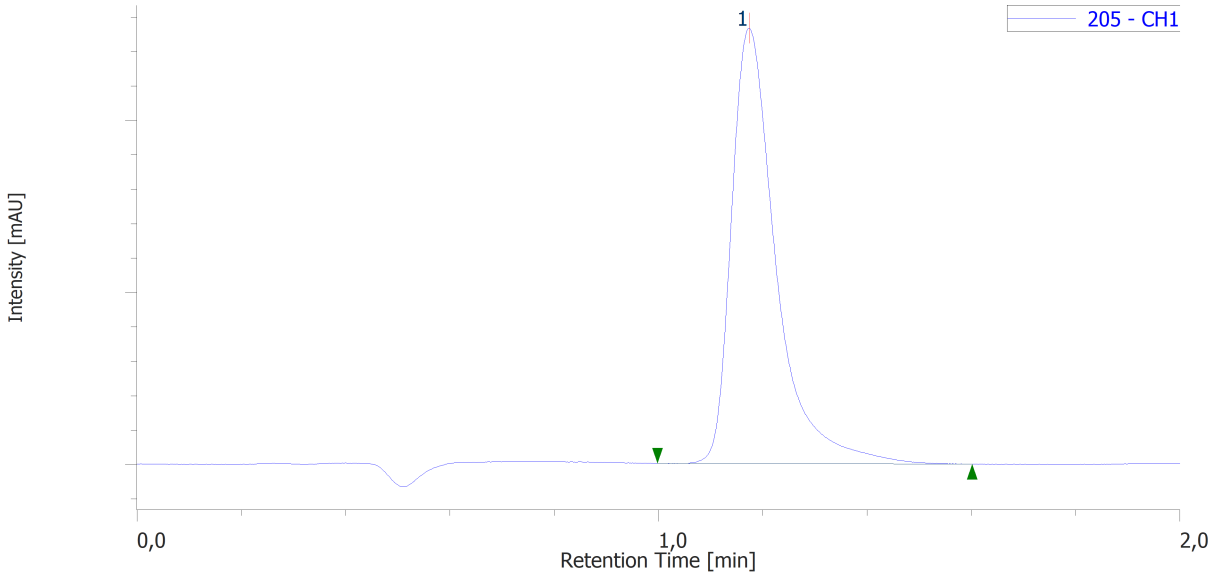

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:41:00
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:38:58
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	205
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	205-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	751606,7	126462,9	100	100	N/A	1060	N/A	1,673	

Creator
Reviewer
Approver

Chromatogram

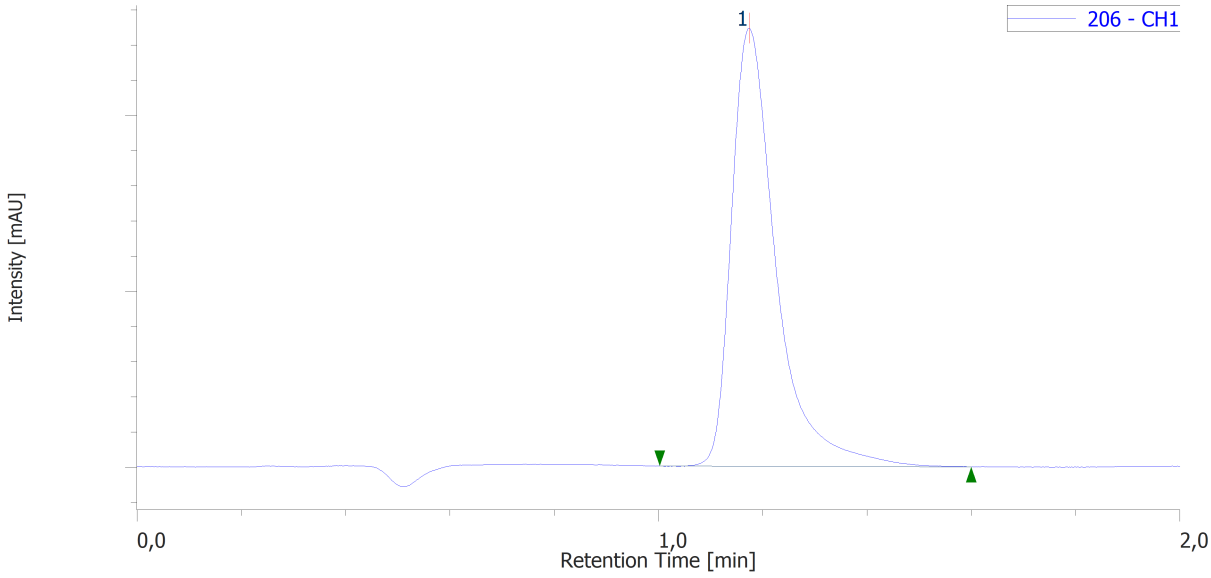

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:43:12
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:41:11
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	206
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	206-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	739726,8	124485,4	100	100	N/A	1062	N/A	1,677	

Creator
Reviewer
Approver

Chromatogram

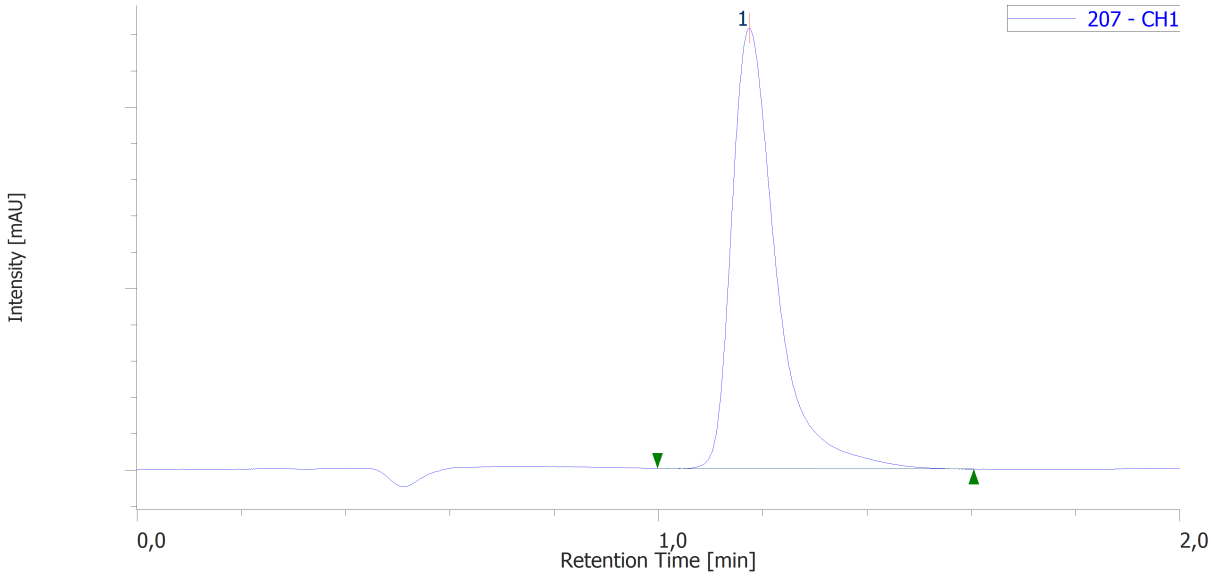

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 11:45:33
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 11:43:24
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	207
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	207-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	719335,8	121309,1	100	100	N/A	1066	N/A	1,669	

Creator
Reviewer
Approver

Chromatogram

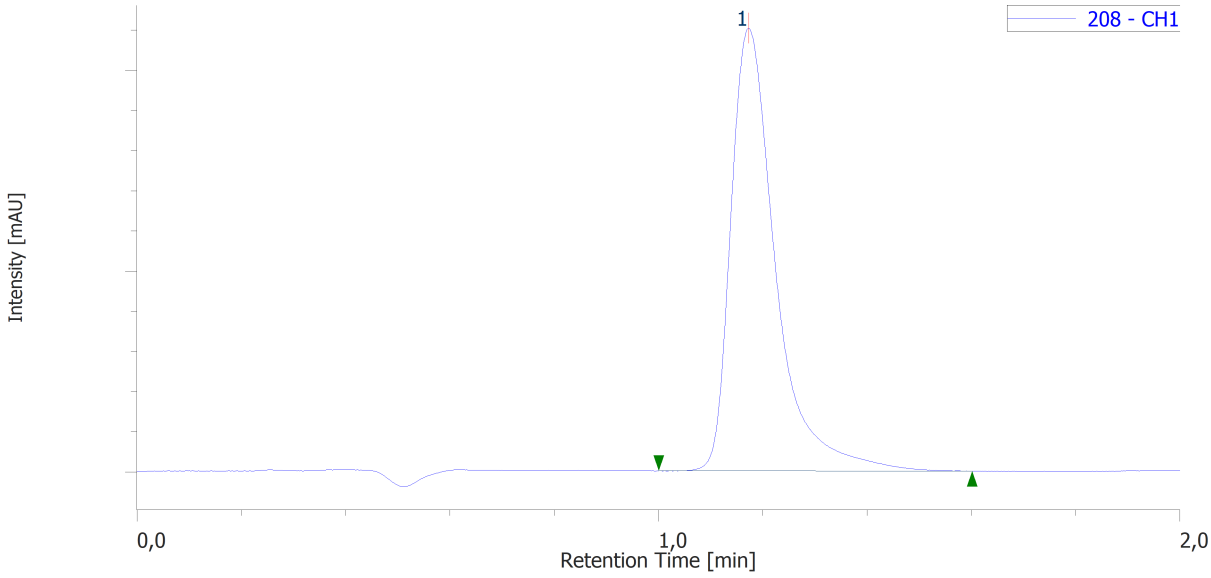

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:25:35
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:23:33
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	208
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	208-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	658741,4	110237,0	100	100	N/A	1036	N/A	1,664	

Creator
Reviewer
Approver

Chromatogram

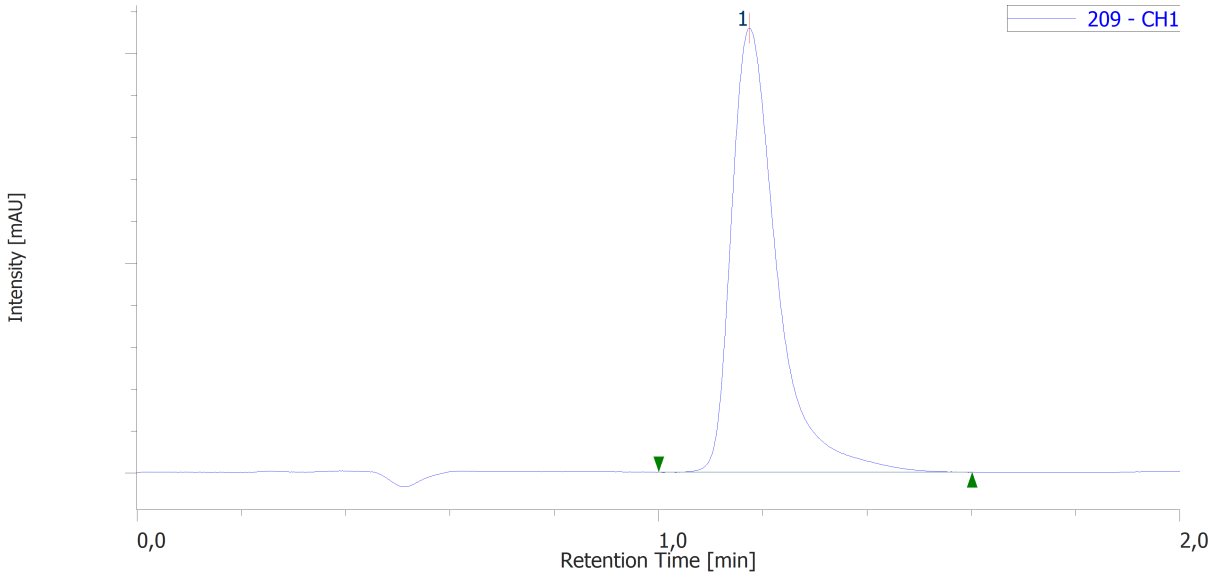

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:27:47
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:25:46
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	209
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	209-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	642031,3	105913,4	100	100	N/A	1011	N/A	1,682	

Creator
Reviewer
Approver

Chromatogram

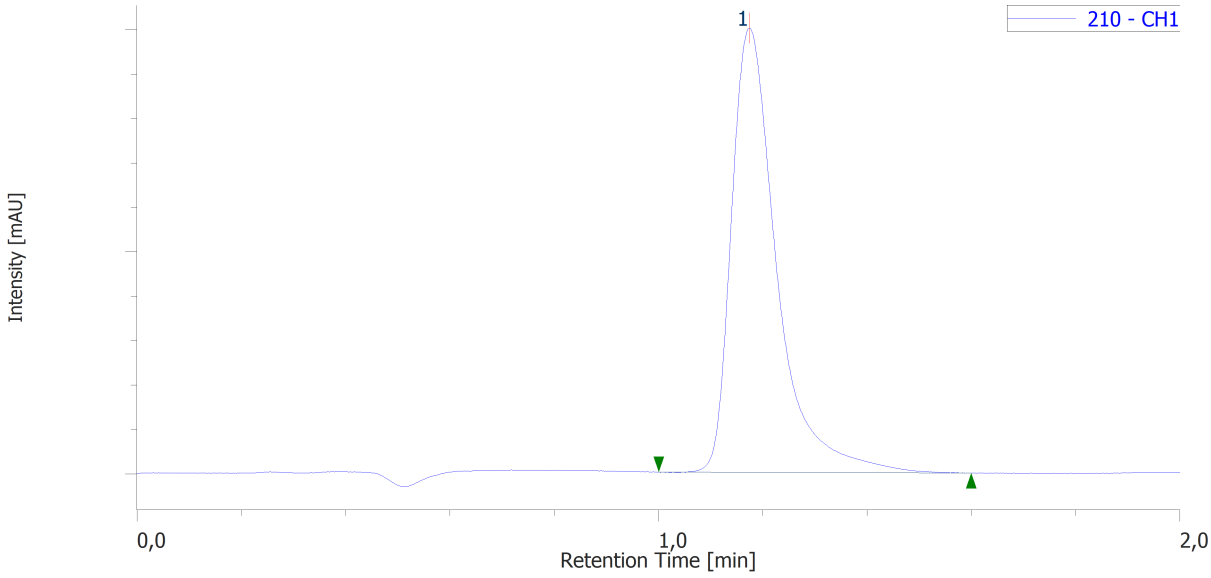

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:30:01
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:27:59
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	210
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	210-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	605285,6	99974,81	100	100	N/A	1016	N/A	1,677	

Creator
Reviewer
Approver

Chromatogram

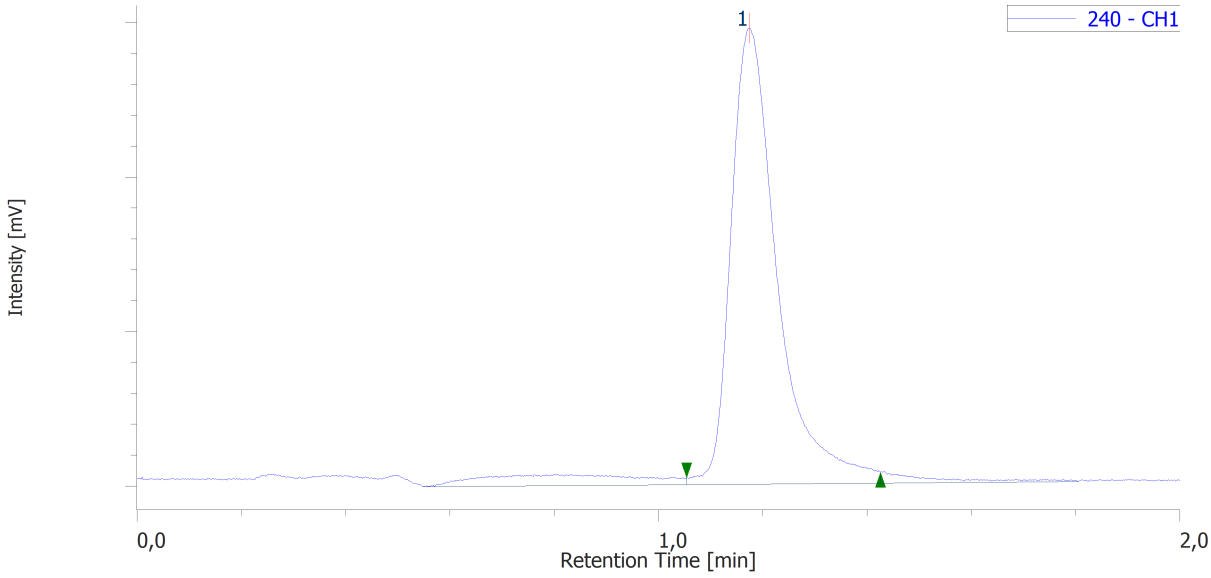

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:32:14
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:30:11
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	240
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	240-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	90999,21	14758,45	100	100	N/A	1000	N/A	1,746	

Creator
Reviewer
Approver

Chromatogram

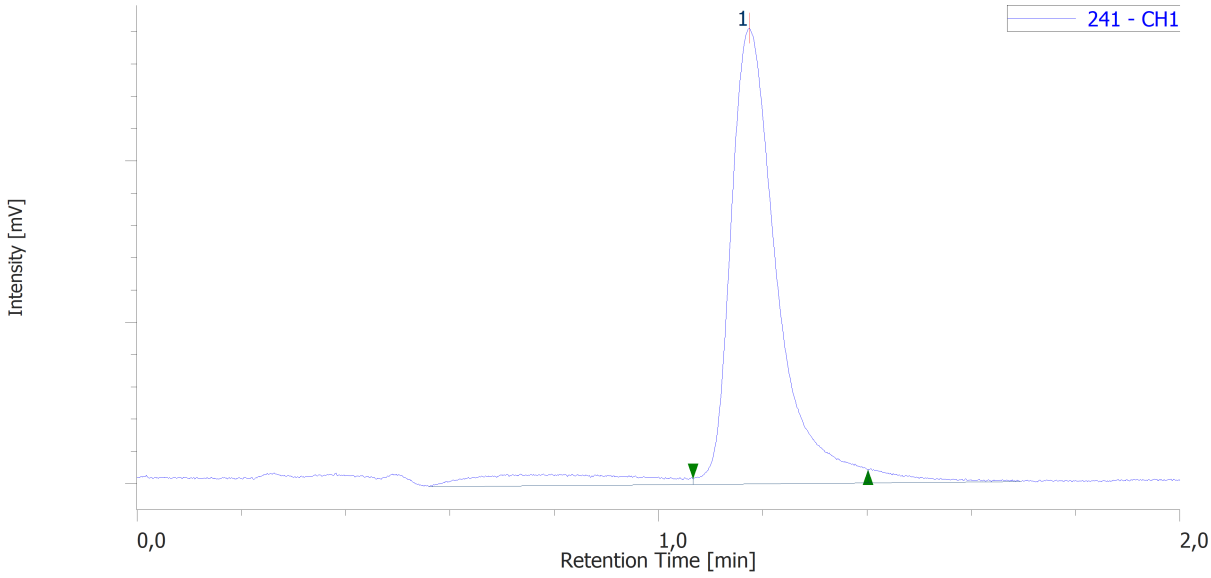

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:34:26
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:32:25
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	241
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	241-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	85844,54	14118,55	100	100	N/A	1005	N/A	1,706	

Creator
Reviewer
Approver

Chromatogram

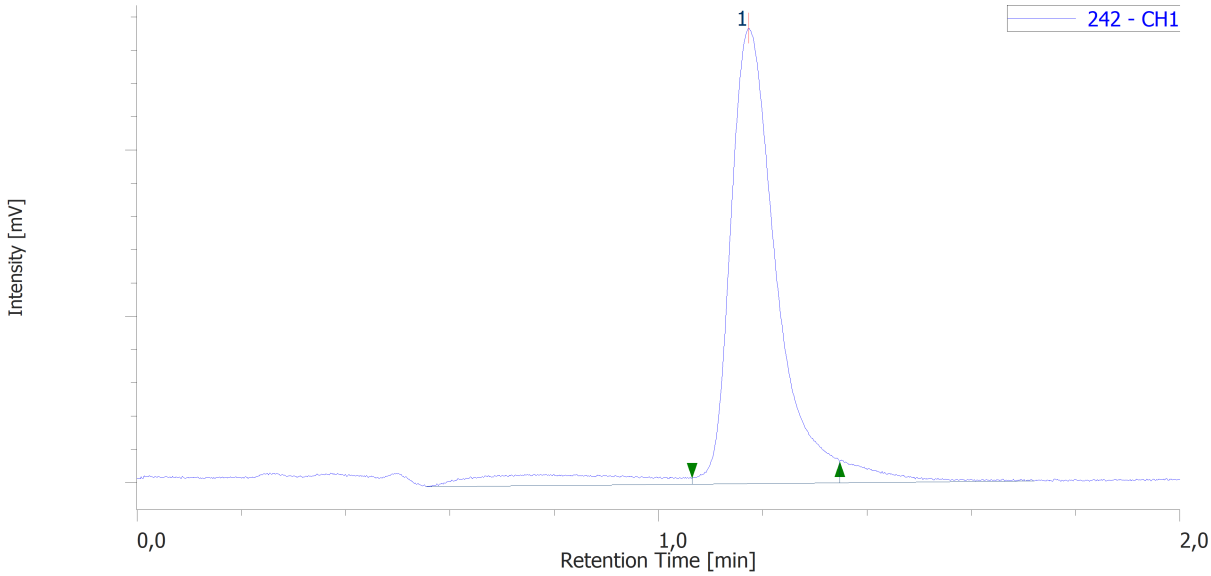

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:36:37
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:34:36
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	242
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	242-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	81560,52	13692,79	100	100	N/A	998	N/A	1,699	

Creator
Reviewer
Approver

Chromatogram

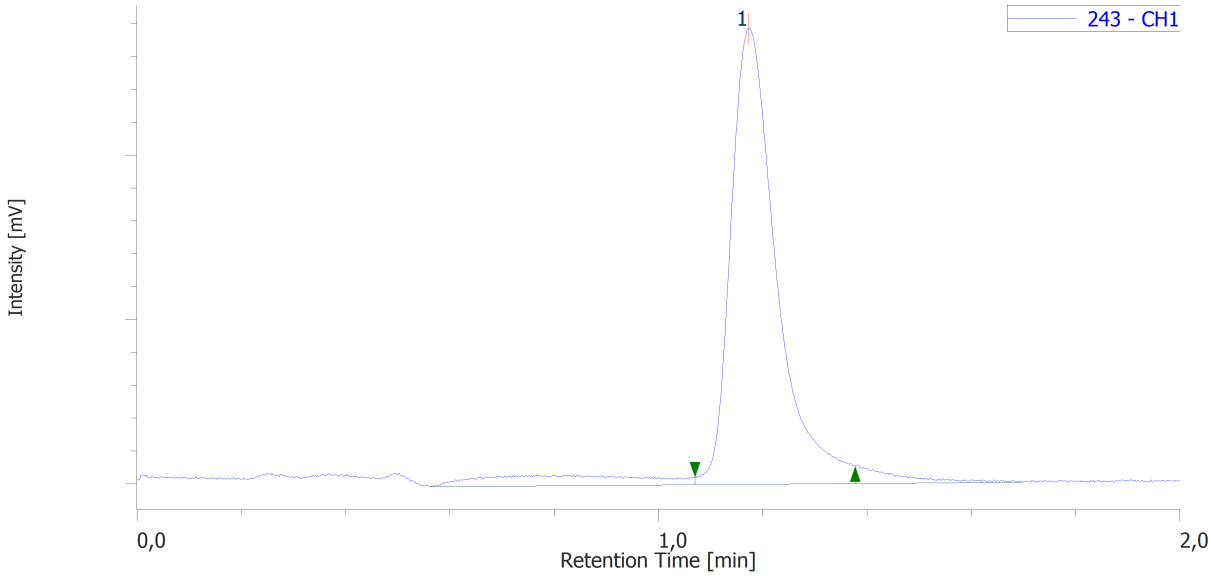

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 12:38:51
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 12:36:49
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	243
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	243-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,17	83676,67	13862,63	100	100	N/A	997	N/A	1,733	

Creator
Reviewer
Approver

Chromatogram

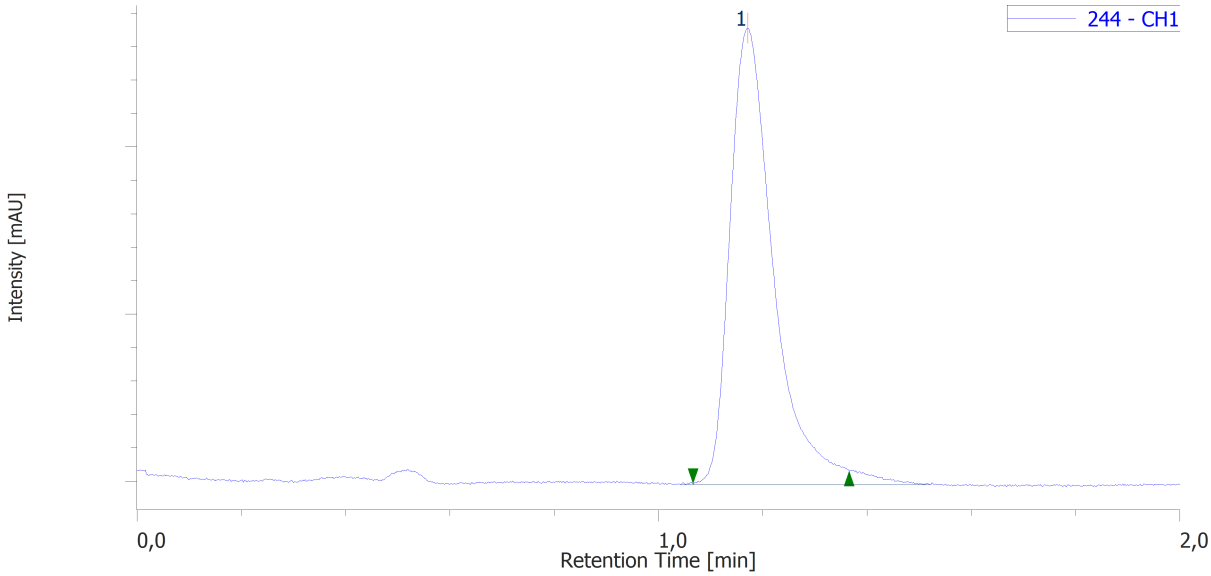

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 13:57:13
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 13:55:18
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	244
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	244-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	78461,86	13650,00	100	100	N/A	1077	N/A	1,624	

Creator
Reviewer
Approver

Chromatogram

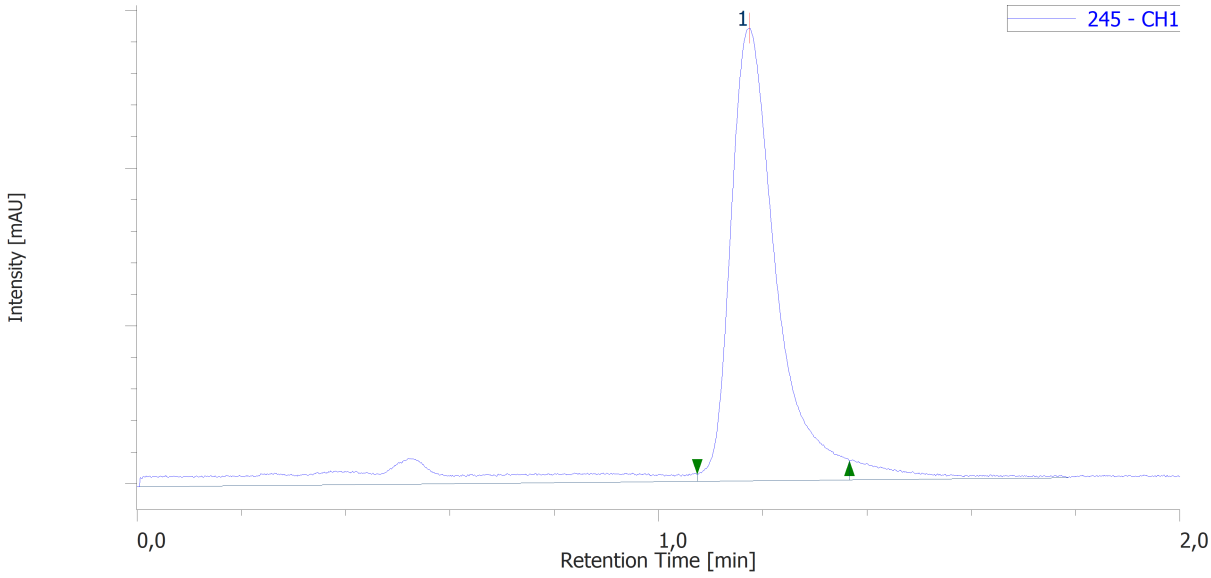

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 13:59:24
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 13:57:23
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	245
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	245-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	85602,84	14340,80	100	100	N/A	1035	N/A	1,742	

Creator
Reviewer
Approver

Chromatogram

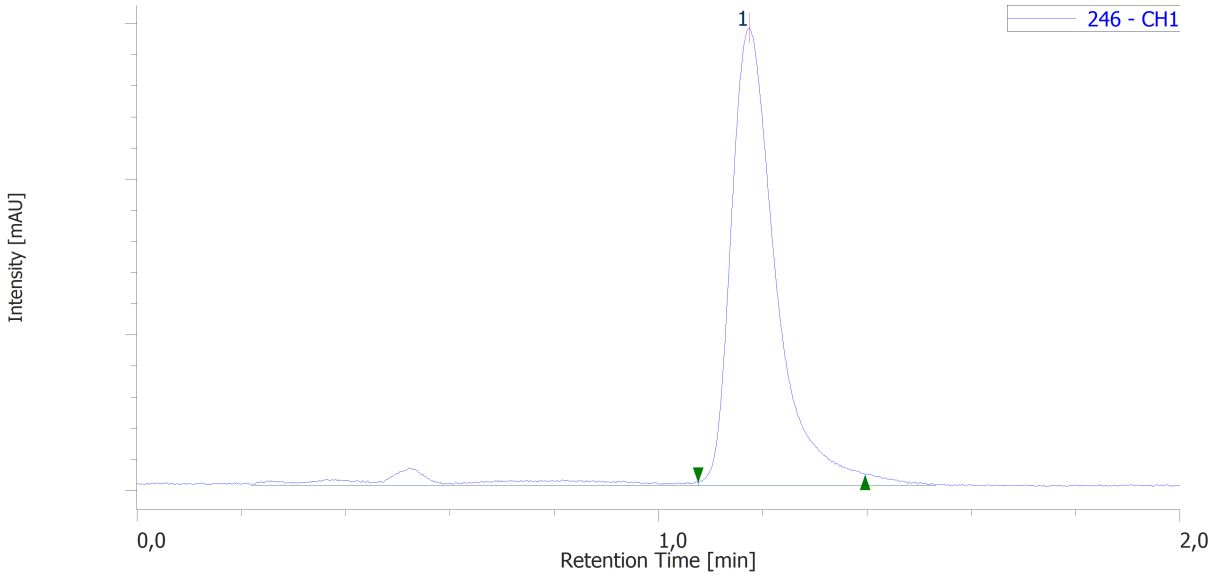

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:01:38
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 13:59:36
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	246
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	246-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	86380,42	14681,82	100	100	N/A	1057	N/A	1,663	

Creator
Reviewer
Approver

Chromatogram

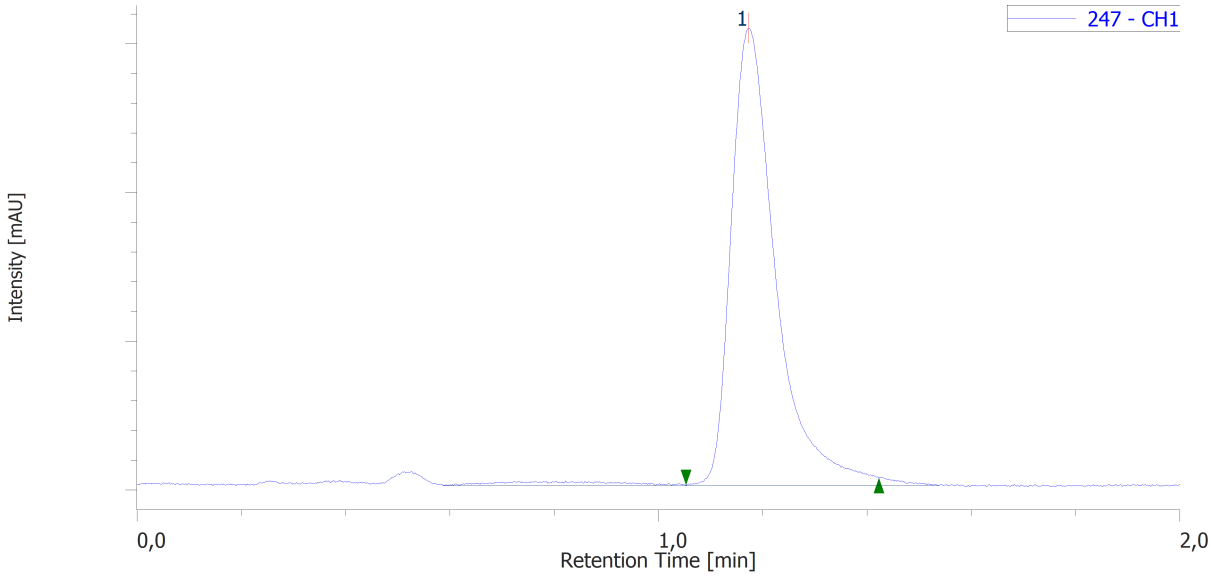

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:03:50
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:01:48
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	247
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	247-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	91088,77	15384,47	100	100	N/A	1051	N/A	1,698	

Creator
Reviewer
Approver

Chromatogram

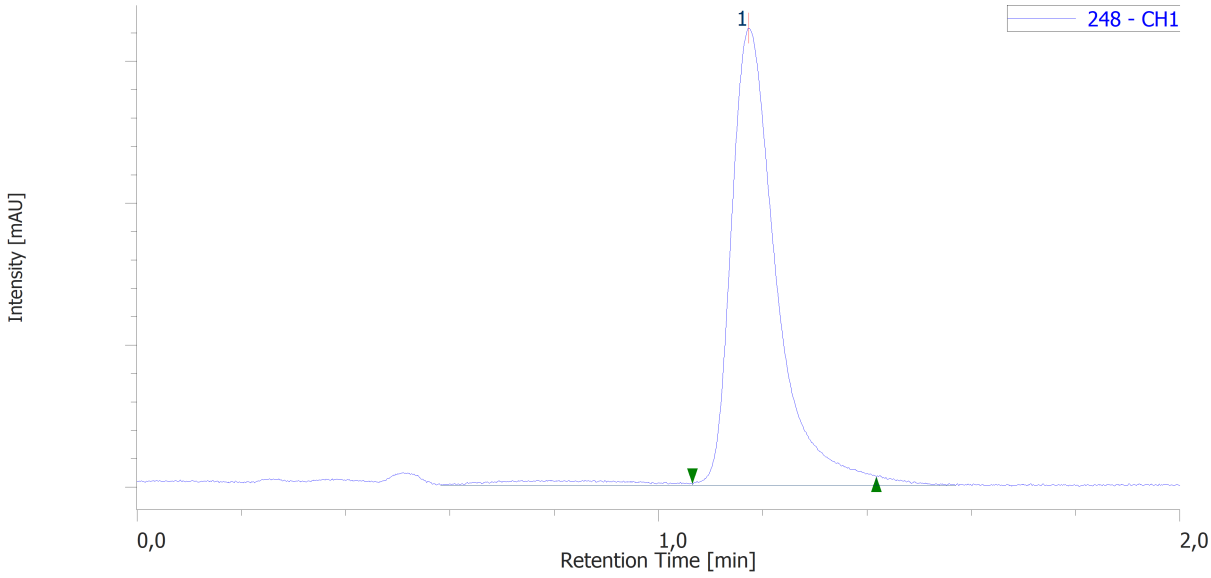

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:06:02
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:04:01
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	248
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	248-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	95473,97	16095,79	100	100	N/A	1047	N/A	1,705	

Creator
Reviewer
Approver

Chromatogram

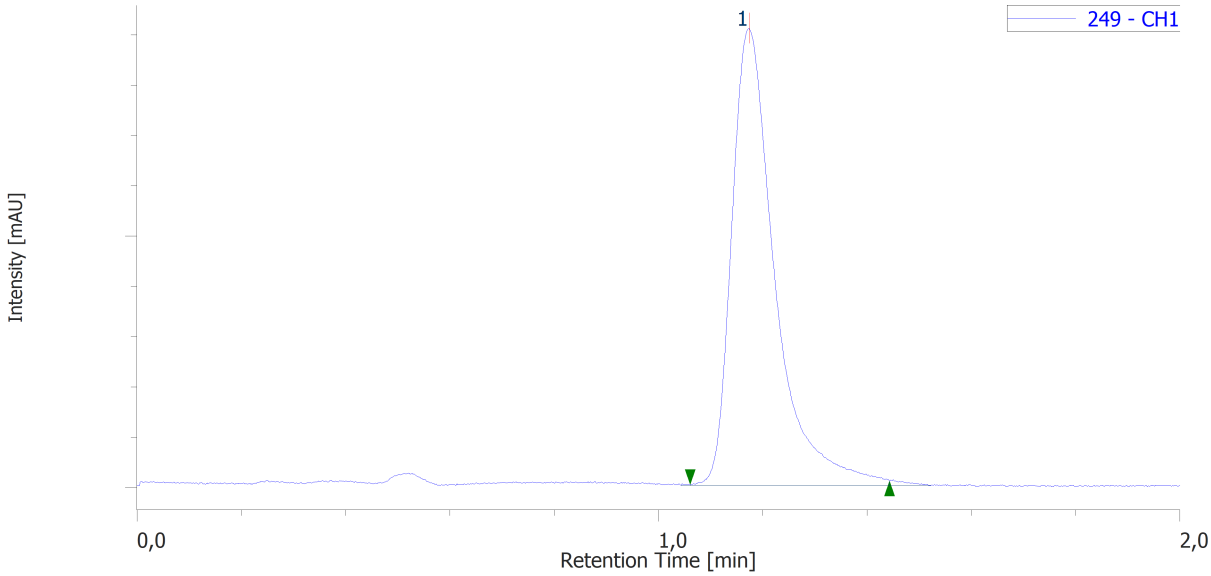

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:08:15
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:06:13
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	249
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	249-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	104566,5	18176,27	100	100	N/A	1149	N/A	1,682	

Creator
Reviewer
Approver

Chromatogram

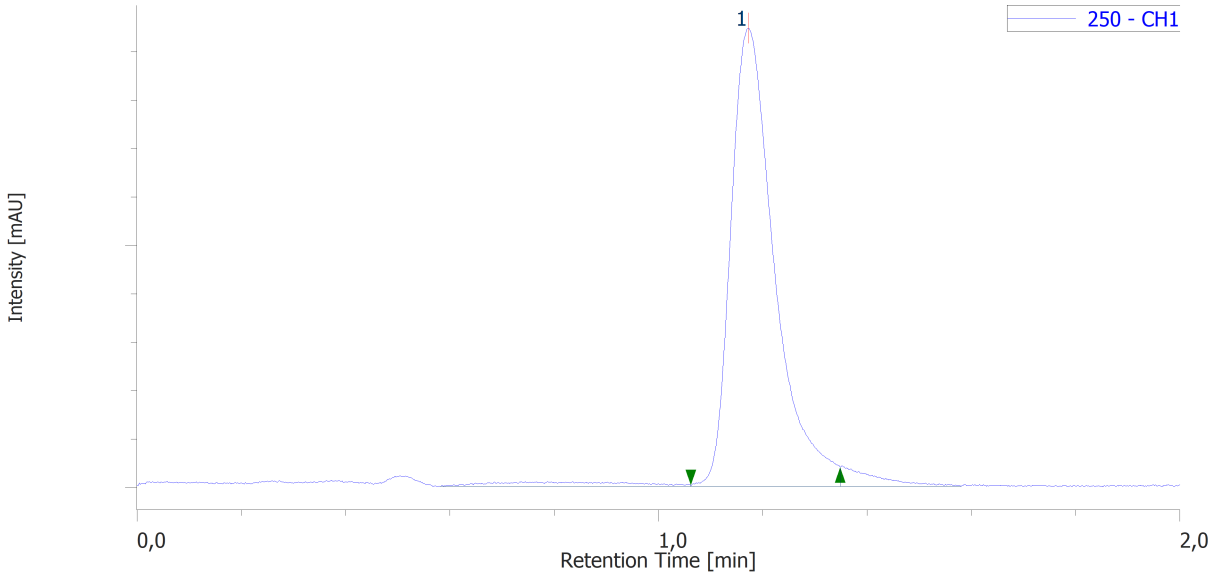

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:10:28
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:08:26
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	250
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	250-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	109698,4	18939,45	100	100	N/A	1065	N/A	1,711	

Creator
Reviewer
Approver

Chromatogram

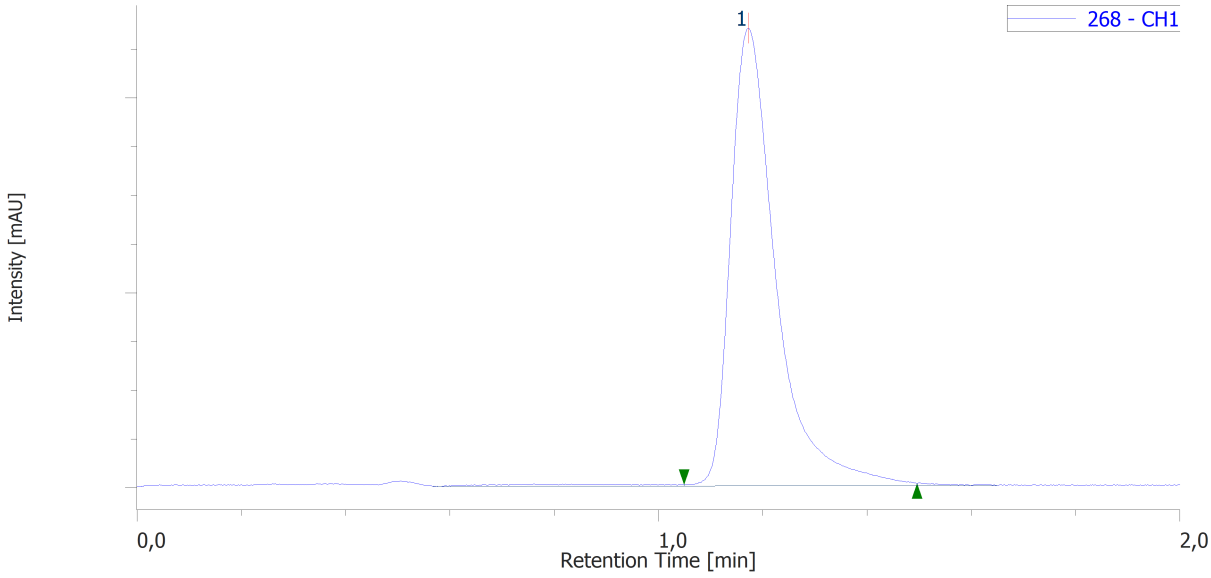

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:12:40
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:10:38
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	268
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	268-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	284174,6	46965,36	100	100	N/A	1035	N/A	1,731	

Creator
Reviewer
Approver

Chromatogram

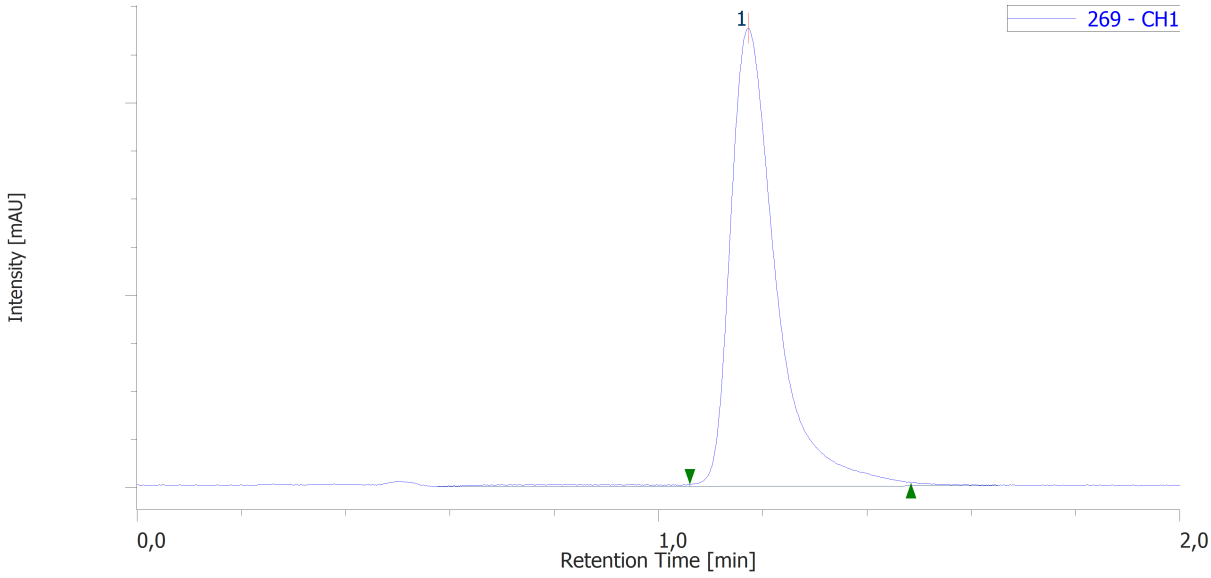

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:14:53
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:12:51
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	269
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	269-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	287971,0	47641,57	100	100	N/A	1031	N/A	1,719	

Creator
Reviewer
Approver

Chromatogram

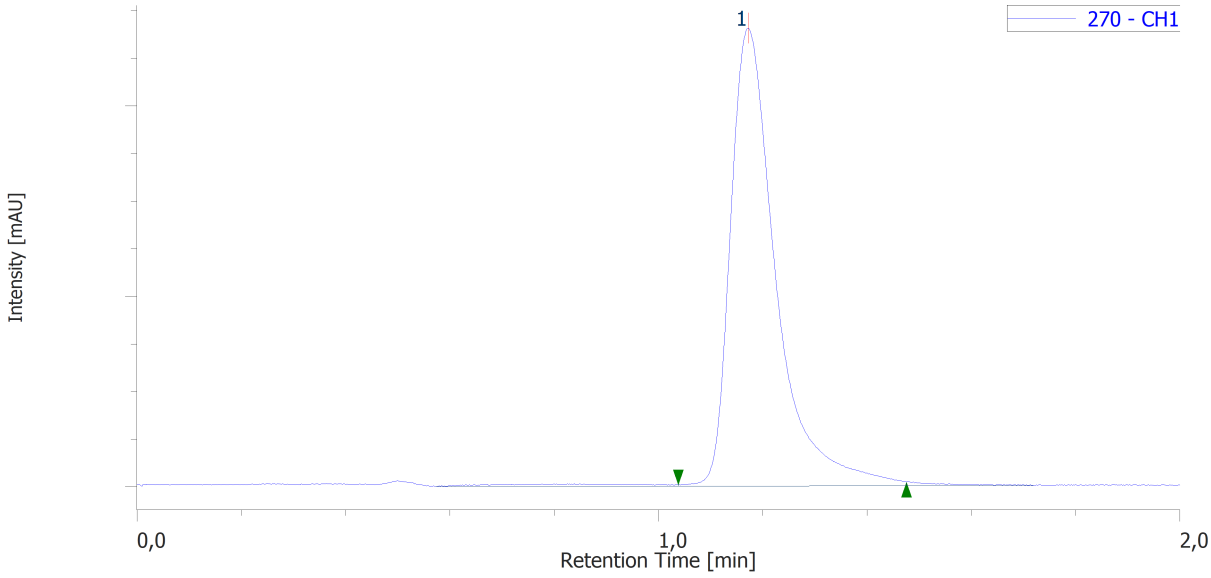

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:17:04
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:15:03
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	270
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	270-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	291084,4	48045,55	100	100	N/A	1026	N/A	1,730	

Creator
Reviewer
Approver

Chromatogram

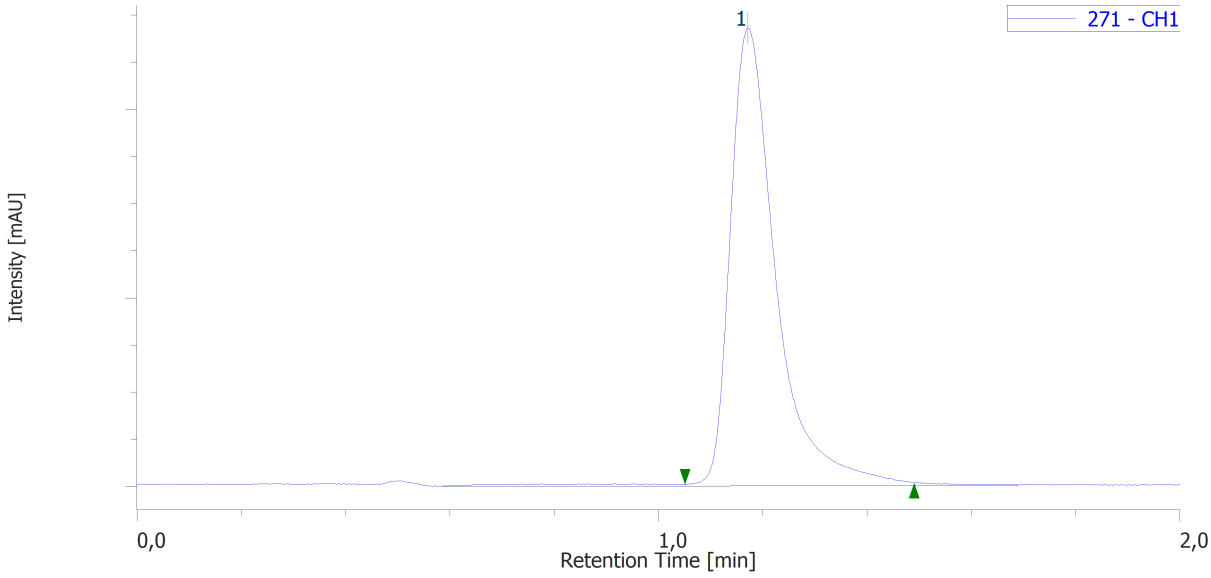

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:19:18
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:17:15
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	271
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	271-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	294776,0	48546,12	100	100	N/A	1020	N/A	1,740	

Creator
Reviewer
Approver

Chromatogram

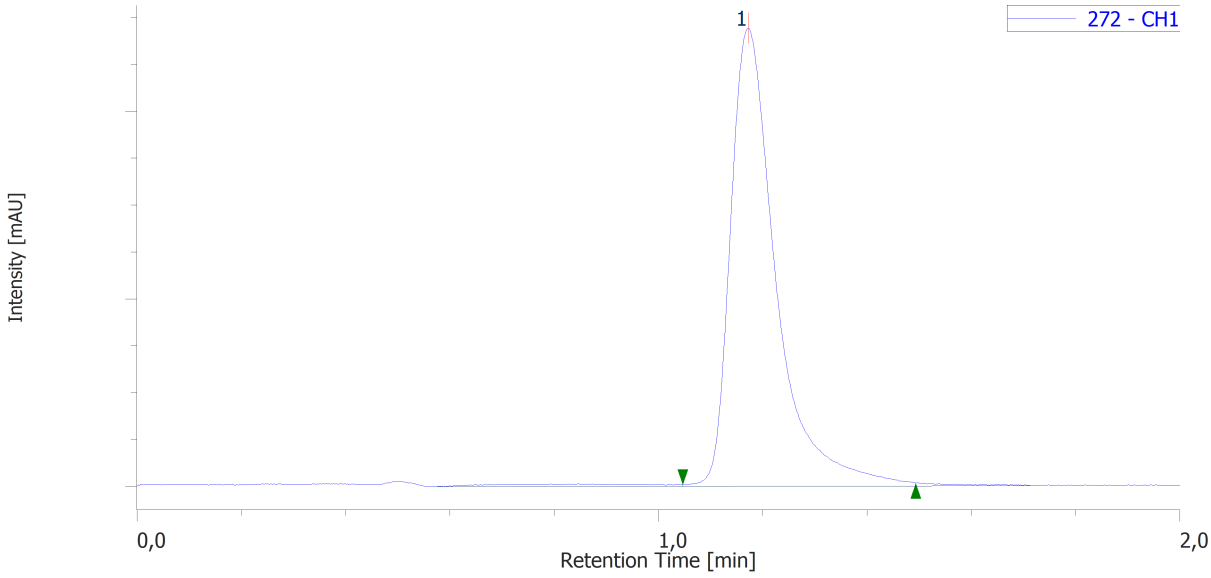

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:21:30
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:19:28
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	272
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	272-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	295946,6	48789,63	100	100	N/A	1035	N/A	1,750	

Creator
Reviewer
Approver

Chromatogram

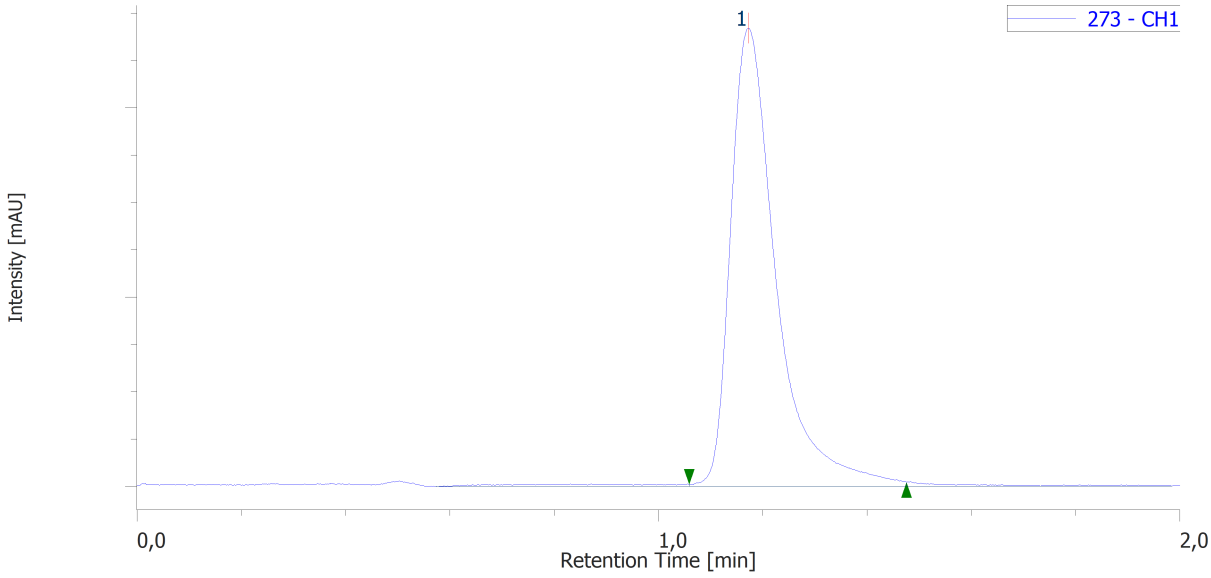

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:23:44
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:21:41
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	273
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	273-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	293786,4	48388,16	100	100	N/A	1032	N/A	1,751	

Creator
Reviewer
Approver

Chromatogram

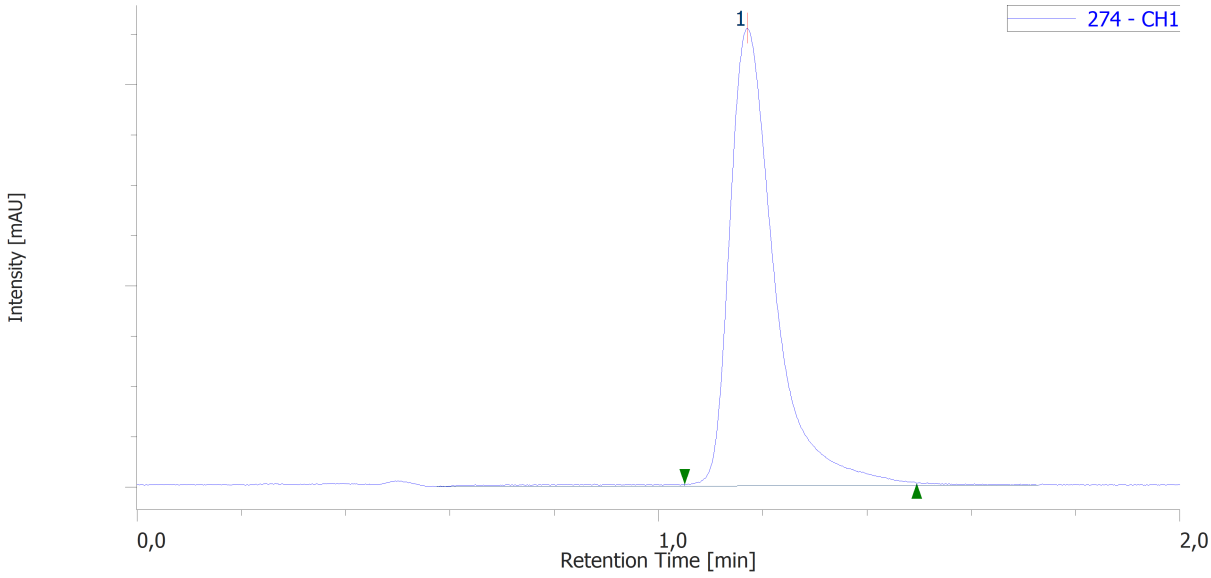

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:27:16
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:25:14
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	274
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	274-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	272553,4	45486,74	100	100	N/A	1050	N/A	1,732	

Creator
Reviewer
Approver

Chromatogram

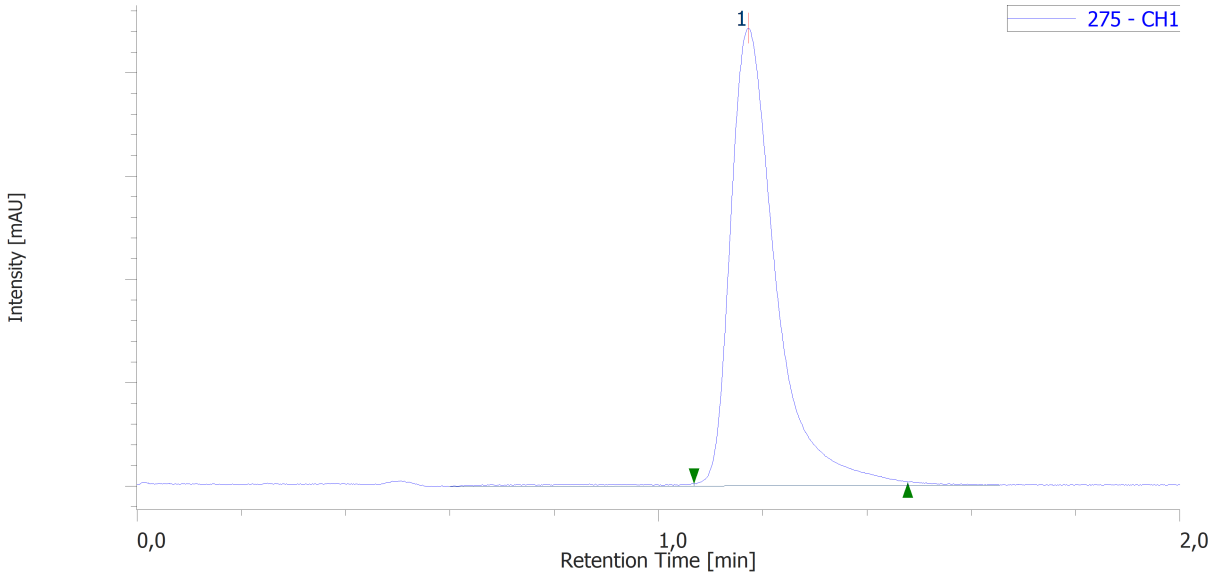

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:29:28
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:27:26
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	275
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	275-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	267181,9	44286,02	100	100	N/A	1035	N/A	1,723	

Creator
Reviewer
Approver

Chromatogram

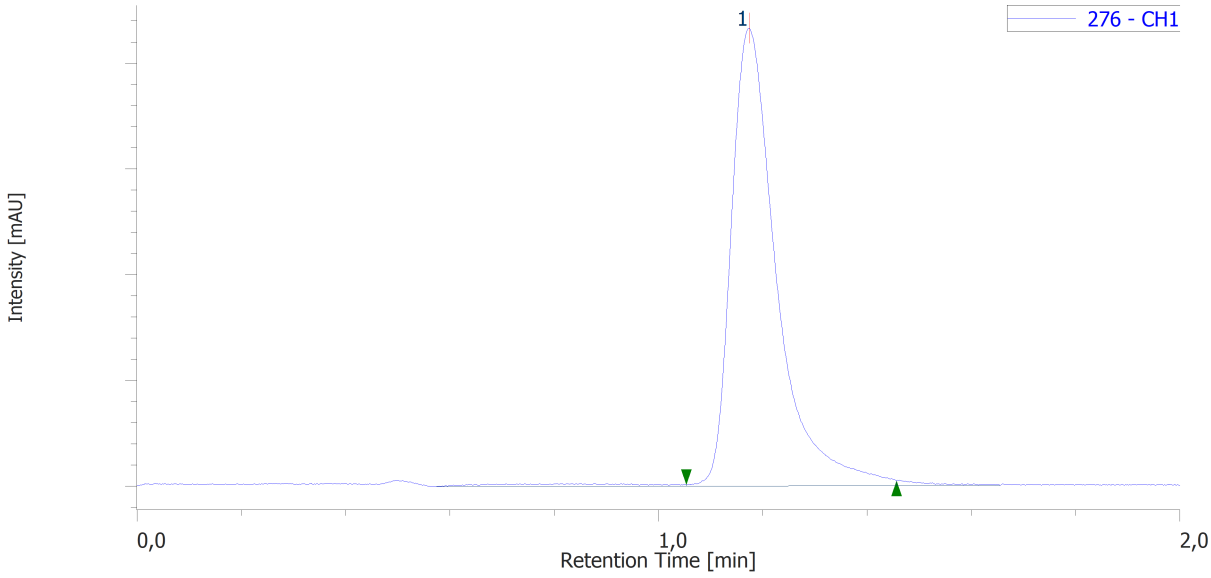

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:31:40
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:29:38
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	276
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	276-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	261333,1	43296,20	100	100	N/A	1034	N/A	1,726	

Creator
Reviewer
Approver

Chromatogram

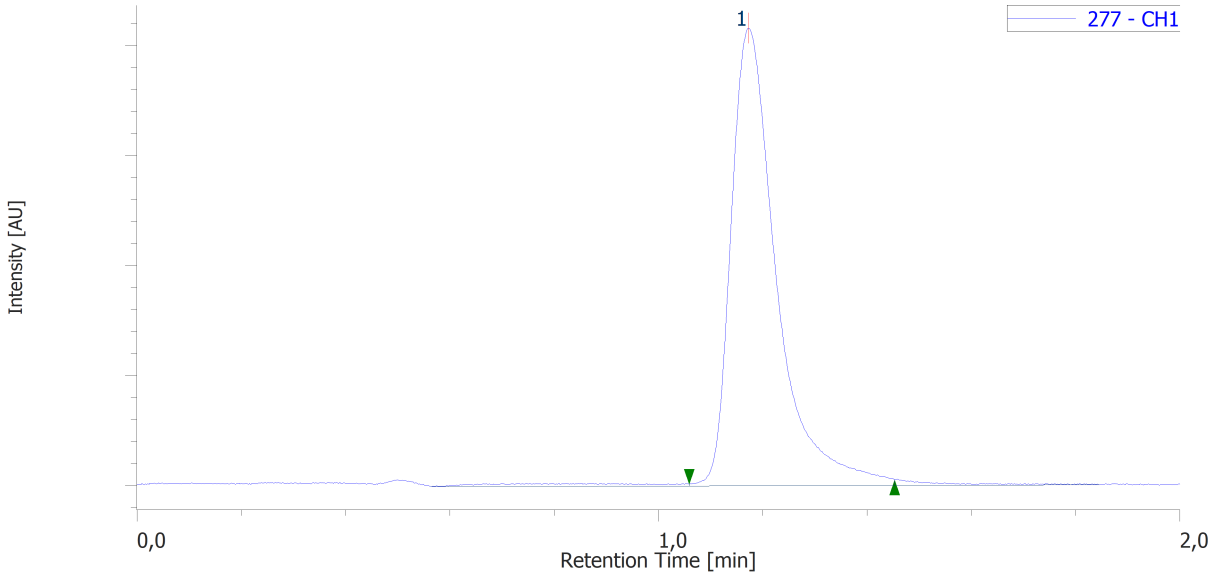

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:33:52
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:31:51
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	277
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	277-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	251176,7	41576,87	100	100	N/A	1031	N/A	1,749	

Creator
Reviewer
Approver

Chromatogram

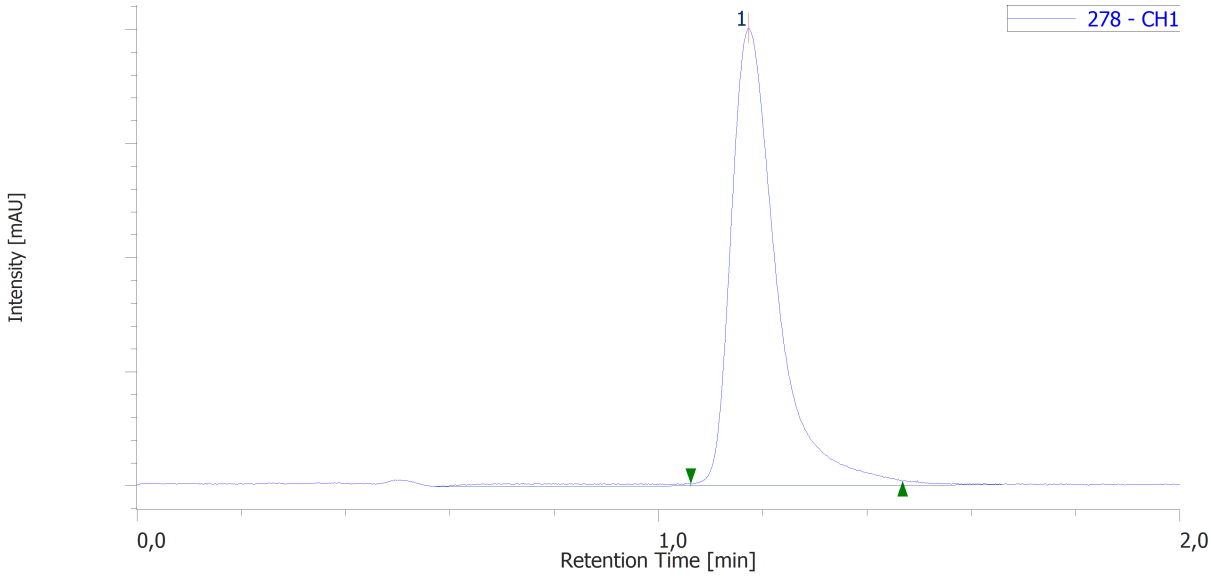

Chromatogram Information	
User Name	QPackSA
Date Modified	23/04/2024 14:36:06
Description	
HPLC System Name	HPL 29
Injection Date	23/04/2024 14:34:03
Volume	10,0 [µL]
Sample #	1
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	EDUV
Control Method	278
Peak ID Table	EDUV
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	278-CH1
Sample Name	
Channel Name	
Sampling Interval	40 [msec]
Peak Method	EDUV_02

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,17	242353,9	40080,91	100	100	N/A	1028	N/A	1,767	

Creator
Reviewer
Approver

Chromatogram

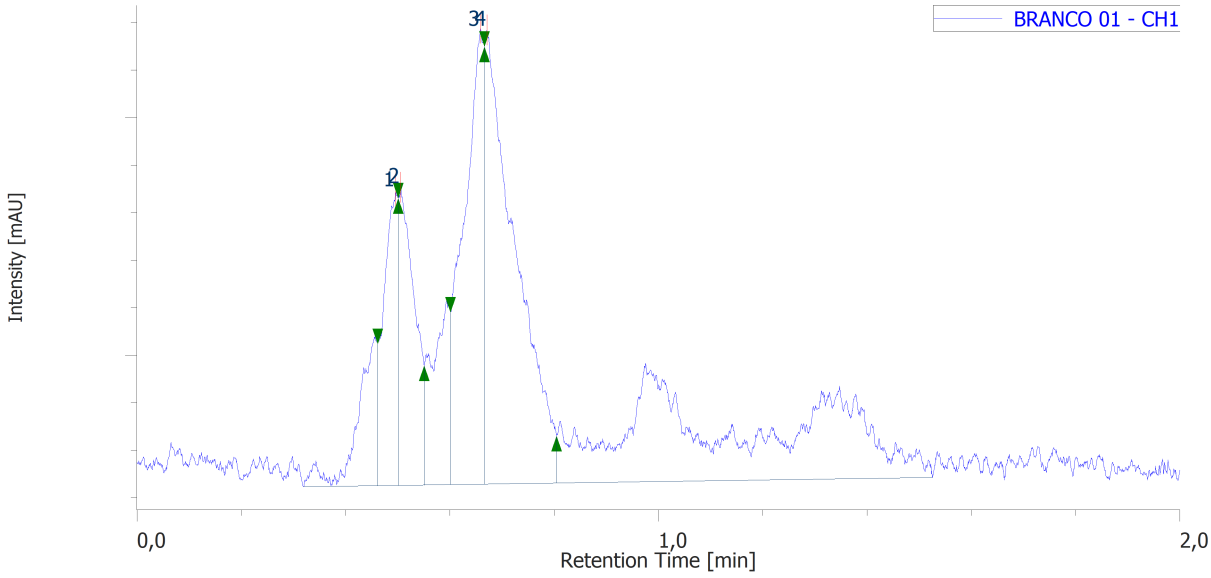

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:20
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:37:12
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	BRANCO 01-CH1
Sample Name	BRANCO 01
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,496	1132,413	620,0702	12,7	19,6	N/A	N/A	N/A	N/A	
2	Peak-001	1	0,505	1349,855	626,9154	15,1	19,8	N/A	N/A	N/A	N/A	
3	Unknown	1	0,659	2568,167	959,3726	28,8	30,3	N/A	N/A	N/A	N/A	
4	Unknown	1	0,671	3881,663	955,1736	43,5	30,2	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

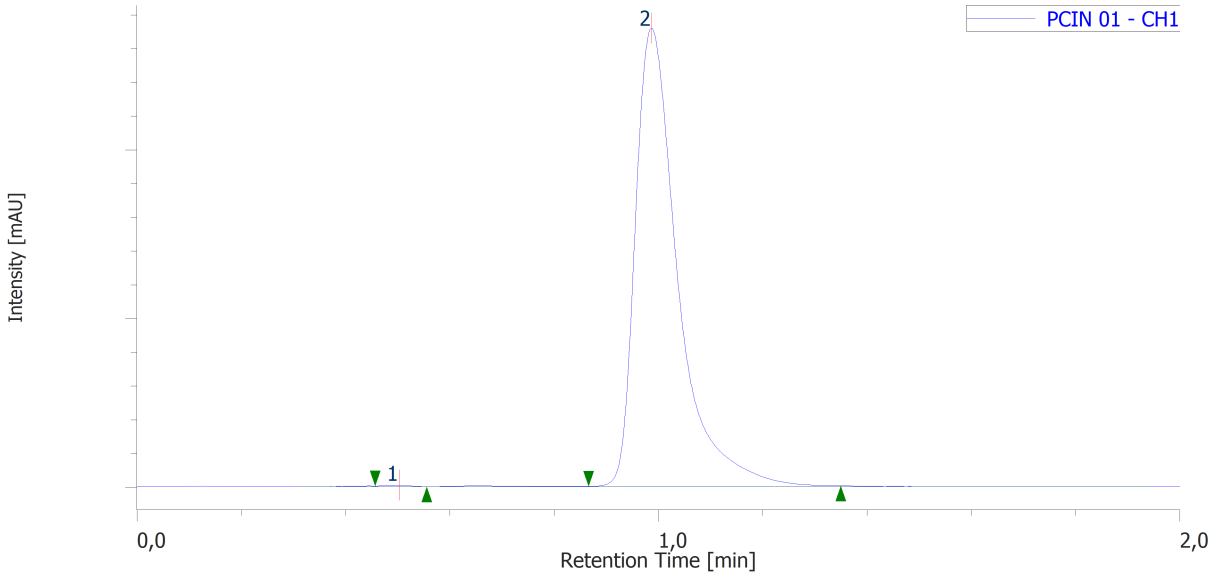

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:21
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:39:25
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	PCIN 01
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,503	1700,292	483,1541	0,220	0,354	N/A	351	3,974	N/A	
2	Cafeína	1	0,987	769442,1	135871,3	99,8	99,6	N/A	830	N/A	1,793	

Creator
Reviewer
Approver

Chromatogram

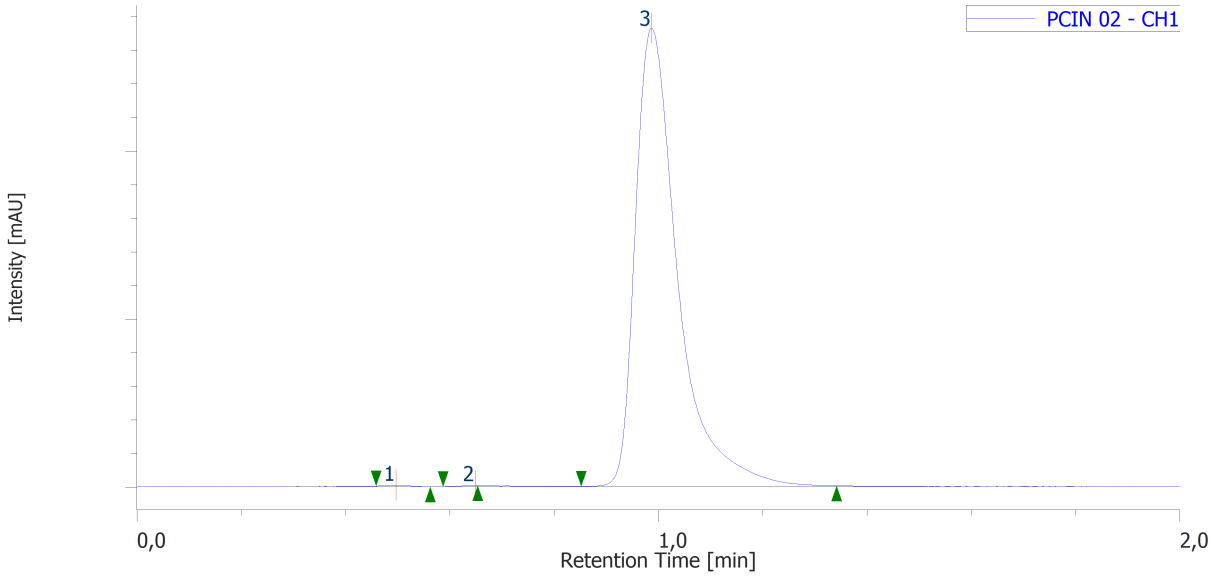

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:21
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:41:37
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	PCIN 02
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,497	1629,978	478,0300	0,211	0,348	N/A	378	N/A	N/A	
2	Unknown	1	0,648	975,1365	393,5766	0,126	0,287	N/A	N/A	N/A	N/A	
3	Cafeína	1	0,987	771027,1	136354,4	99,7	99,4	N/A	831	N/A	1,794	

Creator
Reviewer
Approver

Chromatogram

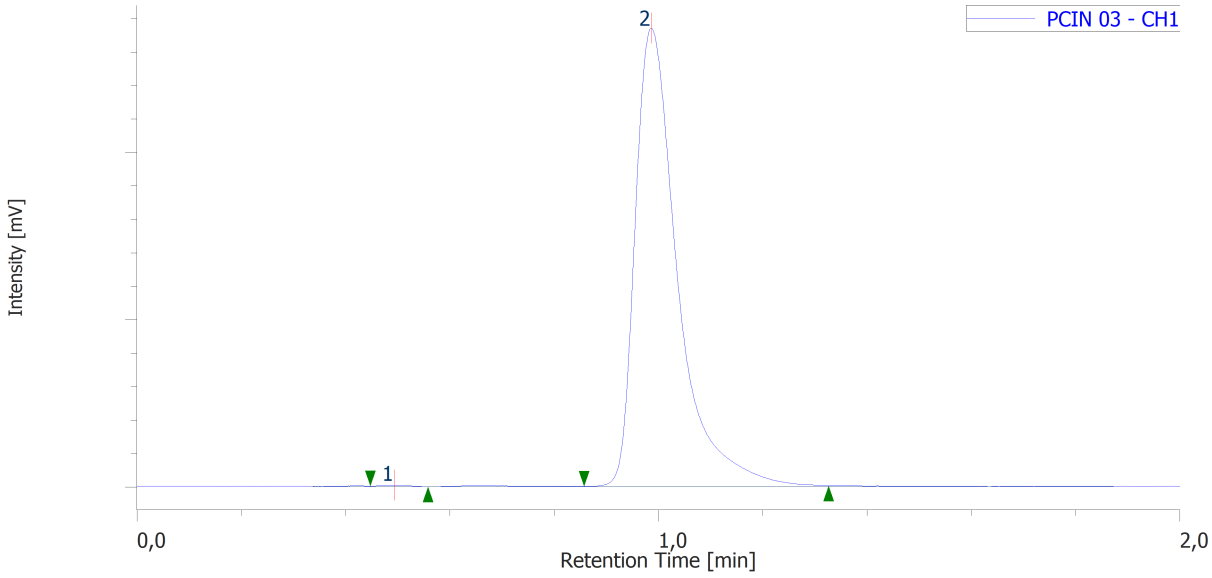

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:22
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:43:49
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	PCIN 03
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,493	1833,893	485,6490	0,236	0,353	N/A	331	4,021	N/A	
2	Cafeína	1	0,986	775023,8	136960,7	99,8	99,6	N/A	825	N/A	1,803	

Creator QPackSA
Reviewer
Approver

Chromatogram

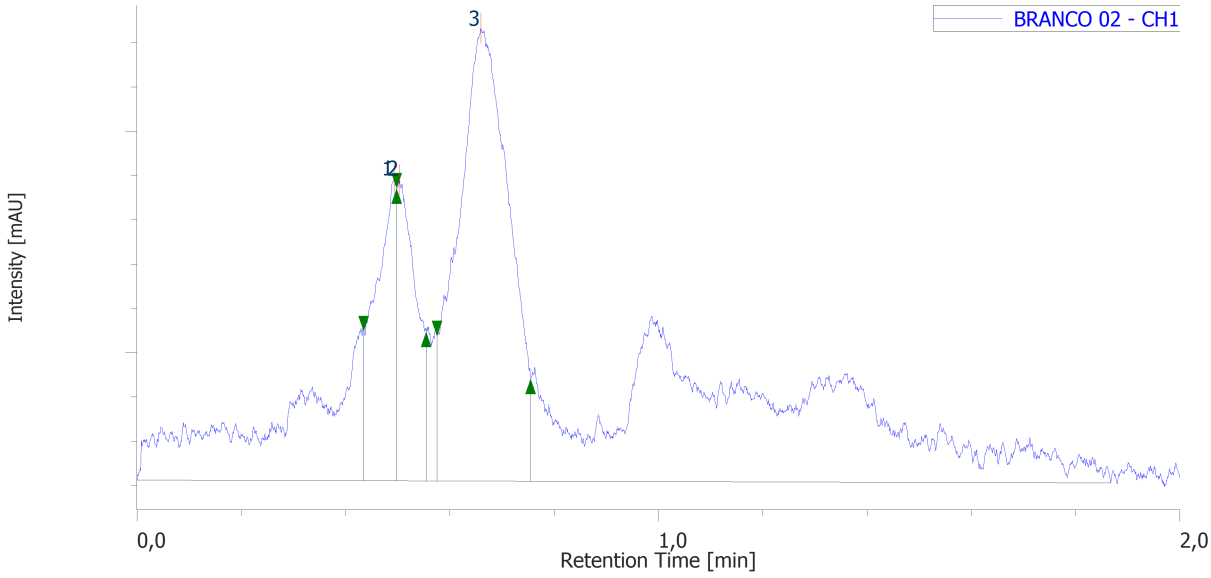

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:23
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:46:02
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	BRANCO 02-CH1
Sample Name	BRANCO 02
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	0,493	1885,416	679,5836	17,7	28,6	N/A	N/A	N/A	N/A	
2	Peak-001	1	0,503	1706,341	678,6179	16,0	28,5	N/A	N/A	N/A	N/A	
3	Unknown	1	0,659	7048,719	1022,119	66,2	42,9	N/A	172	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

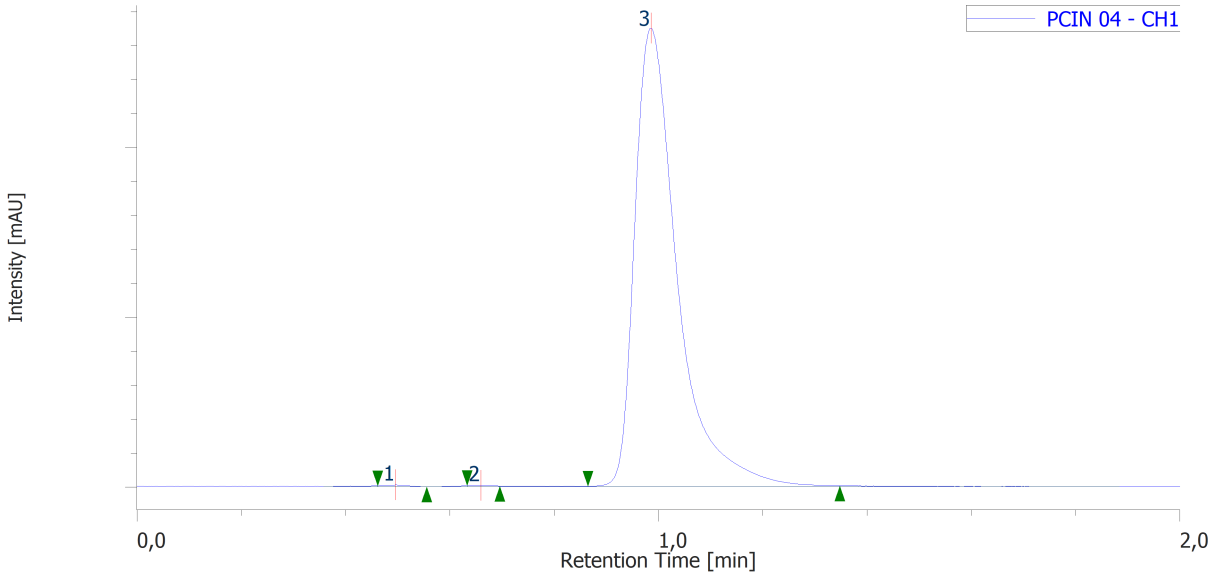

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:23
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:48:15
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	PCIN 04
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,496	1566,904	513,5455	0,204	0,378	N/A	506	N/A	N/A	
2	Unknown	1	0,659	1234,631	384,5602	0,161	0,283	N/A	N/A	N/A	N/A	
3	Cafeína	1	0,985	766328,8	135009,2	99,6	99,3	N/A	822	N/A	1,817	

Creator
Reviewer
Approver

Chromatogram

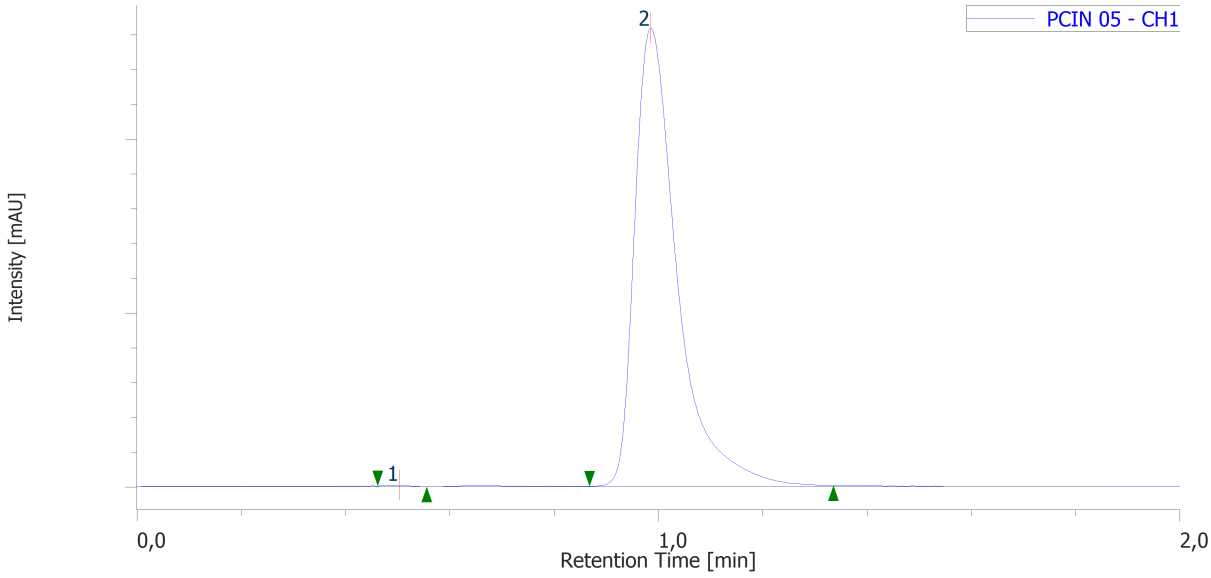

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:24
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:50:27
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	PCIN 05
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,503	1537,168	454,2273	0,205	0,344	N/A	N/A	N/A	N/A	
2	Cafeína	1	0,985	748010,9	131698,4	99,8	99,7	N/A	816	N/A	1,823	

Creator
Reviewer
Approver

Chromatogram

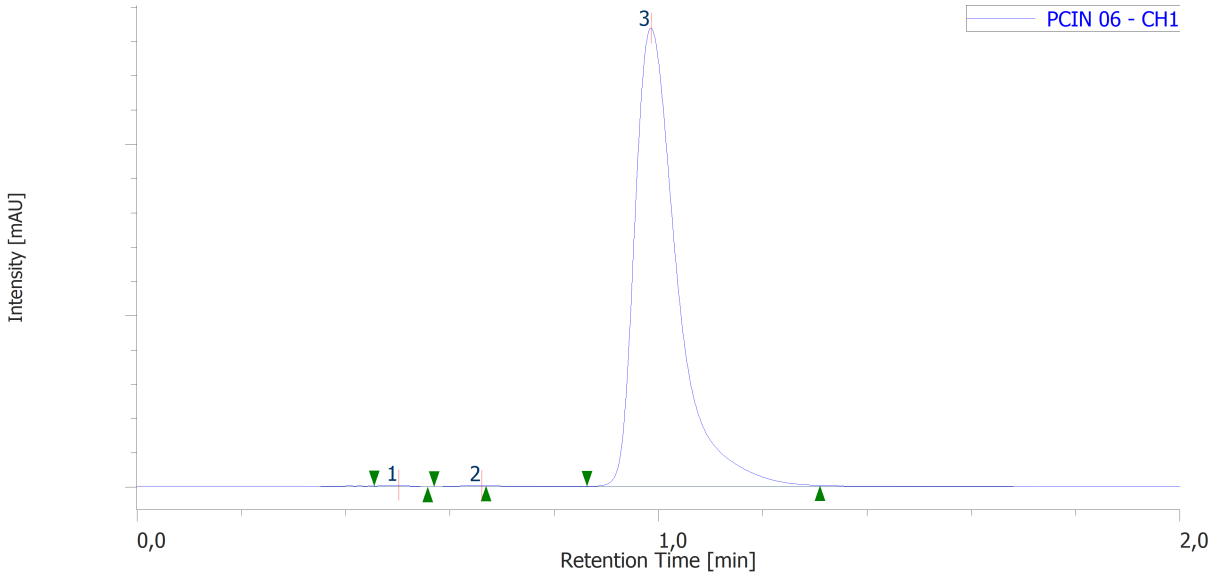

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:25
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:52:39
Volume	10,0 [µL]
Sample #	3
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	PCIN 06
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,502	1572,029	454,8746	0,207	0,338	N/A	427	N/A	N/A	
2	Unknown	1	0,661	1325,539	351,3692	0,174	0,261	N/A	N/A	N/A	N/A	
3	Cafeína	1	0,985	757612,5	133739,8	99,6	99,4	N/A	821	N/A	1,812	

Creator
Reviewer
Approver

Chromatogram

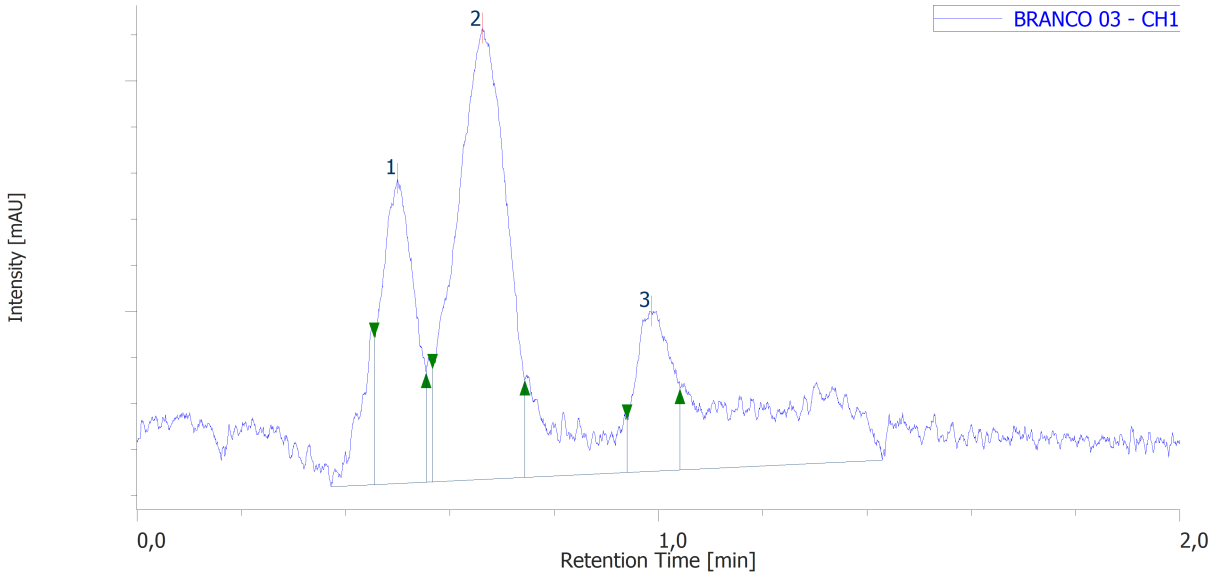

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:25
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:54:52
Volume	10,0 [µL]
Sample #	2
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	BRANCO 03-CH1
Sample Name	BRANCO 03
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,499	2832,648	662,0107	25,7	33,3	N/A	208	0,988	N/A	
2	Unknown	1	0,662	6575,002	979,0820	59,7	49,2	N/A	191	N/A	N/A	
3	Cafeína	1	0,986	1601,836	347,2978	14,5	17,5	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

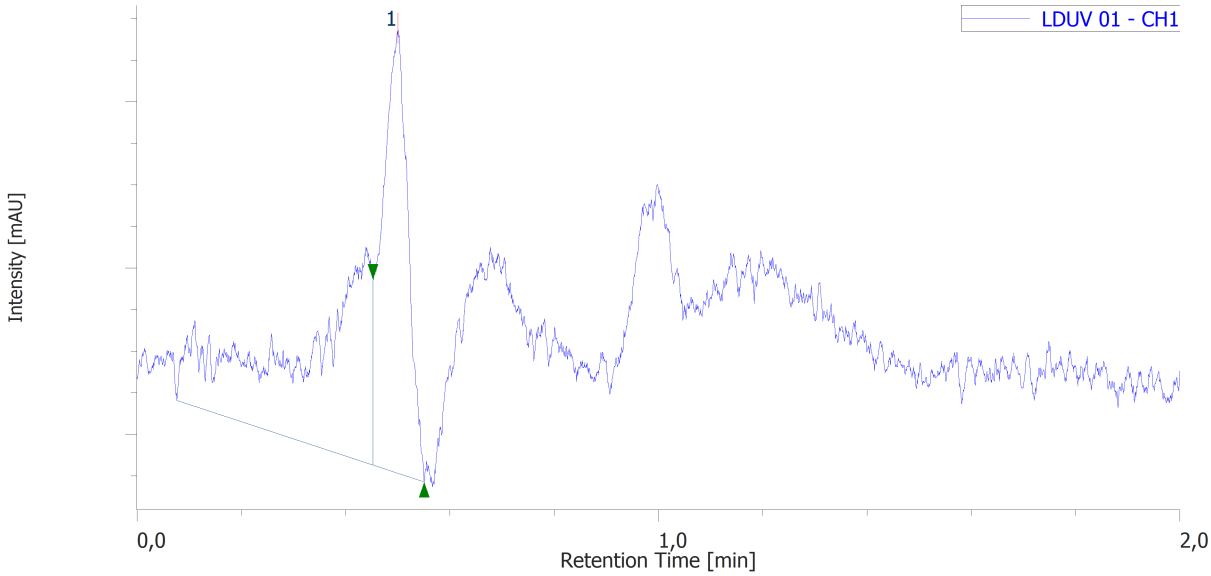

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:26
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:57:05
Volume	10,0 [µL]
Sample #	4
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	LDUV 01
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,500	1800,082	534,5393	100	100	N/A	429	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

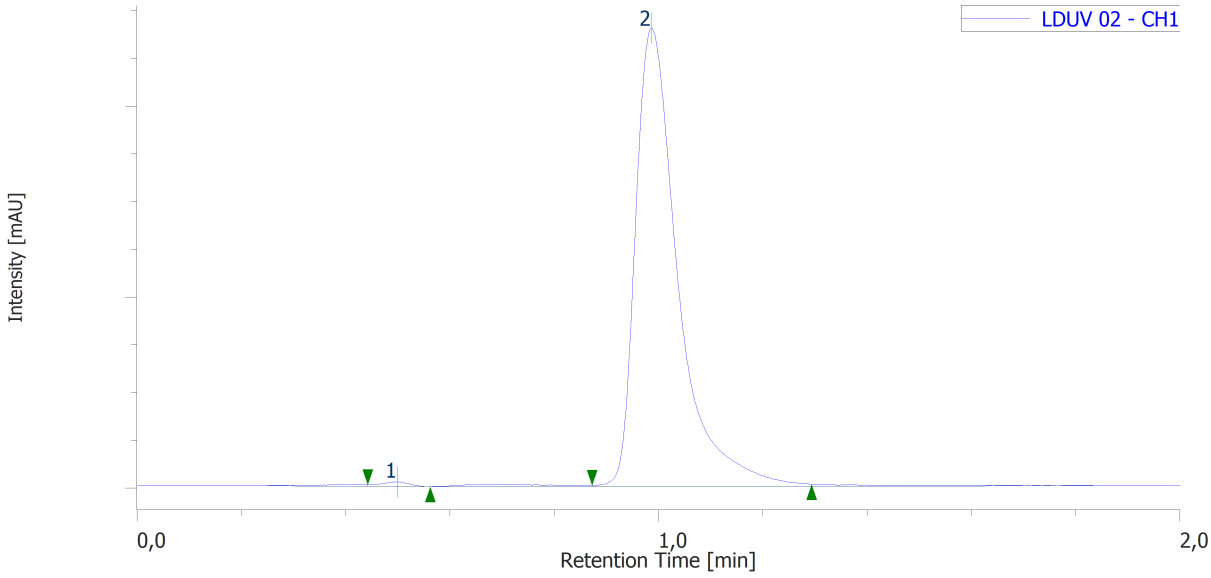

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:27
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 15:59:17
Volume	10,0 [µL]
Sample #	5
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	LDUV 02
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,499	1891,787	500,2000	0,694	1,03	N/A	382	4,095	N/A	
2	Cafeína	1	0,987	270892,7	47977,85	99,3	99,0	N/A	837	N/A	1,832	

Creator
Reviewer
Approver

Chromatogram

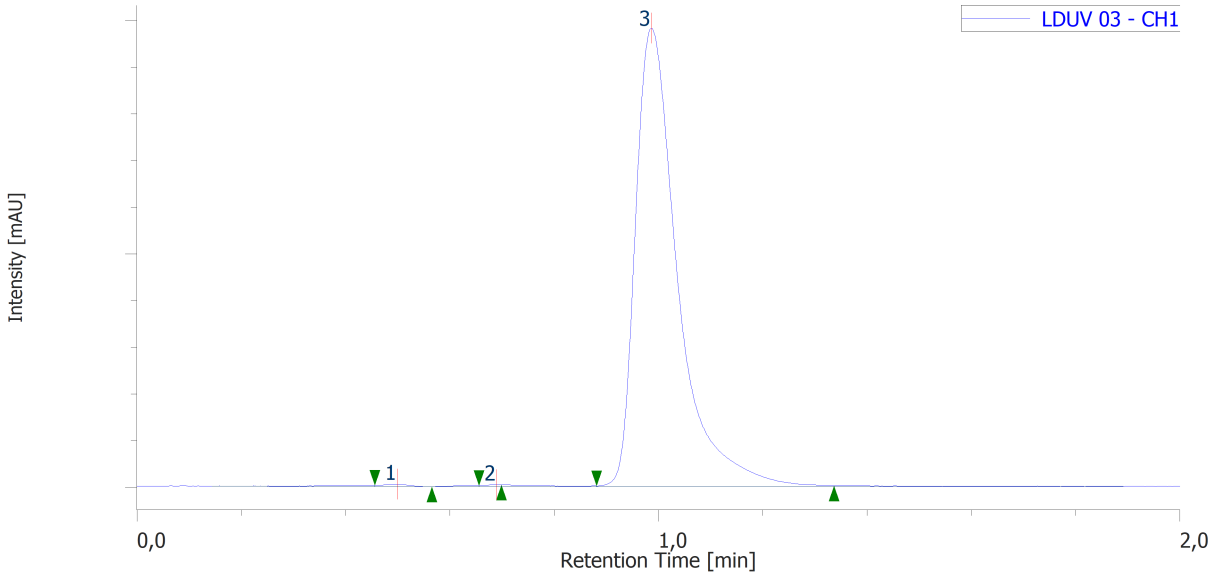

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:27
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:01:29
Volume	10,0 [µL]
Sample #	6
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	LDUV 03
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,499	1962,036	545,2152	0,354	0,550	N/A	N/A	N/A	N/A	
2	Unknown	1	0,689	950,1771	424,5264	0,171	0,429	N/A	N/A	N/A	N/A	
3	Cafeína	1	0,986	551150,6	98089,47	99,5	99,0	N/A	840	N/A	1,828	

Creator
Reviewer
Approver

Chromatogram

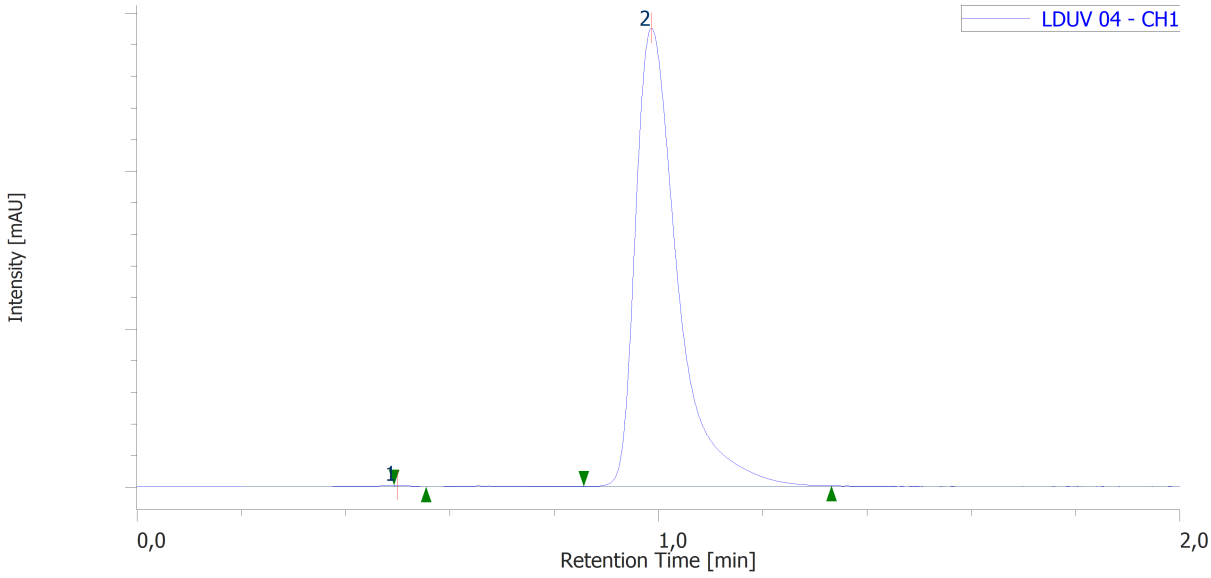

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:28
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:03:42
Volume	10,0 [µL]
Sample #	7
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	LDUV 04
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,499	994,0254	509,0876	0,122	0,350	N/A	N/A	N/A	N/A	
2	Cafeína	1	0,987	814317,3	145030,6	99,9	99,7	N/A	841	N/A	1,806	

Creator
Reviewer
Approver

Chromatogram

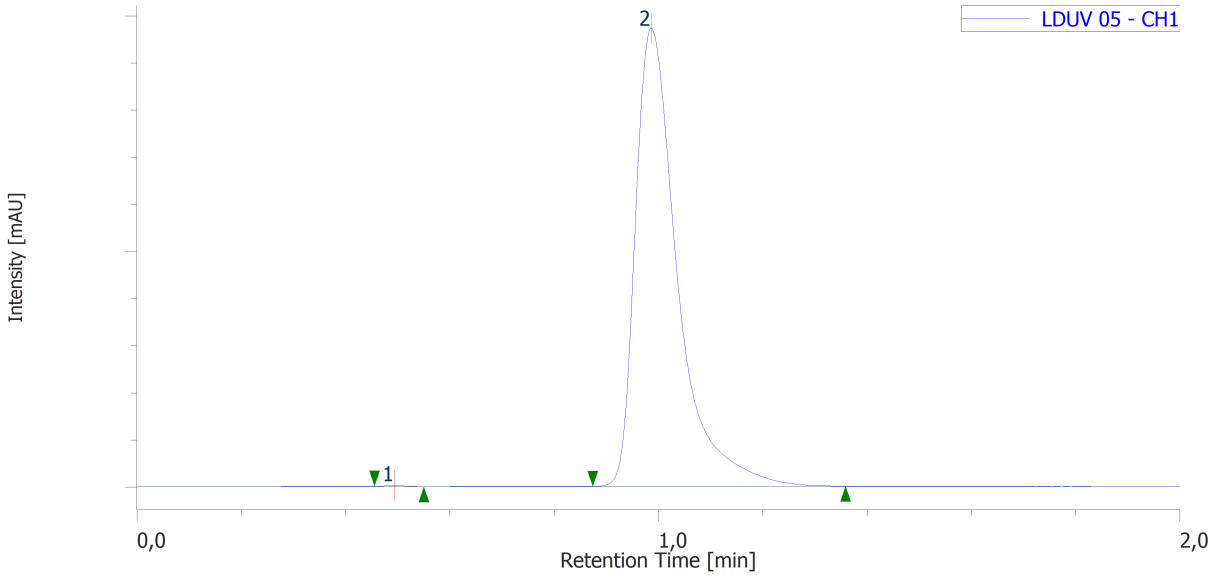

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:29
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:05:54
Volume	10,0 [µL]
Sample #	8
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	LDUV 05
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,494	1737,318	514,1191	0,159	0,264	N/A	378	4,147	N/A	
2	Cafeína	1	0,986	1094340	194569,5	99,8	99,7	N/A	836	N/A	1,819	

Creator
Reviewer
Approver

Chromatogram

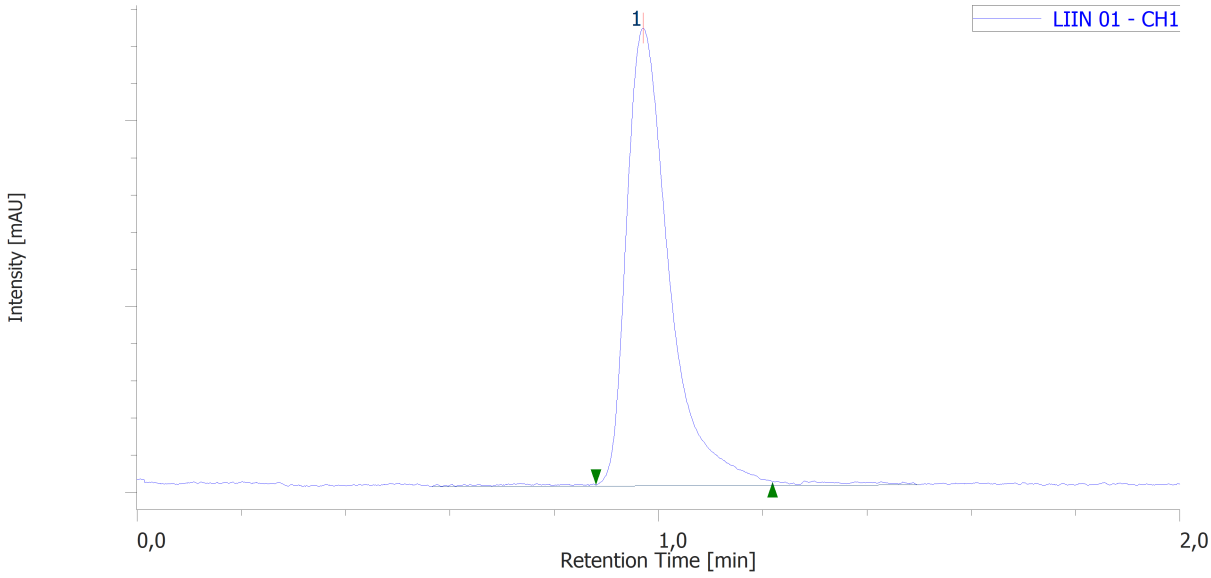

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:29
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:29:42
Volume	0,1 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	LIIN 01
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,970	70080,06	12319,90	100	100	N/A	773	N/A	1,759	

Creator
Reviewer
Approver

Chromatogram

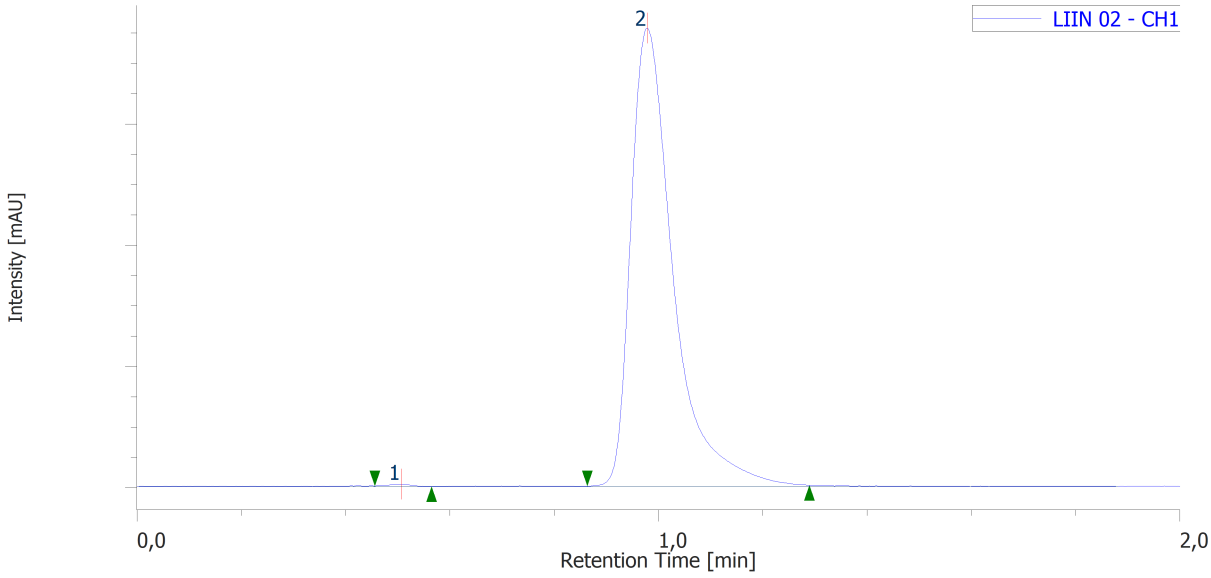

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:30
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:31:55
Volume	5,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	LIIN 02
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,506	1426,964	396,0671	0,333	0,521	N/A	439	4,045	N/A	
2	Cafeína	1	0,978	427473,8	75565,46	99,7	99,5	N/A	810	N/A	1,793	

Creator
Reviewer
Approver

Chromatogram

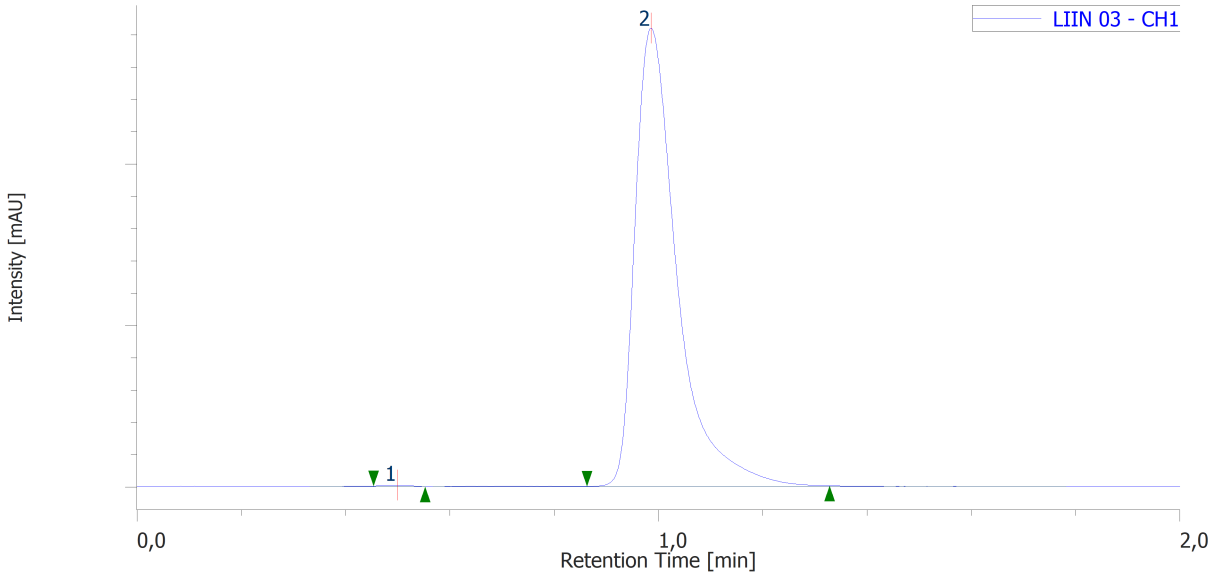

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:31
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:34:07
Volume	10,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	LIIN 03
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,499	1834,108	512,1416	0,229	0,360	N/A	372	4,071	N/A	
2	Cafeína	1	0,985	797857,2	141883,5	99,8	99,6	N/A	836	N/A	1,823	

Creator
Reviewer
Approver

Chromatogram

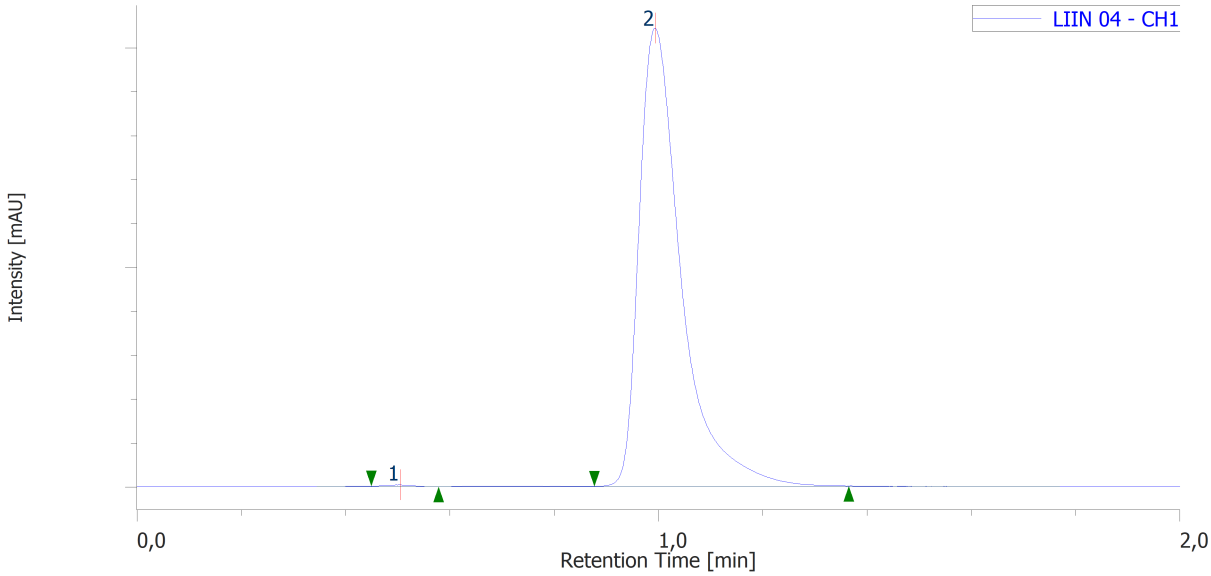

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:31
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:36:20
Volume	15,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	LIIN 04
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,505	3146,749	803,6000	0,267	0,383	N/A	339	3,997	N/A	
2	Cafeína	1	0,993	1173341	208783,6	99,7	99,6	N/A	859	N/A	1,838	

Creator
Reviewer
Approver

Chromatogram

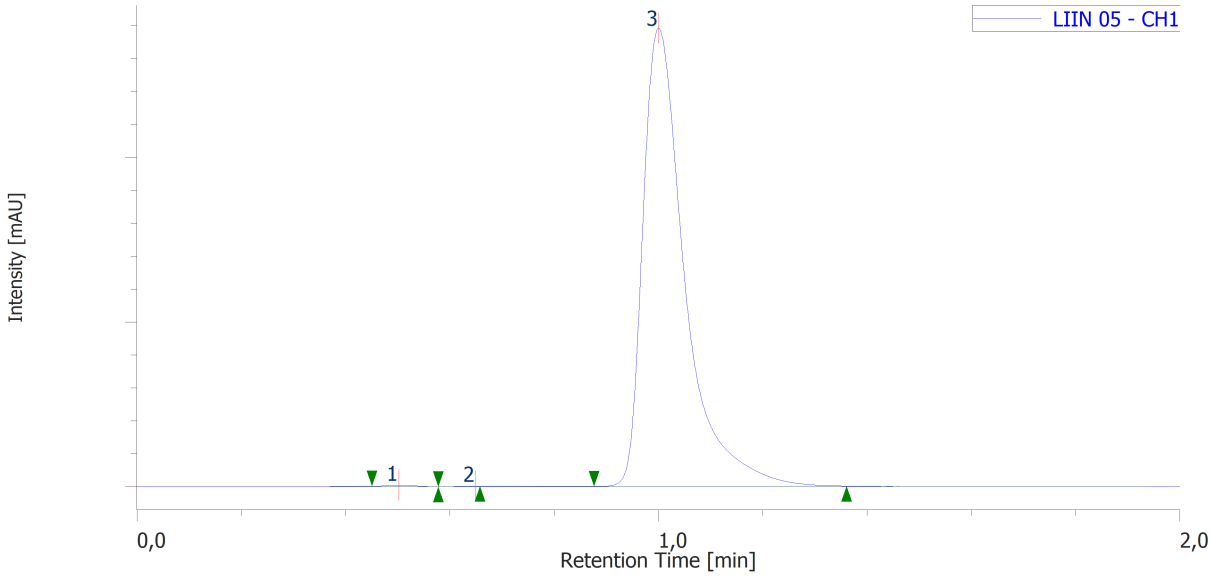

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:04:32
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:38:32
Volume	20,0 [µL]
Sample #	9
Project Name	QUALIFICAÇÃO
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	QUALIFICAÇÃO
Peak ID Table	CAFEÍNA_2024
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	LIIN 05
Channel Name	
Sampling Interval	40 [msec]
Peak Method	QUALIFICAÇÃO-2024

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Peak-001	1	0,502	4210,391	1056,538	0,270	0,378	N/A	326	N/A	N/A	
2	Unknown	1	0,649	1072,616	419,9419	0,0688	0,150	N/A	N/A	N/A	N/A	
3	Cafeína	1	1,00	1553143	278117,5	99,7	99,5	N/A	883	N/A	1,863	

Creator
Reviewer
Approver

Chromatogram

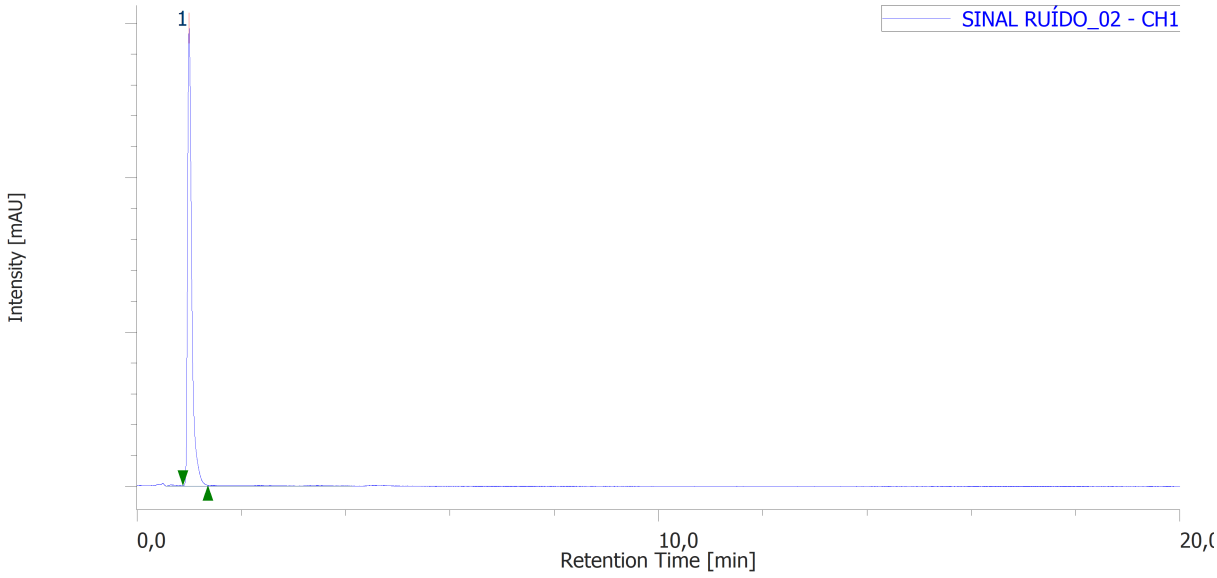

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:00:46
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:40:45
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	SINAL RUÍDO
Peak ID Table	SINAL RUÍDO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	SINAL RUÍDO_02-CH1
Sample Name	SINAL RUÍDO
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Sinal Ruido

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,997	829087,2	148185,0	100	100	N/A	878	N/A	1,899	

Creator
Reviewer
Approver

Chromatogram

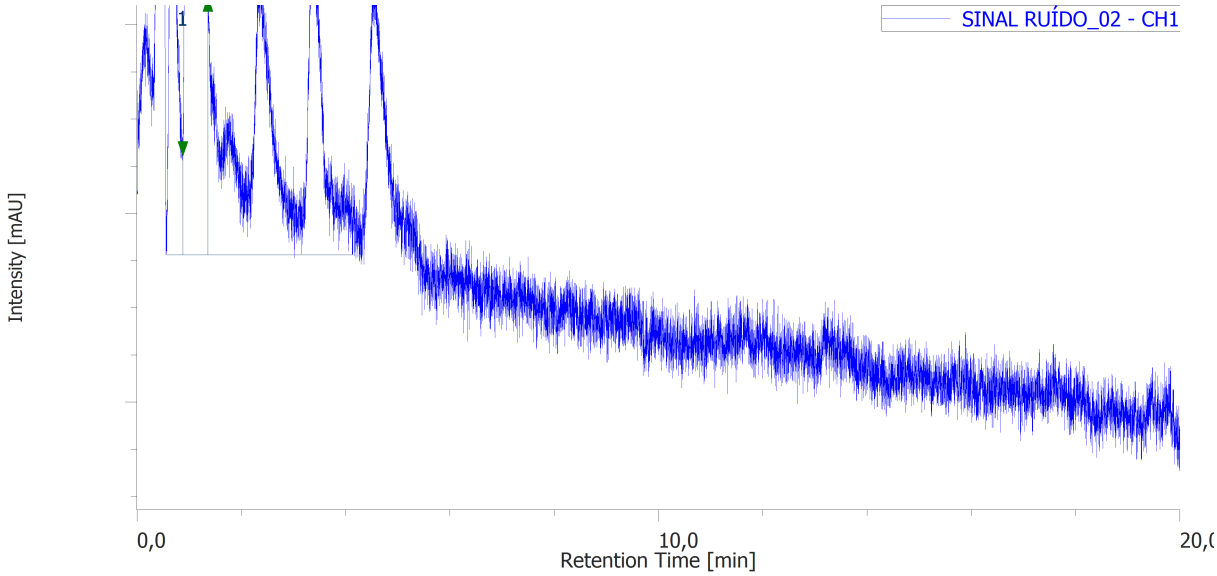

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:00:46
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:40:45
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	SINAL RUÍDO
Peak ID Table	SINAL RUÍDO
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	SINAL RUÍDO_02-CH1
Sample Name	SINAL RUÍDO
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Sinal Ruido

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,997	829087,2	148185,0	100	100	N/A	878	N/A	1,899	

Creator
Reviewer
Approver

Chromatogram

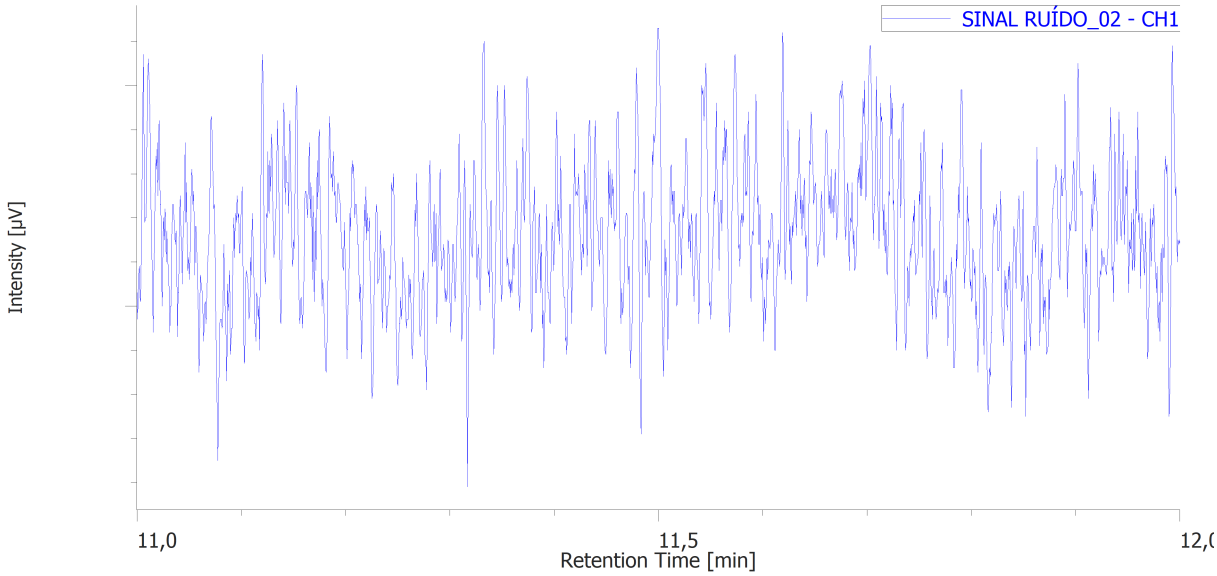

Chromatogram Information	
User Name	QPackSA
Date Modified	22/04/2024 17:00:46
Description	
HPLC System Name	HPL 29
Injection Date	22/04/2024 16:40:45
Volume	20,0 [µL]
Sample #	10
Project Name	QUALIFICAÇÃO
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação 2024
Control Method	SINAL RUÍDO
Peak ID Table	SINAL RUÍDO
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	SINAL RUÍDO_02-CH1
Sample Name	SINAL RUÍDO
Channel Name	
Sampling Interval	40 [msec]
Peak Method	Sinal Ruido

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	0,997	829087,2	148185,0	100	100	N/A	878	N/A	1,899	

Creator
Reviewer
Approver