
Peak Find - EDUV_001 PDA_2,9300.JWS

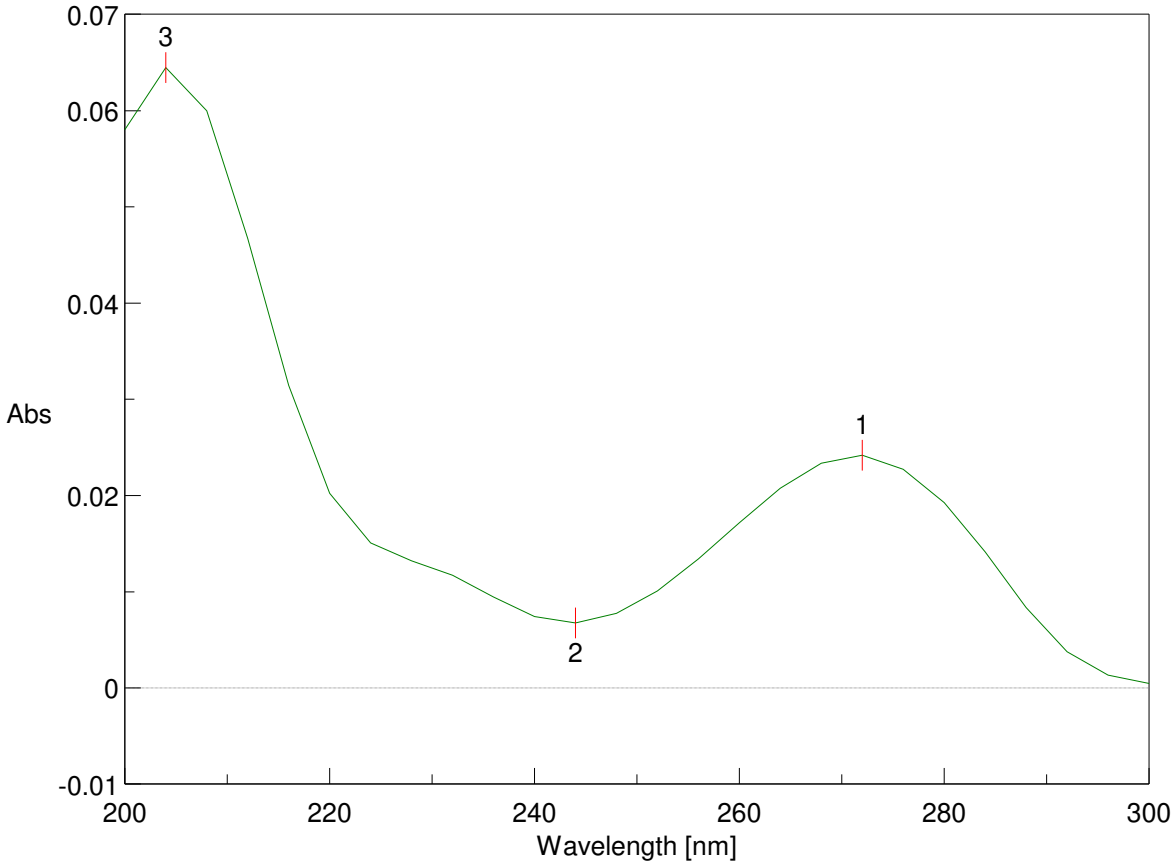

[Comments]

User	Administrator
Division	---
Company	Valer
Creation date	08/08/2019 09:52

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A031161665
ROM version	V1.02.03

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.024172	2	244	0.006727
3	204	0.06444			

Chromatogram

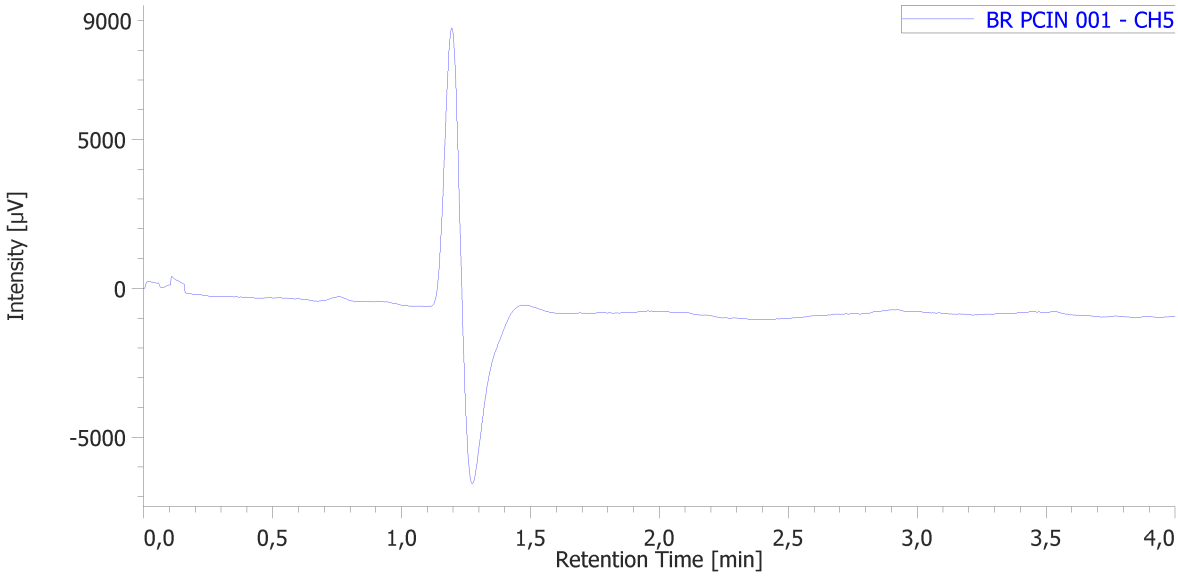


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 13:43:54
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 13:39:52
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

Creator
Reviewer
Approver

Chromatogram

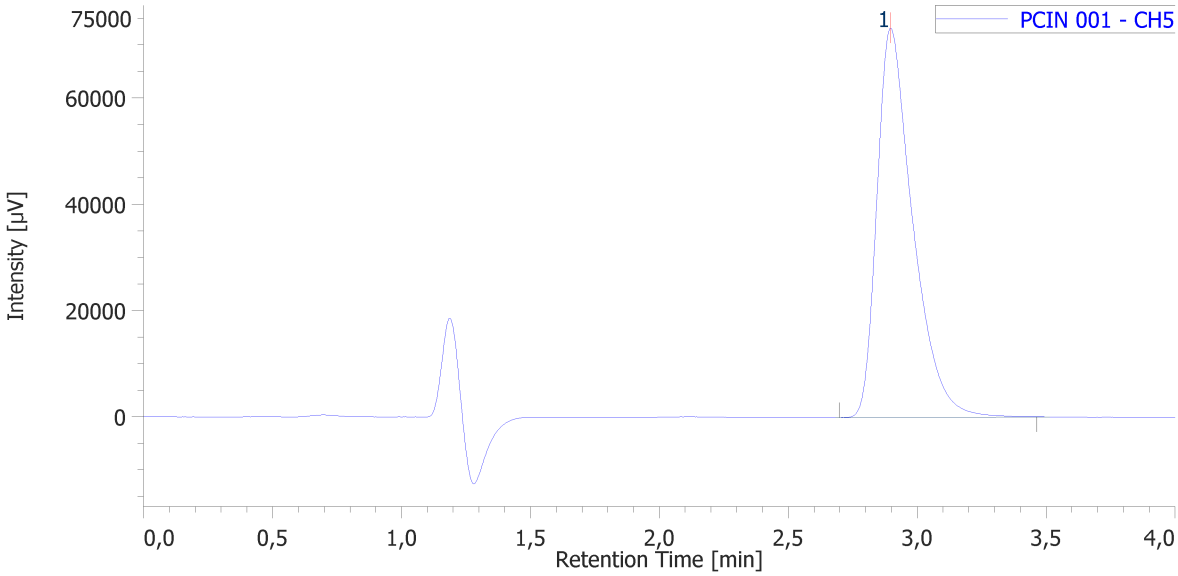

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 13:48:06
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 13:44:04
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,897	708149	73258	100,000	100,000	N/A	2242	N/A	1,520	

Creator
Reviewer
Approver

Chromatogram

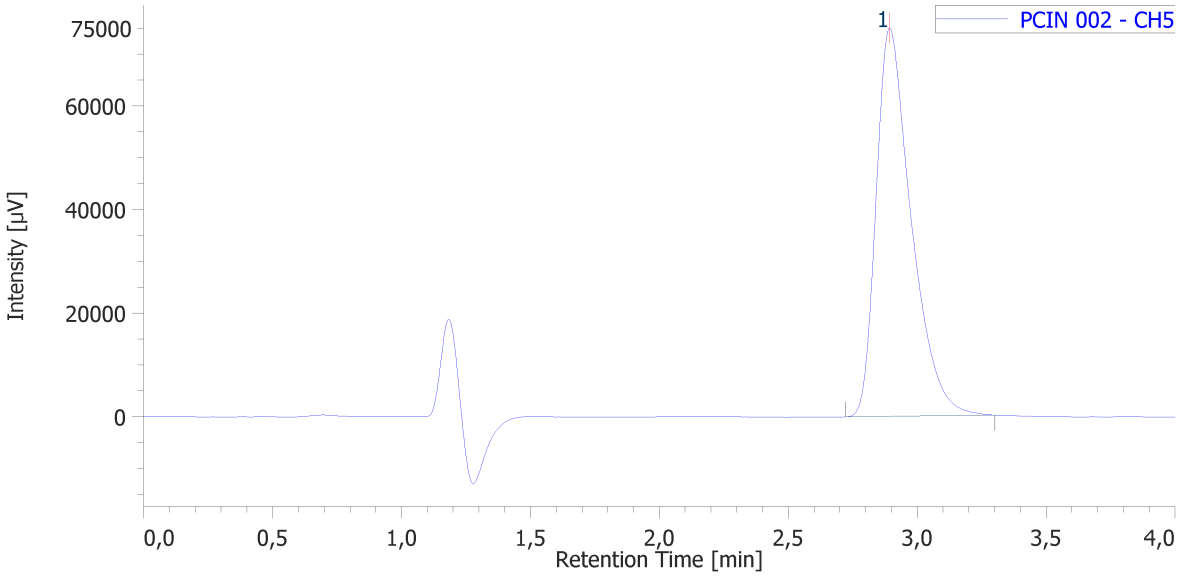

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 13:52:18
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 13:48:17
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,893	709350	74926	100,000	100,000	N/A	2303	N/A	1,494	

Creator
Reviewer
Approver

Chromatogram

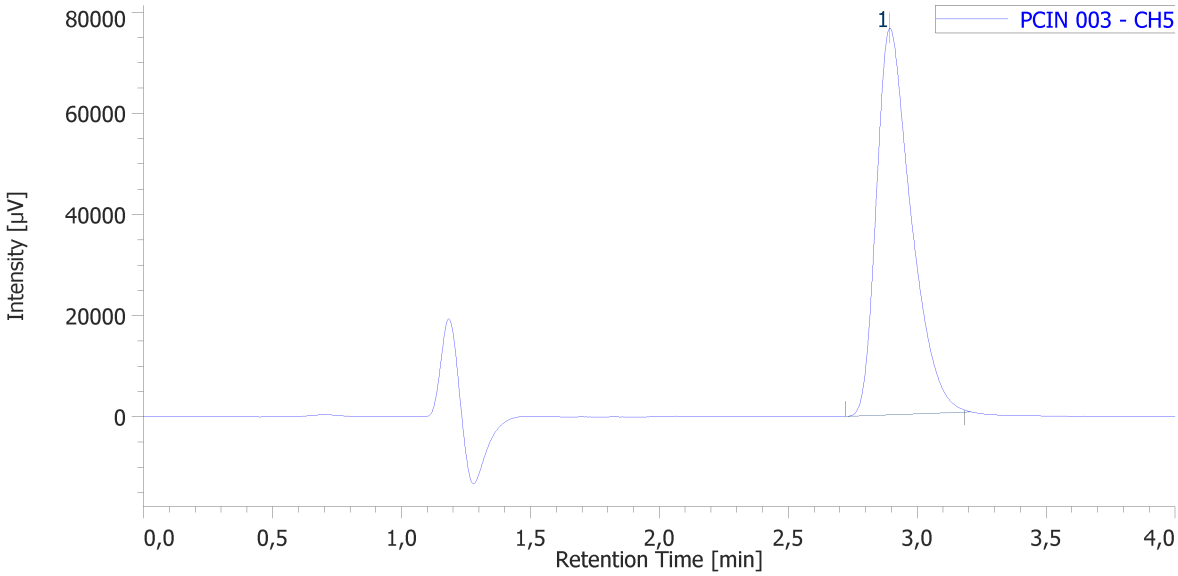

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 13:56:30
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 13:52:29
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,893	713886	76441	100,000	100,000	N/A	2315	N/A	1,473	

Creator
Reviewer
Approver

Chromatogram

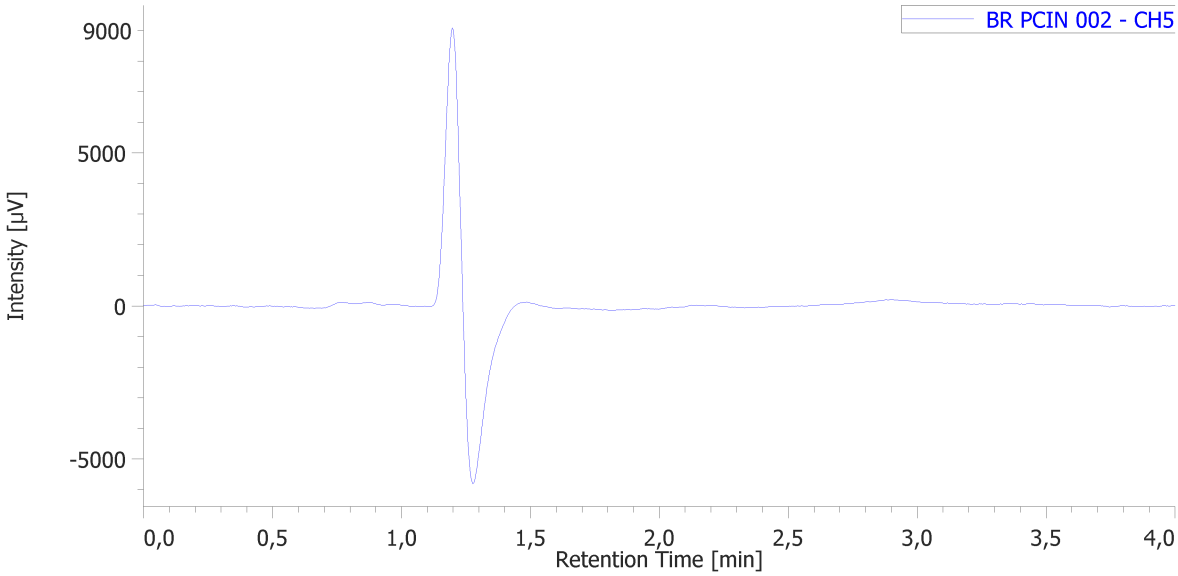


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:00:44
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 13:56:41
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

Creator
Reviewer
Approver

Chromatogram

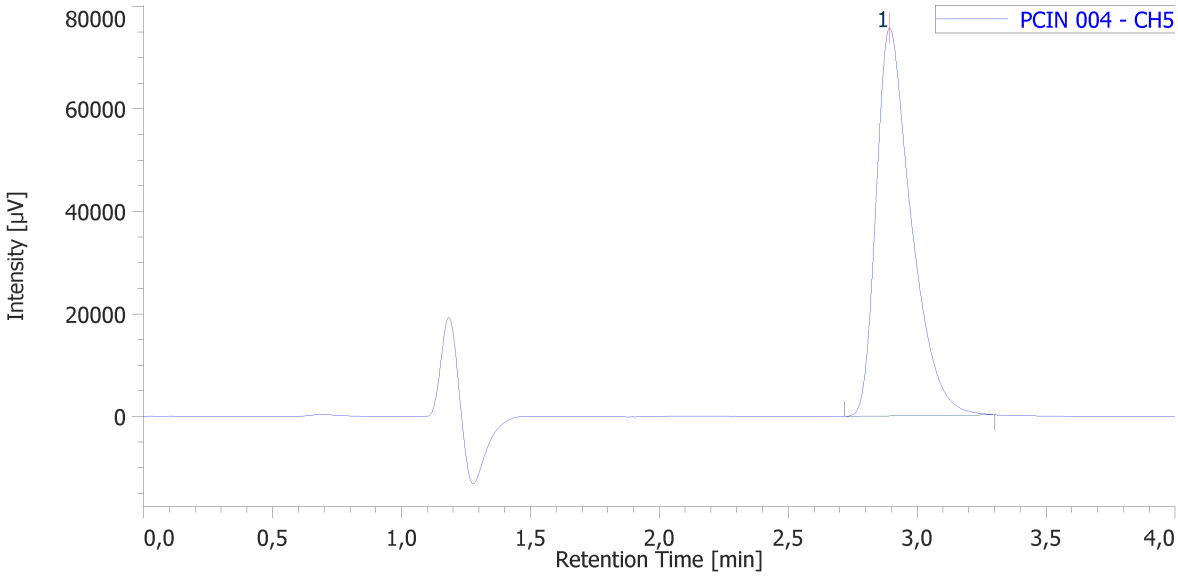

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 14:04:56
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:00:54
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,893	715247	75640	100,000	100,000	N/A	2313	N/A	1,499	

Creator
Reviewer
Approver

Chromatogram

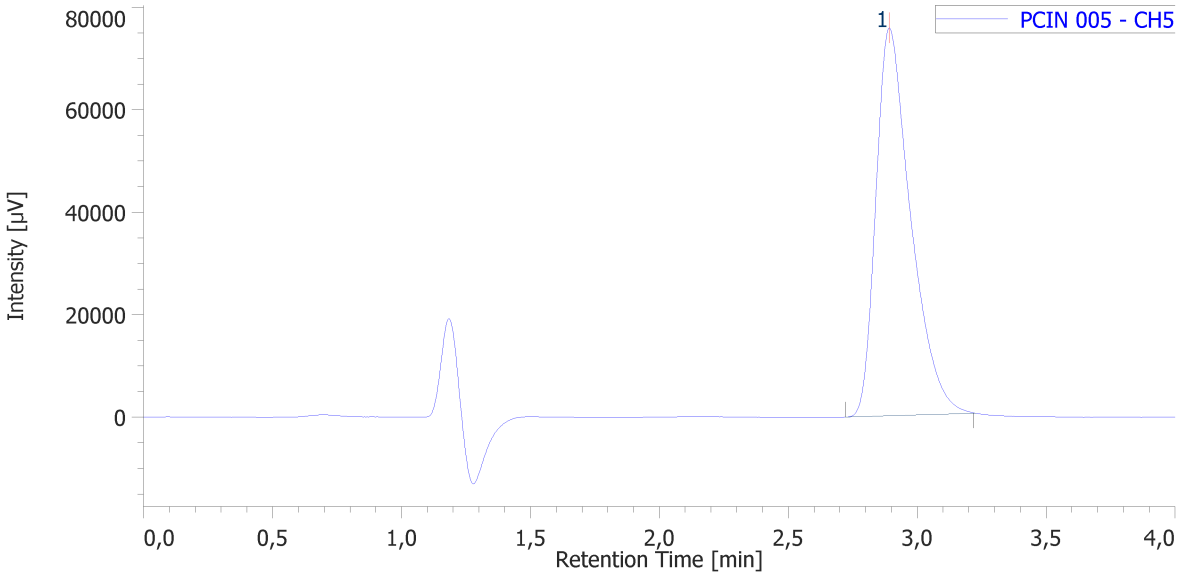

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 14:09:08
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:05:06
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,890	710752	75667	100,000	100,000	N/A	2310	N/A	1,516	

Creator
Reviewer
Approver

Chromatogram

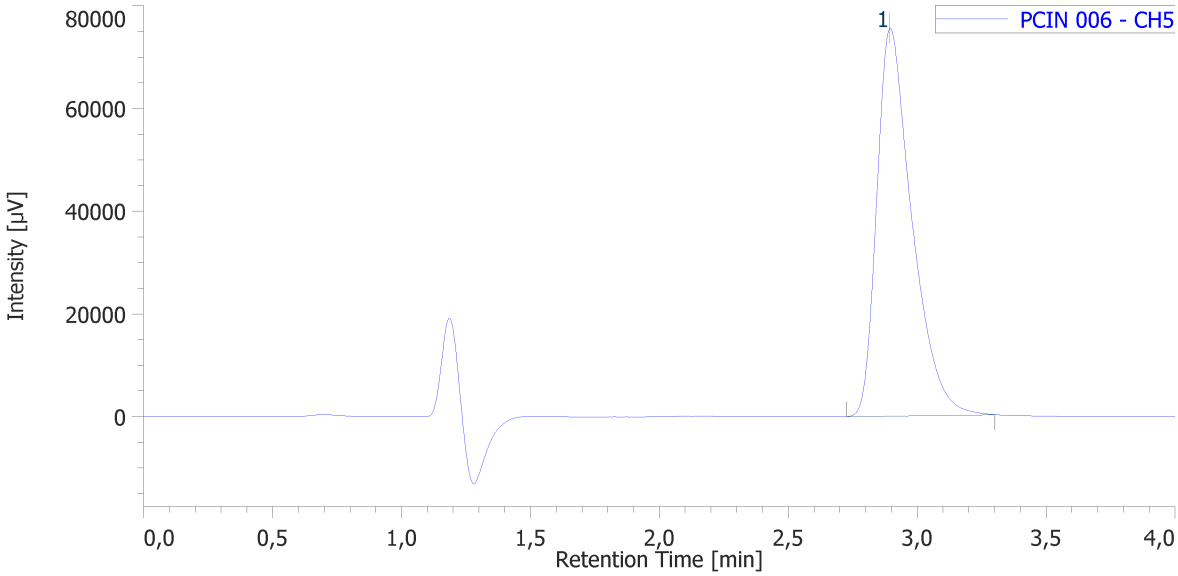

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 14:13:20
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:09:18
Volume	10,00 [µL]
Sample #	3
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,893	715079	75521	100,000	100,000	N/A	2304	N/A	1,534	

Creator
Reviewer
Approver

Chromatogram

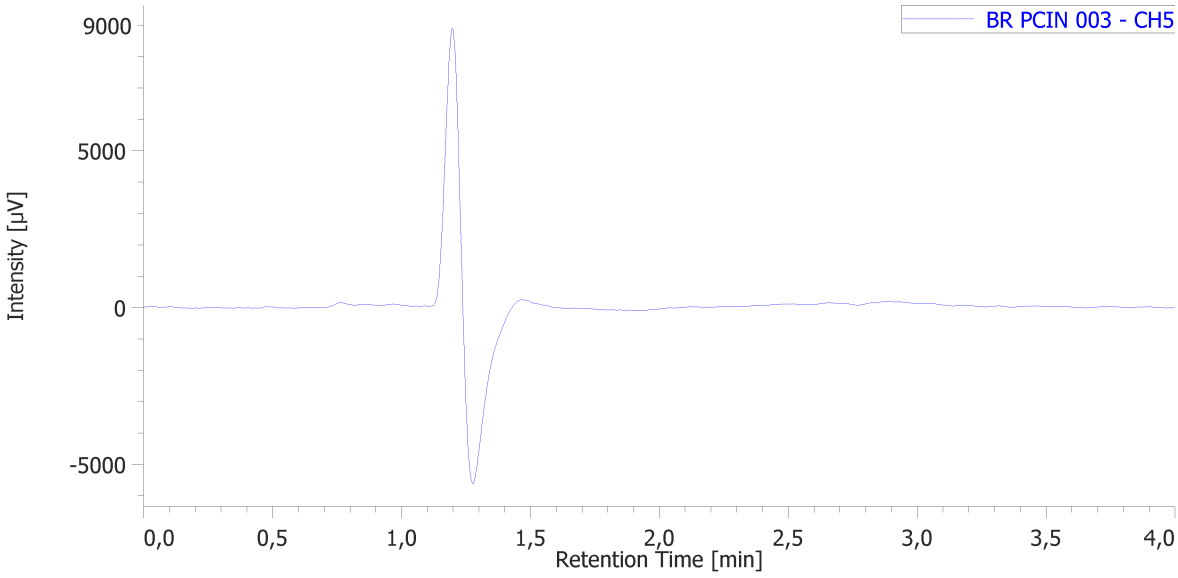


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:17:32
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:13:30
Volume	10,00 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BR PCIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

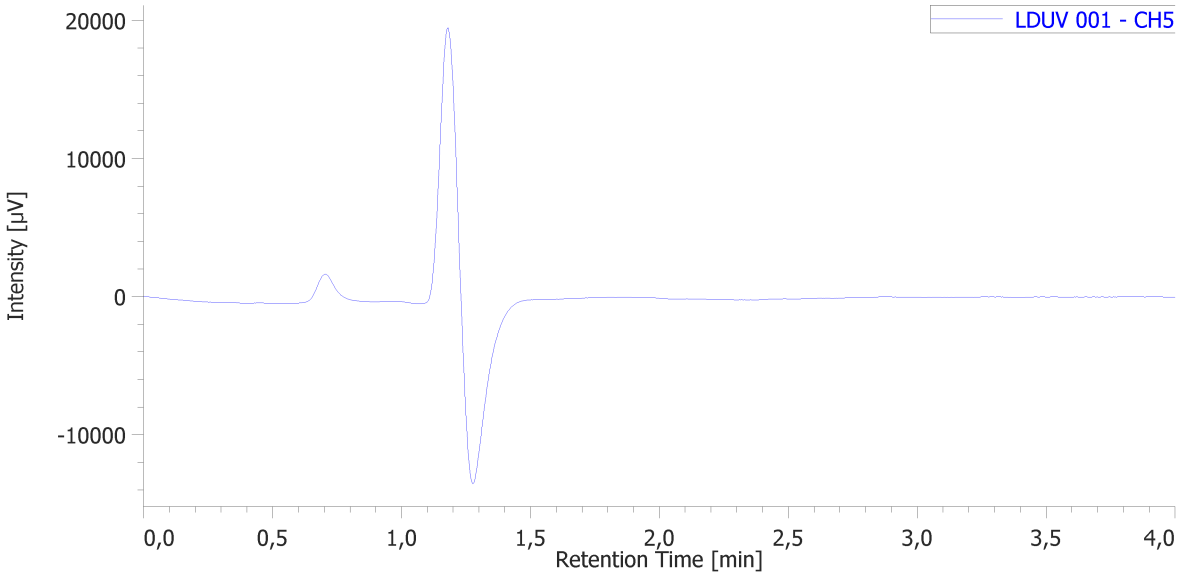


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:25:32
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:21:30
Volume	10,00 [µL]
Sample #	4
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

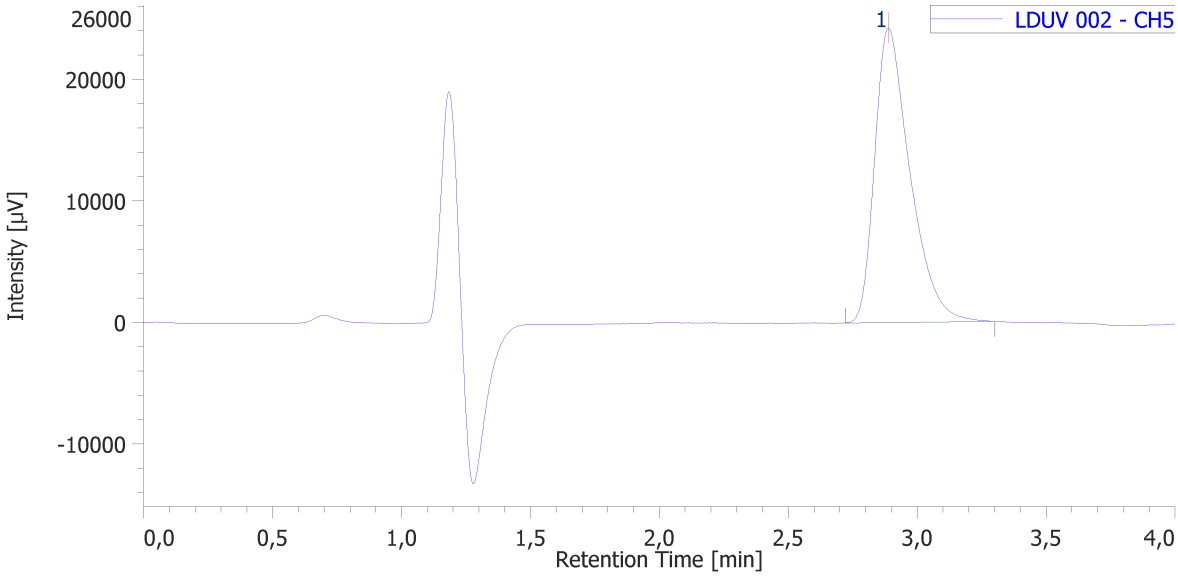

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 14:29:44
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:25:42
Volume	10,00 [µL]
Sample #	5
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,887	230548	24229	100,000	100,000	N/A	2261	N/A	1,505	

Creator
Reviewer
Approver

Chromatogram

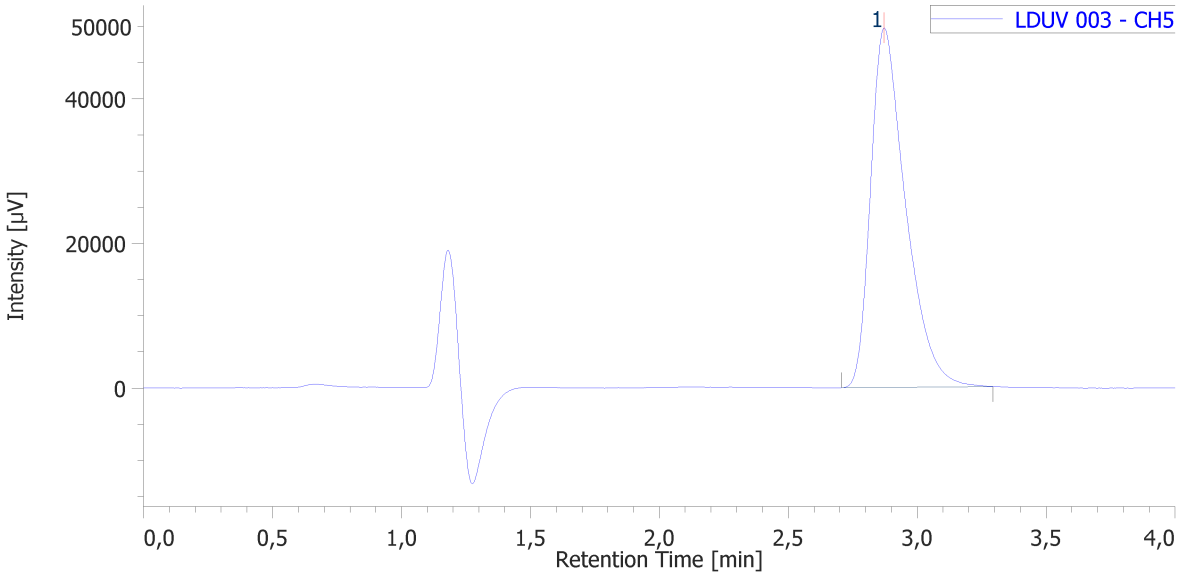

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:33:56
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:29:54
Volume	10,00 [µL]
Sample #	6
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,870	468169	49682	100,000	100,000	N/A	2279	N/A	1,514	

Creator
Reviewer
Approver

Chromatogram

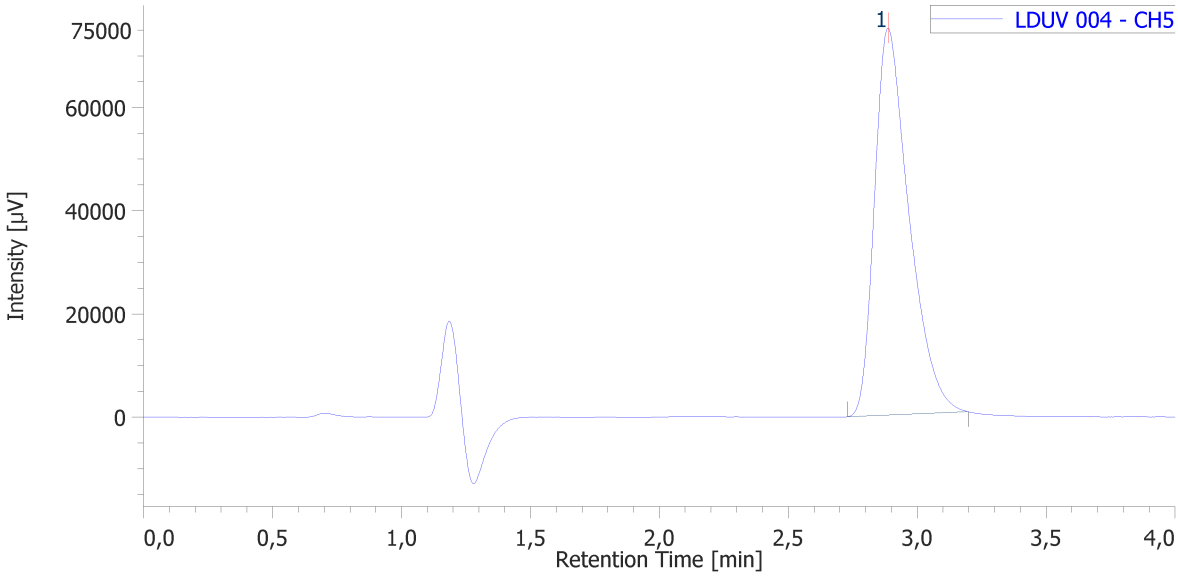

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:38:08
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:34:06
Volume	10,00 [µL]
Sample #	7
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,887	697268	74960	100,000	100,000	N/A	2319	N/A	1,467	

Creator
Reviewer
Approver

Chromatogram

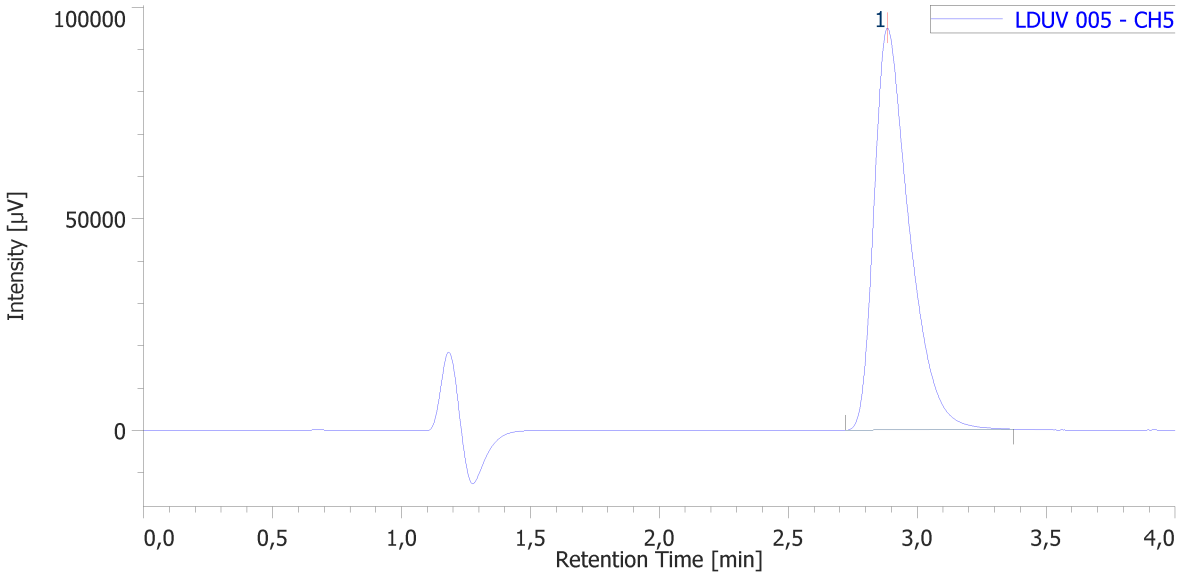

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:42:20
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:38:19
Volume	10,00 [µL]
Sample #	8
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,883	901492	94970	100,000	100,000	N/A	2285	N/A	1,539	

Creator
Reviewer
Approver

Chromatogram

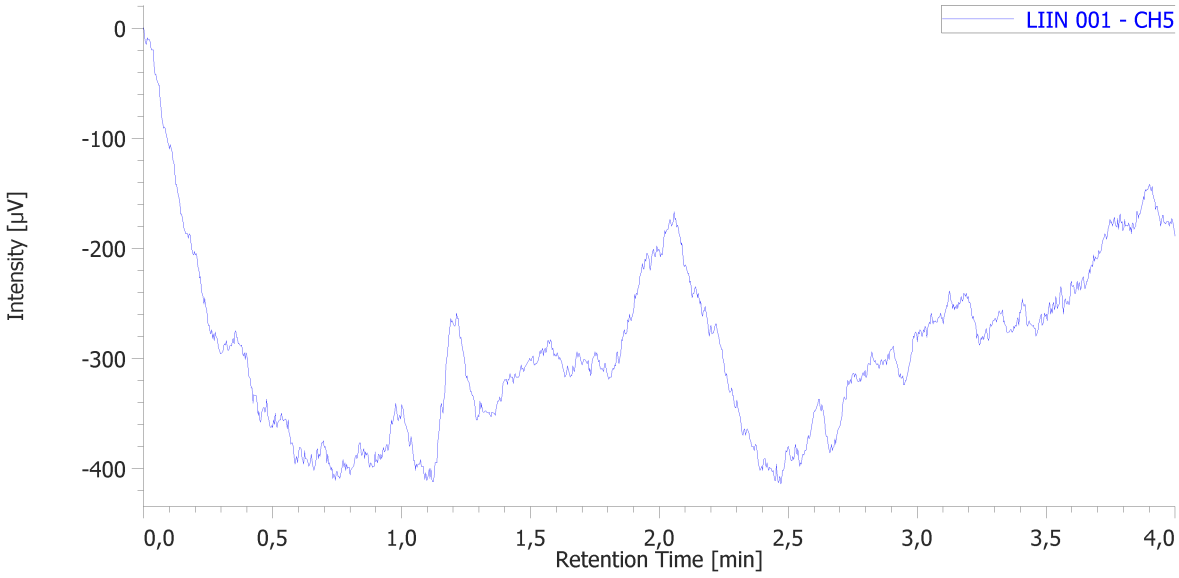


Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:49:26
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:45:24
Volume	0,10 [µL]
Sample #	2
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

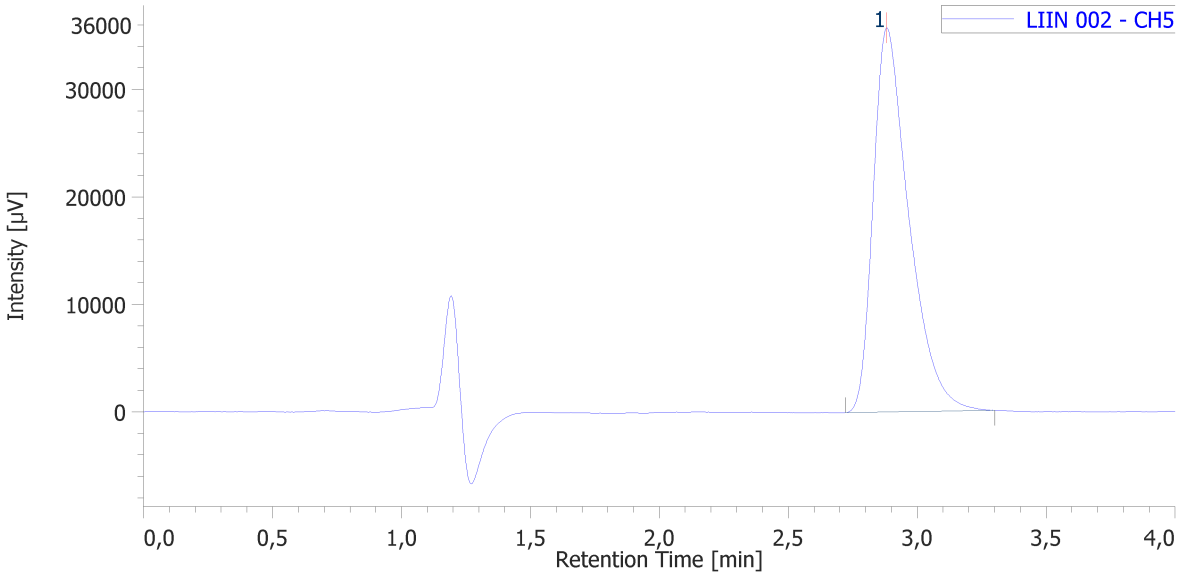

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 14:53:38
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:49:37
Volume	5,00 [µL]
Sample #	9
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,880	344129	35717	100,000	100,000	N/A	2205	N/A	1,558	

Creator
Reviewer
Approver

Chromatogram

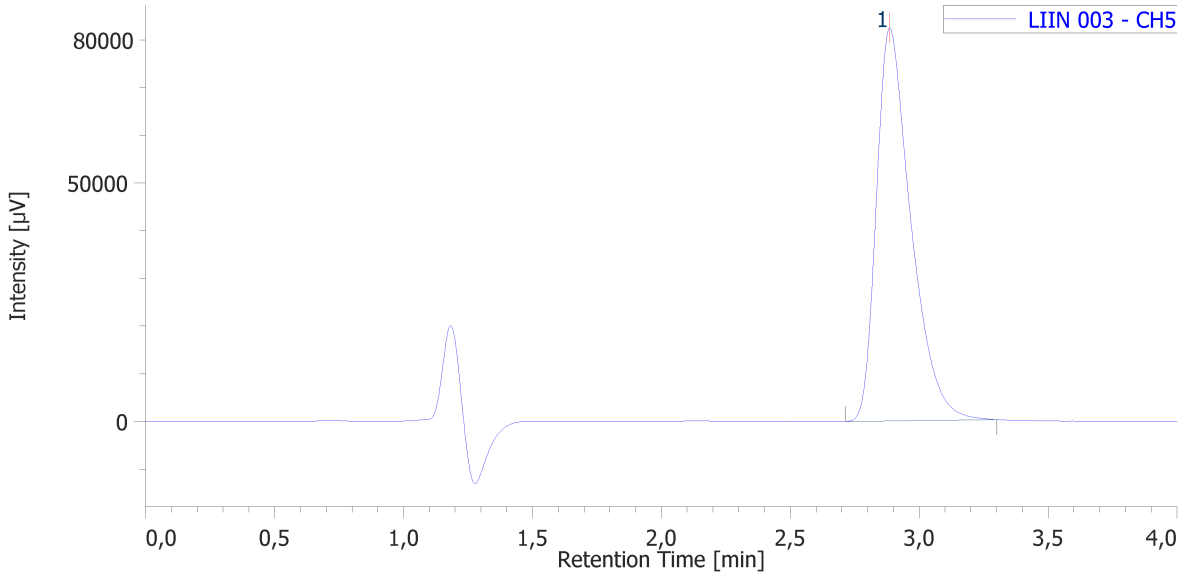

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 14:57:52
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:53:49
Volume	10,00 [µL]
Sample #	9
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,883	767237	82371	100,000	100,000	N/A	2357	N/A	1,523	

Creator
Reviewer
Approver

Chromatogram

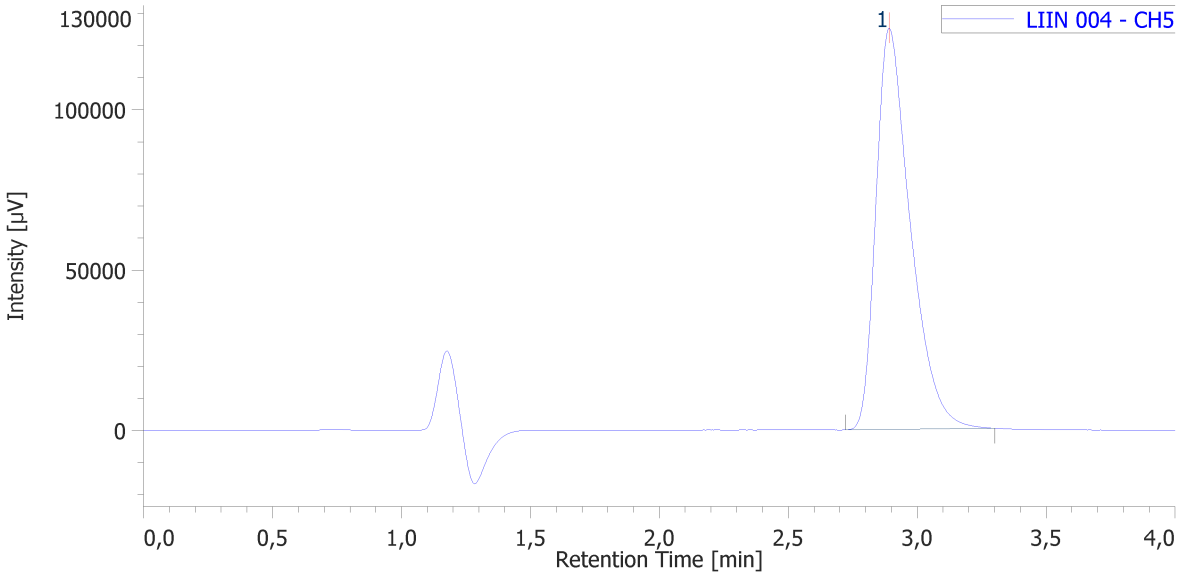

Chromatogram Information

User Name	Administrator
Date Modified	08/08/2019 15:02:04
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 14:58:01
Volume	15,00 [µL]
Sample #	9
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,890	1161008	125177	100,000	100,000	N/A	2375	N/A	1,512	

Creator
Reviewer
Approver

Chromatogram

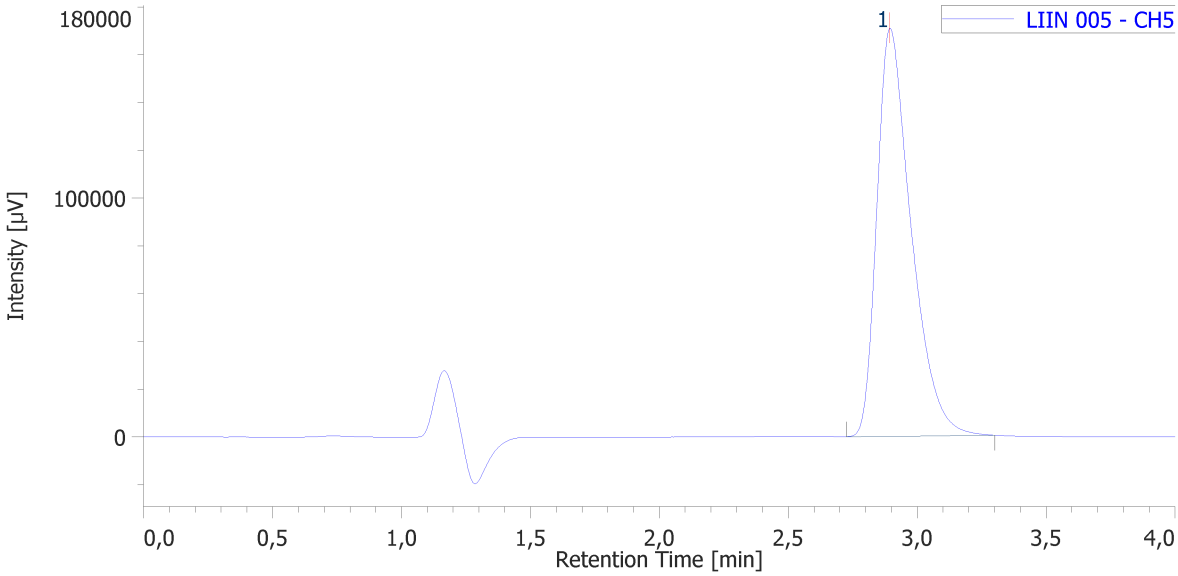

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 15:06:16
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 15:02:14
Volume	20,00 [µL]
Sample #	9
Project Name	Treinamento QPack
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	2,893	1574959	170806	100,000	100,000	N/A	2405	N/A	1,516	

Creator
Reviewer
Approver

Chromatogram

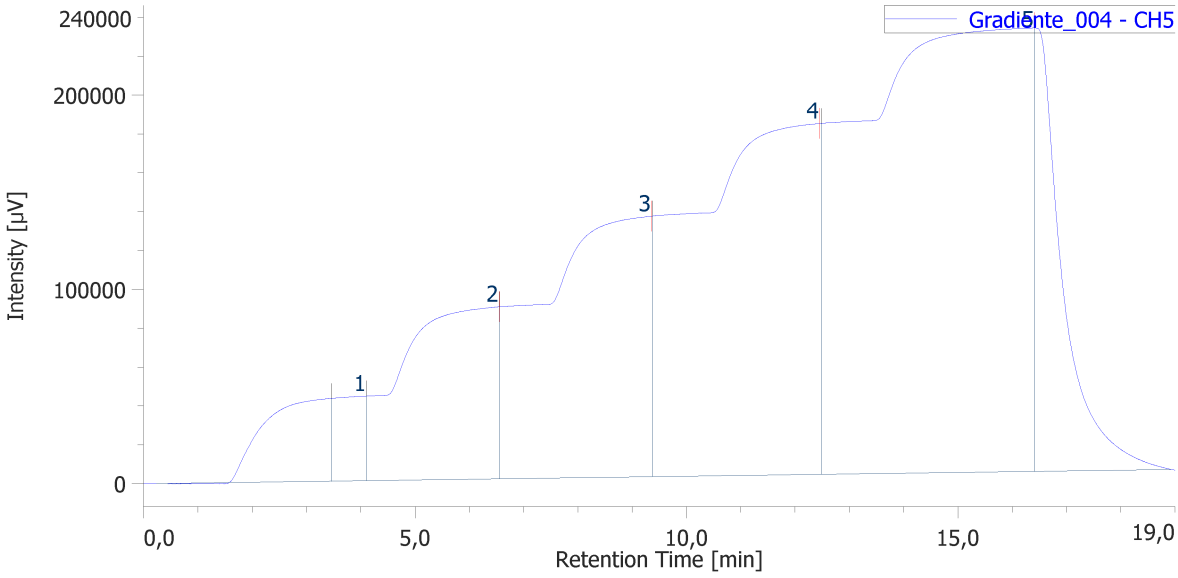

Chromatogram Information	
User Name	Administrator
Date Modified	08/08/2019 16:07:21
Description	
HPLC System Name	HPL 09
Injection Date	08/08/2019 15:48:19
Volume	0,00 [µL]
Sample #	–
Project Name	Treinamento QPack
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Gradiente HPL 09
Peak ID Table	ID Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Integração1 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,107	1681209	43522	1,529	6,453	N/A	N/A	N/A	N/A	
2	Unknown	5	6,543	10632394	88469	9,668	13,117	N/A	N/A	N/A	N/A	
3	Unknown	5	9,357	18908453	134027	17,194	19,871	N/A	N/A	N/A	N/A	
4	Unknown	5	12,450	29327387	180418	26,669	26,749	N/A	N/A	N/A	N/A	
5	Unknown	5	16,407	49420068	228042	44,940	33,810	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver