
Peak Find - EDUV_006 PDA_1,1483.JWS

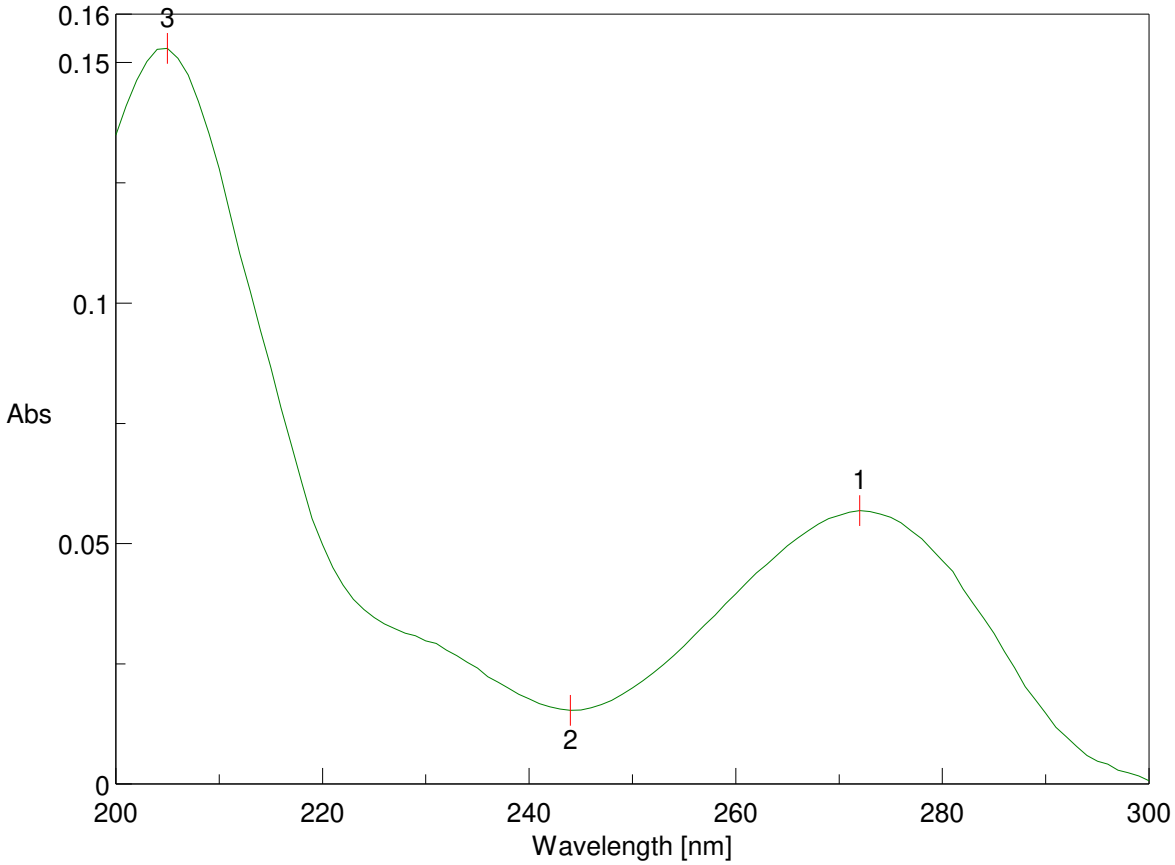

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	26/08/2021 10:23

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A000661665
ROM version	V1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.056822	2	244	0.015301
3	205	0.15289			

Chromatogram

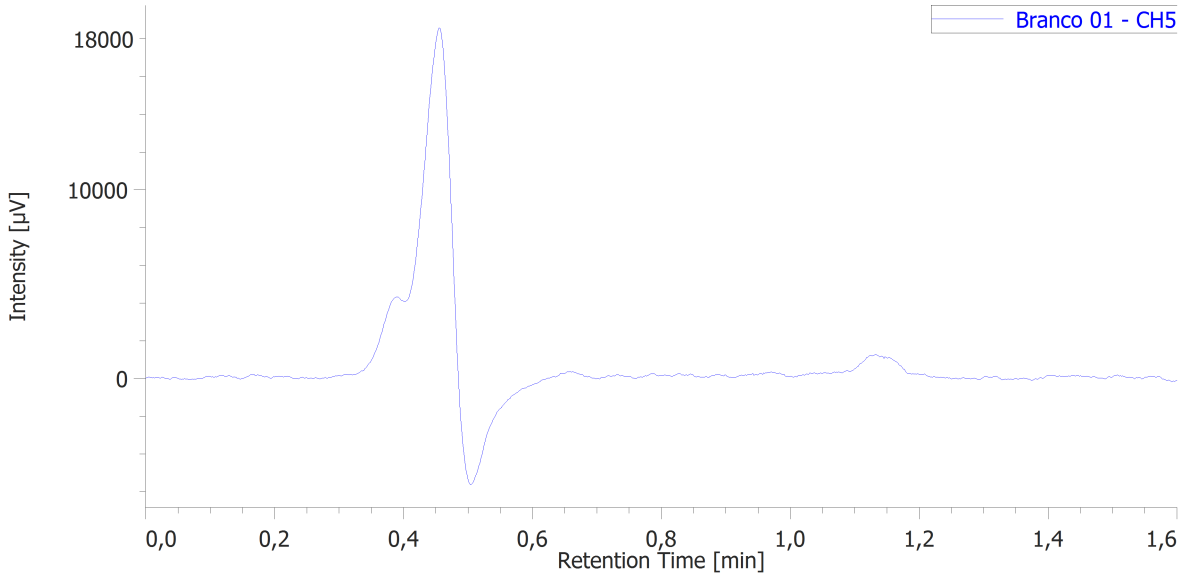


Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:39:11
Volume	10,0 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	Branco 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

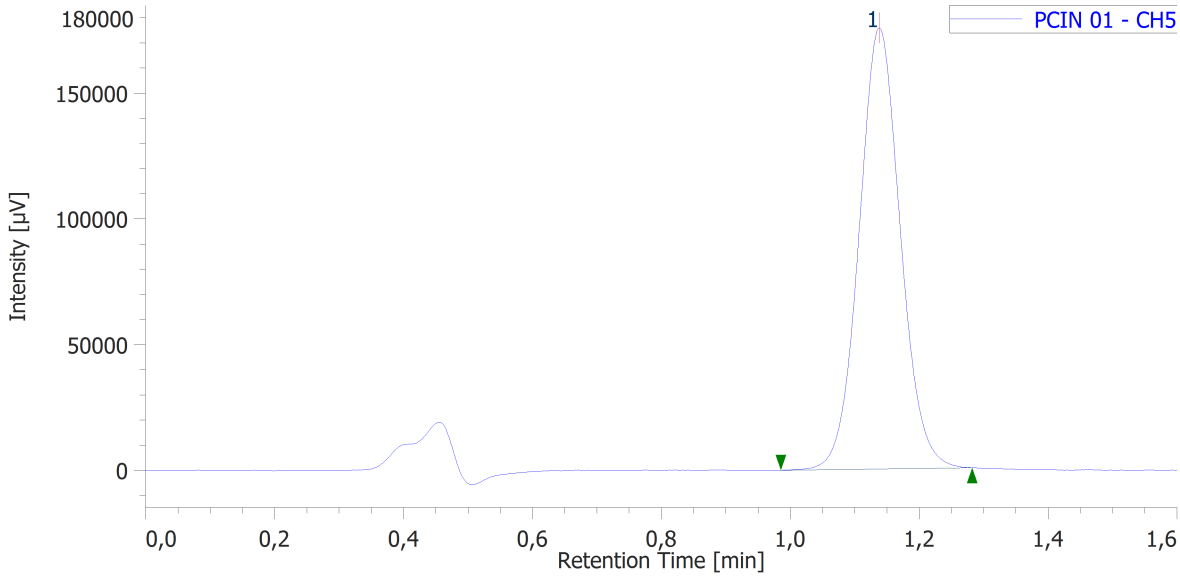

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:42:05
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	PCIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,138	780279	175248	100,000	100,000	N/A	1557	N/A	1,051	

Creator QPackSA
Reviewer
Approver

Chromatogram

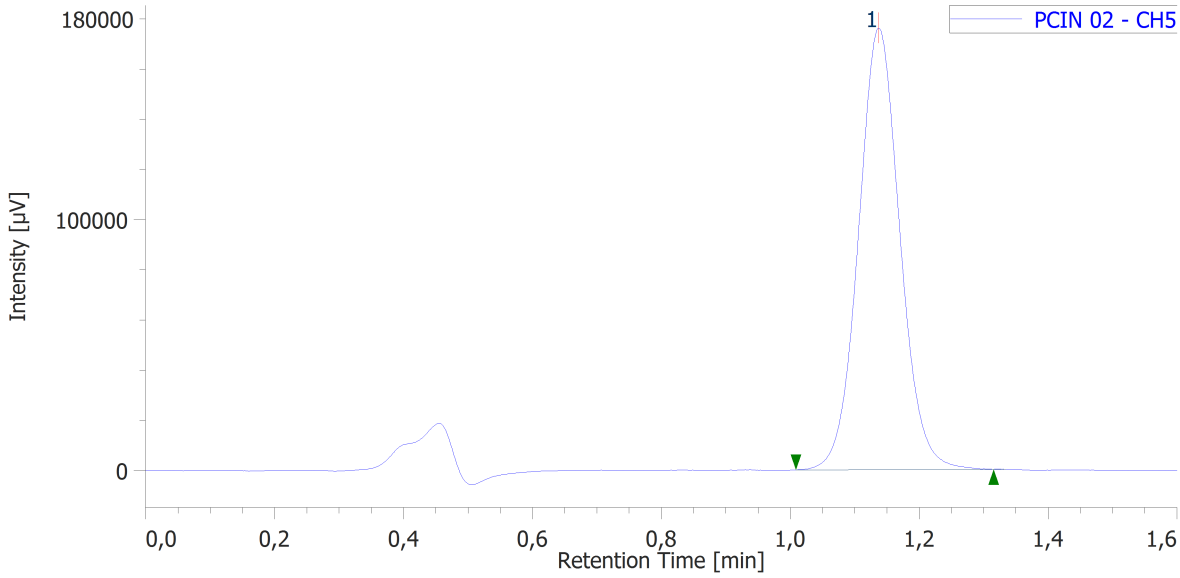

Chromatogram Information

User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:44:58
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	PCIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,137	785856	175962	100,000	100,000	N/A	1557	N/A	1,063	

Creator QPackSA
Reviewer
Approver

Chromatogram

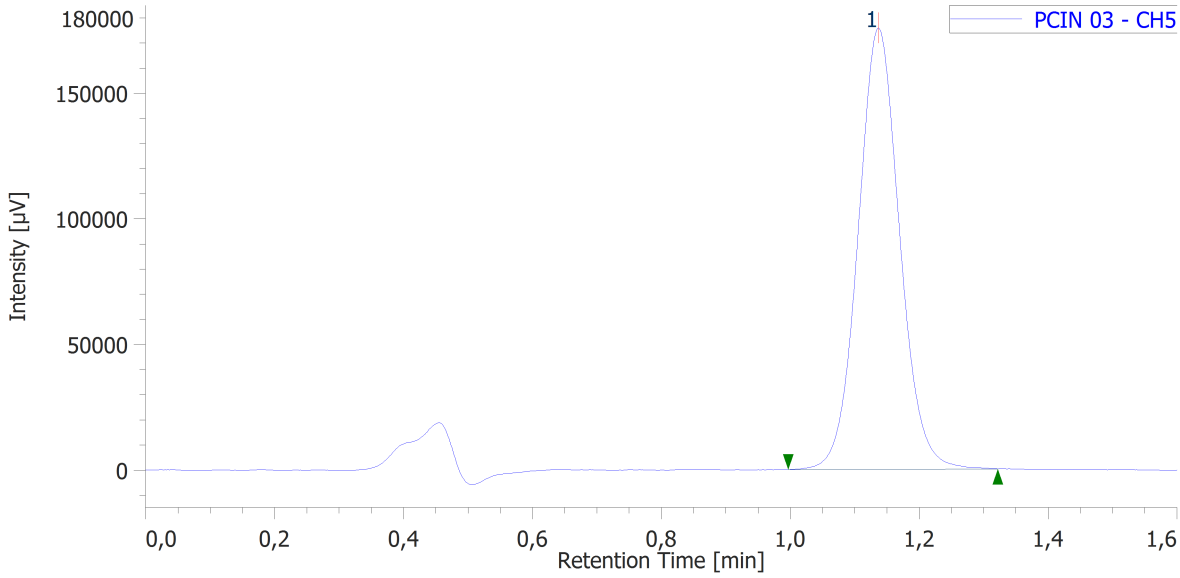

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:47:50
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	PCIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,137	785685	175507	100,000	100,000	N/A	1550	N/A	1,057	

Creator QPackSA
Reviewer
Approver

Chromatogram

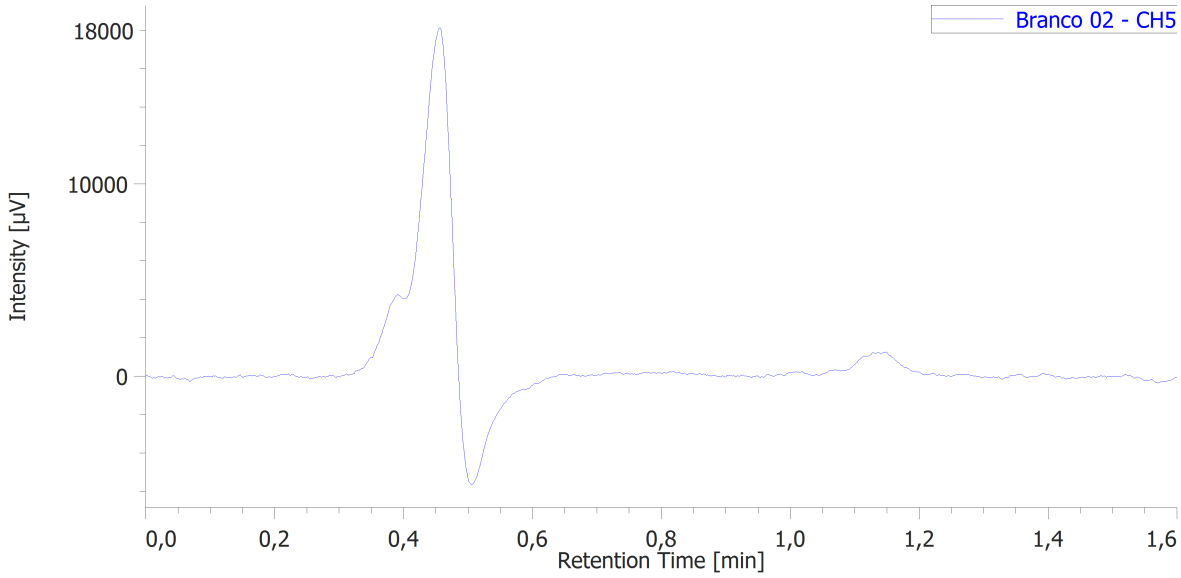


Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:50:43
Volume	10,0 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	Branco 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

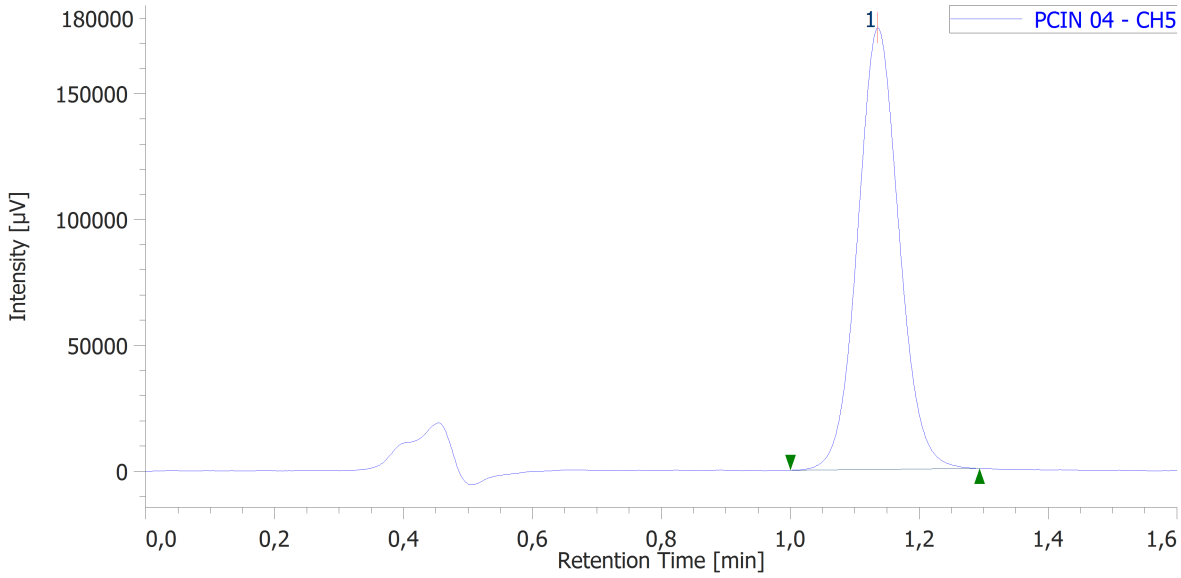

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:50
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:53:38
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	PCIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,135	782913	175331	100,000	100,000	N/A	1542	N/A	1,068	

Creator QPackSA
Reviewer
Approver

Chromatogram

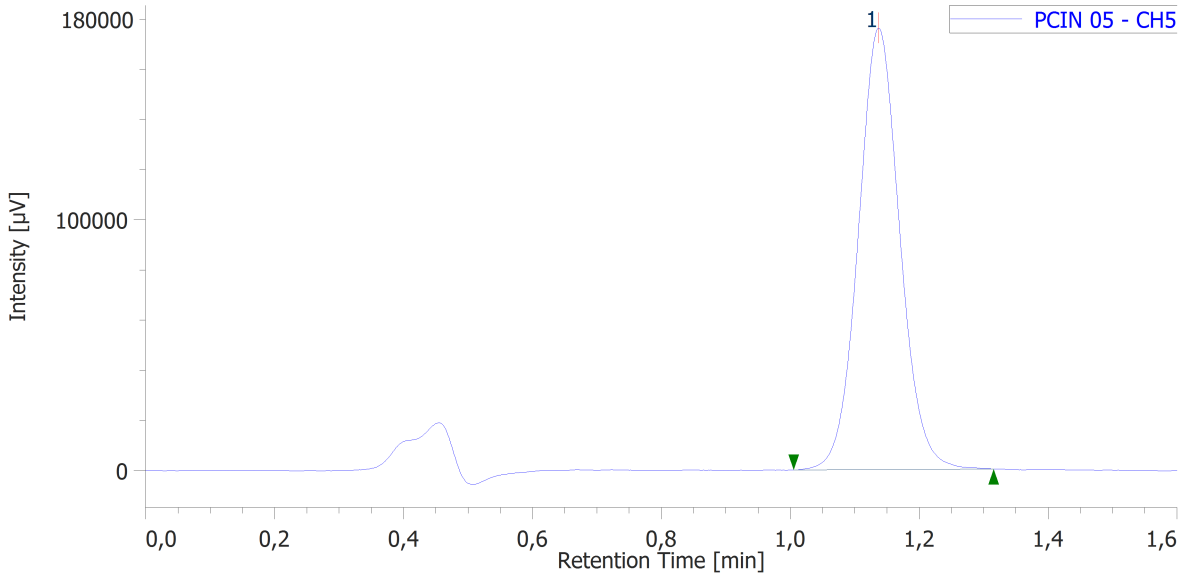

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:51
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:56:32
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	PCIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,137	787398	176065	100,000	100,000	N/A	1552	N/A	1,061	

Creator QPackSA
Reviewer
Approver

Chromatogram

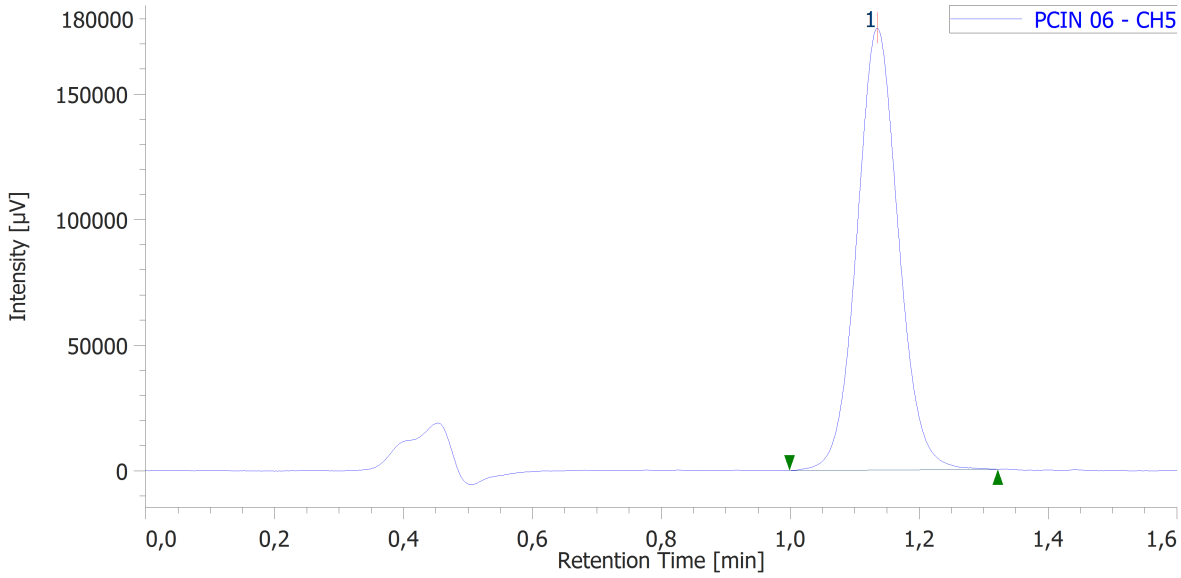

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:51
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 10:59:27
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	PCIN 06
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,135	787269	175901	100,000	100,000	N/A	1548	N/A	1,054	

Creator QPackSA
Reviewer
Approver

Chromatogram

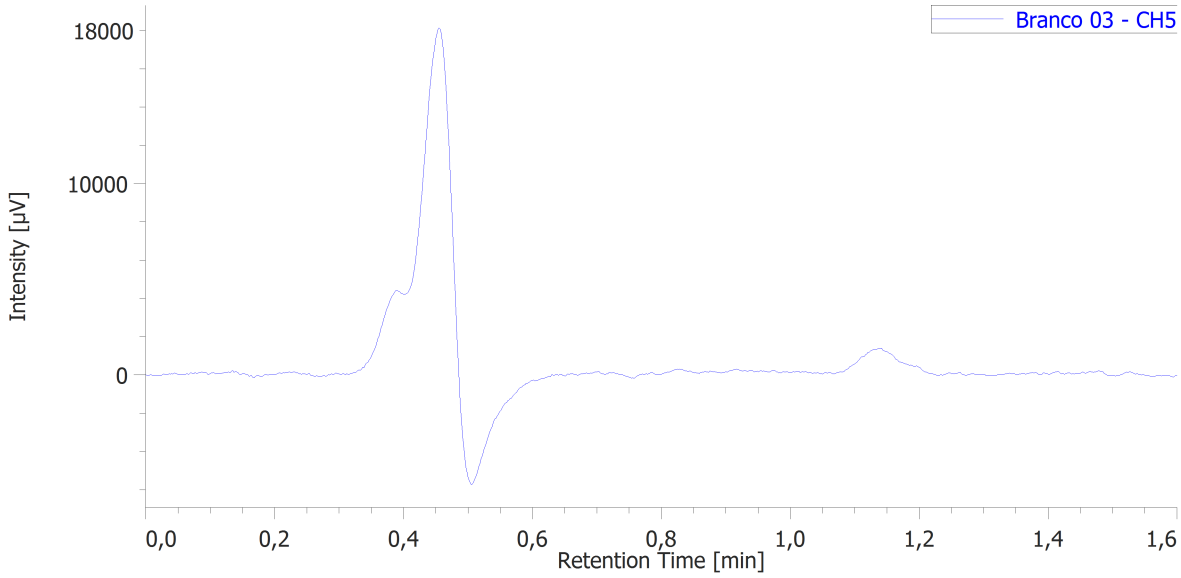


Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:09:51
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:02:20
Volume	10,0 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	Branco 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

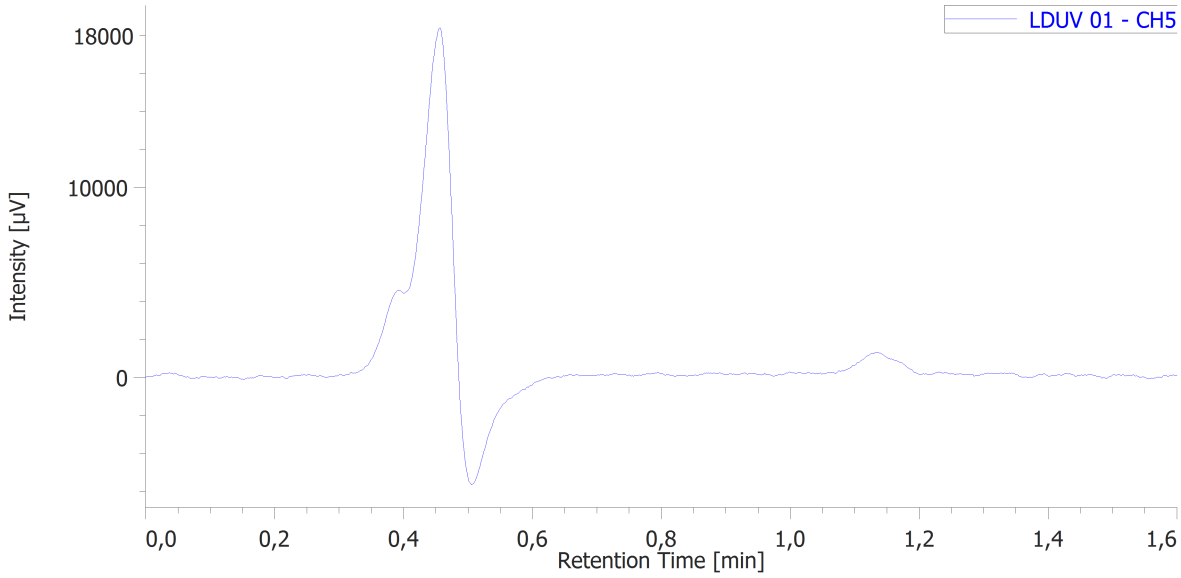


Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:18:47
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:07:48
Volume	10,0 [µL]
Sample #	26
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	LDUV 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

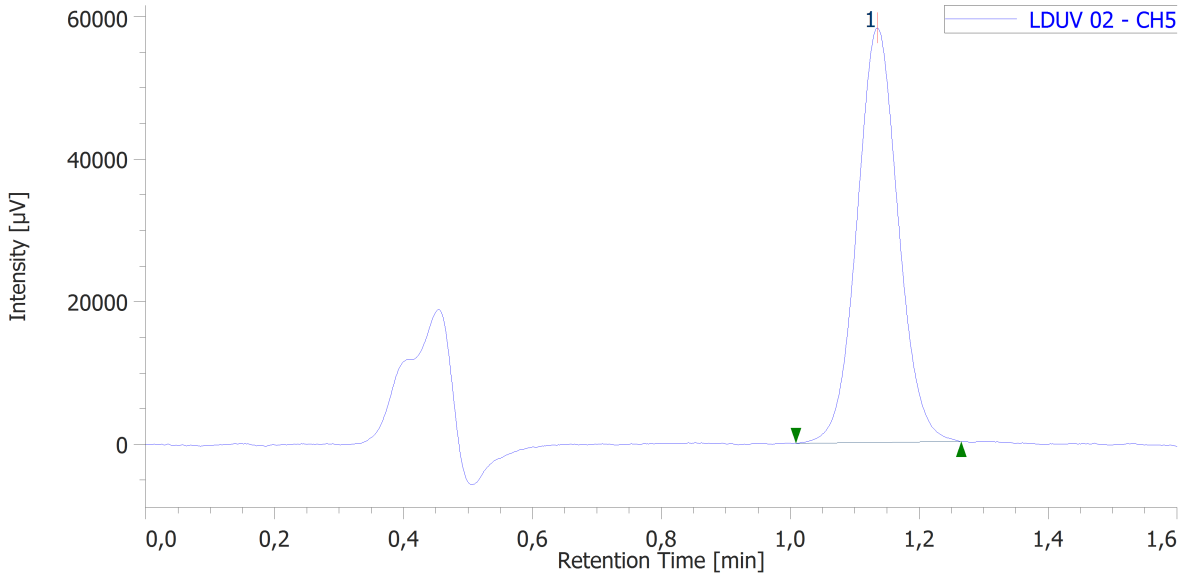

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:18:48
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:10:43
Volume	10,0 [µL]
Sample #	27
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	LDUV 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,135	258743	58111	100,000	100,000	N/A	1547	N/A	1,051	

Creator QPackSA
Reviewer
Approver

Chromatogram

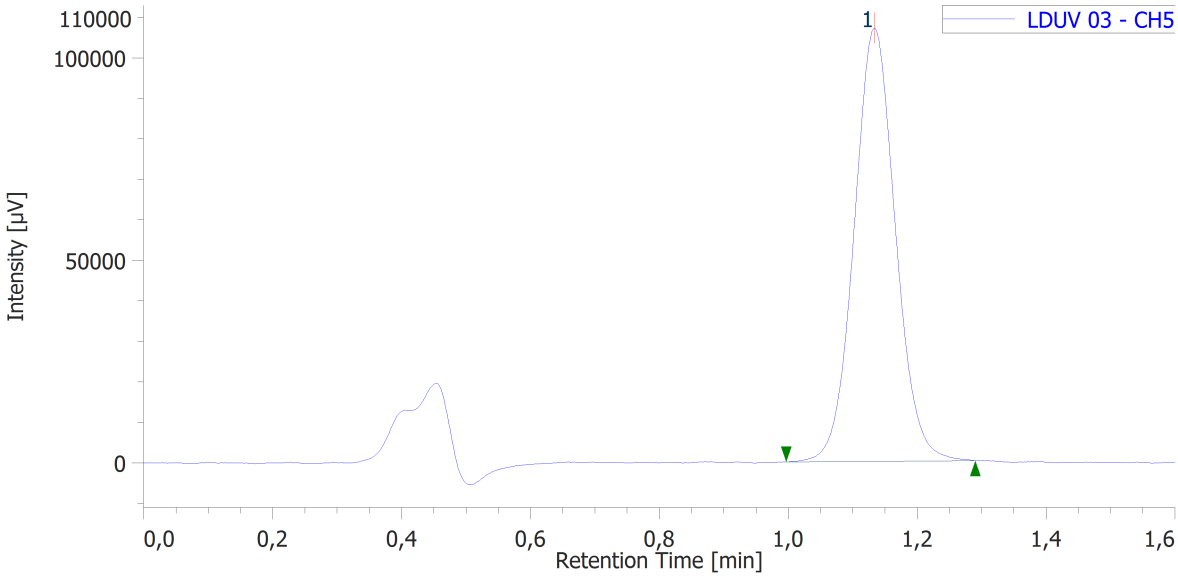

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:18:48
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:13:37
Volume	10,0 [µL]
Sample #	28
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	LDUV 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,133	476712	106945	100,000	100,000	N/A	1547	N/A	1,056	

Creator QPackSA
Reviewer
Approver

Chromatogram

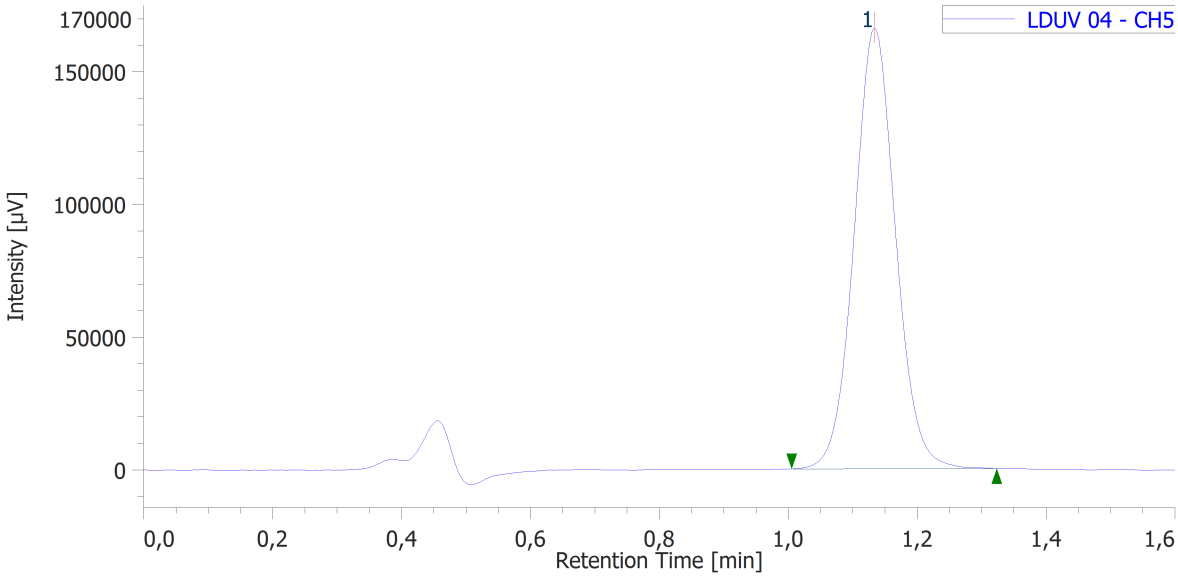

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:18:48
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:16:29
Volume	10,0 [µL]
Sample #	29
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	LDUV 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,133	740265	166033	100,000	100,000	N/A	1552	N/A	1,056	

Creator QPackSA
Reviewer
Approver

Chromatogram

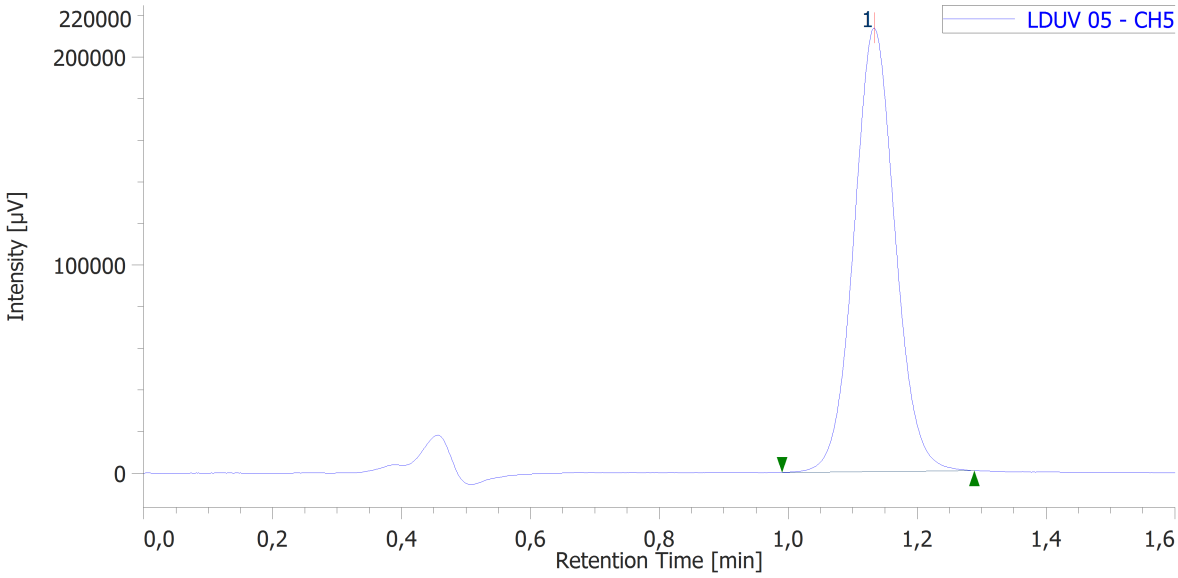

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 11:21:30
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:19:24
Volume	10,0 [µL]
Sample #	30
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	LDUV 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,133	947402	213200	100,000	100,000	N/A	1558	N/A	1,049	

Creator QPackSA
Reviewer
Approver

Chromatogram

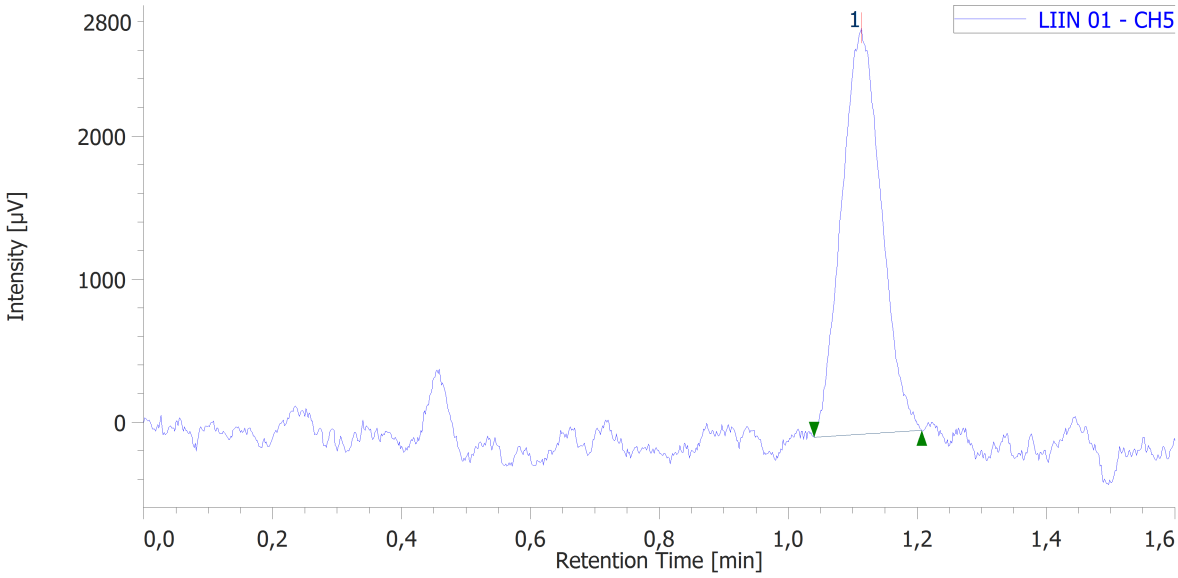

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 12:14:59
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:26:08
Volume	0,1 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	LIIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,113	12134	2837	100,000	100,000	N/A	1452	N/A	1,080	

Creator QPackSA
Reviewer
Approver

Chromatogram

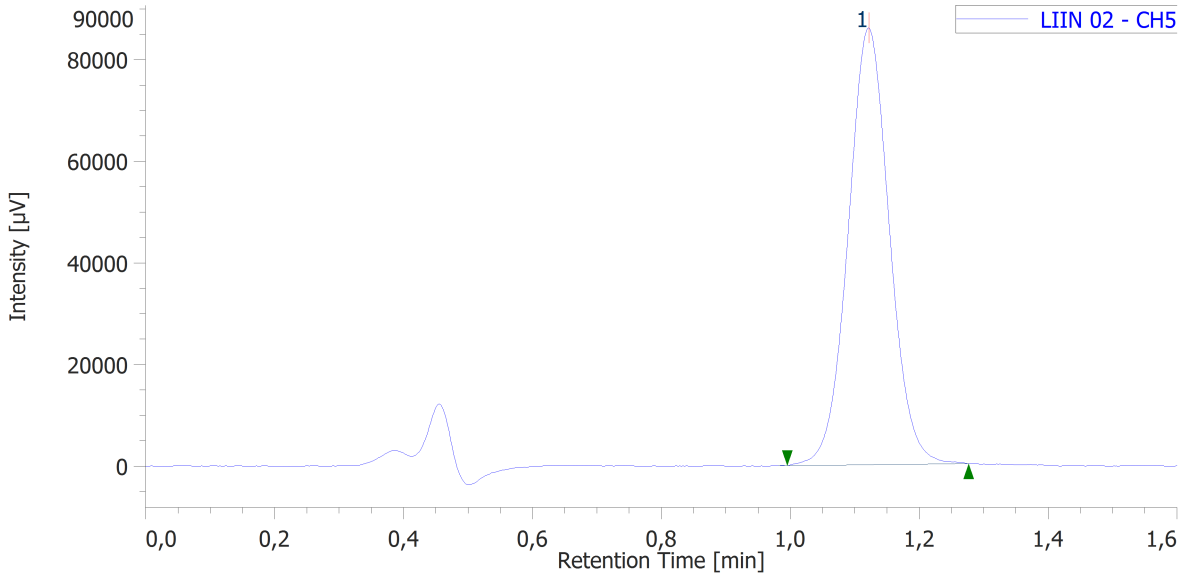

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 12:14:59
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:29:00
Volume	5,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	LIIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,122	382900	85943	100,000	100,000	N/A	1514	N/A	1,029	

Creator QPackSA
Reviewer
Approver

Chromatogram

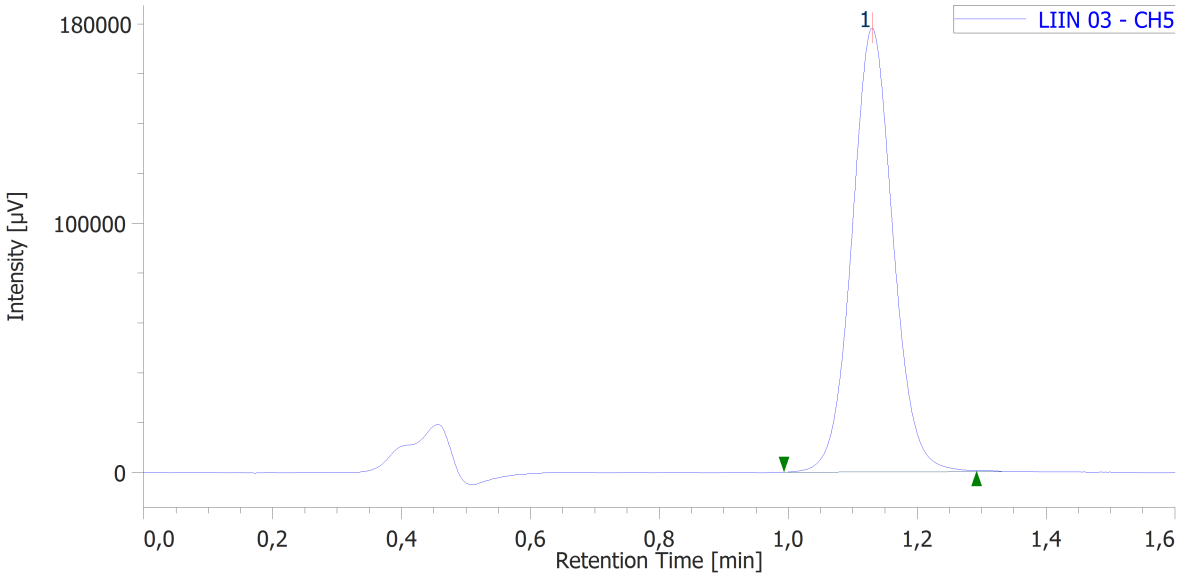

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 12:14:59
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:31:55
Volume	10,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	LIIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,130	789121	178097	100,000	100,000	N/A	1571	N/A	1,051	

Creator QPackSA
Reviewer
Approver

Chromatogram

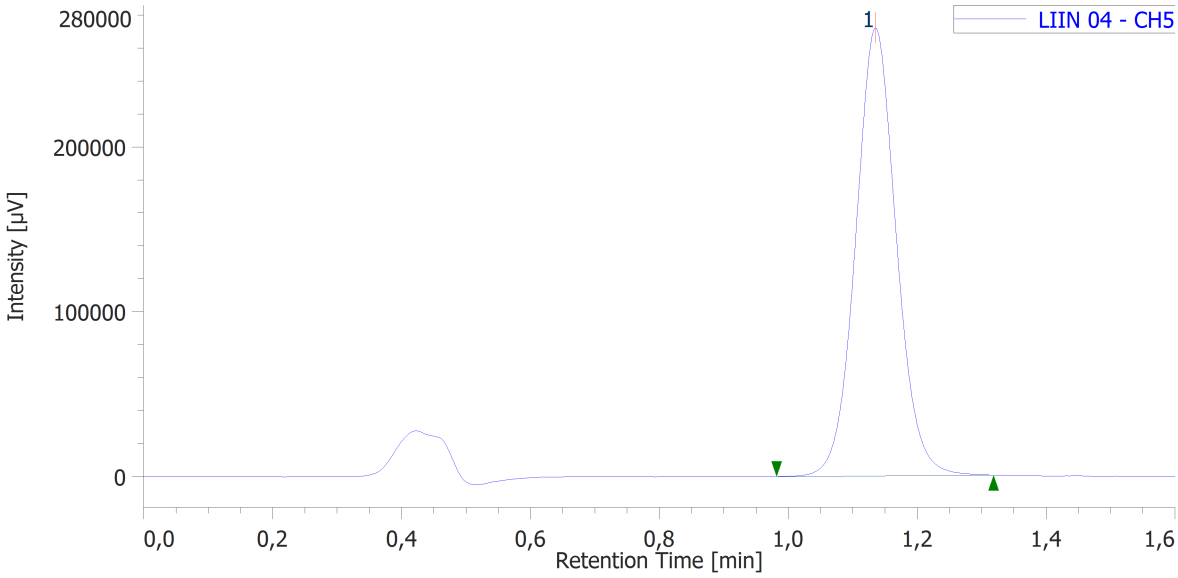

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 12:14:59
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:34:52
Volume	15,0 [μL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	LIIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,135	1190964	271607	100,000	100,000	N/A	1622	N/A	1,063	

Creator QPackSA
Reviewer
Approver

Chromatogram

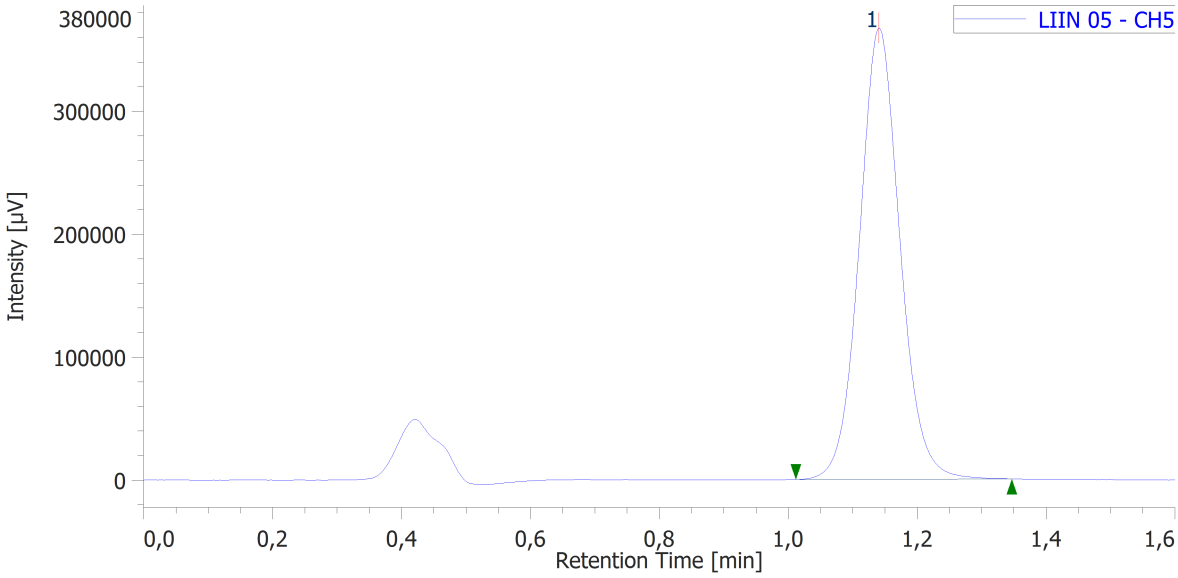

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 12:15:00
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 11:37:52
Volume	20,0 [µL]
Sample #	40
Project Name	Qualificação
Acquisition Time	1,6 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	LIIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,140	1603619	366878	100,000	100,000	N/A	1658	N/A	1,082	

Creator QPackSA
Reviewer
Approver

Chromatogram

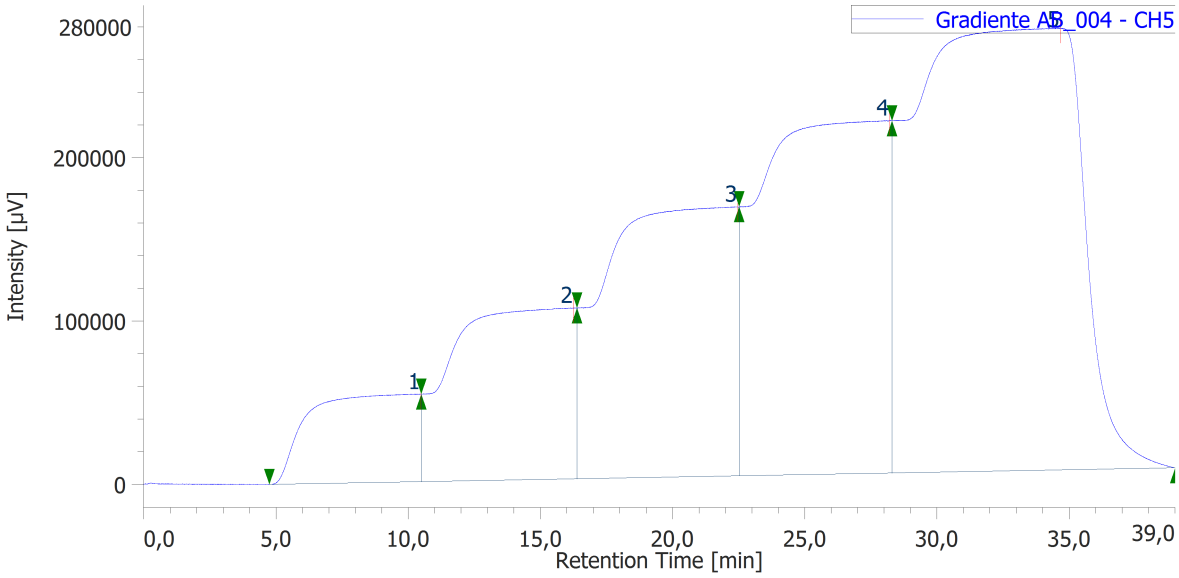

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 16:45:38
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 15:46:18
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	39,0 [min]
Acquisition Sequence	
Control Method	Grad LP – AB
Peak ID Table	Grad LP
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	10,483	14912594	53664	5,132	6,634	N/A	N/A	N/A	N/A	
2	40%	5	16,245	32705197	104640	11,256	12,936	N/A	N/A	N/A	N/A	
3	60%	5	22,461	55233557	164626	19,009	20,351	N/A	N/A	N/A	N/A	
4	80%	5	28,188	70570580	215684	24,287	26,663	N/A	N/A	N/A	N/A	
5	100%	5	34,656	117148112	270311	40,317	33,416	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

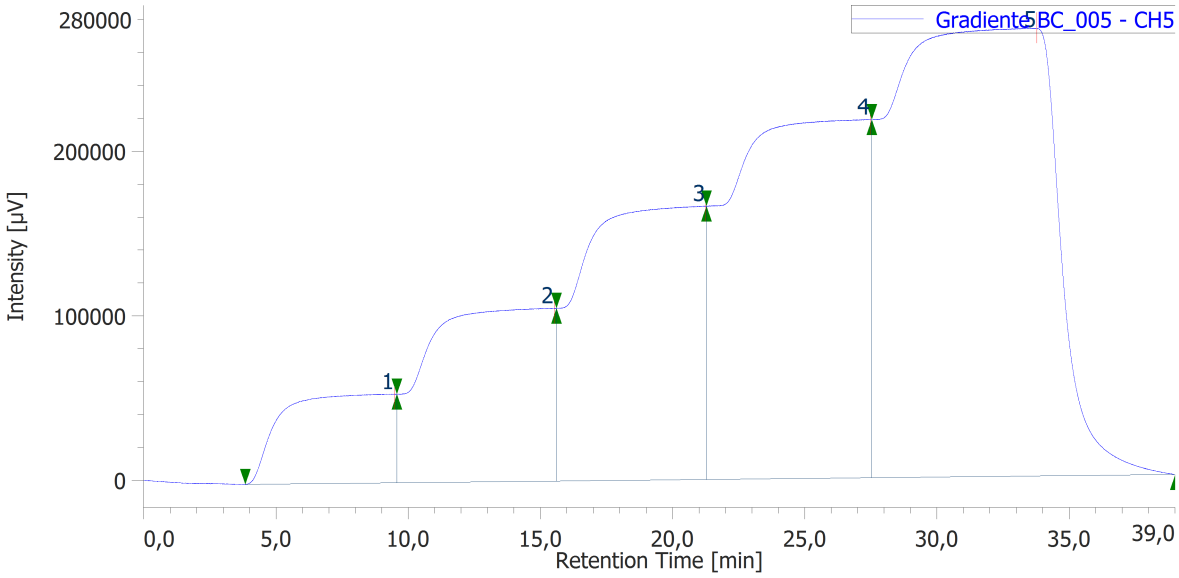

Chromatogram Information	
User Name	QPackSA
Date Modified	26/08/2021 17:08:23
Description	
HPLC System Name	HPL 09_PDA
Injection Date	26/08/2021 16:27:59
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	39,0 [min]
Acquisition Sequence	
Control Method	Grad LP – BC
Peak ID Table	Grad LP
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente BC_005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	50 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	9,482	15263146	54019	5,199	6,625	N/A	N/A	N/A	N/A	
2	40%	5	15,523	34030552	105159	11,593	12,896	N/A	N/A	N/A	N/A	
3	60%	5	21,253	51808724	166285	17,649	20,393	N/A	N/A	N/A	N/A	
4	80%	5	27,472	76684409	217756	26,123	26,705	N/A	N/A	N/A	N/A	
5	100%	5	33,767	115768767	272197	39,437	33,381	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver