
Peak Find - EDUV.jws

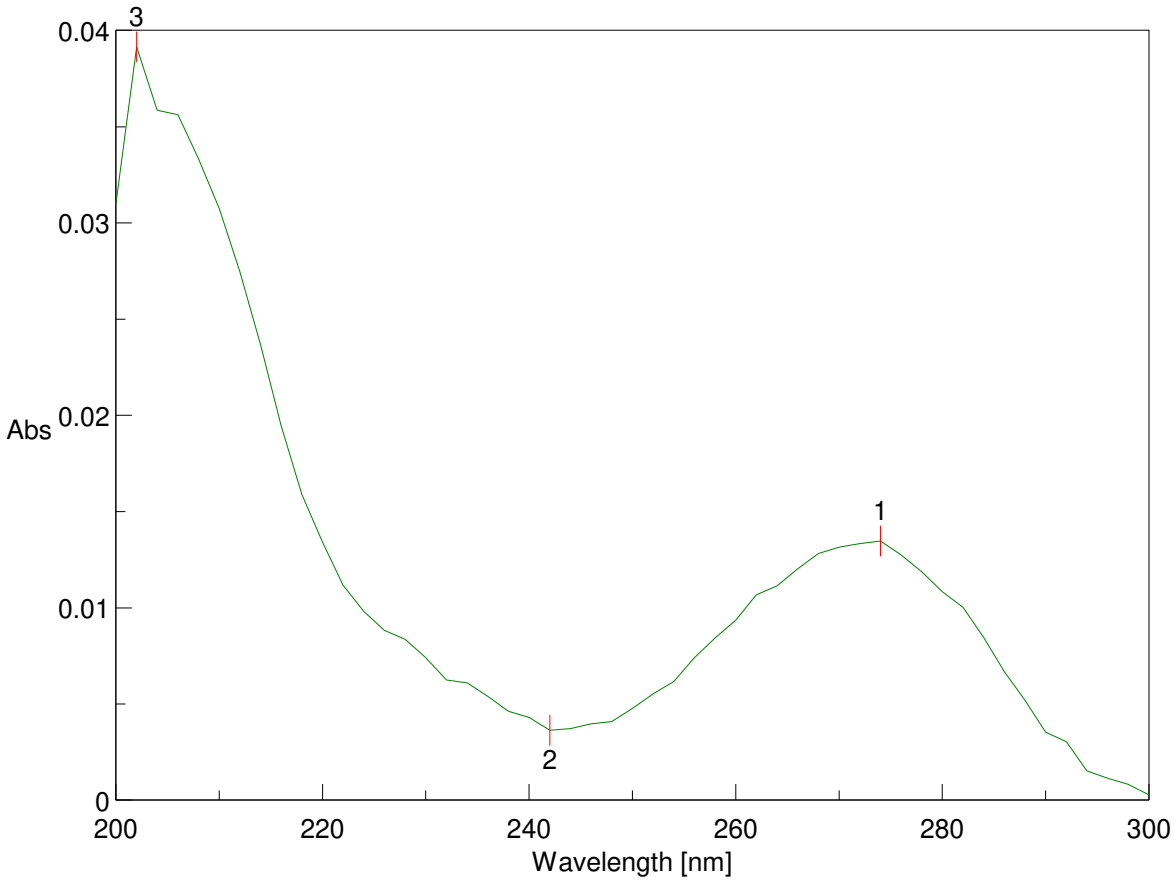

[Comments]

User	QPackSA
Workgroup	QPack
Division	Suporte Técnico
Company	JP INDÚSTRIA FARMACÊTICA S.A
Creation date	04/05/2023 09:25


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	600 nm	
Data interval	2 nm	
Data points	200	

[Result of Peak Picking]


No.	Position	Intensity	No.	Position	Intensity
1	274	0.0134575	2	244	0.00363296
3	204	0.0391369			

Relatório SRELB

Detector UV – UV-2075 – N/S B113160866	Data: 04/05/2023
Ruído:	
Valor máximo: 134,8 mAU	**Diferença: 6,9 mAU**
Valor mínimo: 127,9 mAU	

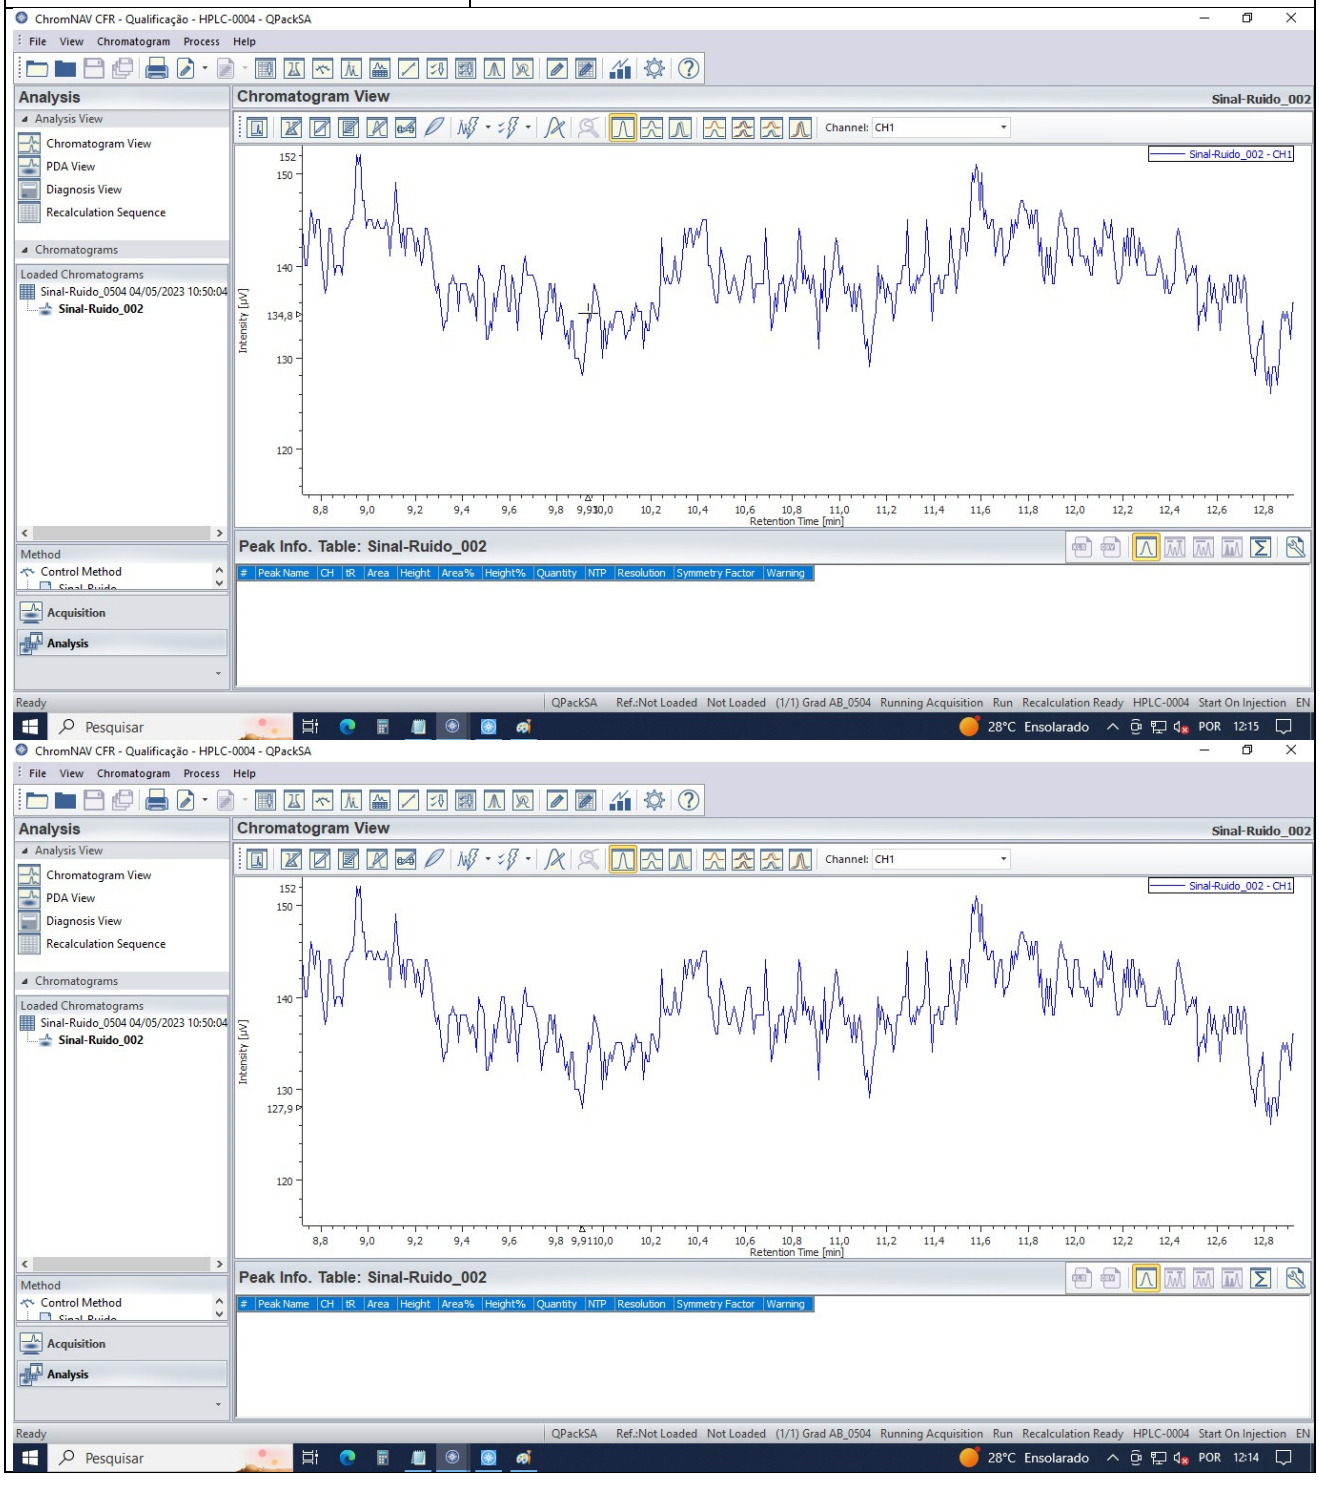


Estabilidade da Linha de Base:	
Valor máximo: 126,8 mAU	**Diferença (em 20 minutos): 8,3 mAU**
Valor mínimo: 118,5 mAU	**Diferença (em 60 minutos): 8,3 x 3 = 24,9 mAU**

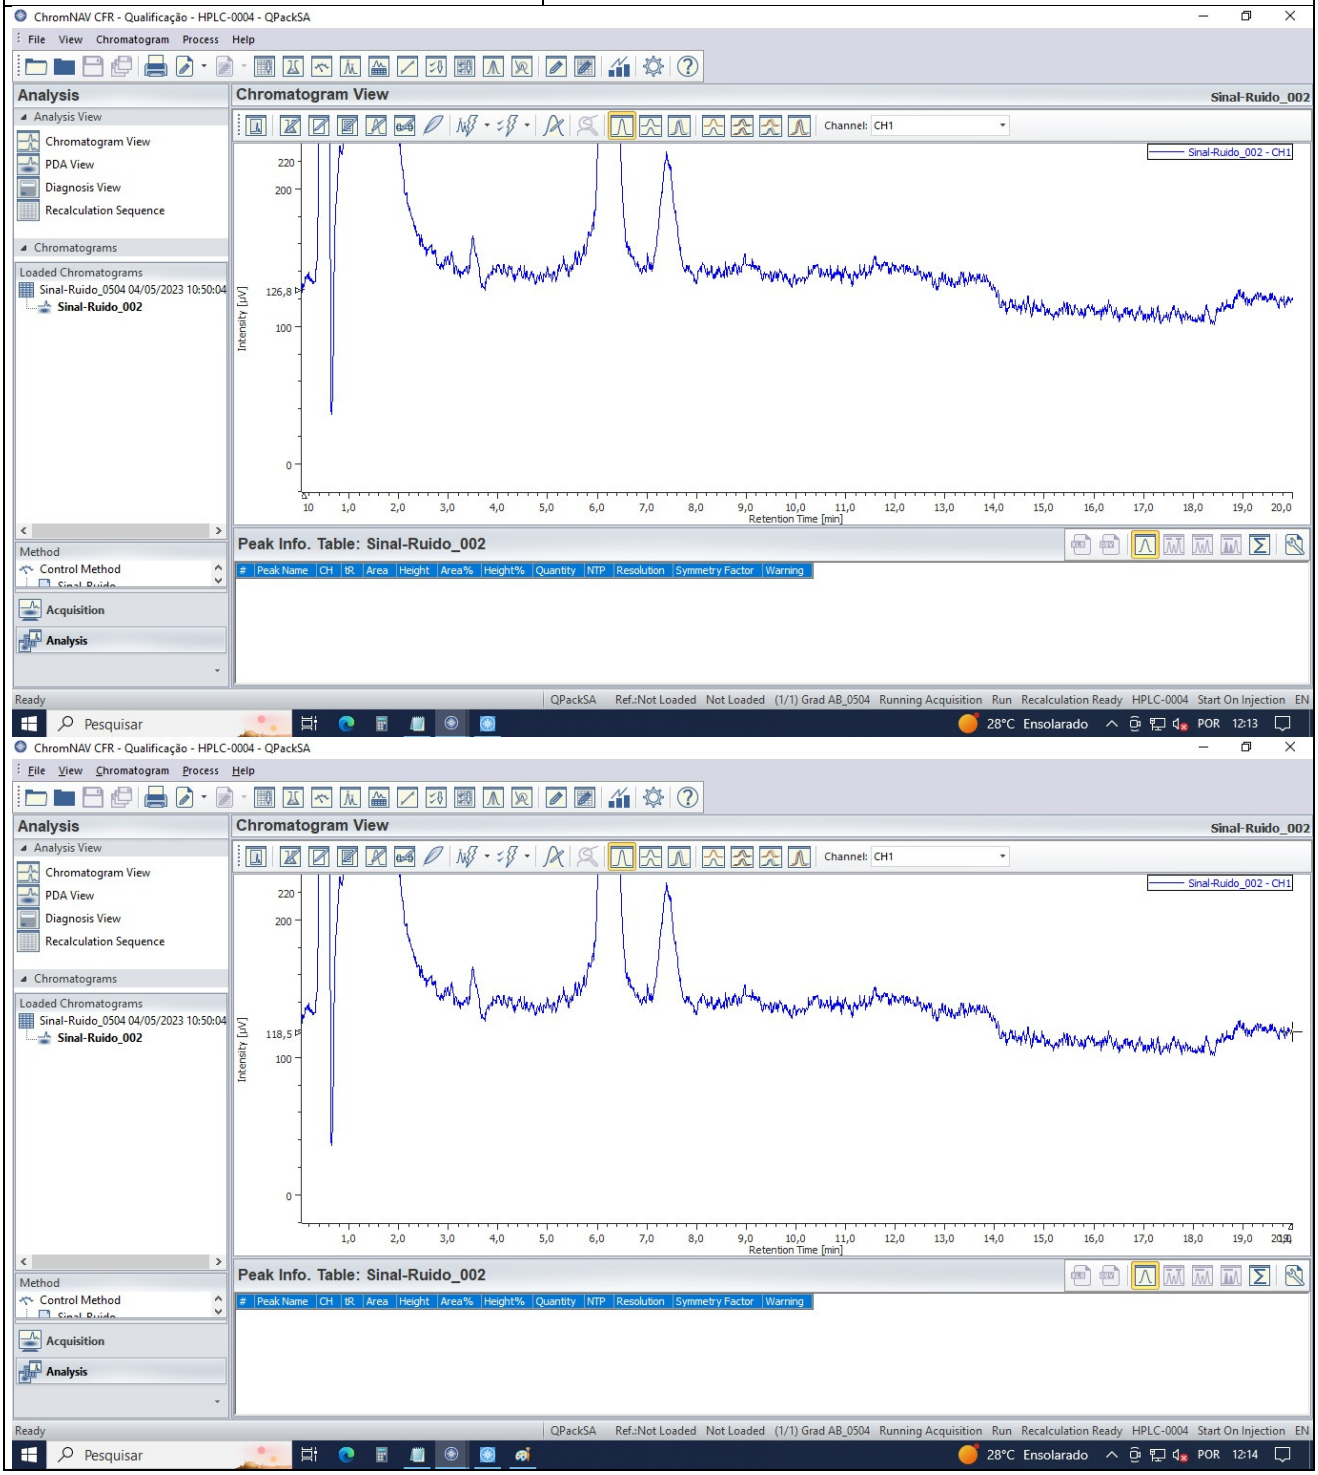


Altura do Pico:

Valor: 109671,1 mAU

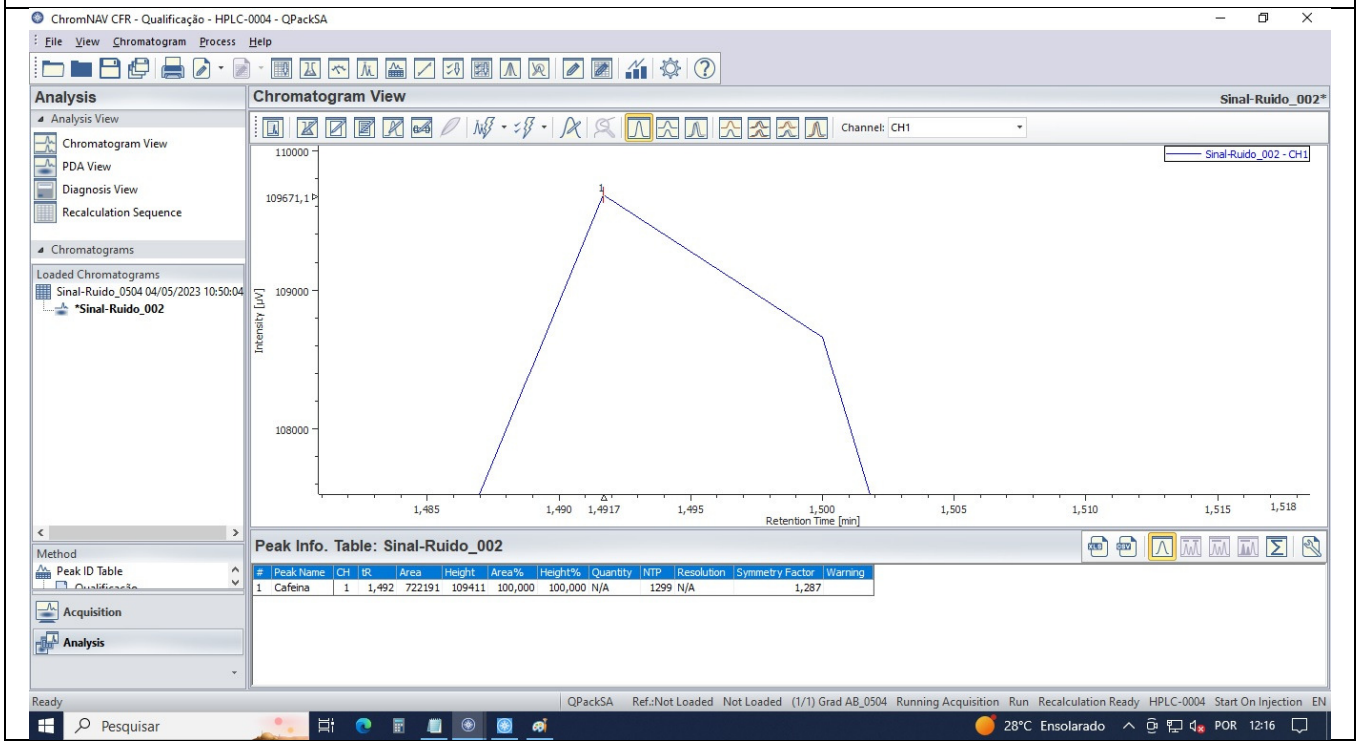

Chromatogram

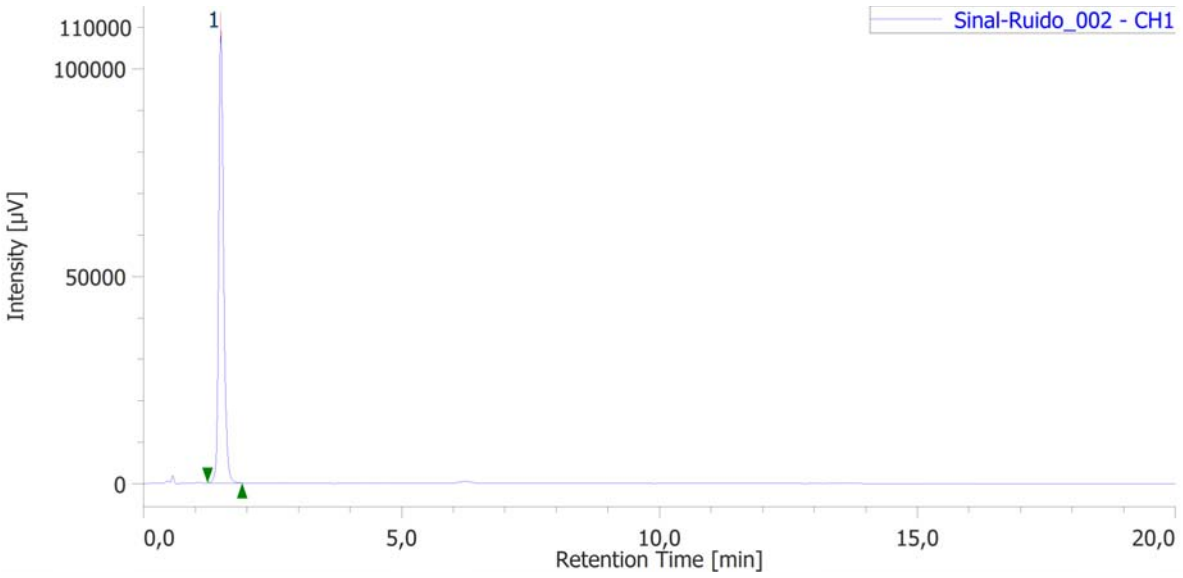

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 12:17:12
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 11:14:24
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal-Ruido_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,492	722191	109411	100,000	100,000	N/A	1299	N/A	1,287	

Creator QPackSA
Reviewer
Approver

Chromatogram

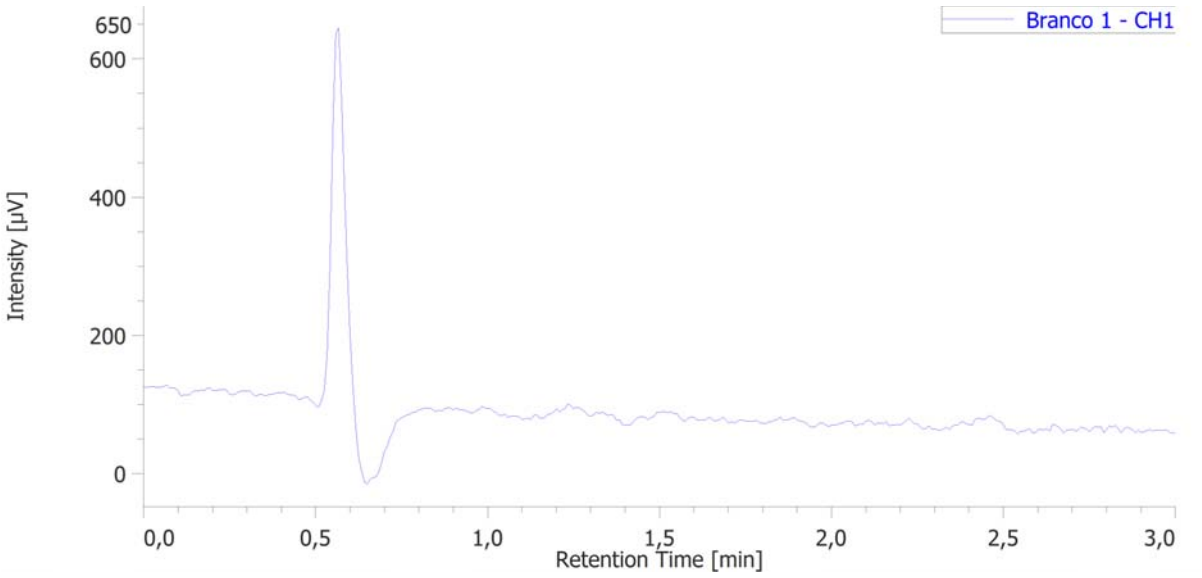


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:39:11
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

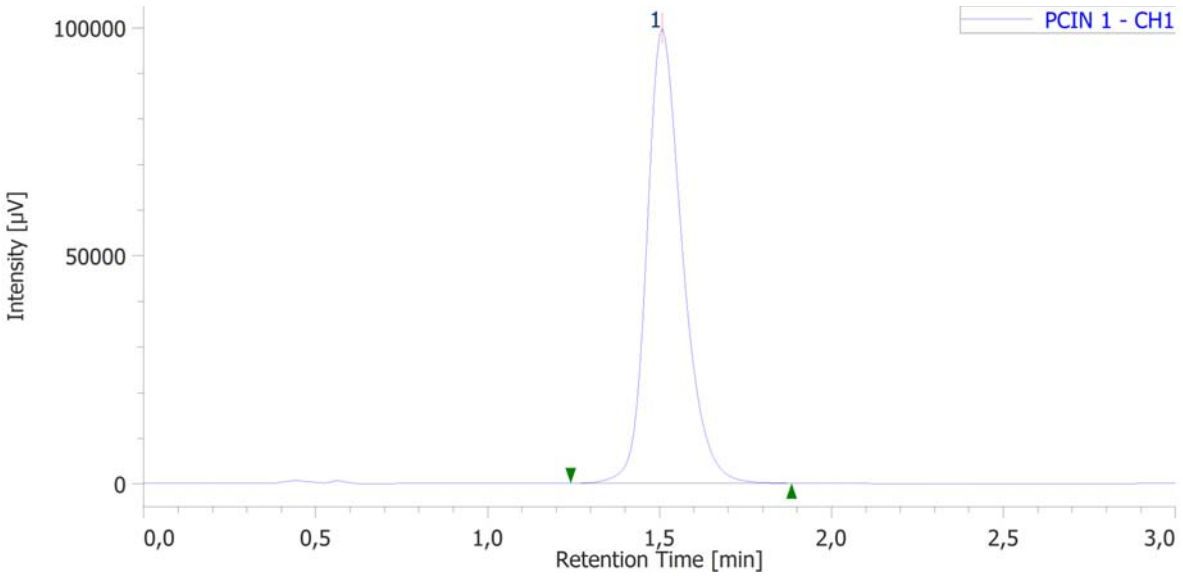

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:42:31
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,508	719533	99674	100,000	100,000	N/A	1093	N/A	1,254	

Creator QPackSA
Reviewer
Approver

Chromatogram

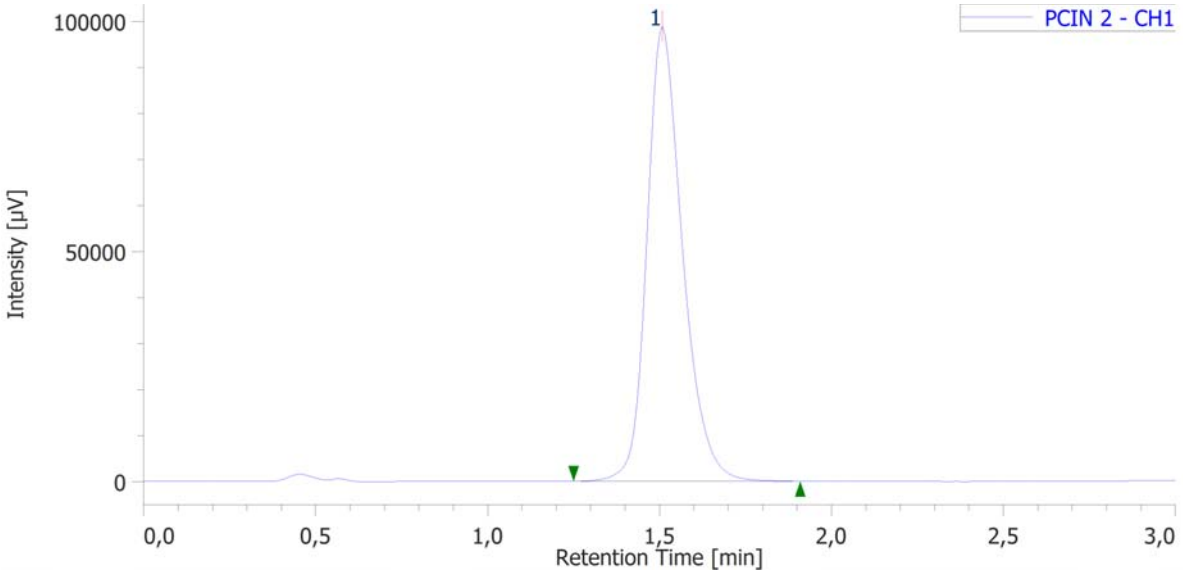

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:45:51
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,508	712662	98832	100,000	100,000	N/A	1095	N/A	1,261	

Creator QPackSA
Reviewer
Approver

Chromatogram

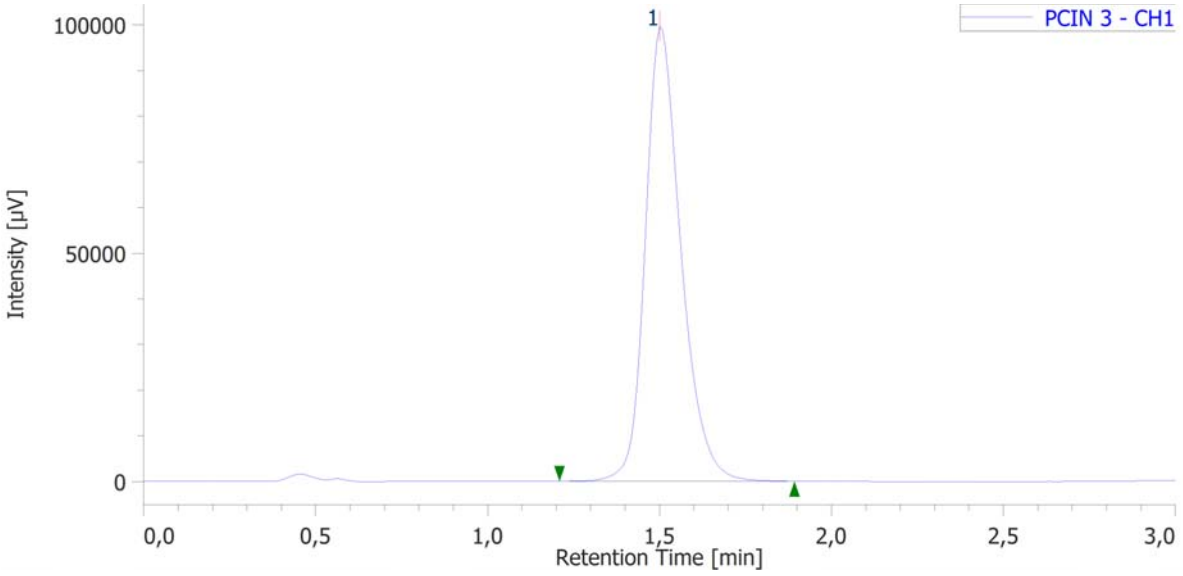

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:49:11
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	717417	99515	100,000	100,000	N/A	1084	N/A	1,307	

Creator QPackSA
Reviewer
Approver

Chromatogram

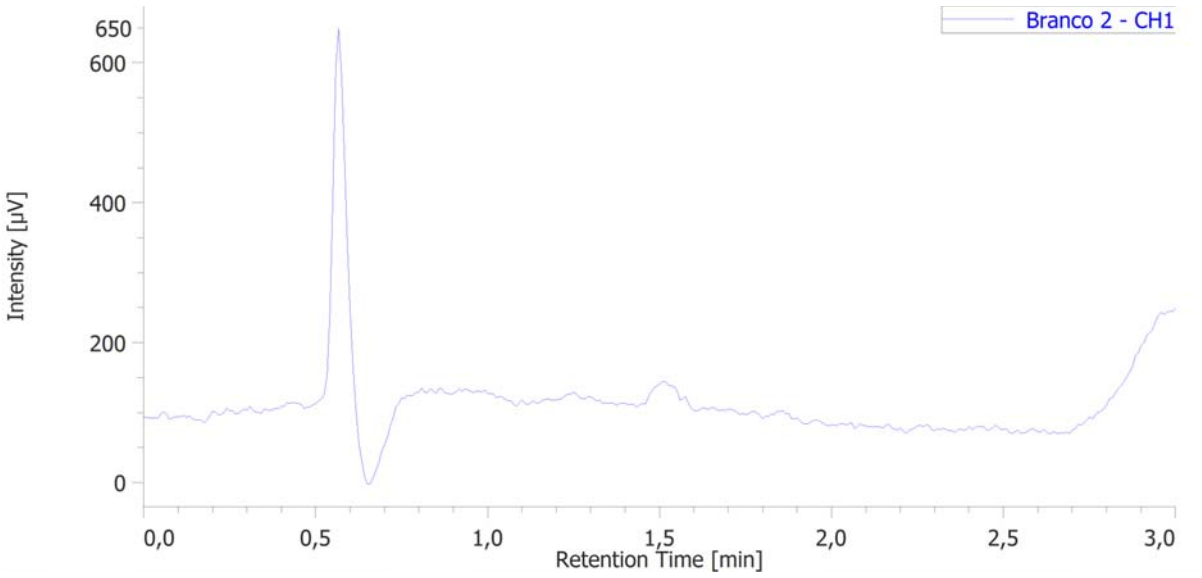


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:52:31
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

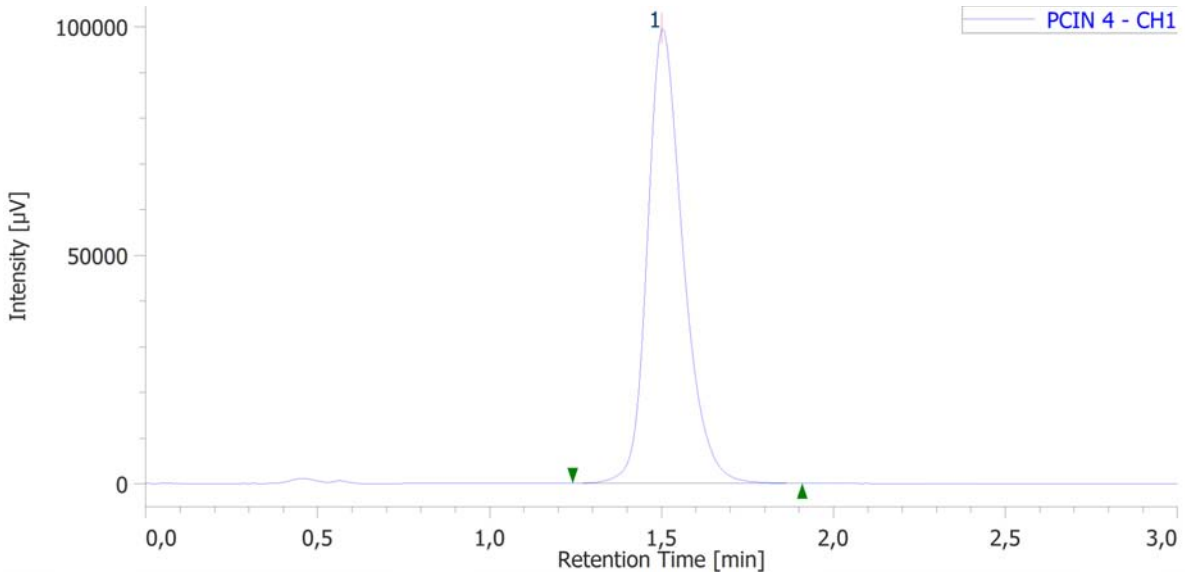

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:55:51
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	717859	99556	100,000	100,000	N/A	1082	N/A	1,314	

Creator QPackSA
Reviewer
Approver

Chromatogram

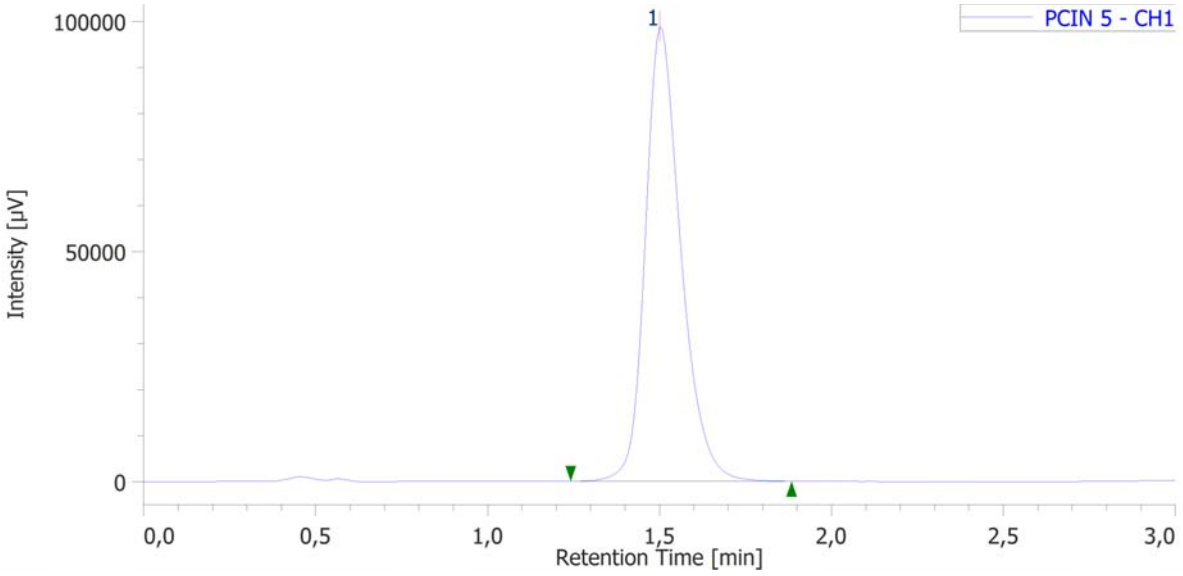

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:24
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 09:59:11
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	711236	98783	100,000	100,000	N/A	1084	N/A	1,307	

Creator QPackSA
Reviewer
Approver

Chromatogram

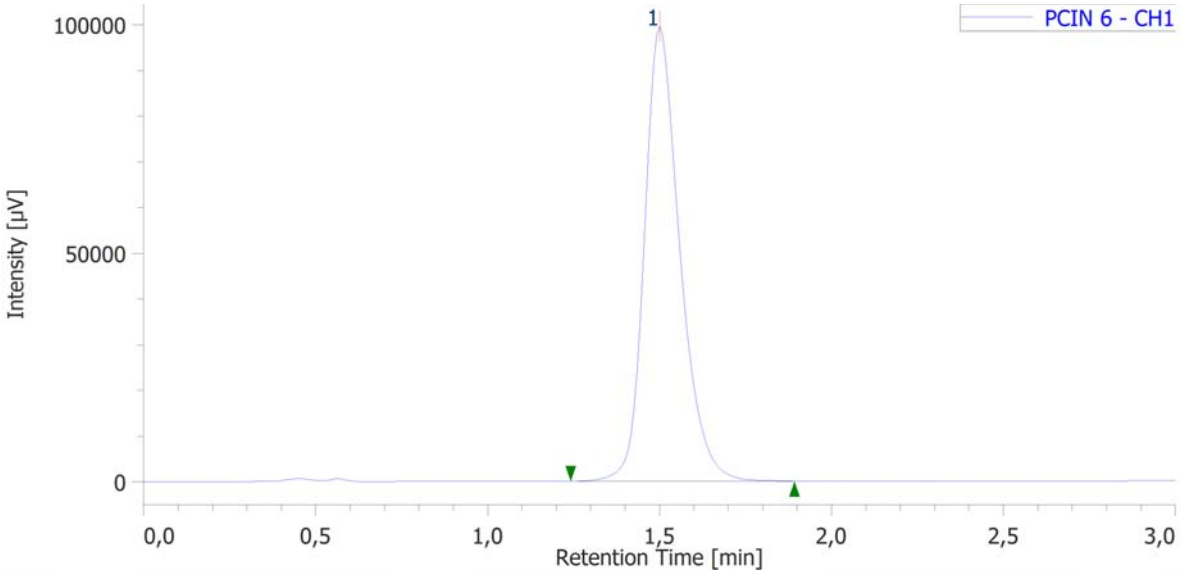

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:25
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:02:31
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.500	714561	99486	100.000	100.000	N/A	1091	N/A	1.276	

Creator QPackSA
Reviewer
Approver

Chromatogram

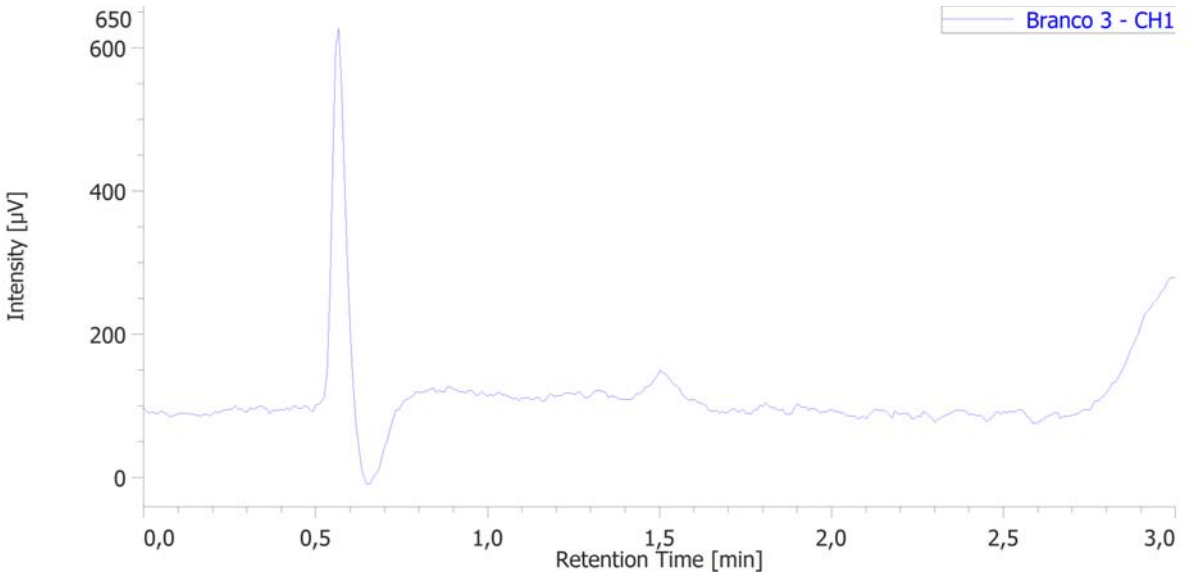


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:11:25
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:05:48
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

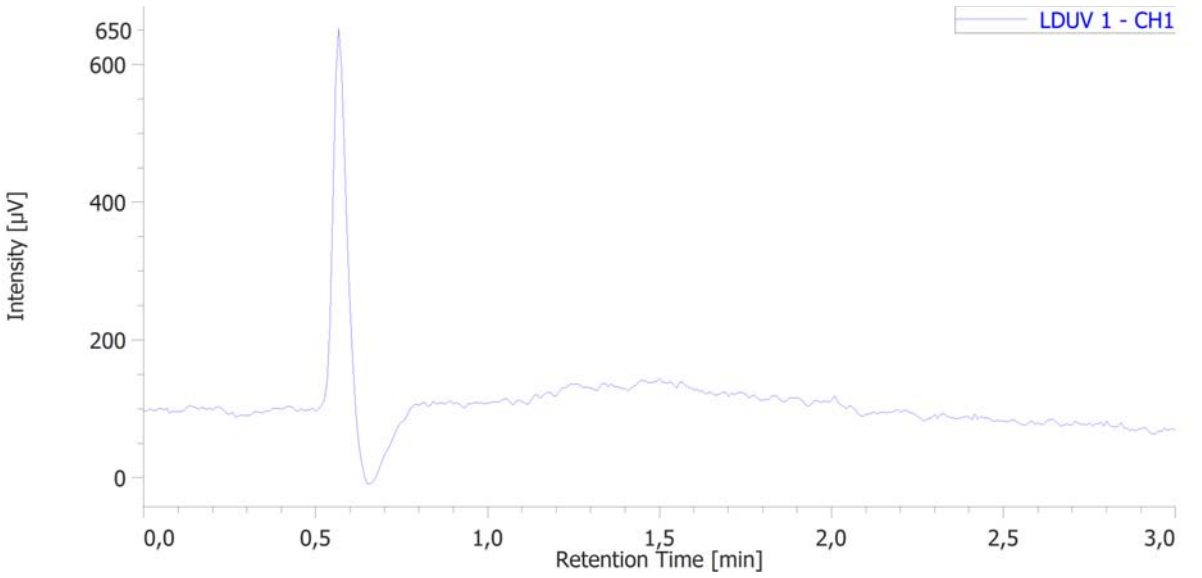


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:29:04
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:11:57
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

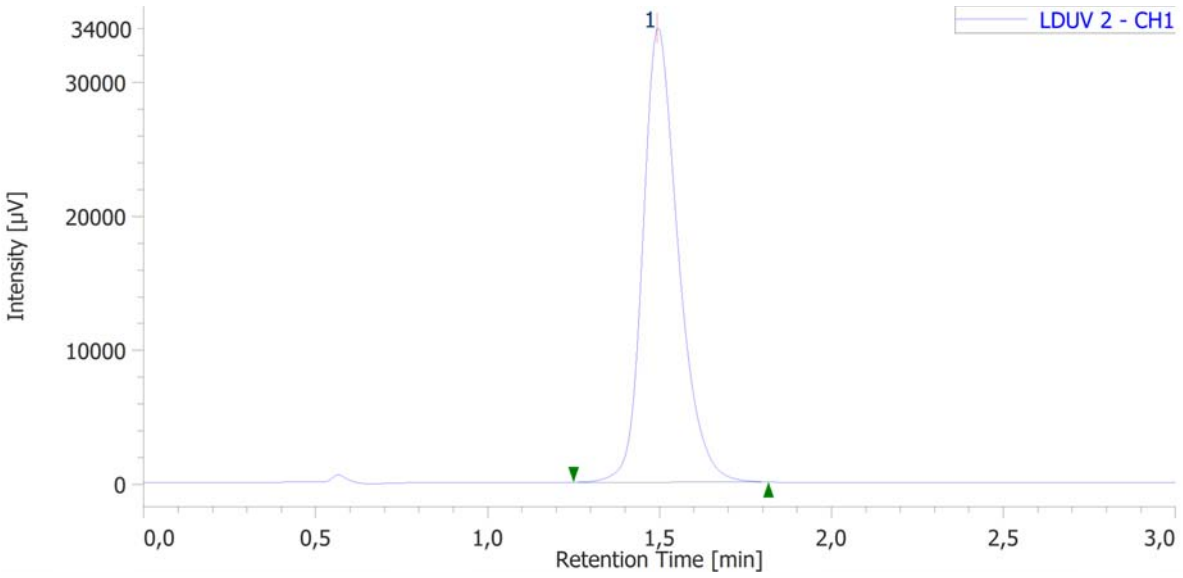

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:29:05
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:15:17
Volume	10.0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,492	243089	33866	100,000	100,000	N/A	1079	N/A	1,325	

Creator QPackSA
Reviewer
Approver

Chromatogram

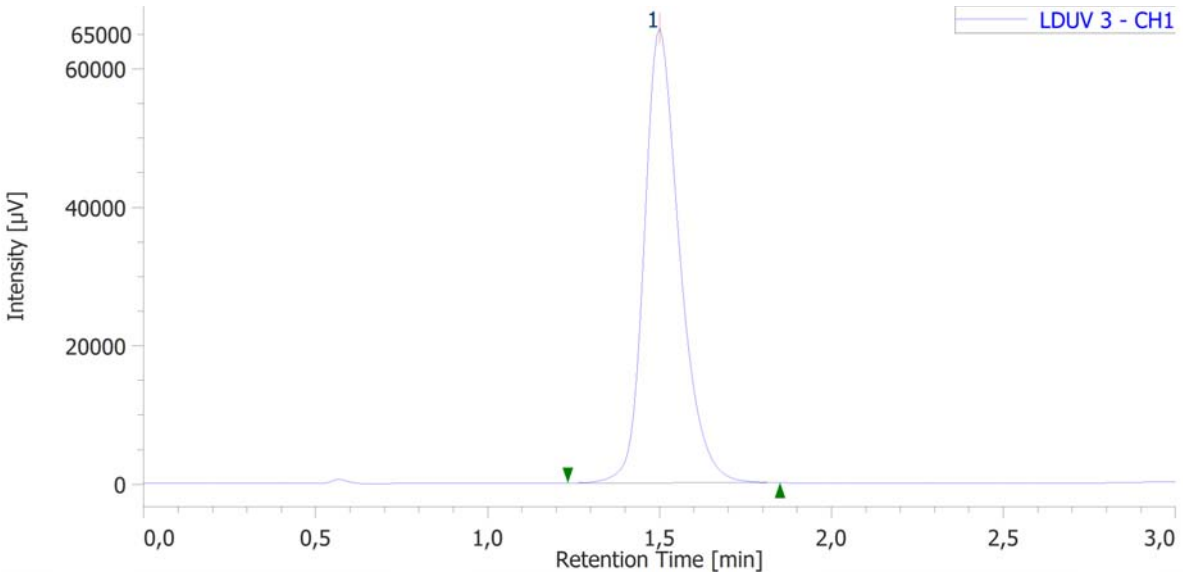

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:29:05
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:18:37
Volume	10.0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	470419	65639	100,000	100,000	N/A	1096	N/A	1,272	

Creator QPackSA
Reviewer
Approver

Chromatogram

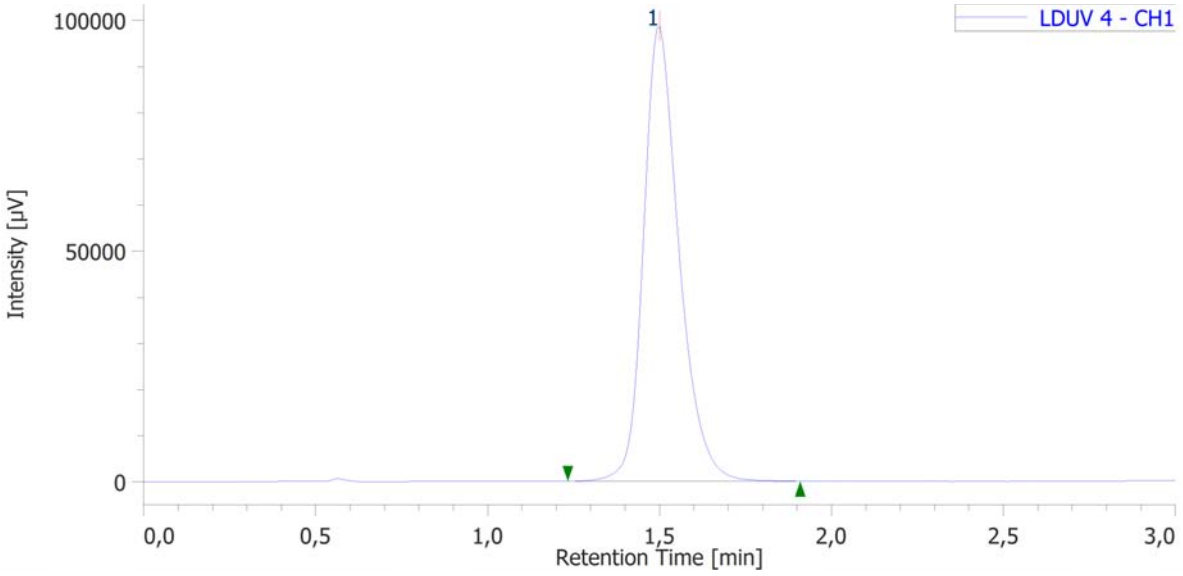

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:29:06
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:21:57
Volume	10.0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	708287	98552	100,000	100,000	N/A	1094	N/A	1,246	

Creator QPackSA
Reviewer
Approver

Chromatogram

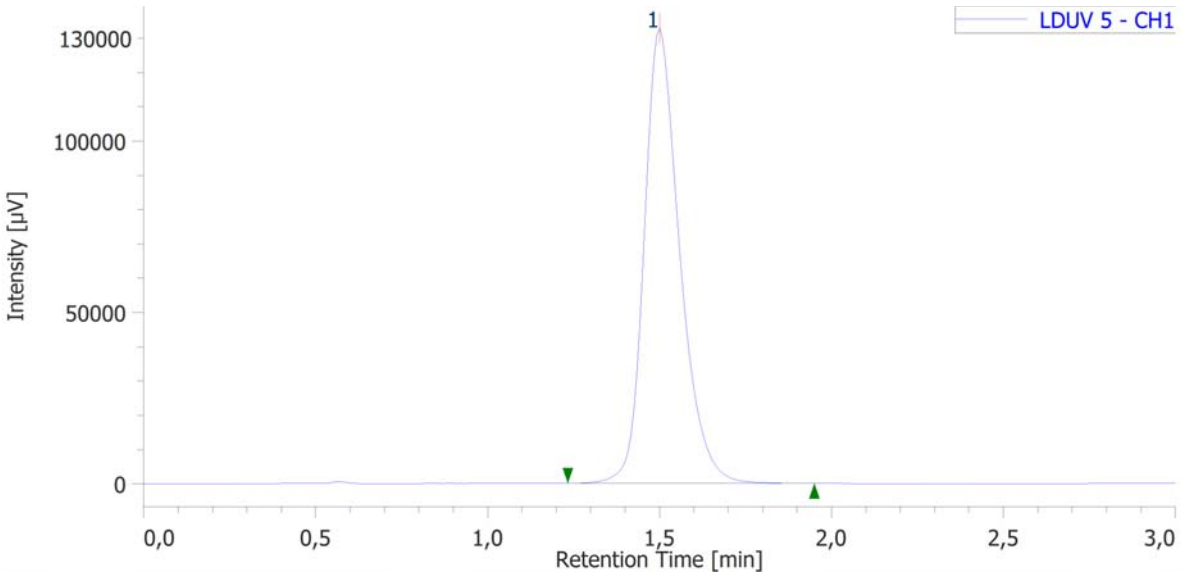

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:29:06
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:25:19
Volume	10.0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.500	956546	132705	100.000	100.000	N/A	1084	N/A	1.275	

Creator QPackSA
Reviewer
Approver

Chromatogram

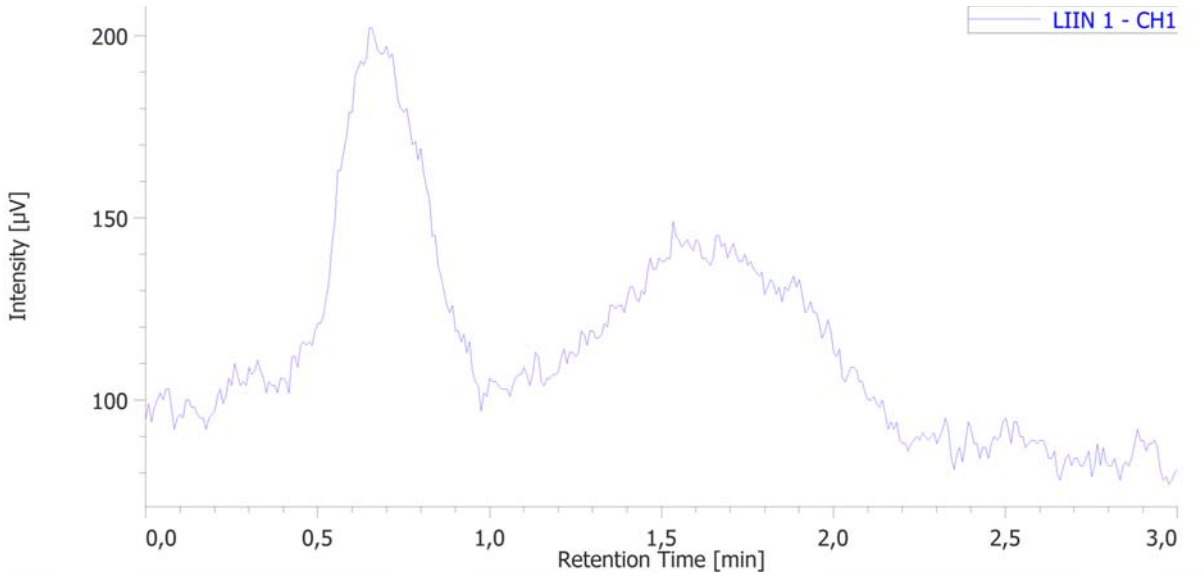


Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:48:13
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:30:55
Volume	0.1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

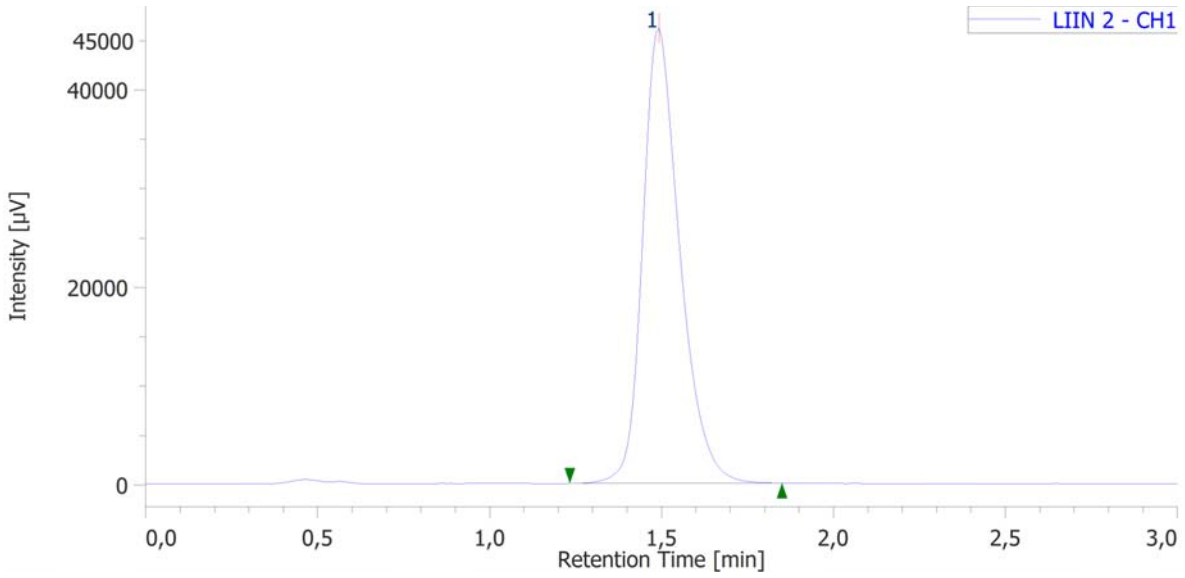

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:48:14
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:34:12
Volume	5.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,492	345953	46049	100,000	100,000	N/A	979	N/A	1,289	

Creator QPackSA
Reviewer
Approver

Chromatogram

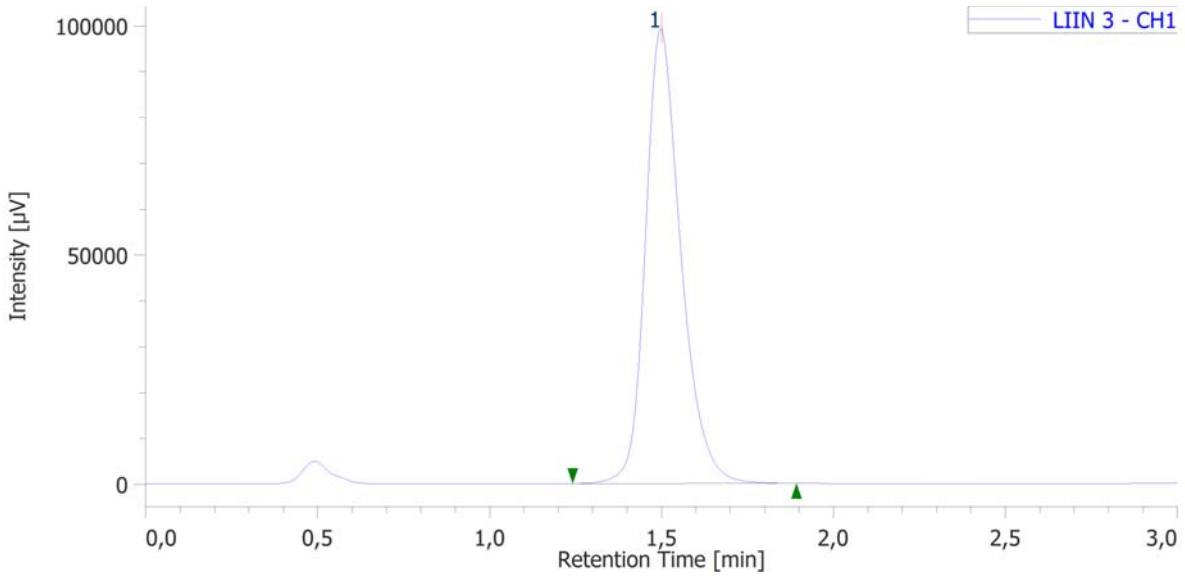

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:48:15
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:37:30
Volume	10.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	711576	99218	100,000	100,000	N/A	1098	N/A	1,243	

Creator QPackSA
Reviewer
Approver

Chromatogram

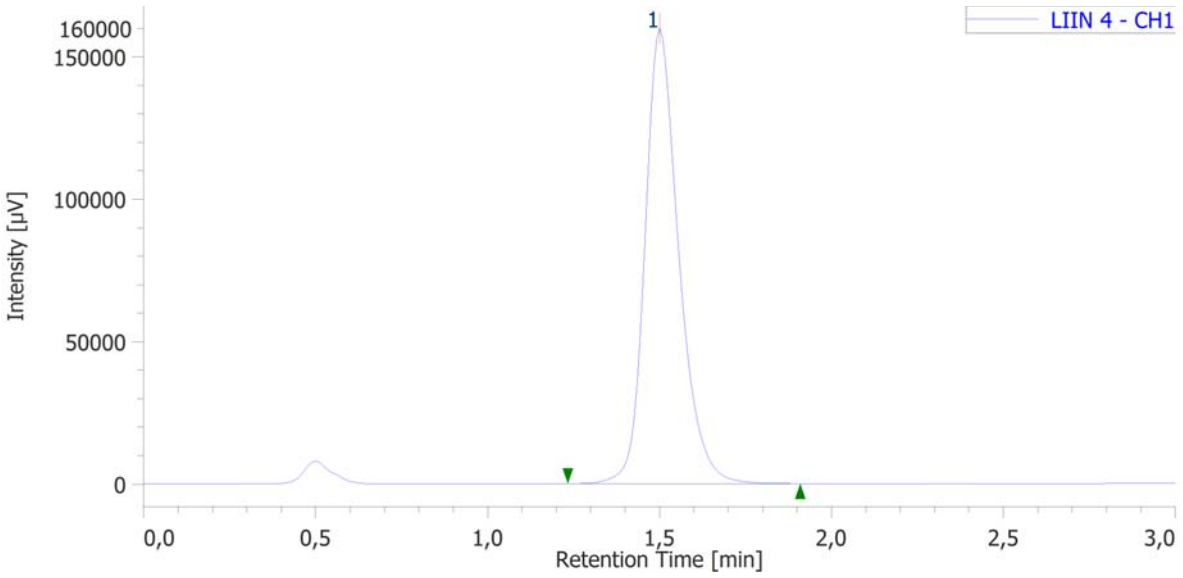

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:48:15
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:40:52
Volume	15,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	1094567	159772	100,000	100,000	N/A	1209	N/A	1,258	

Creator QPackSA
Reviewer
Approver

Chromatogram

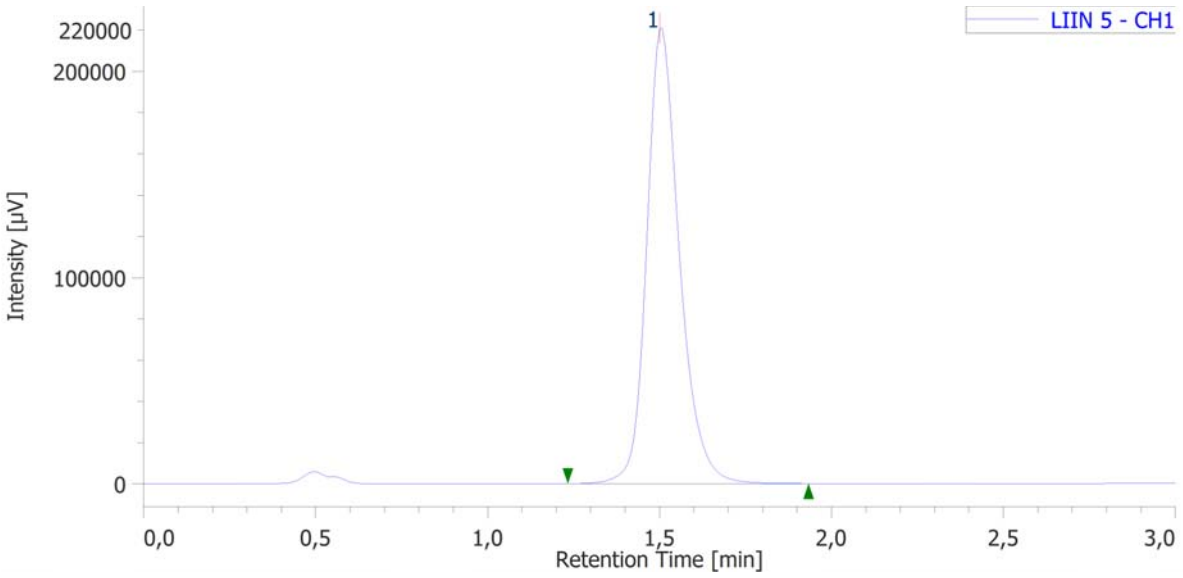

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 10:48:15
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 10:44:15
Volume	20.0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,500	1459170	220556	100,000	100,000	N/A	1308	N/A	1,302	

Creator QPackSA
Reviewer
Approver

Chromatogram

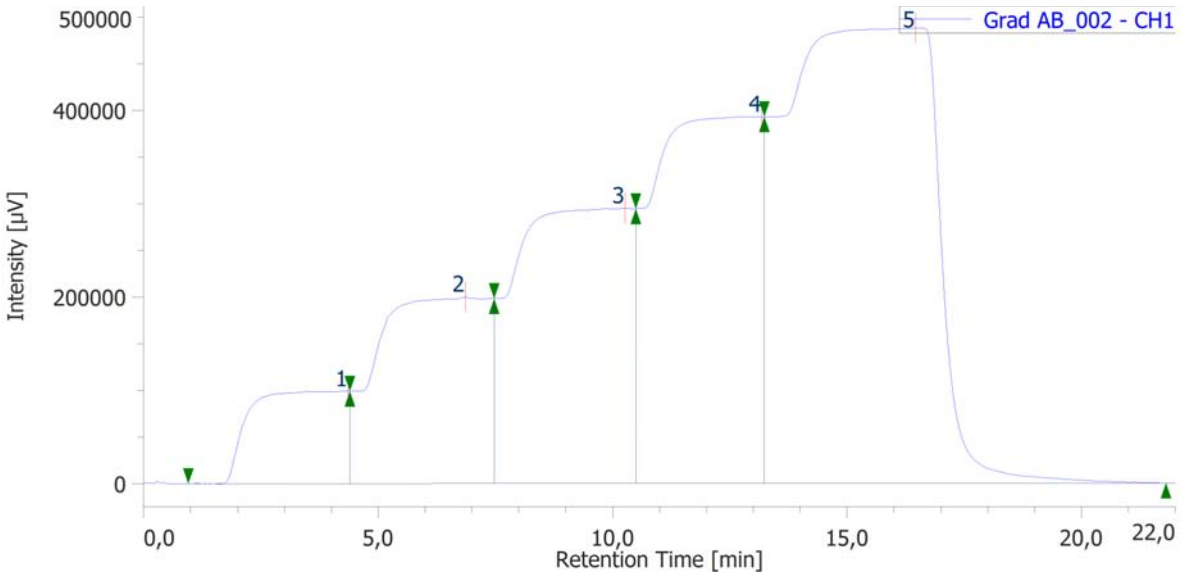

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 13:04:30
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 12:36:19
Volume	0.0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	22.0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4.358	13568335	98892	5.109	6.712	N/A	N/A	N/A	N/A	
2	40 %	1	6.858	32489400	200153	12.233	13.585	N/A	N/A	N/A	N/A	
3	60 %	1	10.267	49803723	294775	18.752	20.007	N/A	N/A	N/A	N/A	
4	80 %	1	13.175	61050811	392503	22.987	26.640	N/A	N/A	N/A	N/A	
5	100 %	1	16.458	108677099	487017	40.919	33.055	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

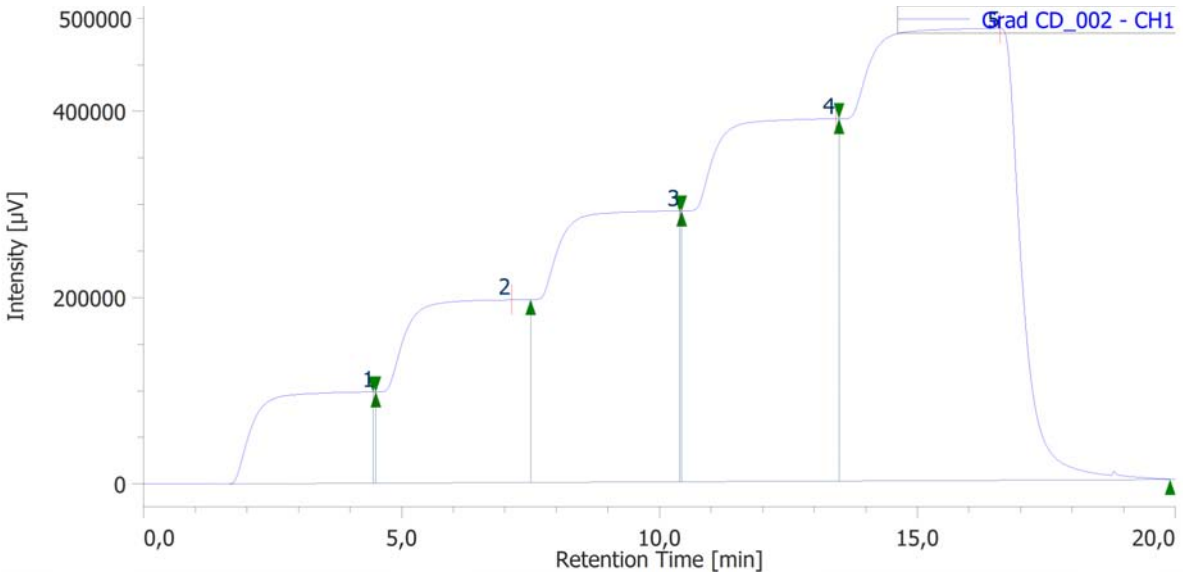

Chromatogram Information	
User Name	QPackSA
Date Modified	04/05/2023 14:10:36
Description	
HPLC System Name	HPLC-0004
Injection Date	04/05/2023 13:37:53
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad CD_002-CH1
Sample Name	
Channel Name	UV
Sampling Interval	500 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	1	4,483	342499	97865	0,170	6,714	N/A	N/A	N/A	N/A	
2	40 %	1	7,125	31985741	196294	15,853	13,466	N/A	N/A	N/A	N/A	
3	60 %	1	10,400	726135	290447	0,360	19,925	N/A	N/A	N/A	N/A	
4	80 %	1	13,417	67337065	388378	33,374	26,643	N/A	N/A	N/A	N/A	
5	100 %	1	16,600	101374867	484751	50,244	33,254	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver