
Spectral Library Screening Results

Injection Details

Injection Name:	**EDUV Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 09:45**	*Sample Weight:*	**1,0000**

UV Spectra — Cafeína

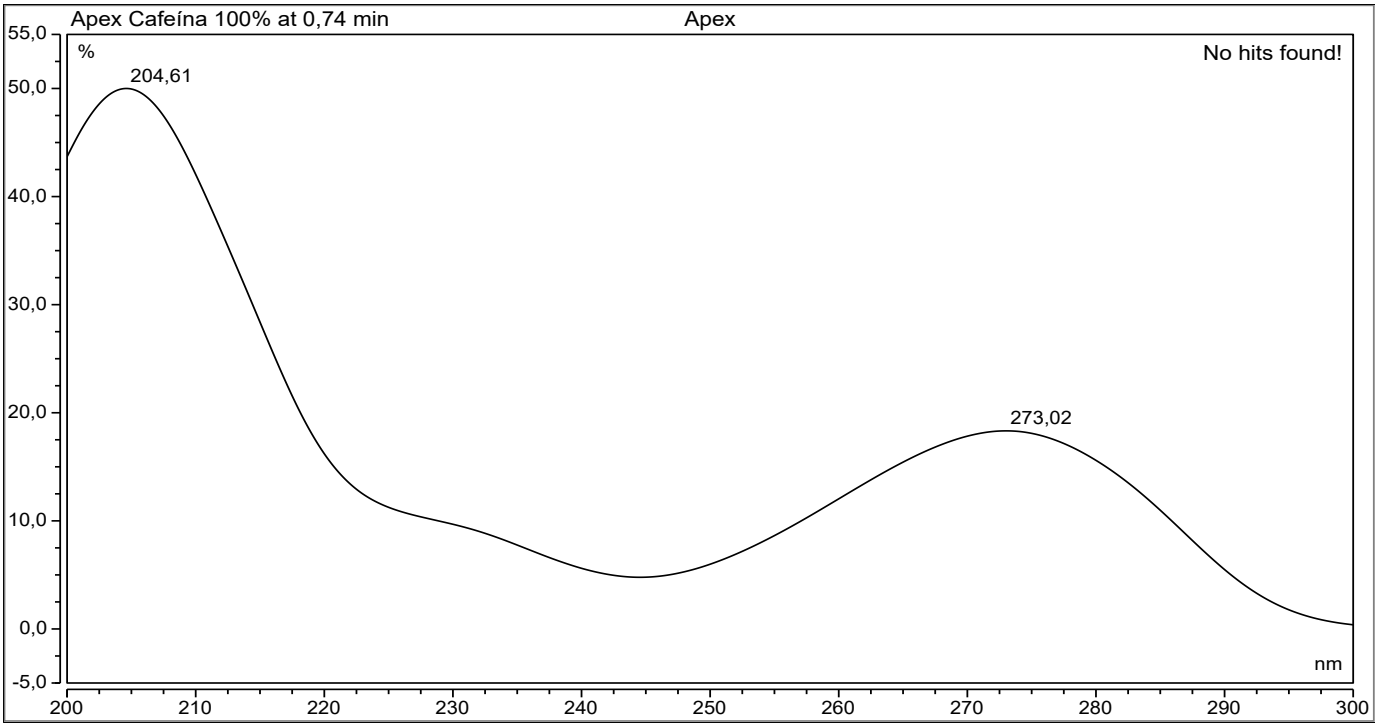

Spectral Library Screening Results

	Hit# 1		Hit# 2		Hit# 3	
Library:	n.a.		n.a.		n.a.	
Component:	n.a.		n.a.		n.a.	
Match Factor:		n.a.		n.a.		n.a.
Ret.Time:		n.a.		n.a.		n.a.
Origin:						
Acq.Date:	n.a.		n.a.		n.a.	
Instrument Method:	n.a.		n.a.		n.a.	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Spectral Library Screening Results

Injection Details

Injection Name:	**EDUV Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 09:45**	*Sample Weight:*	**1,0000**

UV Spectra — Cafeína



Spectral Library Screening Results

	Hit# 1	Hit# 2	Hit# 3
Library:	n.a.	n.a.	n.a.
Component:	n.a.	n.a.	n.a.
Match Factor:	n.a.	n.a.	n.a.
Ret.Time:	n.a.	n.a.	n.a.
Origin:			
Acq.Date:	n.a.	n.a.	n.a.
Instrument Method:	n.a.	n.a.	n.a.


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Left 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 10:39**	*Sample Weight:*	**1,0000**

Chromatogram

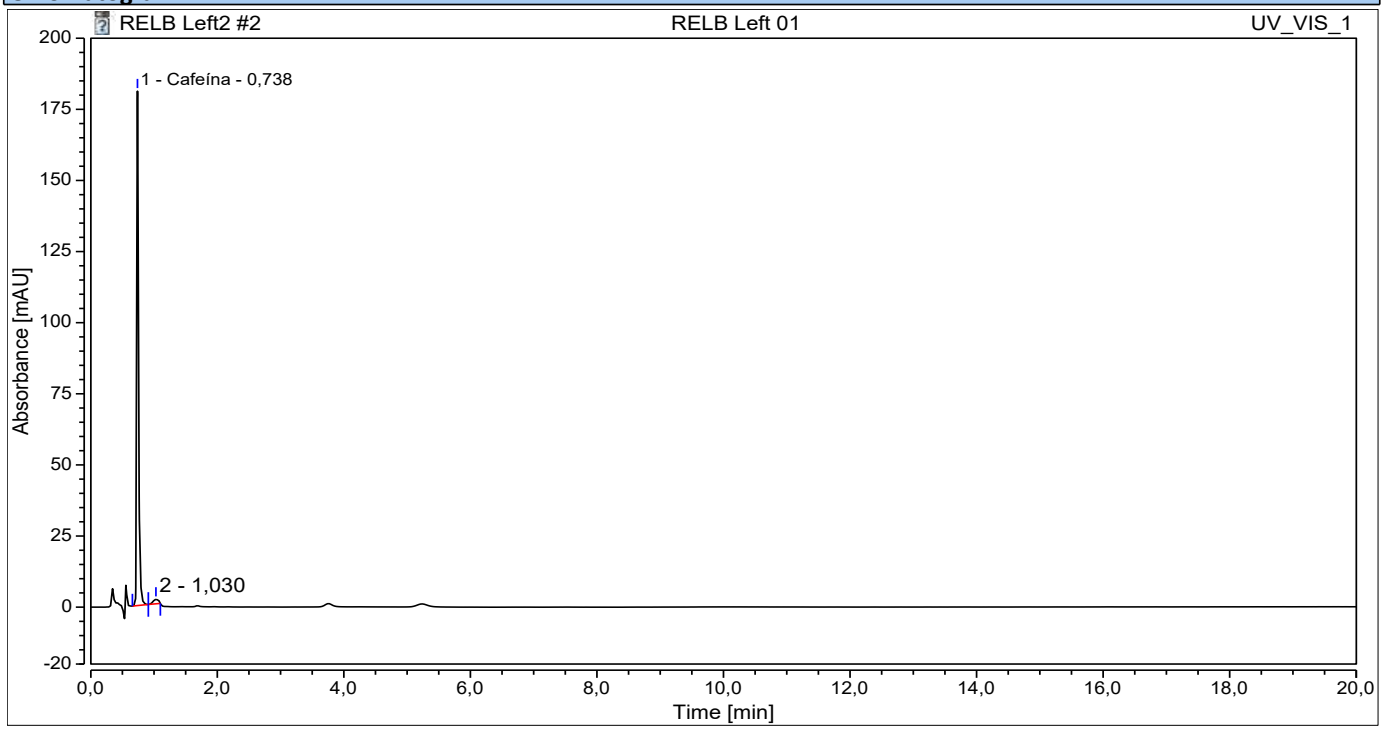

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,738	5,9498	180,841	97,43	99,16	n.a.
Total:			**5,950**	**180,841**	**97,430**	**99,163**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Left 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 10:39**	*Sample Weight:*	**1,0000**

Chromatogram

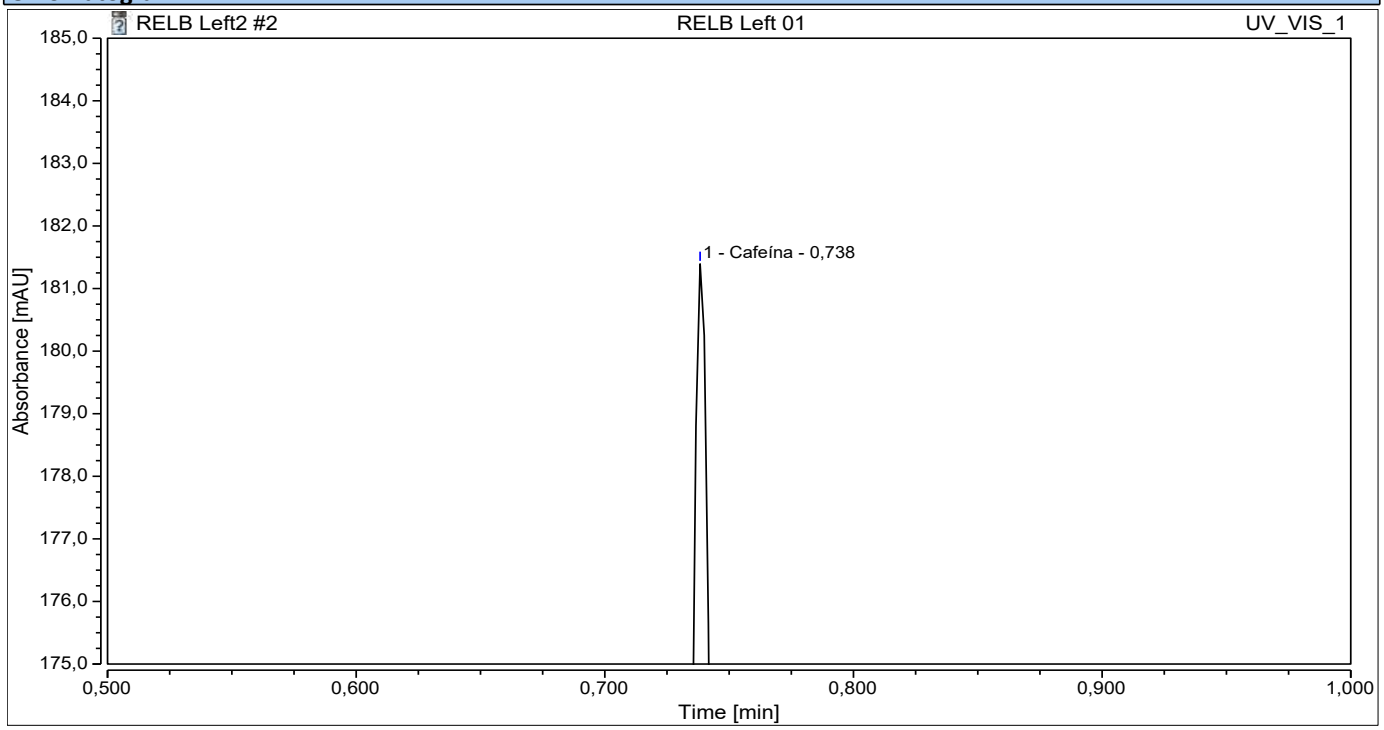

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,738	5,9498	180,841	97,43	99,16	n.a.
Total:			**5,950**	**180,841**	**97,430**	**99,163**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Left 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 10:39**	*Sample Weight:*	**1,0000**

Chromatogram

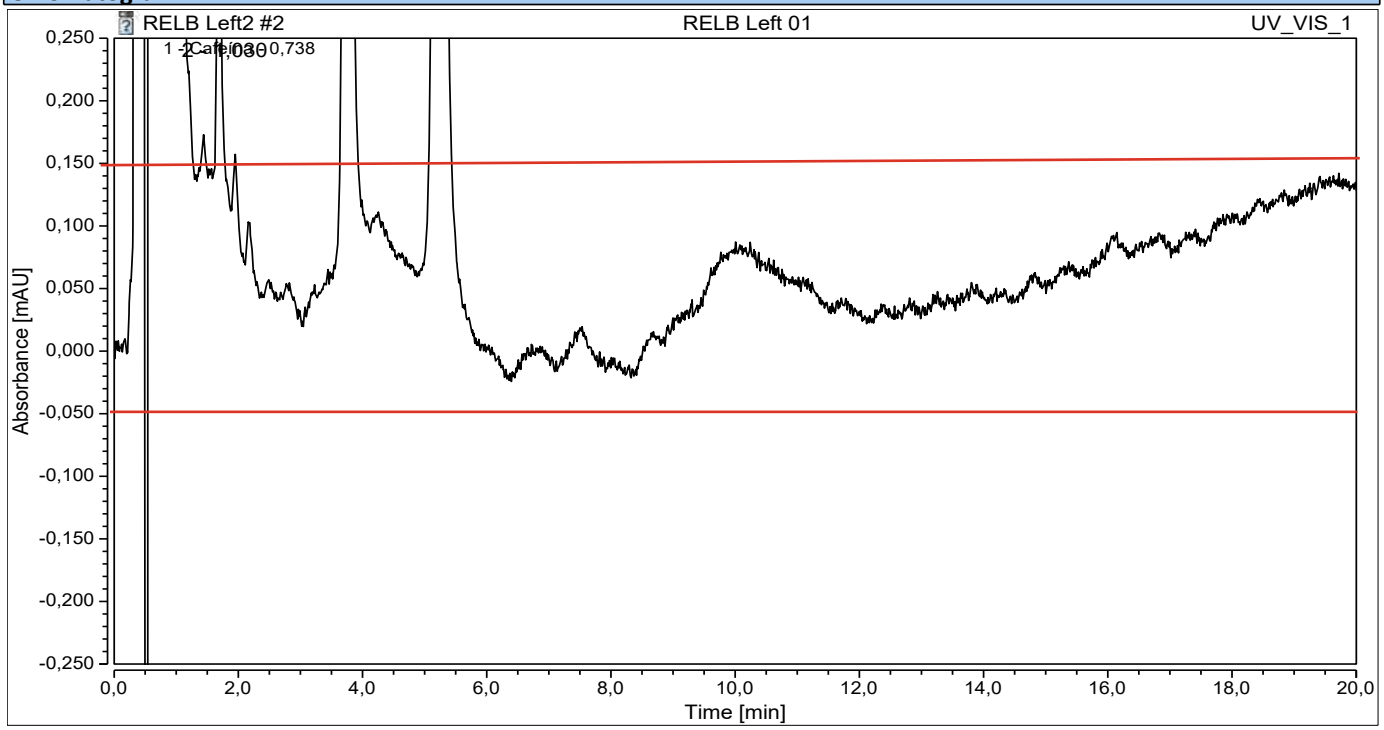

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,738	5,9498	180,841	97,43	99,16	n.a.
Total:			**5,950**	**180,841**	**97,430**	**99,163**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Left 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**Qualificação**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 10:39**	*Sample Weight:*	**1,0000**

Chromatogram

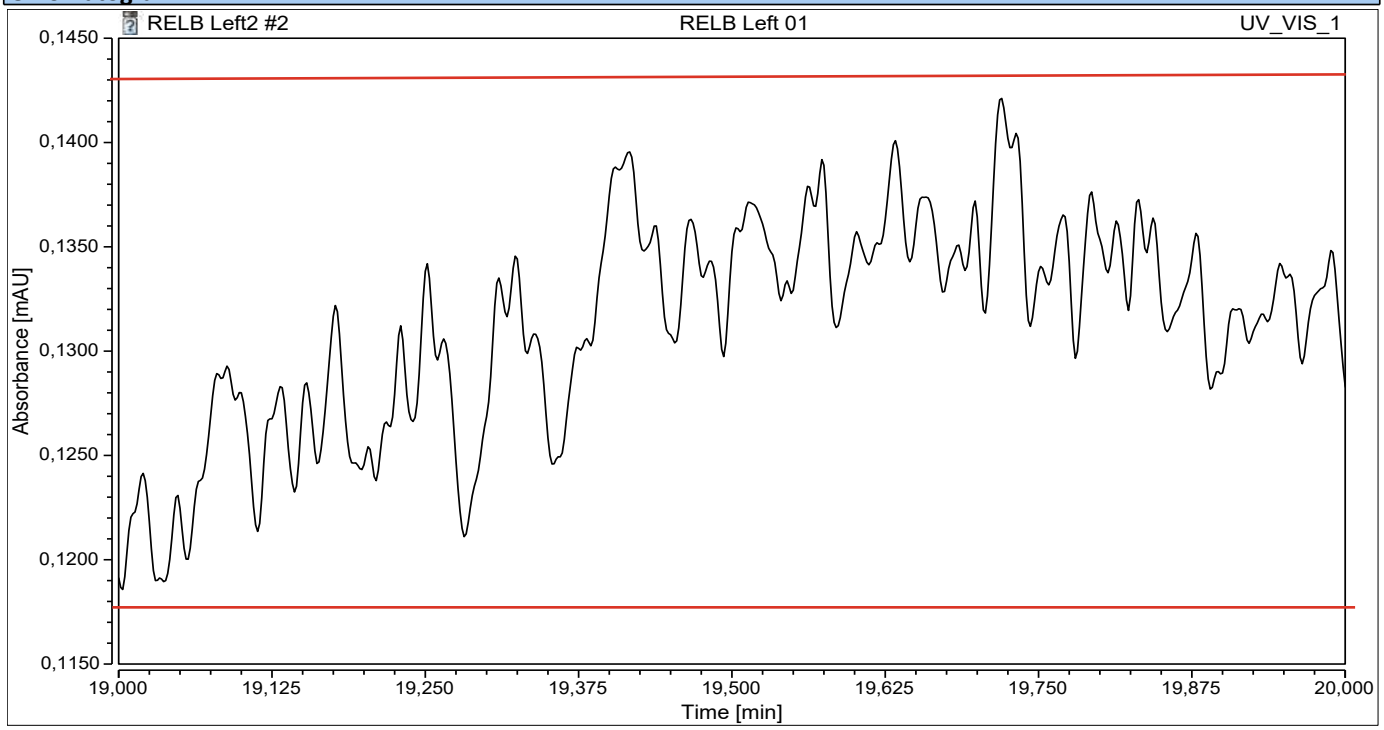

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,738	5,9498	180,841	97,43	99,16	n.a.
Total:			**5,950**	**180,841**	**97,430**	**99,163**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:23**	*Sample Weight:*	**1,0000**

Chromatogram

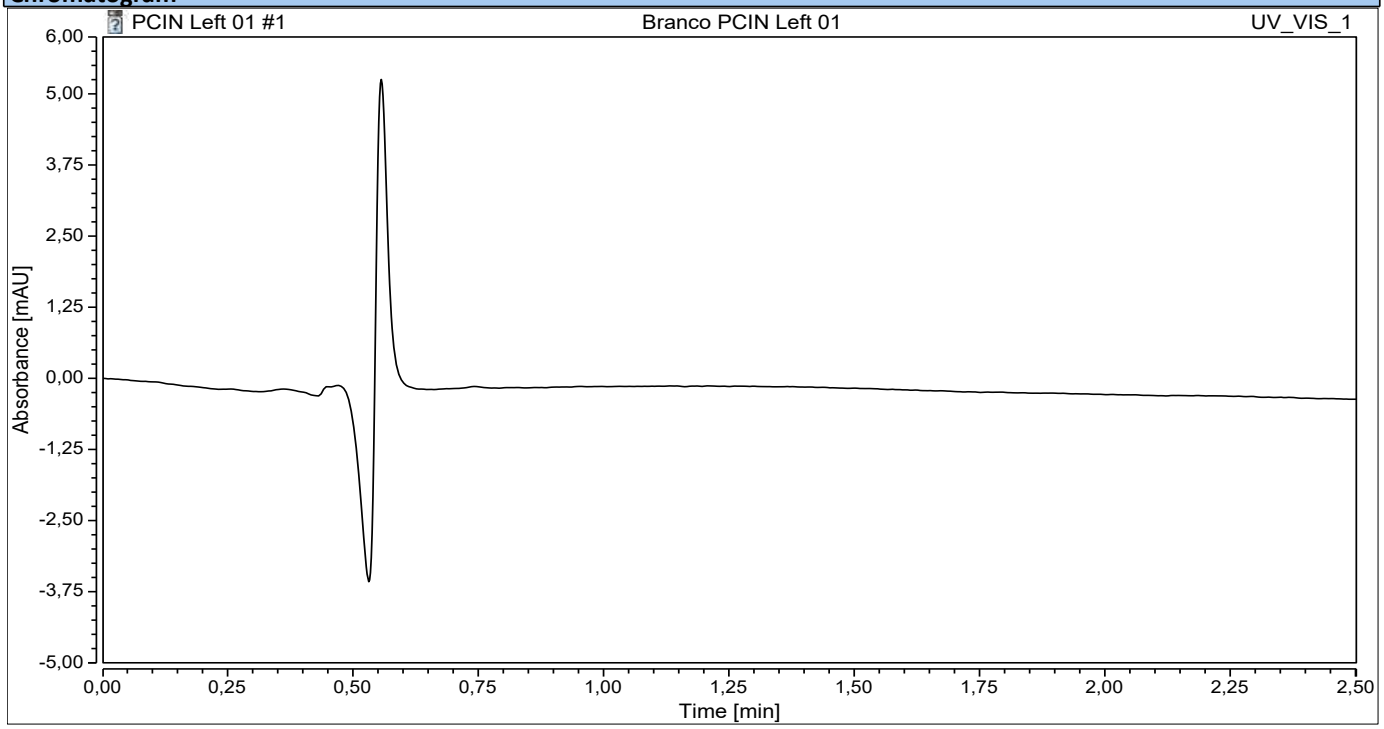

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:26**	*Sample Weight:*	**1,0000**

Chromatogram

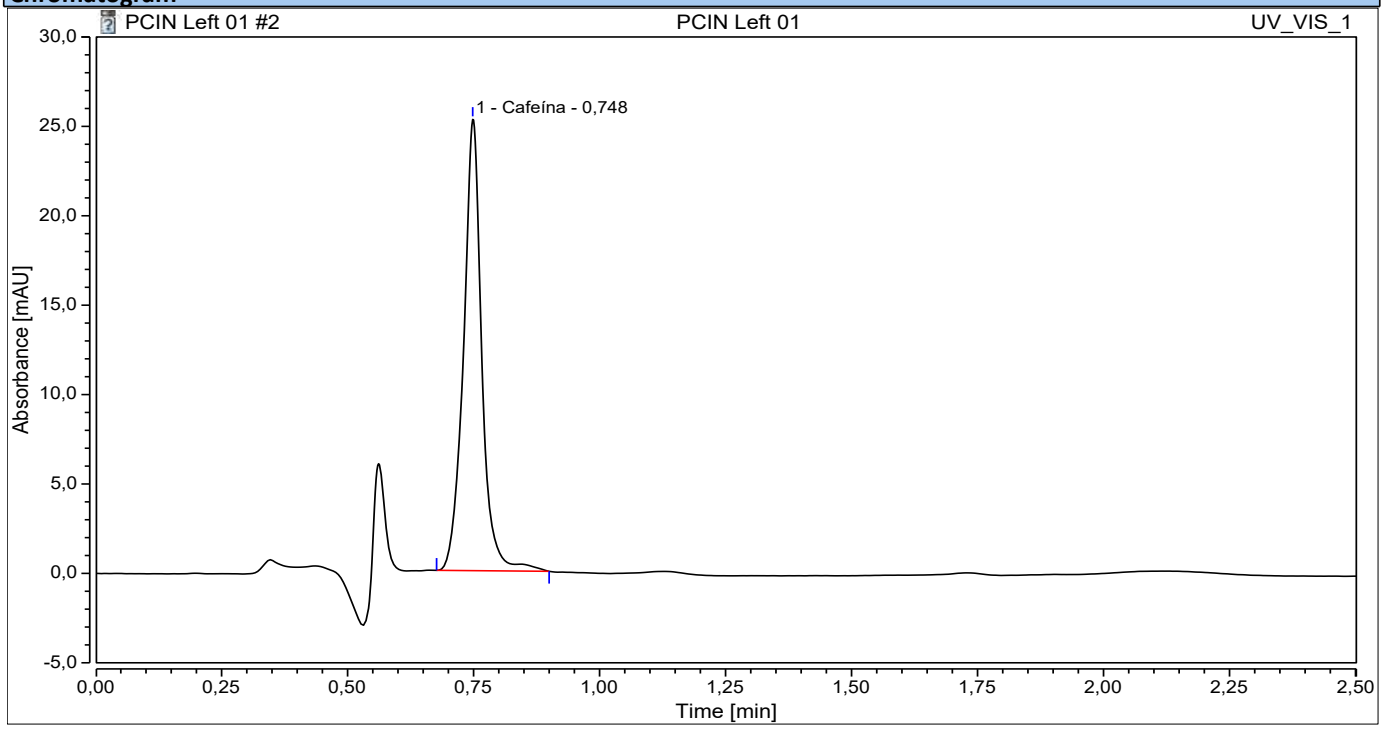

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,748	1,0596	25,236	100,00	100,00	n.a.
Total:			**1,060**	**25,236**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 02**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:29**	*Sample Weight:*	**1,0000**

Chromatogram

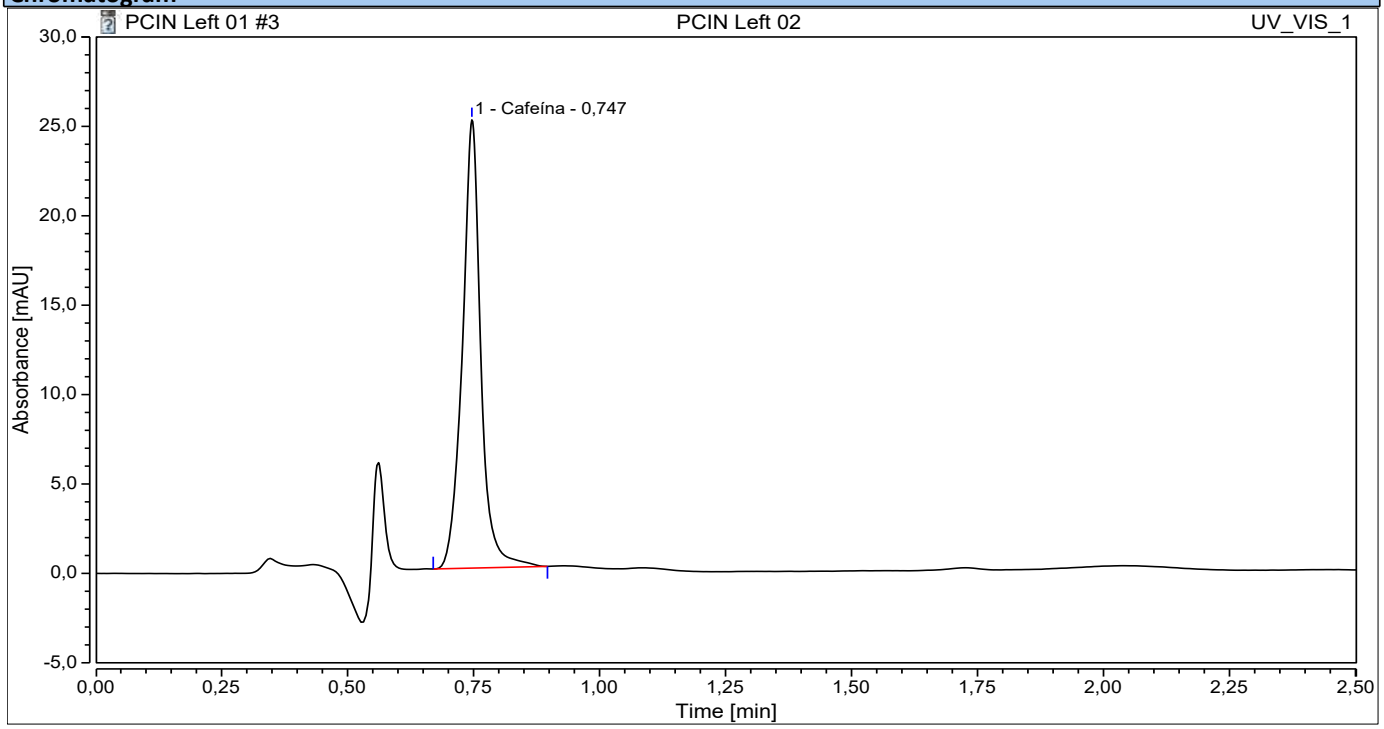

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	1,0628	25,069	100,00	100,00	n.a.
Total:			**1,063**	**25,069**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 03**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:31**	*Sample Weight:*	**1,0000**

Chromatogram

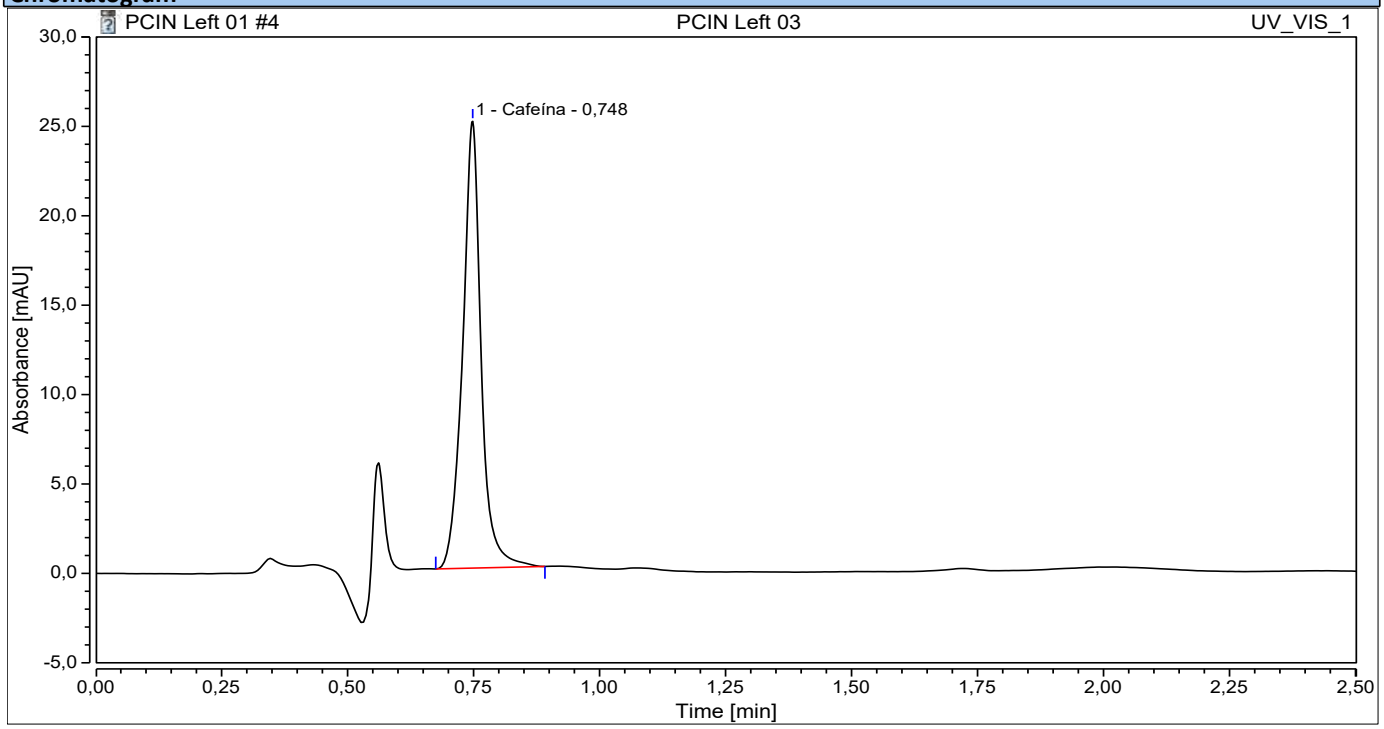

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,748	1,0609	24,989	100,00	100,00	n.a.
Total:			**1,061**	**24,989**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Left 02**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:35**	*Sample Weight:*	**1,0000**

Chromatogram

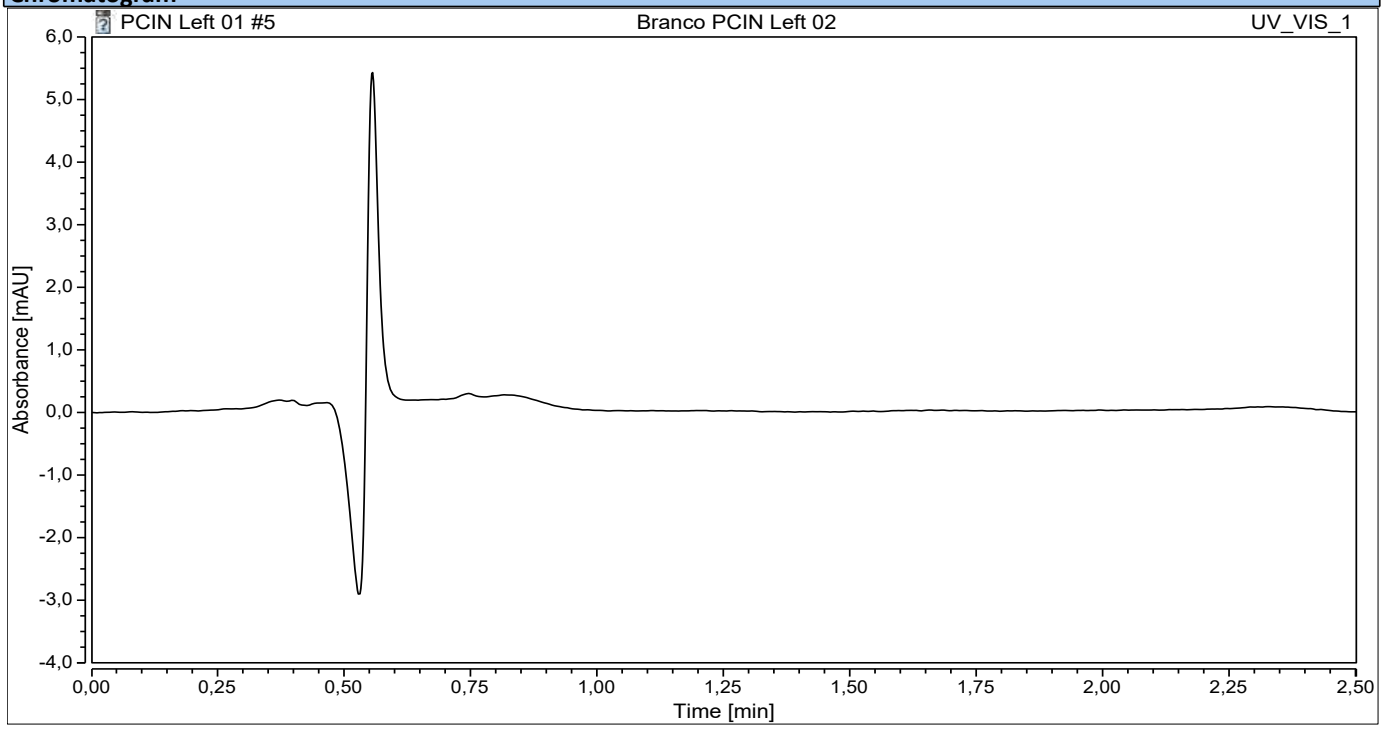

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 04**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:37**	*Sample Weight:*	**1,0000**

Chromatogram

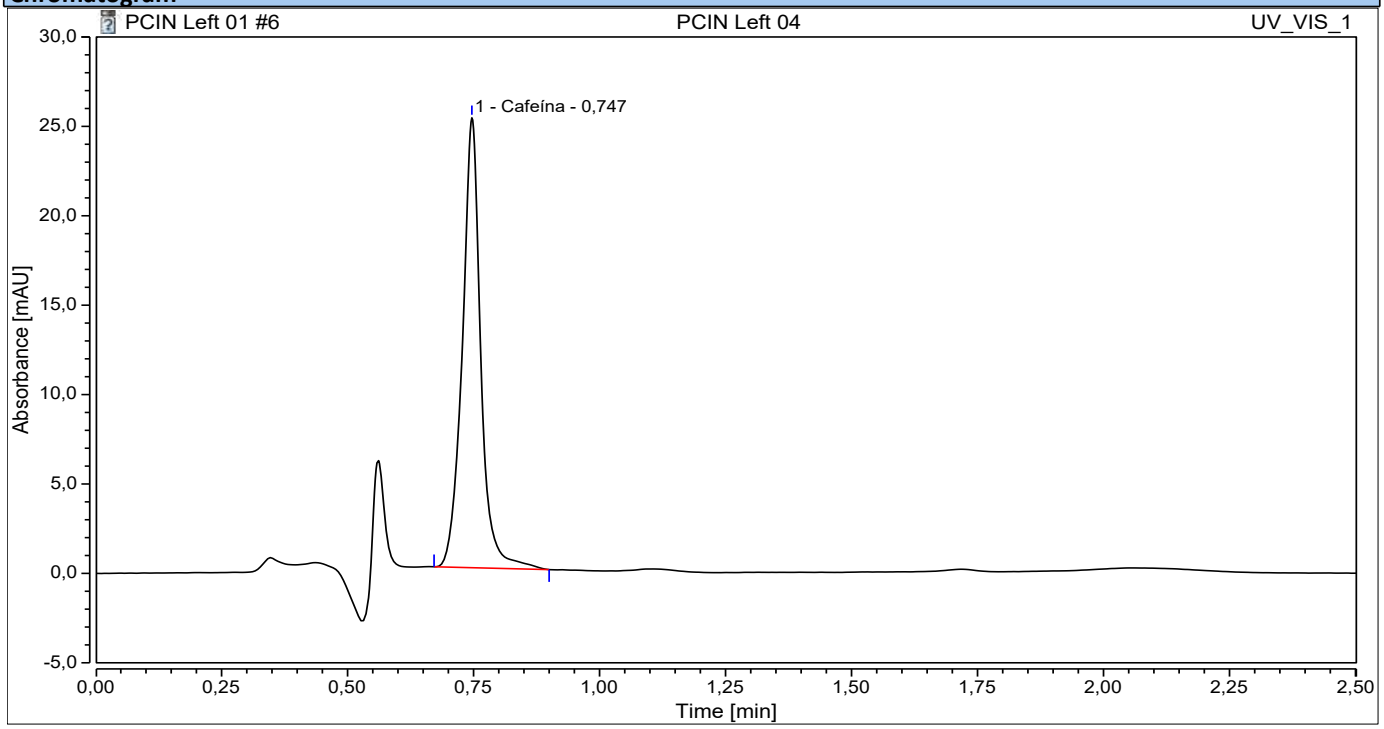

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	1,0663	25,162	100,00	100,00	n.a.
Total:			**1,066**	**25,162**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 05**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:40**	*Sample Weight:*	**1,0000**

Chromatogram

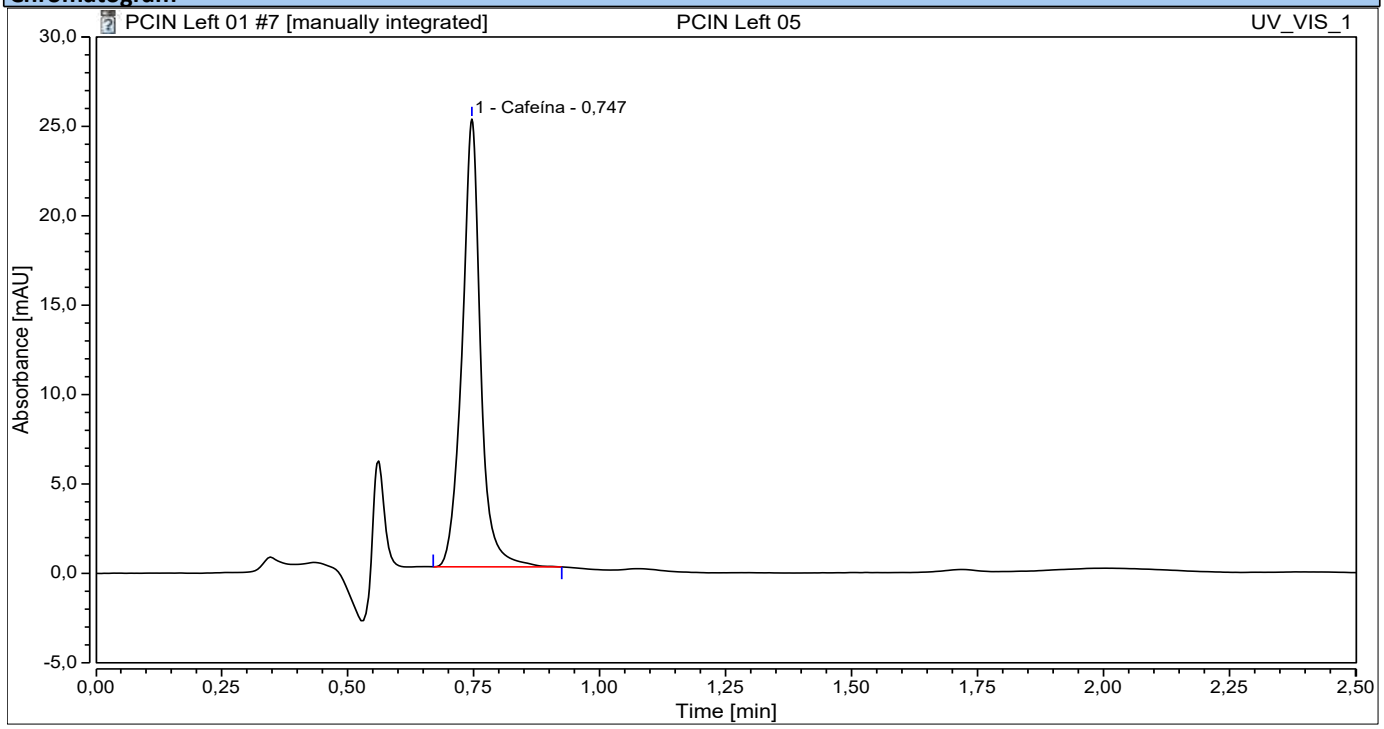

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	1,0631	25,042	100,00	100,00	n.a.
Total:			**1,063**	**25,042**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Left 06**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:43**	*Sample Weight:*	**1,0000**

Chromatogram

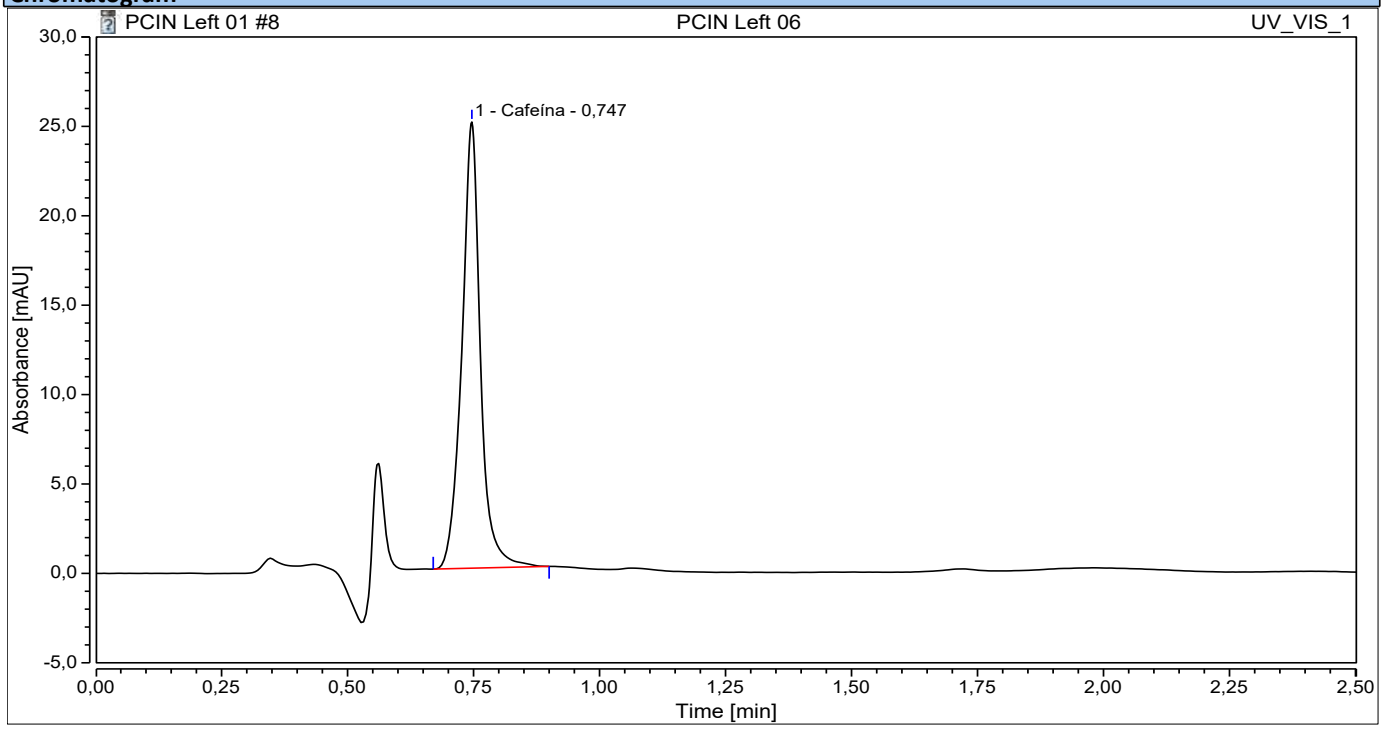

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	1,0626	24,953	100,00	100,00	n.a.
Total:			**1,063**	**24,953**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Left 03**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 13:46**	*Sample Weight:*	**1,0000**

Chromatogram

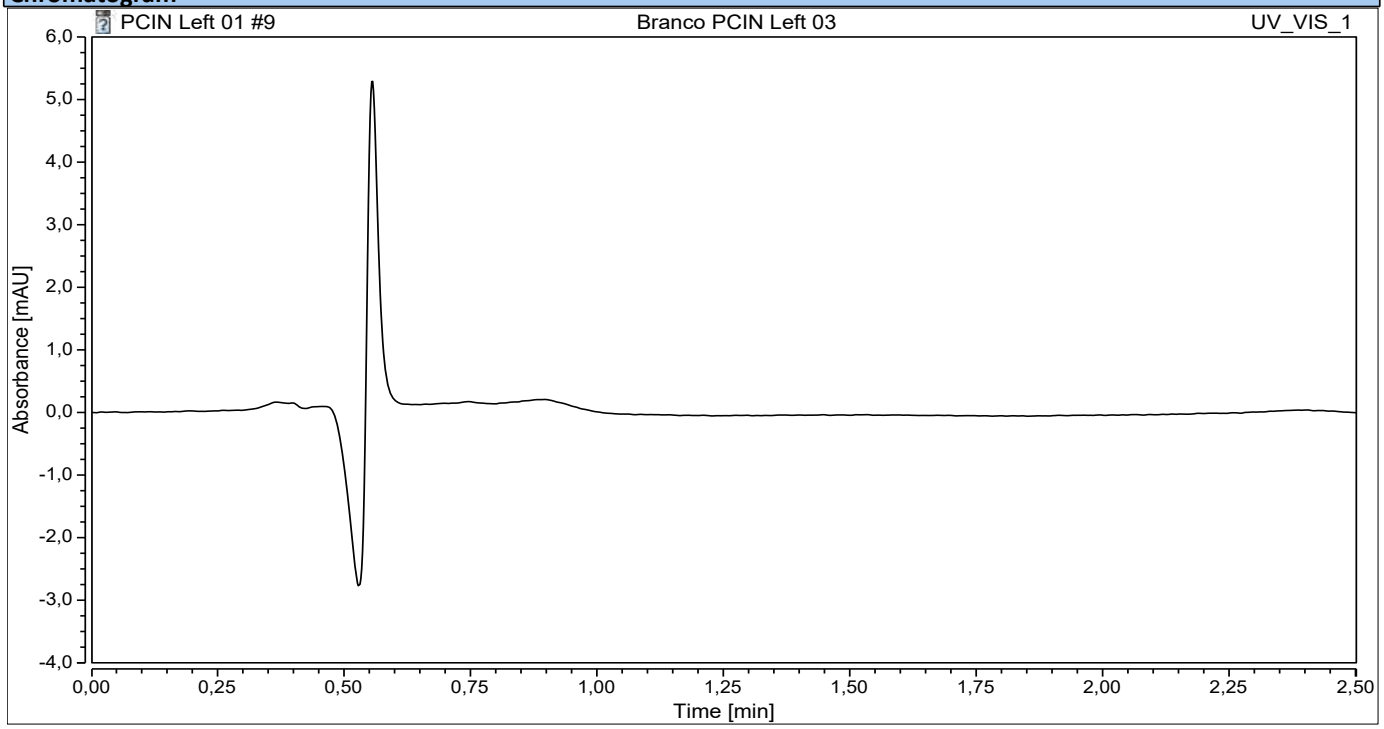

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 14:32**	*Sample Weight:*	**1,0000**

Chromatogram

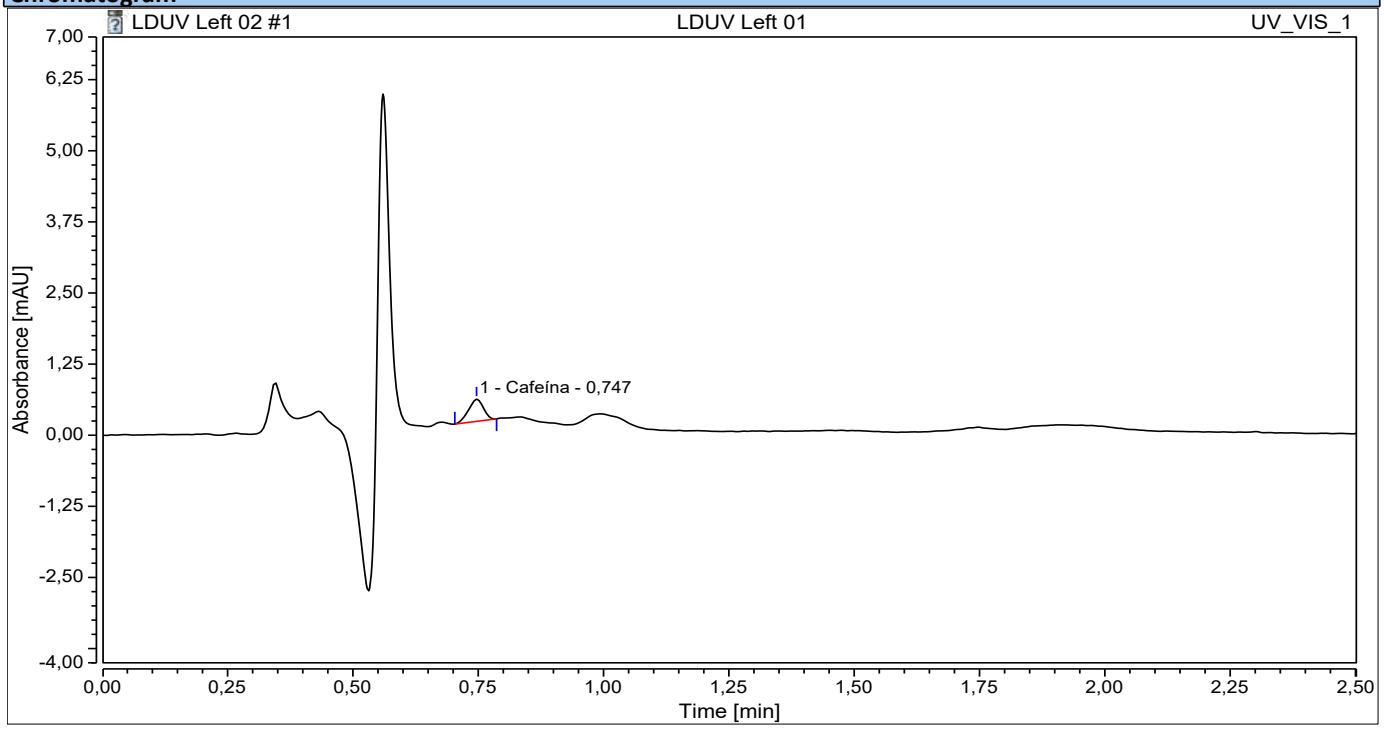

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	0,0135	0,391	100,00	100,00	n.a.
Total:			**0,013**	**0,391**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Left 02**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 14:35**	*Sample Weight:*	**1,0000**

Chromatogram

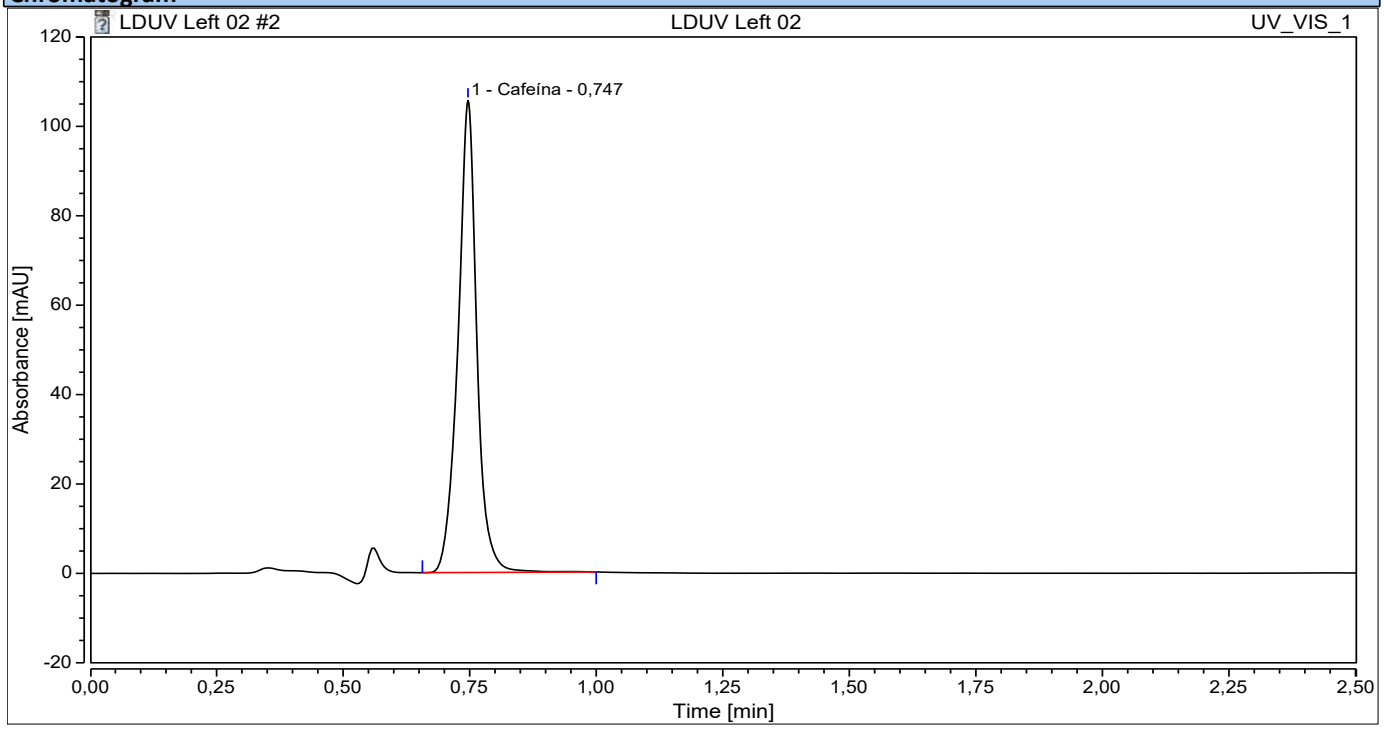

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,747	4,5460	105,595	100,00	100,00	n.a.
Total:			**4,546**	**105,595**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Left 03**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 14:38**	*Sample Weight:*	**1,0000**

Chromatogram

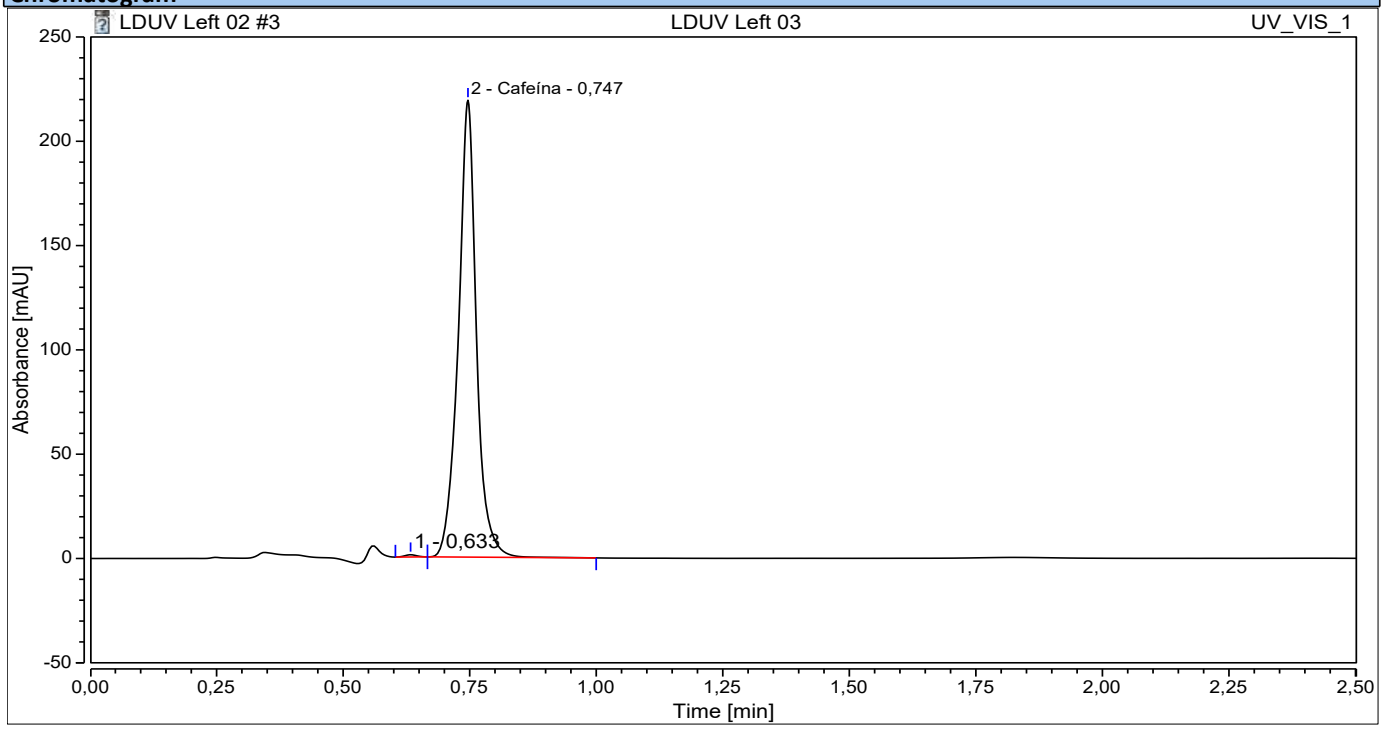

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	Cafeína	0,747	9,0584	219,005	99,68	99,51	n.a.
Total:			**9,058**	**219,005**	**99,684**	**99,506**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Left 04**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 14:41**	*Sample Weight:*	**1,0000**

Chromatogram

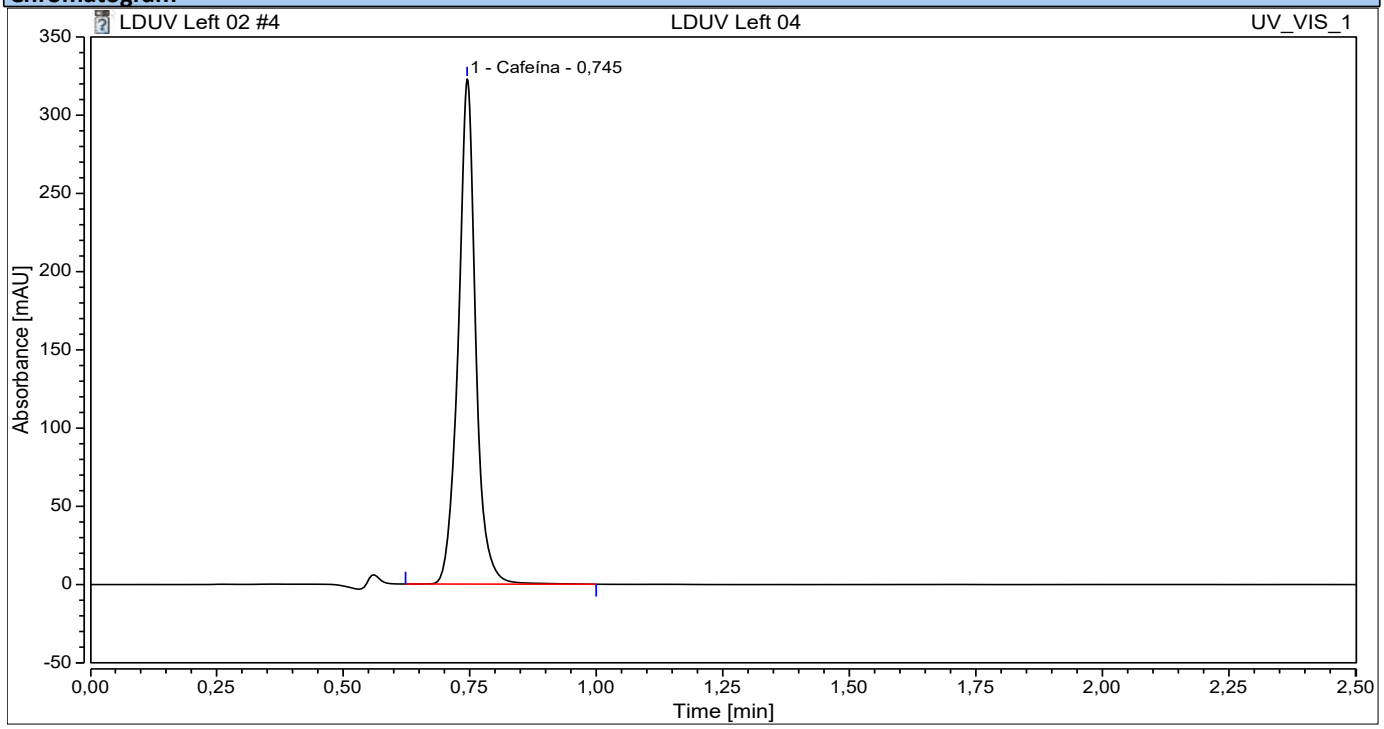

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,745	12,8438	322,801	100,00	100,00	n.a.
Total:			**12,844**	**322,801**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Left 05**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 14:44**	*Sample Weight:*	**1,0000**

Chromatogram

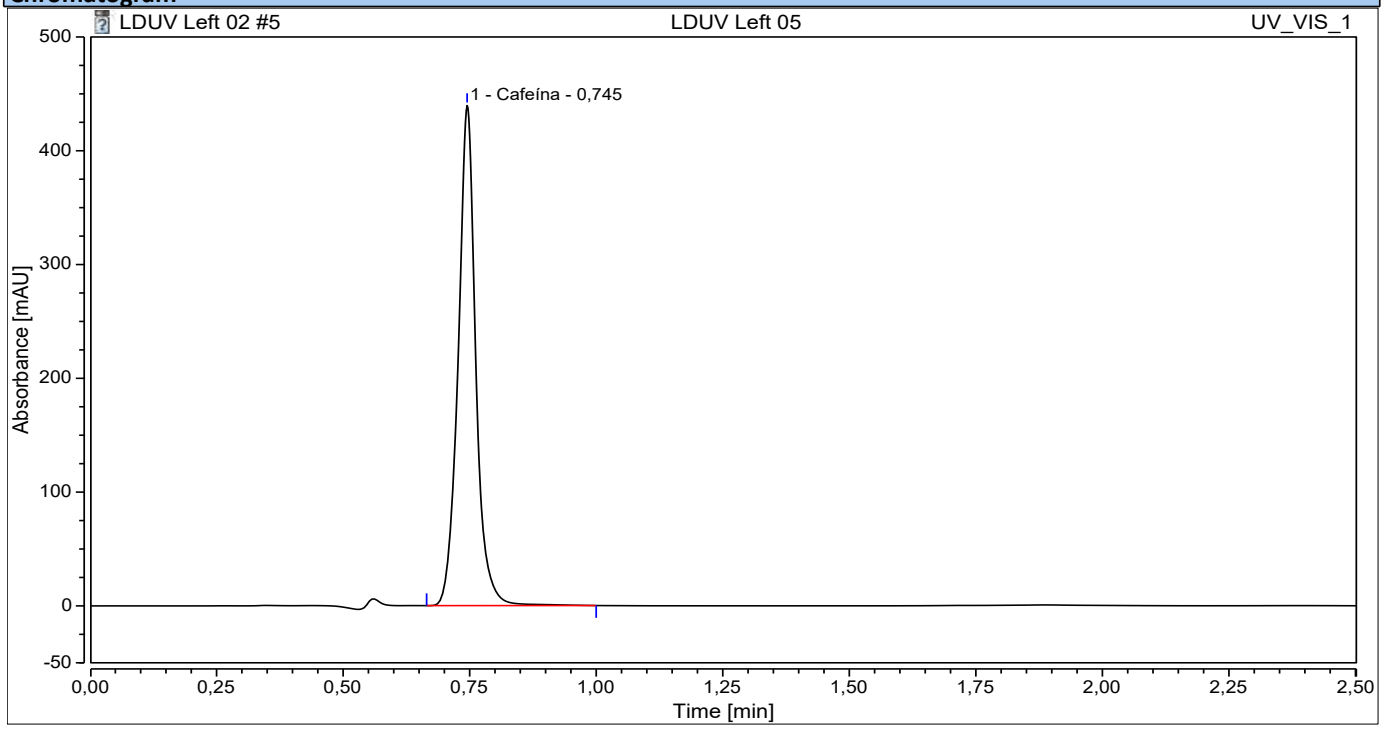

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,745	17,6889	439,487	100,00	100,00	n.a.
Total:			**17,689**	**439,487**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Left 01**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A9**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:01**	*Sample Weight:*	**1,0000**

Chromatogram

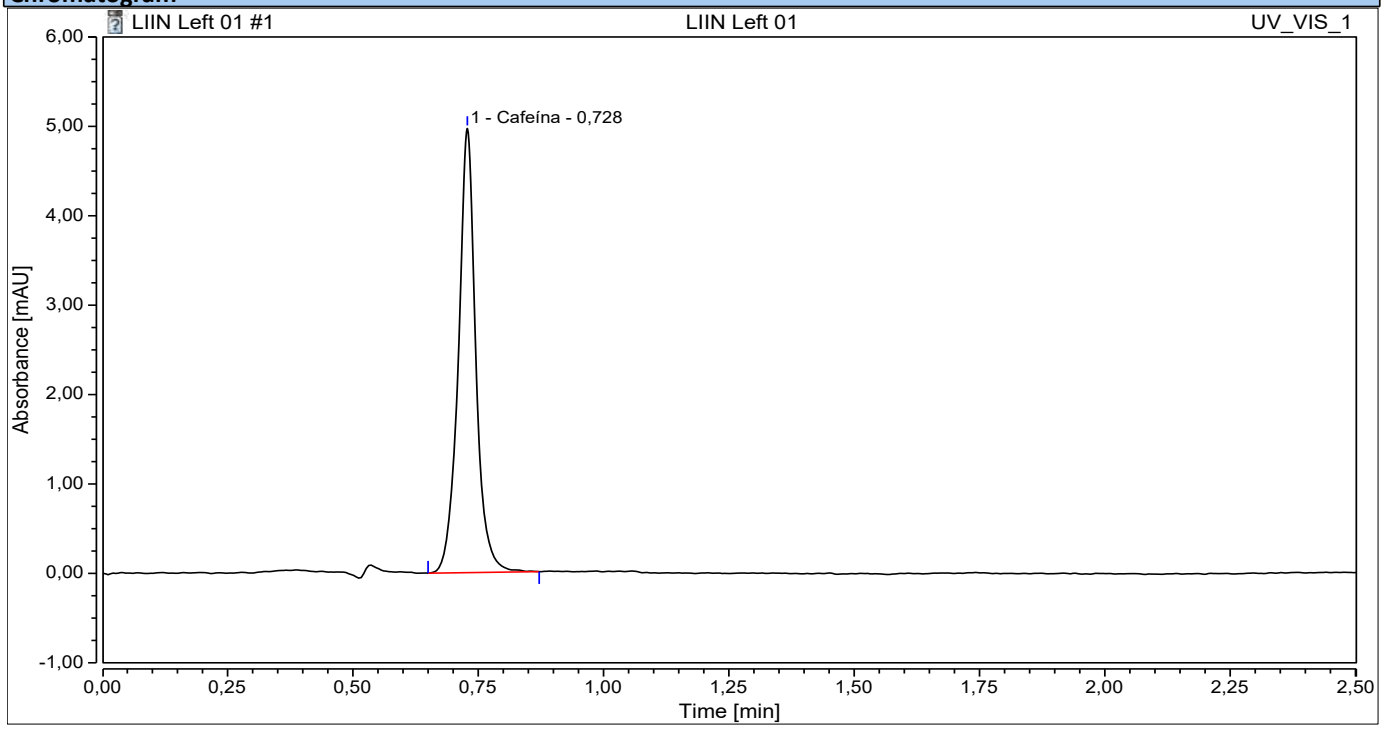

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,728	0,2001	4,968	100,00	100,00	n.a.
Total:			**0,200**	**4,968**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Left 02**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A9**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:04**	*Sample Weight:*	**1,0000**

Chromatogram

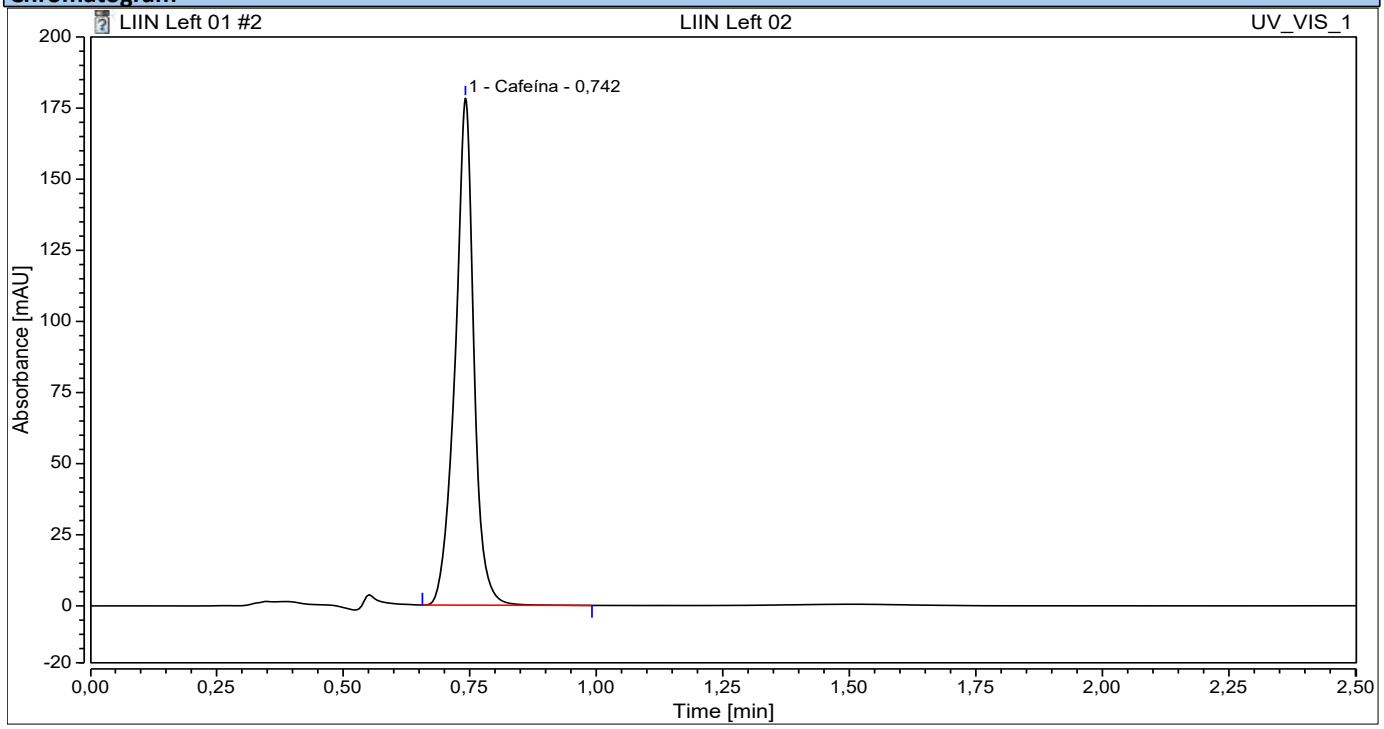

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,742	7,6052	178,209	100,00	100,00	n.a.
Total:			**7,605**	**178,209**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Left 03**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A9**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:07**	*Sample Weight:*	**1,0000**

Chromatogram

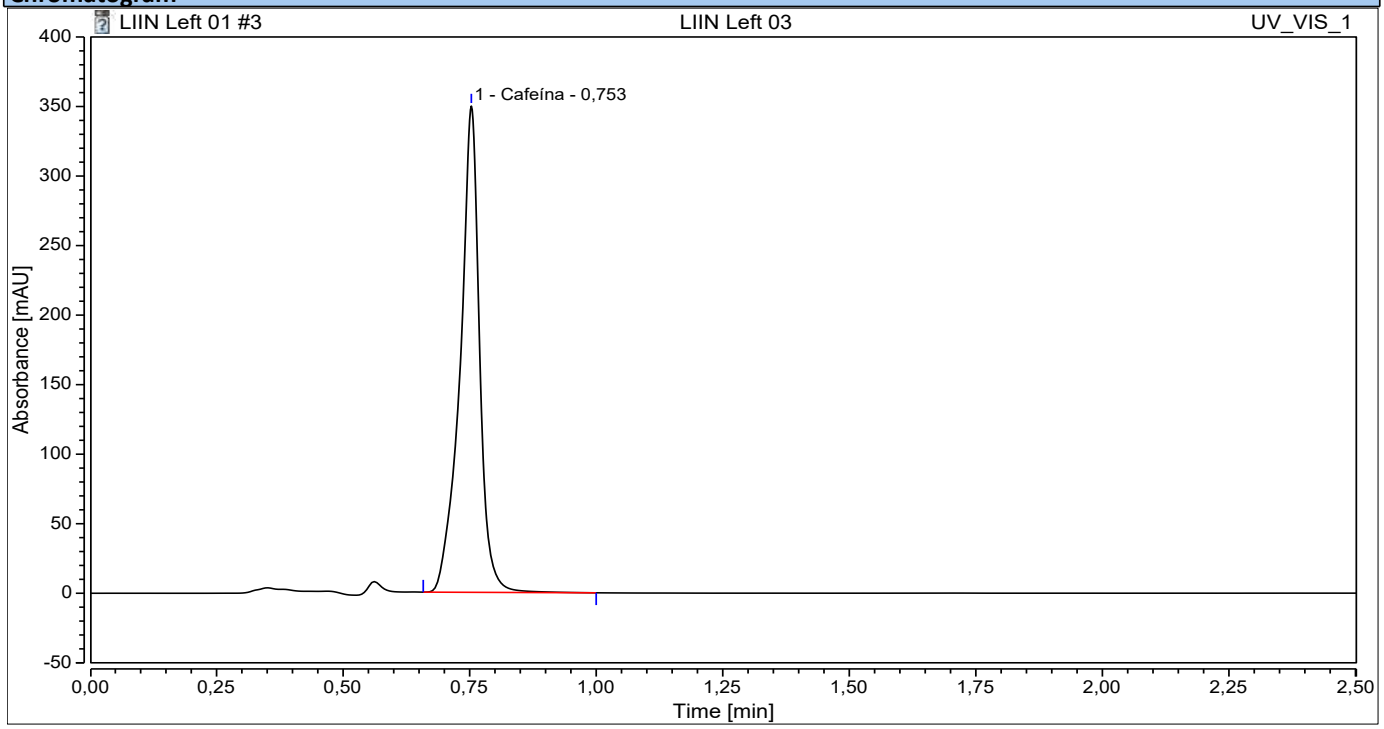

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,753	15,5720	349,645	100,00	100,00	n.a.
Total:			**15,572**	**349,645**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Left 04**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A9**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:10**	*Sample Weight:*	**1,0000**

Chromatogram

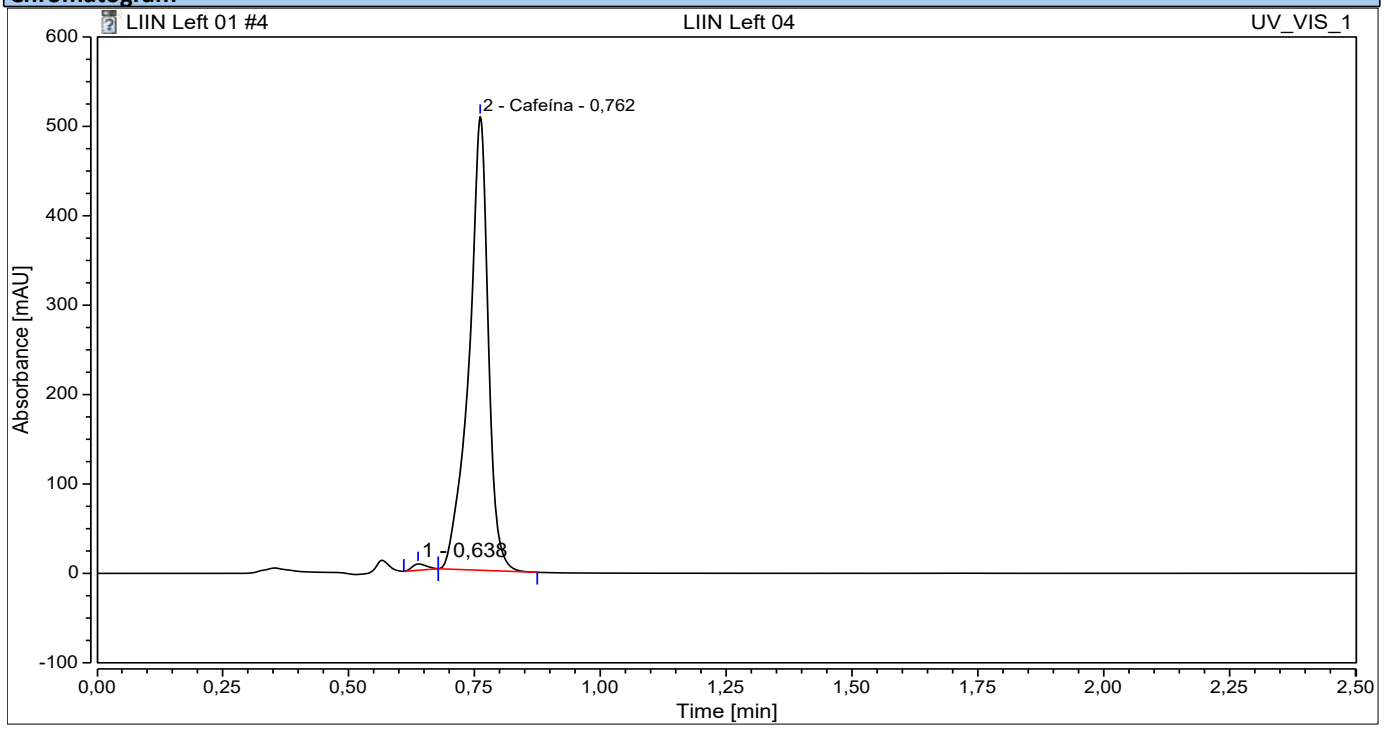

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	Cafeína	0,762	22,4698	507,431	98,98	98,63	n.a.
Total:			**22,470**	**507,431**	**98,978**	**98,626**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Left 05**	*Run Time (min):*	**2,50**
Vial Number:	**Y:A9**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Left**	*Bandwidth:*	**4**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:13**	*Sample Weight:*	**1,0000**

Chromatogram

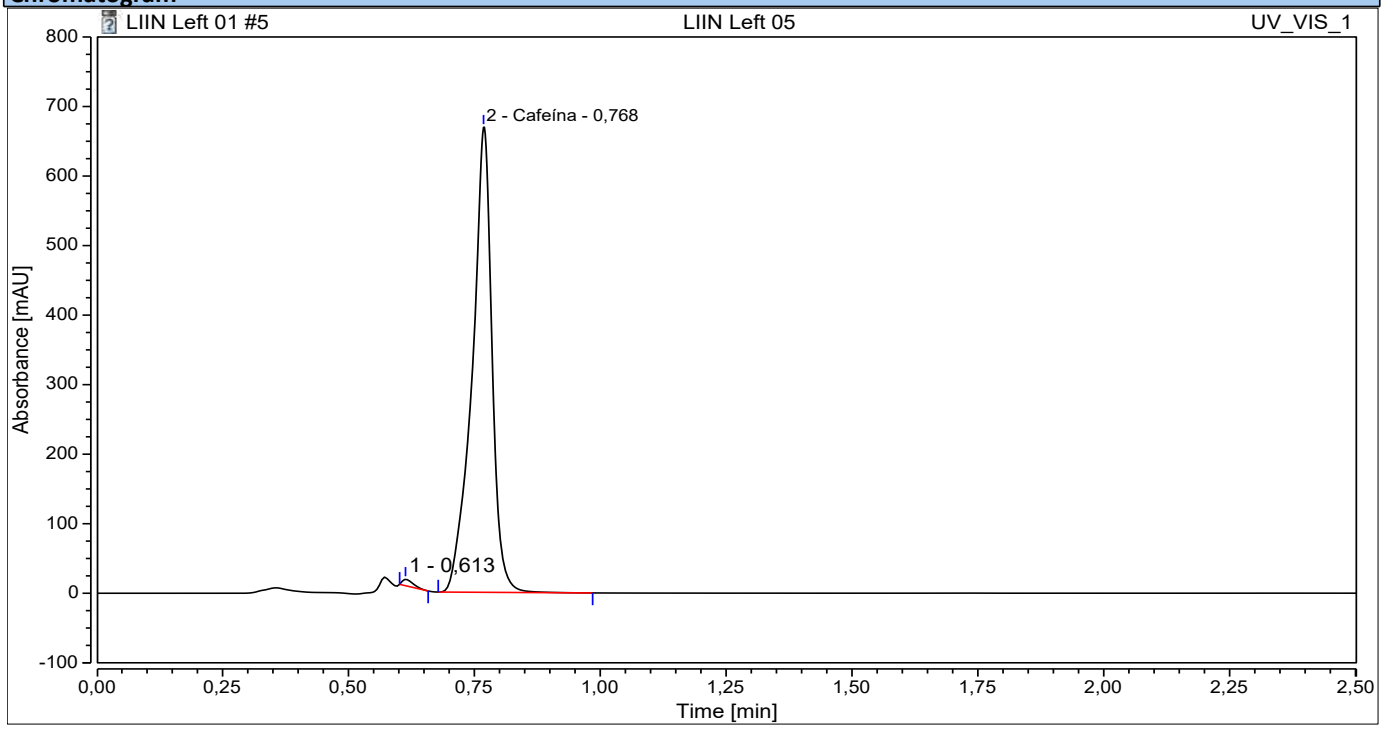

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	Cafeína	0,768	30,4901	668,871	99,25	98,64	n.a.
Total:			**30,490**	**668,871**	**99,246**	**98,643**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB Left**	*Run Time (min):*	**19,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB Left**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 14:26**	*Sample Weight:*	**1,0000**

Chromatogram

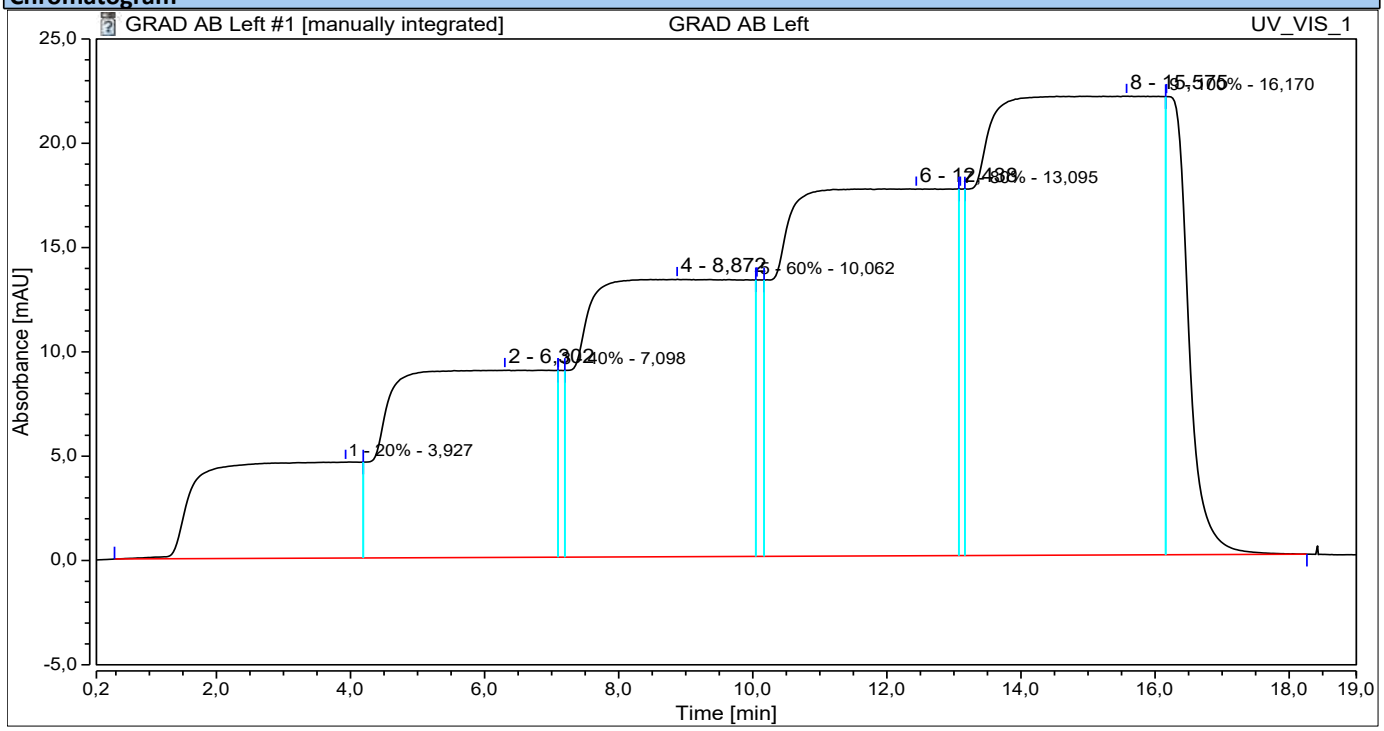

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	20%	3,927	11,9863	4,604	6,02	3,59	n.a.
3	40%	7,098	0,9100	8,960	0,46	6,99	n.a.
5	60%	10,062	1,6345	13,266	0,82	10,34	n.a.
7	80%	13,095	1,5813	17,582	0,79	13,71	n.a.
9	100%	16,170	8,3071	21,981	4,17	17,14	n.a.
Total:			**24,419**	**66,394**	**12,263**	**51,766**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AC Left**	*Run Time (min):*	**19,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,01**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AC Left**	*Bandwidth:*	**4**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 14:52**	*Sample Weight:*	**1,0000**

Chromatogram

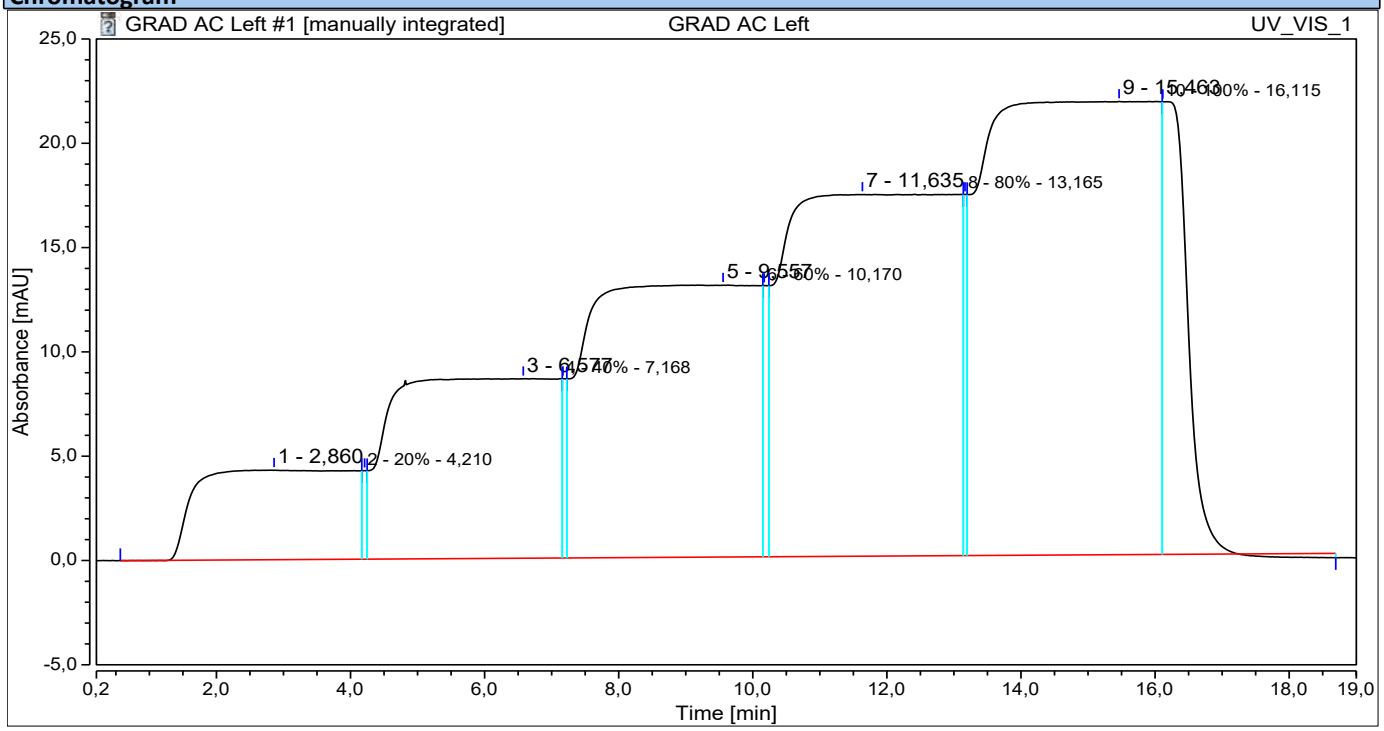

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,210	0,3393	4,246	0,17	3,27	n.a.
4	40%	7,168	0,5869	8,596	0,30	6,62	n.a.
6	60%	10,170	1,1701	13,007	0,60	10,01	n.a.
8	80%	13,165	0,9807	17,314	0,50	13,33	n.a.
10	100%	16,115	8,8921	21,706	4,58	16,71	n.a.
Total:			**11,969**	**64,869**	**6,160**	**49,944**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.