


204,24
272,99
nm
mAU
200
210
220
230
240
250
260
270
280
290
300
-50
0
50
100
150
200
250
300
350
400

Contour Spectral View

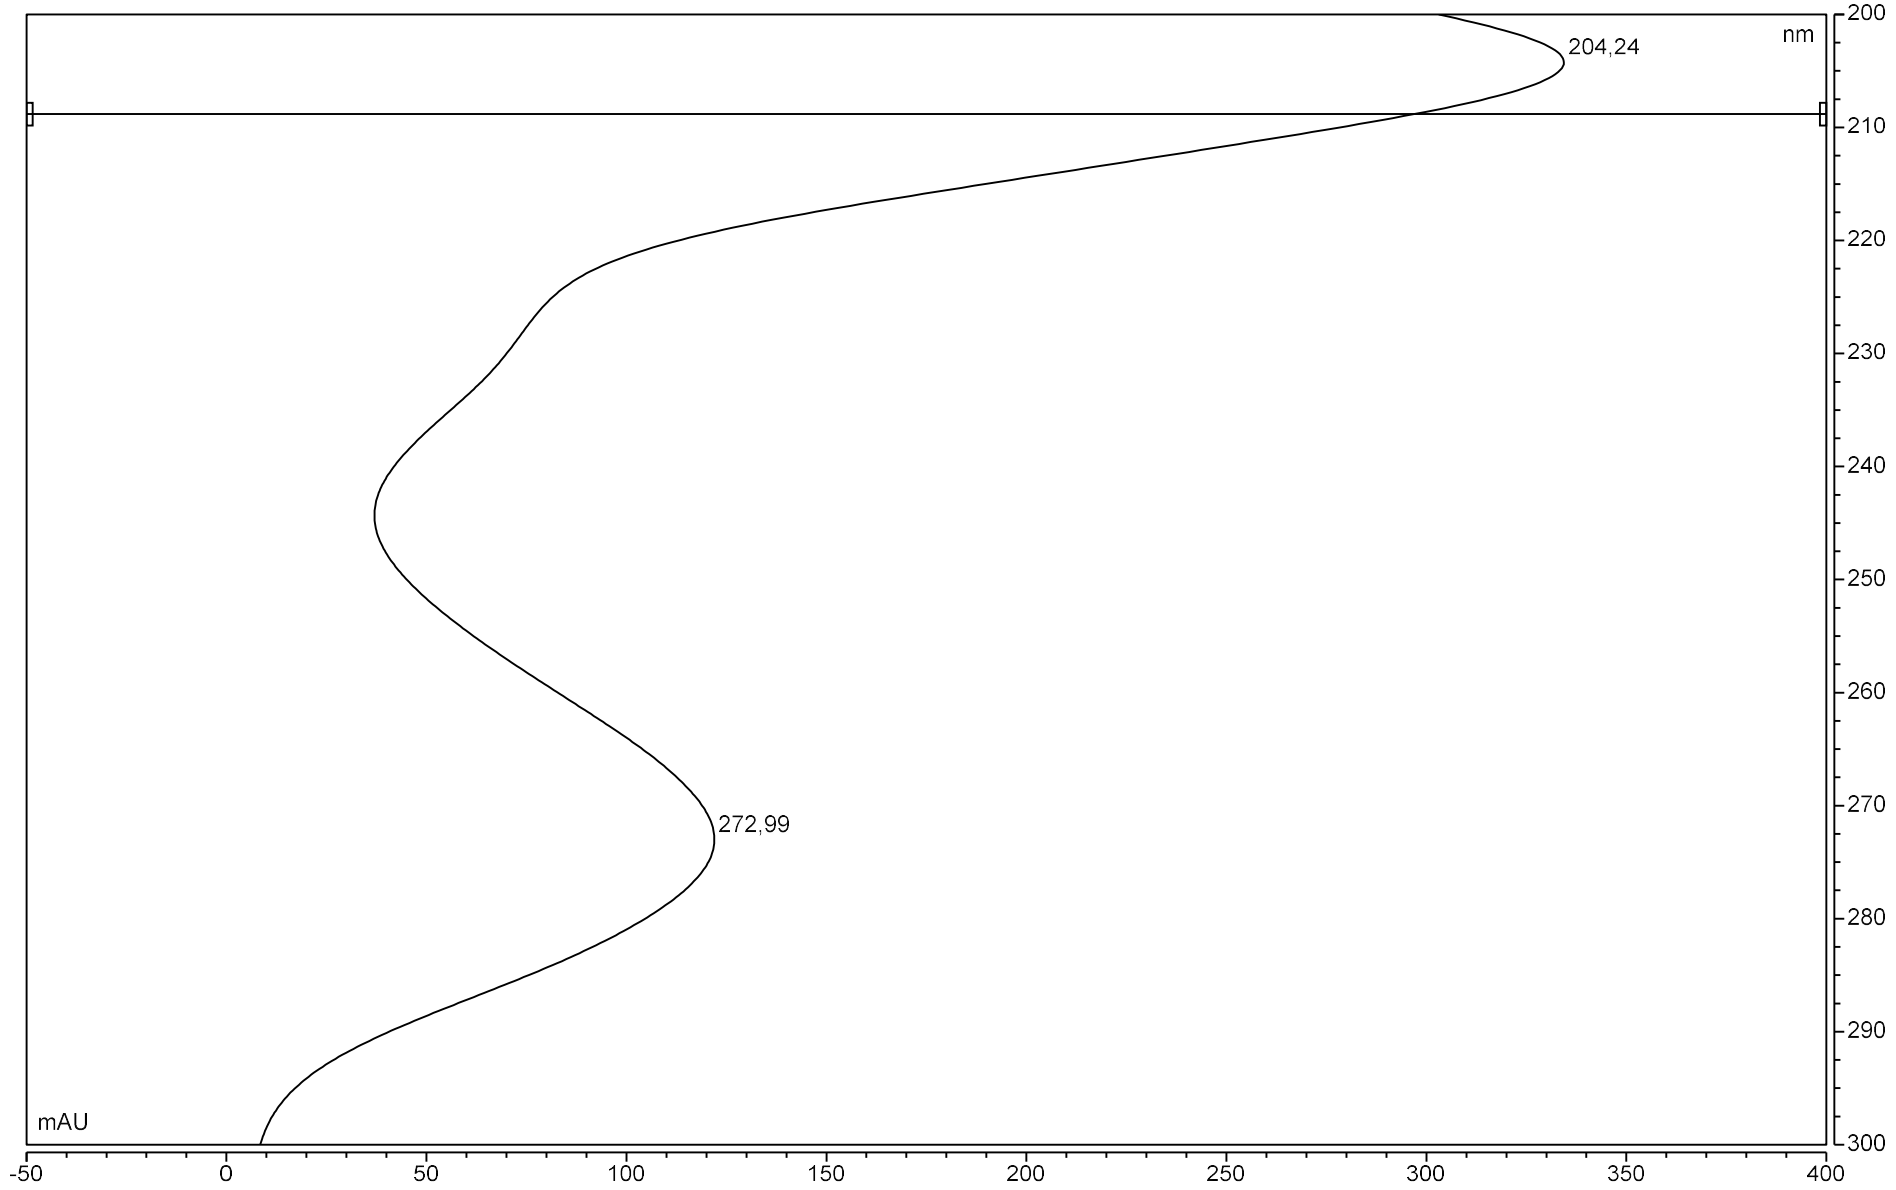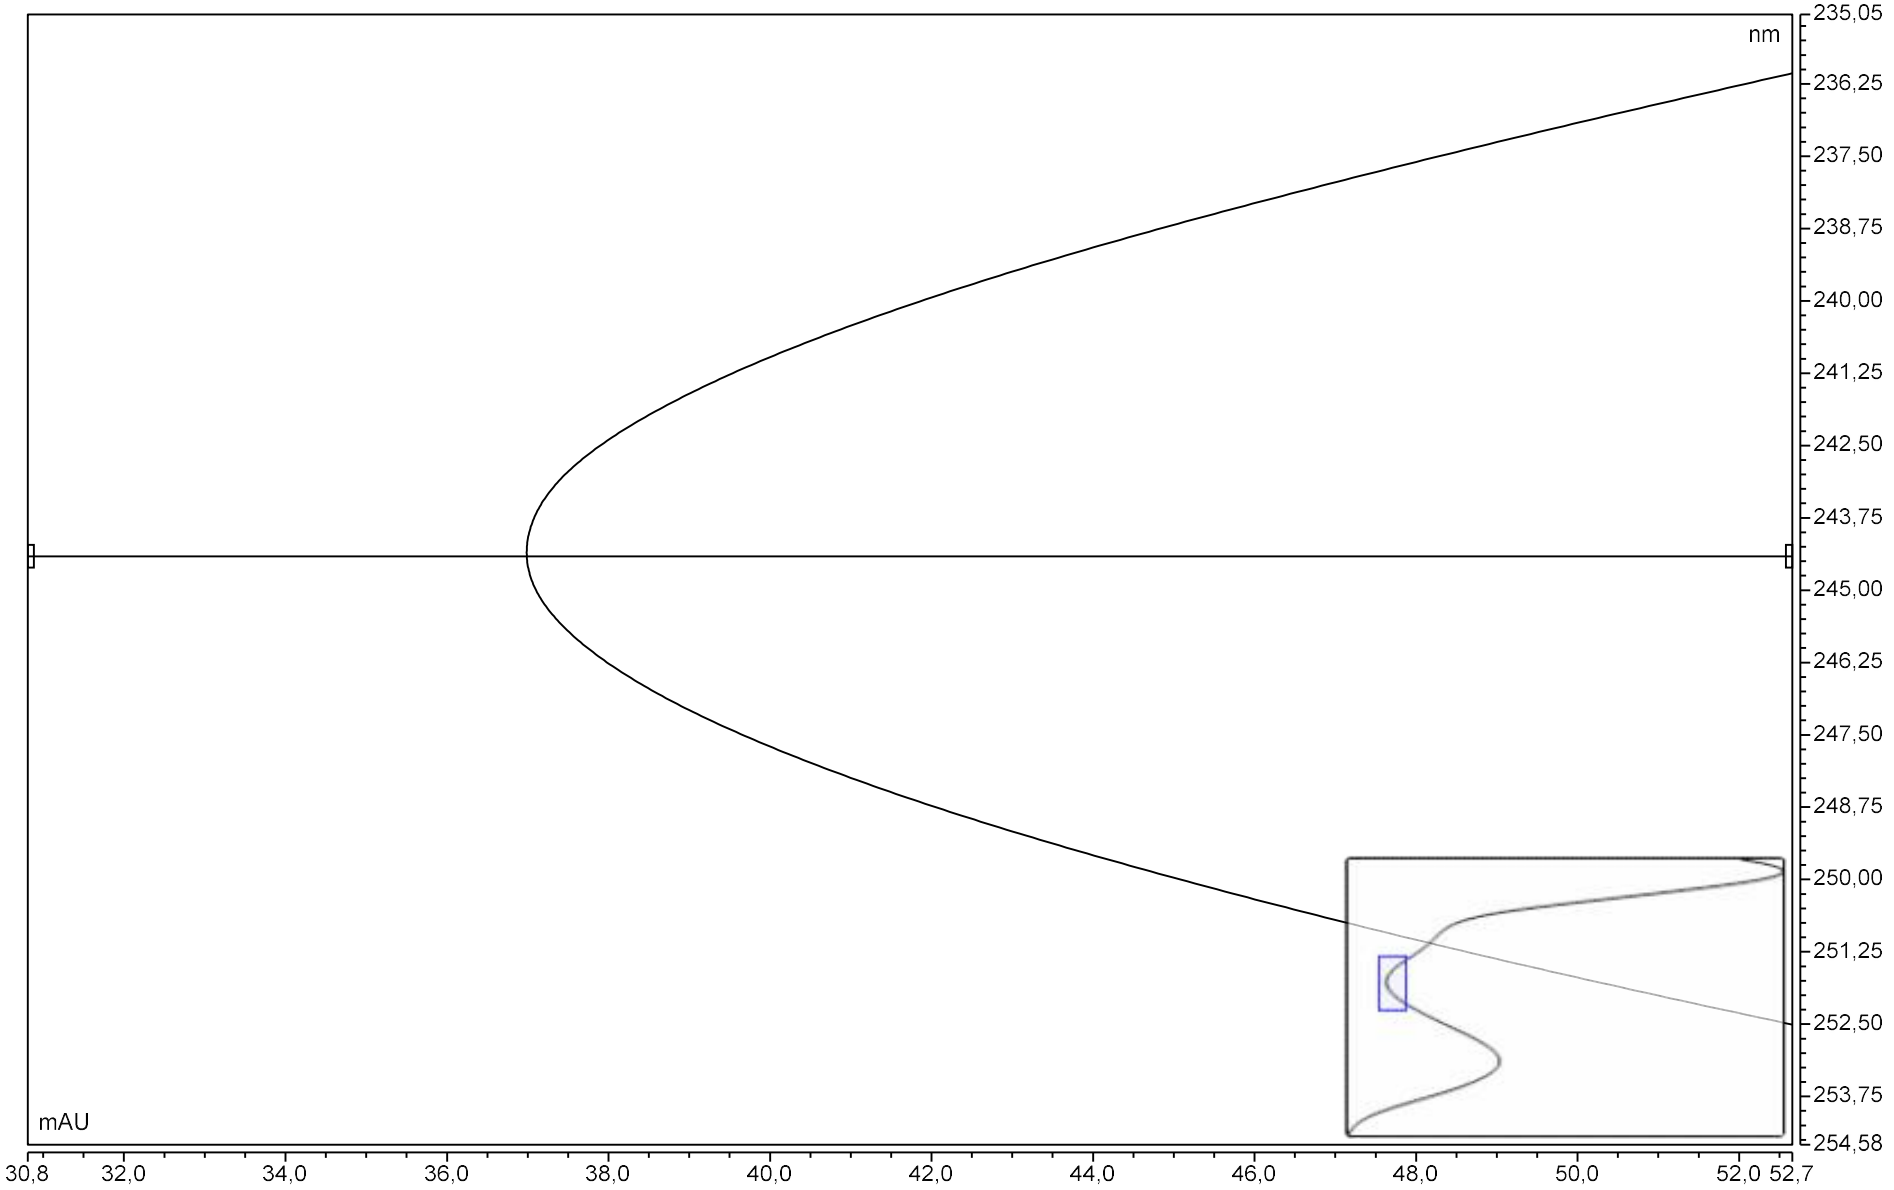


Chromatogram and Results

Injection Details

Injection Name:	**RELB Right 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:43**	*Sample Weight:*	**1,0000**

Chromatogram

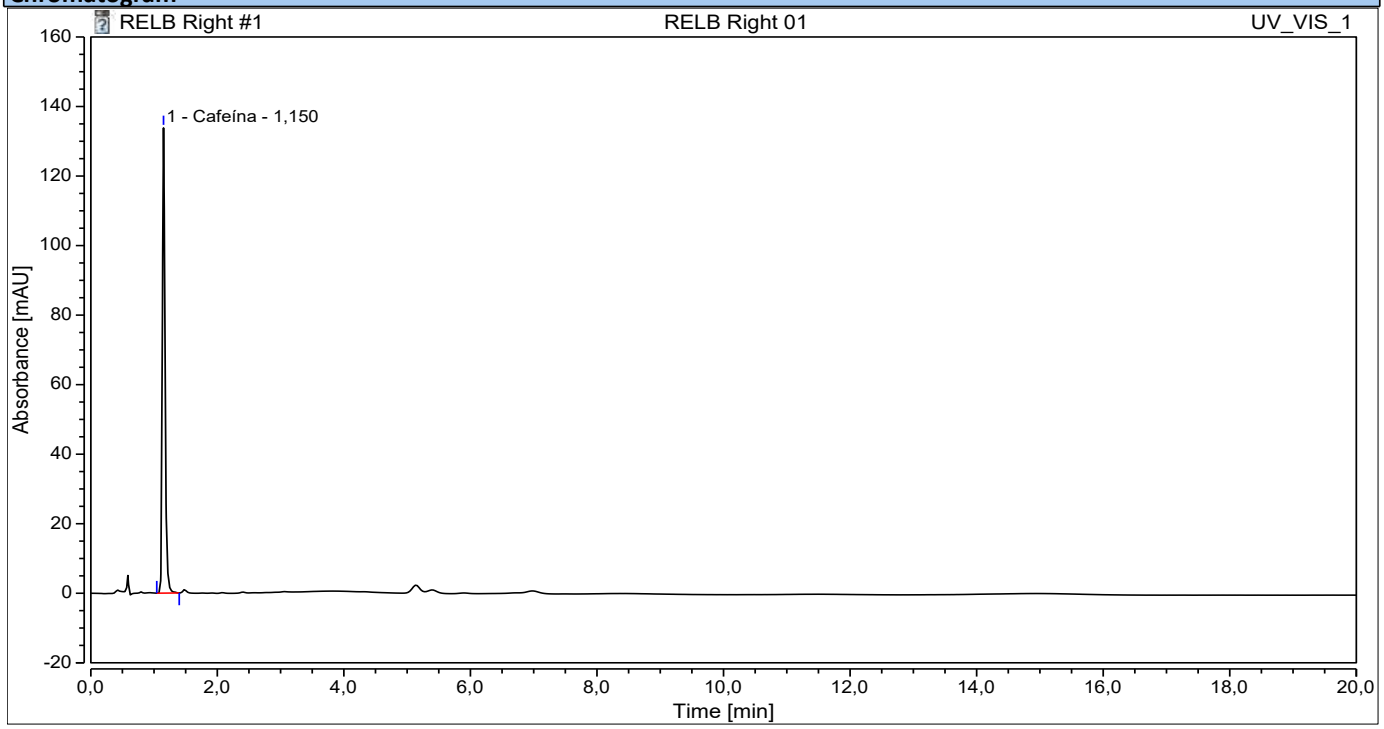

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,150	6,5111	133,803	100,00	100,00	n.a.
Total:			**6,511**	**133,803**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:43**	*Sample Weight:*	**1,0000**

Chromatogram

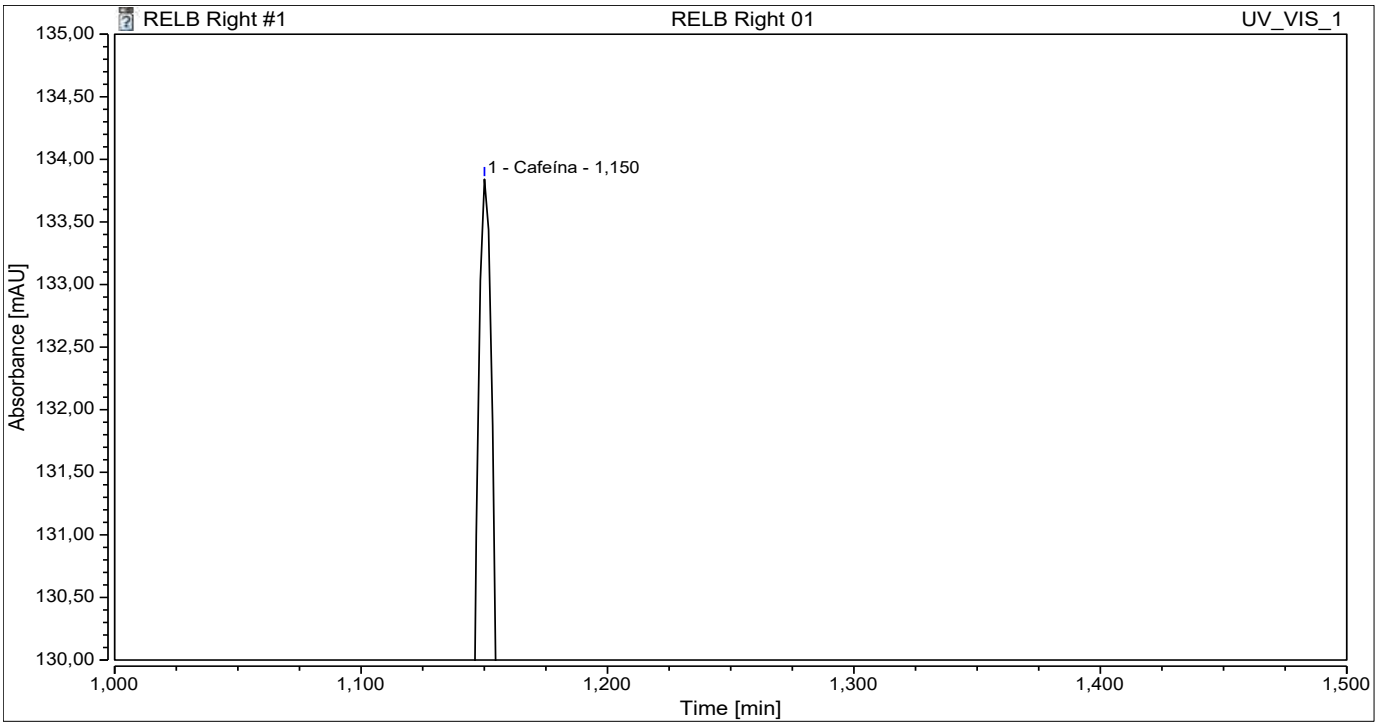

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,150	6,5111	133,803	100,00	100,00	n.a.
Total:			**6,511**	**133,803**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:43**	*Sample Weight:*	**1,0000**

Chromatogram

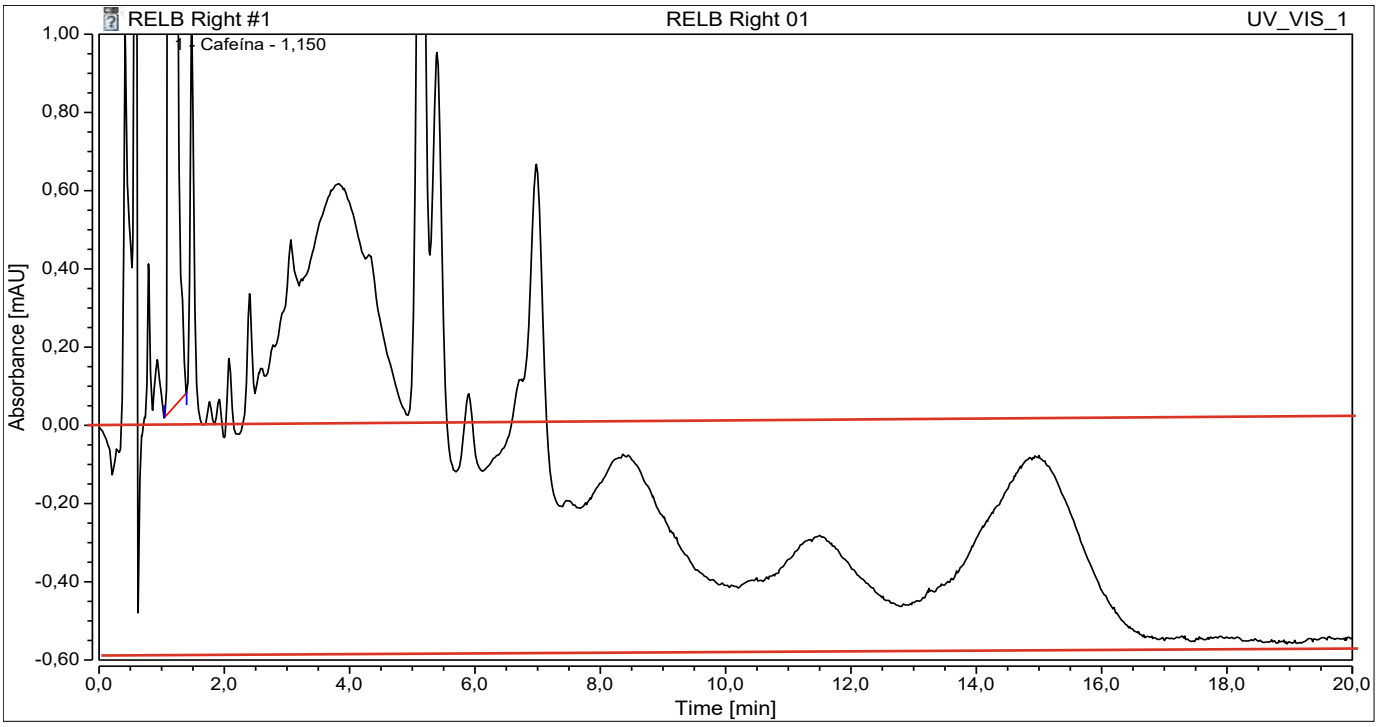

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,150	6,5111	133,803	100,00	100,00	n.a.
Total:			**6,511**	**133,803**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**RELB Right 01**	*Run Time (min):*	**20,00**
Vial Number:	**Y:B1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**250**
Instrument Method:	**RELB HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 15:43**	*Sample Weight:*	**1,0000**

Chromatogram

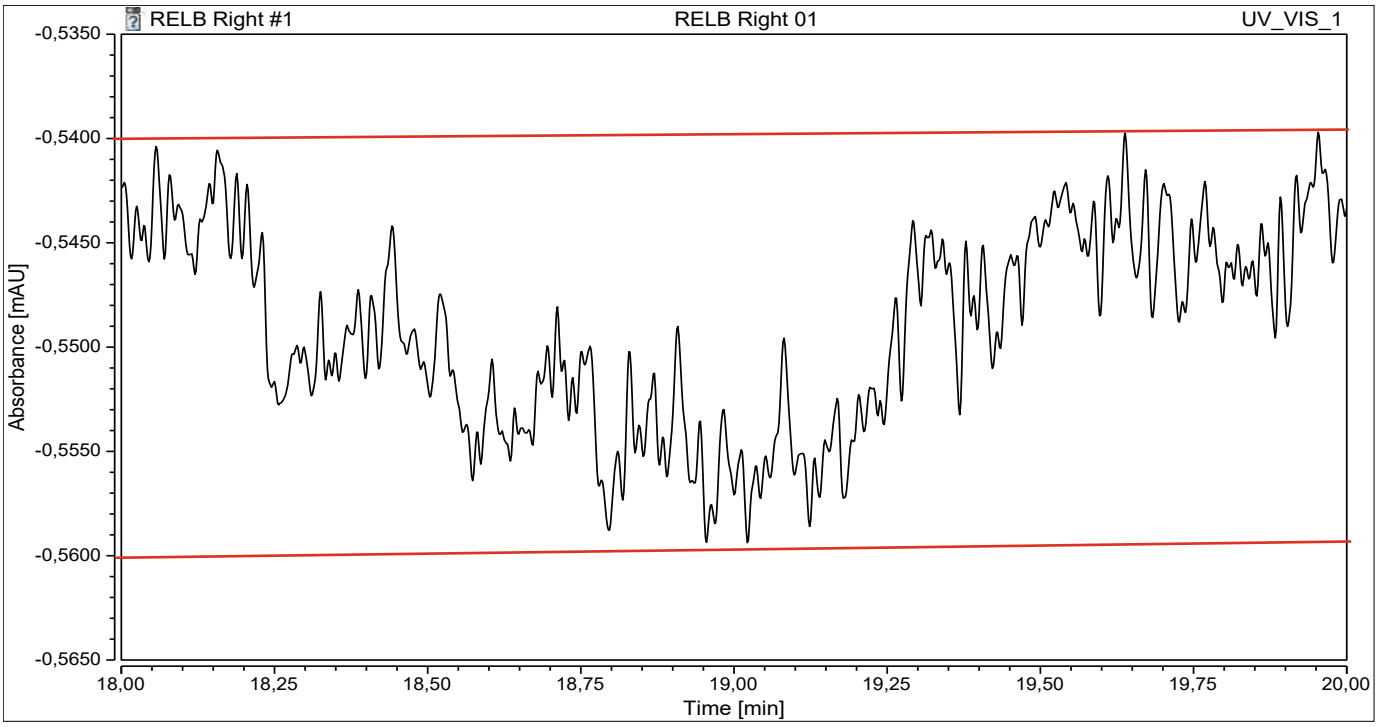

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	1,150	6,5111	133,803	100,00	100,00	n.a.
Total:			**6,511**	**133,803**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Right 01**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:44**	*Sample Weight:*	**1,0000**

Chromatogram

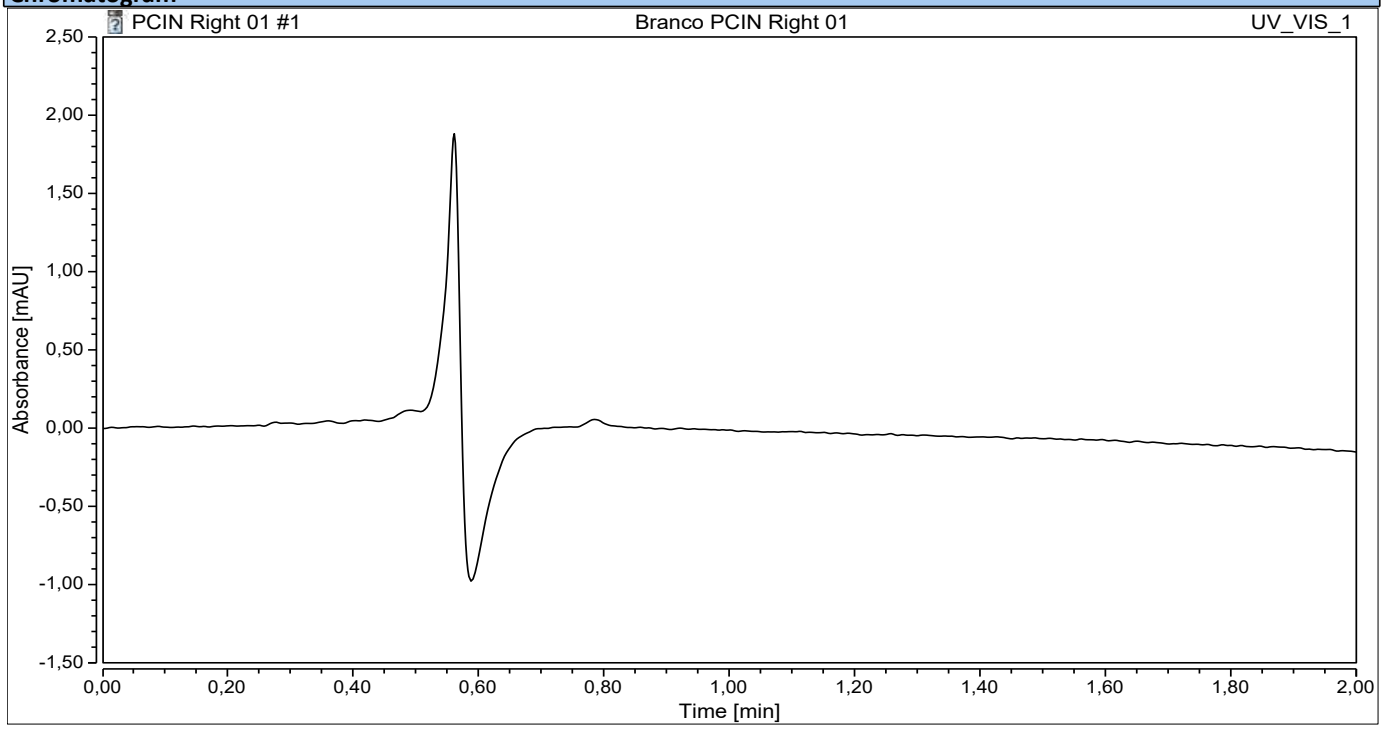

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 01**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:47**	*Sample Weight:*	**1,0000**

Chromatogram

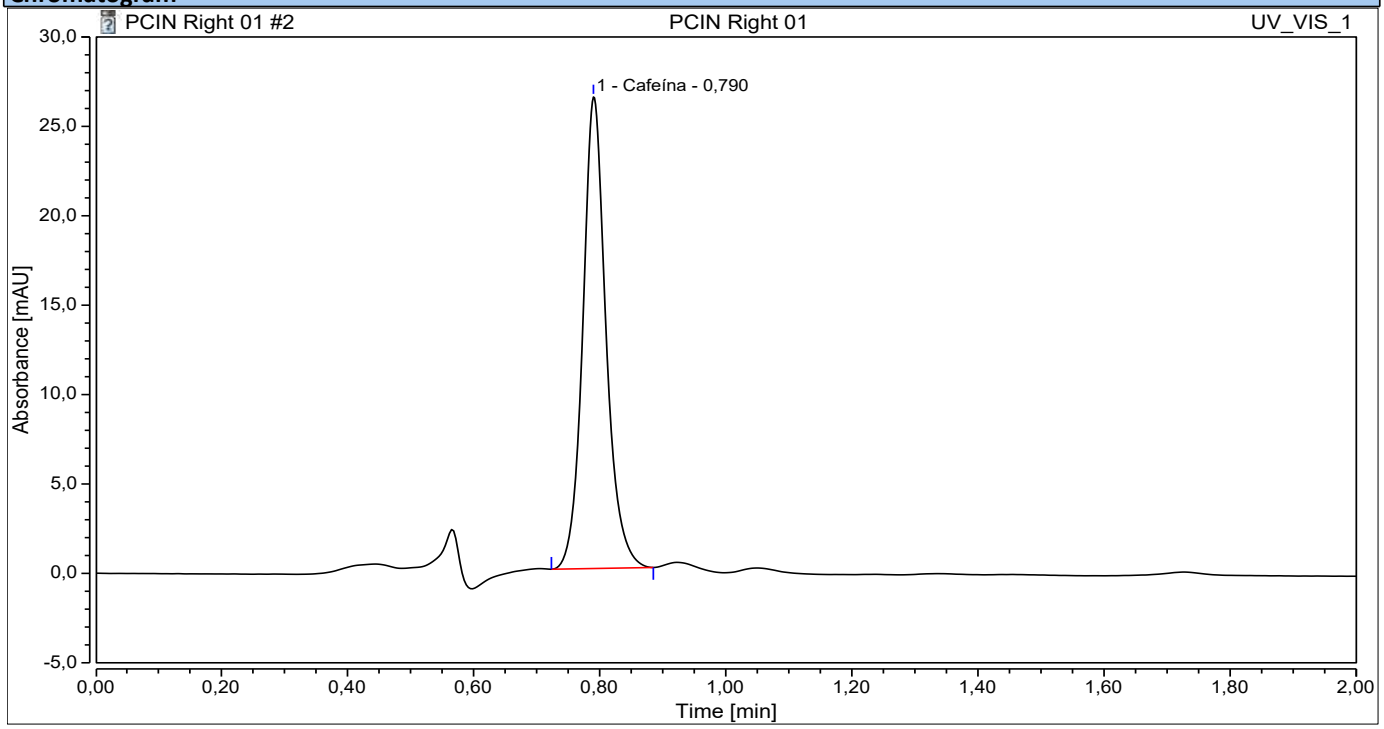

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	1,1236	26,374	100,00	100,00	n.a.
Total:			**1,124**	**26,374**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 02**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:49**	*Sample Weight:*	**1,0000**

Chromatogram

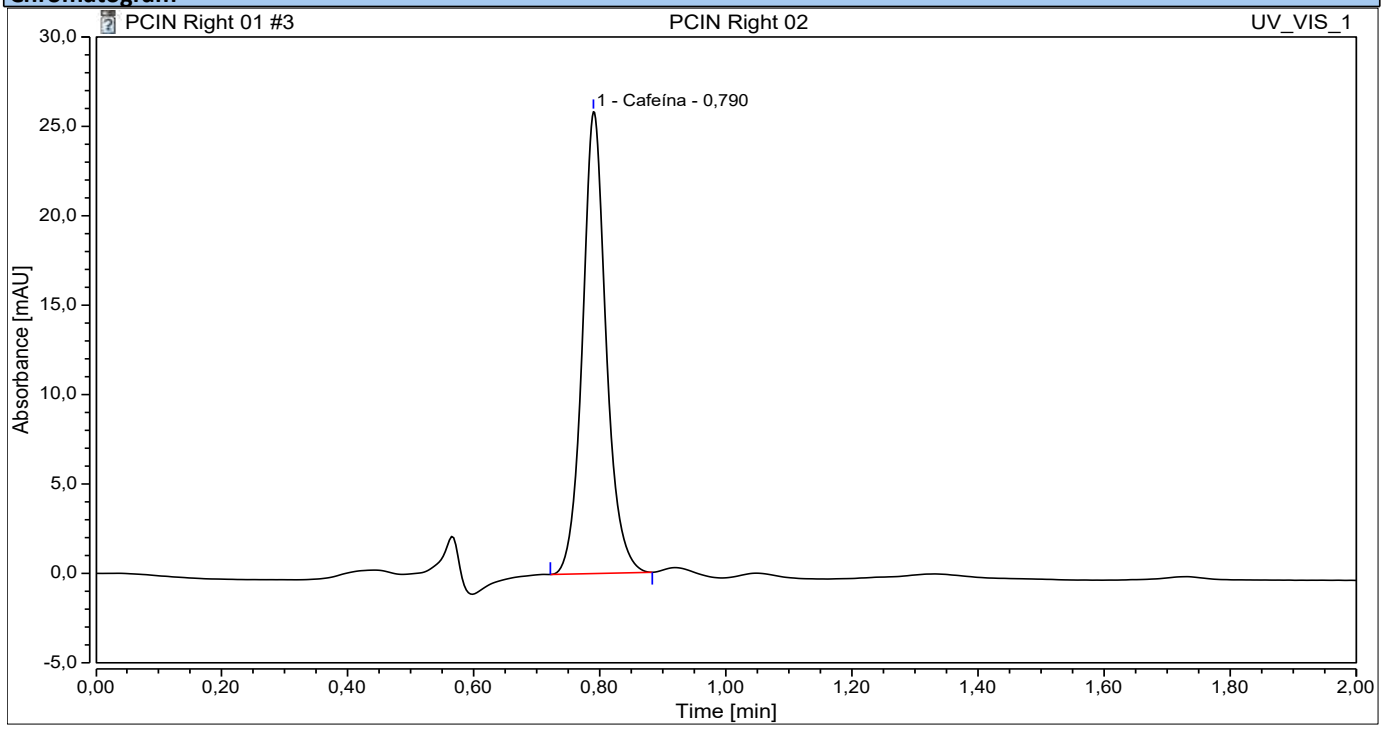

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	1,1197	25,831	100,00	100,00	n.a.
Total:			**1,120**	**25,831**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 03**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:52**	*Sample Weight:*	**1,0000**

Chromatogram

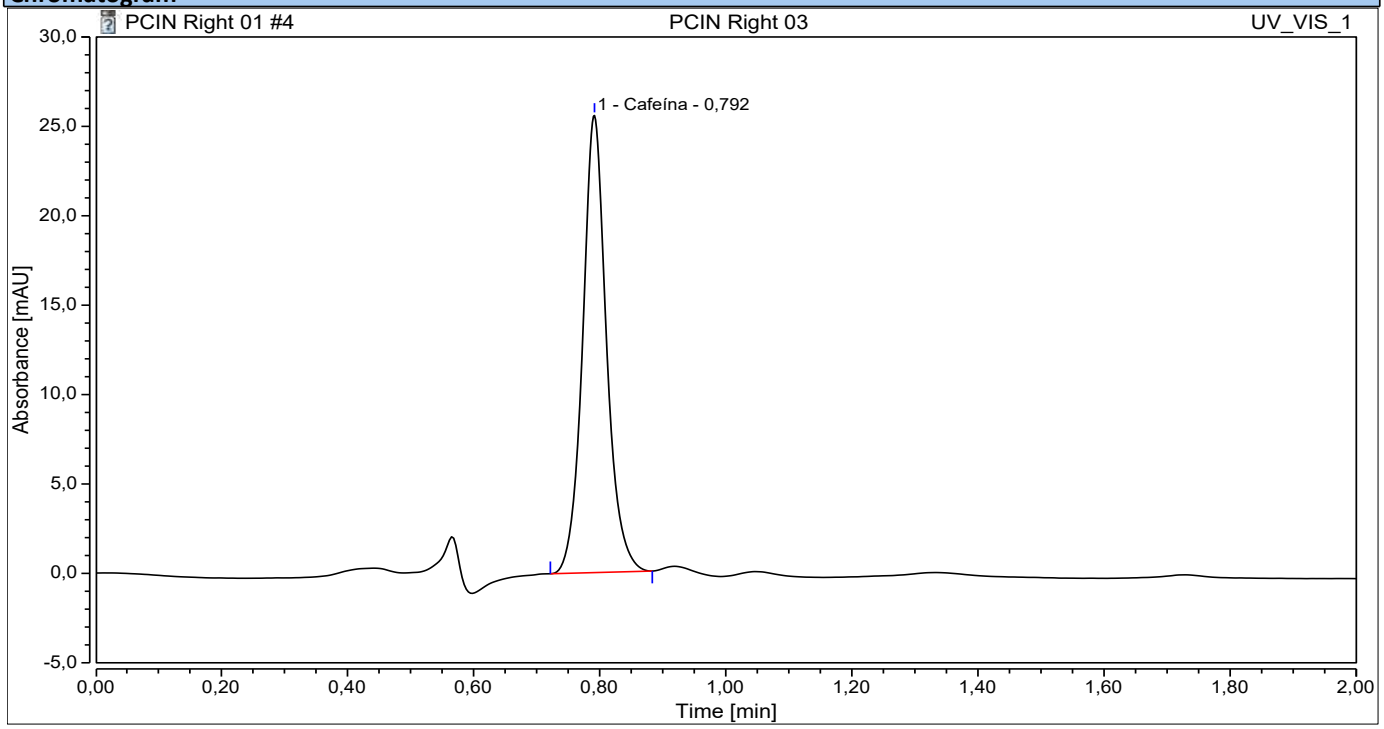

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,792	1,1167	25,567	100,00	100,00	n.a.
Total:			**1,117**	**25,567**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Right 02**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:54**	*Sample Weight:*	**1,0000**

Chromatogram

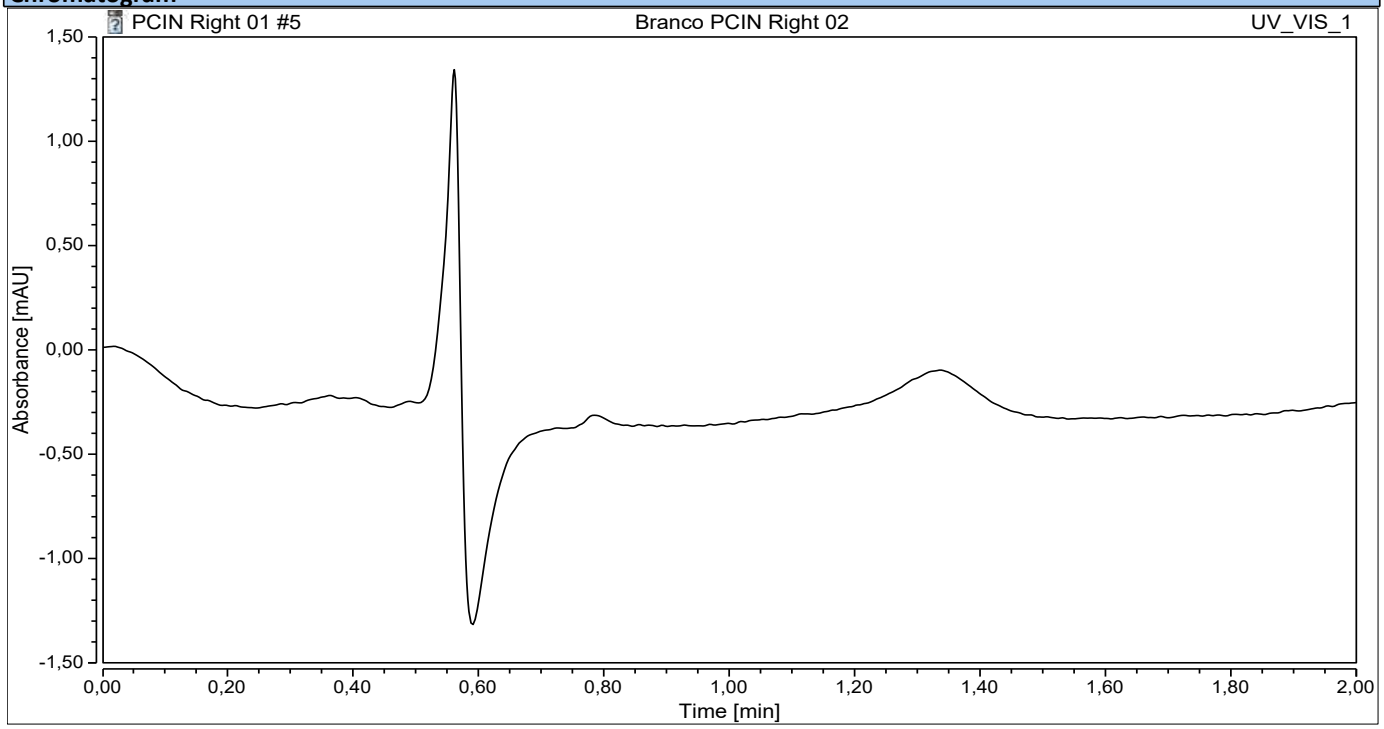

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 04**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:57**	*Sample Weight:*	**1,0000**

Chromatogram

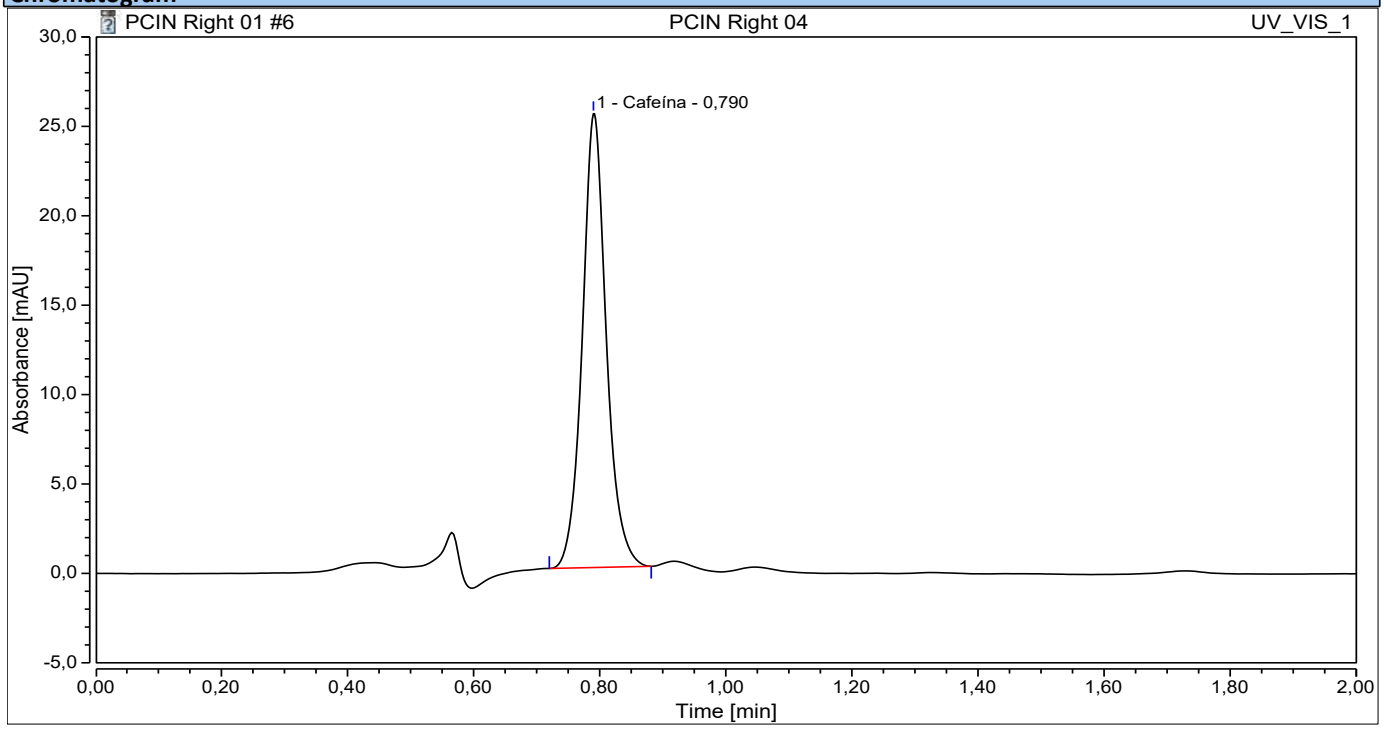

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	1,1166	25,385	100,00	100,00	n.a.
Total:			**1,117**	**25,385**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 05**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 16:59**	*Sample Weight:*	**1,0000**

Chromatogram

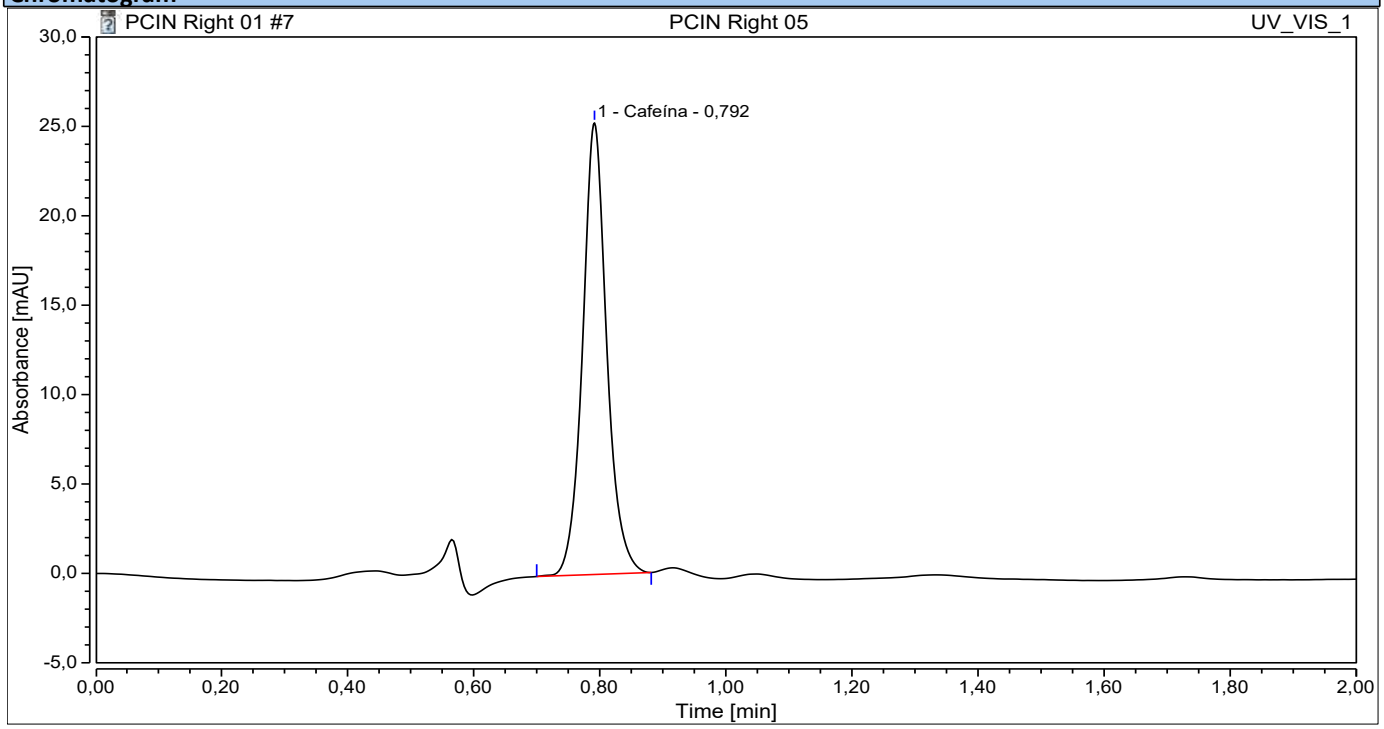

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,792	1,1196	25,258	100,00	100,00	n.a.
Total:			**1,120**	**25,258**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**PCIN Right 06**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:02**	*Sample Weight:*	**1,0000**

Chromatogram

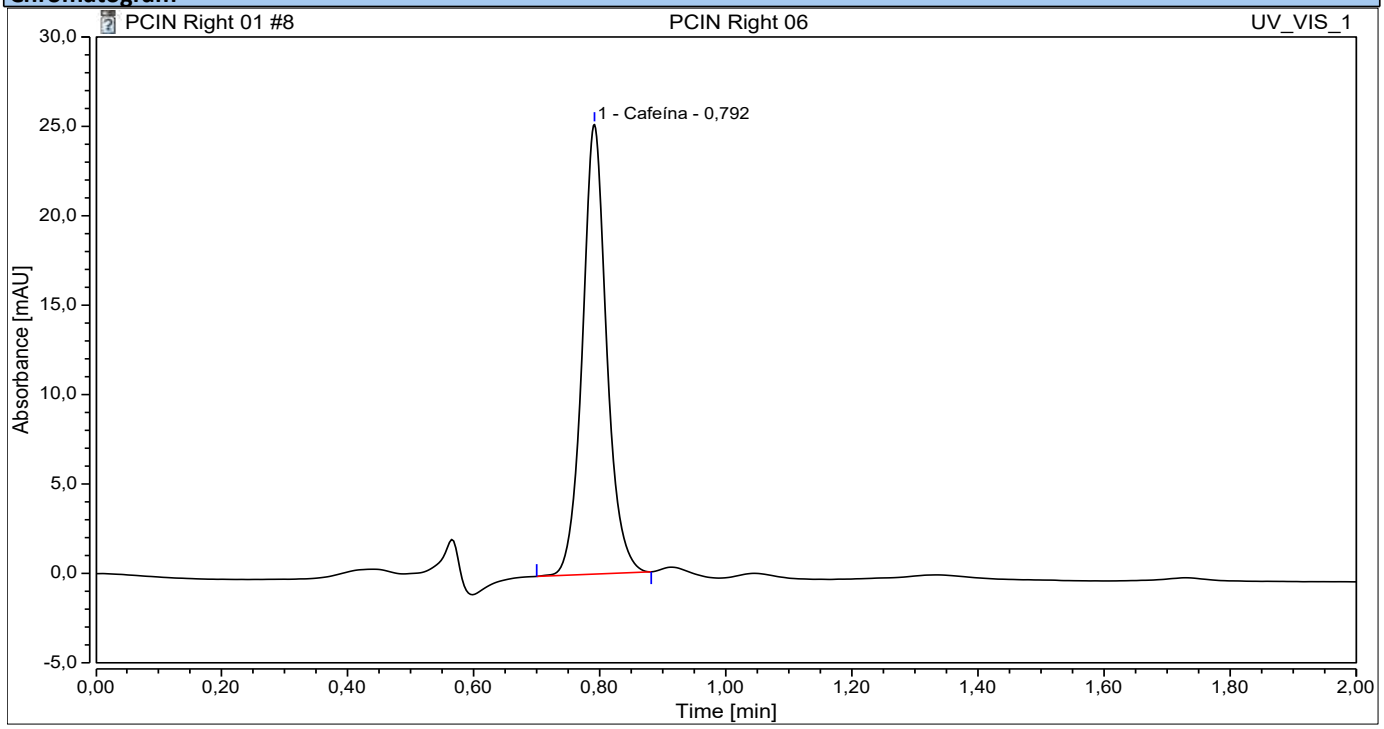

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,792	1,1184	25,149	100,00	100,00	n.a.
Total:			**1,118**	**25,149**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN Right 03**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:04**	*Sample Weight:*	**1,0000**

Chromatogram

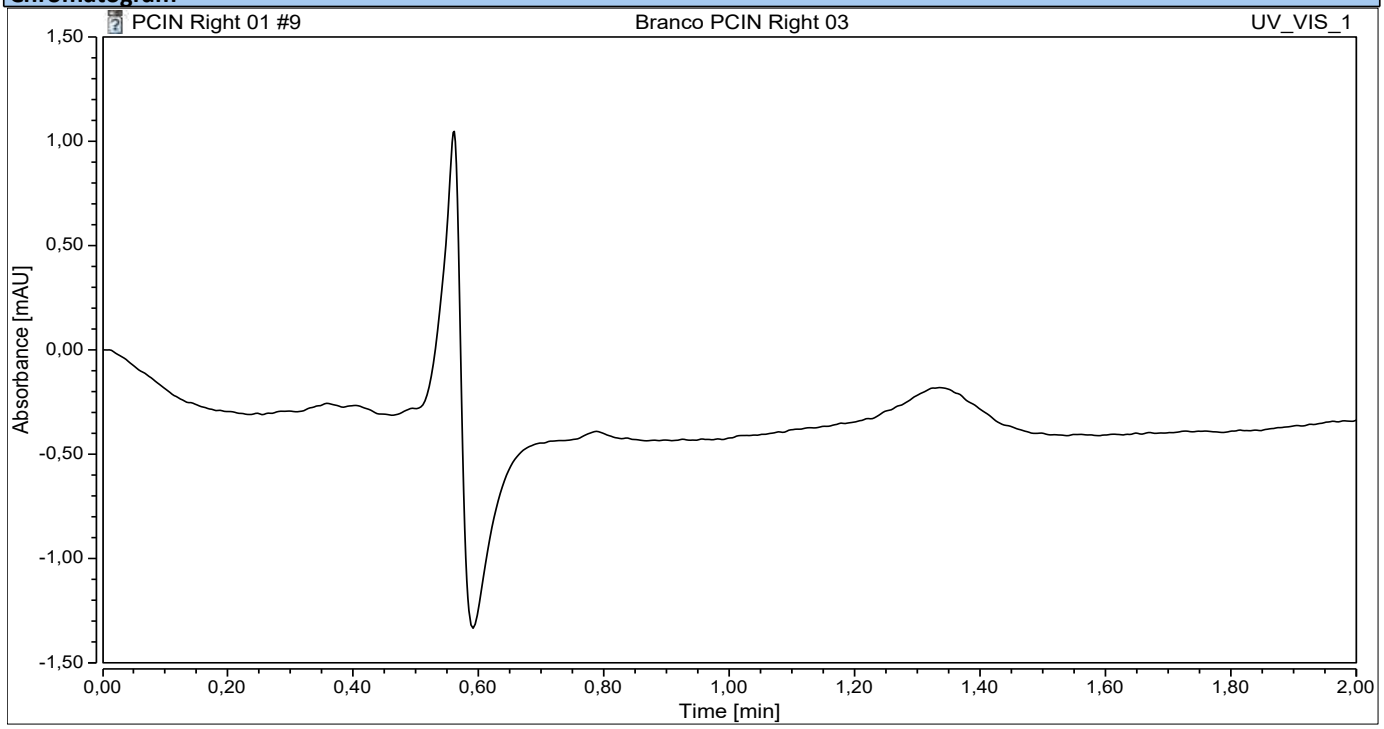

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,000**	**0,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 01**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:07**	*Sample Weight:*	**1,0000**

Chromatogram

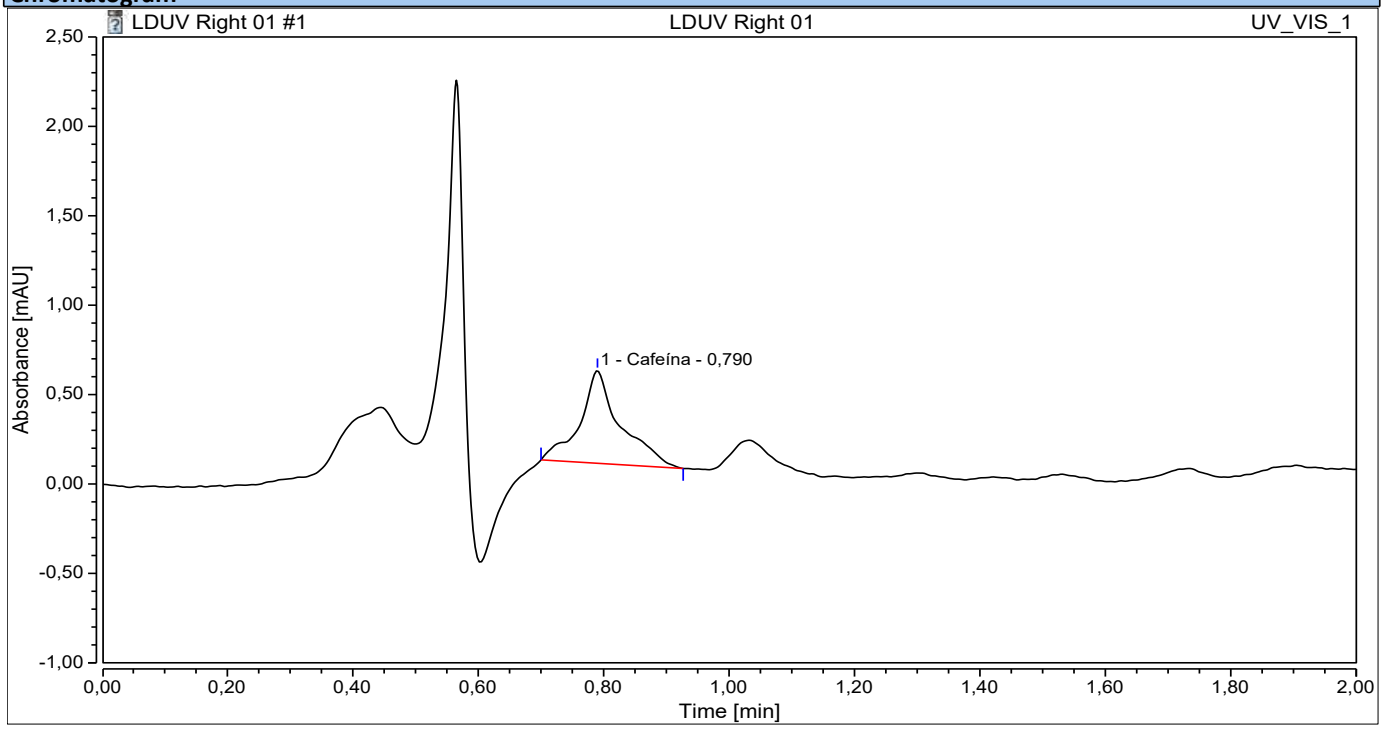

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	0,0386	0,518	100,00	100,00	n.a.
Total:			**0,039**	**0,518**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 02**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:09**	*Sample Weight:*	**1,0000**

Chromatogram

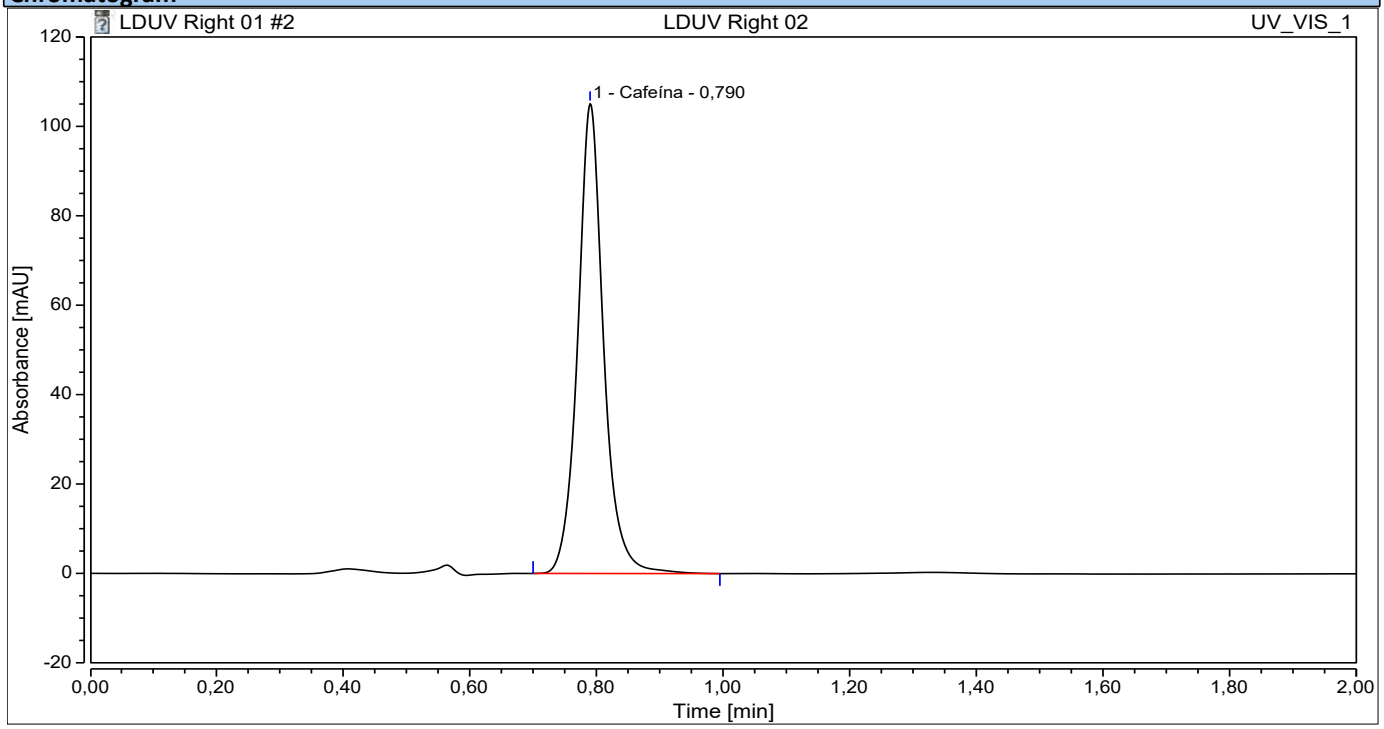

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	4,9663	105,105	100,00	100,00	n.a.
Total:			**4,966**	**105,105**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 03**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:12**	*Sample Weight:*	**1,0000**

Chromatogram

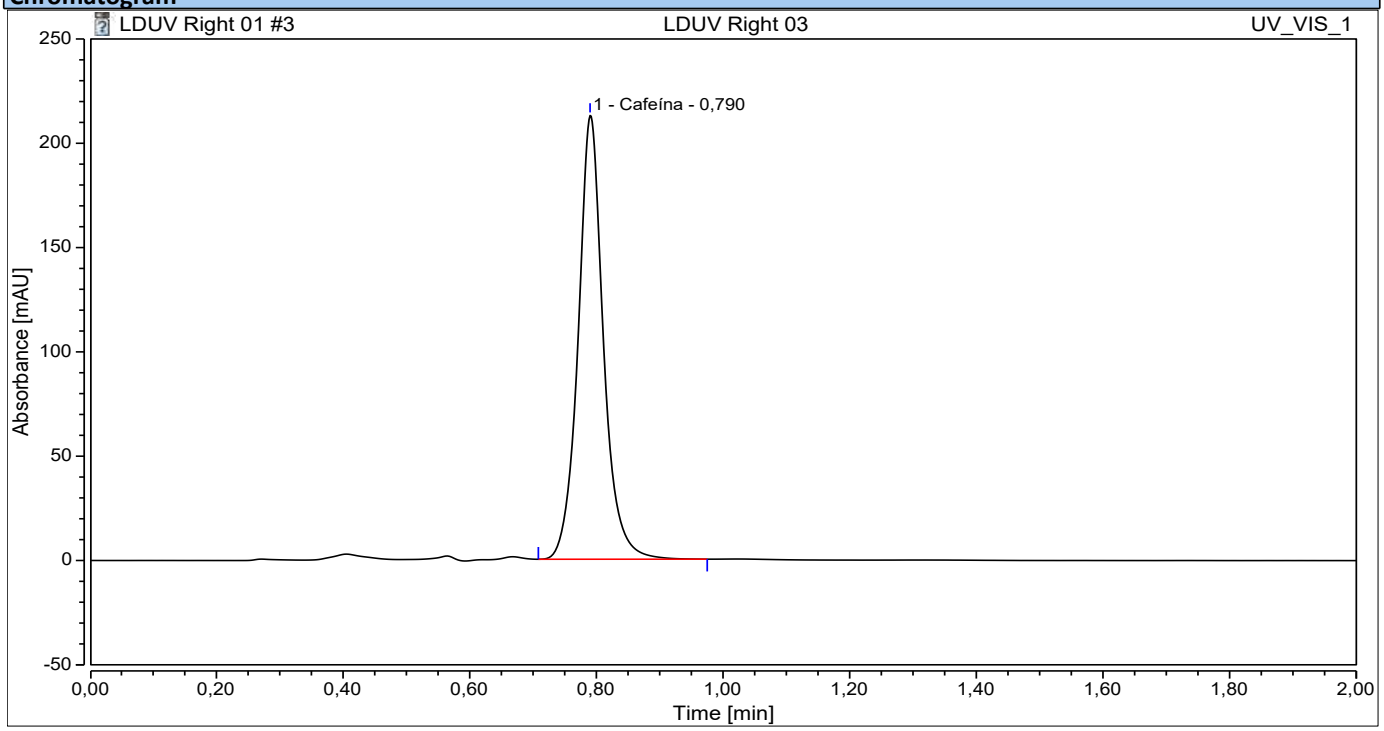

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	9,8187	212,718	100,00	100,00	n.a.
Total:			**9,819**	**212,718**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 04**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:14**	*Sample Weight:*	**1,0000**

Chromatogram

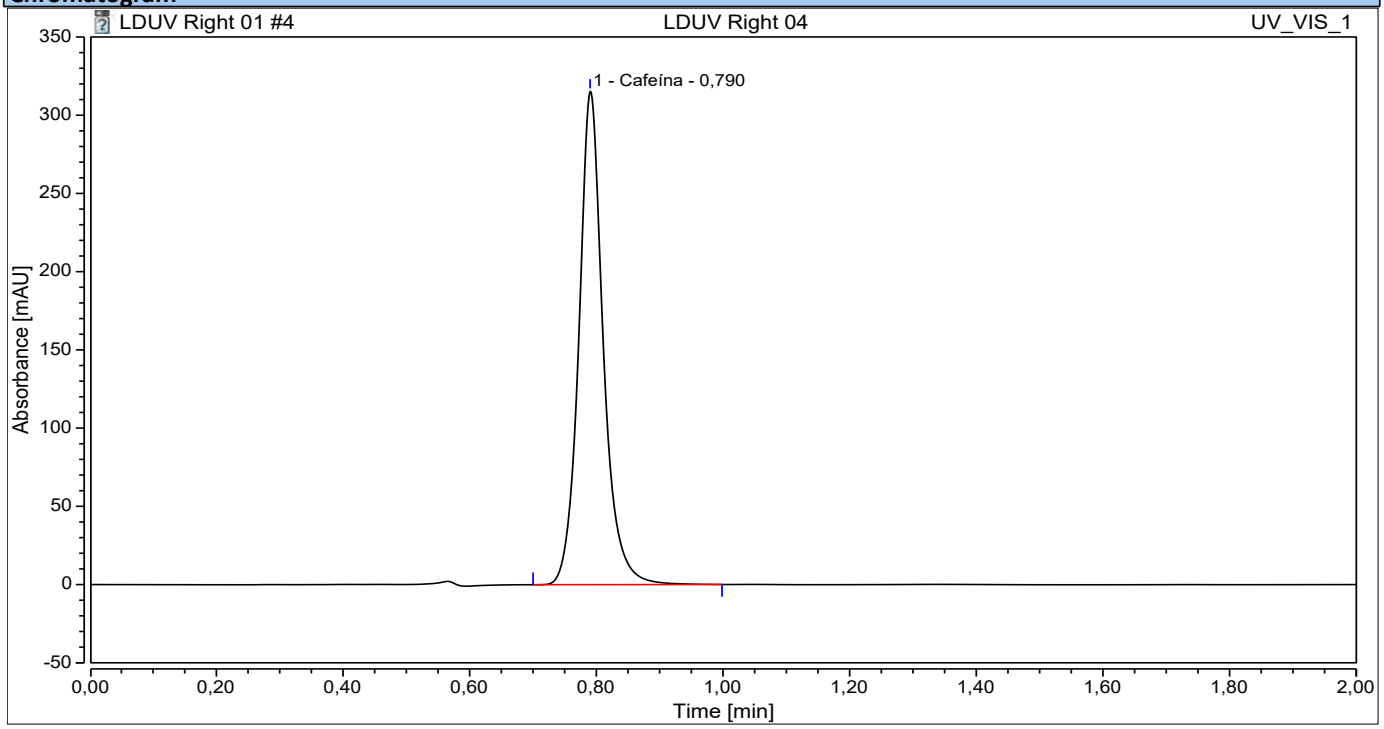

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,790	14,0478	315,255	100,00	100,00	n.a.
Total:			**14,048**	**315,255**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LDUV Right 05**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**06/mai/25 17:17**	*Sample Weight:*	**1,0000**

Chromatogram

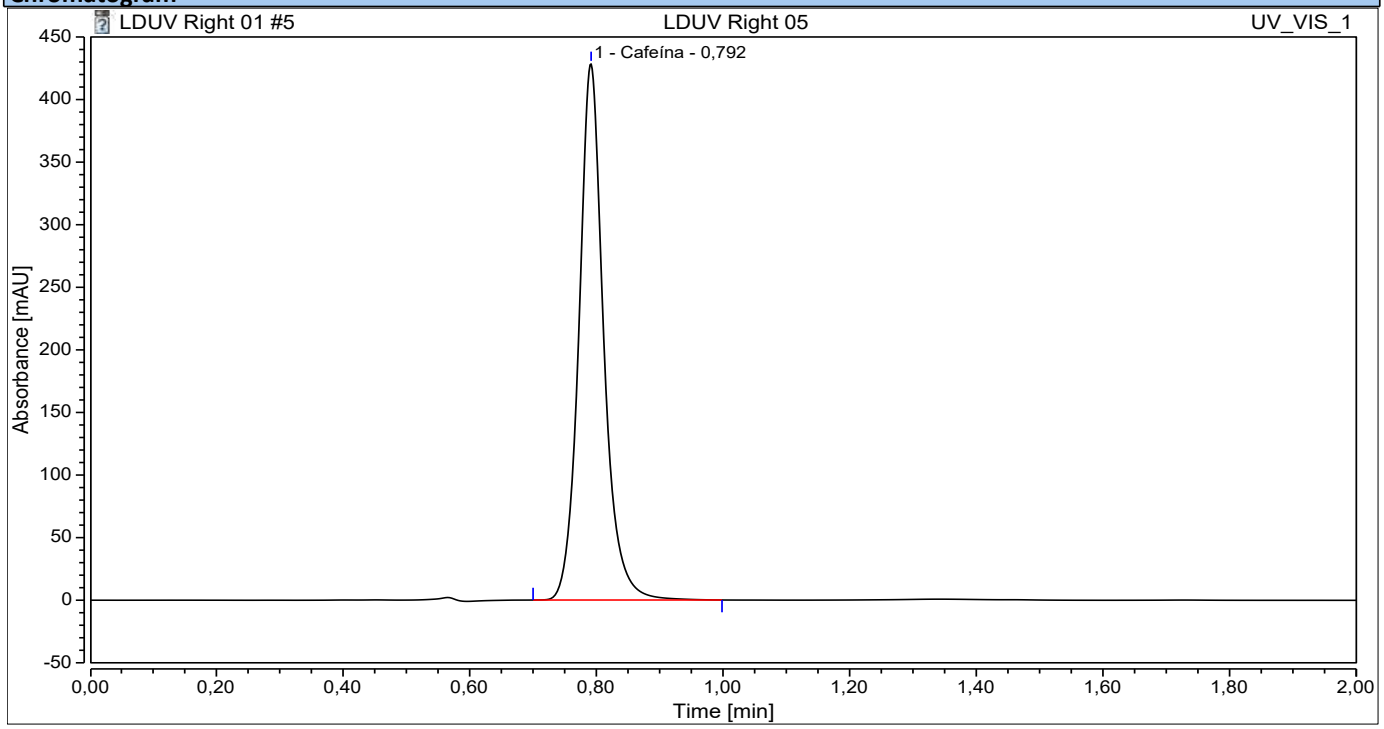

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,792	19,3639	428,328	100,00	100,00	n.a.
Total:			**19,364**	**428,328**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Right**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 10:03**	*Sample Weight:*	**1,0000**

Chromatogram

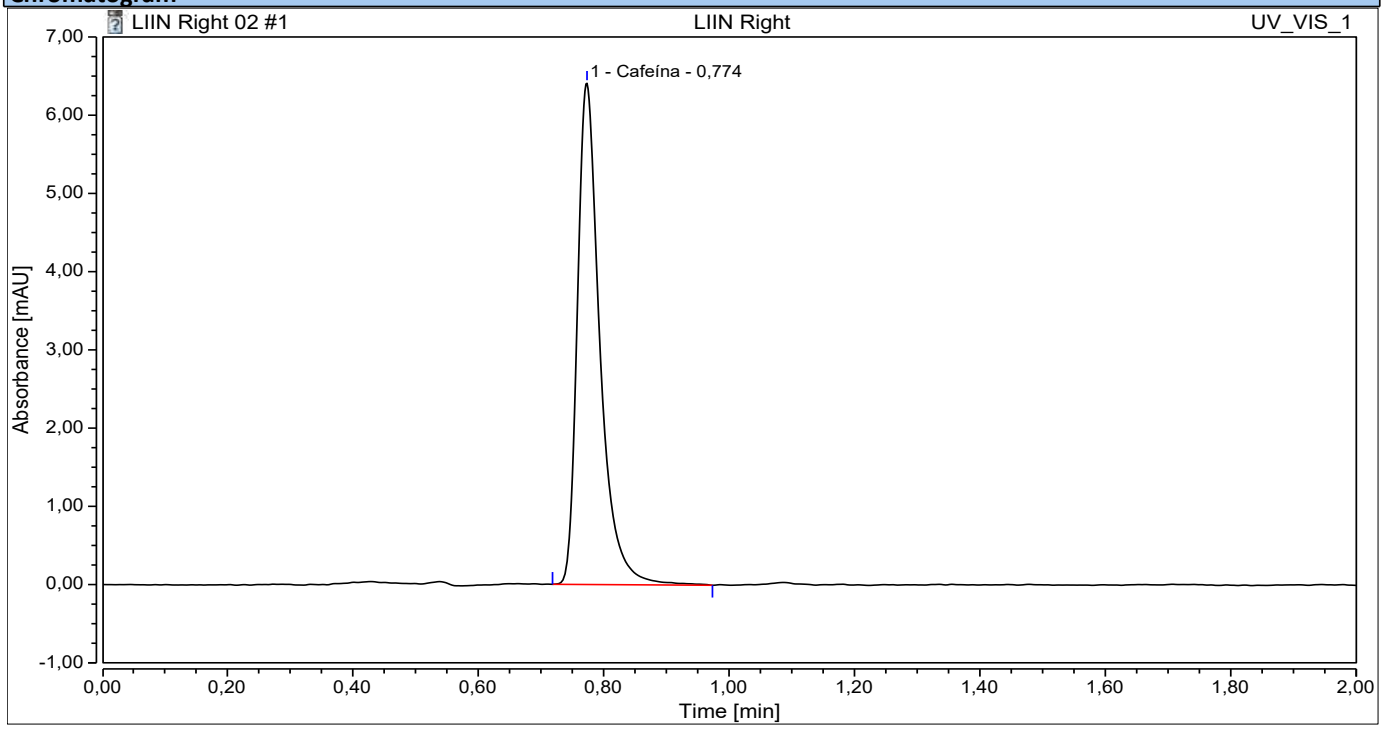

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,774	0,2671	6,408	100,00	100,00	n.a.
Total:			**0,267**	**6,408**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Right**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 10:06**	*Sample Weight:*	**1,0000**

Chromatogram

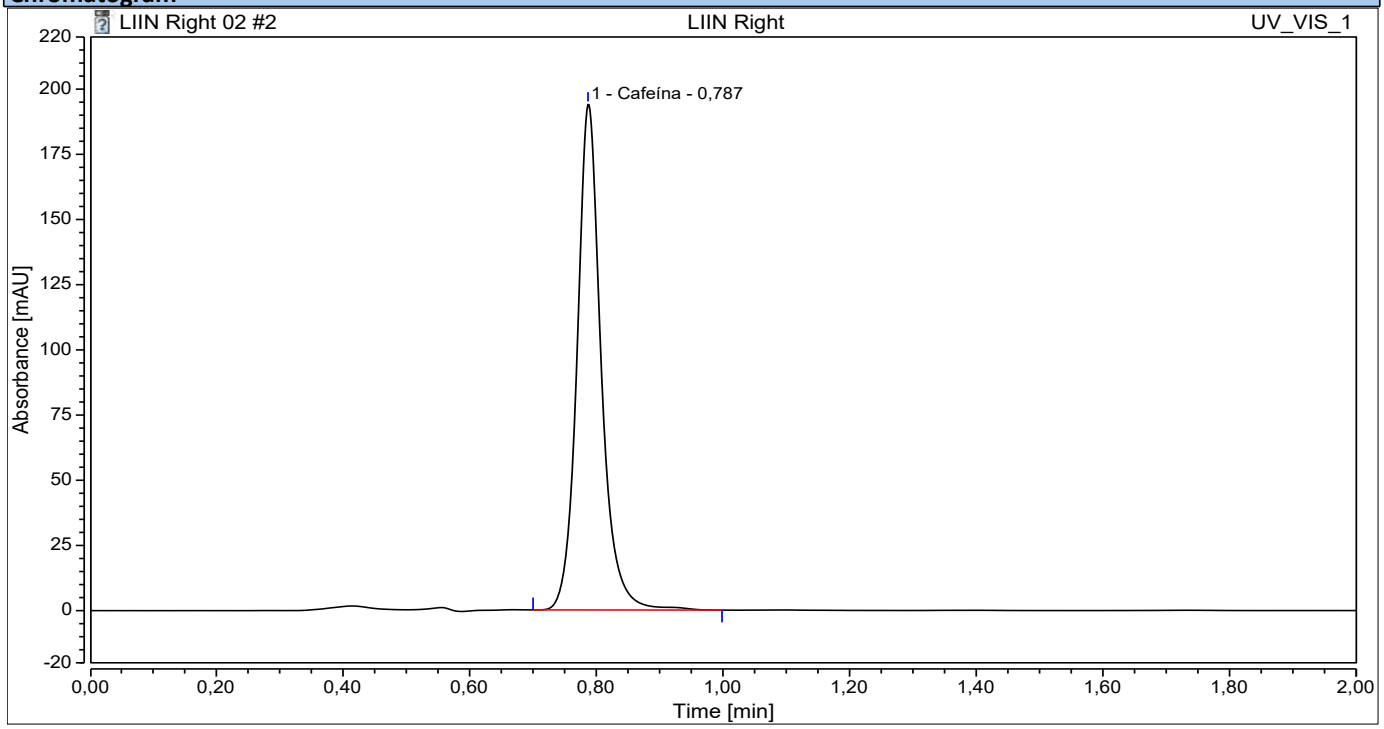

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,787	8,5477	193,865	100,00	100,00	n.a.
Total:			**8,548**	**193,865**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Right**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 10:08**	*Sample Weight:*	**1,0000**

Chromatogram

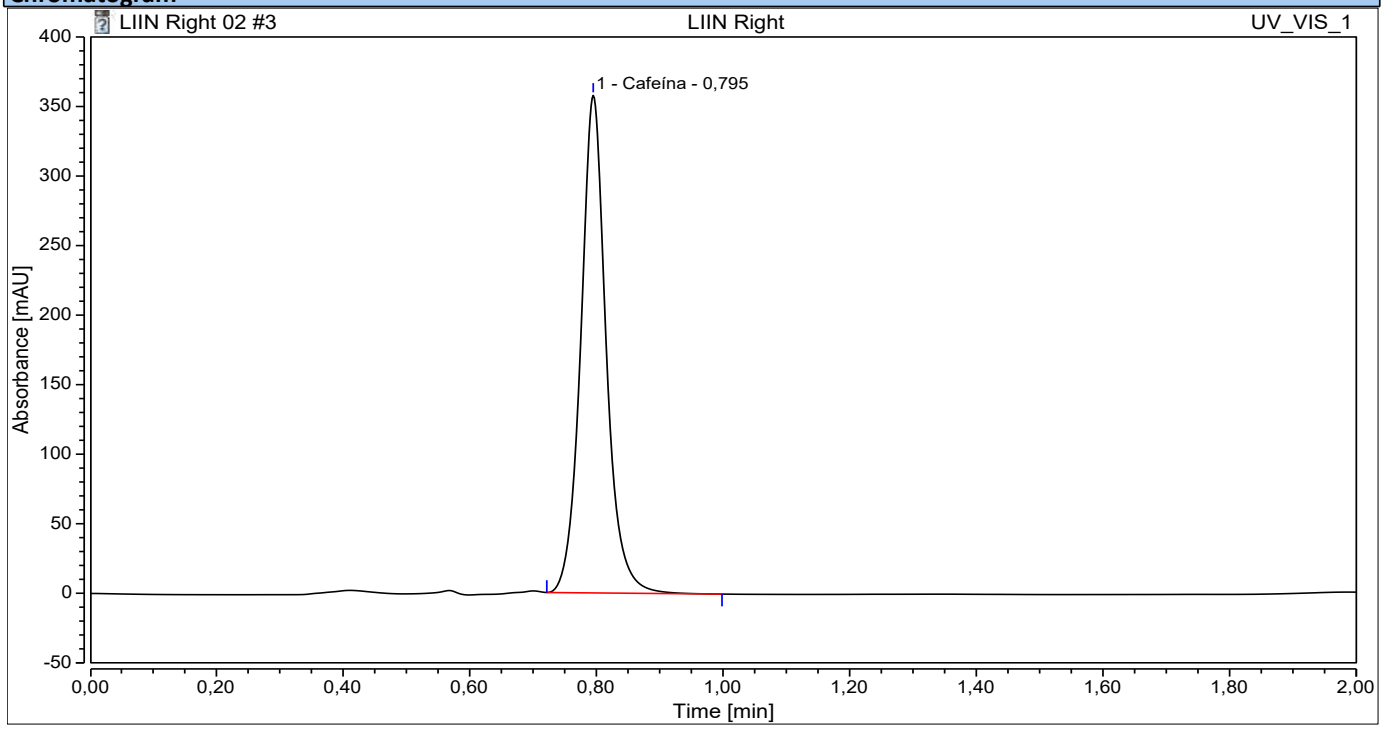

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,795	16,5959	357,758	100,00	100,00	n.a.
Total:			**16,596**	**357,758**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Right**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 10:11**	*Sample Weight:*	**1,0000**

Chromatogram

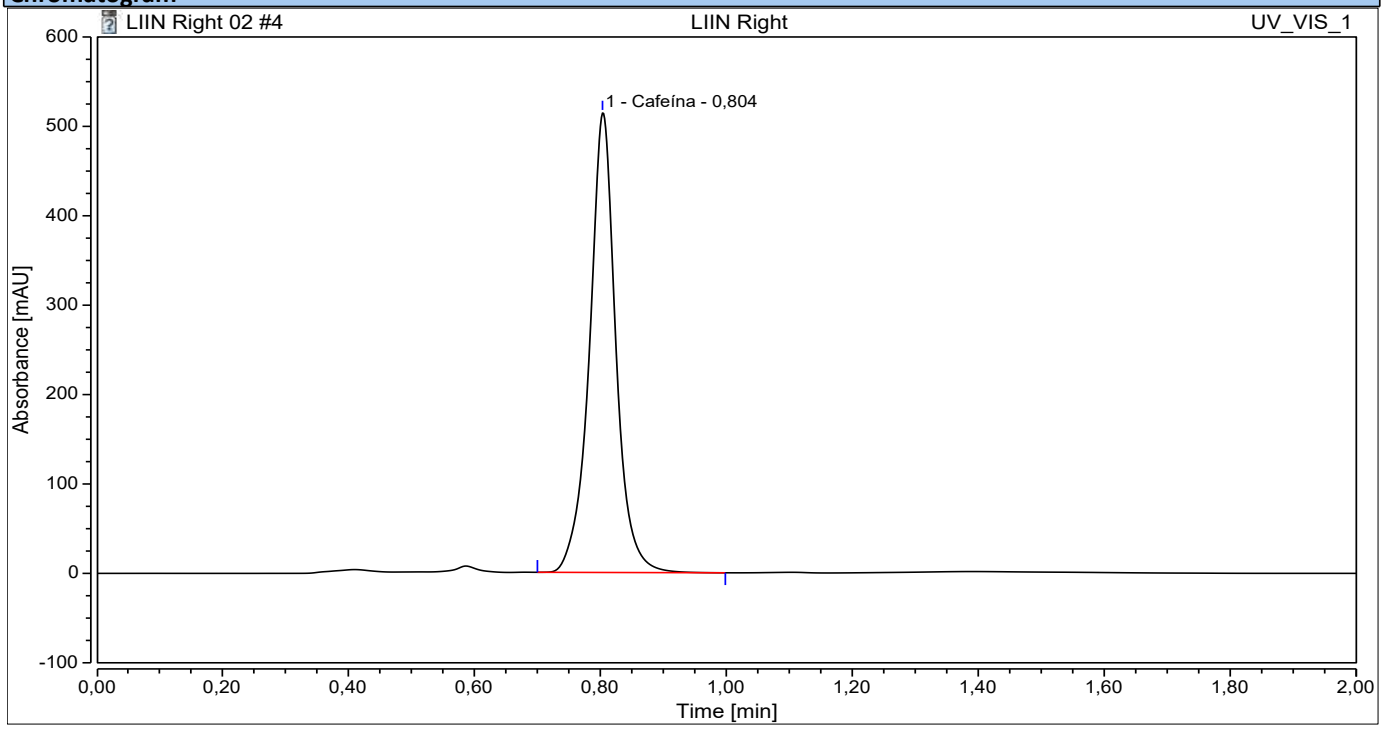

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,804	24,9315	513,928	100,00	100,00	n.a.
Total:			**24,931**	**513,928**	**100,000**	**100,000**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**LIIN Right**	*Run Time (min):*	**2,00**
Vial Number:	**Y:A9**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação HPLC 08 Right**	*Bandwidth:*	**n.a.**
Processing Method:	**EDUV**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 10:13**	*Sample Weight:*	**1,0000**

Chromatogram

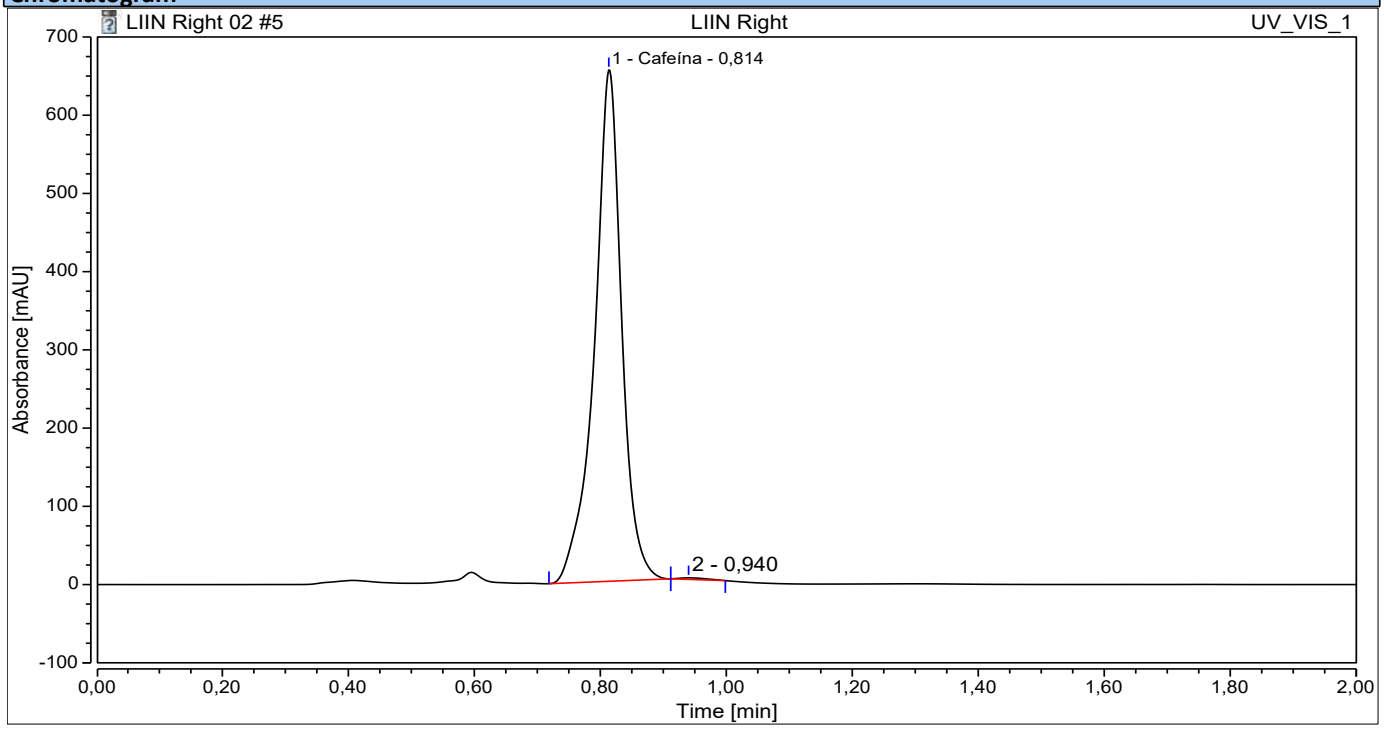

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
1	Cafeína	0,814	32,6361	653,826	99,68	99,70	n.a.
Total:			**32,636**	**653,826**	**99,677**	**99,700**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB Right**	*Run Time (min):*	**19,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB Right**	*Bandwidth:*	**n.a.**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 11:19**	*Sample Weight:*	**1,0000**

Chromatogram

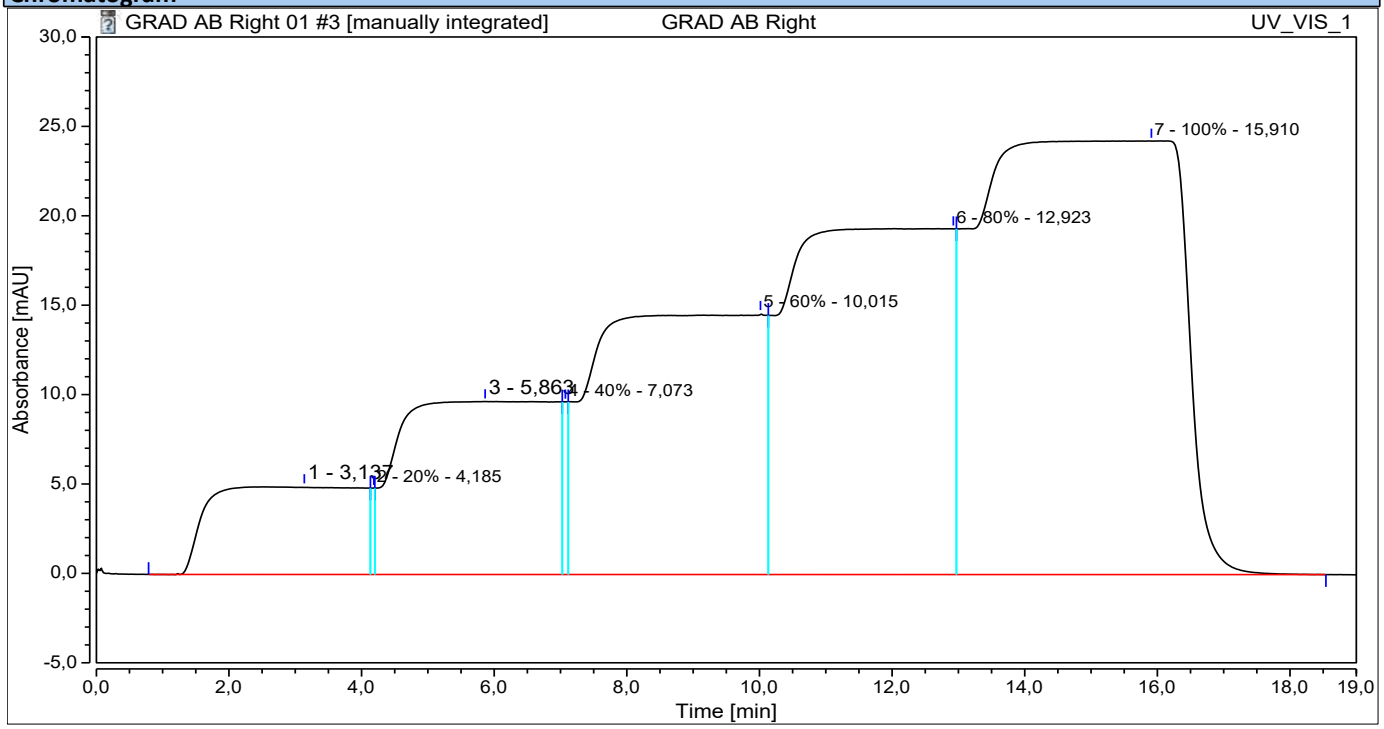

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	4,185	0,3222	4,838	0,15	5,54	n.a.
4	40%	7,073	0,8692	9,662	0,40	11,06	n.a.
5	60%	10,015	41,6492	14,619	19,12	16,74	n.a.
6	80%	12,923	52,8901	19,351	24,28	22,16	n.a.
7	100%	15,910	83,9322	24,257	38,52	27,78	n.a.
Total:			**179,663**	**72,727**	**82,460**	**83,282**	


© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AC Right**	*Run Time (min):*	**19,00**
Vial Number:	**Y:A2**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AC Right**	*Bandwidth:*	**n.a.**
Processing Method:	**GRAD**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**07/mai/25 12:36**	*Sample Weight:*	**1,0000**

Chromatogram

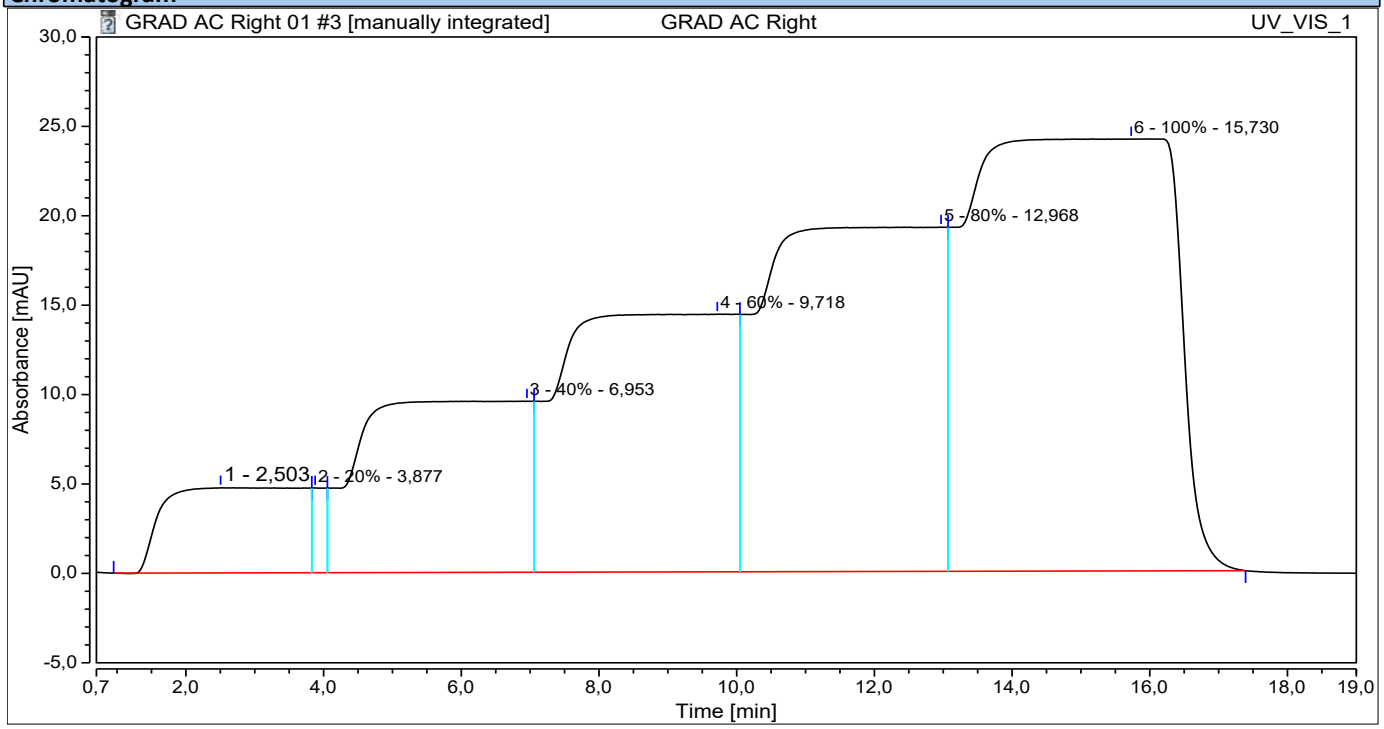

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount
2	20%	3,877	1,0725	4,742	0,50	6,17	n.a.
3	40%	6,953	26,3024	9,571	12,17	12,45	n.a.
4	60%	9,718	40,6828	14,412	18,82	18,74	n.a.
5	80%	12,968	55,7938	19,252	25,81	25,04	n.a.
6	100%	15,730	81,5191	24,162	37,71	31,42	n.a.
Total:			**205,371**	**72,138**	**95,010**	**93,807**	

© 2009-2023 Thermo Fisher Scientific Inc. All rights reserved.