
Peak Find - EDUV PDA_4,2133.JWS

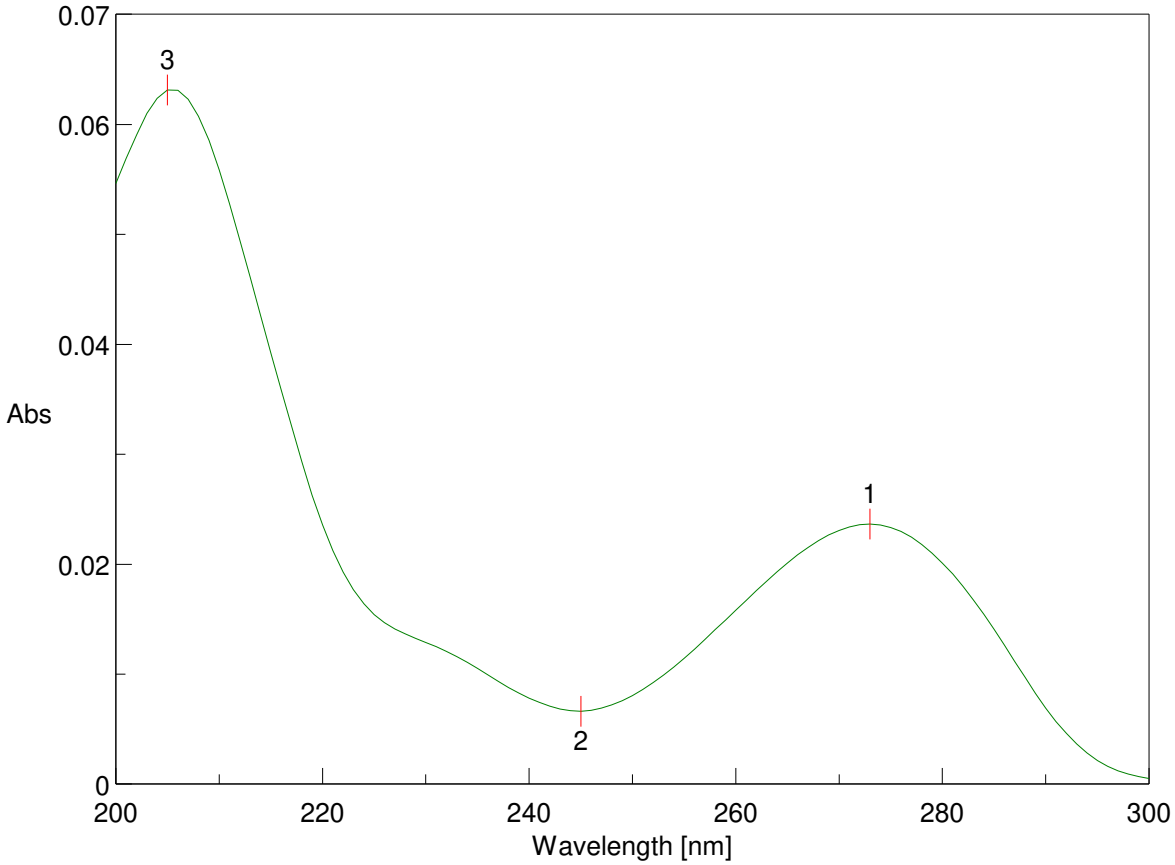

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	04/05/2023 17:18

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A011361665
ROM version	V1.02.14

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.023623	2	245	0.006615
3	205	0.063092			

Chromatogram

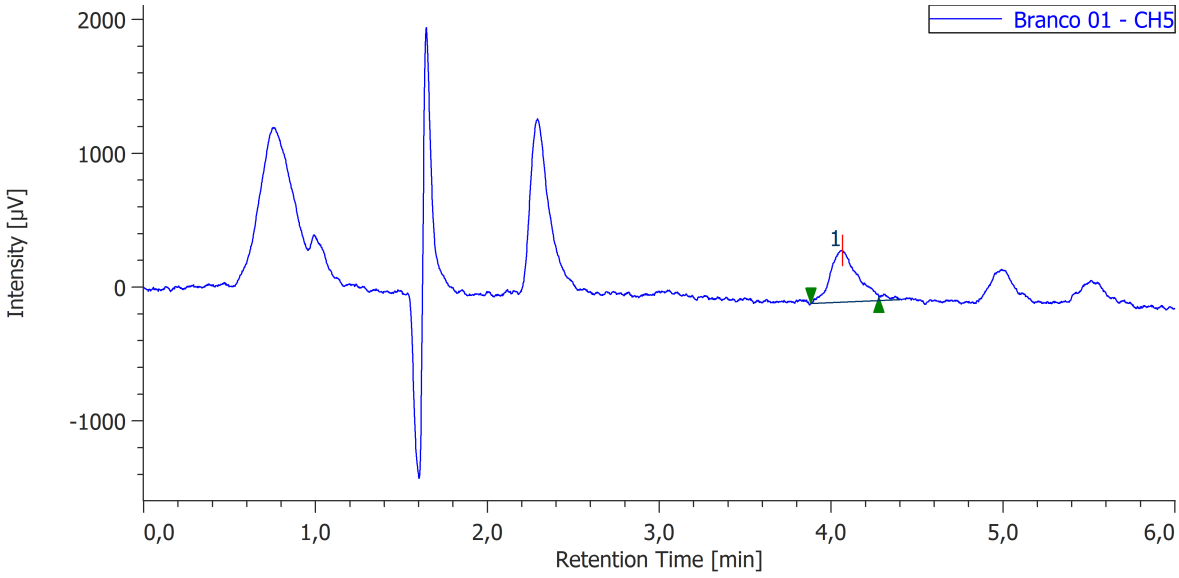

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:51
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:22:19
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,065	4215	387	100,000	100,000	N/A	3279	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

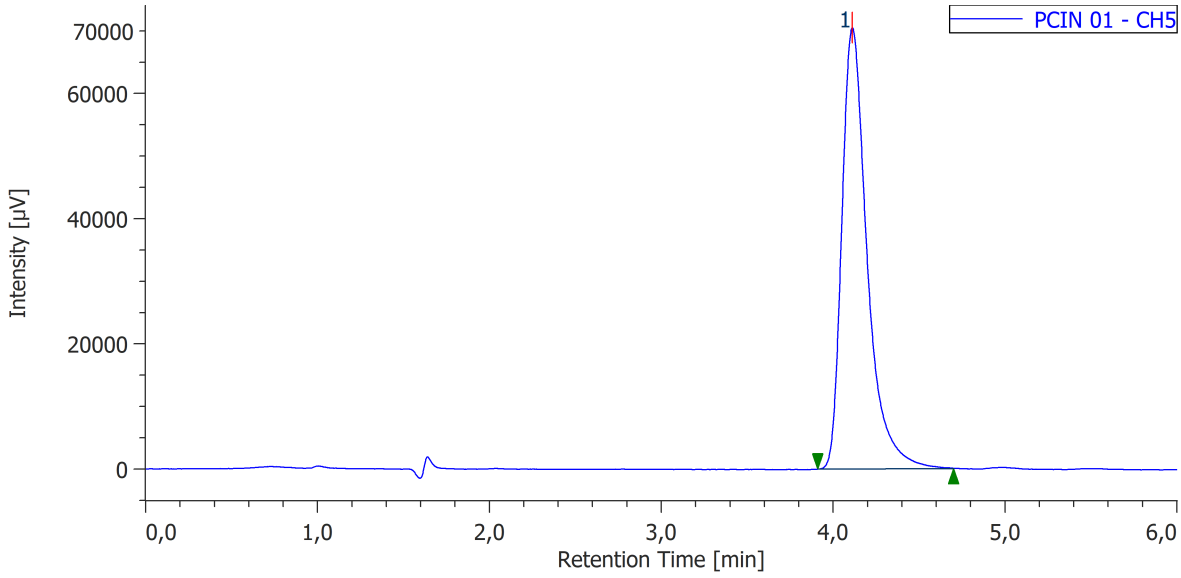

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:38
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:28:31
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,110	721786	70474	100,000	100,000	N/A	4189	N/A	1,508	

Creator QPackSA
Reviewer
Approver

Chromatogram

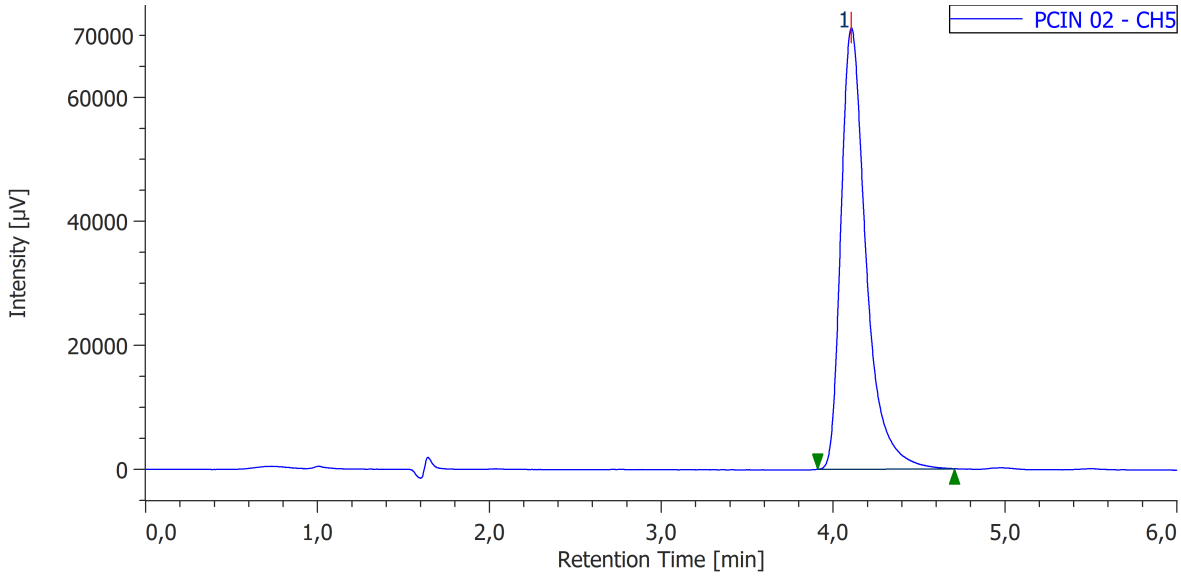

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:39
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:34:43
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,105	723186	71174	100,000	100,000	N/A	4244	N/A	1,504	

Creator QPackSA
Reviewer
Approver

Chromatogram

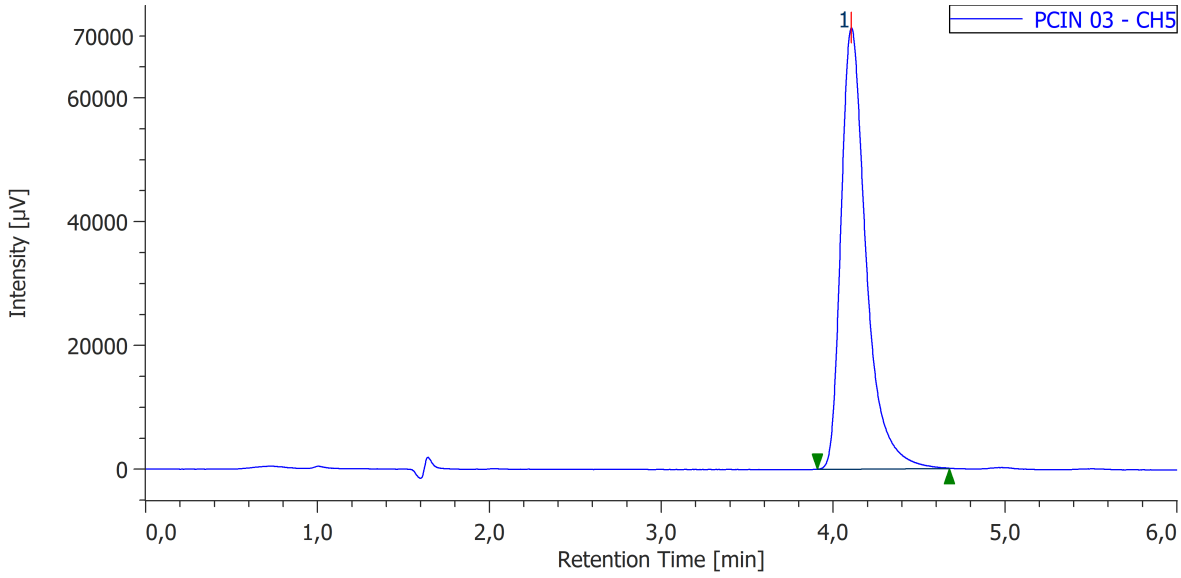

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:39
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:40:55
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,105	723597	71278	100,000	100,000	N/A	4244	N/A	1,504	

Creator QPackSA
Reviewer
Approver

Chromatogram

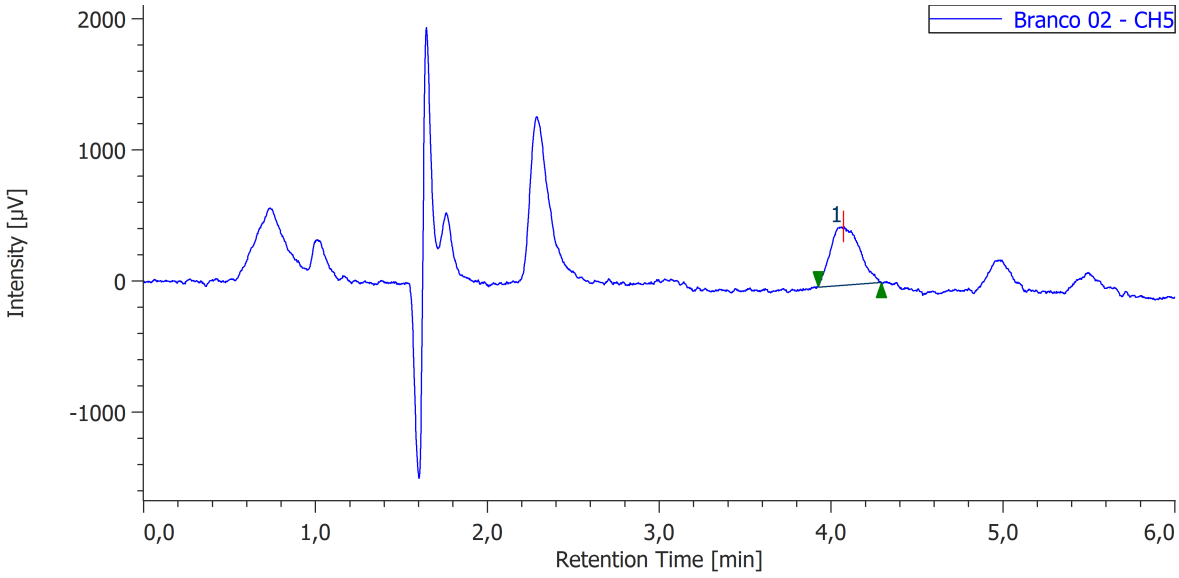

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:51
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:47:06
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,072	5271	448	100,000	100,000	N/A	2523	N/A	1,222	

Creator QPackSA
Reviewer
Approver

Chromatogram

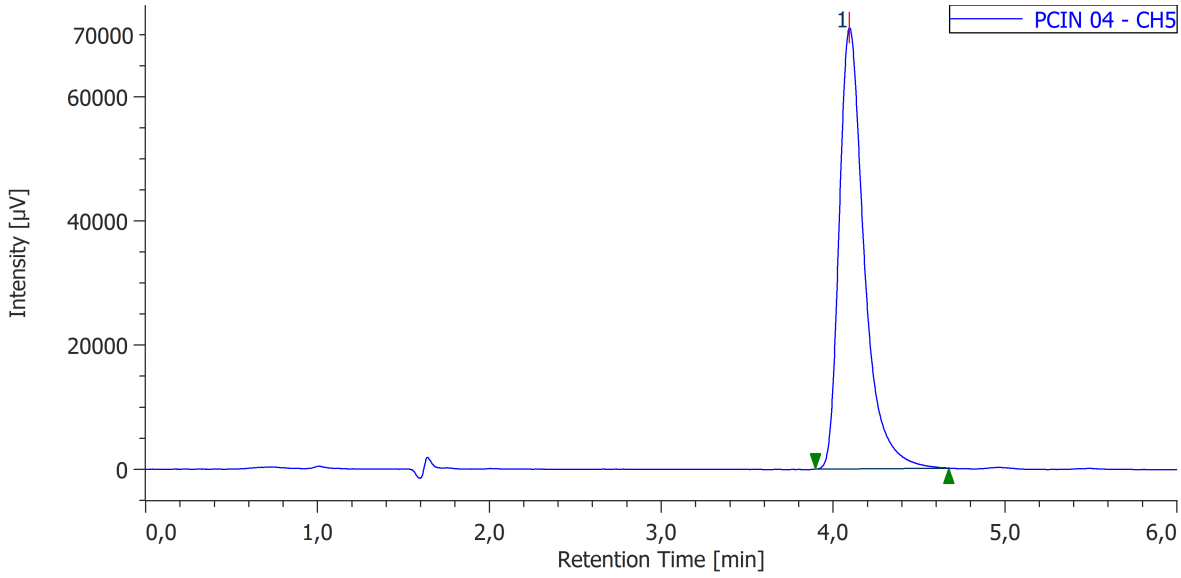

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:39
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:53:18
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,093	719740	71031	100,000	100,000	N/A	4242	N/A	1,518	

Creator QPackSA
Reviewer
Approver

Chromatogram

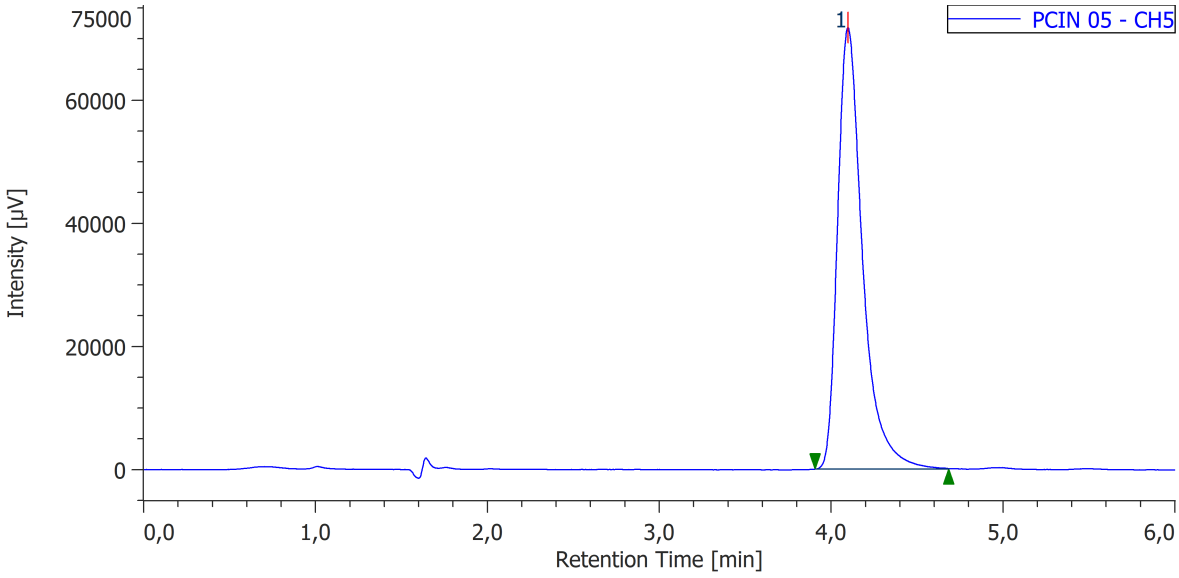

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:40
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 19:59:30
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,097	724253	71681	100,000	100,000	N/A	4285	N/A	1,507	

Creator QPackSA
Reviewer
Approver

Chromatogram

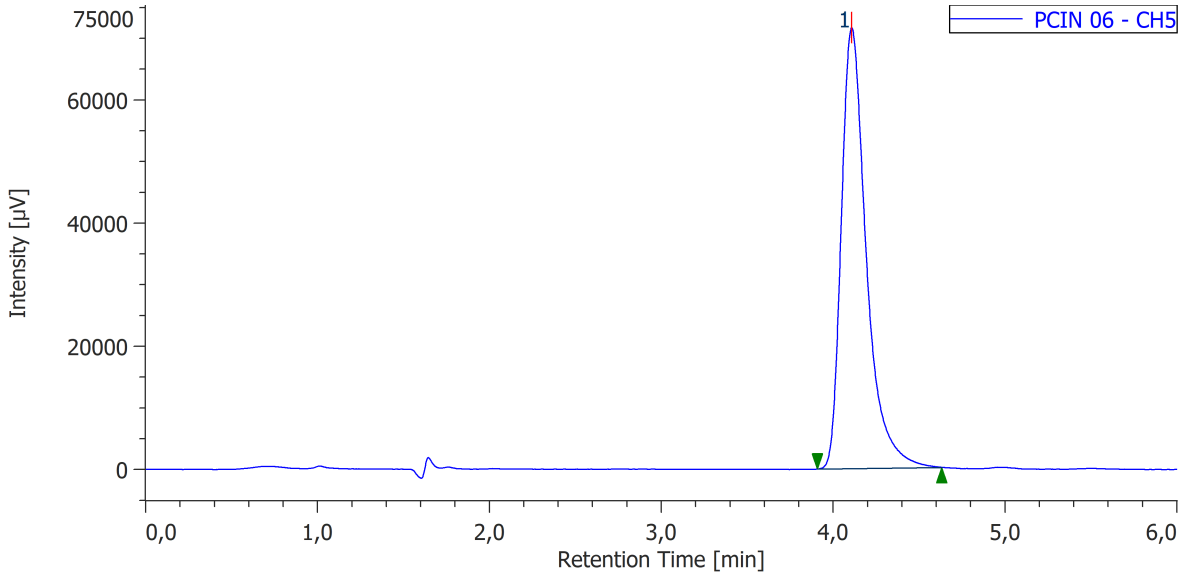

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:40
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:05:42
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,107	723308	71563	100,000	100,000	N/A	4265	N/A	1,500	

Creator QPackSA
Reviewer
Approver

Chromatogram

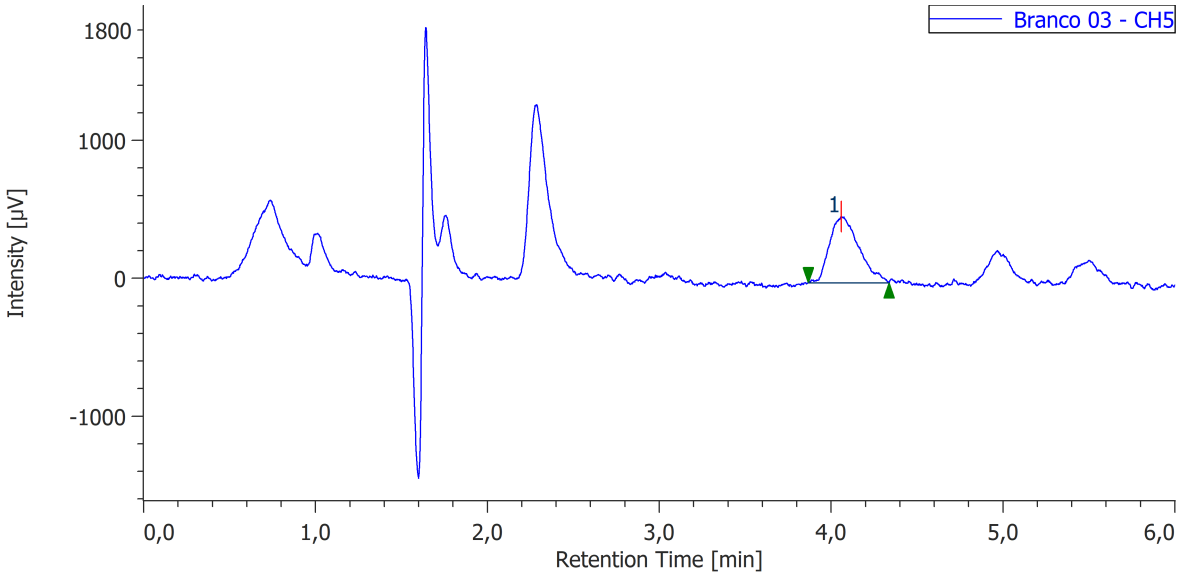

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:52
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:11:54
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,058	5689	480	100,000	100,000	N/A	2492	N/A	1,475	

Creator QPackSA
Reviewer
Approver

Chromatogram

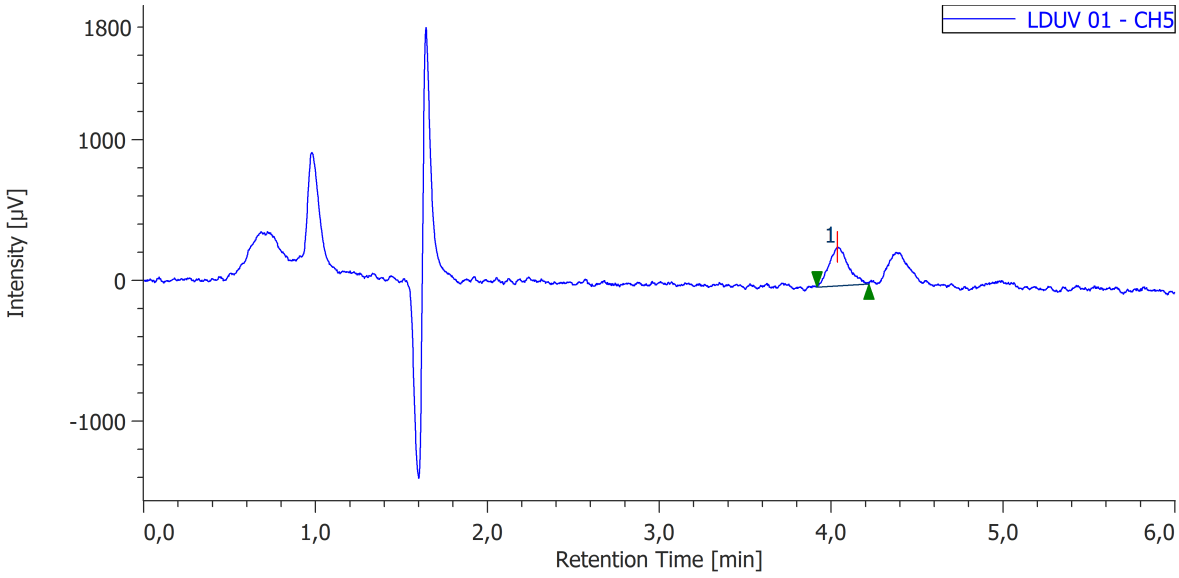

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:52
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:18:06
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração Branco

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,035	2148	276	100,000	100,000	N/A	6650	N/A	1,207	

Creator QPackSA
Reviewer
Approver

Chromatogram

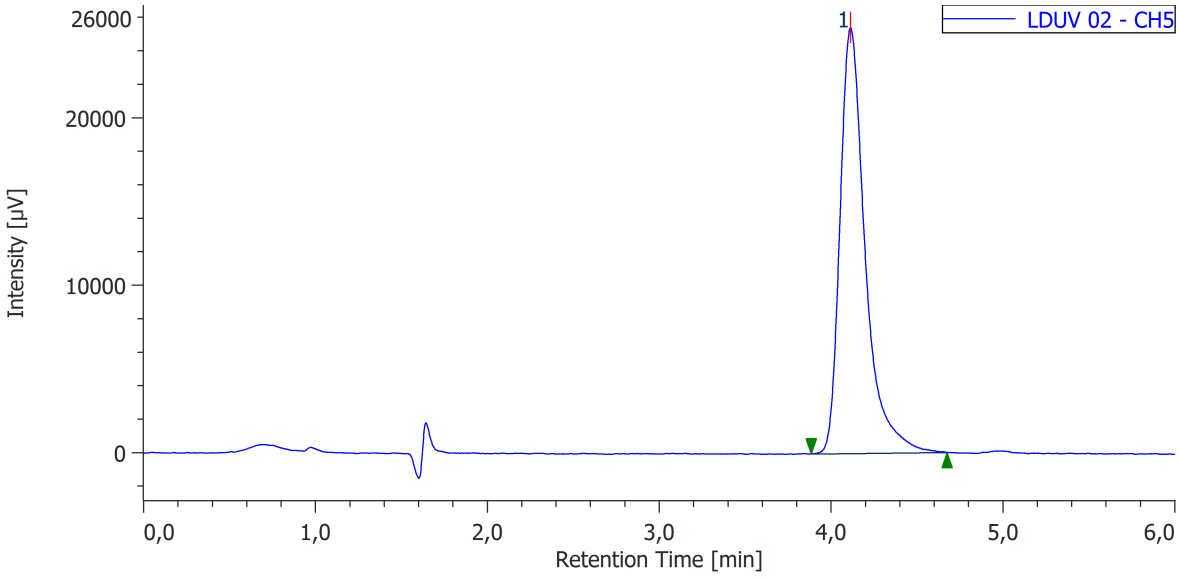

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:52
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:24:18
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,112	259301	25434	100,000	100,000	N/A	4338	N/A	1,523	

Creator QPackSA
Reviewer
Approver

Chromatogram

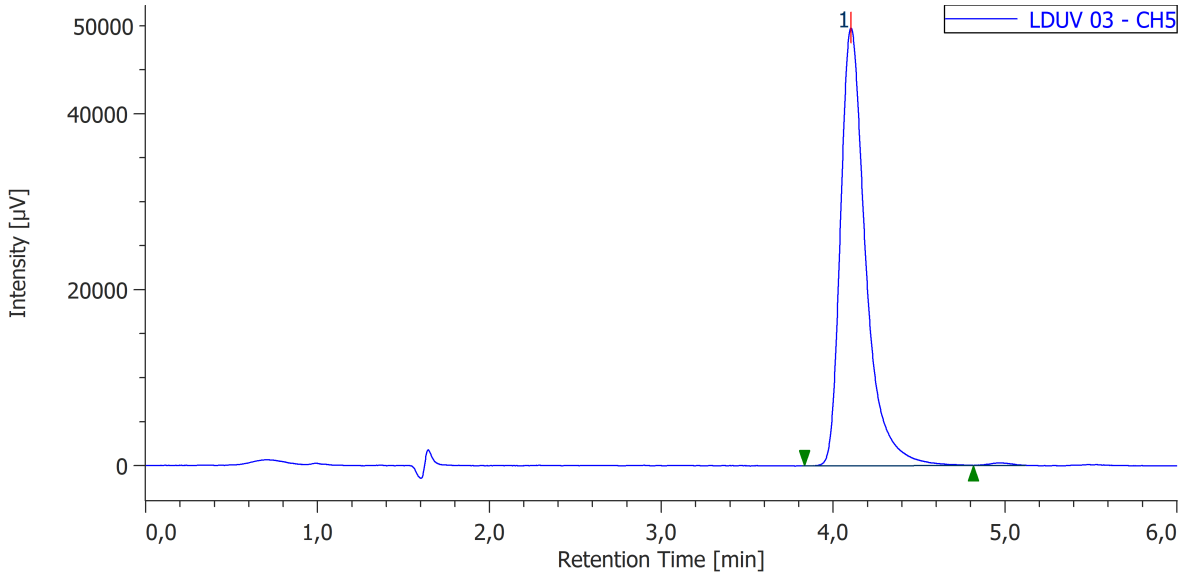

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:58:53
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:30:30
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,102	506866	49783	100,000	100,000	N/A	4283	N/A	1,507	

Creator QPackSA
Reviewer
Approver

Chromatogram

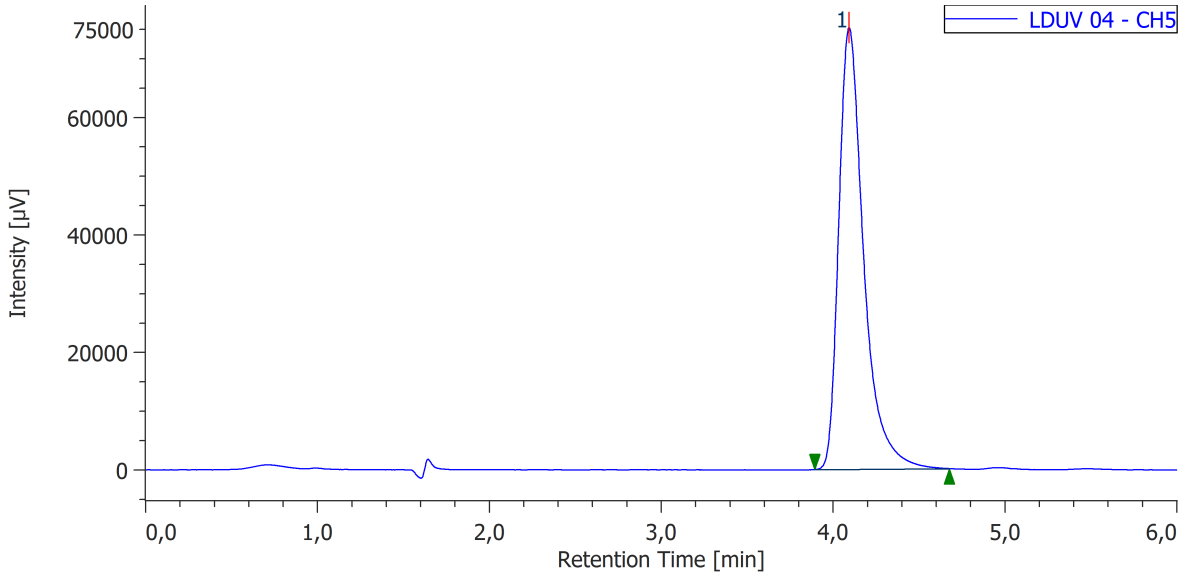

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:42
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:36:42
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,092	758332	75151	100,000	100,000	N/A	4285	N/A	1,512	

Creator QPackSA
Reviewer
Approver

Chromatogram

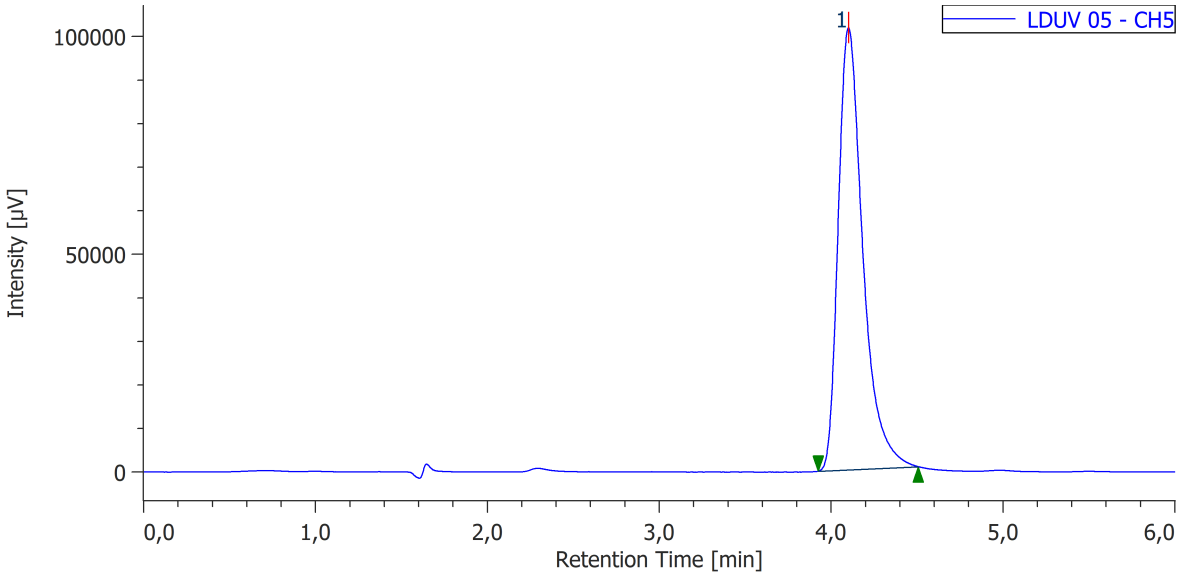

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:51:38
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:42:54
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,100	1009567	101477	100,000	100,000	N/A	4277	N/A	1,481	

Creator QPackSA
Reviewer
Approver

Chromatogram

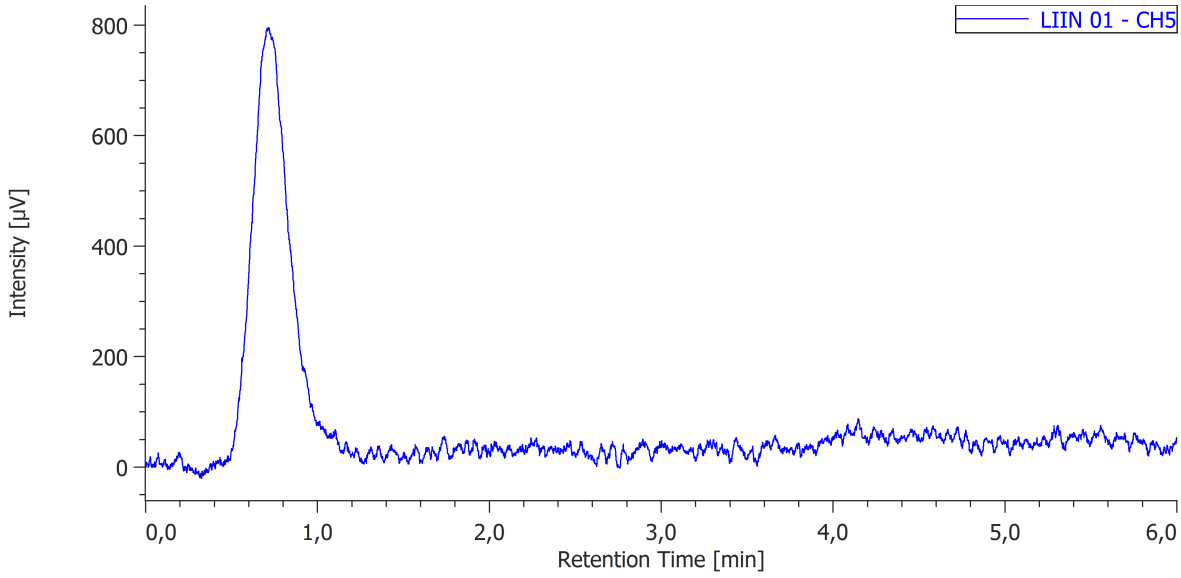


Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:42
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:49:06
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

Creator QPackSA
Reviewer
Approver

Chromatogram

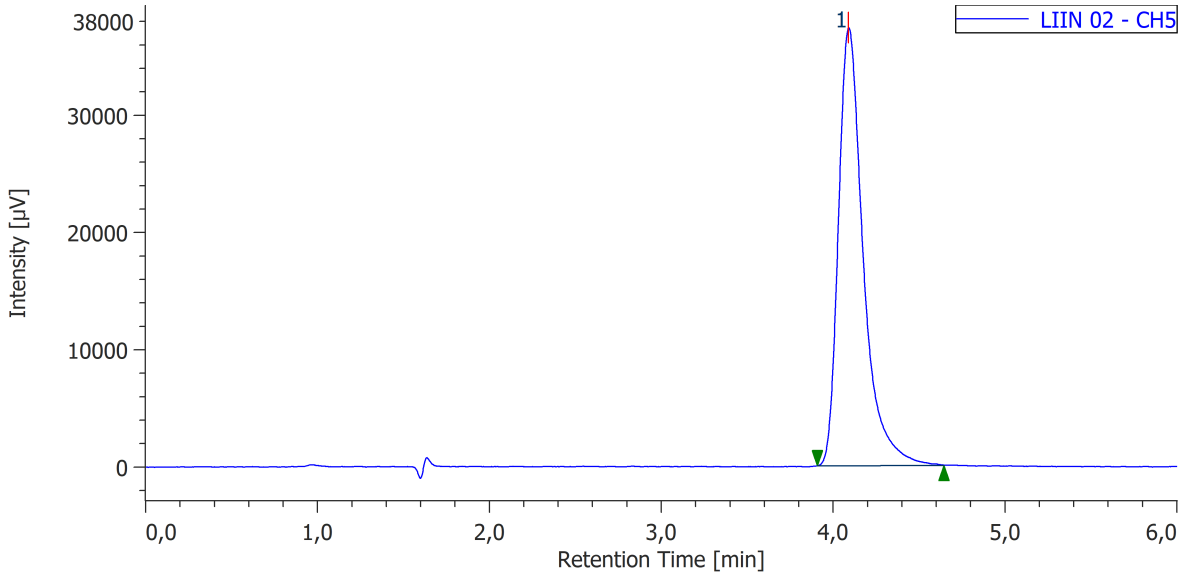

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:43
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 20:55:18
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,088	375099	37339	100,000	100,000	N/A	4355	N/A	1,525	

Creator QPackSA
Reviewer
Approver

Chromatogram

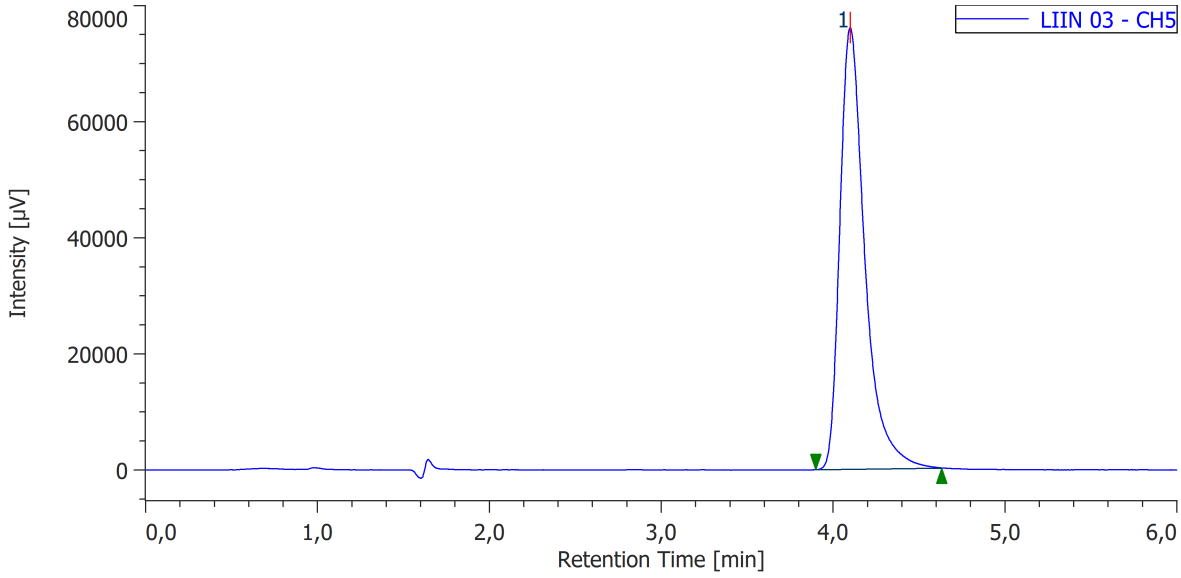

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:43
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 21:01:30
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,098	768390	76026	100,000	100,000	N/A	4283	N/A	1,526	

Creator QPackSA
Reviewer
Approver

Chromatogram

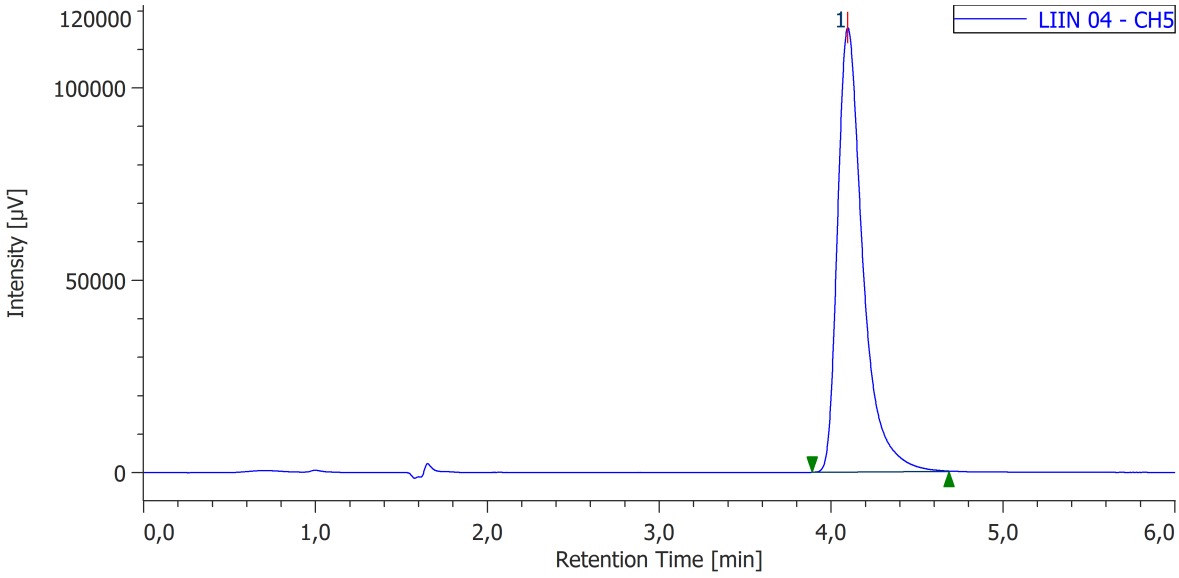

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:43
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 21:07:42
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,095	1178749	115439	100,000	100,000	N/A	4210	N/A	1,578	

Creator QPackSA
Reviewer
Approver

Chromatogram

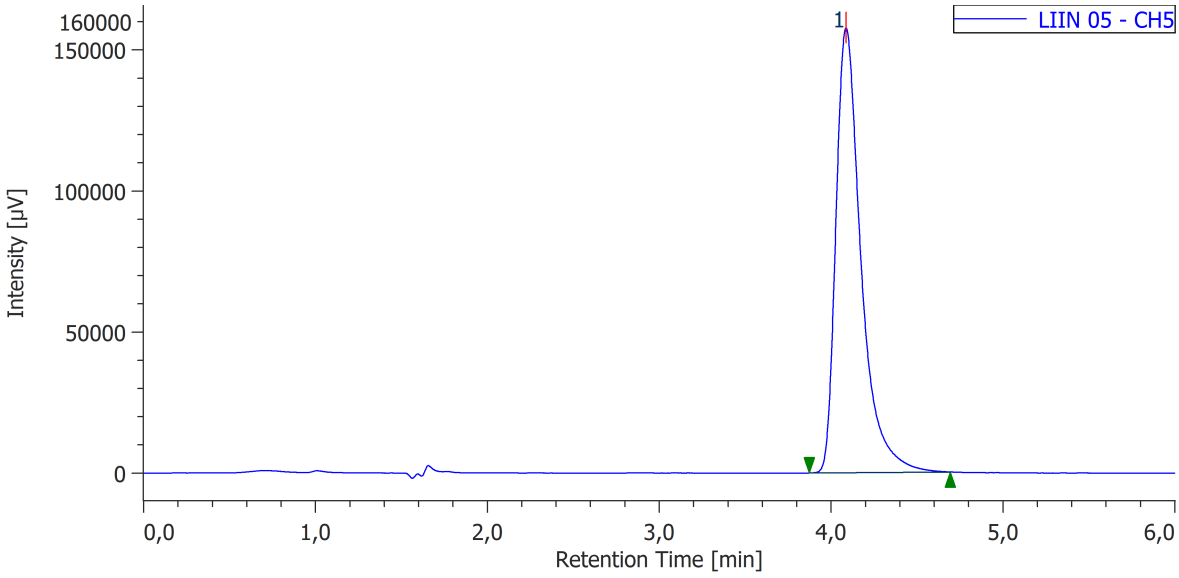

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 07:35:44
Description	
HPLC System Name	HPL 19
Injection Date	04/05/2023 21:13:54
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação Operacional
Acquisition Time	6,0 [min]
Acquisition Sequence	Qualificação 2023
Control Method	Quali_QPACK
Peak ID Table	Identificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD Cafeina	5	4,085	1600662	157699	100,000	100,000	N/A	4245	N/A	1,590	

Creator QPackSA
Reviewer
Approver

Chromatogram

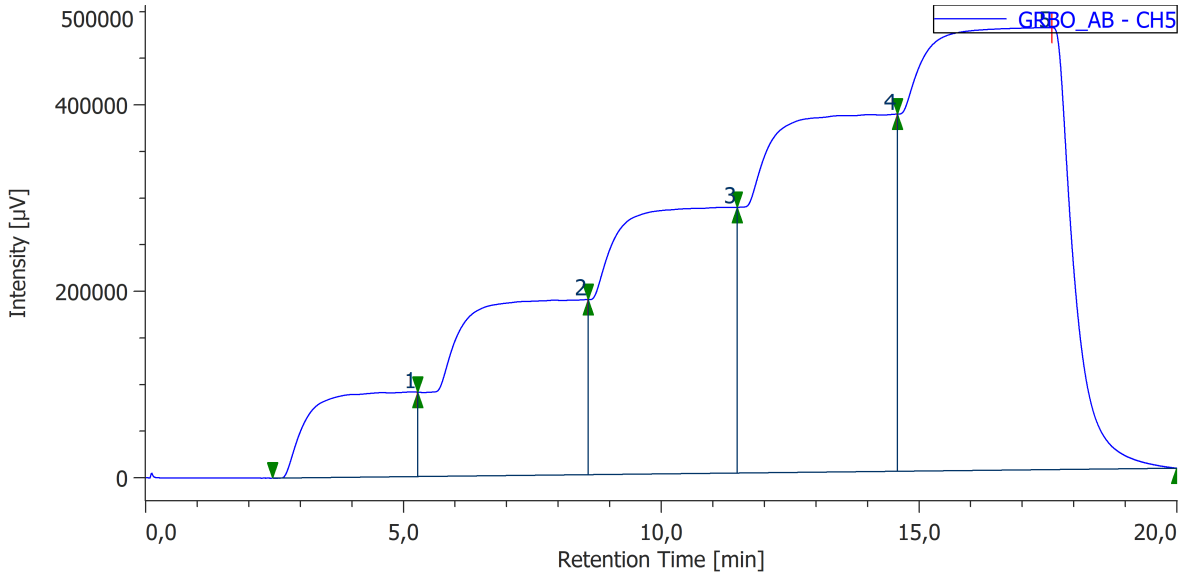

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 12:26:38
Description	
HPLC System Name	HPL 19
Injection Date	05/05/2023 11:14:41
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	GRBO
Control Method	GRBO_AB
Peak ID Table	GRBOAB_01
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRBO_AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20	5	5,272	12072385	90454	4,722	6,371	N/A	N/A	N/A	N/A	
2	40	5	8,577	32669750	187725	12,778	13,223	N/A	N/A	N/A	N/A	
3	60	5	11,467	46615946	284742	18,233	20,056	N/A	N/A	N/A	N/A	
4	80	5	14,572	67860463	382873	26,542	26,968	N/A	N/A	N/A	N/A	
5	100	5	17,570	96452868	473924	37,725	33,382	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

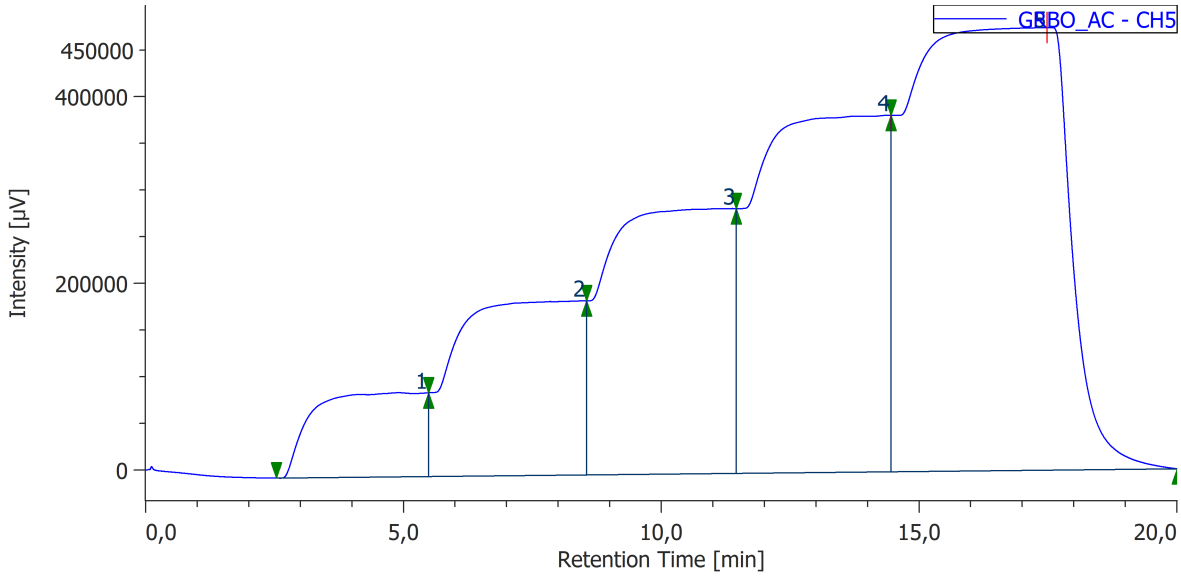

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 12:26:40
Description	
HPLC System Name	HPL 19
Injection Date	05/05/2023 11:34:53
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	GRBO
Control Method	GRBO_AC
Peak ID Table	GRBO_02
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRBO_AC-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20	5	5,487	13052851	89713	5,125	6,339	N/A	N/A	N/A	N/A	
2	40	5	8,545	30924145	186484	12,142	13,176	N/A	N/A	N/A	N/A	
3	60	5	11,452	46506860	283441	18,260	20,026	N/A	N/A	N/A	N/A	
4	80	5	14,448	65038804	381710	25,536	26,969	N/A	N/A	N/A	N/A	
5	100	5	17,478	99169734	474011	38,937	33,491	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

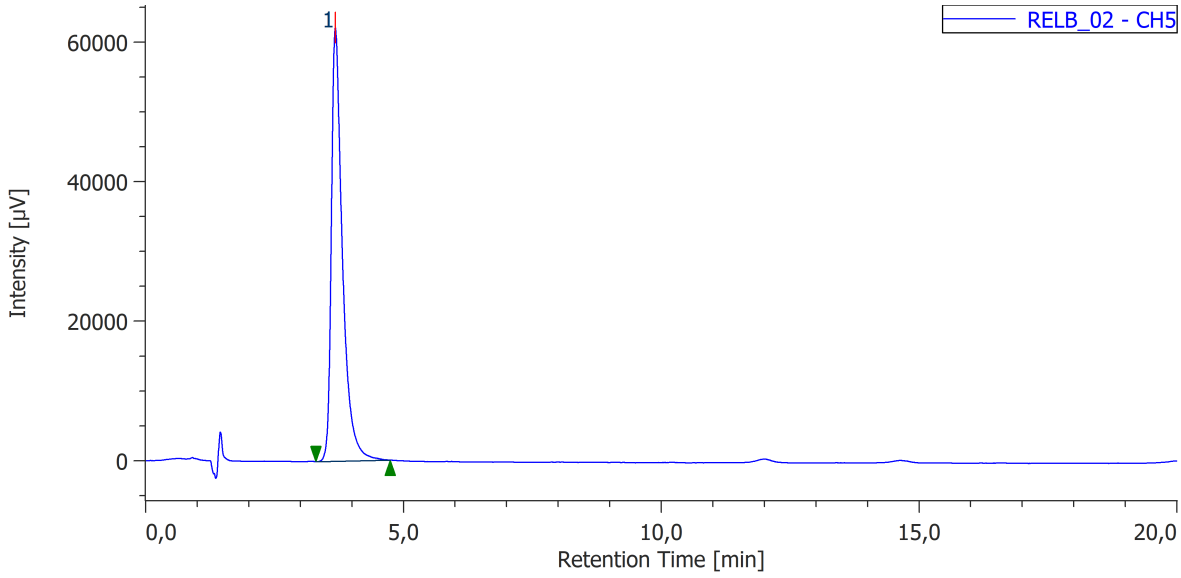

Chromatogram Information	
User Name	QPackSA
Date Modified	05/05/2023 14:11:38
Description	
HPLC System Name	HPL 19
Injection Date	05/05/2023 13:51:27
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação Operacional
Acquisition Time	20,0 [min]
Acquisition Sequence	RELB
Control Method	RELB
Peak ID Table	RELB
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	RELB_02-CH5
Sample Name	
Channel Name	254,0nm
Sampling Interval	200 [msec]
Peak Method	RELB

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,677	932316	62149	100,000	100,000	N/A	1660	N/A	1,693	

Creator
Reviewer
Approver