
Chromatogram

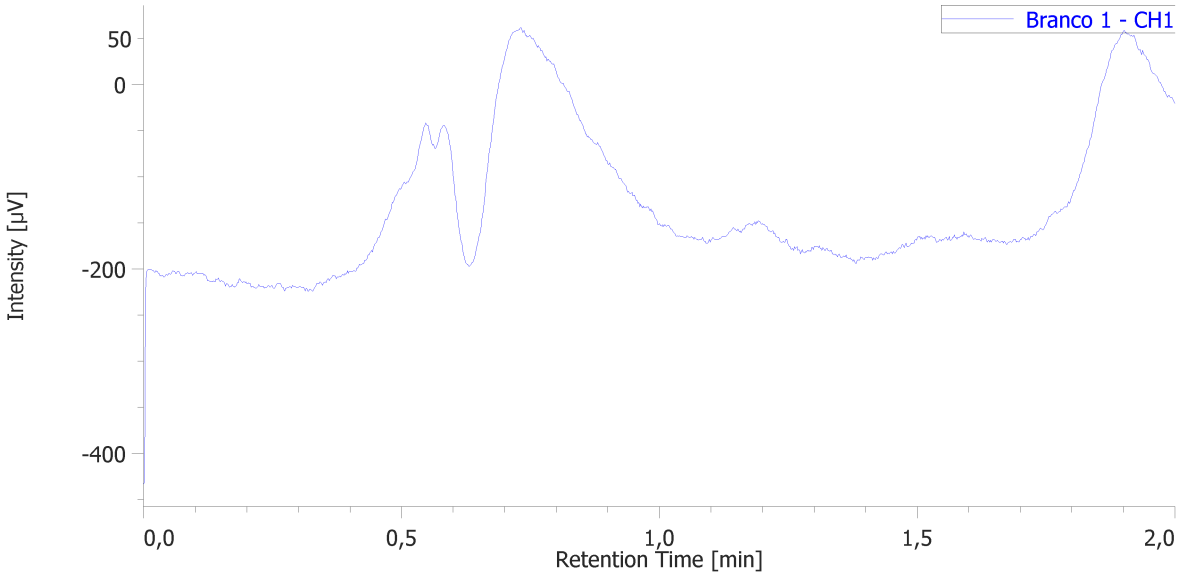


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:50:06
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

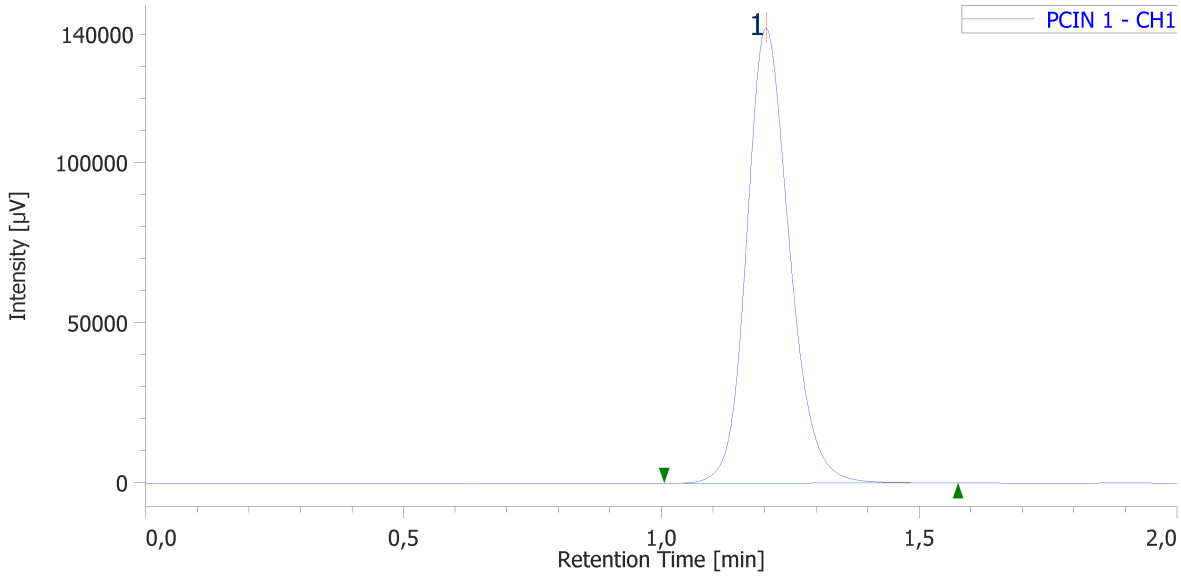

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:52:40
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,203	817640	142013	100,000	100,000	N/A	1066	N/A	1,168	

Creator
Reviewer
Approver

Chromatogram

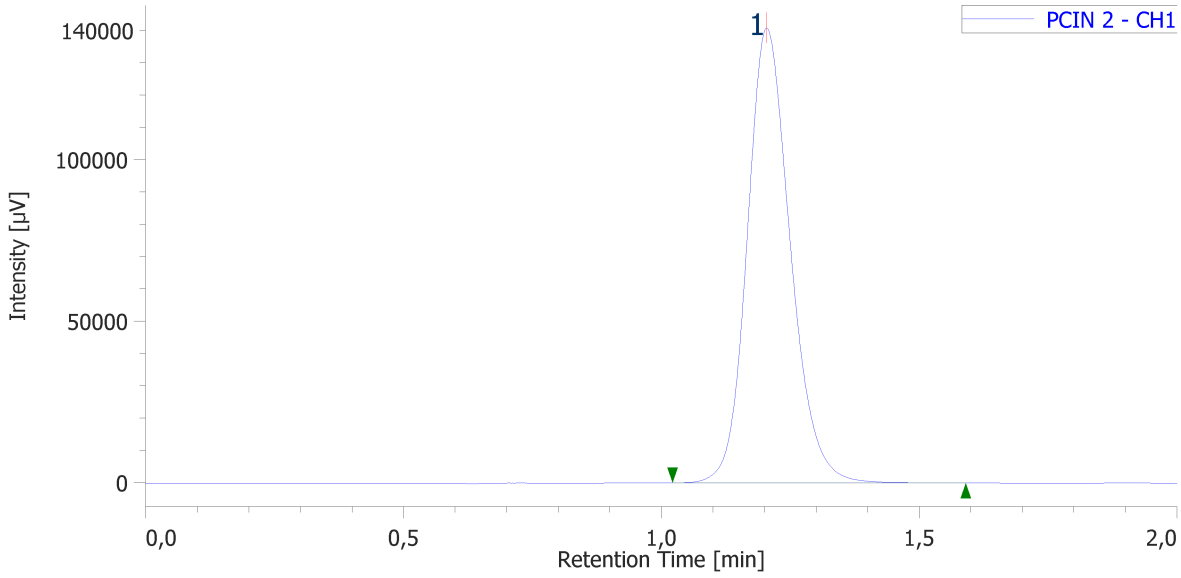

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:55:17
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,203	818234	140742	100,000	100,000	N/A	1044	N/A	1,185	

Creator
Reviewer
Approver

Chromatogram

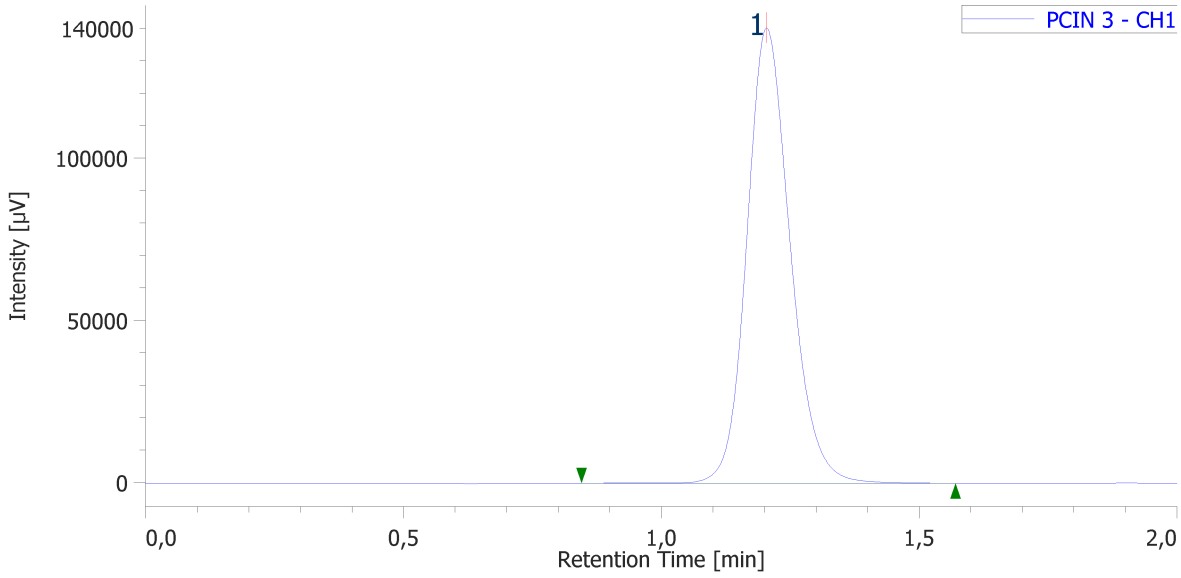

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:57:51
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,203	819248	140230	100,000	100,000	N/A	1034	N/A	1,173	

Creator
Reviewer
Approver

Chromatogram

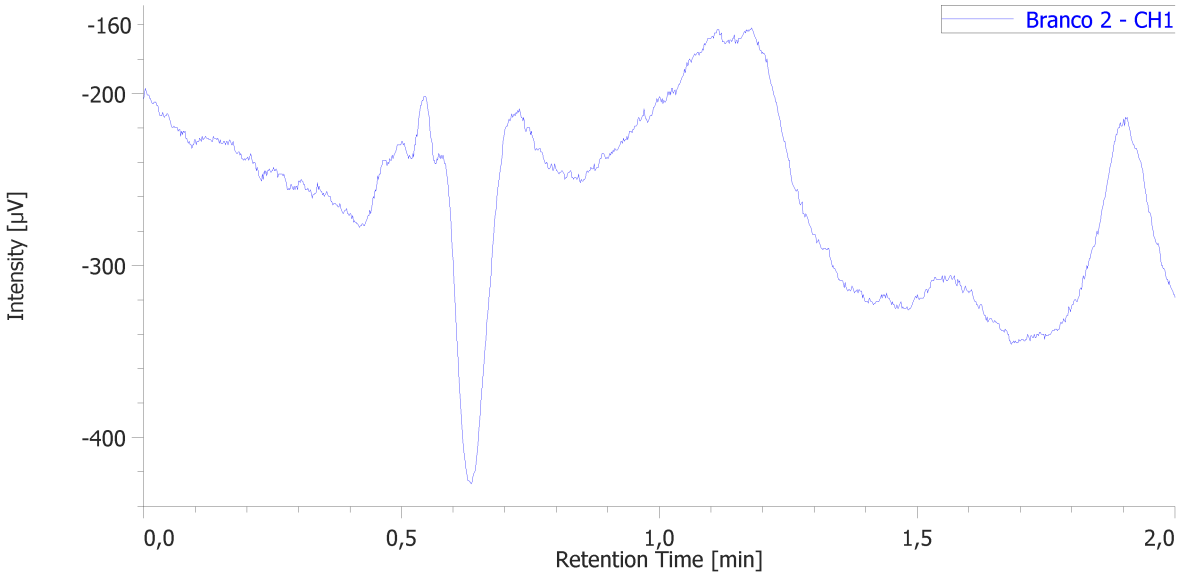


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:41
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:00:25
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

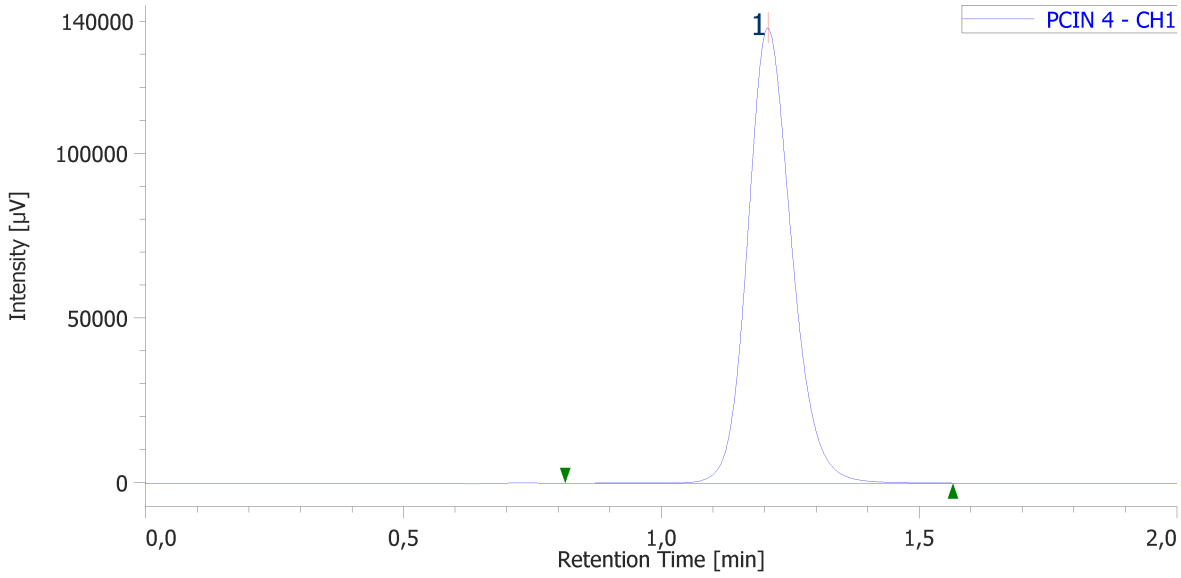

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:41
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:03:02
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,207	819123	138027	100,000	100,000	N/A	1007	N/A	1,151	

Creator
Reviewer
Approver

Chromatogram

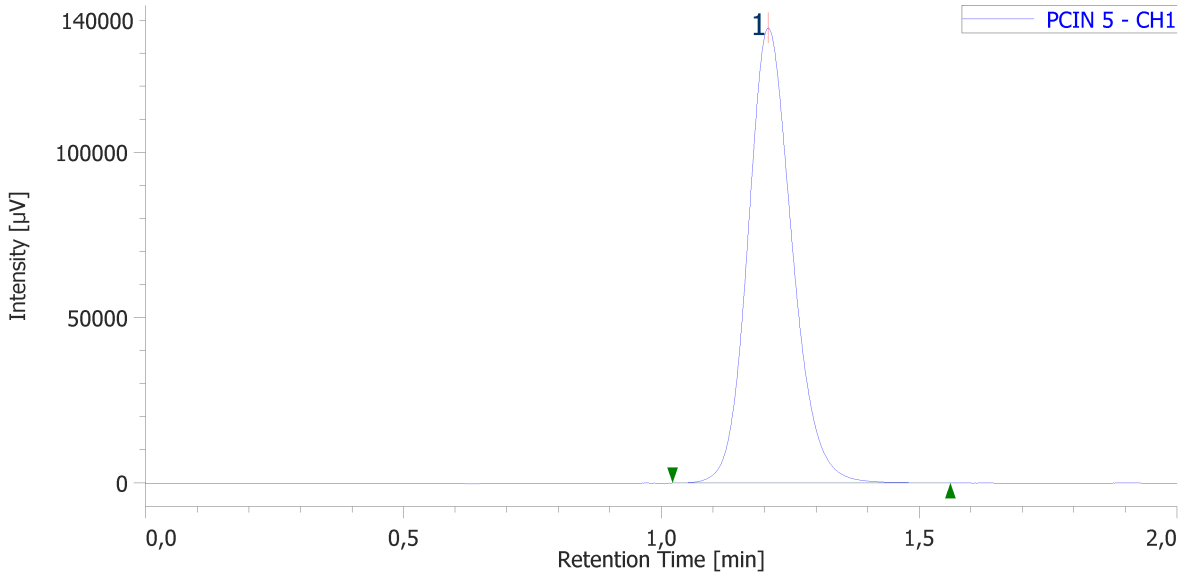

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:41
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:05:36
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,207	819196	137626	100,000	100,000	N/A	996	N/A	1,158	

Creator
Reviewer
Approver

Chromatogram

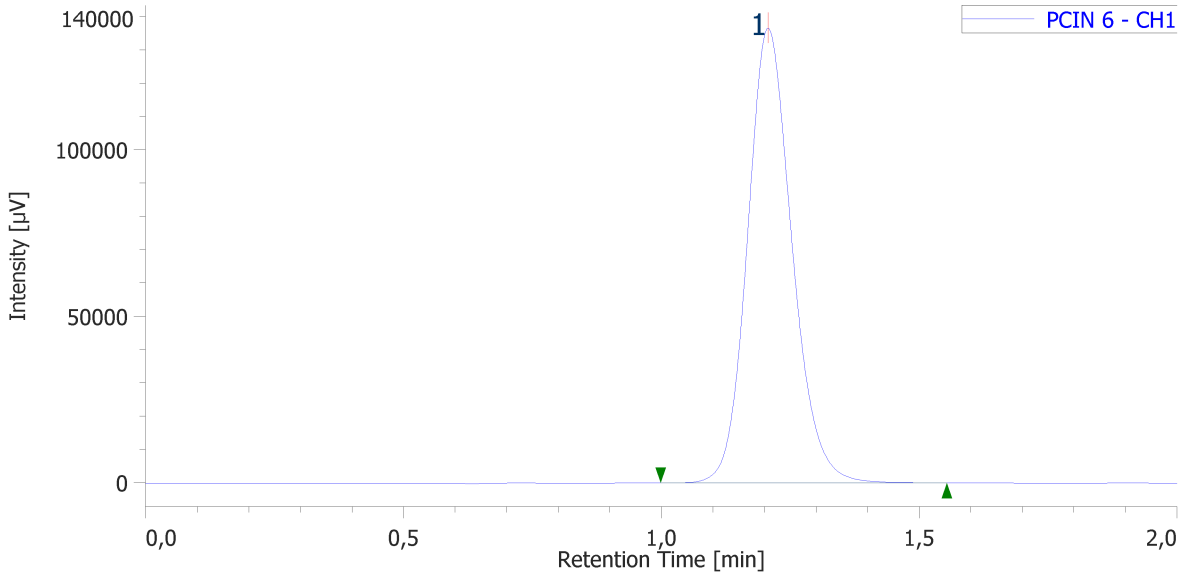

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:41
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:08:10
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,207	819741	136582	100,000	100,000	N/A	979	N/A	1,151	

Creator
Reviewer
Approver

Chromatogram

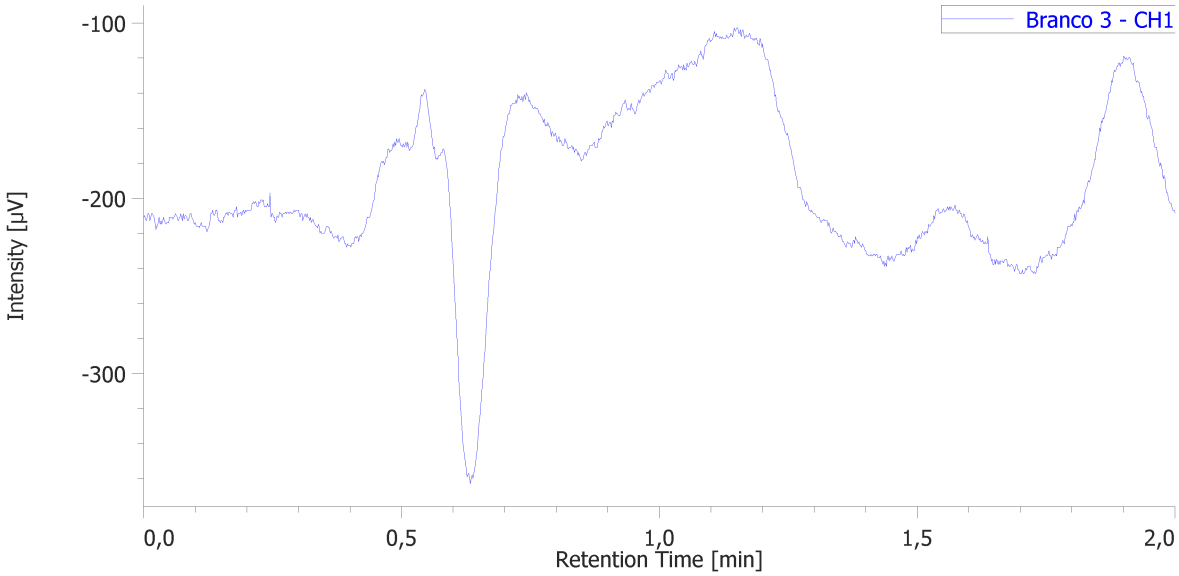


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:41
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:10:47
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

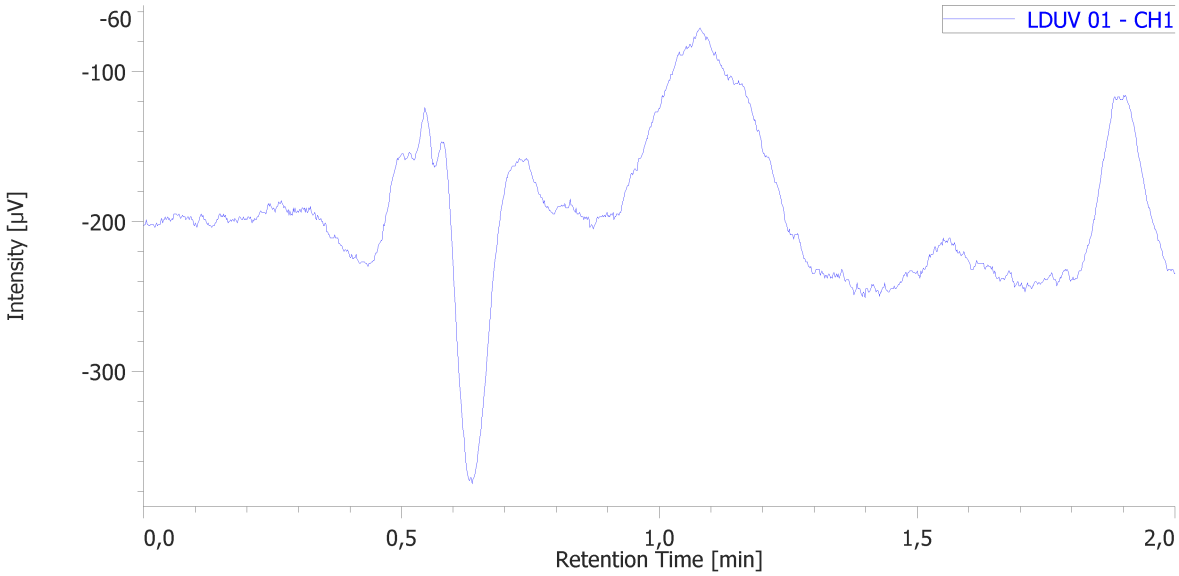


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:39
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 11:54:16
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

Creator
Reviewer
Approver

Chromatogram

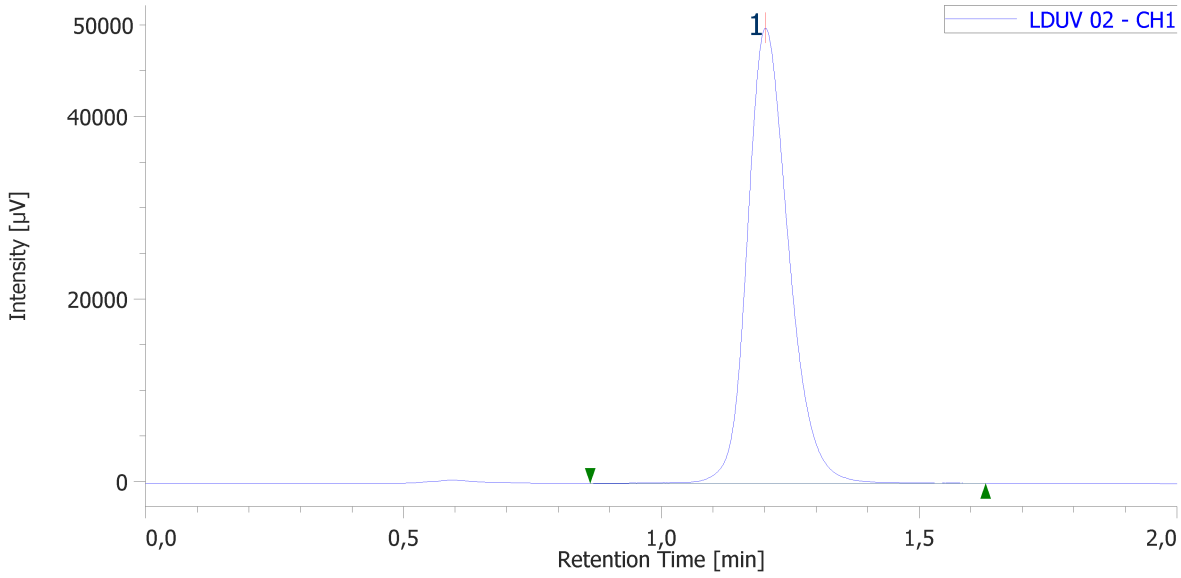

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:39
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 11:56:50
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,202	277038	49831	100,000	100,000	N/A	1146	N/A	1,218	

Creator
Reviewer
Approver

Chromatogram

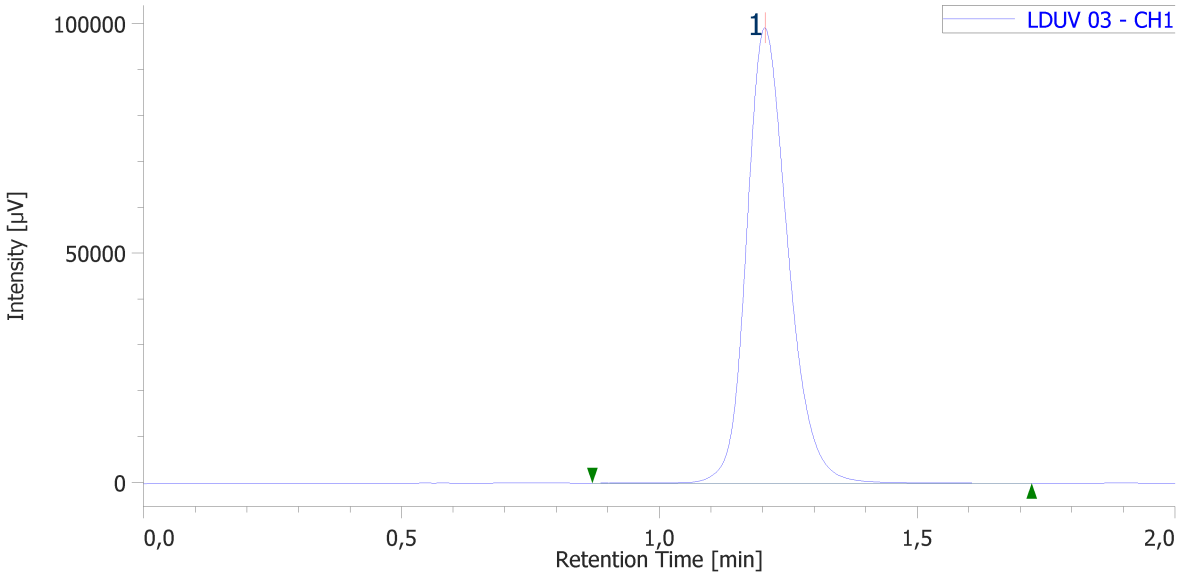

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:39
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 11:59:24
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,205	551724	99122	100,000	100,000	N/A	1149	N/A	1,206	

Creator
Reviewer
Approver

Chromatogram

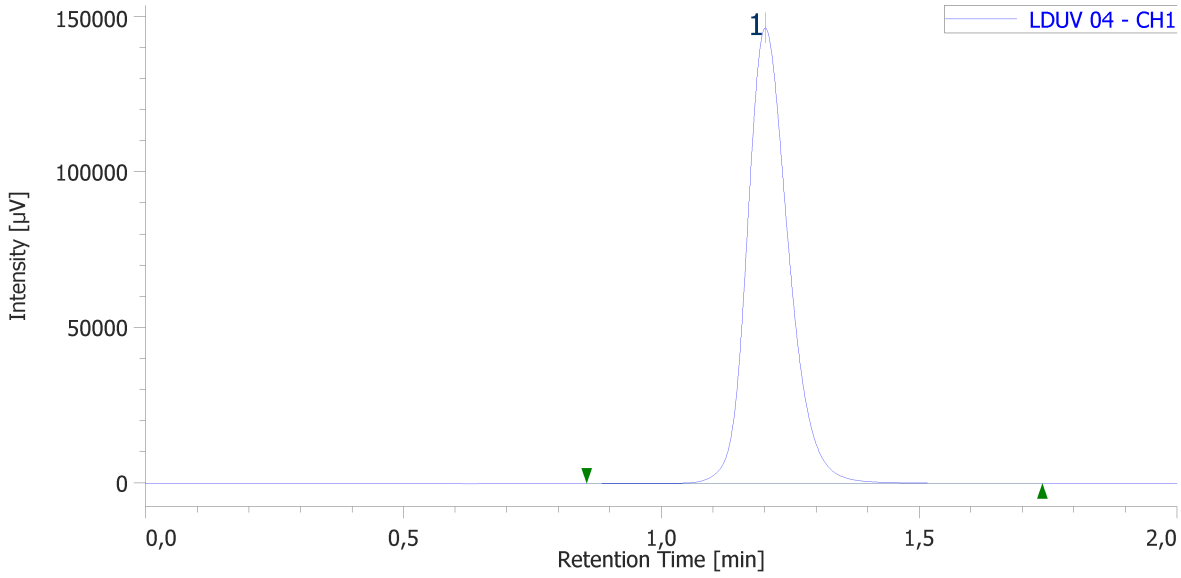

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:39
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:01:59
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,202	815207	146329	100,000	100,000	N/A	1141	N/A	1,214	

Creator
Reviewer
Approver

Chromatogram

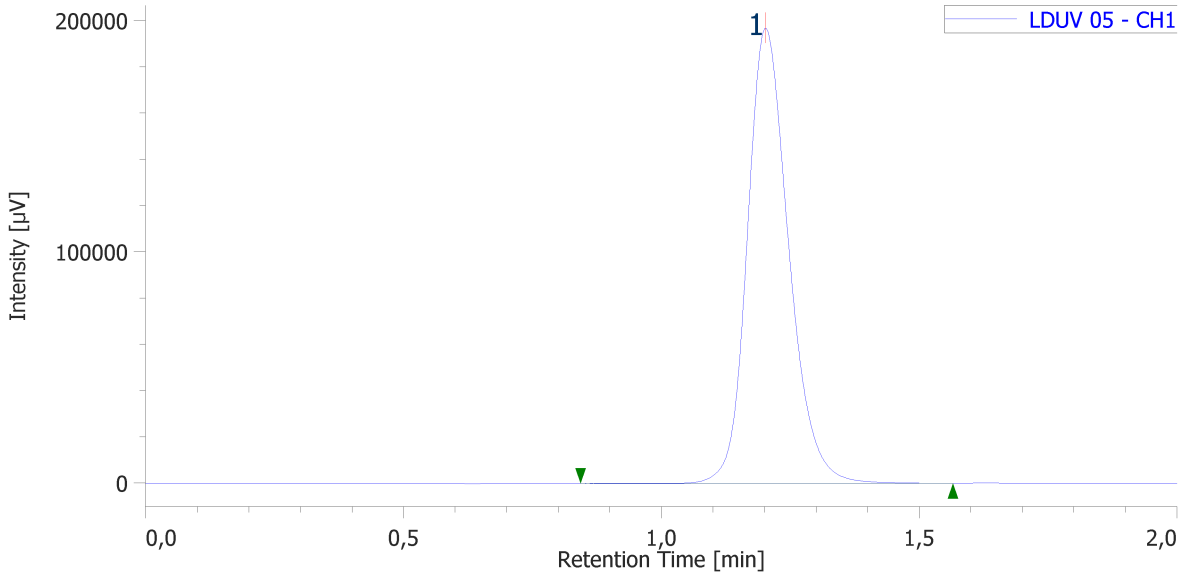

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:04:33
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,202	1097253	196793	100,000	100,000	N/A	1135	N/A	1,215	

Creator
Reviewer
Approver

Chromatogram

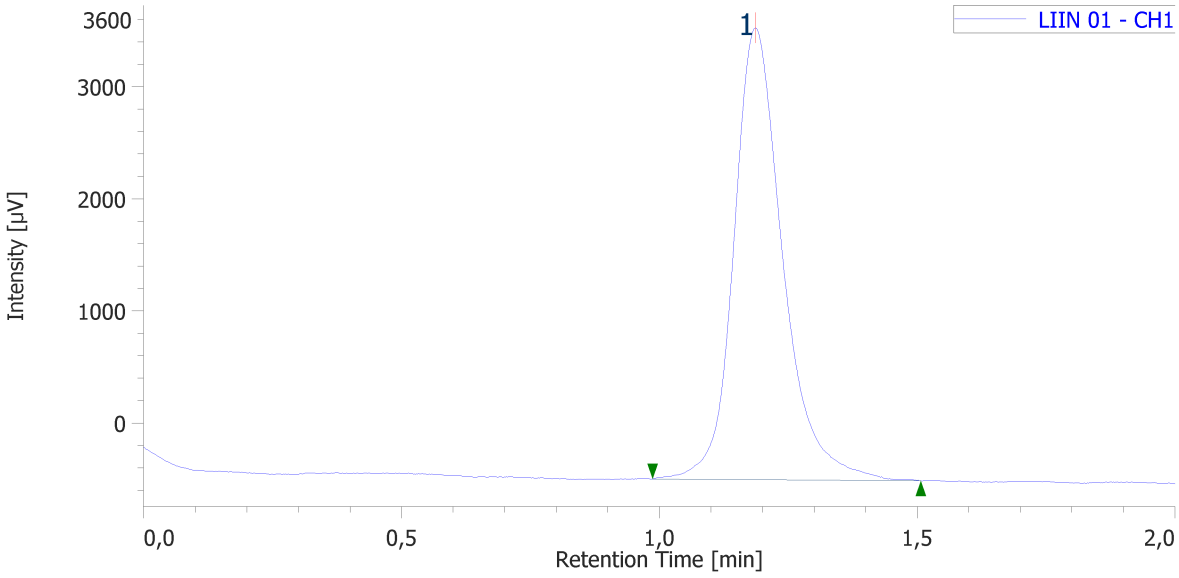

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:06:57
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,187	26588	4026	100,000	100,000	N/A	853	N/A	1,233	

Creator
Reviewer
Approver

Chromatogram

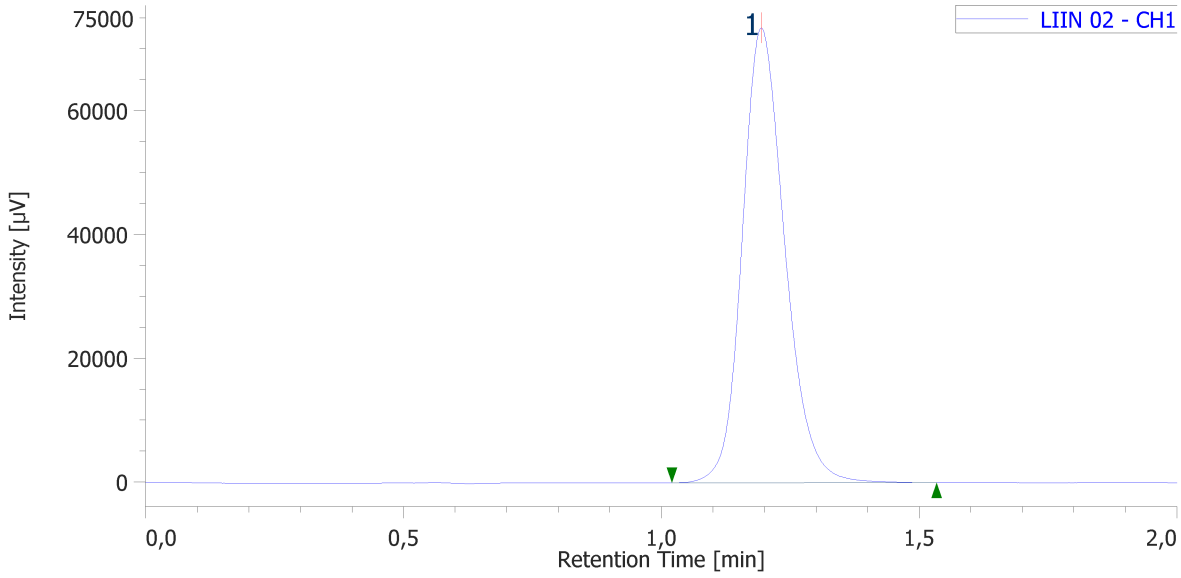

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:09:26
Volume	5,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,193	421658	73458	100,000	100,000	N/A	1053	N/A	1,195	

Creator
Reviewer
Approver

Chromatogram

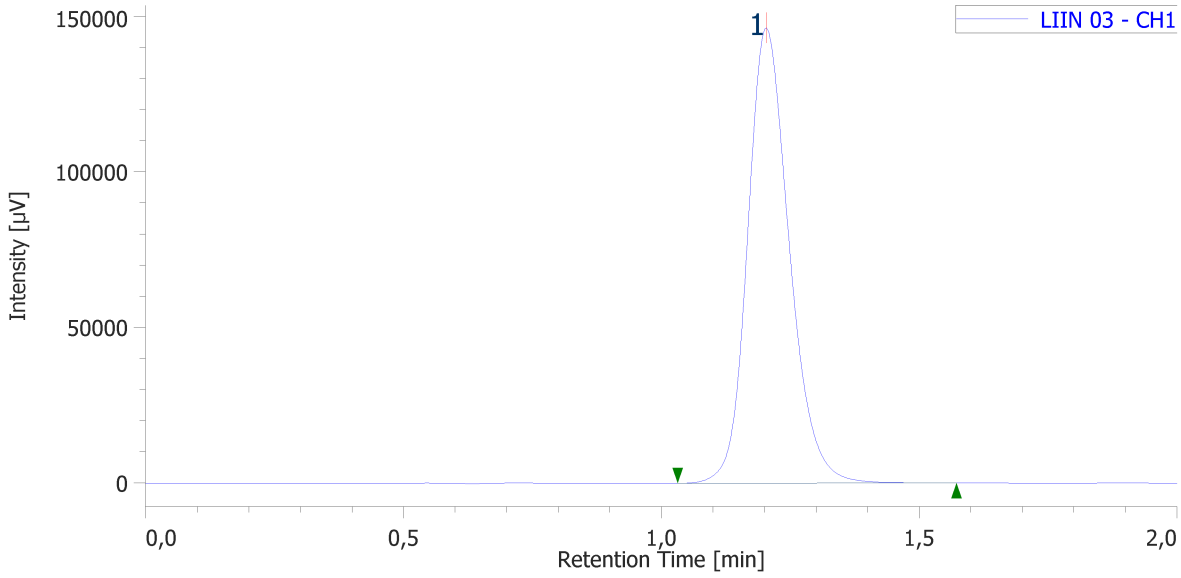

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:12:00
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,203	822357	146308	100,000	100,000	N/A	1117	N/A	1,195	

Creator
Reviewer
Approver

Chromatogram

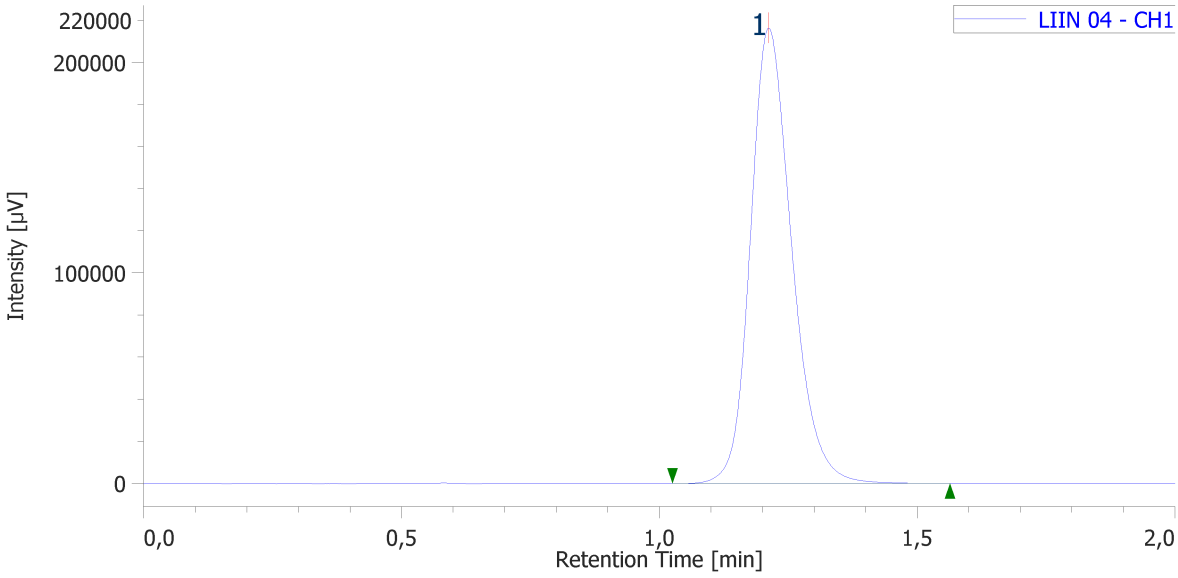

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:14:39
Volume	15,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,212	1203643	216321	100,000	100,000	N/A	1161	N/A	1,221	

Creator
Reviewer
Approver

Chromatogram

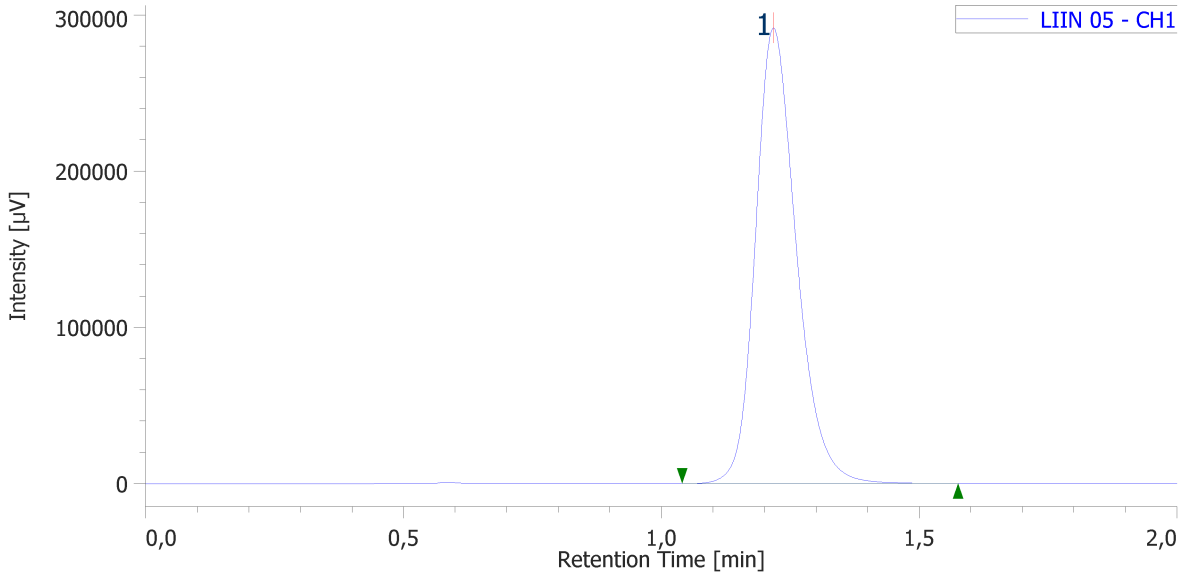

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 13:23:40
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 12:17:24
Volume	20,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	QUALIFICAÇÃO 2025
Control Method	Qualificação 2025
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,217	1607525	291509	100,000	100,000	N/A	1194	N/A	1,244	

Creator
Reviewer
Approver

Chromatogram

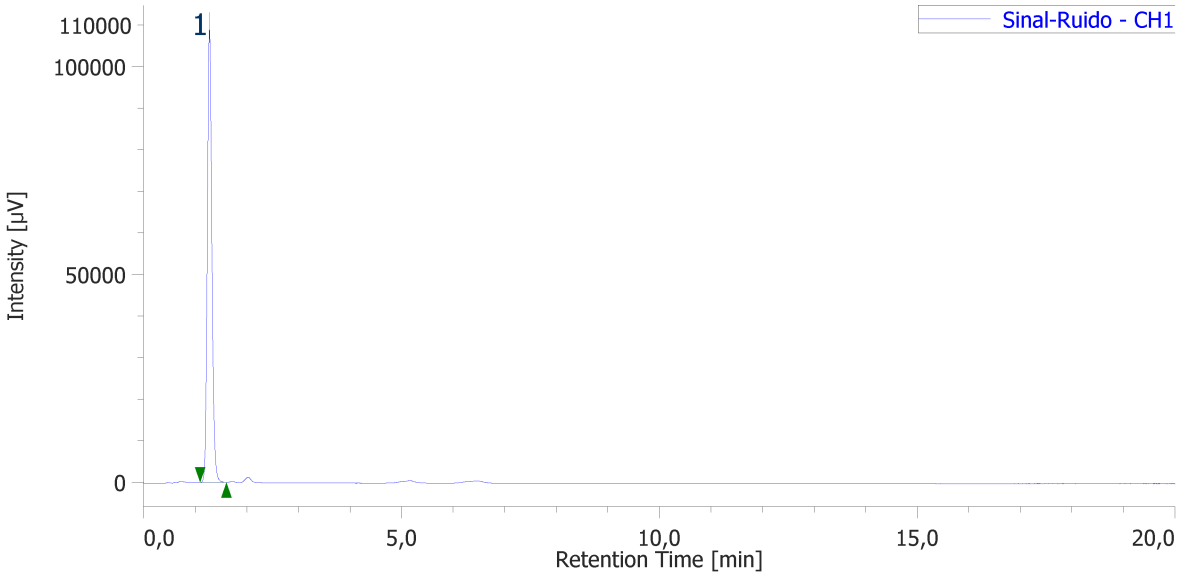

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 14:06:05
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:43:24
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sinal-Ruido 2025
Control Method	Sinal-Ruido
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal-Ruido-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,273	668405	109267	100,000	100,000	N/A	1046	N/A	1,164	

Creator
Reviewer
Approver

Chromatogram

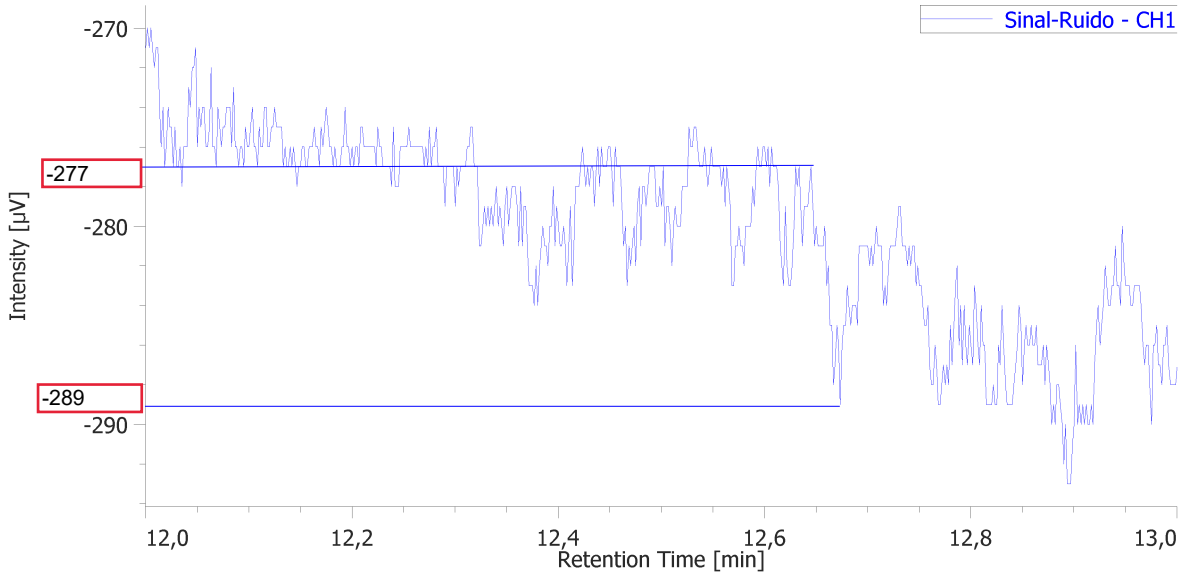

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 14:06:05
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:43:24
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sinal-Ruido 2025
Control Method	Sinal-Ruido
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal-Ruido-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,273	668405	109267	100,000	100,000	N/A	1046	N/A	1,164	

Creator
Reviewer
Approver

Chromatogram

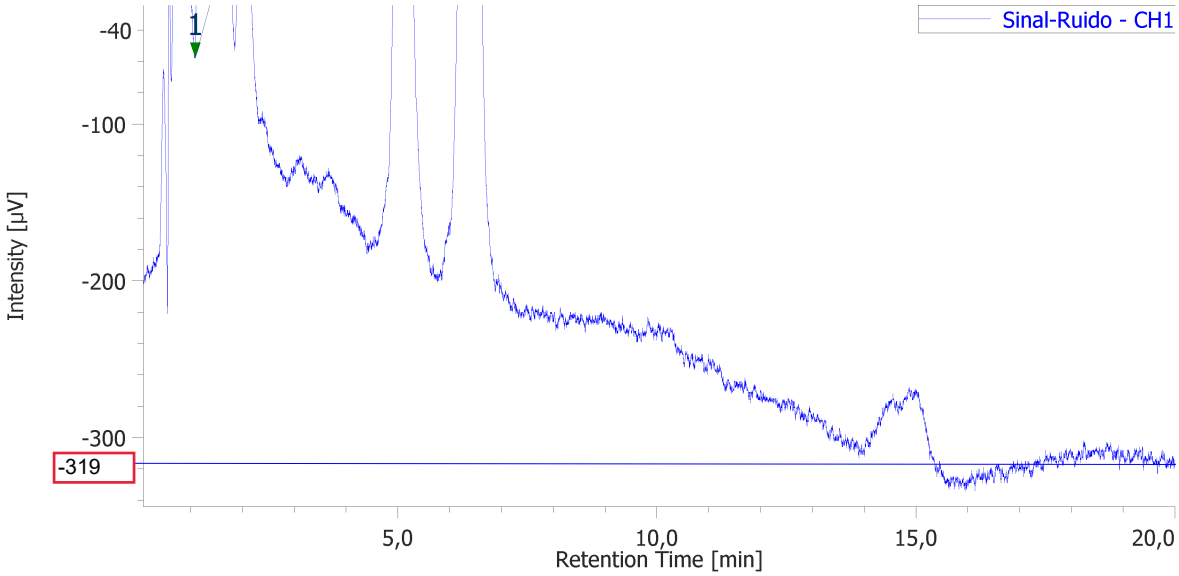

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2025 14:06:05
Description	
HPLC System Name	01-HP-01
Injection Date	08/05/2025 13:43:24
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Sinal-Ruido 2025
Control Method	Sinal-Ruido
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Sinal-Ruido-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,273	668405	109267	100,000	100,000	N/A	1046	N/A	1,164	

Creator
Reviewer
Approver