
Peak Find - Exatidão Do Comprimento De Onda.jws

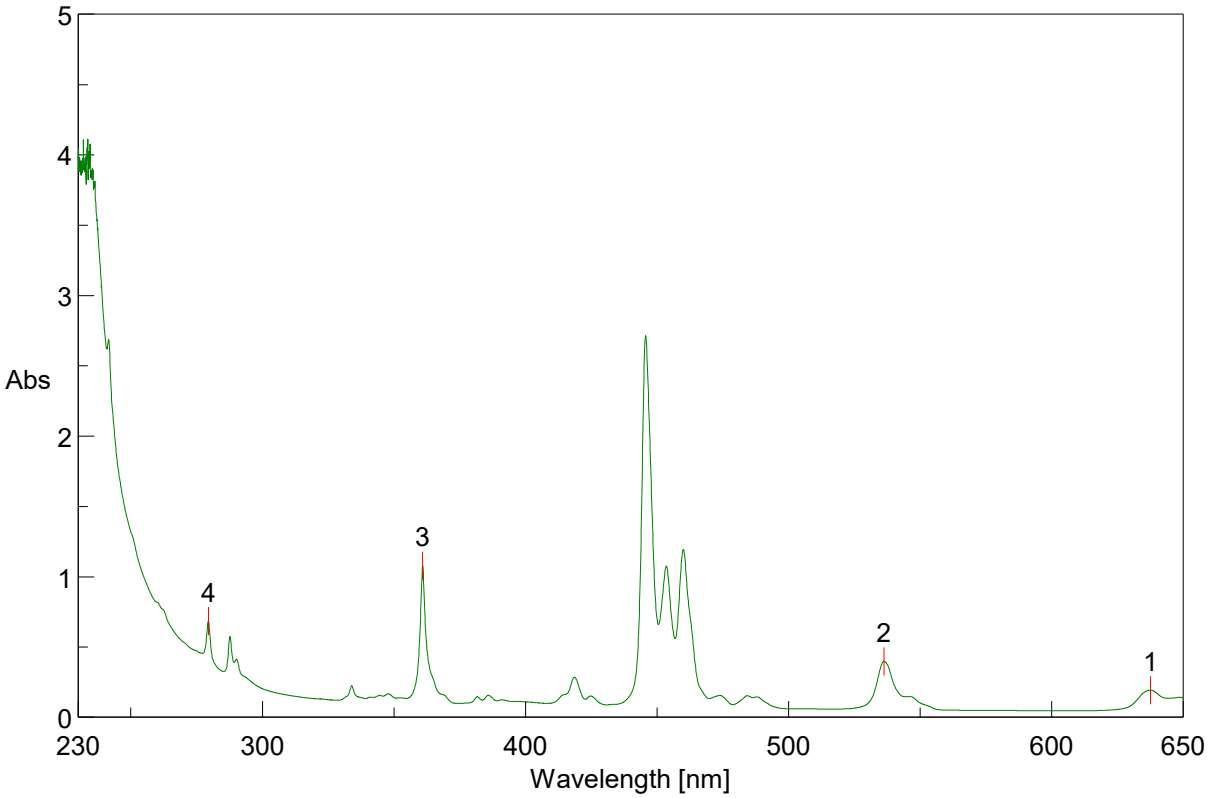

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 12:12
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 12:10
Parameter file	C:\Jasco\2025\Exatidão Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	637.6	0.192061	2	536.3	0.395905
3	360.9	1.0761	4	279.5	0.681632

Exatidão Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	07/05/2025 12:18
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2025\Exatidão Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Sample-1	G1	G1	0.3239
Sample-2	G2	G2	1.0642
Sample-3	G3	G3	0.5019

Creation	QPackSA
Review	
Approval	

Linearidade Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	07/05/2025 12:25
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2025\Linearidade Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Sample-1	G1	G1	0.3261
Sample-2	G2	G2	1.0642
Sample-3	G3	G3	0.5024
Sample-4	G1 + G3	G1 + G3	0.8293
Sample-5	G2 + G3	G2 + G3	1.5682

Creation	QPackSA
Review	
Approval	


Stray Light.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	07/05/2025 12:35
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2025\Stray Light.uvfw
Photometric mode	%T
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	430.0 nm
Wavelength-2	380.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	430.0 nm	380.0 nm
Sample-1	Stray Light	Stray Light	99.0280	0.0189

Creation	QPackSA
Review	
Approval	

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 1.jws

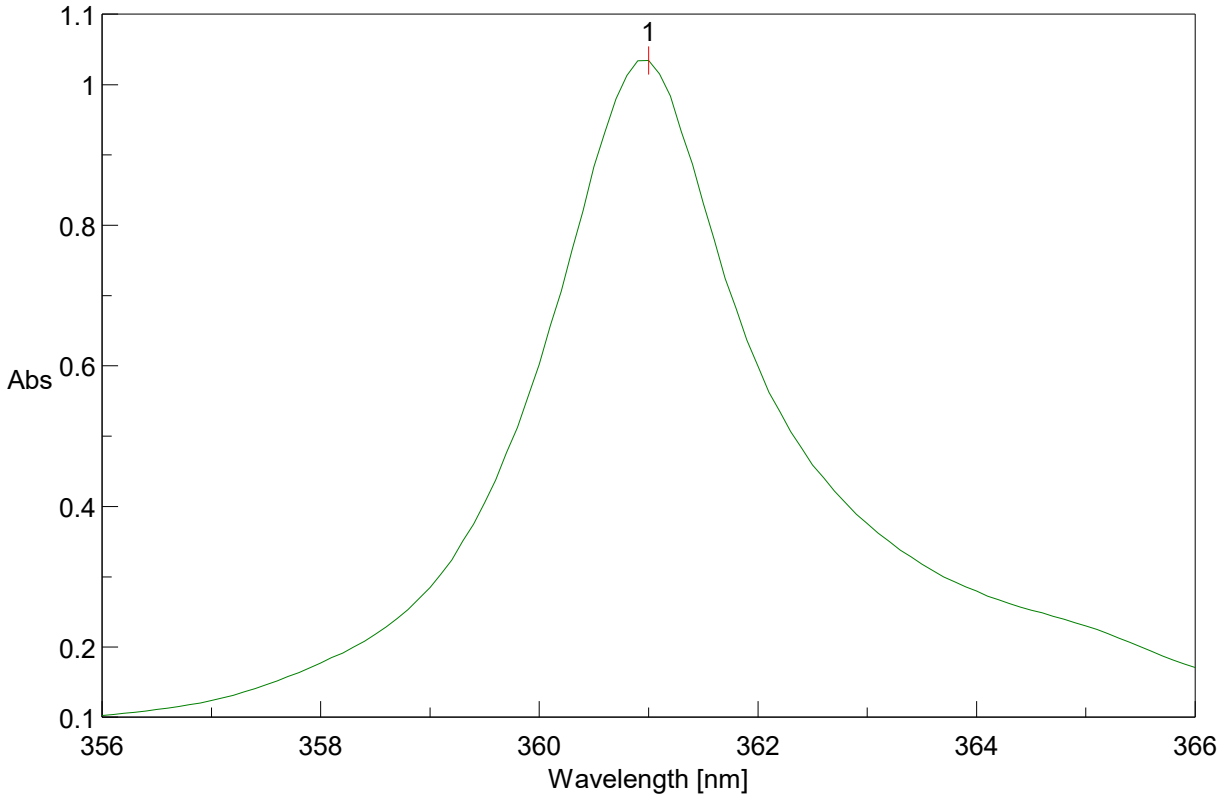

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 12:41
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 12:39
Parameter file	C:\Jasco\2025\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	361	1.03418			

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 2.jws

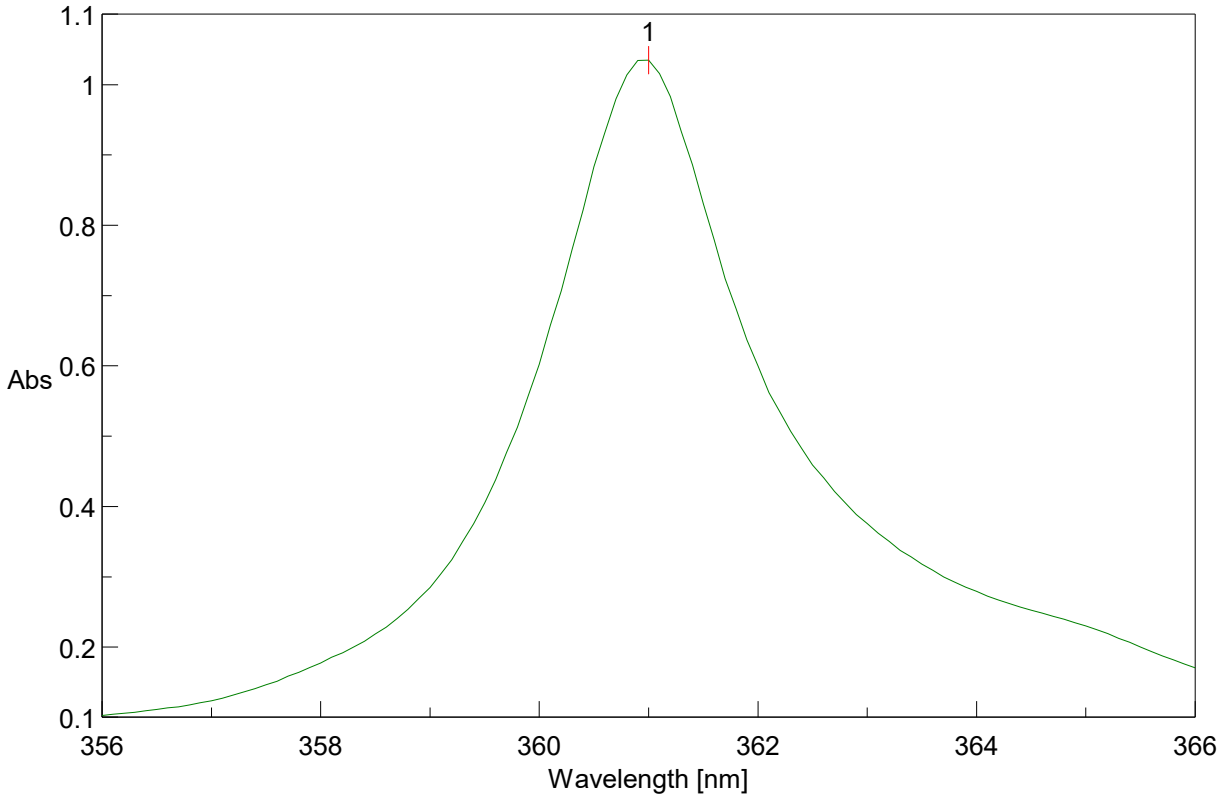

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 12:42
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 12:40
Parameter file	C:\Jasco\2025\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1


Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	361	1.03452			

Creation QPackSA
Review
Approval

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 3.jws

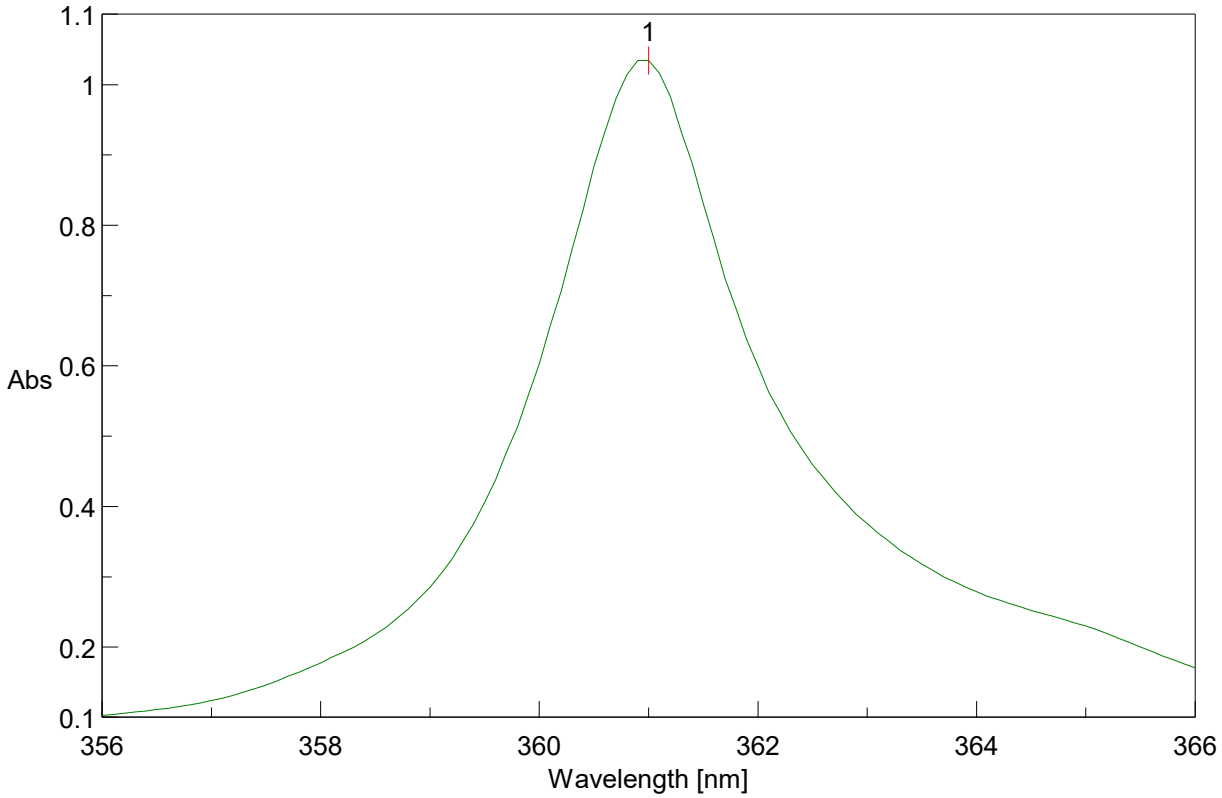

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 12:42
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 12:41
Parameter file	C:\Jasco\2025\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	361	1.03402			

Full Width at Half Maximum - Resolução.jws

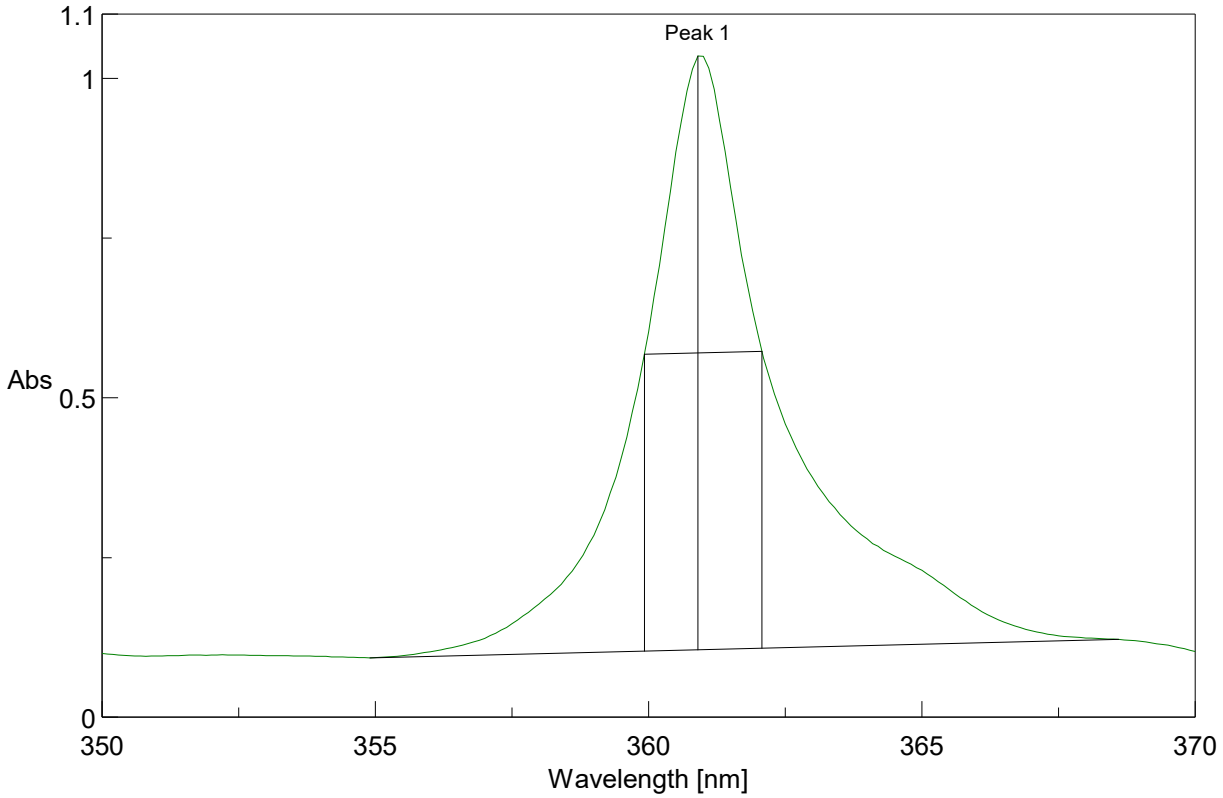

[Result of FWHM Calculation]

Base 1	Base 2	Peak	Height	FWHM
354.9	368.6	360.9	0.928933	2.14864

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 12:46
Date modified	07/05/2025 12:47
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	370 nm
End	350 nm
Data interval	0.1 nm
Data points	201

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 12:46
Parameter file	C:\Jasco\2025\Resolução.uvsp
Photometric mode	Abs
Measurement range	370 - 350 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step

Creation	QPackSA
Review	
Approval	


Repetibilidade Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	07/05/2025 12:51
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2025\Repetibilidade Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	361.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	361.0 nm
Sample-1	Rep. 1	Rep. 1	1.0517
Sample-2	Rep. 2	Rep. 2	1.0515
Sample-3	Rep. 3	Rep. 3	1.0514

Creation	QPackSA
Review	
Approval	

Peak Find - Estabilidade Da Linha De Base.jws

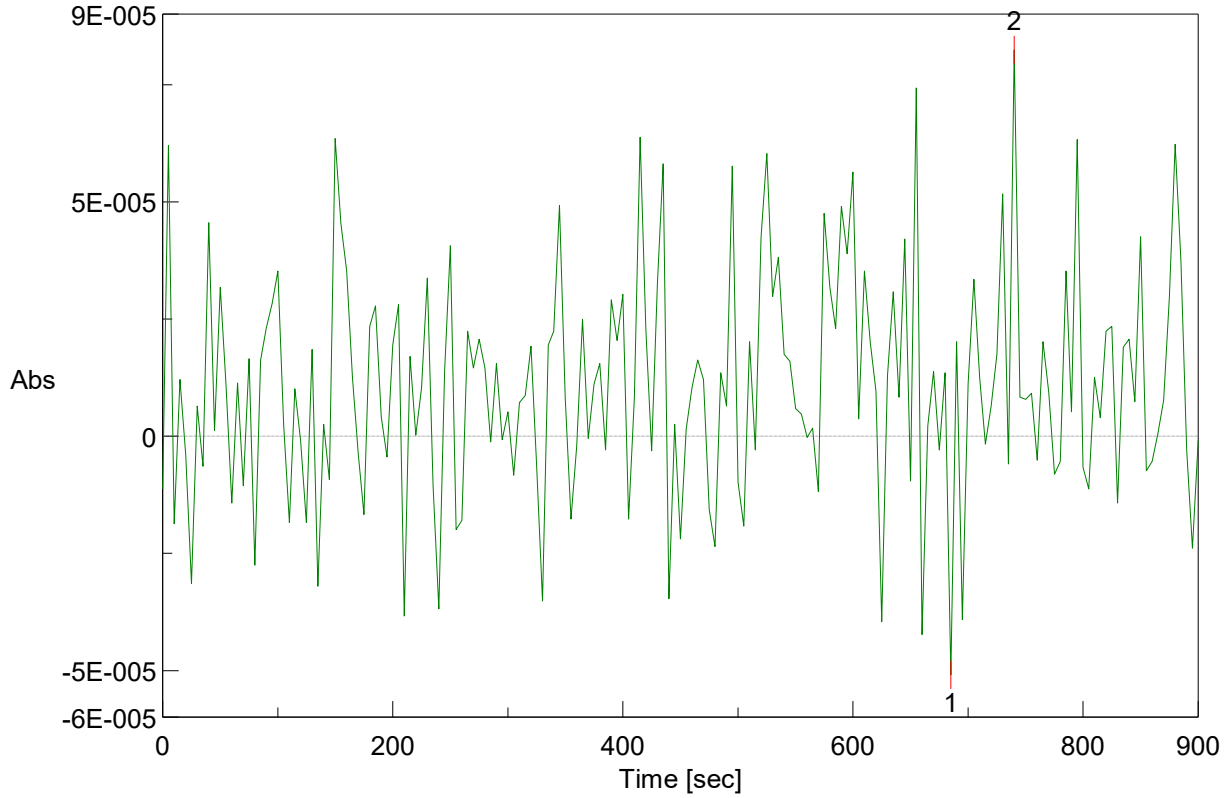

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 13:11
Date modified	07/05/2025 13:12
Data array type	Linear data array
Horizontal axis	Time [sec]
Vertical axis	Abs
Start	0 sec
End	900 sec
Data interval	5 sec
Data points	181

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 13:09
Parameter file	C:\Jasco\2025\Estabilidade Da Linha De Base.uvtm
Photometric mode	Abs
Measurement range	0 - 900 sec
Data interval	5 sec
UV/Vis bandwidth	1.0 nm
Response	0.96 sec
Monitor wavelength	250 nm
Change source at	340 nm
Light source	D2/WI
Correction	Blank

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	685	-5.09785E-005	2	740	8.2378E-005

Peak Find - Uniformidade Da Linha De Base.jws

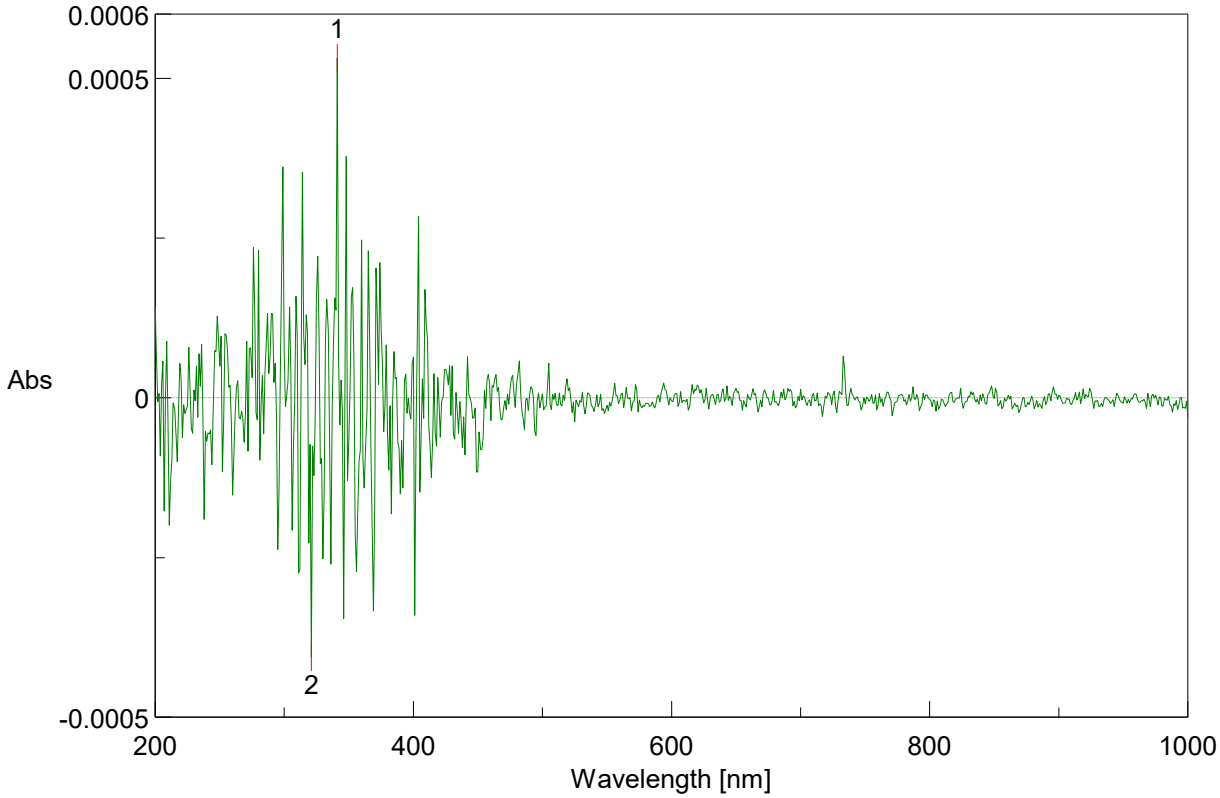

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	07/05/2025 13:20
Date modified	07/05/2025 13:20
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	1000 nm
End	200 nm
Data interval	1 nm
Data points	801

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	07/05/2025 13:20
Parameter file	C:\Jasco\2025\Uniformidade Da Linha De Base.uvsp
Photometric mode	Abs
Measurement range	1000 - 200 nm
Data interval	1 nm
Bandwidth	1.0 nm
Response	0.24 sec
Scan mode	Continuous
Scan speed	400 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	Baseline
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	341	0.000531396	2	321	-0.000405979