
EDUV PDA_1,0667.JWS

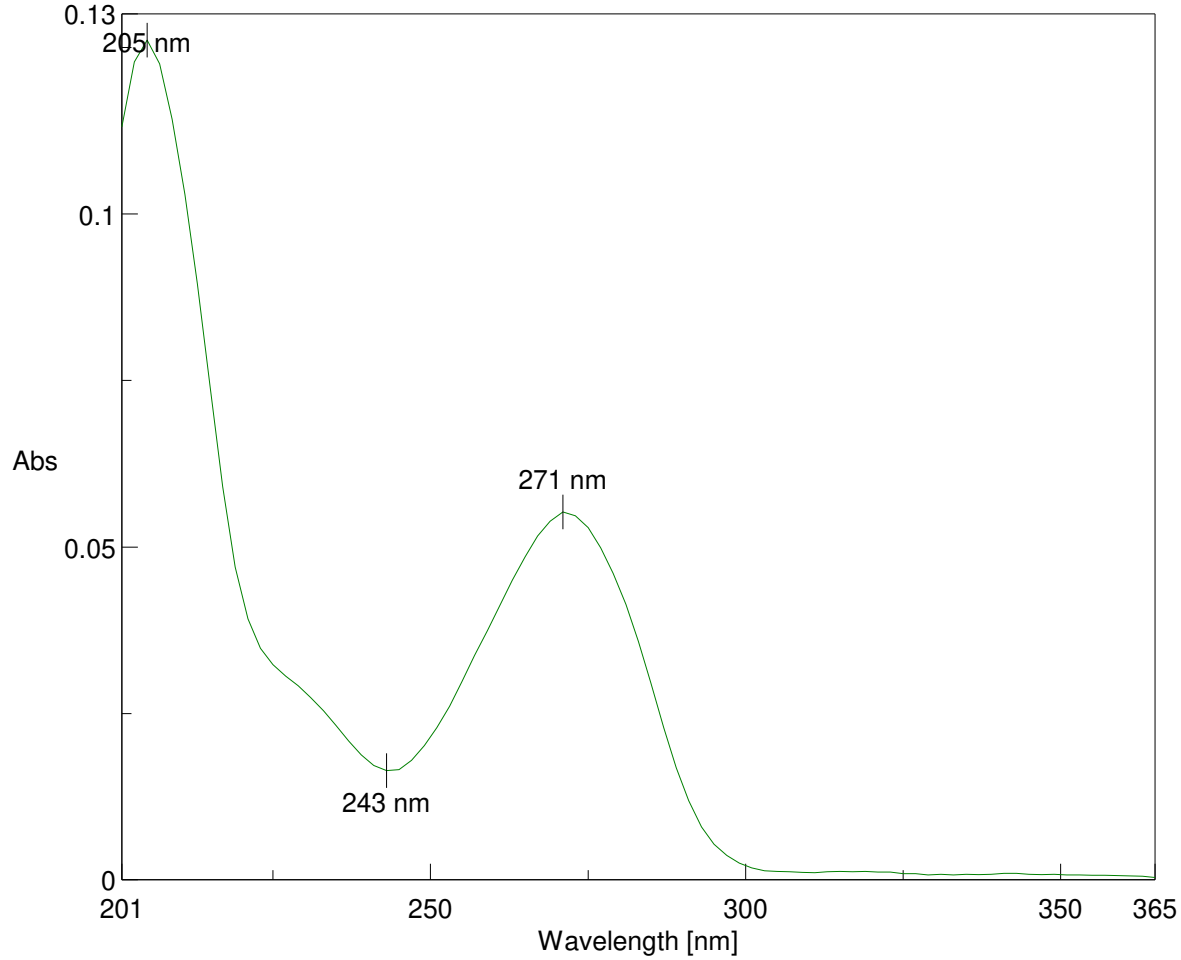

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	08/05/2024 10:47
Date modified	08/05/2024 10:55

EDUV PDA_1,0667.JWS


[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	201 nm
End	365 nm
Data interval	2 nm
Data points	83

[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	0000000000
ROM version	V2.36

Chromatogram

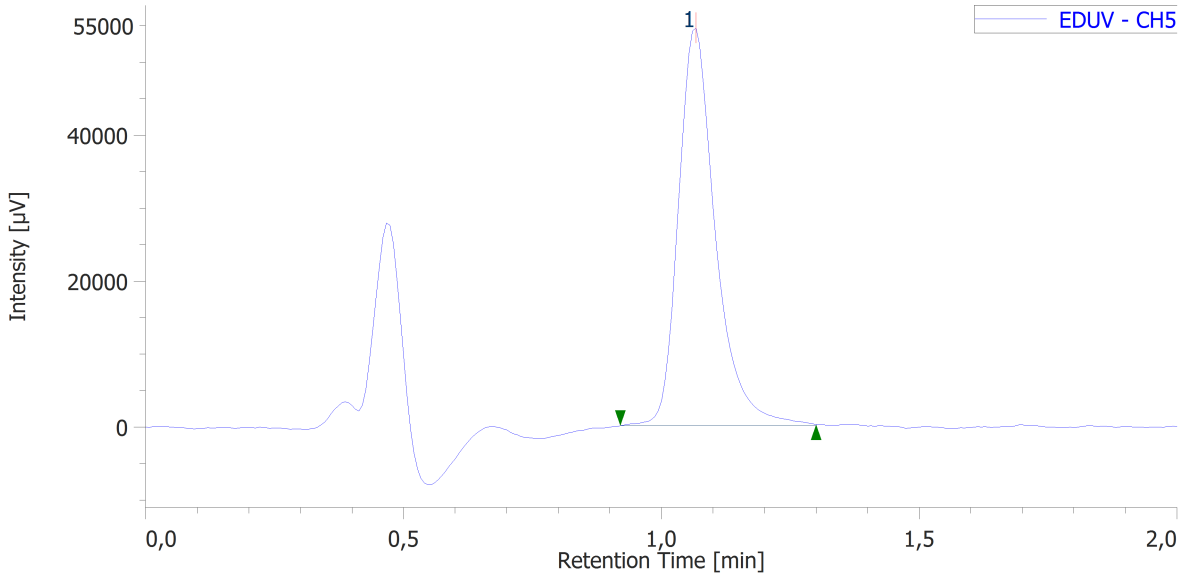

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 10:49:53
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 10:47:50
Volume	10,0 [µL]
Sample #	1
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	EDUV-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,067	273674	54464	100,000	100,000	N/A	1180	N/A	1,305	

Creator
Reviewer
Approver

Chromatogram

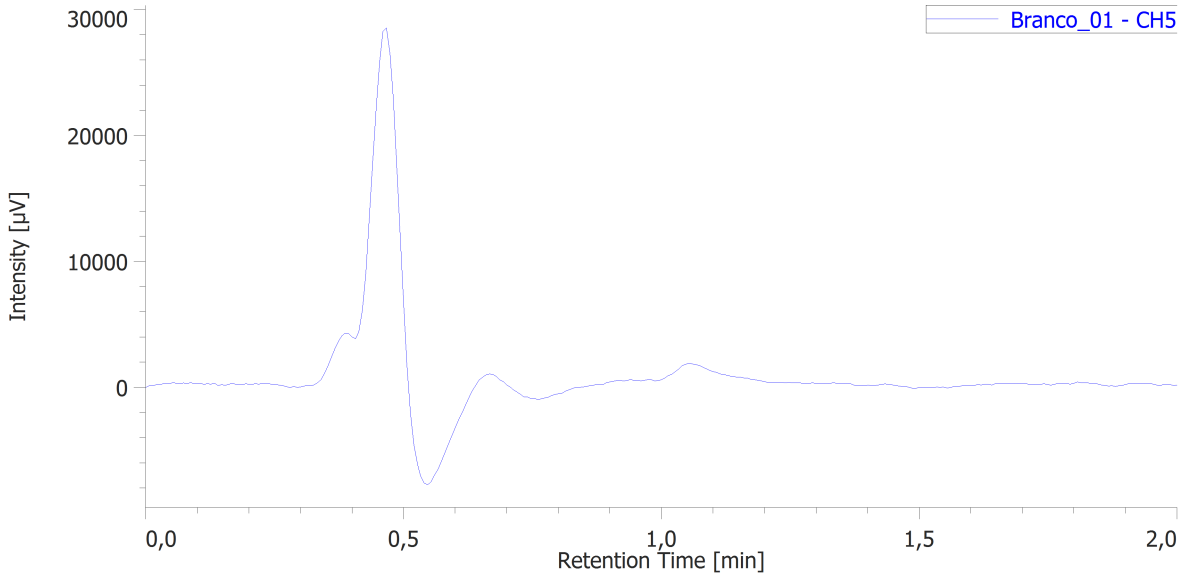


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 10:52:37
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 10:50:35
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

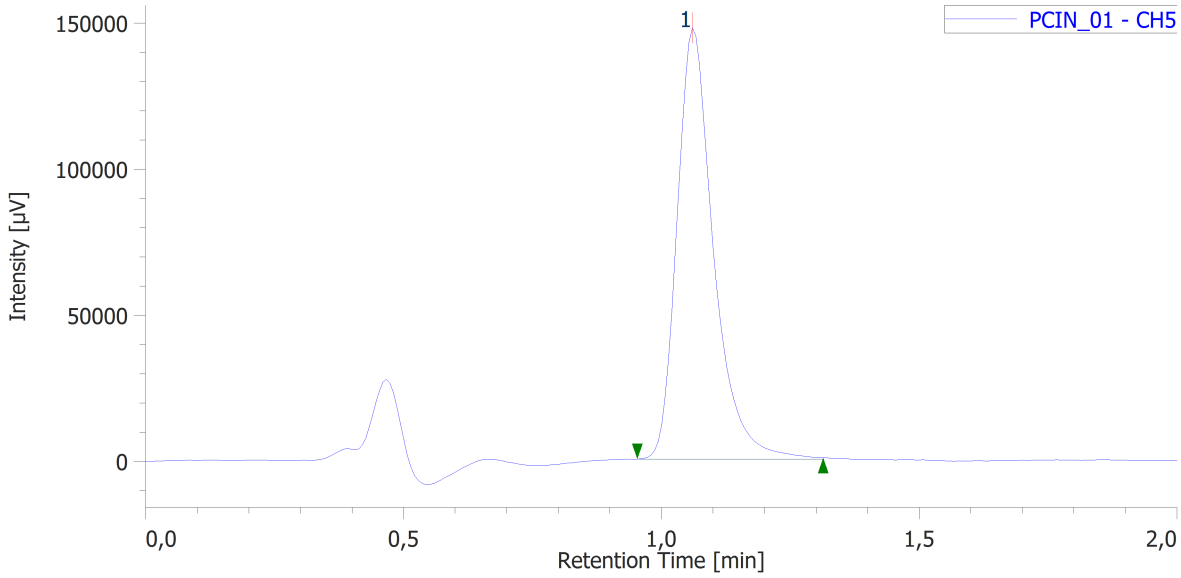

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 10:55:21
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 10:53:19
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,060	726870	147466	100,000	100,000	N/A	1204	N/A	1,376	

Creator
Reviewer
Approver

Chromatogram

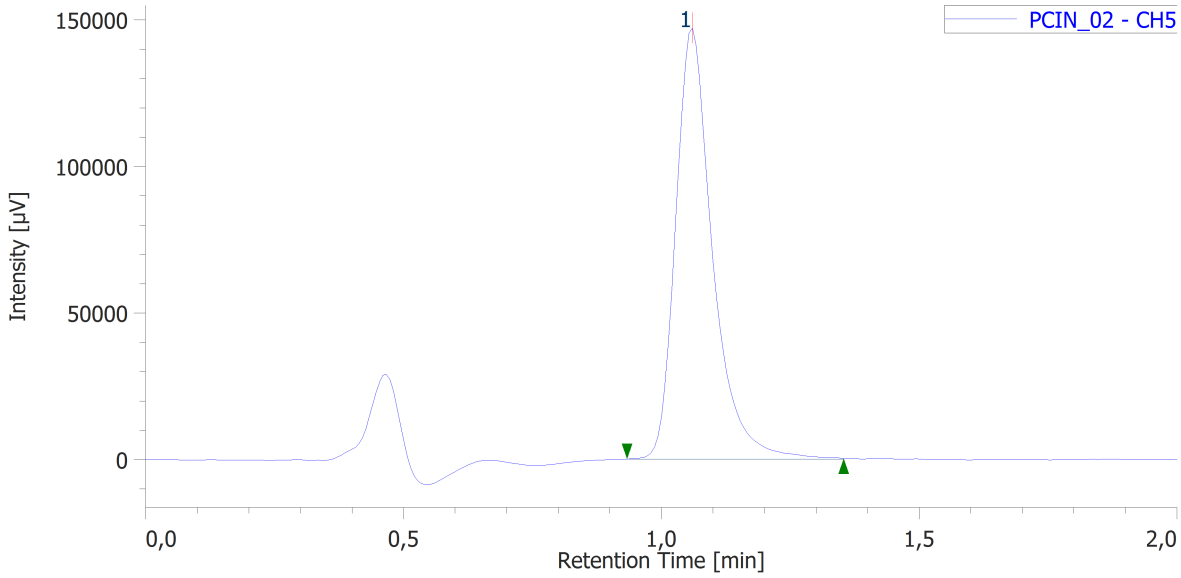

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 10:58:06
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 10:56:04
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,060	730985	146993	100,000	100,000	N/A	1195	N/A	1,338	

Creator
Reviewer
Approver

Chromatogram

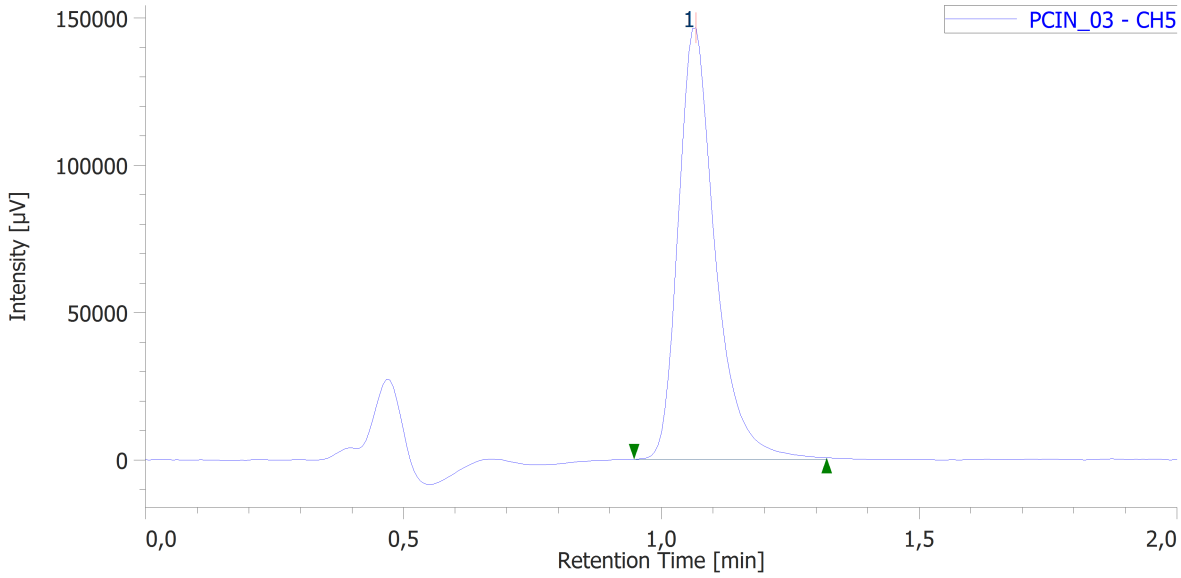

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:00:50
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 10:58:48
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,067	731445	146296	100,000	100,000	N/A	1190	N/A	1,306	

Creator
Reviewer
Approver

Chromatogram

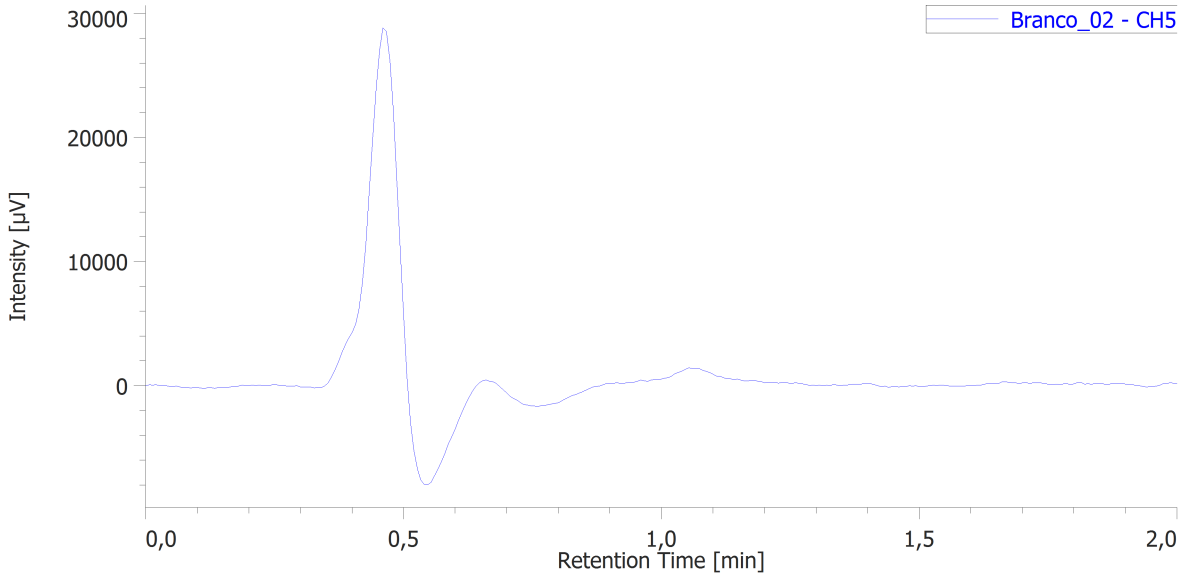


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:03:34
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:01:33
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

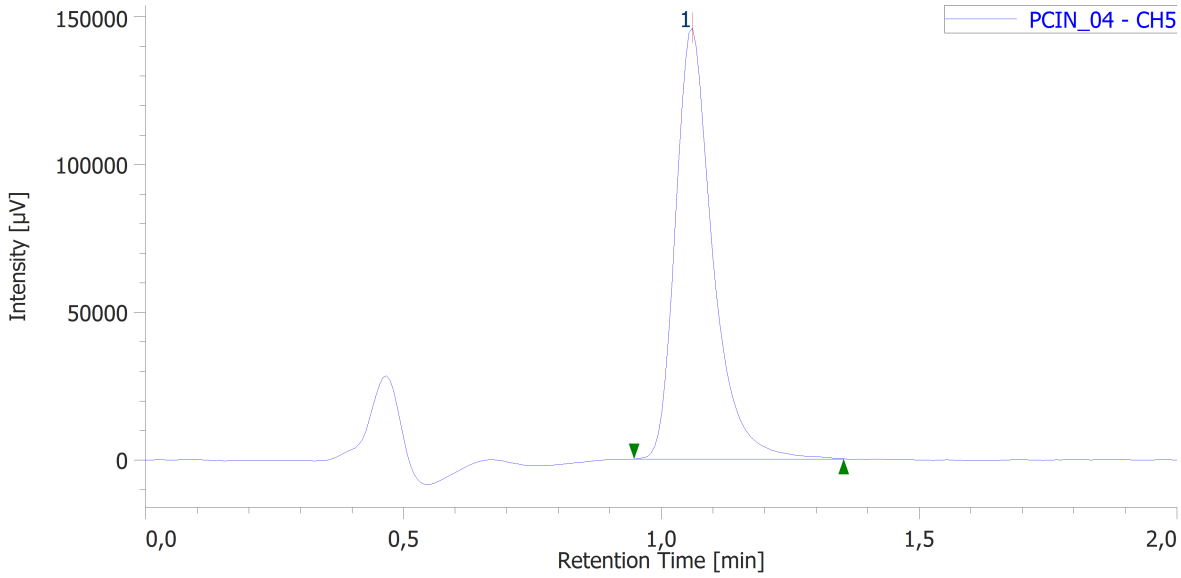

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:06:18
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:04:17
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,060	729802	145713	100,000	100,000	N/A	1170	N/A	1,337	

Creator
Reviewer
Approver

Chromatogram

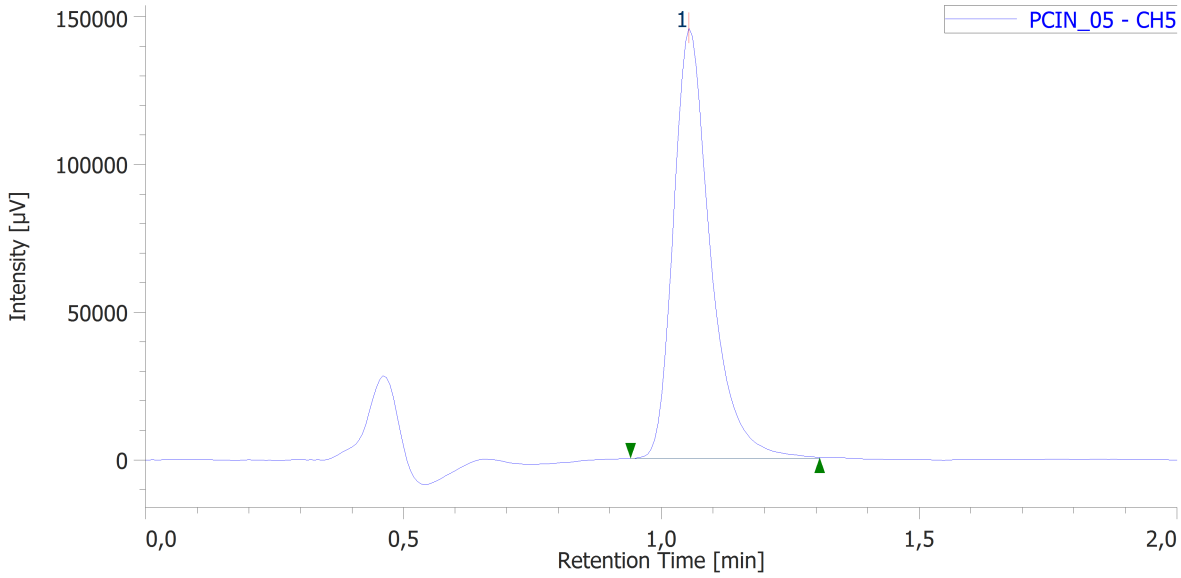

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:09:04
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:07:02
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,053	726419	145594	100,000	100,000	N/A	1165	N/A	1,393	

Creator
Reviewer
Approver

Chromatogram

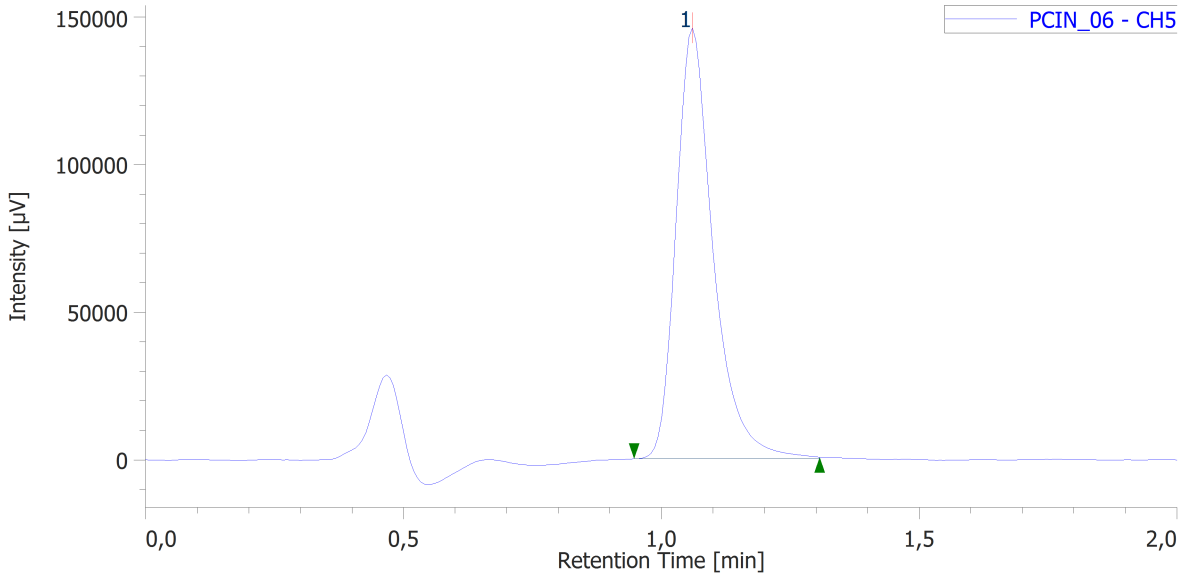

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:11:48
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:09:46
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,060	730538	145813	100,000	100,000	N/A	1172	N/A	1,363	

Creator
Reviewer
Approver

Chromatogram

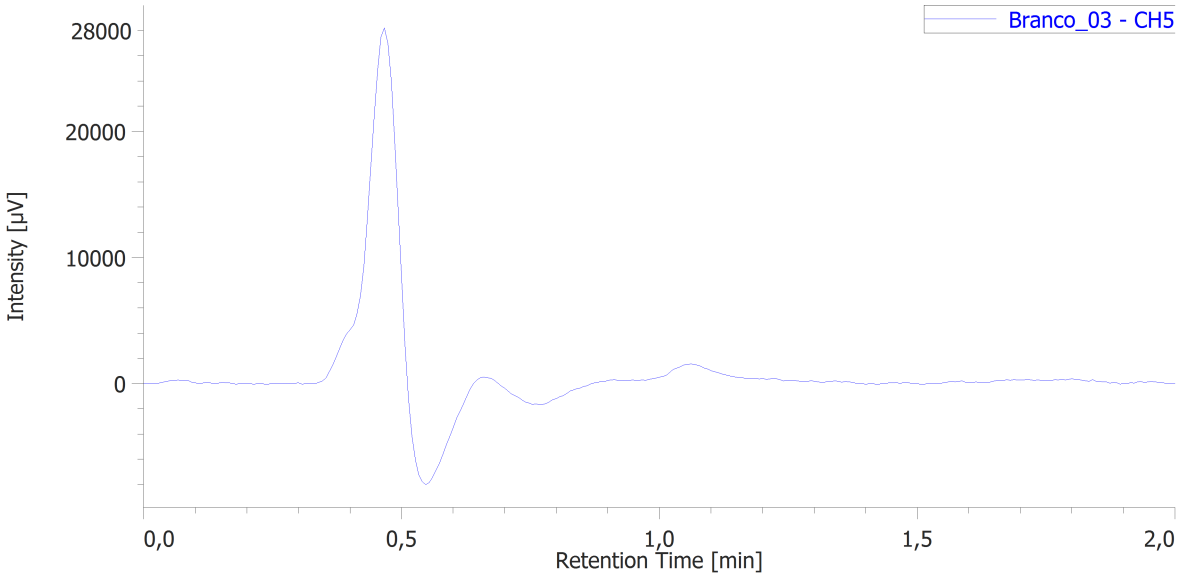


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:14:32
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:12:31
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	

Creator QPackSA
Reviewer
Approver

Chromatogram

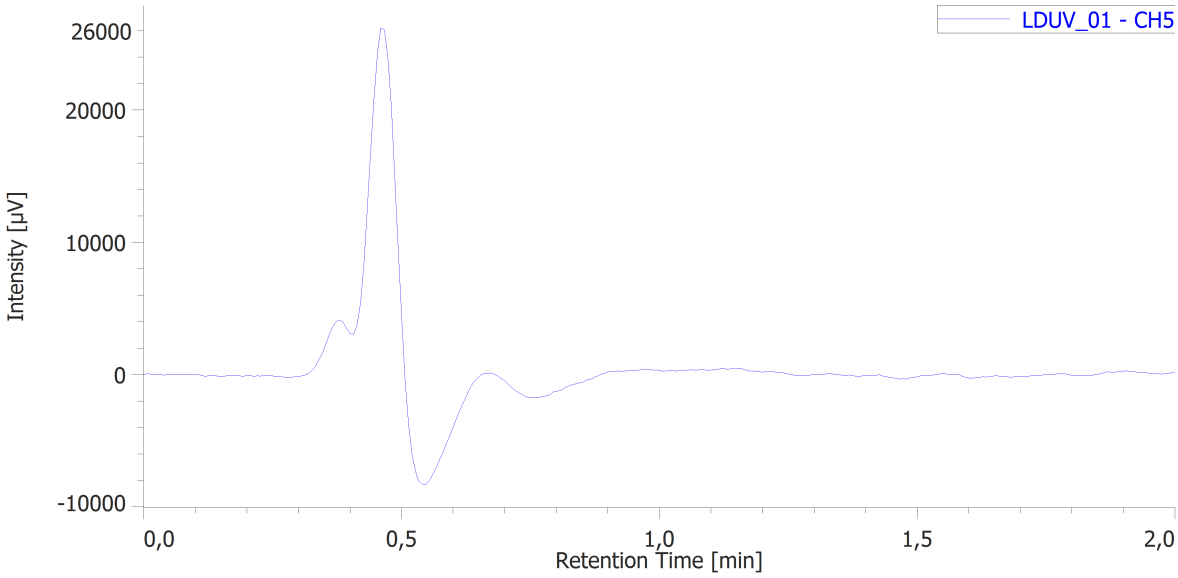


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:17:20
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:15:17
Volume	10,0 [µL]
Sample #	4
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

Creator
Reviewer
Approver

Chromatogram

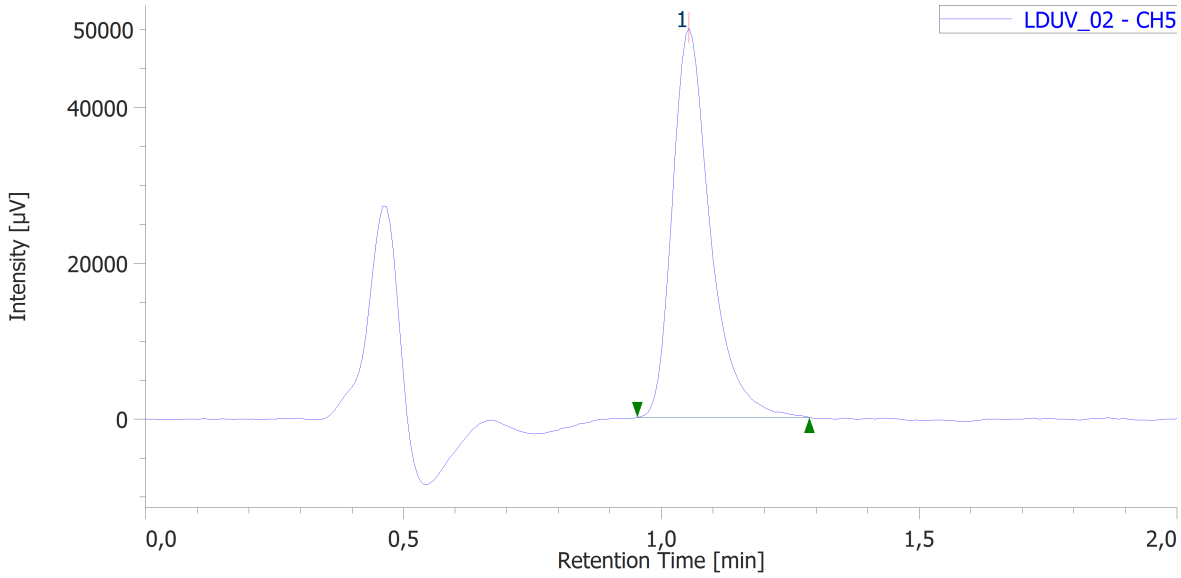

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:20:04
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:18:02
Volume	10,0 [µL]
Sample #	5
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,053	255368	49972	100,000	100,000	N/A	1101	N/A	1,383	

Creator
Reviewer
Approver

Chromatogram

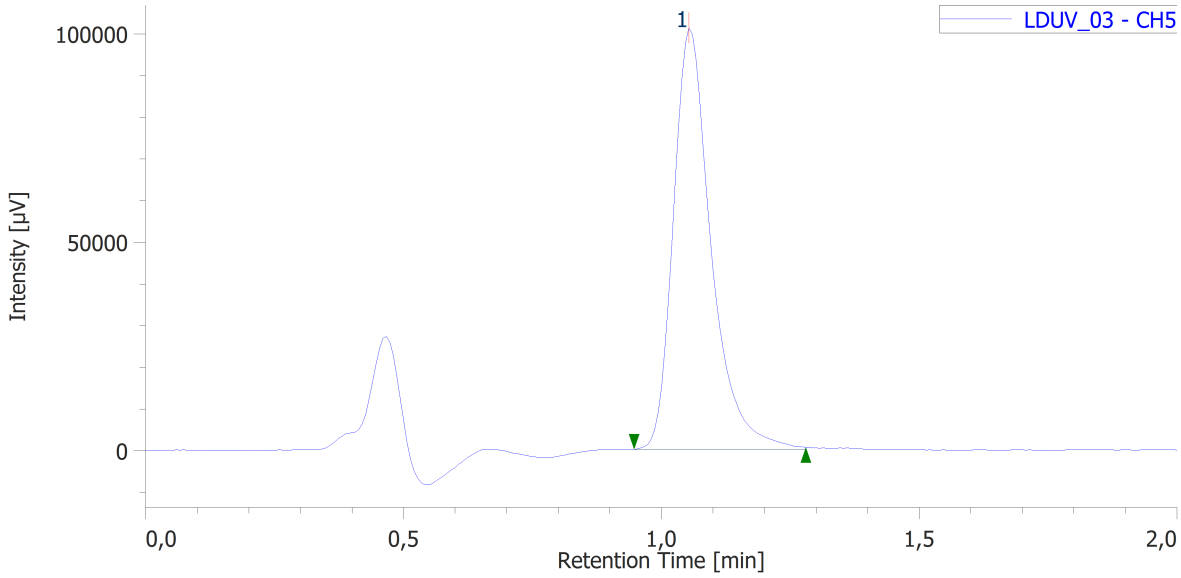

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:22:50
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:20:48
Volume	10,0 [µL]
Sample #	6
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,053	514619	101041	100,000	100,000	N/A	1121	N/A	1,414	

Creator
Reviewer
Approver

Chromatogram

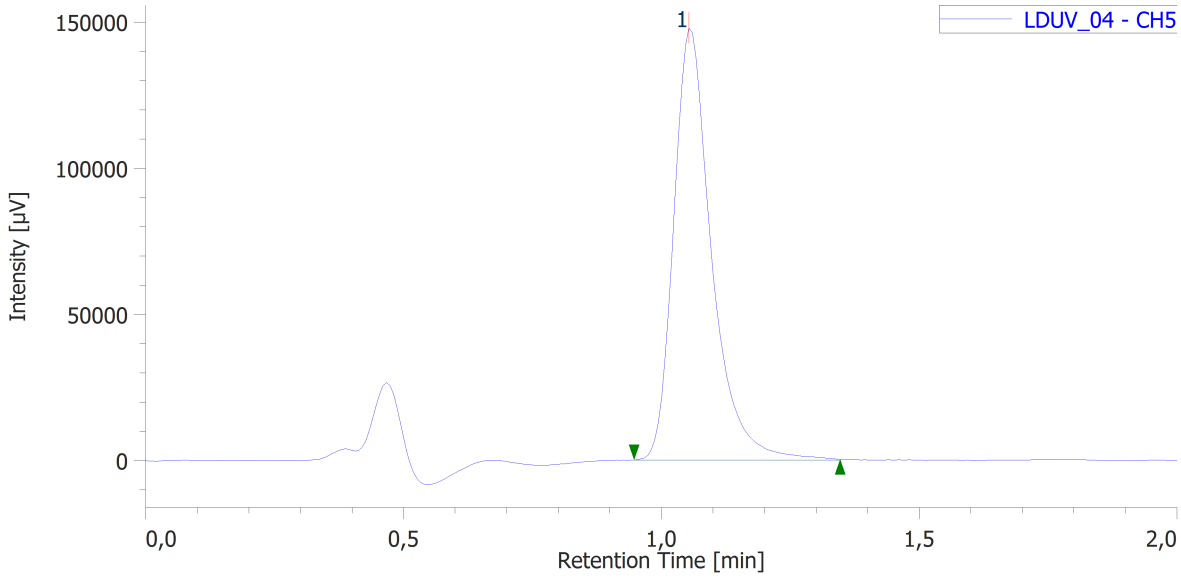

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:25:36
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:23:35
Volume	10,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,053	754171	147692	100,000	100,000	N/A	1124	N/A	1,415	

Creator
Reviewer
Approver

Chromatogram

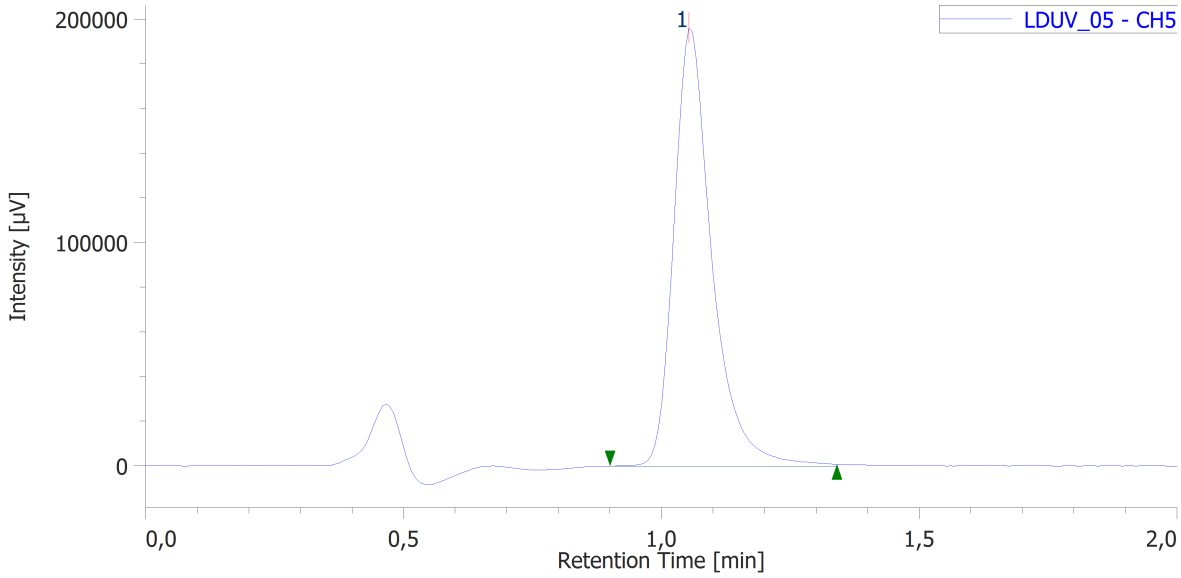

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:28:24
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:26:21
Volume	10,0 [µL]
Sample #	8
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,053	1009621	196217	100,000	100,000	N/A	1127	N/A	1,435	

Creator
Reviewer
Approver

Chromatogram

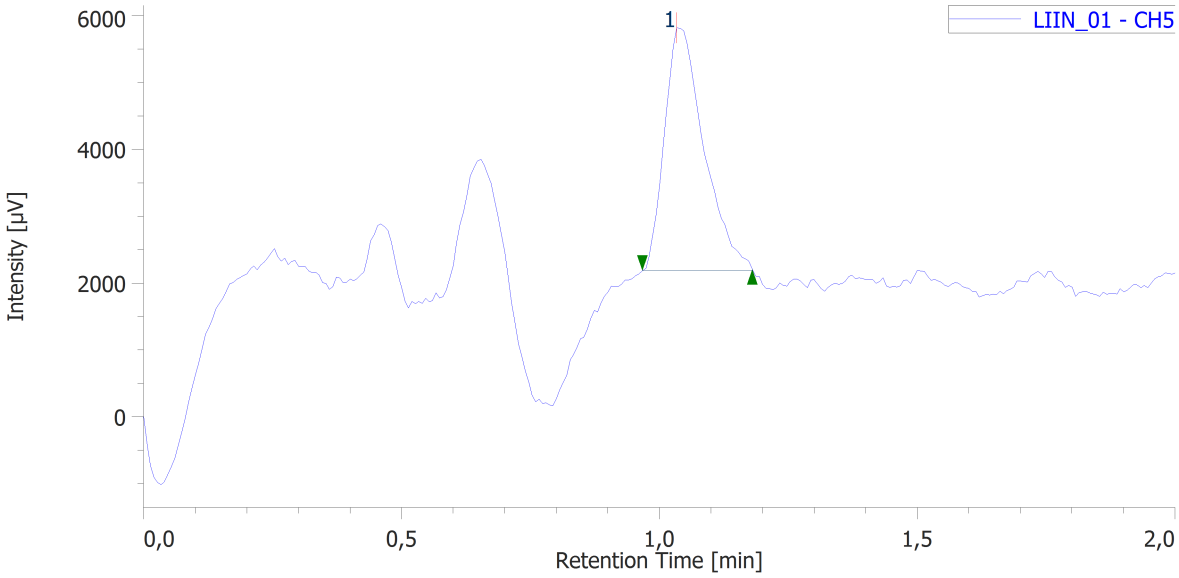

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:51:40
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:49:38
Volume	0,1 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	PCIN
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,033	19267	3626	100,000	100,000	N/A	948	N/A	1,706	

Creator
Reviewer
Approver

Chromatogram

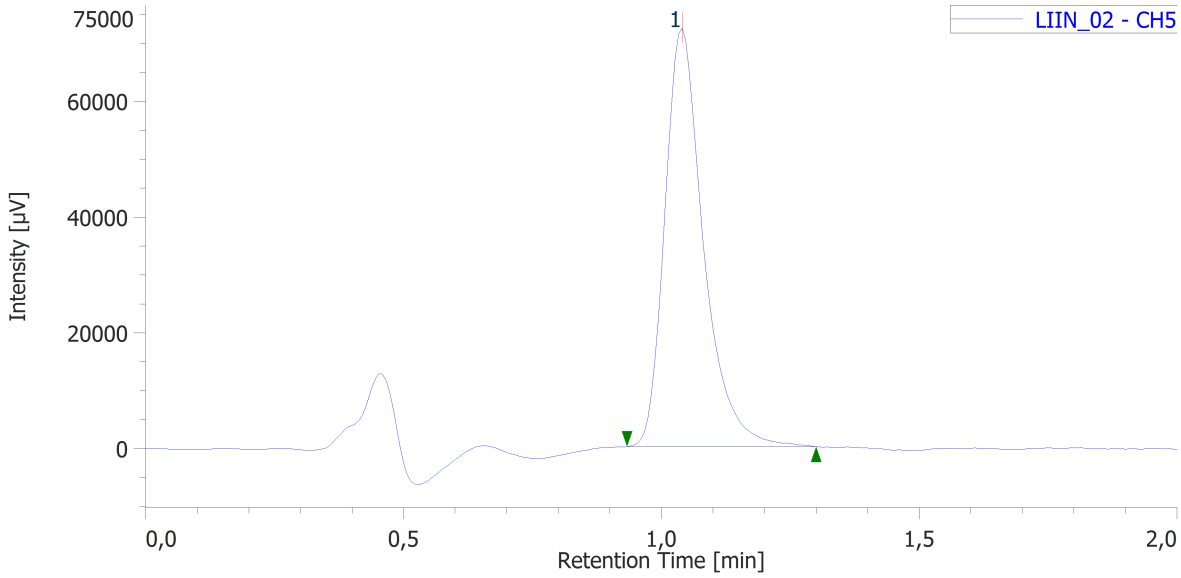

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:54:26
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:52:23
Volume	5,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,040	376981	72312	100,000	100,000	N/A	1033	N/A	1,339	

Creator
Reviewer
Approver

Chromatogram

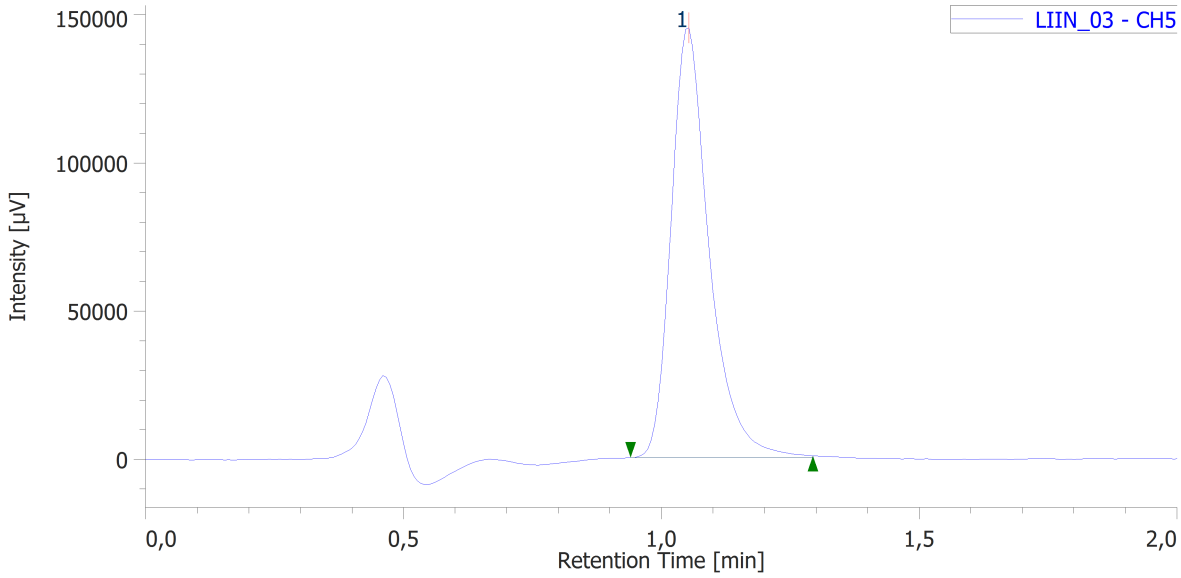

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 11:57:12
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:55:10
Volume	10,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,053	746832	144898	100,000	100,000	N/A	1092	N/A	1,307	

Creator
Reviewer
Approver

Chromatogram

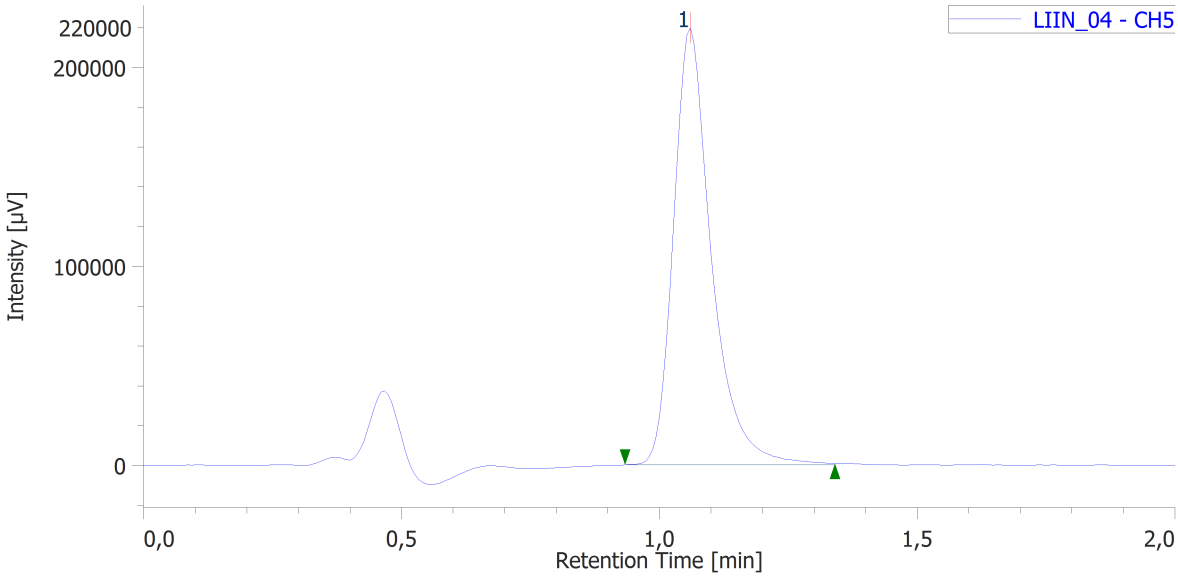

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 12:00:02
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 11:58:00
Volume	15,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,060	1124648	219432	100,000	100,000	N/A	1140	N/A	1,349	

Creator
Reviewer
Approver

Chromatogram

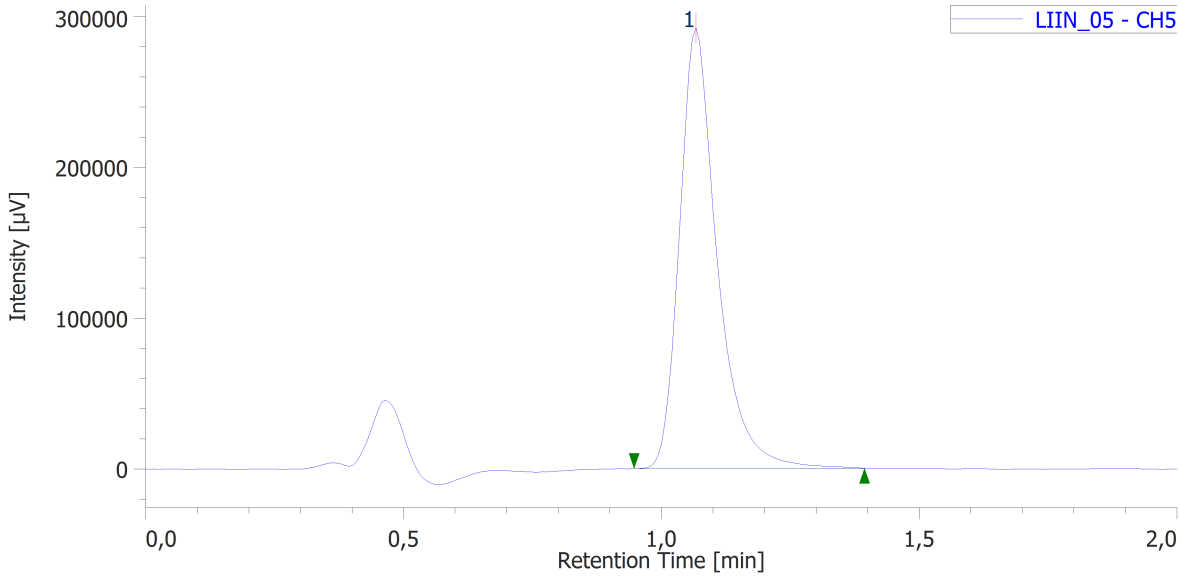


Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 12:02:54
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 12:00:53
Volume	20,0 [µL]
Sample #	9
Project Name	QPack
Acquisition Time	2,0 [min]
Acquisition Sequence	Quali
Control Method	Qualificação
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table


Chromatogram Name	LIIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	PCIN_01


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,067	1486230	291992	100,000	100,000	N/A	1183	N/A	1,372	

Creator
Reviewer
Approver

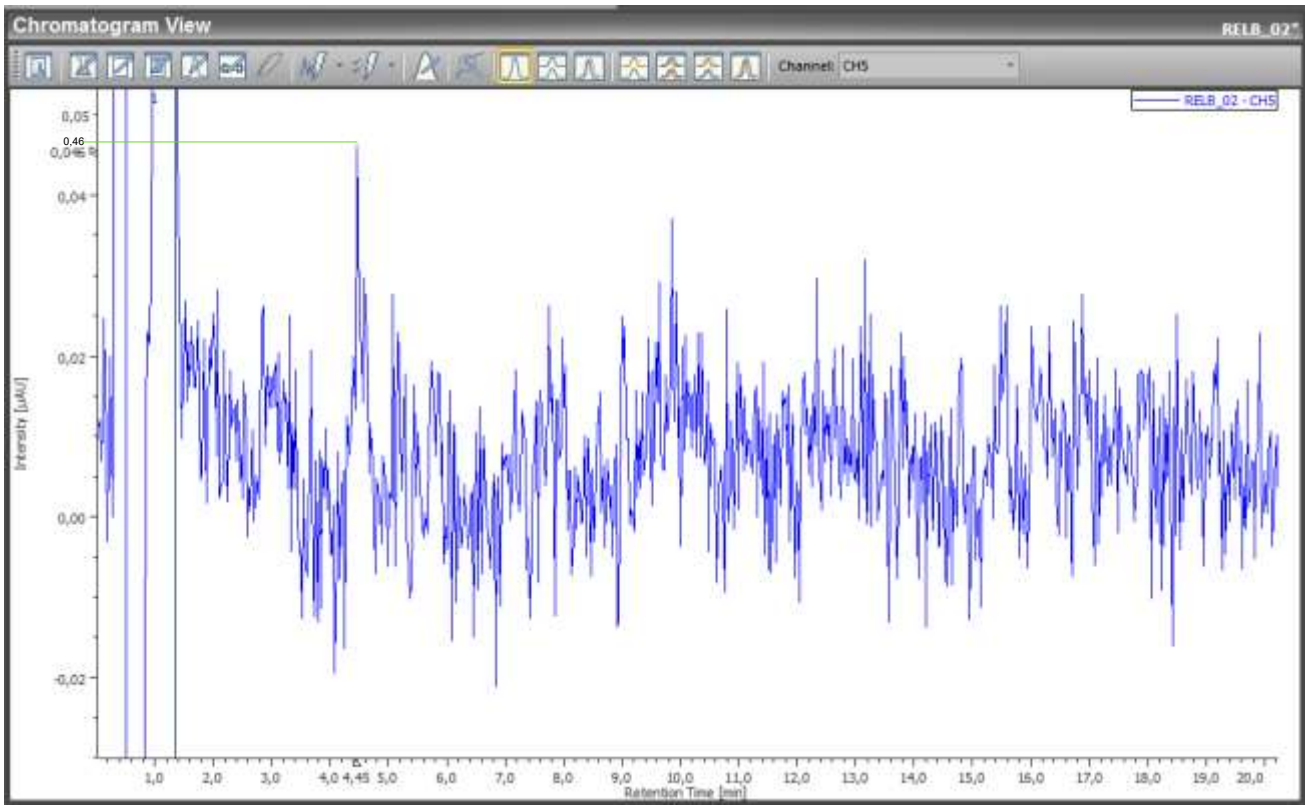

Chromatogram View
RELB_02*
Channel: CH5
RELB_02 - CH5
0,05
0,46
0,04
0,02
0,00
-0,02
Intensity [µAU]
1,0
2,0
3,0
4,0
4,45
5,0
6,0
7,0
8,0
9,0
10,0
11,0
12,0
13,0
14,0
15,0
16,0
17,0
18,0
19,0
20,0
Retention Time [min]

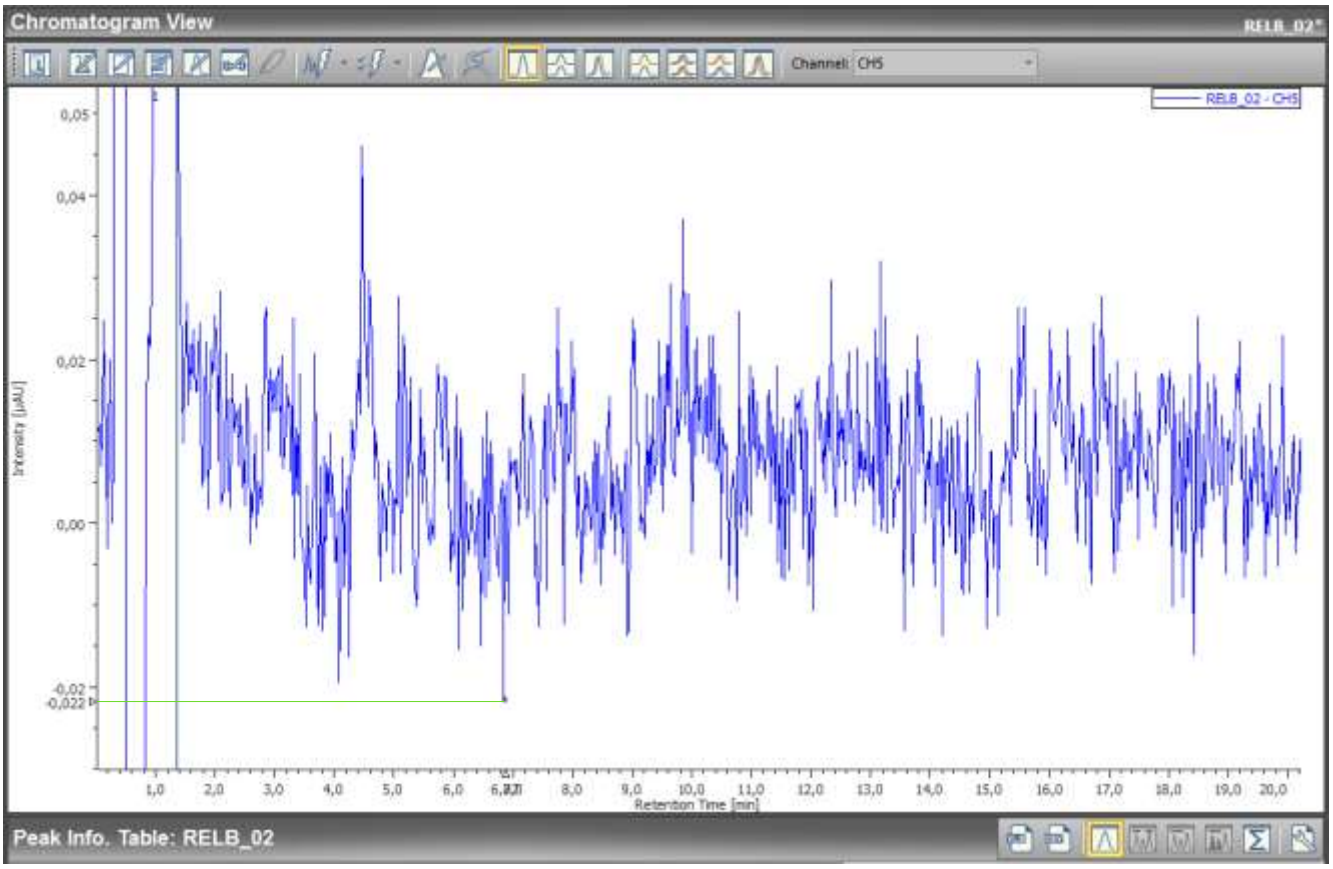
Chromatogram View
RELB_02*
Channel: CH5
RELB_02 - CH5
0,05
0,04
0,02
0,00
-0,02
-0,022
Intensity [µAU]
1,0
2,0
3,0
4,0
5,0
6,0
7,0
8,0
9,0
10,0
11,0
12,0
13,0
14,0
15,0
16,0
17,0
18,0
19,0
20,0
Retention Time [min]
Peak Info. Table: RELB_02

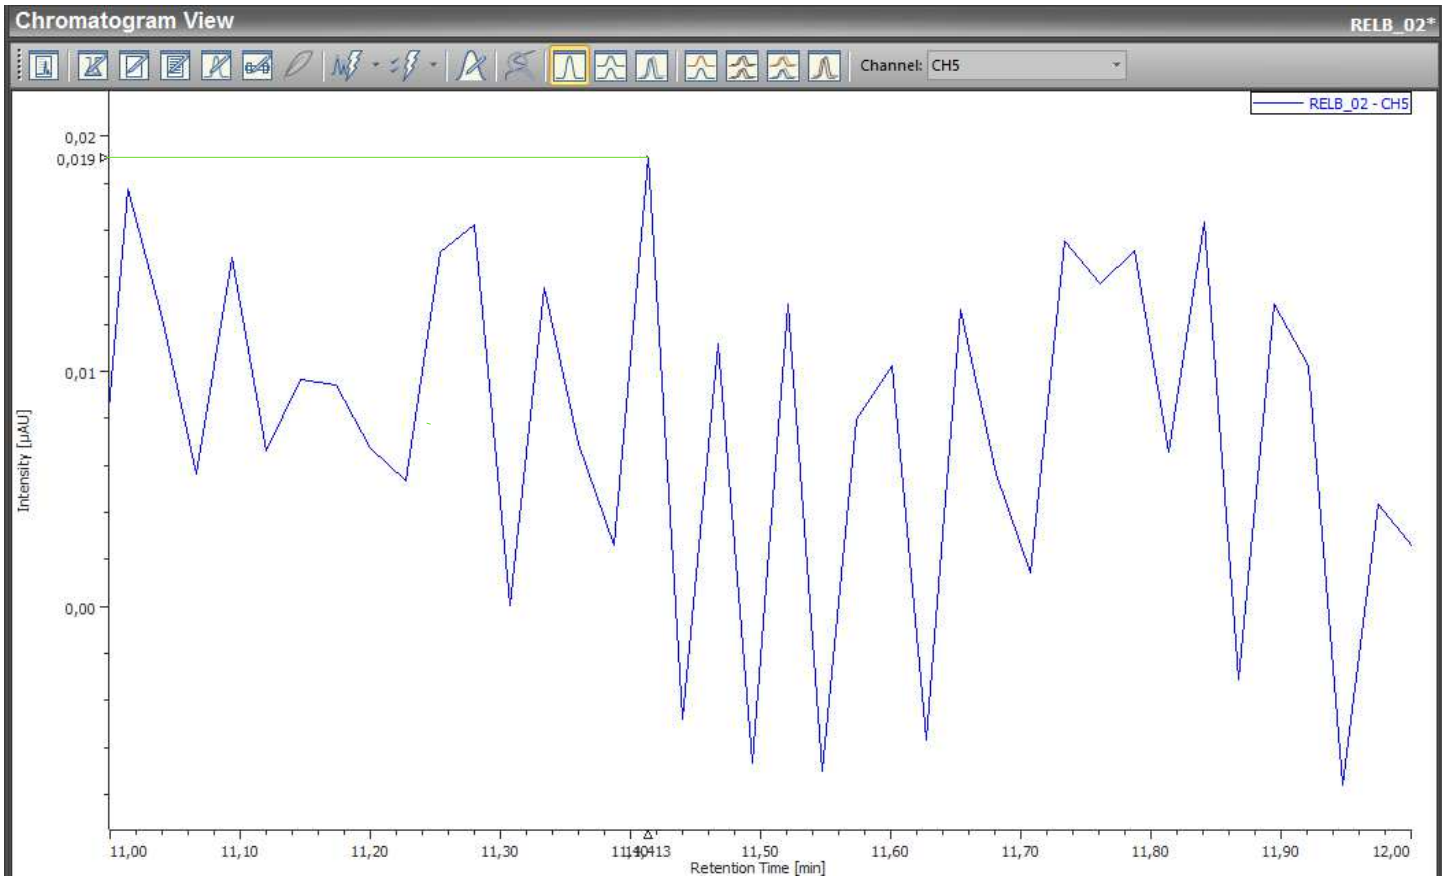
Chromatogram View
RELB_02*
Channel: CH5
RELB_02 - CH5
0,02
0,019
0,01
0,00
Intensity [µAU]
11,00
11,10
11,20
11,30
11,40
11,50
11,60
11,70
11,80
11,90
12,00
Retention Time [min]

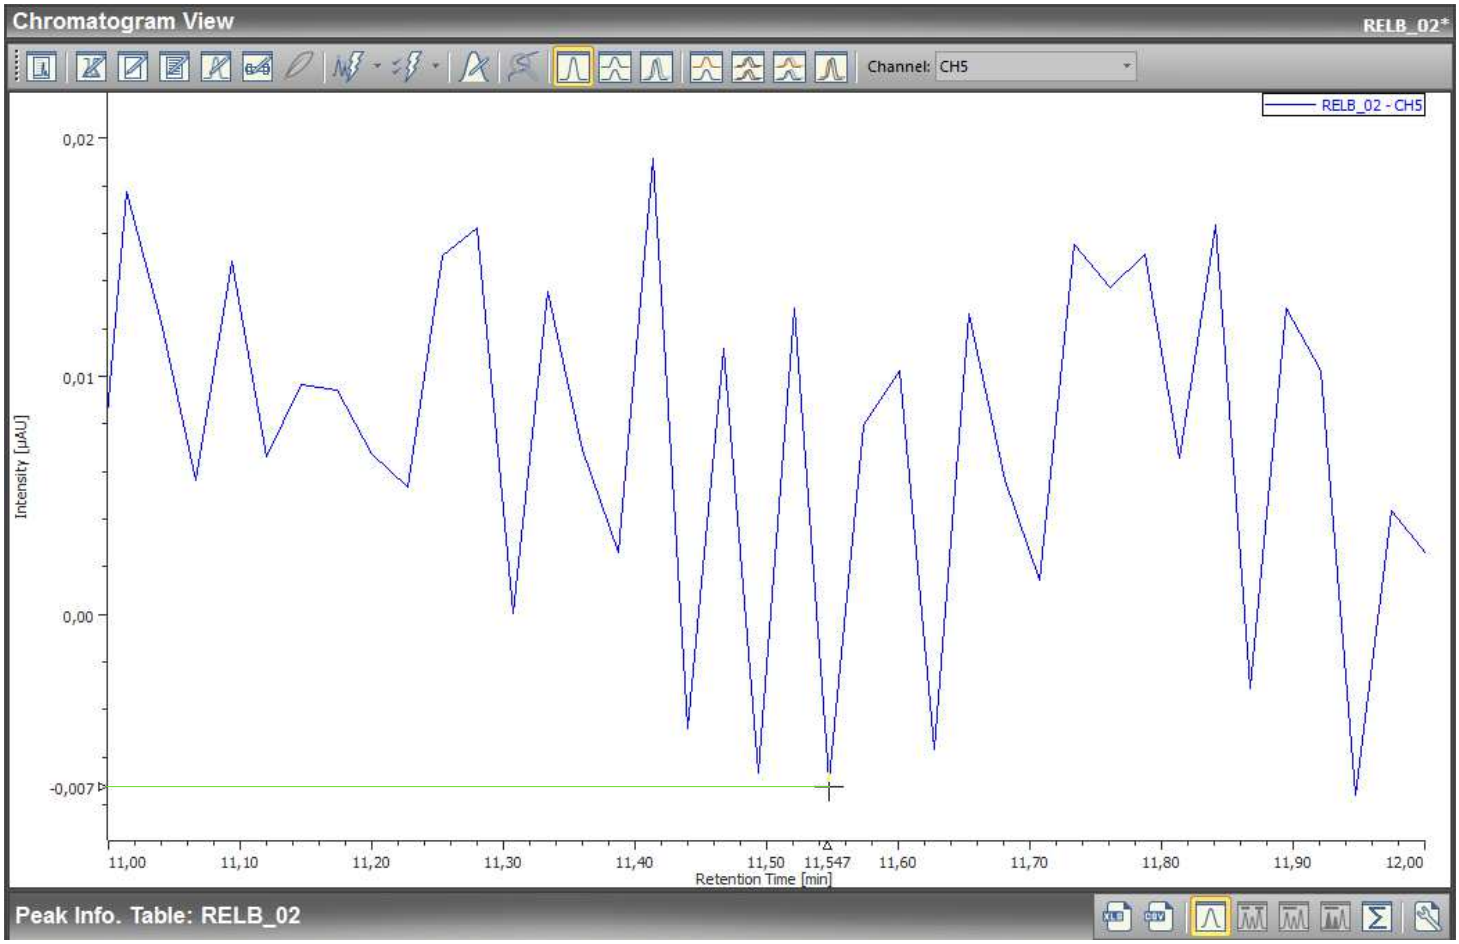
Chromatogram View
RELB_02*
Channel: CH5
RELB_02 - CH5
0,02
0,01
0,00
-0,007
Intensity [µAU]
11,00
11,10
11,20
11,30
11,40
11,50
11,547
11,60
11,70
11,80
11,90
12,00
Retention Time [min]
Peak Info. Table: RELB_02

Chromatogram

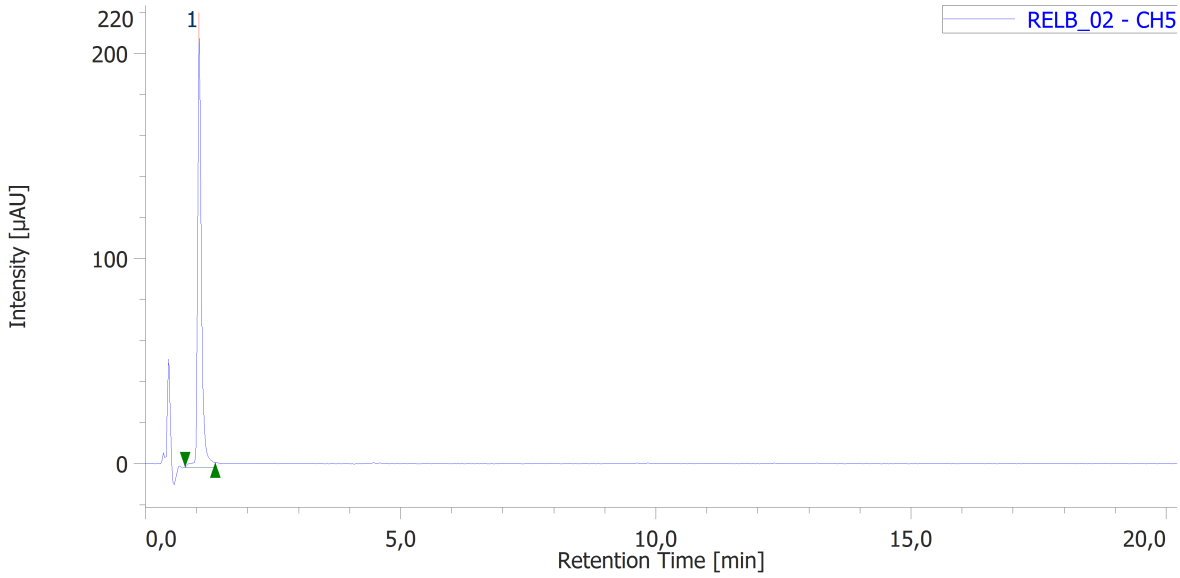

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 12:24:00
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 12:03:45
Volume	20,0 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	20,2 [min]
Acquisition Sequence	Quali
Control Method	RELB
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB_02-CH5
Sample Name	
Channel Name	254,0nm
Sampling Interval	1600 [msec]
Peak Method	PCIN_01

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,040	1080995	213969	100,000	100,000	N/A	1272	N/A	1,756	

Creator
Reviewer
Approver

Chromatogram

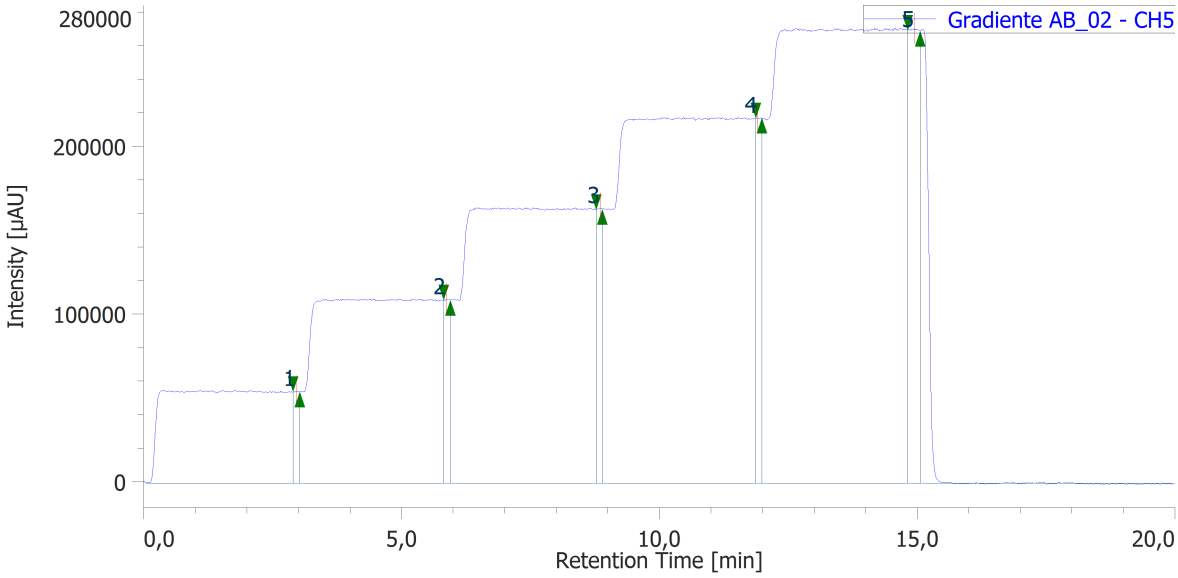

Chromatogram Information	
User Name	QPackSA
Date Modified	08/05/2024 15:07:06
Description	
HPLC System Name	HPL30
Injection Date	08/05/2024 14:35:30
Volume	0,1 [µL]
Sample #	11
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	GRBO
Control Method	GRBO
Peak ID Table	GRBO_
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	GRBO (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	2,960	435985	54866	5,489	6,718	N/A	3139	N/A	N/A	
2	40%	5	5,867	873910	109517	11,003	13,410	N/A	12226	N/A	N/A	
3	60%	5	8,853	1176699	163878	14,816	20,066	N/A	34388	N/A	N/A	
4	80%	5	11,907	1565192	217624	19,707	26,647	N/A	61993	N/A	N/A	
5	100%	5	14,947	3890416	270792	48,984	33,158	N/A	24482	N/A	N/A	

Creator
Reviewer
Approver