
Chromatogram

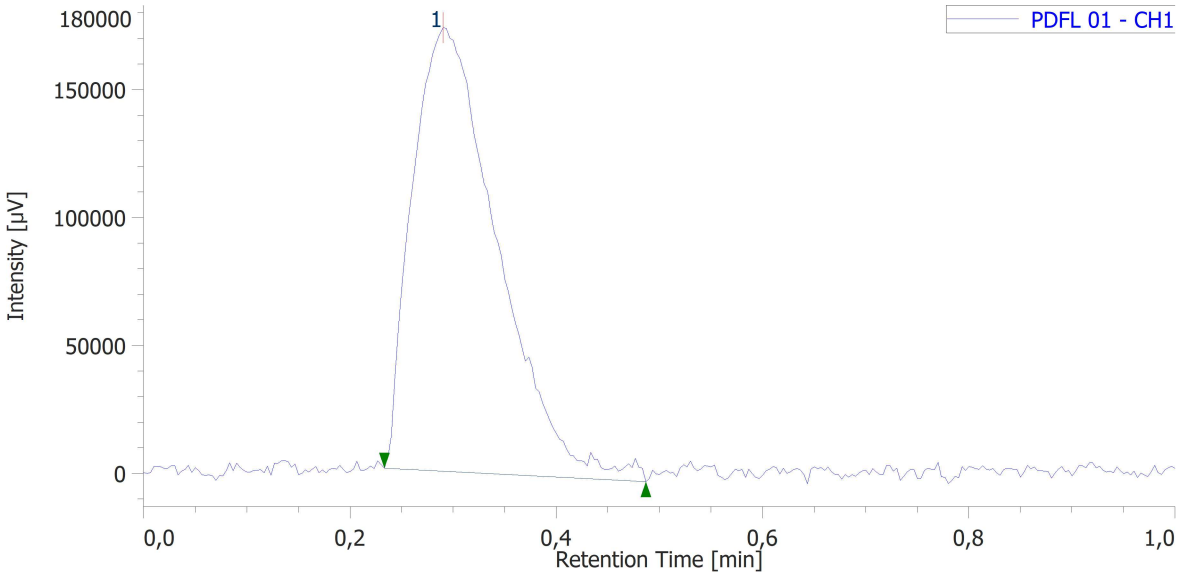

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:41
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:07:34
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,290	994010	173187	100,000	100,000	N/A	55	N/A	2,306		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

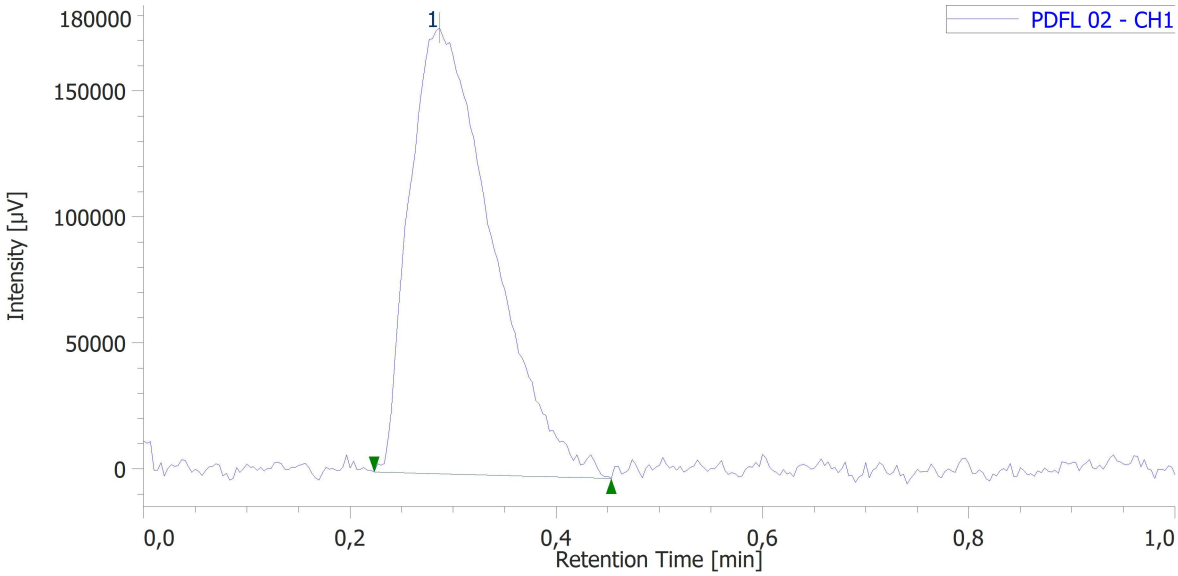

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:41
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:10:16
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,287	989969	176895	100,000	100,000	N/A	57	N/A	1,929		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

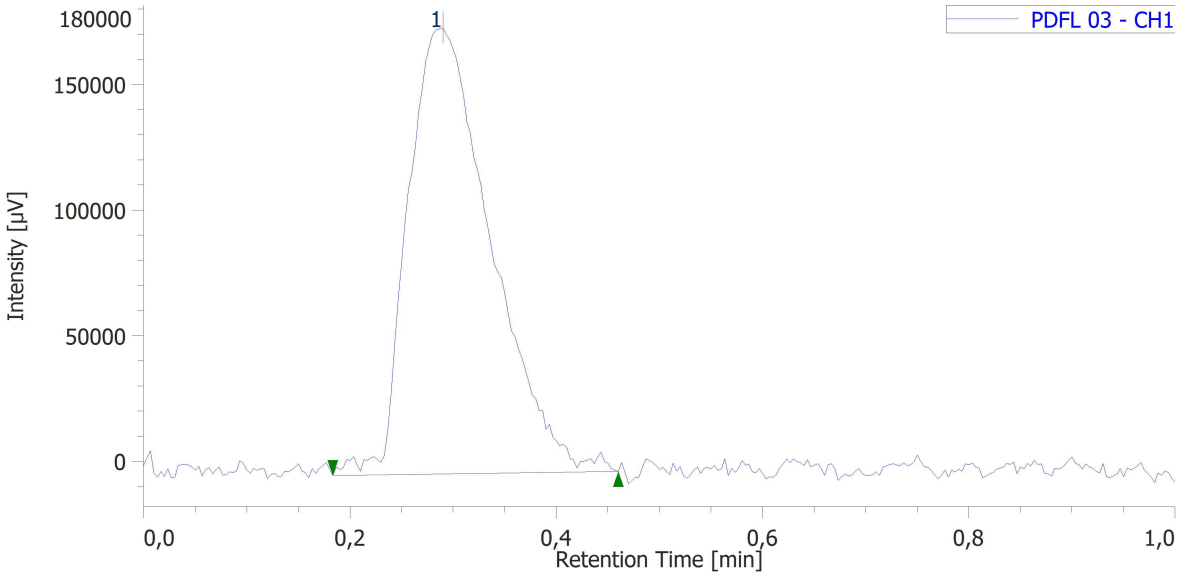

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:42
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:12:58
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,290	994682	177365	100,000	100,000	N/A	62	N/A	1,572		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

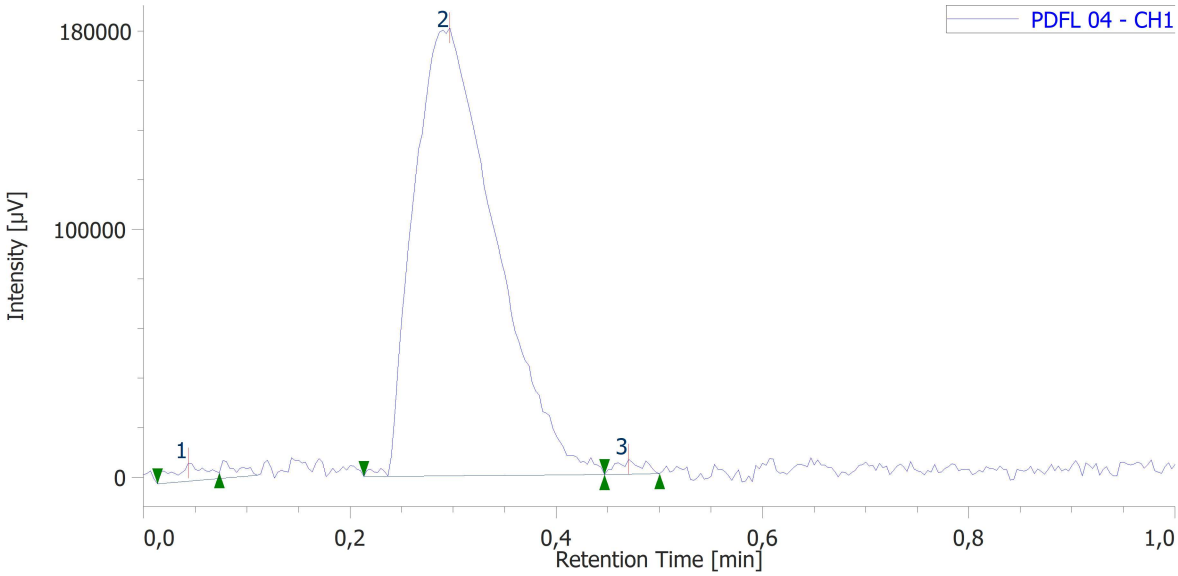

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:42
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:15:40
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	1	0,043	14916	7301	1,472	3,766	N/A	4	2,138	N/A		N/A
2	Quinina	1	0,297	988422	180562	97,515	93,134	N/A	62	1,629	1,492		N/A
3	Unknown	1	0,470	10276	6011	1,014	3,100	N/A	904	N/A	1,113		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

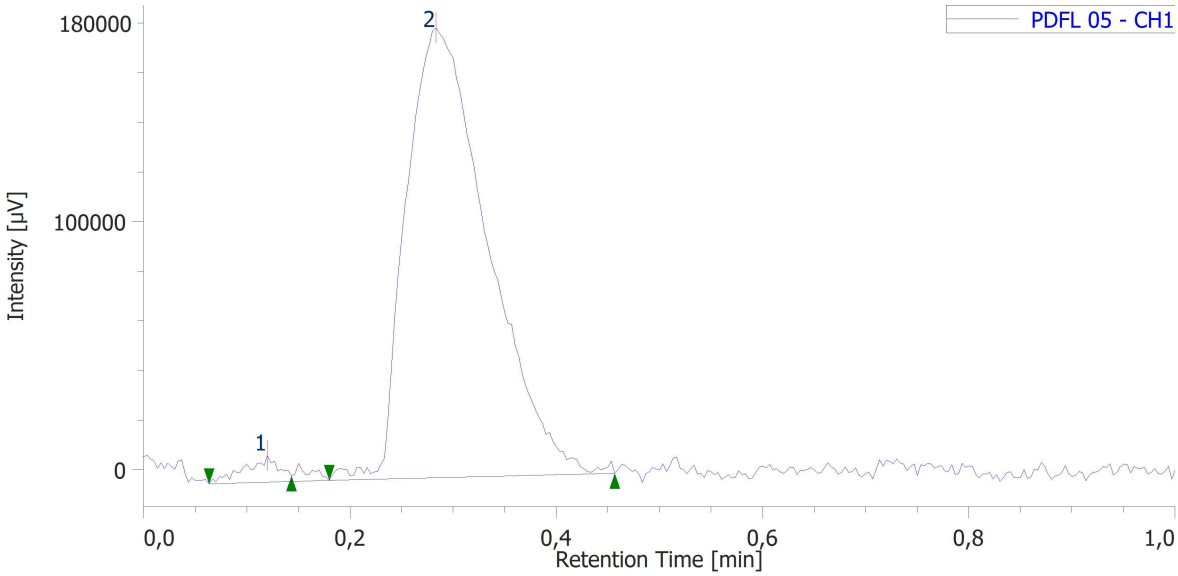

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:42
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:18:22
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Unknown	1	0,120	23894	10793	2,336	5,623	N/A	69	1,602	N/A		N/A
2	Quinina	1	0,283	998745	181168	97,664	94,377	N/A	60	N/A	1,739		N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

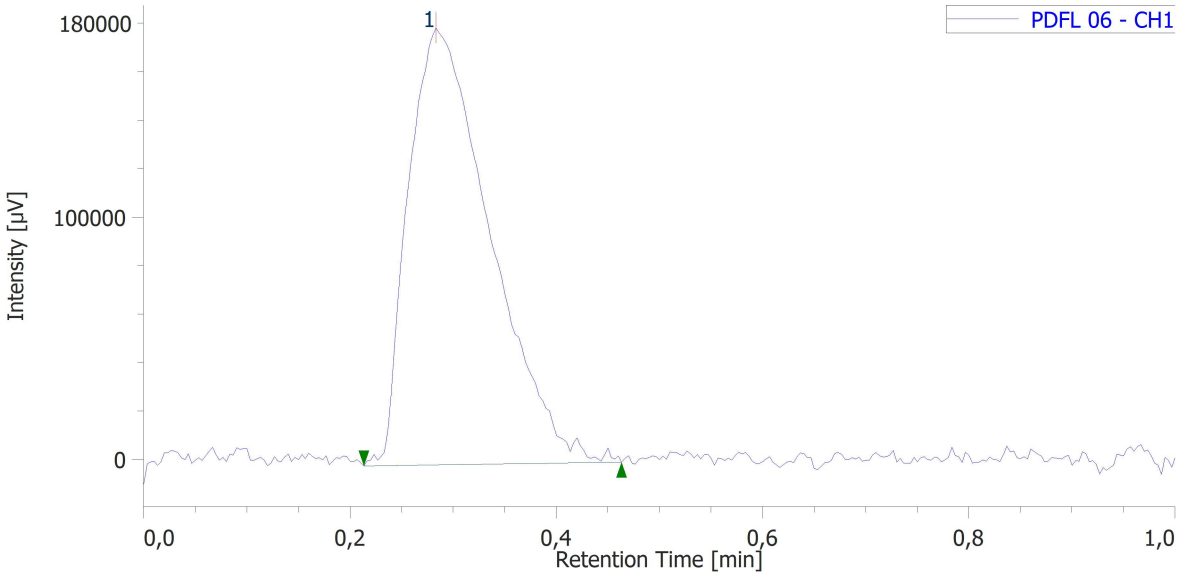

Chromatogram Information	
User Name	QPackSA
Date Modified	29/04/2025 14:28:42
Description	
HPLC System Name	HP06 – Det FL
Injection Date	29/04/2025 14:21:03
Volume	20,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	PDFL
Control Method	Qualificação FL2
Peak ID Table	PDFL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PDFL 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	FL Peak Process

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	S/N
1	Quinina	1	0,283	995303	180226	100,000	100,000	N/A	58	N/A	1,914		N/A

Creator QPackSA
Reviewer
Approver

Peak Find - EDFL_002 FPEm_tR0,27 D.jws

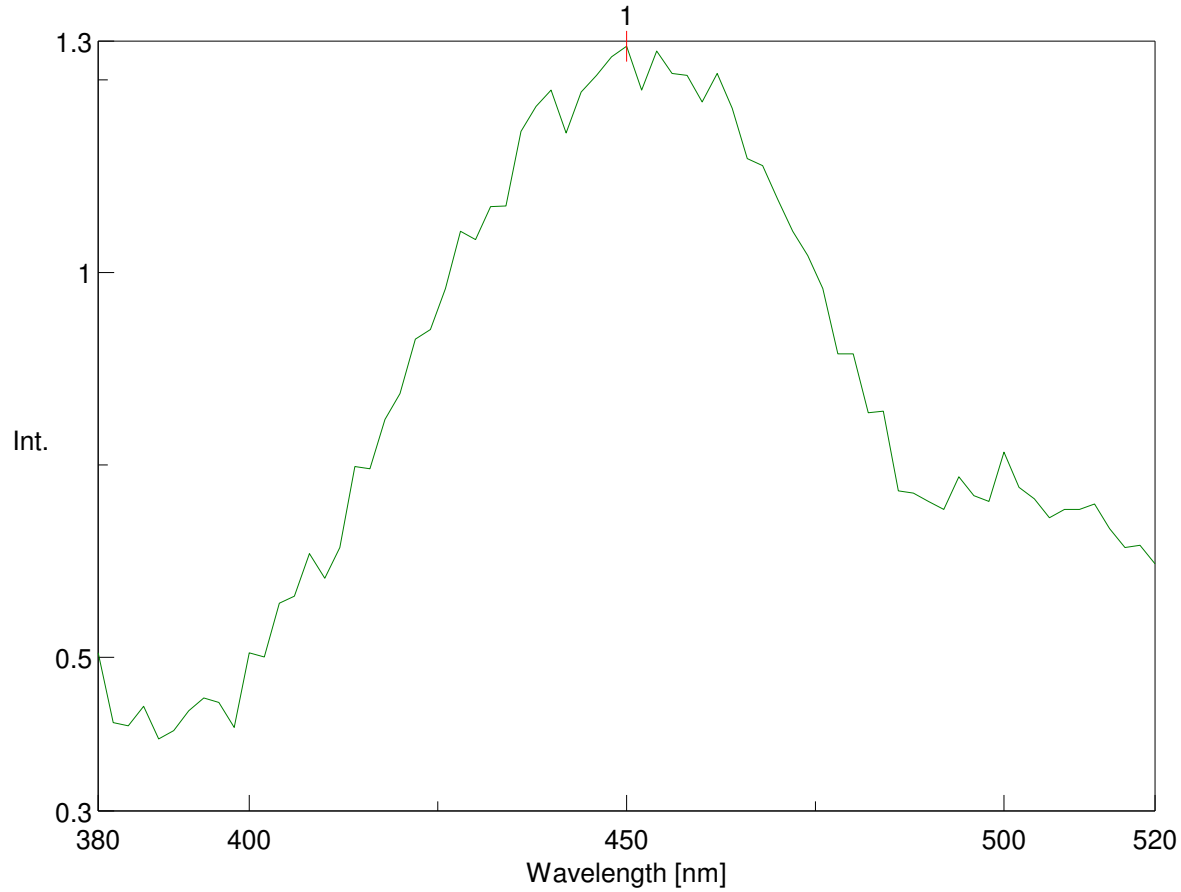

[Comments]

User	QPackSA
Division	---
Company	DLA PHARMA
Creation date	29/04/2025 13:12

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	2 nm
Data points	171

[Measurement Information]

Instrument Name	X-LC 3120FP
Model Name	X-LC 3120FP
Serial No.	007961214
ROM version	V6.34
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	450	1.29347			