
01 Energia

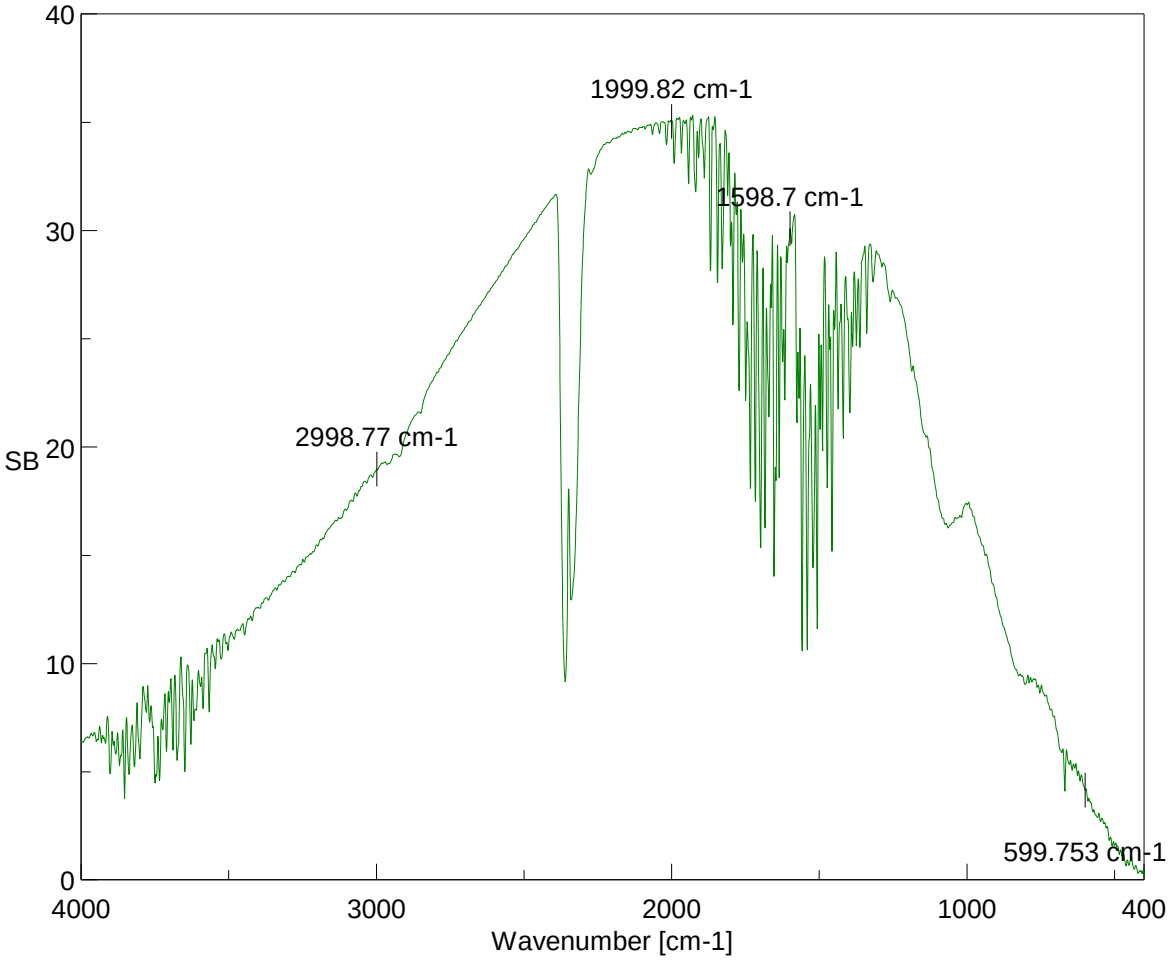

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 11/05/2026 14:30

Light Source Standard
Detector TGS
Accumulation 16
Resolution 4 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (2)
Aperture Auto (7.1 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


01 Energia

[Detailed Information]
Creation date 11/05/2026 14:33

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis SB
Start 399.193 cm-1
End 4000.6 cm-1
Data interval 0.964233 cm-1
Data points 3736

Creation QPack
Review
Approval

02 Exatidão Numero de onda

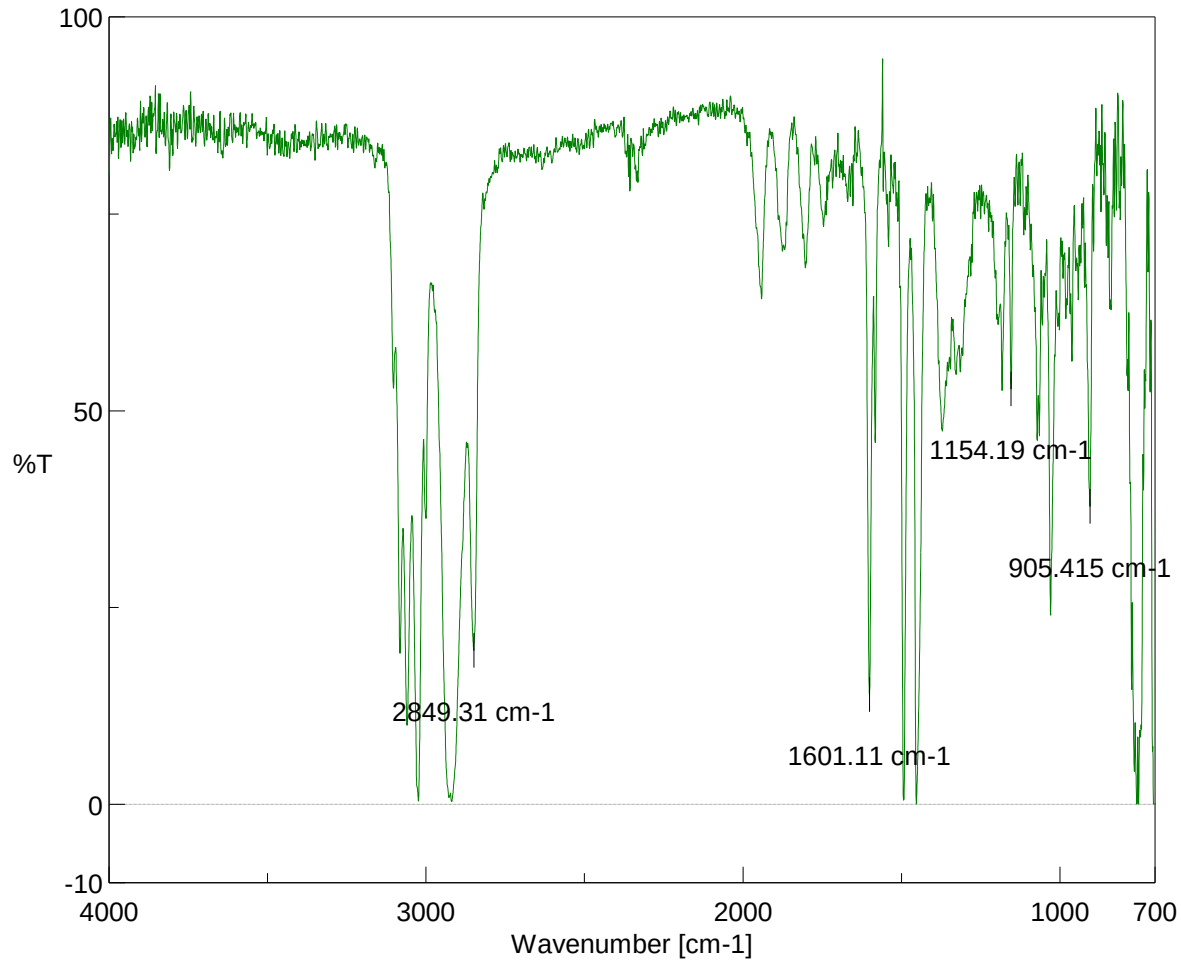

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 11/05/2026 14:45

Light Source Standard
Detector TGS
Accumulation 16
Resolution 2 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (4)
Aperture Auto (5 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


02 Exatidão Numero de onda

[Detailed Information]
Creation date 11/05/2026 14:50

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 699.551 cm-1
End 4000.12 cm-1
Data interval 0.482117 cm-1
Data points 6847

Creation QPack
Review
Approval

03 repetibilidade no numero de onda

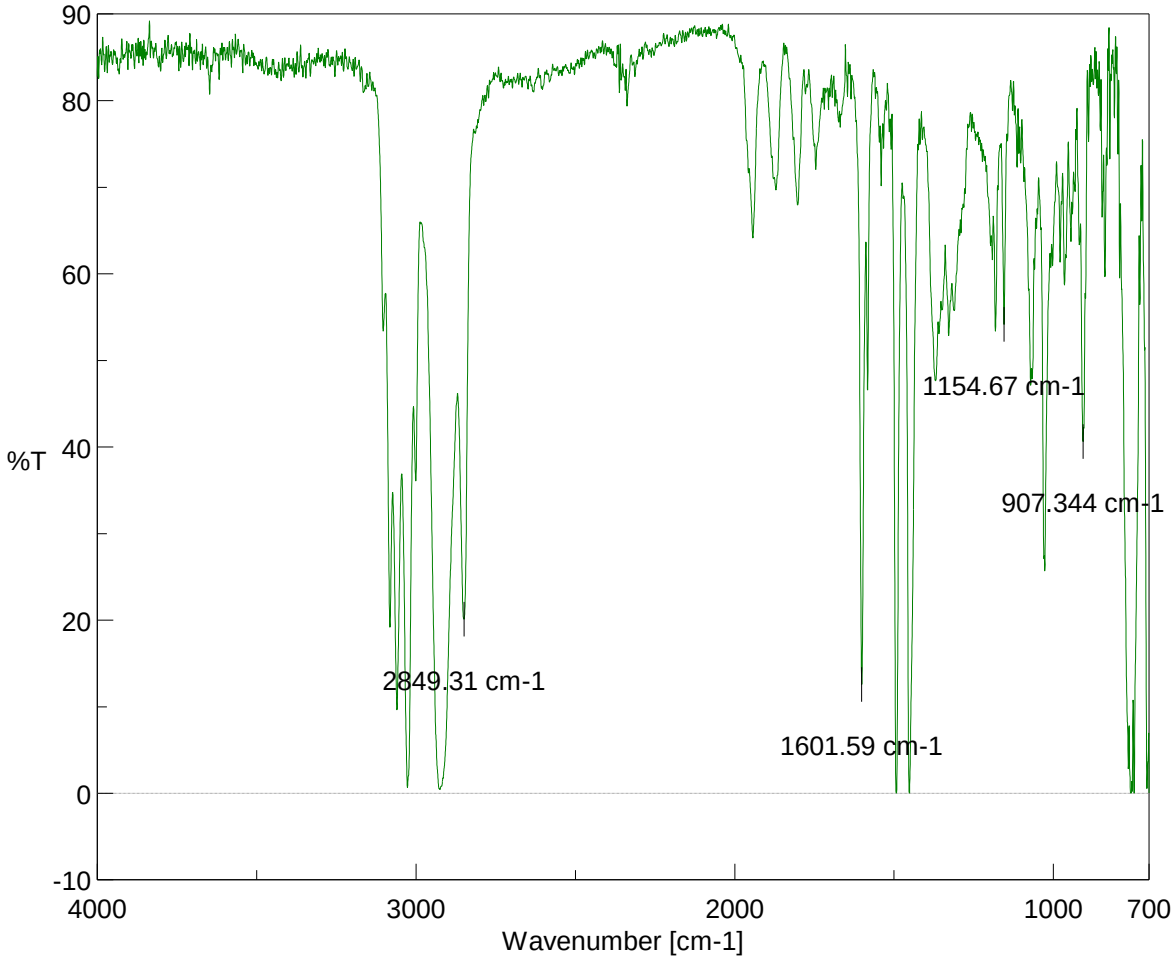

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 12/05/2026 10:31

Light Source Standard
Detector TGS
Accumulation 16
Resolution 2 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (4)
Aperture Auto (5 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


03 repetibilidade no numero de onda

[Detailed Information]
Creation date 12/05/2026 10:34

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 699.551 cm-1
End 4000.12 cm-1
Data interval 0.482117 cm-1
Data points 6847

Creation QPack
Review
Approval

03 repetibilidade no numero de onda_02

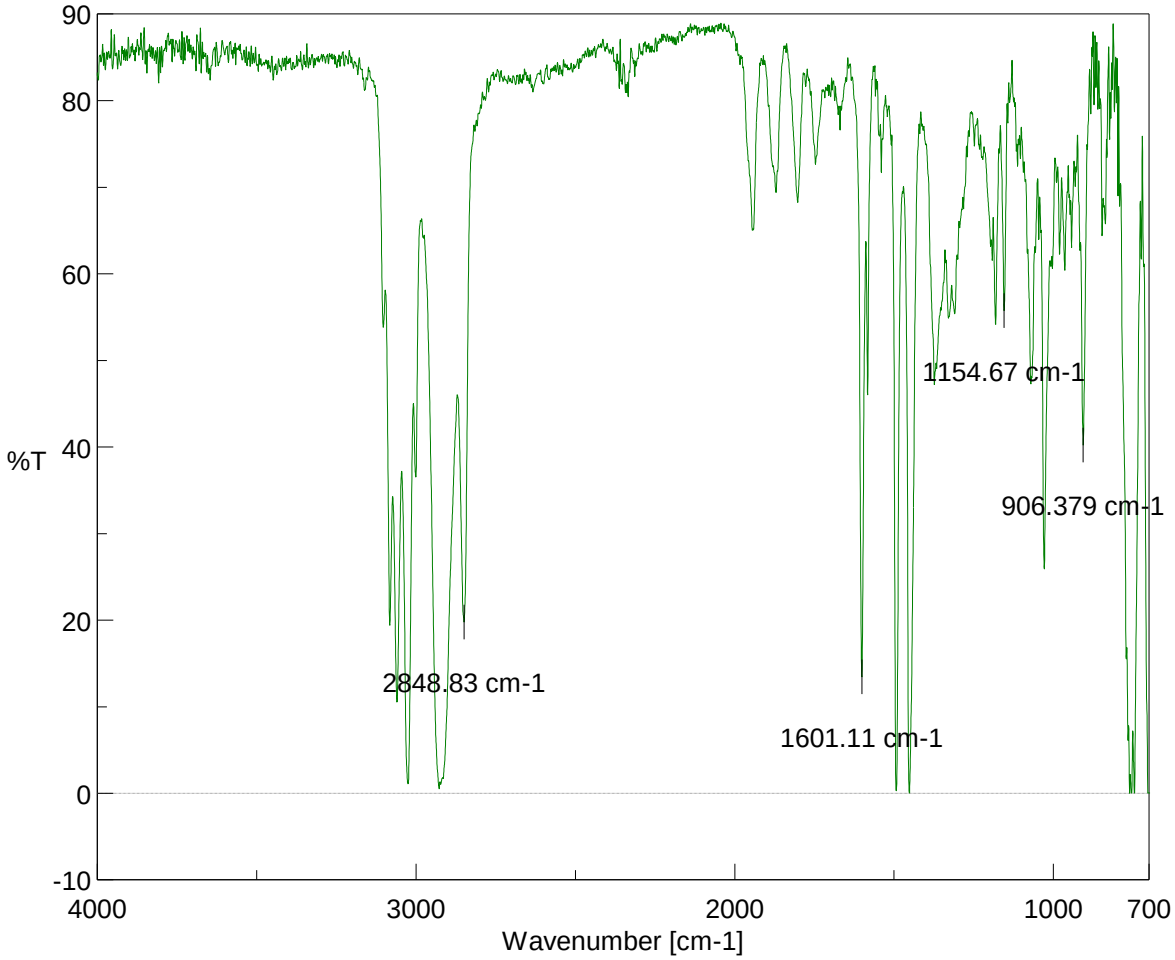

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 12/05/2026 10:31

Light Source Standard
Detector TGS
Accumulation 16
Resolution 2 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (4)
Aperture Auto (5 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


03 repetibilidade no numero de onda_02

[Detailed Information]
Creation date 12/05/2026 10:35

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 699.551 cm-1
End 4000.12 cm-1
Data interval 0.482117 cm-1
Data points 6847

Creation QPack
Review
Approval

04 repetibilidade fotometrica_01

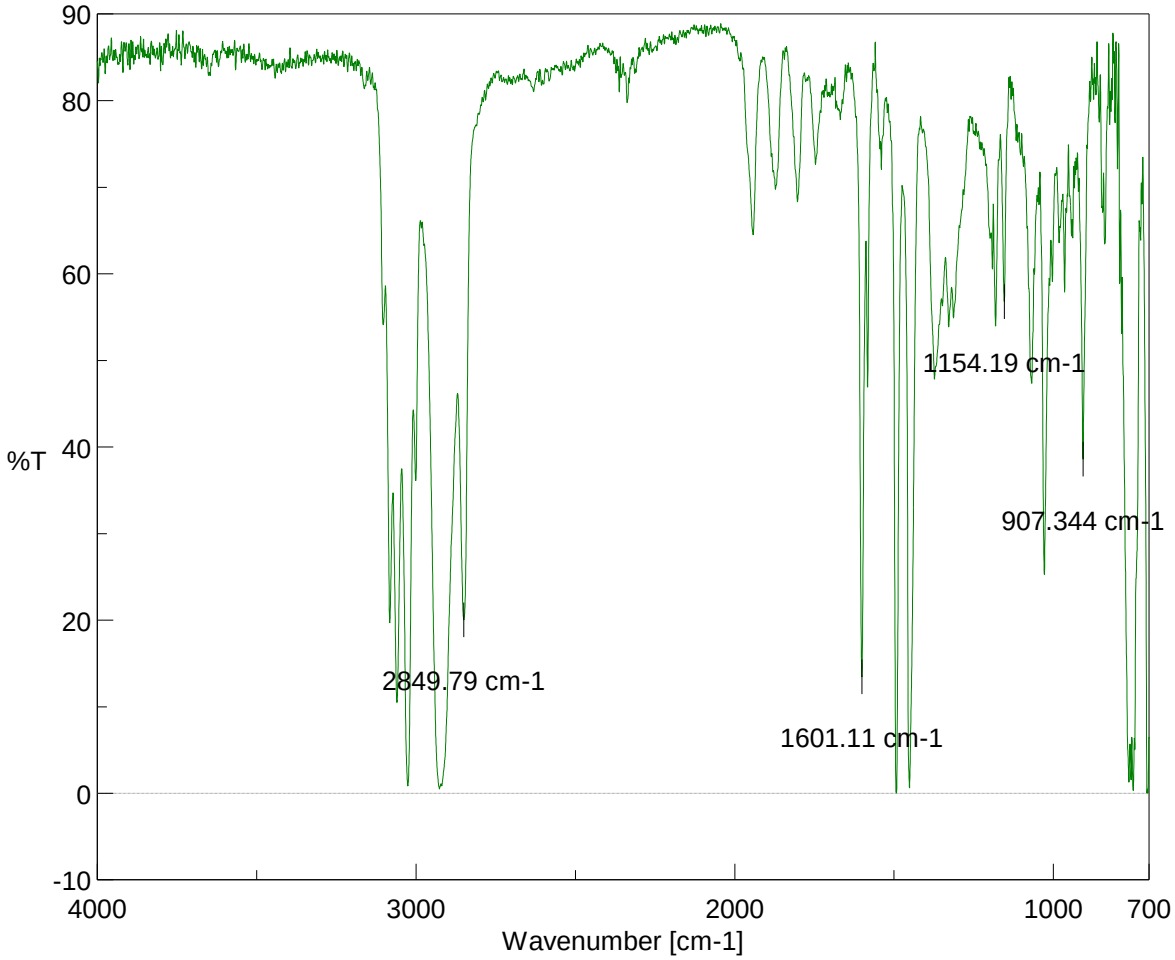

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 12/05/2026 10:36

Light Source Standard
Detector TGS
Accumulation 16
Resolution 2 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (4)
Aperture Auto (5 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


04 repetibilidade fotometrica_01

[Detailed Information]
Creation date 12/05/2026 10:46

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 699.551 cm-1
End 4000.12 cm-1
Data interval 0.482117 cm-1
Data points 6847

Creation QPack
Review
Approval

04 repetibilidade fotometrica_02

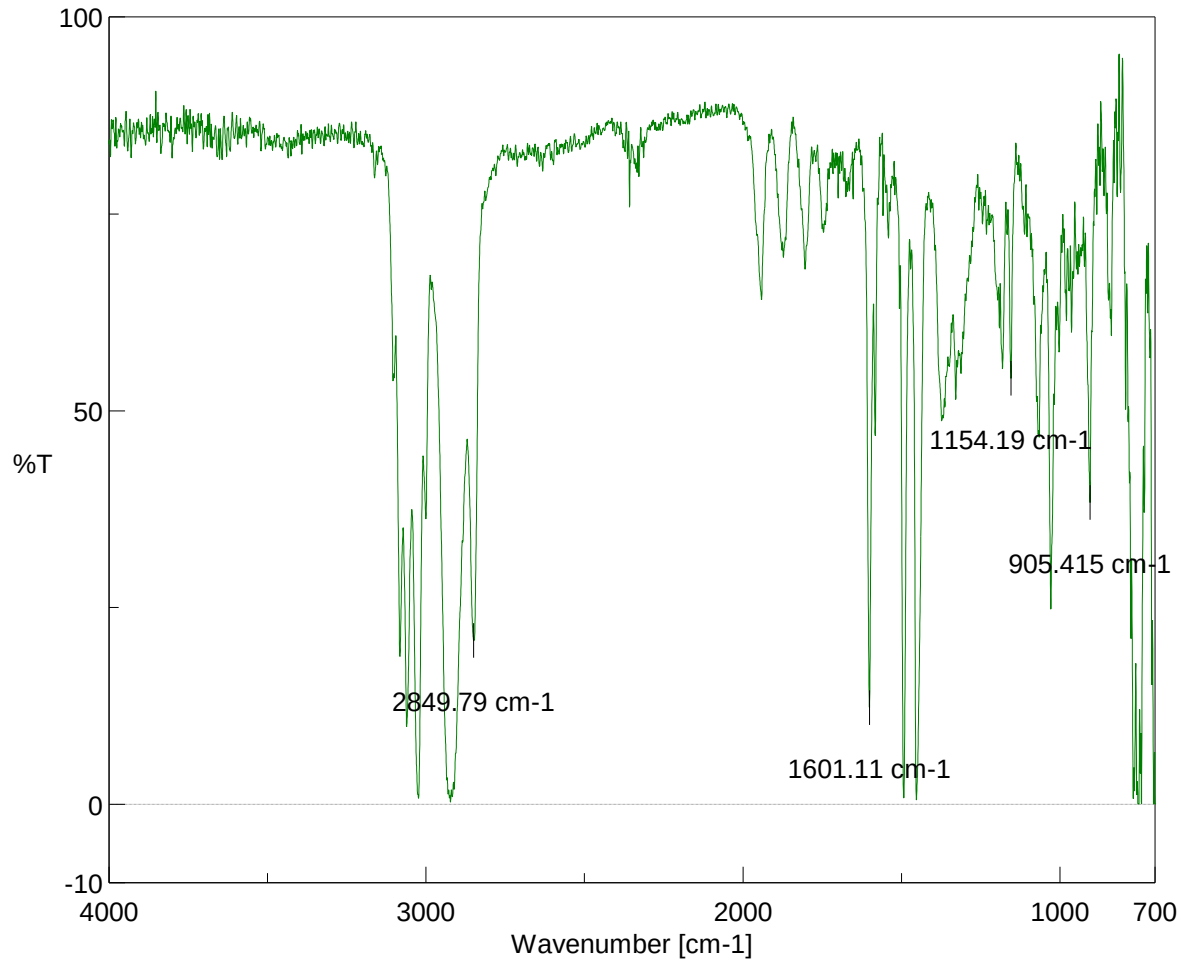

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco_Treinamento
Division Assistência
Company TRB Pharma

[Measurement Information]
Model Name FT/IR-4100typeA
Serial Number B005561016

Measurement Date 12/05/2026 10:37

Light Source Standard
Detector TGS
Accumulation 16
Resolution 2 cm-1
Zero Filling On
Apodization Cosine
Gain Auto (4)
Aperture Auto (5 mm)
Scanning Speed Auto (2 mm/sec)
Filter Auto (30000 Hz)


04 repetibilidade fotometrica_02

[Detailed Information]
Creation date 12/05/2026 10:46

Data array type Linear data array
Horizontal axis Wavenumber [cm-1]
Vertical axis %T
Start 699.551 cm-1
End 4000.12 cm-1
Data interval 0.482117 cm-1
Data points 6847

Creation QPack
Review
Approval

05 Sensibilidade

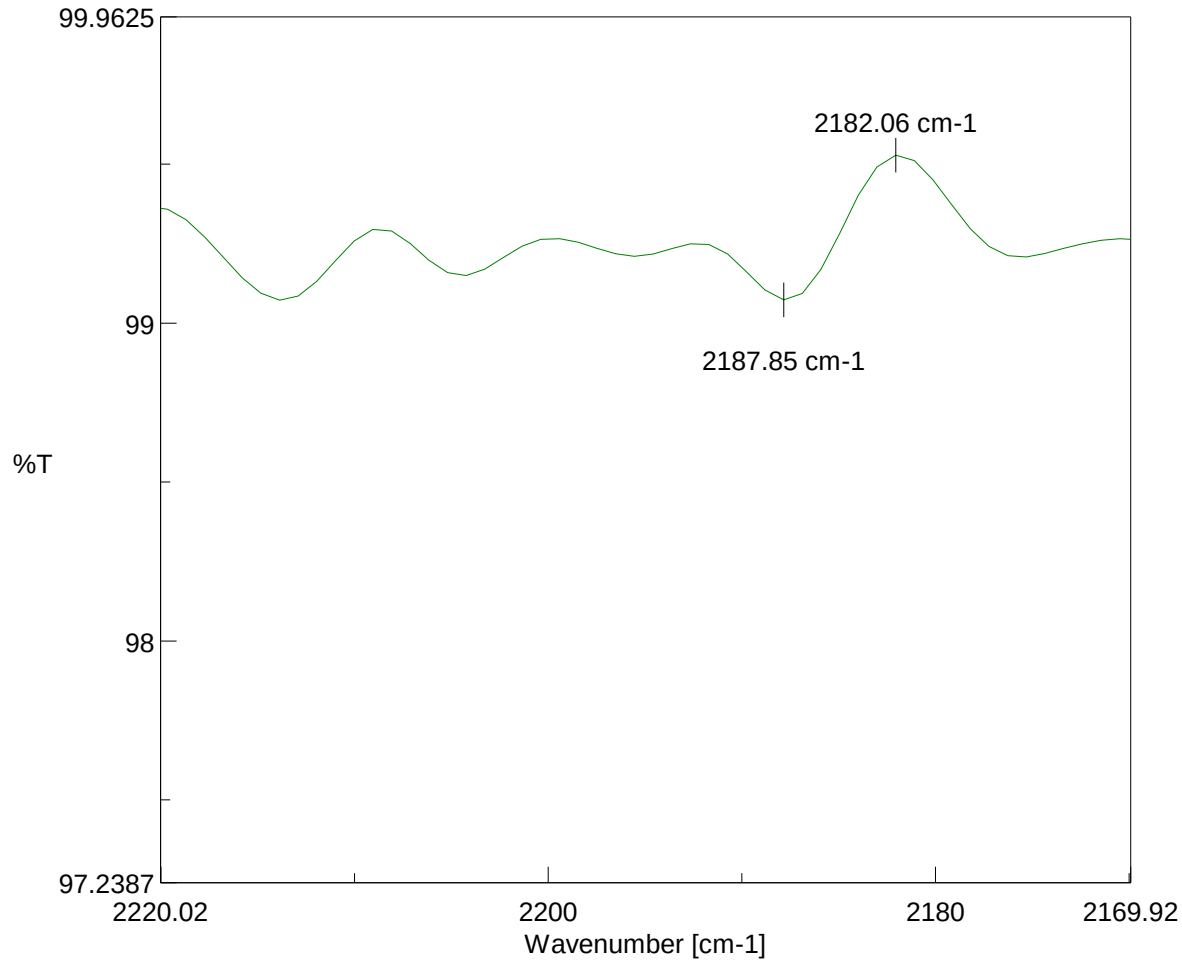

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco_Treinamento
Division	Assistência
Company	TRB Pharma

[Measurement Information]

Model Name	FT/IR-4100typeA
Serial Number	B005561016
Measurement Date	12/05/2026 10:54
Light Source	Standard
Detector	TGS
Accumulation	48
Resolution	4 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (7.1 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

05 Sensibilidade

[Detailed Information]

Creation date	12/05/2026 10:57
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.6 cm-1
Data interval	0.964233 cm-1
Data points	3528

Creation	QPack
Review	
Approval	