

MicroLab
MicroLab
User: marcos.cagliari
Status: Ready
Method: Metodo Padrao para Analise dispositivo AT
21CFR11 Enabled
Current Instrument Type: Cary 630
Current Sampling Technology: ATR 1-Bounce
Instrument Status
Energy: 26365
Battery: On AC power
Source: 1,862 / 2,704
Laser: 8200
Gain Adjust
Temperatures (°C)
Detector: 40,002
CPU: 43,875
IR board: 48,927
Power: 42,375
Version Information
Version: 4.5.93.0
DLL Version: 1,521
Firmware Version: 1,920
Instrument Serial Number:
MY13500009
Resetting the Clean validity will cause the next clean run to be stored as the new 'Good' Clean run.
Reset Clean Validity
For methods that do not require a new background on every sample, the 'Reset Background Validity' button will force a new background to be collected before the next sample collection occurs.
Reset Background Validity
Date Time format configuration (for generation of DateTime in files' names) :
Fixed: yyyy-MM-ddThh-mm-ss
Home
< Back
Agilent Technologies



MicroLab
MicroLab
User: marcos.cagliari
Status: Ready
Method: Sensibilidade DialPath
21CFR11 Enabled
Current Instrument Type: Cary 630
Current Sampling Technology: DialPath
Instrument Status
Energy: 24884
Battery: On AC power
Source: 1,862 / 2,7
Laser: 8143
Gain Adjust
Temperatures (°C)
Detector: 40,006
CPU: 43,625
IR board: 48,328
Power: 42
Version Information
Version: 4.5.93.0
DLL Version: 1,521
Firmware Version: 1,920
Instrument Serial Number:
MY13500009
Resetting the Clean validity will cause the next clean run to be stored as the new 'Good' Clean run.
Reset Clean Validity
For methods that do not require a new background on every sample, the 'Reset Background Validity' button will force a new background to be collected before the next sample collection occurs.
Reset Background Validity
Date Time format configuration (for generation of DateTime in files' names) :
Fixed: yyyy-MM-ddThh-mm-ss
Home
< Back
Agilent Technologies

Agilent Resolutions Pro

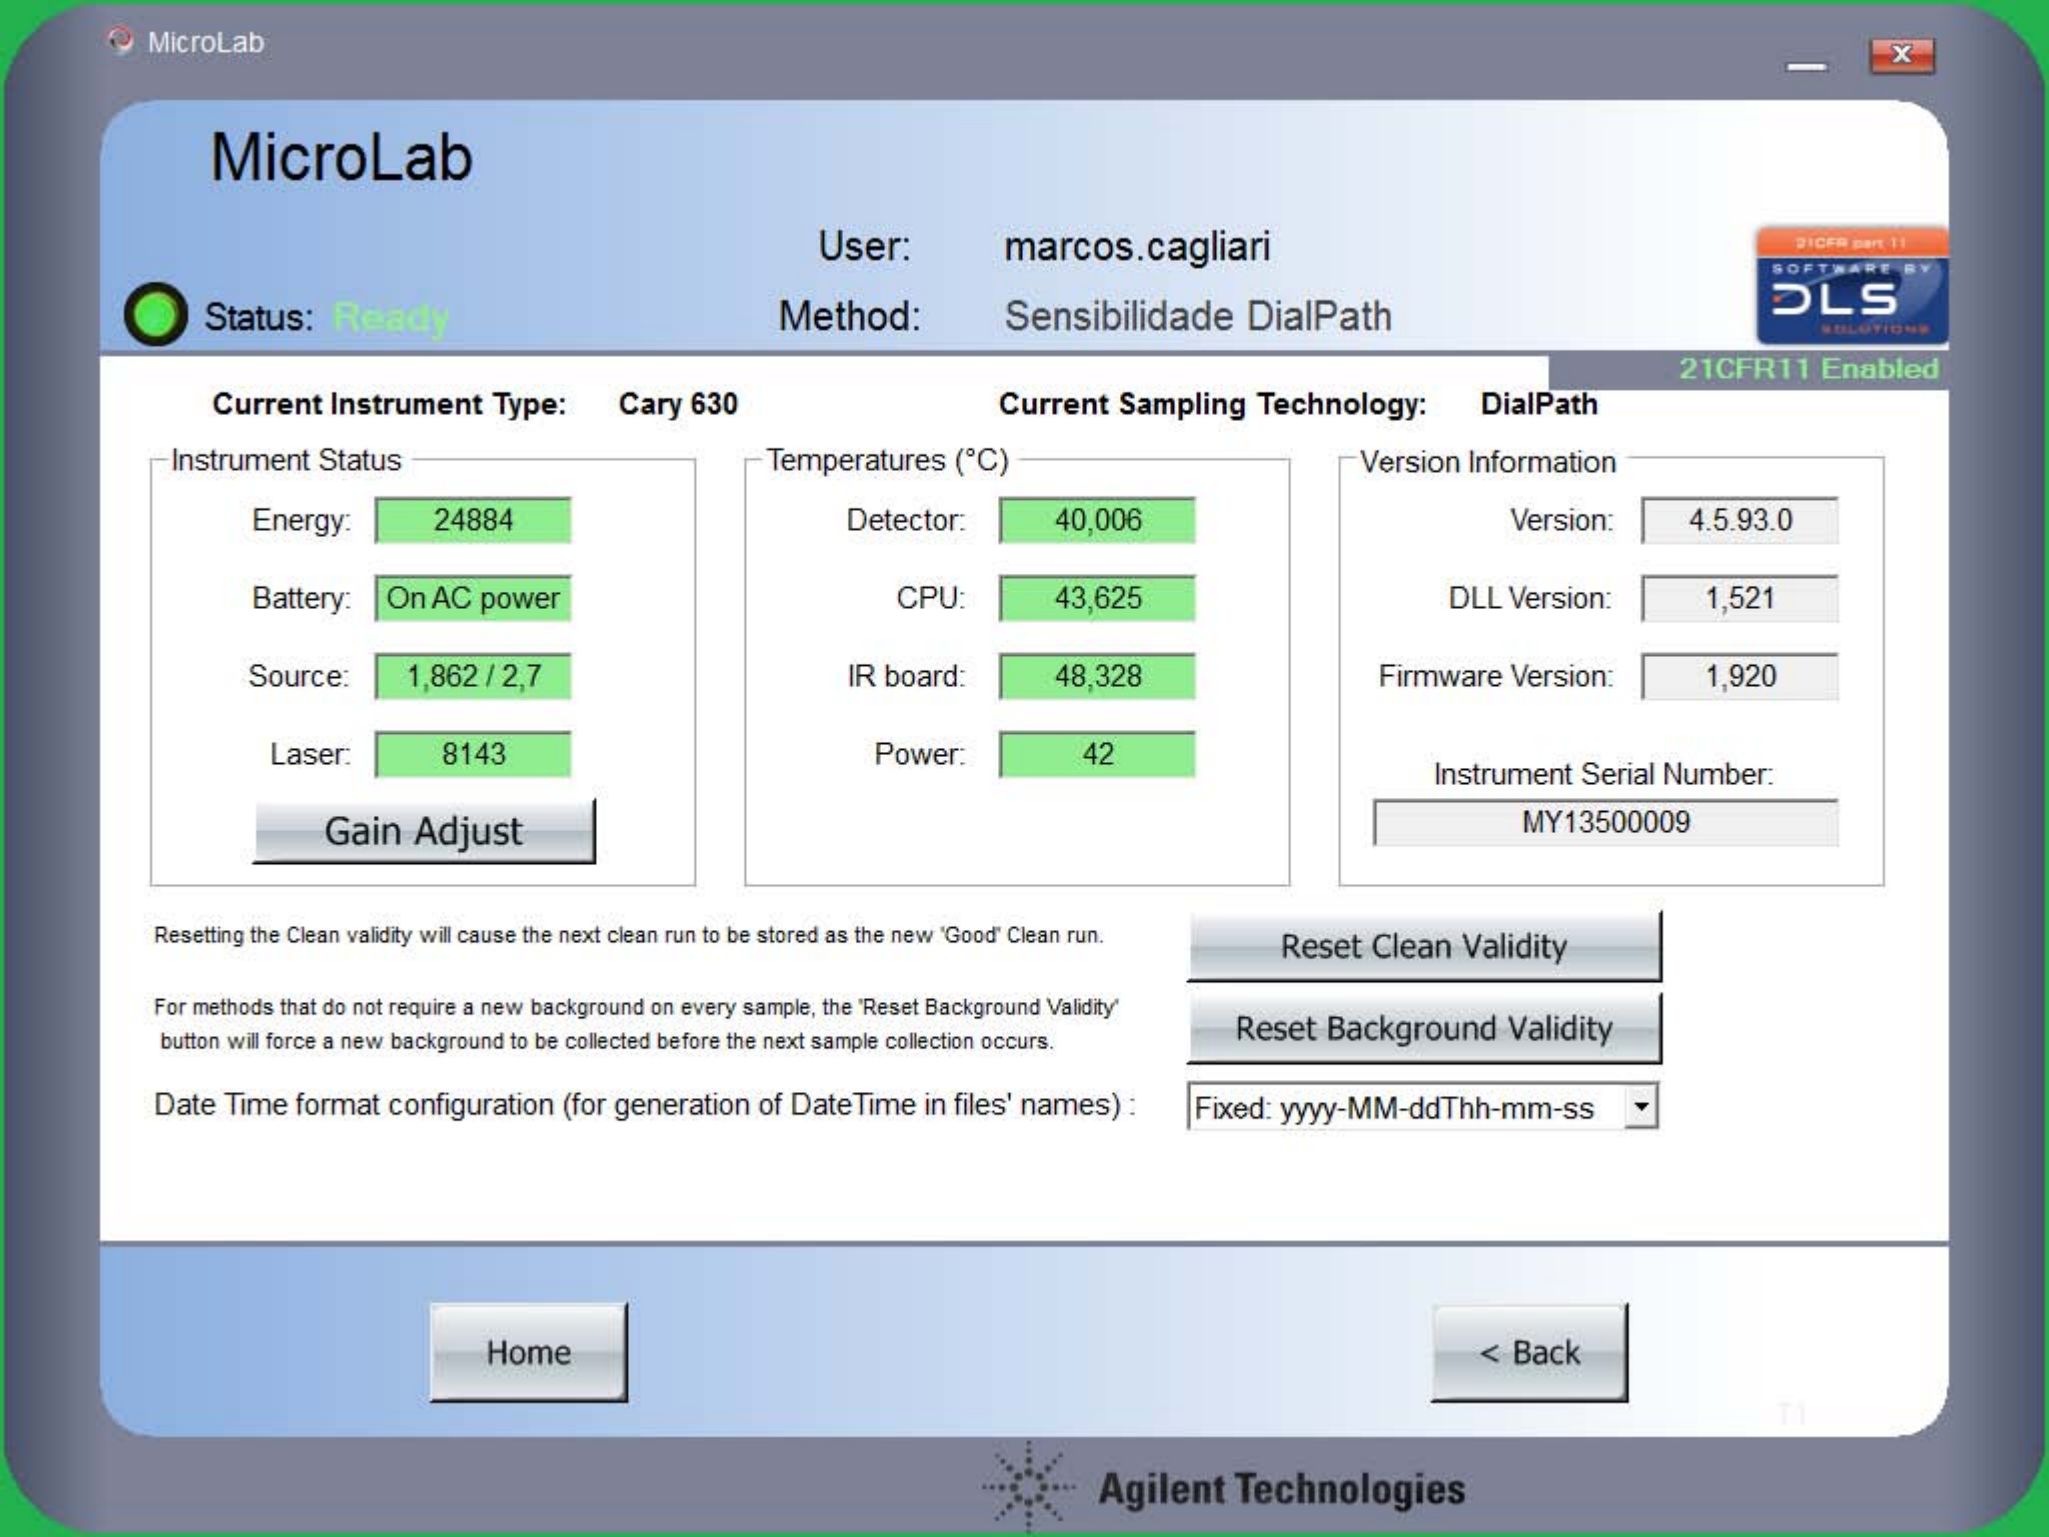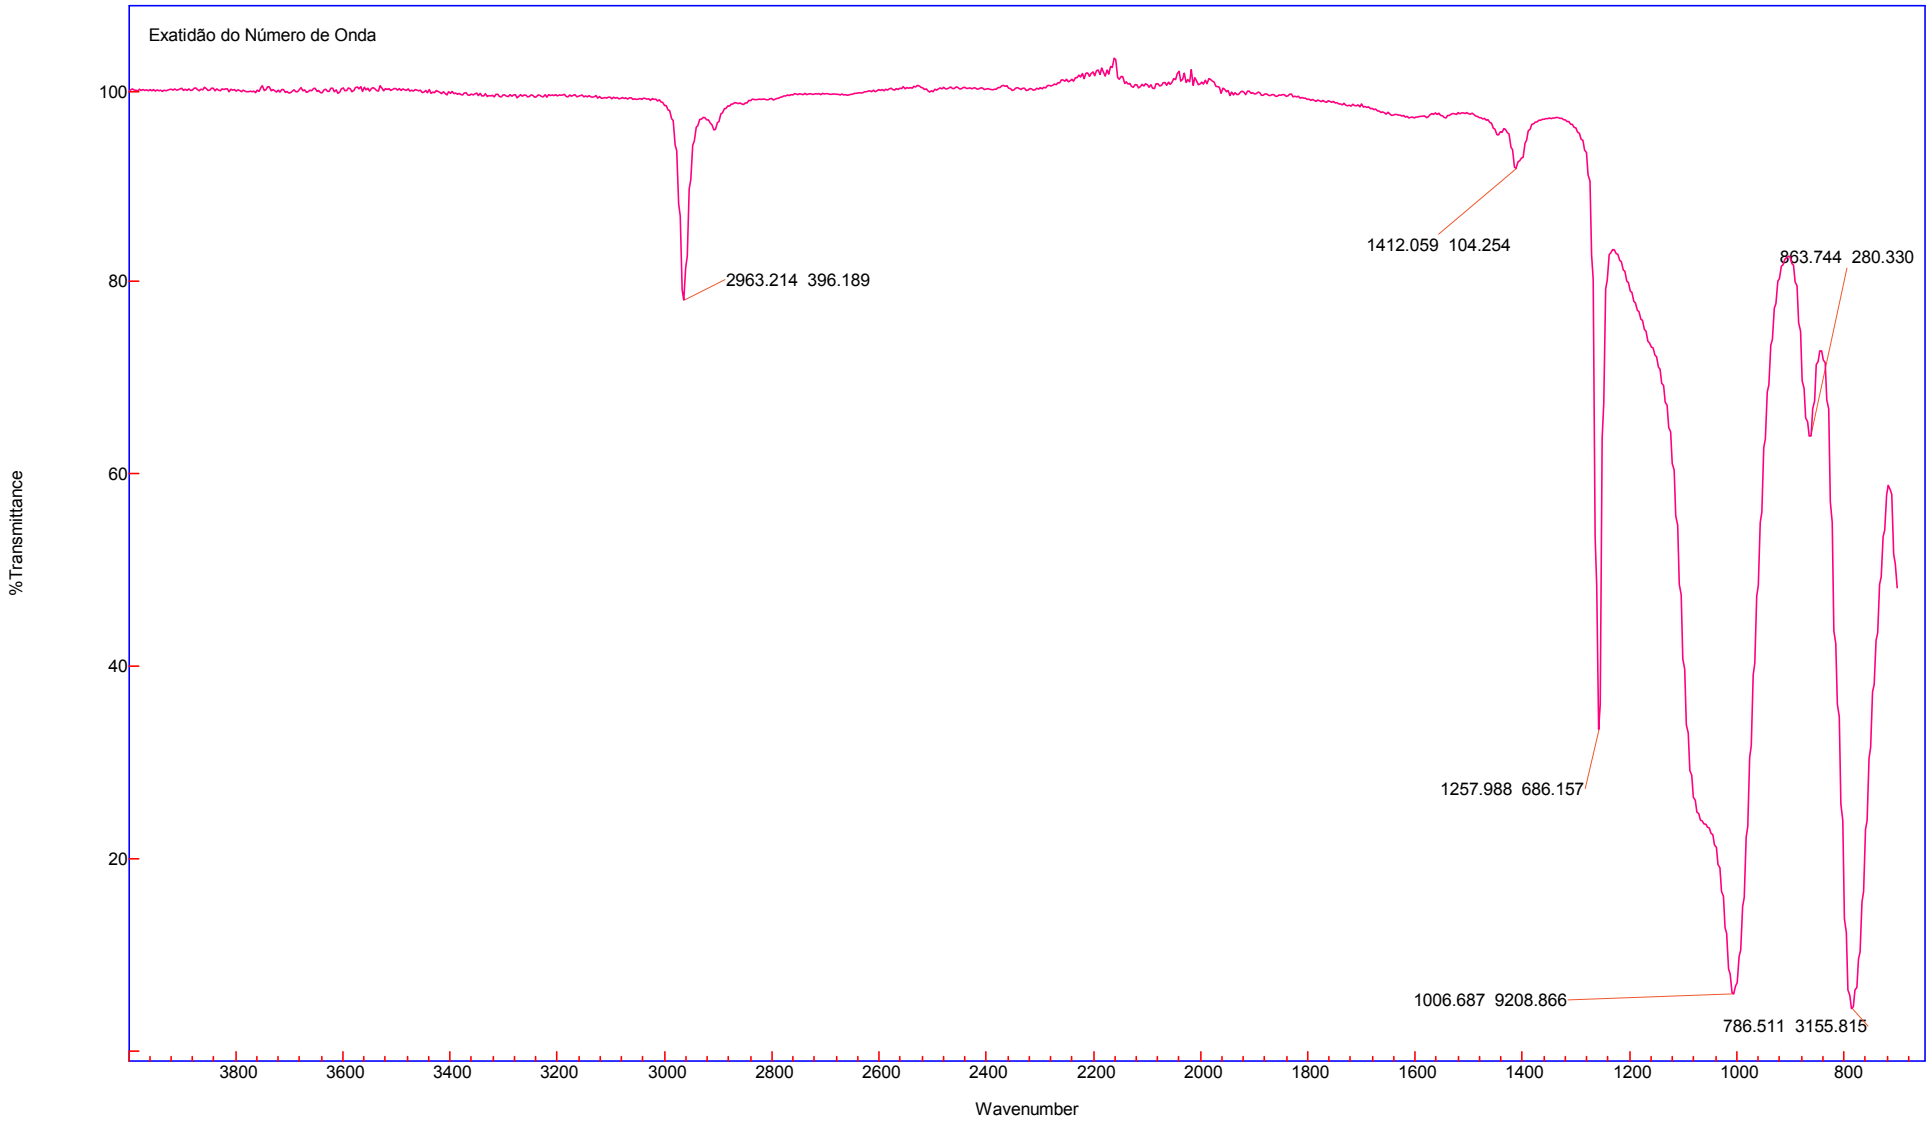


Name
Exatidão do Número de Onda

Agilent Resolutions Pro

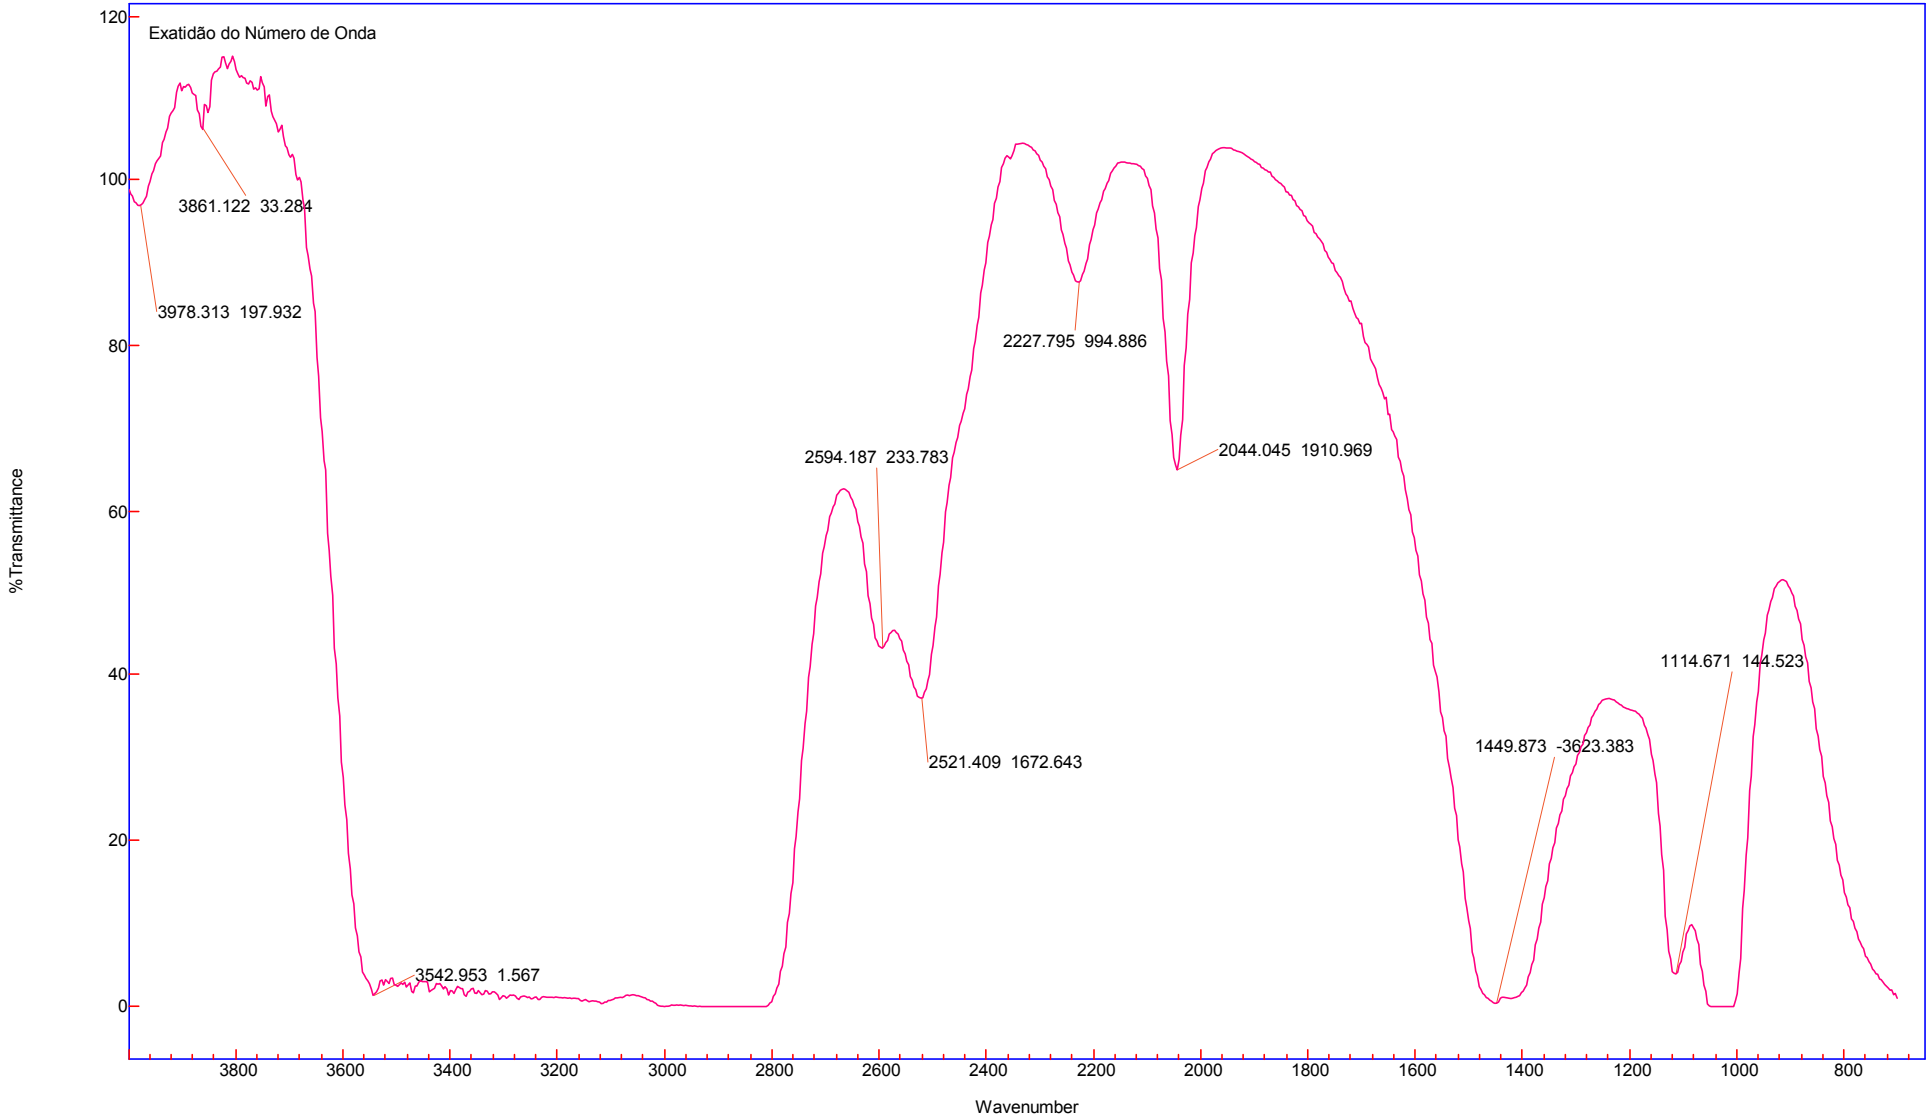


Name
Exatidão do Número de Onda

Agilent Resolutions Pro

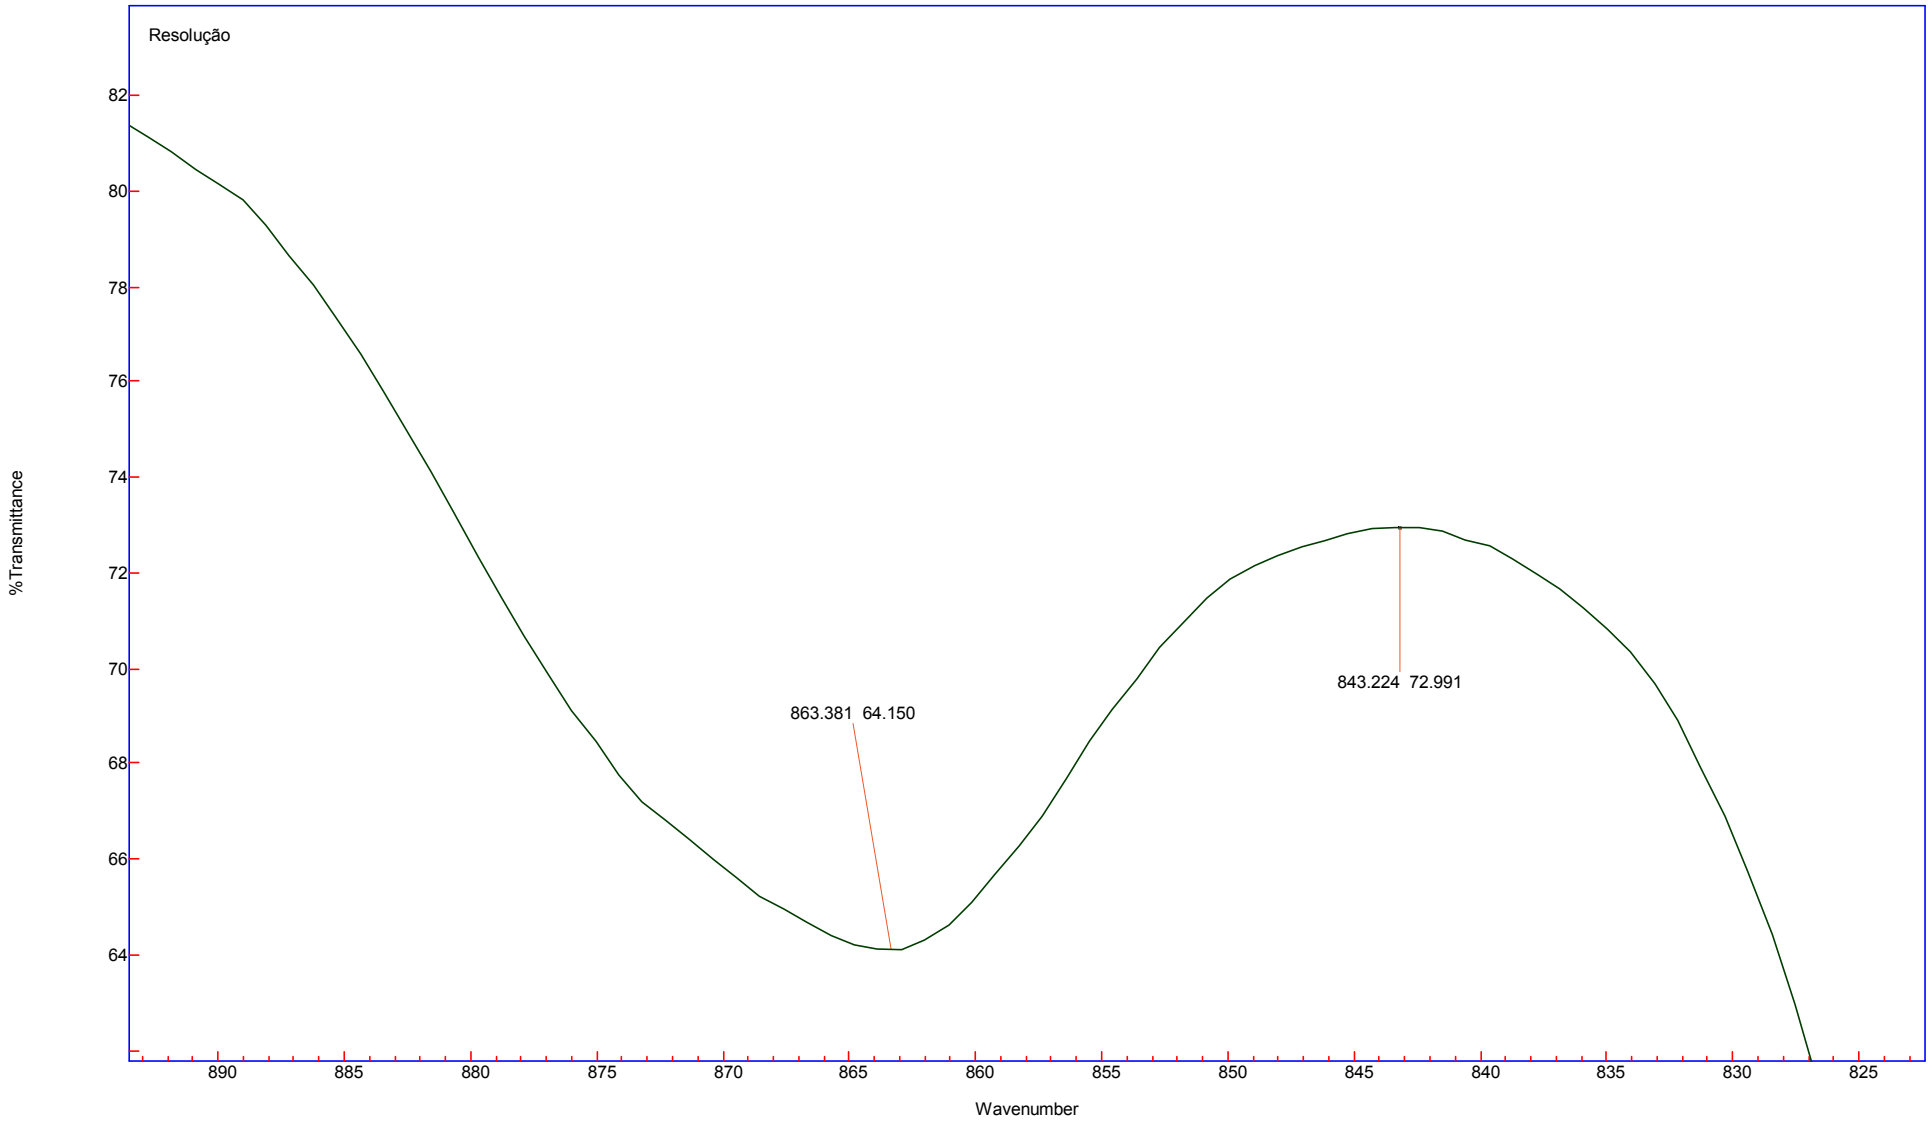

Name
Resolução

Agilent Resolutions Pro

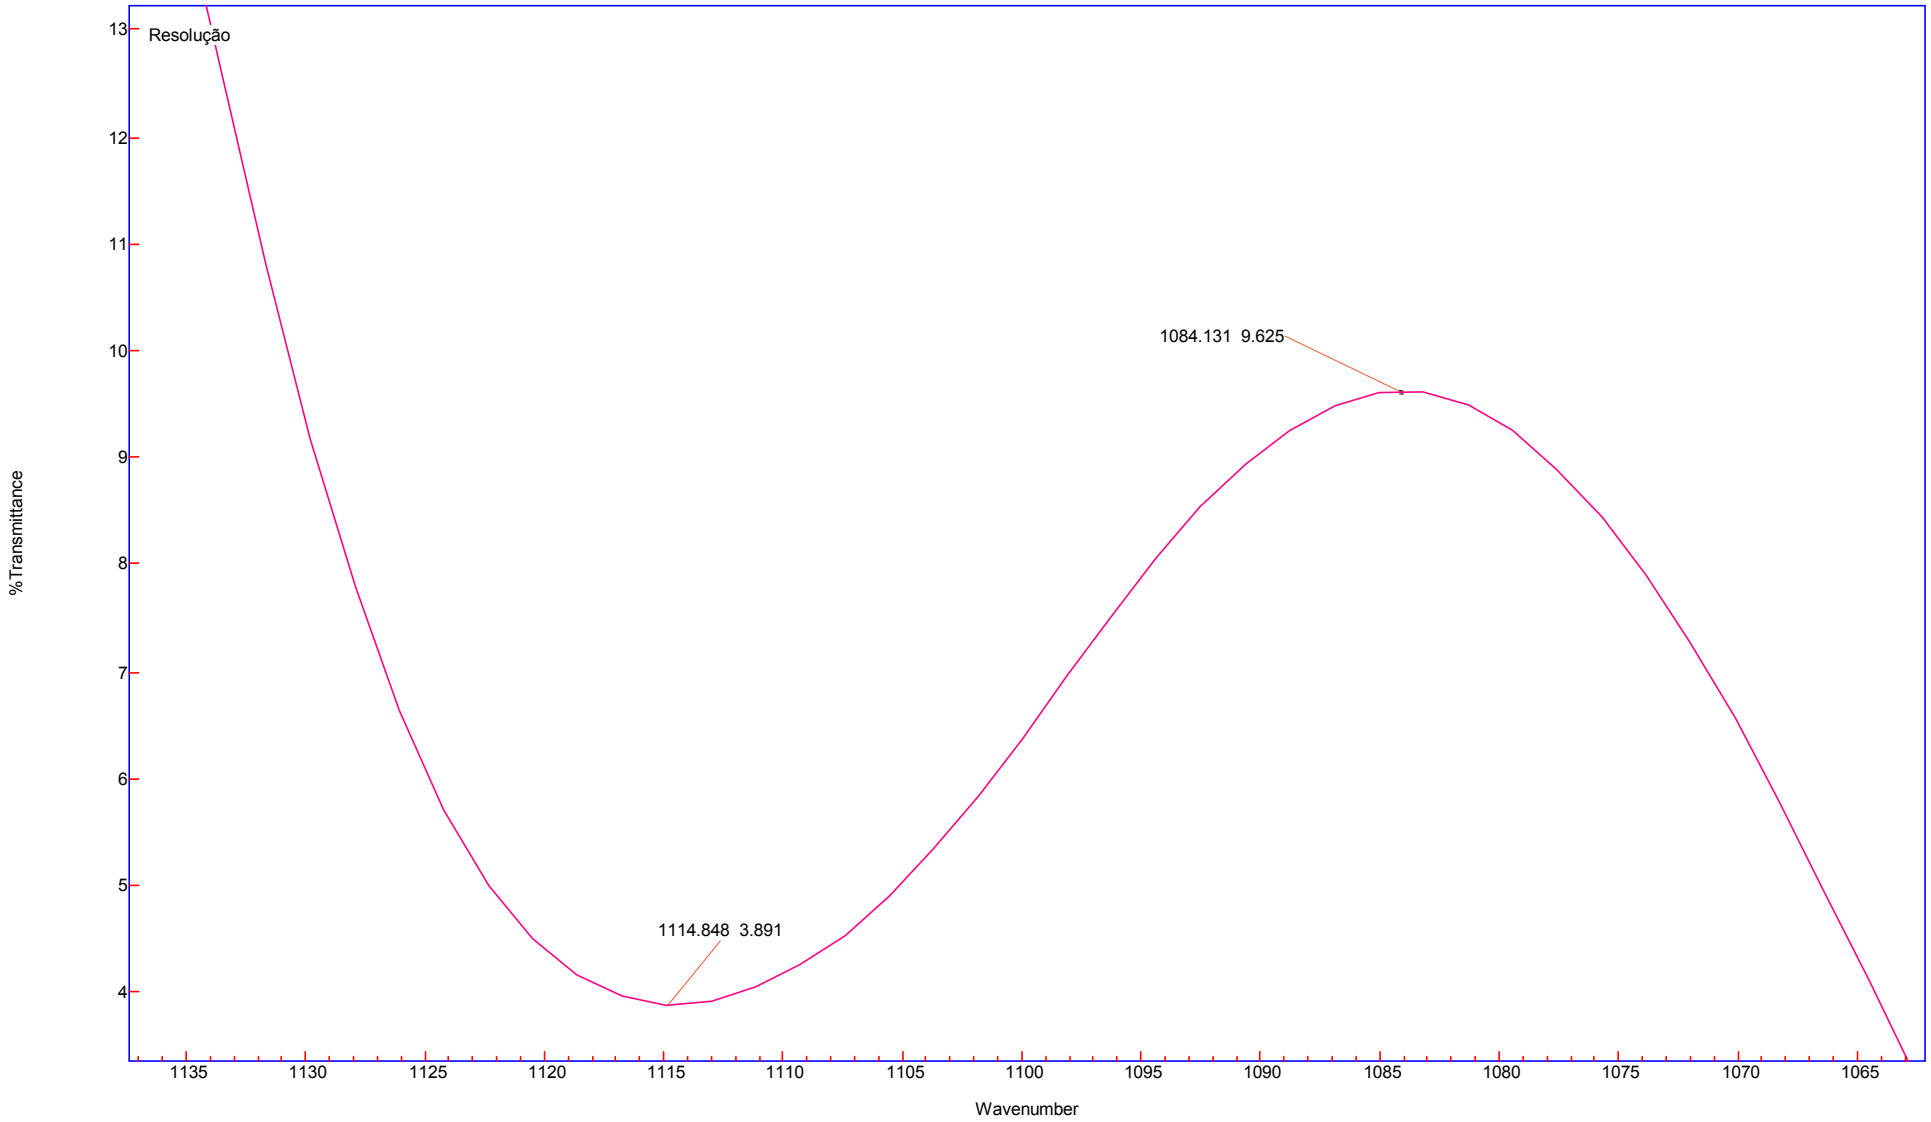


Name
Resolução

Agilent Resolutions Pro



Name
Repetibilidade do Número de Onda

Agilent Resolutions Pro

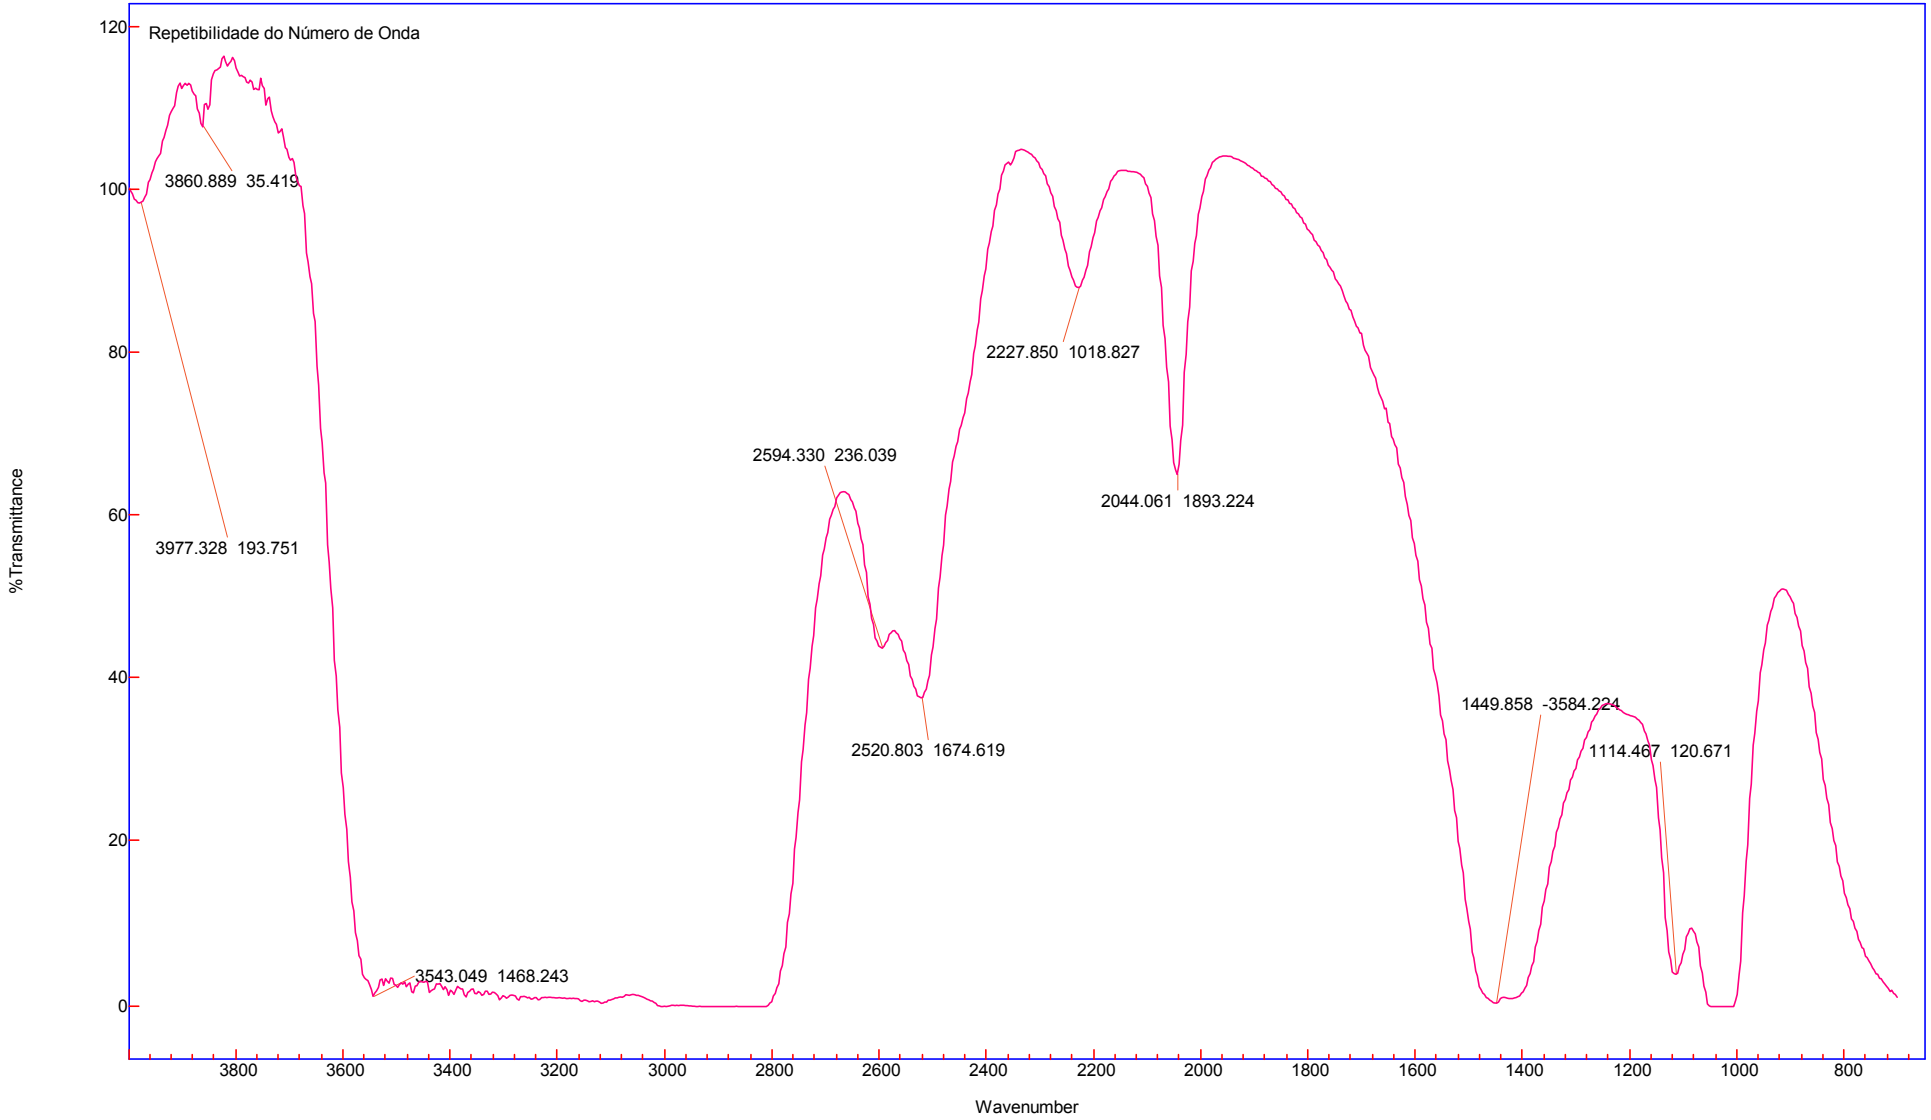


Name
Repetibilidade do Número de Onda

Agilent Resolutions Pro



Name
Repetibilidade do Número de Onda

Agilent Resolutions Pro

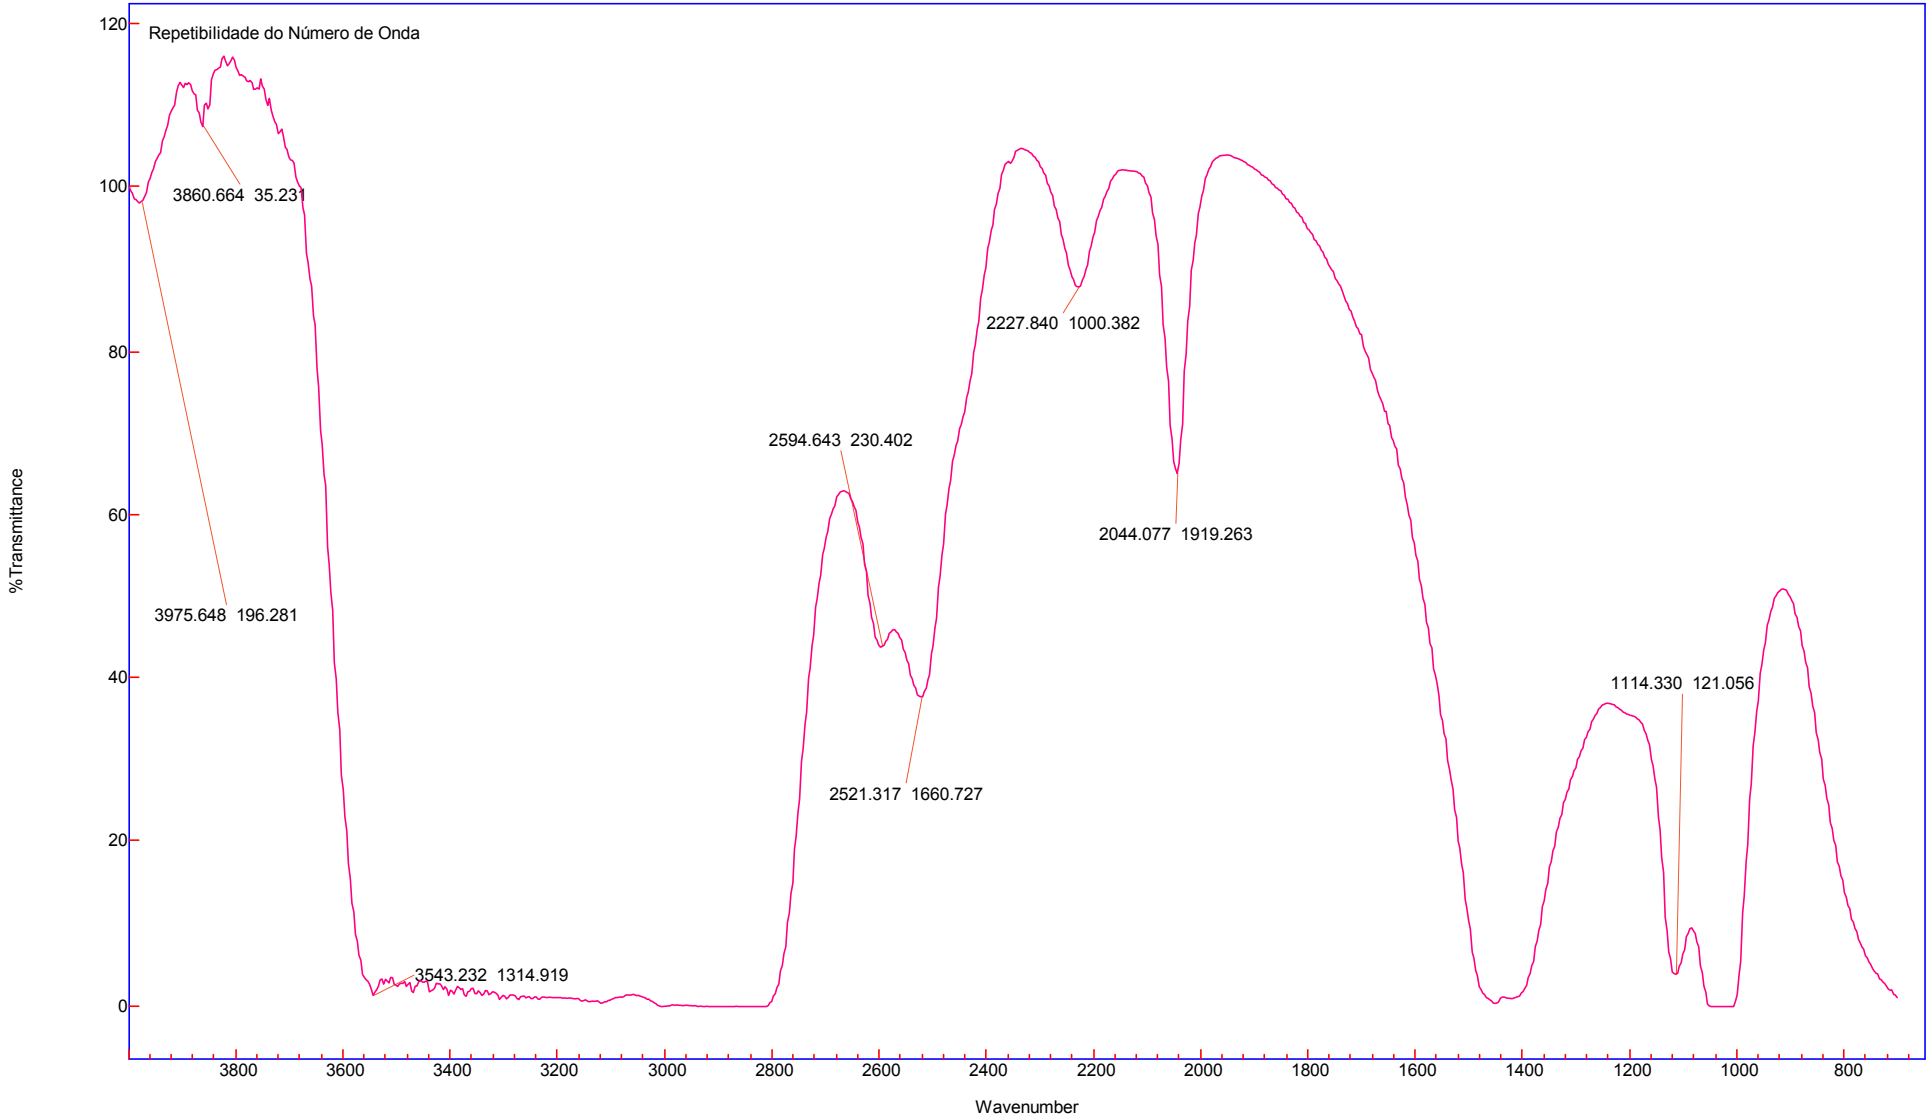


Name
Repetibilidade do Número de Onda

Agilent Resolutions Pro




Name
Repetibilidade Fotométrica

Agilent Resolutions Pro

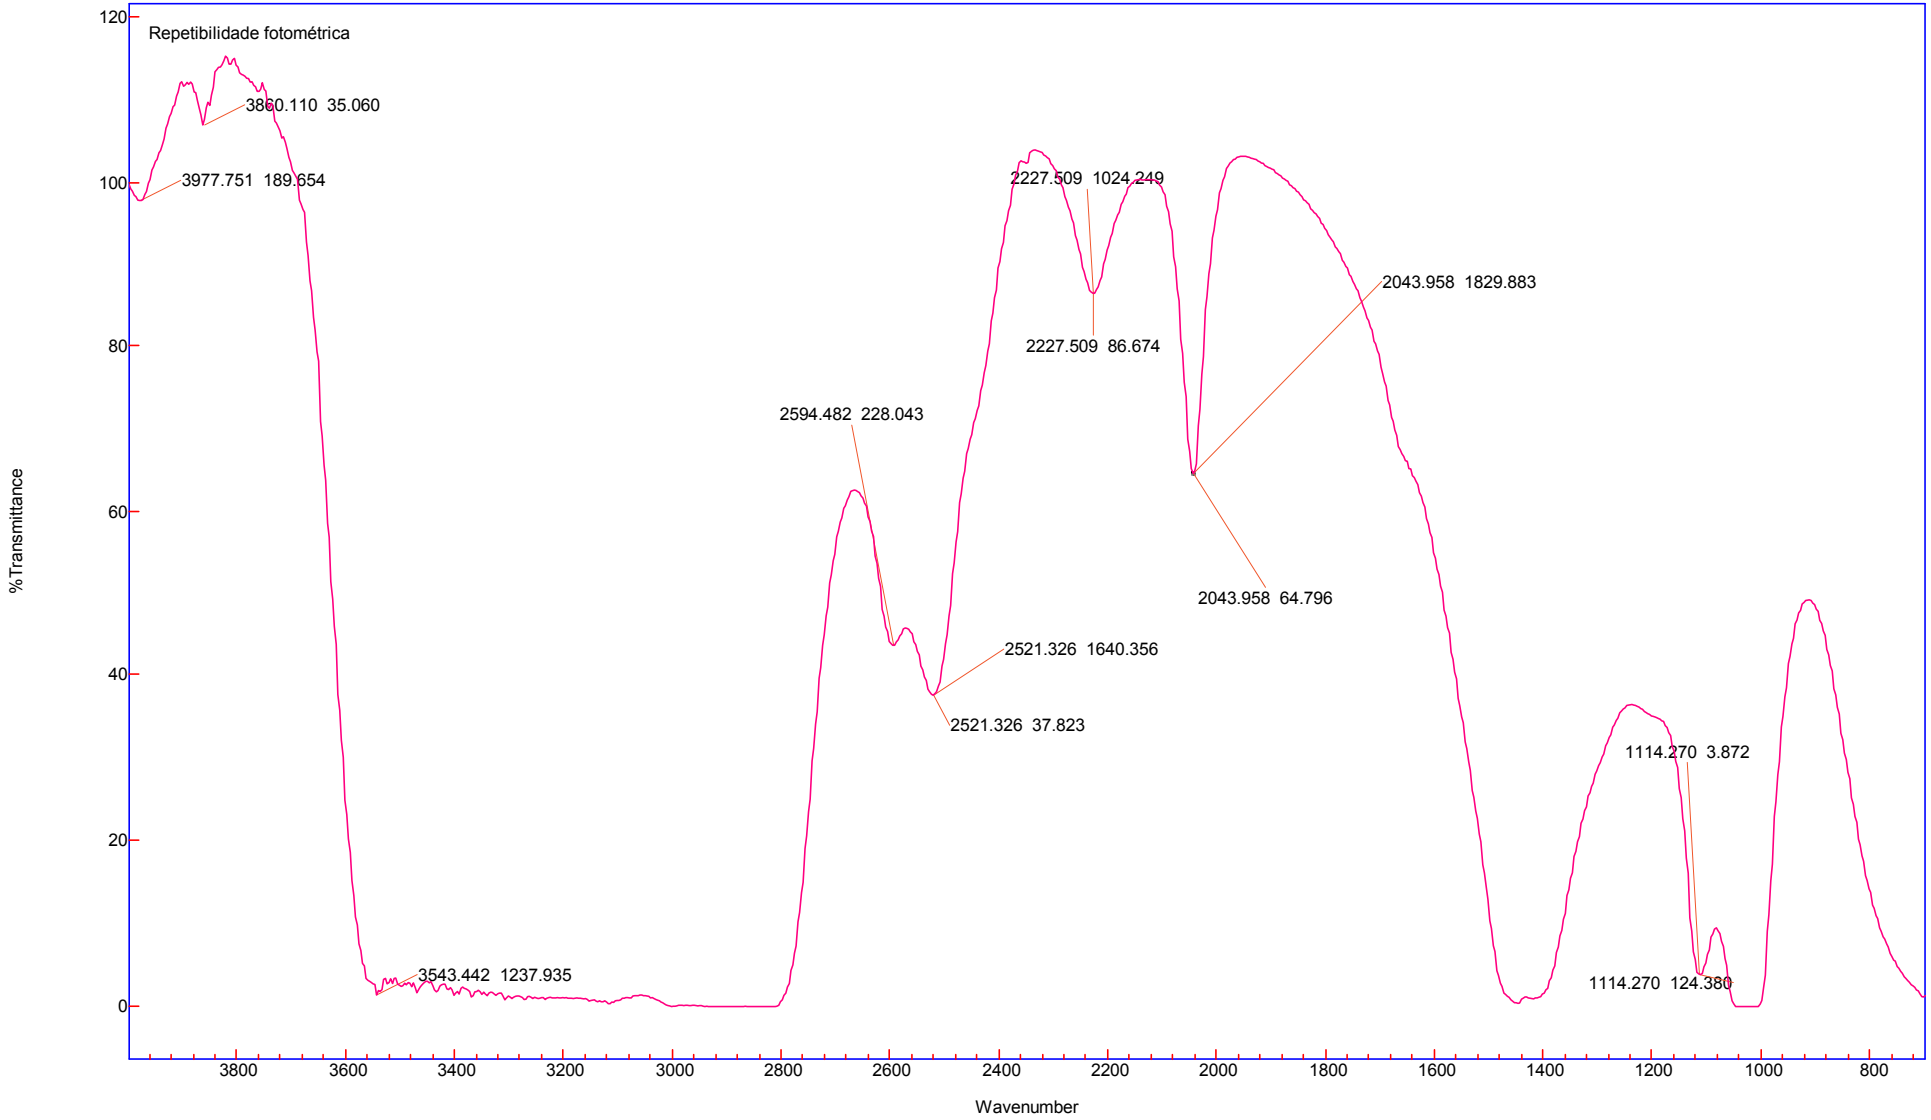


Name
Repetibilidade fotométrica

Agilent Resolutions Pro

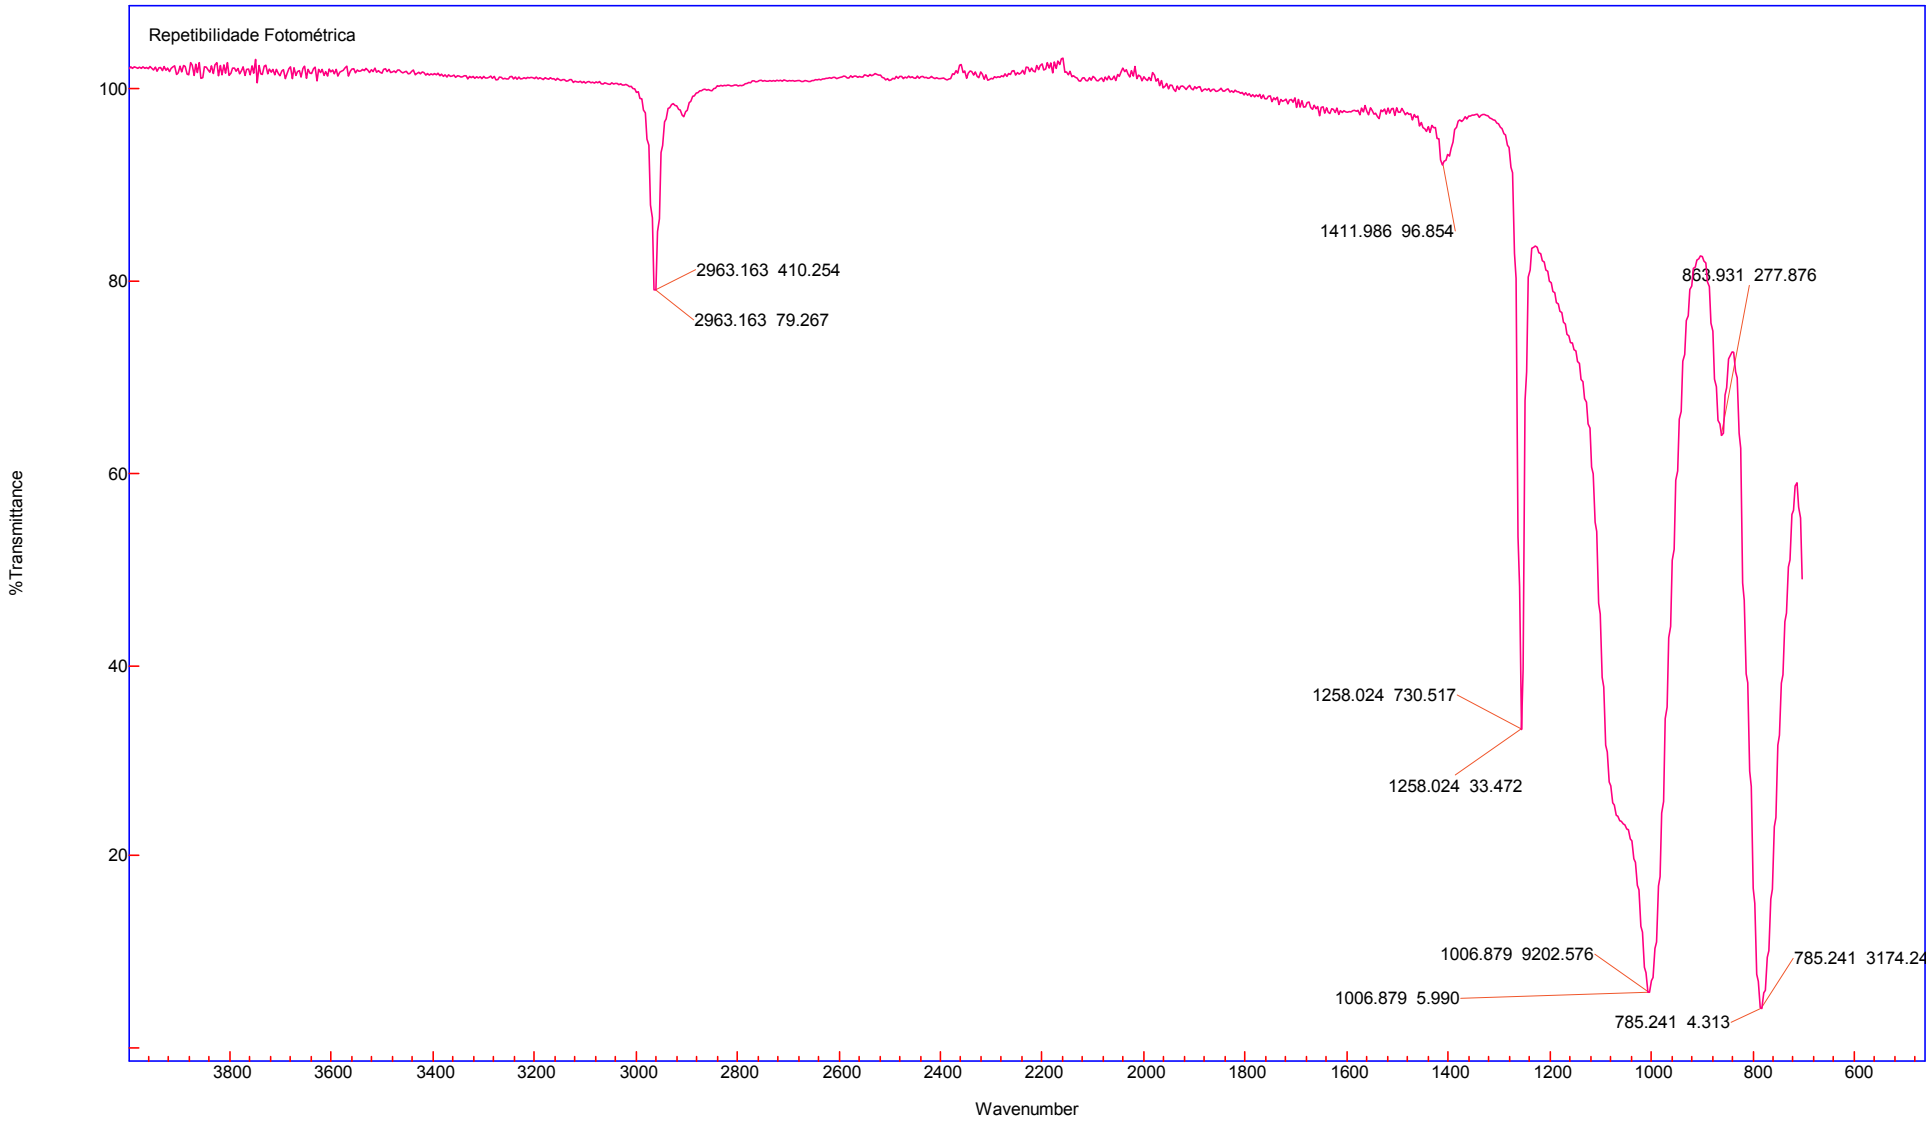

Name
Repetibilidade Fotométrica

Agilent Resolutions Pro

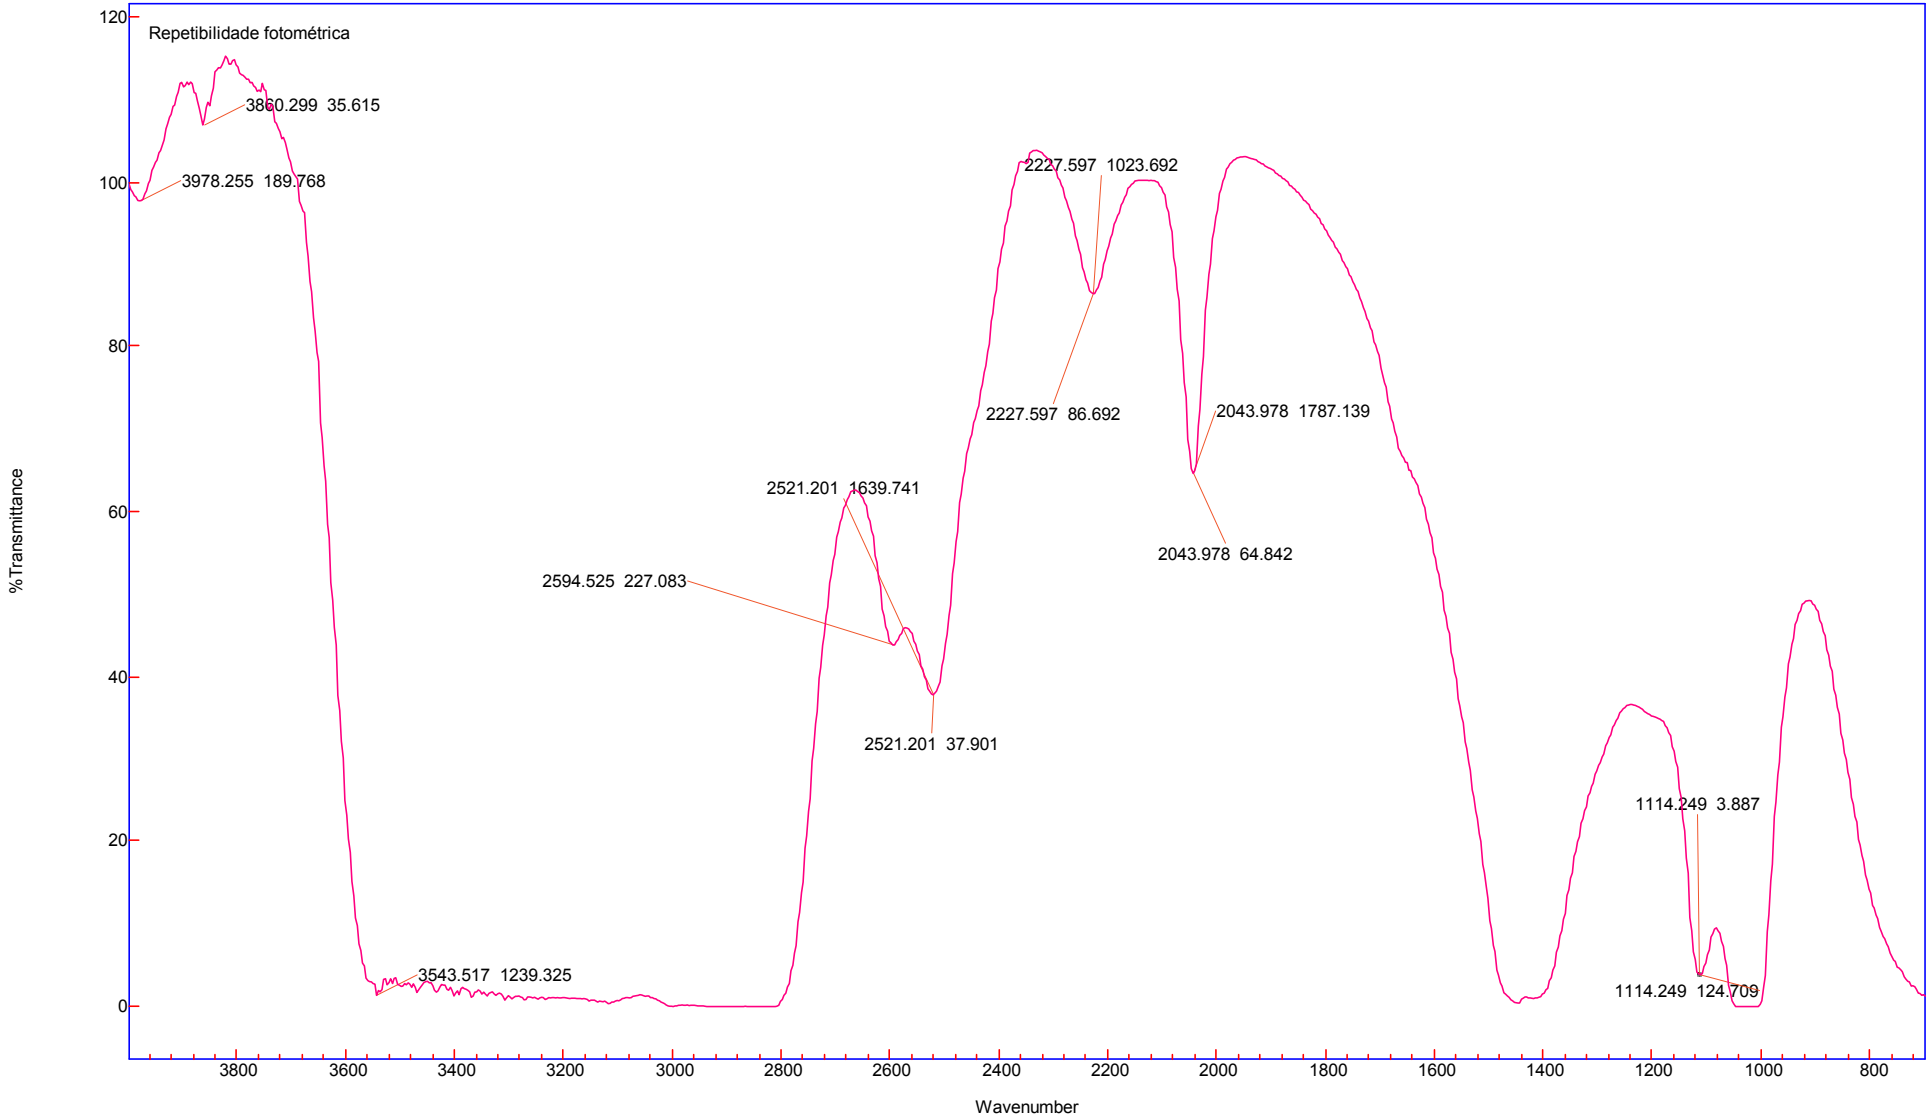

Name
Repetibilidade fotométrica

Agilent Resolutions Pro



Name
Sensibilidade

Agilent Resolutions Pro



Name
Sensibilidade