
Peak Find - LDUV 4_002 PDA_1,7600.JWS

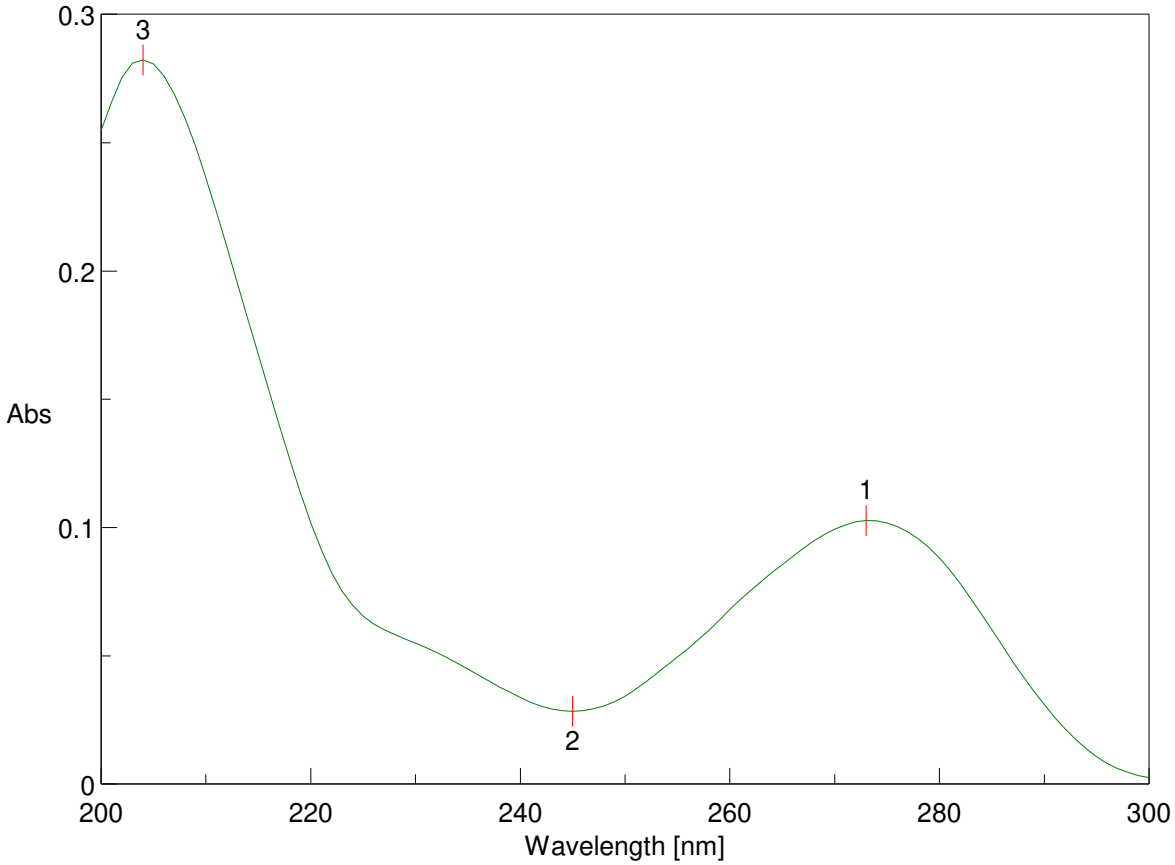

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	22/10/2020 15:34
Date modified	22/10/2020 15:40

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	072260870
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.102632	2	245	0.028304
3	204	0.28217			

Chromatogram

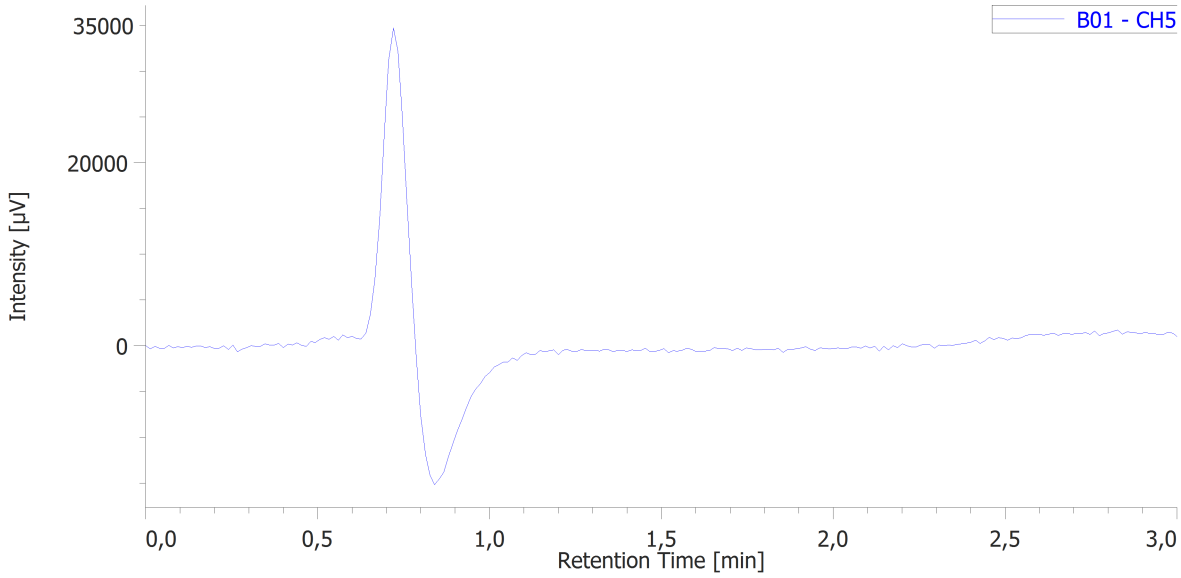


Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:53
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:23:17
Volume	10,0 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	B01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

Creator QPackSA
Reviewer
Approver

Chromatogram

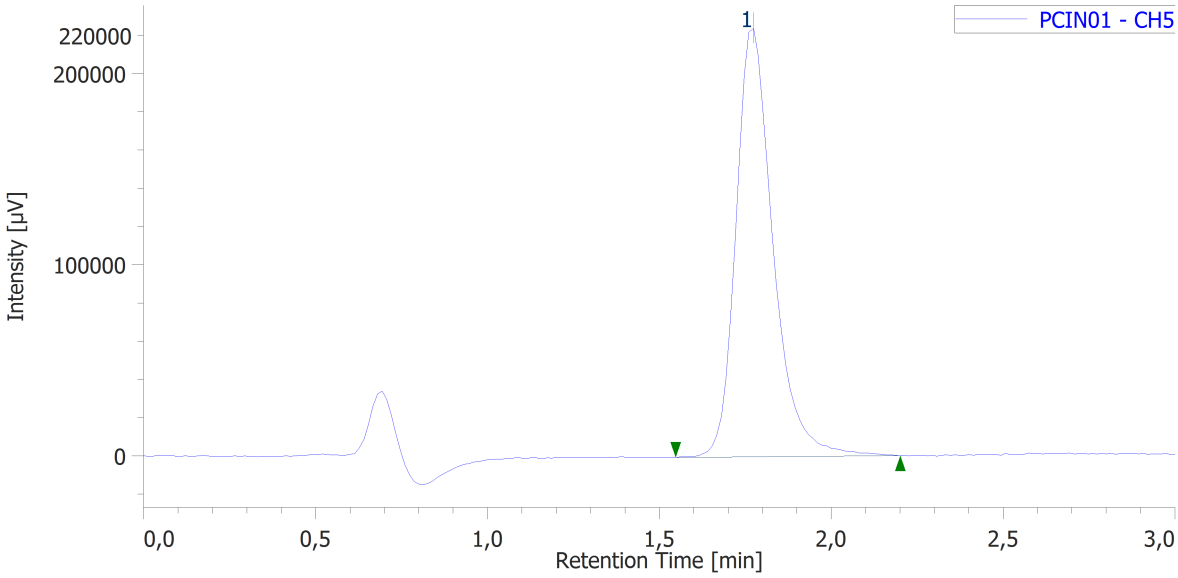

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:53
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:27:07
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,773	1689802	224358	100,000	100,000	N/A	1432	N/A	1,254	

Creator QPackSA
Reviewer
Approver

Chromatogram

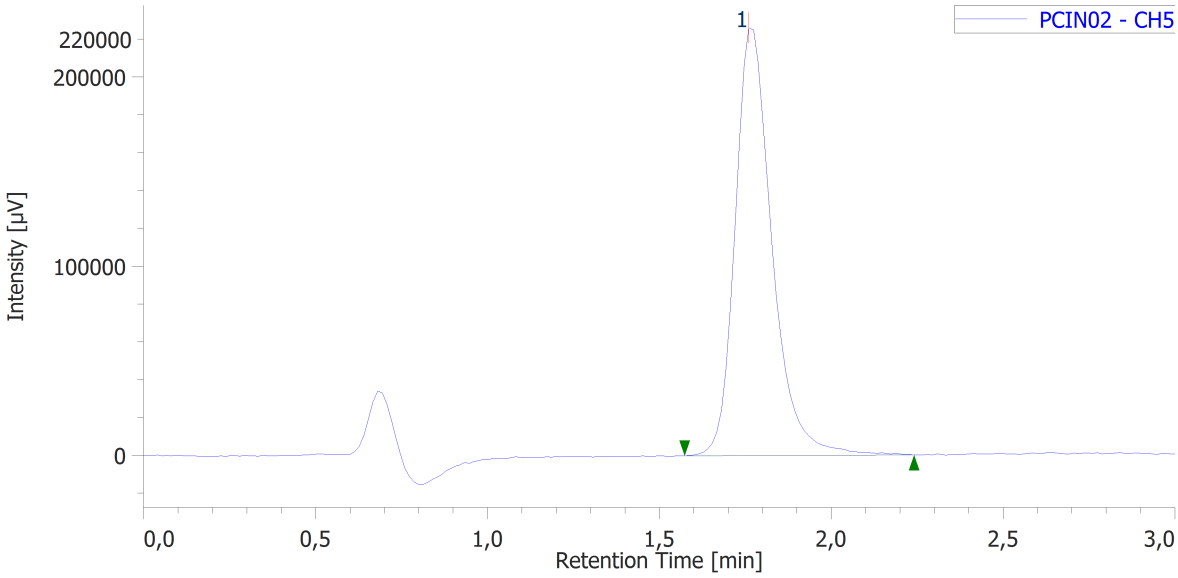

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:30:57
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,760	1685926	225840	100,000	100,000	N/A	1432	N/A	1,382	

Creator QPackSA
Reviewer
Approver

Chromatogram

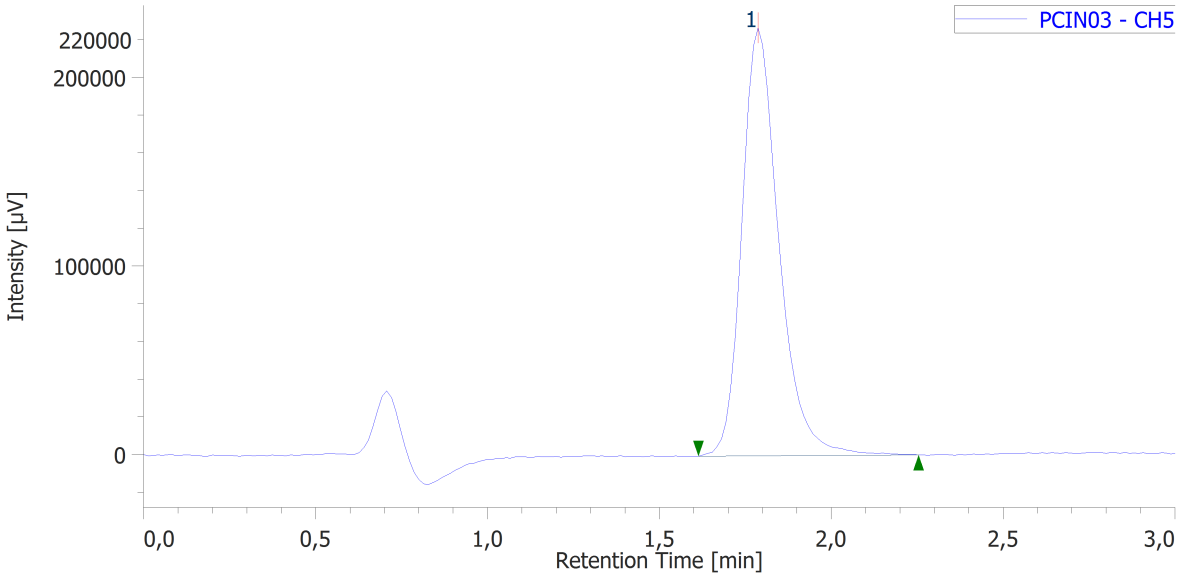

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:34:47
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,787	1696489	226753	100,000	100,000	N/A	1442	N/A	1,275	

Creator QPackSA
Reviewer
Approver

Chromatogram

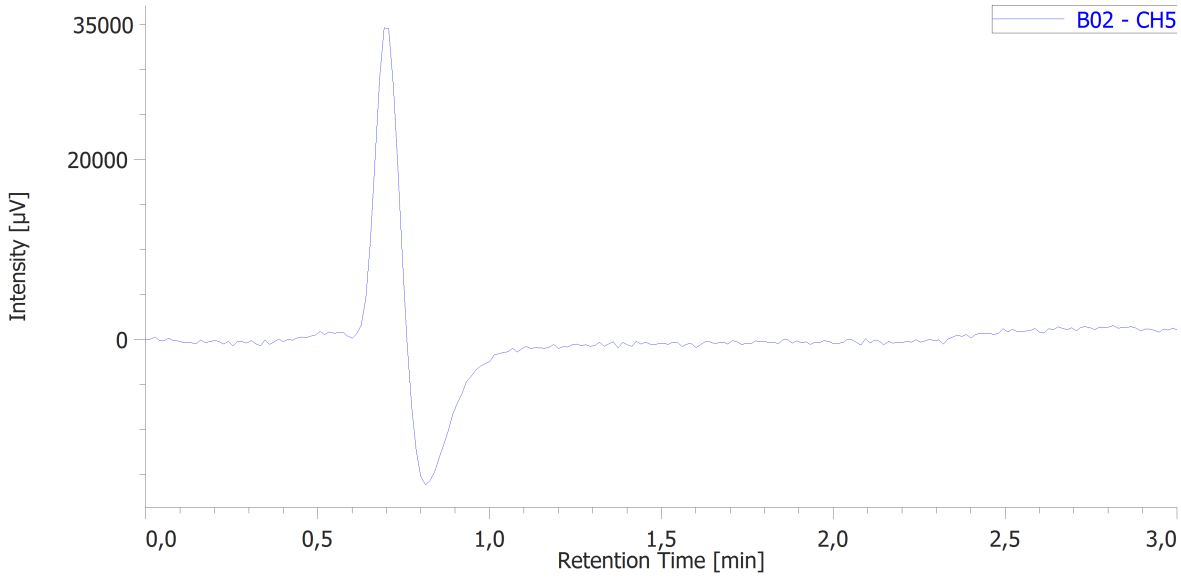


Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:38:34
Volume	10,0 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	B02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

Creator QPackSA
Reviewer
Approver

Chromatogram

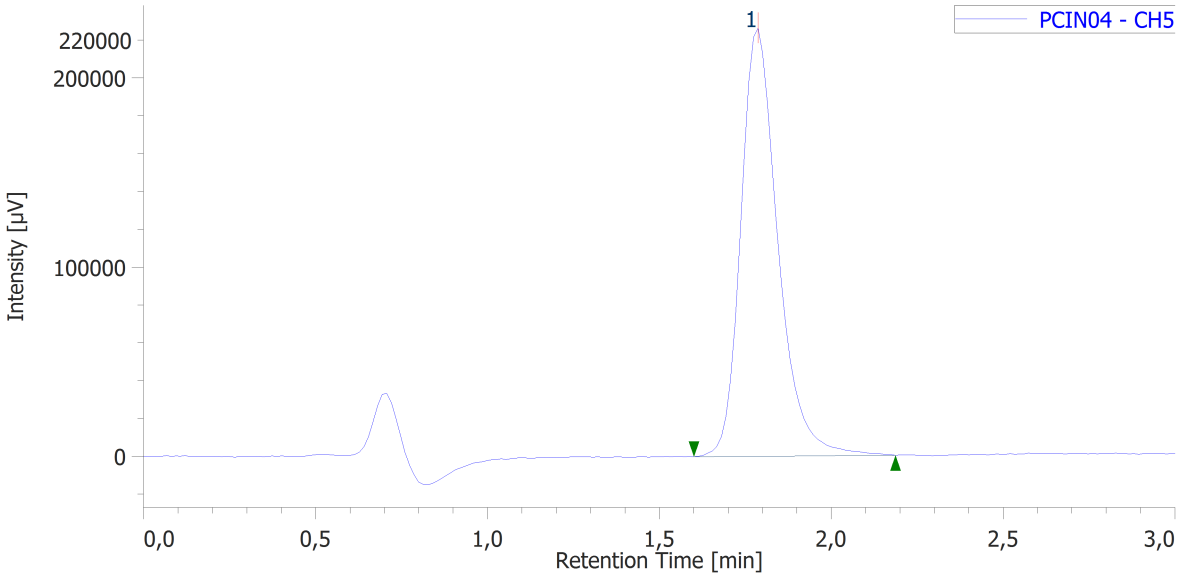

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:42:24
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,787	1699918	226388	100,000	100,000	N/A	1429	N/A	1,253	

Creator QPackSA
Reviewer
Approver

Chromatogram

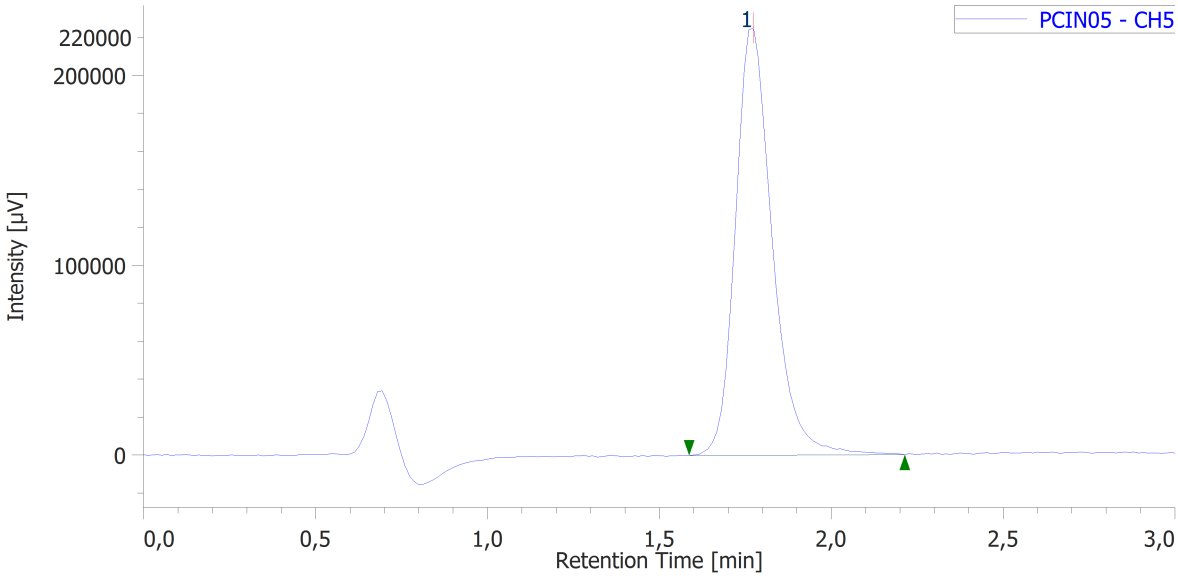

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:46:12
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,773	1686150	224973	100,000	100,000	N/A	1421	N/A	1,200	

Creator QPackSA
Reviewer
Approver

Chromatogram

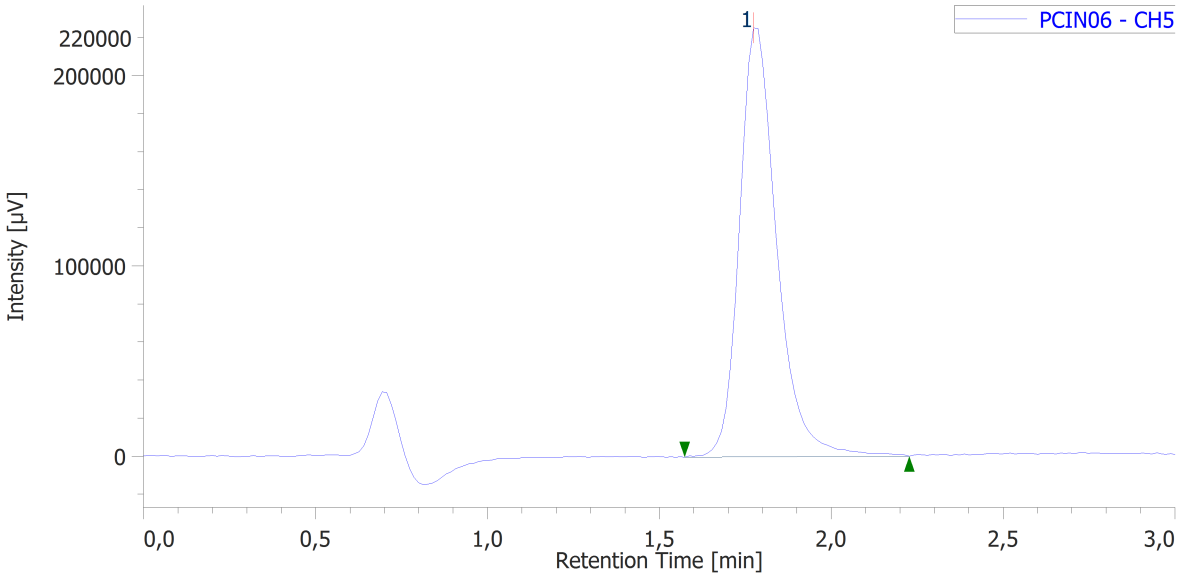

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:50:02
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,773	1705961	225313	100,000	100,000	N/A	1411	N/A	1,365	

Creator QPackSA
Reviewer
Approver

Chromatogram

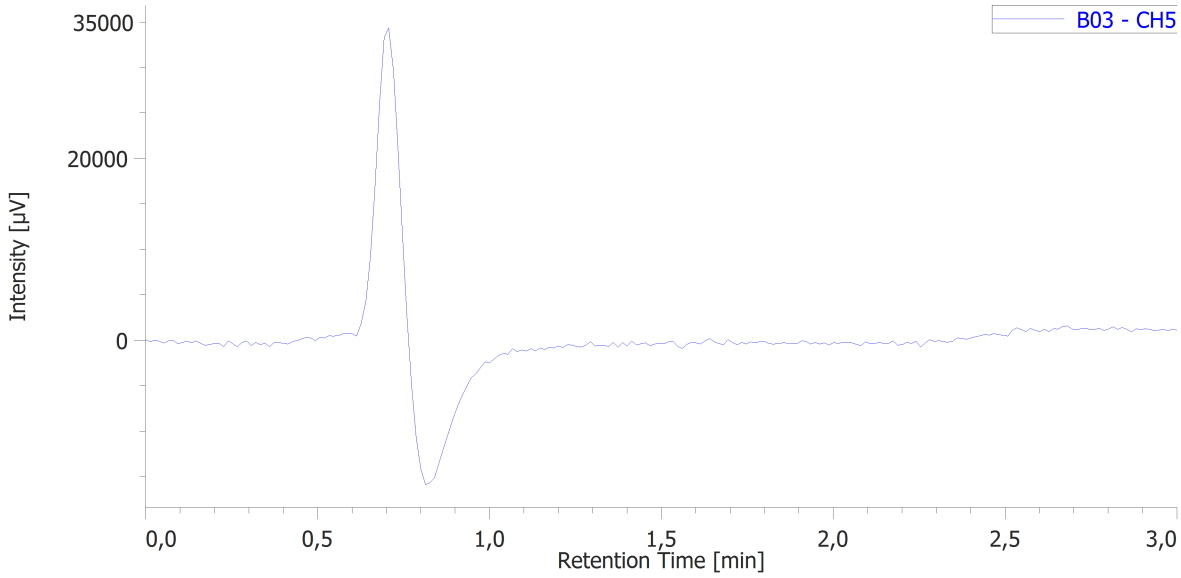


Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:20:54
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:53:47
Volume	10,0 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	B03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

Creator QPackSA
Reviewer
Approver

Chromatogram

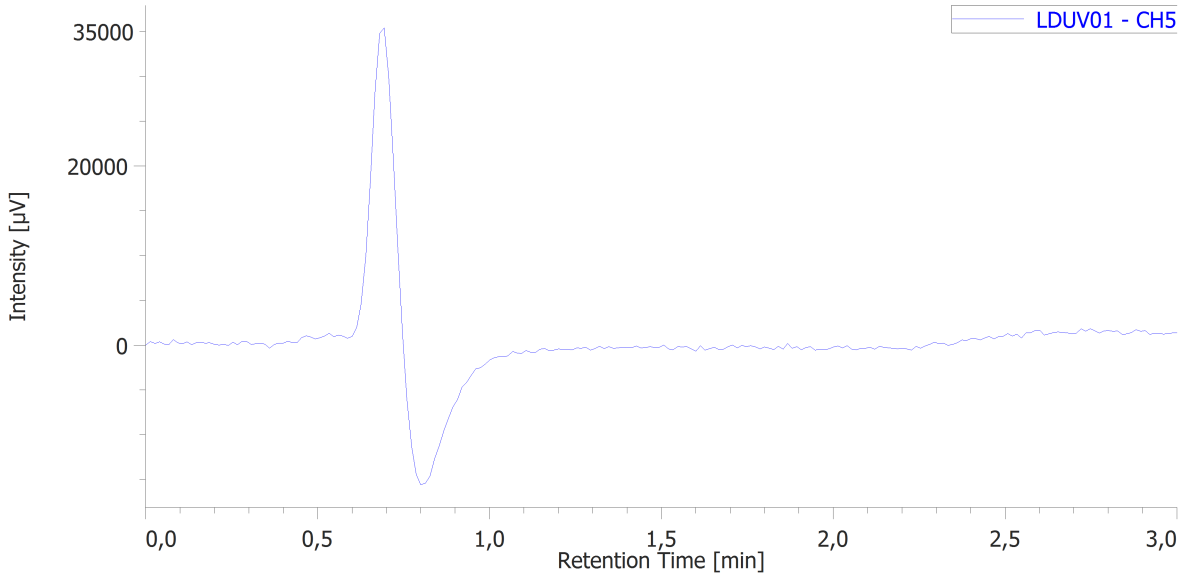


Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:41:13
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 12:57:34
Volume	10,0 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

Creator QPackSA
Reviewer
Approver

Chromatogram

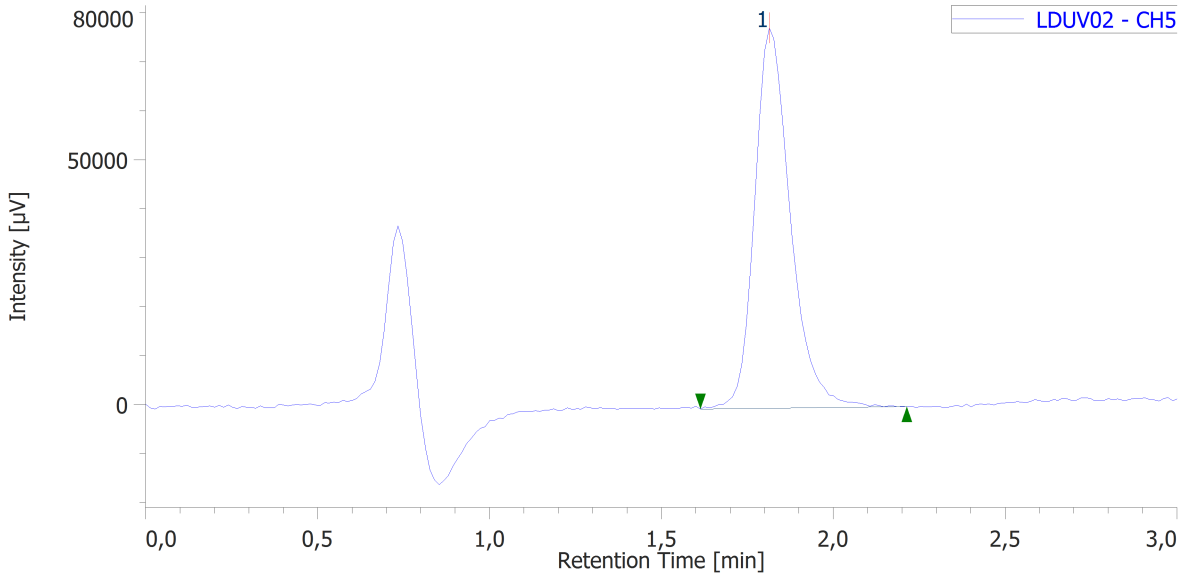

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:41:13
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:01:22
Volume	10,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,813	560987	77623	100,000	100,000	N/A	1586	N/A	1,330	

Creator QPackSA
Reviewer
Approver

Chromatogram

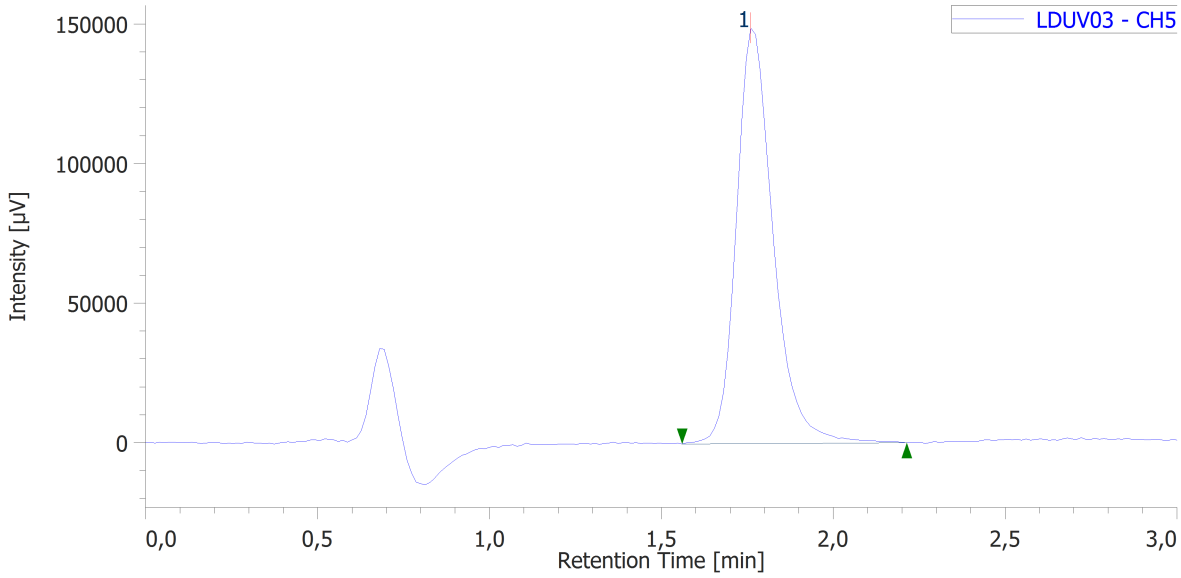

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:41:13
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:05:12
Volume	10,0 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,760	1110316	148818	100,000	100,000	N/A	1422	N/A	1,320	

Creator QPackSA
Reviewer
Approver

Chromatogram

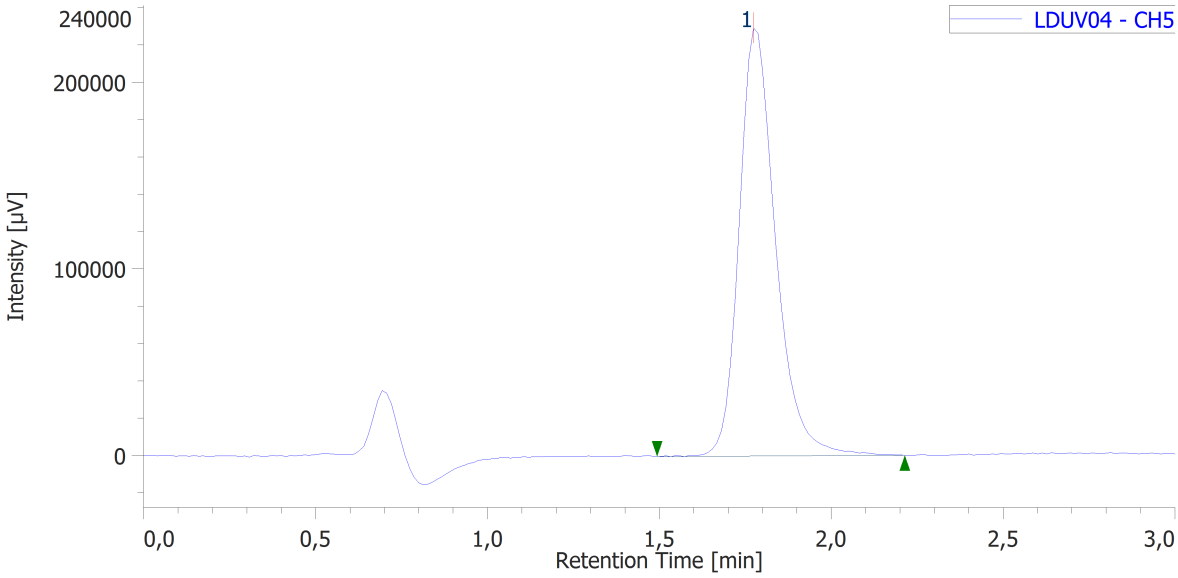

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:41:13
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:09:01
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,773	1692537	229340	100,000	100,000	N/A	1460	N/A	1,327	

Creator QPackSA
Reviewer
Approver

Chromatogram

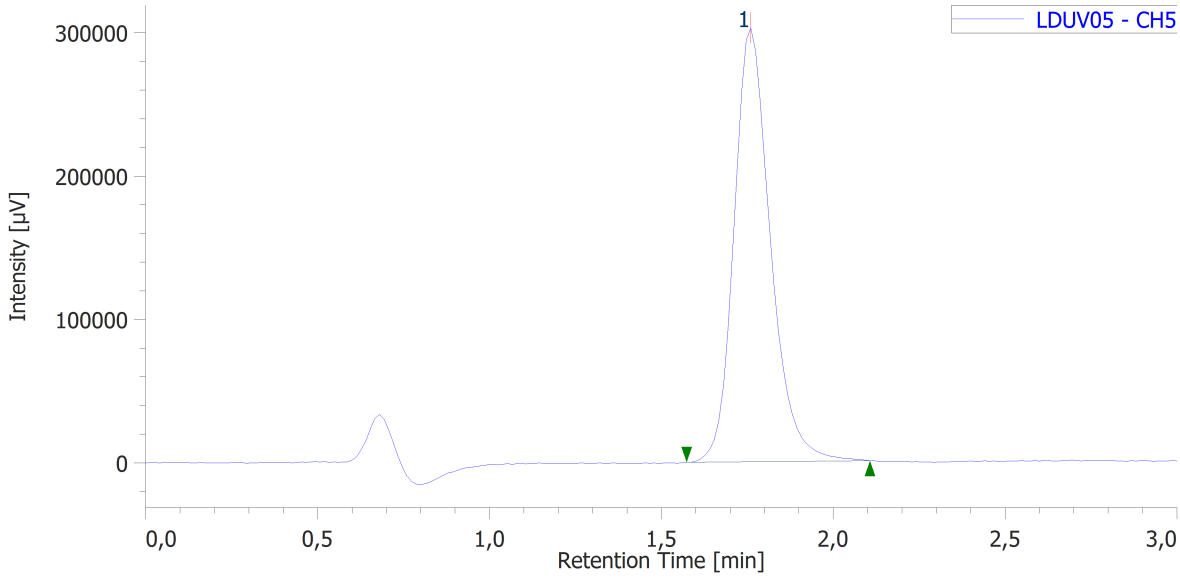

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:44:38
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:12:51
Volume	10,0 [µL]
Sample #	50
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,760	2228814	302338	100,000	100,000	N/A	1419	N/A	1,210	

Creator QPackSA
Reviewer
Approver

Chromatogram

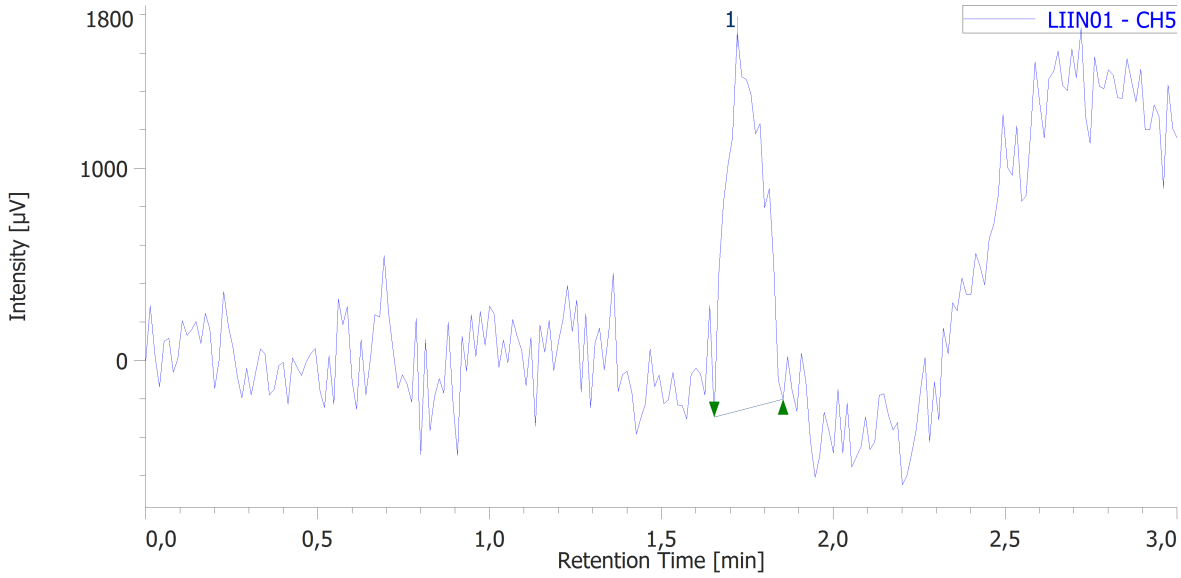

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:53:34
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:16:39
Volume	0,1 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,720	13954	1973	100,000	100,000	N/A	816	N/A	1,431	

Creator QPackSA
Reviewer
Approver

Chromatogram

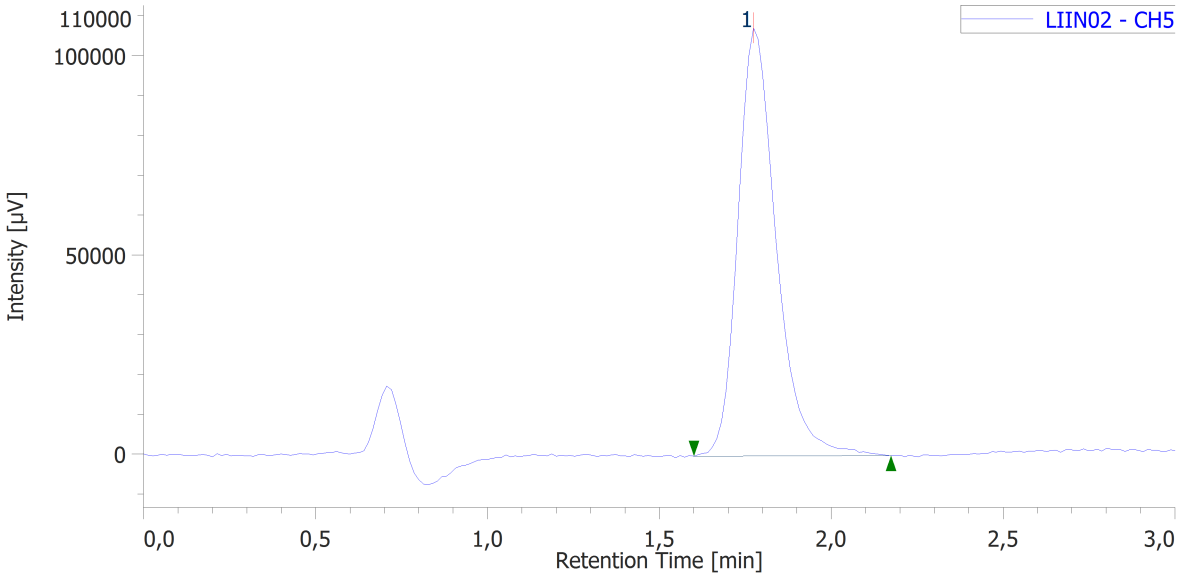

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:53:34
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:20:26
Volume	5,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,773	832075	107376	100,000	100,000	N/A	1321	N/A	1,326	

Creator QPackSA
Reviewer
Approver

Chromatogram

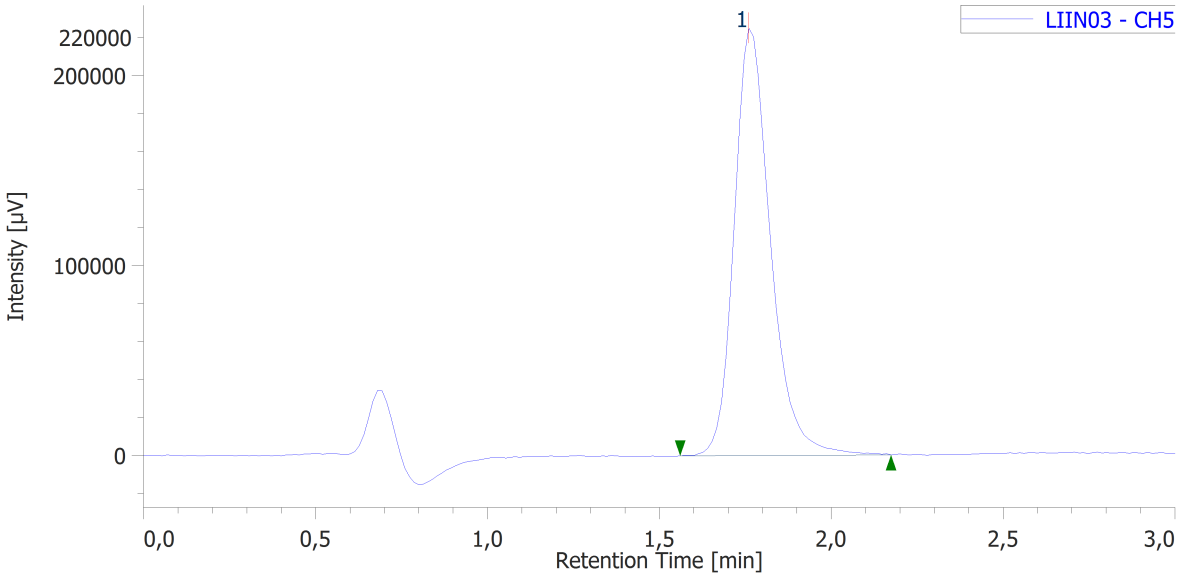

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:53:34
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:24:14
Volume	10,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,760	1649048	224885	100,000	100,000	N/A	1448	N/A	1,295	

Creator QPackSA
Reviewer
Approver

Chromatogram

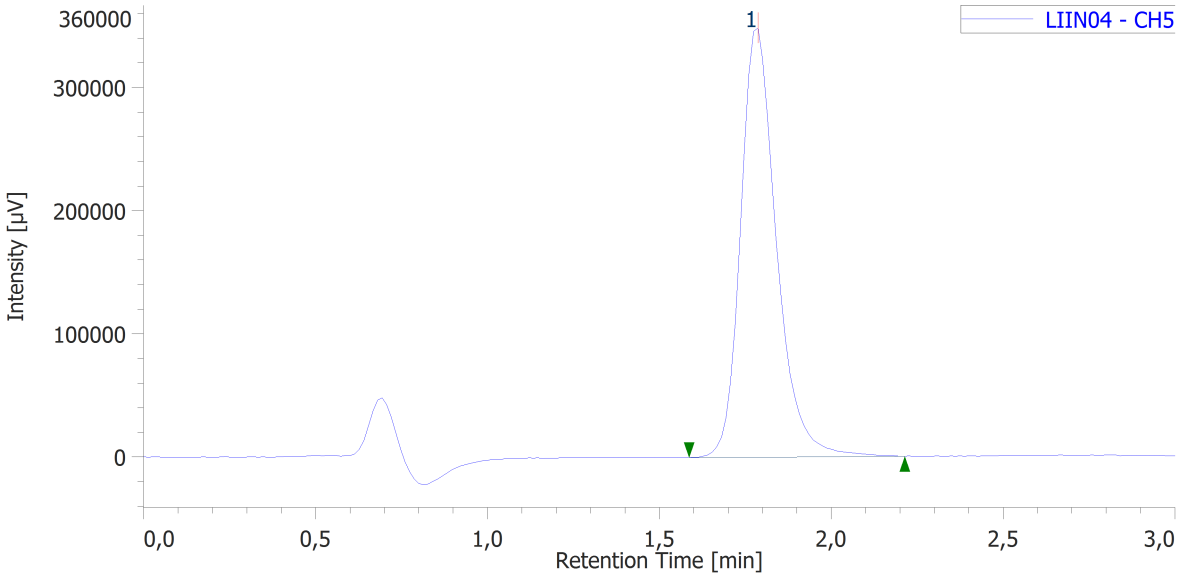

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:53:34
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:28:04
Volume	15,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,787	2527286	348297	100,000	100,000	N/A	1547	N/A	1,212	

Creator QPackSA
Reviewer
Approver

Chromatogram

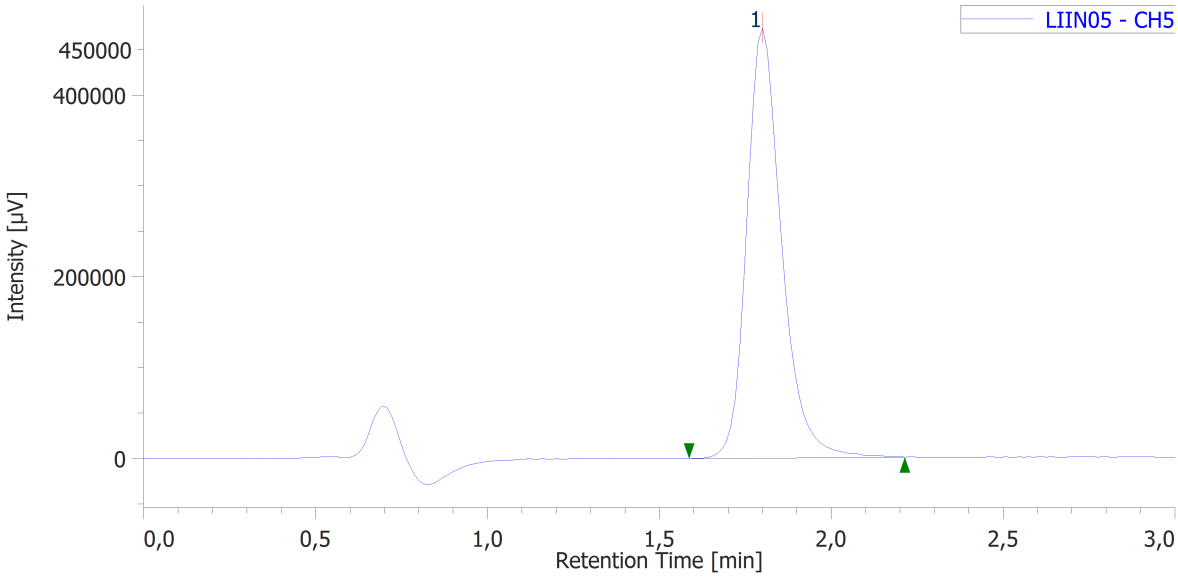

Chromatogram Information	
User Name	QPackSA
Date Modified	21/10/2020 13:53:34
Description	
HPLC System Name	HPL 25
Injection Date	21/10/2020 13:31:56
Volume	20,0 [µL]
Sample #	49
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	OQ_Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	OQ_Peak Method

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,800	3344893	473368	100,000	100,000	N/A	1649	N/A	1,240	

Creator QPackSA
Reviewer
Approver

Chromatogram

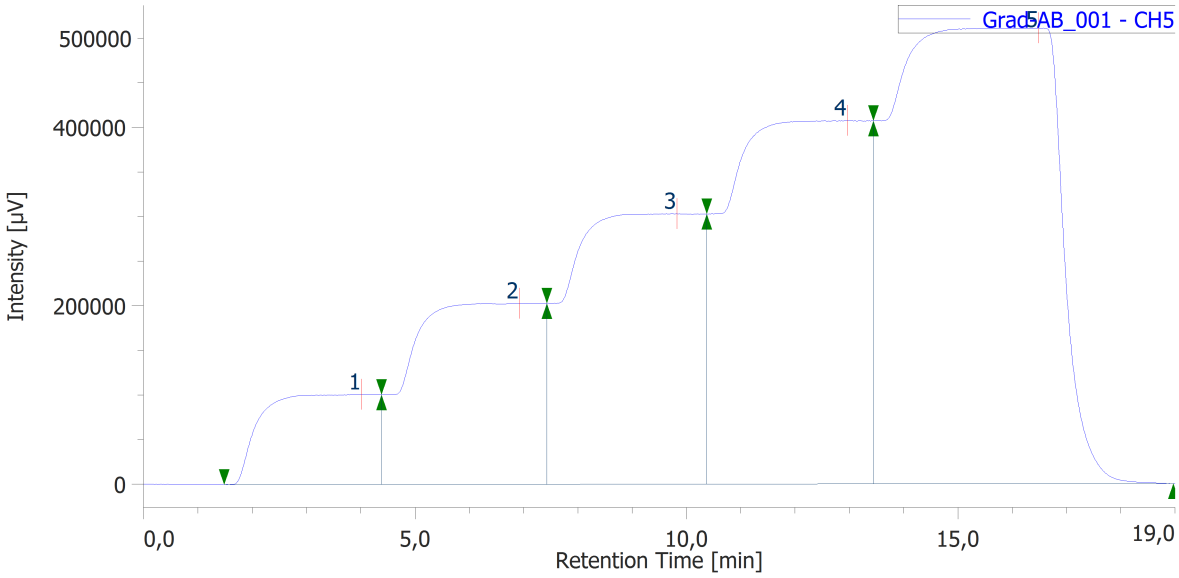

Chromatogram Information	
User Name	QPackSA
Date Modified	22/10/2020 10:42:38
Description	
HPLC System Name	HPL 25
Injection Date	22/10/2020 10:18:27
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	OQ_Grad-AB
Peak ID Table	OQ_Grad Peak ID Table
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad-AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	4,013	14144476	100707	5,164	6,612	N/A	N/A	N/A	N/A	
2	40%	5	6,920	33099288	202624	12,085	13,303	N/A	N/A	N/A	N/A	
3	60%	5	9,820	49942405	302703	18,234	19,874	N/A	N/A	N/A	N/A	
4	80%	5	12,953	70753438	406813	25,833	26,709	N/A	N/A	N/A	N/A	
5	100%	5	16,487	105952541	510278	38,684	33,502	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

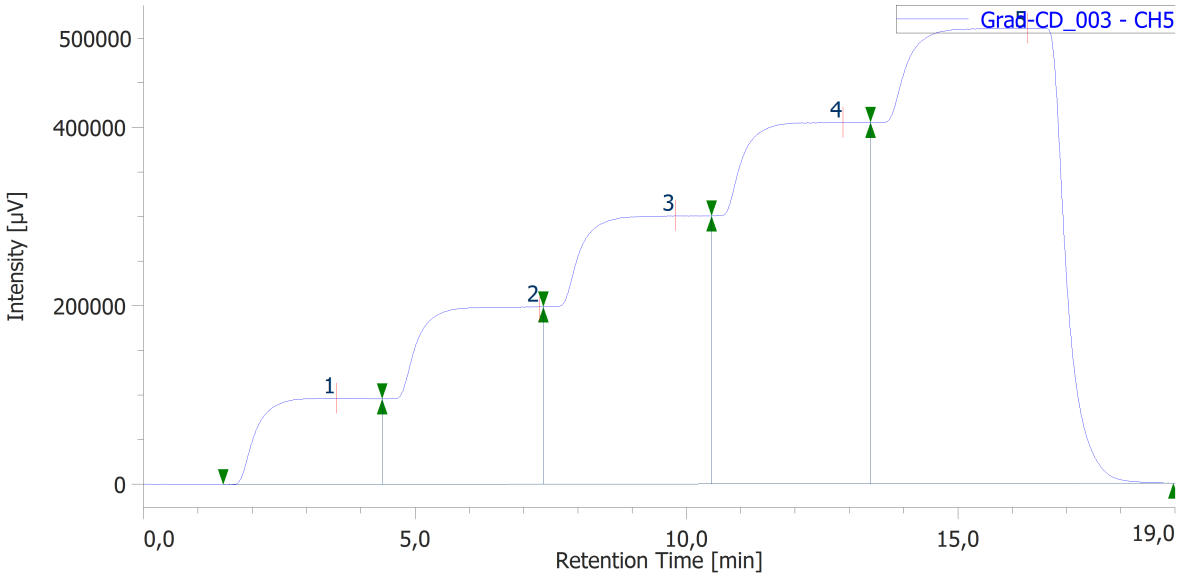

Chromatogram Information	
User Name	QPackSA
Date Modified	22/10/2020 11:19:25
Description	
HPLC System Name	HPL 25
Injection Date	22/10/2020 10:55:56
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	OQ_Grad-CD
Peak ID Table	OQ_Grad Peak ID Table
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad-CD_003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,547	13496173	96531	4,972	6,391	N/A	N/A	N/A	N/A	
2	40%	5	7,293	31372278	198783	11,557	13,160	N/A	N/A	N/A	N/A	
3	60%	5	9,793	51687245	300367	19,041	19,885	N/A	N/A	N/A	N/A	
4	80%	5	12,880	67479586	404708	24,859	26,793	N/A	N/A	N/A	N/A	
5	100%	5	16,280	107412092	510102	39,570	33,771	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver