





tR = [3,1300 min]
Intensity [µAU]
130000
120000
110000
100000
90000
80000
70000
60000
50000
40000
30000
20000
10000
0
200
210
220
230
240
250
260
270
280
290
300
Wavelength [nm]


tR = [3,1300 min]
131500
130000
128000
126000
124000
122000
120000
118000
116000
Intensity [µAU]
200
201
202
203
204
205
206
207
208
209
210
Wavelength [nm]


tR = [3,1300 min]
28000
26000
24000
22000
20000
18000
16000
14000
Intensity [µAU]
232
234
236
238
240
242
244
246
248
250
252
Wavelength [nm]


tR = [3,1300 min]
53800
53000
52000
51000
50000
49000
48000
47000
46000
45000
44000
Intensity [µAU]
266
268
270
272
274
276
278
Wavelength [nm]

Chromatogram

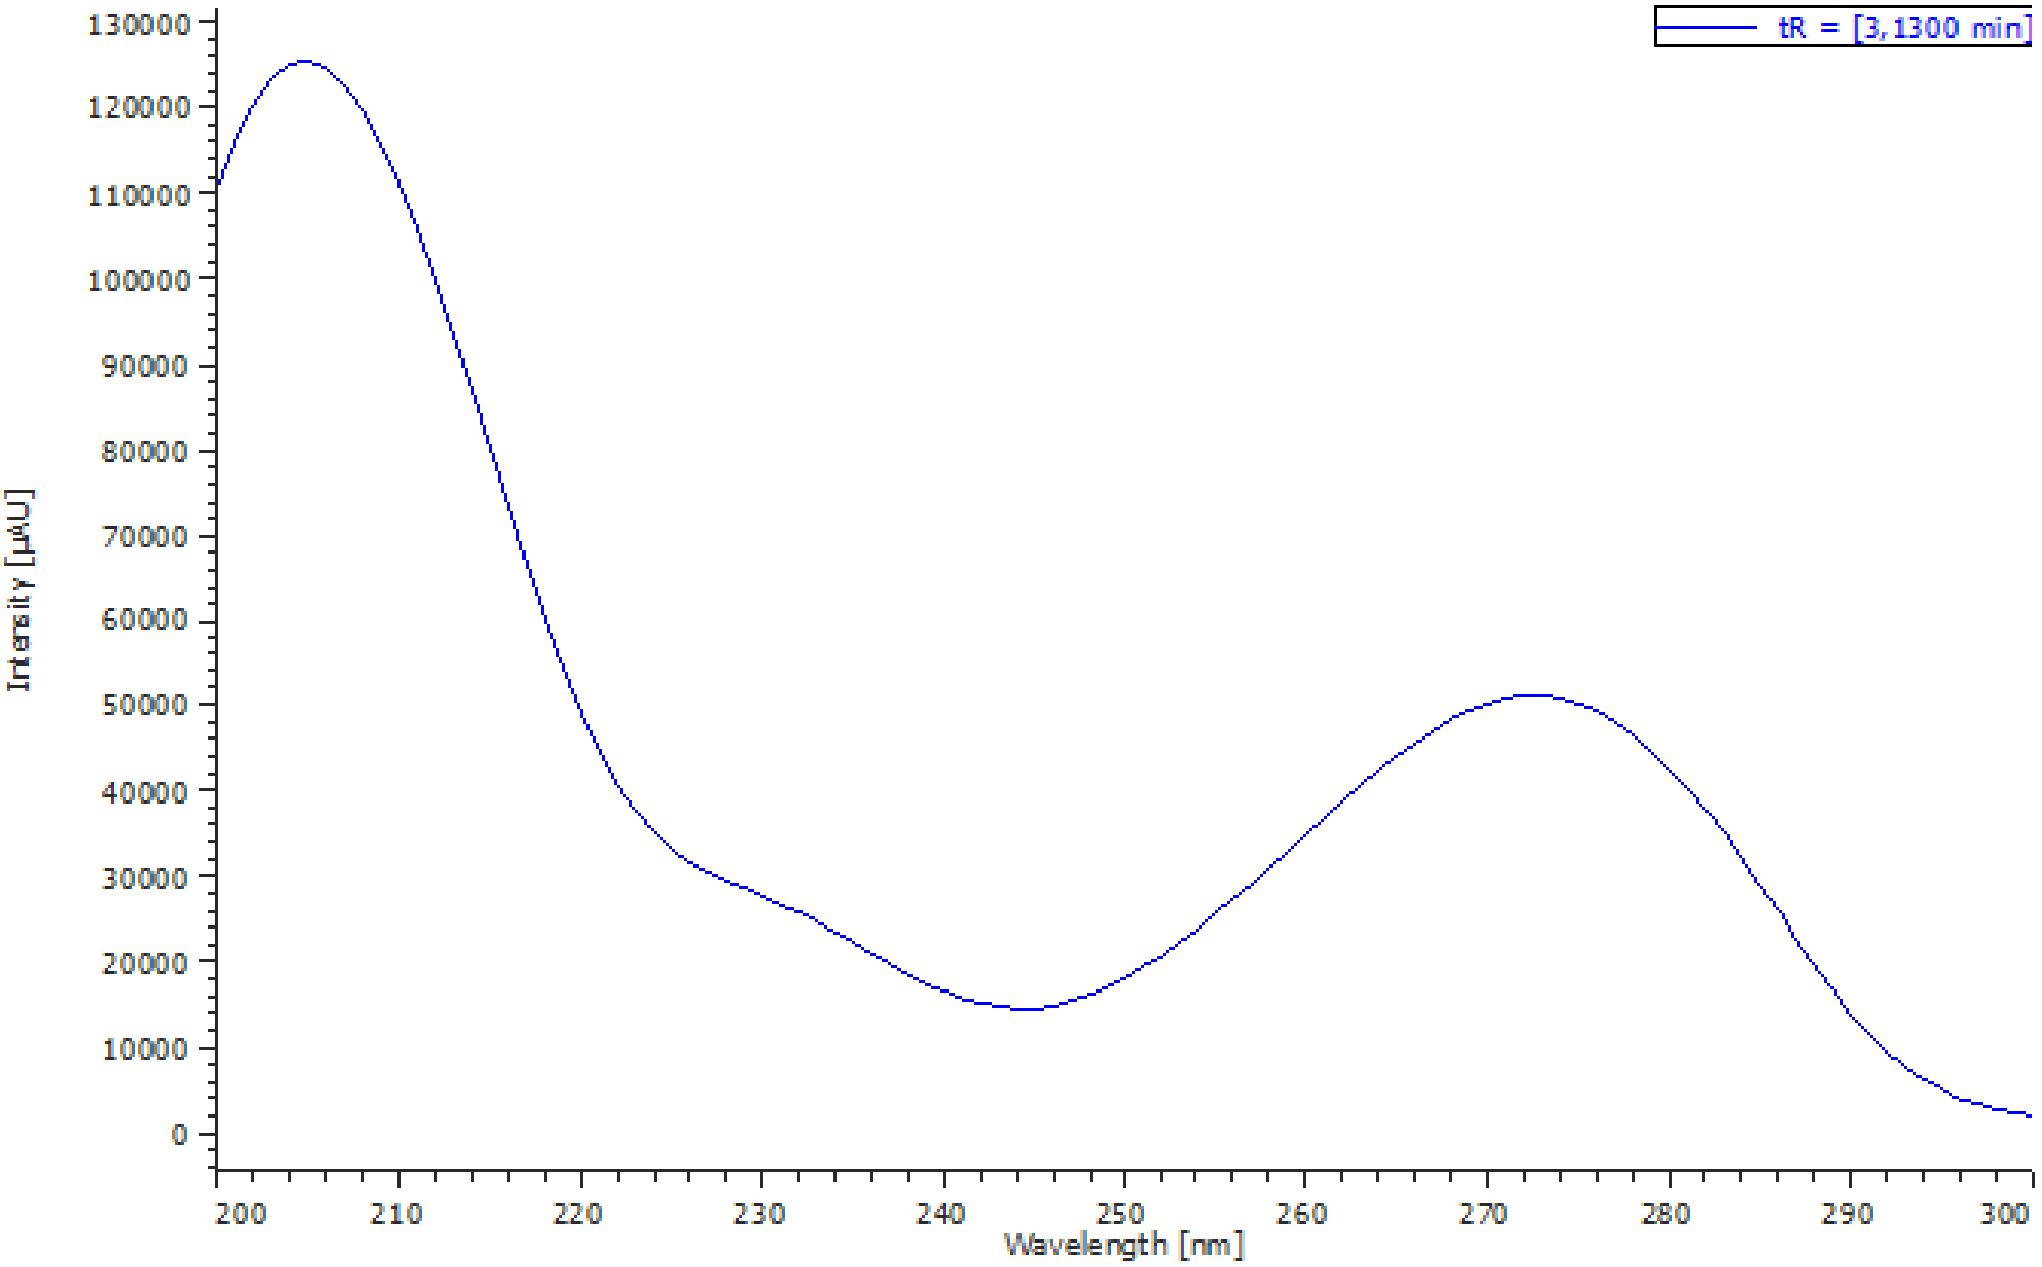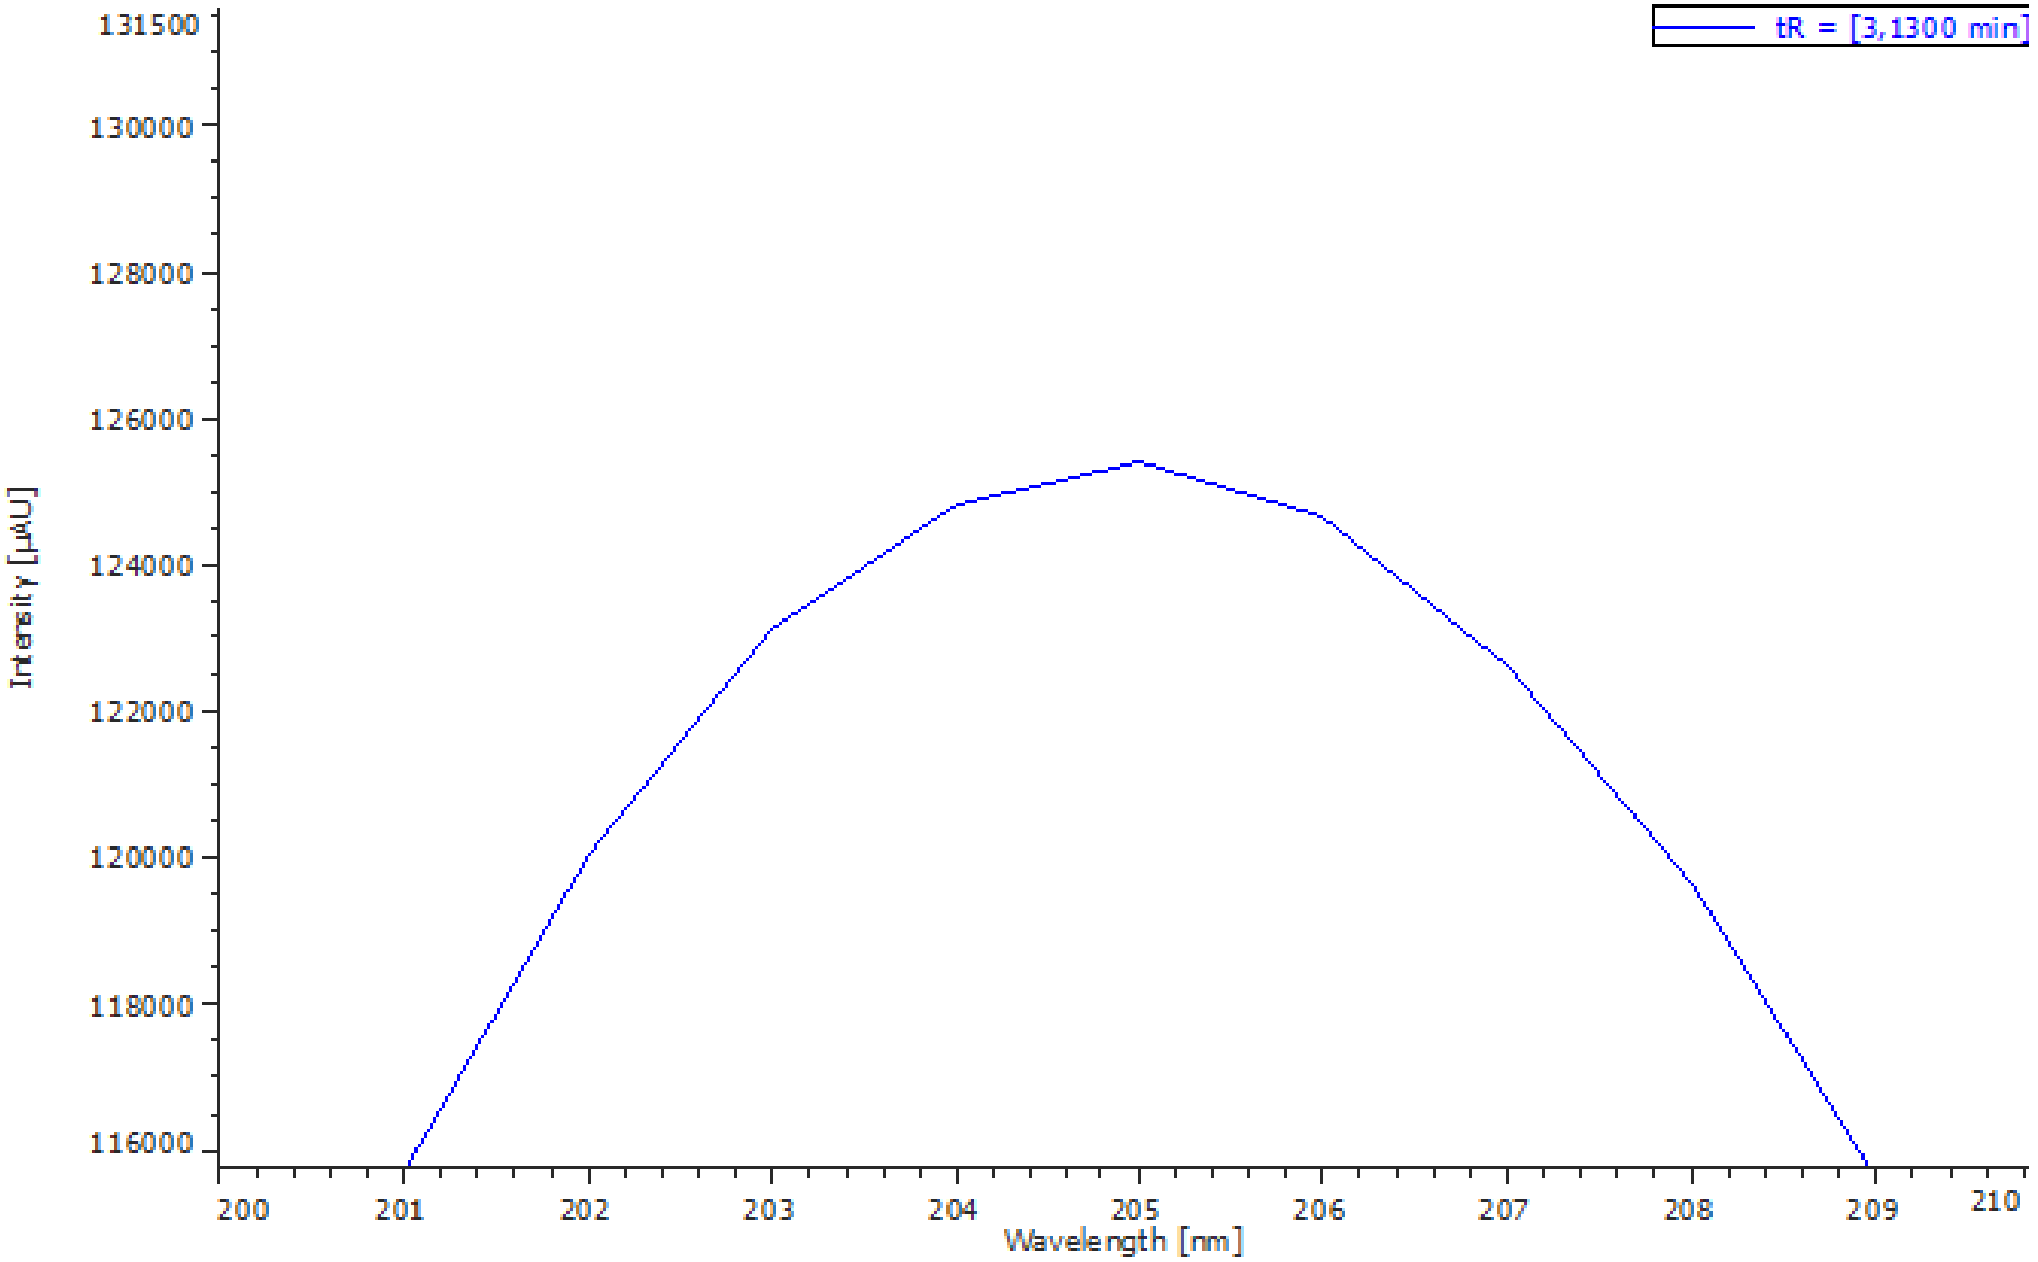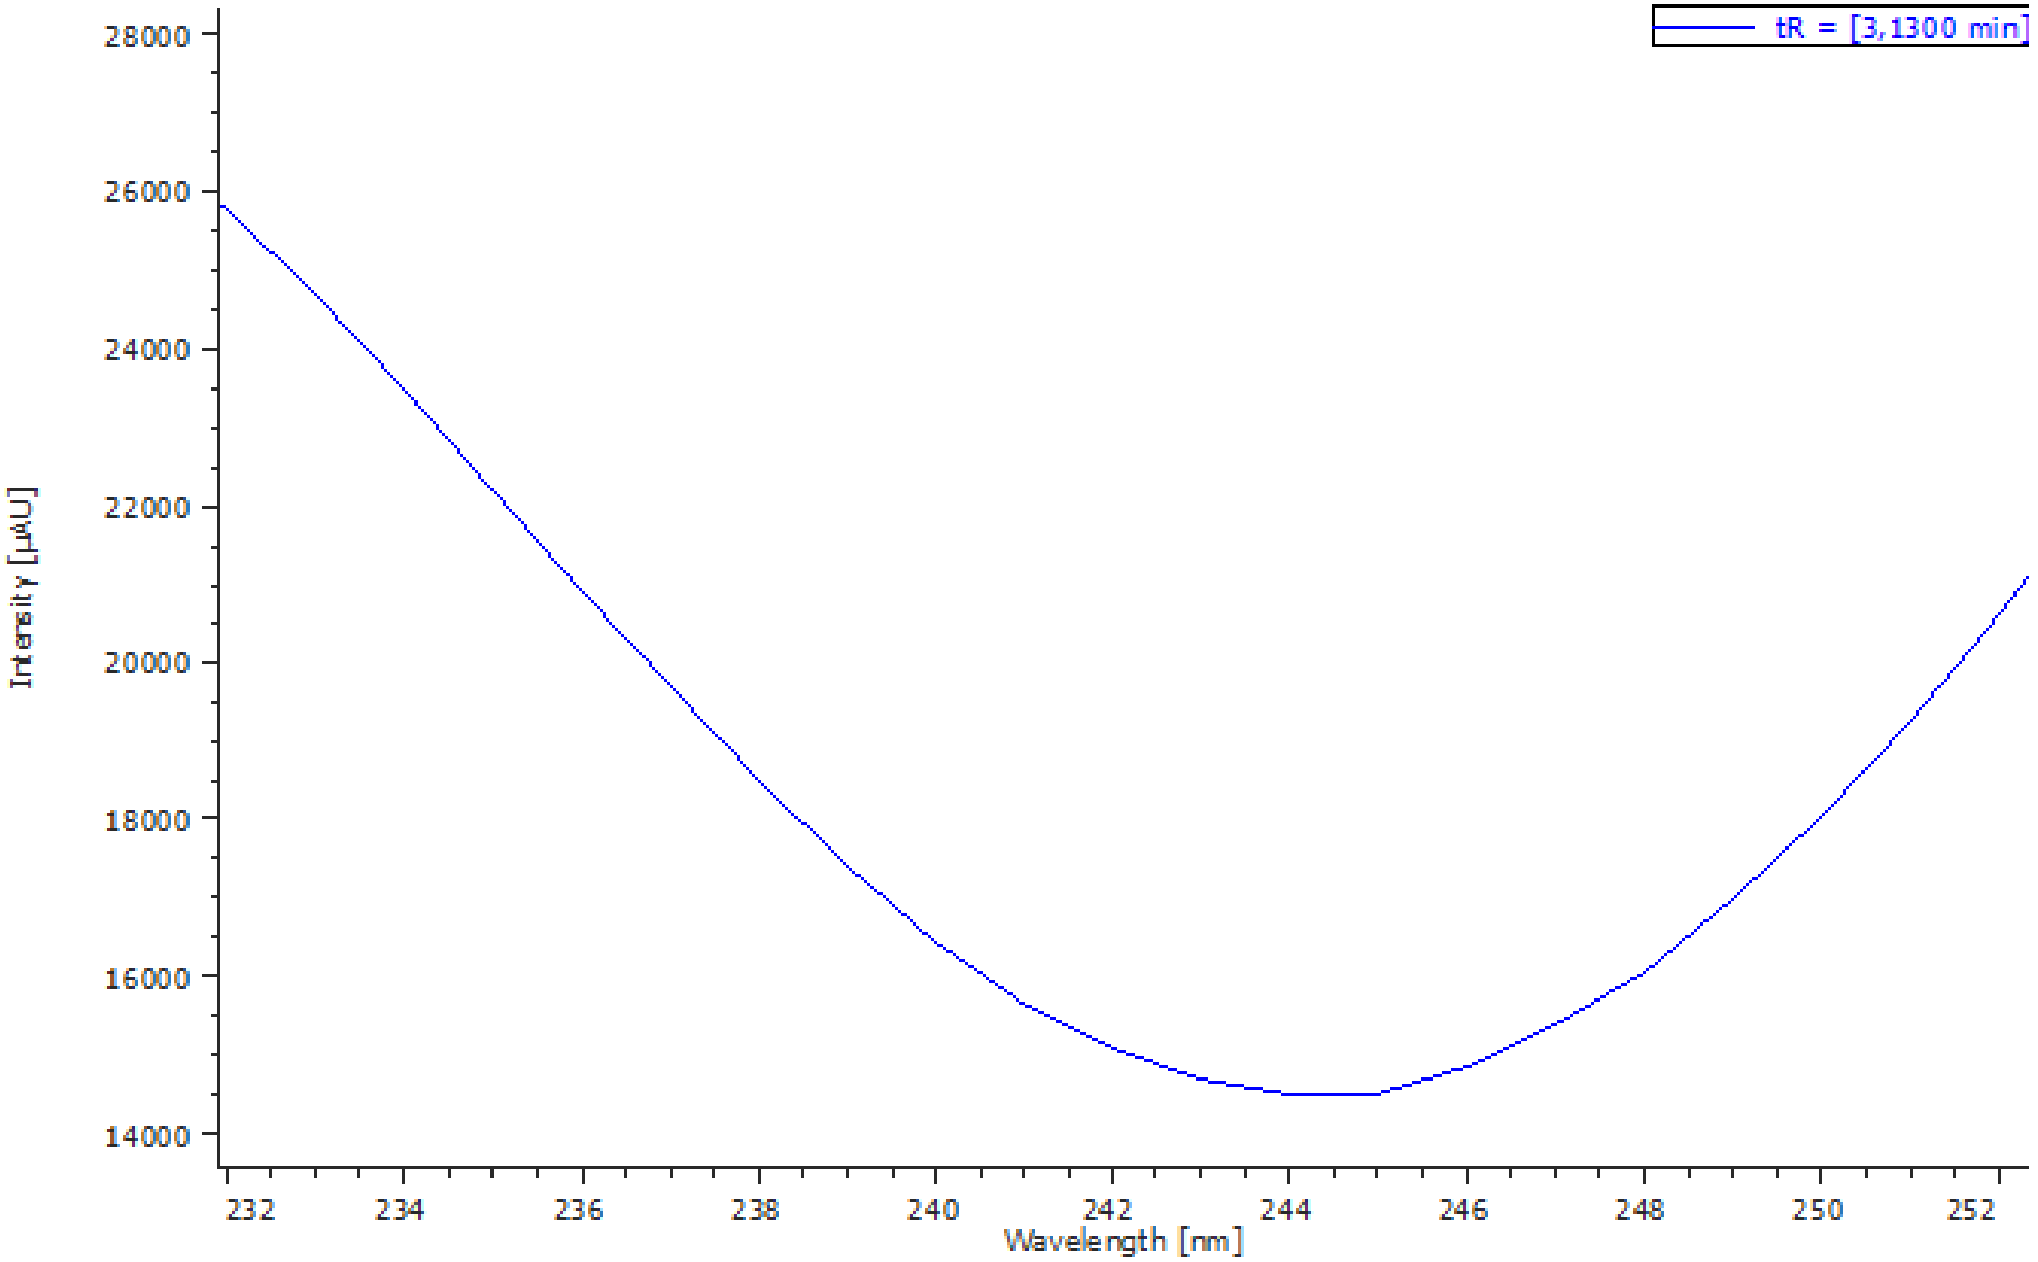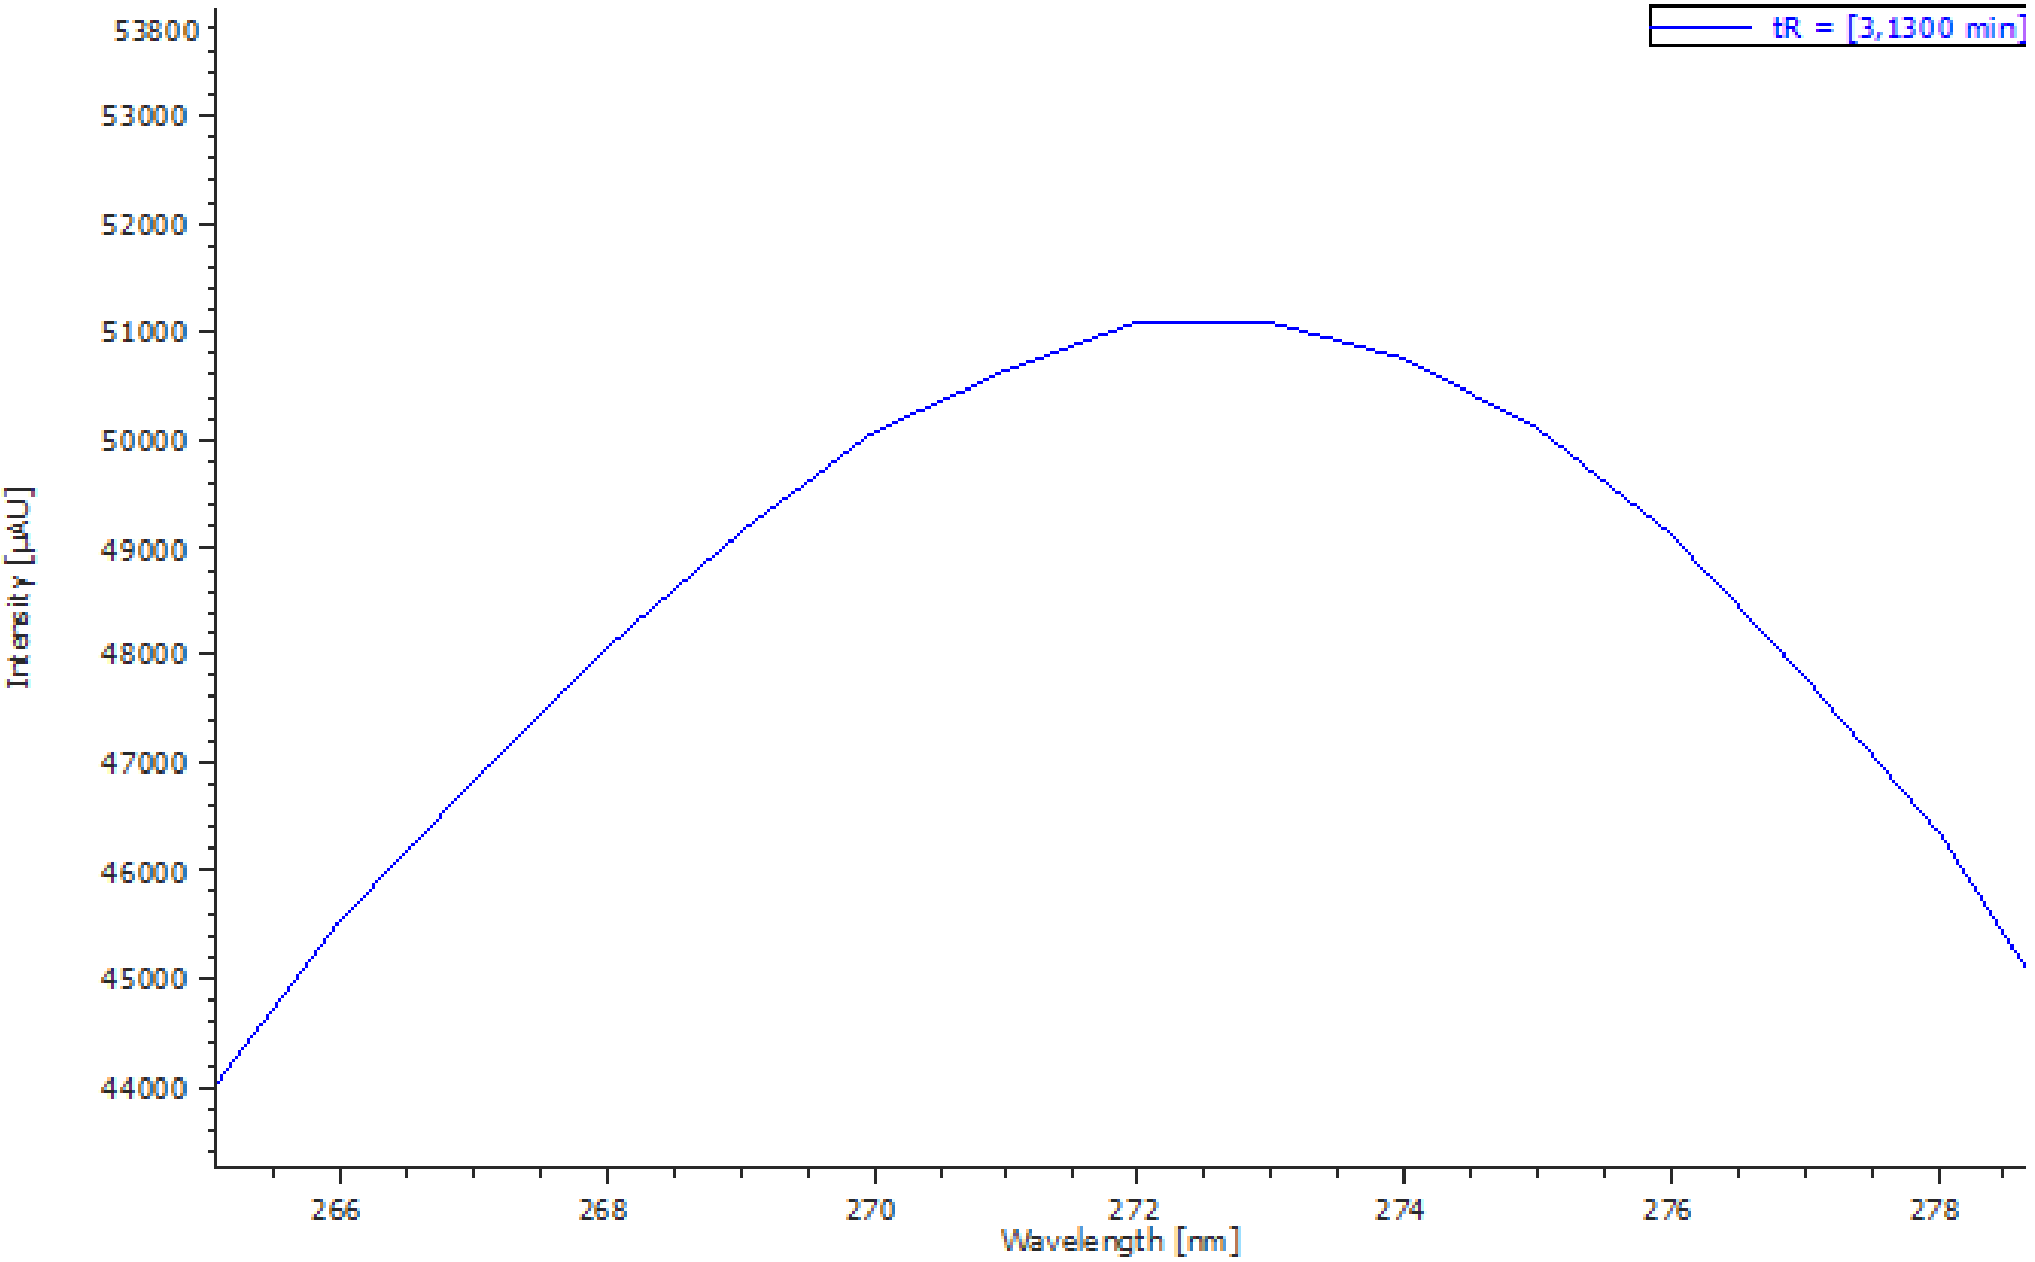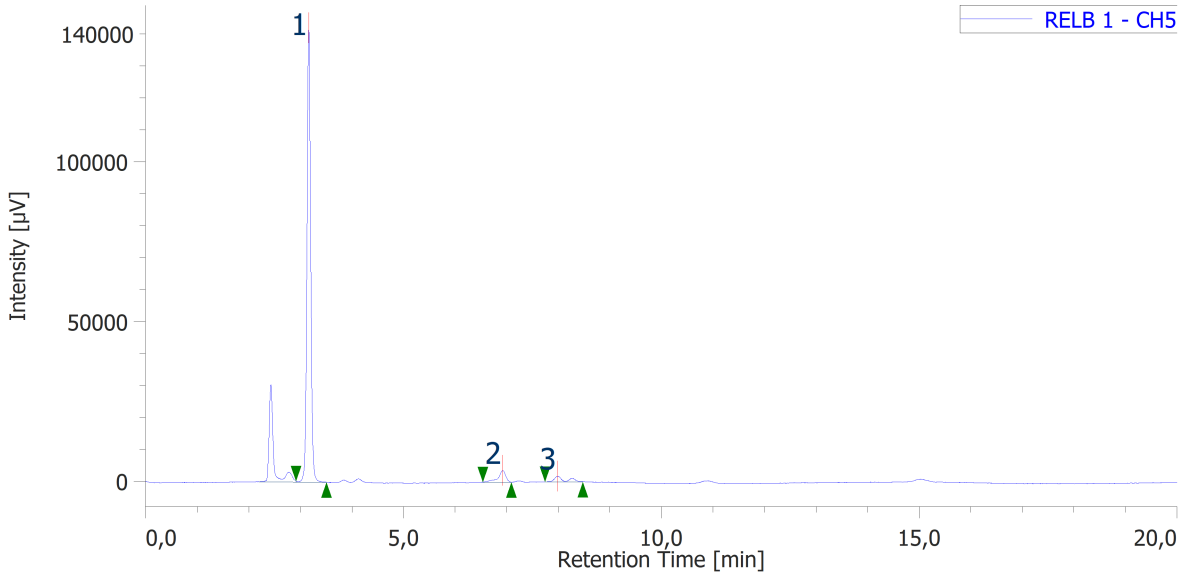


Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:59:00
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:39:00
Volume	20,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	LIIN
Control Method	Sinal - Ruído
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	RELB 1-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,160	708297	142058	91,841	96,284	N/A	9910	22,007	1,080	
2	Unknown	5	6,923	37093	3676	4,810	2,492	N/A	16445	2,448	0,692	
3	Unknown	5	7,983	25833	1806	3,350	1,224	N/A	2395	N/A	1,892	

Creator QPackSA
Reviewer
Approver

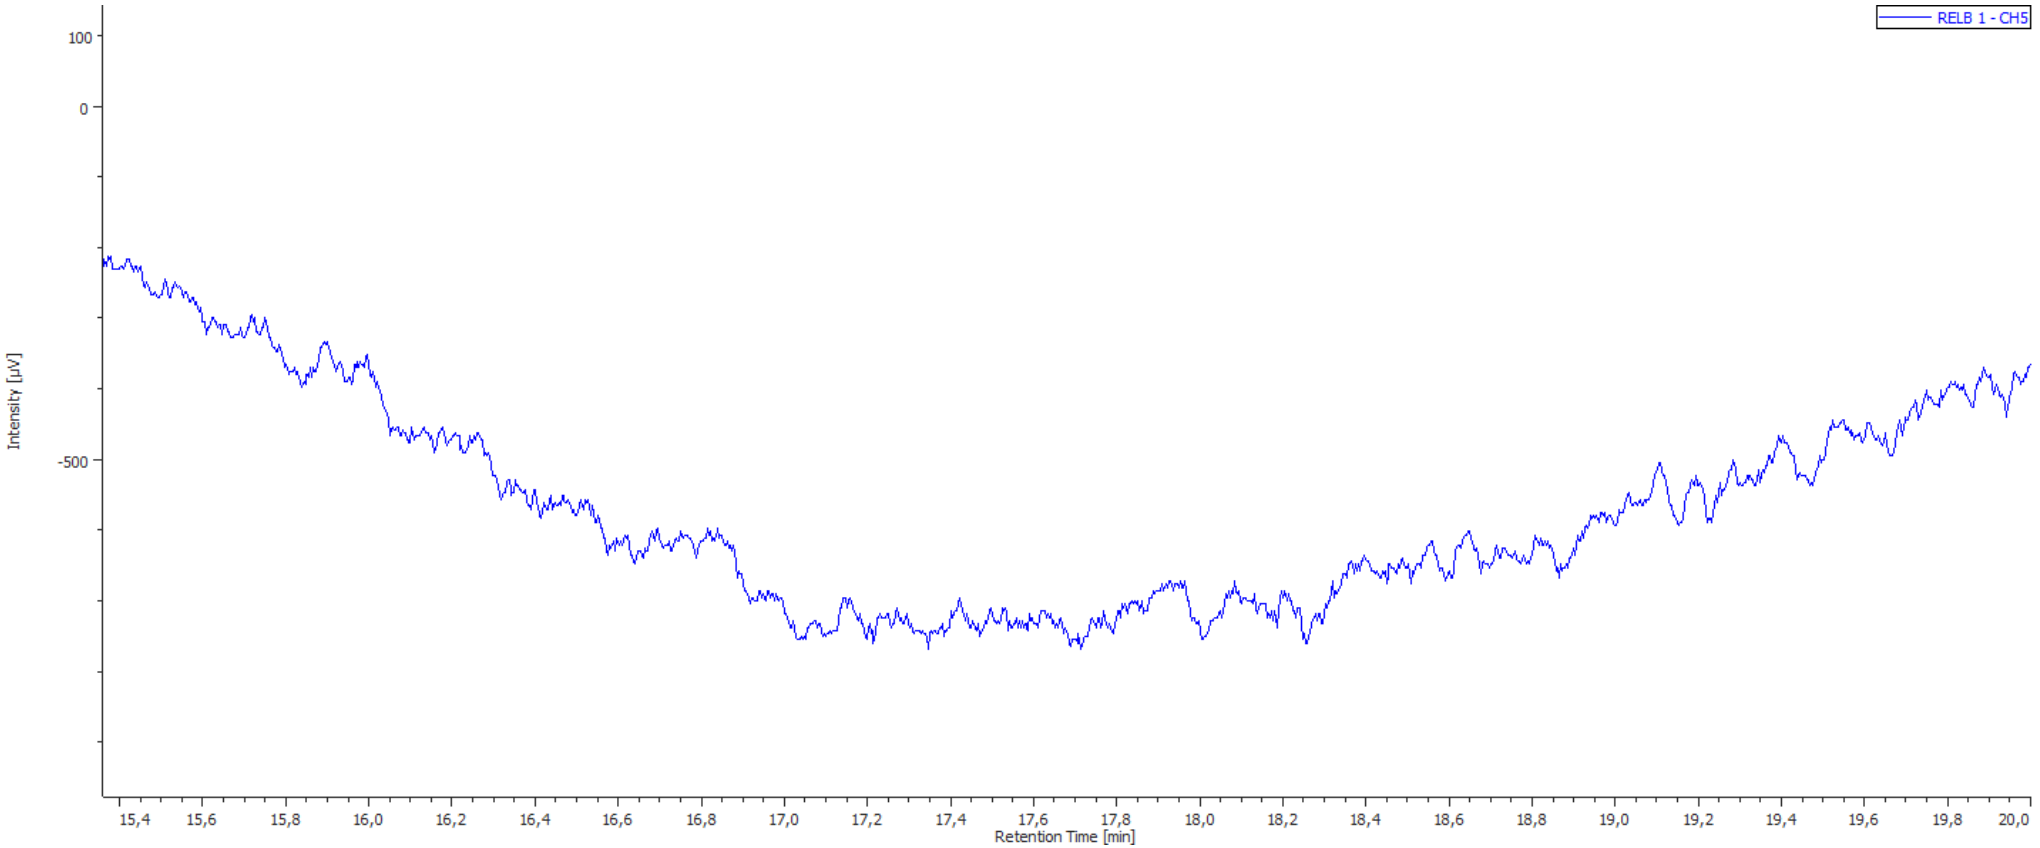
RELB 1 - CH5
100
0
-500
Intensity [µV]
15,4
15,6
15,8
16,0
16,2
16,4
16,6
16,8
17,0
17,2
17,4
17,6
17,8
18,0
18,2
18,4
18,6
18,8
19,0
19,2
19,4
19,6
19,8
20,0
Retention Time [min]

PCIN Branco 1 29/05/2023 15:59:37


Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 15:46:11
HPLC System Name	01-HP-03
Injection Date	29/05/2023 15:41:57
Volume	10,0 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Sequence	PCIN
Control Method	Qualificação

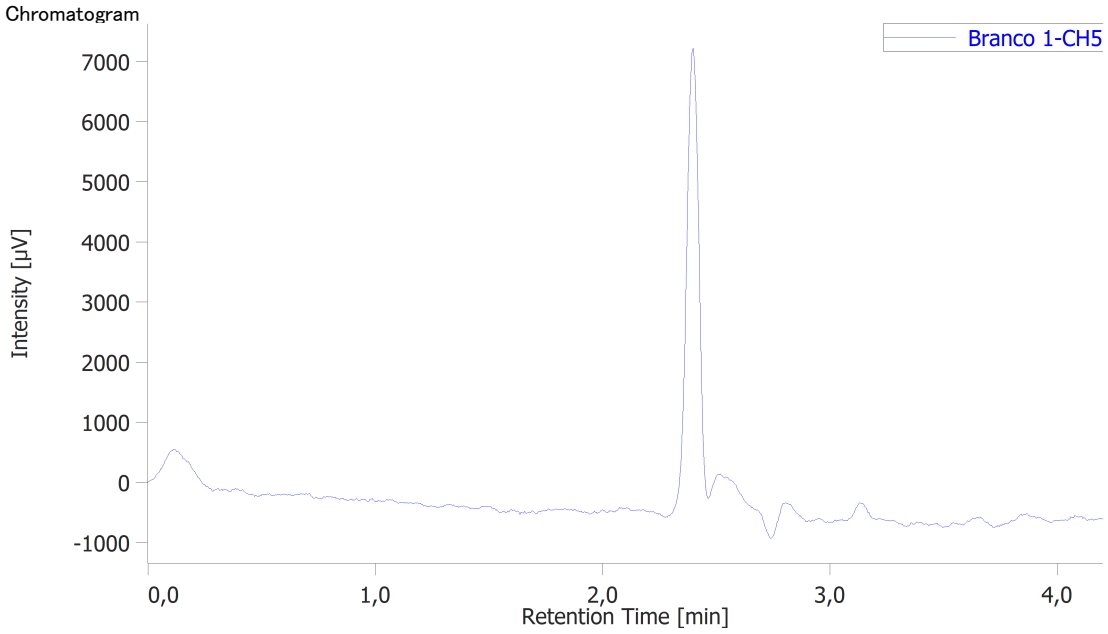

Peak Information – No data.

Creator
Reviewer
Approver

Chromatogram

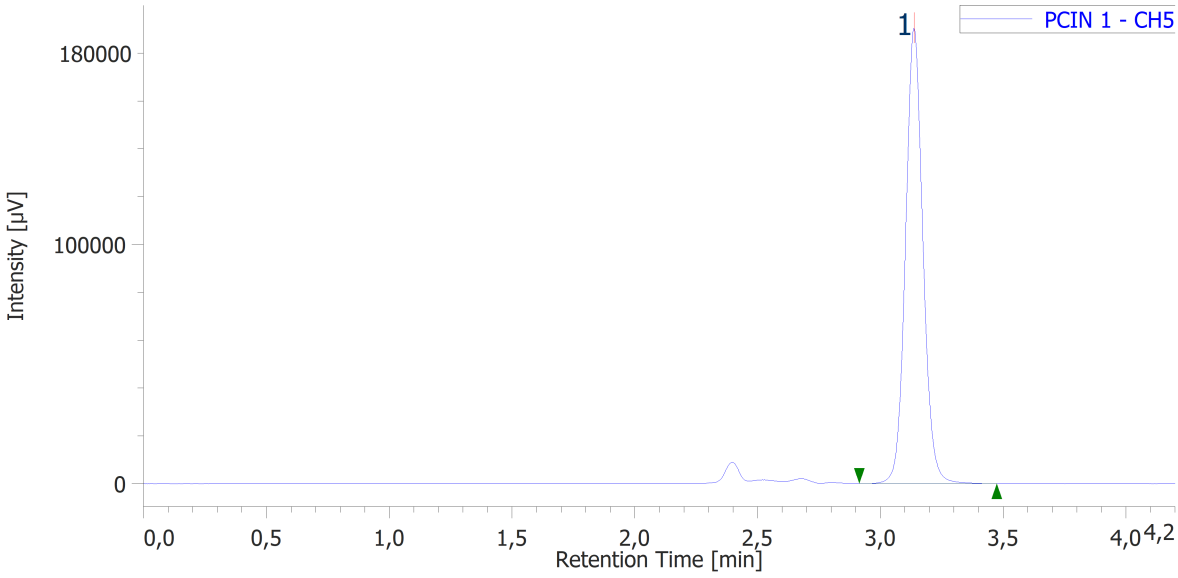

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 15:50:35
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 15:46:21
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,137	940024	190414	100,000	100,000	N/A	9854	N/A	1,073	

Creator
Reviewer
Approver

Chromatogram

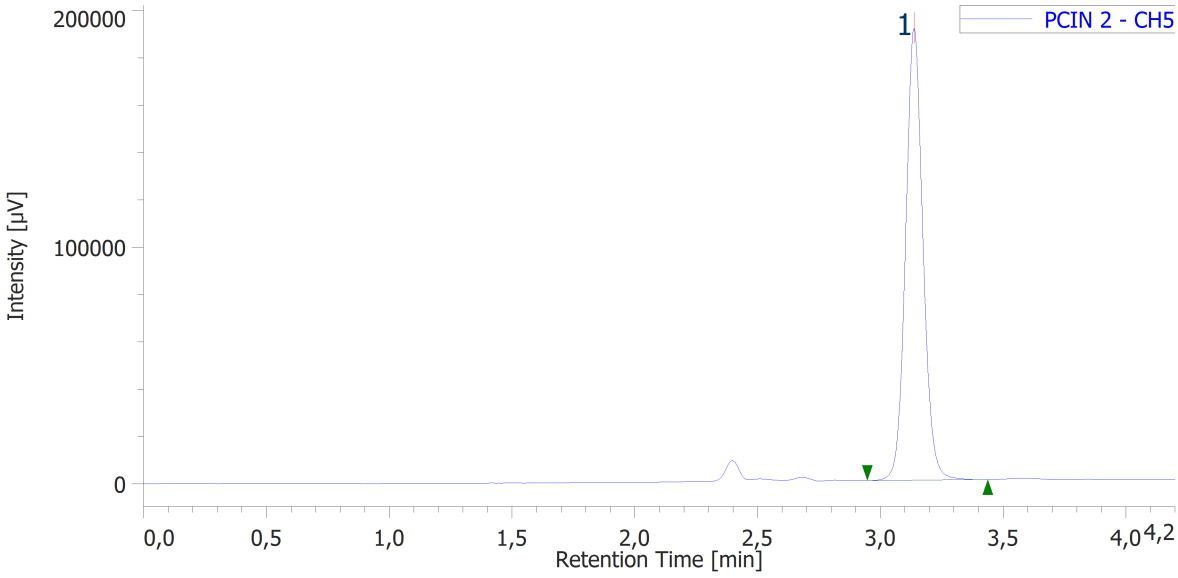

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 15:54:59
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 15:50:45
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,137	940011	191029	100,000	100,000	N/A	9883	N/A	1,078	

Creator
Reviewer
Approver

Chromatogram

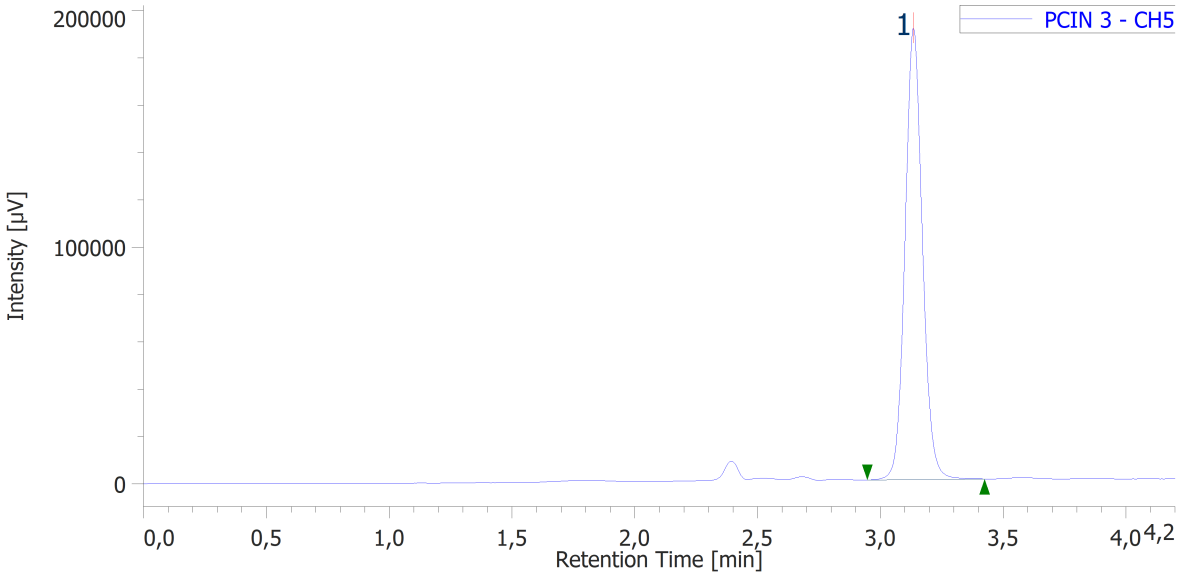

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 15:59:23
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 15:55:09
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,133	939200	190777	100,000	100,000	N/A	9844	N/A	1,095	

Creator QPackSA
Reviewer
Approver

Chromatogram

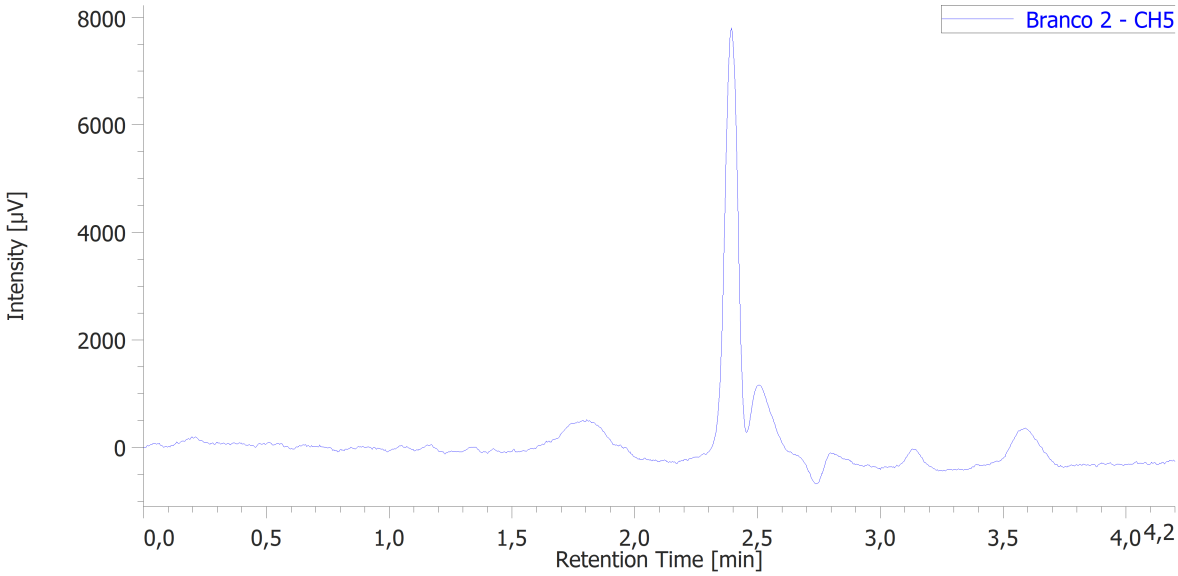


Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:03:47
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 15:59:33
Volume	10,0 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

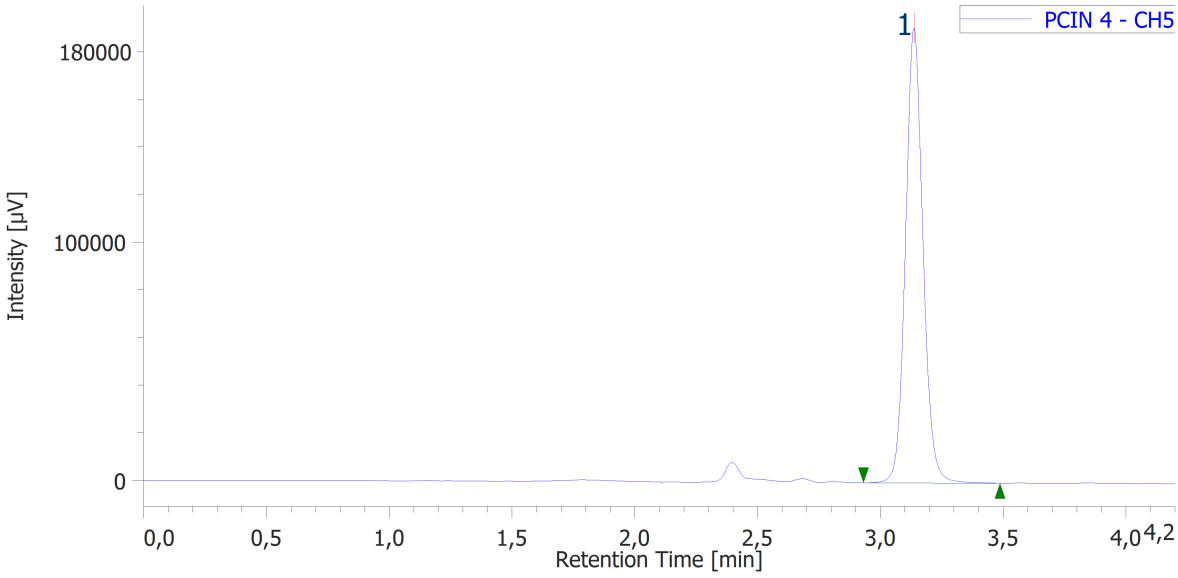

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:08:11
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:03:57
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,137	943496	190760	100,000	100,000	N/A	9821	N/A	1,081	

Creator QPackSA
Reviewer
Approver

Chromatogram

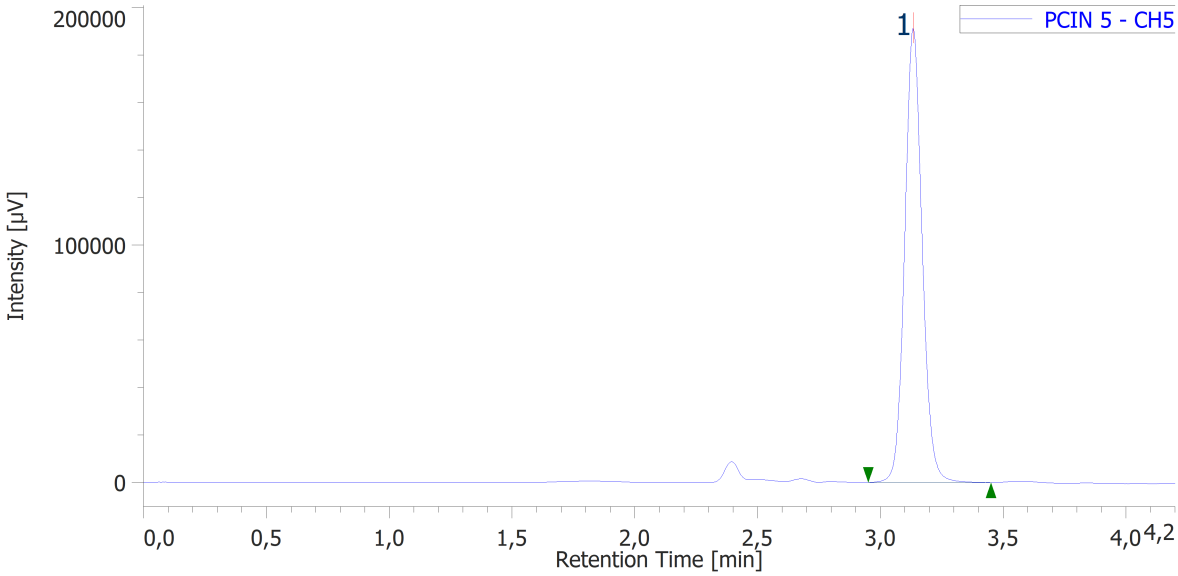

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:12:35
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:08:21
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,133	943185	191280	100,000	100,000	N/A	9813	N/A	1,082	

Creator QPackSA
Reviewer
Approver

Chromatogram

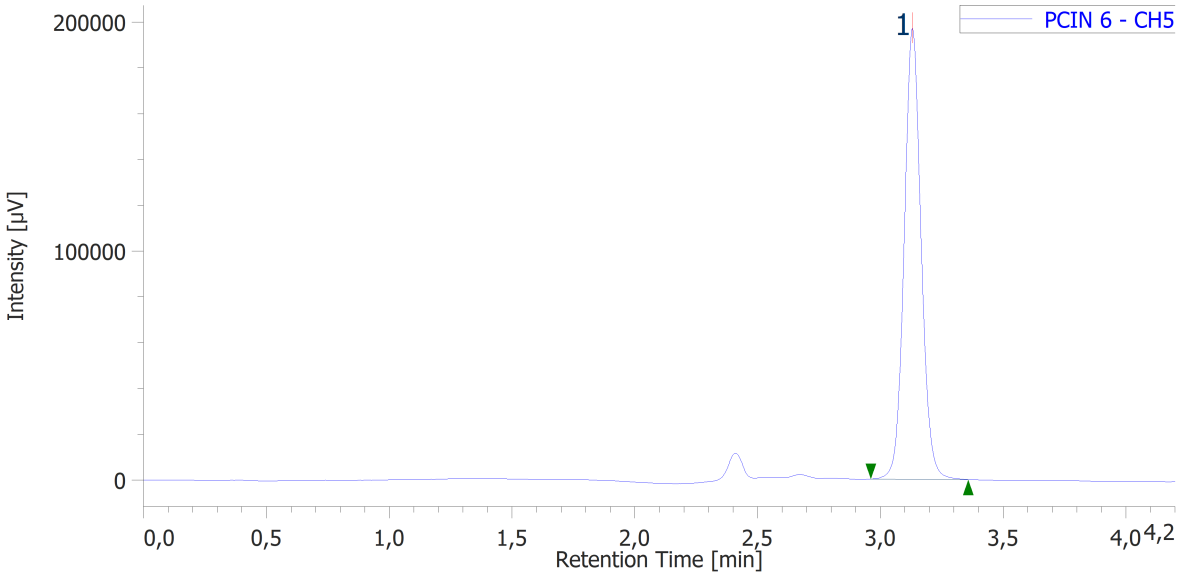

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:40:37
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:36:24
Volume	10,0 [µL]
Sample #	42
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Identificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,130	942532	197063	100,000	100,000	N/A	10400	N/A	1,068	

Creator
Reviewer
Approver

Chromatogram

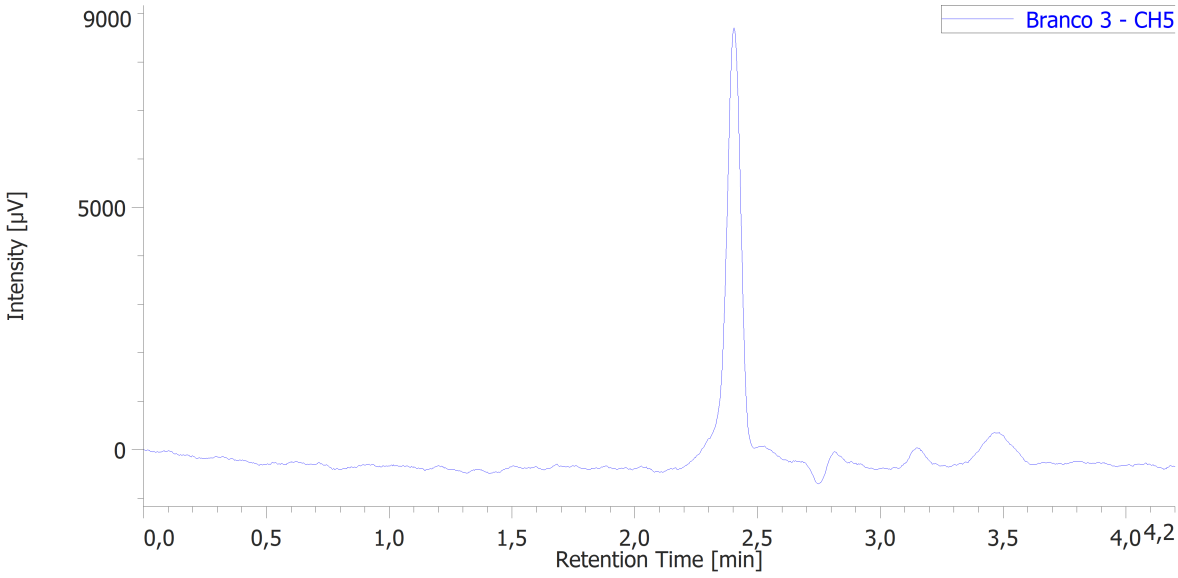


Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:45:01
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:40:48
Volume	10,0 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	4,2 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

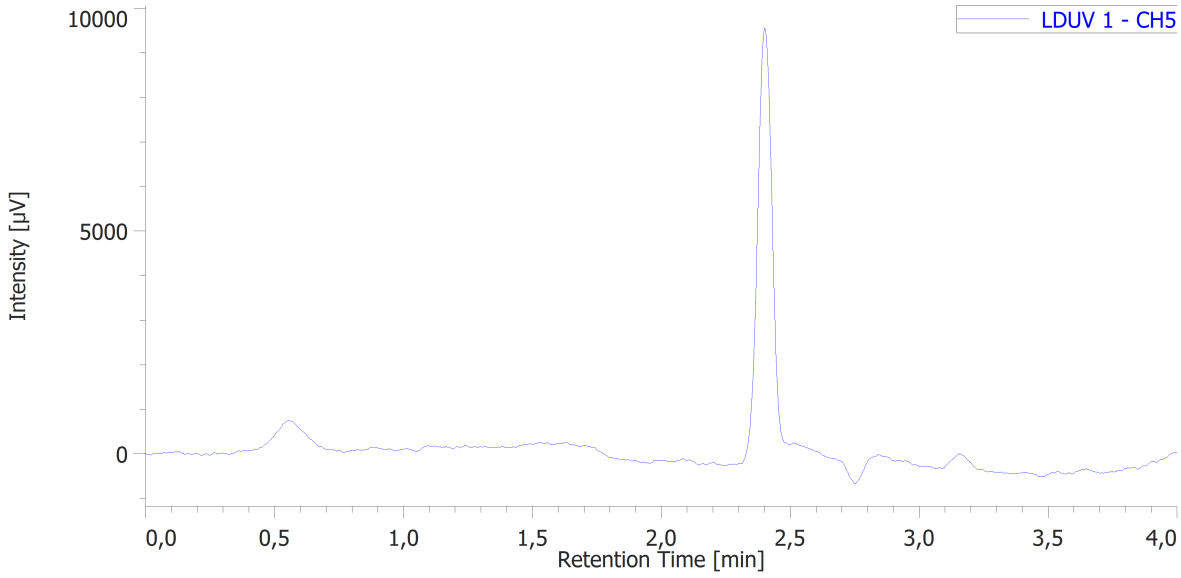


Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:53:45
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:49:44
Volume	10,0 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

Creator QPackSA
Reviewer
Approver

Chromatogram

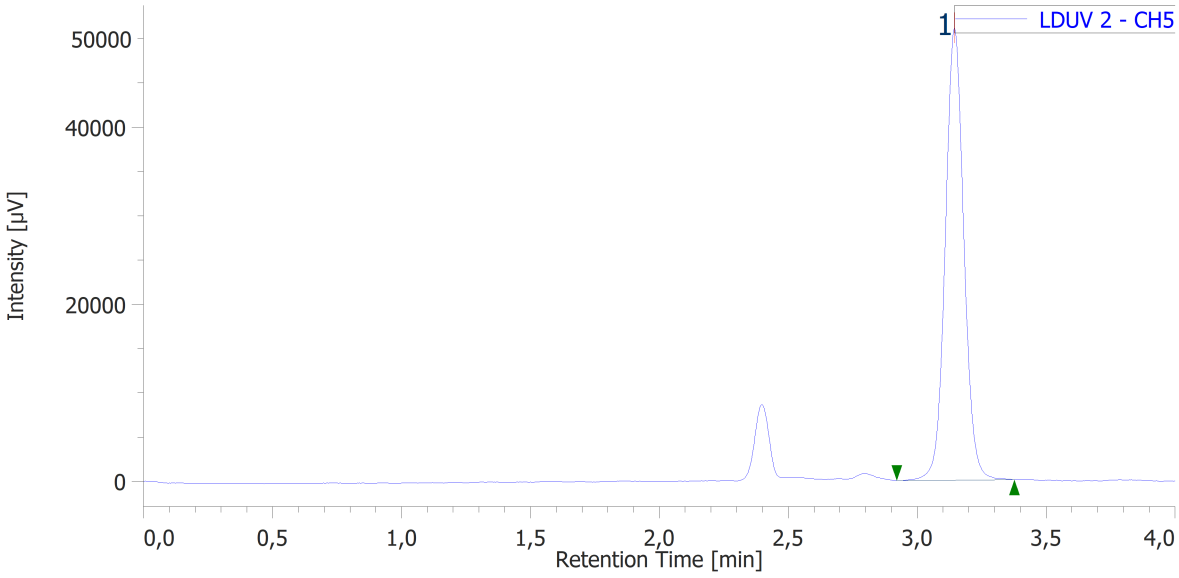

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 16:57:57
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:53:56
Volume	10,0 [µL]
Sample #	44
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,143	256814	51056	100,000	100,000	N/A	9469	N/A	1,057	

Creator QPackSA
Reviewer
Approver

Chromatogram

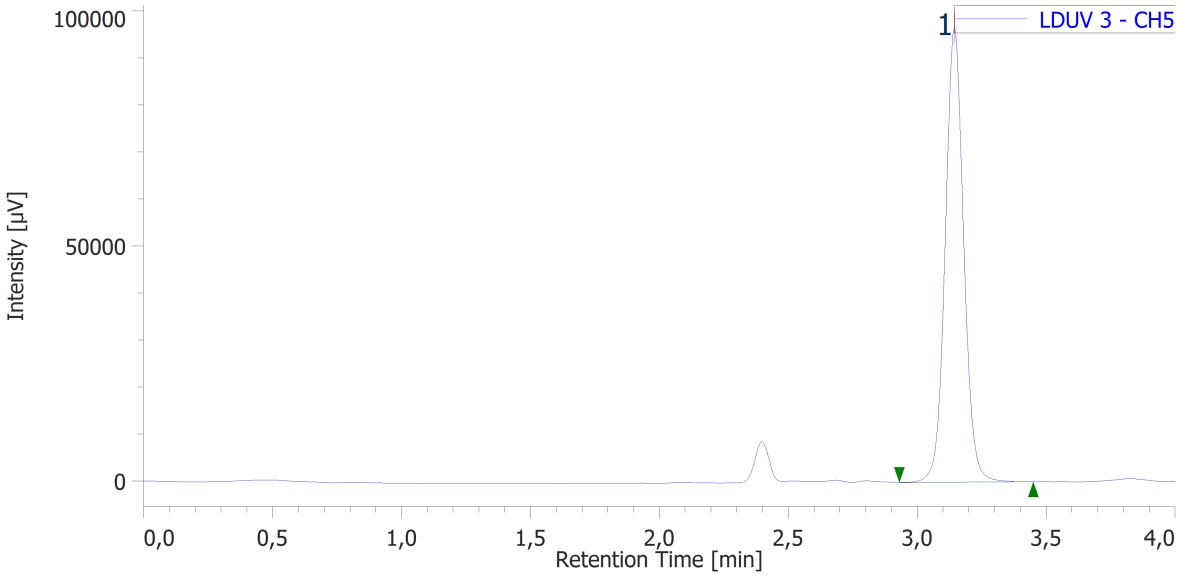

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:02:09
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 16:58:08
Volume	10,0 [µL]
Sample #	45
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,143	482172	96541	100,000	100,000	N/A	9644	N/A	1,054	

Creator QPackSA
Reviewer
Approver

Chromatogram

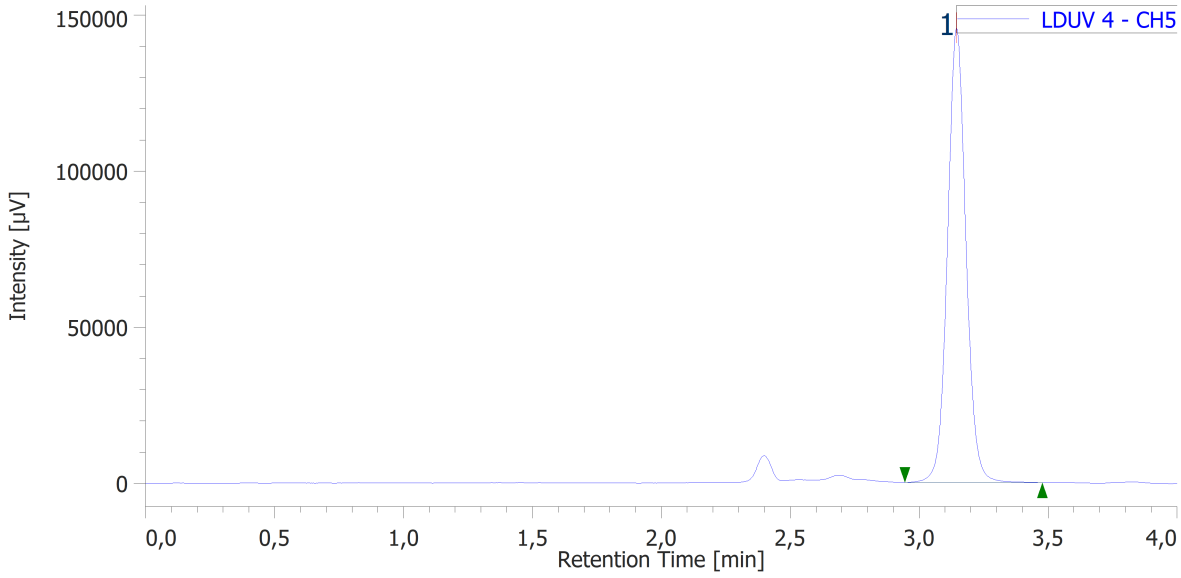

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:06:20
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:02:20
Volume	10,0 [µL]
Sample #	46
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,143	725495	145554	100,000	100,000	N/A	9749	N/A	1,071	

Creator QPackSA
Reviewer
Approver

Chromatogram

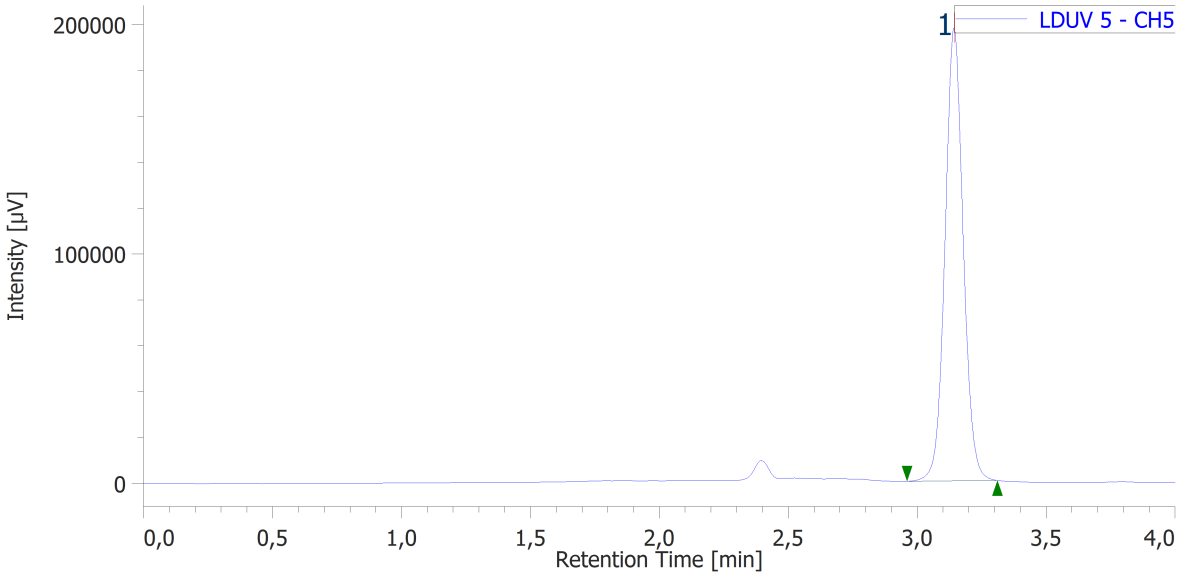

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:10:33
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:06:32
Volume	10,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Identificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,143	967537	197185	100,000	100,000	N/A	9933	N/A	1,035	

Creator
Reviewer
Approver

Chromatogram

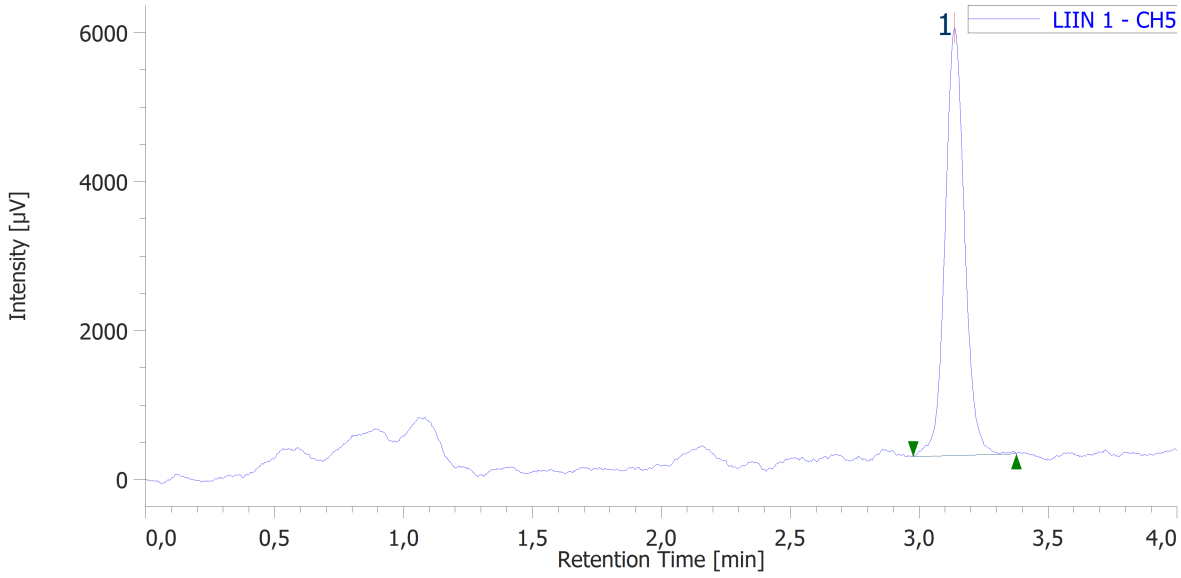

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:22:02
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:18:00
Volume	0,1 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,137	30197	5737	100,000	100,000	N/A	8784	N/A	1,073	

Creator QPackSA
Reviewer
Approver

Chromatogram

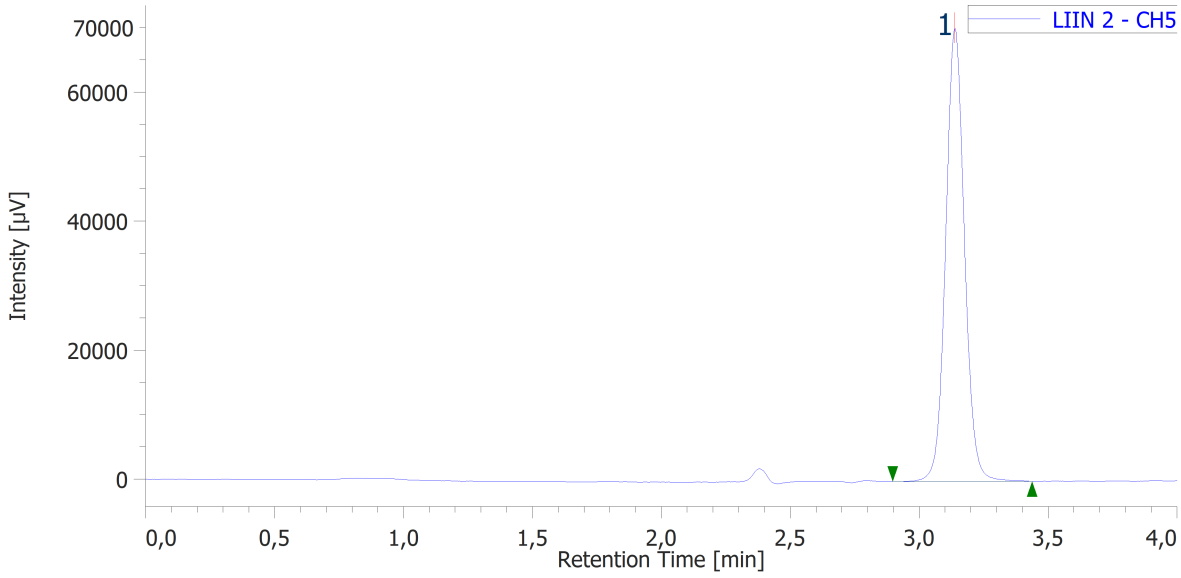

Chromatogram Information

User Name	QPackSA
Date Modified	29/05/2023 17:26:12
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:22:12
Volume	5,0 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,137	356571	70296	100,000	100,000	N/A	9298	N/A	1,075	

Creator QPackSA
Reviewer
Approver

Chromatogram

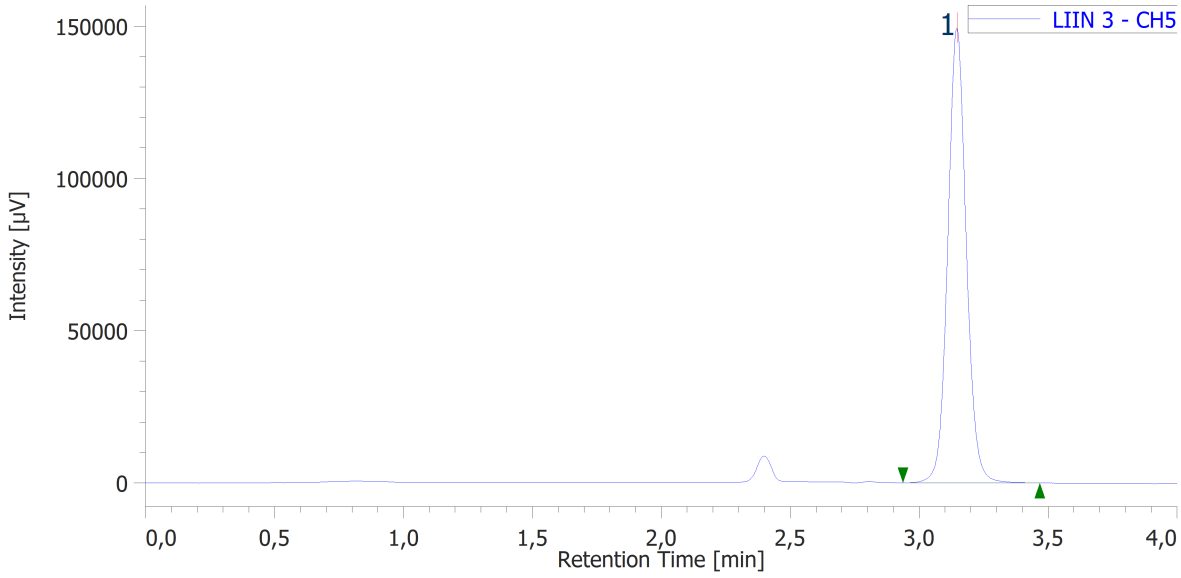

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:30:26
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:26:24
Volume	10,0 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,147	745992	149341	100,000	100,000	N/A	9713	N/A	1,048	

Creator QPackSA
Reviewer
Approver

Chromatogram

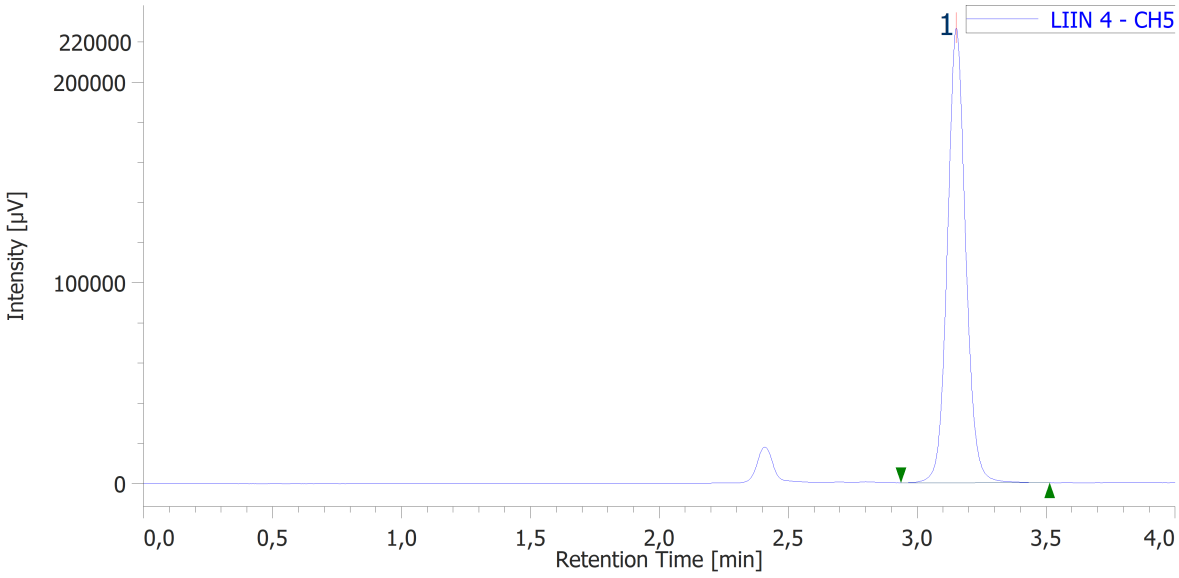

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:34:38
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:30:36
Volume	15,0 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,150	1115700	226570	100,000	100,000	N/A	10112	N/A	1,085	

Creator QPackSA
Reviewer
Approver

Chromatogram

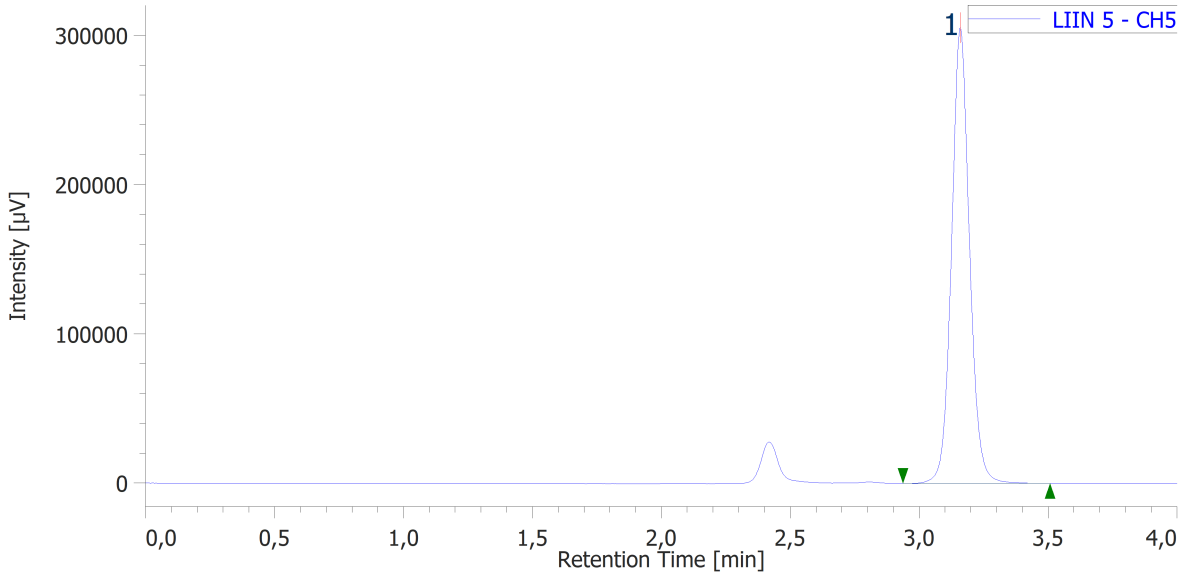

Chromatogram Information	
User Name	QPackSA
Date Modified	29/05/2023 17:38:49
Description	
HPLC System Name	01-HP-03
Injection Date	29/05/2023 17:34:48
Volume	20,0 [µL]
Sample #	48
Project Name	Qualificação
Acquisition Time	4,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	3,160	1482375	304974	100,000	100,000	N/A	10534	N/A	1,055	

Creator QPackSA
Reviewer
Approver

Chromatogram

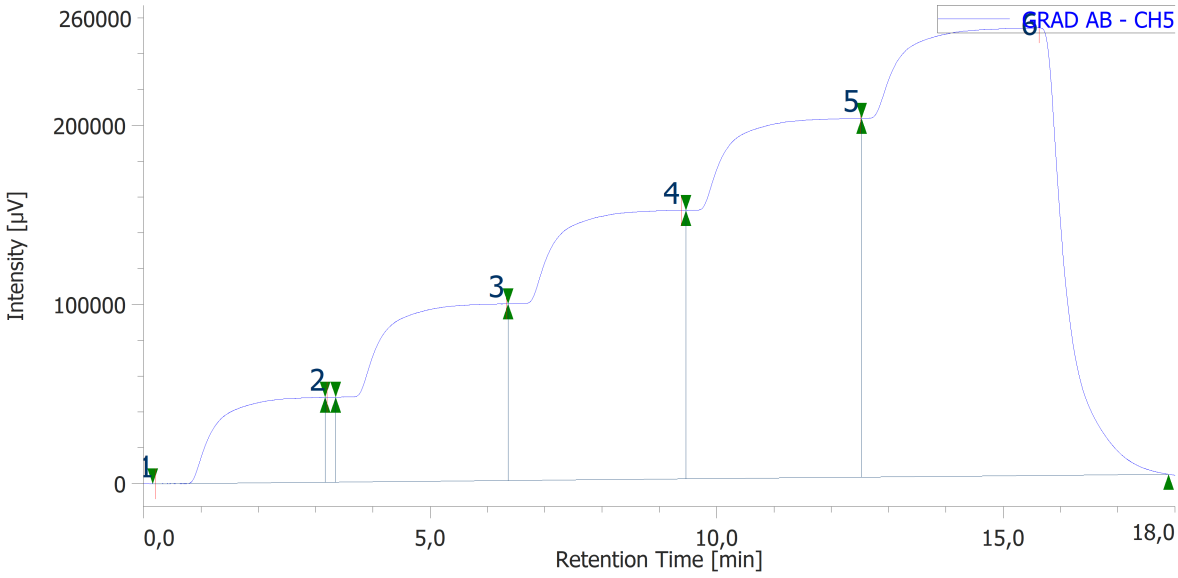

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 11:17:50
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 10:59:49
Volume	0,1 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	GRAD
Control Method	Grad_AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	0,200	-1638	39	N/A	0,005	N/A	1	N/A	8,935	
2	20%	5	3,200	520602	47328	0,405	6,348	N/A	N/A	N/A	N/A	
3	40%	5	6,323	15309891	98566	11,922	13,221	N/A	N/A	N/A	N/A	
4	60%	5	9,380	25423766	149802	19,797	20,094	N/A	N/A	N/A	N/A	
5	80%	5	12,507	34682766	200109	27,007	26,841	N/A	N/A	N/A	N/A	
6	100%	5	15,623	52485730	249679	40,870	33,490	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

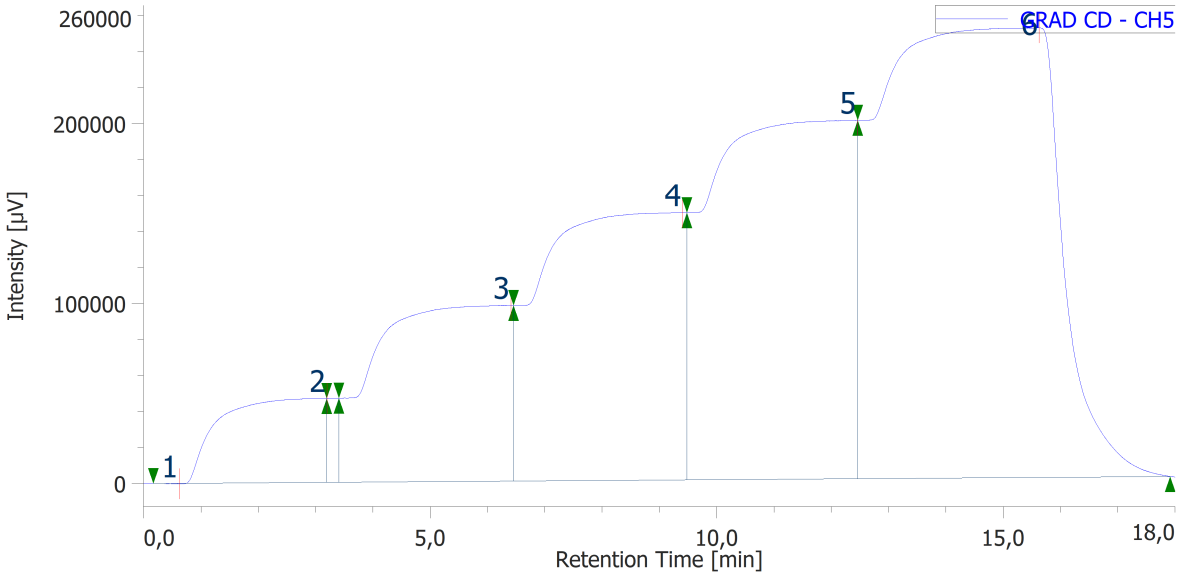

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 12:04:30
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 11:46:28
Volume	0,1 [µL]
Sample #	43
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	GRAD
Control Method	Grad_CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD CD-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	0,620	774	248	0,001	0,033	N/A	14	N/A	0,641	
2	20%	5	3,200	588266	46602	0,461	6,286	N/A	N/A	N/A	N/A	
3	40%	5	6,407	15556294	97527	12,182	13,154	N/A	N/A	N/A	N/A	
4	60%	5	9,400	24776407	148418	19,402	20,018	N/A	N/A	N/A	N/A	
5	80%	5	12,453	33548129	199002	26,271	26,841	N/A	N/A	N/A	N/A	
6	100%	5	15,623	53230782	249611	41,684	33,667	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

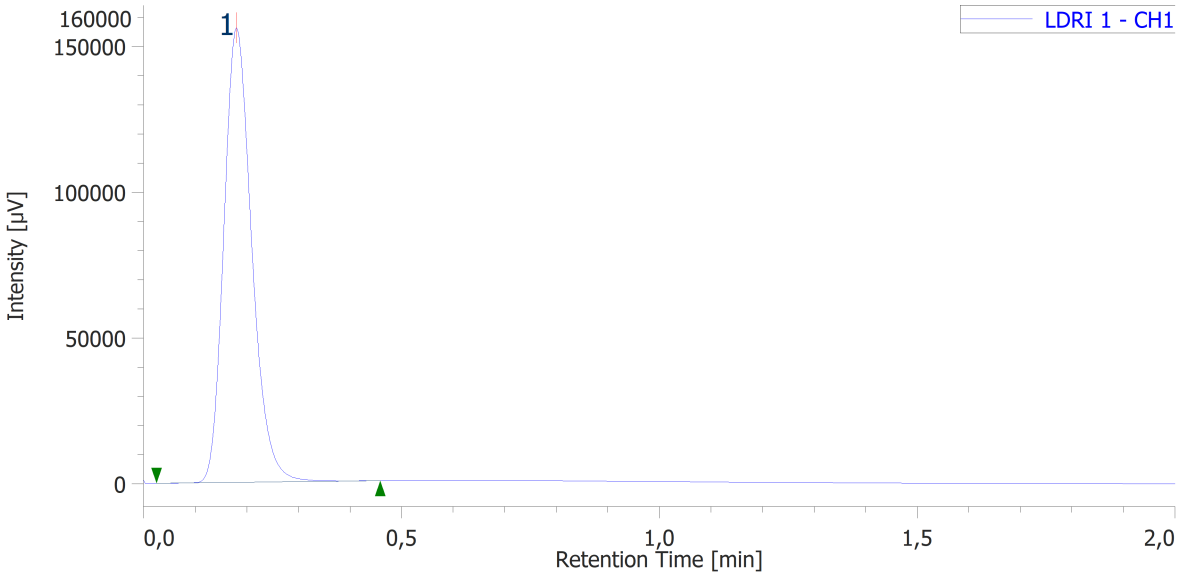

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 14:43:45
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 14:41:42
Volume	5,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Glicose
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicose	1	0,180	585005	155820	100,000	100,000	N/A	55	N/A	1,230	

Creator
Reviewer
Approver

Chromatogram

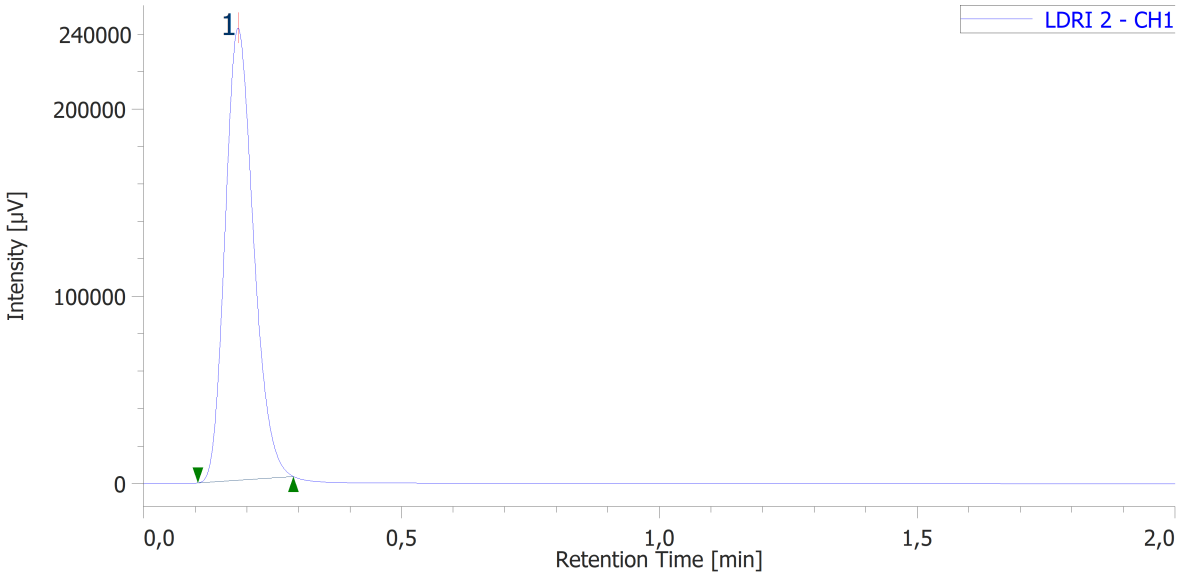

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 14:46:15
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 14:44:13
Volume	10,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Glicose
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicose	1	0,183	922831	241446	100,000	100,000	N/A	53	N/A	1,204	

Creator
Reviewer
Approver

Chromatogram

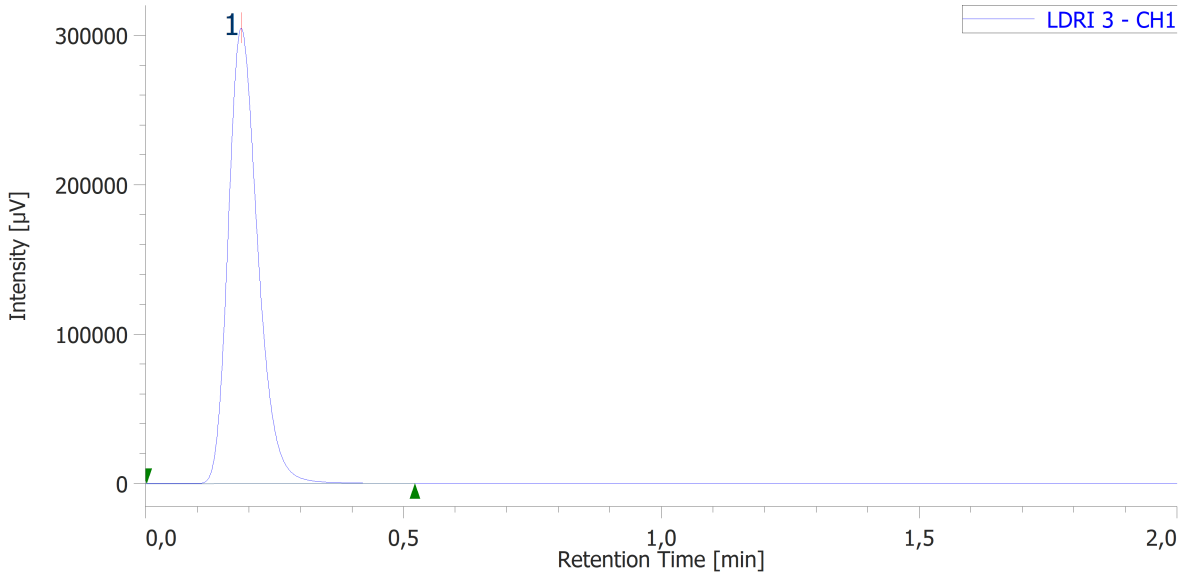

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 14:48:55
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 14:46:53
Volume	15,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Glicose
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicose	1	0,185	1214574	304694	100,000	100,000	N/A	52	N/A	1,272	

Creator
Reviewer
Approver

Chromatogram

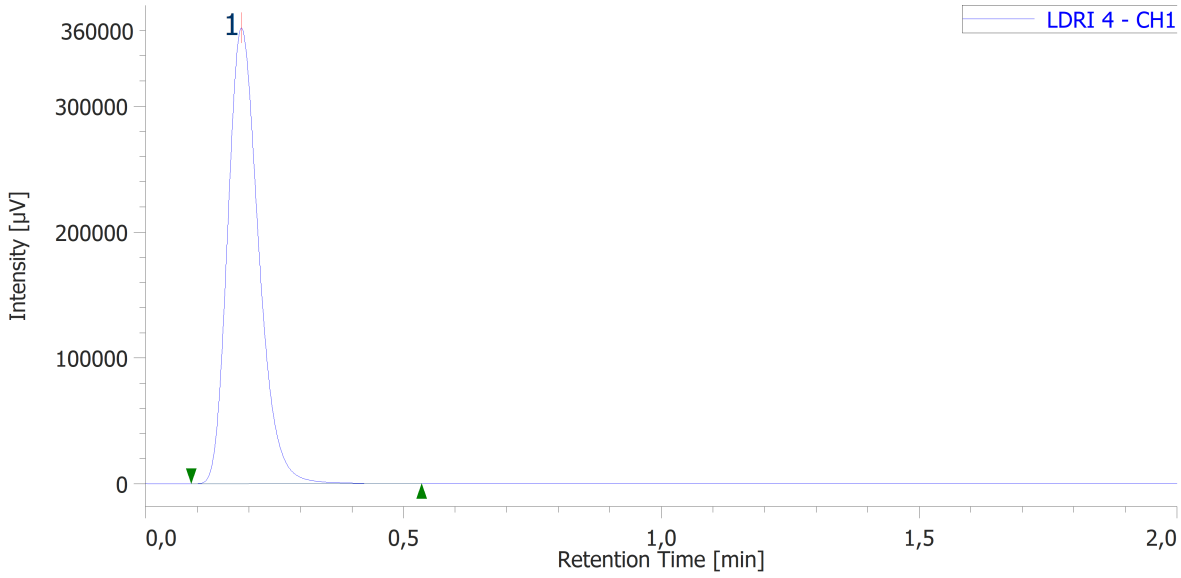

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 14:51:45
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 14:49:44
Volume	20,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Glicose
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicose	1	0,185	1506646	361753	100,000	100,000	N/A	47	N/A	1,273	

Creator
Reviewer
Approver

Chromatogram

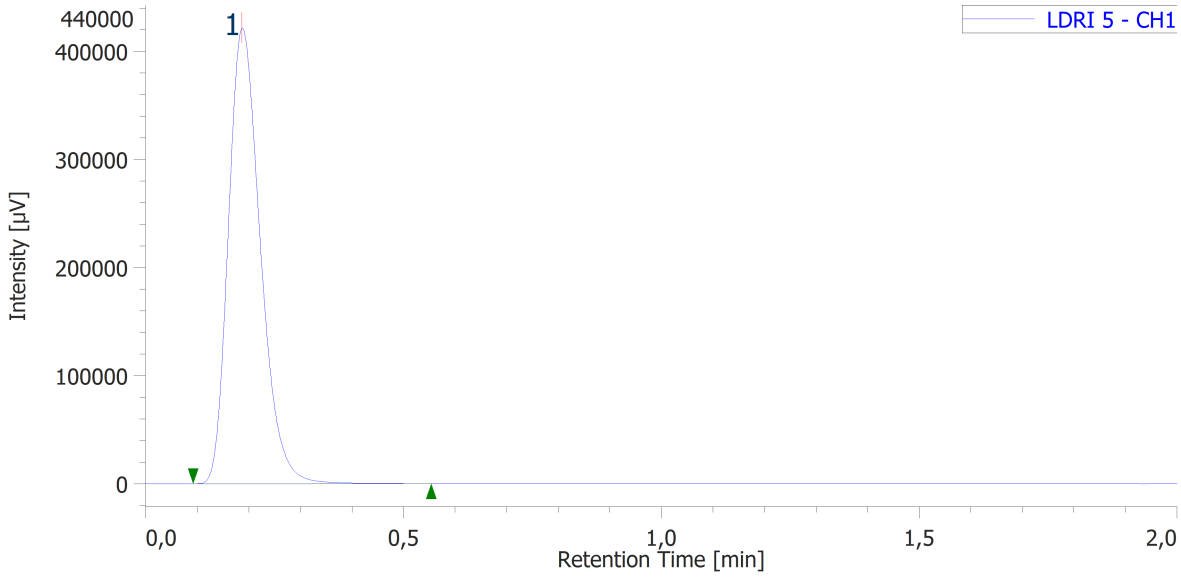

Chromatogram Information	
User Name	QPackSA
Date Modified	30/05/2023 14:54:47
Description	
HPLC System Name	01-HP-03
Injection Date	30/05/2023 14:52:45
Volume	25,0 [µL]
Sample #	47
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	Glicose
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Glicose	1	0,187	1814334	421402	100,000	100,000	N/A	44	N/A	1,298	

Creator
Reviewer
Approver