HPLC 1220 - Agilent Lab Advisor

Agilent Lab Advisor for LC & CE

Service & Diagnostics

Basic Version

Tasks

Lab Advisor

- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1220

- Service & Diagnostics
- Instrument Control
- EMFs
- Status Report


Help

- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan - VWD [DECAD00126]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1 | Export Data

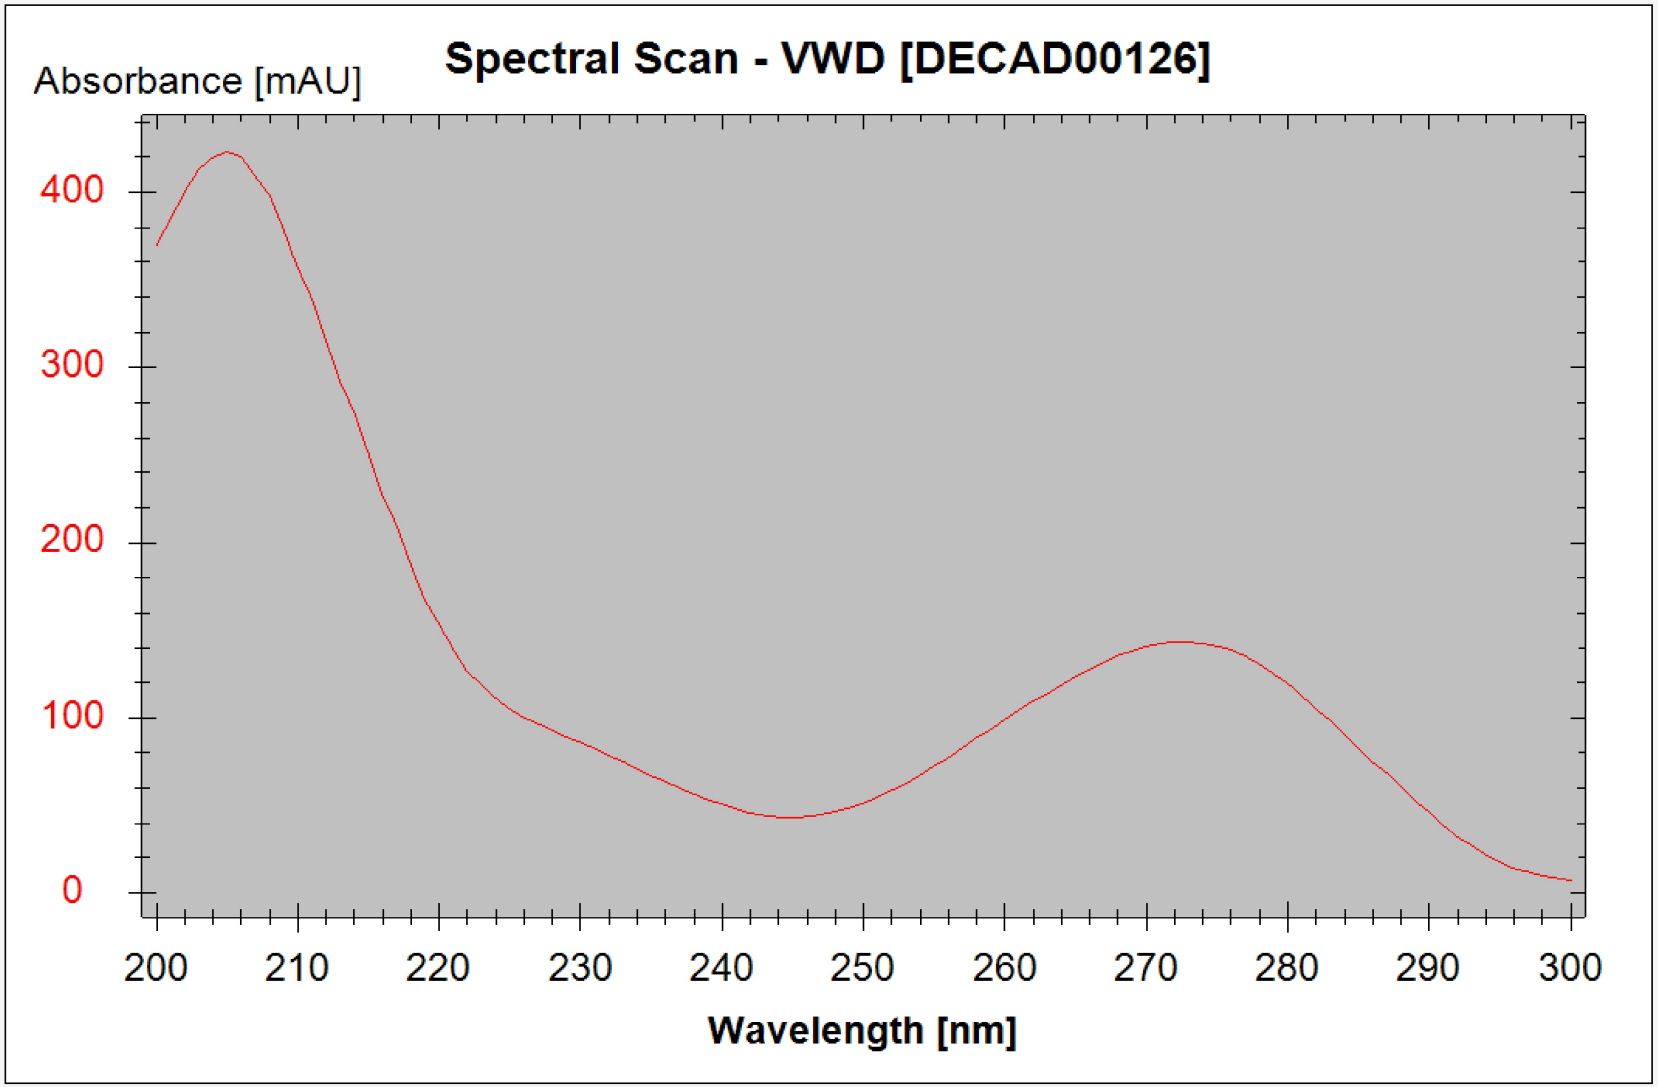

more... | Print Result | Rerun | Back

Connection Address: 100.1.1.102

Version B.02.03 [064] - Basic | Licenses 4/10

PT 11:37 AM 10/28/2020

HPLC 1220 - Agilent Lab Advisor

Agilent Lab Advisor for LC & CE

Service & Diagnostics

Basic Version

Tasks

Lab Advisor

- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1220

- Service & Diagnostics
- Instrument Control
- EMFs
- Status Report


Help

- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan - VWD [DECAD00126]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1 | Export Data

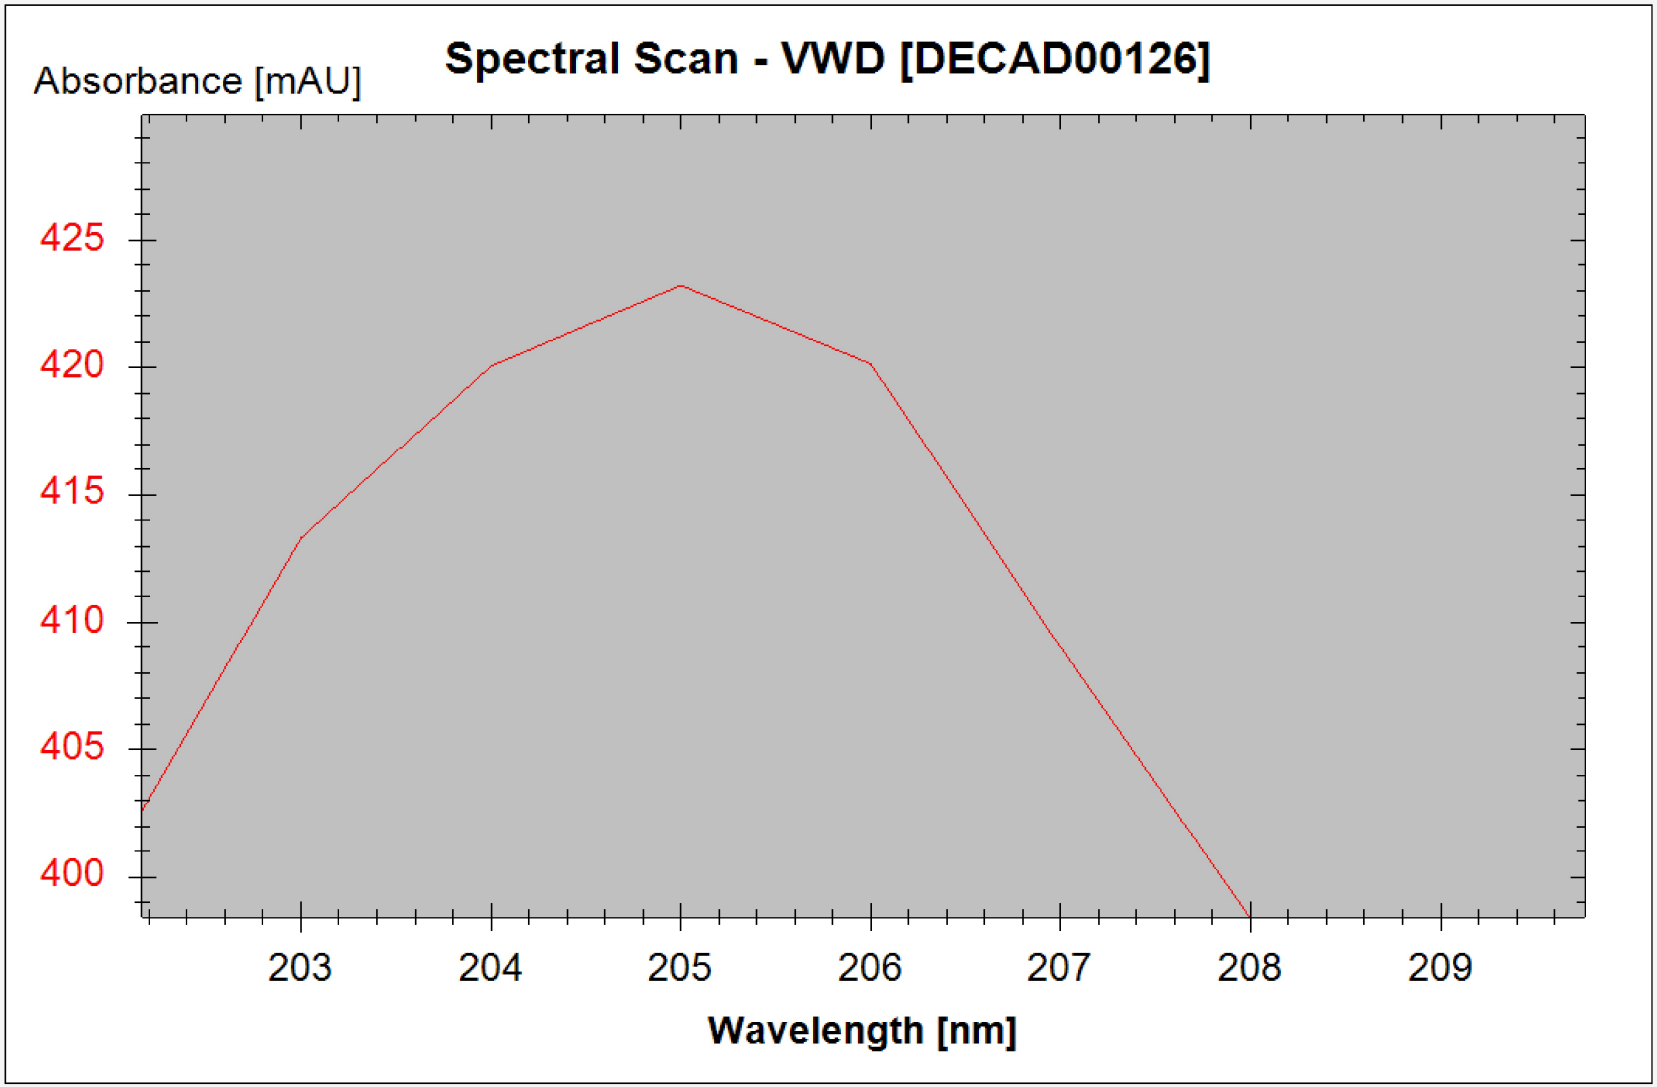

more... | Print Result | Rerun | Back

Connection Address: 100.1.1.102

Version B.02.03 [064] - Basic | Licenses 4/10

PT 11:38 AM 10/28/2020

HPLC 1220 - Agilent Lab Advisor

Agilent Lab Advisor for LC & CE

Service & Diagnostics

Basic Version

Tasks

Lab Advisor

- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1220

- Service & Diagnostics
- Instrument Control
- EMFs
- Status Report


Help

- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan - VWD [DECAD00126]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1 | Export Data

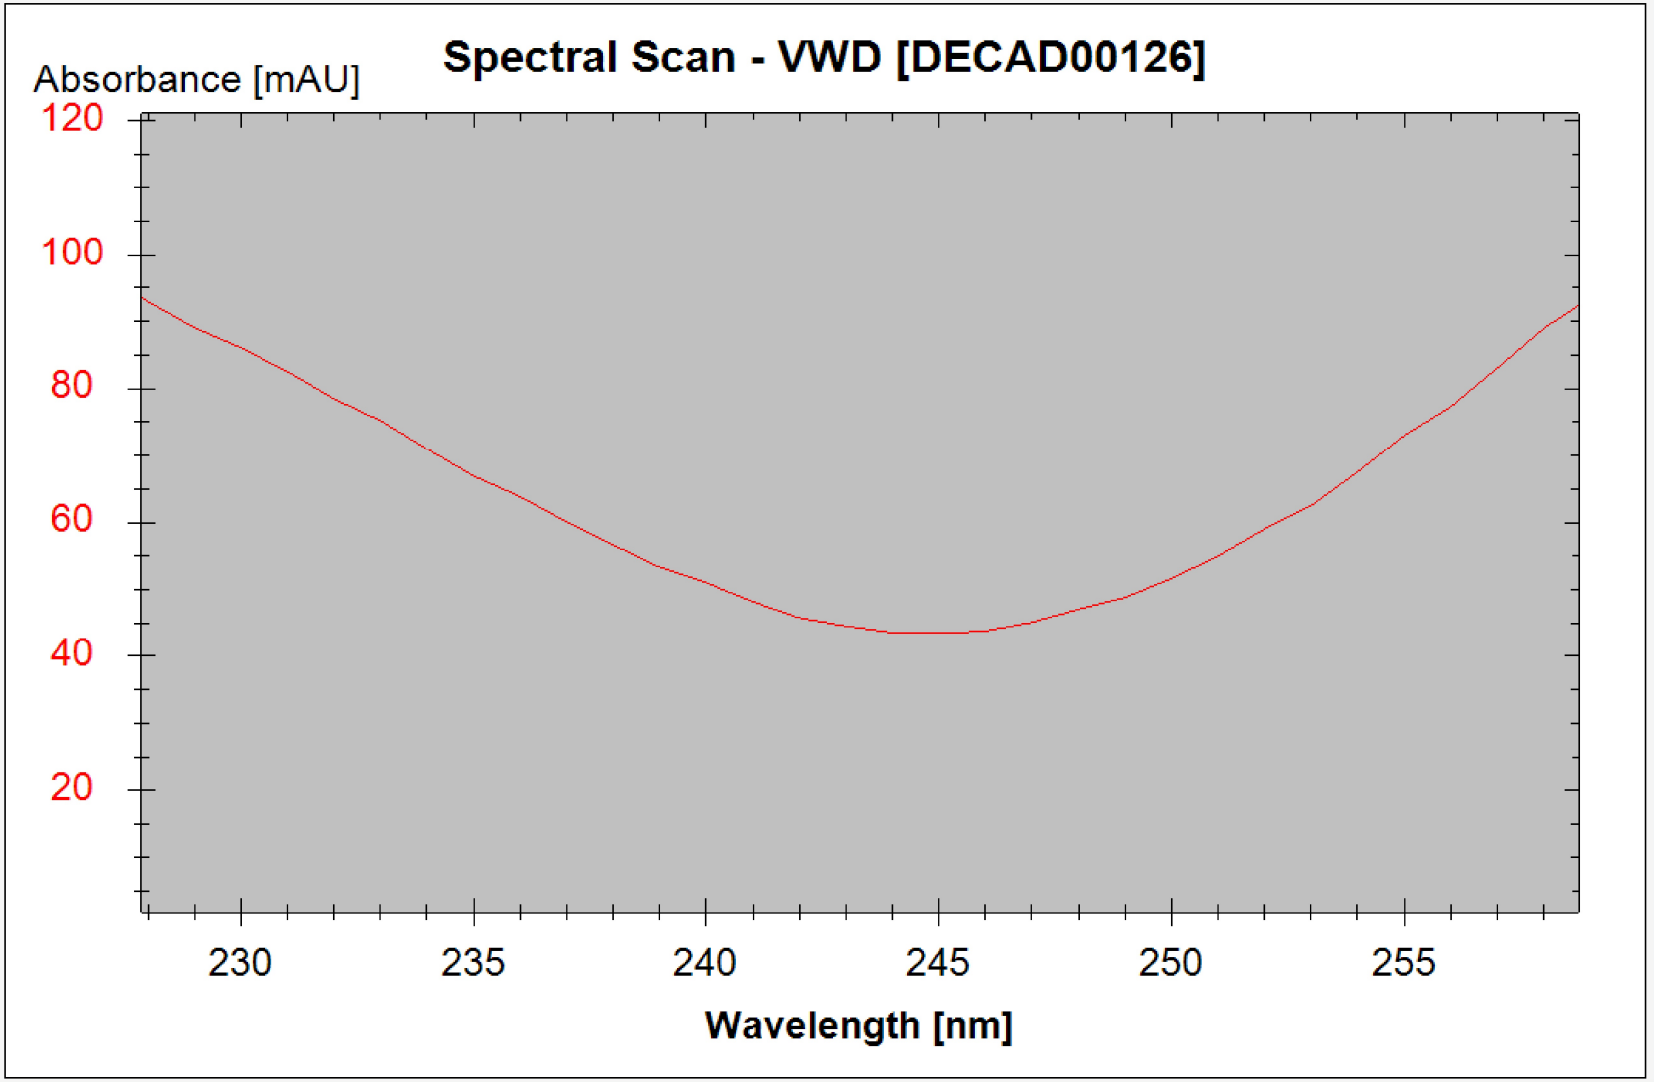

more... | Print Result | Rerun | Back

Connection Address: 100.1.1.102

Version B.02.03 [064] - Basic | Licenses 4/10

PT 11:39 AM 10/28/2020

HPLC 1220 - Agilent Lab Advisor

Agilent Lab Advisor for LC & CE

Service & Diagnostics

Basic Version

Tasks

Lab Advisor

- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1220

- Service & Diagnostics
- Instrument Control
- EMFs
- Status Report


Help

- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan - VWD [DECAD00126]

UV Lamp On | Blank Scan

Sample Scan | from 200 | to 300 | step 1 | Export Data

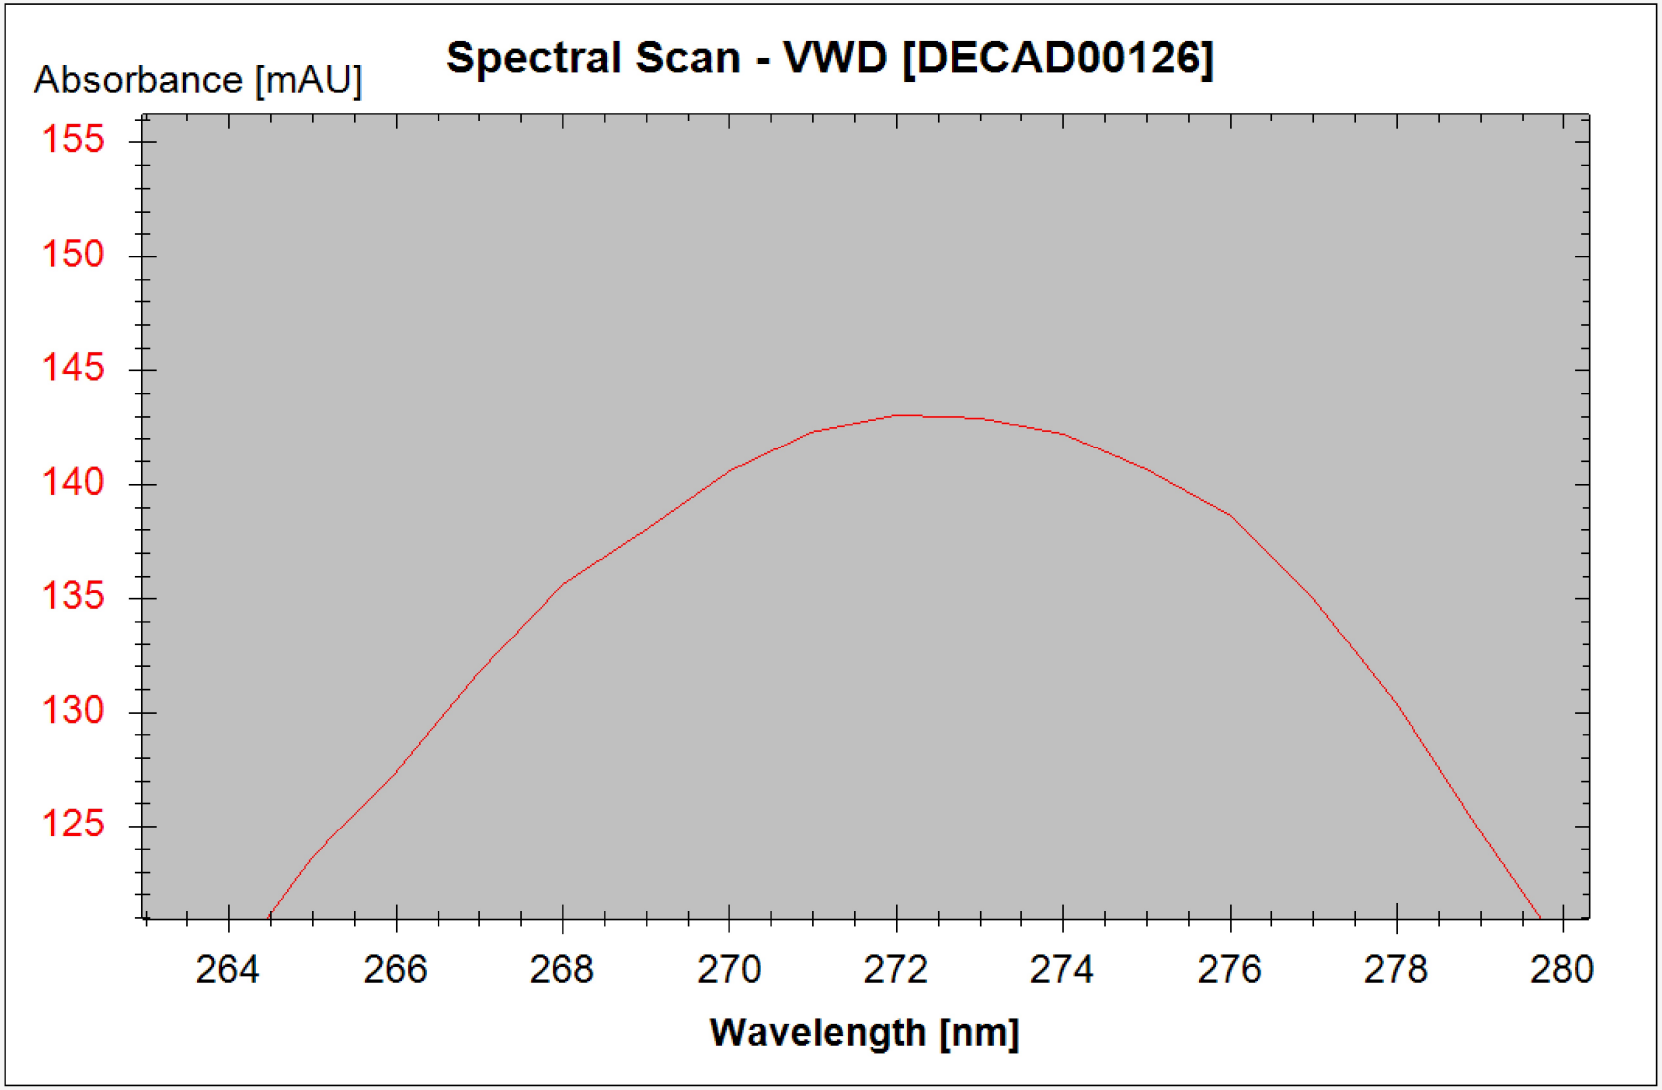

more... | Print Result | Rerun | Back

Connection Address: 100.1.1.102


Version B.02.03 [064] - Basic | Licenses 4/10

PT 11:39 AM 10/28/2020

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0101.D
Sample Name: Branco 01

==========

Acq. Operator : Rodolfo (QPack) Seq. Line : 1
Acq. Instrument : HPLC Location : Vial 2
Injection Date : 10/28/2020 11:58:28 AM Inj : 1
Inj Volume : 10.000 µl
Acq. Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
(modified after loading)

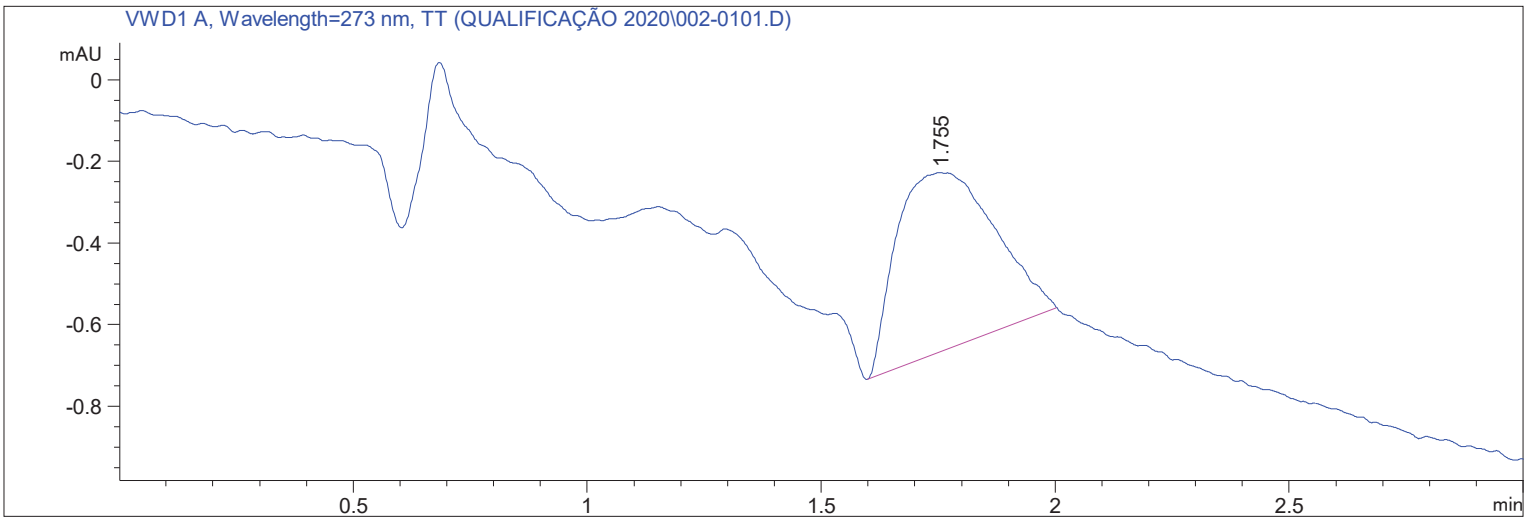

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.596		-	-	-		Cafeína

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0101.D
Sample Name: Branco 01

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	1.596		0.0000	0.00000	0.0000	Cafeína
2	1.755	BBA	0.1760	6.38107	100.0000	?

Totals : 6.38107

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0201.D
Sample Name: PCIN 01

```
==========================================================================
Acq. Operator    : Rodolfo (QPack)                 Seq. Line :   2
Acq. Instrument : HPLC                              Location : Vial 3
Injection Date  : 10/28/2020 12:02:18 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

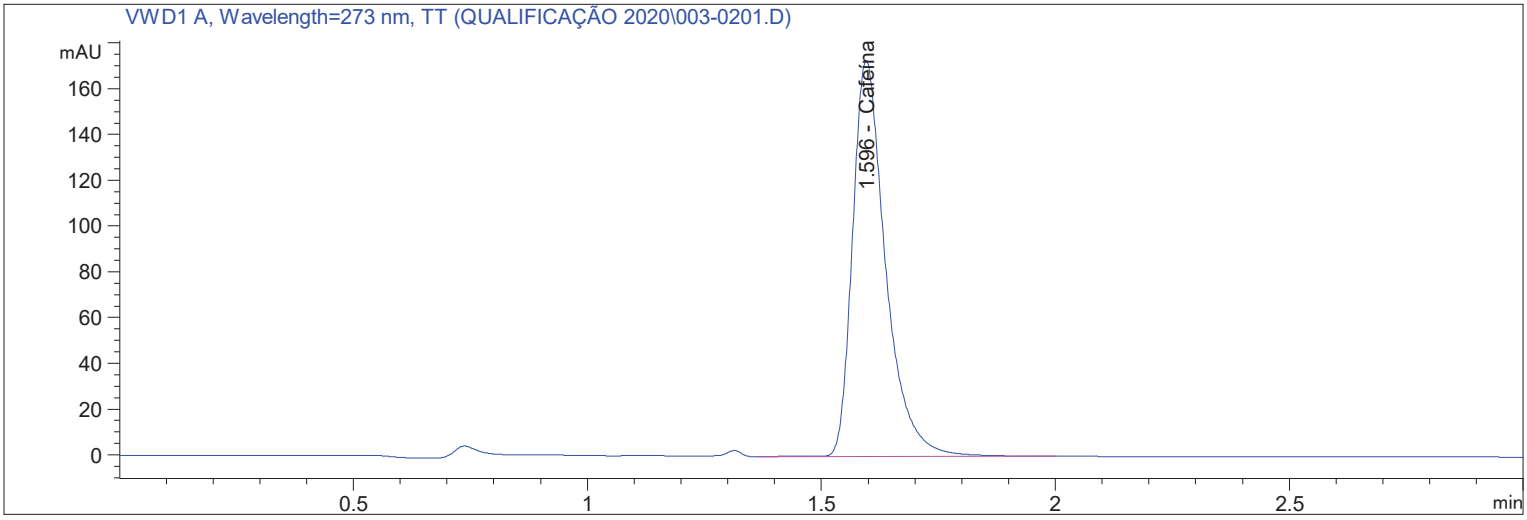


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.596 BBA     850.16327 1.17624e-3    1.00000    Cafeína

Totals :                                1.00000


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0301.D
Sample Name: PCIN 02

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   3
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 10/28/2020 12:06:09 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

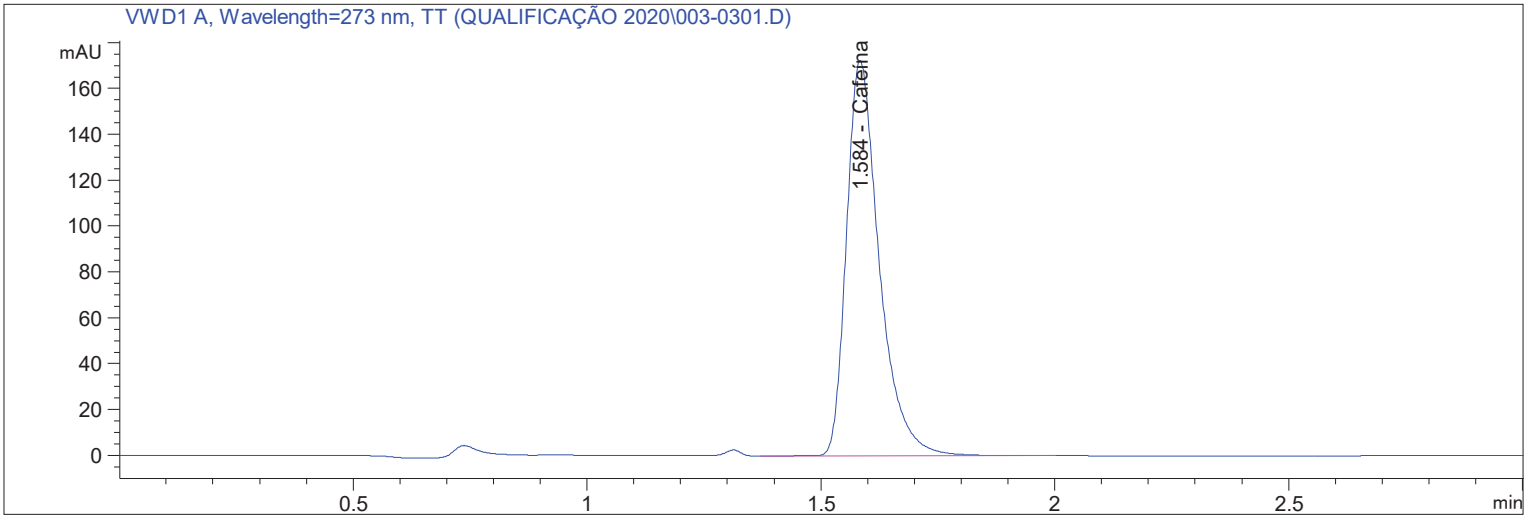


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.584 BBA     842.35205 1.17624e-3 9.90812e-1    Cafeína

Totals :                              9.90812e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0401.D
Sample Name: PCIN 03

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   4
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 10/28/2020 12:09:59 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

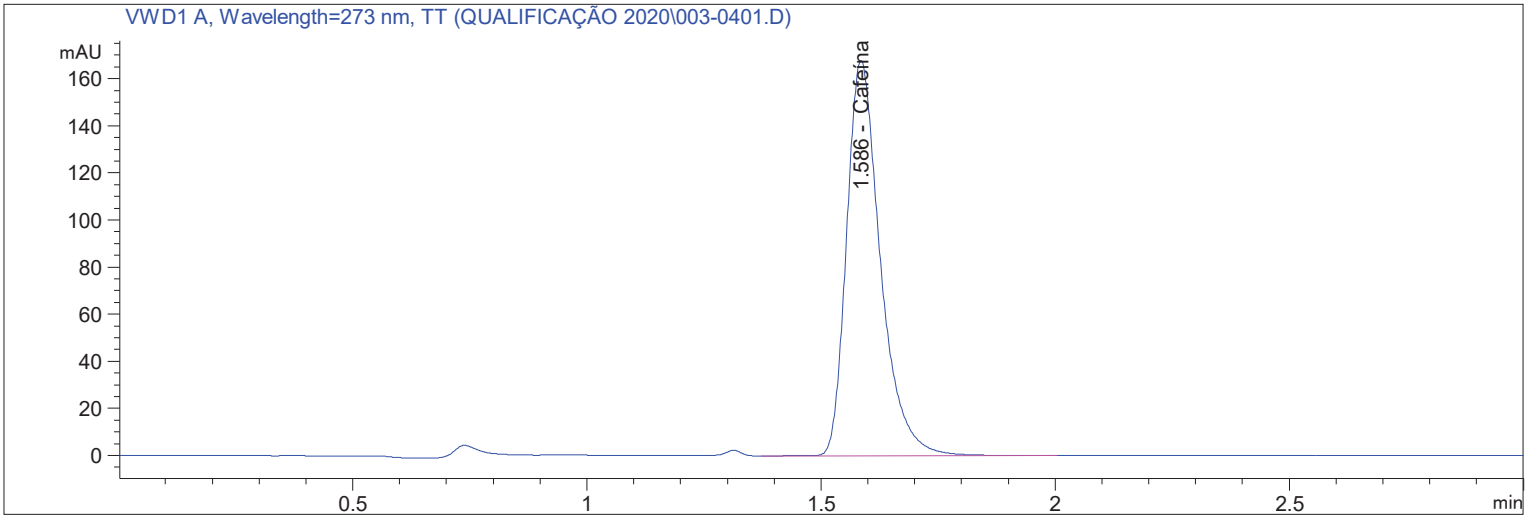


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.586 BBA     842.85297 1.17624e-3 9.91401e-1    Cafeína

Totals :                              9.91401e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0501.D
Sample Name: Branco 02

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   5
Acq. Instrument : HPLC                            Location : Vial 2
Injection Date  : 10/28/2020 12:13:50 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

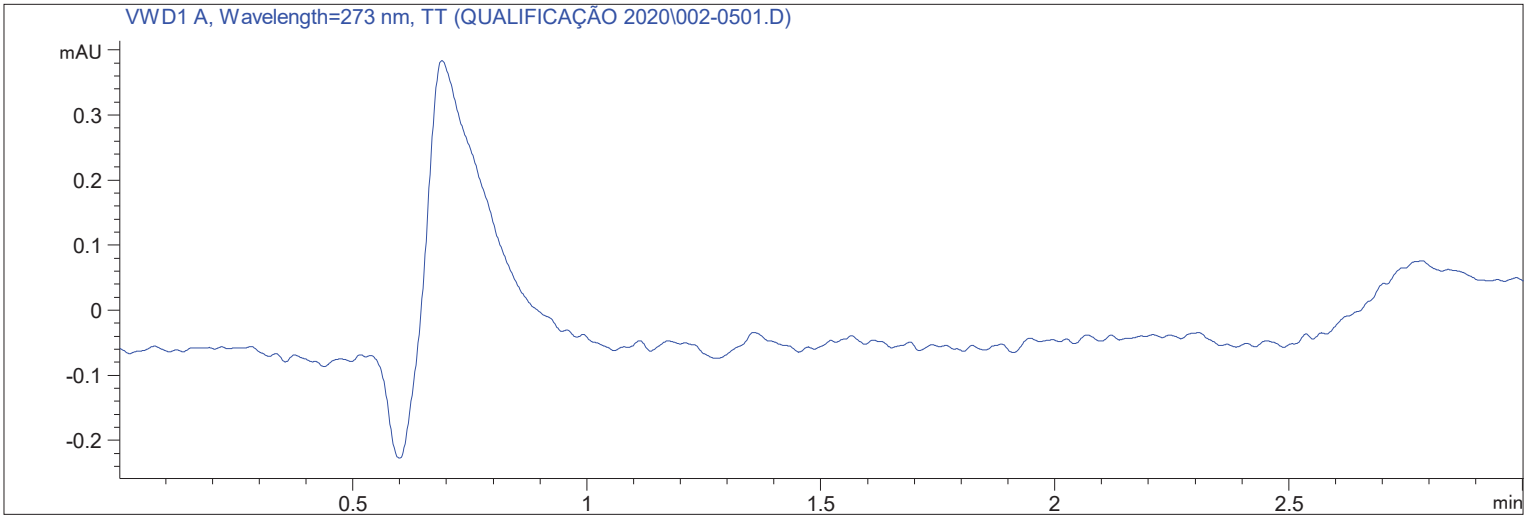


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|------------------
  1.596            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0501.D
Sample Name: Branco 02

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	1.596		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0601.D
Sample Name: PCIN 04

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   6
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 10/28/2020 12:17:39 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

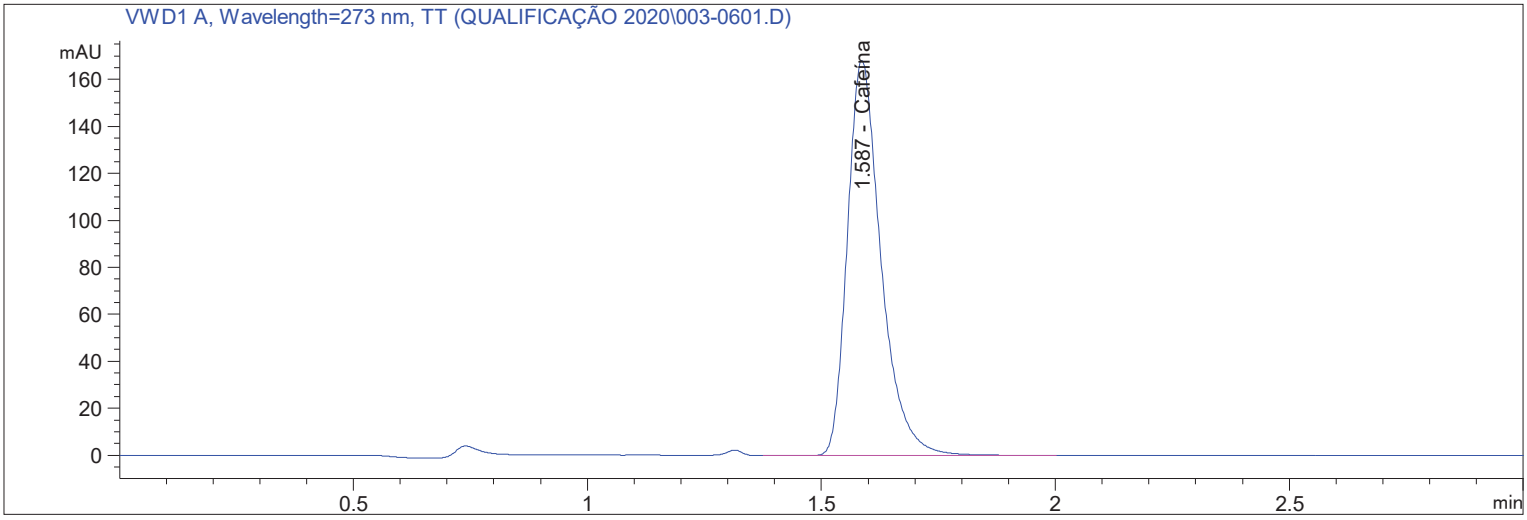


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.587 BBA     842.33942 1.17624e-3 9.90797e-1    Cafeína

Totals :                              9.90797e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0701.D
Sample Name: PCIN 05

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   7
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 10/28/2020 12:21:27 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

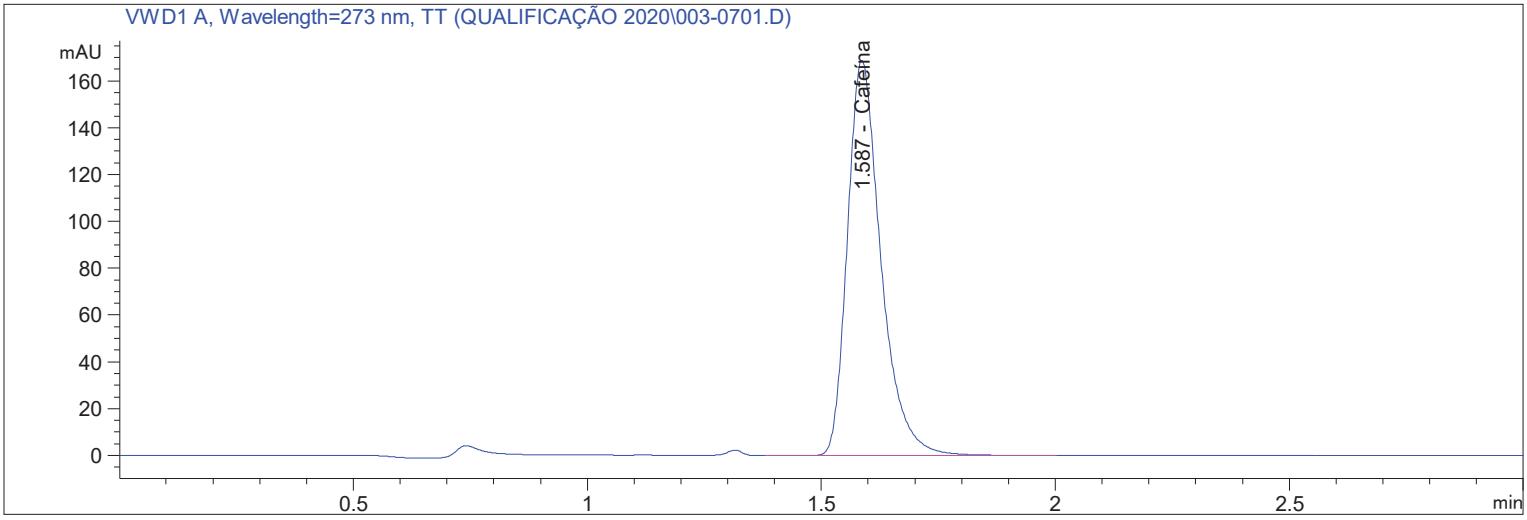


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.587 BBA     842.47217 1.17624e-3 9.90953e-1    Cafeína

Totals :                              9.90953e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\003-0801.D
Sample Name: PCIN 06

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :   8
Acq. Instrument : HPLC                            Location : Vial 3
Injection Date  : 10/28/2020 12:25:17 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

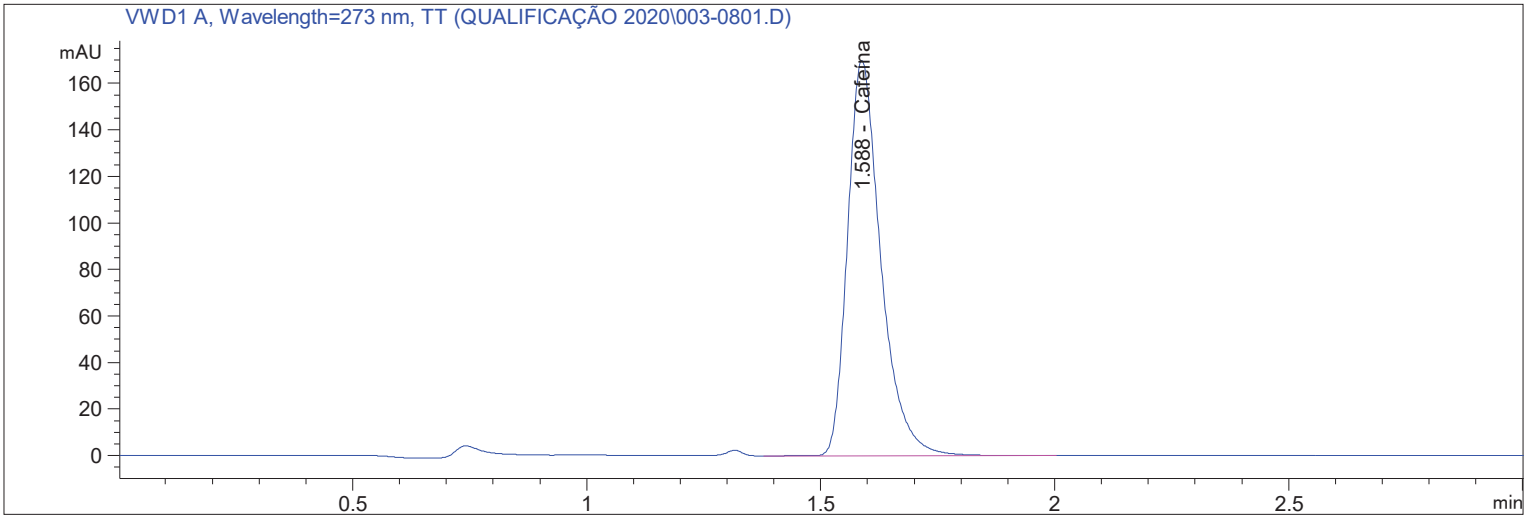


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.588 BBA     842.08374 1.17624e-3 9.90496e-1    Cafeína

Totals :                              9.90496e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0901.D
Sample Name: Branco 03

```
==========================================================================
Acq. Operator    : Rodolfo (QPack)                Seq. Line :   9
Acq. Instrument : HPLC                             Location : Vial 2
Injection Date  : 10/28/2020 12:29:09 PM                Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

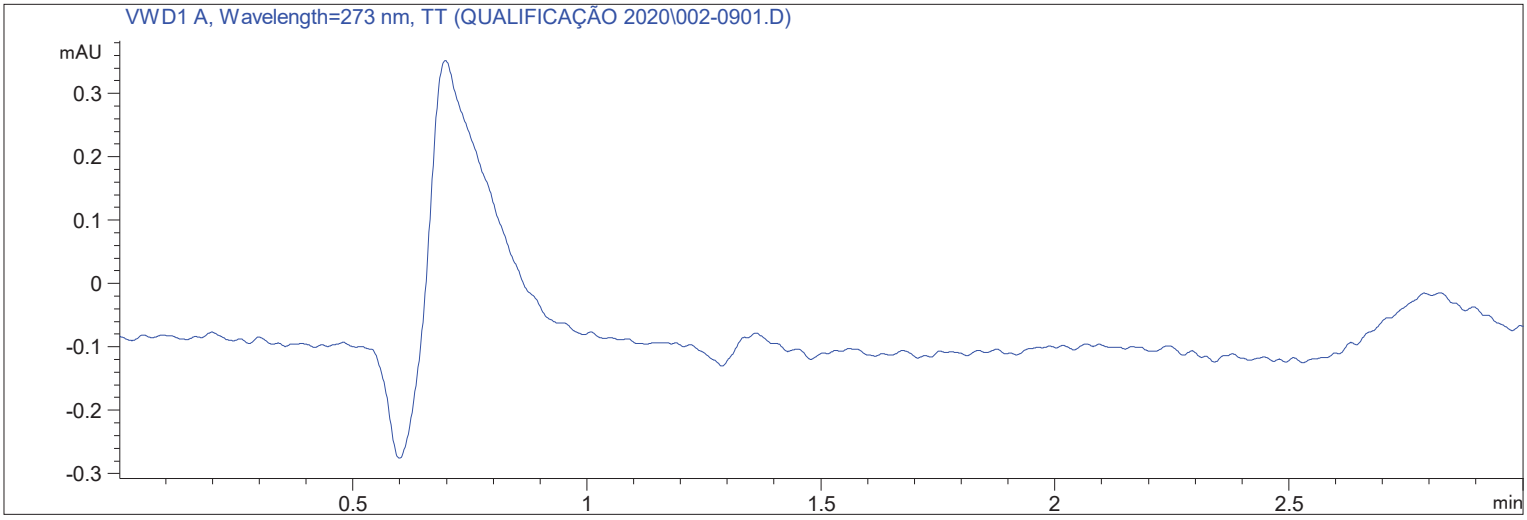


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.596            -          -          -         Cafeína

Totals :                                0.00000


1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========================================================================
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\002-0901.D
Sample Name: Branco 03

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	1.596		0.0000	0.00000	0.0000	Cafeína

Totals : 0.00000

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\004-1001.D
Sample Name: LDUV 01

```
==========================================================================
Acq. Operator    : Rodolfo (QPack)                 Seq. Line :  10
Acq. Instrument : HPLC                              Location : Vial 4
Injection Date  : 10/28/2020 12:33:01 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

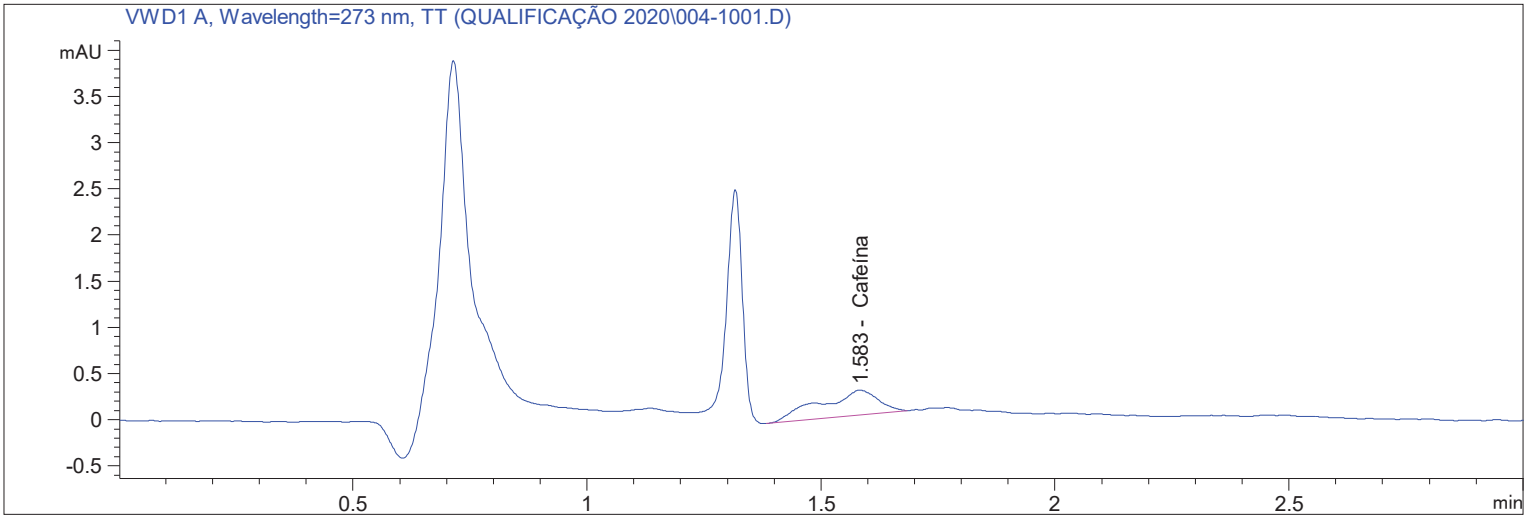


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.583 BB        2.38361 1.17624e-3 2.80370e-3    Cafeína

Totals :                              2.80370e-3


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\005-1101.D
Sample Name: LDUV 02

```
==========================================================================
Acq. Operator    : Rodolfo (QPack)                 Seq. Line :  11
Acq. Instrument : HPLC                              Location : Vial 5
Injection Date  : 10/28/2020 12:36:56 PM                 Inj :   1
                                                  Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

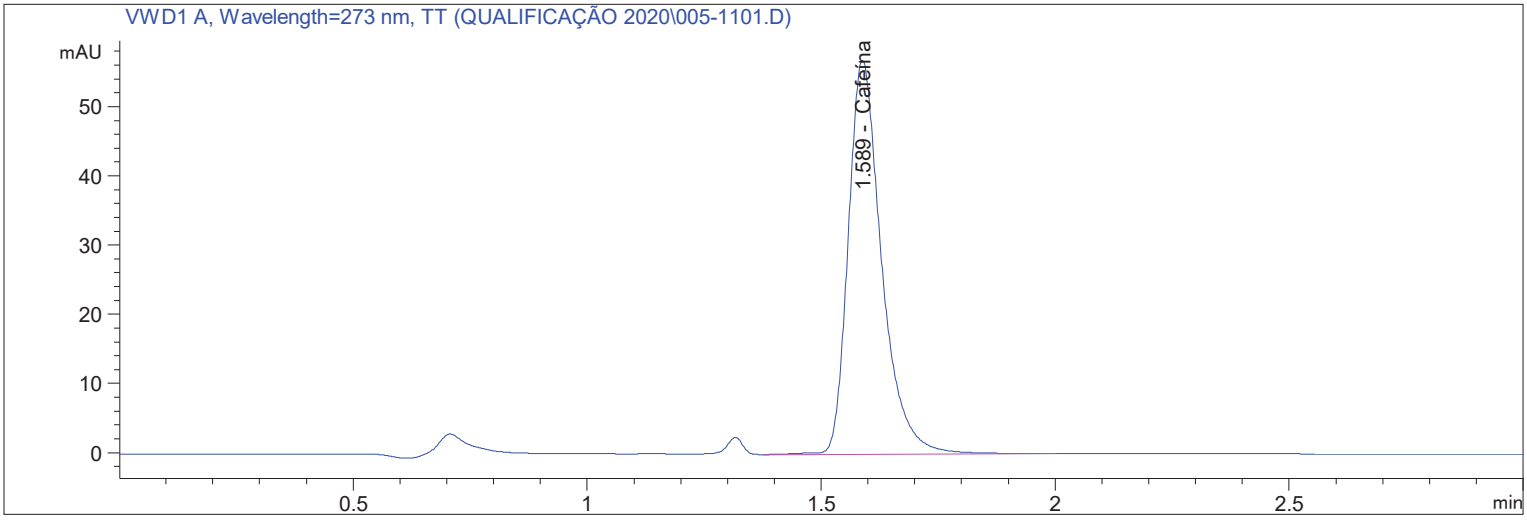


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.589 BBA     282.39255 1.17624e-3 3.32163e-1    Cafeína

Totals :                              3.32163e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\006-1201.D
Sample Name: LDUV 03

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :  12
Acq. Instrument : HPLC                            Location : Vial 6
Injection Date  : 10/28/2020 12:40:47 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

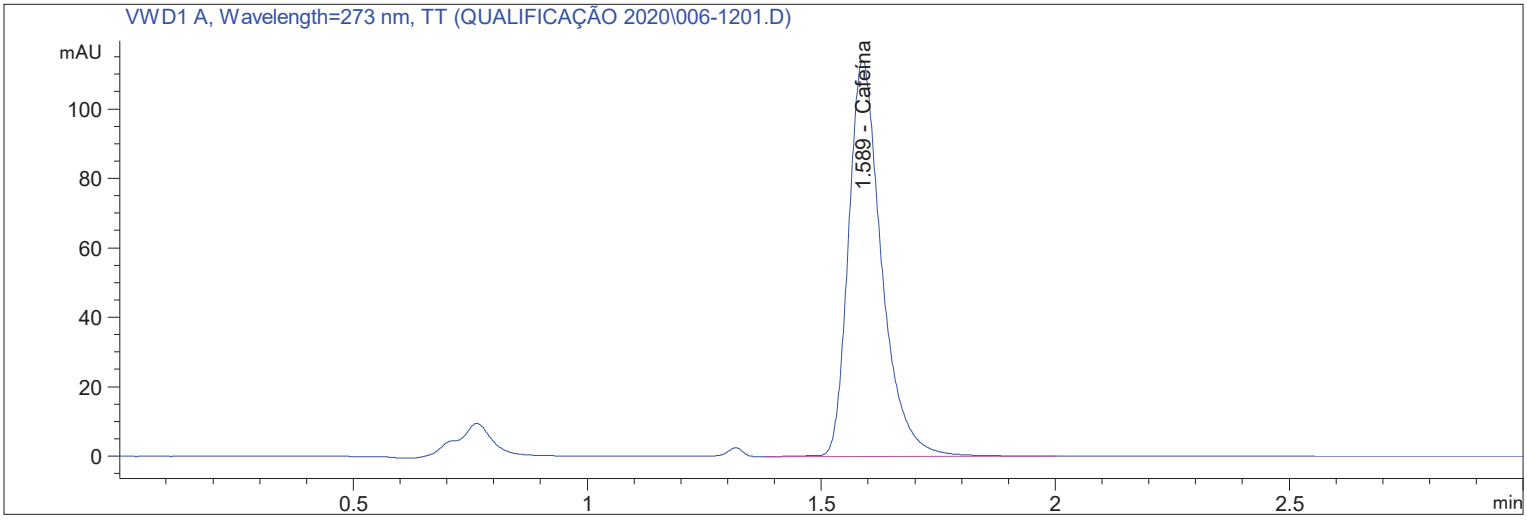


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount    Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.589 BBA     559.75006 1.17624e-3 6.58403e-1    Cafeína

Totals :                              6.58403e-1


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\007-1301.D
Sample Name: LDUV 04

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :  13
Acq. Instrument : HPLC                            Location : Vial 7
Injection Date  : 10/28/2020 12:44:37 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

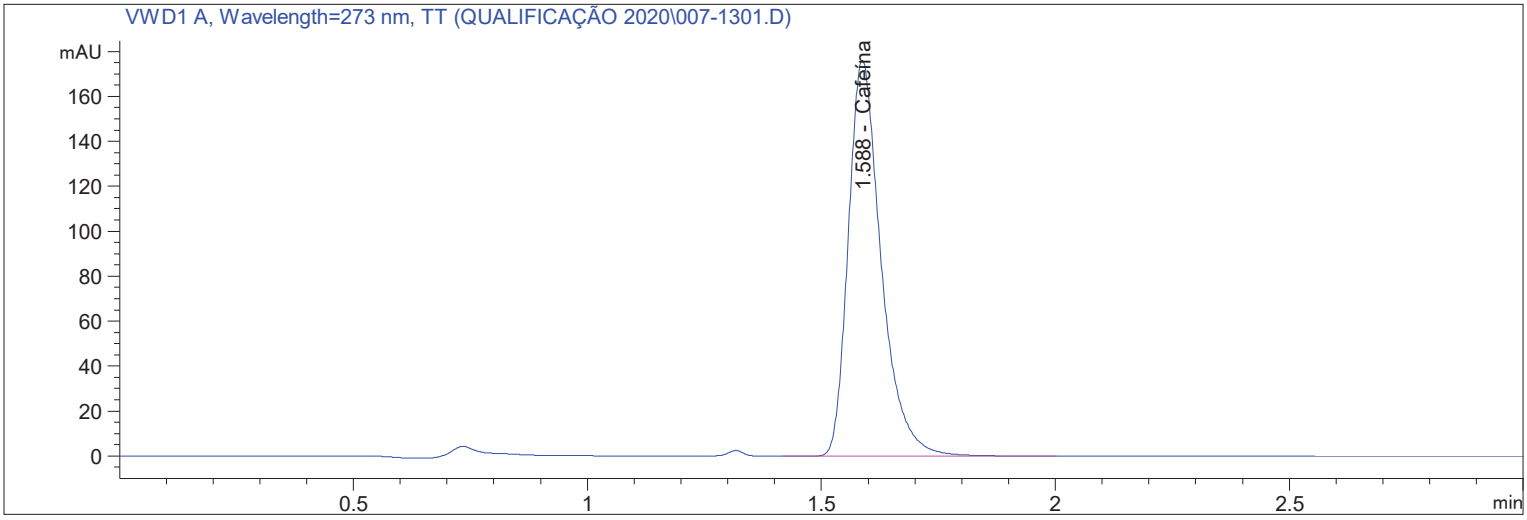


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.588 BBA     858.95465 1.17624e-3    1.01034    Cafeína

Totals :                                1.01034


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\008-1401.D
Sample Name: LDUV 05

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :  14
Acq. Instrument : HPLC                            Location : Vial 8
Injection Date  : 10/28/2020 12:48:28 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

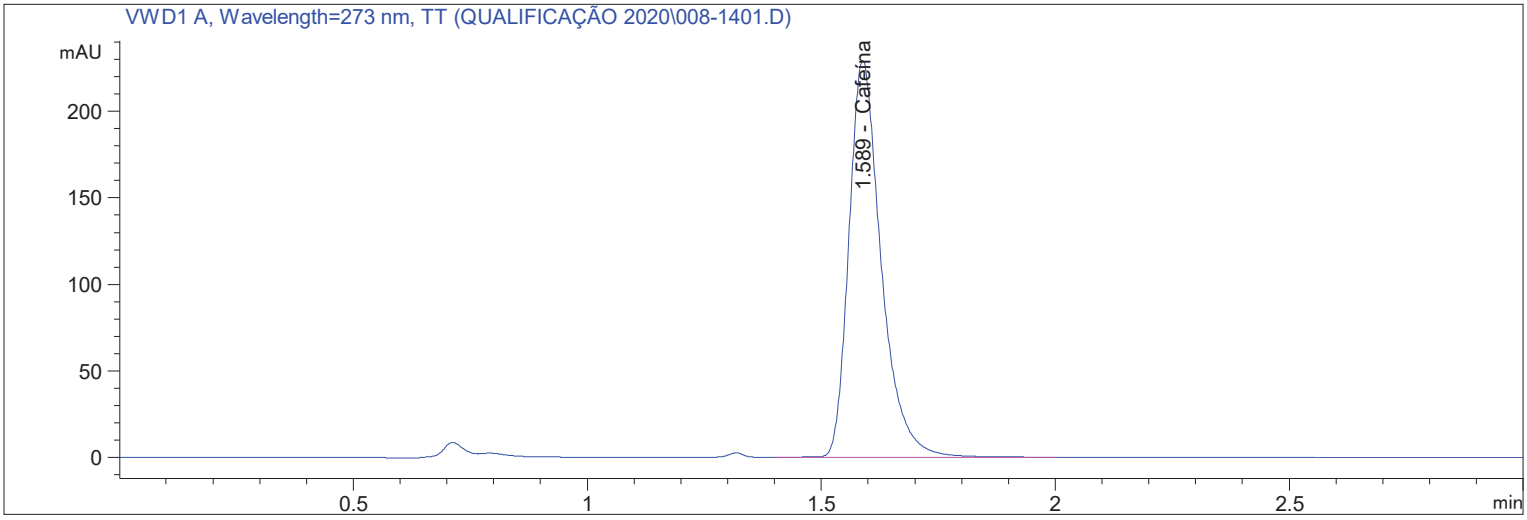


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.589 BBA    1098.70972 1.17624e-3    1.29235    Cafeína


Totals :                                1.29235


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1501.D
Sample Name: LIIN 01

==========

Acq. Operator : Rodolfo (QPack) Seq. Line : 15
Acq. Instrument : HPLC Location : Vial 9
Injection Date : 10/28/2020 12:51:37 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 0.000 µl
Acq. Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
(modified after loading)

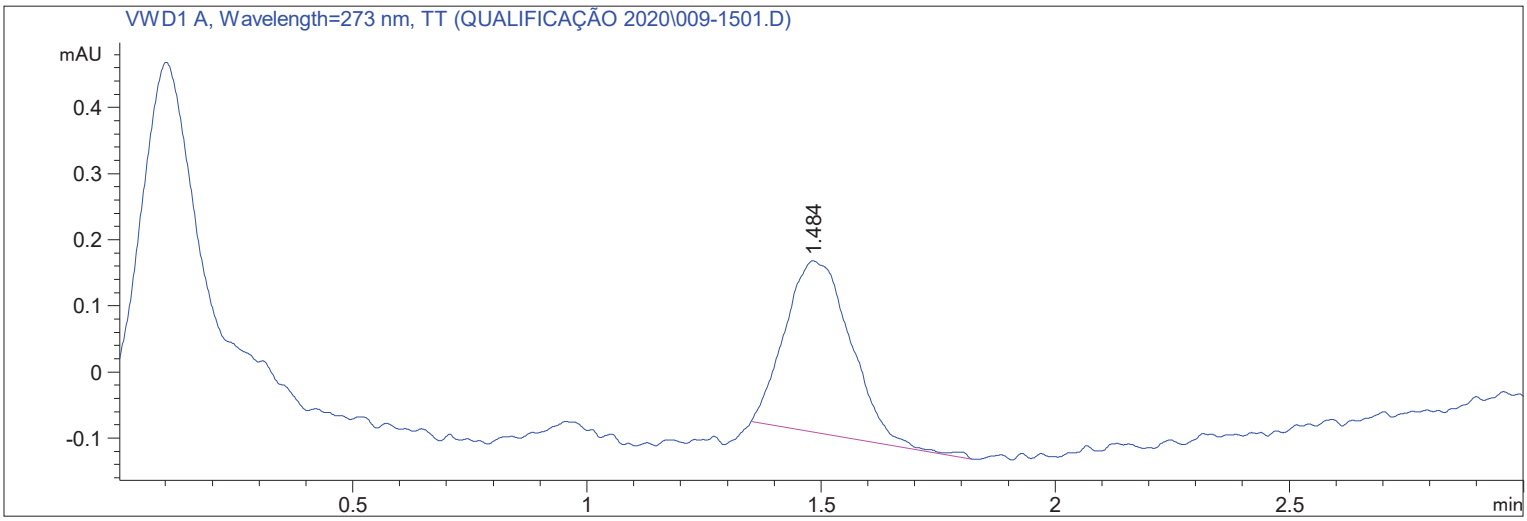

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.596		-	-	-		Cafeína

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

==========

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1501.D
Sample Name: LIIN 01

==========

Area Percent Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Area %	Name
1	1.484	BB	0.1333	2.55807	100.0000	?
2	1.596		0.0000	0.00000	0.0000	Cafeína

Totals : 2.55807

1 Warnings or Errors :


Warning : Calibrated compound(s) not found

==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1601.D
Sample Name: LIIN 02

Acq. Operator : Rodolfo (QPack) Seq. Line : 16
Acq. Instrument : HPLC Location : Vial 9
Injection Date : 10/28/2020 12:55:34 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 5.000 µl
Acq. Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
(modified after loading)

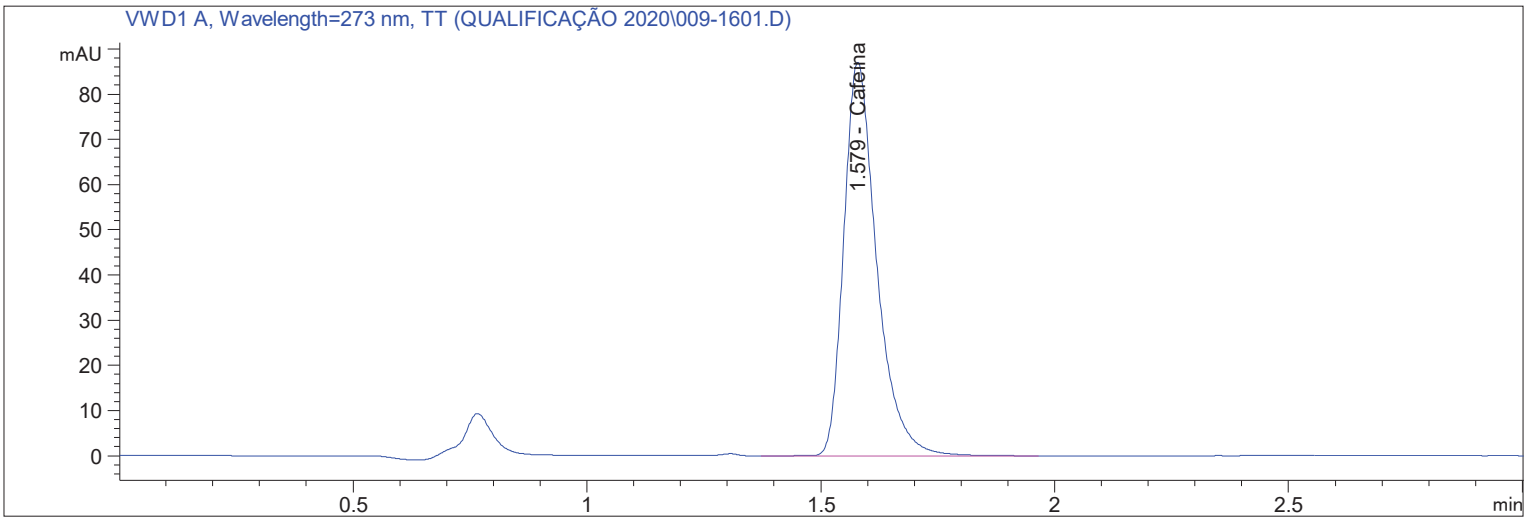

External Standard Report

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT


RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.579	BBA	426.45297	1.17624e-3	5.01613e-1		Cafeína

Totals : 5.01613e-1

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1701.D
Sample Name: LIIN 03

```
==========================================================================
Acq. Operator   : Rodolfo (QPack)                Seq. Line :  17
Acq. Instrument : HPLC                            Location : Vial 9
Injection Date  : 10/28/2020 12:59:26 PM               Inj :   1
                                                 Inj Volume : 10.000 µl
Acq. Method     : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed    : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
                  (modified after loading)
```

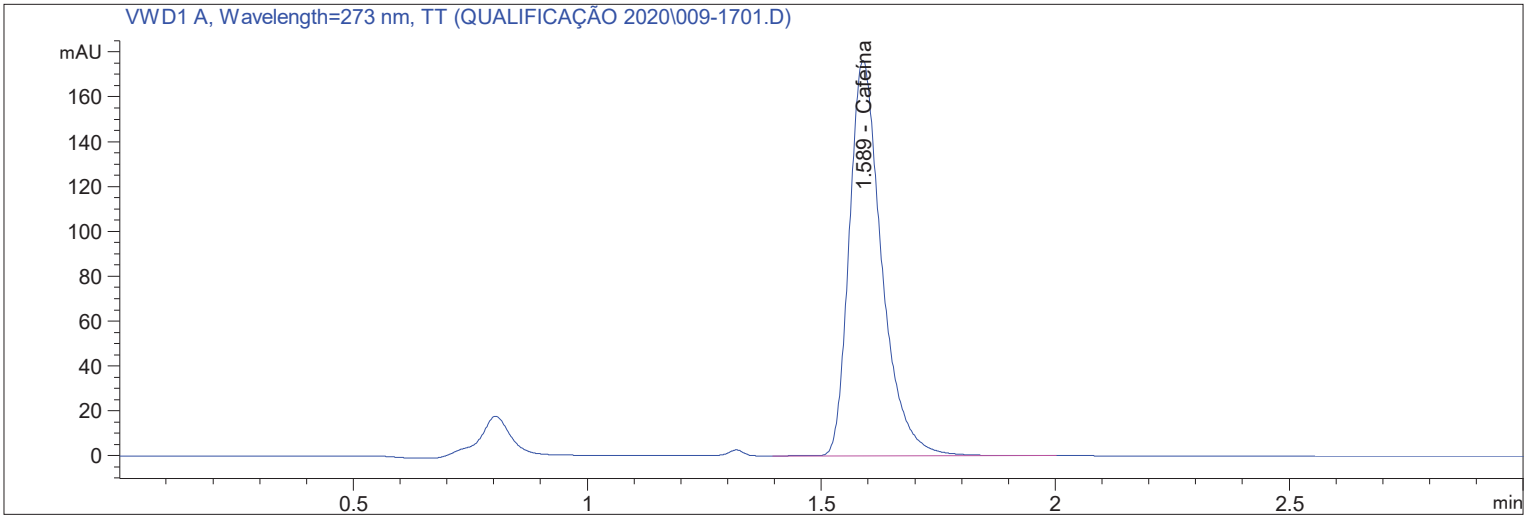


```
==========================================================================
                      External Standard Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      Wednesday, October 28, 2020 12:16:24 PM
Multiplier:                   :      1.0000
Dilution:                     :      1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime  Type     Area     Amt/Area    Amount   Grp   Name
 [min]          [mAU*s]               [ng/ul]
-------|------|----------|----------|----------|--|-----------------
  1.589 BBA     850.32220 1.17624e-3    1.00019    Cafeína


Totals :                                1.00019


==========================================================================
                          *** End of Report ***
```

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1801.D
Sample Name: LIIN 04

==========

Acq. Operator : Rodolfo (QPack) Seq. Line : 18
Acq. Instrument : HPLC Location : Vial 9
Injection Date : 10/28/2020 1:03:21 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 15.000 µl
Acq. Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
(modified after loading)

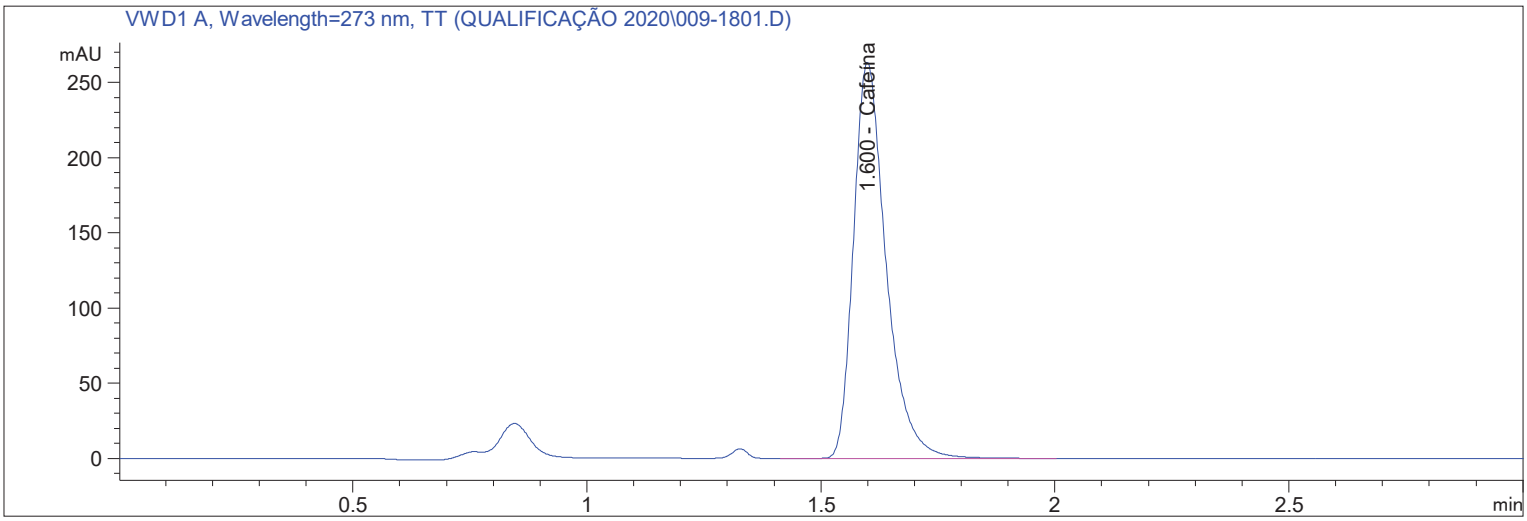

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.600	BBA	1274.80518	1.17624e-3	1.49948		Cafeína

Totals : 1.49948


==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\009-1901.D
Sample Name: LIIN 05

==========

Acq. Operator : Rodolfo (QPack) Seq. Line : 19
Acq. Instrument : HPLC Location : Vial 9
Injection Date : 10/28/2020 1:07:19 PM Inj : 1
Inj Volume : 10.000 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 20.000 µl
Acq. Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 11:57:35 AM by Rodolfo (QPack)
Analysis Method : C:\CHEM32\2\METHODS\QUALIFICAÇÃO.M
Last changed : 10/28/2020 12:16:36 PM by Rodolfo (QPack)
(modified after loading)

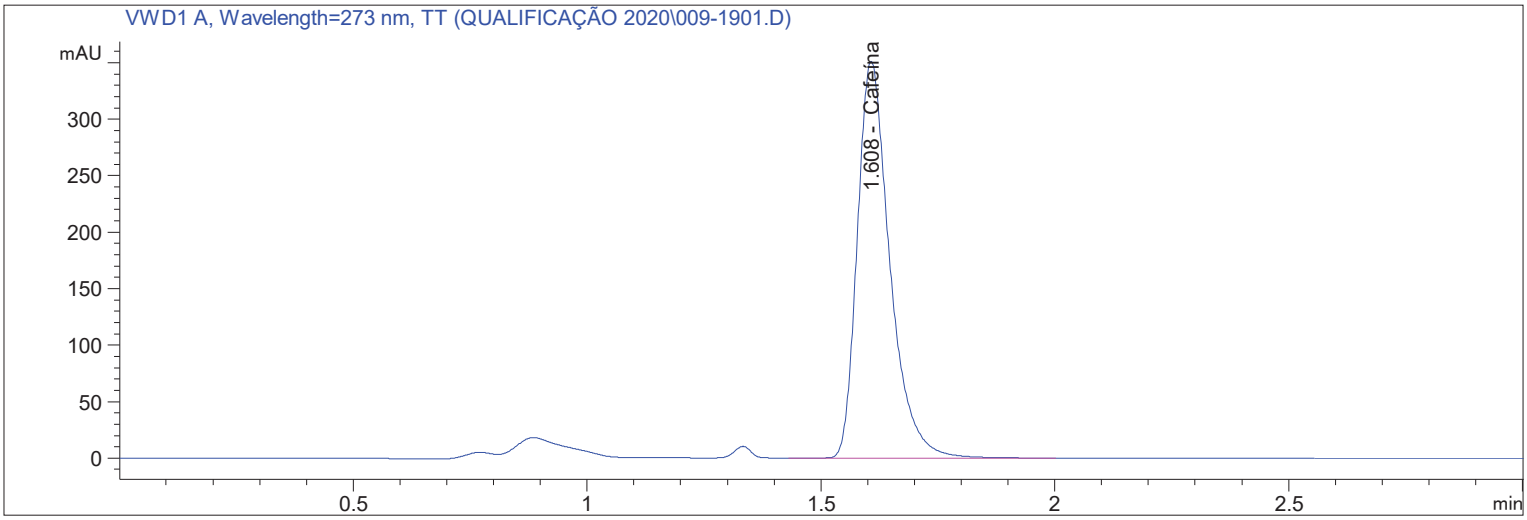

==========

External Standard Report

==========

Sorted By : Signal
Calib. Data Modified : Wednesday, October 28, 2020 12:16:24 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=273 nm, TT

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.608	BBA	1697.09558	1.17624e-3	1.99620		Cafeína

Totals : 1.99620


==========

*** End of Report ***

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\GRADAB000003.D
Sample Name: GRAD AB

==========

Acq. Operator : Rodolfo (QPack)
Acq. Instrument : HPLC Location : Vial 2
Injection Date : 10/28/2020 2:10:42 PM
Inj Volume : 0.000 µl
Acq. Method : C:\CHEM32\2\METHODS\GRAD AB.M
Last changed : 10/28/2020 2:08:53 PM by Rodolfo (QPack)
(modified after loading)
Analysis Method : C:\CHEM32\2\METHODS\GRAD AB.M
Last changed : 1/17/2019 3:43:07 PM by Rodolfo (QPack)
Additional Info : Peak(s) manually integrated

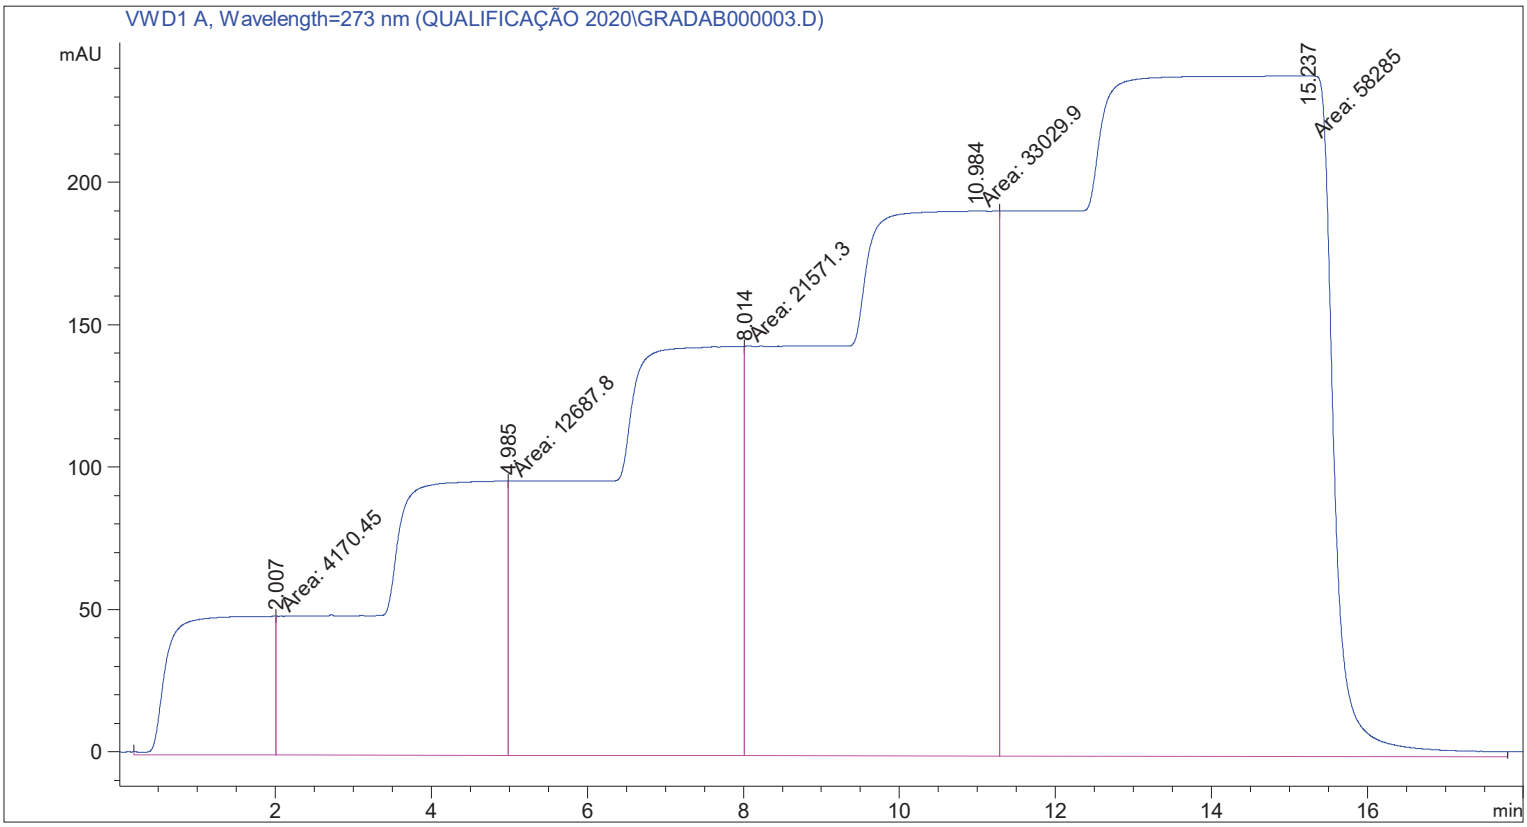

==========

External Standard Report

==========

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

==========

==========

Area Percent Report

==========

Sorted By : Signal
Multiplier: : 1.0000
Dilution: : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Data File C:\CHEM32\2\DATA\QUALIFICAÇÃO 2020\GRADAB000003.D
Sample Name: GRAD AB

Signal 1: VWD1 A, Wavelength=273 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.007	MF	1.4270	4170.44971	48.71007	3.2144
2	4.985	FM	2.1963	1.26878e4	96.27975	9.7790
3	8.014	FM	2.5009	2.15713e4	143.75421	16.6260
4	10.984	FM	2.8758	3.30299e4	191.42549	25.4577
5	15.237	FM	4.0649	5.82850e4	238.97389	44.9229
Totals :				1.29744e5	719.14341	

*** End of Report ***