
Peak Find - Exatidão Do Comprimento De Onda.jws

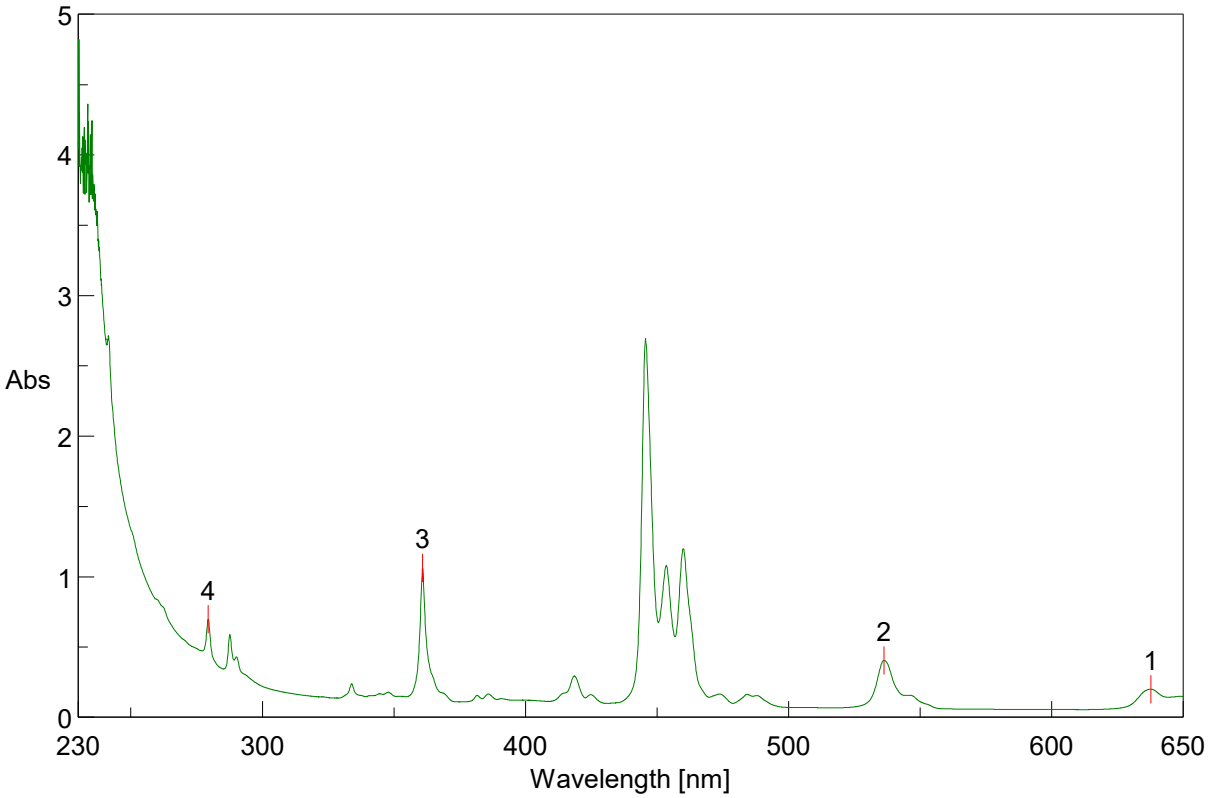

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 14:07
Date modified	06/06/2024 14:10
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 14:04
Parameter file	C:\Jasco\2024\Exatidão Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	637.7	0.198883	2	536.3	0.403621
3	360.9	1.05956	4	279.4	0.697085

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 1.jws

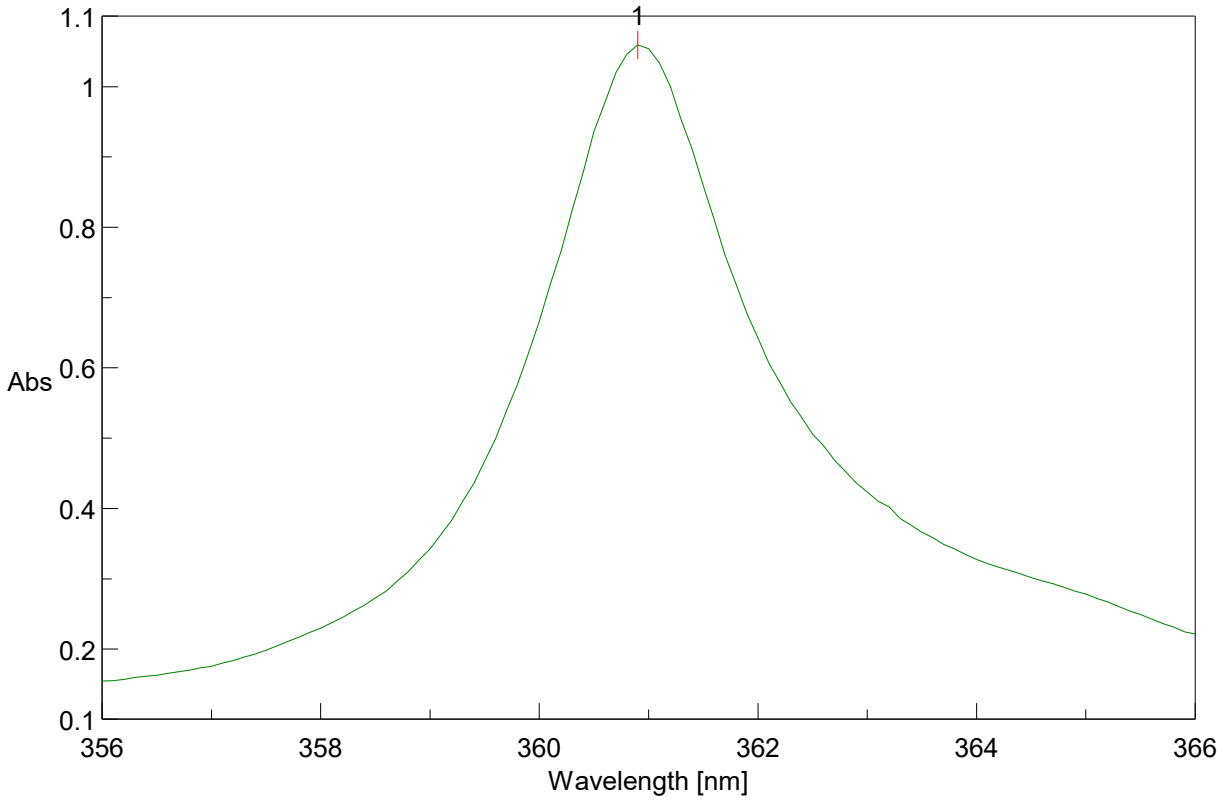

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 14:17
Date modified	06/06/2024 14:18
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 14:15
Parameter file	C:\Jasco\2024\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1


Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	1.05888			

Creation QPackSA
Review
Approval

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 2.jws

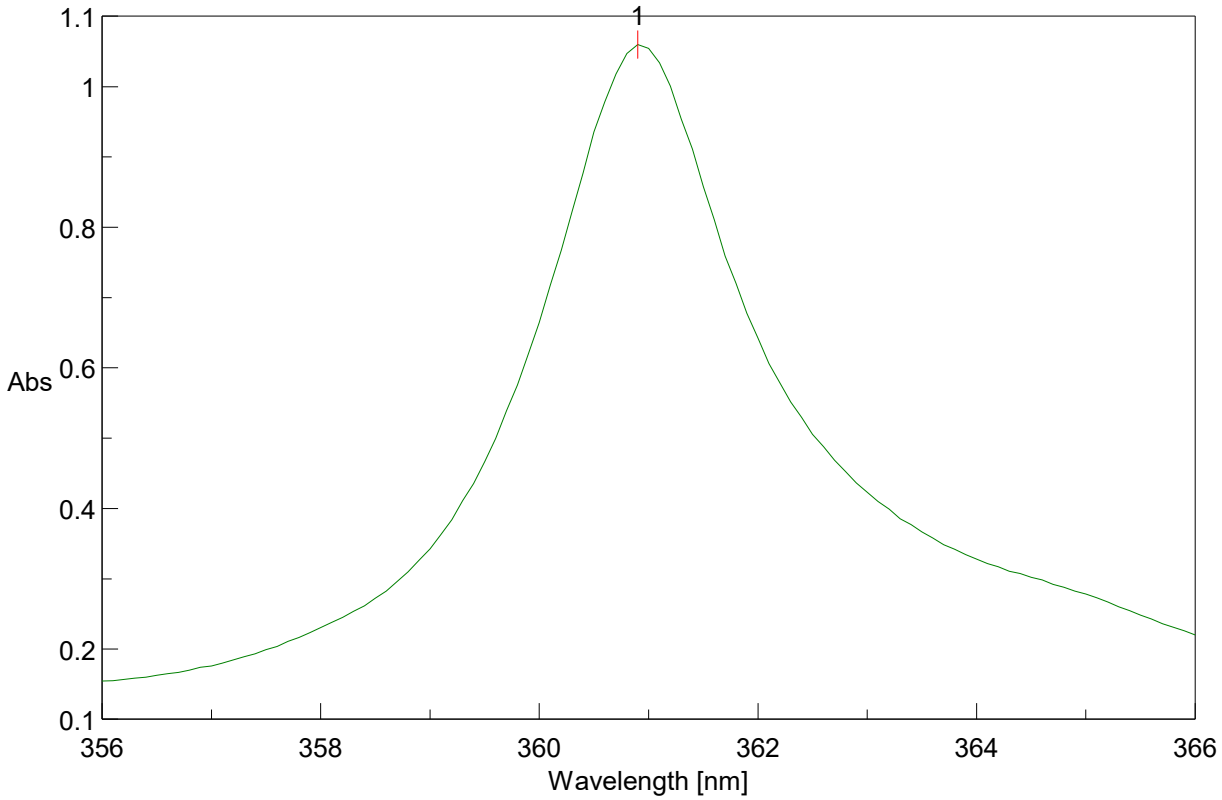

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 14:17
Date modified	06/06/2024 14:18
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 14:16
Parameter file	C:\Jasco\2024\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1


Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	1.05942			

Creation QPackSA
Review
Approval

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 3.jws

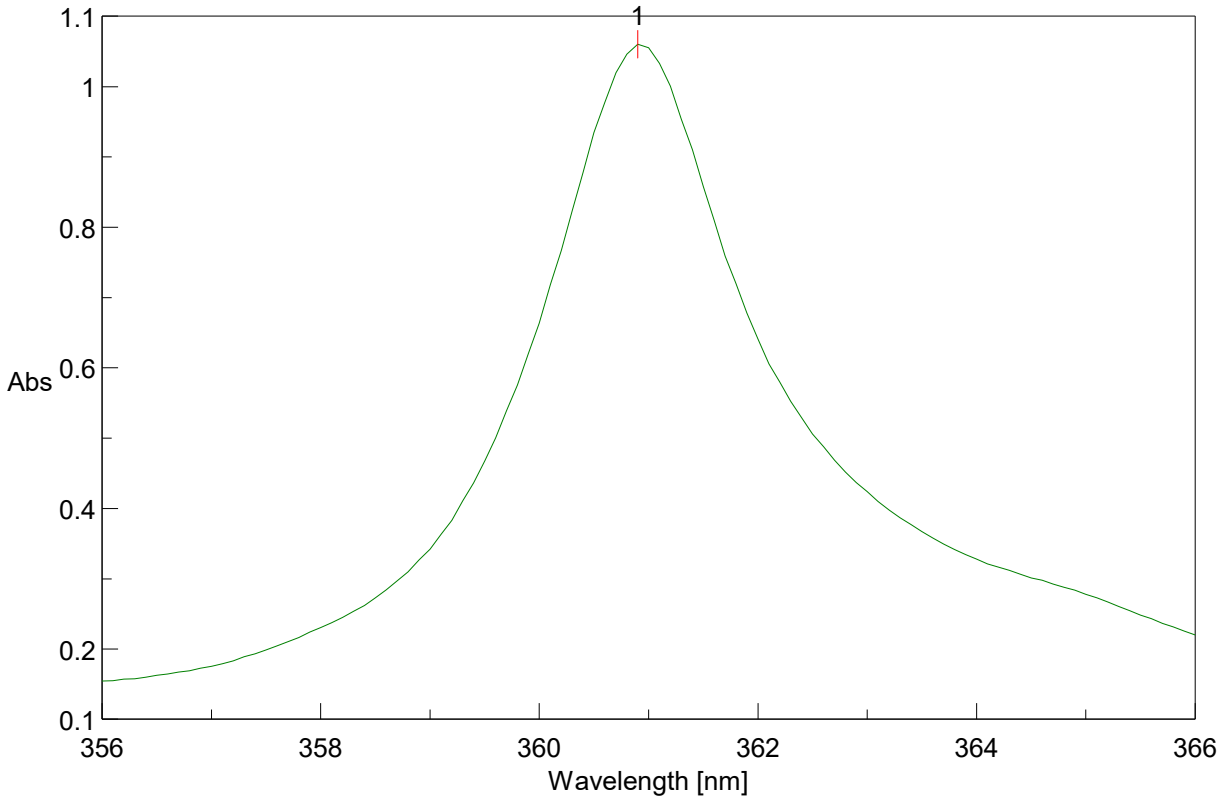

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 14:18
Date modified	06/06/2024 14:18
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 14:17
Parameter file	C:\Jasco\2024\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI
Filter exchange	Step
Correction	None
No. of cycles	1

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.9	1.05999			

Full Width at Half Maximum - Resolução.jws

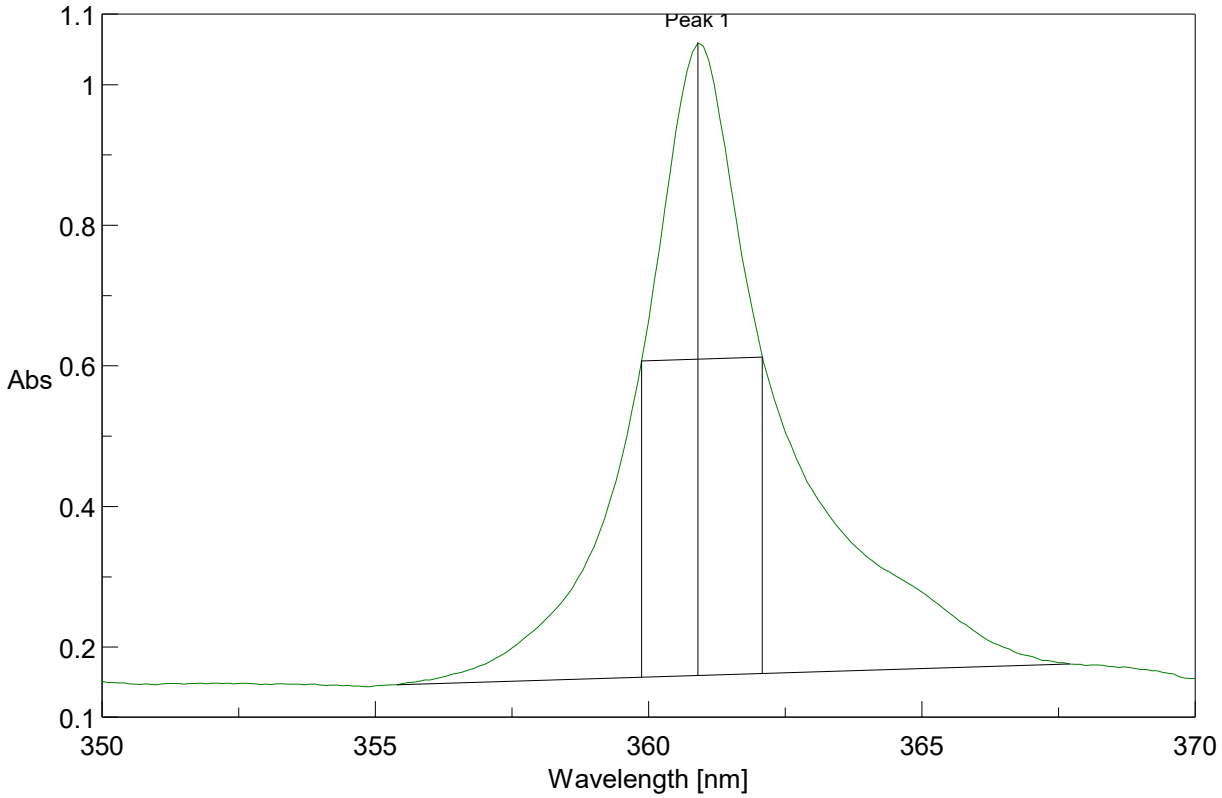

[Result of FWHM Calculation]

Base 1	Base 2	Peak	Height	FWHM
355.4	367.7	360.9	0.89969	2.21115

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 14:21
Date modified	06/06/2024 14:21
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	370 nm
End	350 nm
Data interval	0.1 nm
Data points	201

[Measurement Information]

Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 14:21
Parameter file	C:\Jasco\2024\Resolução.uvsp
Photometric mode	Abs
Measurement range	370 - 350 nm
Data interval	0.1 nm
Bandwidth	1.0 nm
Response	0.06 sec
Scan mode	Continuous
Scan speed	40 nm/min
Change source at	340 nm
Light source	D2/WI

Creation	QPackSA
Review	
Approval	

Exatidão Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	06/06/2024 14:27
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2024\Exatidão Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Sample-1	G1	G1	0.3306
Sample-2	G2	G2	1.0725
Sample-3	G3	G3	0.5066

Creation	QPackSA
Review	
Approval	

Repetibilidade Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	06/06/2024 14:31
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2024\Repetibilidade Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	361.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	361.0 nm
Sample-1	Rep. 1	Rep. 1	1.0179
Sample-2	Rep. 2	Rep. 2	1.0176
Sample-3	Rep. 3	Rep. 3	1.0179

Creation	QPackSA
Review	
Approval	


Linearidade Fotométrica.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	06/06/2024 14:39
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2024\Linearidade Fotométrica.uvfw
Photometric mode	Abs
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	440.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	440.0 nm
Sample-1	G1	G1	0.3306
Sample-2	G2	G2	1.0724
Sample-3	G3	G3	0.5062
Sample-4	G1 + G3	G1 + G3	0.8375
Sample-5	G2 + G3	G2 + G3	1.5809

Creation	QPackSA
Review	
Approval	

Peak Find - Estabilidade Da Linha De Base.jws

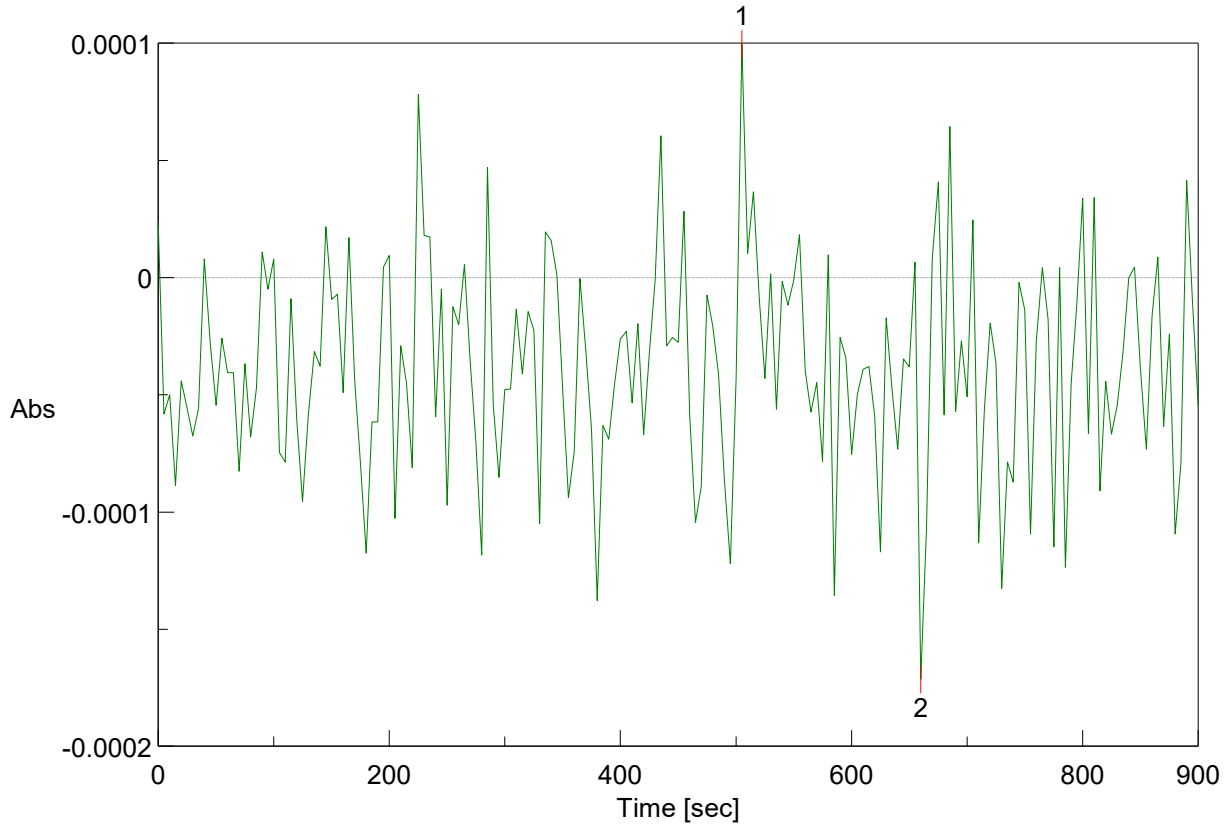

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Jasco
Division	Assistência Técnica
Company	VicPharma

[Detailed Information]

Creation date	06/06/2024 15:07
Date modified	06/06/2024 15:07
Data array type	Linear data array
Horizontal axis	Time [sec]
Vertical axis	Abs
Start	0 sec
End	900 sec
Data interval	5 sec
Data points	181

[Measurement Information]


Instrument name	V-730
Model name	V-730
Serial No.	D334661798
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Measurement date	06/06/2024 15:01
Parameter file	C:\Jasco\2024\Estabilidade Da Linha De Base.uvtm
Photometric mode	Abs
Measurement range	0 - 900 sec
Data interval	5 sec
UV/Vis bandwidth	1.0 nm
Response	0.96 sec
Monitor wavelength	250 nm
Change source at	340 nm
Light source	D2/WI
Correction	Blank

Creation	QPackSA
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	505	9.9403E-005	2	660	-0.000171429

Peak Find - Uniformidade Da Linha De Base.jws

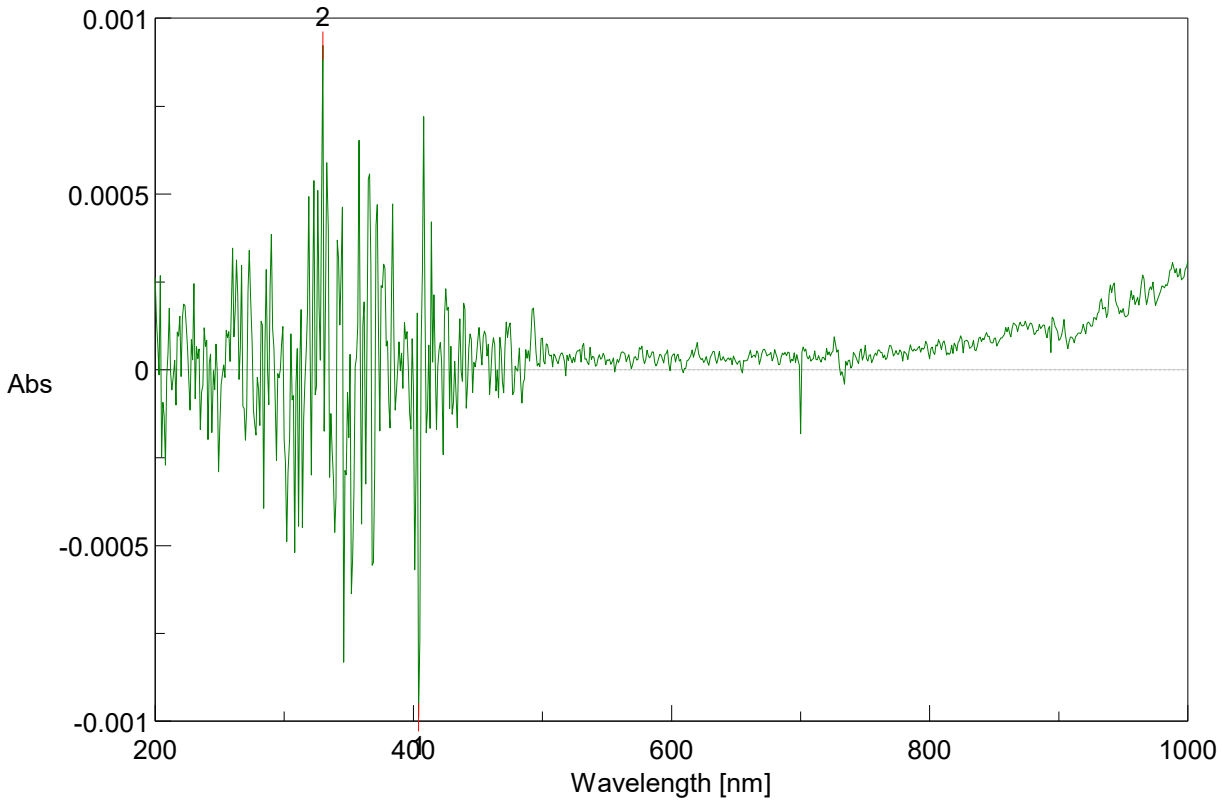

[Comments]
Sample name
Comment
User QPackSA
Workgroup Jasco
Division Assistência Técnica
Company VicPharma

[Detailed Information]
Creation date 06/06/2024 15:16
Date modified 06/06/2024 15:16

Data array type Linear data array
Horizontal axis Wavelength [nm]
Vertical axis Abs
Start 1000 nm
End 200 nm
Data interval 1 nm
Data points 801

[Measurement Information]
Instrument name V-730
Model name V-730
Serial No. D334661798

Accessory USE-753
Accessory S/N D334661798
Cell
Ref. beam

Measurement date 06/06/2024 15:15

Parameter file C:\Jasco\2024\Uniformidade Da Linha De Base.uvsp
Photometric mode Abs
Measurement range 1000 - 200 nm
Data interval 1 nm
Bandwidth 1.0 nm
Response 0.24 sec
Scan mode Continuous
Scan speed 400 nm/min
Change source at 340 nm
Light source D2/WI
Filter exchange Step
Correction Baseline
No. of cycles 1

Creation QPackSA
Review
Approval

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	404	-0.000988832	2	330	0.000921975

Stray Light.ufwd

Sample name	
Comment	
User	QPackSA
Division	Assistência Técnica
Company	VicPharma
Creation date	06/06/2024 15:36
Instrument name	V-730
Model name	V-730
Serial No.	D334661798
ROM version	1.02.01
Accessory	USE-753
Accessory S/N	D334661798
Cell	
Ref. beam	
Parameter file	C:\Jasco\2024\Stray Light.uvfw
Photometric mode	%T
Bandwidth	1.0 nm
Response	0.24 sec
Wavelength-1	430.0 nm
Wavelength-2	380.0 nm
Change source at	340 nm
Light source	D2/WI
Dark correction	Off
Blank correction	Off
No. of cycles	1

Mode	Sample Name	Comment	430.0 nm	380.0 nm
Sample-1	Stray Light	Stray Light	99.5342	0.0139

Creation	QPackSA
Review	
Approval	