

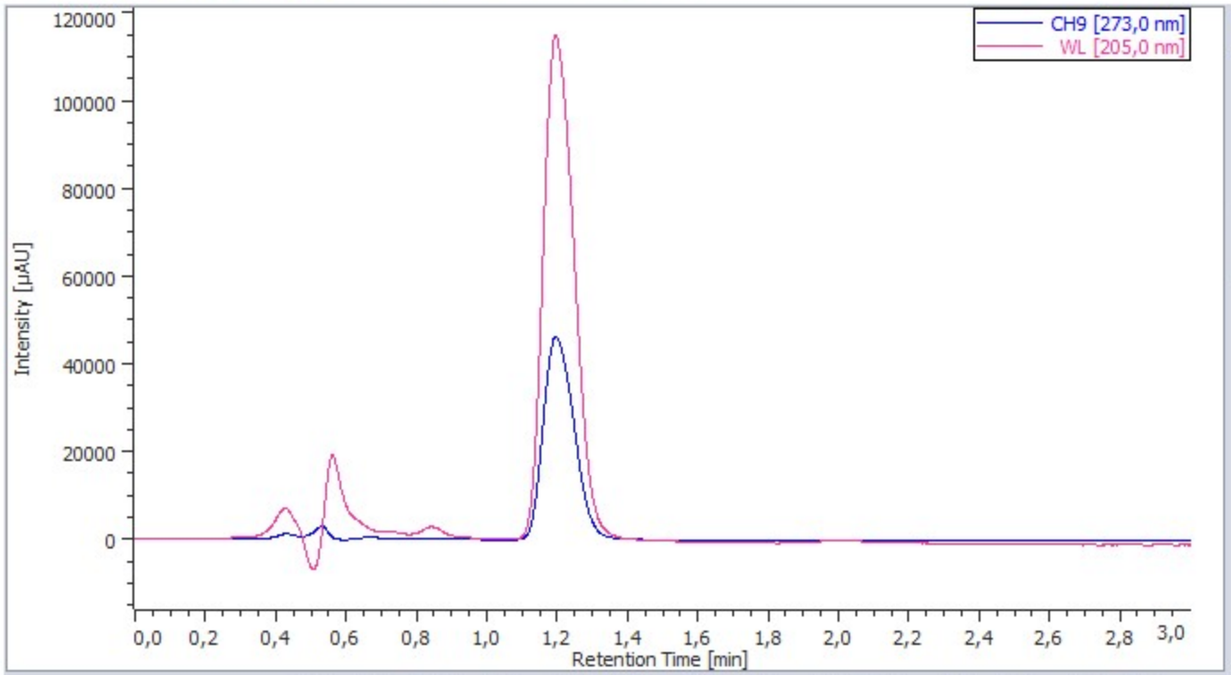



PDA Data Information

General	
Wavelength Range	200,0 -- 300,0 nm
Wavelength Interval	1,0 nm
Sampling Interval	0,100 second
Autozero Time	---
Virtual Channel #9	
Wavelength	273,0 nm

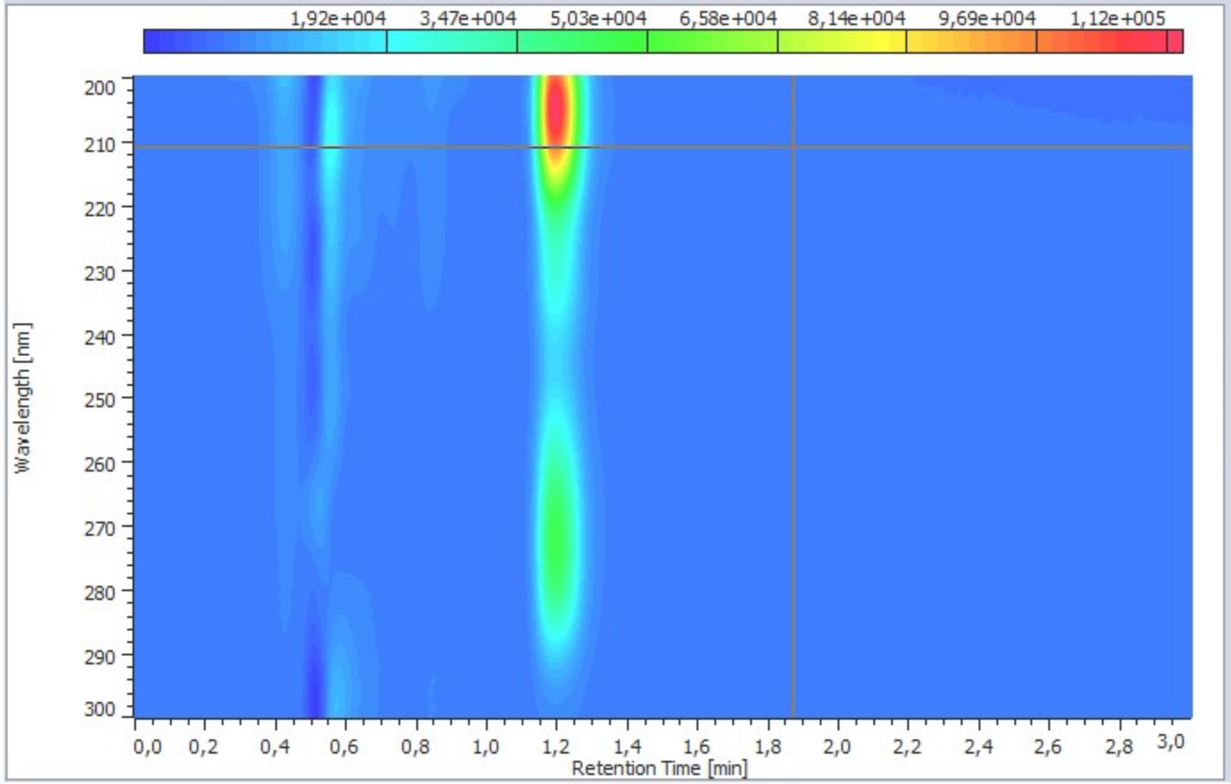

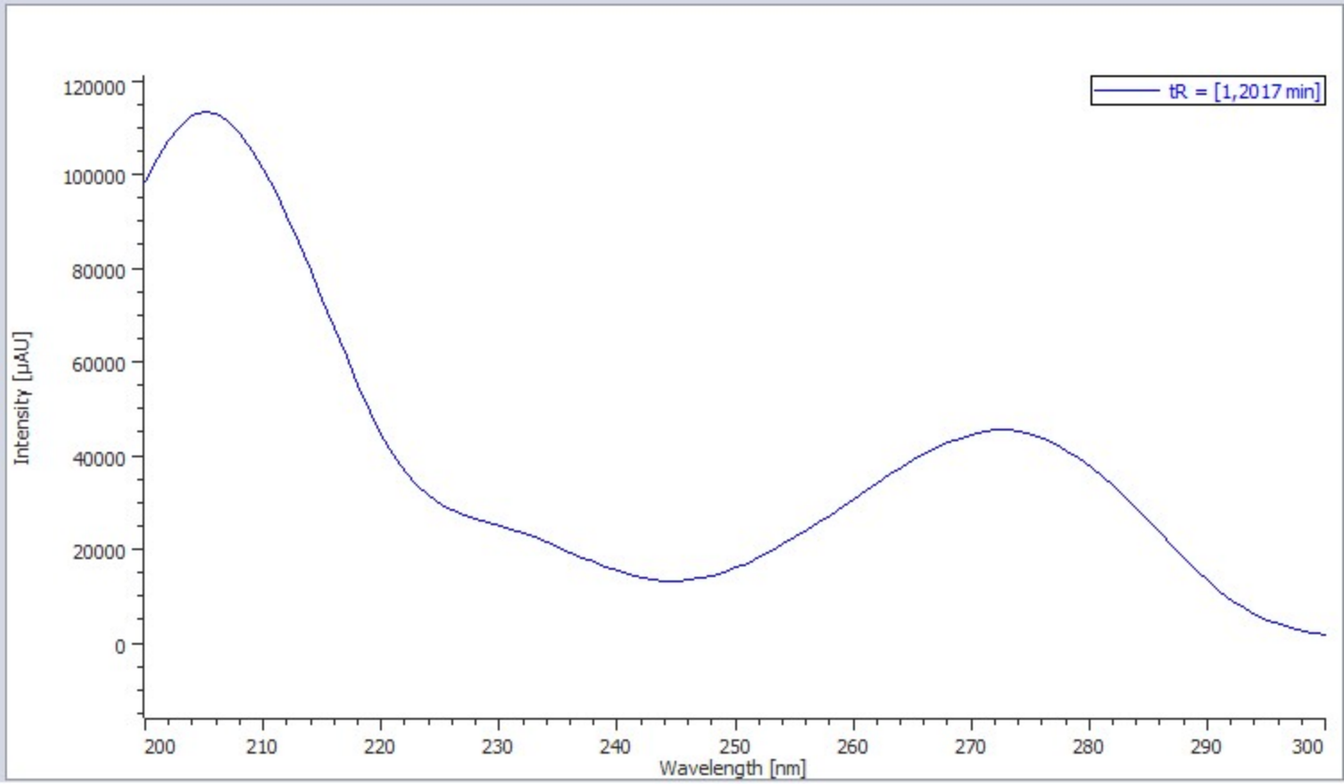

Chromatogram

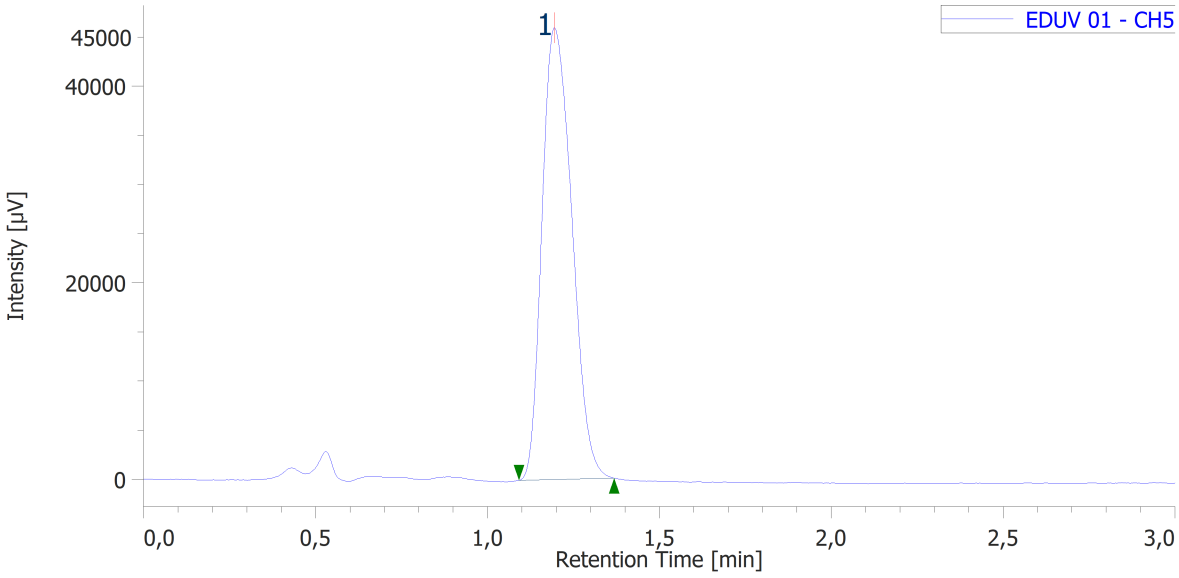

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:18
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 11:50:13
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	EDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,195	277475	45933	100,000	100,000	N/A	840	N/A	1,263	

Creator QPackSA
Reviewer
Approver

Chromatogram

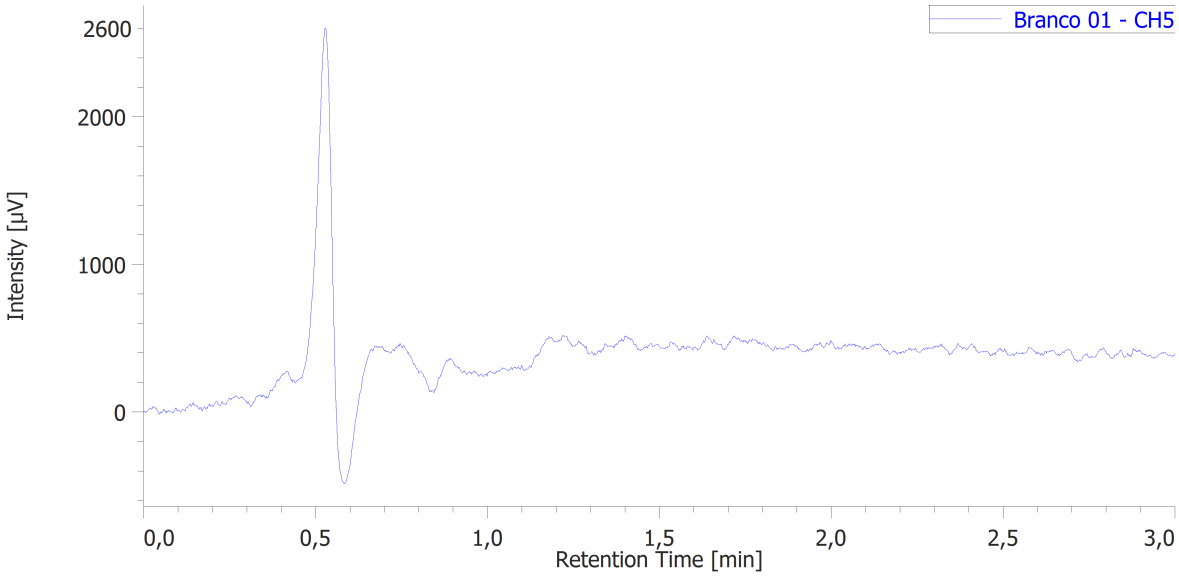


Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 11:54:01
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

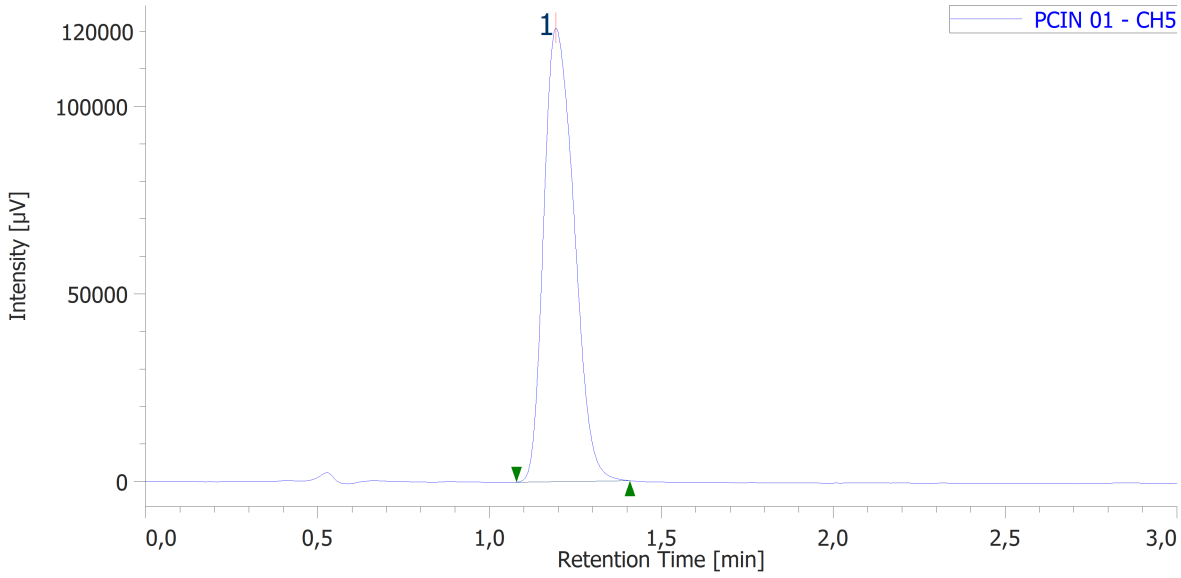

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 11:57:49
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,193	741269	120889	100,000	100,000	N/A	814	N/A	1,298	

Creator QPackSA
Reviewer
Approver

Chromatogram

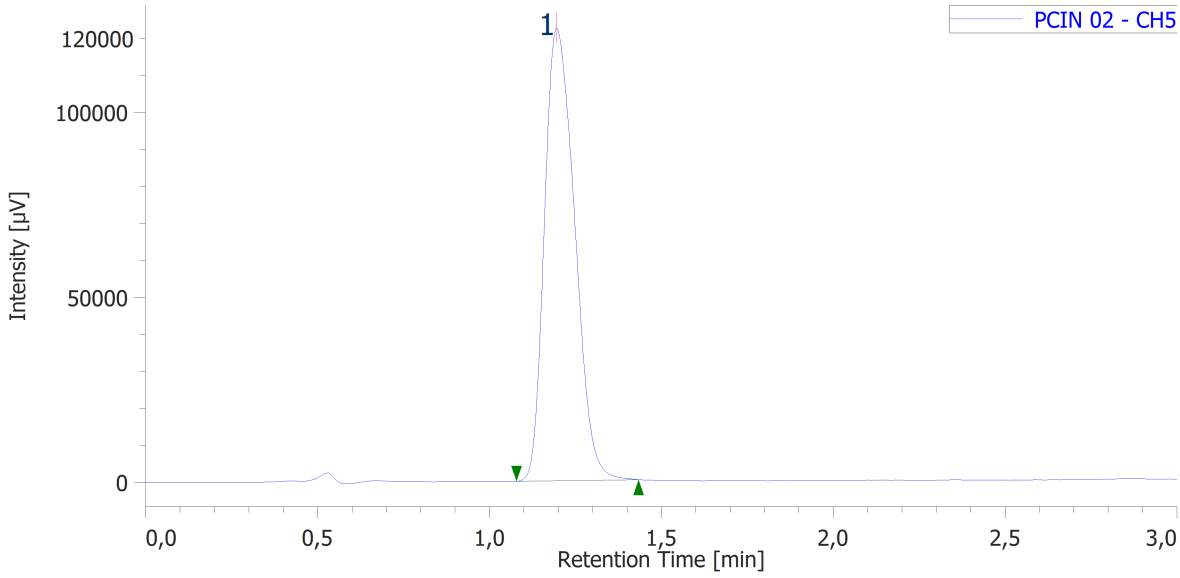

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:01:38
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,195	747066	122300	100,000	100,000	N/A	827	N/A	1,307	

Creator QPackSA
Reviewer
Approver

Chromatogram

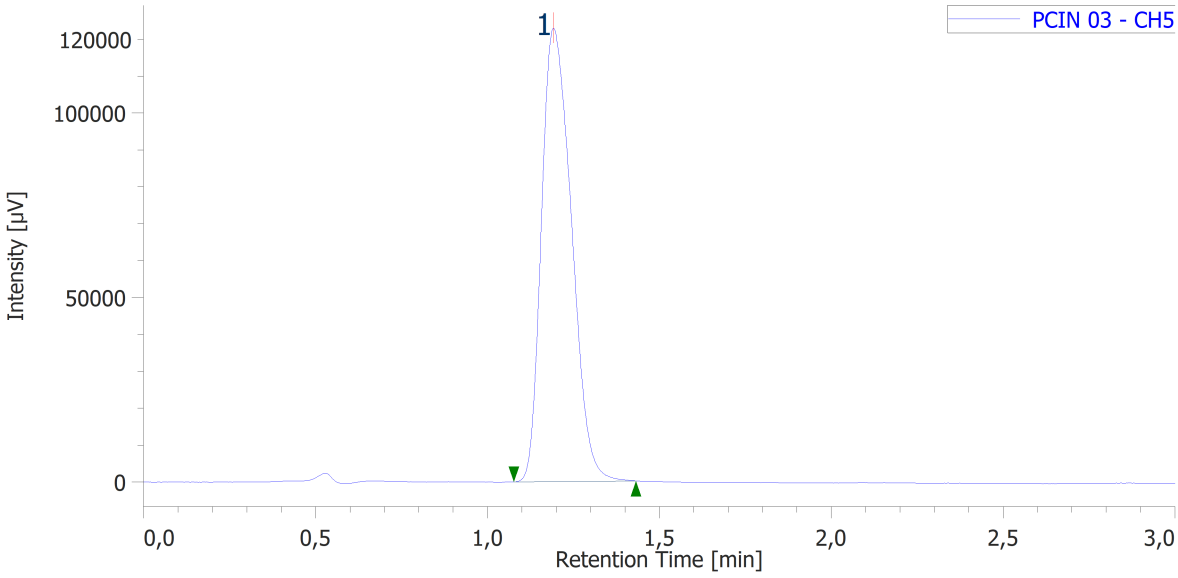

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:05:26
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	745793	122889	100,000	100,000	N/A	833	N/A	1,313	

Creator QPackSA
Reviewer
Approver

Chromatogram

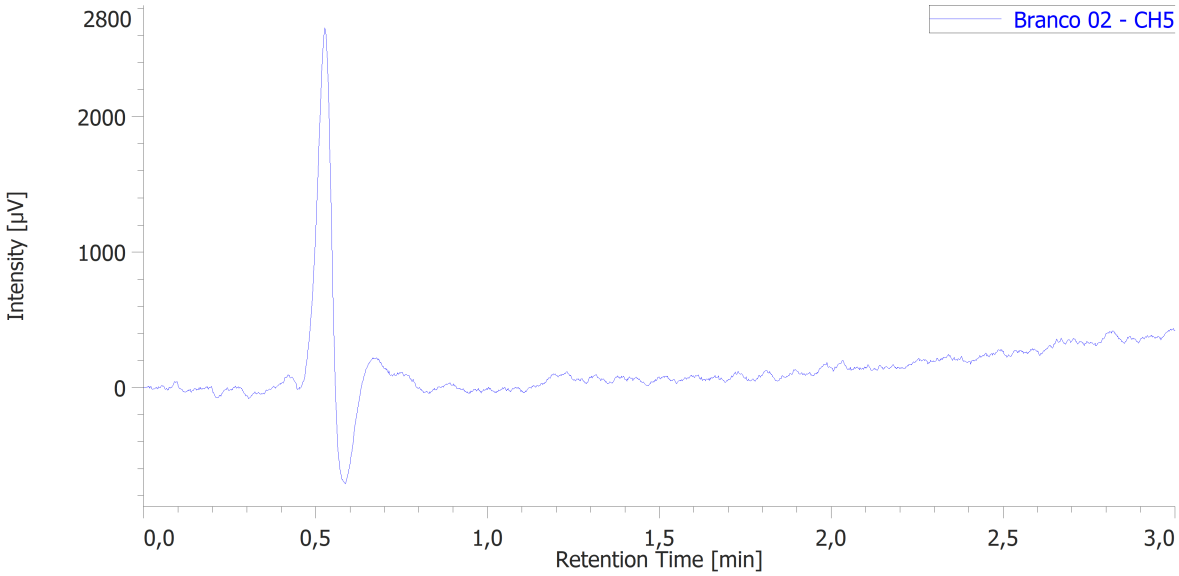


Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:09:14
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

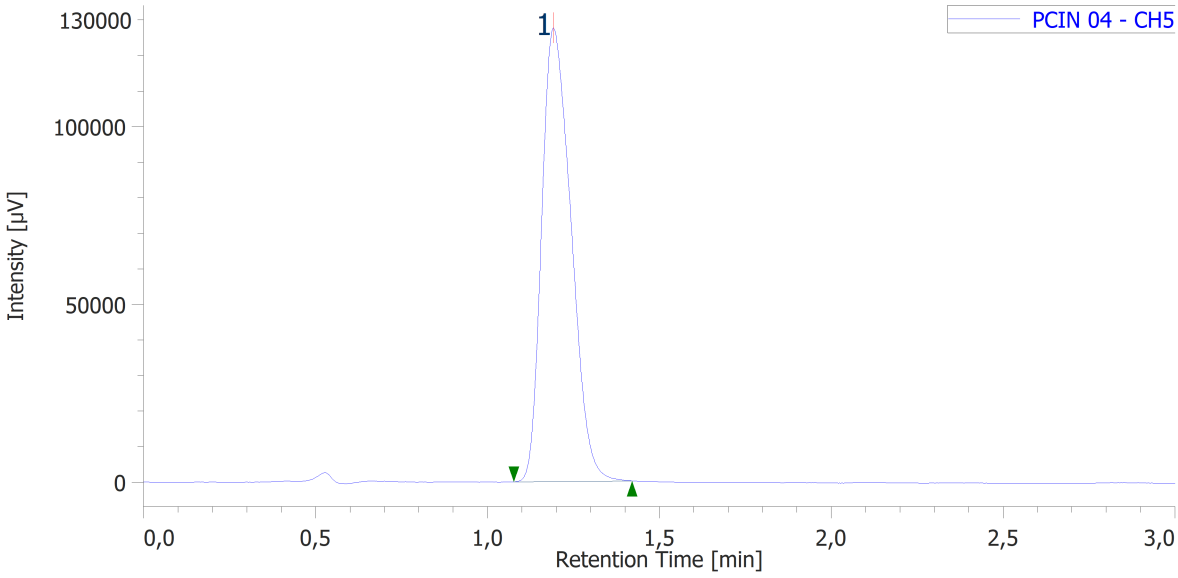

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:13:02
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	758150	127532	100,000	100,000	N/A	870	N/A	1,319	

Creator QPackSA
Reviewer
Approver

Chromatogram

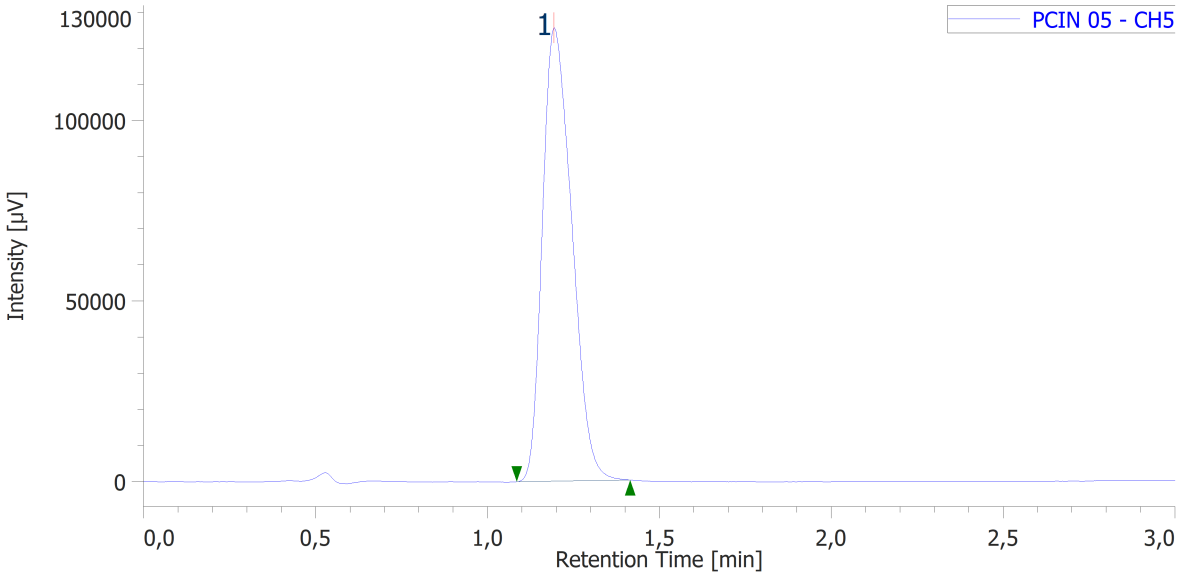

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:16:50
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,193	745686	125400	100,000	100,000	N/A	874	N/A	1,330	

Creator QPackSA
Reviewer
Approver

Chromatogram

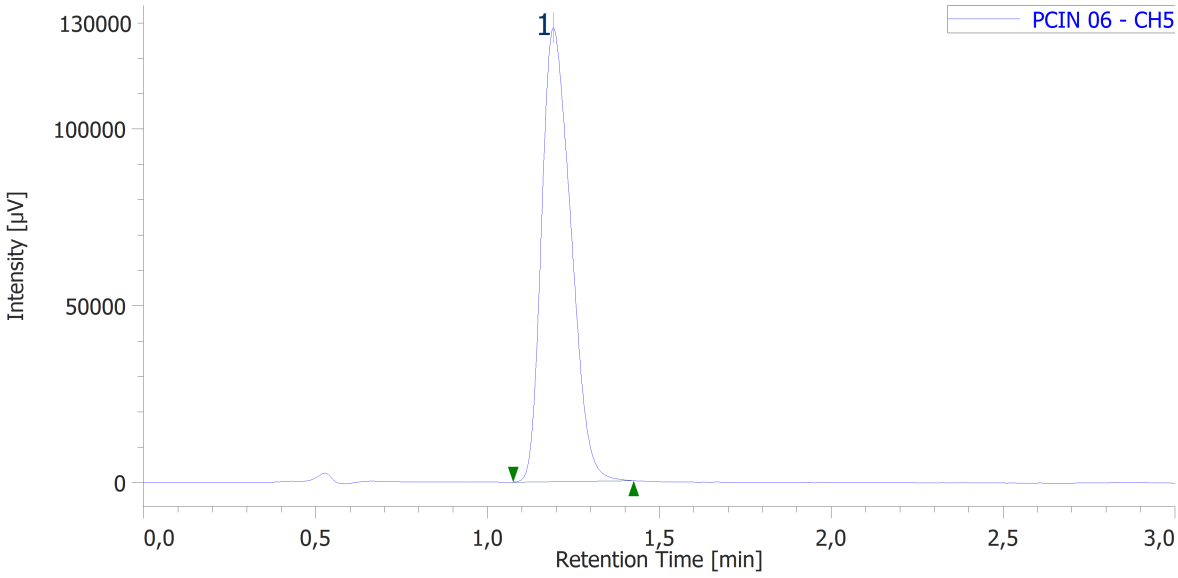

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:20:39
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	758709	128318	100,000	100,000	N/A	884	N/A	1,316	

Creator QPackSA
Reviewer
Approver

Chromatogram

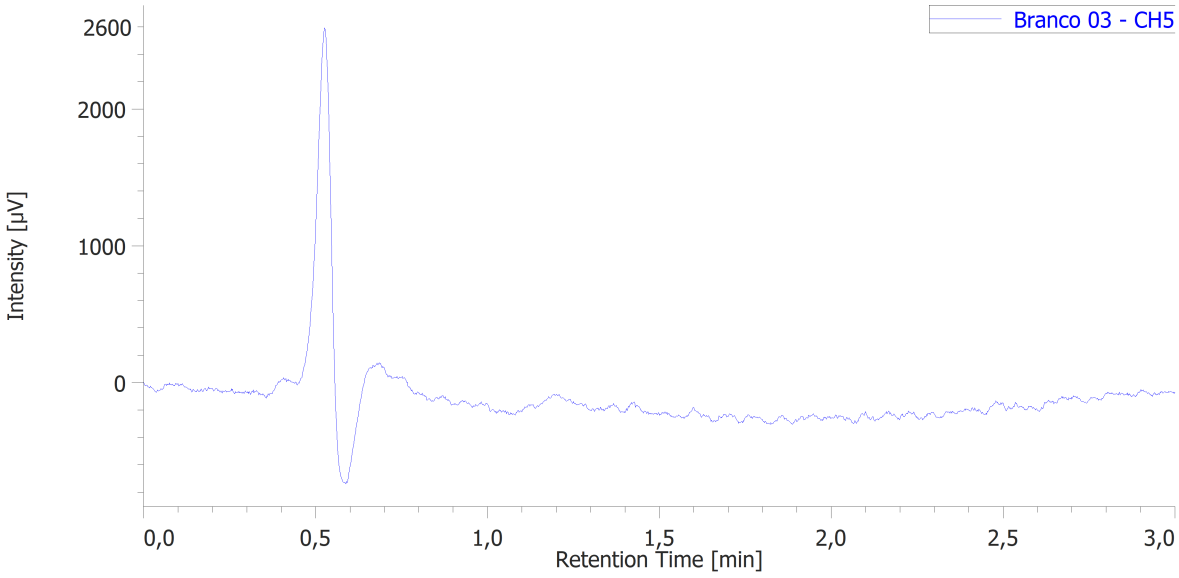


Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:24:27
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

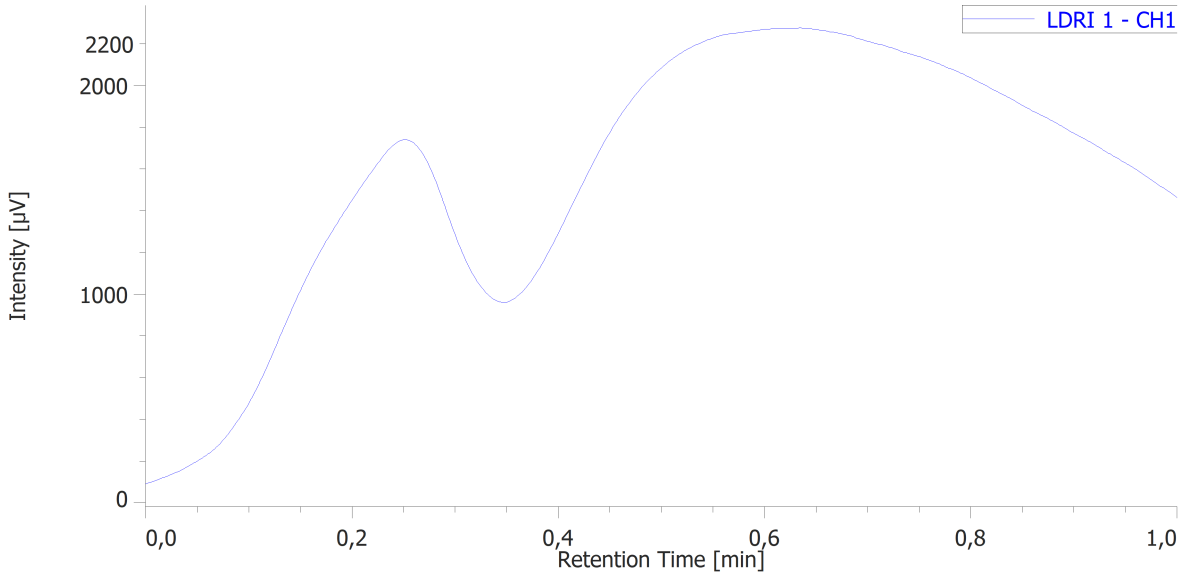


Chromatogram Information	
User Name	QPackSA
Date Modified	10/06/2024 14:10:23
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 16:57:06
Volume	2,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	LDIR
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR (Manual)

Creator QPackSA
Reviewer
Approver

Chromatogram

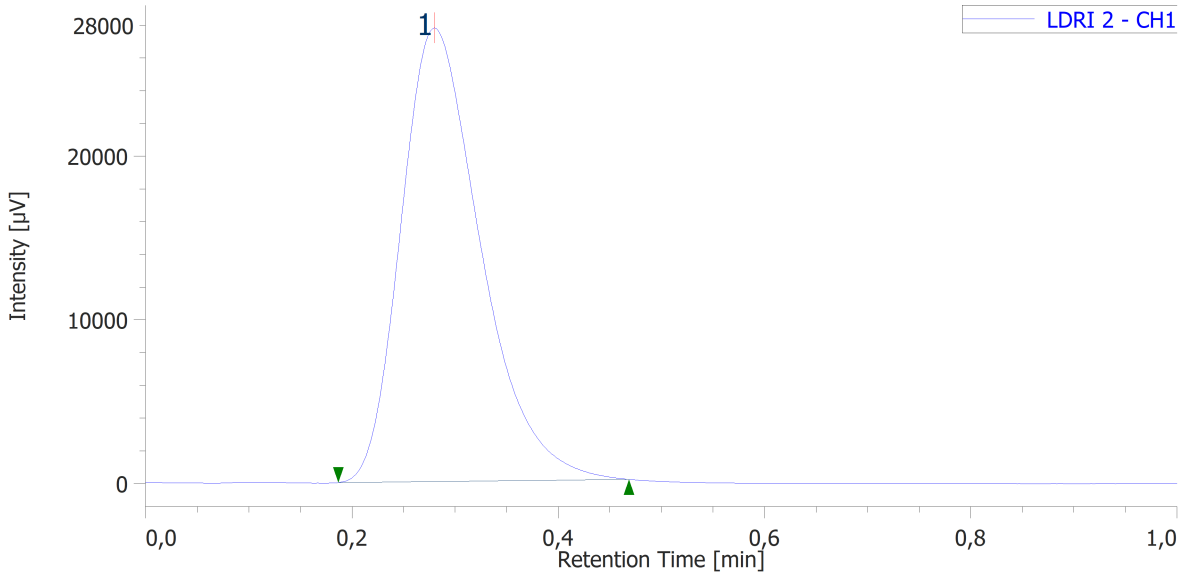

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 17:13:47
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 17:00:20
Volume	2,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	LDIR
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0,280	148897	27694	100,000	100,000	N/A	65	N/A	1,368	

Creator QPackSA
Reviewer
Approver

Chromatogram

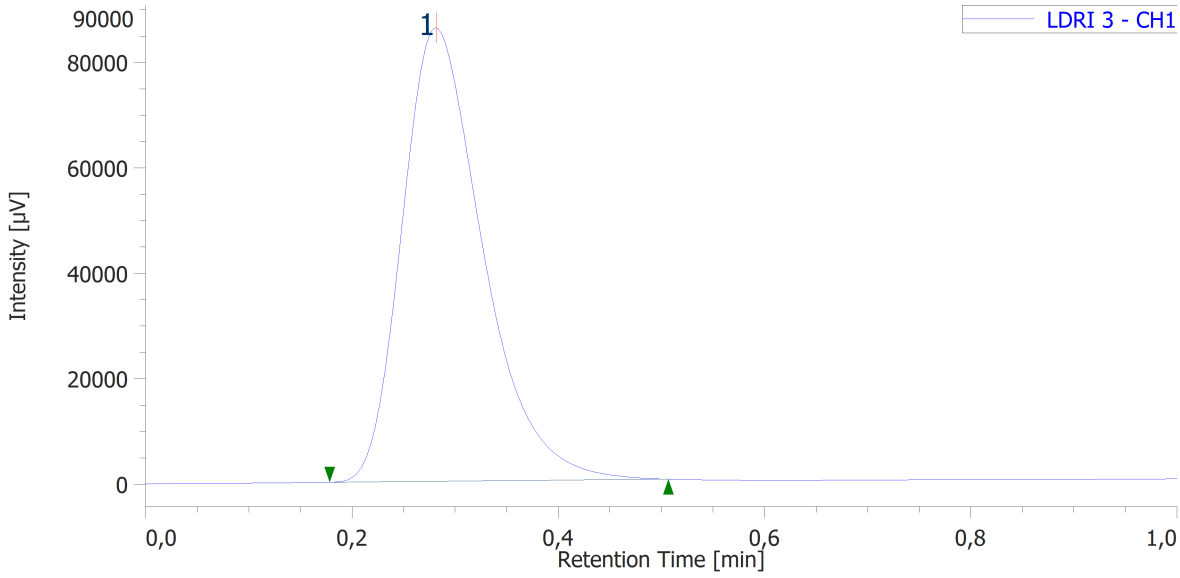

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 17:13:47
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 17:03:35
Volume	2,0 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	LDIR
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0,282	467816	85947	100,000	100,000	N/A	64	N/A	1,374	

Creator QPackSA
Reviewer
Approver

Chromatogram

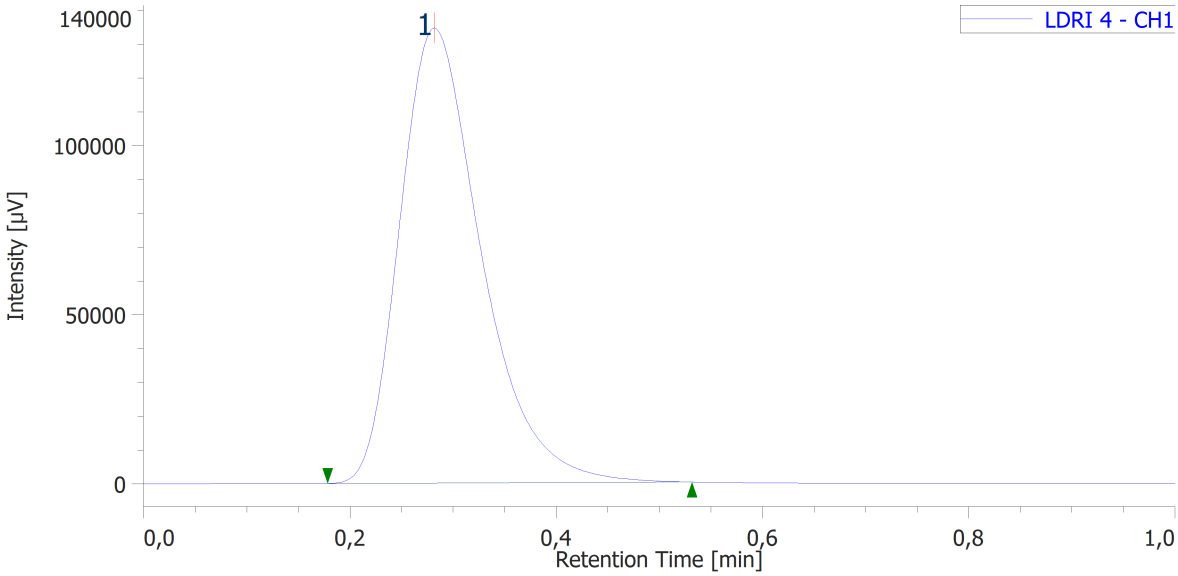

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 17:13:47
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 17:06:51
Volume	2,0 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	LDIR
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0,282	739082	134432	100,000	100,000	N/A	64	N/A	1,382	

Creator QPackSA
Reviewer
Approver

Chromatogram

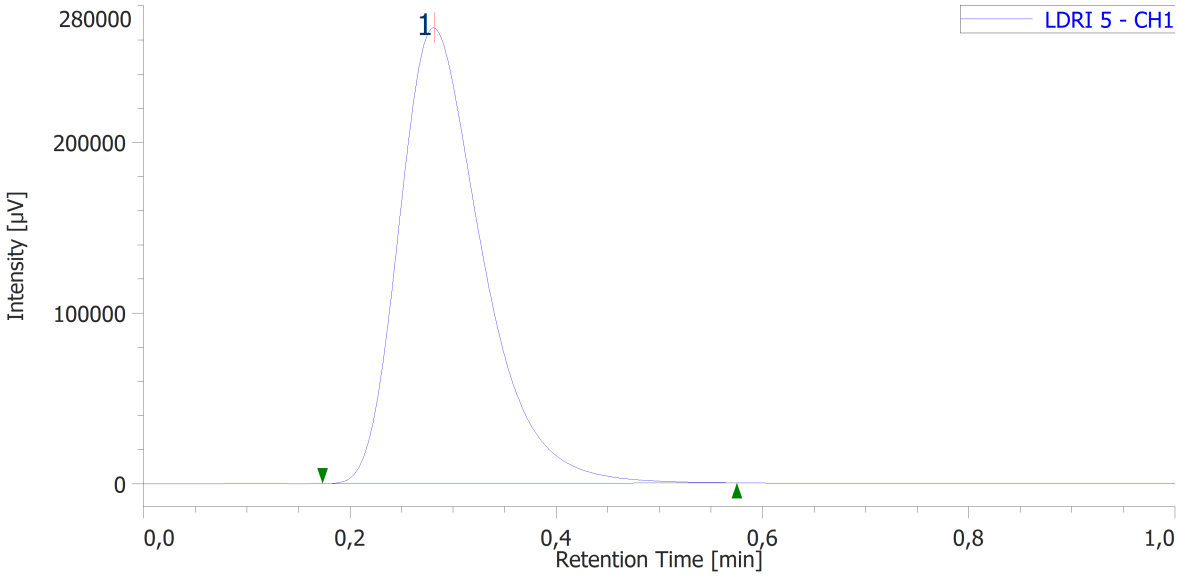

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 17:13:47
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 17:10:06
Volume	2,0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	1,0 [min]
Acquisition Sequence	LDRI
Control Method	Qualificação RI
Peak ID Table	LDIR
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	LDIR

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	1	0,282	1491943	266666	100,000	100,000	N/A	62	N/A	1,390	

Creator QPackSA
Reviewer
Approver

Chromatogram

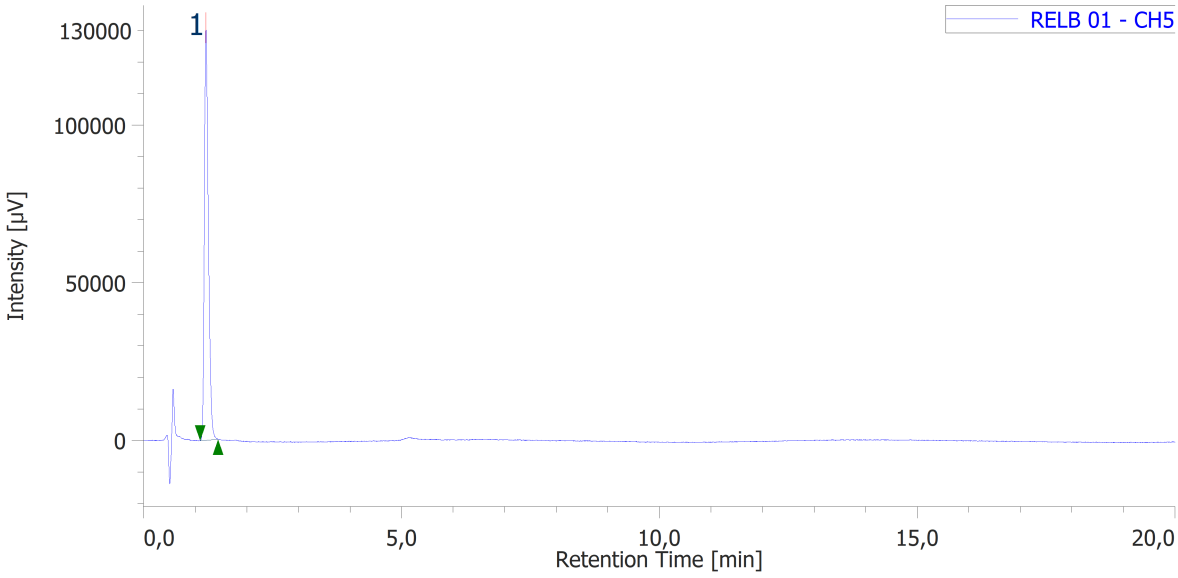

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:47:22
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,207	709716	130674	100,000	100,000	N/A	1195	N/A	1,393	

Creator QPackSA
Reviewer
Approver

Chromatogram

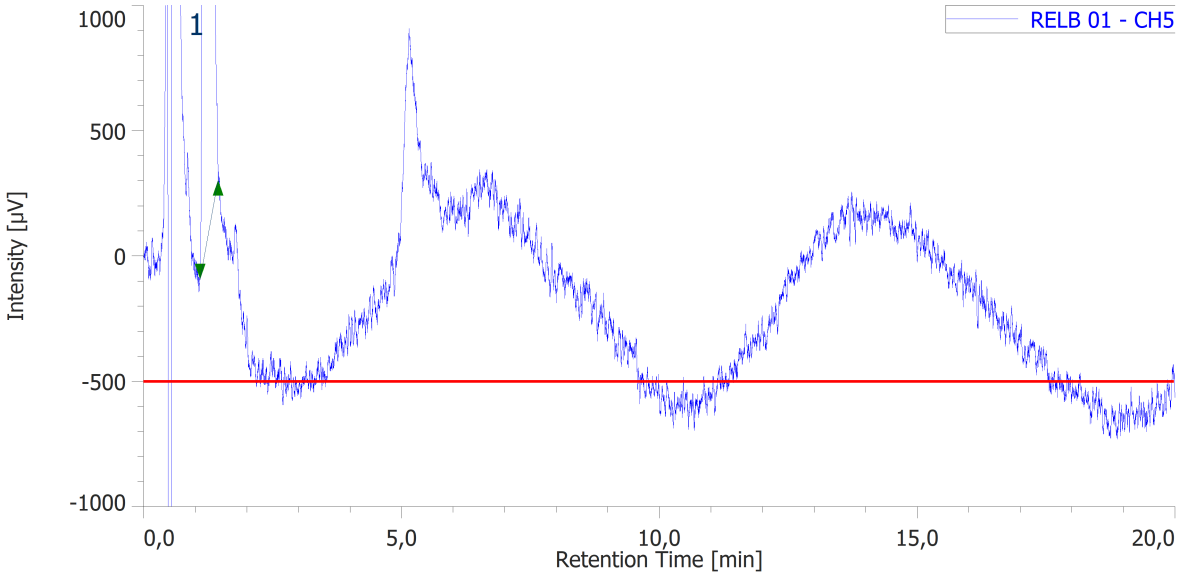

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:47:22
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,207	709716	130674	100,000	100,000	N/A	1195	N/A	1,393	

Creator QPackSA
Reviewer
Approver

Chromatogram

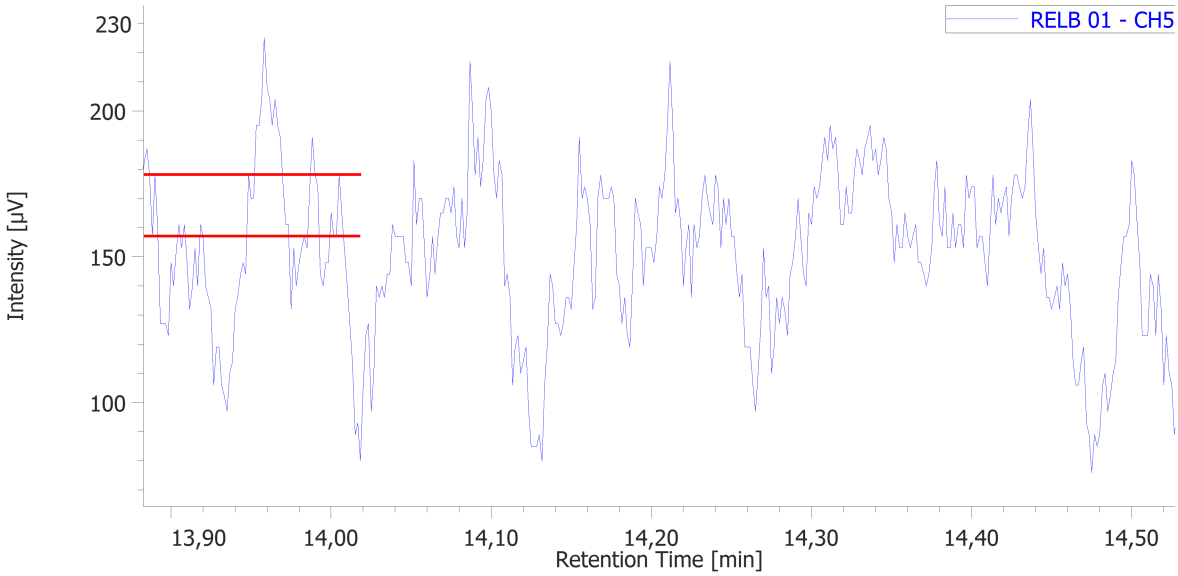

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:47:22
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	RELB 01-CH5
Sample Name	
Channel Name	250,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,207	709716	130674	100,000	100,000	N/A	1195	N/A	1,393	

Creator QPackSA
Reviewer
Approver

Chromatogram

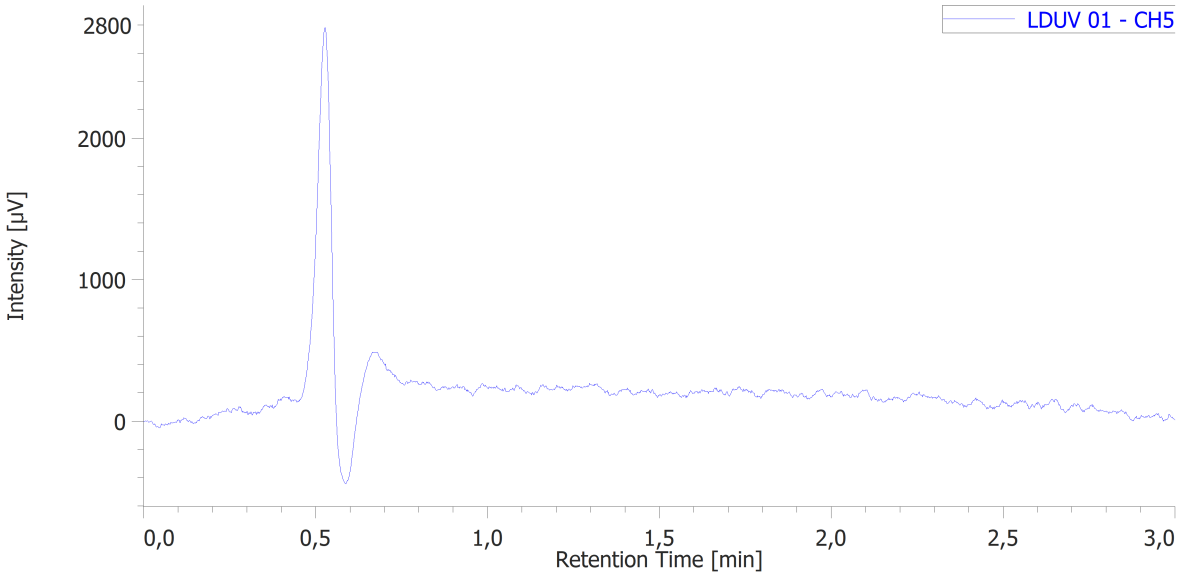


Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:28:15
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

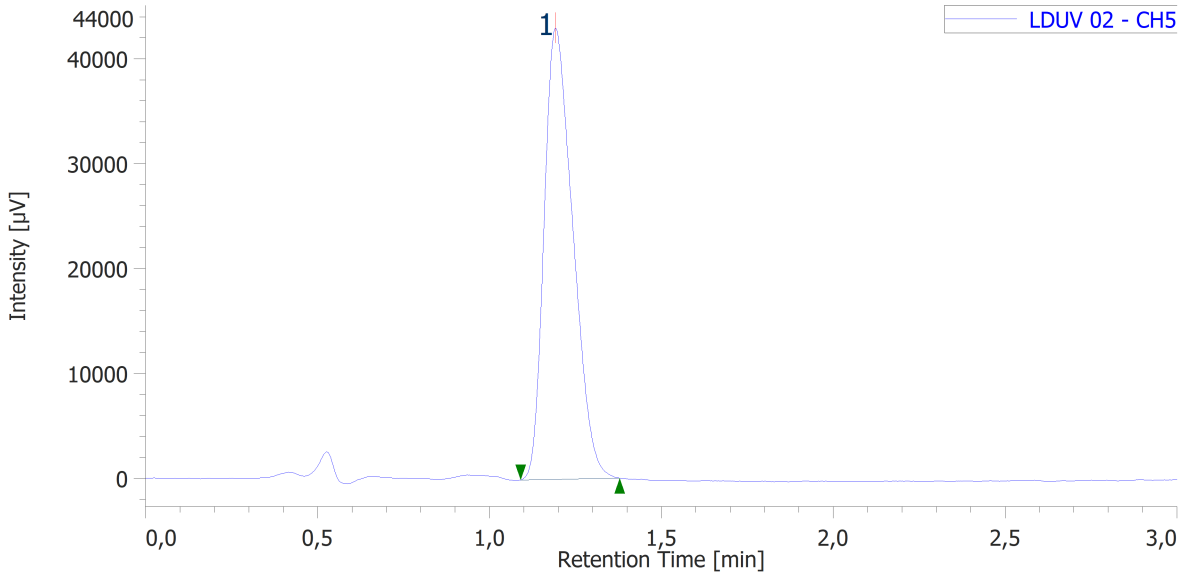

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:32:03
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	250403	43033	100,000	100,000	N/A	925	N/A	1,356	

Creator QPackSA
Reviewer
Approver

Chromatogram

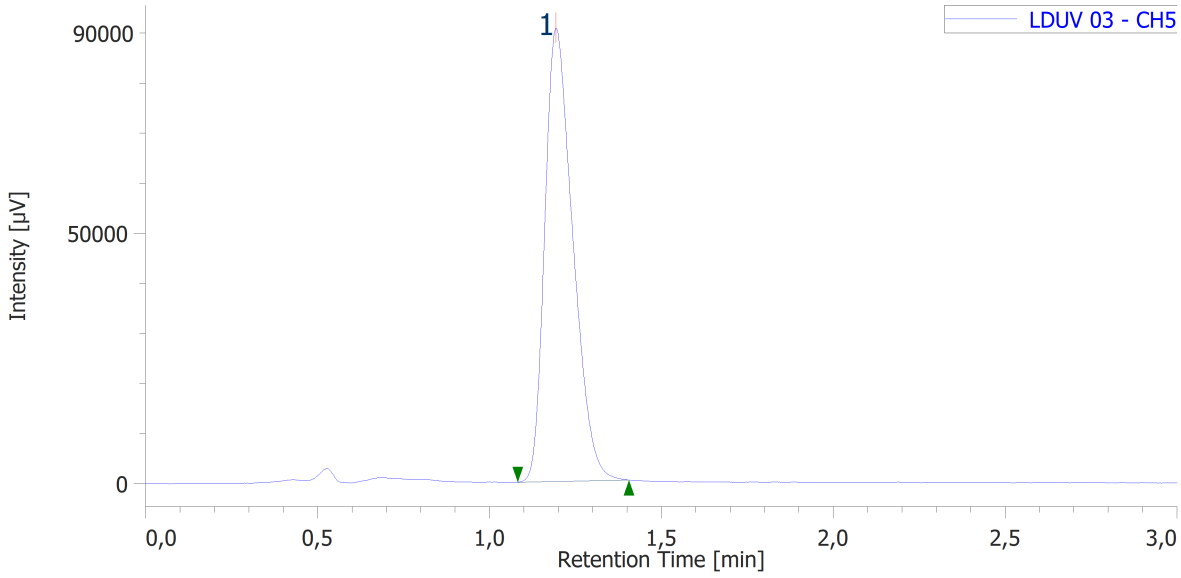

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:35:52
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,193	514215	90522	100,000	100,000	N/A	1015	N/A	1,372	

Creator QPackSA
Reviewer
Approver

Chromatogram

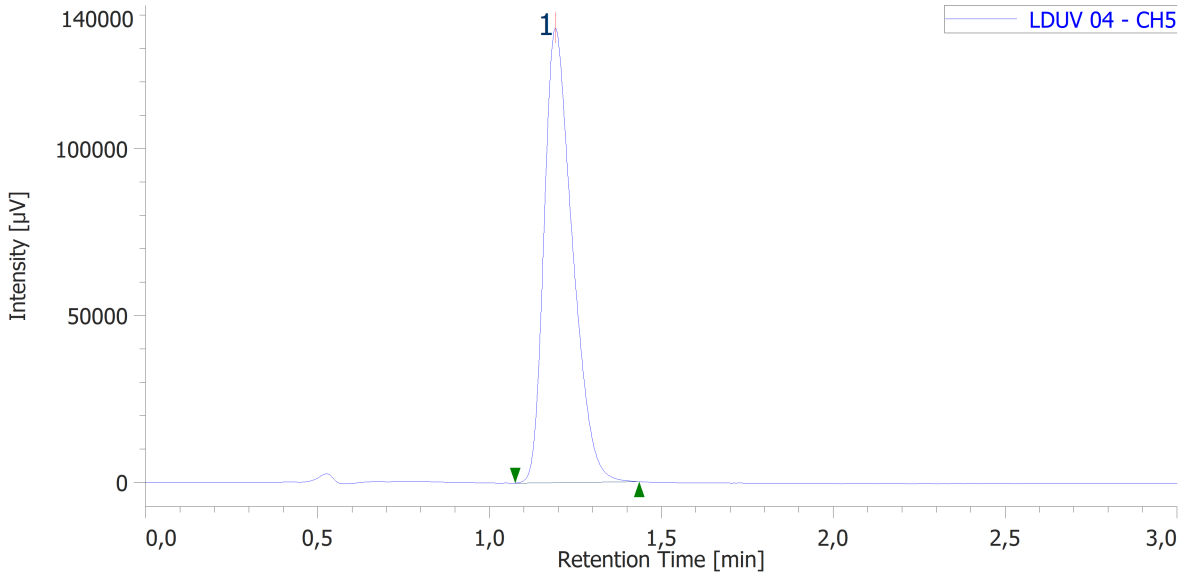

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:21
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:39:40
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	779688	136223	100,000	100,000	N/A	1018	N/A	1,387	

Creator QPackSA
Reviewer
Approver

Chromatogram

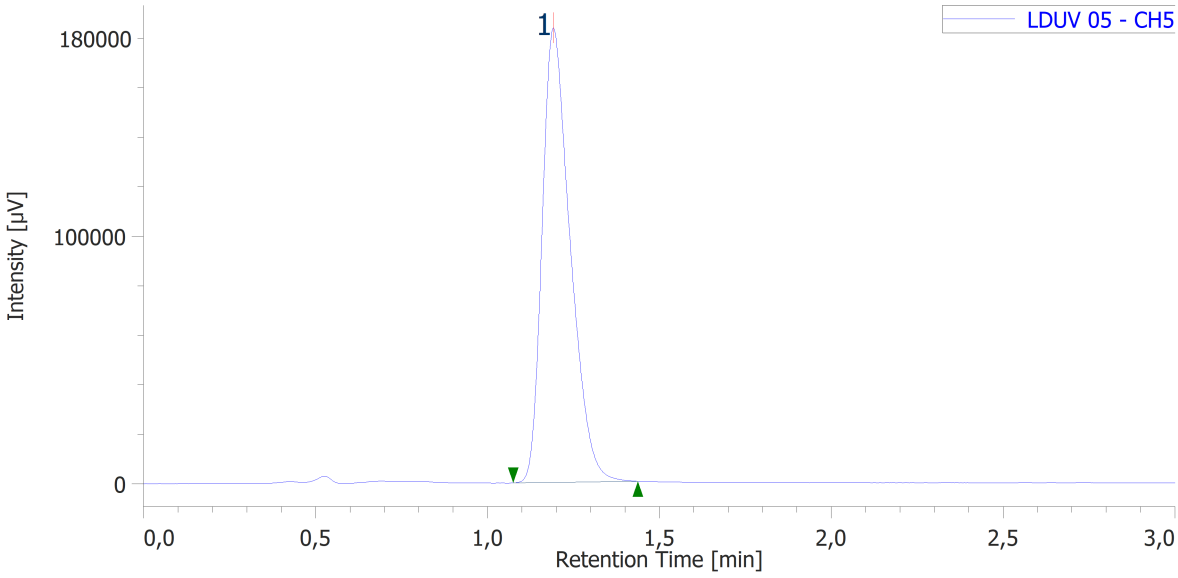

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 12:43:28
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,192	1041230	183513	100,000	100,000	N/A	1042	N/A	1,385	

Creator QPackSA
Reviewer
Approver

Chromatogram

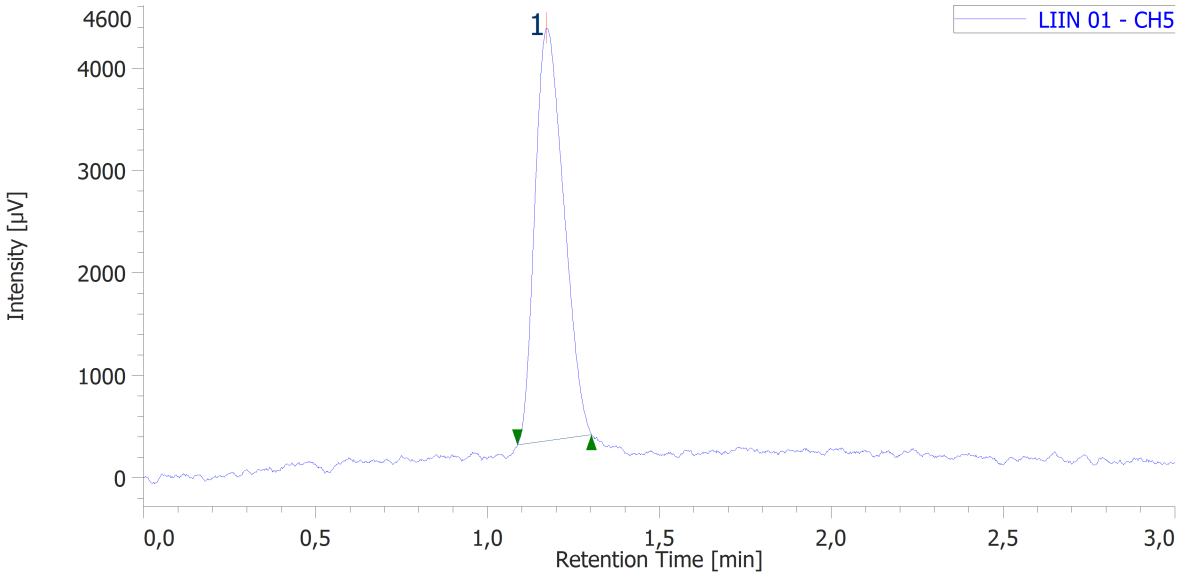

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 13:08:02
Volume	0,1 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,172	23470	4030	100,000	100,000	N/A	854	N/A	1,309	

Creator QPackSA
Reviewer
Approver

Chromatogram

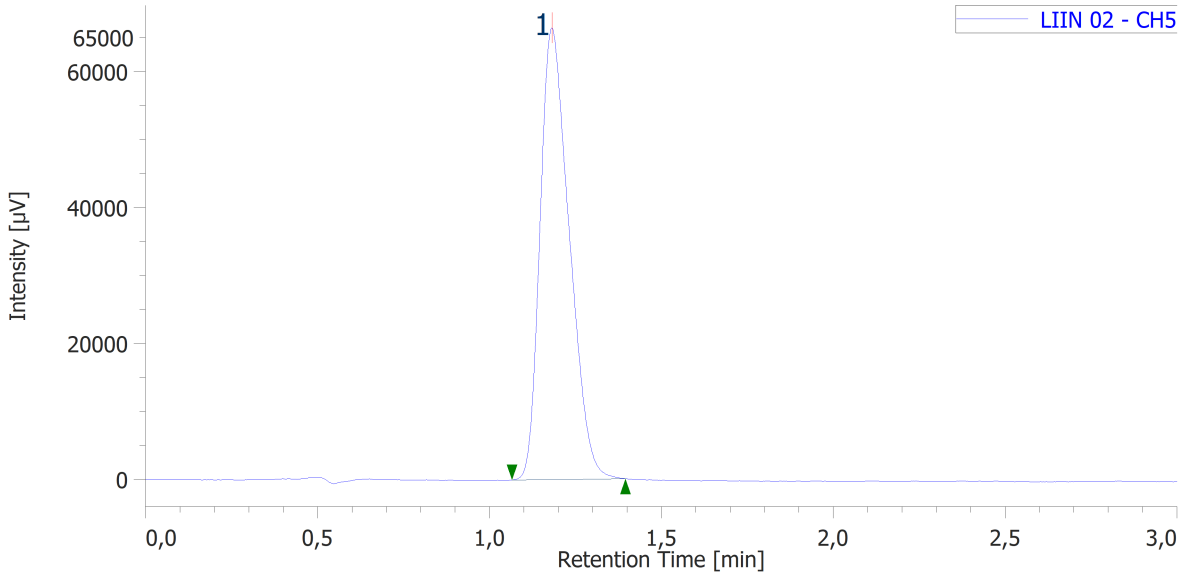

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 13:11:46
Volume	5,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,182	391986	66382	100,000	100,000	N/A	896	N/A	1,333	

Creator QPackSA
Reviewer
Approver

Chromatogram

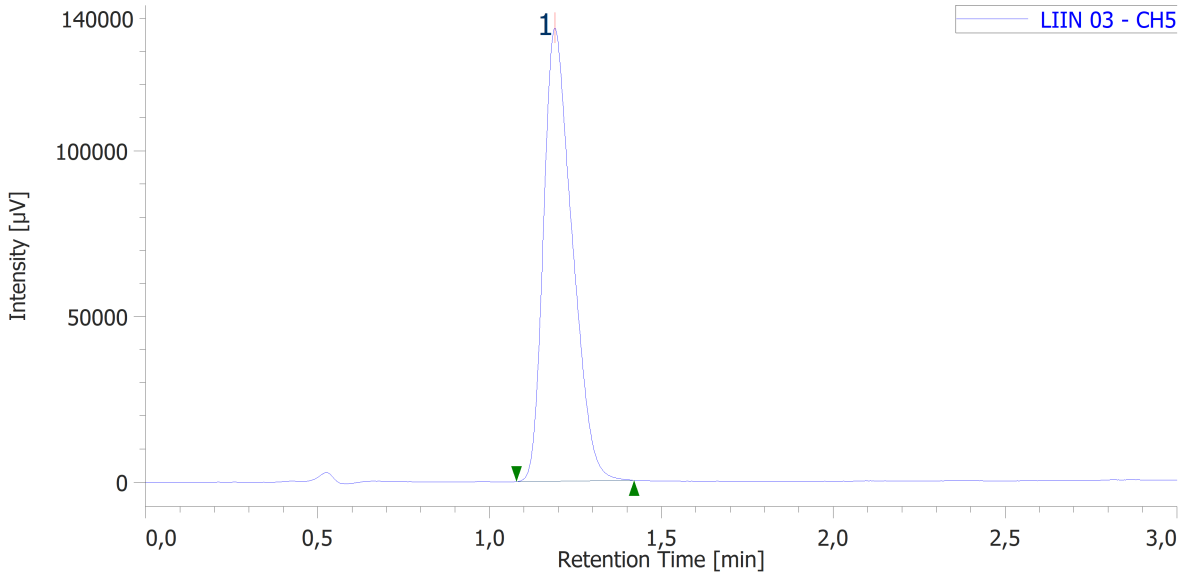

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 13:15:35
Volume	10,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,190	790727	136783	100,000	100,000	N/A	961	N/A	1,369	

Creator QPackSA
Reviewer
Approver

Chromatogram

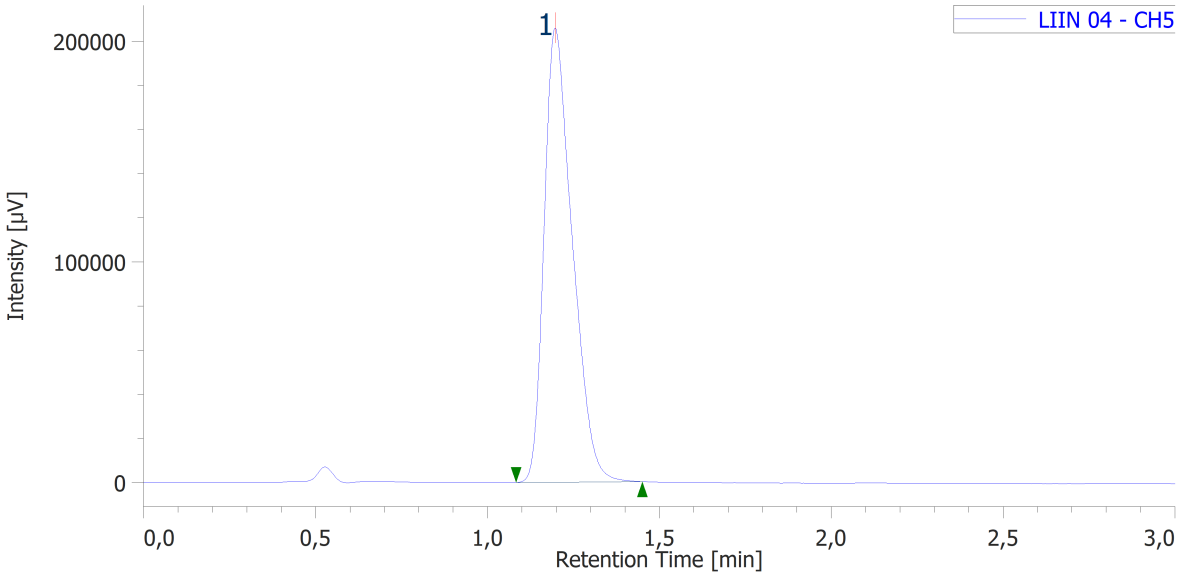

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 13:19:25
Volume	15,0 [µL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,197	1172579	205825	100,000	100,000	N/A	1018	N/A	1,394	

Creator QPackSA
Reviewer
Approver

Chromatogram

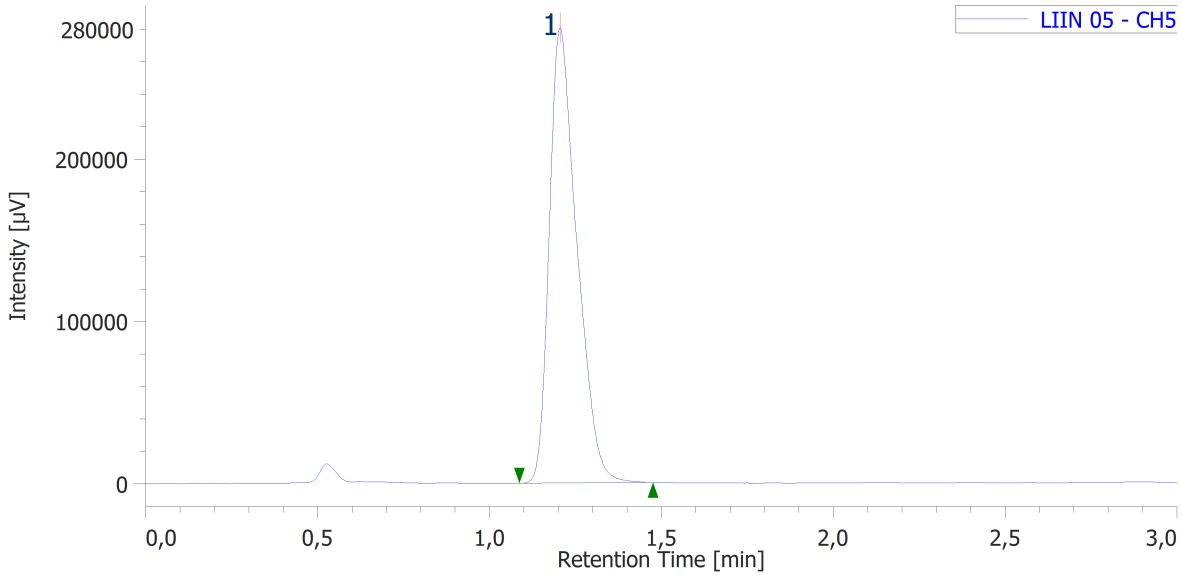

Chromatogram Information	
User Name	QPackSA
Date Modified	07/06/2024 14:01:22
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 13:23:19
Volume	20,0 [μL]
Sample #	10
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,205	1563260	280313	100,000	100,000	N/A	1099	N/A	1,410	

Creator QPackSA
Reviewer
Approver

Chromatogram

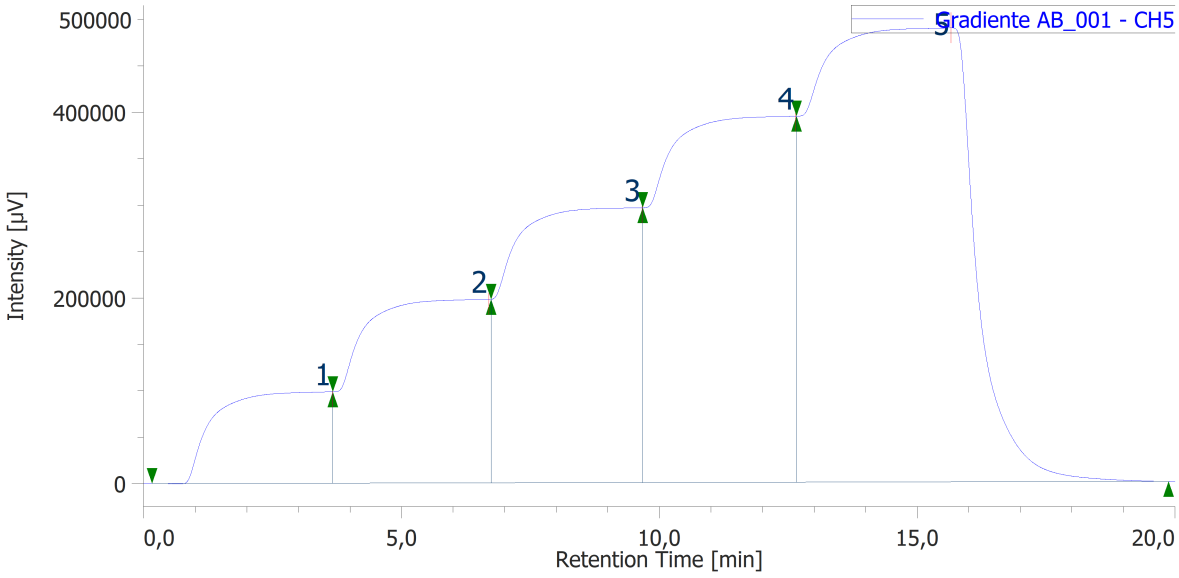

Chromatogram Information	
User Name	QPackSA
Date Modified	18/06/2024 13:32:19
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 14:30:43
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,660	14185699	98441	5,332	6,673	N/A	N/A	N/A	N/A	
2	40%	5	6,690	33001327	197516	12,404	13,388	N/A	N/A	N/A	N/A	
3	60%	5	9,660	49269750	296011	18,519	20,065	N/A	N/A	N/A	N/A	
4	80%	5	12,637	67221767	394340	25,267	26,730	N/A	N/A	N/A	N/A	
5	100%	5	15,653	102369928	488970	38,478	33,144	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

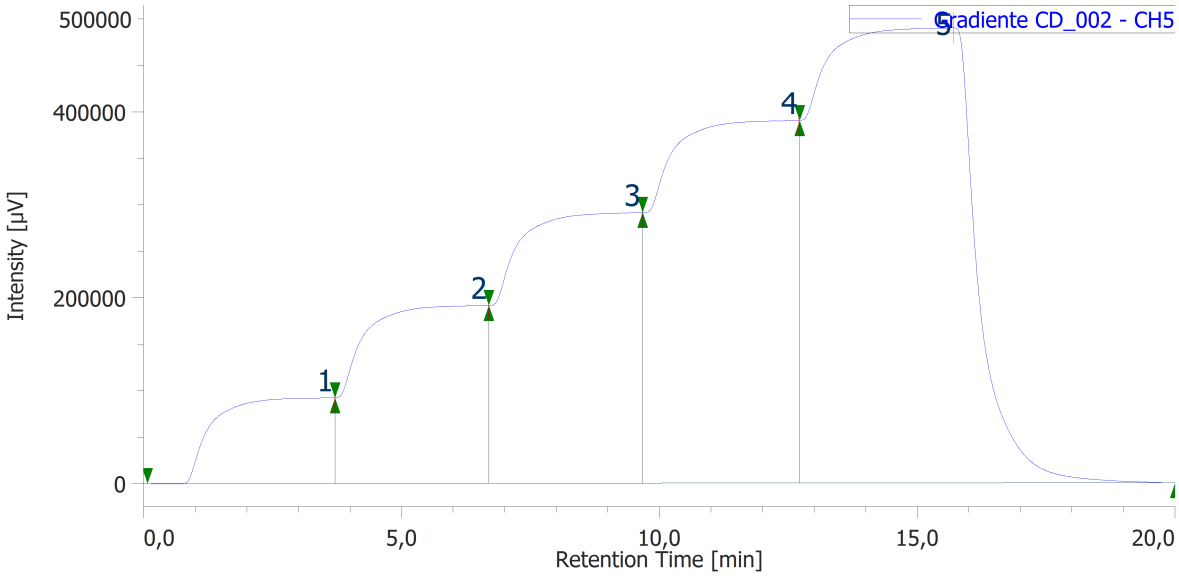

Chromatogram Information	
User Name	QPackSA
Date Modified	18/06/2024 13:32:20
Description	
HPLC System Name	01-HP-03
Injection Date	07/06/2024 14:52:38
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,700	13516220	92103	5,154	6,338	N/A	N/A	N/A	N/A	
2	40%	5	6,683	31038536	191222	11,835	13,159	N/A	N/A	N/A	N/A	
3	60%	5	9,660	48723435	290971	18,578	20,023	N/A	N/A	N/A	N/A	
4	80%	5	12,700	67778615	389770	25,844	26,821	N/A	N/A	N/A	N/A	
5	100%	5	15,697	101206275	489137	38,590	33,659	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver