
Peak Find - EDUV_001 PDA_tR4,79 D.jws

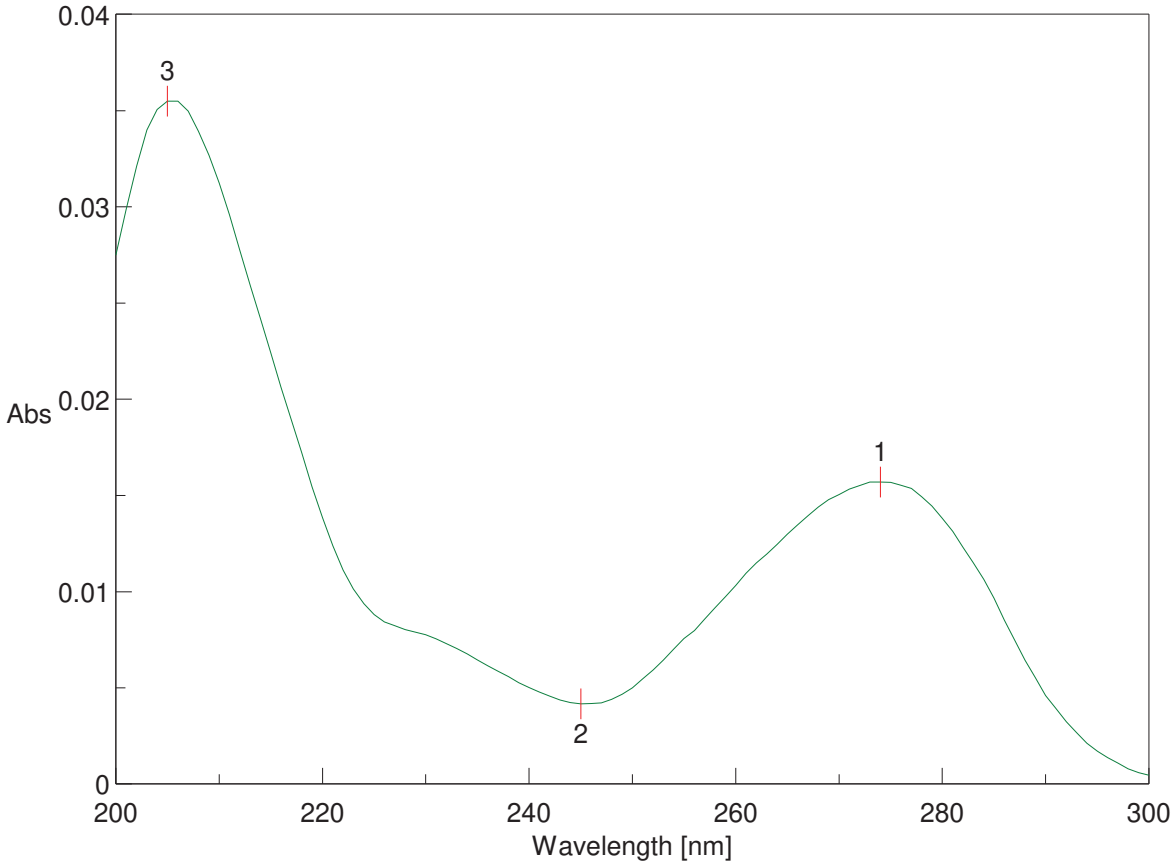

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	21/10/2021 00:46

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	072260870
ROM version	2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.015686	2	245	0.004155
3	205	0.035483			

Chromatogram

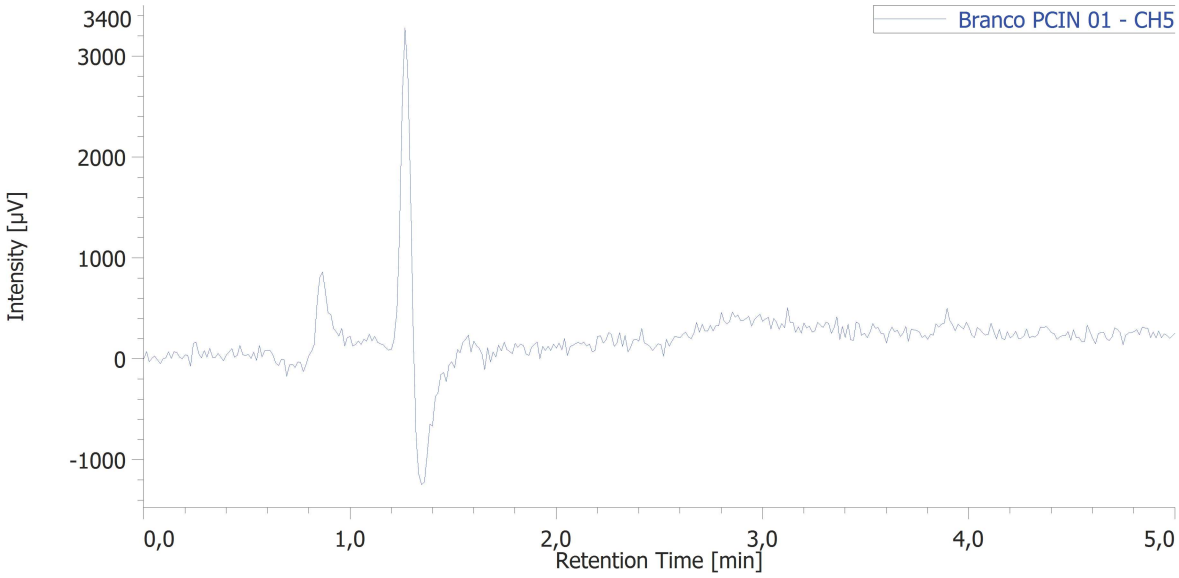


Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:05
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:04:50
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

Creator QPackSA
Reviewer
Approver

Chromatogram

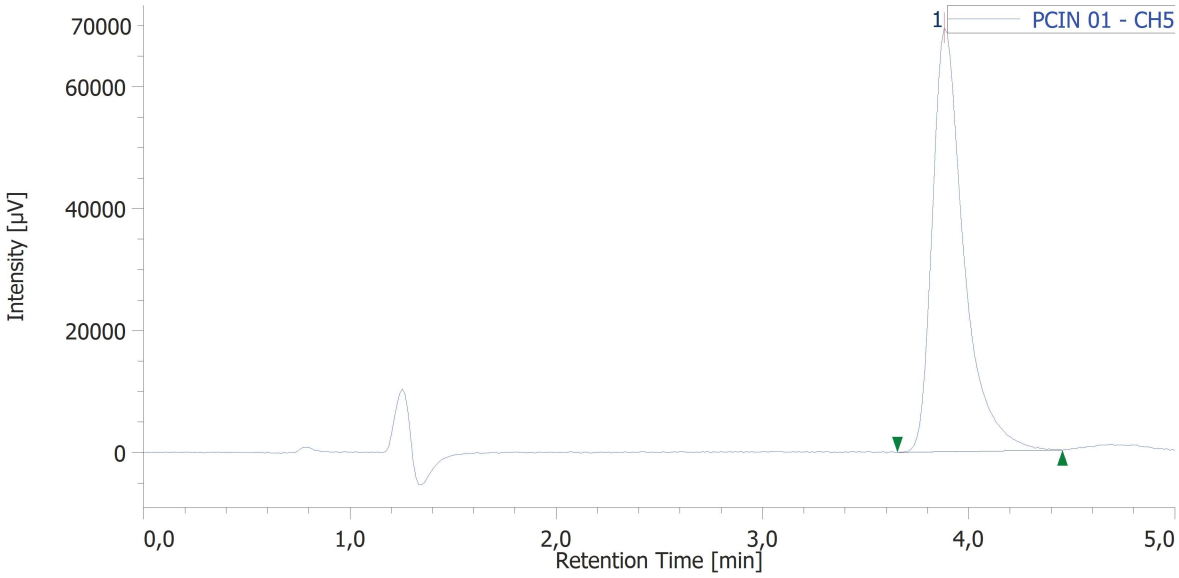

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:07
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:10:38
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,880	735536	69452	100,000	100,000	N/A	3623	N/A	1,618	

Creator QPackSA
Reviewer
Approver

Chromatogram

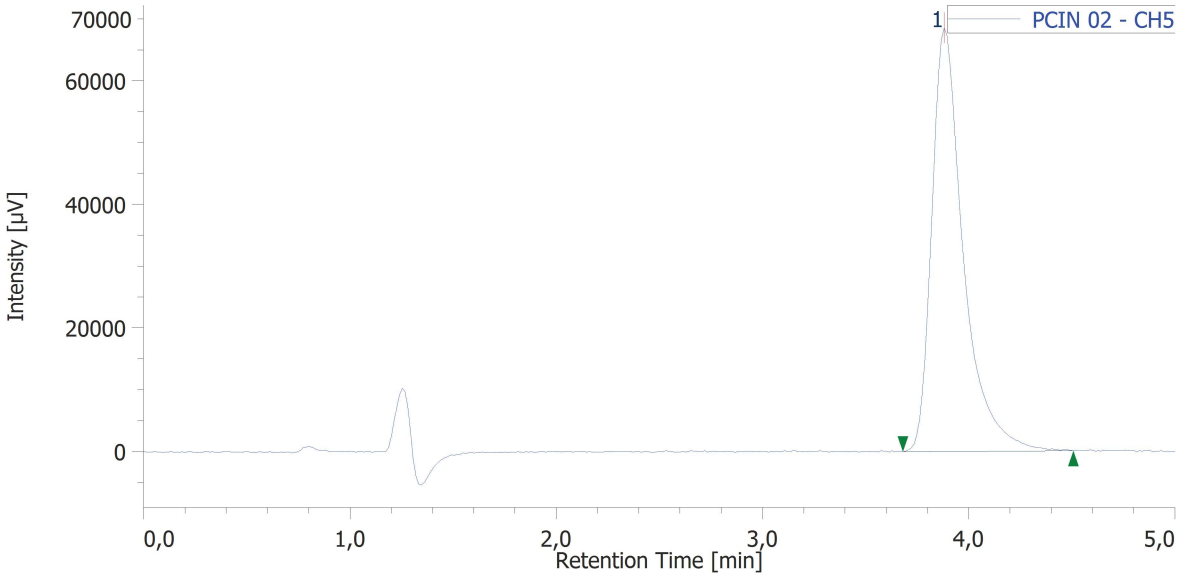

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:07
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:16:25
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,880	729418	68521	100,000	100,000	N/A	3646	N/A	1,599	

Creator QPackSA
Reviewer
Approver

Chromatogram

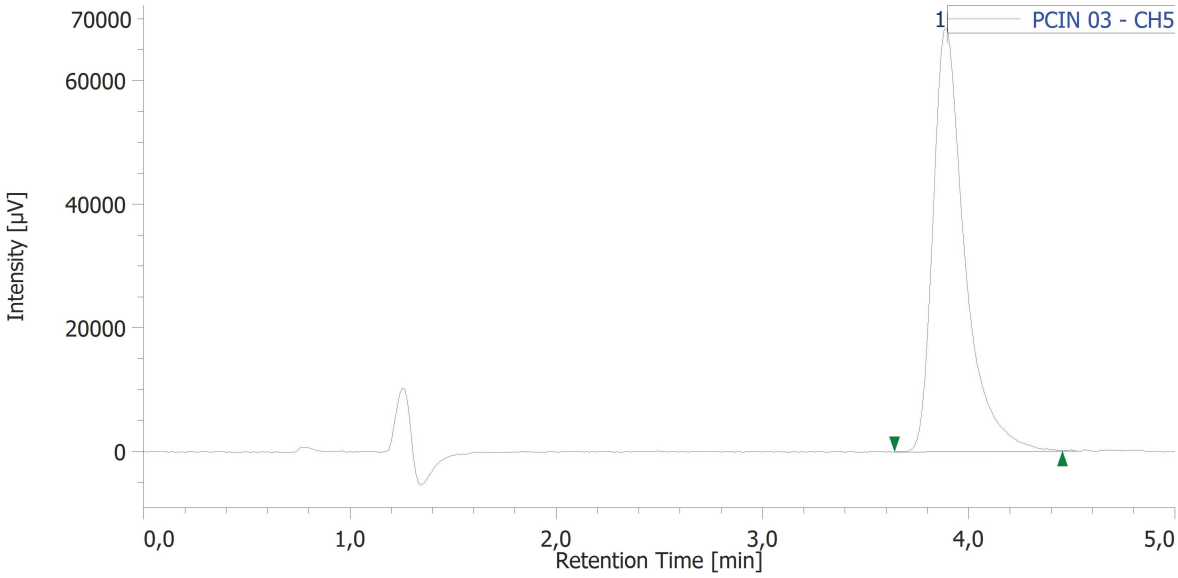

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:07
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:22:13
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,893	734230	68552	100,000	100,000	N/A	3613	N/A	1,536	

Creator QPackSA
Reviewer
Approver

Chromatogram

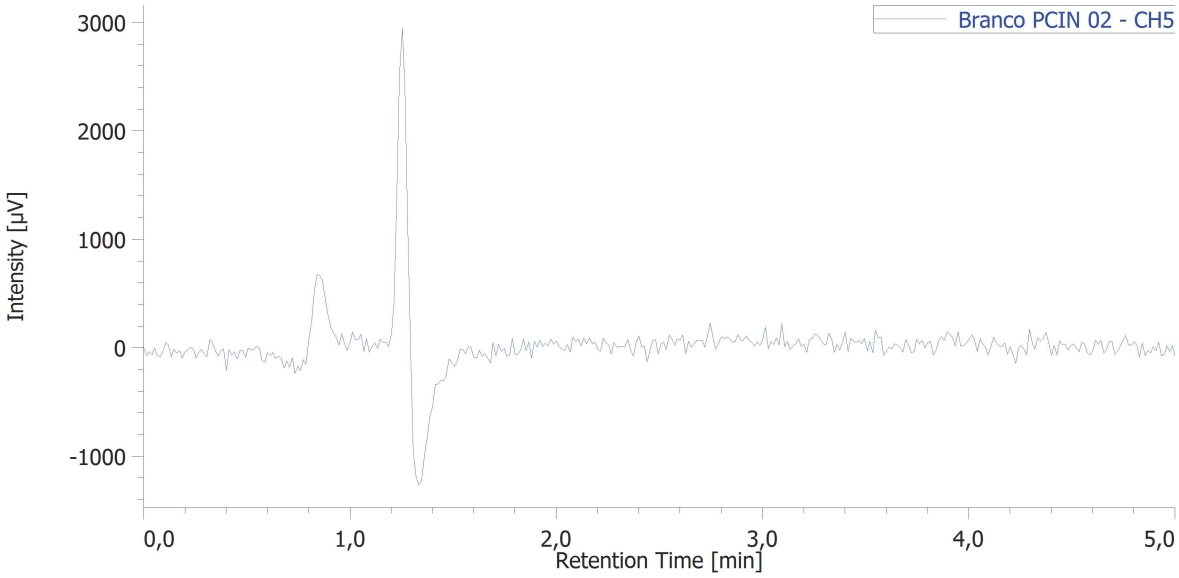


Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:07
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:28:00
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

Creator QPackSA
Reviewer
Approver

Chromatogram

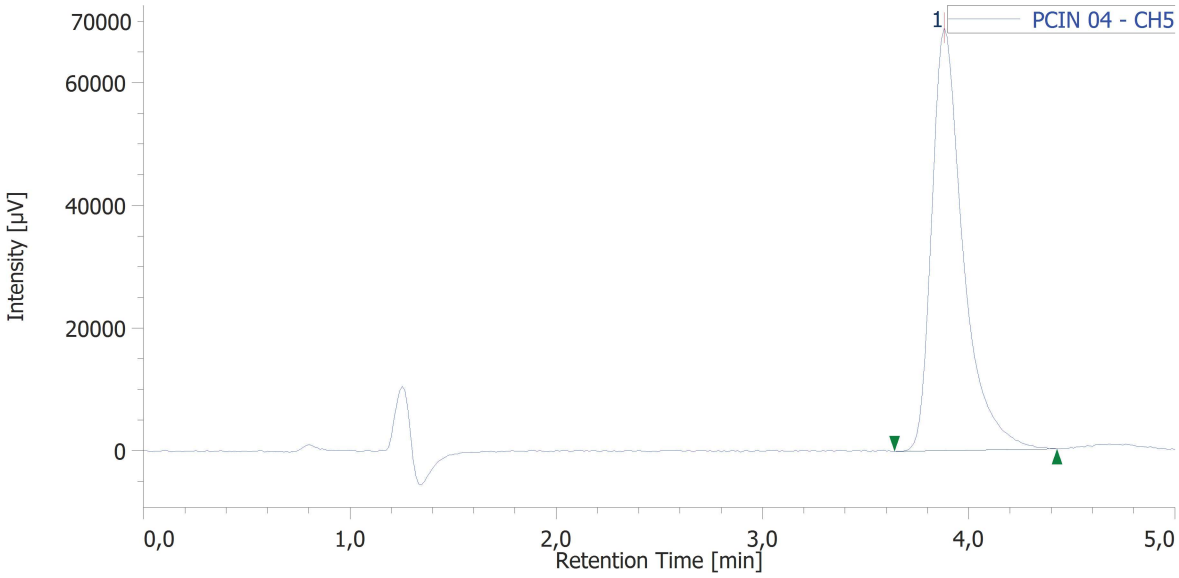

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:07
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:33:48
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,880	727870	68830	100,000	100,000	N/A	3617	N/A	1,569	

Creator QPackSA
Reviewer
Approver

Chromatogram

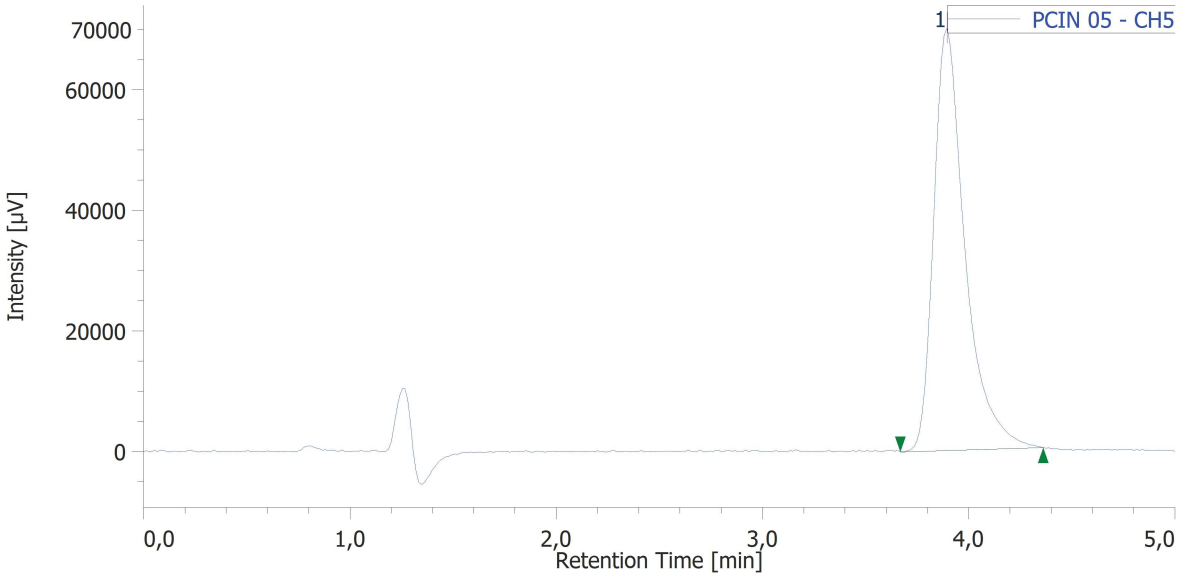

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:08
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:39:35
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,893	737981	70097	100,000	100,000	N/A	3648	N/A	1,523	

Creator QPackSA
Reviewer
Approver

Chromatogram

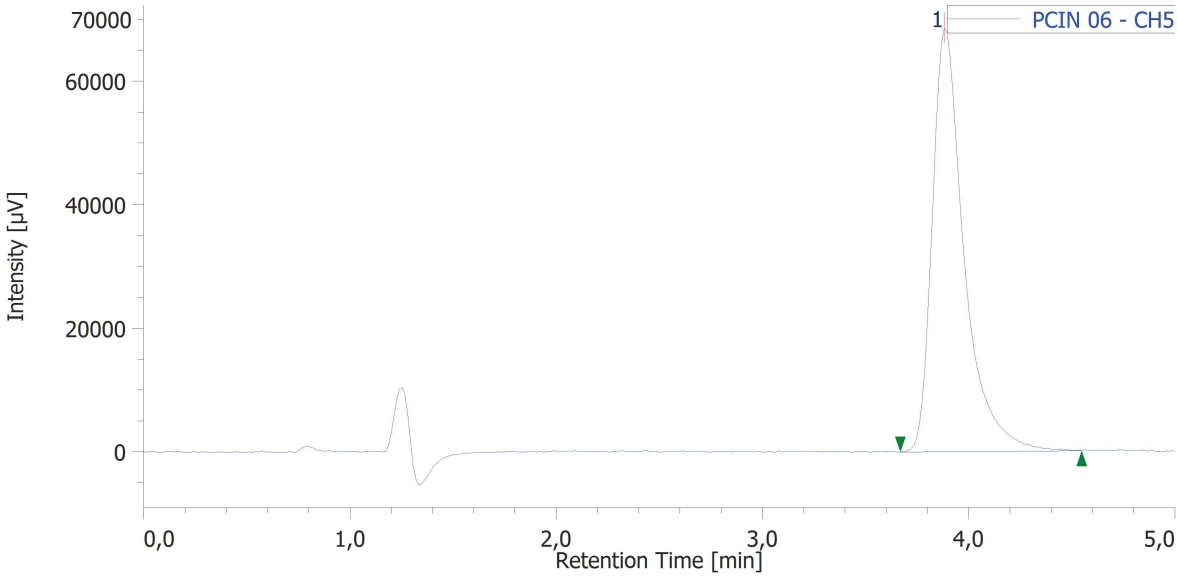

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:08
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:45:23
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,880	734885	68565	100,000	100,000	N/A	3590	N/A	1,633	

Creator QPackSA
Reviewer
Approver

Chromatogram

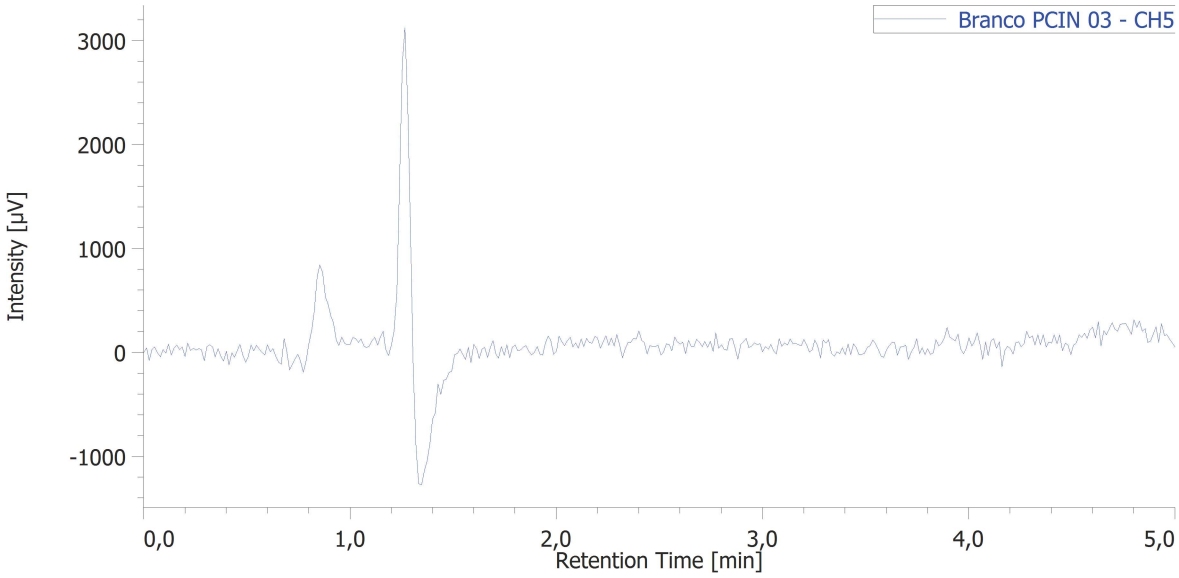


Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 03:09:08
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 02:51:10
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco PCIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

Creator QPackSA
Reviewer
Approver

Chromatogram

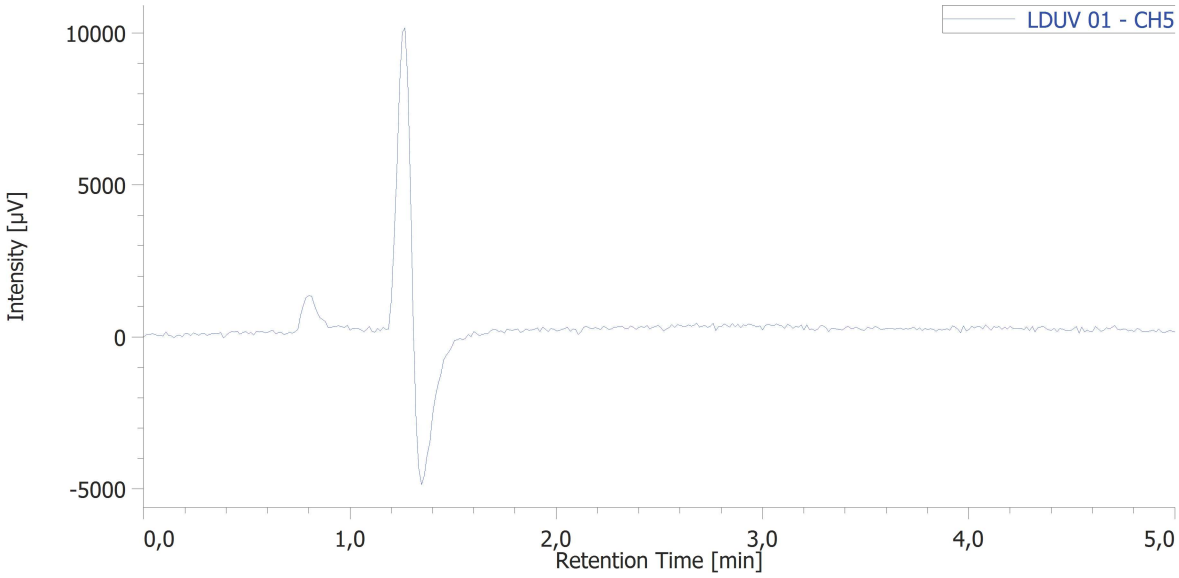


Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 20:30:56
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 20:25:54
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

Creator
Reviewer
Approver

Chromatogram

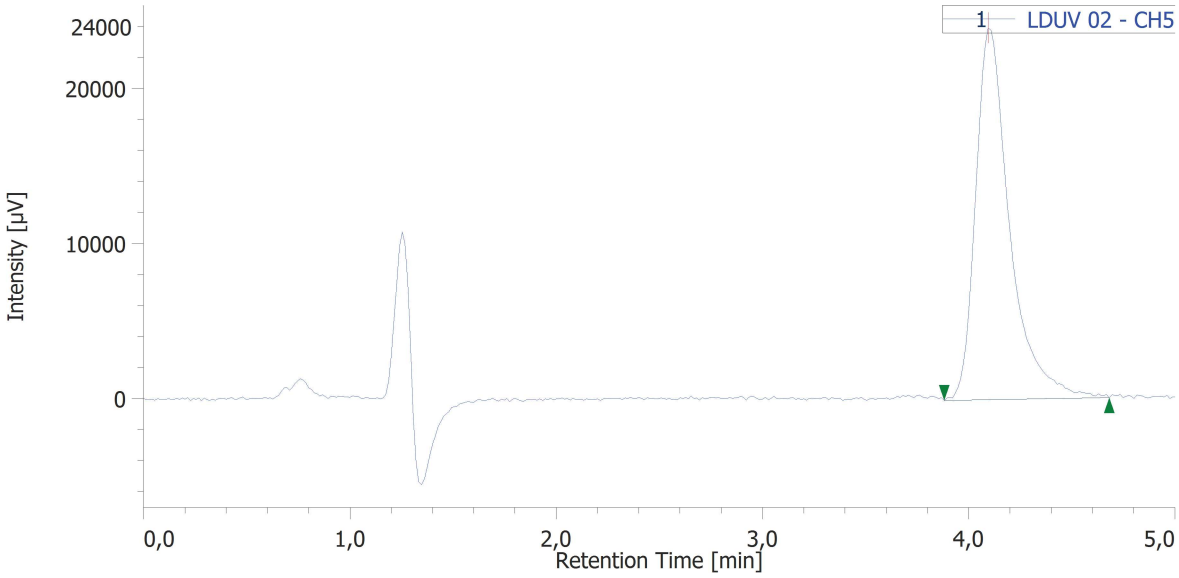

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 20:36:44
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 20:31:41
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,093	275258	23958	100,000	100,000	N/A	3488	N/A	1,649	

Creator
Reviewer
Approver

Chromatogram

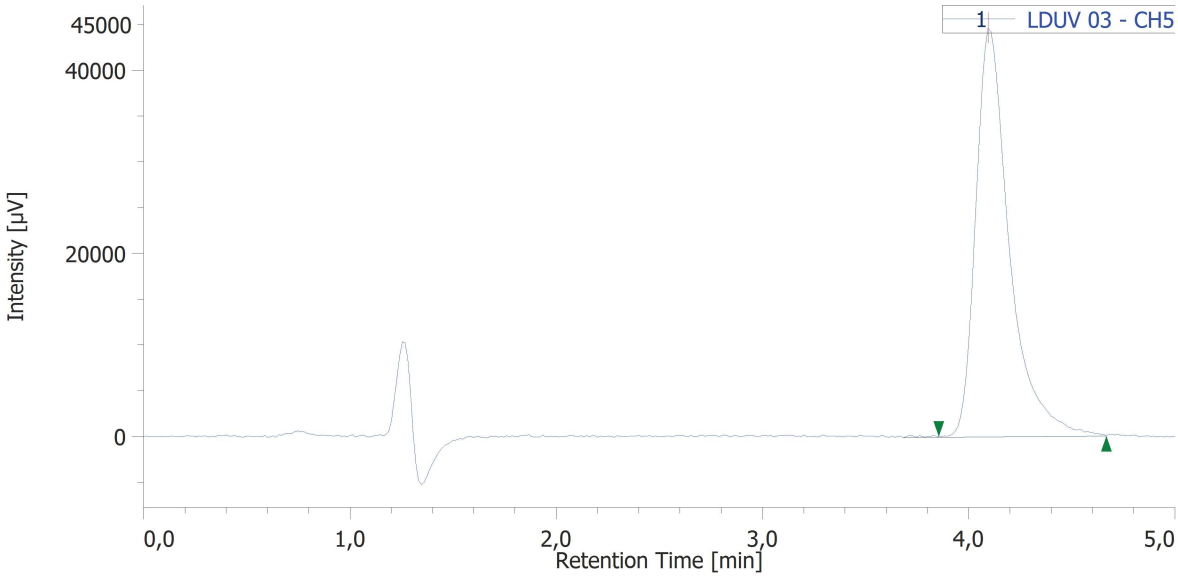

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 20:42:34
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 20:37:31
Volume	10,0 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,093	507035	44653	100,000	100,000	N/A	3565	N/A	1,640	

Creator
Reviewer
Approver

Chromatogram

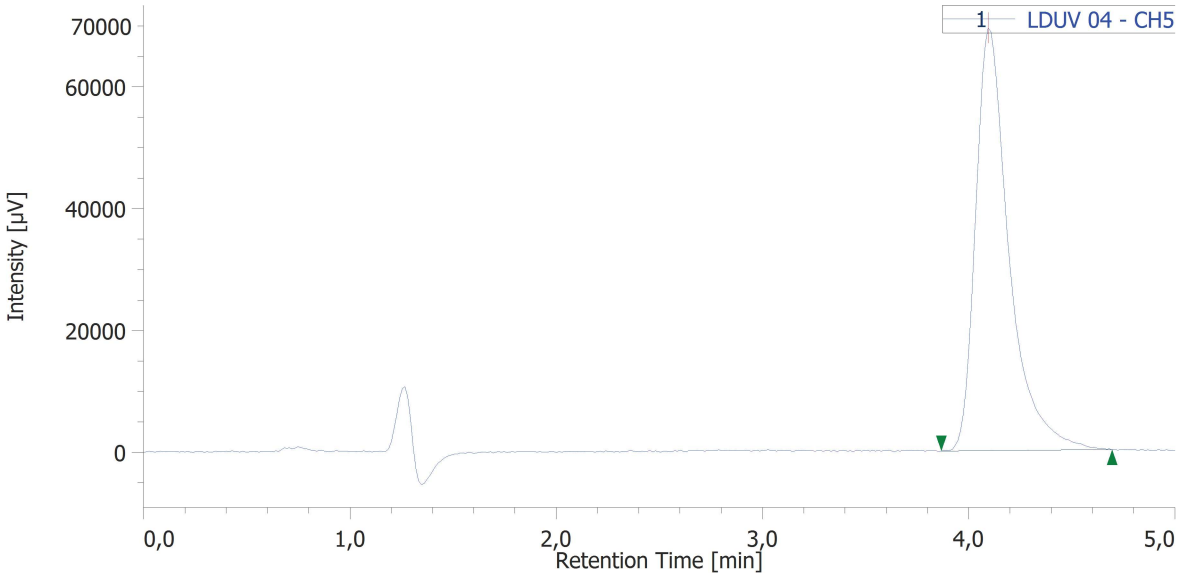

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 20:48:23
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 20:43:21
Volume	10,0 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,093	783900	69340	100,000	100,000	N/A	3579	N/A	1,648	

Creator
Reviewer
Approver

Chromatogram

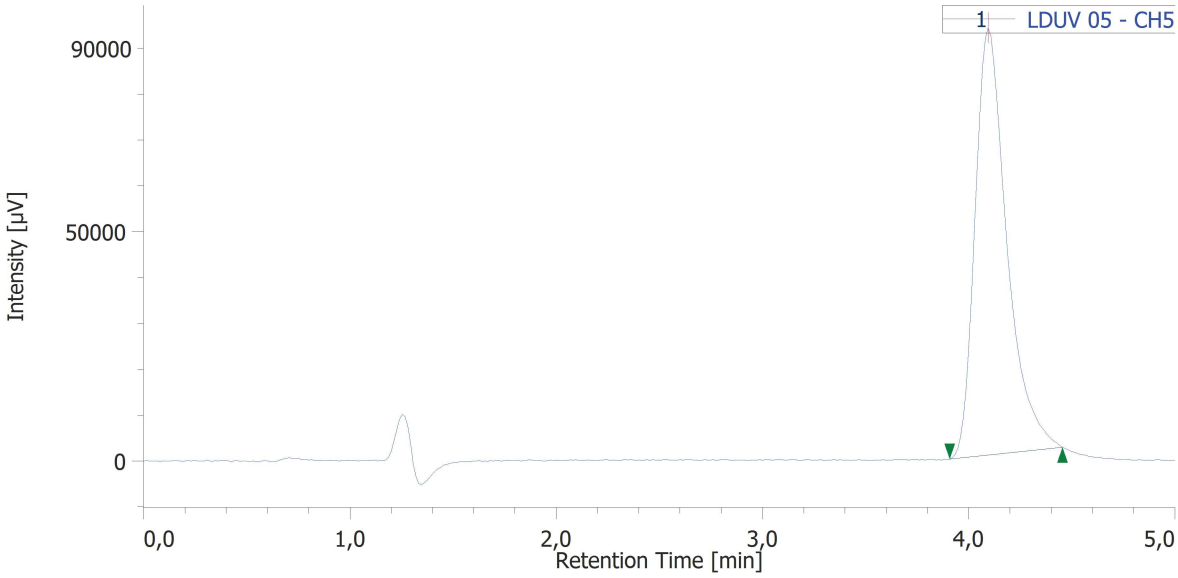

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 21:41:01
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 21:35:58
Volume	10,0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,093	997705	93056	100,000	100,000	N/A	3678	N/A	1,480	

Creator
Reviewer
Approver

Chromatogram

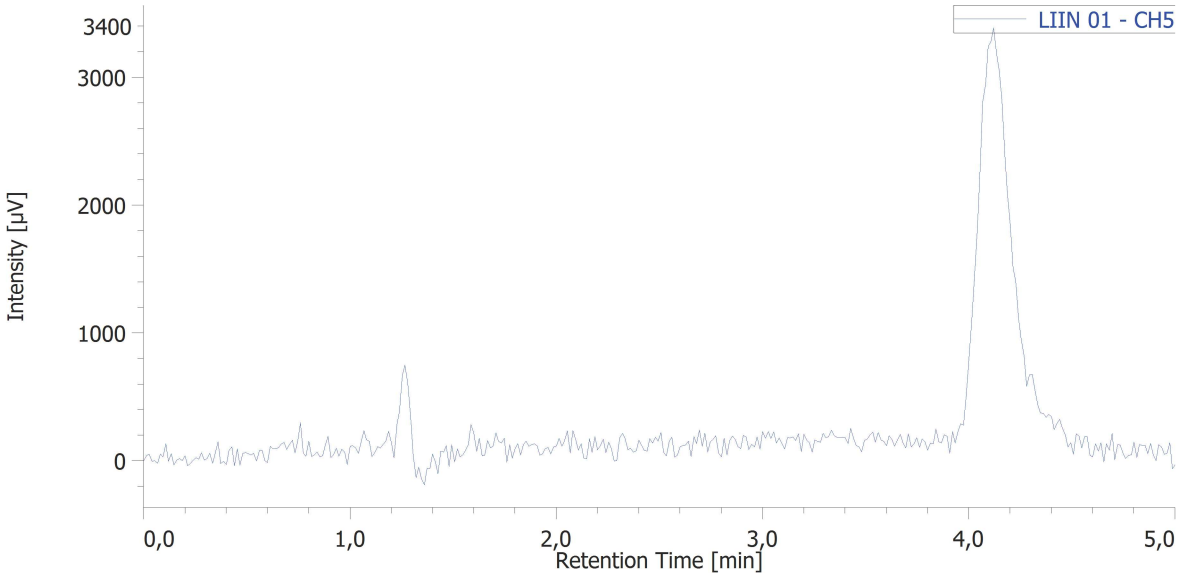


Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 22:00:15
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 21:55:14
Volume	0,1 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

Creator
Reviewer
Approver

Chromatogram

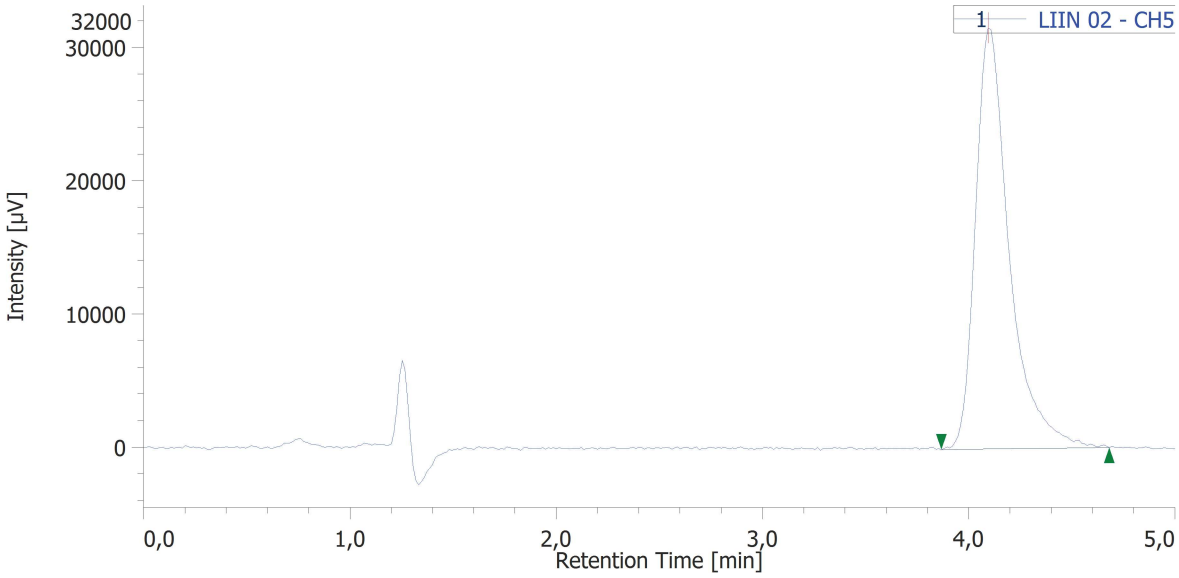

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 22:06:06
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 22:01:04
Volume	5,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,093	360703	31579	100,000	100,000	N/A	3537	N/A	1,625	

Creator
Reviewer
Approver

Chromatogram

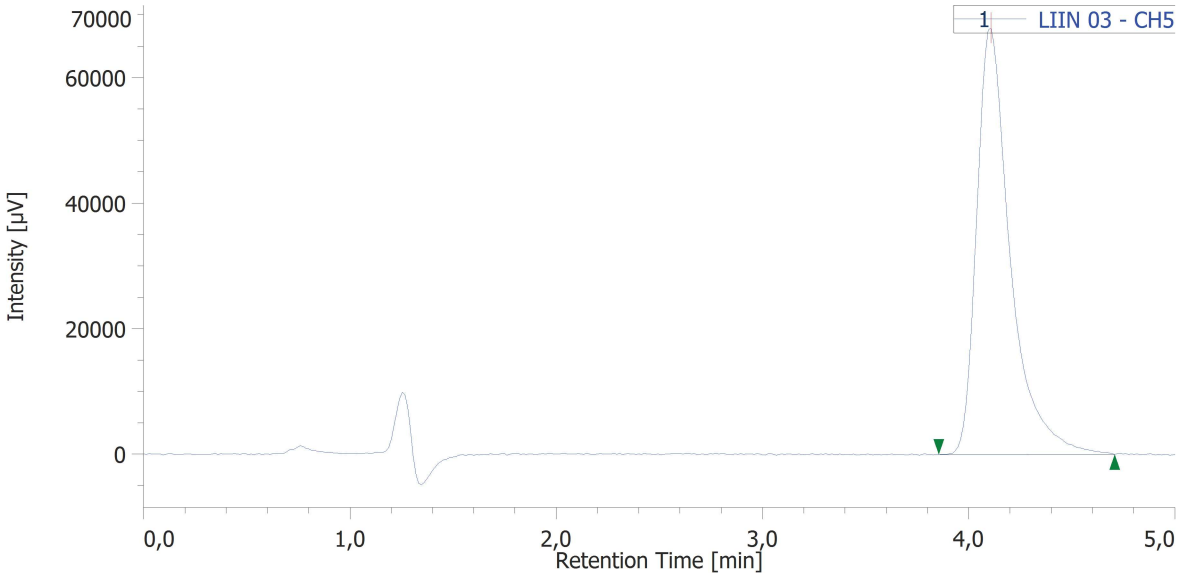

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 22:11:58
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 22:06:56
Volume	10,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,107	770249	67922	100,000	100,000	8,50774	3596	N/A	1,559	Calibration Curve

Creator
Reviewer
Approver

Chromatogram

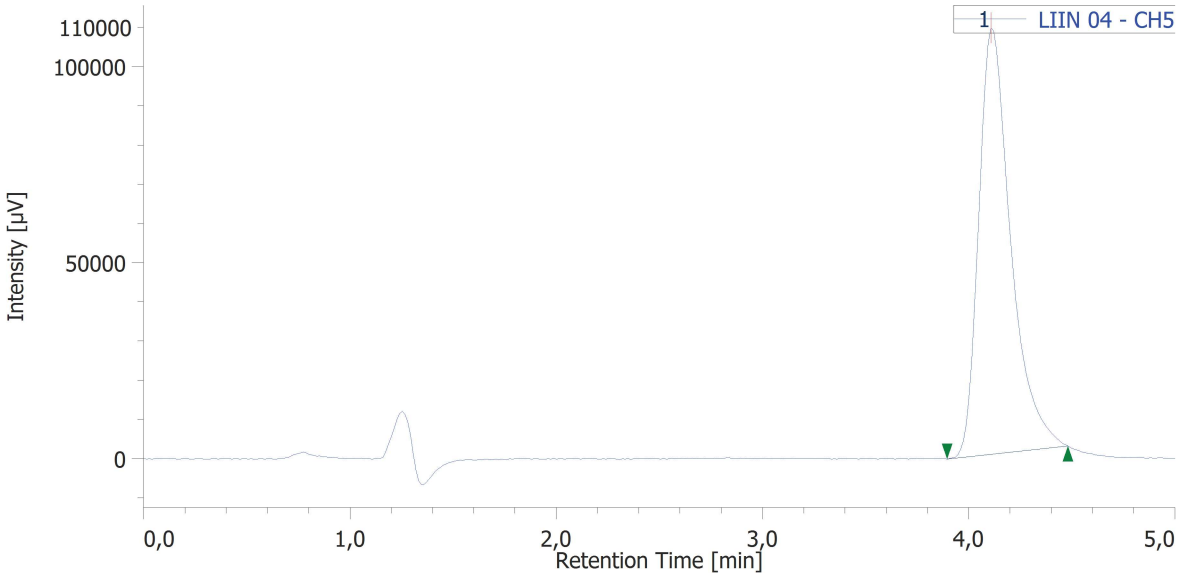

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 22:17:53
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 22:12:51
Volume	15,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,107	1174498	108679	100,000	100,000	16,0739	3668	N/A	1,538	Calibration Curve

Creator
Reviewer
Approver

Chromatogram

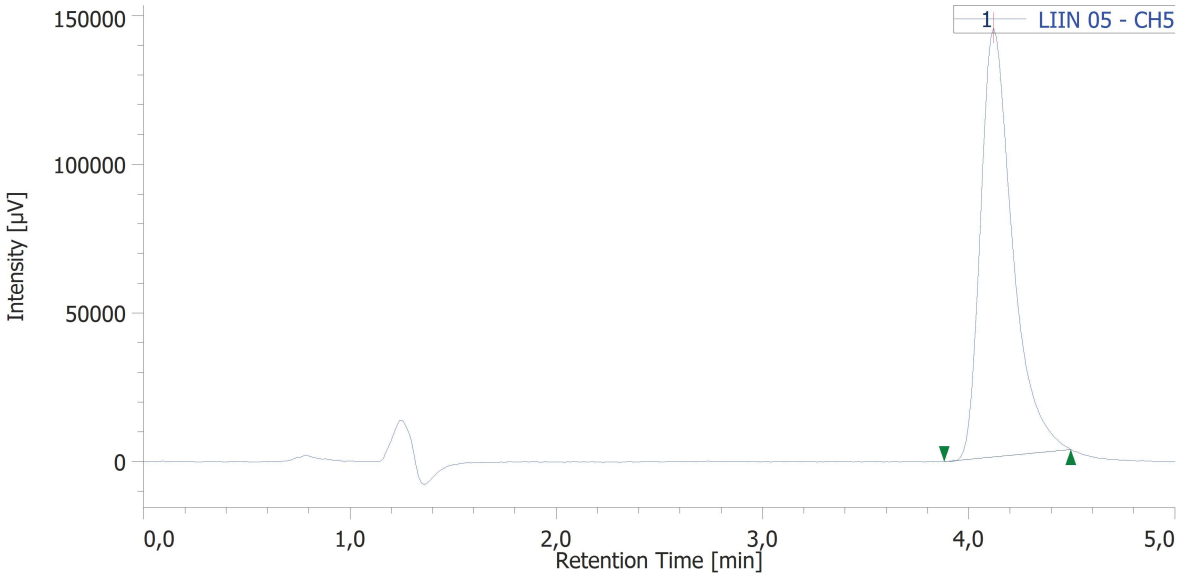

Chromatogram Information	
User Name	QPackSA
Date Modified	26/10/2021 22:23:47
Description	
HPLC System Name	HPL 25
Injection Date	26/10/2021 22:18:45
Volume	20,0 [µL]
Sample #	9
Project Name	Qualificação
Acquisition Time	5,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação2
Peak ID Table	Identificação 10-2021
Calibration Method	Linear LIIN - curva
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Integração 10-2021 (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	4,120	1550403	144167	100,000	100,000	23,1095	3727	N/A	1,513	Calibration Curve, Extrapolation

Creator
Reviewer
Approver

Chromatogram

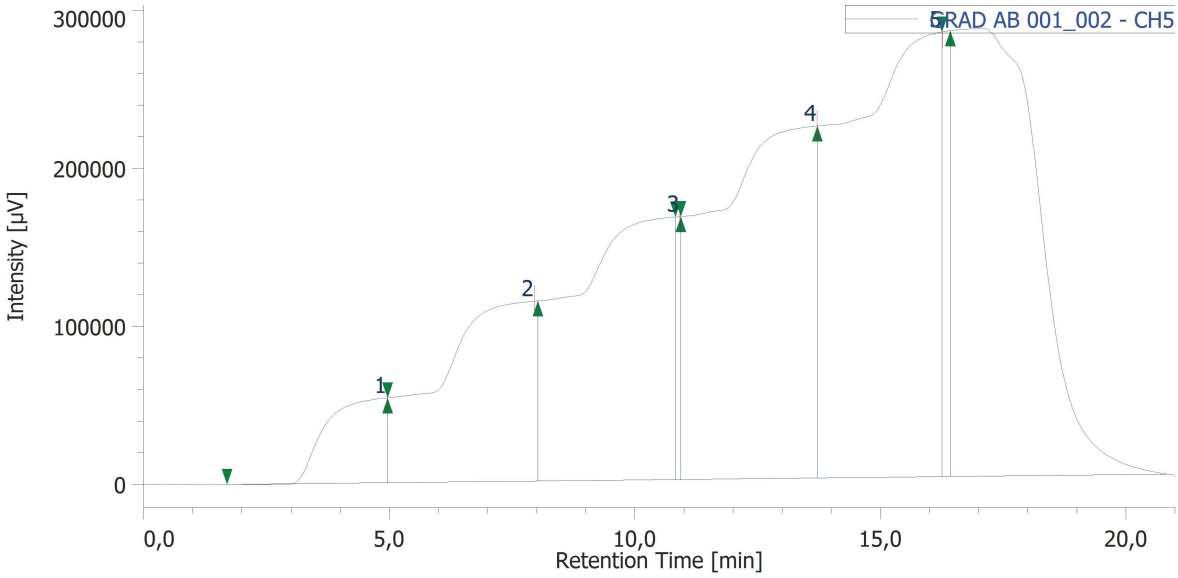

Chromatogram Information	
User Name	QPackSA
Date Modified	03/11/2021 23:52:04
Description	
HPLC System Name	HPL 25
Injection Date	03/11/2021 23:31:01
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	GRAD AB 001_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	4,960	4372423	53623	7,755	6,402	N/A	N/A	N/A	N/A	
2	Unknown	5	7,953	15583388	113730	27,638	13,579	N/A	N/A	N/A	N/A	
3	Unknown	5	10,913	1129673	166297	2,004	19,855	N/A	N/A	N/A	N/A	
4	Unknown	5	13,707	32482689	222698	57,609	26,589	N/A	N/A	N/A	N/A	
5	Unknown	5	16,260	2816282	281218	4,995	33,576	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

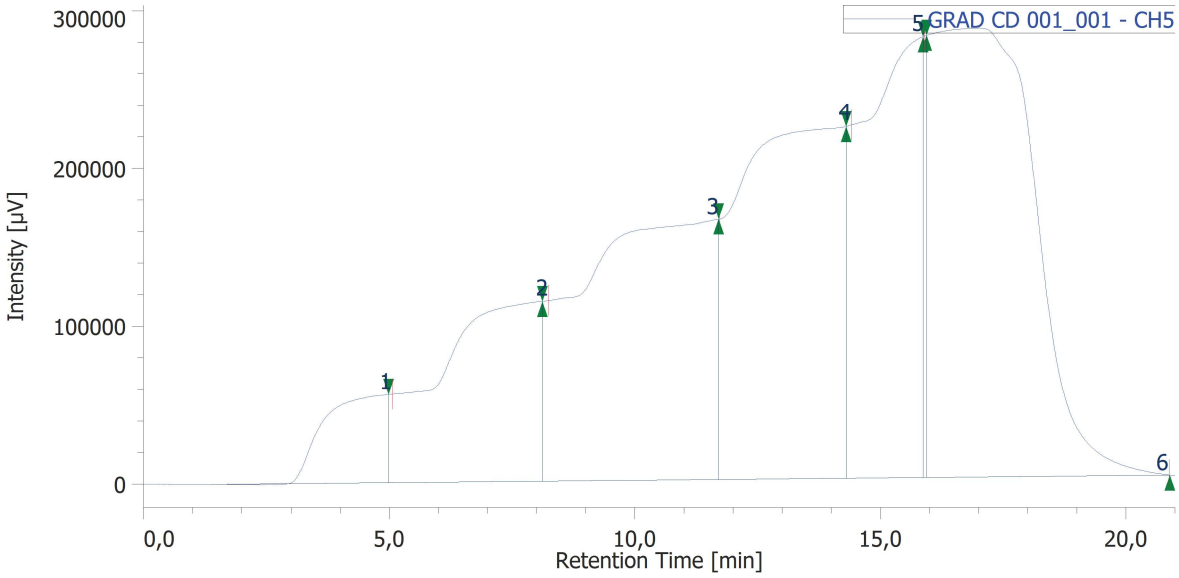

Chromatogram Information	
User Name	QPackSA
Date Modified	04/11/2021 00:28:08
Description	
HPLC System Name	HPL 25
Injection Date	04/11/2021 00:07:06
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	21,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRAD CD 001_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	400 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	5,060	16368187	56190	15,645	6,696	N/A	N/A	N/A	N/A	
2	Unknown	5	8,247	31403798	114460	30,016	13,640	N/A	N/A	N/A	N/A	
3	Unknown	5	11,720	32395913	165008	30,964	19,663	N/A	N/A	N/A	N/A	
4	Unknown	5	14,413	23282259	223783	22,253	26,667	N/A	N/A	N/A	N/A	
5	Unknown	5	15,900	1230676	279717	1,176	33,333	N/A	N/A	N/A	N/A	
6	Unknown	5	20,873	-56007	4	N/A	0,000	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver