
Peak Find - EXATIDAO COMP ONDA.jws

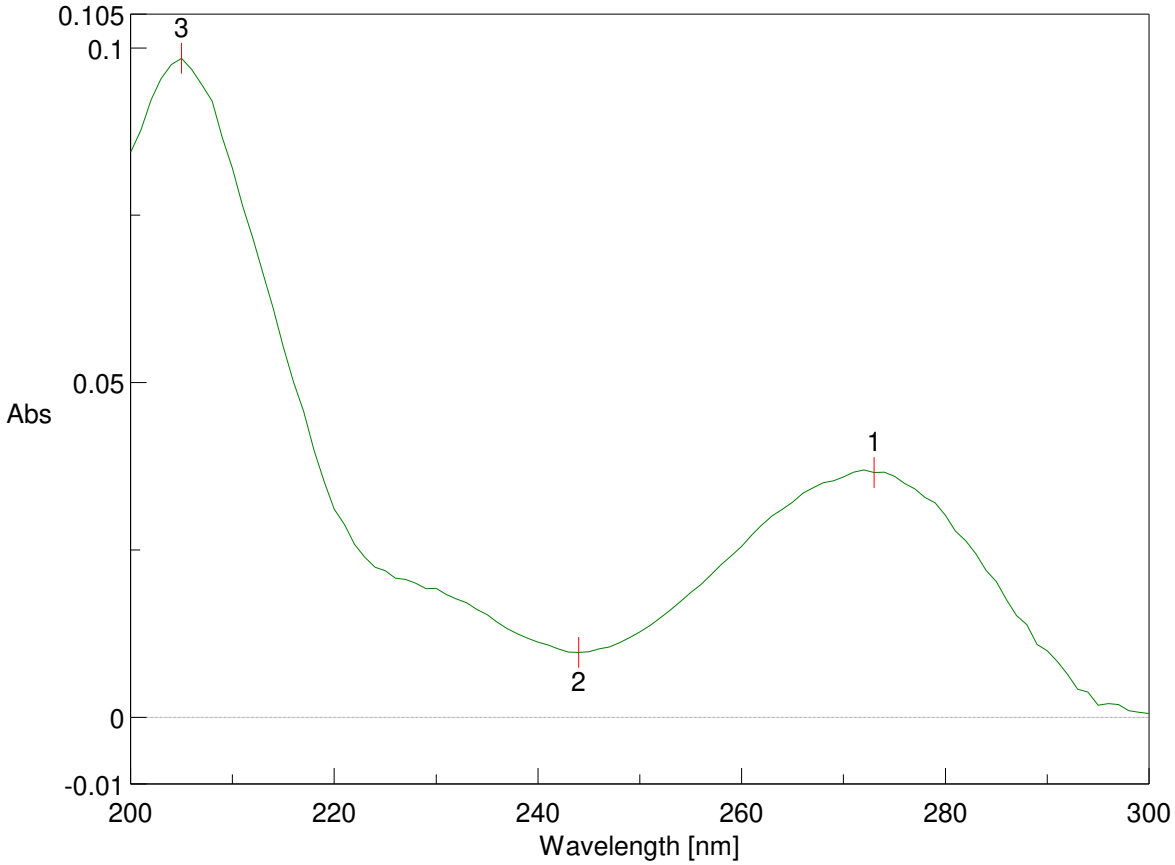

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	01/08/2022 10:47

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	190 nm
End	400 nm
Data interval	1 nm
Data points	211


[Measurement Information]

Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A000661665
ROM version	1.02.02

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.036541	2	244	0.009633
3	205	0.098382			

Chromatogram

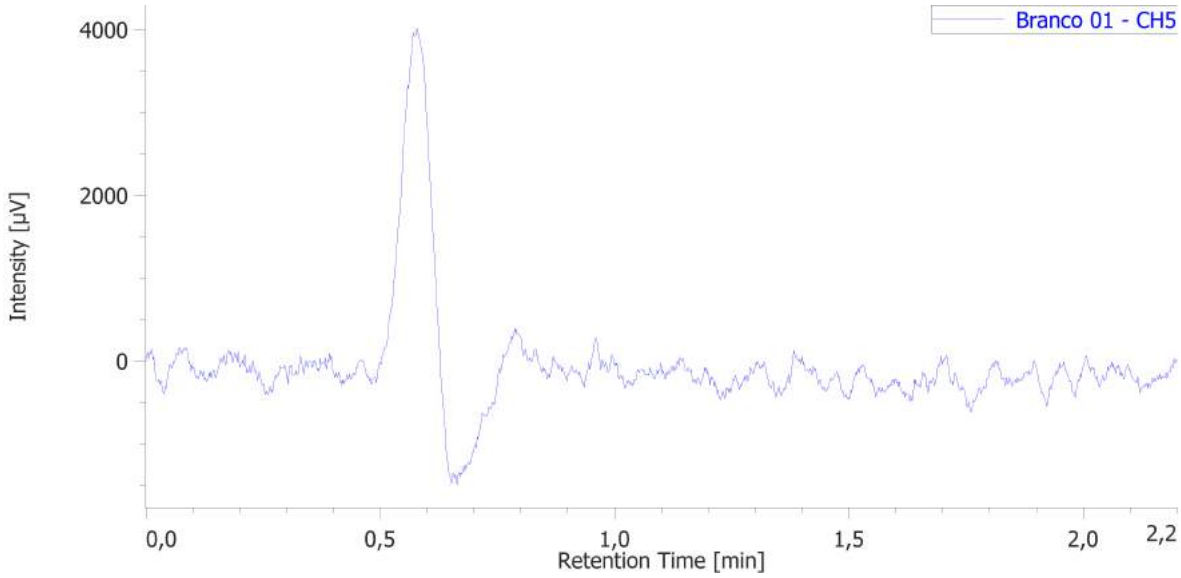


Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:38
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:21:44
Volume	10,0 [µL]
Sample #	102
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	Branco 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

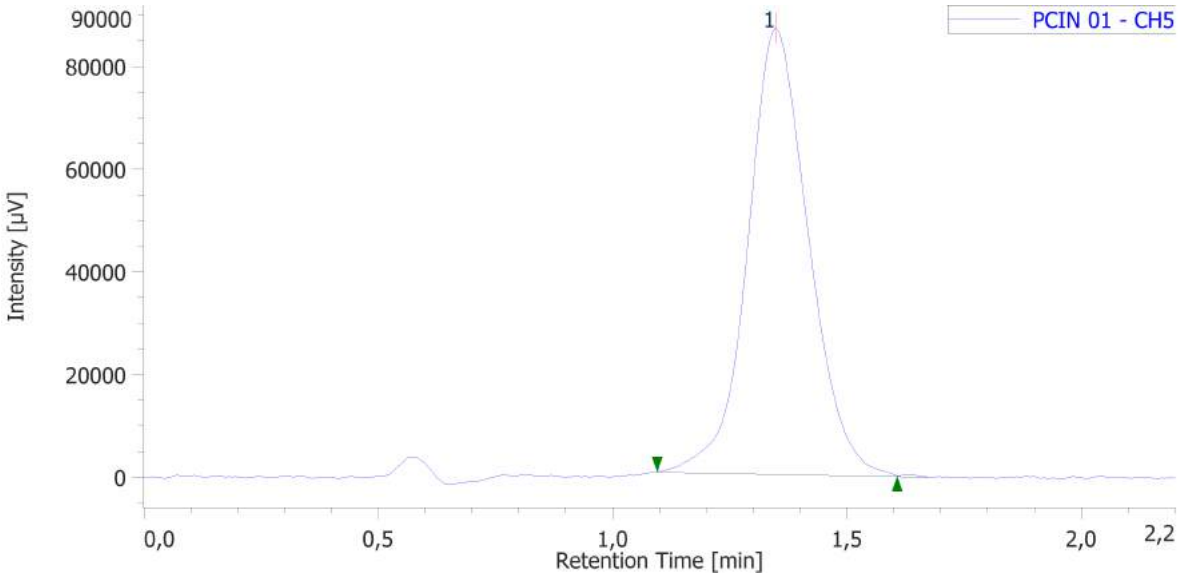

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:38
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:24:43
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH5
Sample Name	PCIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,348	784714	86854	100,000	100,000	N/A	550	N/A	1,040	

Creator QPackSA
Reviewer
Approver

Chromatogram

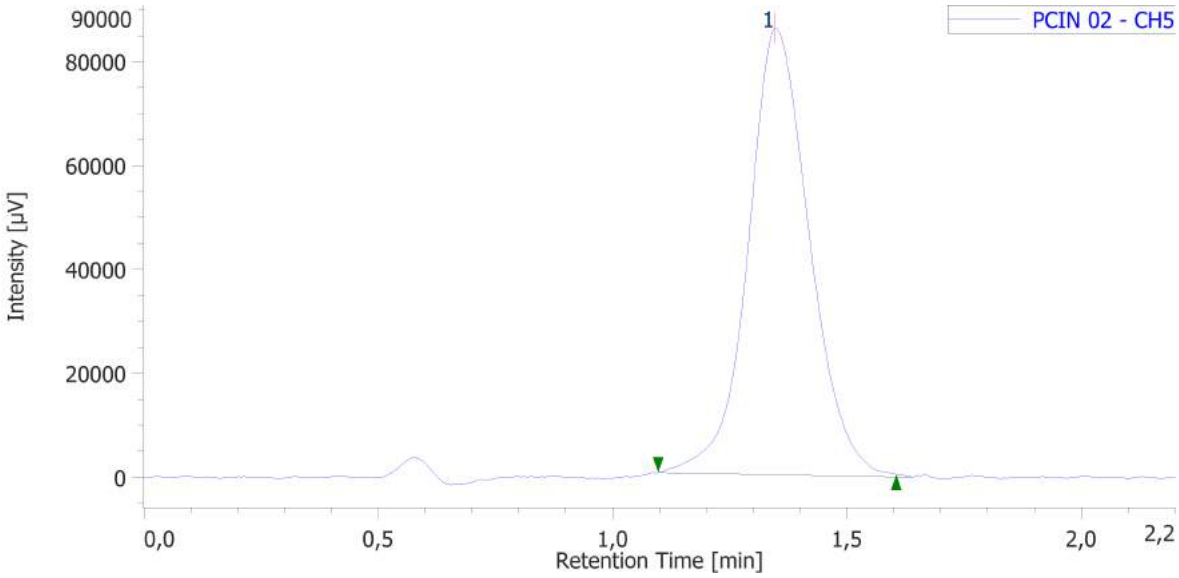

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:38
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:27:44
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH5
Sample Name	PCIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,347	782936	85889	100,000	100,000	N/A	545	N/A	1,072	

Creator QPackSA
Reviewer
Approver

Chromatogram

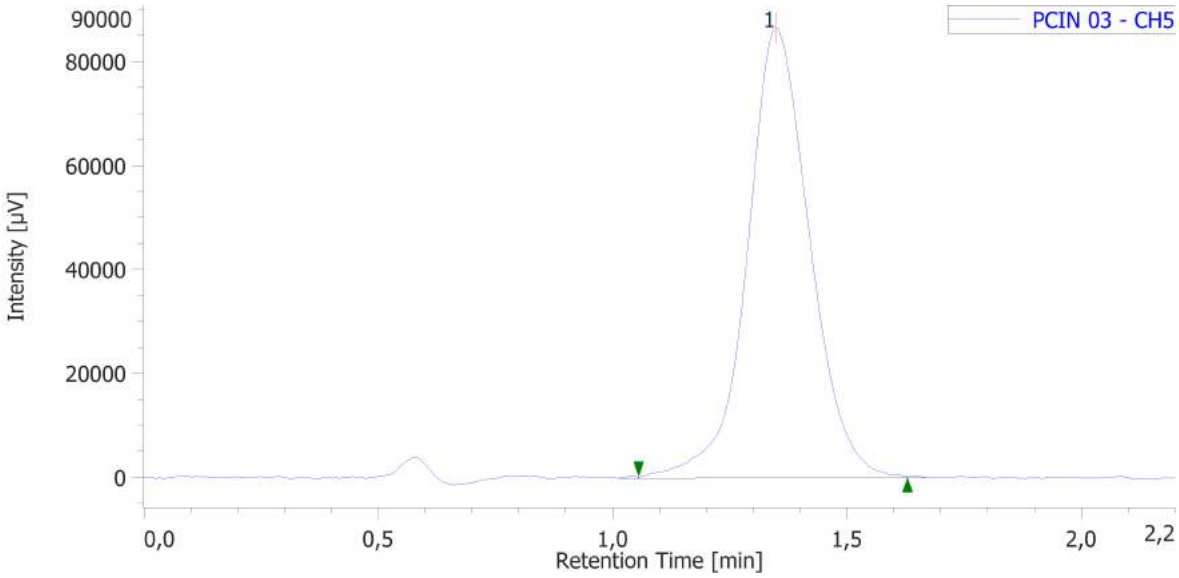

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:39
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:30:44
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH5
Sample Name	PCIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,348	802039	86452	100,000	100,000	N/A	532	N/A	1,025	

Creator QPackSA
Reviewer
Approver

Chromatogram

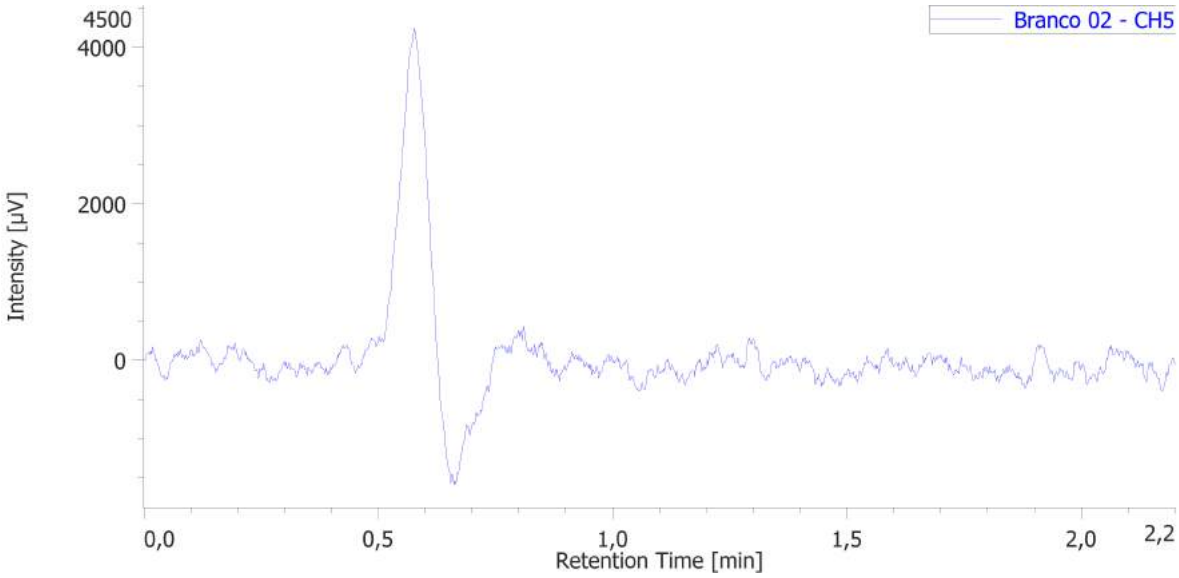


Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:39
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:33:45
Volume	10,0 [µL]
Sample #	102
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	Branco 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

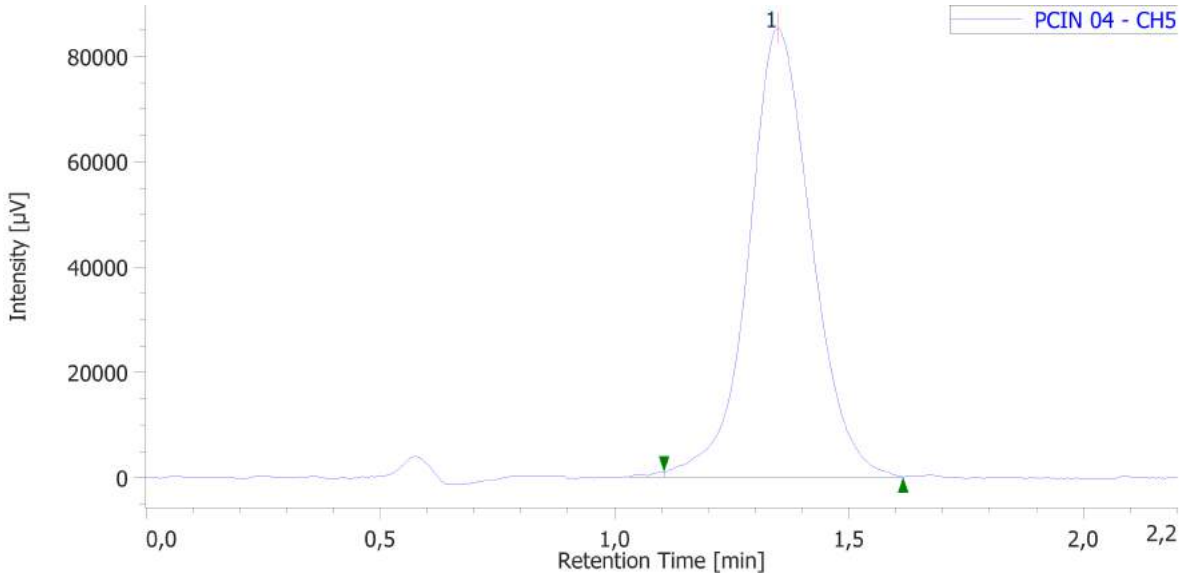

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:39
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:36:45
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH5
Sample Name	PCIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,348	794535	85175	100,000	100,000	N/A	523	N/A	1,026	

Creator
Reviewer
Approver

Chromatogram

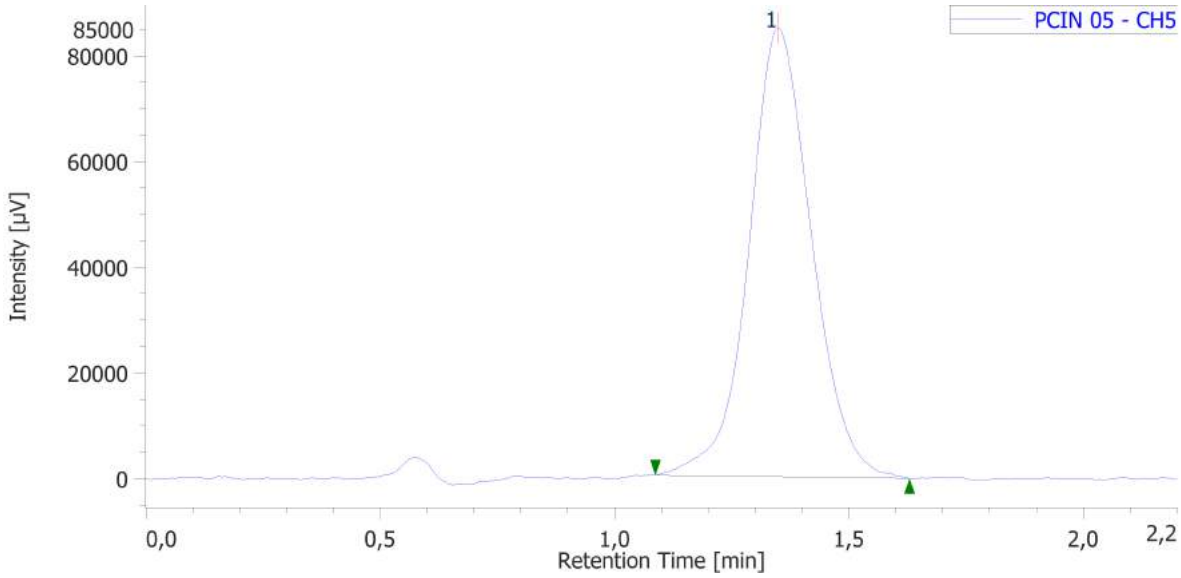

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:39
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:39:46
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH5
Sample Name	PCIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,348	788373	84811	100,000	100,000	N/A	520	N/A	1,031	

Creator QPackSA
Reviewer
Approver

Chromatogram

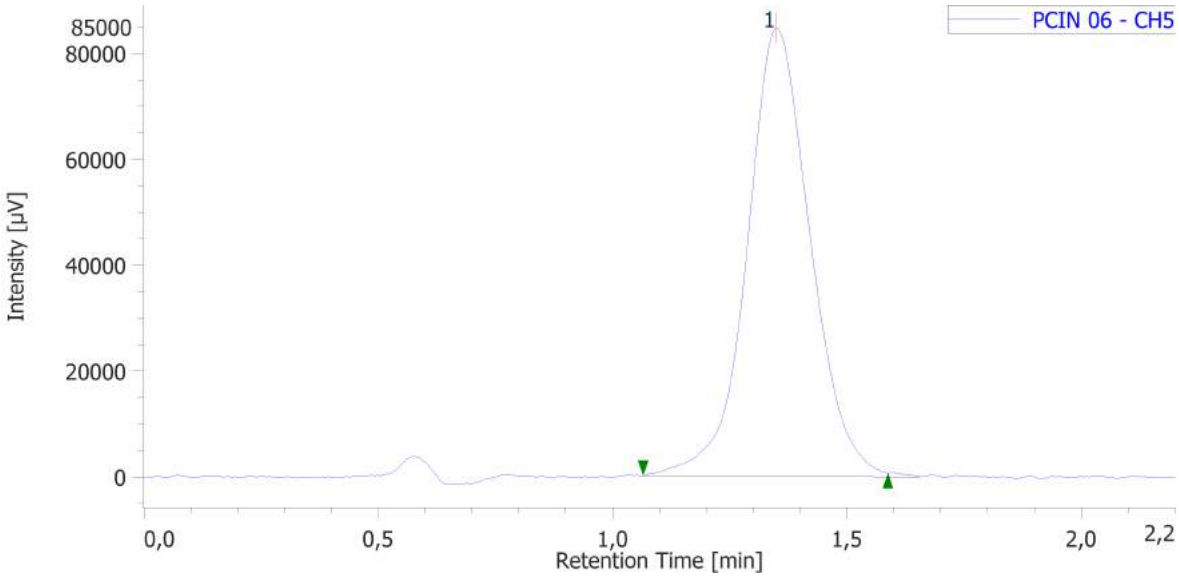

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:39
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:42:47
Volume	10,0 [µL]
Sample #	103
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH5
Sample Name	PCIN 06
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,348	792795	84584	100,000	100,000	N/A	516	N/A	1,042	

Creator QPackSA
Reviewer
Approver

Chromatogram

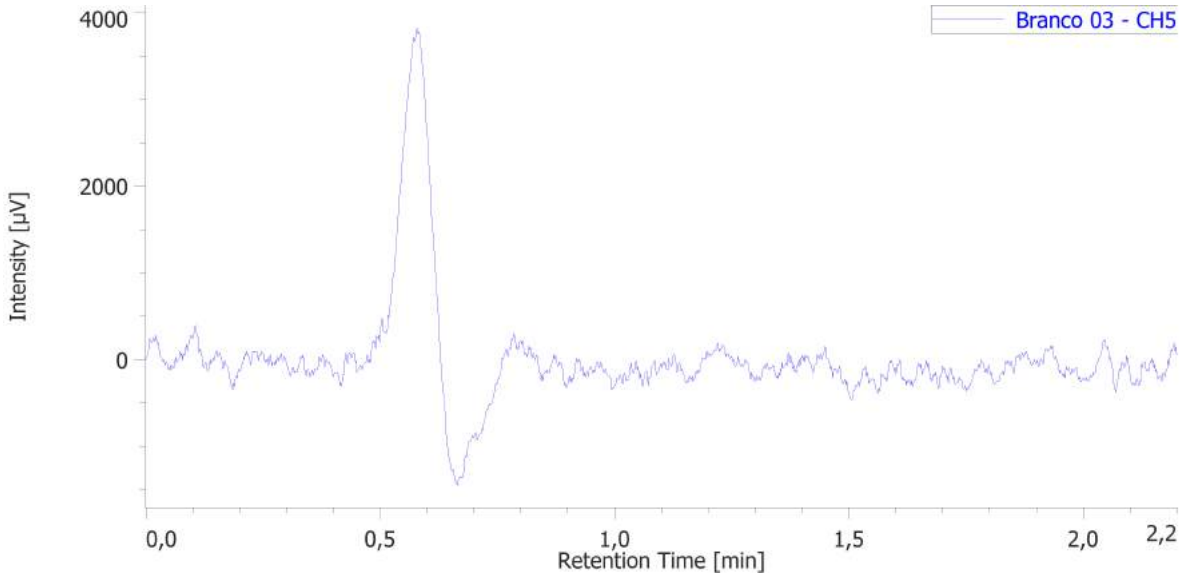


Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:43:40
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 11:45:49
Volume	10,0 [µL]
Sample #	102
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Cafeína
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	Branco 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

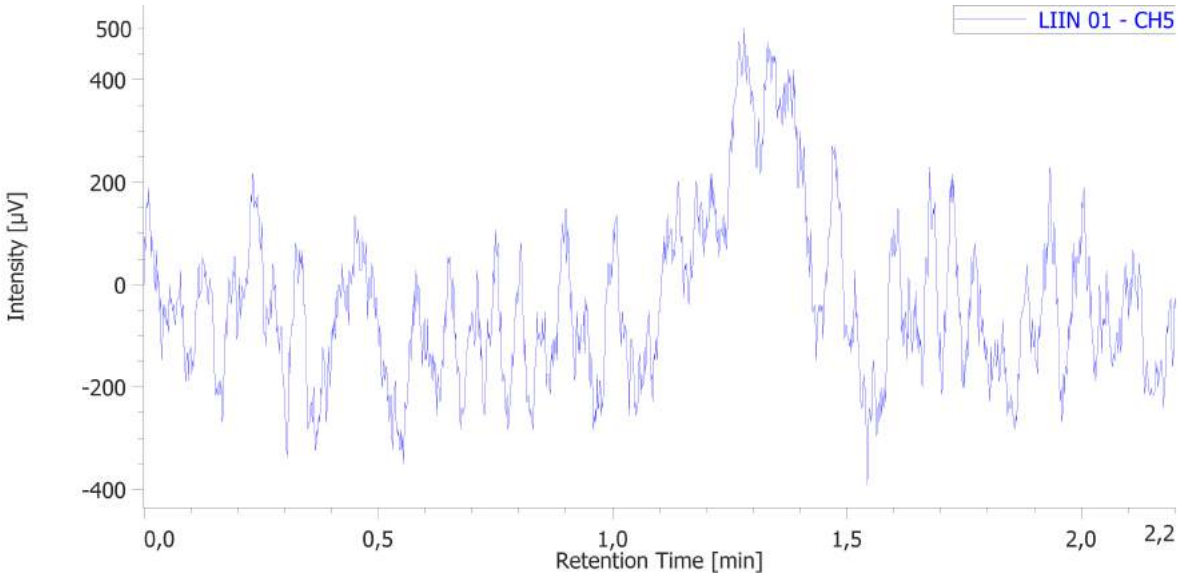


Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:57:15
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 12:03:47
Volume	0,1 [µL]
Sample #	109
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH5
Sample Name	LIIN 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

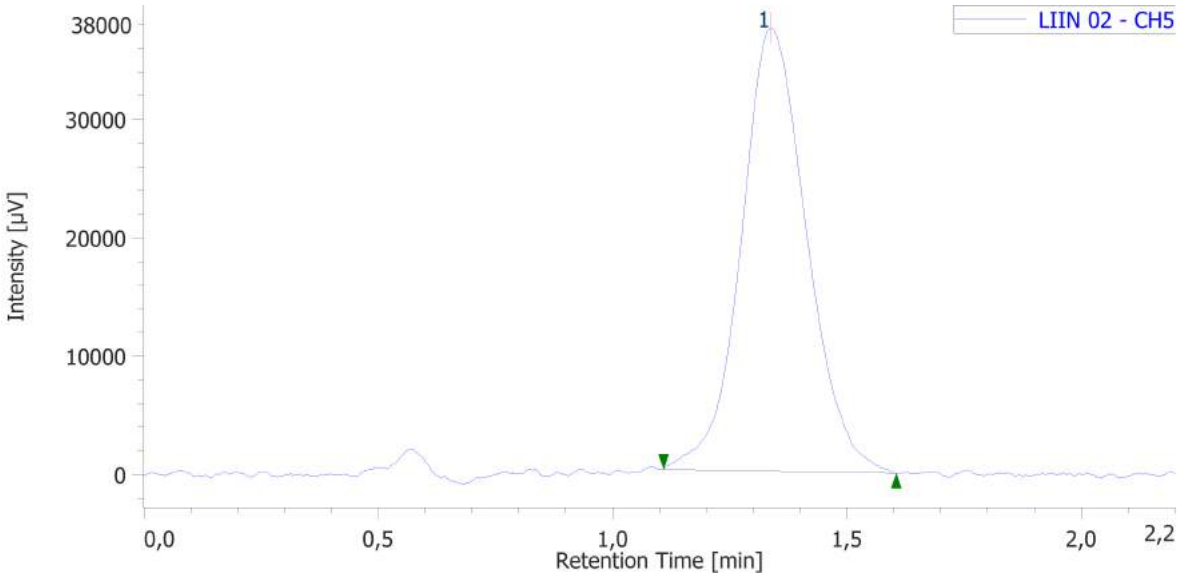

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:57:15
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 12:06:45
Volume	5,0 [µL]
Sample #	109
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH5
Sample Name	LIIN 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,337	363807	37400	100,000	100,000	N/A	463	N/A	1,086	

Creator QPackSA
Reviewer
Approver

Chromatogram

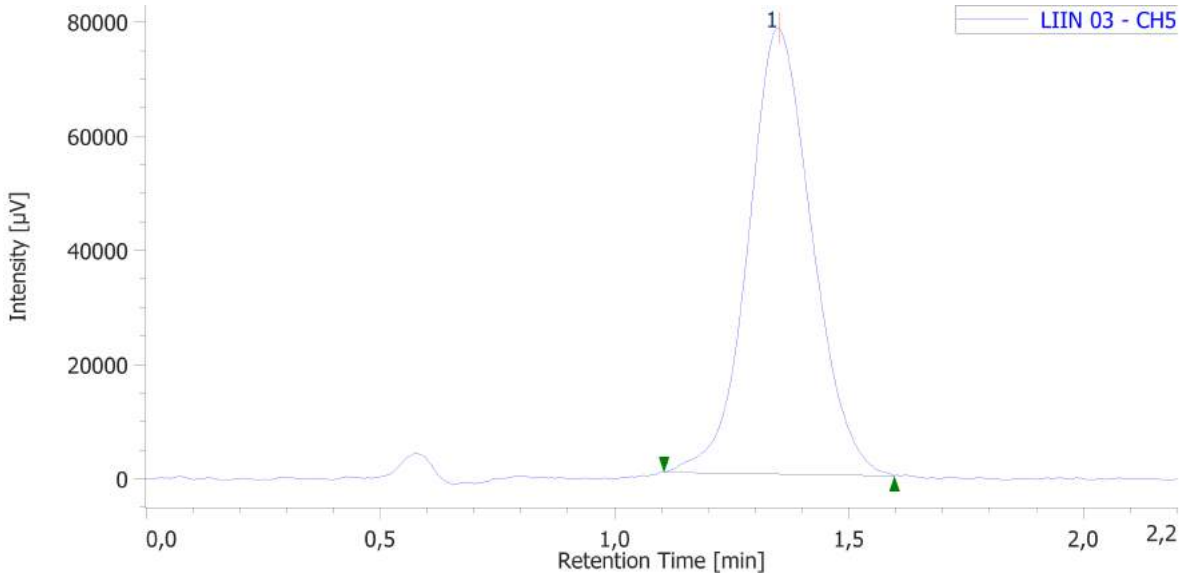

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:57:15
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 12:09:47
Volume	10,0 [µL]
Sample #	109
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH5
Sample Name	LIIN 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,350	739457	78079	100,000	100,000	N/A	490	N/A	1,053	

Creator QPackSA
Reviewer
Approver

Chromatogram

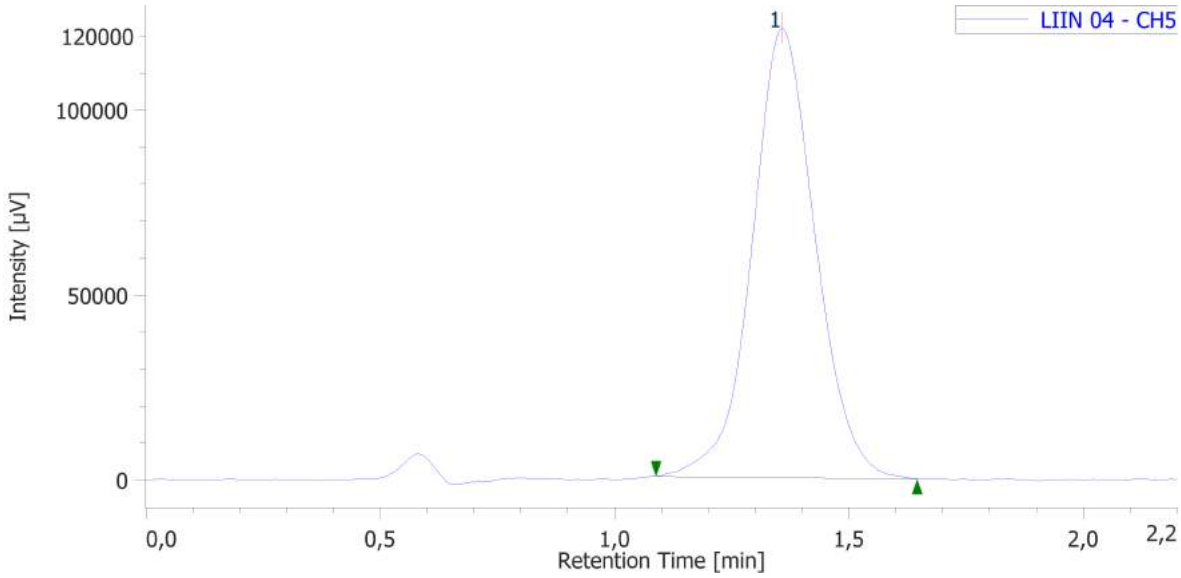

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:57:15
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 12:12:52
Volume	15,0 [µL]
Sample #	109
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH5
Sample Name	LIIN 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,357	1140715	121430	100,000	100,000	N/A	513	N/A	1,028	

Creator QPackSA
Reviewer
Approver

Chromatogram

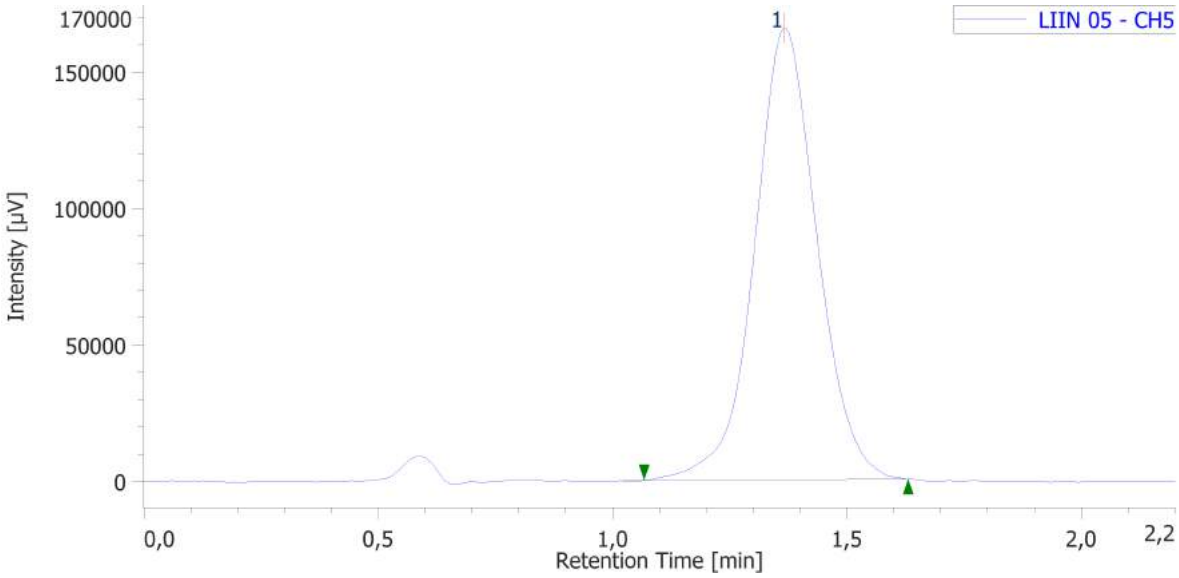

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 13:57:15
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 12:15:57
Volume	20,0 [µL]
Sample #	109
Project Name	Qualificação
Acquisition Time	2,2 [min]
Acquisition Sequence	QUALIFICAÇÃO 2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH5
Sample Name	LIIN 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,365	1537650	165365	100,000	100,000	N/A	534	N/A	1,019	

Creator QPackSA
Reviewer
Approver

Chromatogram

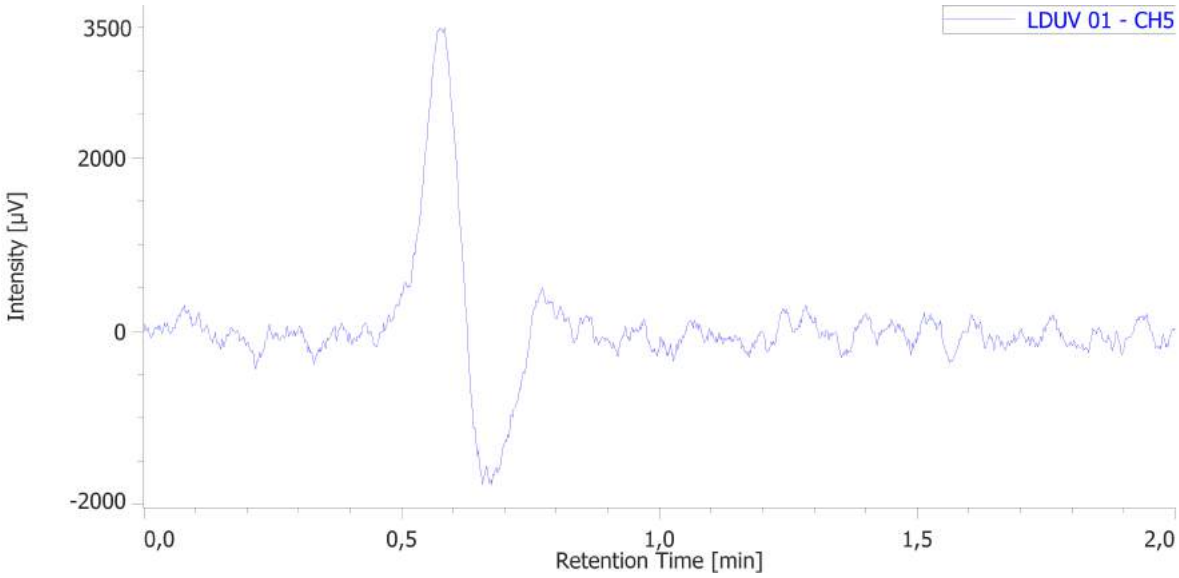


Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 14:35:58
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 14:33:55
Volume	10,0 [µL]
Sample #	104
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	LDUV 01
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

Creator
Reviewer
Approver

Chromatogram

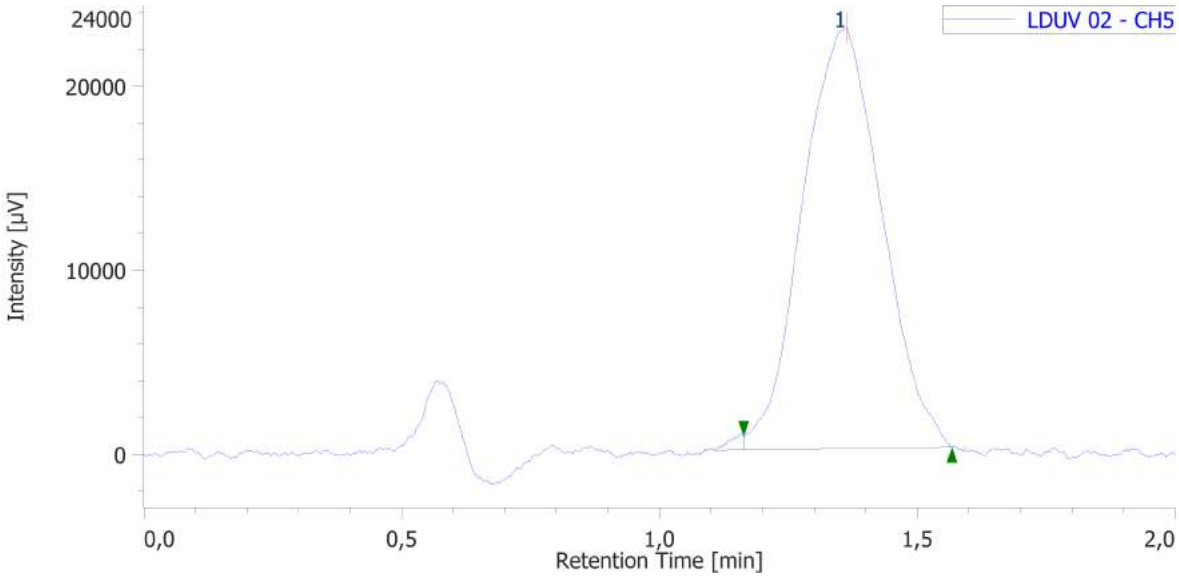

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 14:38:46
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 14:36:44
Volume	10,0 [µL]
Sample #	105
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	LDUV 02
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,363	244384	22824	100,000	100,000	N/A	346	N/A	0,980	

Creator
Reviewer
Approver

Chromatogram

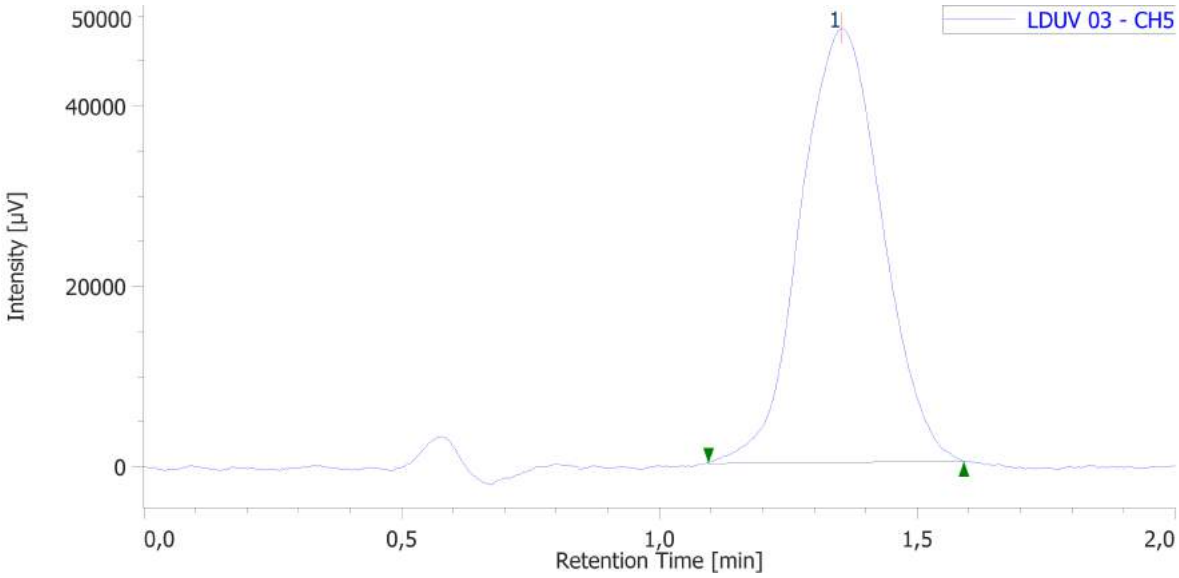

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 14:41:34
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 14:39:32
Volume	10,0 [µL]
Sample #	106
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	LDUV 03
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,353	528221	48131	100,000	100,000	N/A	336	N/A	1,007	

Creator
Reviewer
Approver

Chromatogram

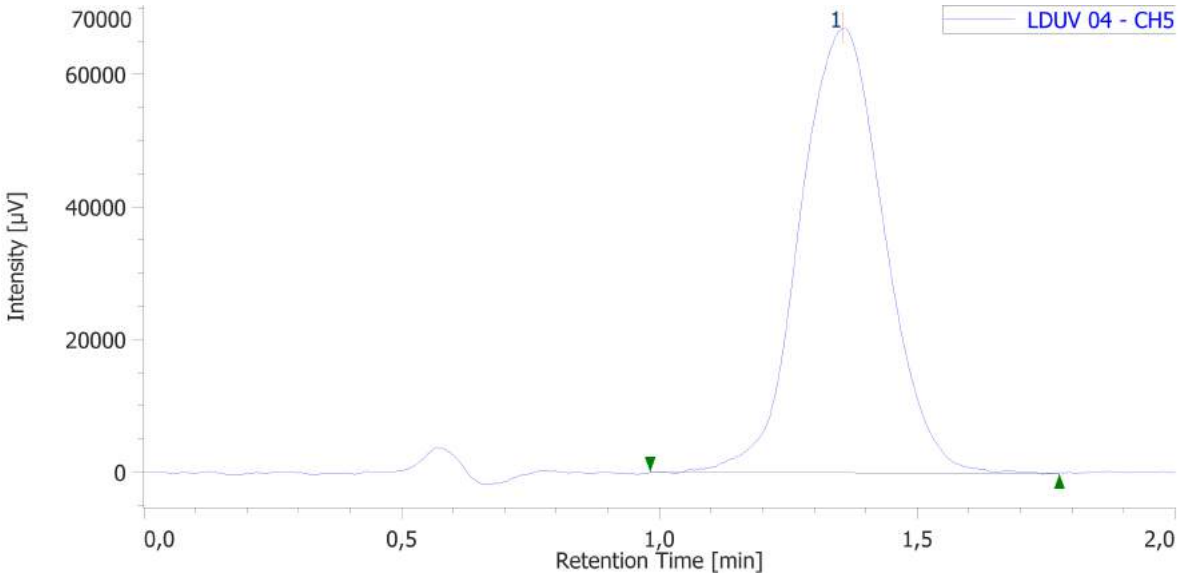

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 14:44:22
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 14:42:21
Volume	10,0 [µL]
Sample #	107
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	LDUV 04
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,355	764103	67029	100,000	100,000	N/A	321	N/A	1,016	

Creator
Reviewer
Approver

Chromatogram

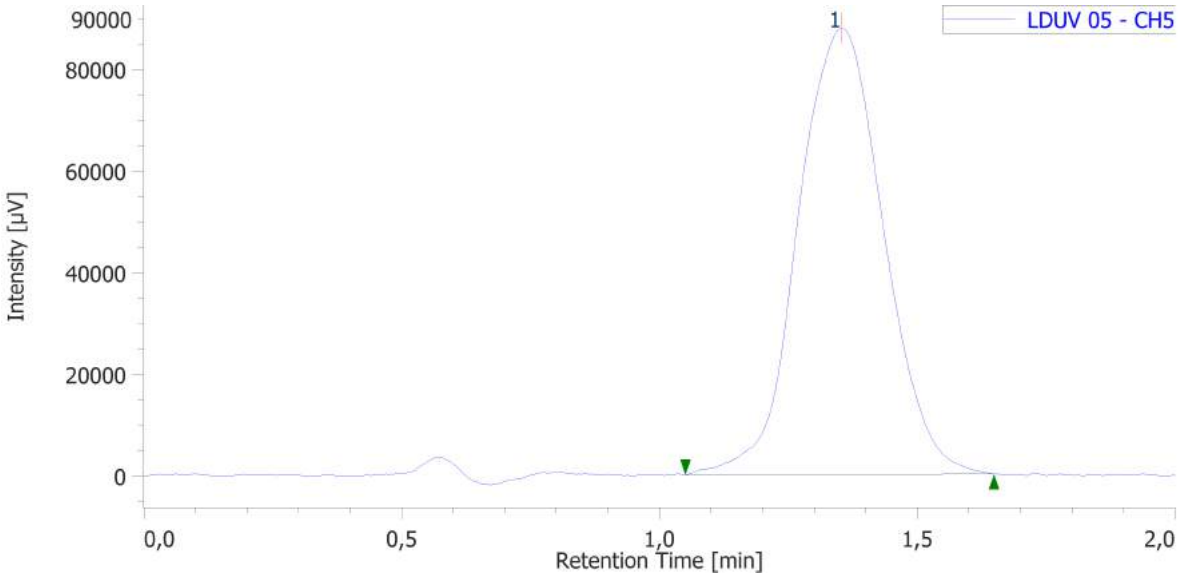

Chromatogram Information	
User Name	QPackSA
Date Modified	01/08/2022 14:47:14
Description	
HPLC System Name	HPL 09_PDA
Injection Date	01/08/2022 14:45:11
Volume	10,0 [µL]
Sample #	108
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	LDUV 05
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína_Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,353	1012490	87844	100,000	100,000	N/A	312	N/A	1,006	

Creator
Reviewer
Approver

Chromatogram

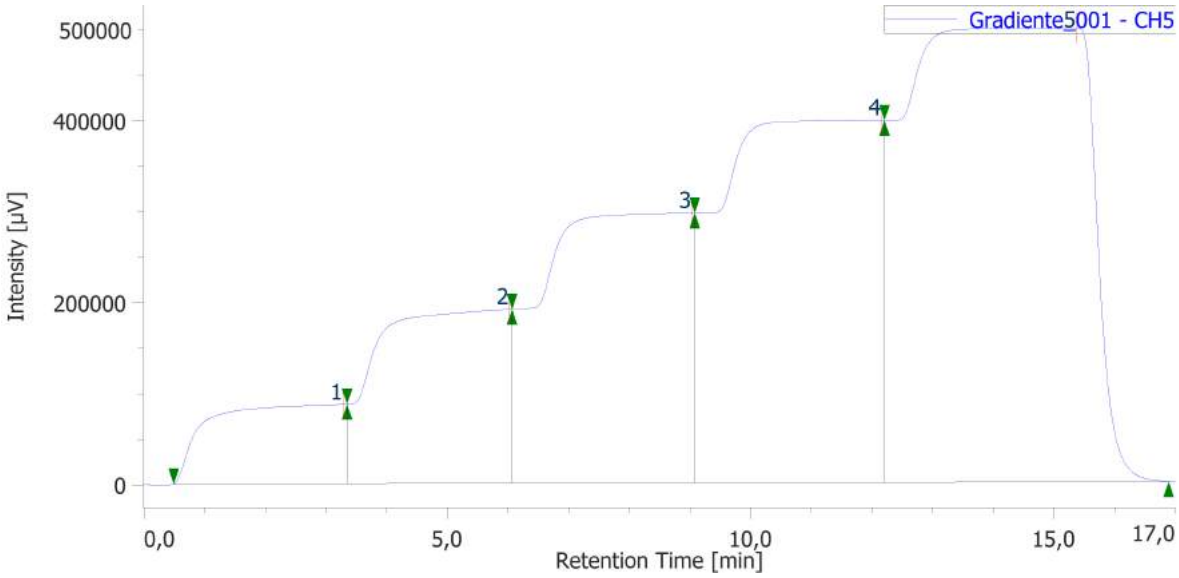

Chromatogram Information	
User Name	Administrator
Date Modified	01/08/2022 16:54:34
Description	
HPLC System Name	HPL 09
Injection Date	01/08/2022 16:37:33
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	17,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,283	12744137	99803	4,847	5,905	N/A	N/A	N/A	N/A	
2	Unknown	5	6,023	27818598	198830	10,580	12,983	N/A	N/A	N/A	N/A	
3	Unknown	5	9,033	48863726	296292	18,584	20,157	N/A	N/A	N/A	N/A	
4	Unknown	5	12,157	70277138	397670	26,728	27,054	N/A	N/A	N/A	N/A	
5	Unknown	5	15,370	103231092	498294	39,261	33,900	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

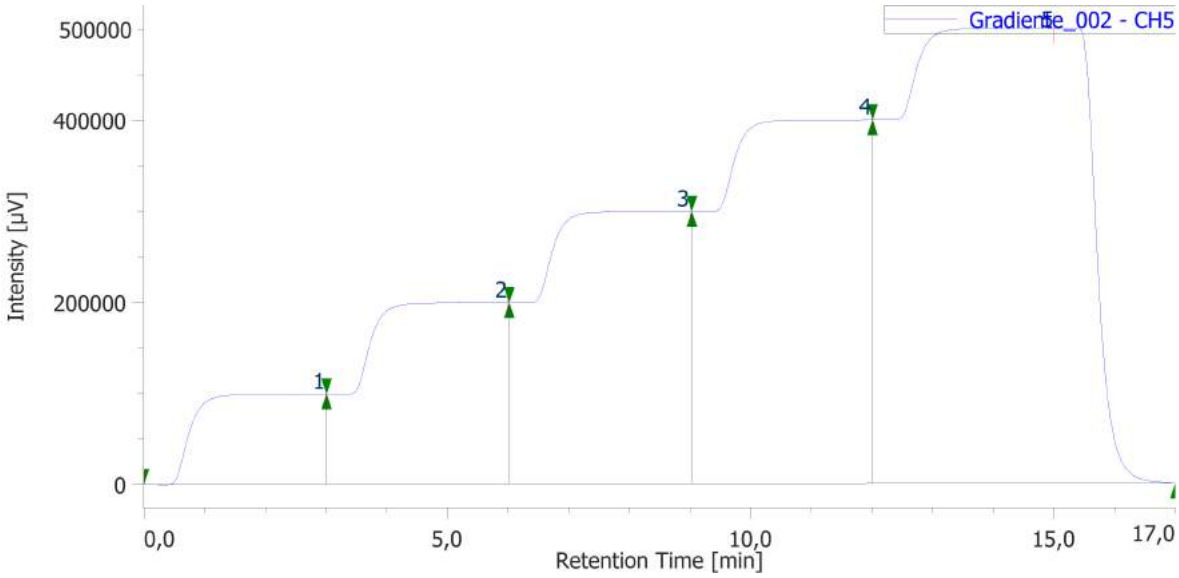

Chromatogram Information	
User Name	Administrator
Date Modified	01/08/2022 17:22:48
Description	
HPLC System Name	HPL 09
Injection Date	01/08/2022 16:55:30
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	17,0 [min]
Acquisition Sequence	
Control Method	Gradiente AC
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	5	3,000	13414654	99138	4,981	6,627	N/A	N/A	N/A	N/A	
2	40%	5	6,000	31548653	199209	11,714	13,317	N/A	N/A	N/A	N/A	
3	60%	5	9,000	49672441	299064	18,444	19,992	N/A	N/A	N/A	N/A	
4	80%	5	12,000	67079937	399201	24,908	26,685	N/A	N/A	N/A	N/A	
5	100%	5	15,000	107600063	499339	39,953	33,379	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver