
Peak Find - Nivel De Energia.jws

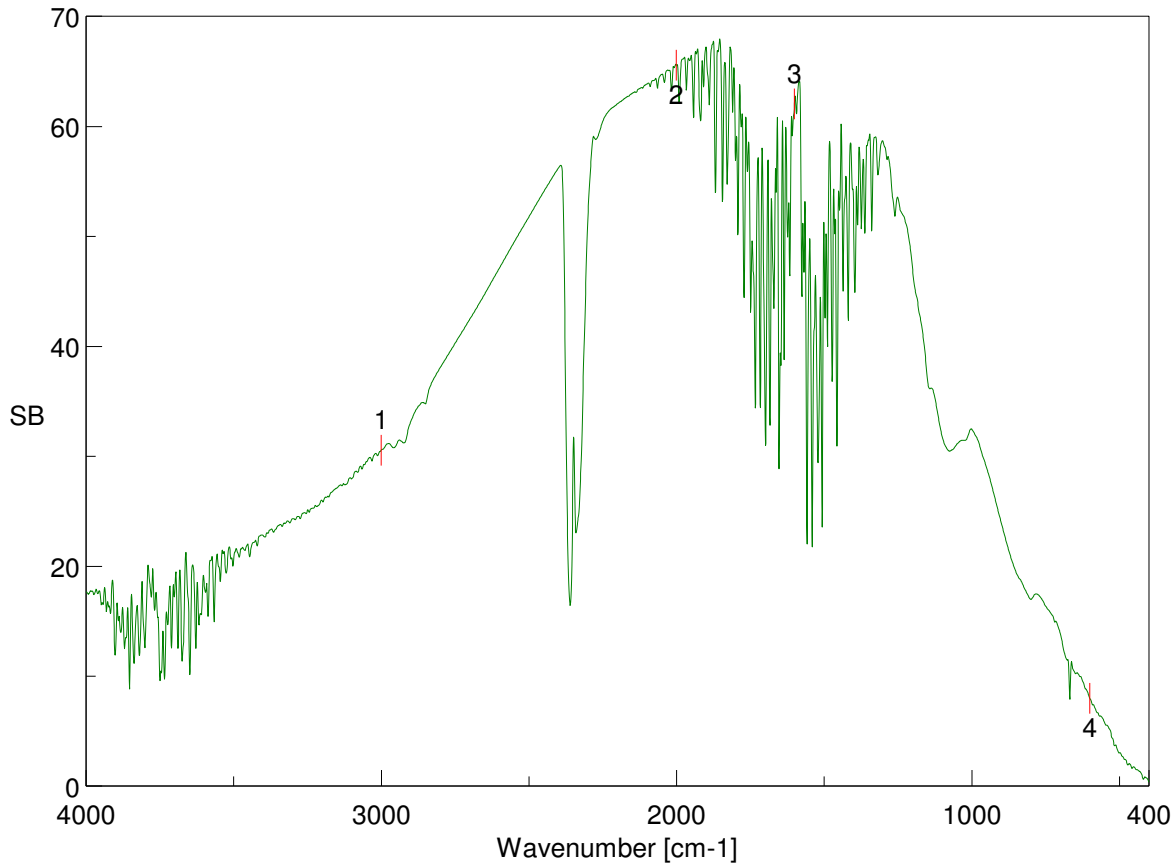

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 11:48 AM
Date modified	6/12/2023 11:51 AM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	SB
Start	399.193 cm-1
End	4000.6 cm-1
Data interval	0.964233 cm-1
Data points	3736

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 11:46 AM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	4 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (1)
Aperture	Auto (7.1 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	3000.69	30.5365	2	2000.78	65.5572
3	1600.63	62.0378	4	600.717	7.97479

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Exatidao Do Numero De Onda.jws

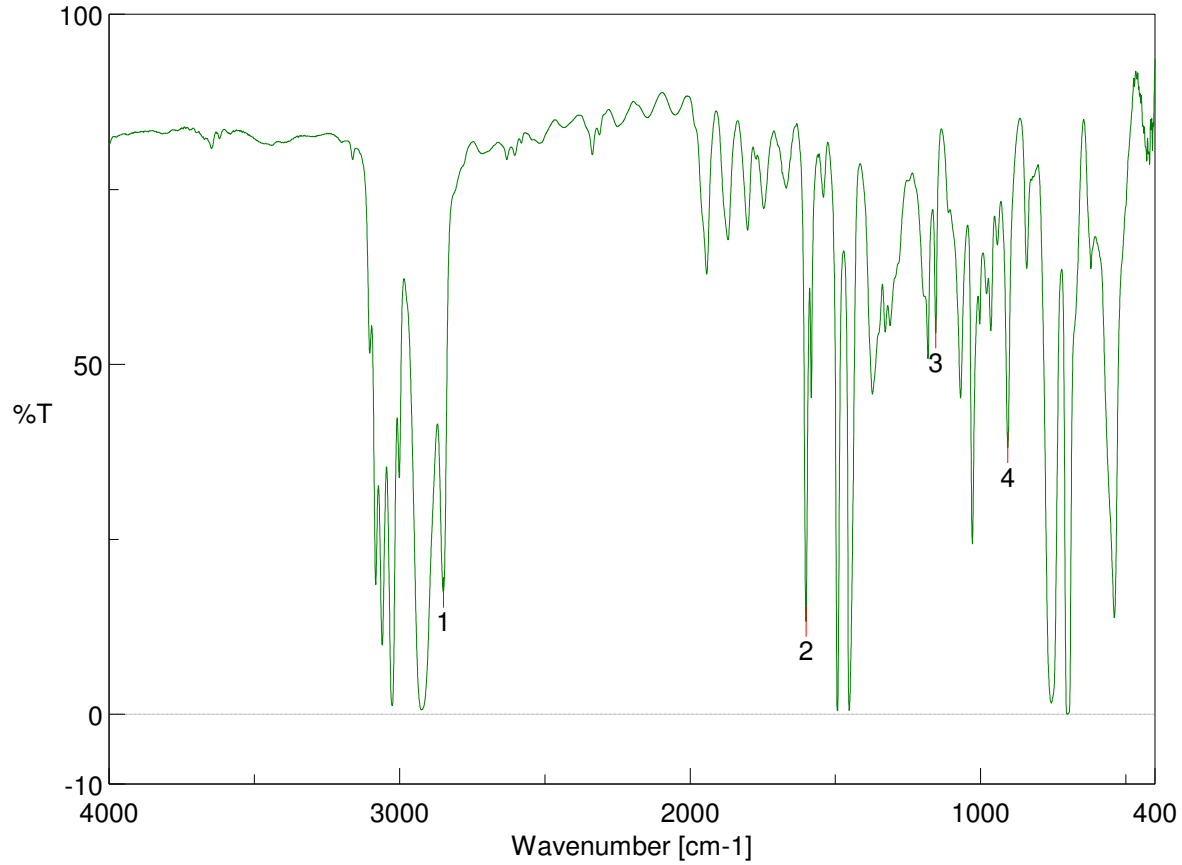

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 11:56 AM
Date modified	6/12/2023 11:57 AM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 11:54 AM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2849.31	17.3942	2	1601.11	13.236
3	1154.67	54.4344	4	906.379	38.0662

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Resolucao.jws

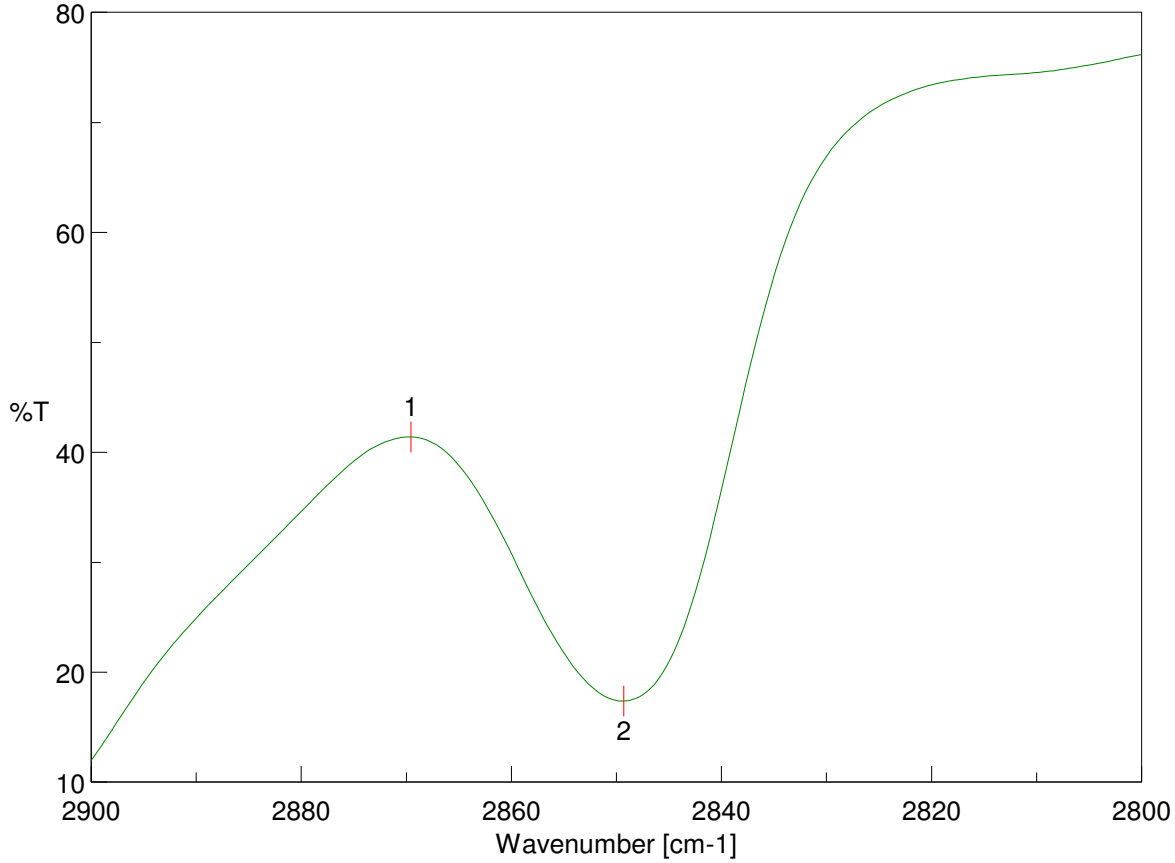

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 11:59 AM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 11:59 AM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2869.56	41.382	2	2849.31	17.3546

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Resolucao.jws

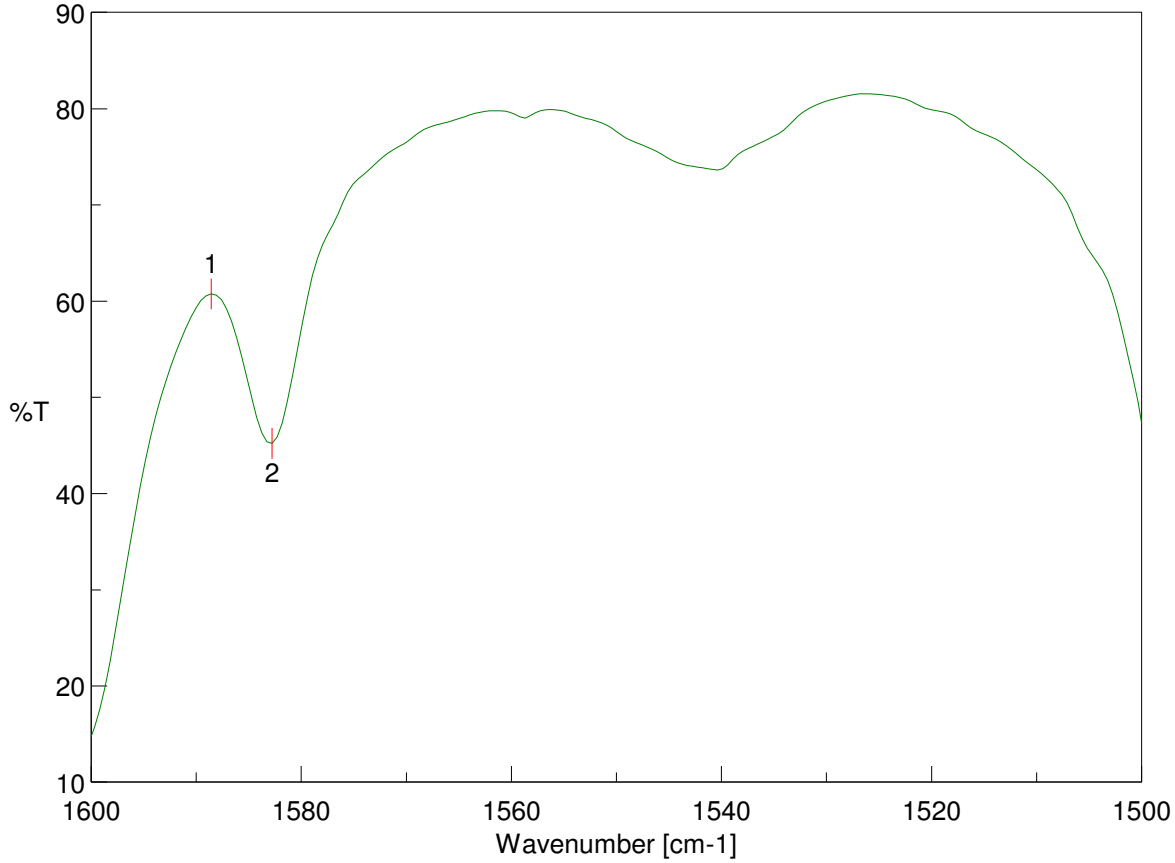

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 11:59 AM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 11:59 AM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	1588.57	60.7414	2	1582.79	45.1781

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Repetibilidade Do Numero De Onda - Rep. 1.jws

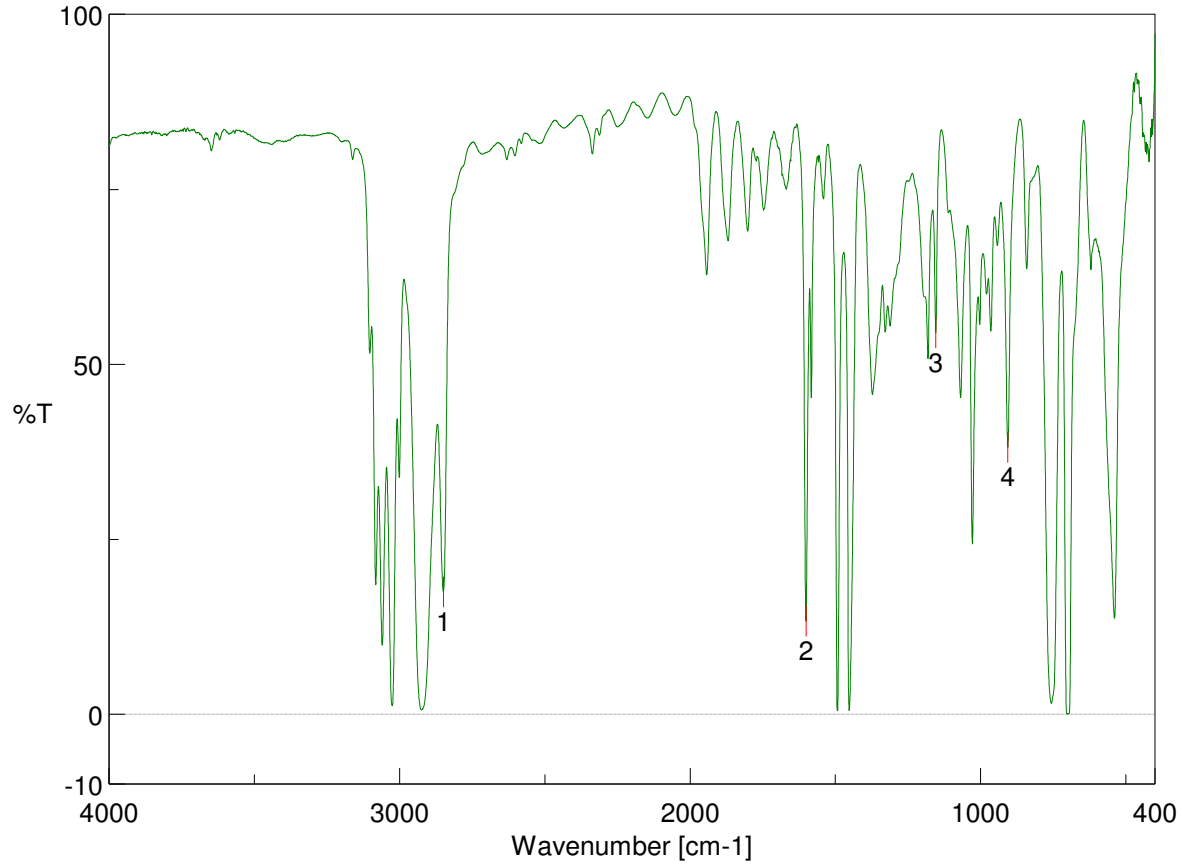

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:04 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 12:03 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2849.31	17.4495	2	1601.11	13.3034
3	1154.67	54.4845	4	906.379	38.1044

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Repetibilidade Do Numero De Onda - Rep. 2.jws

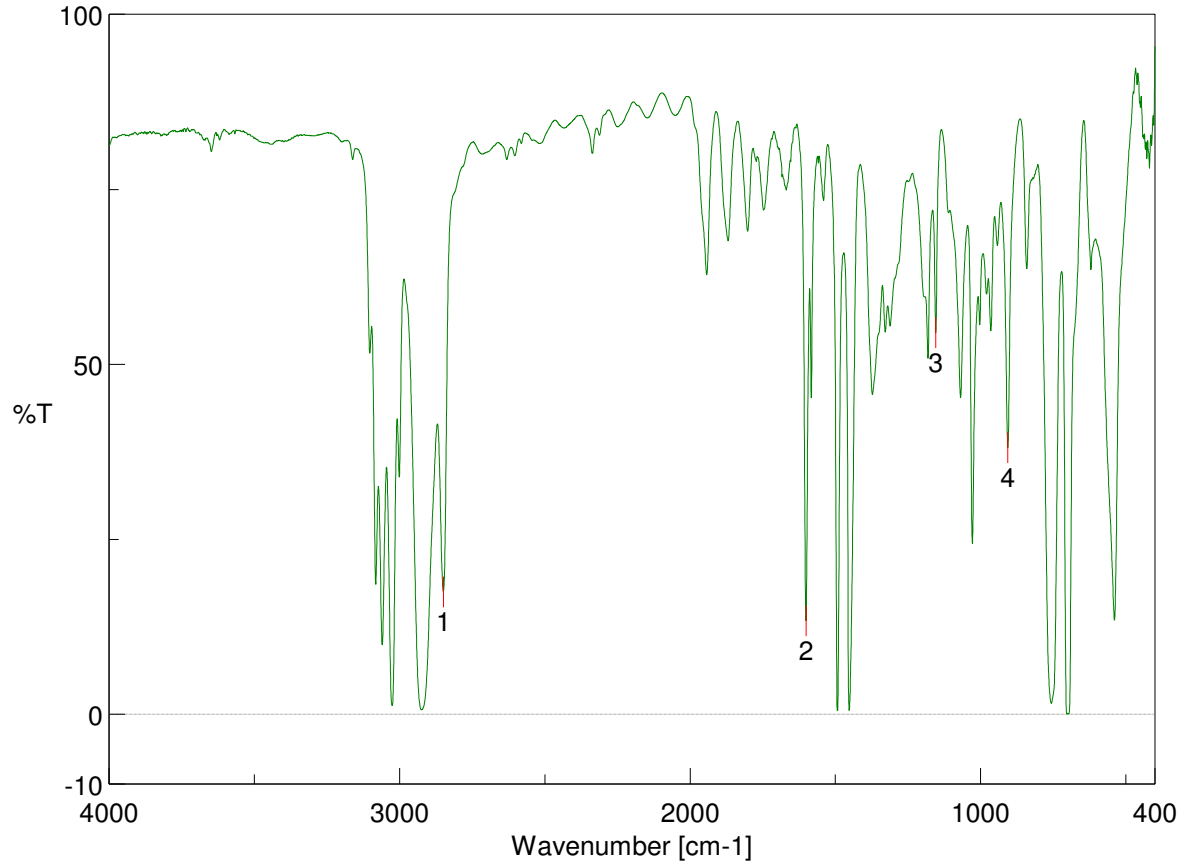

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:05 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 12:04 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2849.31	17.4518	2	1601.11	13.3037
3	1154.67	54.4928	4	906.379	38.0748

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Repetibilidade Fotometrica - Rep. 1.jws

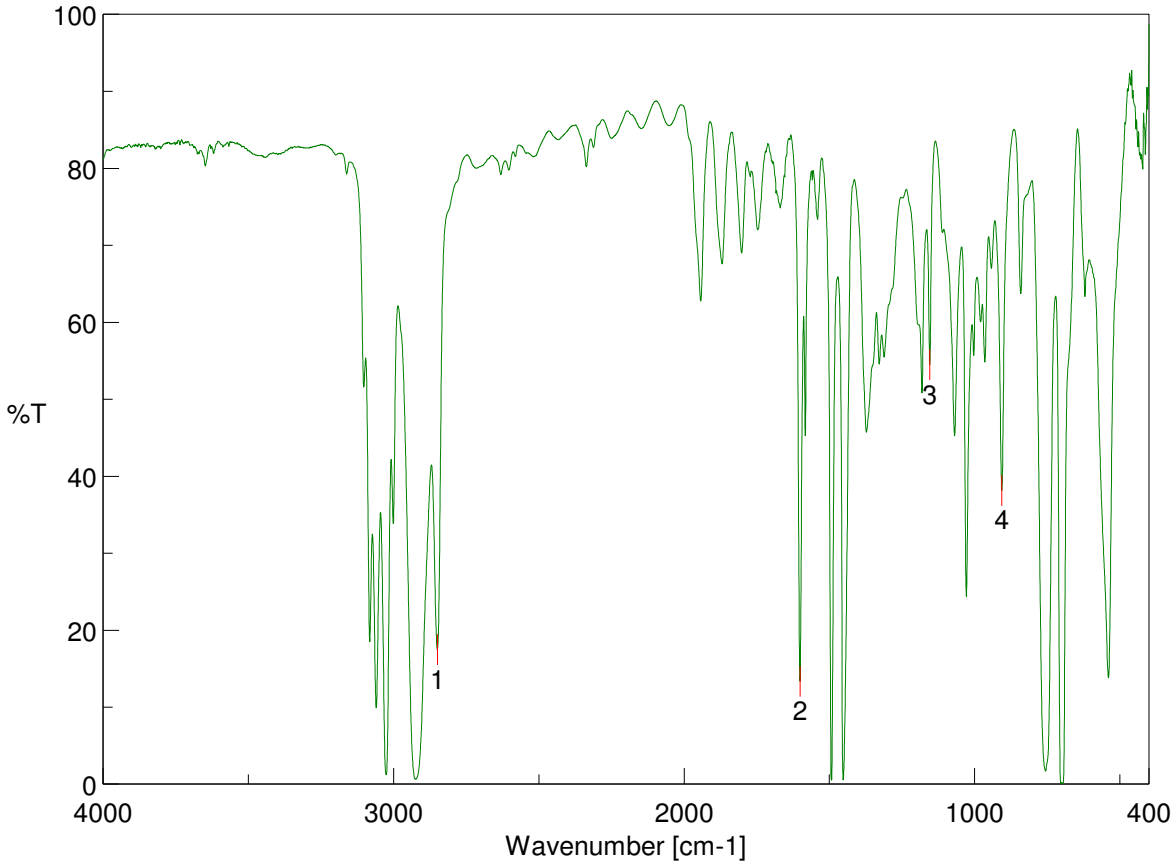

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:09 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 12:09 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2849.31	17.4469	2	1601.11	13.341
3	1154.67	54.4874	4	906.379	38.1311

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Repetibilidade Fotometrica - Rep. 2.jws

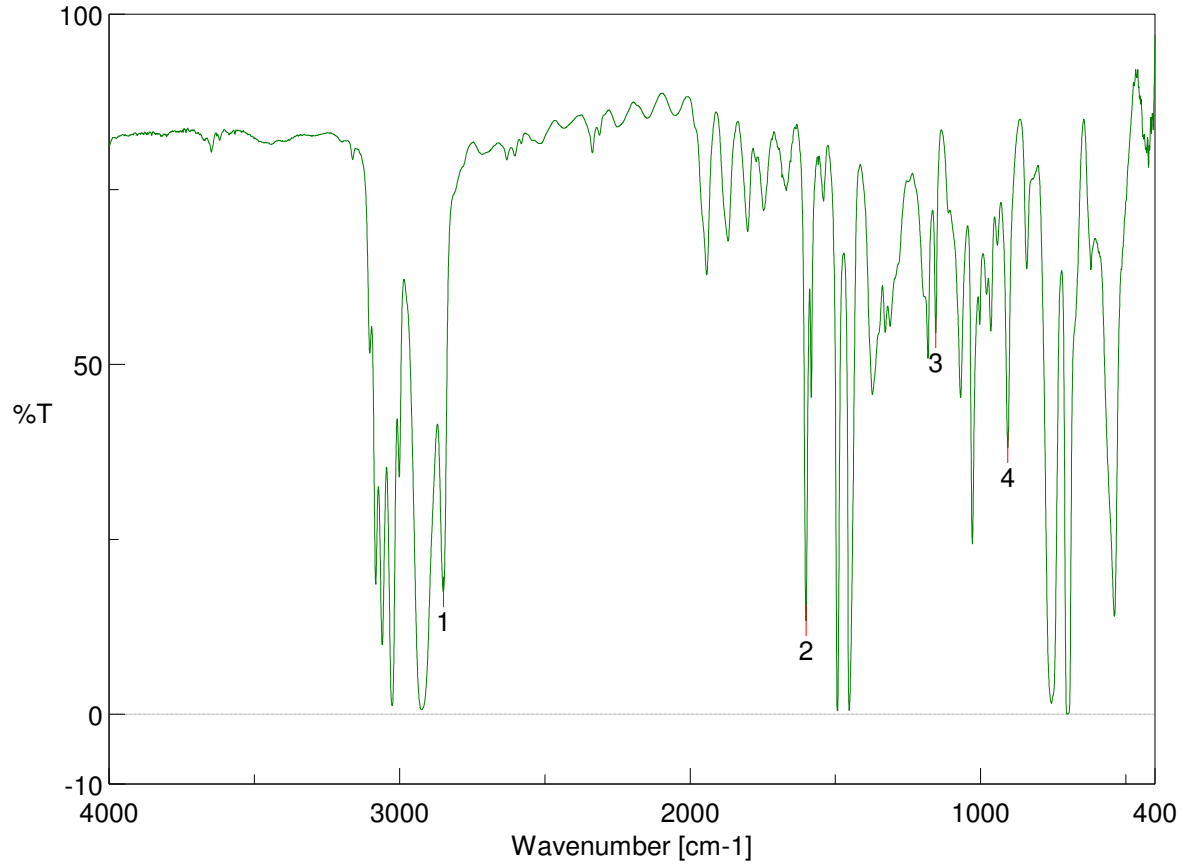

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:10 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.675 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7469

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 12:10 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (2)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2849.31	17.4376	2	1601.11	13.316
3	1154.67	54.4957	4	906.379	38.09

Creation	QPack Soluções Analíticas
Review	
Approval	

Peak Find - Sensibilidade.jws

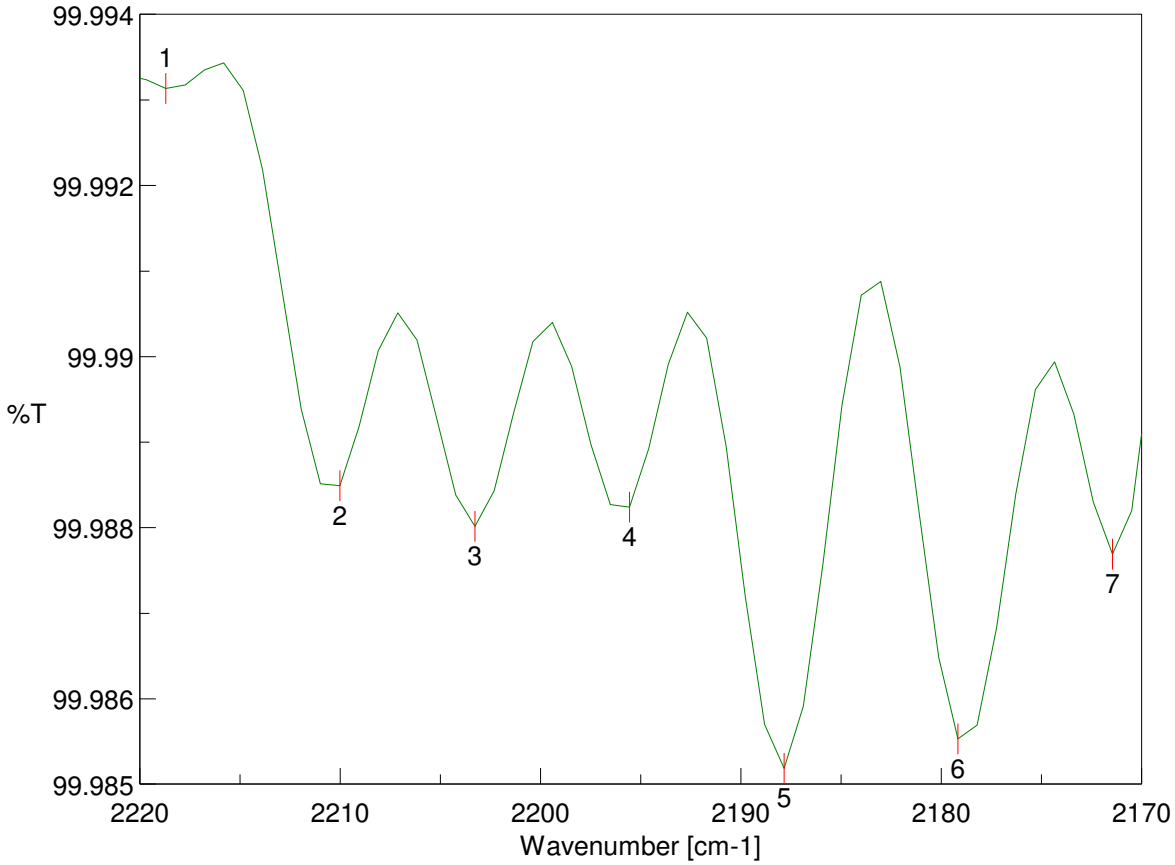

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:21 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	399.193 cm-1
End	4000.6 cm-1
Data interval	0.964233 cm-1
Data points	3736

[Measurement Information]

Model Name	FT/IR-4600typeA
Serial Number	D055461786
Measurement Date	6/12/2023 12:20 PM
Light Source	Standard
Detector	TGS
Accumulation	48
Resolution	4 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (1)
Aperture	Auto (7.1 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

[Result of Peak Picking]


No.	Position	Intensity	No.	Position	Intensity
1	2218.7	99.9931	2	2210.02	99.9885
3	2203.27	99.988	4	2195.56	99.9882

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
5	2187.85	99.9852	6	2179.17	99.9855
7	2171.45	99.9877			

Peak Find - ATR - Nivel De Energia.jws

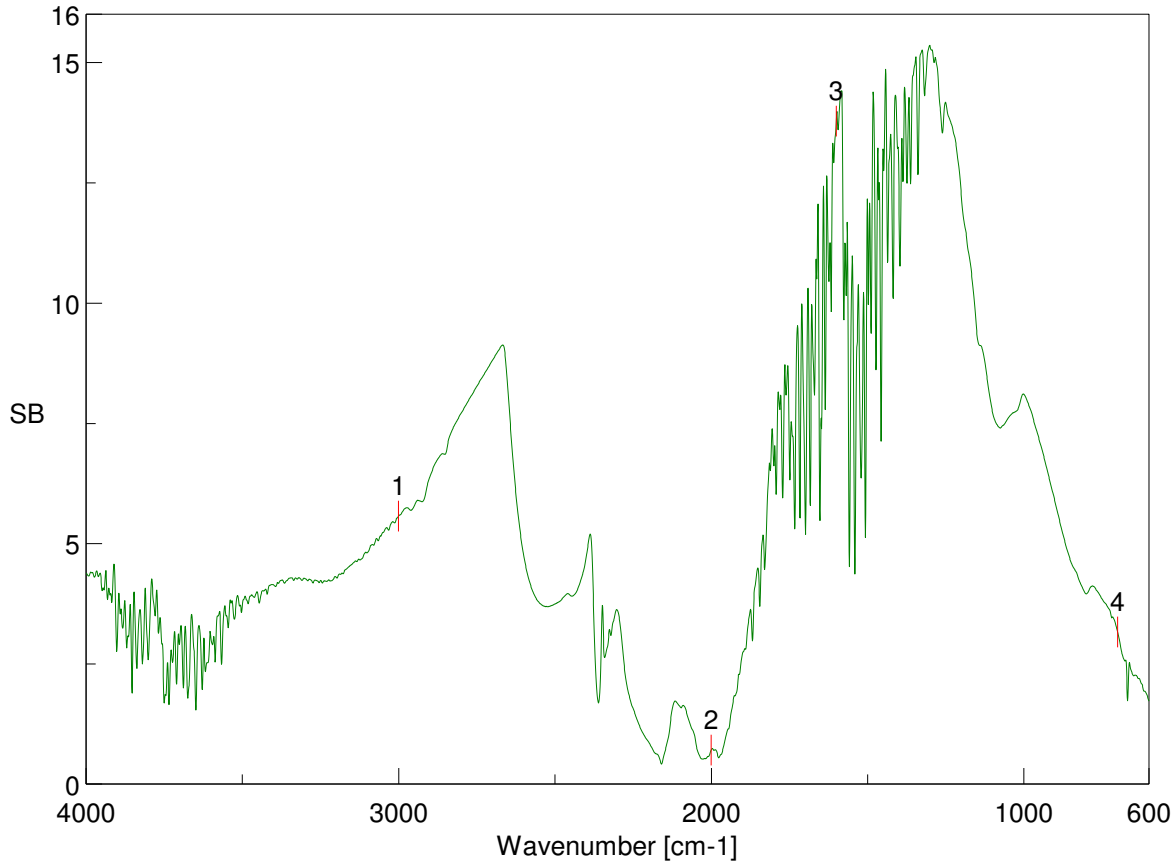

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:31 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	SB
Start	599.753 cm-1
End	4000.6 cm-1
Data interval	0.964233 cm-1
Data points	3528

[Measurement Information]

Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:31 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	4 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (4)
Aperture	Auto (7.1 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)


Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	3000.69	5.56754	2	2000.78	0.704965
3	1600.63	13.7774	4	700.034	3.1632

Creation QPack Soluções Analíticas
Review
Approval

Peak Find - ATR - Exatidao Do Numero De Onda.jws

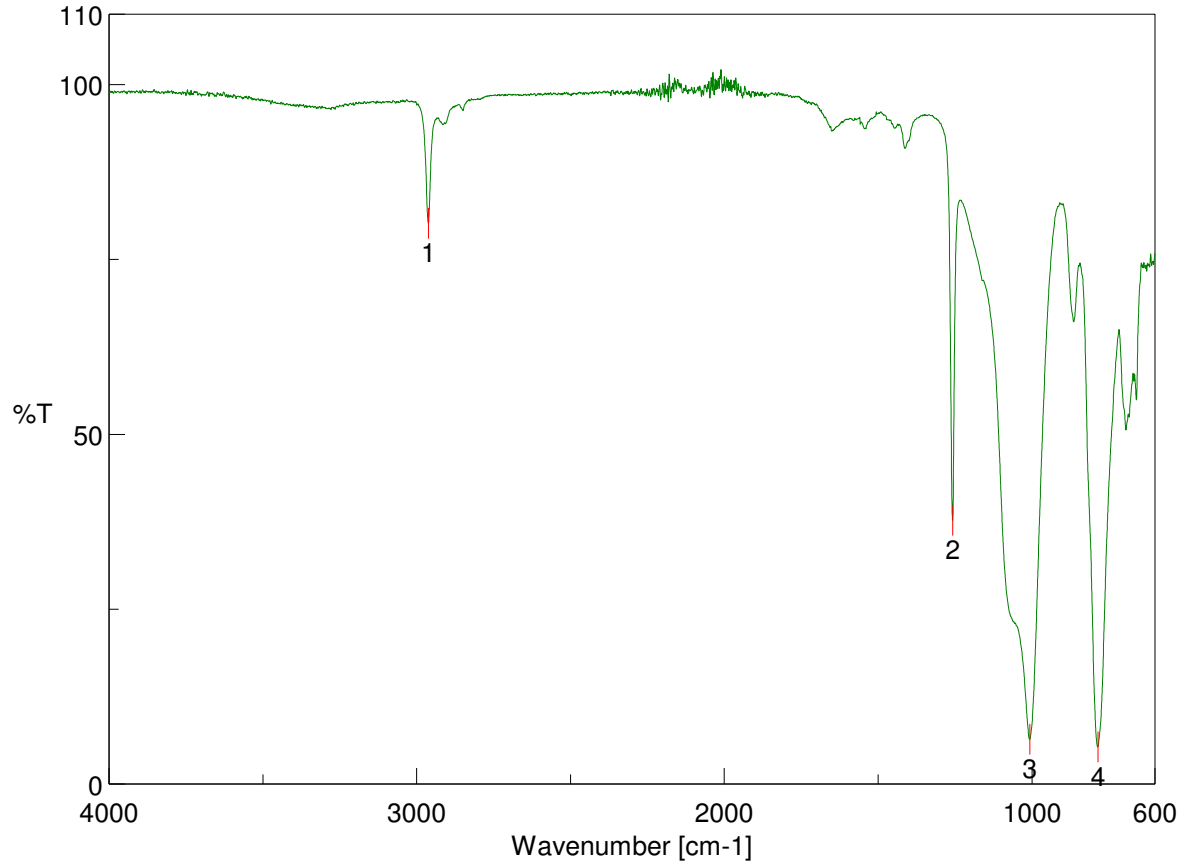

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:38 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:38 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2962.13	80.1265	2	1257.84	37.7058
3	1007.14	6.38771	4	785.368	5.30618

Peak Find - ATR - Resolucao.jws

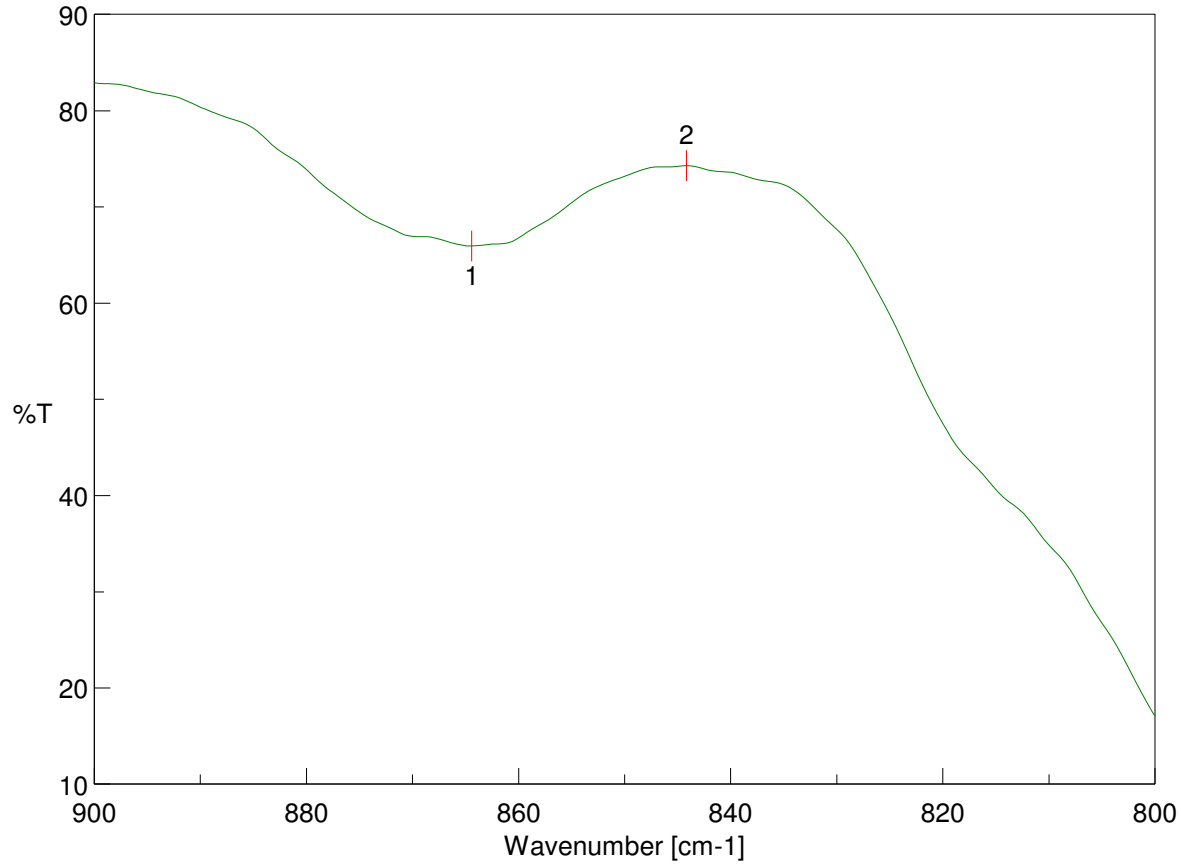

[Comments]

Sample name	
Comment	
User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:42 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:41 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	864.435	65.9046	2	844.186	74.2558

Peak Find - ATR - Repetibilidade Do Numero De Onda - Rep. 1.jws

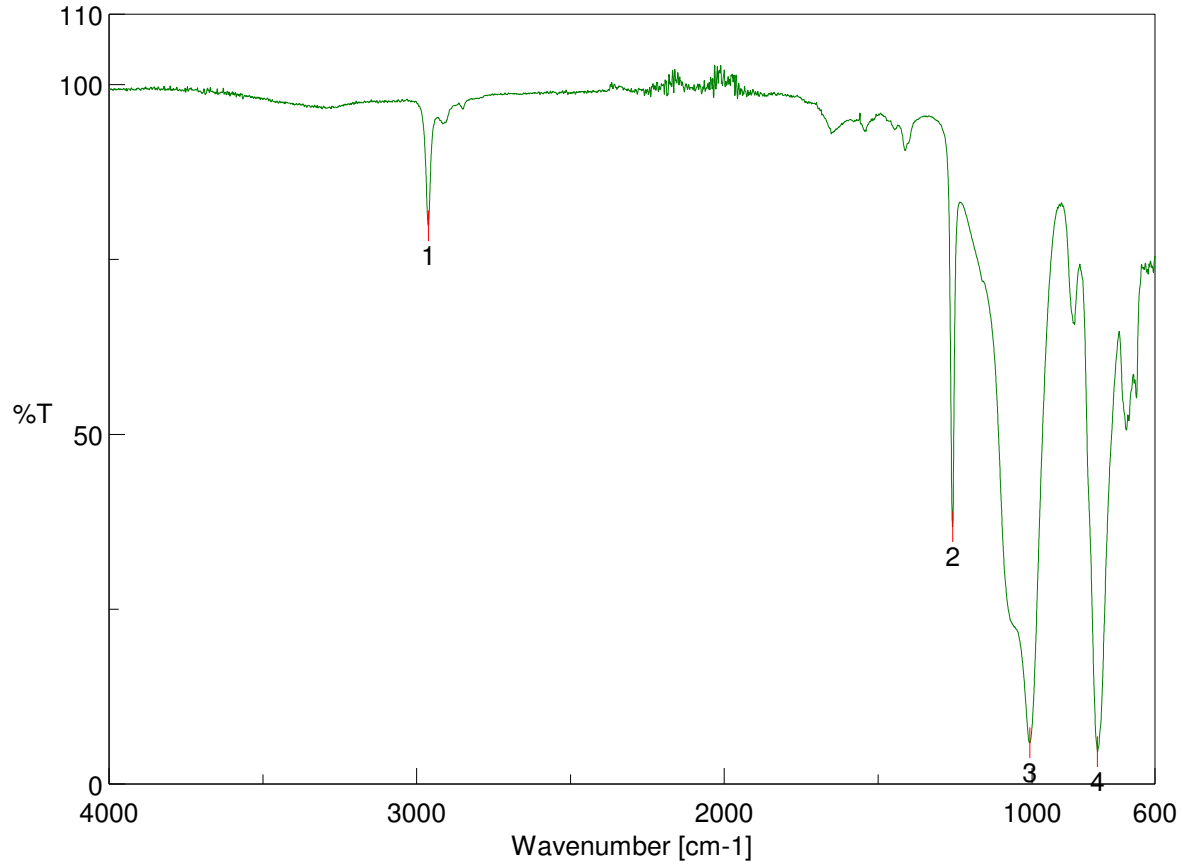

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:47 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:47 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2962.13	79.7474	2	1257.84	36.7538
3	1007.14	5.89205	4	786.815	4.63145

Peak Find - ATR - Repetibilidade Do Numero De Onda - Rep. 2.jws

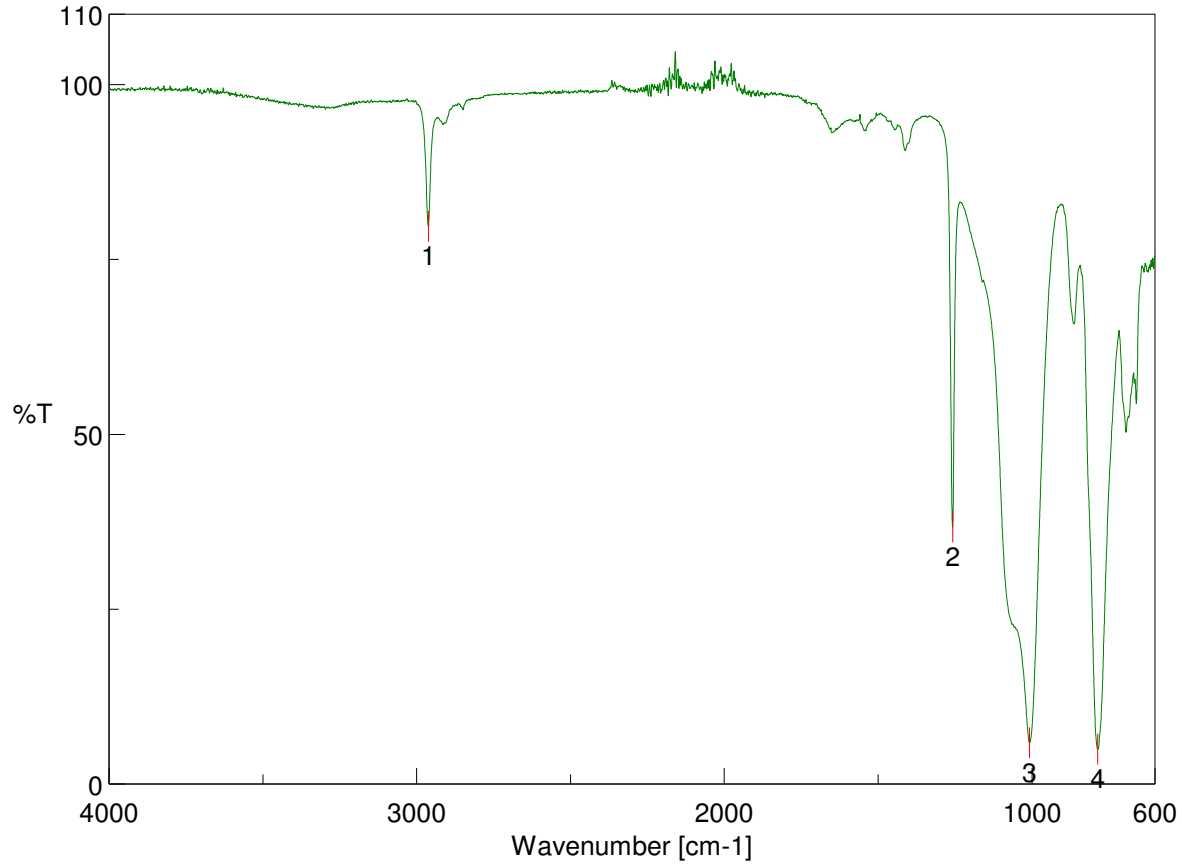

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:49 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:48 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2962.13	79.6576	2	1257.84	36.7127
3	1008.11	5.89333	4	786.332	4.96396

Peak Find - ATR - Repetibilidade Fotometrica - Rep. 1.jws

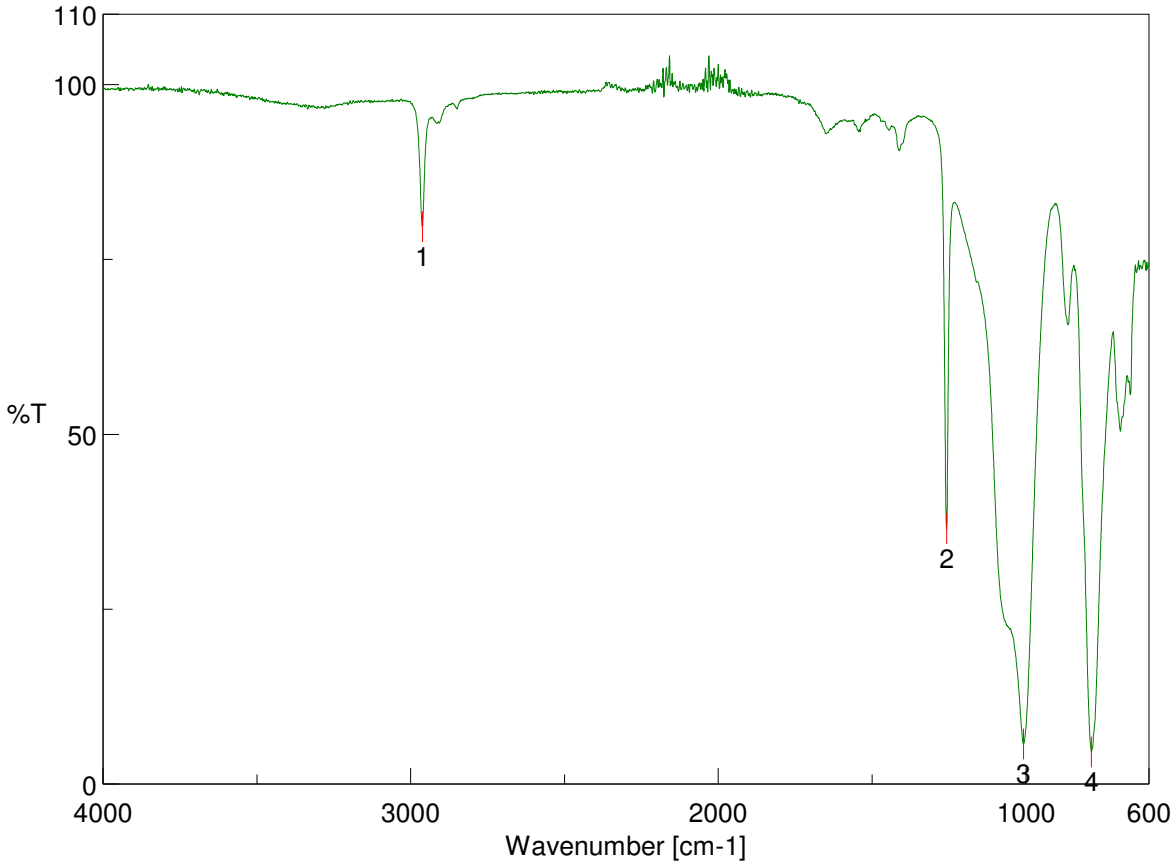

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:53 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:53 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2962.13	79.6502	2	1257.84	36.5075
3	1008.11	5.73814	4	787.297	4.57088

Peak Find - ATR - Repetibilidade Fotometrica - Rep. 2.jws

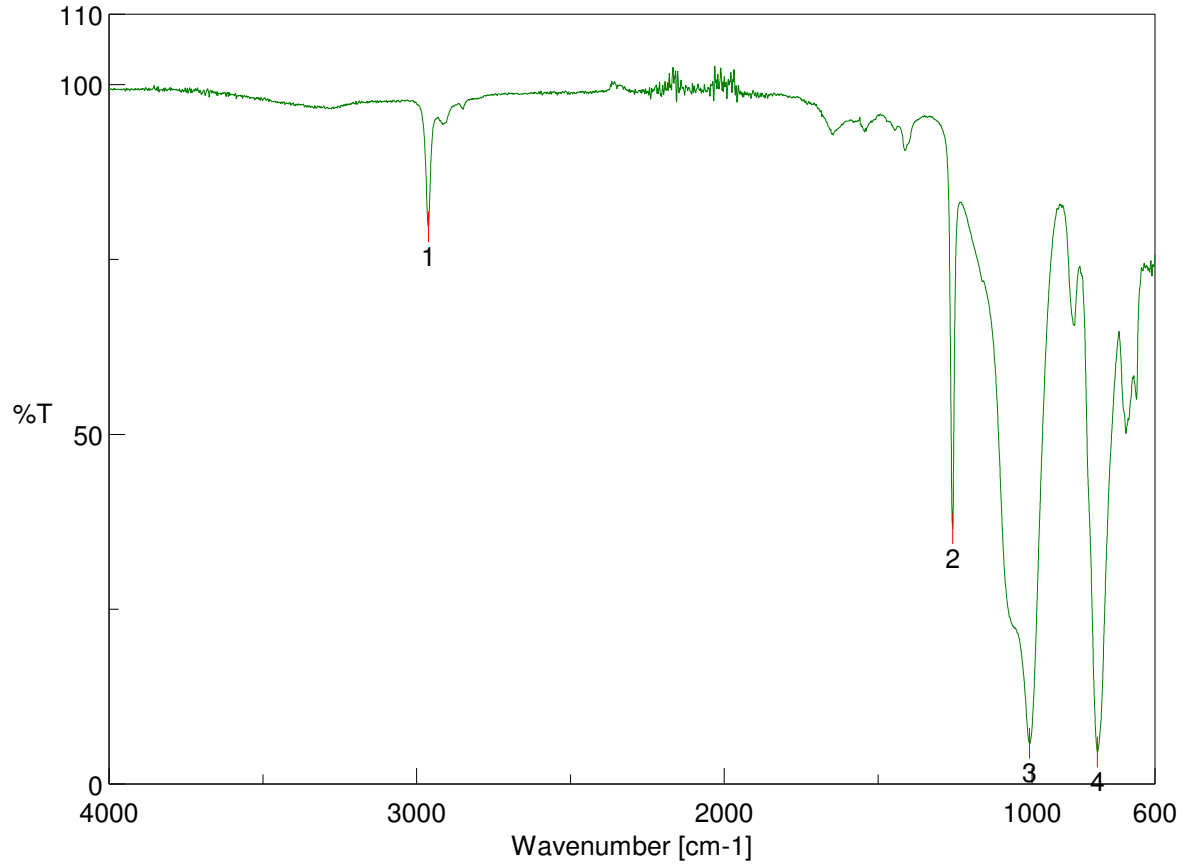

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 12:54 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.12 cm-1
Data interval	0.482117 cm-1
Data points	7054

[Measurement Information]


Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 12:54 PM
Light Source	Standard
Detector	TGS
Accumulation	16
Resolution	2 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (8)
Aperture	Auto (5 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2962.13	79.6115	2	1257.84	36.5056
3	1007.62	5.7901	4	786.815	4.58744

Peak Find - ATR - Sensibilidade.jws

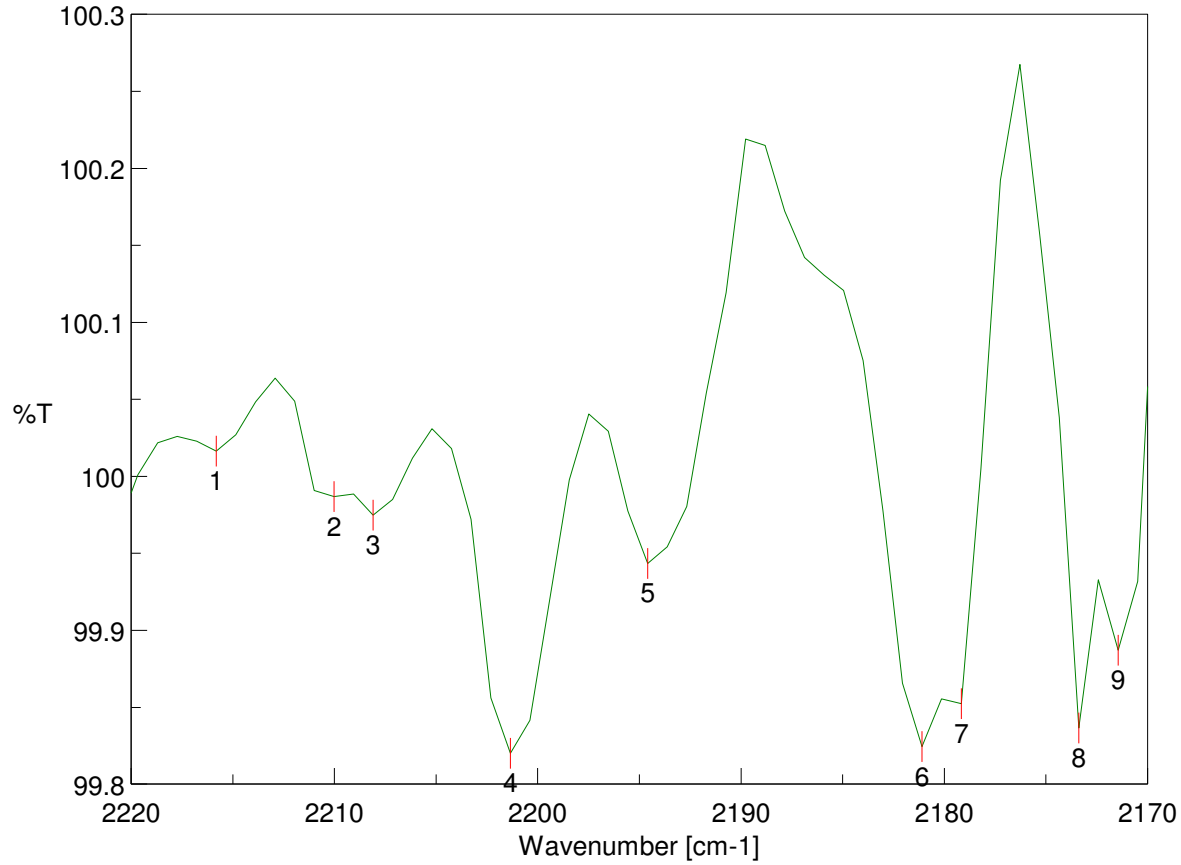

[Comments]
Sample name
Comment

User	QPackSA
Workgroup	Controle de Qualidade Farmoquimica
Division	Suporte Tec. Jasco
Company	libbs

[Detailed Information]

Creation date	6/12/2023 1:28 PM
Data array type	Linear data array
Horizontal axis	Wavenumber [cm-1]
Vertical axis	%T
Start	599.753 cm-1
End	4000.6 cm-1
Data interval	0.964233 cm-1
Data points	3528

[Measurement Information]

Model Name	FT/IR-4600typeA
Serial Number	D055461786
Accessory	ATR PRO ONE
Accessory S/N	A051361809
Incident angle	45 deg
Measurement Date	6/12/2023 1:02 PM
Light Source	Standard
Detector	TGS
Accumulation	48
Resolution	4 cm-1
Zero Filling	On
Apodization	Cosine
Gain	Auto (4)
Aperture	Auto (7.1 mm)
Scanning Speed	Auto (2 mm/sec)
Filter	Auto (30000 Hz)

Creation	QPack Soluções Analíticas
Review	
Approval	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	2215.81	100.016	2	2210.02	99.9867
3	2208.09	99.9746	4	2201.35	99.82
5	2194.6	99.9433	6	2181.1	99.8243
7	2179.17	99.8521	8	2173.38	99.8364
9	2171.45	99.8868			