

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:59:13
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:19:31
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

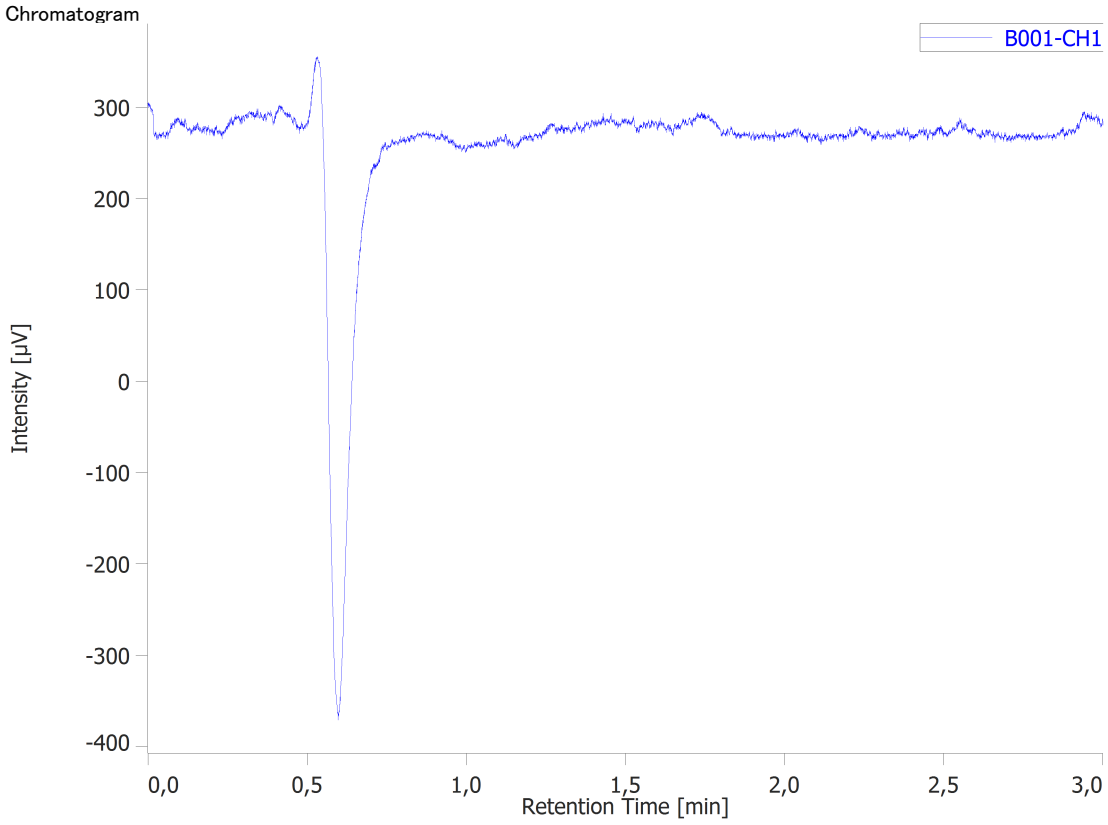

Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:59:51
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:35:05
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

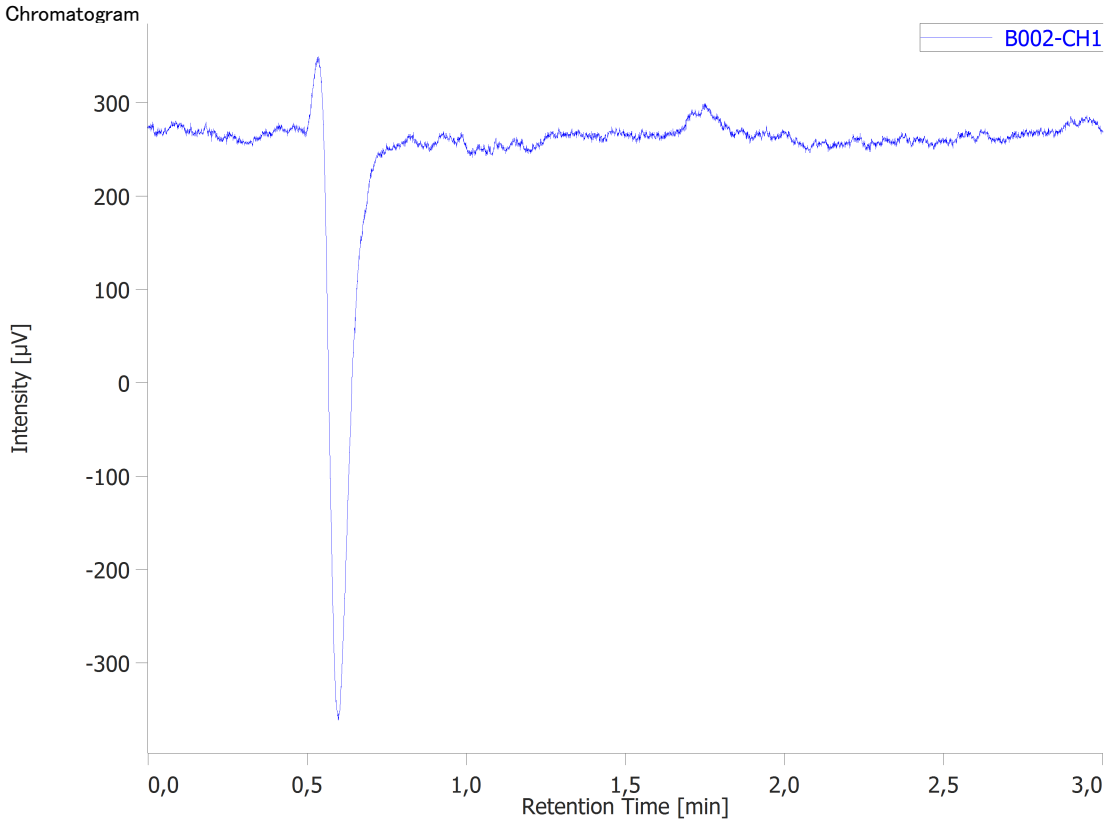


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information


User Name	Administrator
Date Modified	31/10/2019 14:00:29
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:50:38
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

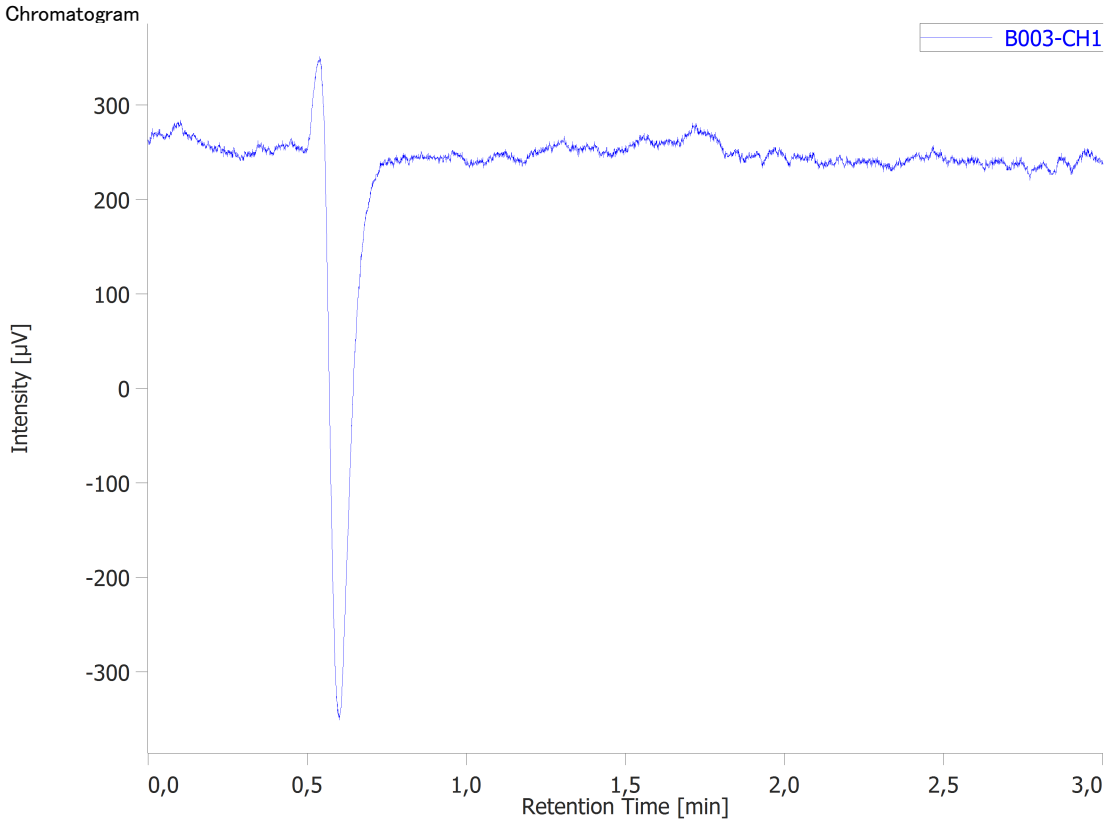

Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Peak Find - EDUV

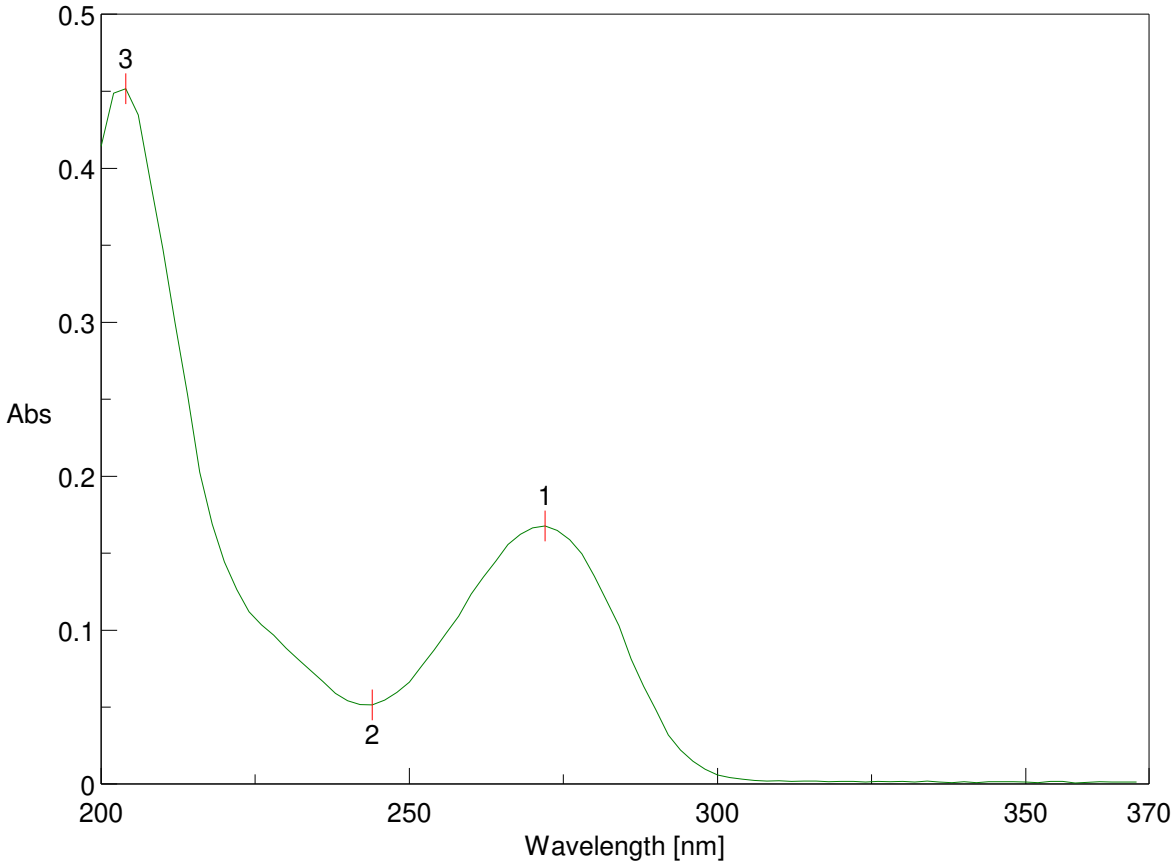

[Comments]

User	Administrator
Division	---
Company	Myralis
Creation date	31/10/2019 10:16
Date modified	31/10/2019 10:47

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	370 nm
Data interval	2 nm
Data points	85


[Measurement Information]

Instrument Name	UV-2070
Model Name	UV-2070
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.167605	2	244	0.0513515
3	204	0.451456			

Chromatogram

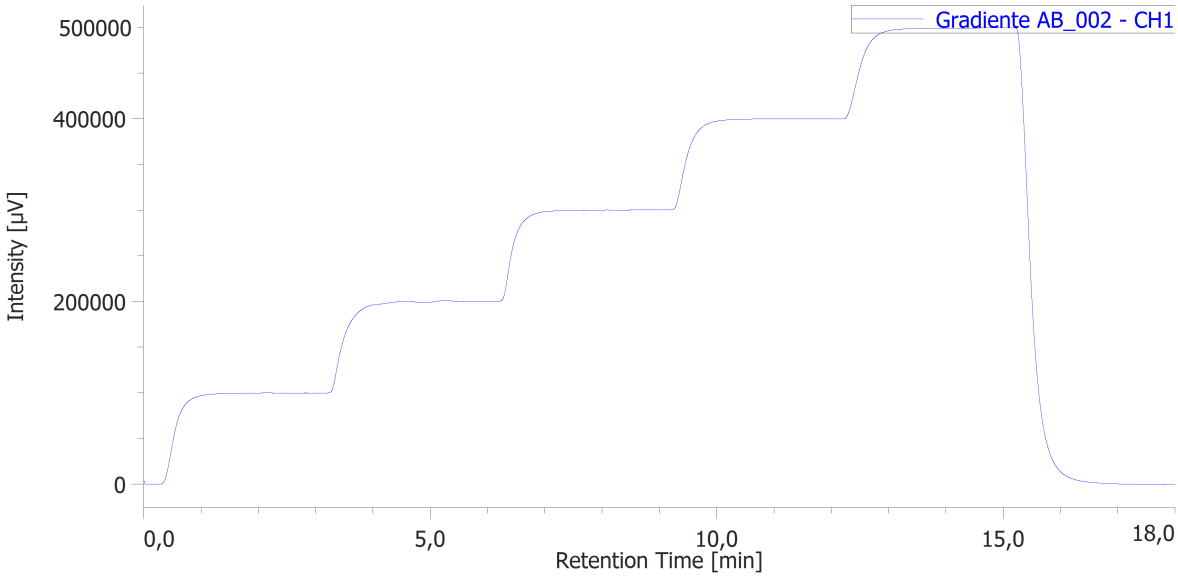


Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 15:19:56
Description	
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 15:01:55
Volume	0,00 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	18,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	40 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:57:39
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:18:38
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LDUV

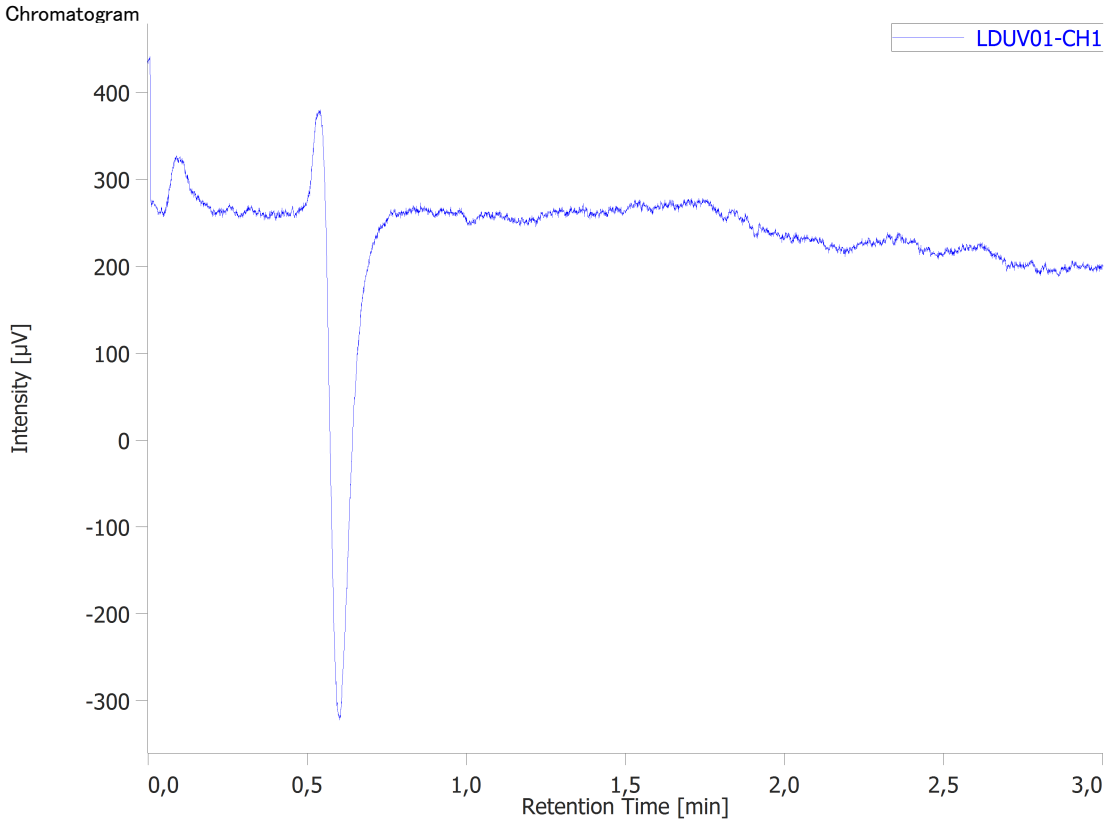


Peak Information – No data.

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 13:57:47
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:22:30
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LDUV

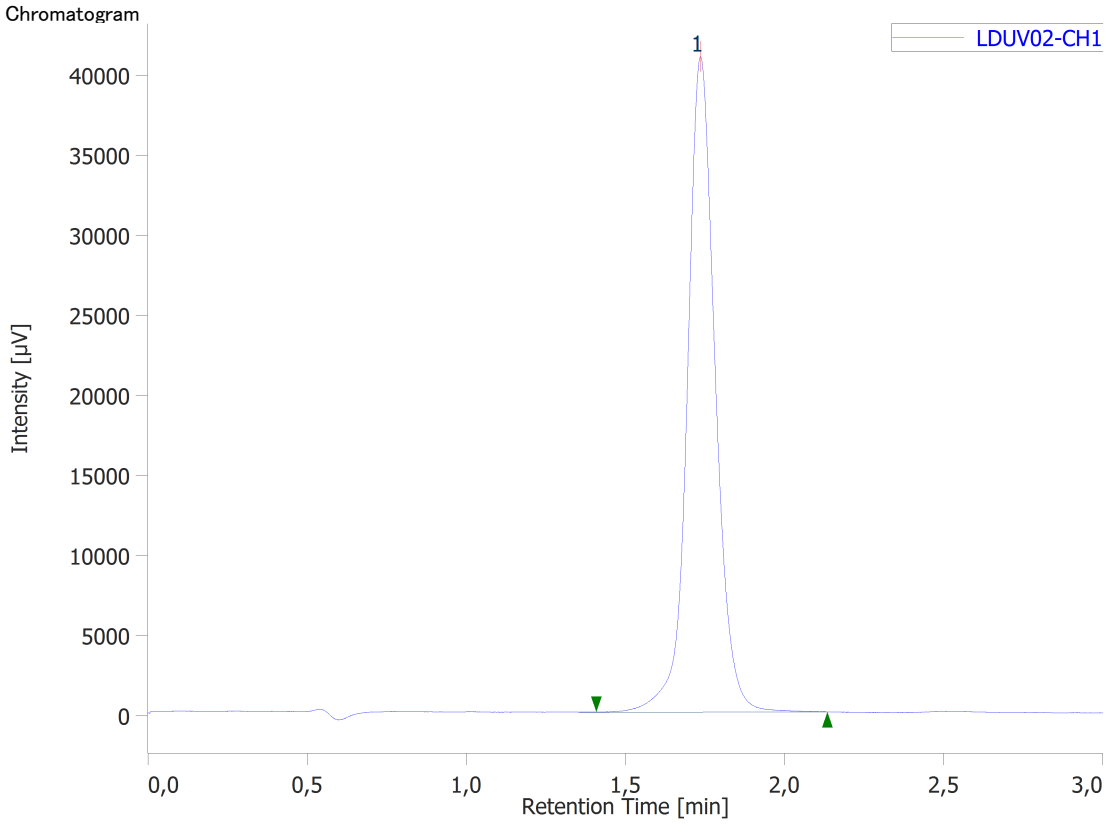


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,735	249308	40923

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:57:57
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:26:23
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LDUV

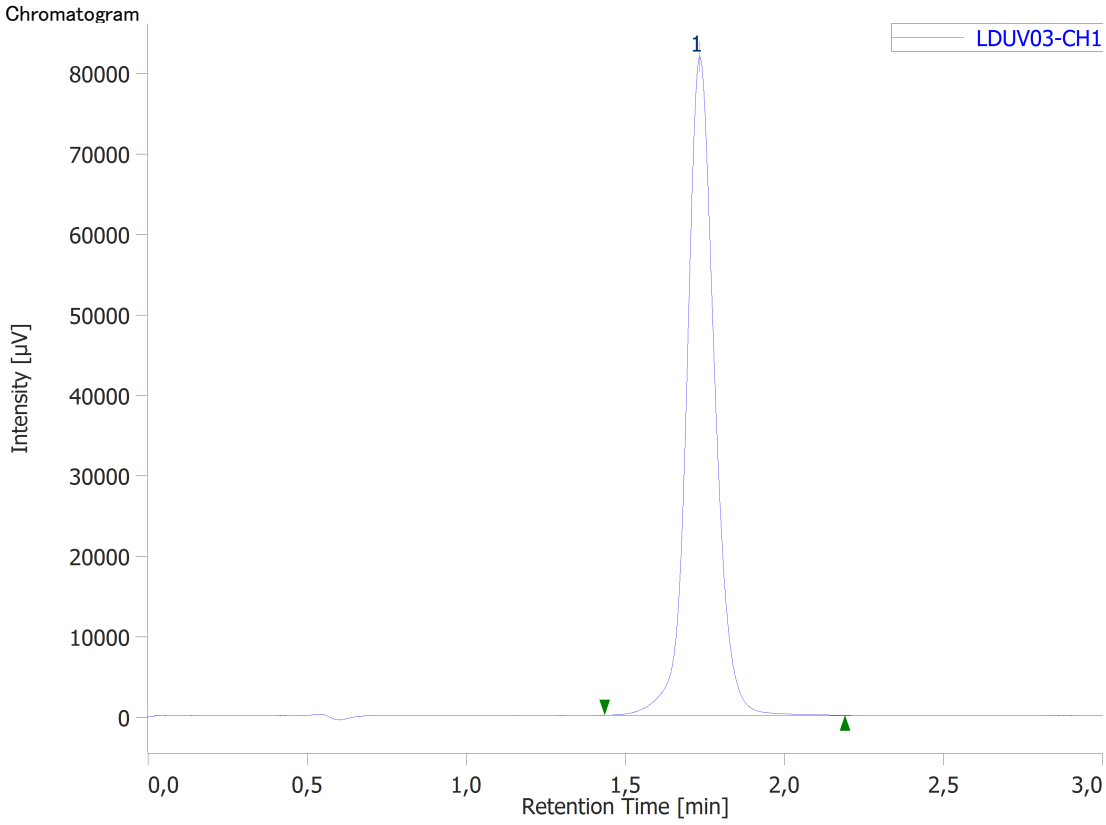


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,733	497124	81785

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:58:07
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:30:18
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LDUV

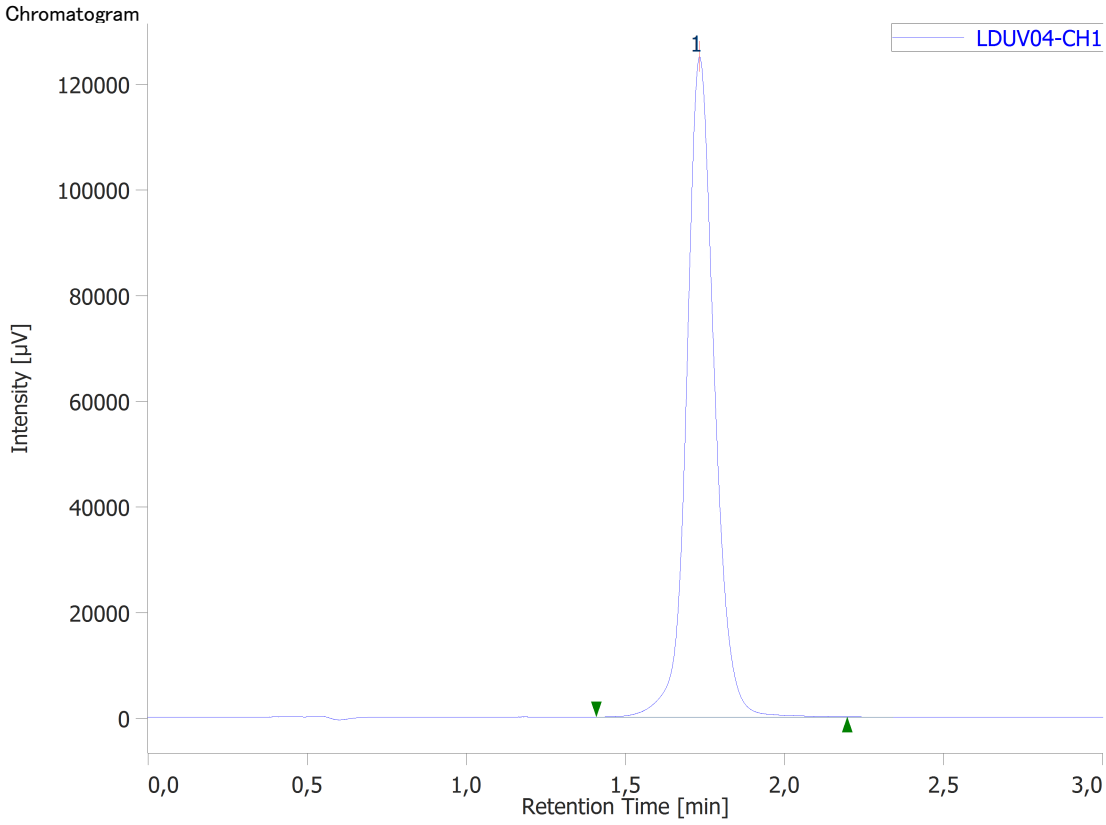


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,733	758347	124920

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 13:58:17
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:34:13
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LDUV

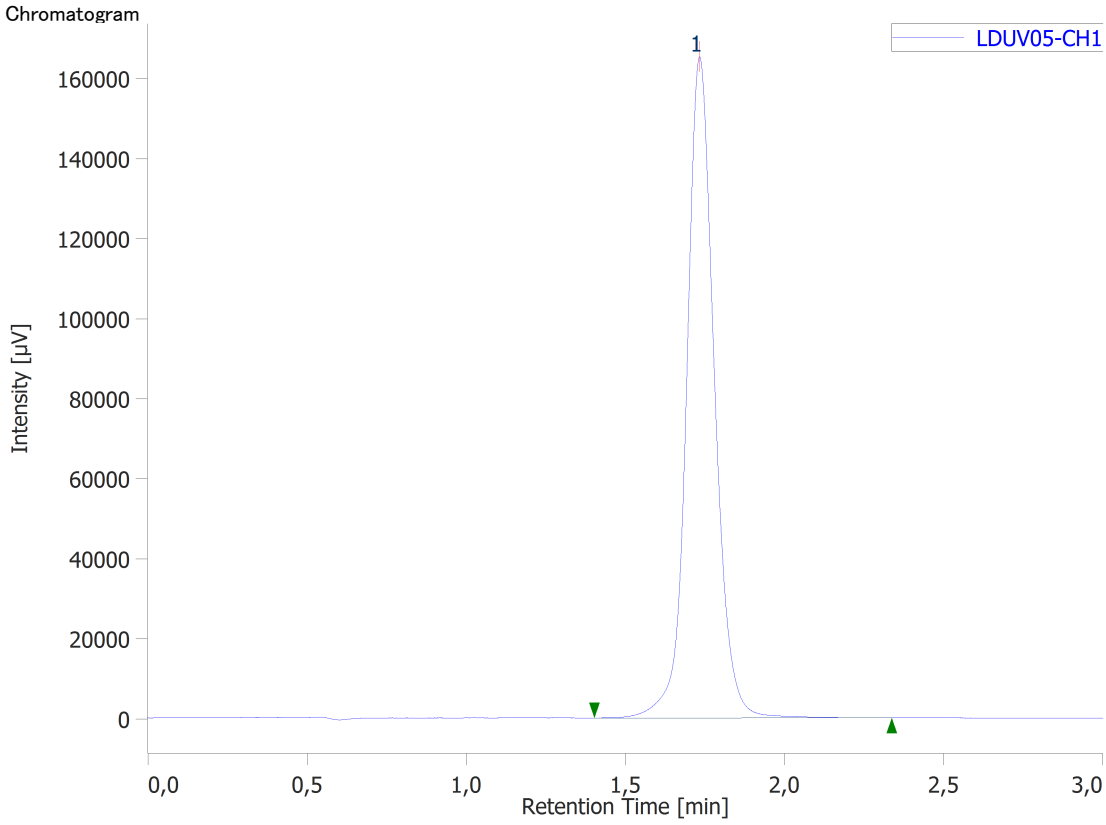


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,732	1002124	165207

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:13:25
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:49:29
Volume	0,10 [µL]
Project Name	Qualificação
Acquisition Sequence	LIIN

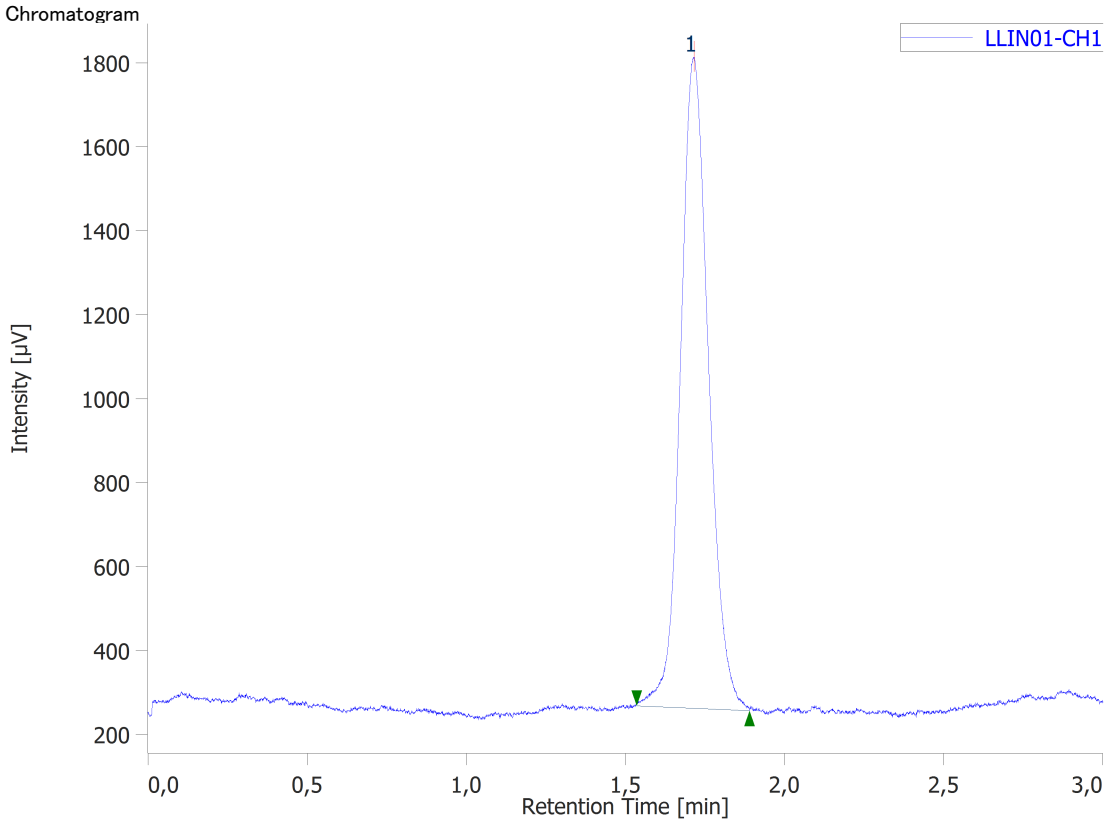


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,715	9539	1552

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:13:35
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:53:21
Volume	5,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LIIN

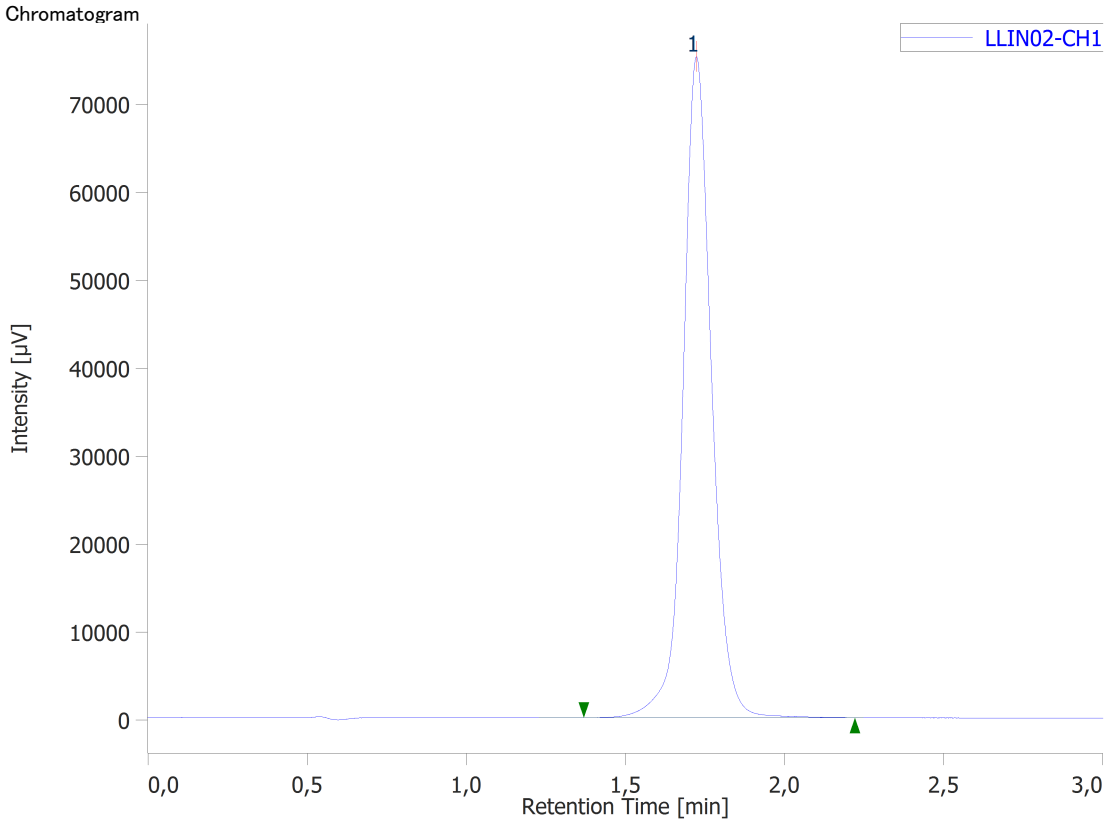


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,723	467359	75142

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:13:45
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 13:57:14
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LIIN

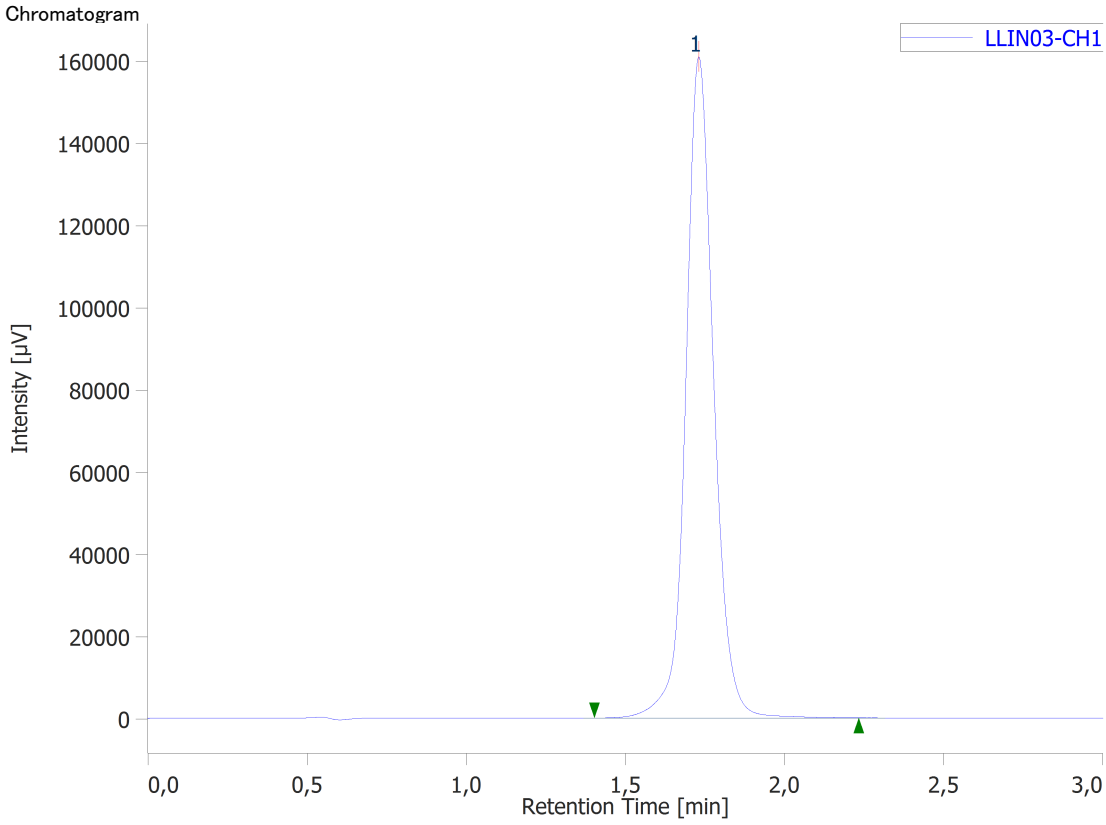


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,730	977028	160803

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:13:55
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 14:01:12
Volume	15,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LIIN

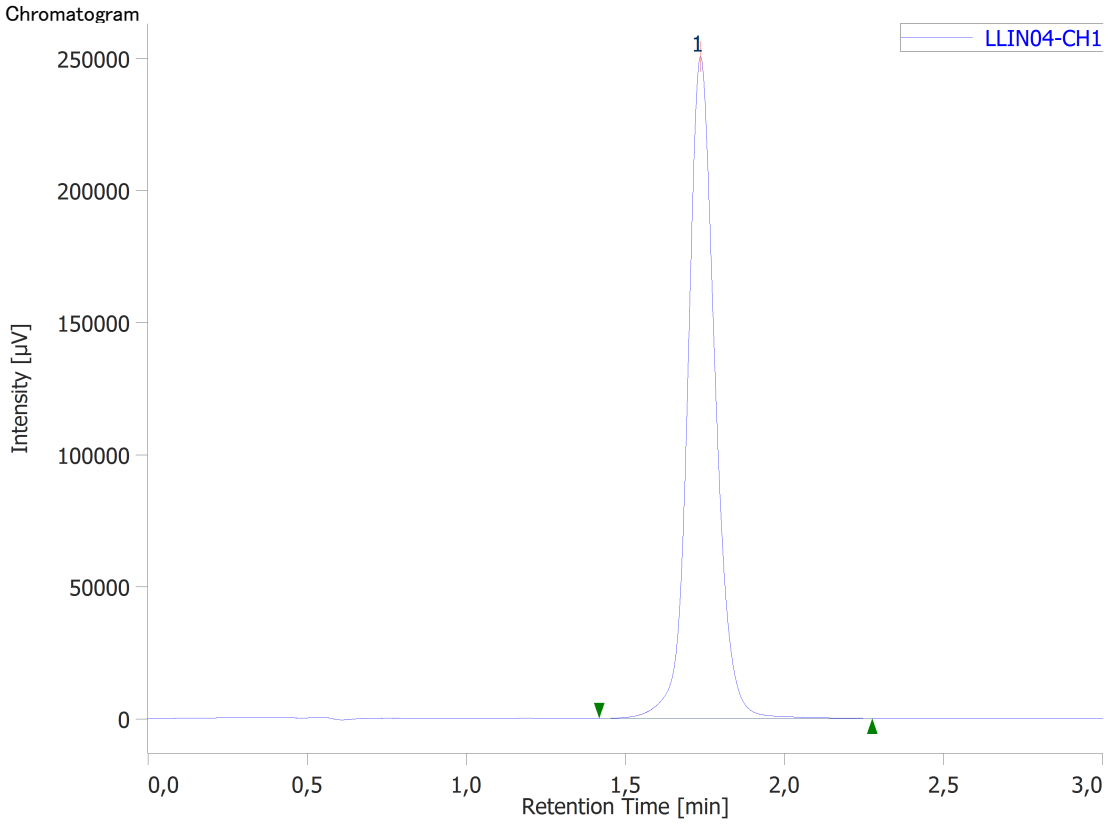


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,736	1495525	250380

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:14:05
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 14:05:12
Volume	20,00 [µL]
Project Name	Qualificação
Acquisition Sequence	LIIN

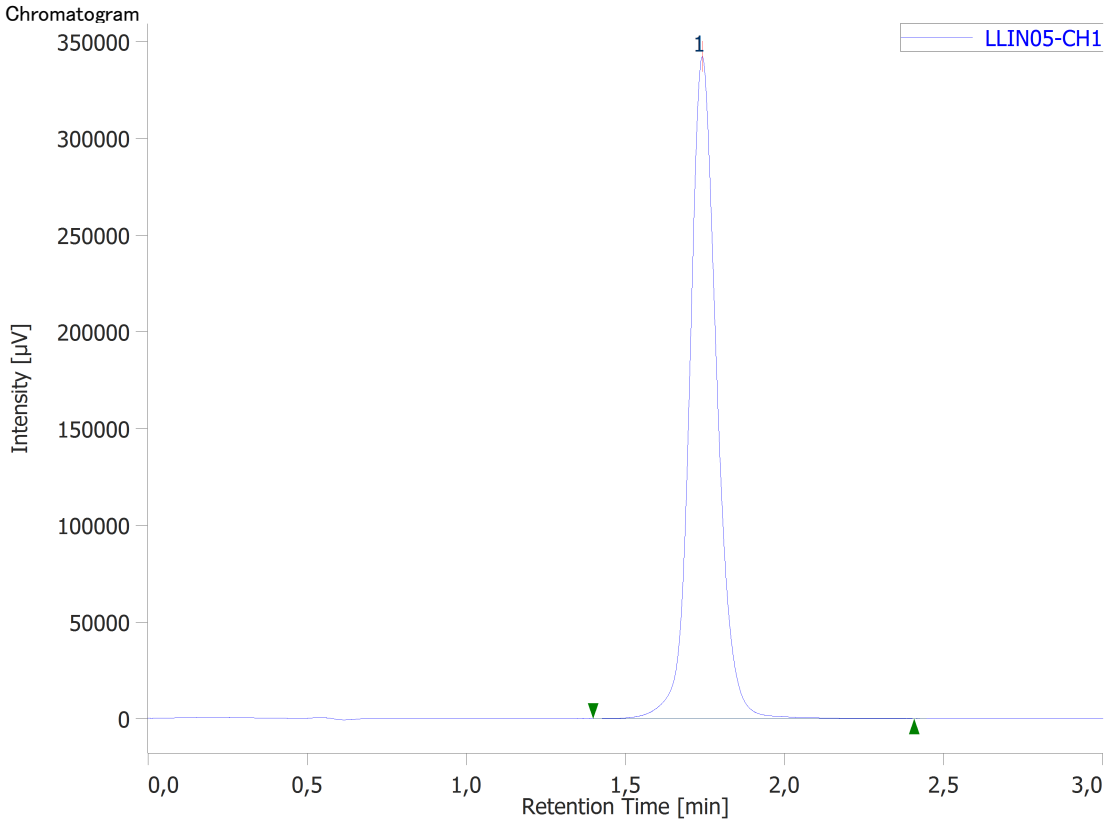


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,741	2023926	341968

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 13:51:18
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:39:00
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

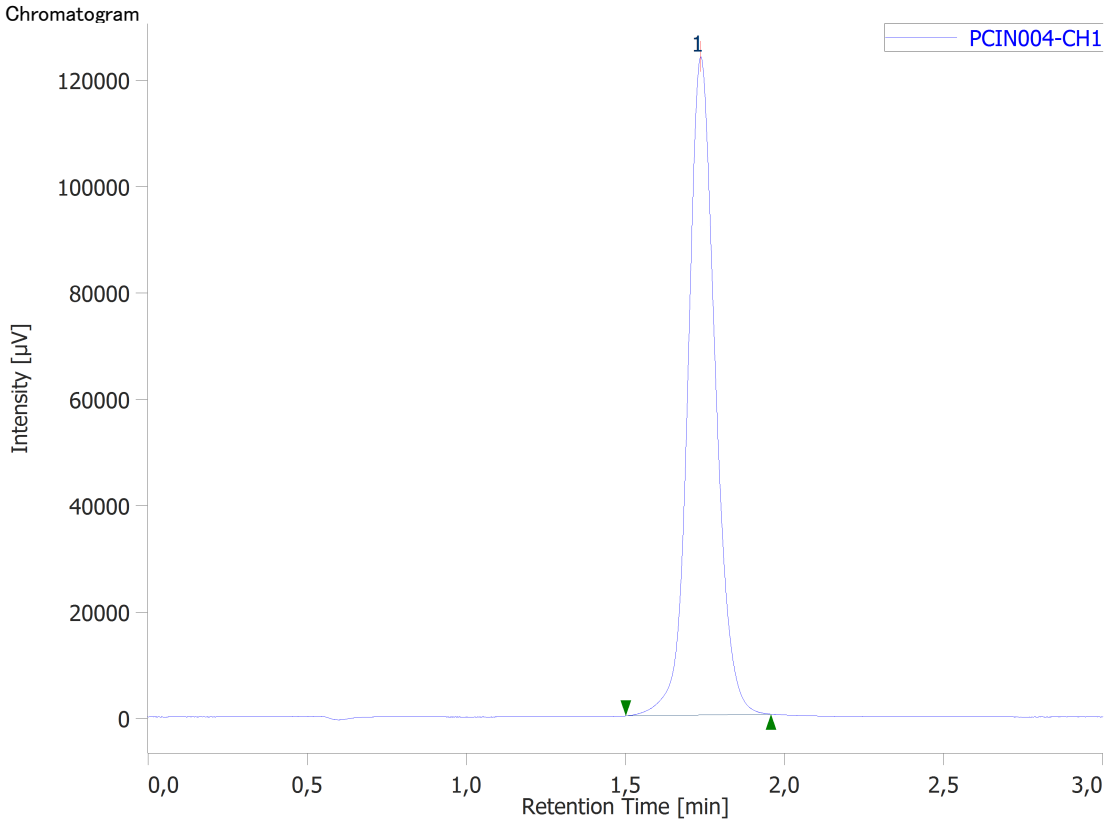


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,737	736553	123747

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 13:59:21
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:23:26
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

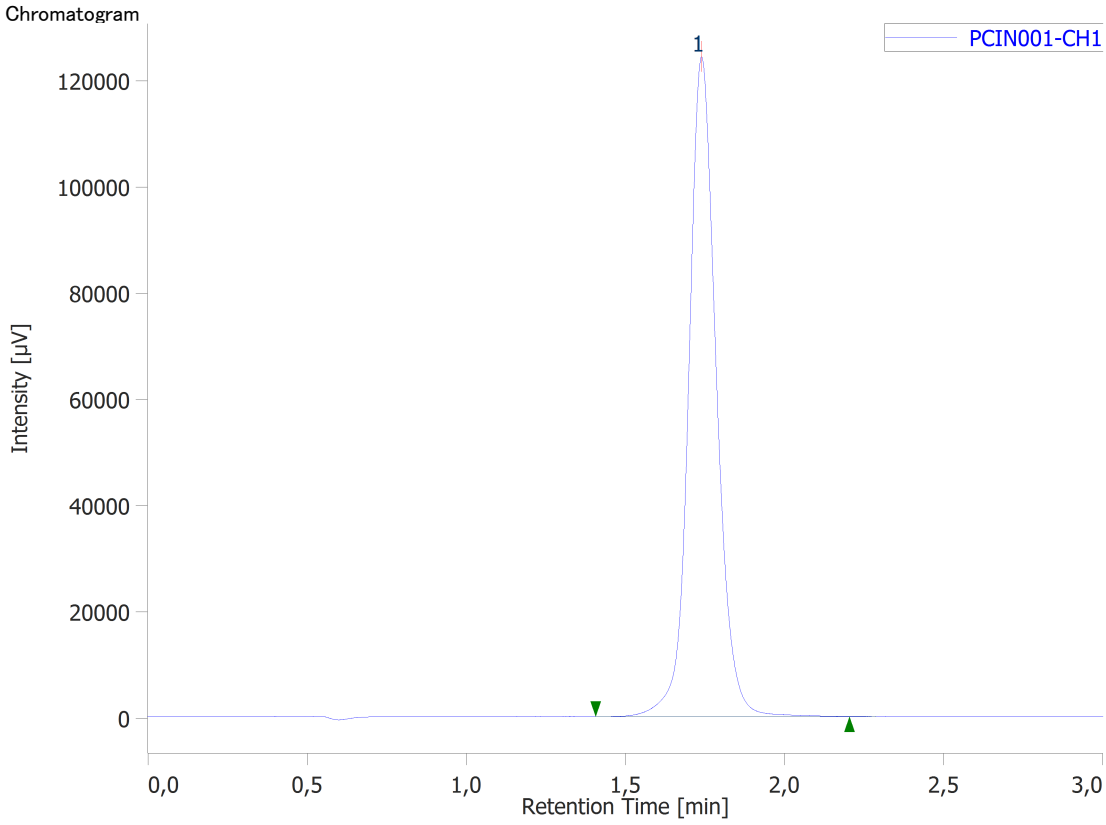


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,739	750001	124193

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:59:31
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:27:21
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

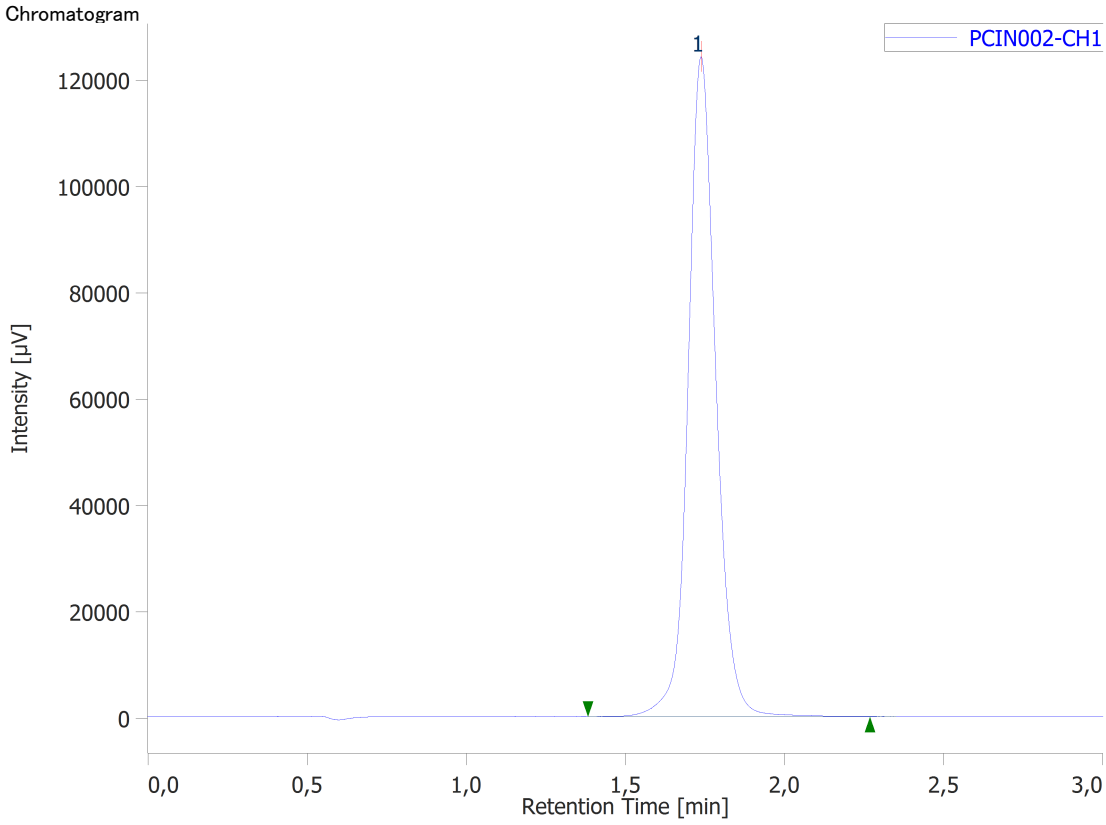


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,737	752218	124105

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:59:41
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:31:13
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

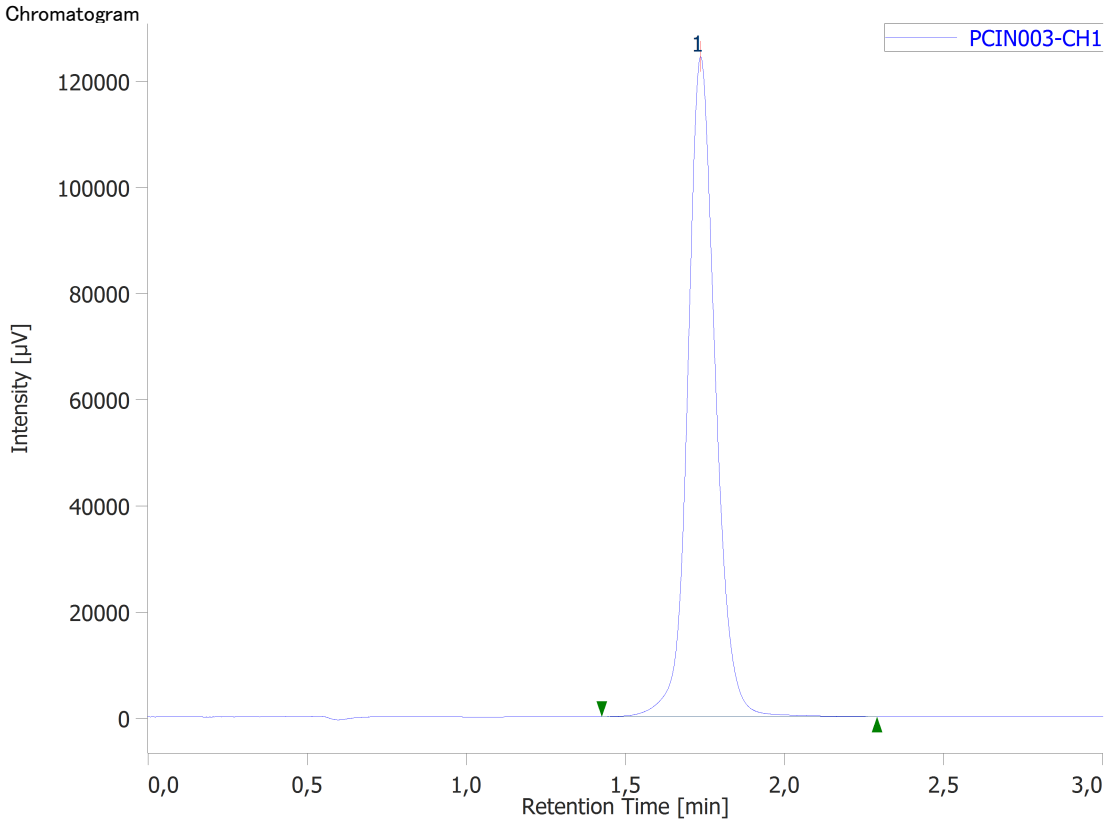


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,736	750510	124321

Creator *Administrator*
Reviewer
Approver

Chromatogram Information	
User Name	Administrator
Date Modified	31/10/2019 13:59:59
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:39:00
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

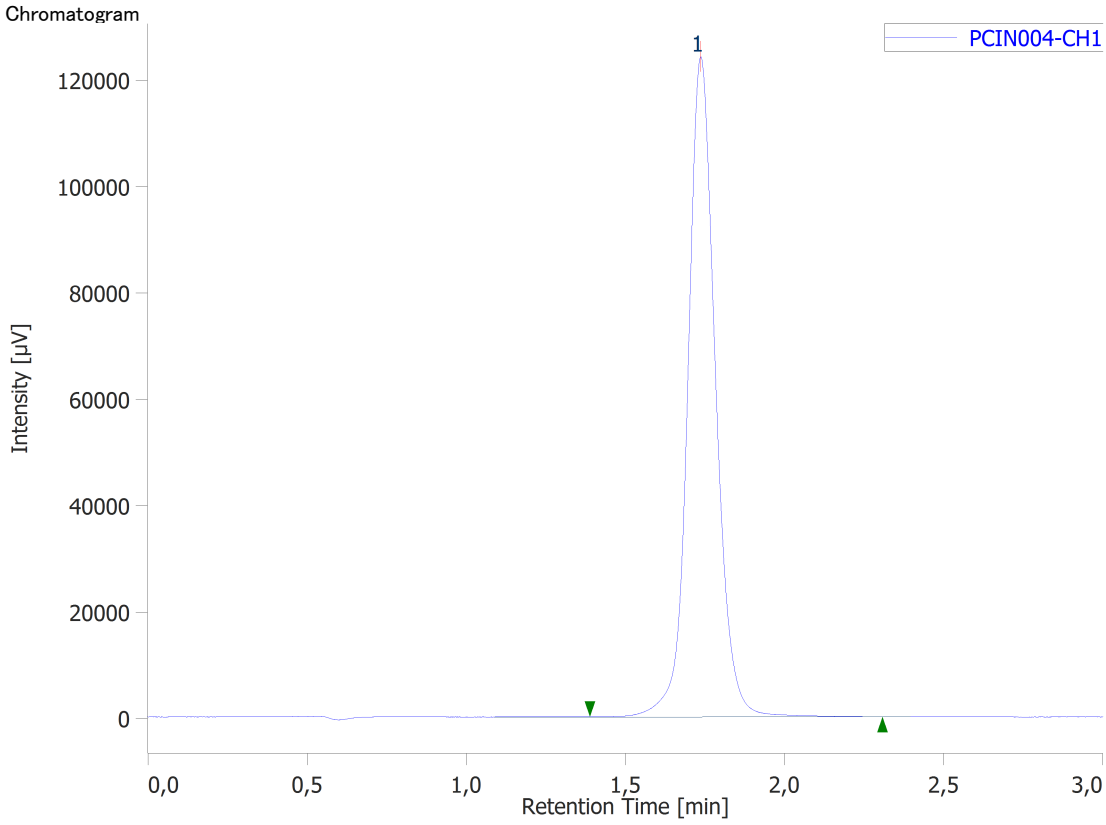


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,737	750280	124106

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:00:09
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:42:53
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

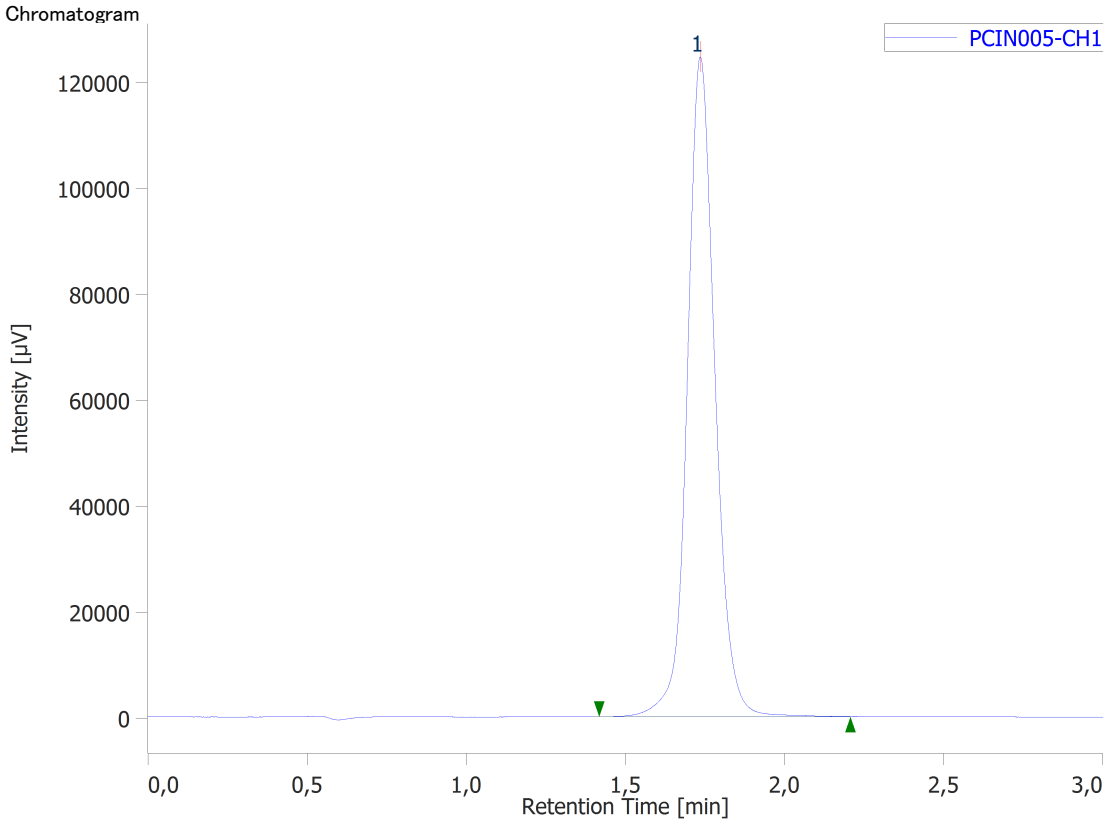


Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,735	753624	124591

Creator *Administrator*
Reviewer
Approver

Chromatogram Information

User Name	Administrator
Date Modified	31/10/2019 14:00:19
HPLC System Name	HPL 14 UV
Injection Date	31/10/2019 12:46:45
Volume	10,00 [µL]
Project Name	Qualificação
Acquisition Sequence	PCIN

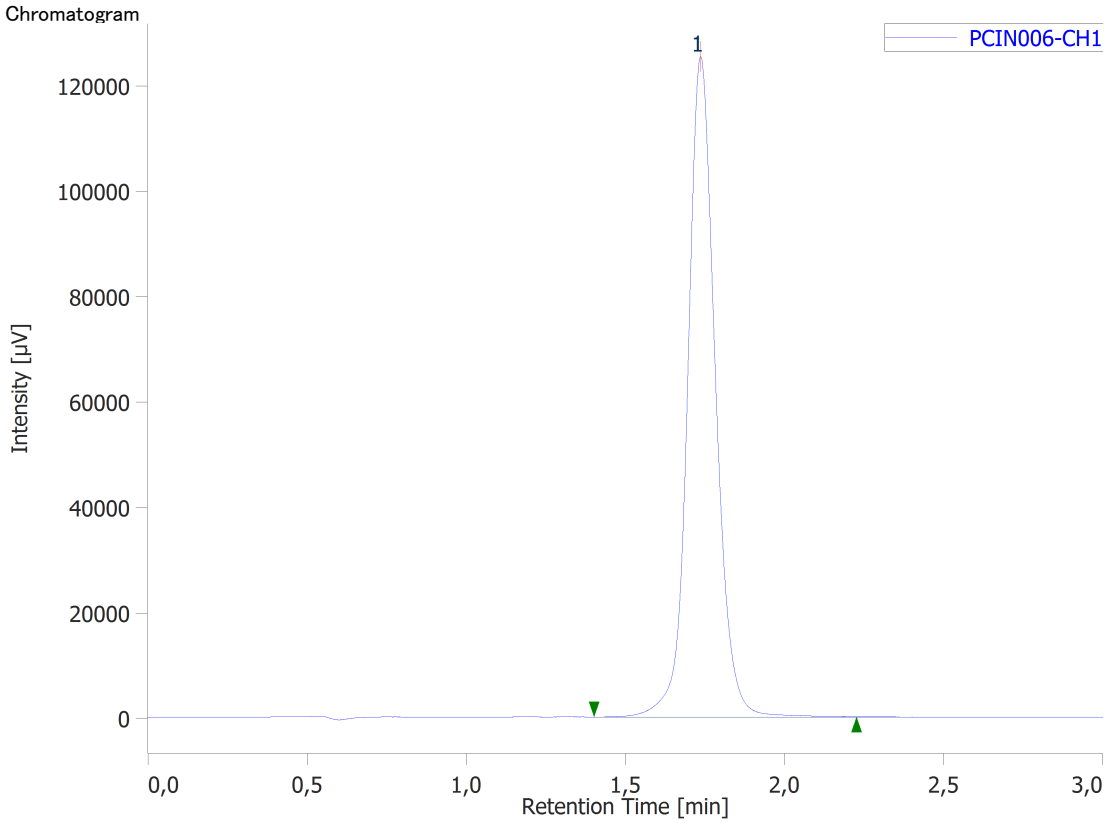

Peak Information

#	Peak Name	tR [min]	Area [µV·sec]	Height [µV]
1	Cafeína	1,736	756356	125213

Creator Administrator
Reviewer
Approver