
Chromatogram

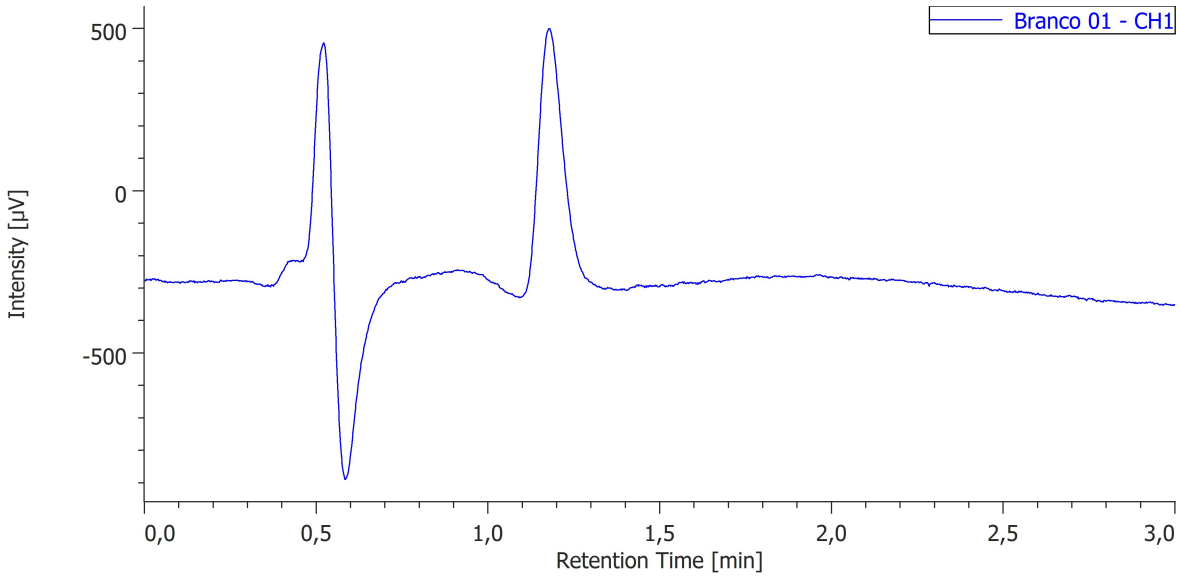


Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:08:11
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 08:55:44
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

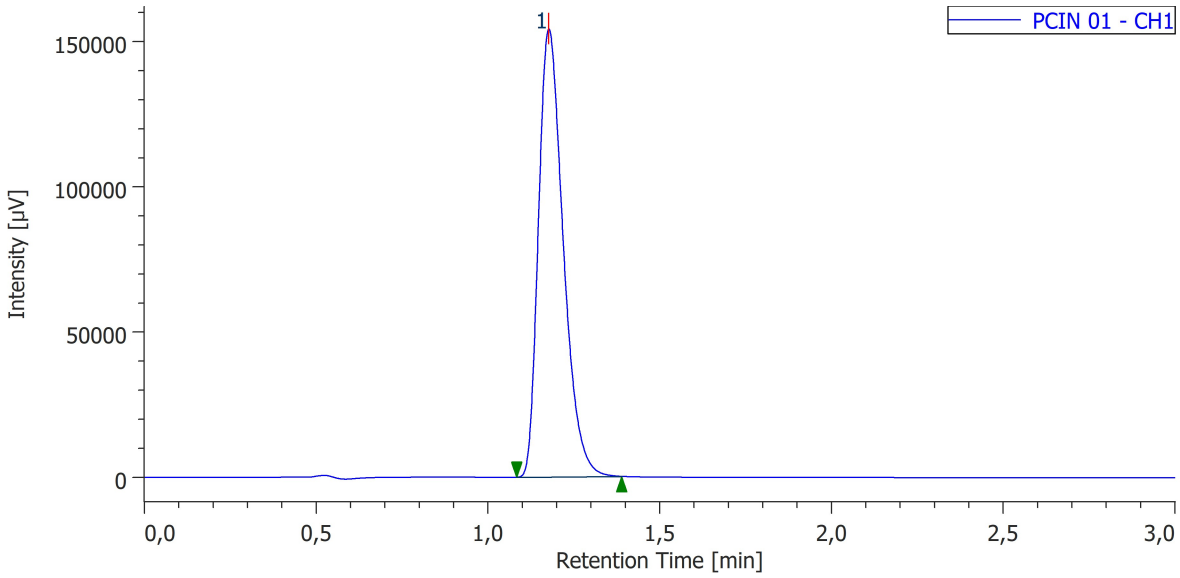

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:08:11
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:01:59
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,177	772501	154296	100,000	100,000	N/A	1298	N/A	1,378	

Creator Administrator
Reviewer
Approver

Chromatogram

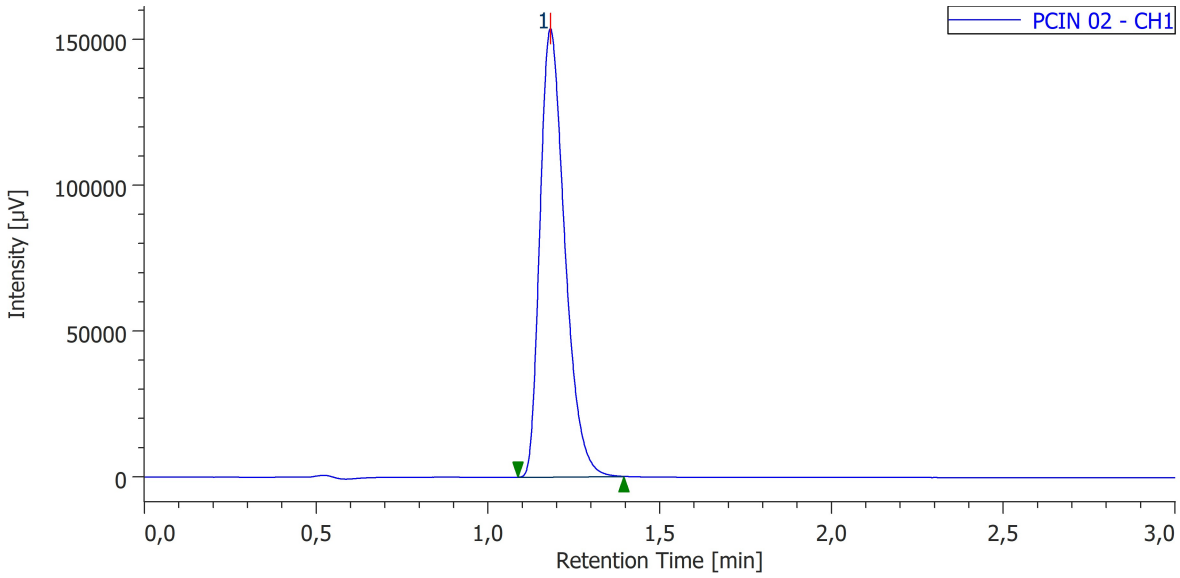

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:11:41
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:08:14
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,182	771766	153708	100,000	100,000	N/A	1303	N/A	1,370	

Creator Administrator
Reviewer
Approver

Chromatogram

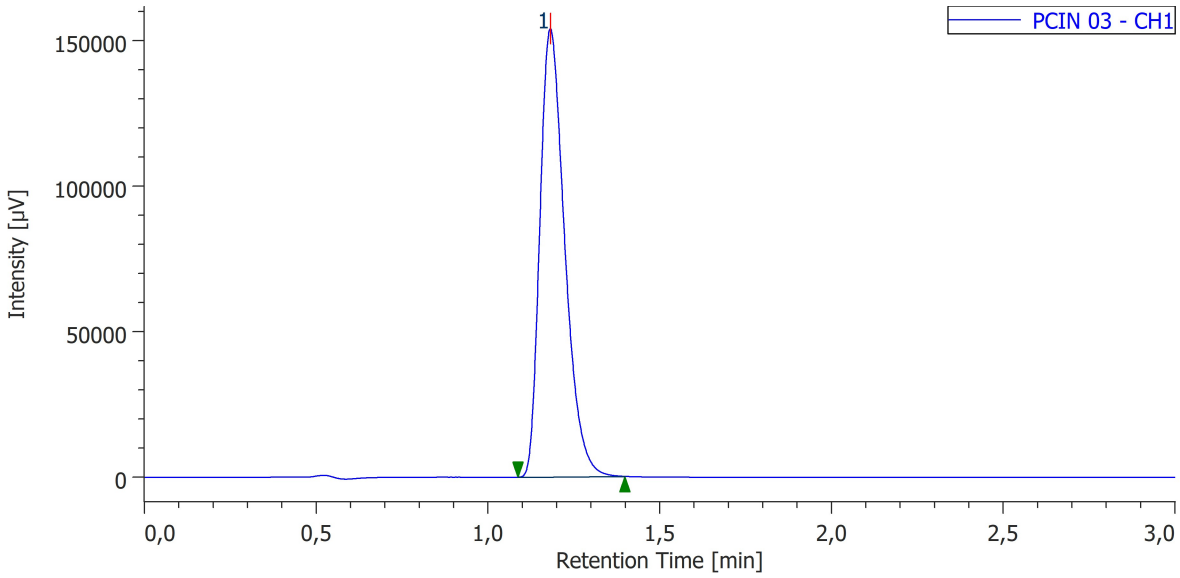

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:18:31
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:14:28
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,182	773459	153987	100,000	100,000	N/A	1301	N/A	1,364	

Creator Administrator
Reviewer
Approver

Chromatogram

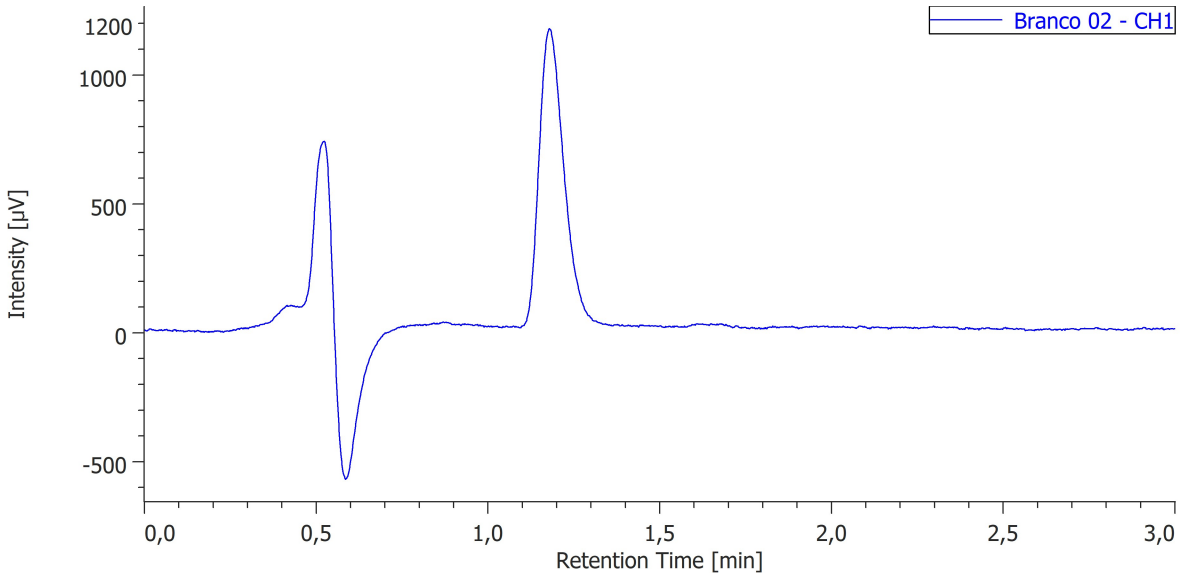


Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:29:21
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:20:43
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator	Administrator
Reviewer	
Approver	

Chromatogram

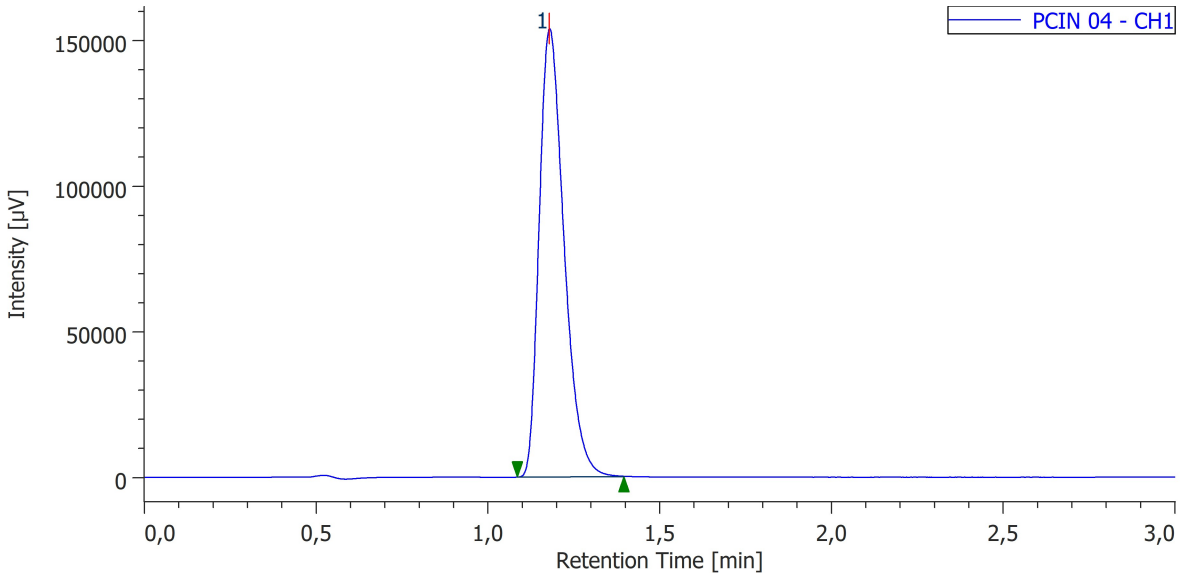

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:30:35
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:26:58
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,178	773256	153781	100,000	100,000	N/A	1291	N/A	1,390	

Creator Administrator
Reviewer
Approver

Chromatogram

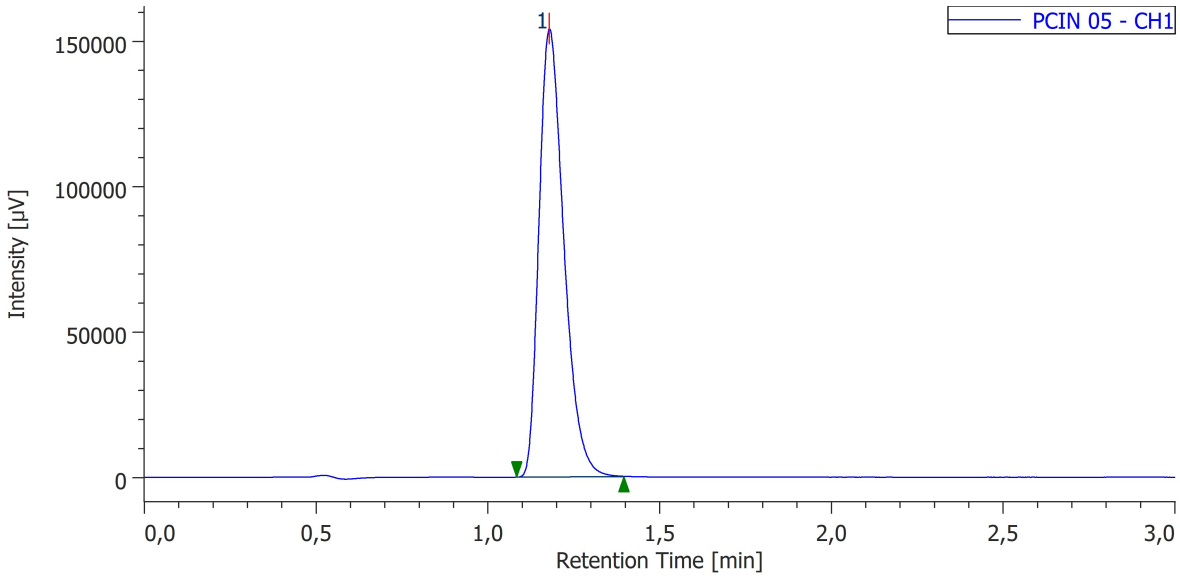

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:36:45
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:33:12
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,178	774357	154054	100,000	100,000	N/A	1292	N/A	1,373	

Creator Administrator
Reviewer
Approver

Chromatogram

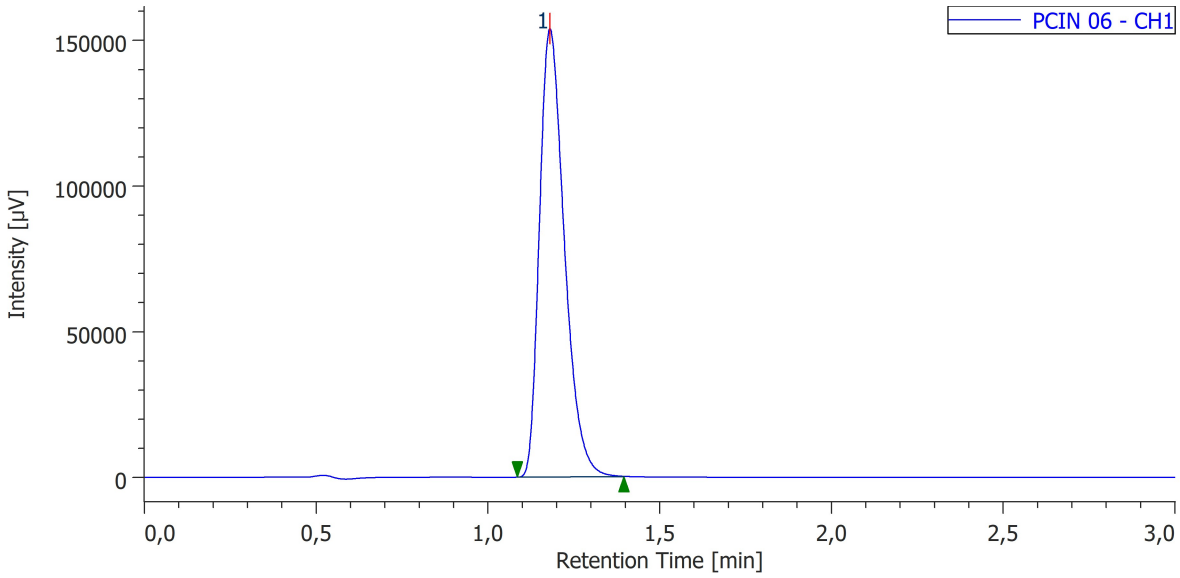

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:45:11
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:39:27
Volume	10,0 [µL]
Sample #	3
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,180	774315	153785	100,000	100,000	N/A	1291	N/A	1,374	

Creator Administrator
Reviewer
Approver

Chromatogram

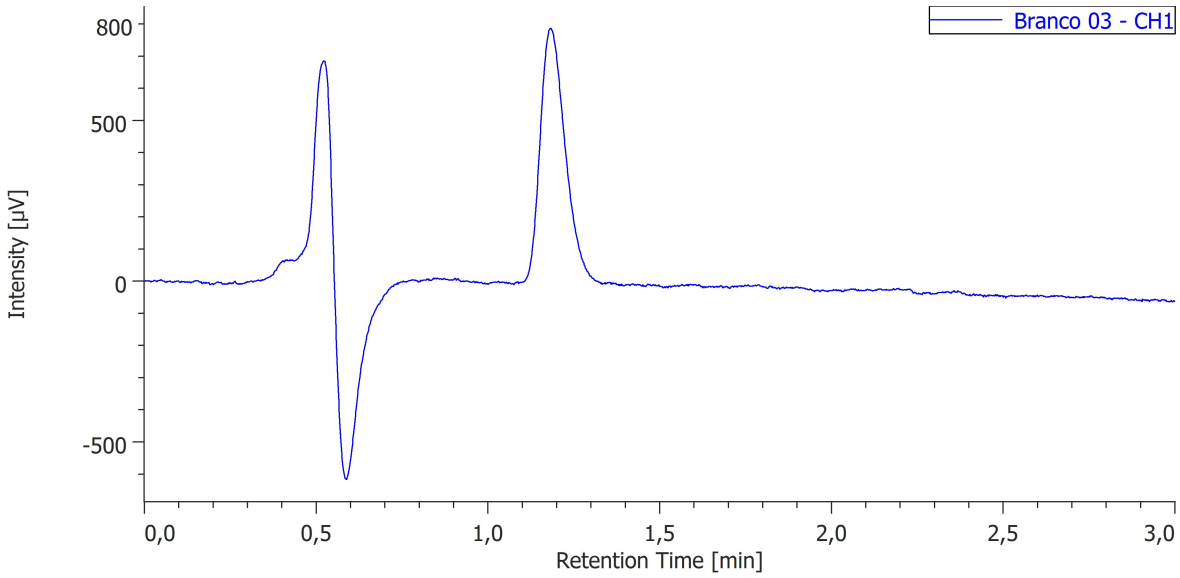

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 09:51:33
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:45:42
Volume	10,0 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

PID = 25561066-077257

Peak Find - EDUV 2026.jws

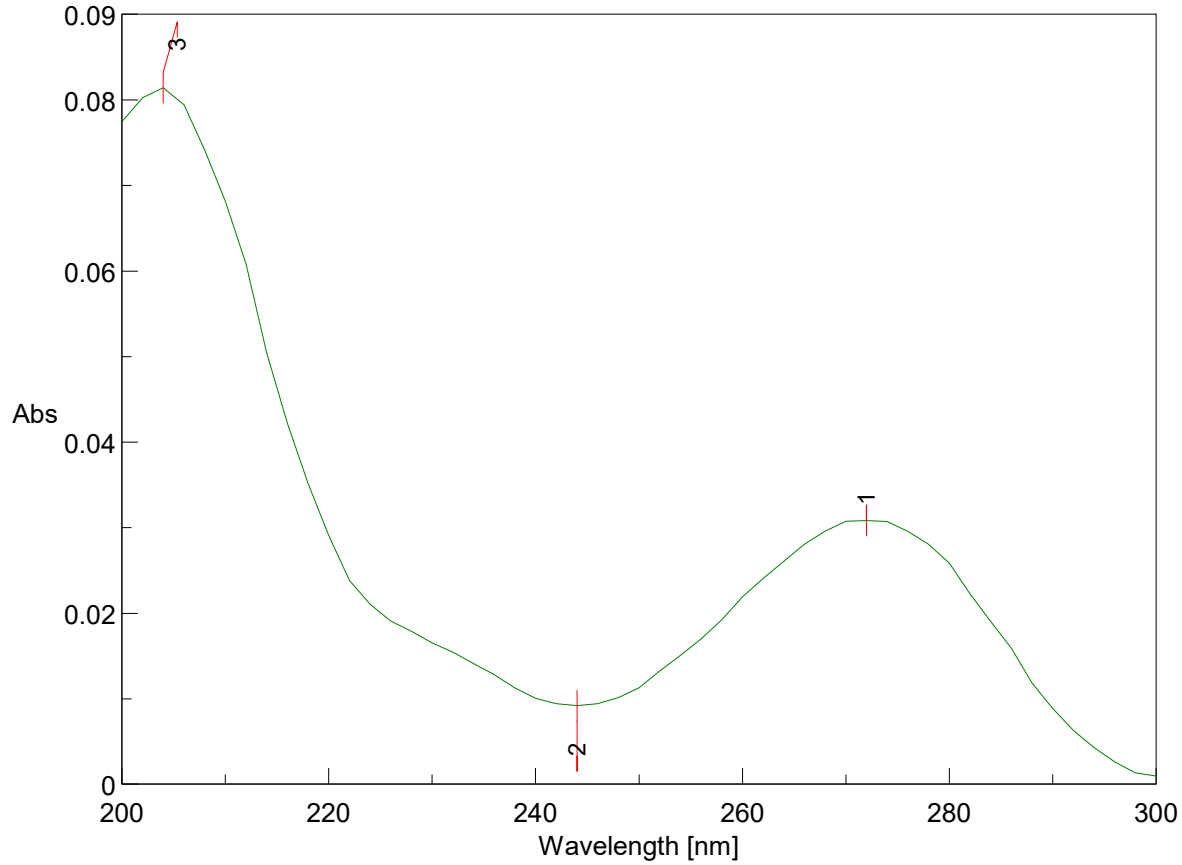

[Comments]

Username	QPackSA
Workgroup	QPack
Division	Assistência
Organization	JP Insdustria Farmacêutica S/A
Creation date	23/06/2026 14:51


[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	600 nm	
Data interval	2 nm	
Data points	200	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.030816	2	244	0.00917846
3	204	0.0813994			

Creation	QPackSA
Review	
Approval	

Chromatogram

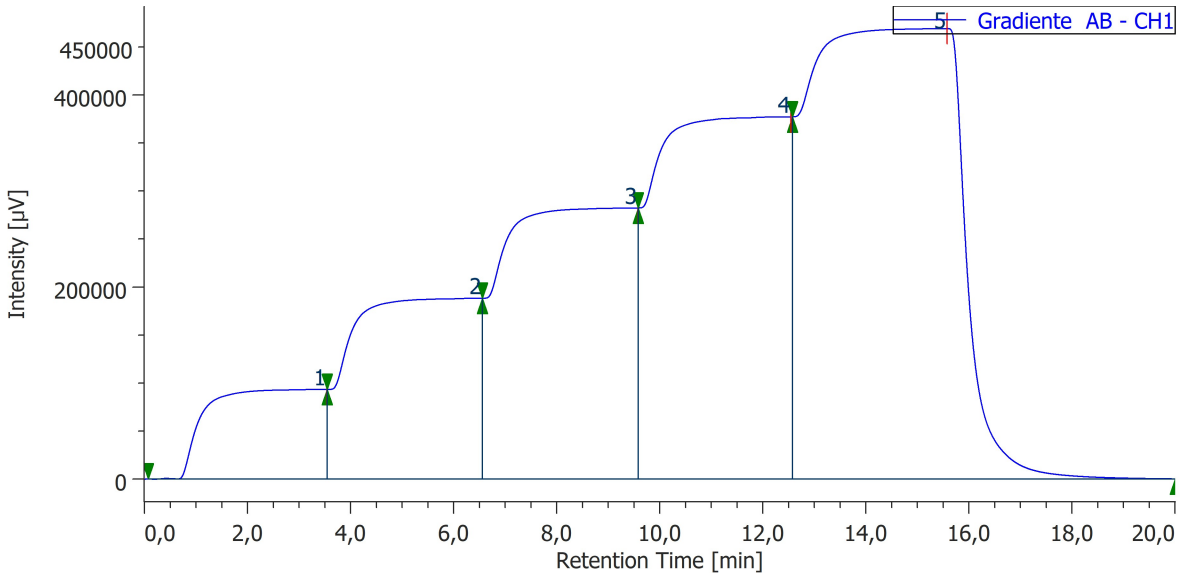

Chromatogram Information

User Name	Administrator
Date Modified	25/06/2026 10:07:27
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 13:49:49
Volume	0,1 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,542	13947277	93290	5,497	6,622	N/A	N/A	N/A	N/A	
2	40%	1	6,558	31242729	188139	12,313	13,354	N/A	N/A	N/A	N/A	
3	60%	1	9,577	48389548	282013	19,070	20,017	N/A	N/A	N/A	N/A	
4	80%	1	12,540	65153405	376740	25,677	26,741	N/A	N/A	N/A	N/A	
5	100%	1	15,570	95012097	468684	37,444	33,267	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

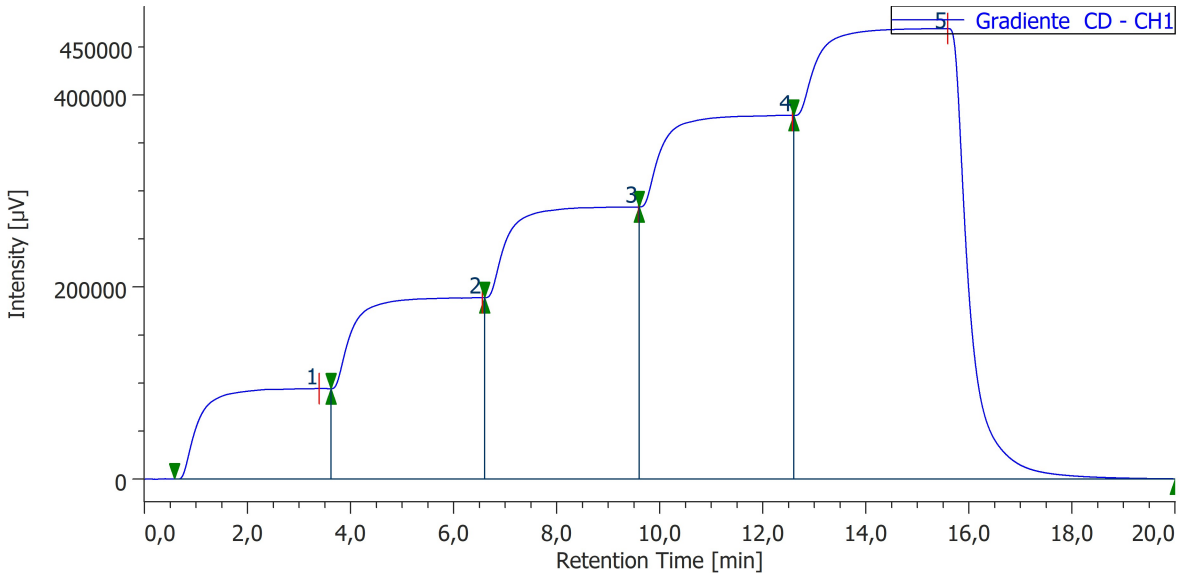

Chromatogram Information

User Name	Administrator
Date Modified	25/06/2026 10:07:27
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 14:10:23
Volume	0,1 [µL]
Sample #	2
Project Name	QPack
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente CD-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,390	14464990	94178	5,684	6,666	N/A	N/A	N/A	N/A	
2	40%	1	6,560	31352319	188744	12,321	13,359	N/A	N/A	N/A	N/A	
3	60%	1	9,590	48422778	283025	19,029	20,032	N/A	N/A	N/A	N/A	
4	80%	1	12,577	65534331	378301	25,753	26,775	N/A	N/A	N/A	N/A	
5	100%	1	15,583	94697390	468616	37,213	33,168	N/A	N/A	N/A	N/A	

Creator Administrator
Reviewer
Approver

Chromatogram

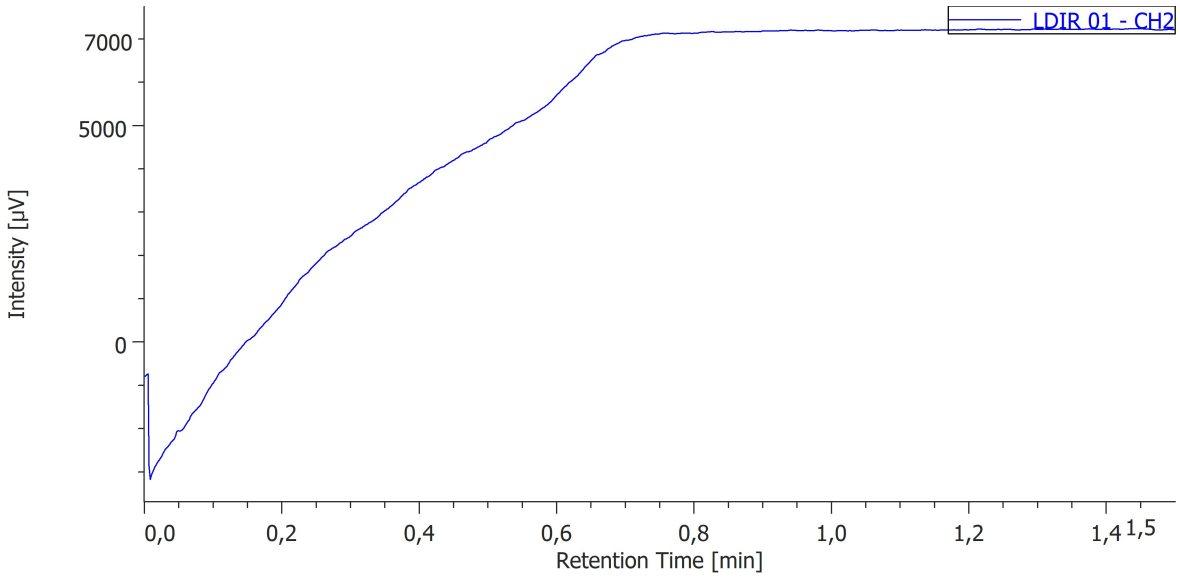


Chromatogram Information	
User Name	Administrator
Date Modified	25/06/2026 11:39:22
Description	
HPLC System Name	HPLC-0006
Injection Date	25/06/2026 11:22:34
Volume	20,0 [µL]
Sample #	11
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	Qualificação RI
Control Method	Qualificação RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDIR 01-CH2
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

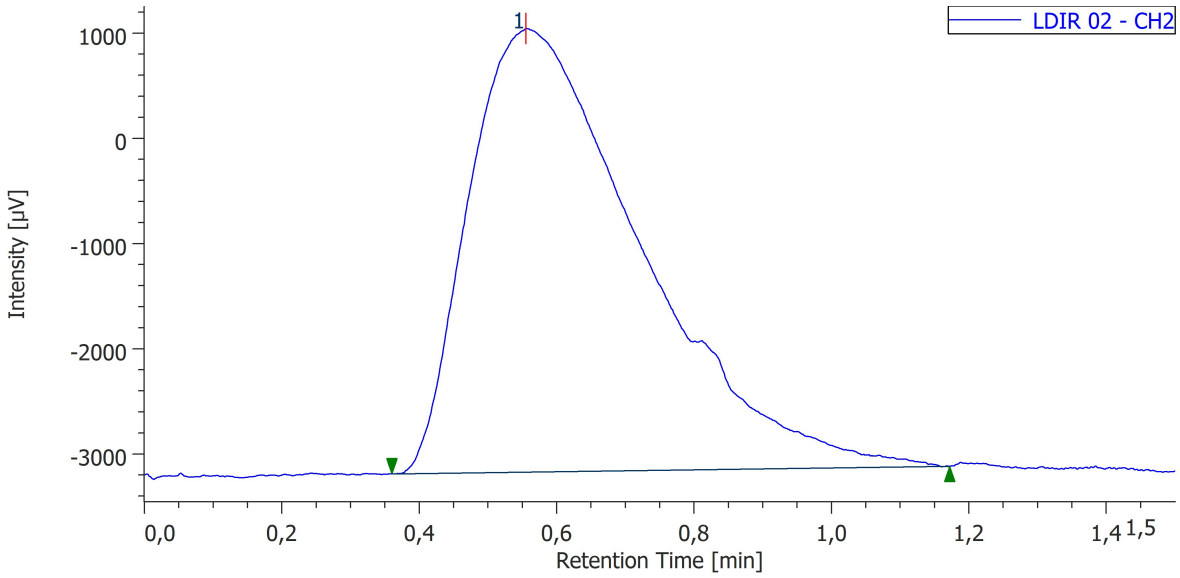

Chromatogram Information	
User Name	Administrator
Date Modified	25/06/2026 11:39:22
Description	
HPLC System Name	HPLC-0006
Injection Date	25/06/2026 11:25:07
Volume	20,0 [µL]
Sample #	12
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	Qualificação RI
Control Method	Qualificação RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 02-CH2
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	2	0,555	73364	4212	100,000	100,000	N/A	24	N/A	1,928	

Creator Administrator
Reviewer
Approver

Chromatogram

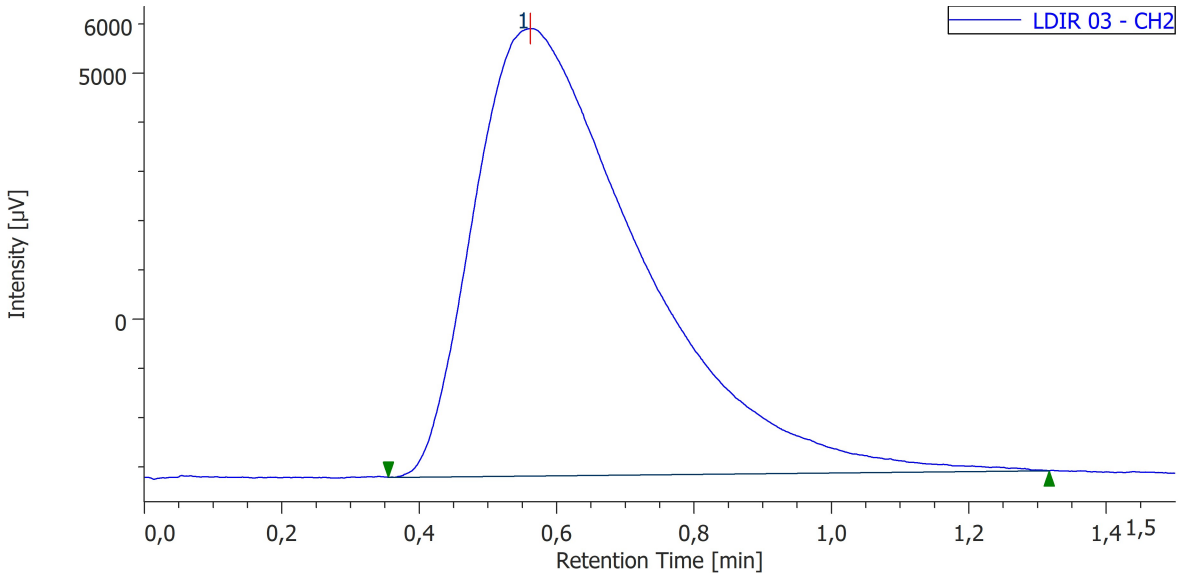

Chromatogram Information	
User Name	Administrator
Date Modified	25/06/2026 11:39:22
Description	
HPLC System Name	HPLC-0006
Injection Date	25/06/2026 11:27:39
Volume	20,0 [µL]
Sample #	13
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	Qualificação RI
Control Method	Qualificação RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 03-CH2
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	2	0,562	153463	9080	100,000	100,000	N/A	28	N/A	1,935	

Creator Administrator
Reviewer
Approver

Chromatogram

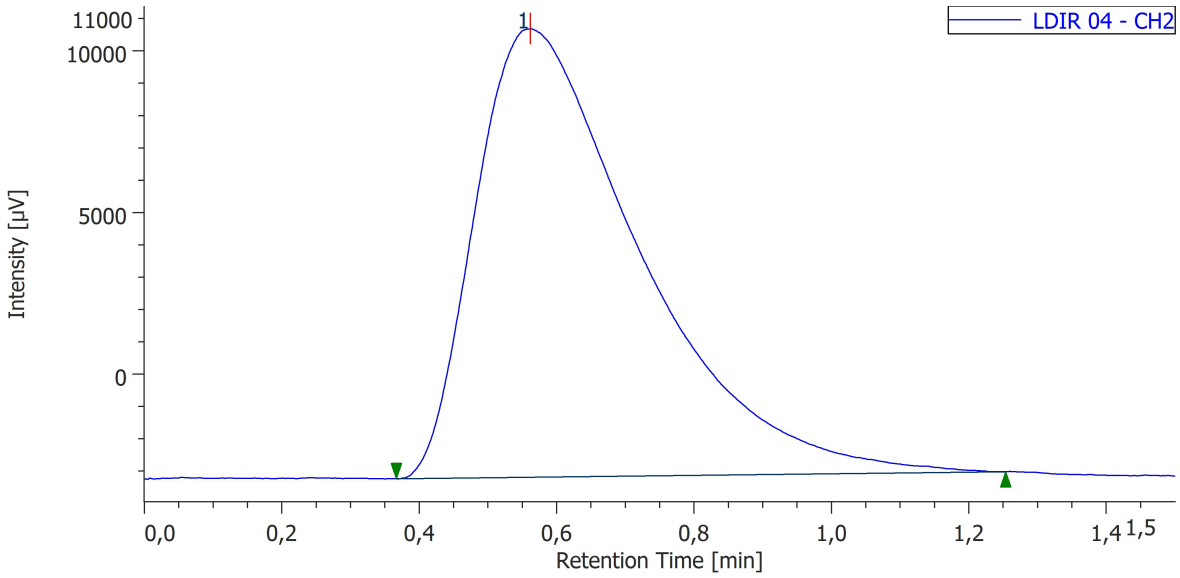

Chromatogram Information	
User Name	Administrator
Date Modified	25/06/2026 11:39:22
Description	
HPLC System Name	HPLC-0006
Injection Date	25/06/2026 11:30:13
Volume	20,0 [µL]
Sample #	14
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	Qualificação RI
Control Method	Qualificação RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 04-CH2
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	2	0,562	231741	13872	100,000	100,000	N/A	28	N/A	1,913	

Creator Administrator
Reviewer
Approver

Chromatogram

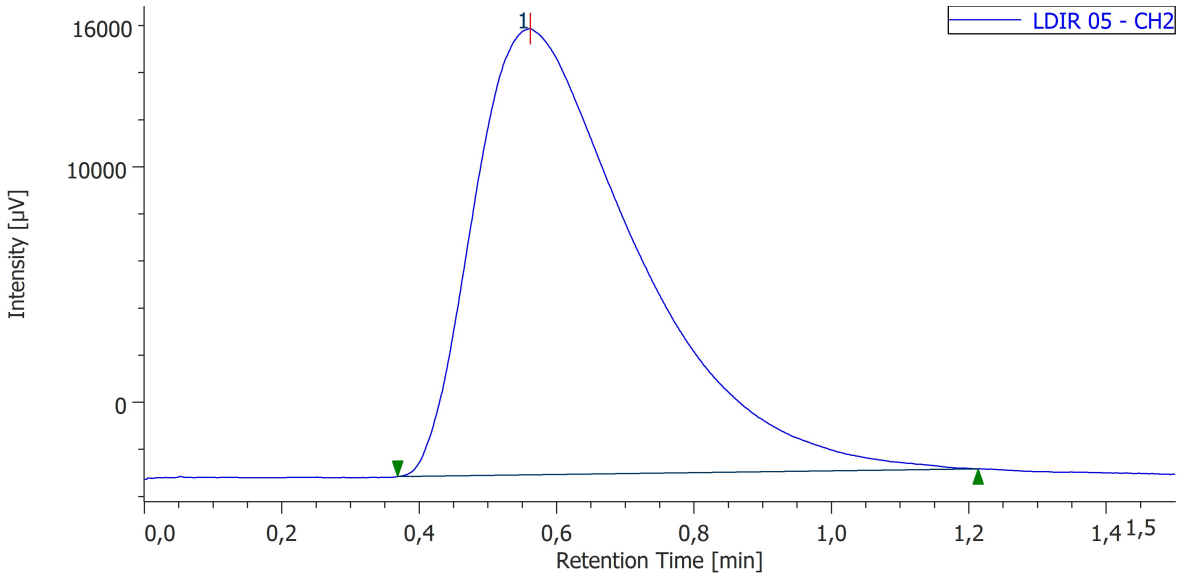

Chromatogram Information	
User Name	Administrator
Date Modified	25/06/2026 11:39:22
Description	
HPLC System Name	HPLC-0006
Injection Date	25/06/2026 11:32:48
Volume	20,0 [µL]
Sample #	15
Project Name	QPack
Acquisition Time	1,5 [min]
Acquisition Sequence	Qualificação RI
Control Method	Qualificação RI
Peak ID Table	Glicerol
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDIR 05-CH2
Sample Name	
Channel Name	RI
Sampling Interval	100 [msec]
Peak Method	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PDRI	2	0,562	313202	18940	100,000	100,000	N/A	28	N/A	1,886	

Creator Administrator
Reviewer
Approver

Chromatogram

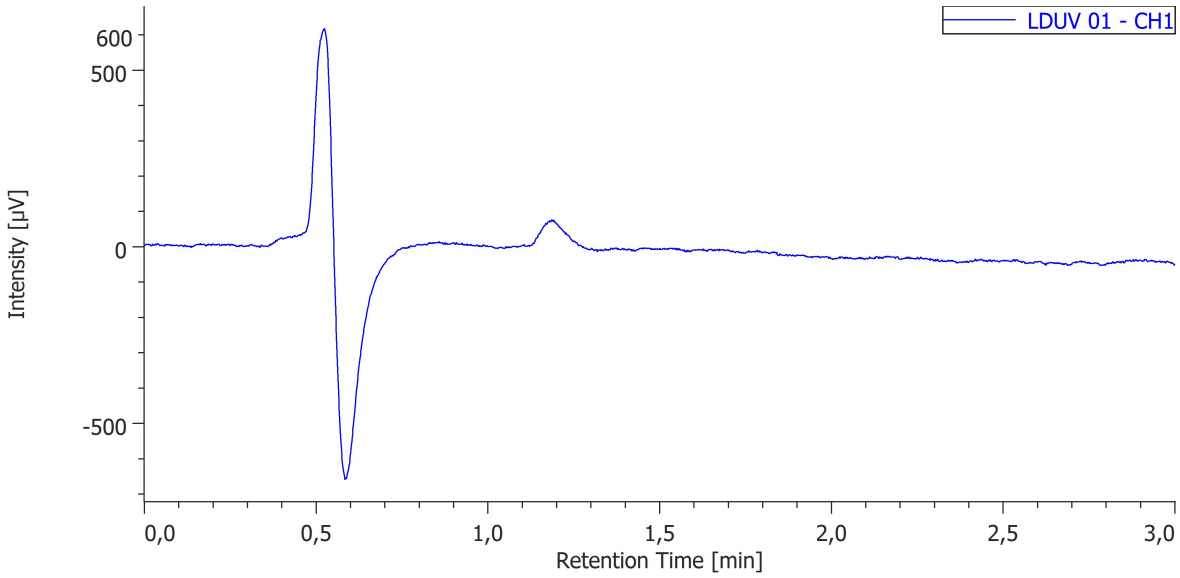


Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 10:01:19
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:51:56
Volume	10,0 [µL]
Sample #	4
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator Administrator
Reviewer
Approver

Chromatogram

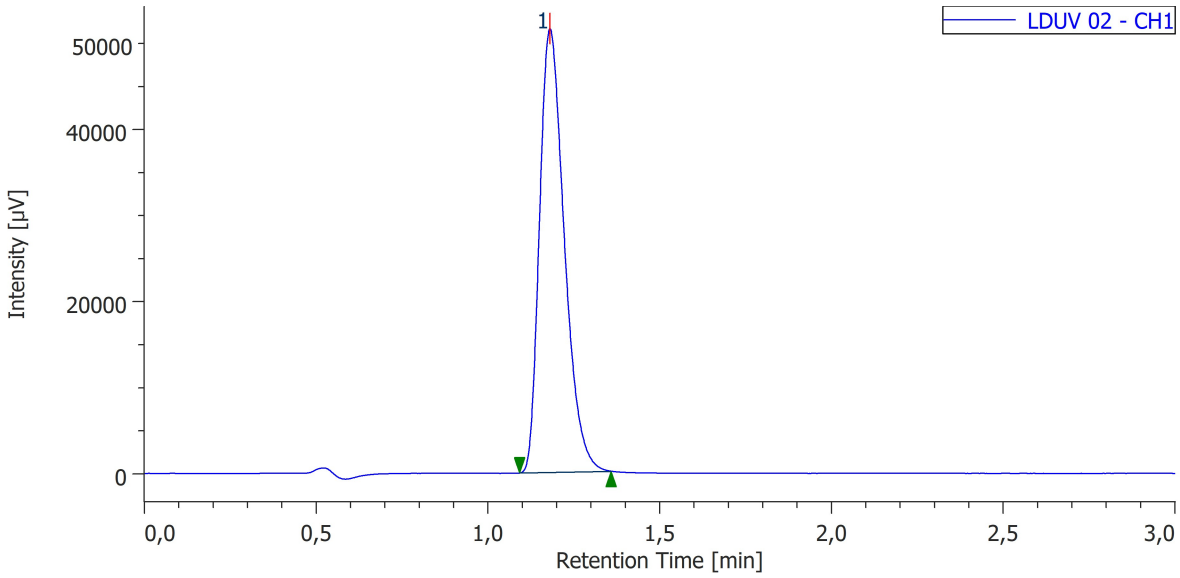

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 10:01:35
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 09:58:11
Volume	10,0 [µL]
Sample #	5
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,180	258360	51548	100,000	100,000	N/A	1293	N/A	1,368	

Creator Administrator
Reviewer
Approver

Chromatogram

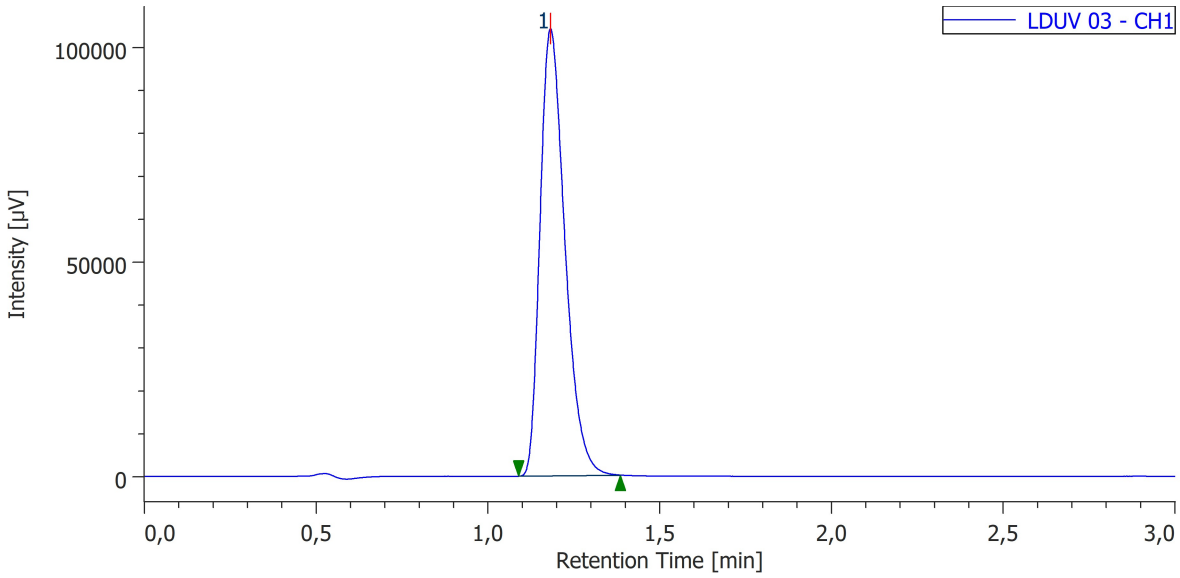

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 10:10:09
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 10:04:28
Volume	10,0 [µL]
Sample #	6
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,182	523450	104159	100,000	100,000	N/A	1297	N/A	1,372	

Creator Administrator
Reviewer
Approver

Chromatogram

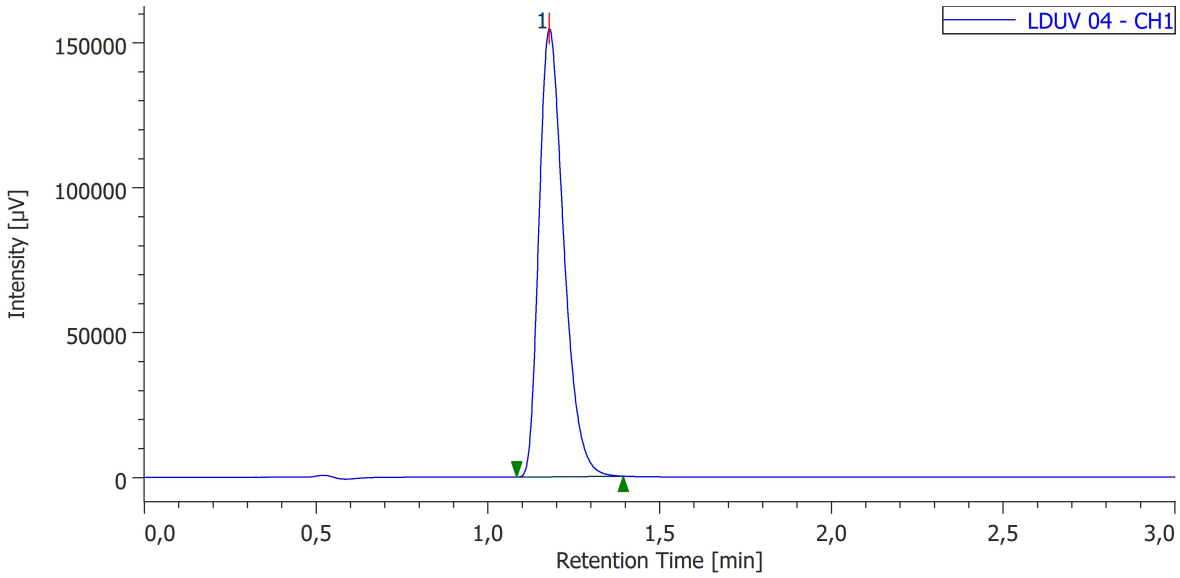

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 10:20:42
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 10:10:45
Volume	10,0 [µL]
Sample #	7
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,178	775080	154560	100,000	100,000	N/A	1298	N/A	1,375	

Creator Administrator
Reviewer
Approver

Chromatogram

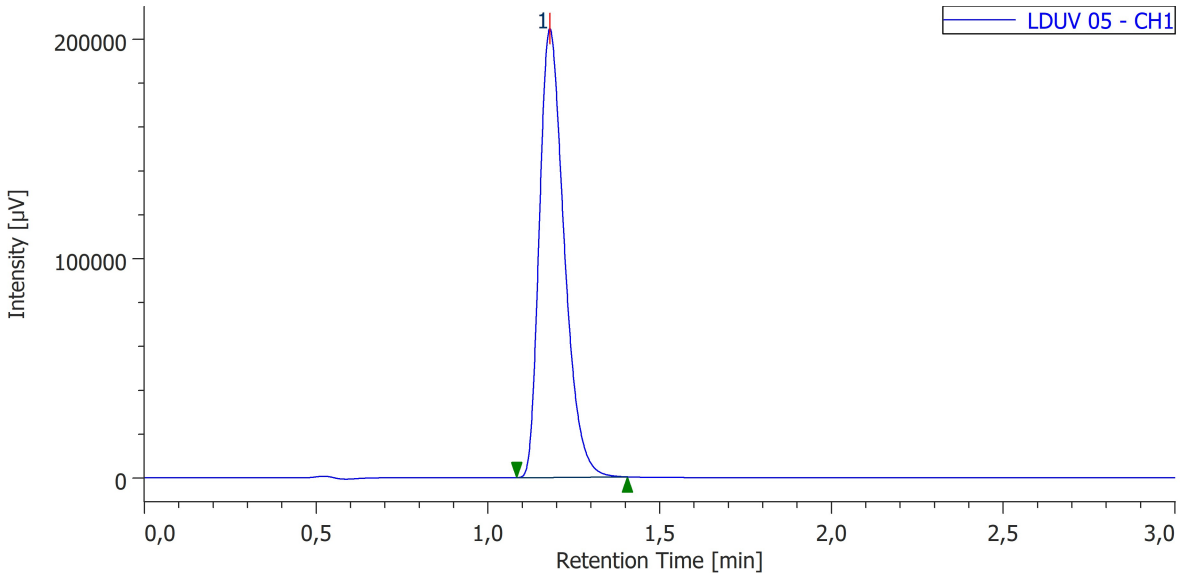

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 10:20:46
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 10:17:05
Volume	10,0 [µL]
Sample #	8
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,180	1026105	204464	100,000	100,000	N/A	1302	N/A	1,366	

Creator Administrator
Reviewer
Approver

Chromatogram

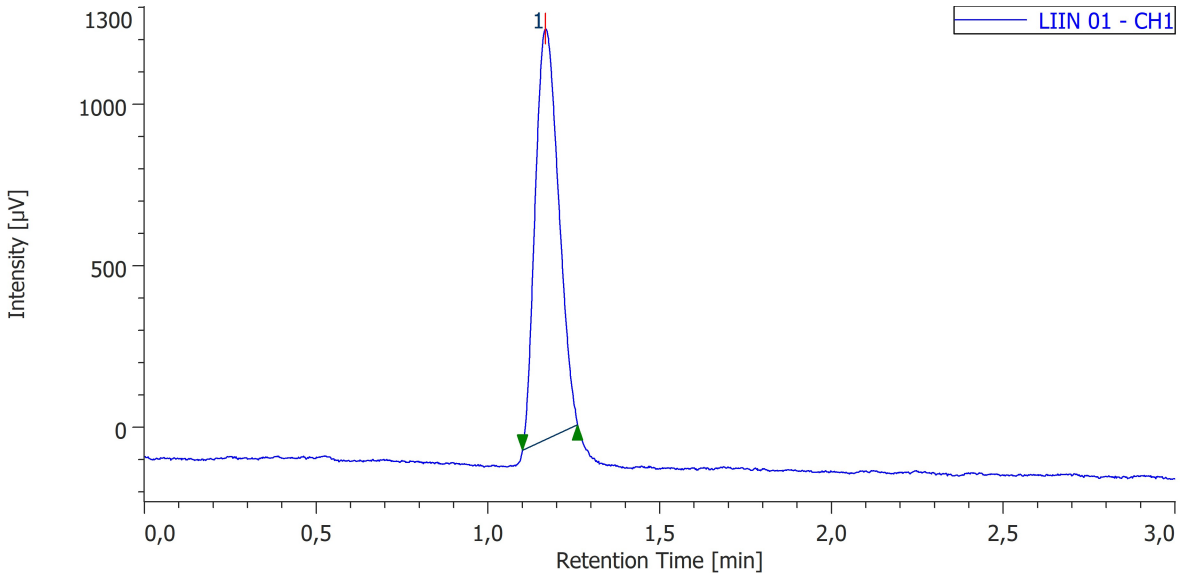

Chromatogram Information

User Name	Administrator
Date Modified	24/06/2026 11:30:08
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 11:20:26
Volume	0,1 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,167	5987	1271	100,000	100,000	N/A	1288	N/A	1,213	

Creator Administrator
Reviewer
Approver

Chromatogram

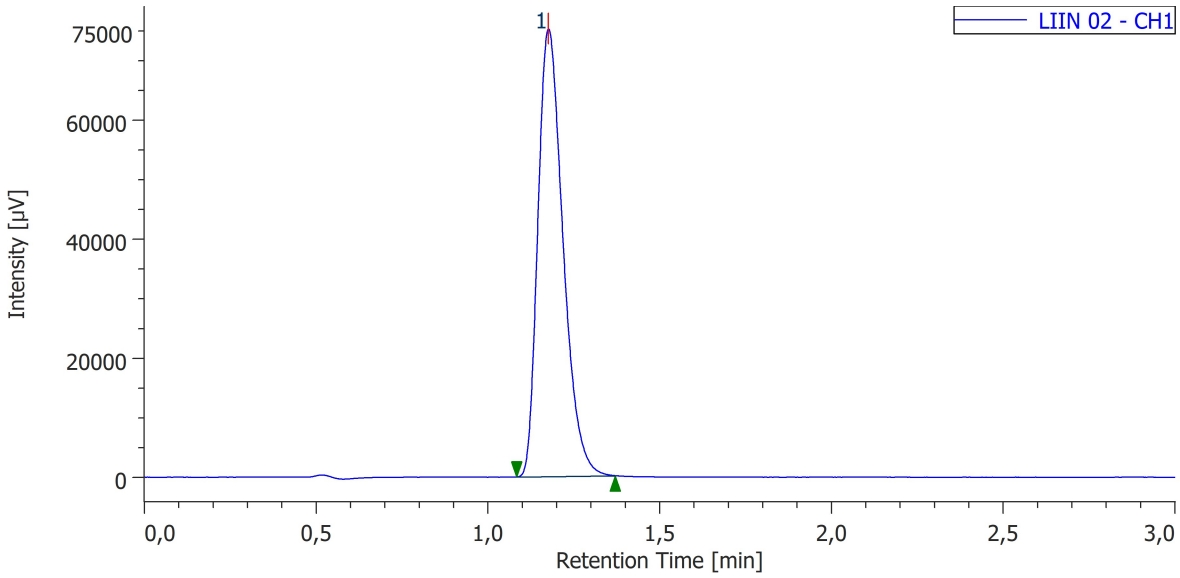

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 11:31:03
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 11:26:41
Volume	5,0 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,175	381692	75182	100,000	100,000	N/A	1251	N/A	1,377	

Creator Administrator
Reviewer
Approver

Chromatogram

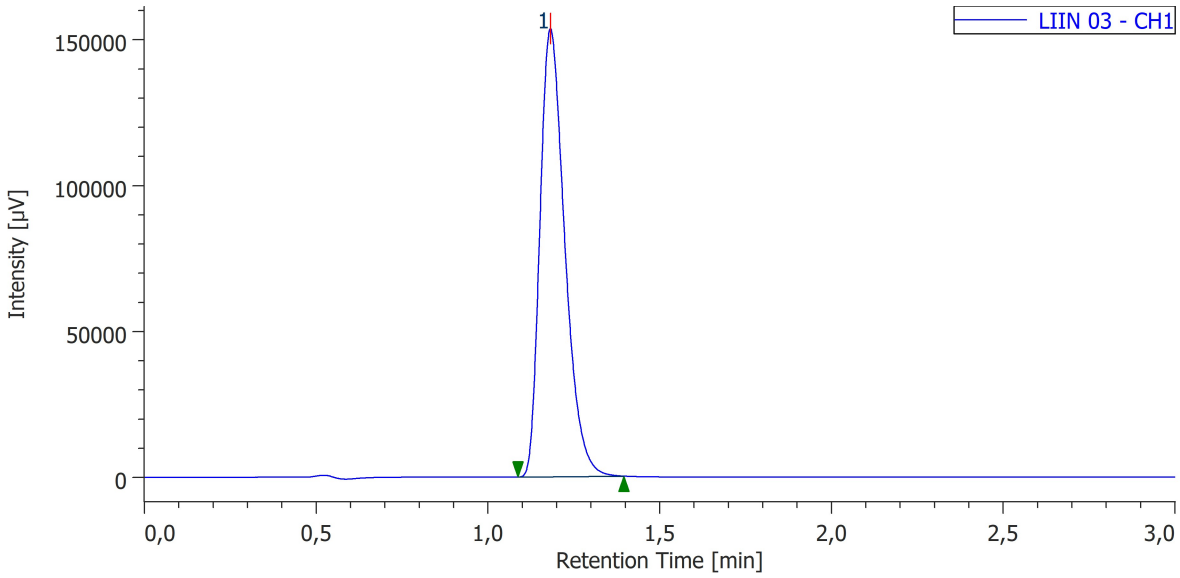

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 11:44:21
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 11:33:01
Volume	10,0 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,182	771132	153494	100,000	100,000	N/A	1300	N/A	1,368	

Creator Administrator
Reviewer
Approver

Chromatogram

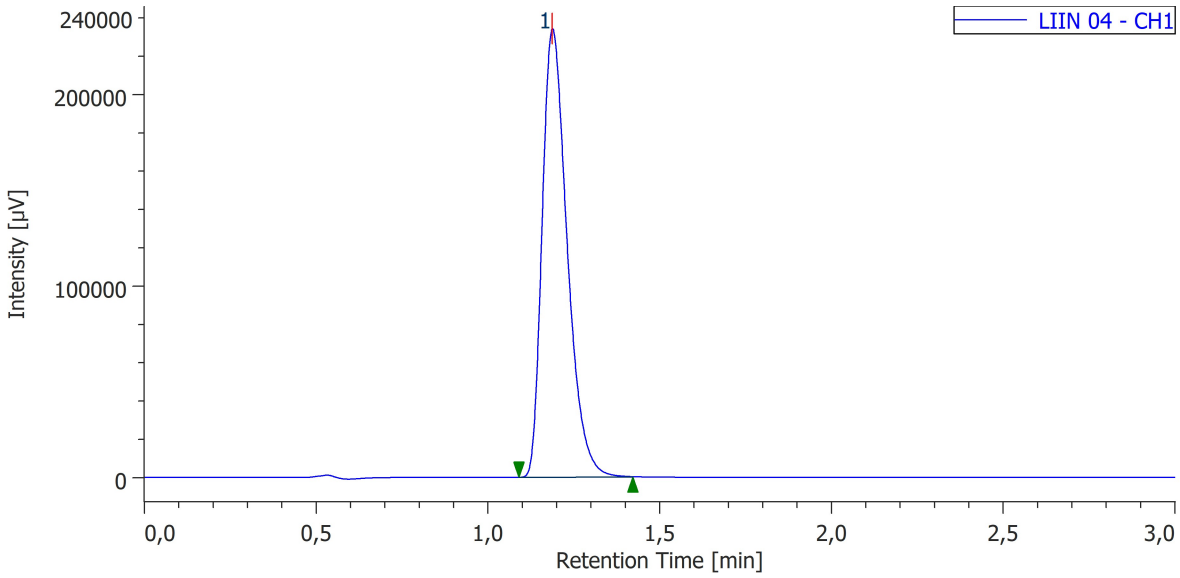

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 11:44:15
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 11:39:26
Volume	15,0 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,187	1181857	233983	100,000	100,000	N/A	1306	N/A	1,419	

Creator Administrator
Reviewer
Approver

Chromatogram

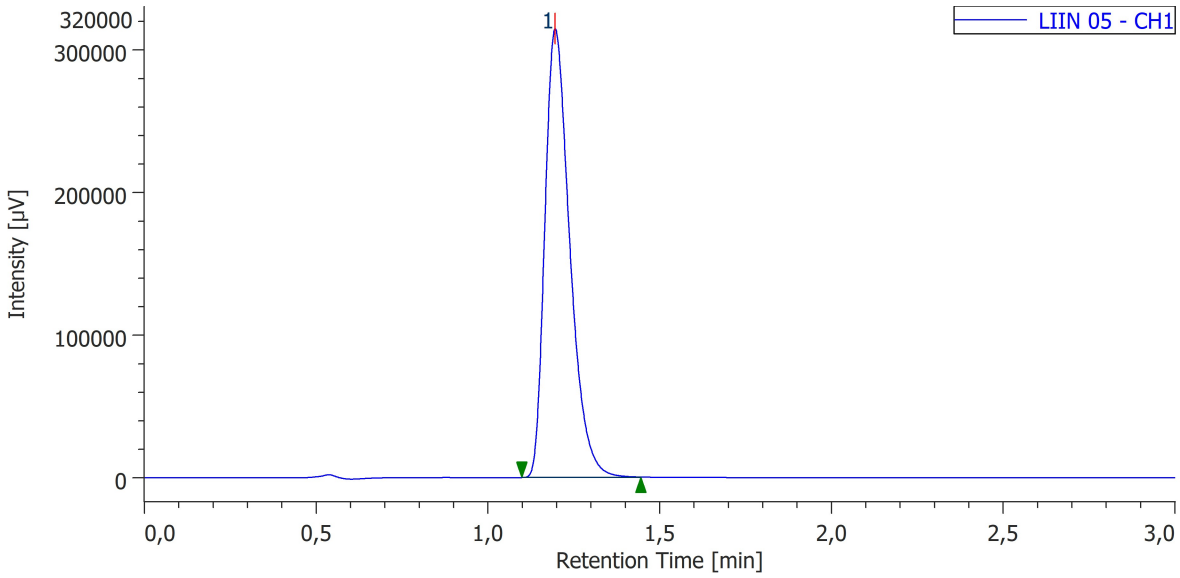

Chromatogram Information	
User Name	Administrator
Date Modified	24/06/2026 11:50:39
Description	
HPLC System Name	HPLC-0006
Injection Date	24/06/2026 11:45:56
Volume	20,0 [µL]
Sample #	10
Project Name	QPack
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	100 [msec]
Peak Method	Qualificação


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,195	1584447	314524	100,000	100,000	N/A	1337	N/A	1,416	

Creator Administrator
Reviewer
Approver

Certificado Nº: 105/25 -RELB	Início da Qualificação: 19/02/2025	Página 1 de 3

Resultado obtido na altura do pico


	ALTURA DO PICO (mAU)
Resultado:	**148,0710**

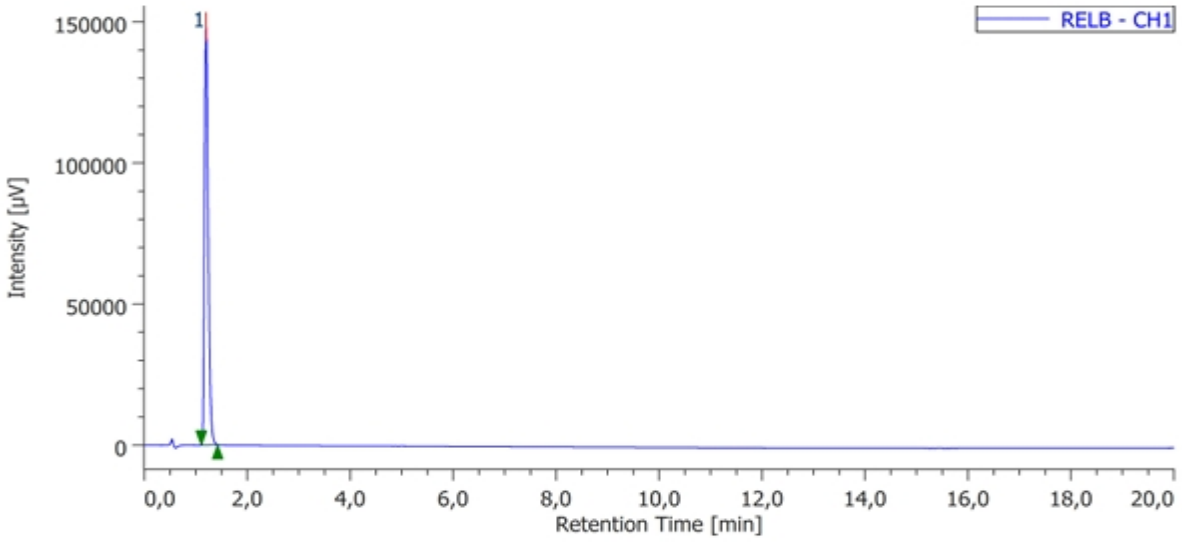

#	Peak Name	CH	tR [min]	Area [µV*sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	1	1,198	751644	148071	100,000	100,000	N/A	1319	N/A	1,422	

Resultado obtido no teste de sinal/ruído

Resultado:	Ruído (mAU)
VALOR MÁXIMO:	-1,1220
VALOR MÍNIMO:	-1,1260
	Ruído
	0,0040

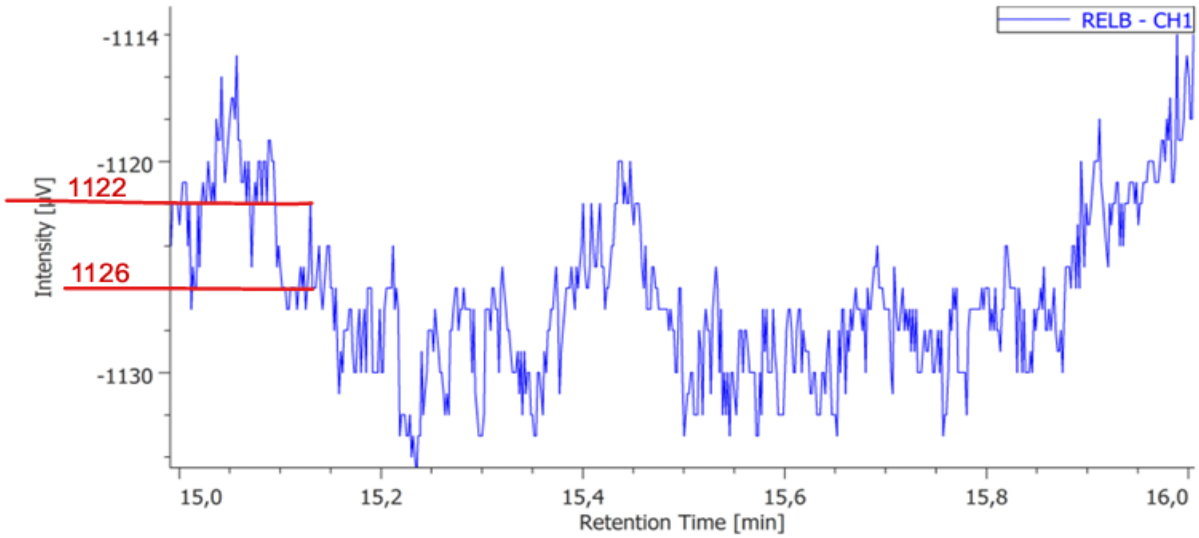

Resultado obtido no teste estabilidade da linha de base

Certificado de Qualificação

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	0,0570	-2,8890
VALOR MÍNIMO:	1,0200	
Resultado:	**-0,9630**	

