
Peak Find - EDUV.jws

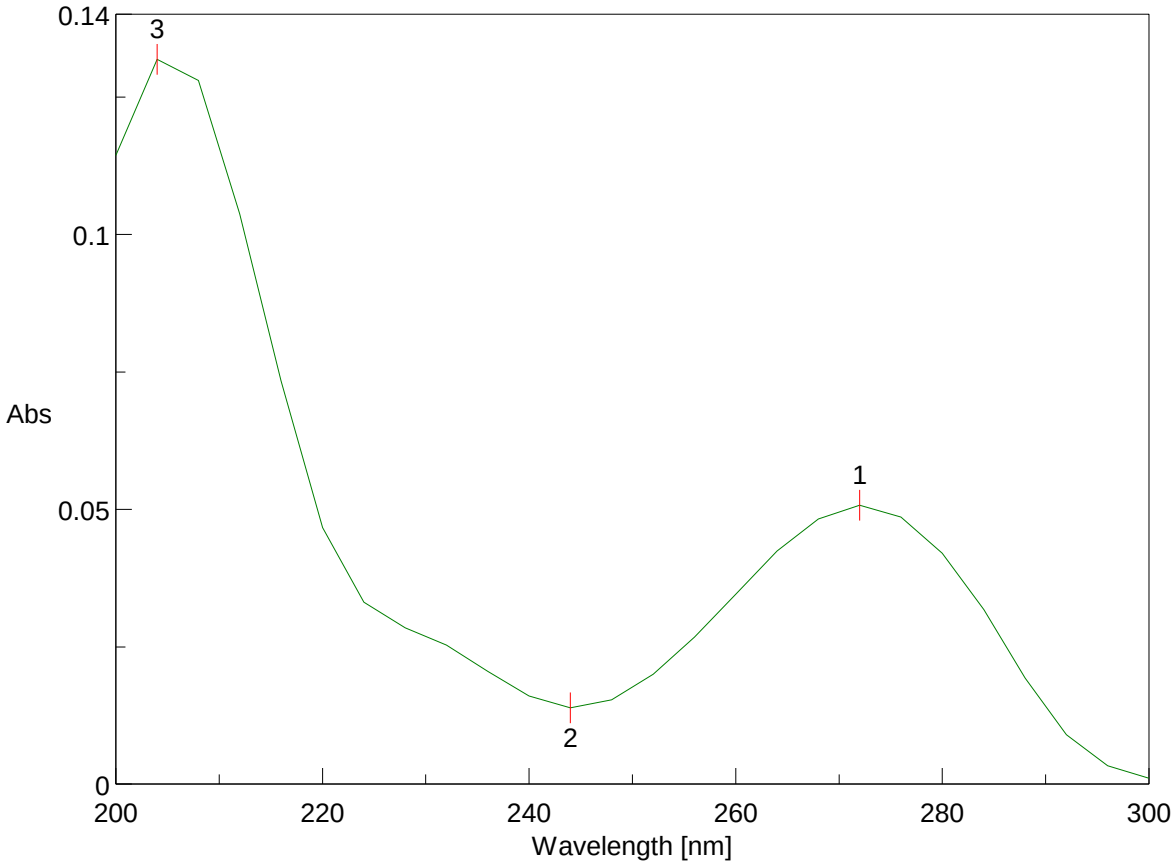

[Comments]

User	QPackSA
Division	---
Company	Cristalia
Creation date	19/06/2023 15:02

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	648 nm
Data interval	4 nm
Data points	113

[Measurement Information]


Instrument Name	MD-4010
Model Name	MD-4010
Serial No.	A024761665
ROM version	V1.02.02

[Result of Peak Picking]


No.	Position	Intensity	No.	Position	Intensity
1	272	0.050729	2	244	0.013858
3	204	0.131766			

Relatório SRELB

Detector UV – MD-4010 – N/S A024761665	Data: 19/06/2023
Ruído:	
Valor máximo: -28.7 mAU	**Diferença: 27.2 mAU**
Valor mínimo: -55.9 mAU	

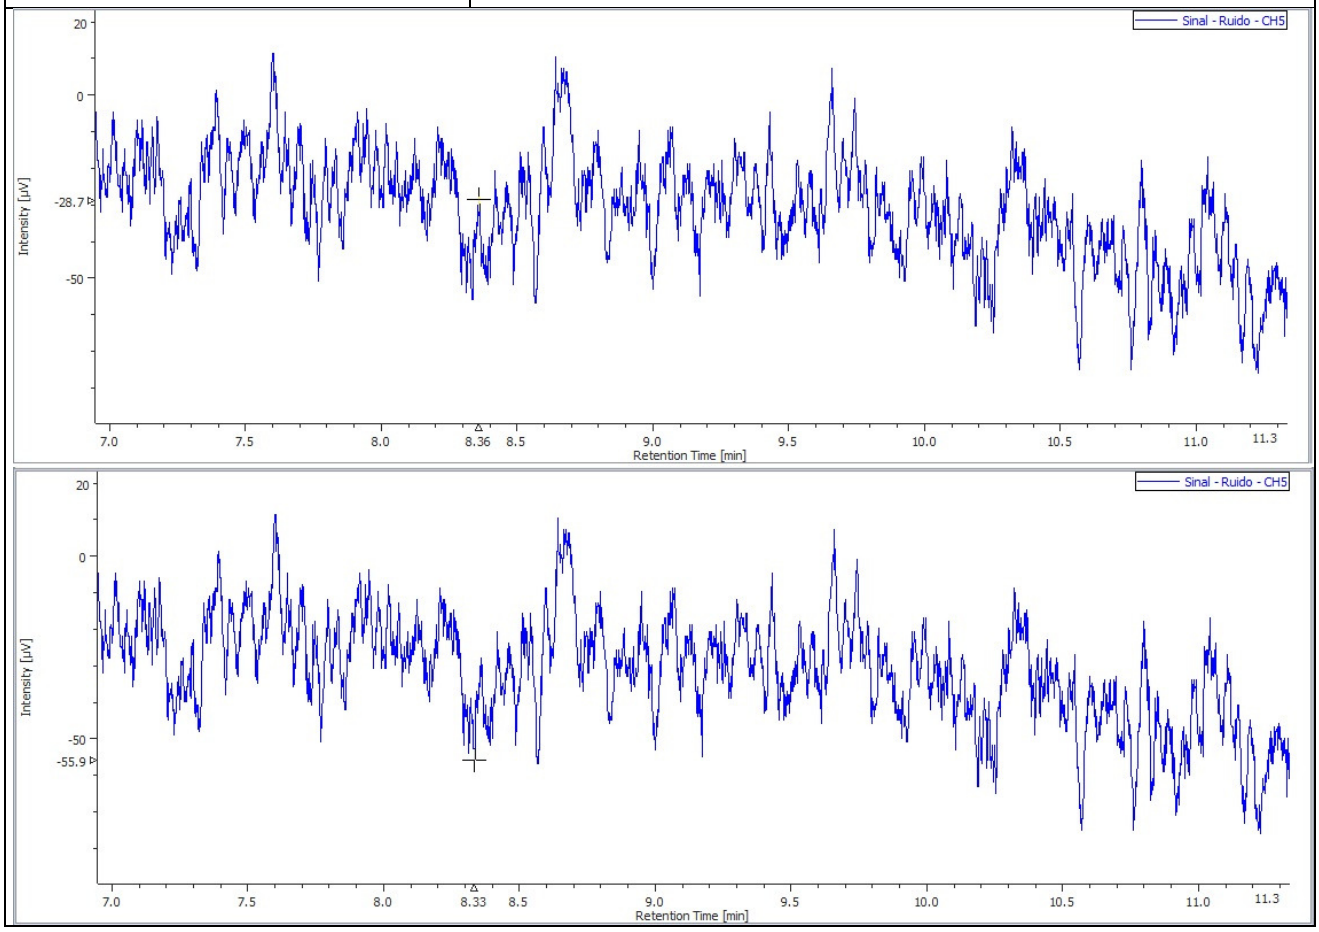


Estabilidade da Linha de Base:		
Valor máximo:	**-35.9 mAU**	**Diferença (em 20 minutos): 102.0 mAU**
Valor mínimo:	**-137.9 mAU**	**Diferença (em 60 minutos): 102.0 x 3 = 306 mAU**

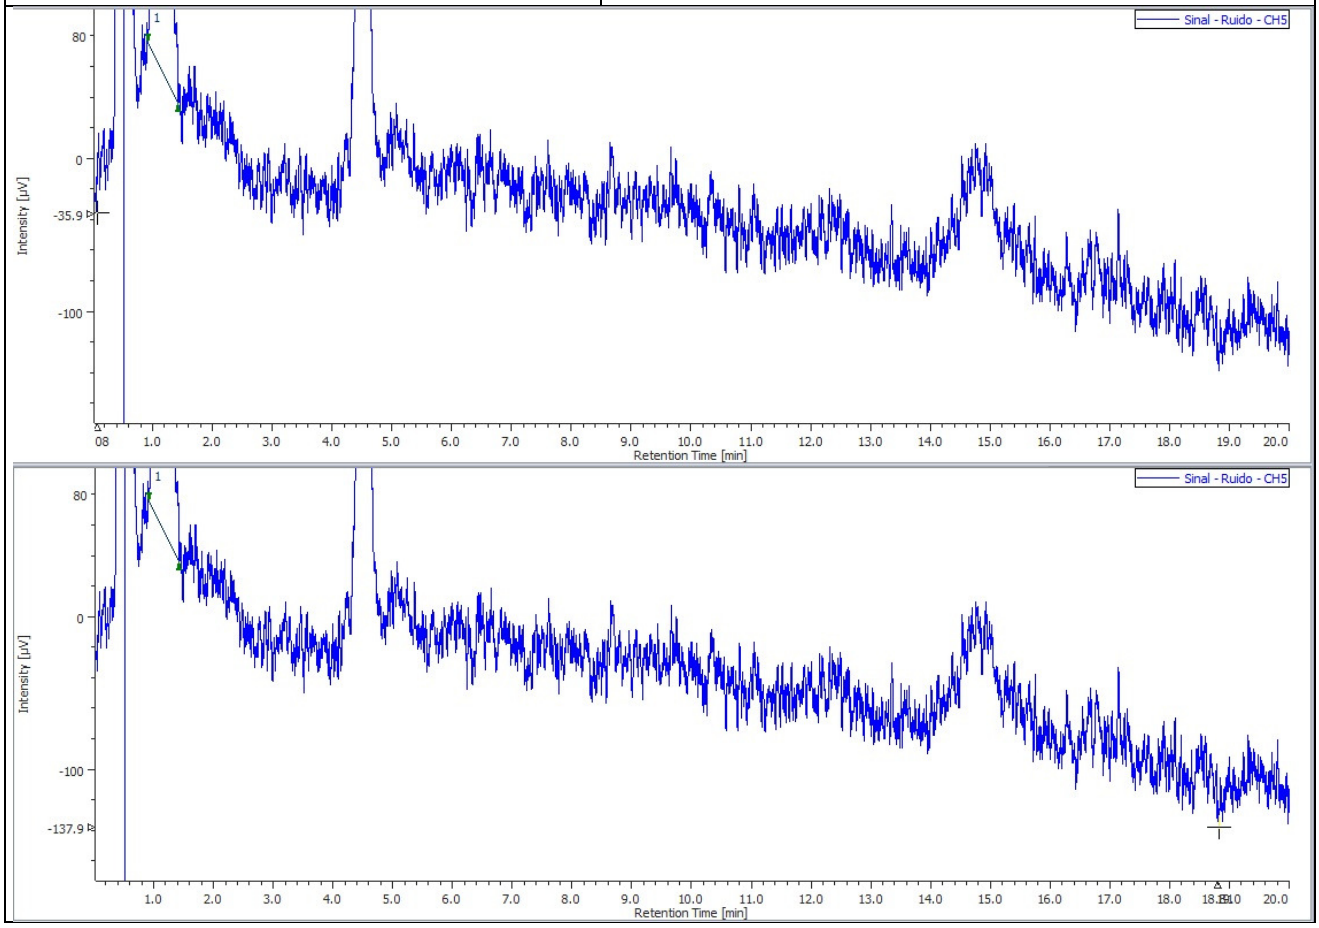


Altura do Pico:

Valor: 64102.2 mAU

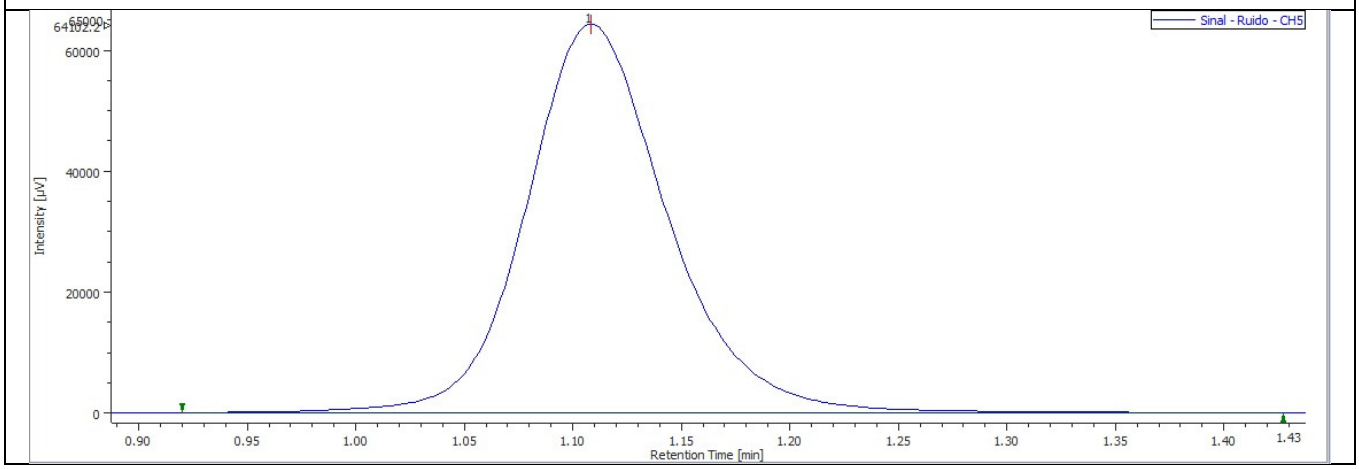

Chromatogram

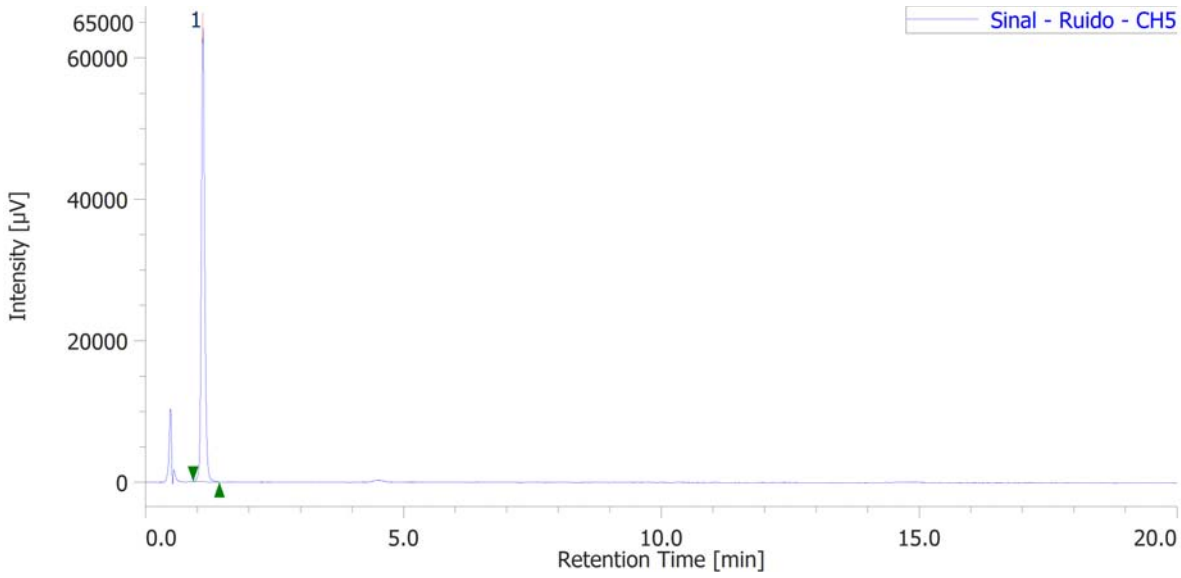

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:49:44
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 17:04:41
Volume	20.00 [µL]
Sample #	31
Project Name	Qualificação
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	Sinal-Ruido
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Sinal - Ruido-CH5
Sample Name	Sinal - Ruido
Channel Name	250.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.108	291287	64090	100.000	100.000	N/A	1521	N/A	1.161	

Creator QPackSA
Reviewer
Approver

Chromatogram

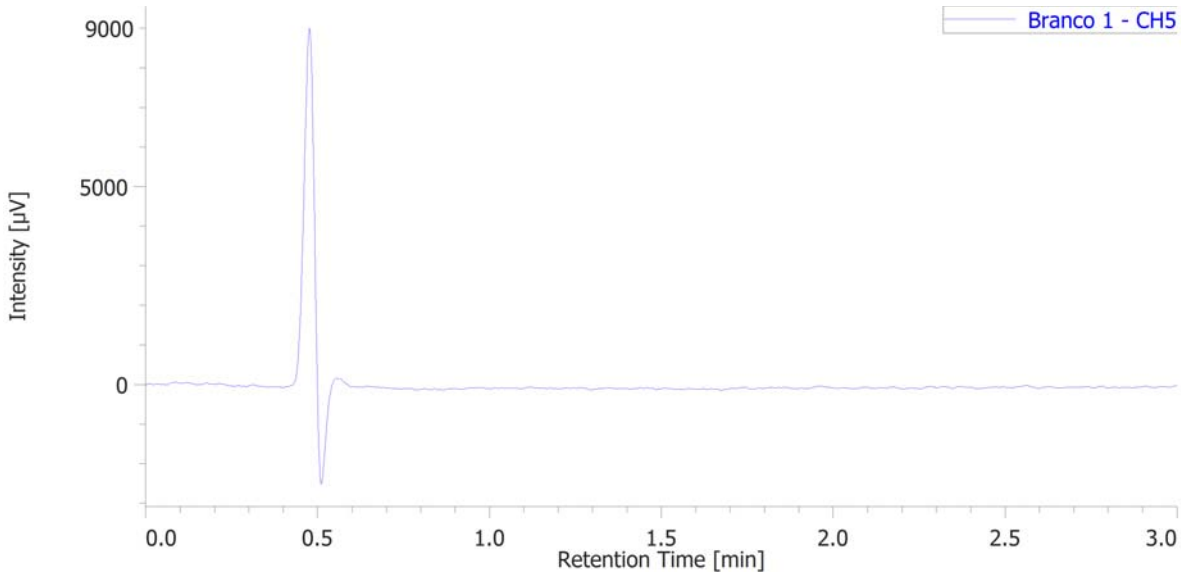


Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:01
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:43:42
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	Branco 1
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

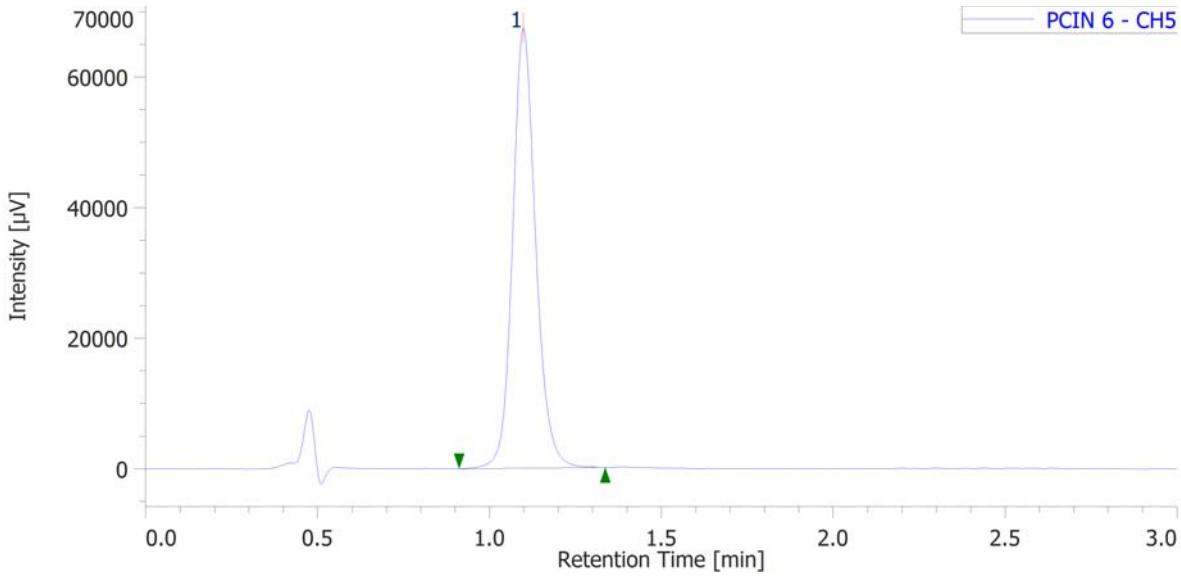

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:05
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:06:05
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	PCIN 6
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	314424	67334	100.000	100.000	N/A	1386	N/A	1.142	

Creator QPackSA
Reviewer
Approver

Chromatogram

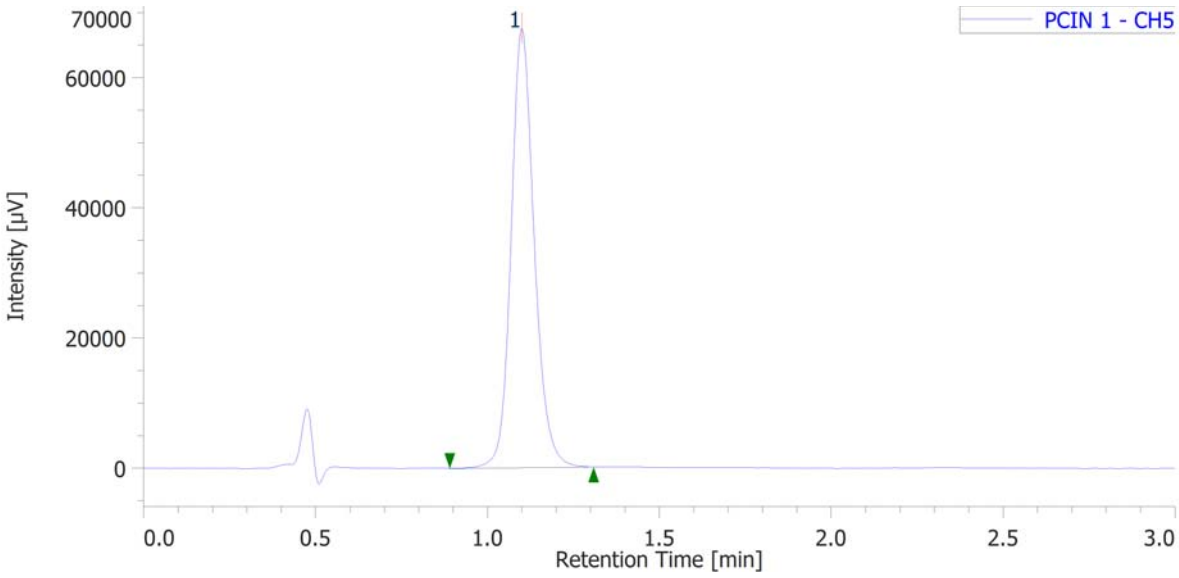

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:02
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:46:54
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	PCIN 1
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.100	316015	67509	100.000	100.000	N/A	1382	N/A	1.153	

Creator QPackSA
Reviewer
Approver

Chromatogram

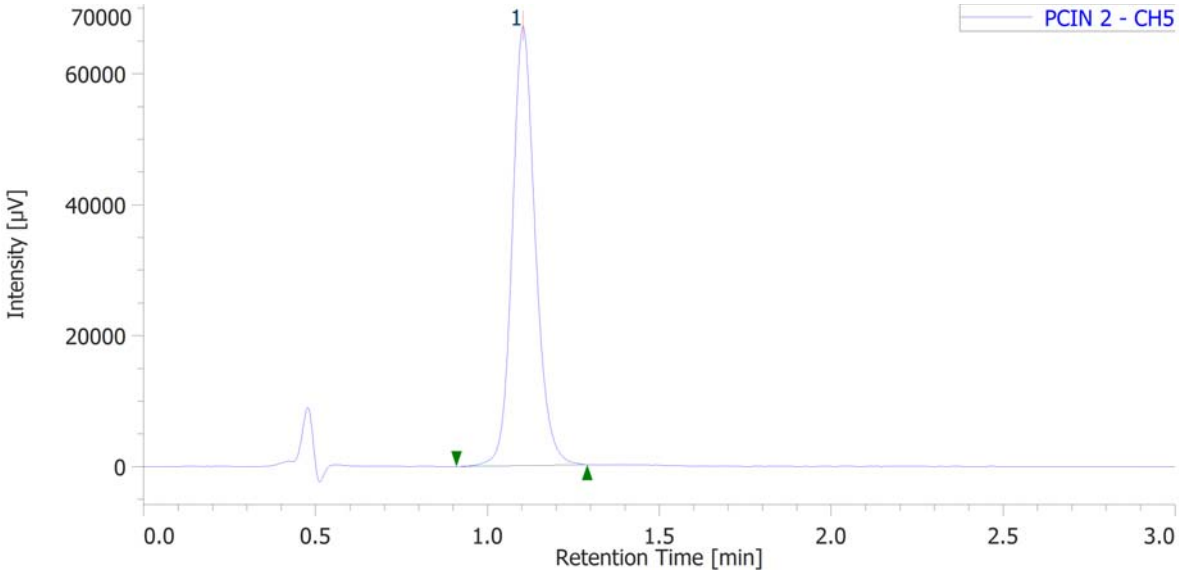

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:03
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:50:06
Volume	10.00 [μL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	PCIN 2
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.103	313589	67102	100.000	100.000	N/A	1391	N/A	1.147	

Creator QPackSA
Reviewer
Approver

Chromatogram

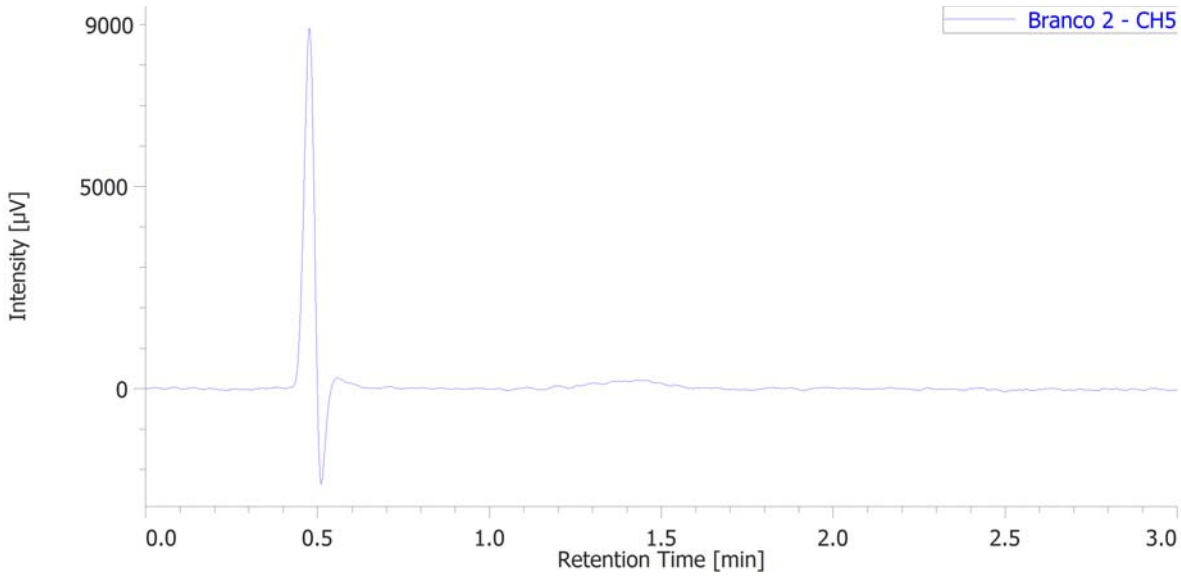


Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:04
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:56:30
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	Branco 2
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

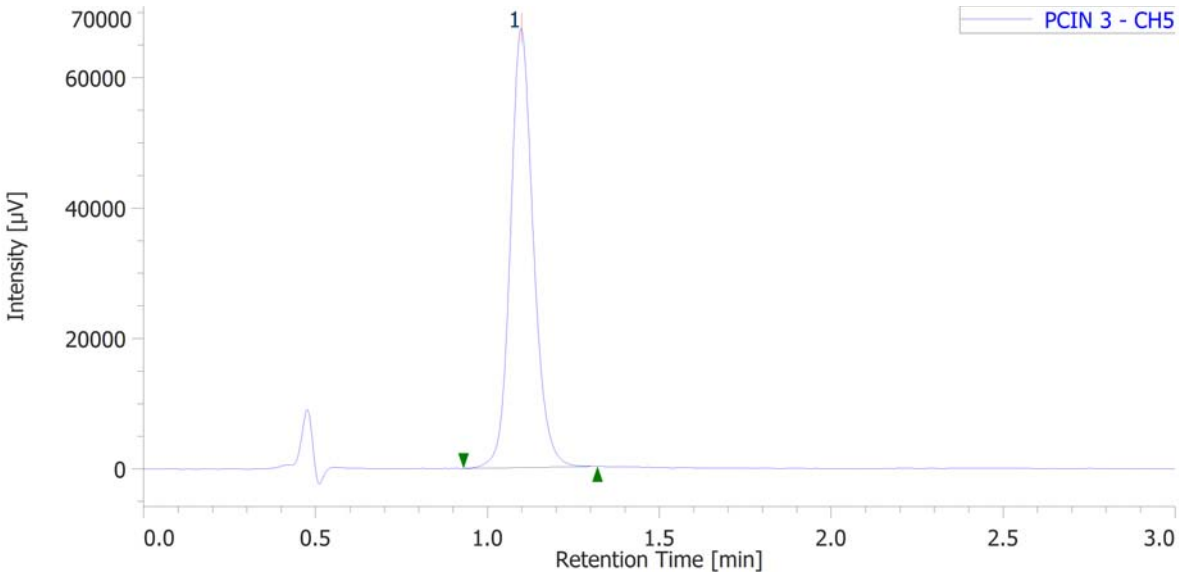

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:03
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:53:18
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	PCIN 3
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	313184	67342	100.000	100.000	N/A	1390	N/A	1.131	

Creator QPackSA
Reviewer
Approver

Chromatogram

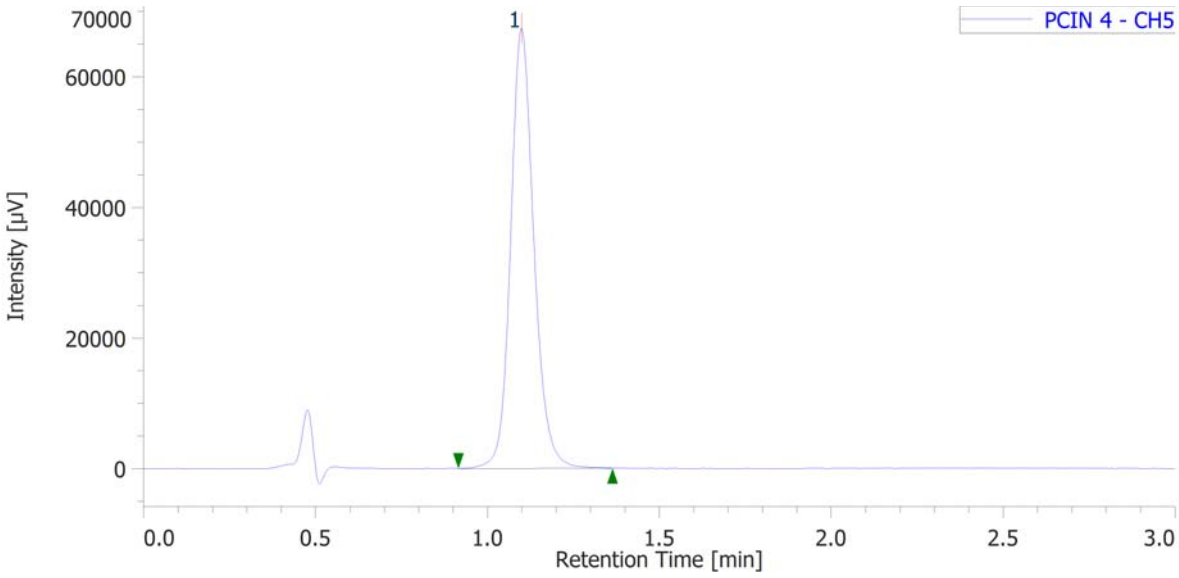

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:04
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 15:59:42
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	PCIN 4
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	316610	67355	100.000	100.000	N/A	1373	N/A	1.154	

Creator QPackSA
Reviewer
Approver

Chromatogram

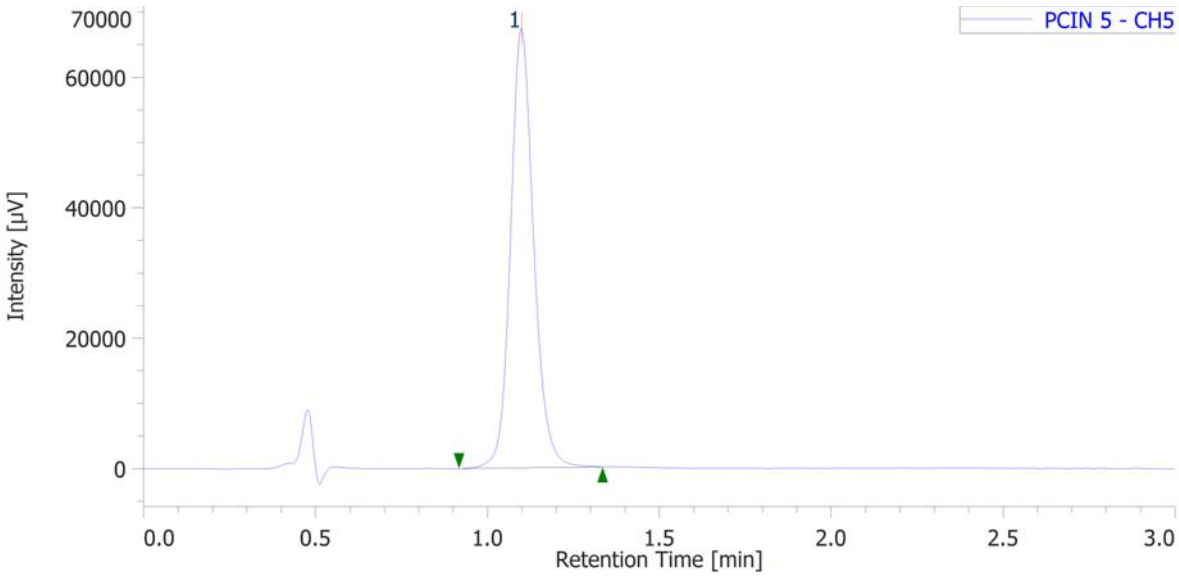

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:05
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:02:53
Volume	10.00 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	PCIN 5
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	315387	67417	100.000	100.000	N/A	1380	N/A	1.144	

Creator QPackSA
Reviewer
Approver

Chromatogram

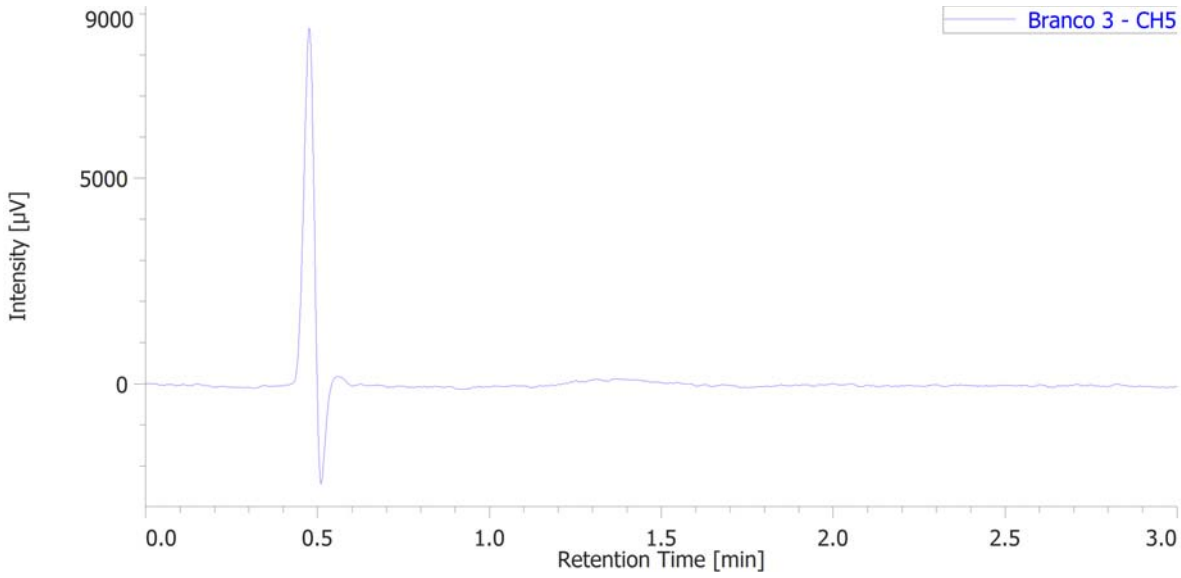


Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 07:47:05
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:09:17
Volume	10.00 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	Branco 3
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

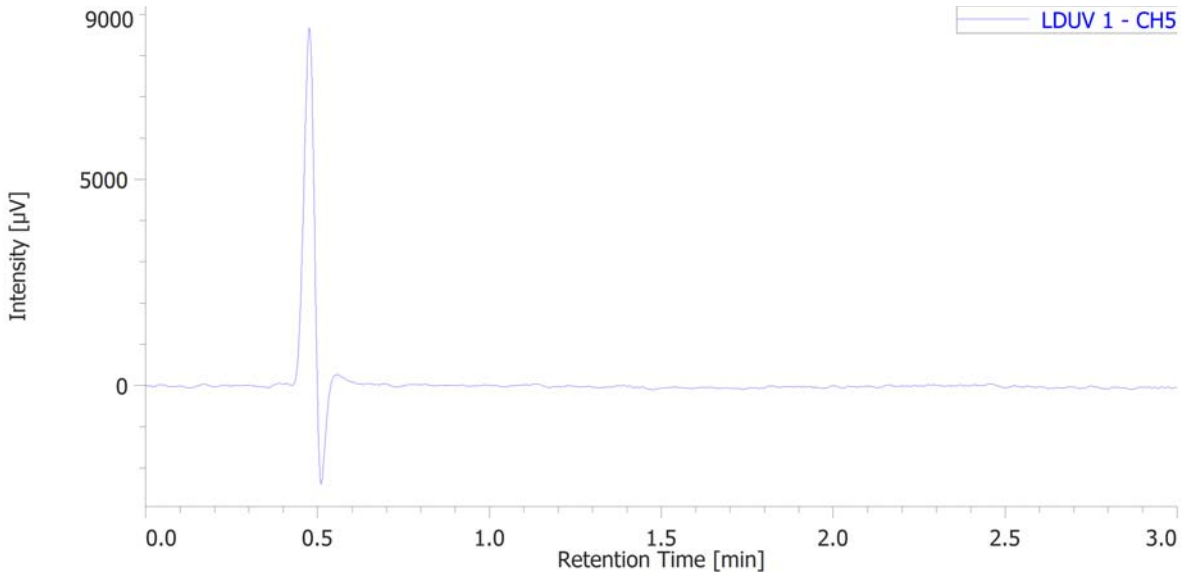


Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:24:53
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:12:29
Volume	10.00 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	LDUV 1
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

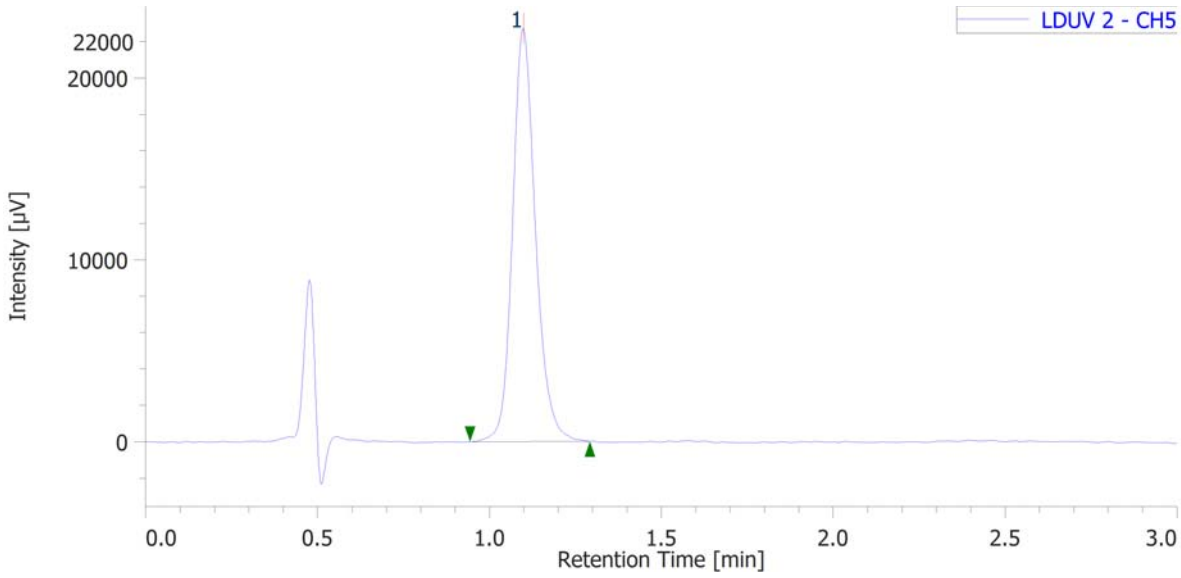

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:24:54
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:15:41
Volume	10.00 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	LDUV 2
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	105432	22713	100.000	100.000	N/A	1410	N/A	1.172	

Creator QPackSA
Reviewer
Approver

Chromatogram

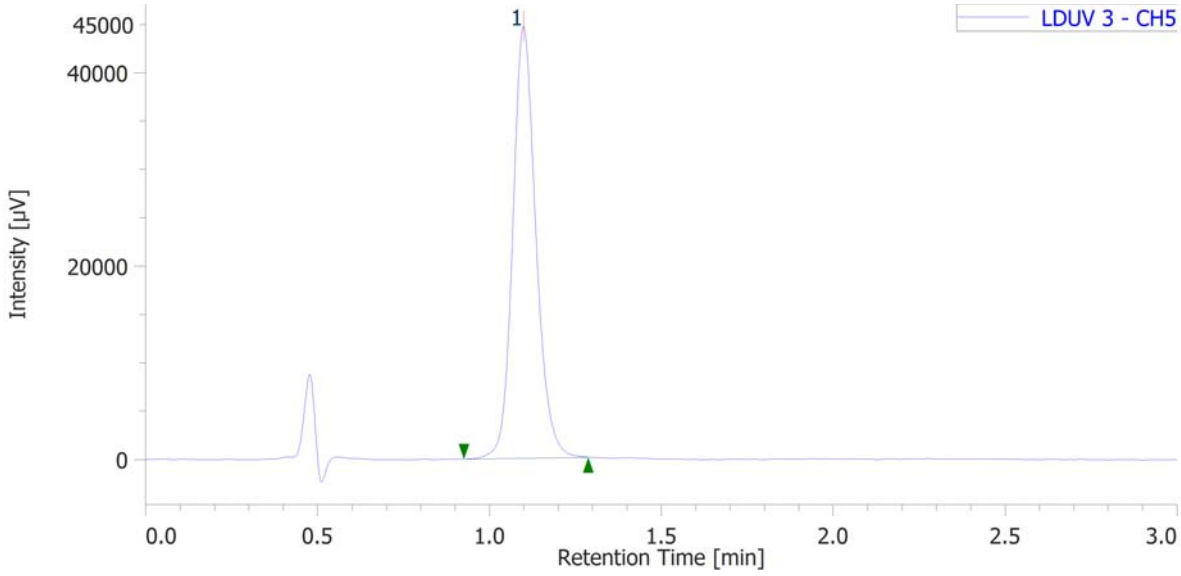

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:24:55
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:18:53
Volume	10.00 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	LDUV 3
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.098	209017	44668	100.000	100.000	N/A	1366	N/A	1.161	

Creator QPackSA
Reviewer
Approver

Chromatogram

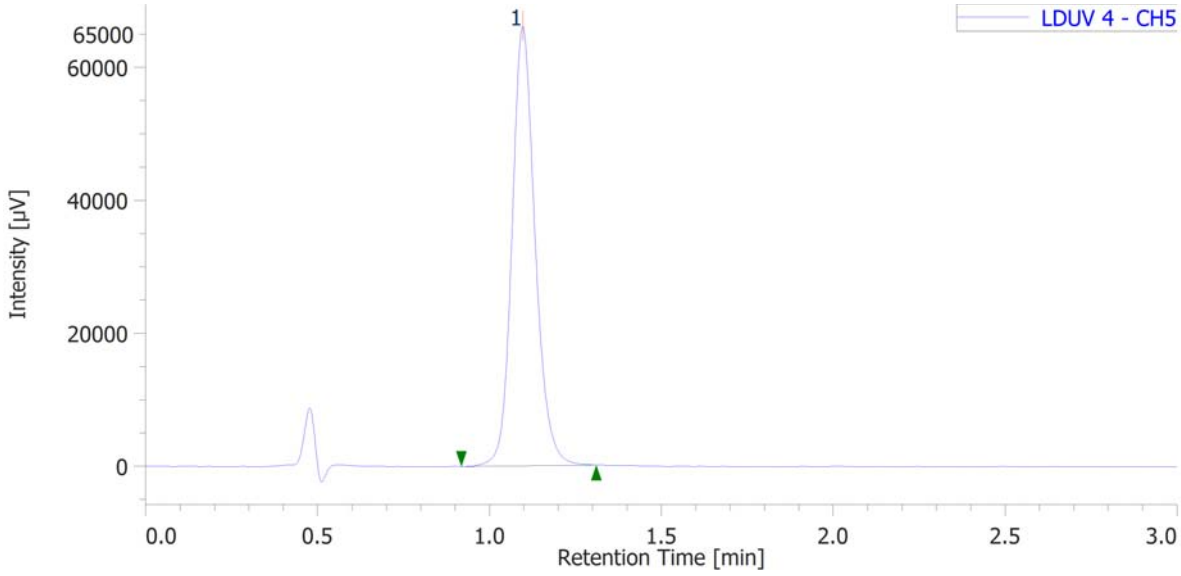

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:24:55
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:22:05
Volume	10.00 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	LDUV 4
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.097	308665	66061	100.000	100.000	N/A	1372	N/A	1.155	

Creator QPackSA
Reviewer
Approver

Chromatogram

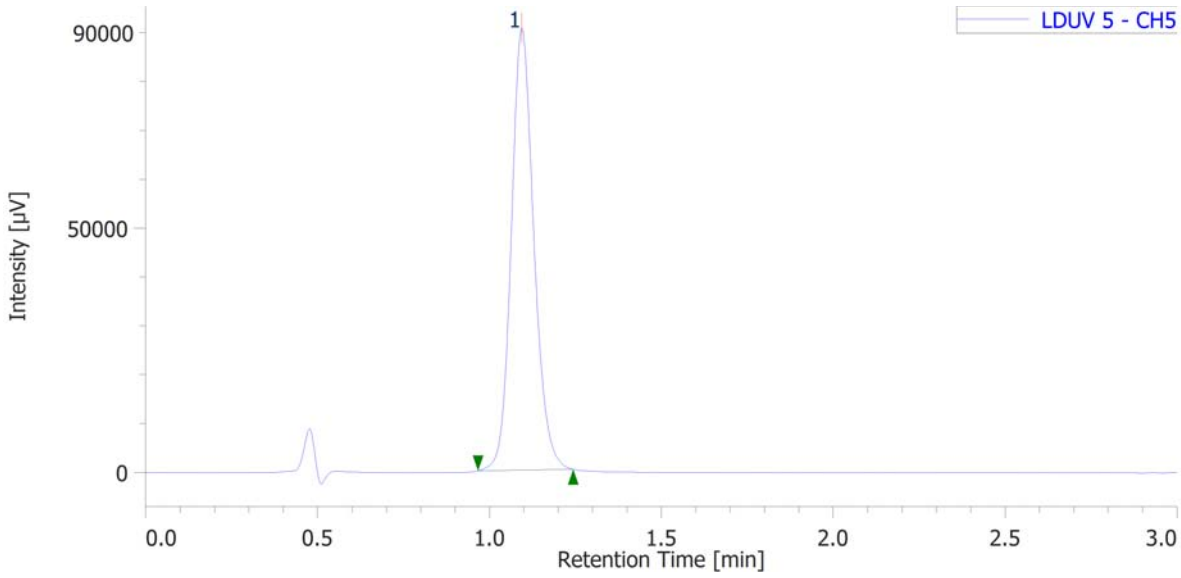

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:33:47
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:25:17
Volume	10.00 [μL]
Sample #	15
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	LDUV 5
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.093	413021	90354	100.000	100.000	N/A	1399	N/A	1.156	

Creator QPackSA
Reviewer
Approver

Chromatogram

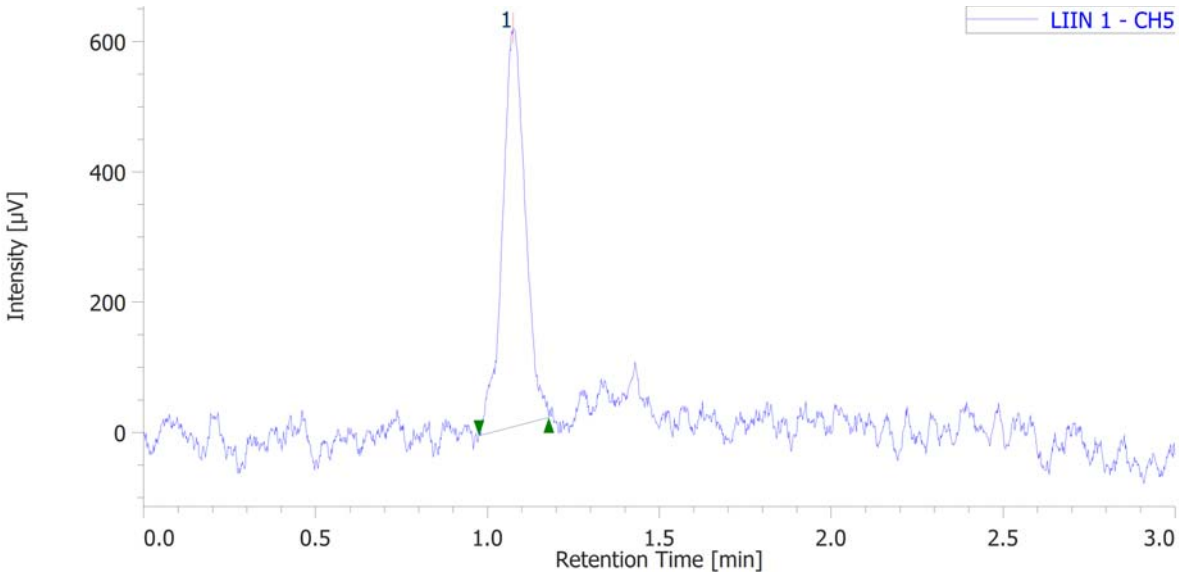

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:38:46
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:28:29
Volume	0.10 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	LIIN 1
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.075	2811	611	100.000	100.000	N/A	1321	N/A	1.049	

Creator QPackSA
Reviewer
Approver

Chromatogram

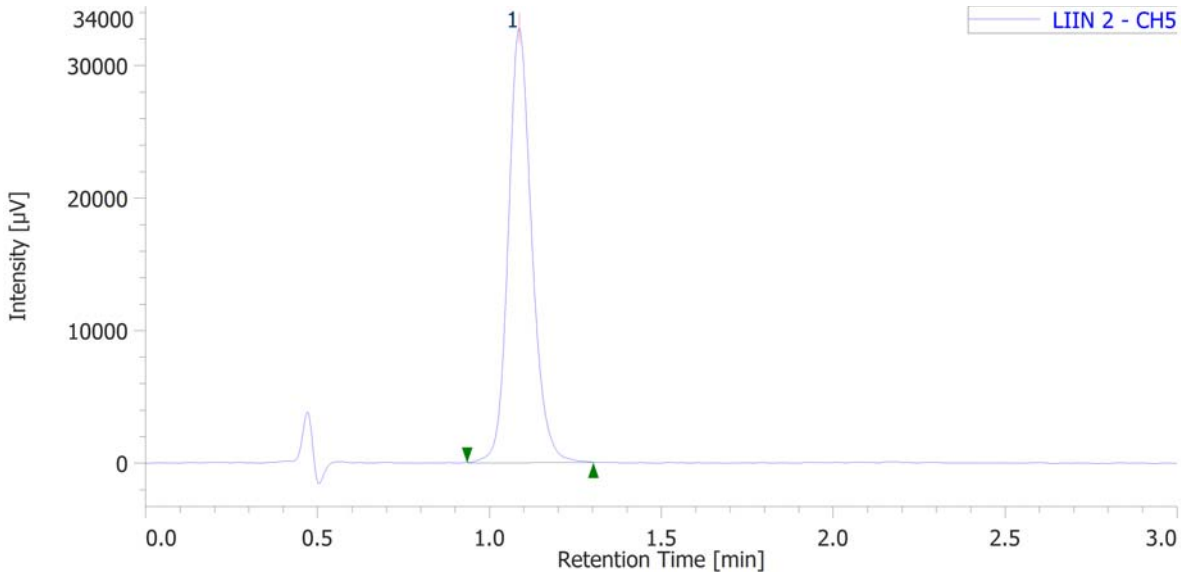

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:38:47
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:31:41
Volume	5.00 [μL]
Sample #	21
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	LIIN 2
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.087	155639	32731	100.000	100.000	N/A	1303	N/A	1.157	

Creator QPackSA
Reviewer
Approver

Chromatogram

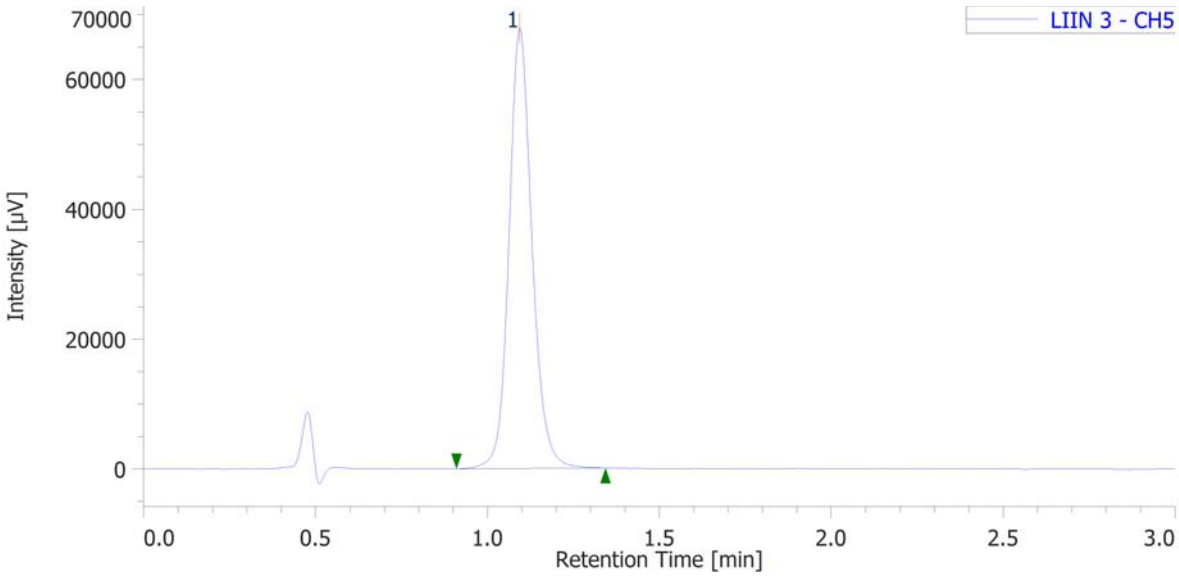

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:38:48
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:34:53
Volume	10.00 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	LIIN 3
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.093	315653	67759	100.000	100.000	N/A	1389	N/A	1.142	

Creator QPackSA
Reviewer
Approver

Chromatogram

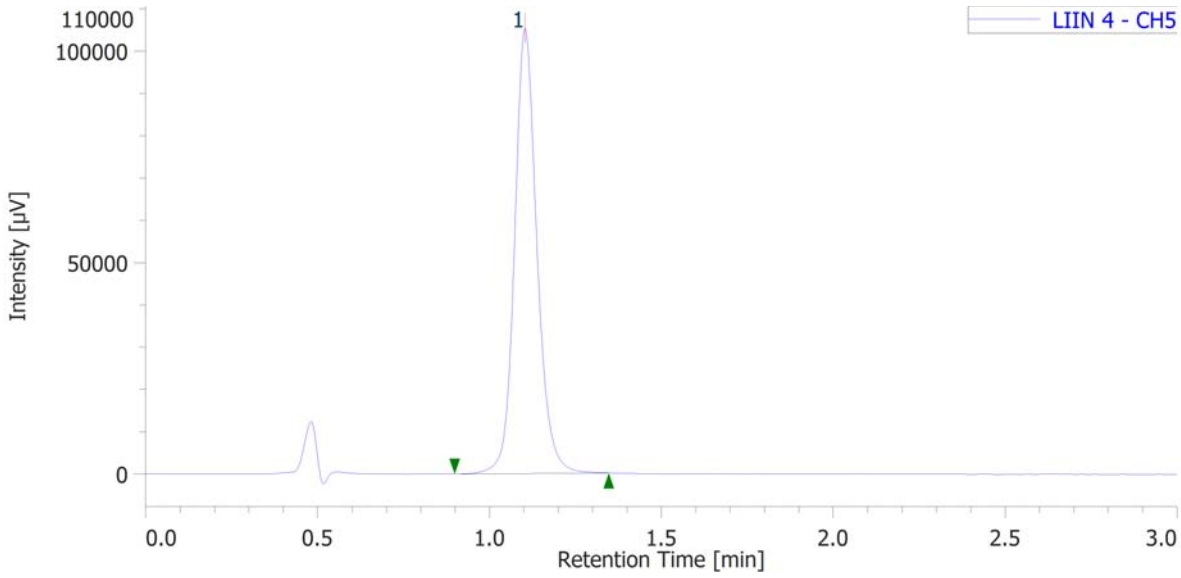

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:38:48
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:38:05
Volume	15.00 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	LIIN 4
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.103	475869	105275	100.000	100.000	N/A	1516	N/A	1.140	

Creator QPackSA
Reviewer
Approver

Chromatogram

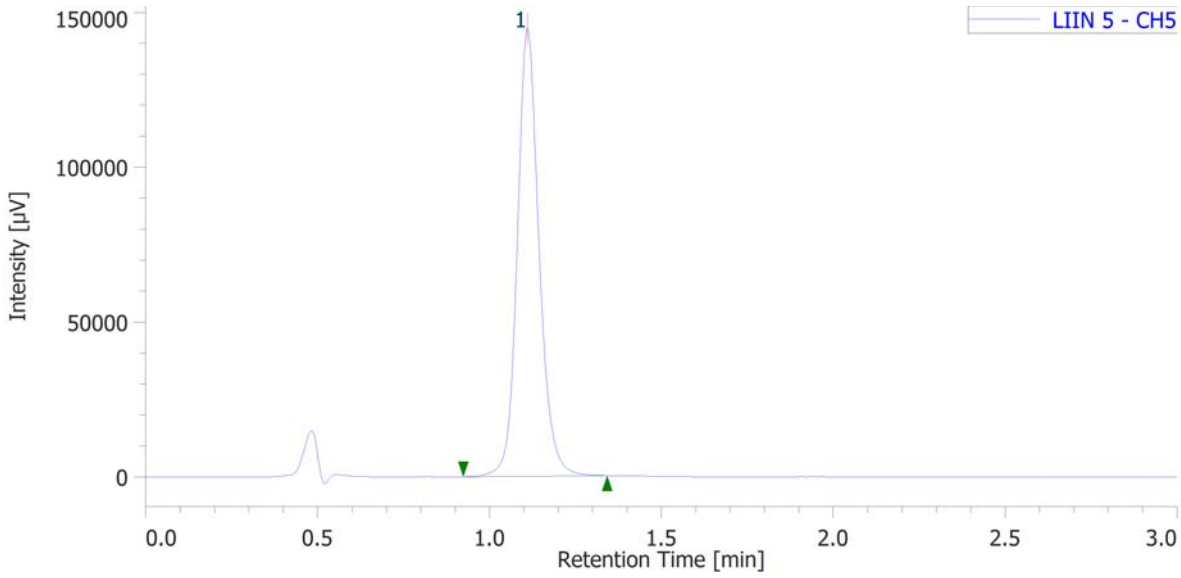

Chromatogram Information	
User Name	QPackSA
Date Modified	20/06/2023 08:38:49
Description	
HPLC System Name	CG033985_001
Injection Date	19/06/2023 16:41:17
Volume	20.00 [µL]
Sample #	21
Project Name	Qualificação
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	LIIN 5
Channel Name	273.0nm
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1.110	636930	144551	100.000	100.000	N/A	1611	N/A	1.150	

Creator QPackSA
Reviewer
Approver