
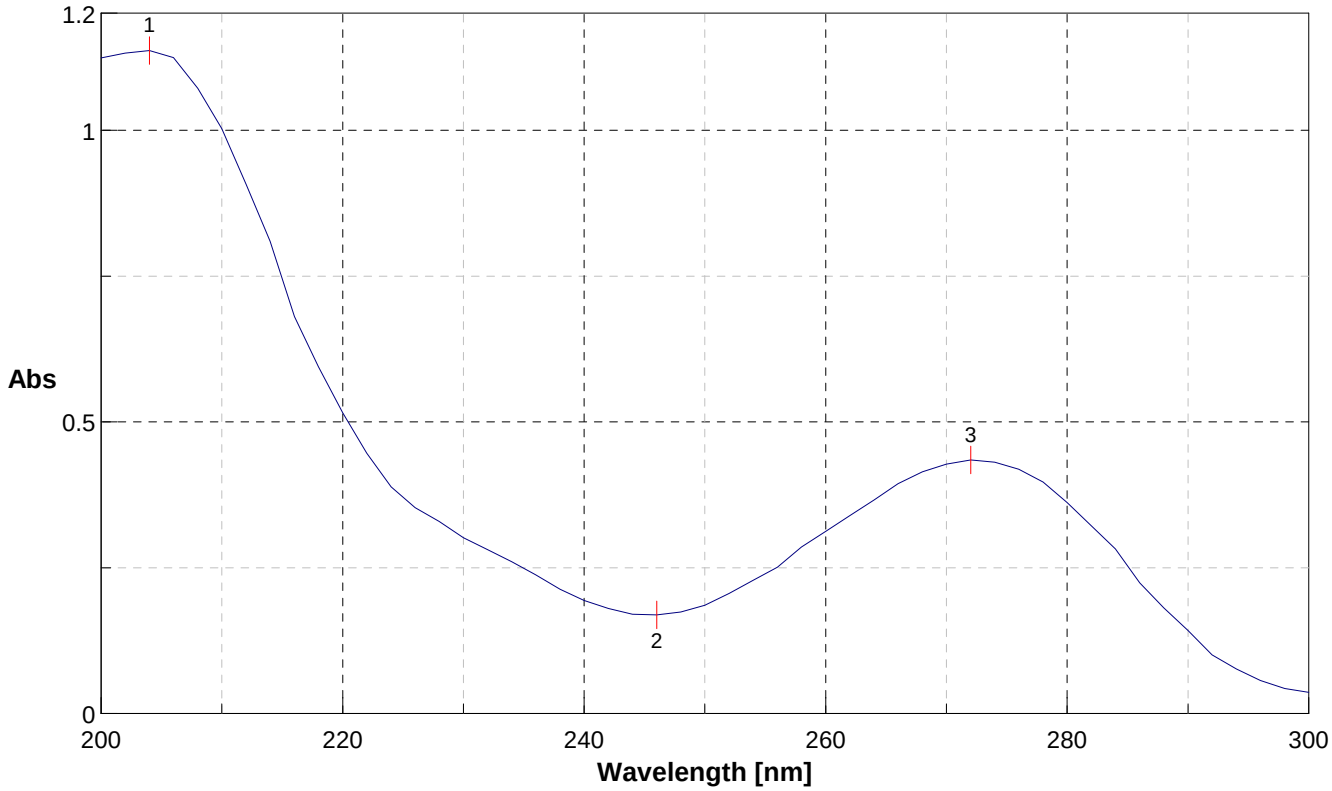


Date	5/12/2016 12:04
File name	EDUV_003 UV_tR0,17 D.jws
Model	UV-2070
Serial No.	0000000000
Sample name	
Operator	Administrator
Comment	---

No.	nm	Abs	No.	nm	Abs	No.	nm	Abs
1	204	1.13638	2	246	0.169376	3	272	0.43483

Chromatogram

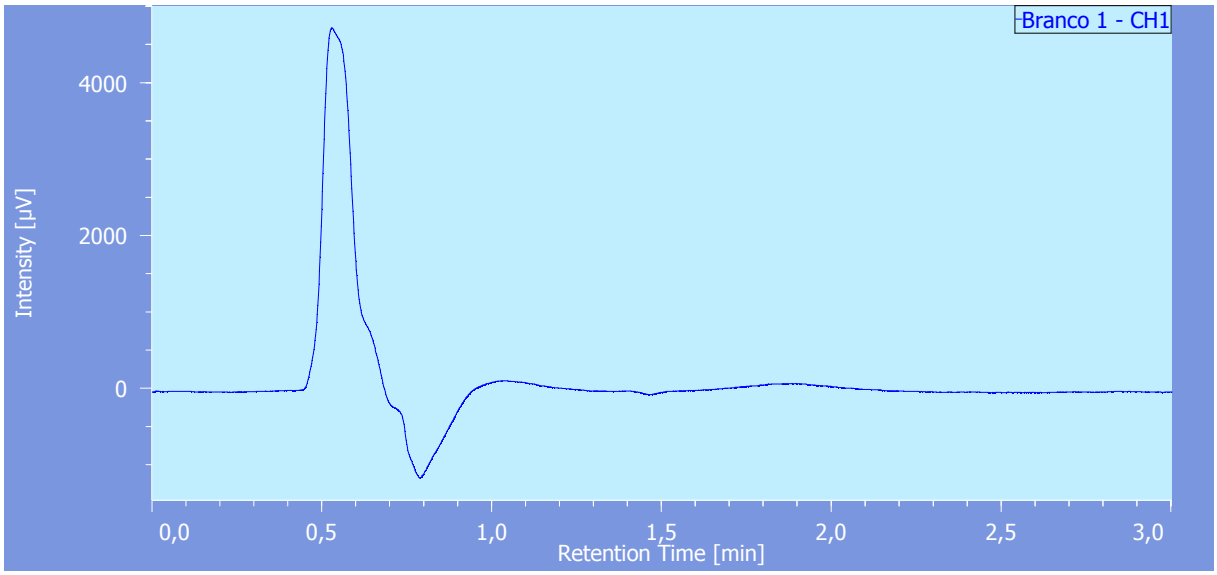


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:01
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:10:41
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

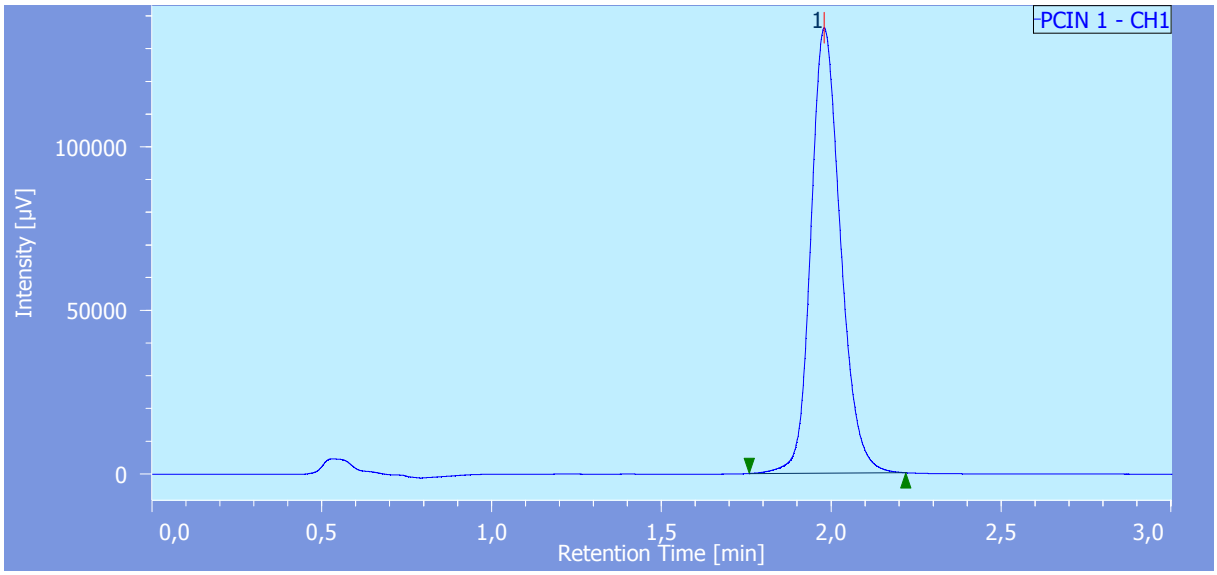

Chromatogram Information

User Name	Administrator
Date Modified	5/12/2016 14:51:02
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:15:05
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,978	824879	135942	100,000	100,000	N/A	2574	N/A	1,202	

Creator Administrator
Reviewer
Approver

Chromatogram

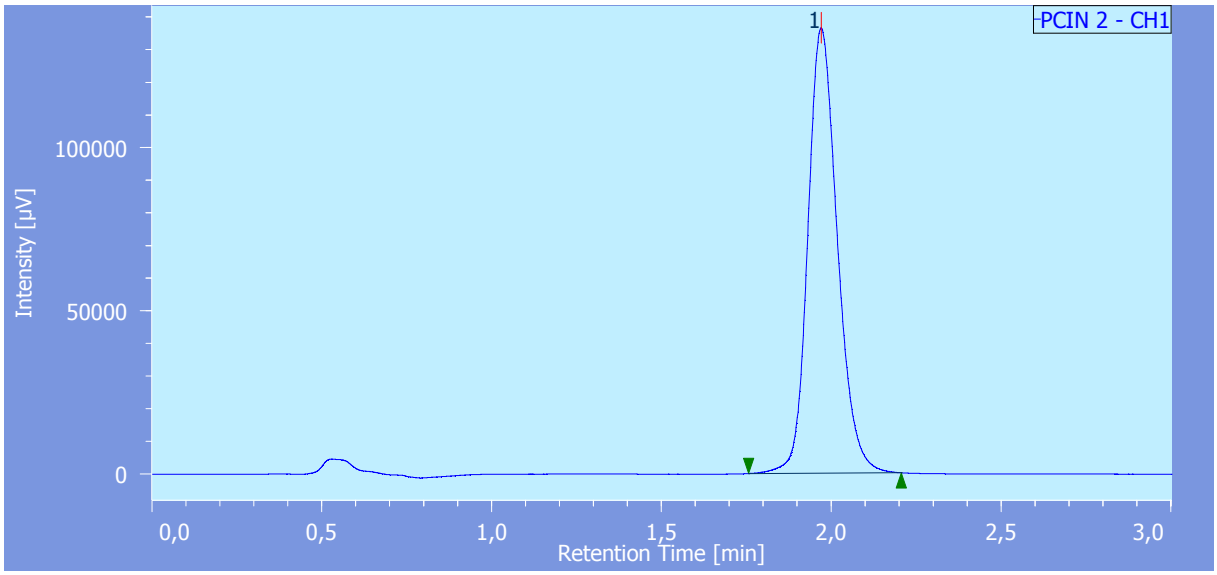


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:02
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:19:29
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,970	822486	136293	100,000	100,000	N/A	2578	N/A	1,196	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

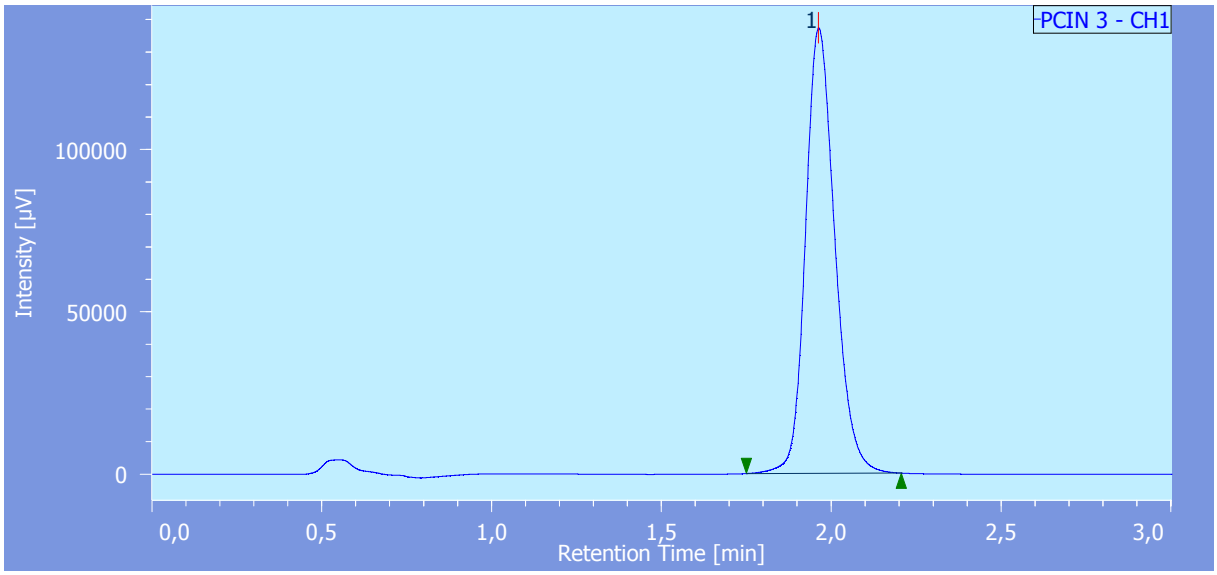


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:03
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:23:52
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,962	822939	137084	100,000	100,000	N/A	2580	N/A	1,216	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

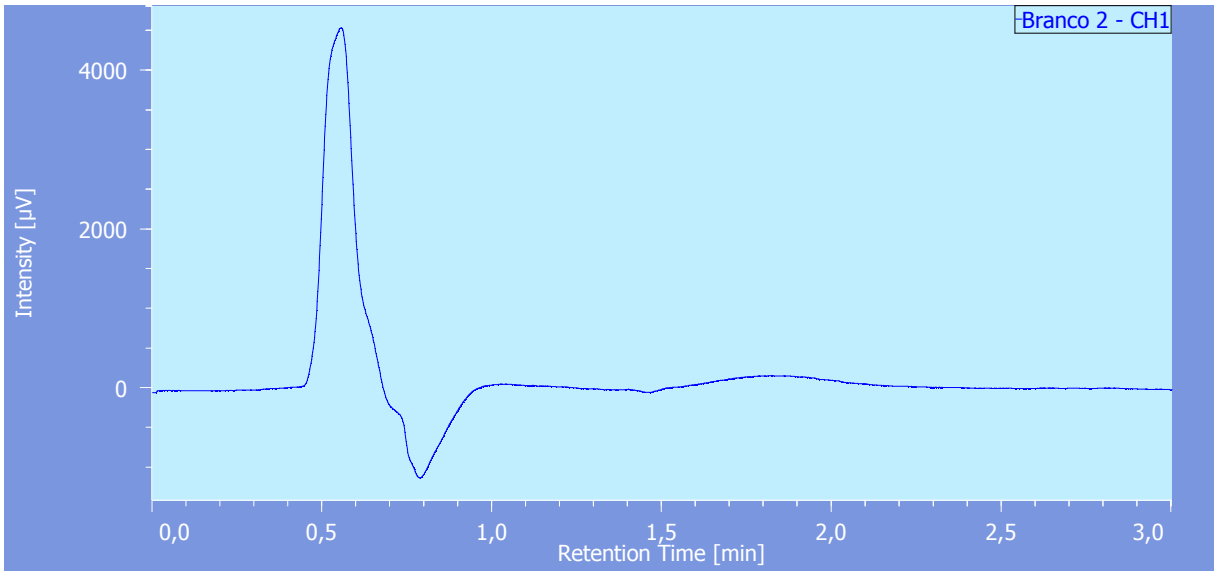


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:03
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:28:15
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

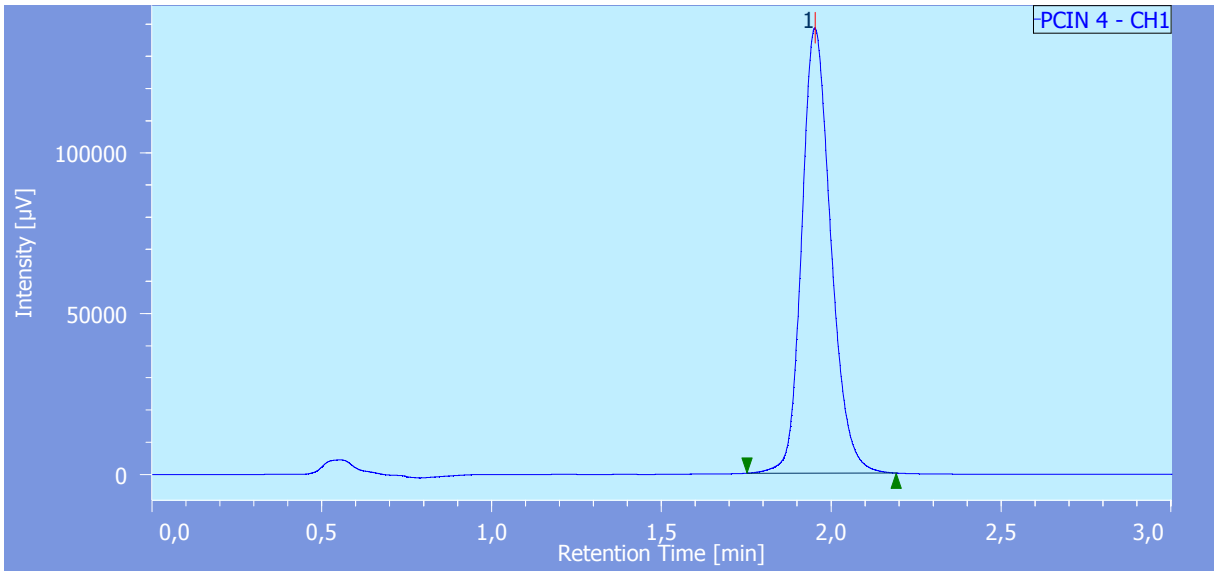

Chromatogram Information

User Name	Administrator
Date Modified	5/12/2016 14:51:03
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:32:39
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,952	822755	138350	100,000	100,000	N/A	2600	N/A	1,203	

Creator Administrator
Reviewer
Approver

Chromatogram

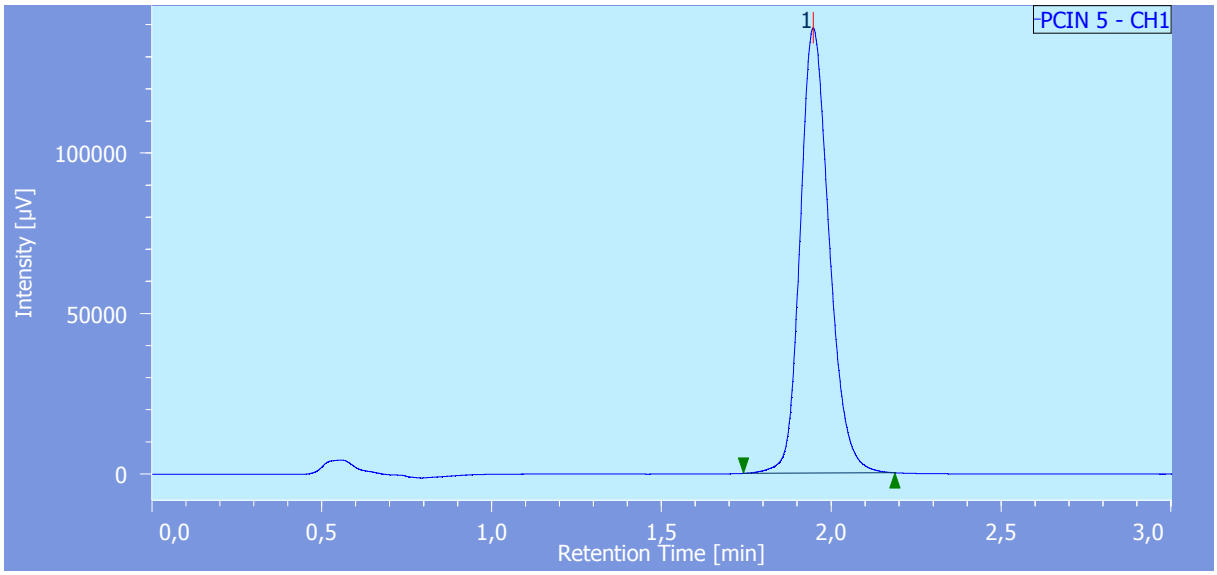

Chromatogram Information

User Name	Administrator
Date Modified	5/12/2016 14:51:04
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:37:02
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,947	822207	138600	100,000	100,000	N/A	2599	N/A	1,209	

Creator Administrator
Reviewer
Approver

Chromatogram

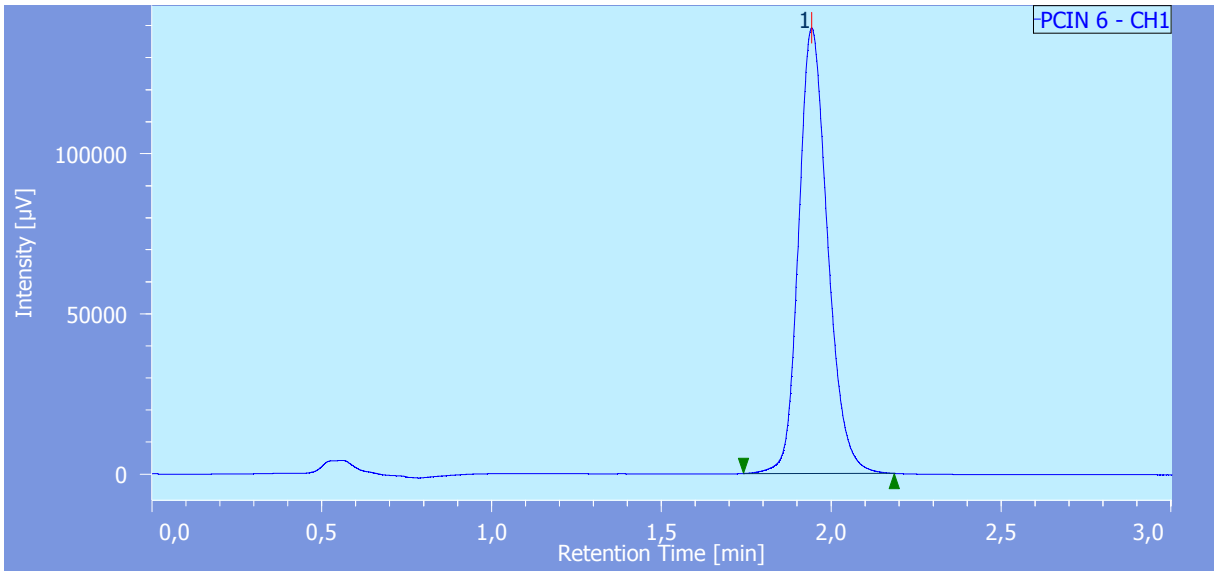


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:04
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:41:26
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 6-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,942	821011	138944	100,000	100,000	N/A	2609	N/A	1,217	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

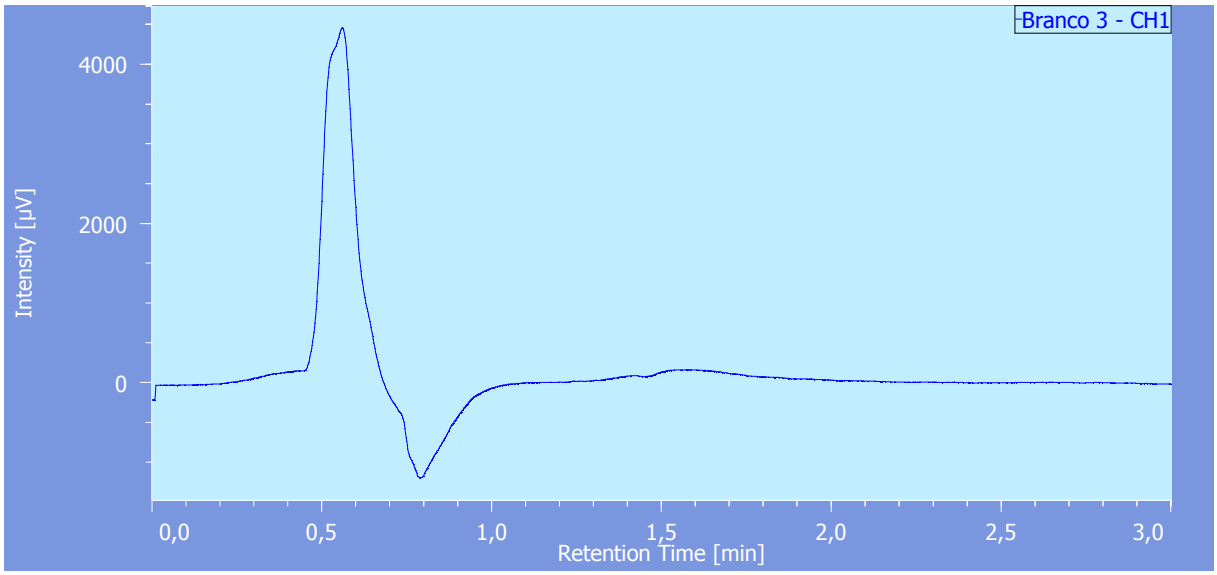


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 14:51:04
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:45:49
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

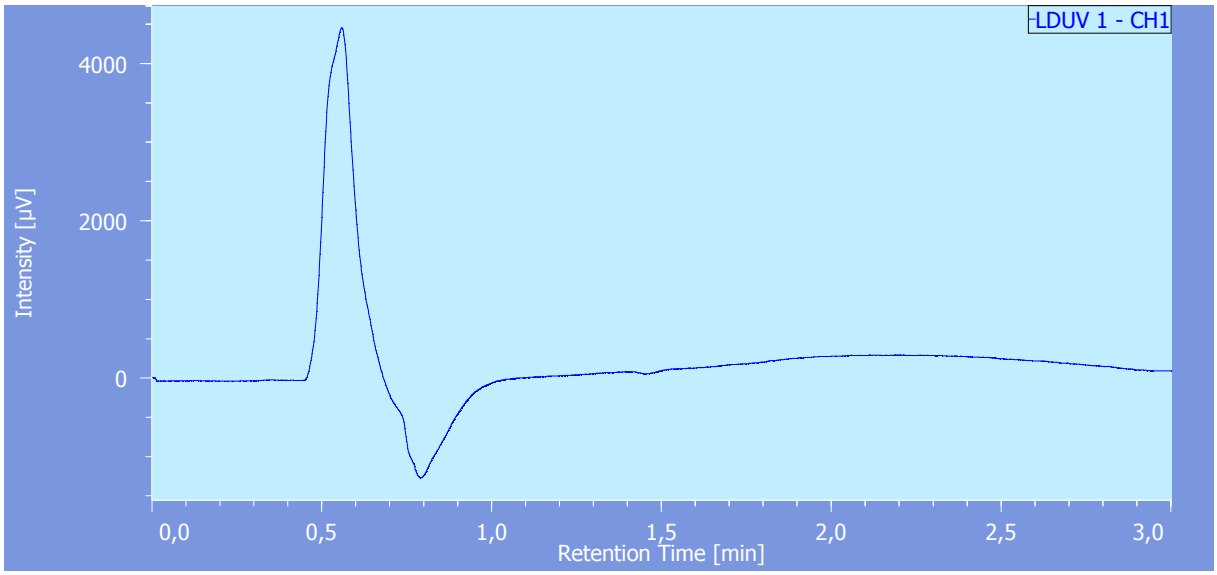


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:15:27
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:52:21
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

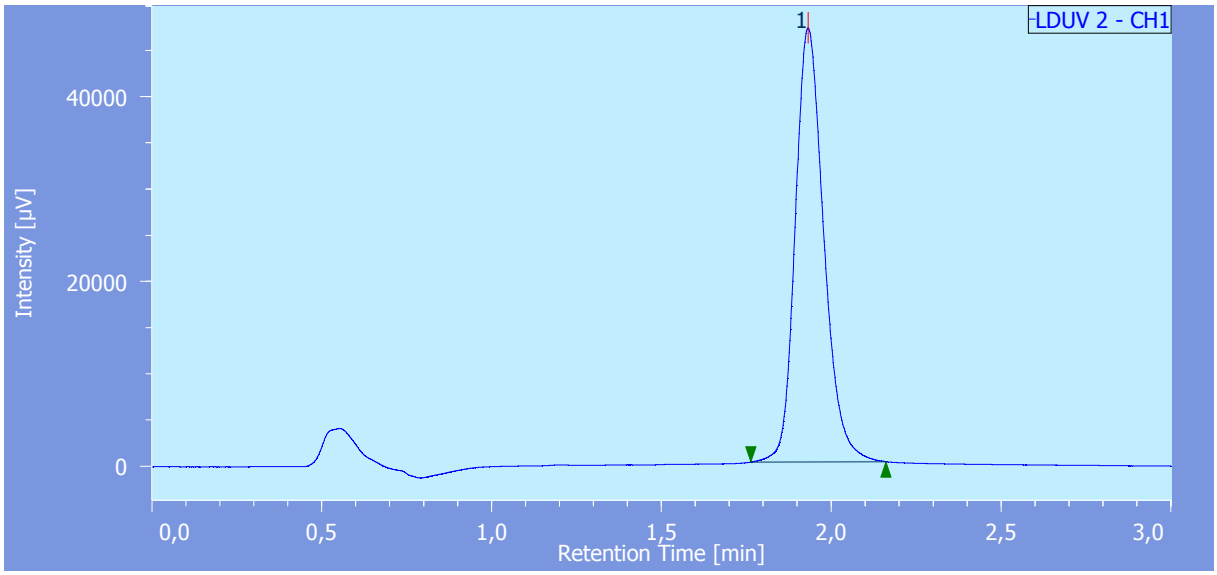


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:15:28
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 14:56:45
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,932	273428	46924	100,000	100,000	N/A	2675	N/A	1,222	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

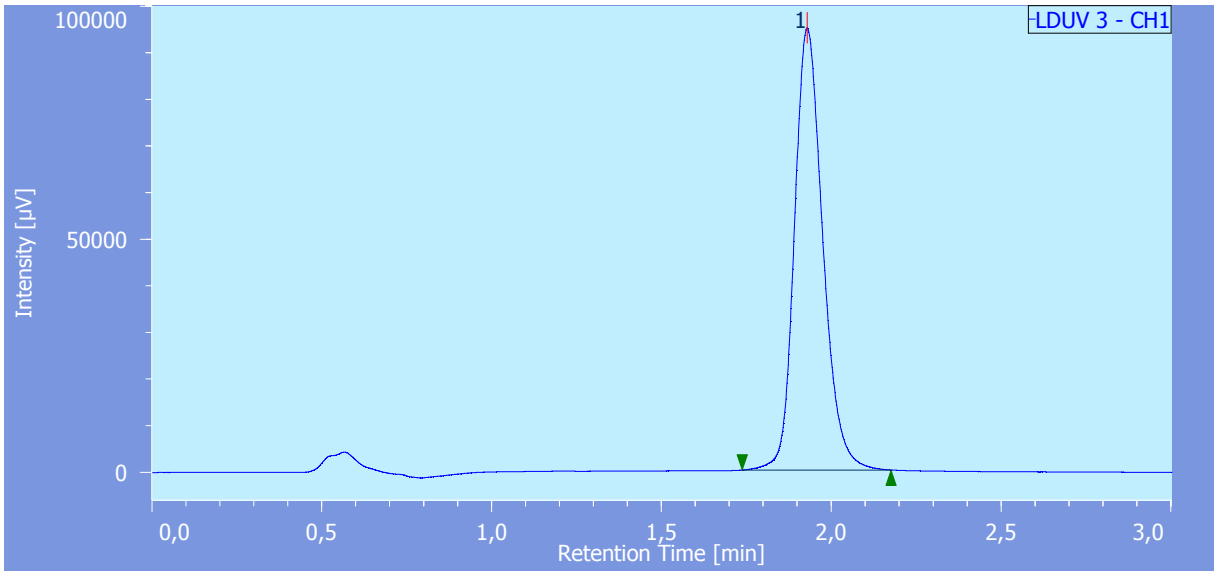


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:15:28
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:01:08
Volume	10,00 [µL]
Sample Number	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,928	547960	94756	100,000	100,000	N/A	2715	N/A	1,224	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

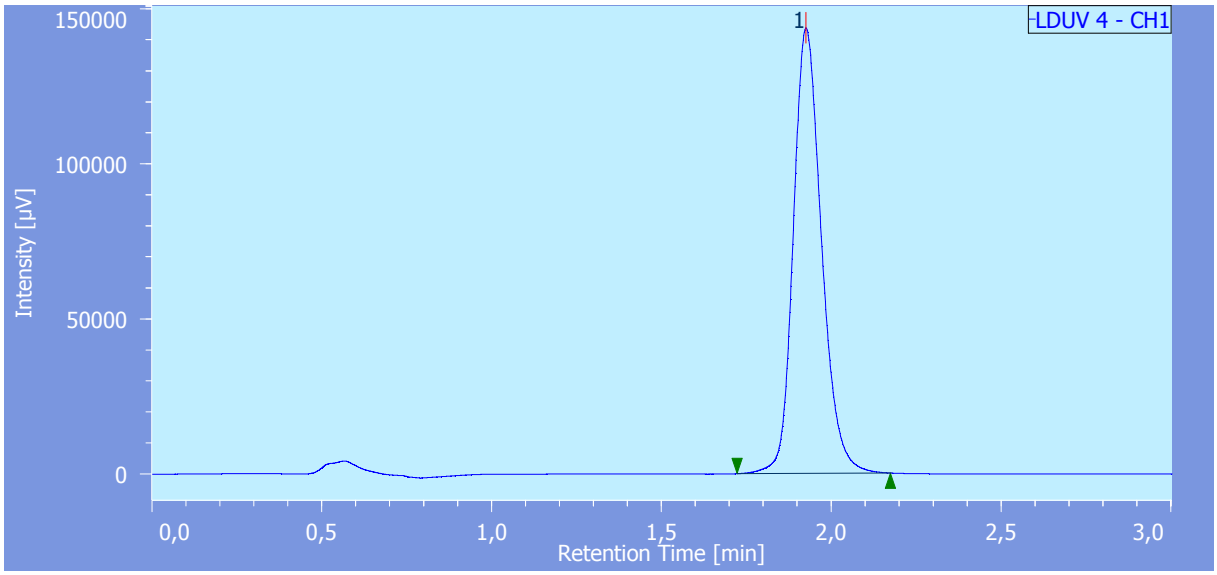

Chromatogram Information

User Name	Administrator
Date Modified	5/12/2016 15:15:29
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:05:34
Volume	10,00 [µL]
Sample Number	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,925	823860	143502	100,000	100,000	N/A	2748	N/A	1,221	

Creator Administrator
Reviewer
Approver

Chromatogram

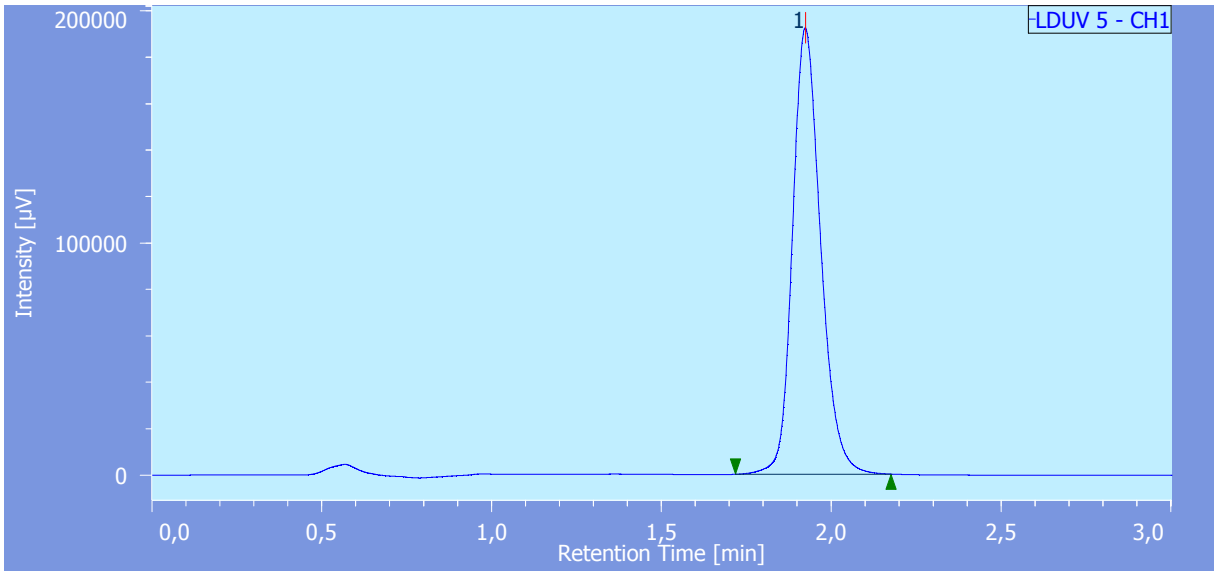

Chromatogram Information

User Name	Administrator
Date Modified	5/12/2016 15:15:29
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:09:59
Volume	10,00 [µL]
Sample Number	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,923	1097291	192042	100,000	100,000	N/A	2772	N/A	1,203	

Creator Administrator
Reviewer
Approver

Chromatogram

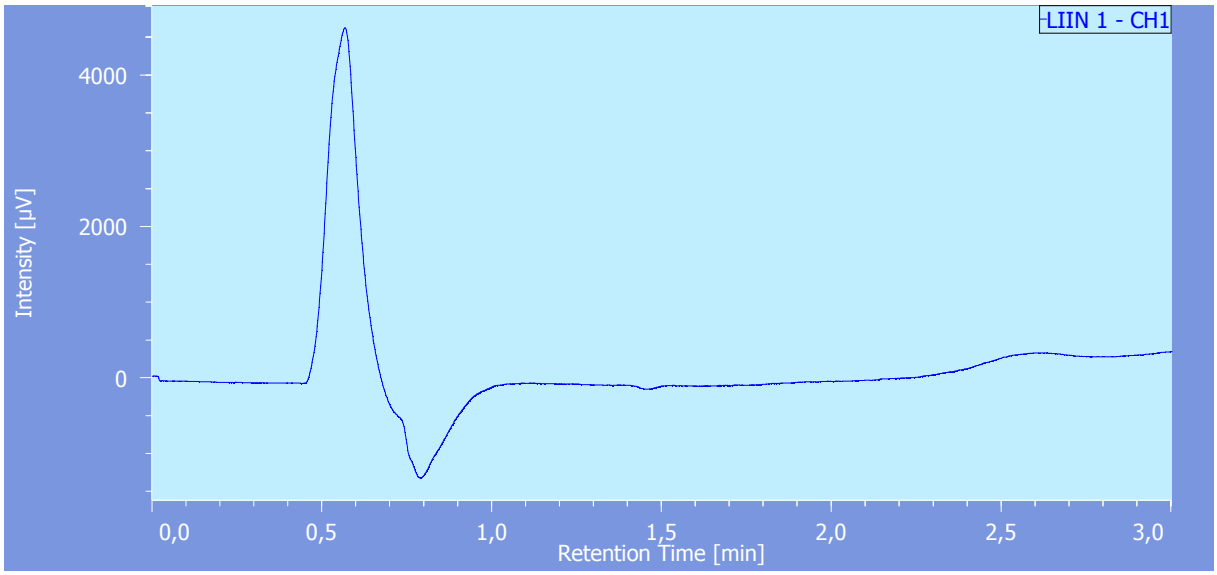


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:39:27
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:16:41
Volume	0,10 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

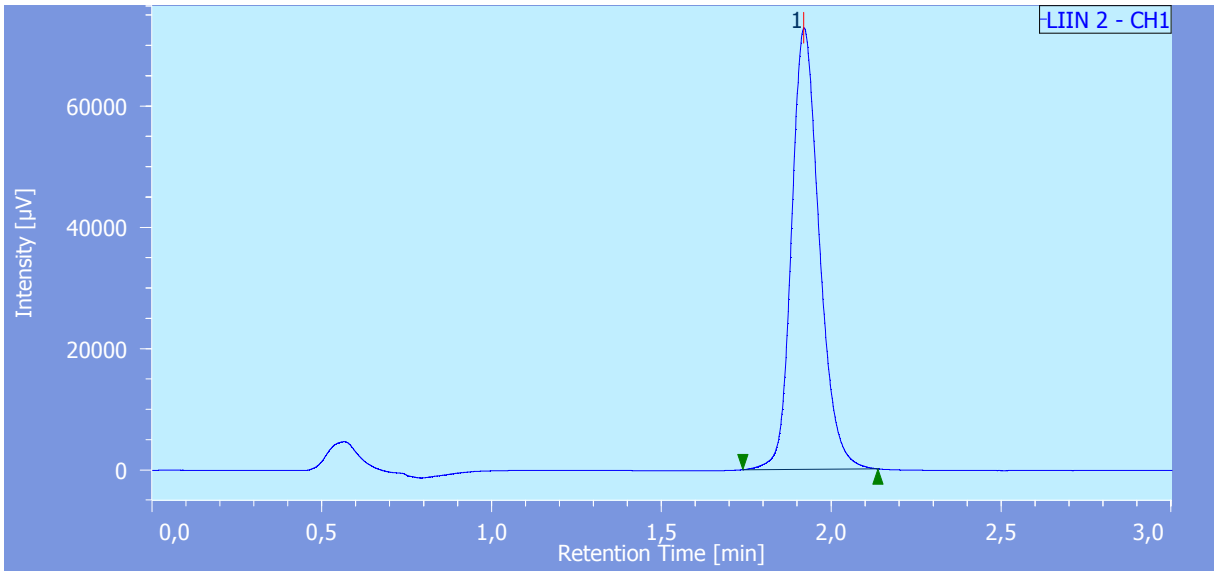


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:39:28
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:21:26
Volume	5,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,918	409400	72708	100,000	100,000	N/A	2839	N/A	1,236	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

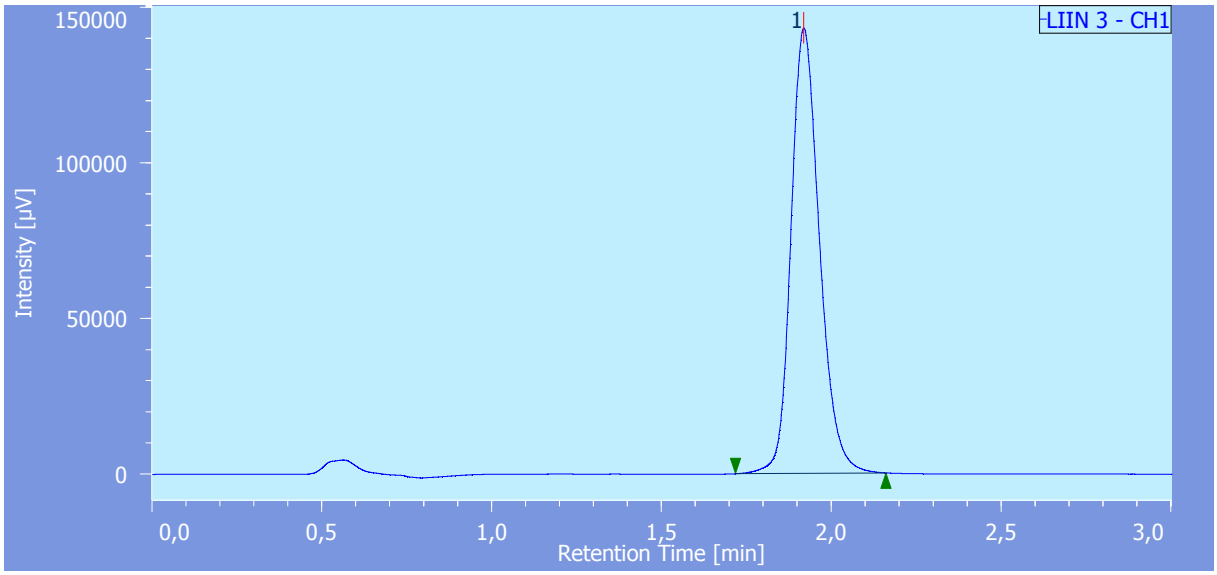


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:39:28
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:26:00
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,918	827068	143008	100,000	100,000	N/A	2682	N/A	1,222	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

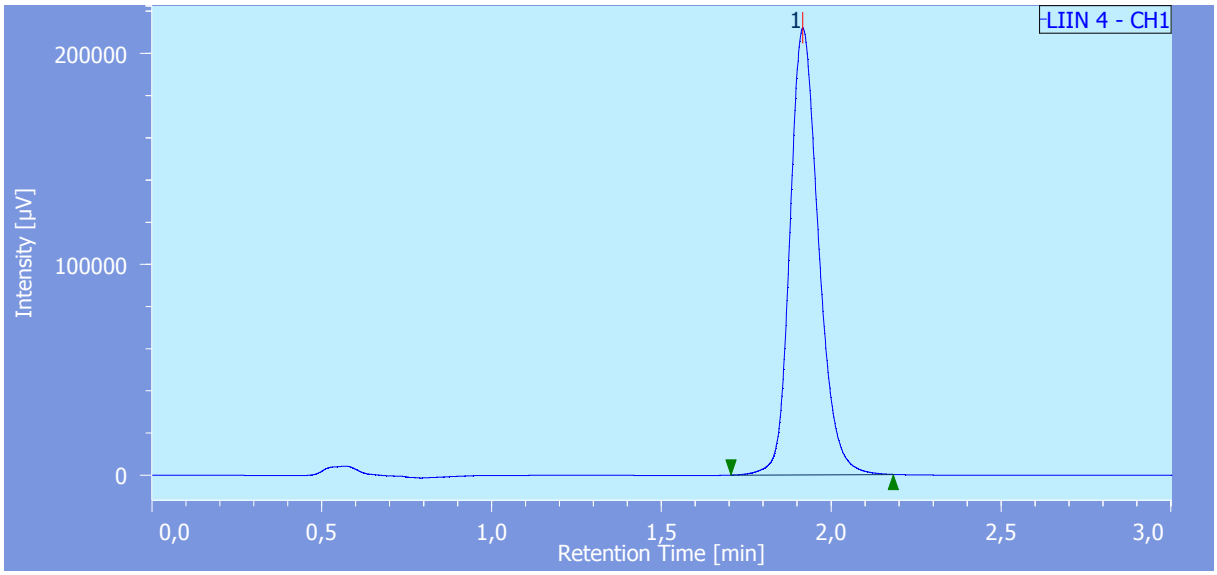


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:39:28
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:30:34
Volume	15,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,915	1232946	211750	100,000	100,000	N/A	2644	N/A	1,230	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

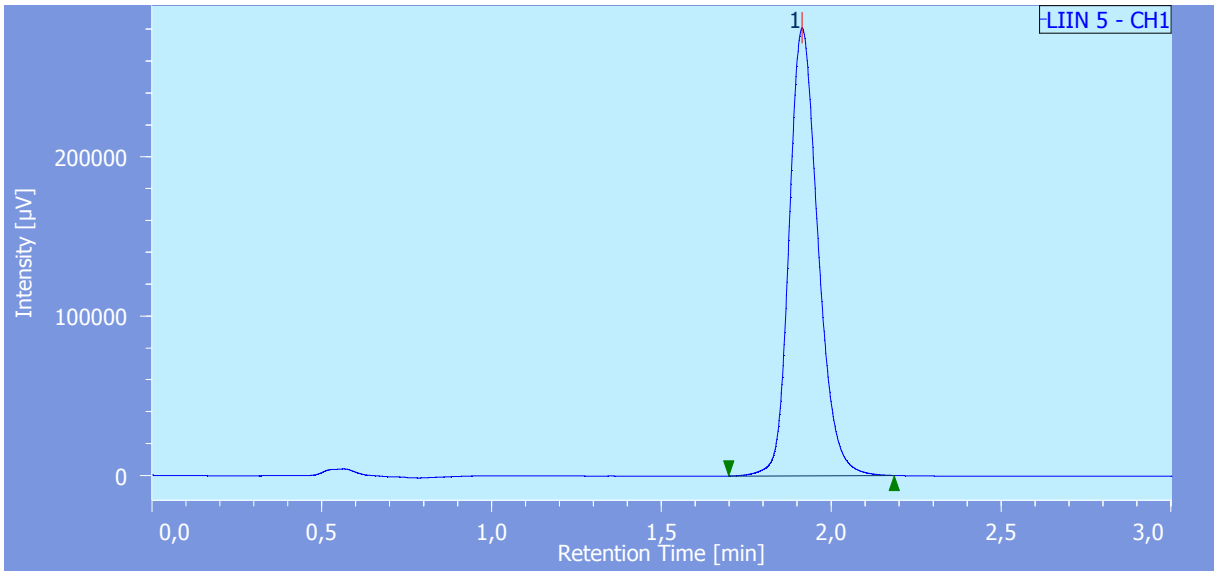


Chromatogram Information	
User Name	Administrator
Date Modified	5/12/2016 15:39:29
Description	
HPLC System Name	01-HP-02
Injection Date	5/12/2016 15:35:11
Volume	20,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,913	1649814	280737	100,000	100,000	N/A	2577	N/A	1,232	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

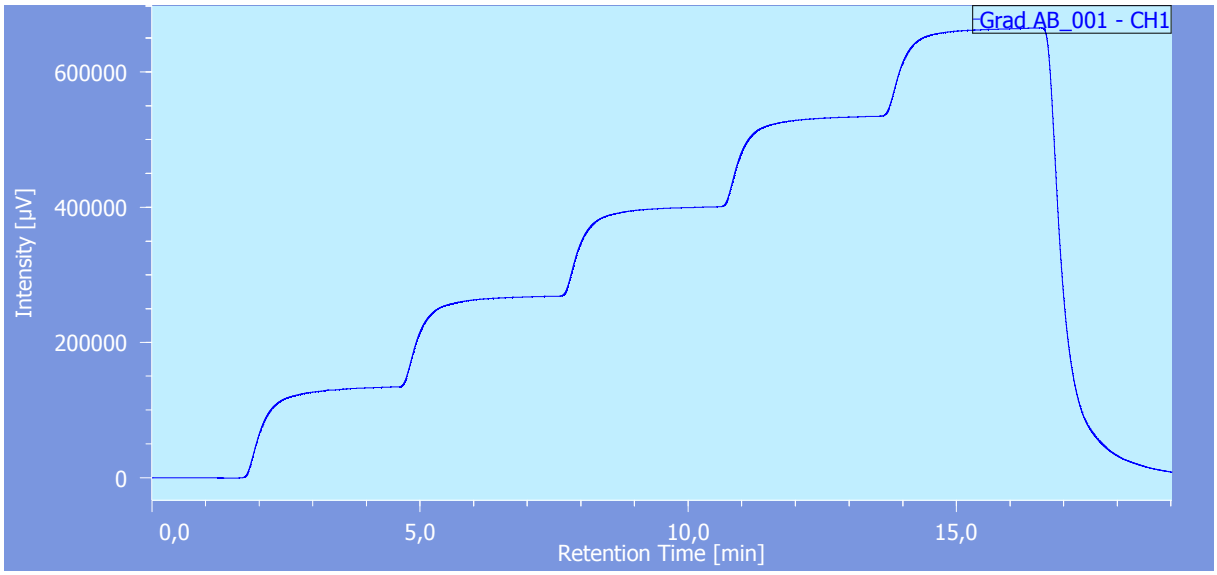


Chromatogram Information	
User Name	Administrator
Date Modified	6/12/2016 09:48:07
Description	
HPLC System Name	01-HP-02
Injection Date	6/12/2016 09:26:09
Volume	10,00 [µL]
Sample Number	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Grad AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Gradiente
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

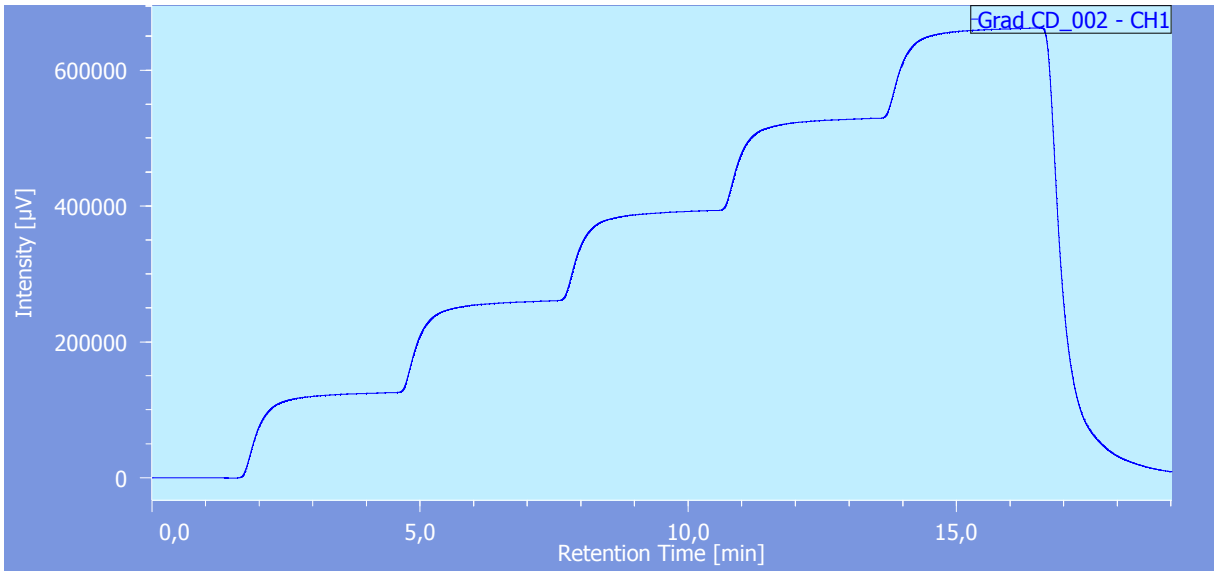

Chromatogram Information	
User Name	Administrator
Date Modified	6/12/2016 10:14:48
Description	
HPLC System Name	01-HP-02
Injection Date	6/12/2016 09:50:37
Volume	10,00 [µL]
Sample Number	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Grad CD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Gradiente
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	