
Peak Find - EDUV.jws

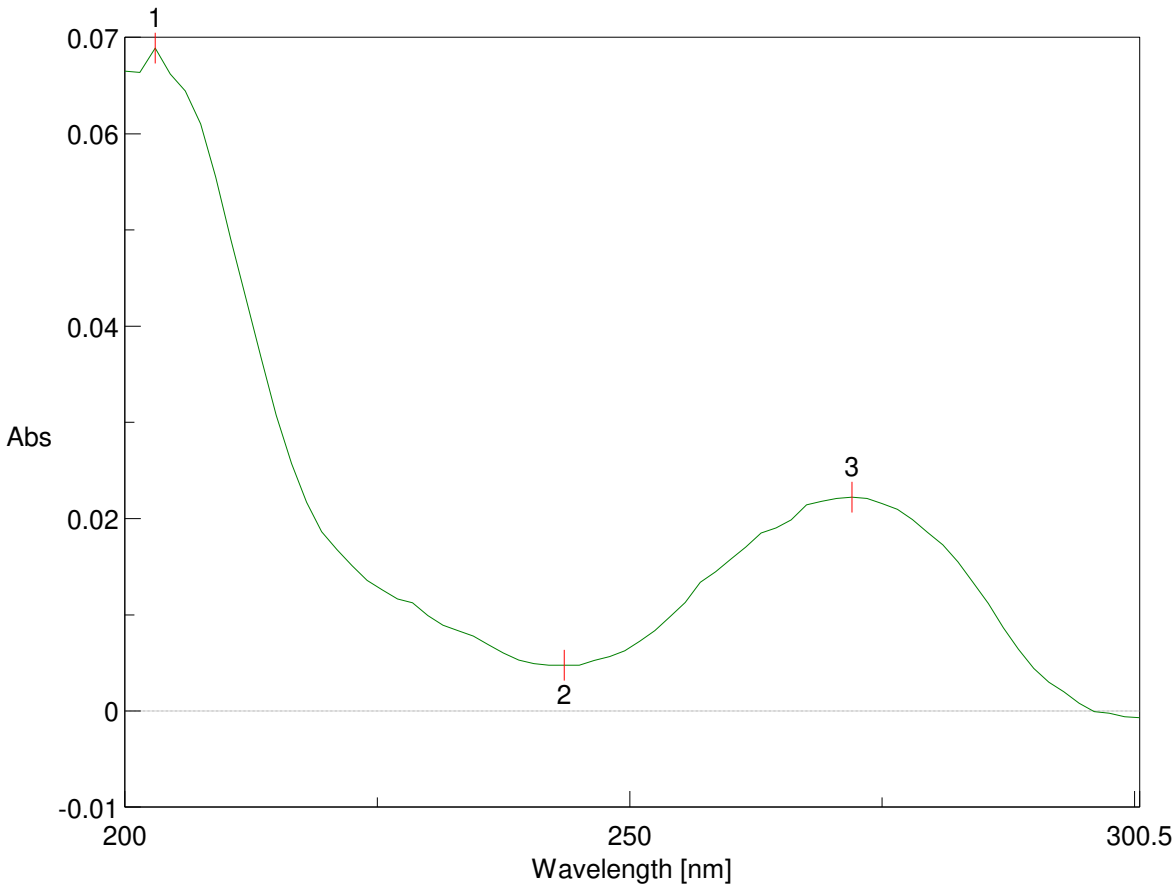

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	16/11/2021 11:03

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300.5 nm
Data interval	1.5 nm
Data points	68


[Measurement Information]

Instrument Name	MD-2015
Model Name	MD-2015
Serial No.	0000000000
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	203	0.06886	2	243.5	0.004728
3	272	0.022185			

Chromatogram

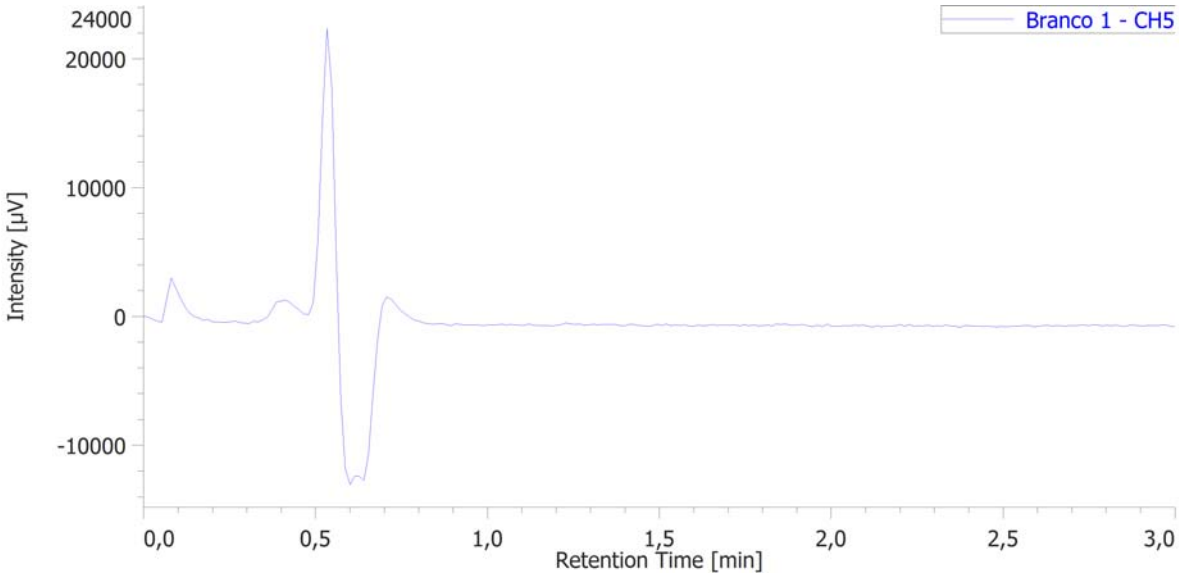


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:05
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:08:55
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

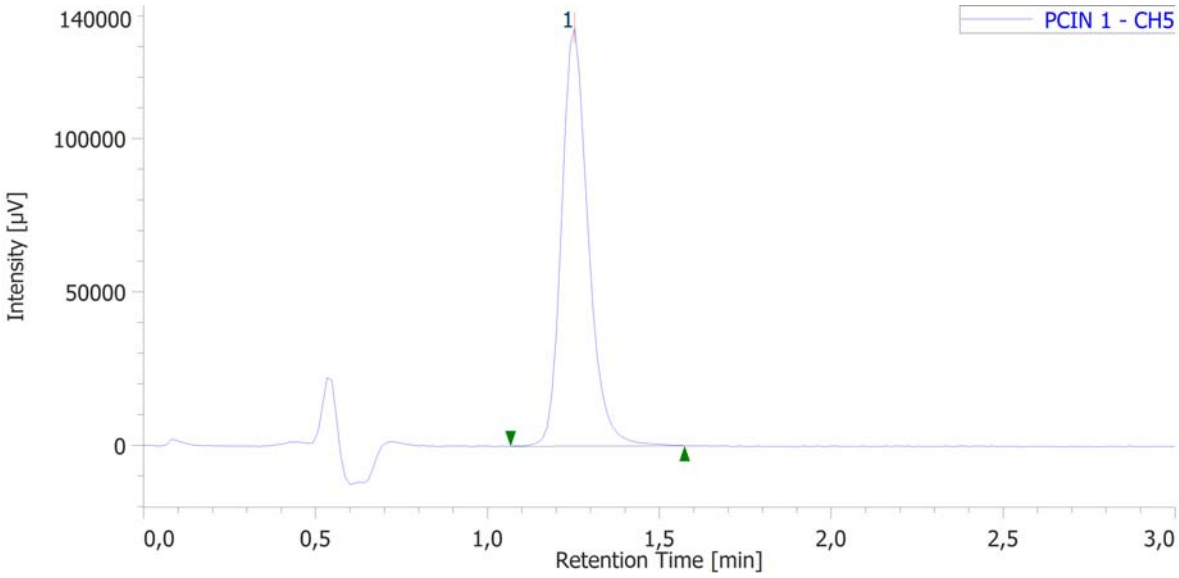

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:13:15
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,253	734464	136133	100,000	100,000	N/A	1345	N/A	1,181	

Creator QPackSA
Reviewer
Approver

Chromatogram

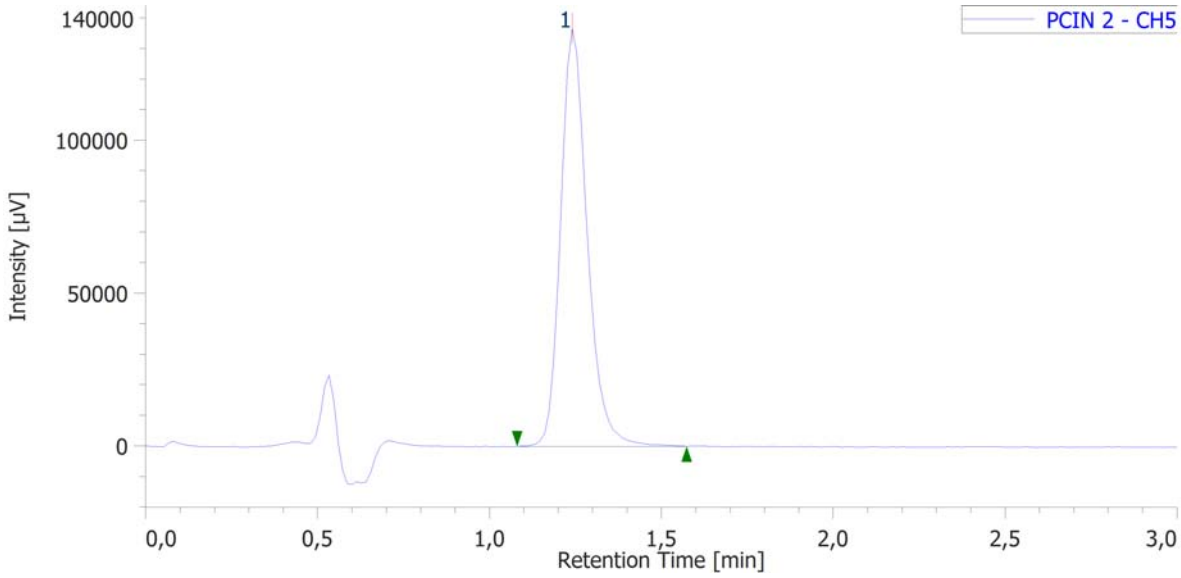

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:17:33
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	735622	136702	100,000	100,000	N/A	1310	N/A	1,253	

Creator QPackSA
Reviewer
Approver

Chromatogram

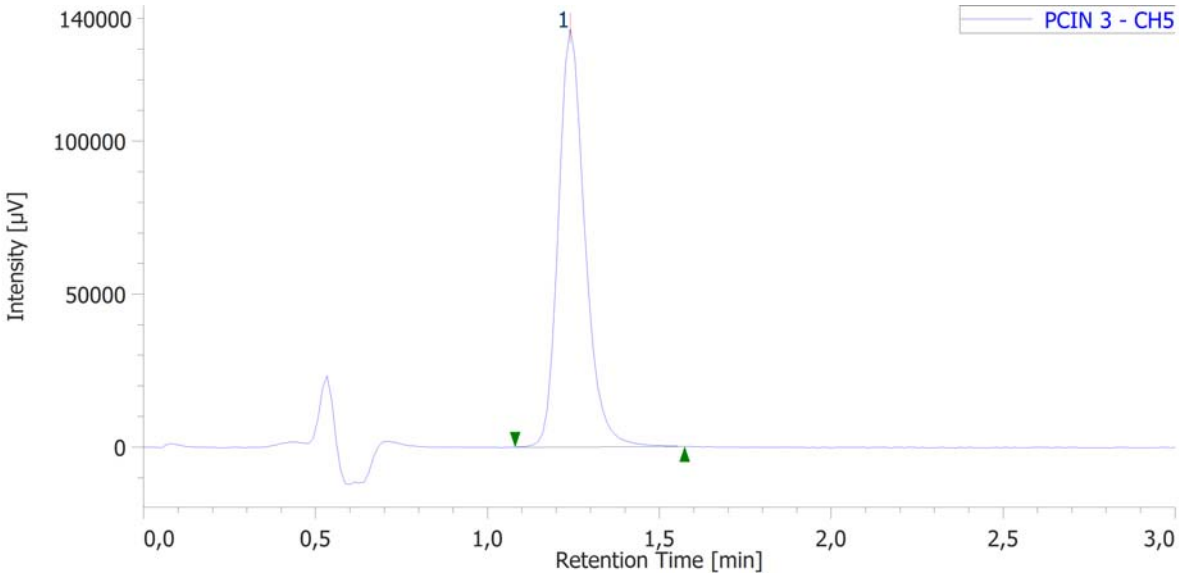

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:21:53
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	734282	136766	100,000	100,000	N/A	1311	N/A	1,242	

Creator QPackSA
Reviewer
Approver

Chromatogram

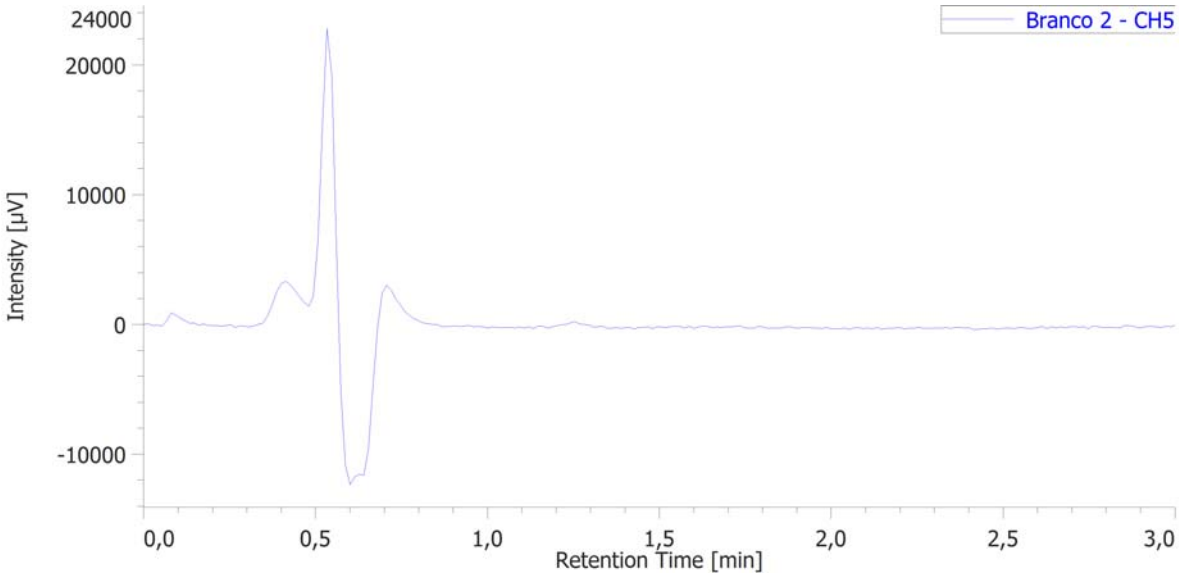


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:26:11
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

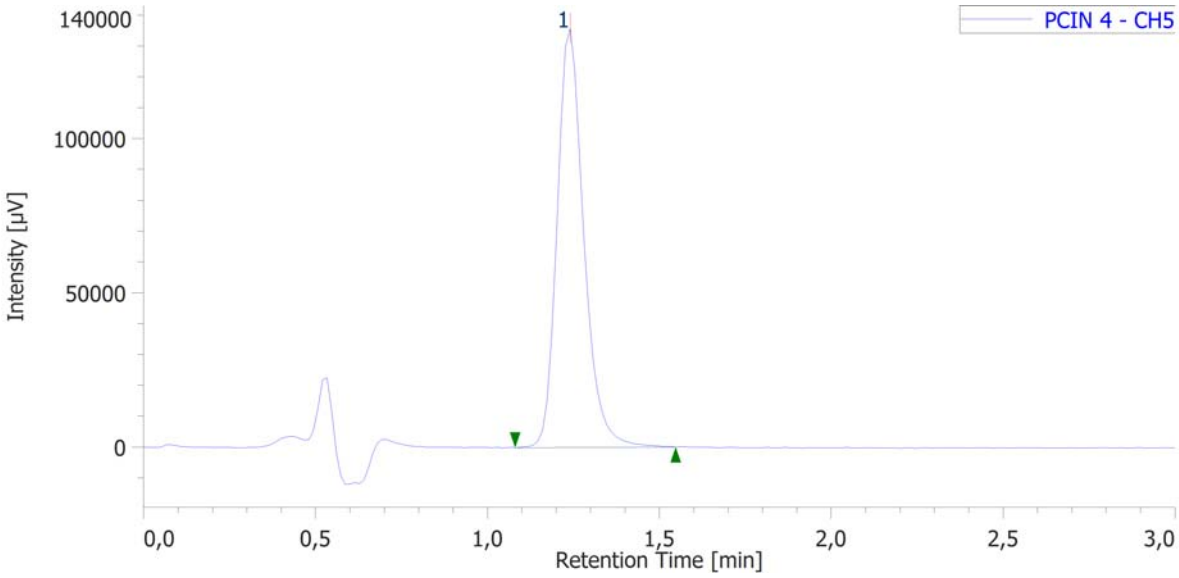

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:30:31
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	732826	135822	100,000	100,000	N/A	1309	N/A	1,195	

Creator QPackSA
Reviewer
Approver

Chromatogram

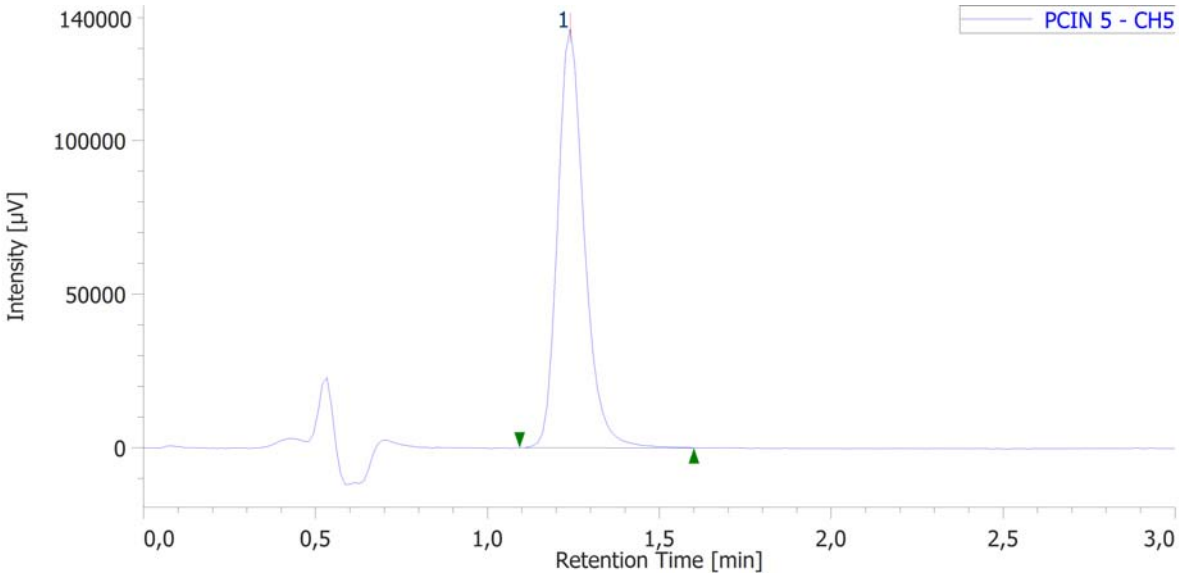

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:34:51
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	735521	136431	100,000	100,000	N/A	1310	N/A	1,221	

Creator QPackSA
Reviewer
Approver

Chromatogram

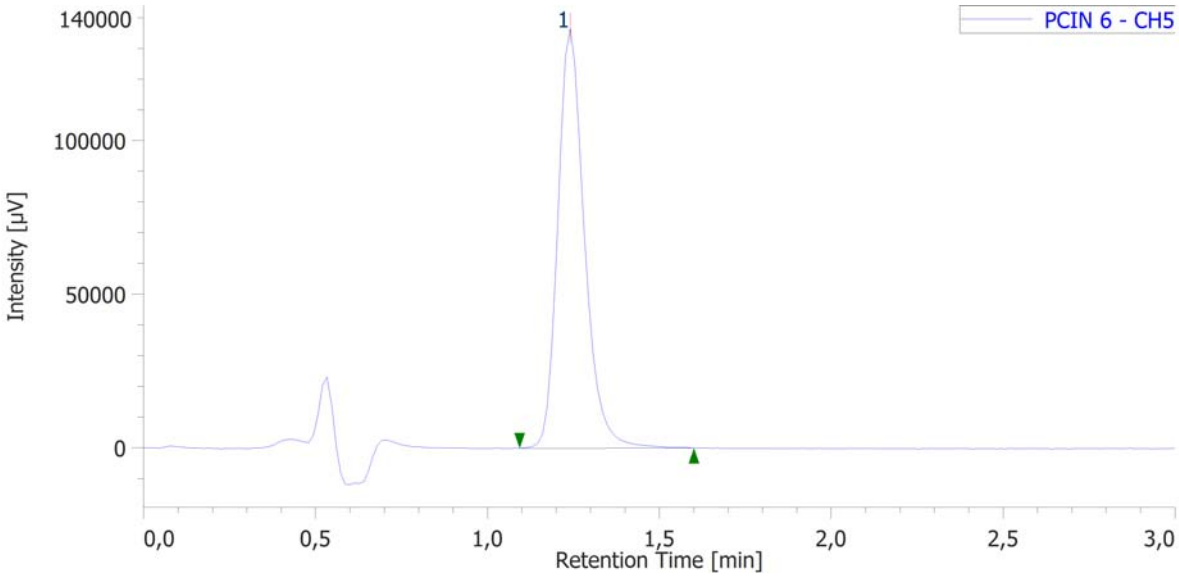

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:07
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:39:11
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	736694	136581	100,000	100,000	N/A	1310	N/A	1,230	

Creator QPackSA
Reviewer
Approver

Chromatogram

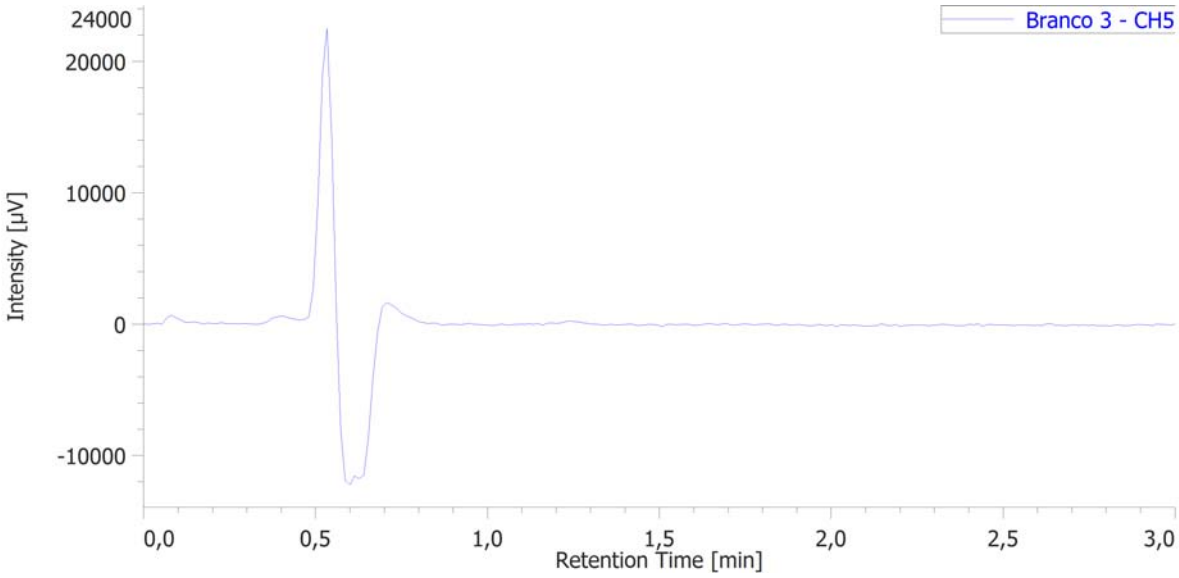


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:08:08
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:43:31
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

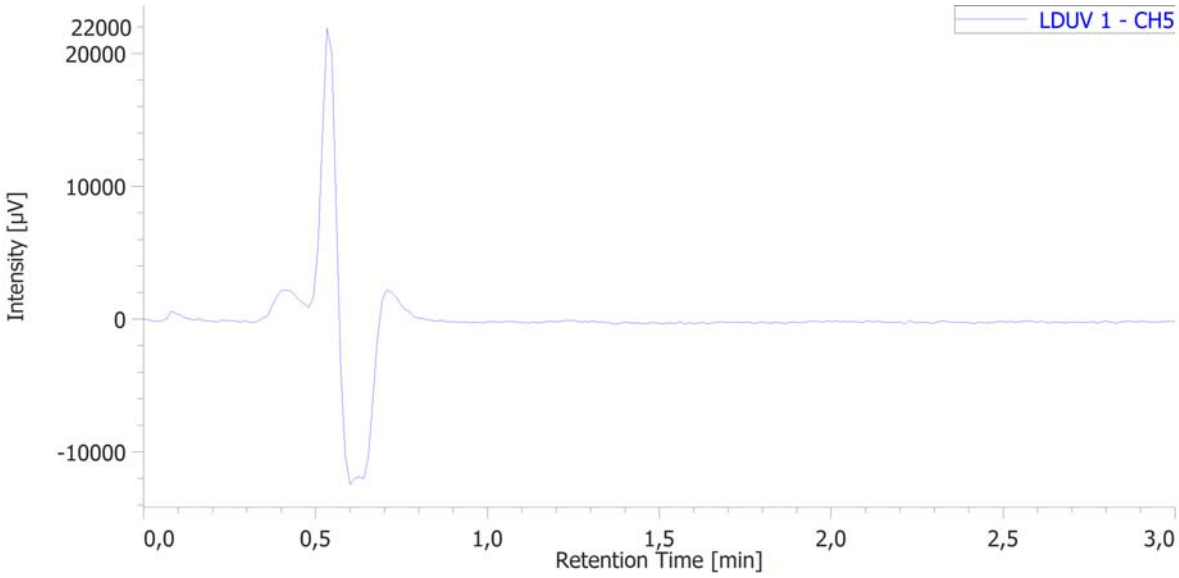


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:16:01
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:52:26
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

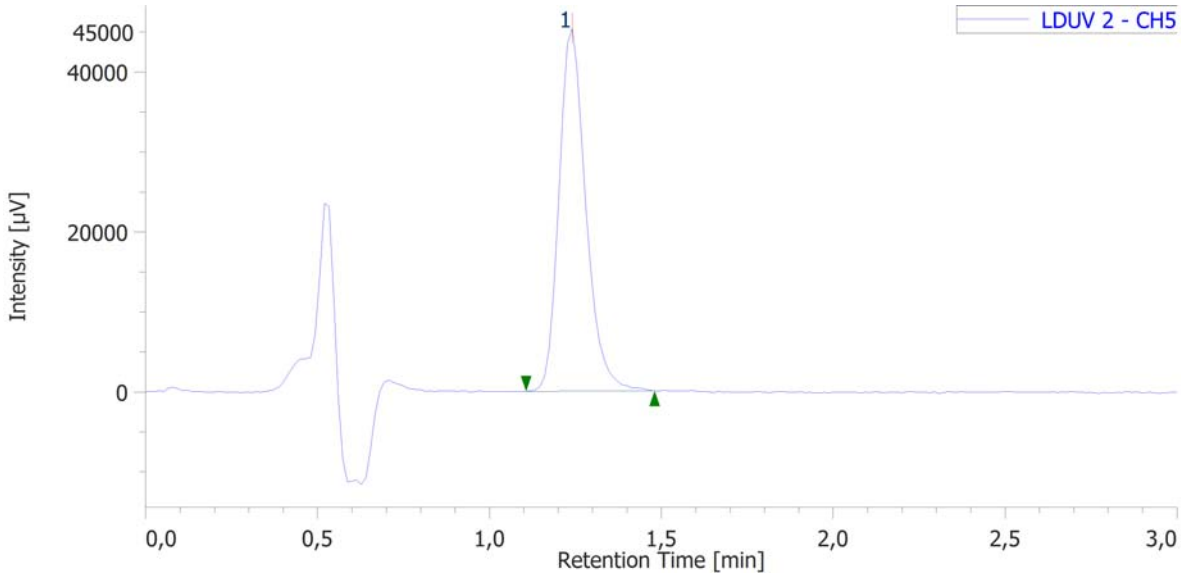

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:16:01
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 11:56:46
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	246160	45351	100,000	100,000	N/A	1272	N/A	1,202	

Creator QPackSA
Reviewer
Approver

Chromatogram

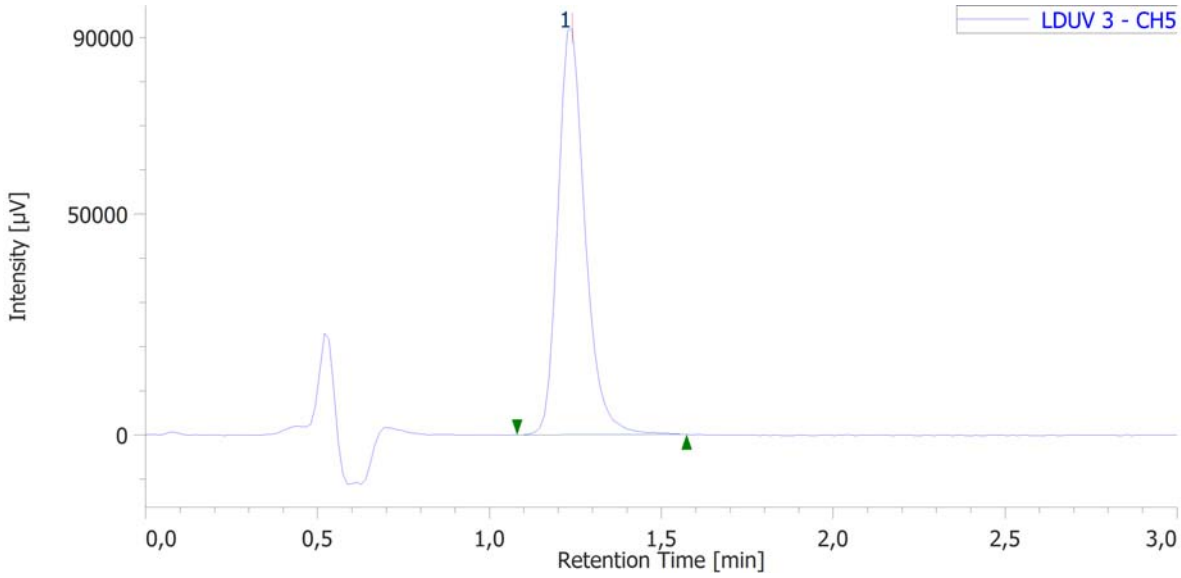

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:16:01
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 12:01:06
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	506806	91975	100,000	100,000	N/A	1257	N/A	1,172	

Creator QPackSA
Reviewer
Approver

Chromatogram

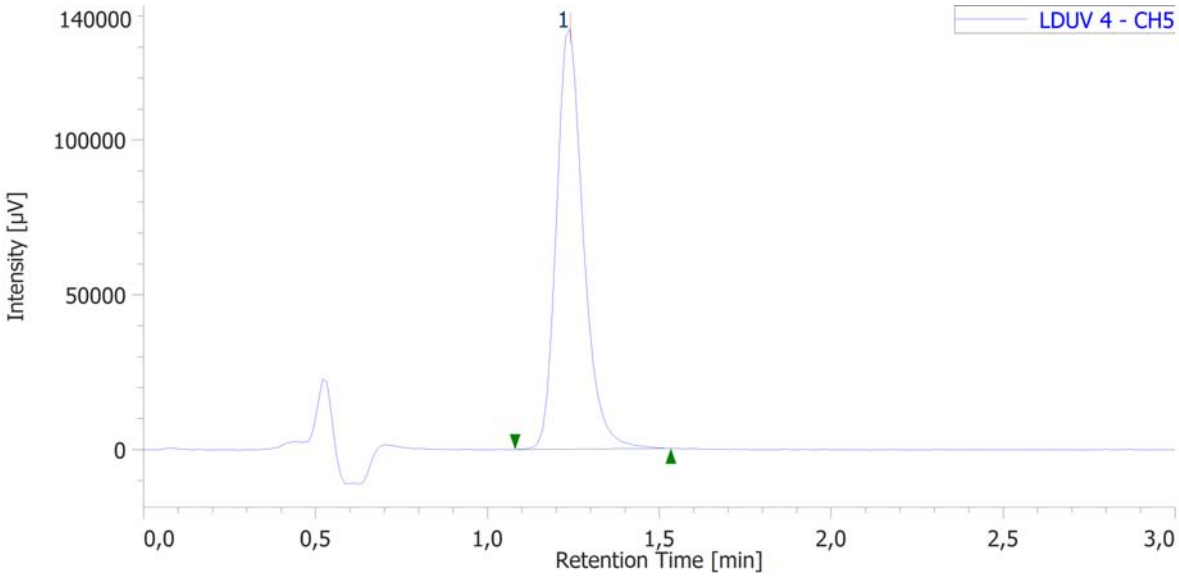

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:16:01
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 12:05:29
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	741354	135829	100,000	100,000	N/A	1275	N/A	1,190	

Creator QPackSA
Reviewer
Approver

Chromatogram

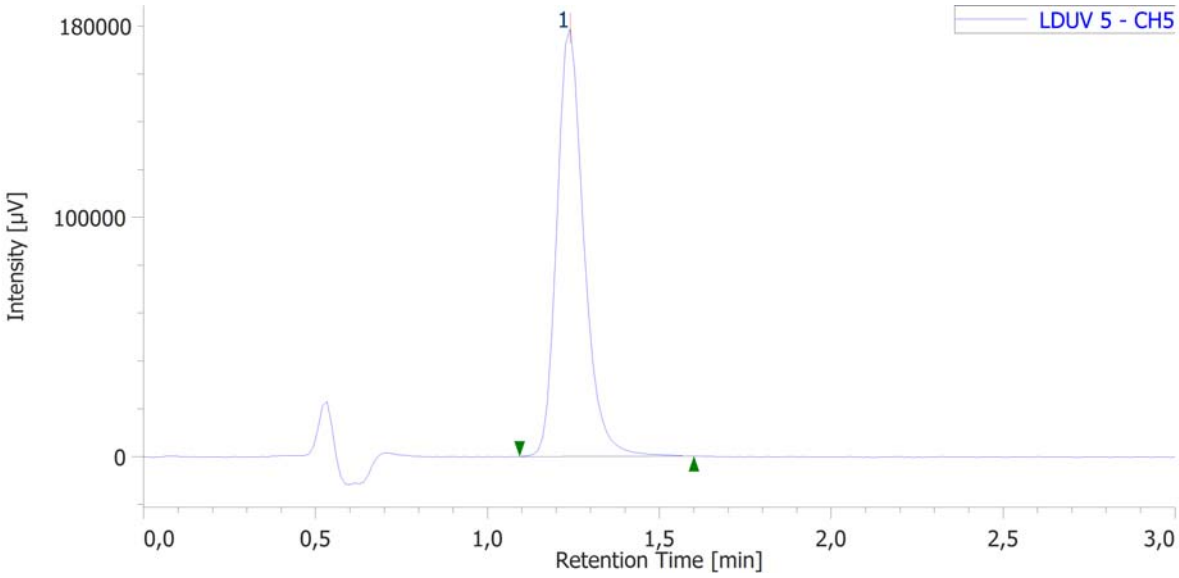

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:16:02
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 12:09:51
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	977896	178907	100,000	100,000	N/A	1277	N/A	1,205	

Creator QPackSA
Reviewer
Approver

Chromatogram

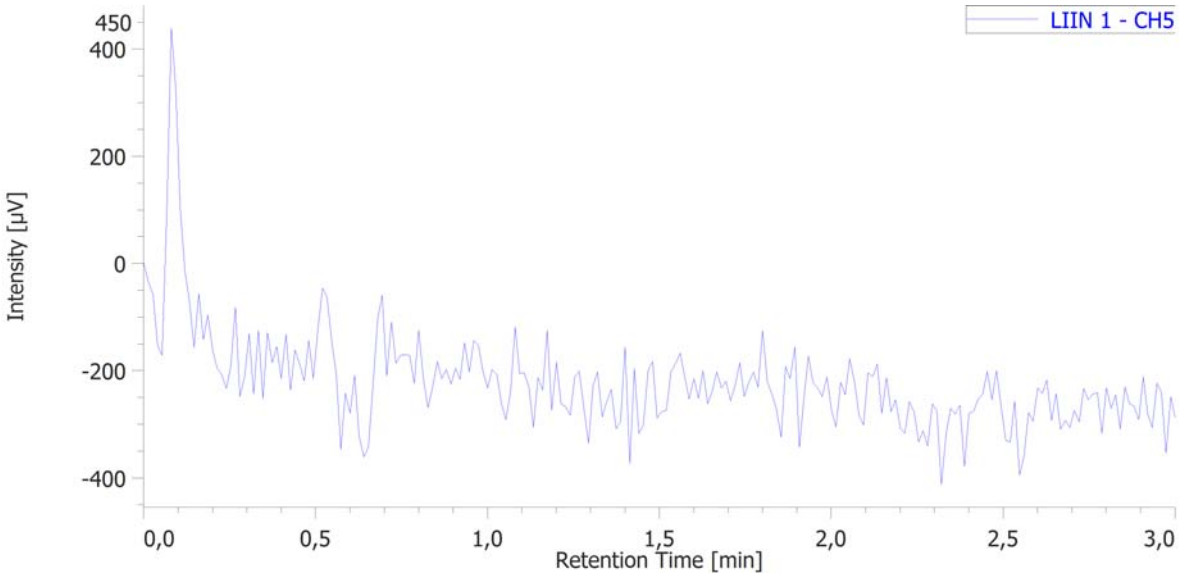


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:57:49
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 13:18:59
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

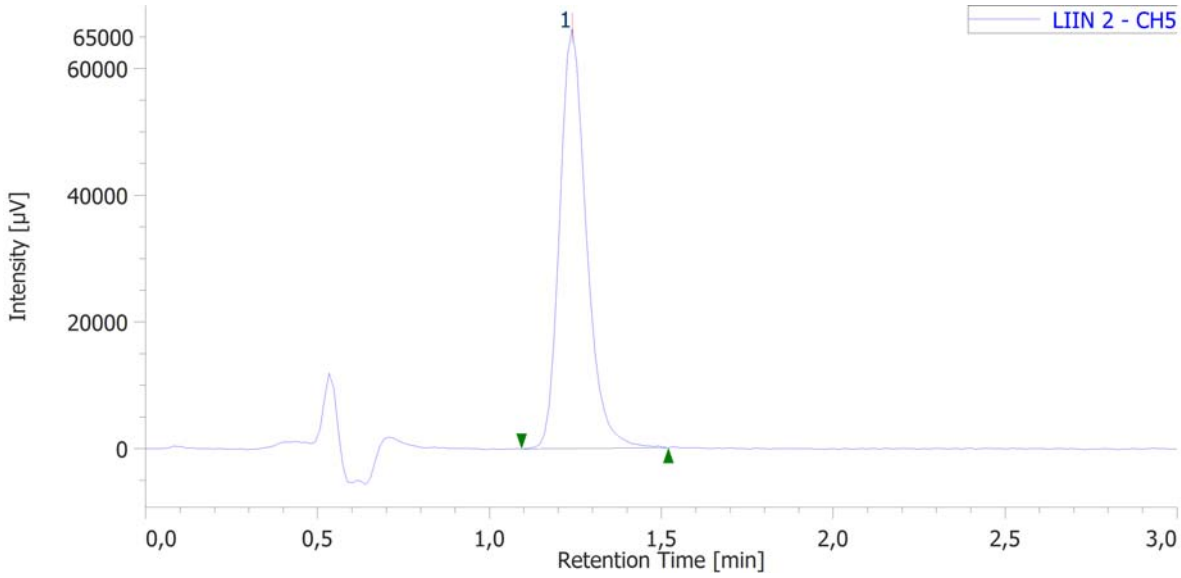

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:57:50
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 13:23:17
Volume	5,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	358262	66249	100,000	100,000	N/A	1286	N/A	1,223	

Creator QPackSA
Reviewer
Approver

Chromatogram

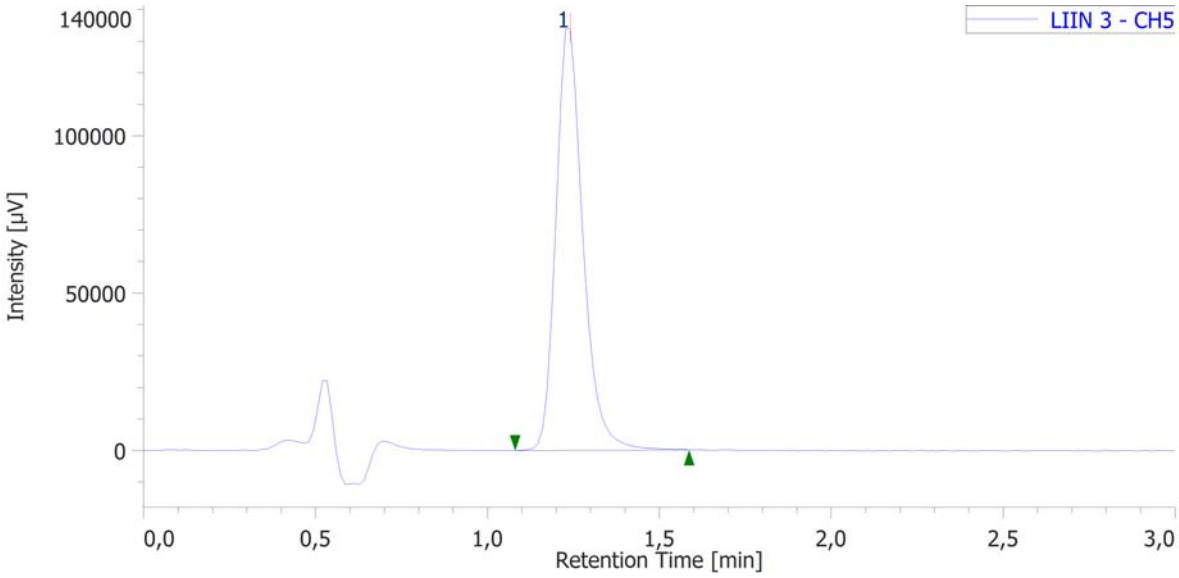

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:57:50
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 13:27:37
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	736907	134013	100,000	100,000	N/A	1264	N/A	1,170	

Creator QPackSA
Reviewer
Approver

Chromatogram

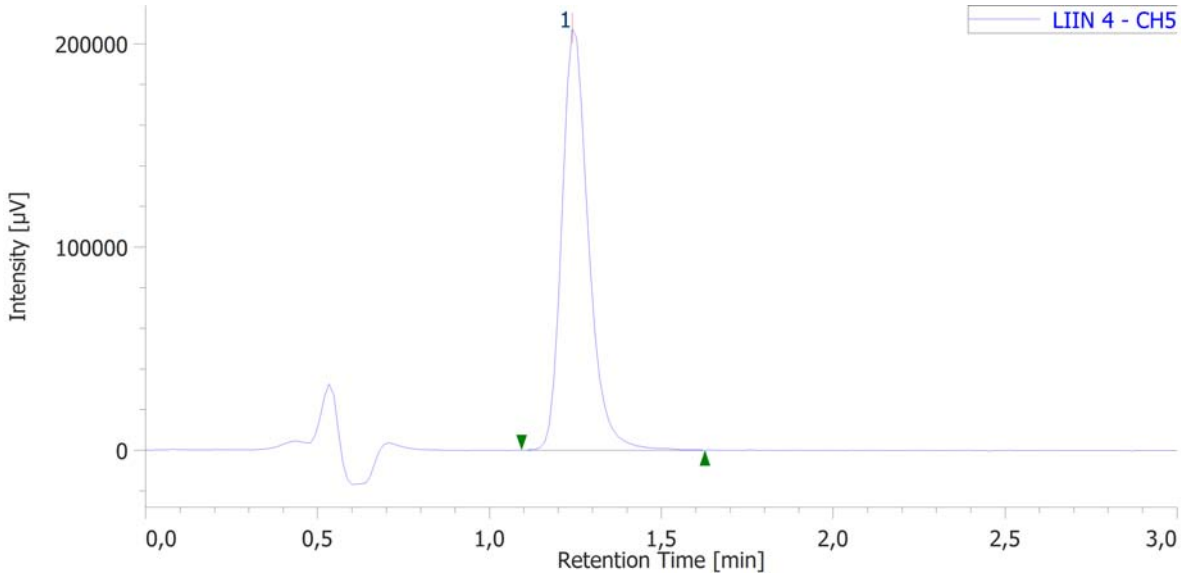

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:57:50
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 13:32:00
Volume	15,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,240	1119934	207545	100,000	100,000	N/A	1309	N/A	1,346	

Creator QPackSA
Reviewer
Approver

Chromatogram

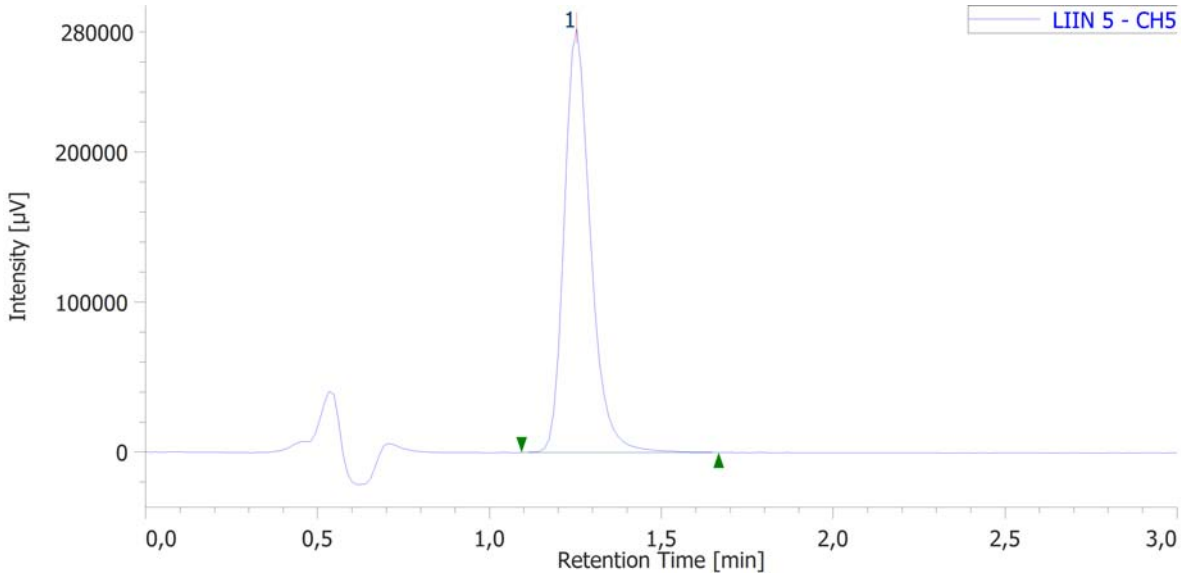

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:57:51
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 13:36:22
Volume	20,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,253	1503170	282699	100,000	100,000	N/A	1390	N/A	1,228	

Creator QPackSA
Reviewer
Approver

Chromatogram

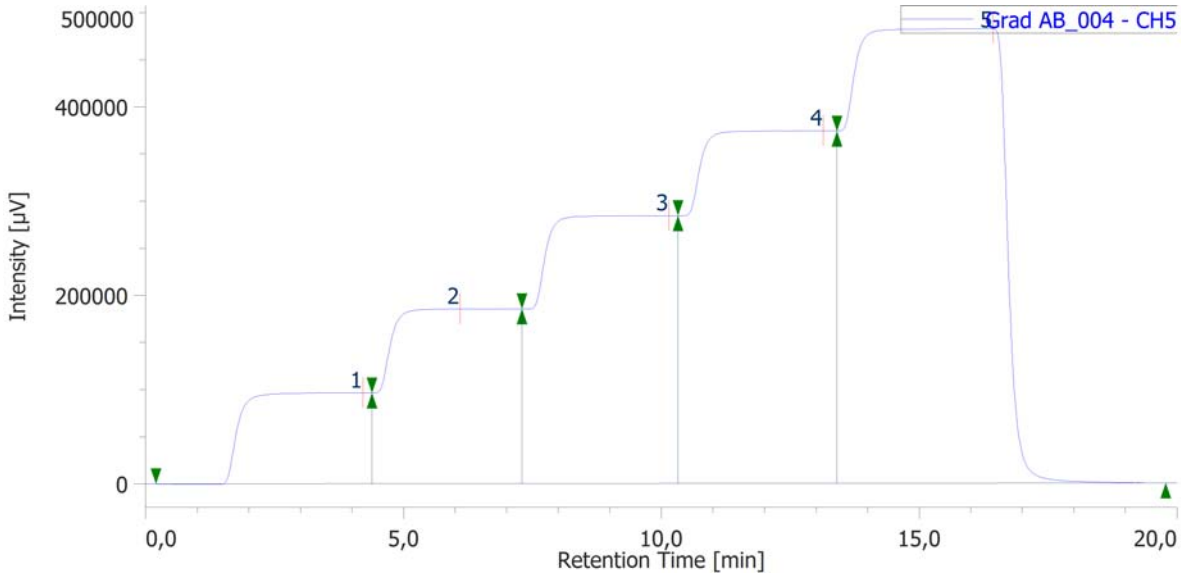

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 16:12:50
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 15:52:48
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AB
Peak ID Table	Grad AB
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	4,213	15096379	96539	5,903	6,789	N/A	N/A	N/A	N/A	
2	40 %	5	6,093	30381006	196426	11,880	13,040	N/A	N/A	N/A	N/A	
3	60 %	5	10,147	48836436	284032	19,097	19,975	N/A	N/A	N/A	N/A	
4	80 %	5	13,133	66720172	383753	26,090	26,285	N/A	N/A	N/A	N/A	
5	100 %	5	16,427	94695835	482183	37,030	33,910	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

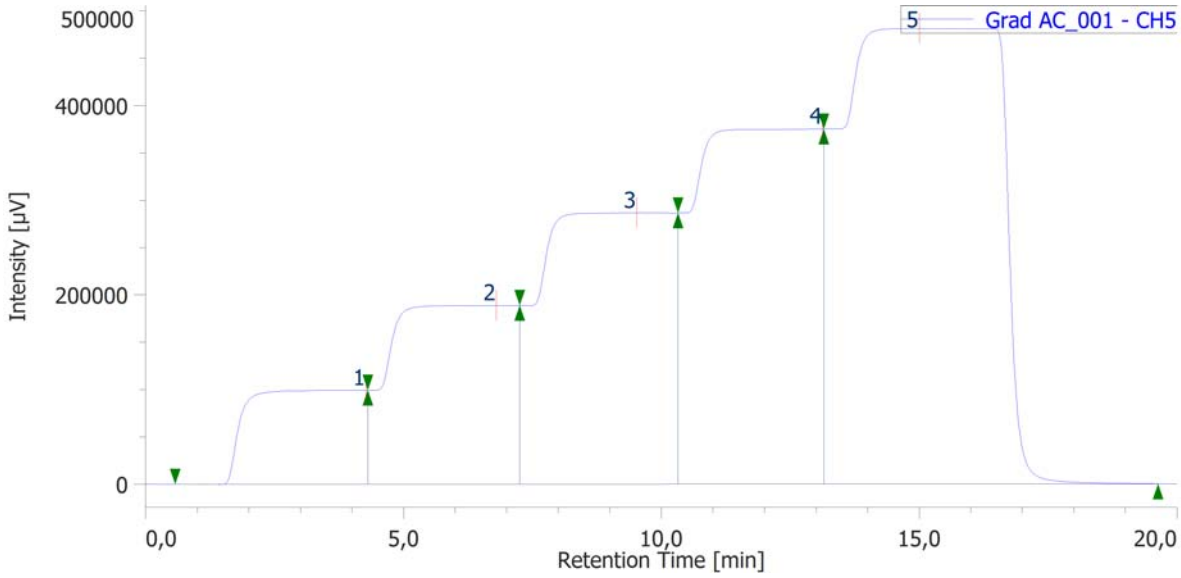

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 16:36:49
Description	
HPLC System Name	HPL 18
Injection Date	16/11/2021 16:13:58
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Grad AC
Peak ID Table	Grad AC
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Grad AC_001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	4,267	14867224	99216	5,779	6,935	N/A	N/A	N/A	N/A	
2	40 %	5	6,800	30778900	188725	11,963	13,191	N/A	N/A	N/A	N/A	
3	60 %	5	9,520	49577980	286500	19,270	20,025	N/A	N/A	N/A	N/A	
4	80 %	5	13,120	61097060	385084	23,747	26,217	N/A	N/A	N/A	N/A	
5	100 %	5	15,000	100961154	481168	39,241	33,632	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver