
Peak Find - Memory-1

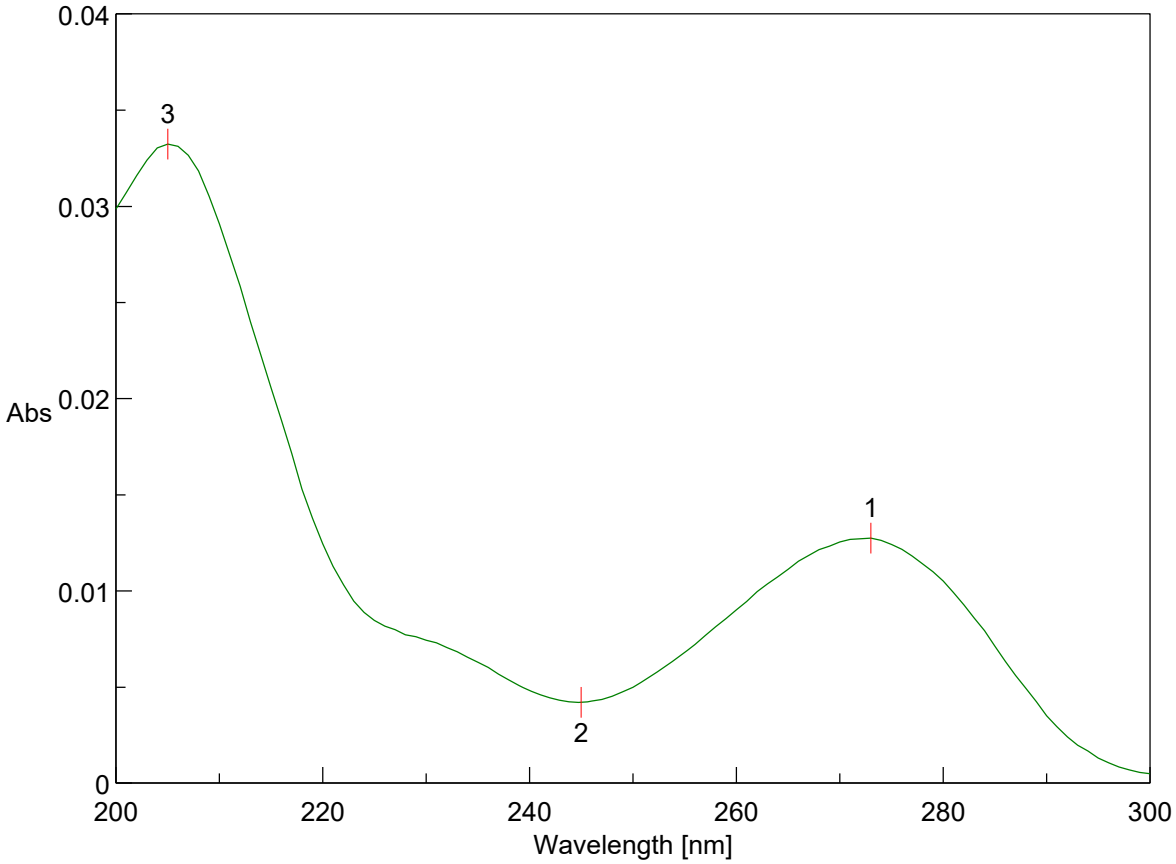

[Comments]


User	Mateus
Division	
Company	QPack
Creation date	16/11/2021 13:45

[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	300 nm	
Data interval	1 nm	
Data points	101	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.01274	2	245	0.004195
3	205	0.033229			

Chromatogram

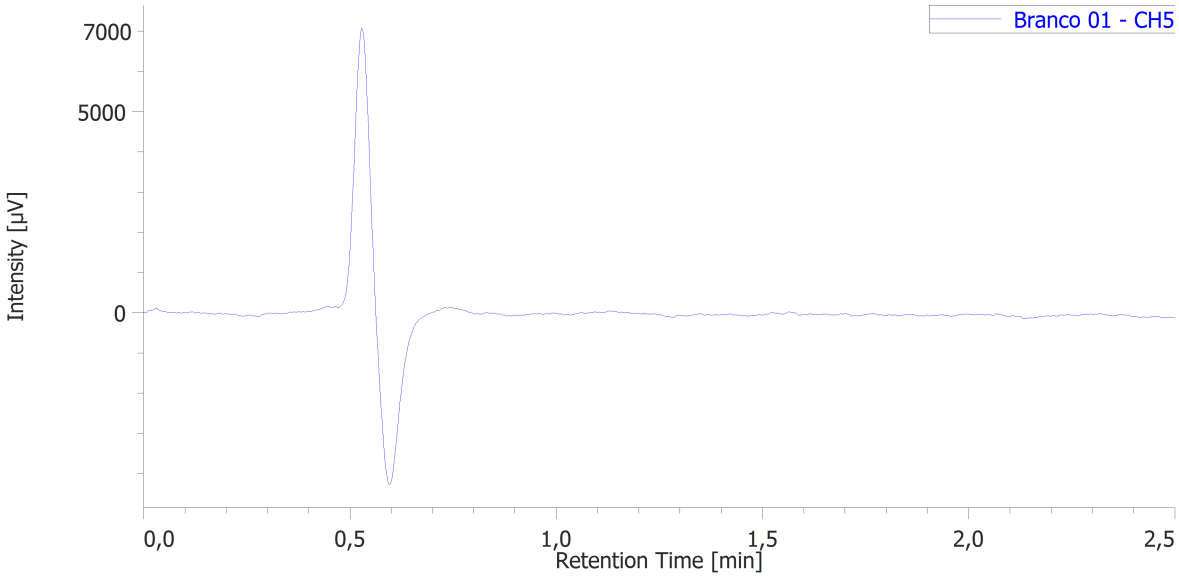


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:55:31
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:39:13
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

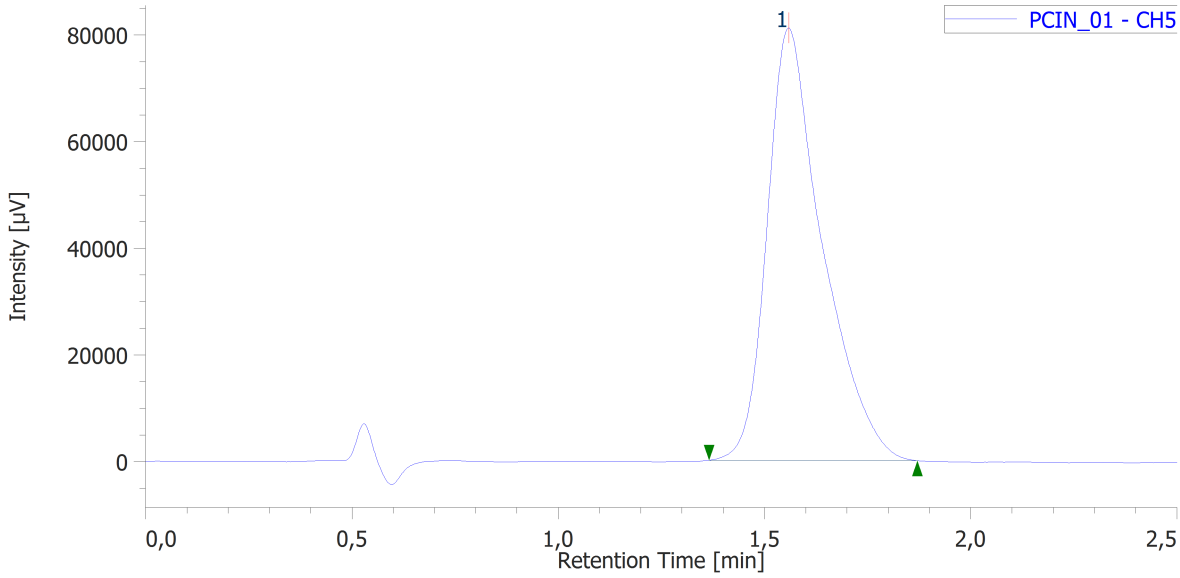

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:54:56
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:42:21
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,558	757785	81061	100,000	100,000	N/A	719	N/A	1,443	

Creator QPackSA
Reviewer
Approver

Chromatogram

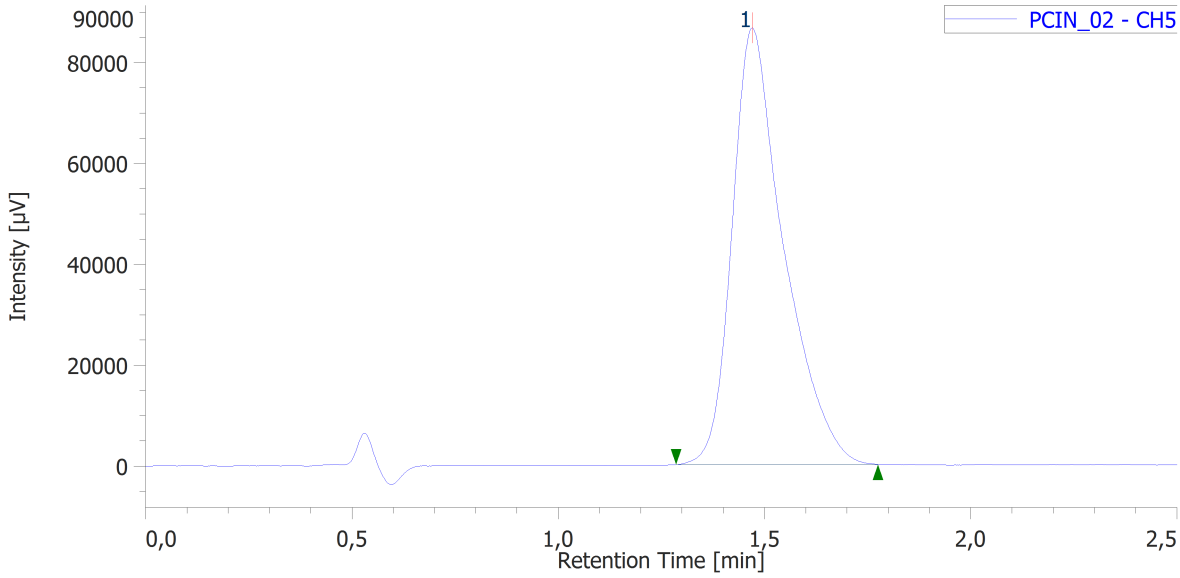

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:55:32
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:45:27
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,470	754787	86528	100,000	100,000	N/A	734	N/A	1,447	

Creator QPackSA
Reviewer
Approver

Chromatogram

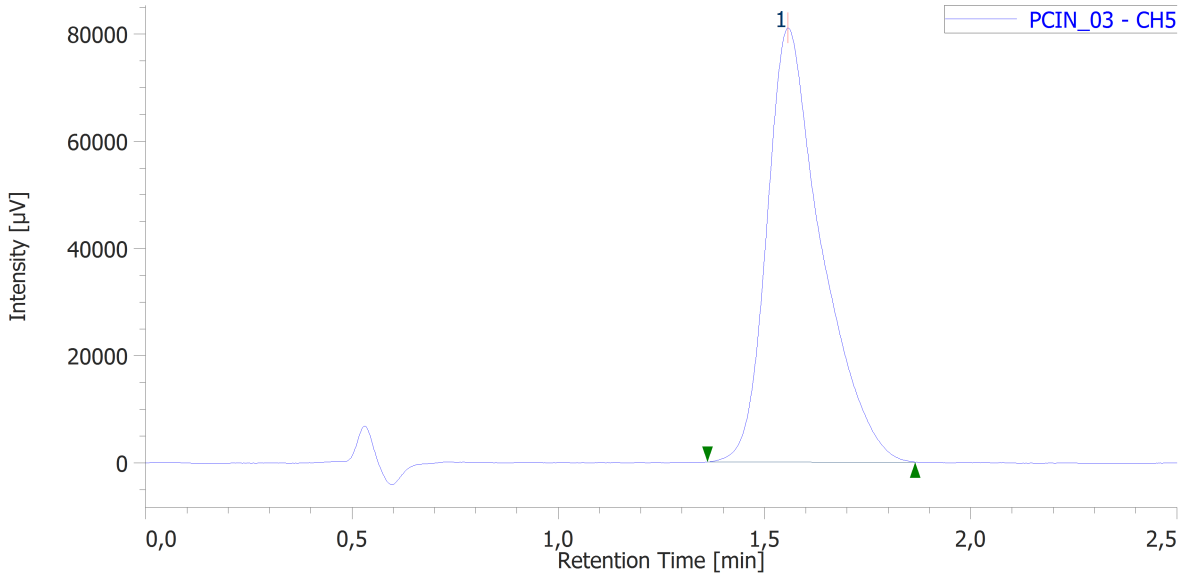

Chromatogram Information

User Name	QPackSA
Date Modified	16/11/2021 13:55:32
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:48:35
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,557	748509	80928	100,000	100,000	N/A	735	N/A	1,451	

Creator QPackSA
Reviewer
Approver

Chromatogram

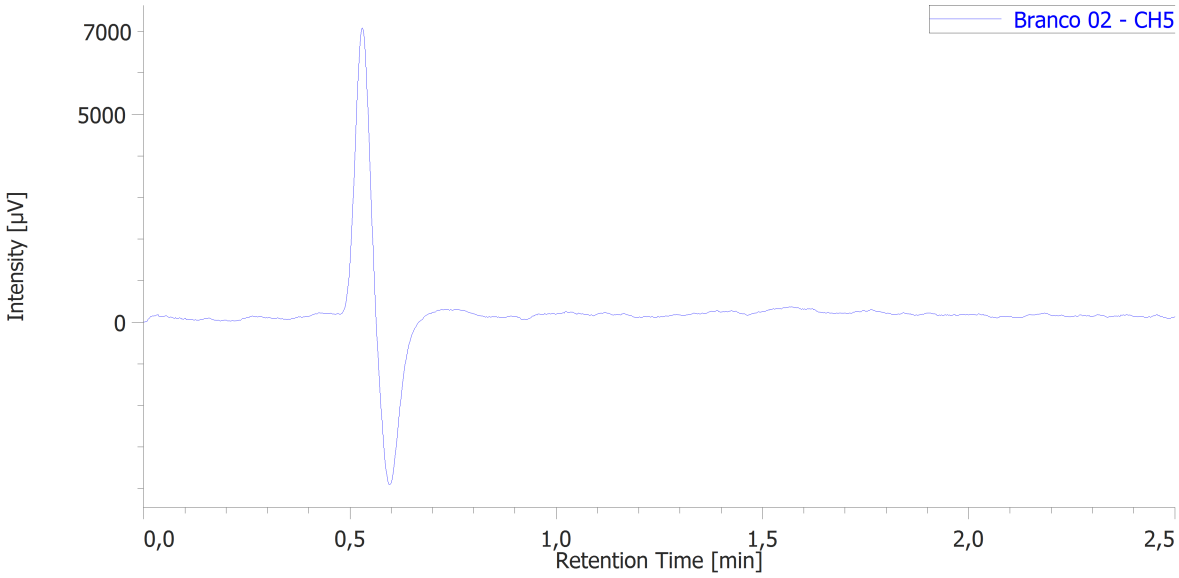


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:55:32
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:51:41
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

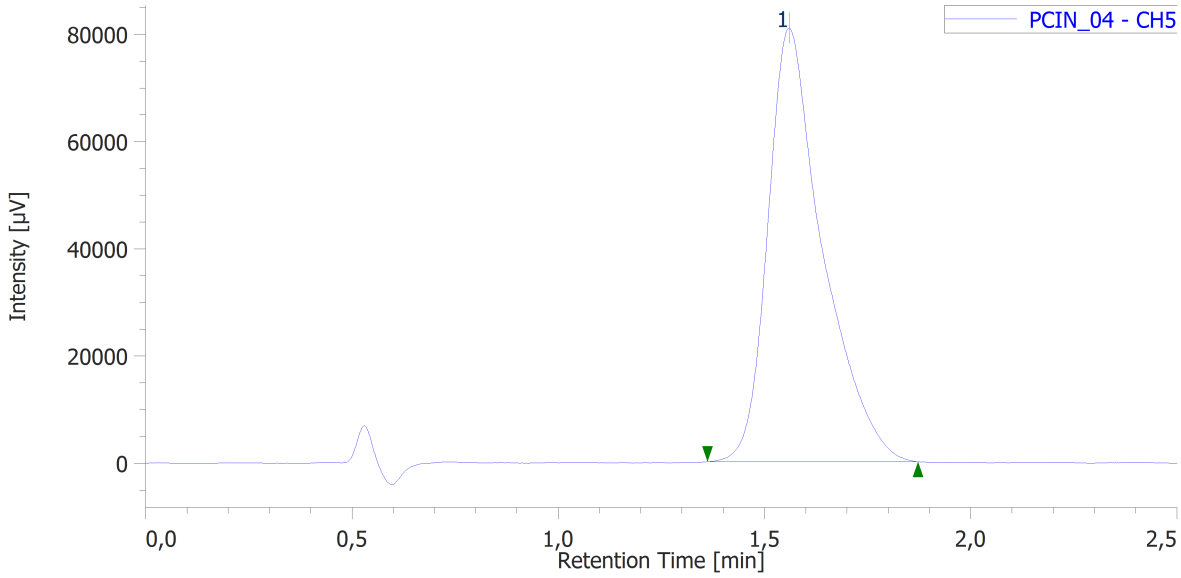

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 13:58:06
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:54:50
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,560	748713	80865	100,000	100,000	N/A	759	N/A	1,462	

Creator QPackSA
Reviewer
Approver

Chromatogram

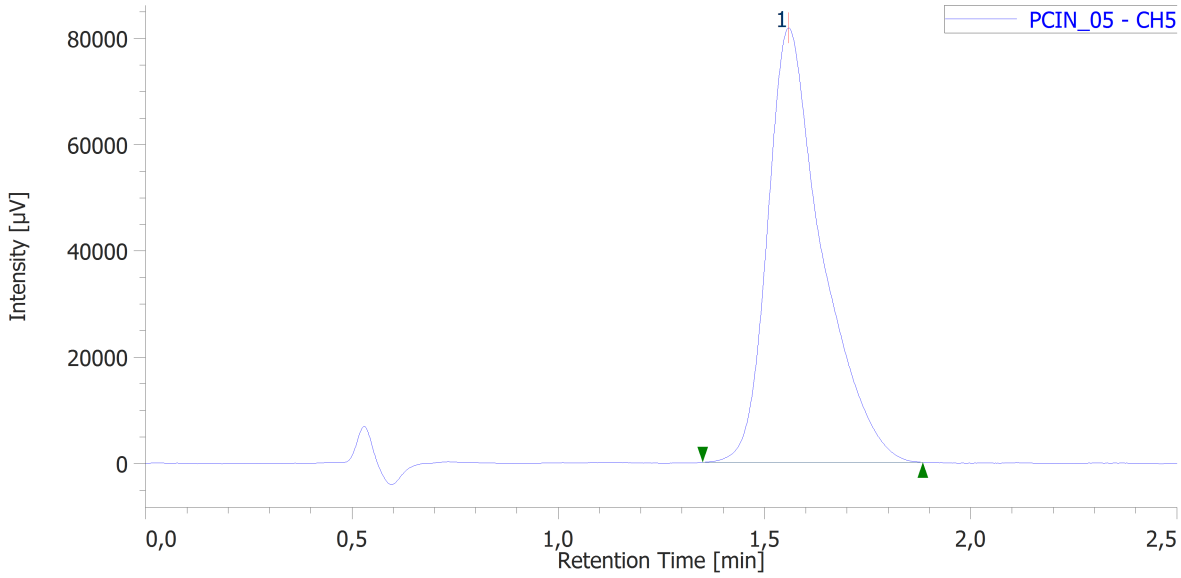

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:01:36
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 13:57:58
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,558	753899	81728	100,000	100,000	N/A	776	N/A	1,476	

Creator QPackSA
Reviewer
Approver

Chromatogram

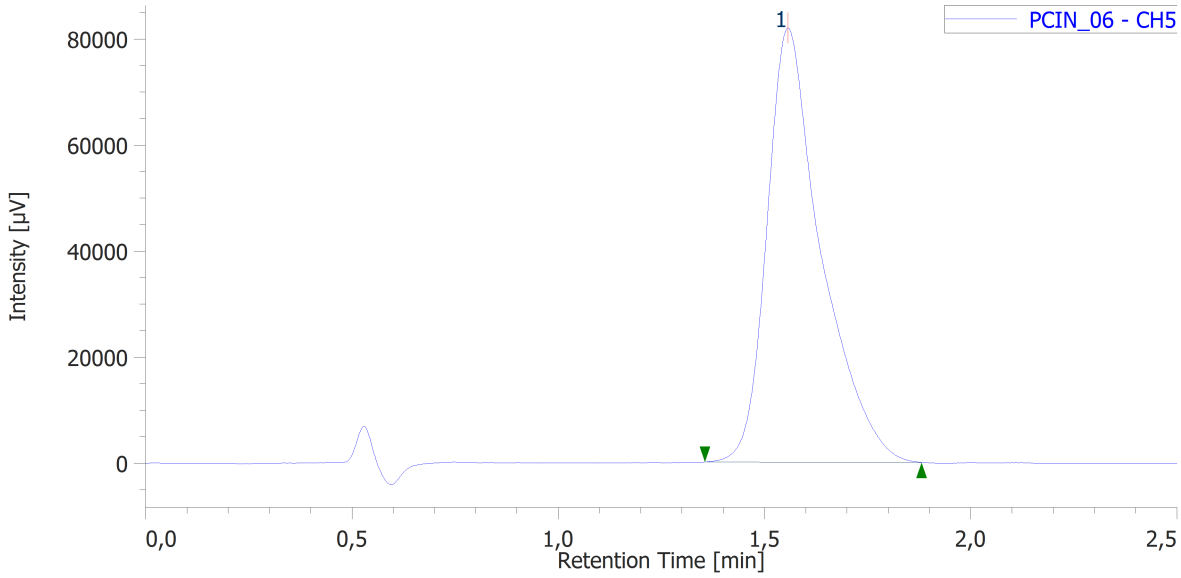

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:04:03
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:01:06
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN_06-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,557	750355	81837	100,000	100,000	N/A	790	N/A	1,482	

Creator QPackSA
Reviewer
Approver

Chromatogram

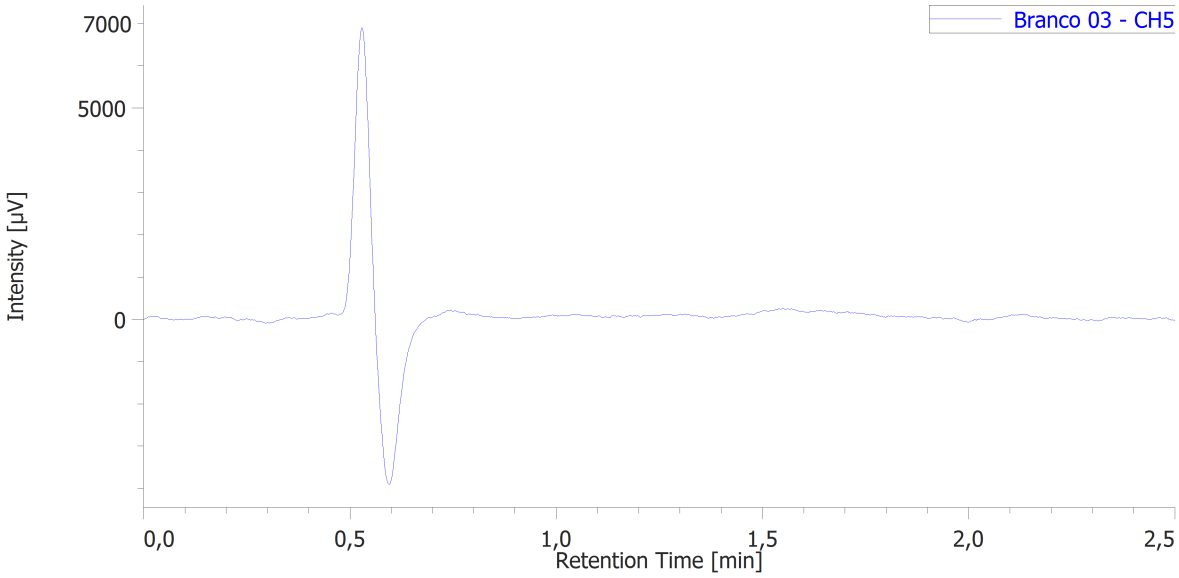


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:07:43
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:04:14
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

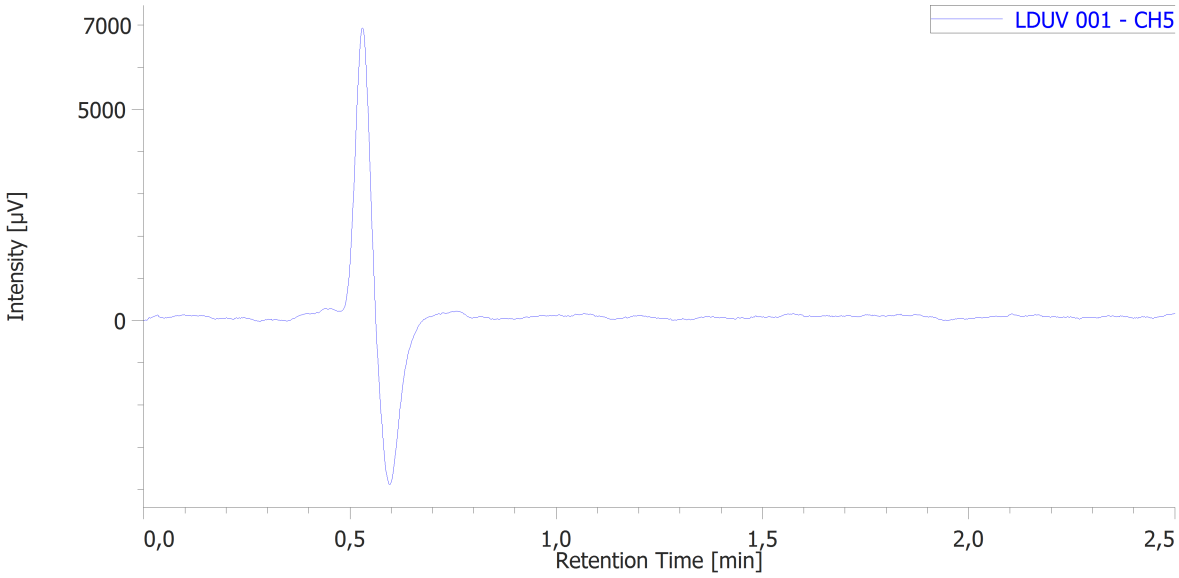


Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:26:39
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:09:17
Volume	10,0 [µL]
Sample #	51
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

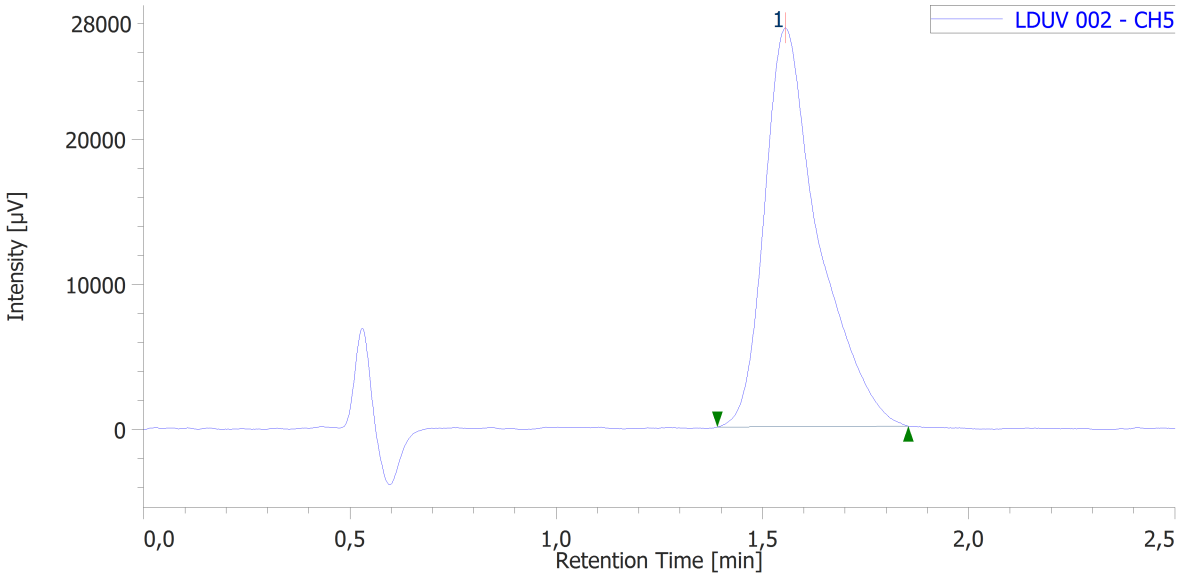

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:26:39
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:12:25
Volume	10,0 [µL]
Sample #	52
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,555	251275	27485	100,000	100,000	N/A	819	N/A	1,512	

Creator QPackSA
Reviewer
Approver

Chromatogram

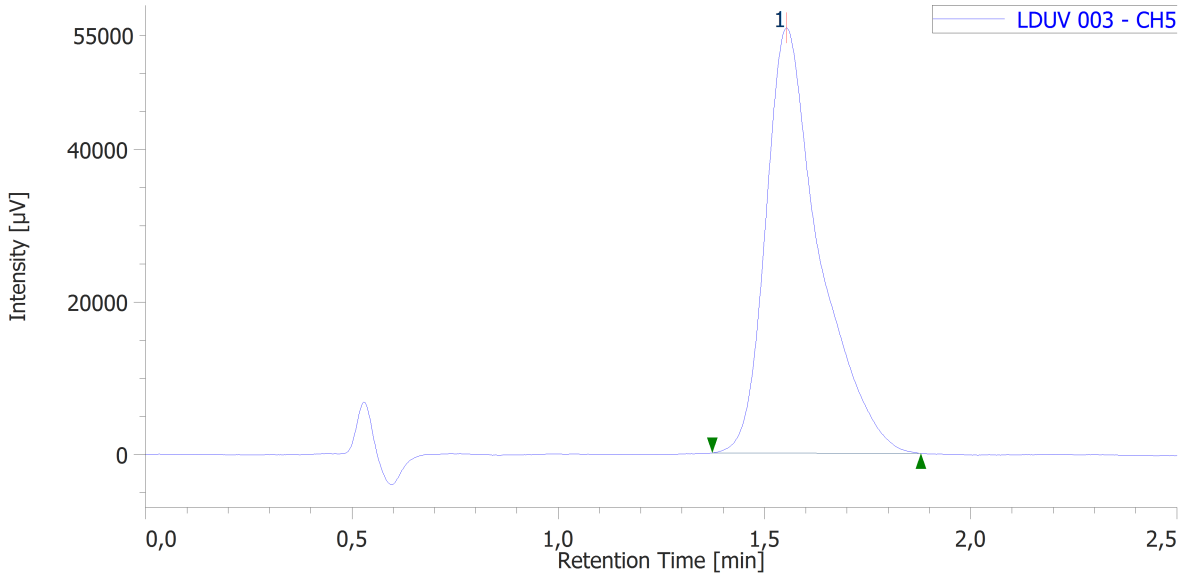

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:26:39
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:15:36
Volume	10,0 [µL]
Sample #	53
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,553	507203	55726	100,000	100,000	N/A	834	N/A	1,507	

Creator QPackSA
Reviewer
Approver

Chromatogram

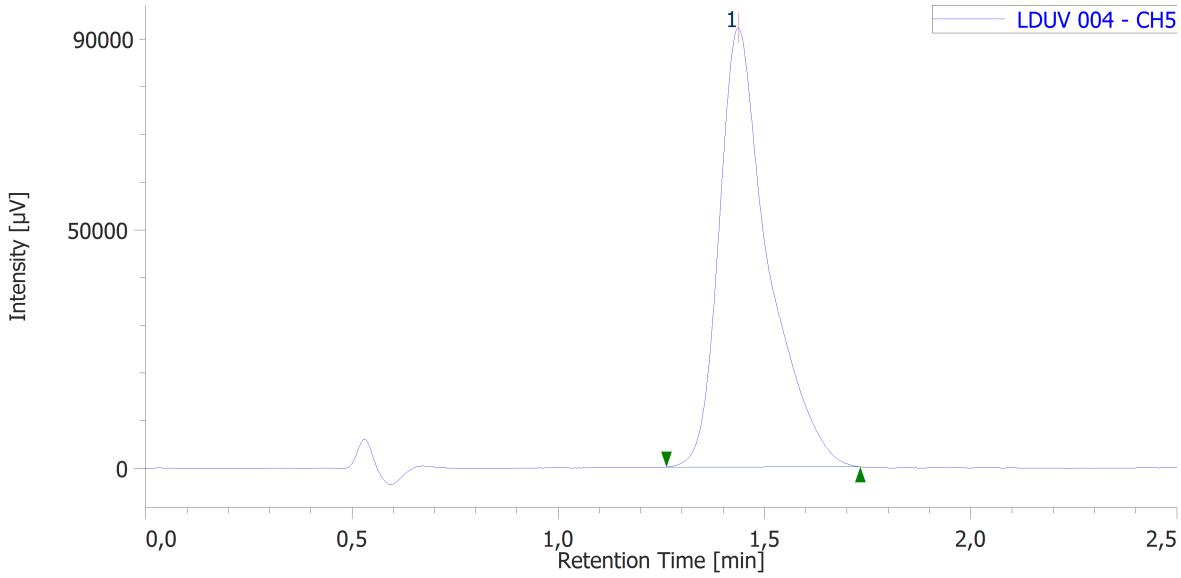

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:26:39
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:18:39
Volume	10,0 [µL]
Sample #	54
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,437	765325	92011	100,000	100,000	N/A	863	N/A	1,504	

Creator QPackSA
Reviewer
Approver

Chromatogram

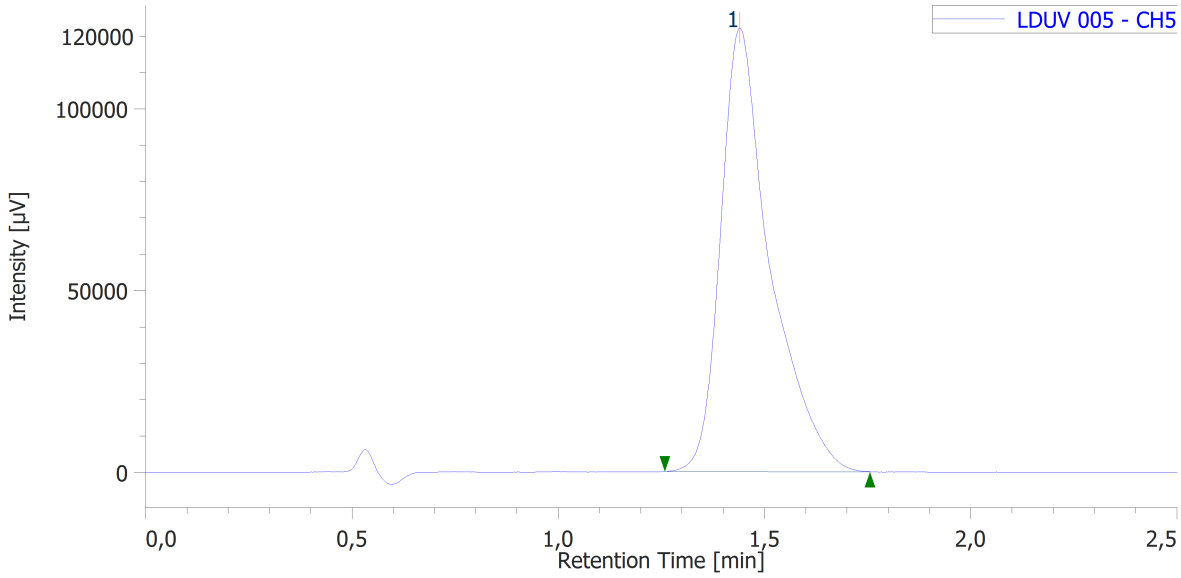

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:26:40
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:21:47
Volume	10,0 [µL]
Sample #	55
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,440	1018594	121923	100,000	100,000	N/A	864	N/A	1,523	

Creator QPackSA
Reviewer
Approver

Chromatogram

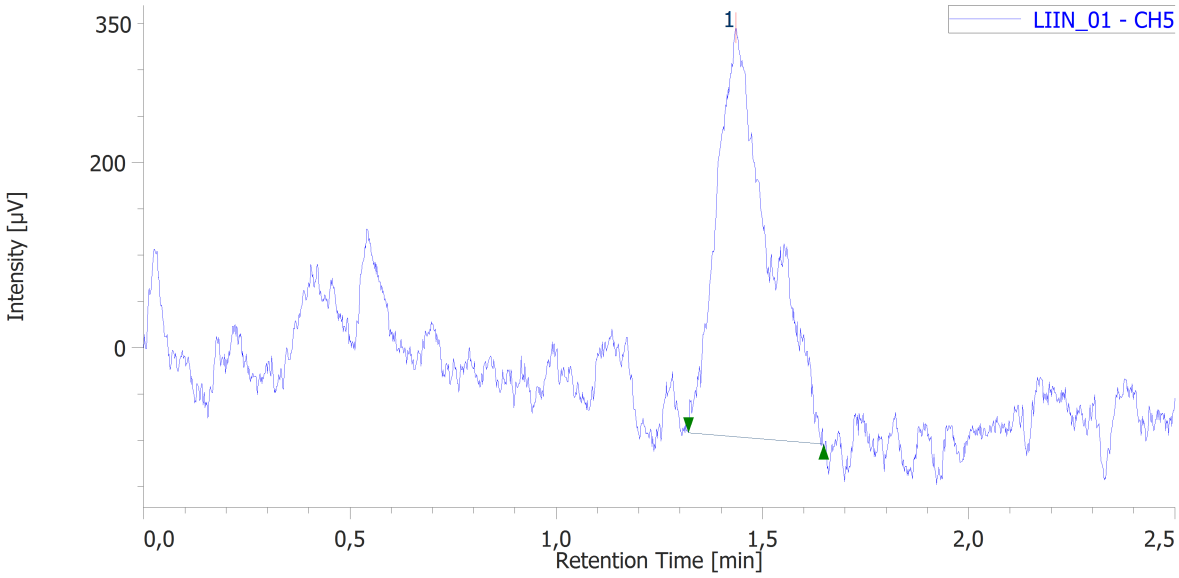

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:36:12
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:28:24
Volume	0,1 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,435	3902	441	100,000	100,000	N/A	780	N/A	1,387	

Creator QPackSA
Reviewer
Approver

Chromatogram

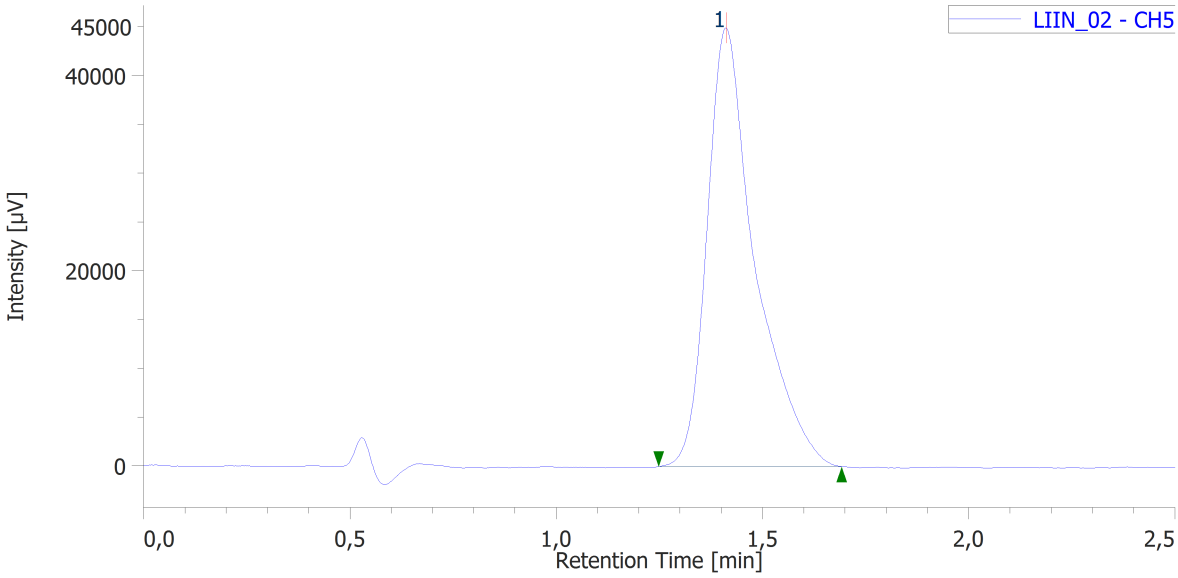

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:36:12
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:31:30
Volume	5,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,412	364247	44915	100,000	100,000	N/A	884	N/A	1,510	

Creator QPackSA
Reviewer
Approver

Chromatogram

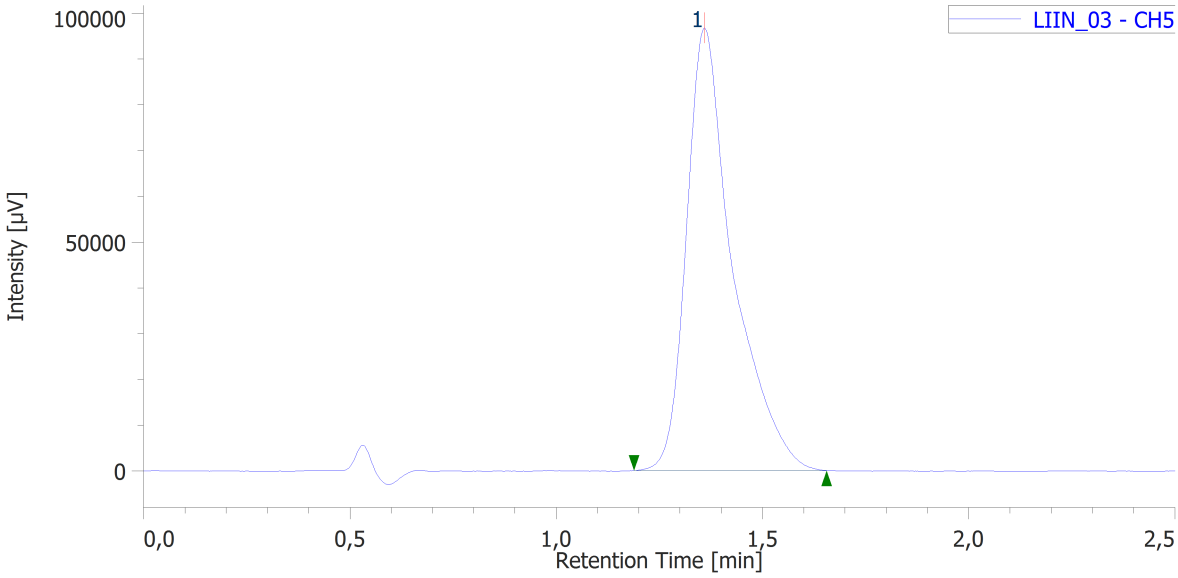

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:46:12
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:34:38
Volume	10,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,358	755648	96601	100,000	100,000	N/A	891	N/A	1,554	

Creator QPackSA
Reviewer
Approver

Chromatogram

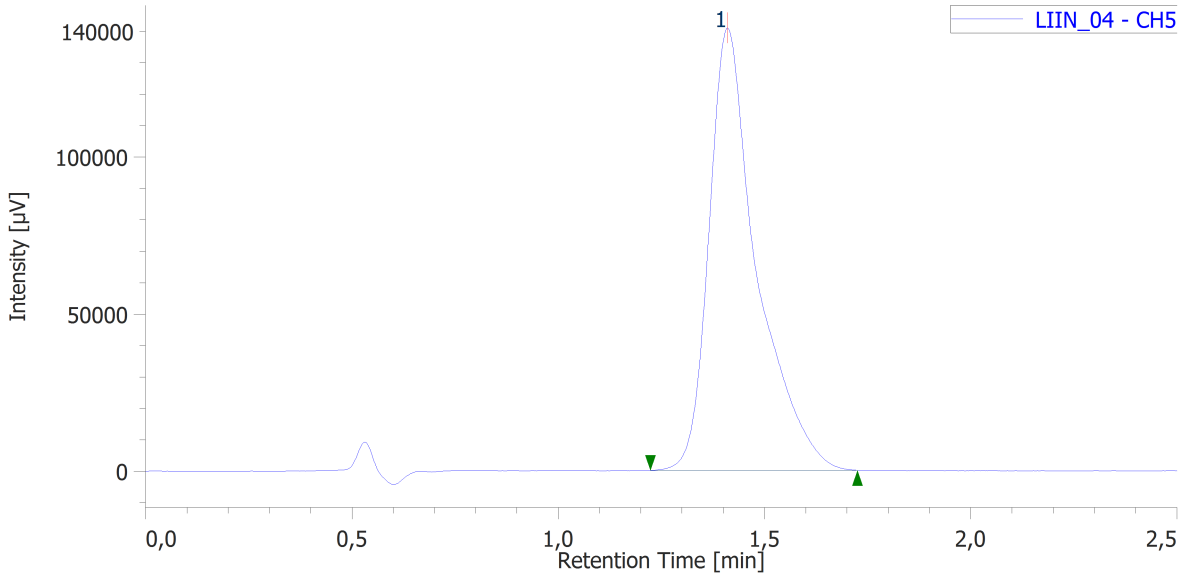

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:46:12
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:37:49
Volume	15,0 [μL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,410	1134031	140765	100,000	100,000	N/A	927	N/A	1,552	

Creator QPackSA
Reviewer
Approver

Chromatogram

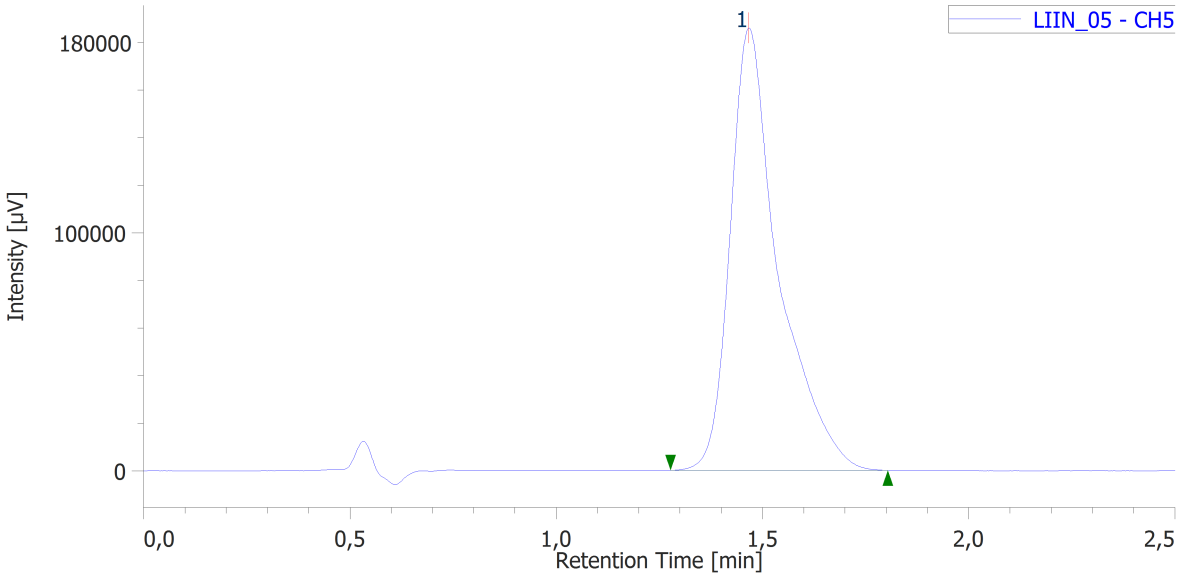

Chromatogram Information	
User Name	QPackSA
Date Modified	16/11/2021 14:46:12
Description	
HPLC System Name	HPL20_PDA
Injection Date	16/11/2021 14:41:01
Volume	20,0 [µL]
Sample #	56
Project Name	Qualificação
Acquisition Time	2,5 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN_05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,467	1515808	185781	100,000	100,000	N/A	995	N/A	1,563	

Creator QPackSA
Reviewer
Approver

Chromatogram

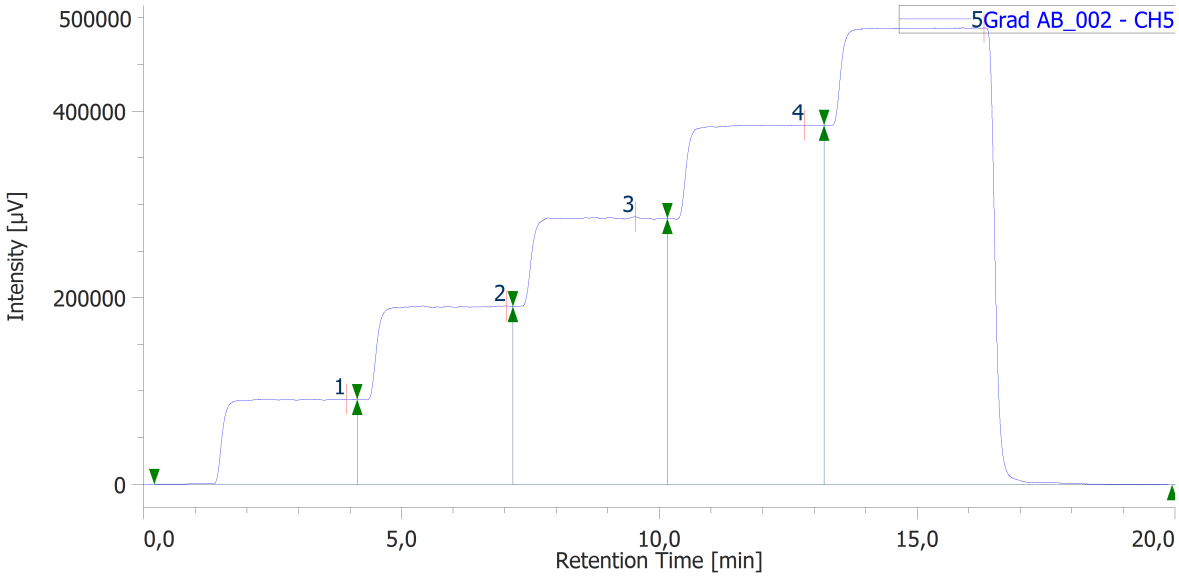

Chromatogram Information	
User Name	QPackSA
Date Modified	18/11/2021 08:19:42
Description	
HPLC System Name	HPL20_PDA
Injection Date	18/11/2021 07:59:41
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Qualificação Gradiente
Peak ID Table	Grad_AB
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Grad AB_002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	3,935	14251519	91123	5,498	6,316	N/A	N/A	N/A	N/A	
2	40 %	5	7,040	32186080	191166	12,417	13,250	N/A	N/A	N/A	N/A	
3	60 %	5	9,532	49227167	286601	18,991	19,865	N/A	N/A	N/A	N/A	
4	80 %	5	12,818	67801428	384861	26,157	26,676	N/A	N/A	N/A	N/A	
5	100 %	5	16,288	95742656	488972	36,936	33,892	N/A	N/A	N/A	N/A	

Creator
Reviewer
Approver

Chromatogram

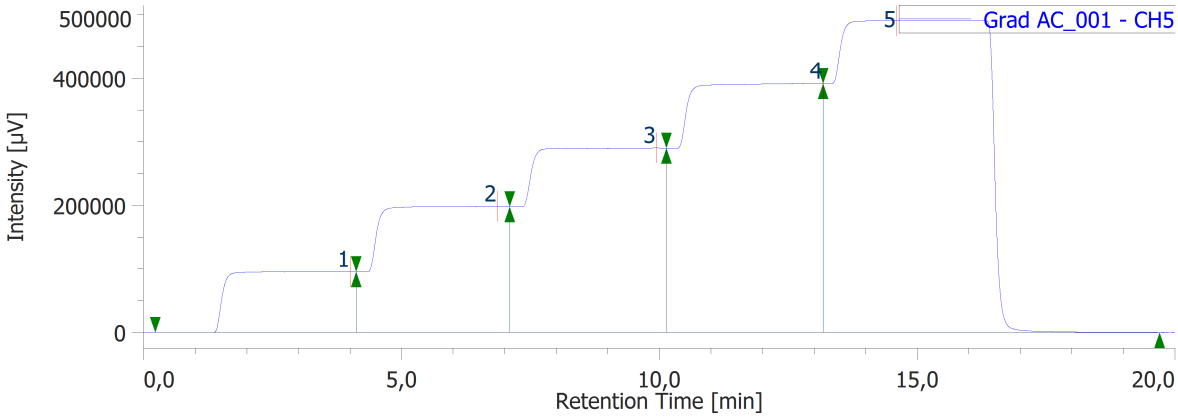

Channel & Peak Information Table

Chromatogram Name: Grad AC_001-CH5
Sample Name:
Channel Name: 273,0nm

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20 %	5	4,010	14896296	95705	5,650	6,531	N/A	N/A	N/A	N/A	
2	40 %	5	6,852	32899804	198117	12,479	13,519	N/A	N/A	N/A	N/A	
3	60 %	5	9,940	50507189	290094	19,157	19,795	N/A	N/A	N/A	N/A	
4	80 %	5	13,167	68789798	391520	26,092	26,716	N/A	N/A	N/A	N/A	
5	100 %	5	14,597	96553723	490063	36,622	33,440	N/A	N/A	N/A	N/A	