
Chromatogram

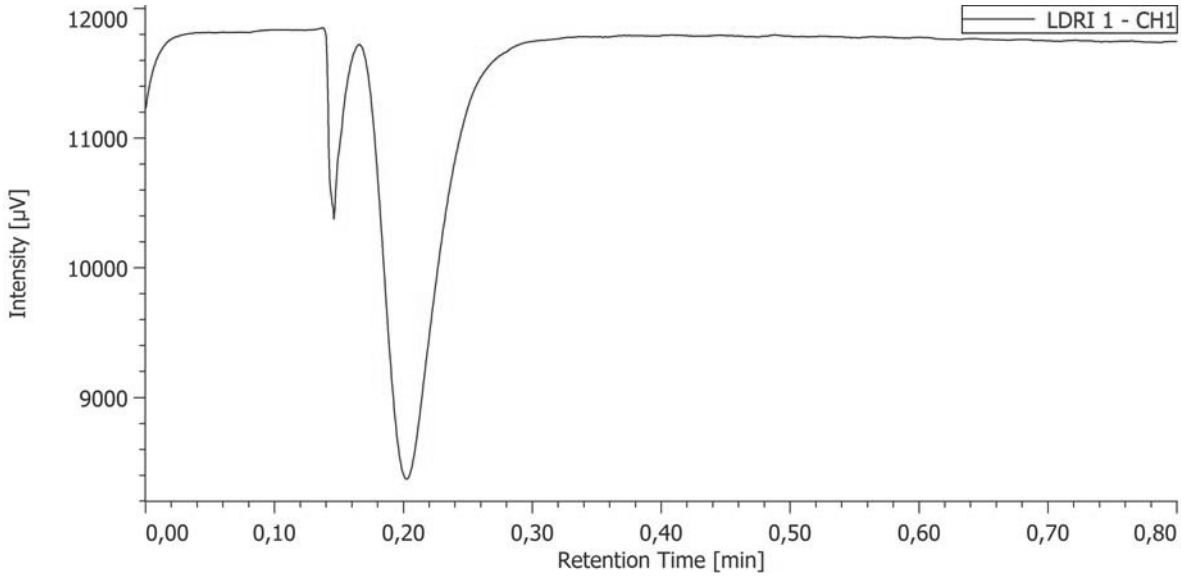


Chromatogram Information	
User Name	QPackSA
Date Modified	17/06/2024 16:08:09
Description	
HPLC System Name	HPL08 RI
Injection Date	17/06/2024 16:07:18
Volume	2,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	0,8 [min]
Acquisition Sequence	Qualificação RID
Control Method	Qualificação_RID
Peak ID Table	Identificação
Calibration Method	Curva RID
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 1-CH1
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	Integração

Creator QPackSA
Reviewer
Approver

Chromatogram

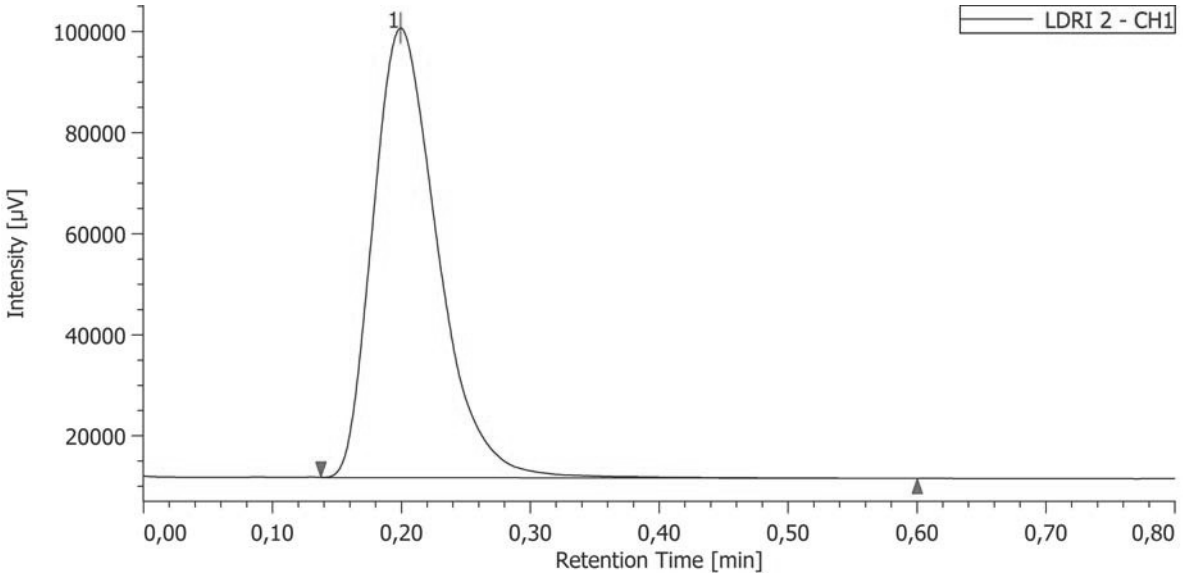

Chromatogram Information	
User Name	QPackSA
Date Modified	17/06/2024 16:12:22
Description	
HPLC System Name	HPL08 RI
Injection Date	17/06/2024 16:11:31
Volume	2,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	0,8 [min]
Acquisition Sequence	Qualificação RID
Control Method	Qualificação_RID
Peak ID Table	Identificação
Calibration Method	Curva RID
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 2-CH1
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão RID	1	0,199	310383	88936	100,000	100,000	N/A	78	N/A	1,371	

Creator QPackSA
Reviewer
Approver

Chromatogram

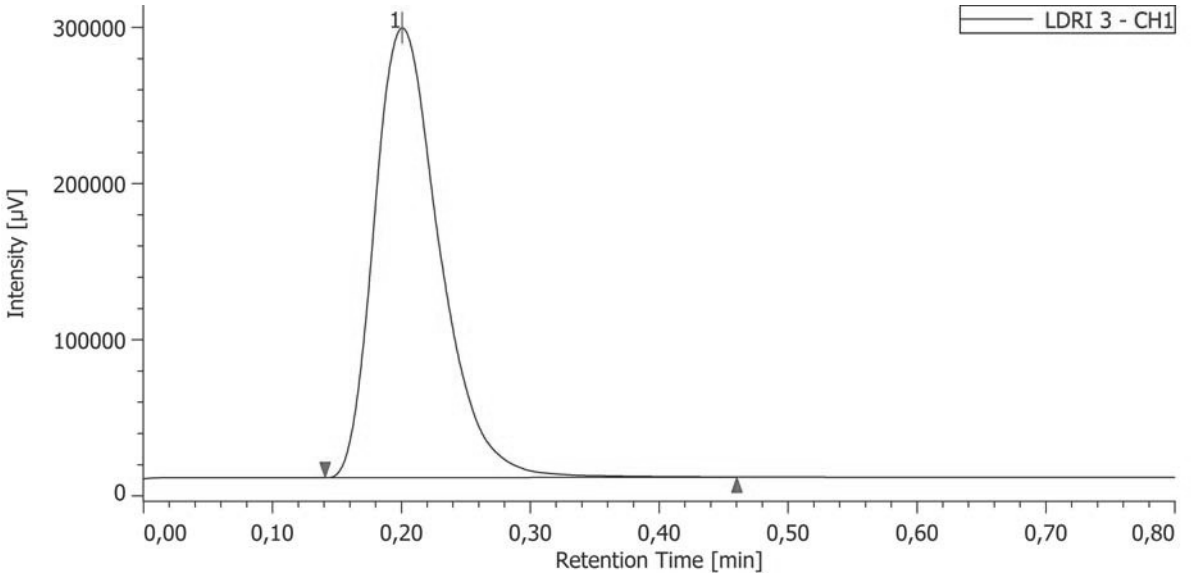

Chromatogram Information	
User Name	QPackSA
Date Modified	17/06/2024 16:16:37
Description	
HPLC System Name	HPL08 RI
Injection Date	17/06/2024 16:15:48
Volume	2,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	0,8 [min]
Acquisition Sequence	Qualificação RID
Control Method	Qualificação_RID
Peak ID Table	Identificação
Calibration Method	Curva RID
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 3-CH1
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão RID	1	0,201	1012041	287791	100,000	100,000	N/A	79	N/A	1,361	

Creator QPackSA
Reviewer
Approver

Chromatogram

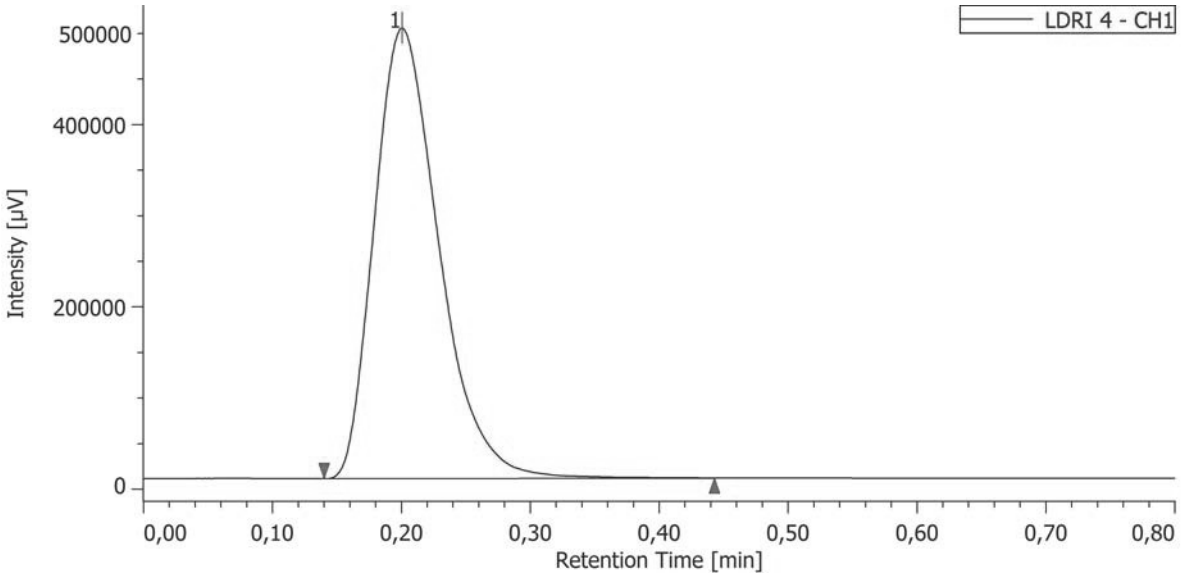

Chromatogram Information	
User Name	QPackSA
Date Modified	17/06/2024 16:20:53
Description	
HPLC System Name	HPL08 RI
Injection Date	17/06/2024 16:20:04
Volume	2,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	0,8 [min]
Acquisition Sequence	Qualificação RID
Control Method	Qualificação_RID
Peak ID Table	Identificação
Calibration Method	Curva RID
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDRI 4-CH1
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão RID	1	0,201	1721592	494053	100,000	100,000	N/A	78	N/A	1,352	

Creator QPackSA
Reviewer
Approver

Chromatogram

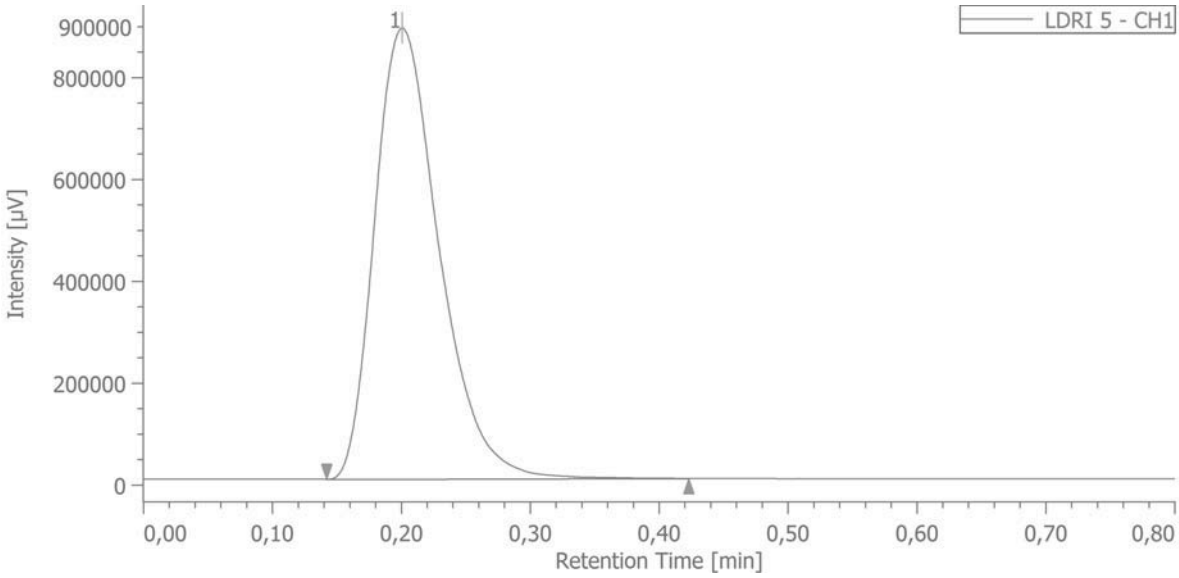

Chromatogram Information	
User Name	QPackSA
Date Modified	17/06/2024 16:25:09
Description	
HPLC System Name	HPL08 RI
Injection Date	17/06/2024 16:24:20
Volume	2,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	0,8 [min]
Acquisition Sequence	Qualificação RID
Control Method	Qualificação_RID
Peak ID Table	Identificação
Calibration Method	Curva RID
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDRI 5-CH1
Sample Name	
Channel Name	RI
Sampling Interval	40 [msec]
Peak Method	Integração

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Padrão RID	1	0,201	3483514	885398	100,000	100,000	N/A	80	N/A	1,360	

Creator QPackSA
Reviewer
Approver