
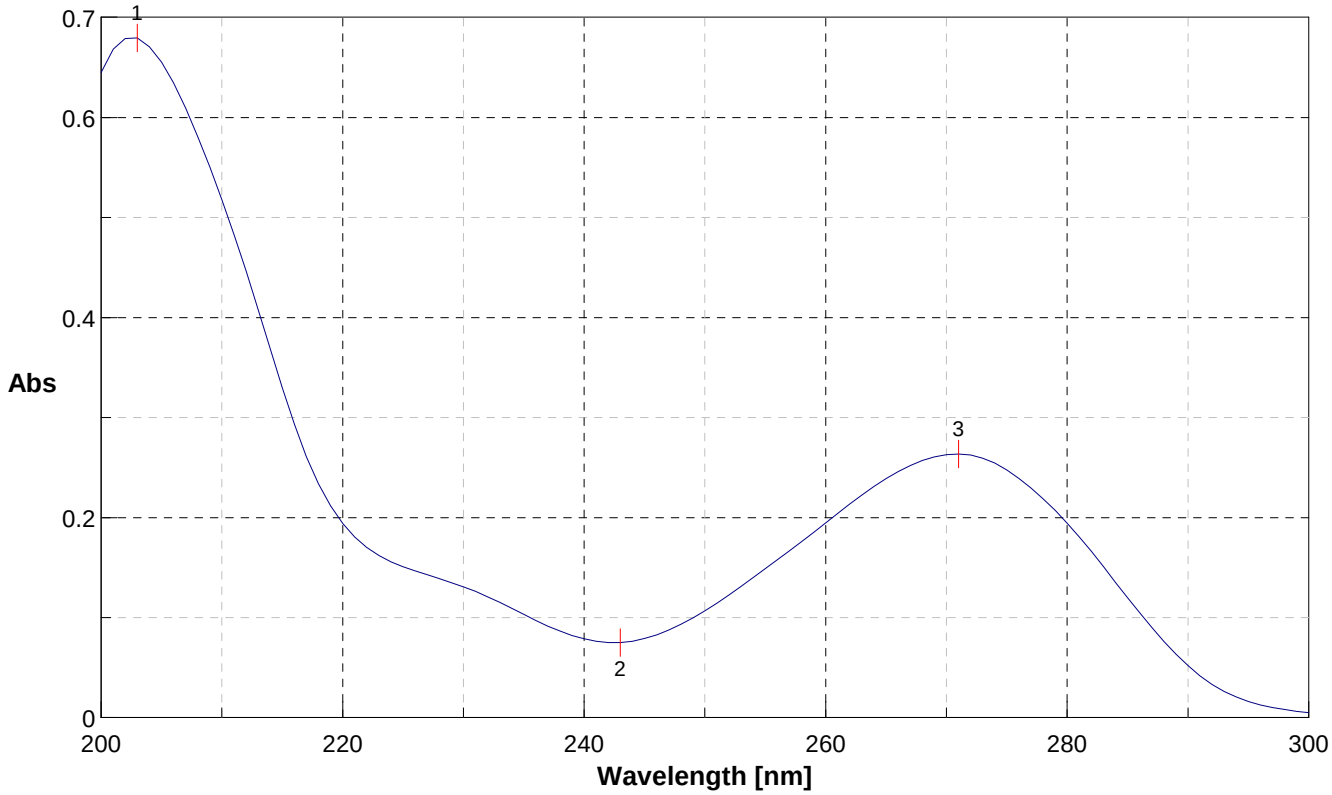


Date	12/12/2016 12:36
File name	EDUV_002 PDA_1,6400.JWS
Model	MD-2010
Serial No.	0000000000
Sample name	
Operator	Administrator
Comment	---

No.	nm	Abs	No.	nm	Abs	No.	nm	Abs
1	203	0.679585	2	243	0.075299	3	271	0.263682

Chromatogram

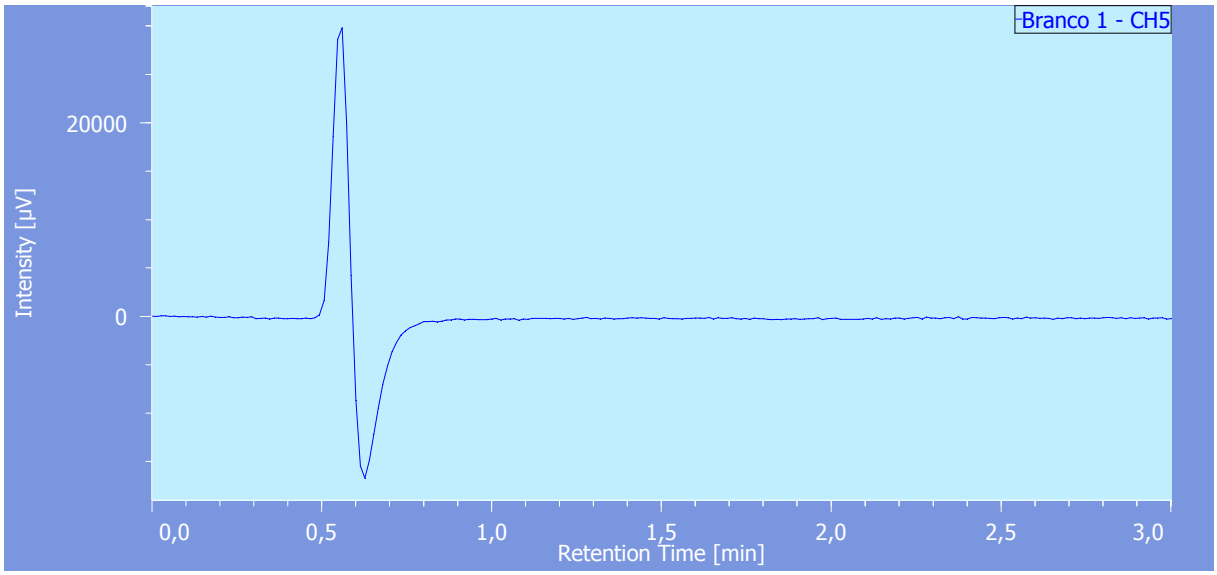


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:34:59
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 11:59:40
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

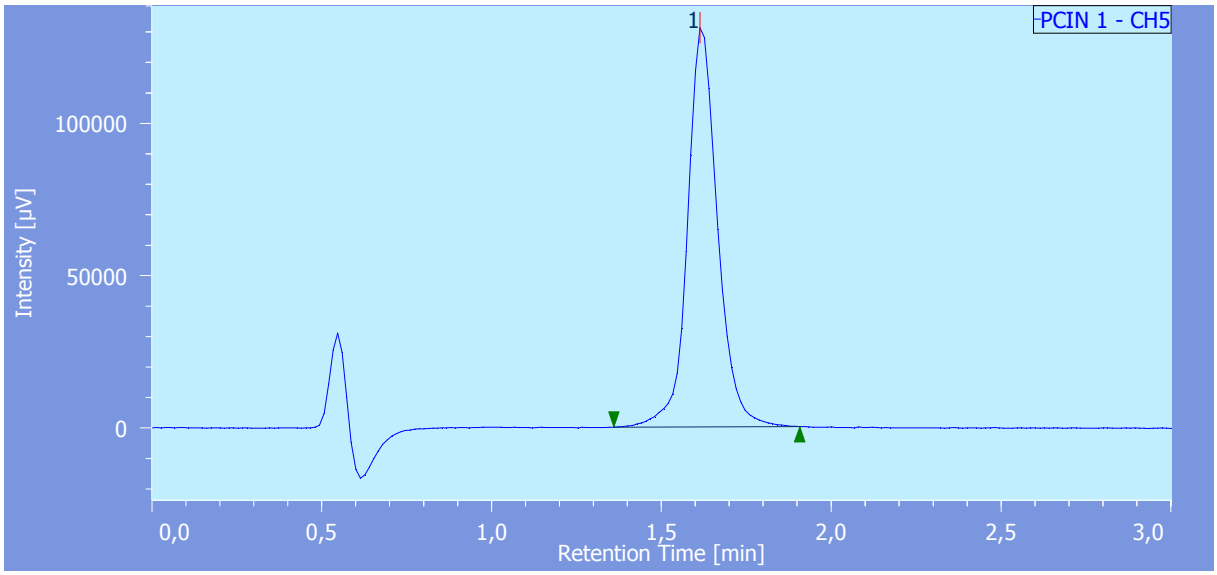

Chromatogram Information

User Name	Administrator
Date Modified	12/12/2016 12:35:00
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:03:22
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,613	810235	130903	100,000	100,000	N/A	1794	N/A	1,123	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

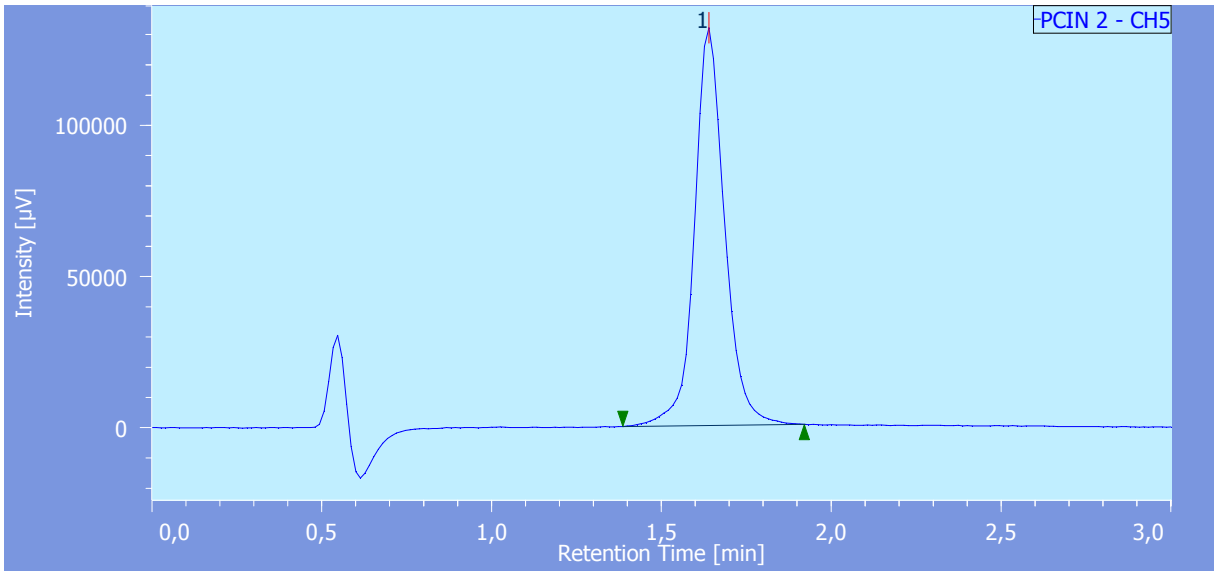


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:01
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:07:02
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,640	813539	131393	100,000	100,000	N/A	1831	N/A	1,066	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

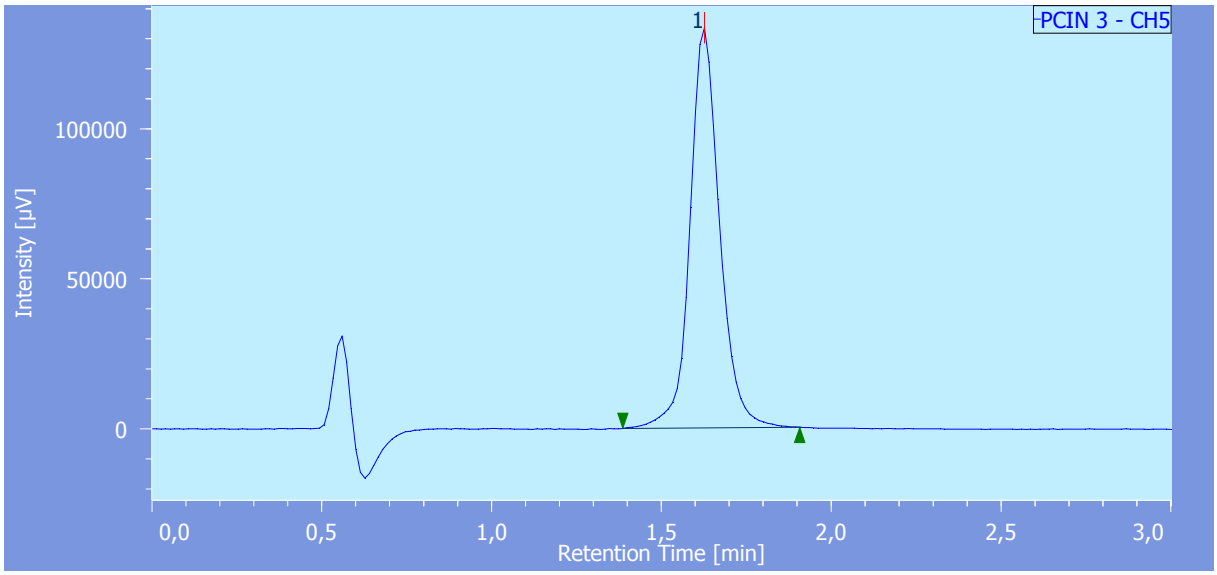

Chromatogram Information

User Name	Administrator
Date Modified	12/12/2016 12:35:01
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:10:44
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,627	809632	133138	100,000	100,000	N/A	1855	N/A	1,070	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

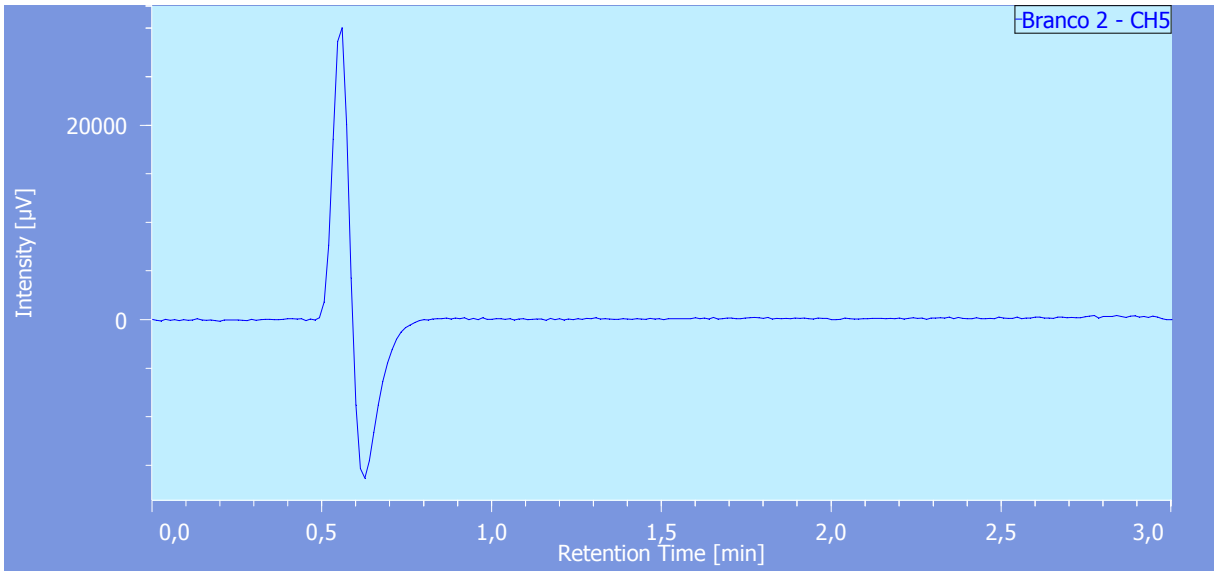


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:01
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:14:24
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

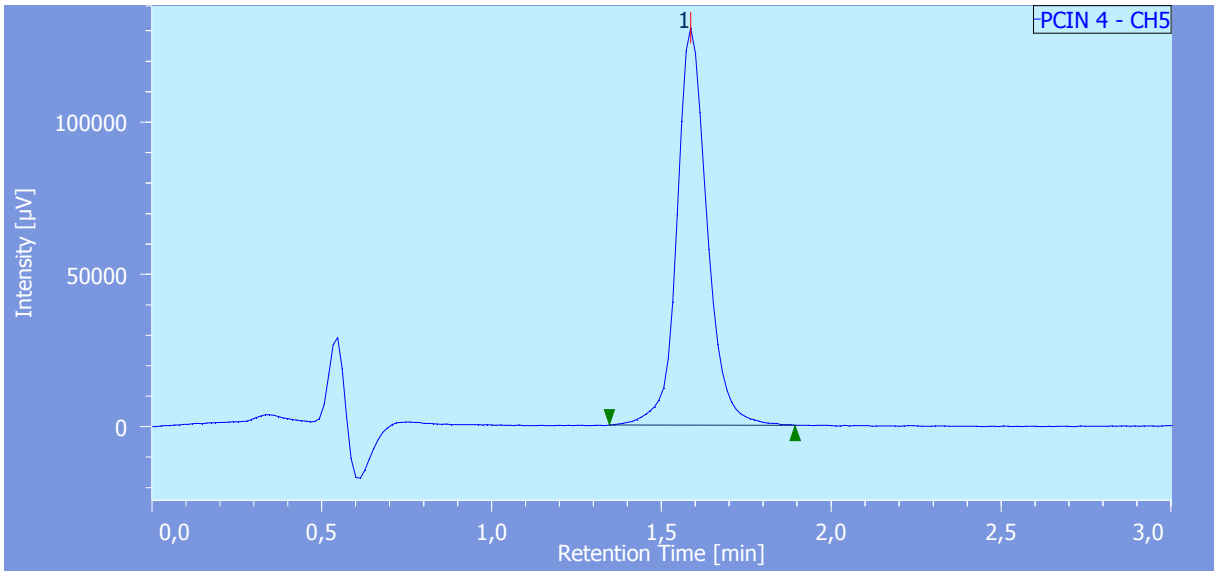


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:02
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:18:07
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,587	808526	130352	100,000	100,000	N/A	1699	N/A	1,107	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

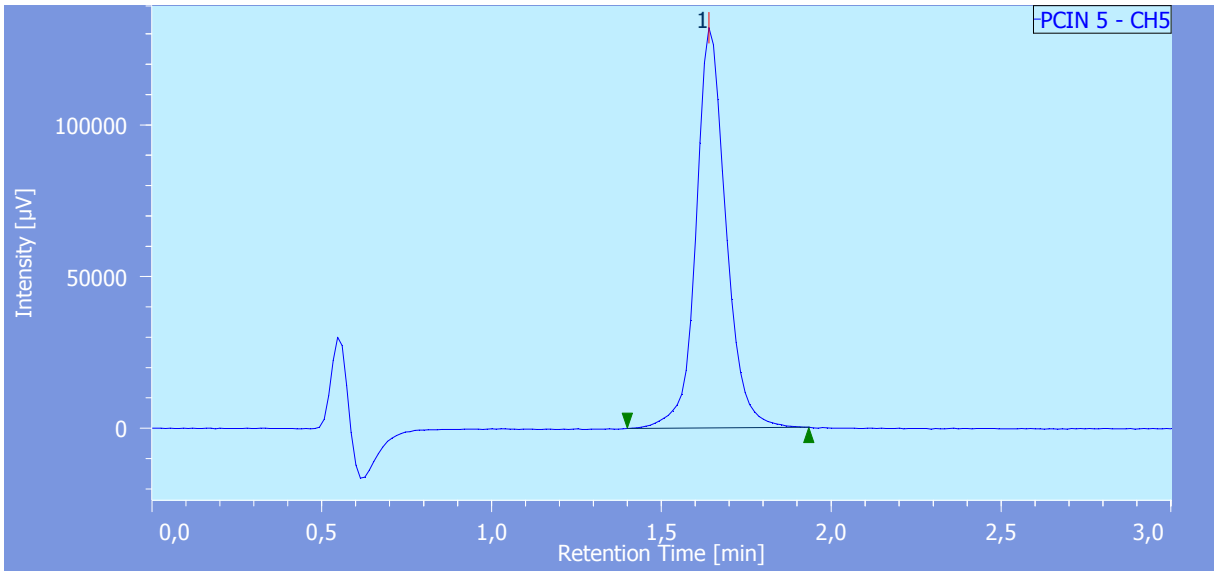


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:02
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:21:49
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,640	807749	131816	100,000	100,000	N/A	1861	N/A	1,124	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

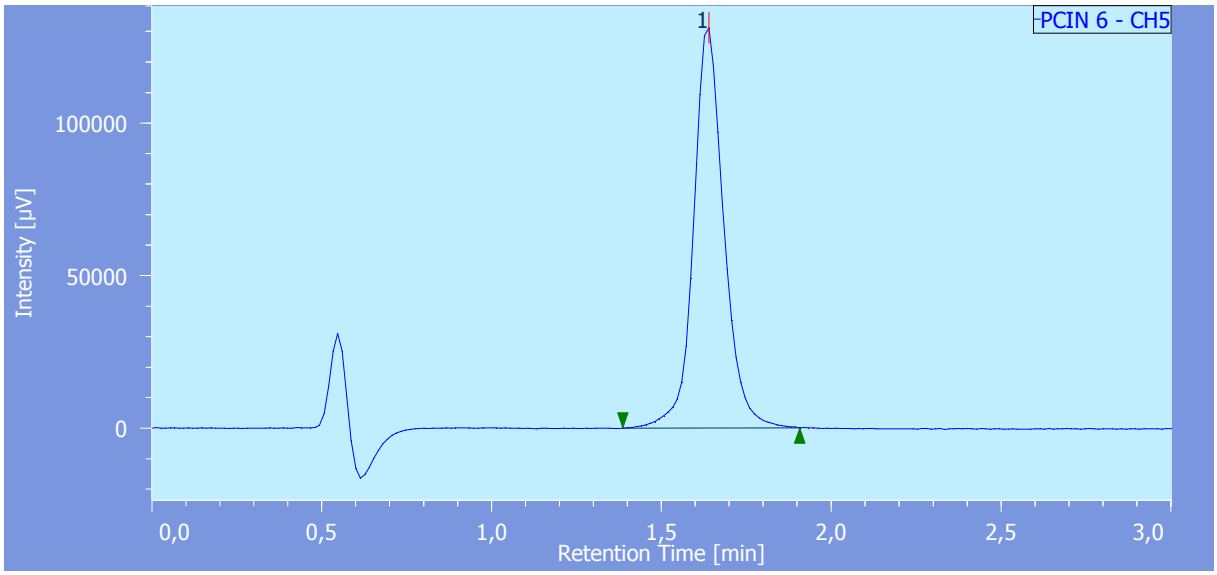


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:03
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:25:31
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	PCIN 6-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,640	816281	130979	100,000	100,000	N/A	1799	N/A	1,051	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

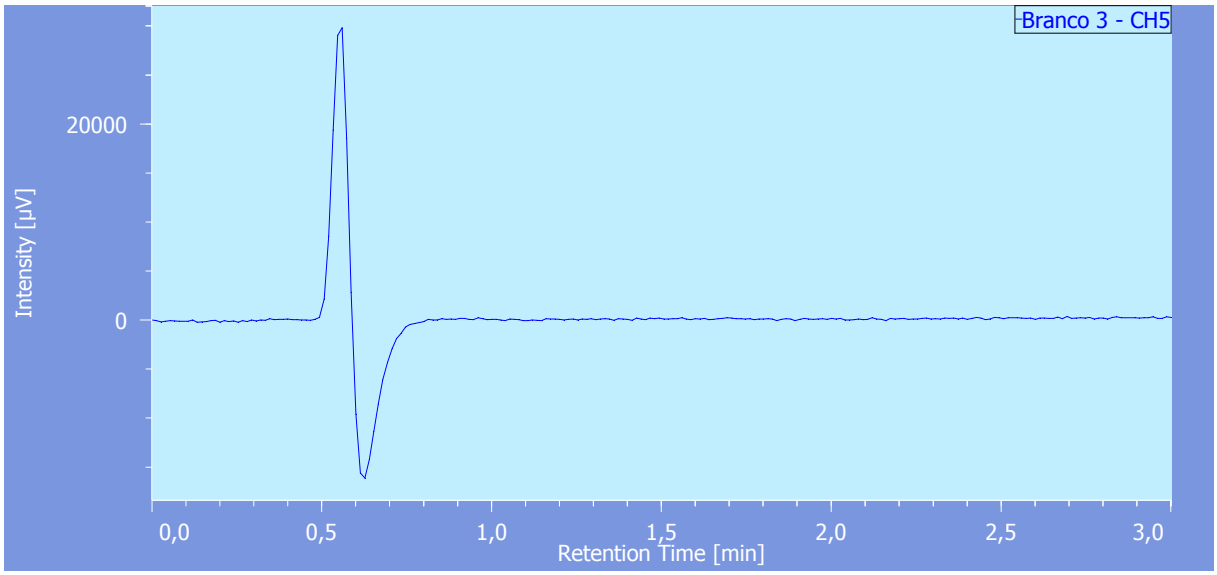


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:35:03
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:29:13
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	PCIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Branco 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

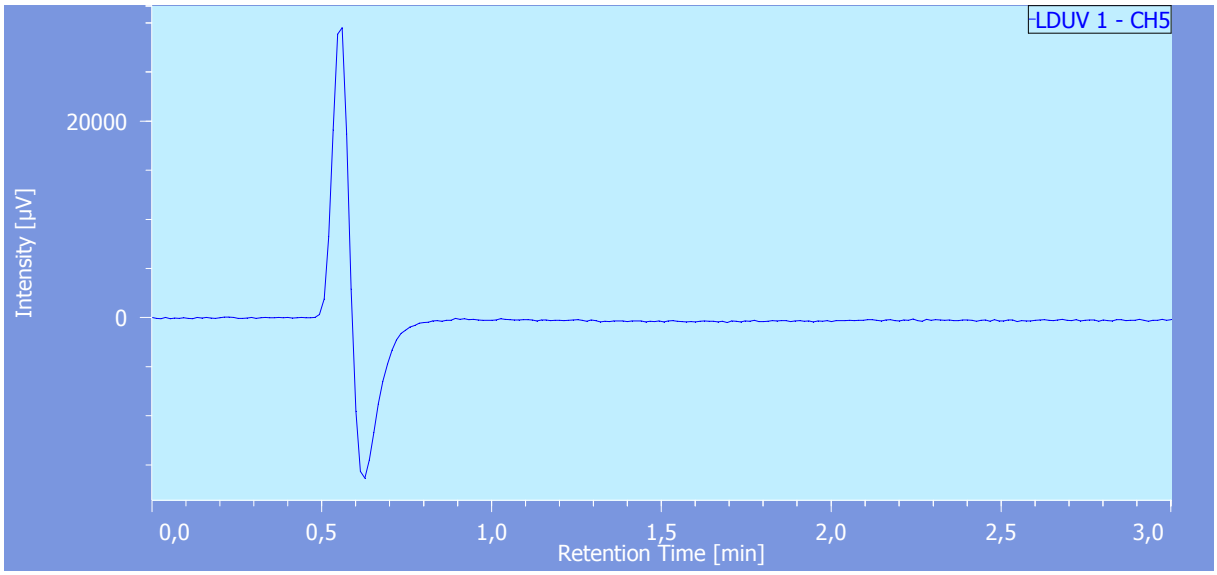


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:54:43
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:35:33
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

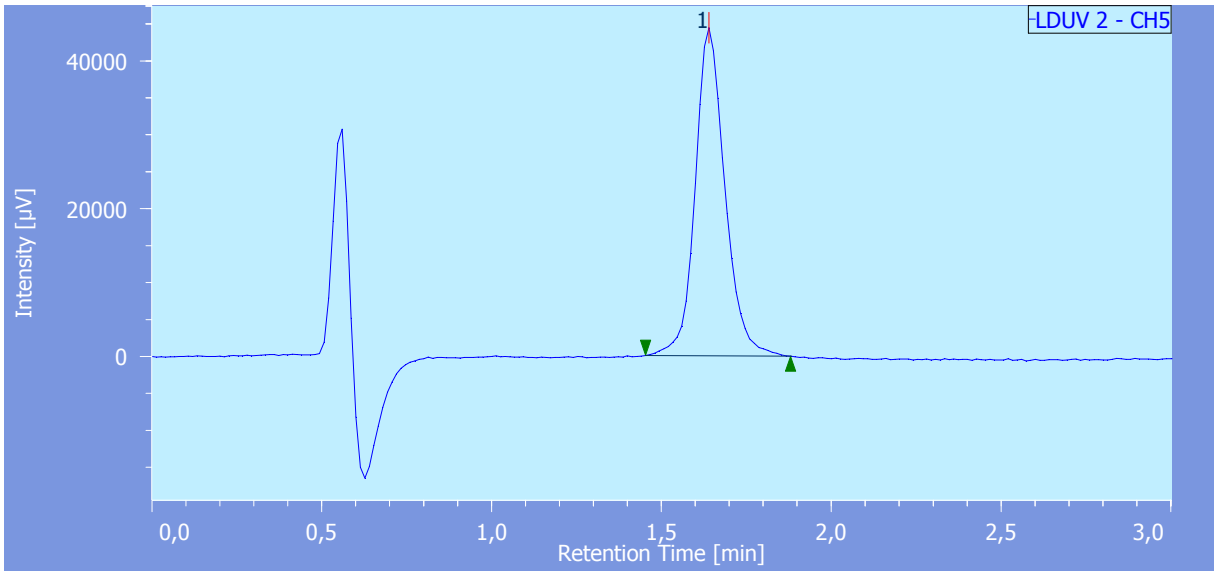


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:54:44
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:39:16
Volume	10,00 [µL]
Sample Number	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,640	270058	44317	100,000	100,000	N/A	1844	N/A	1,116	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

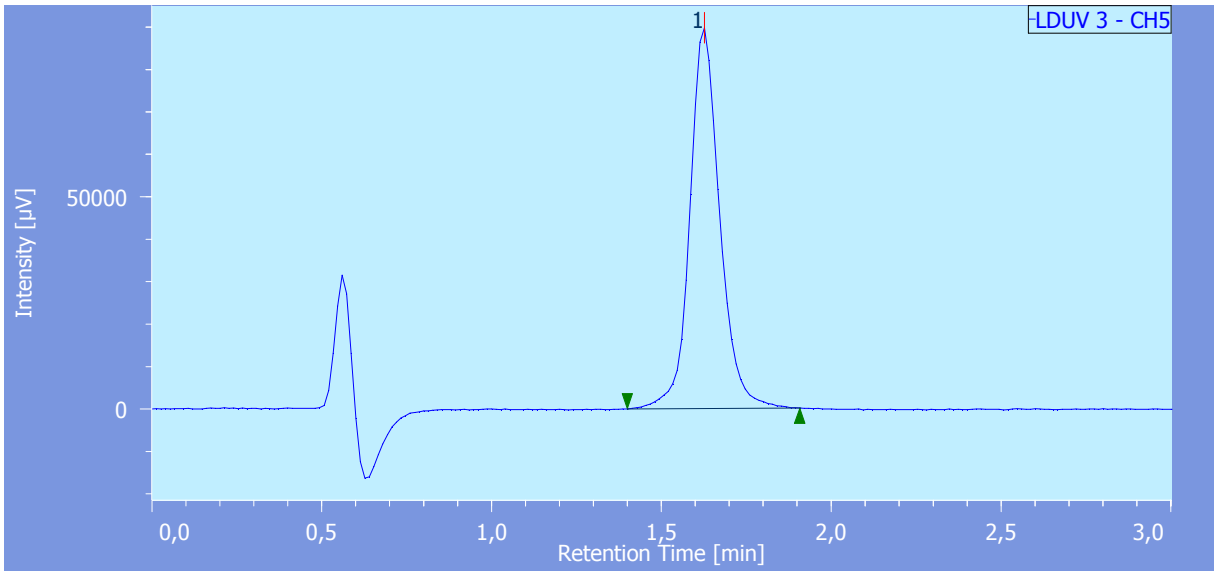


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:54:44
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:42:58
Volume	10,00 [µL]
Sample Number	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,627	550844	89642	100,000	100,000	N/A	1816	N/A	1,085	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

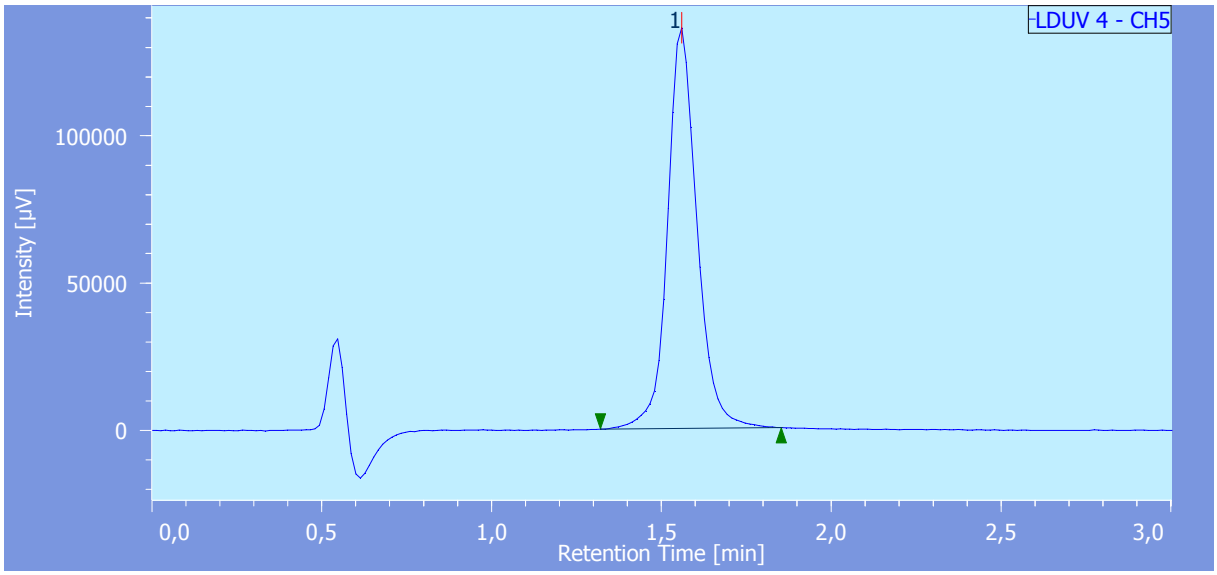


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:54:44
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:46:40
Volume	10,00 [µL]
Sample Number	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,560	822268	135901	100,000	100,000	N/A	1723	N/A	1,082	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

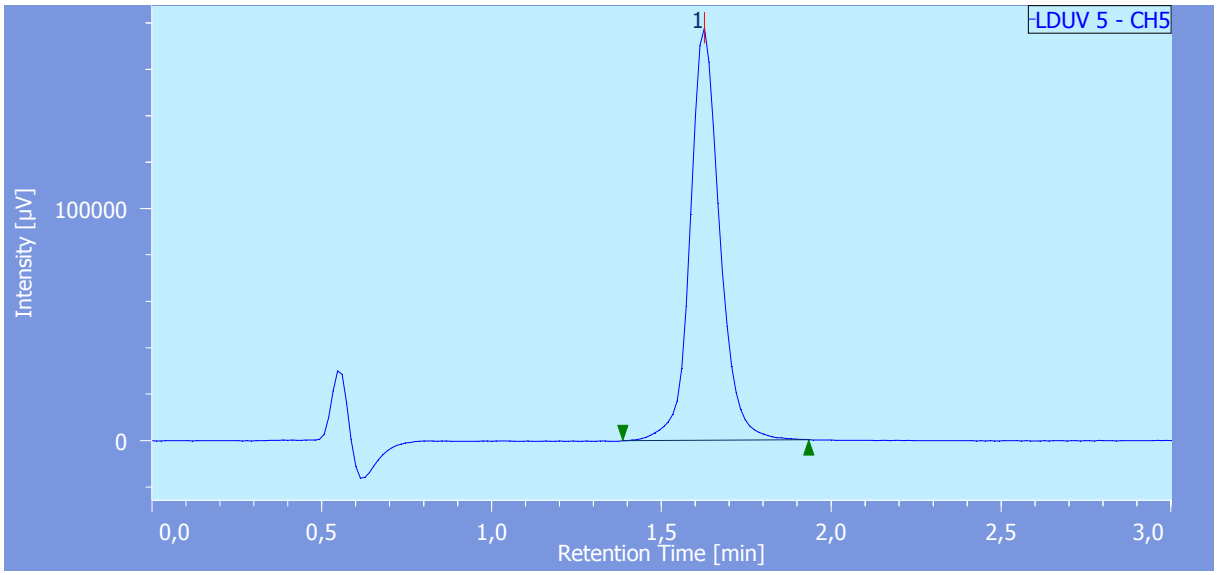


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 12:54:45
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:50:22
Volume	10,00 [µL]
Sample Number	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LDUV
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LDUV 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,627	1079802	177619	100,000	100,000	N/A	1852	N/A	1,080	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

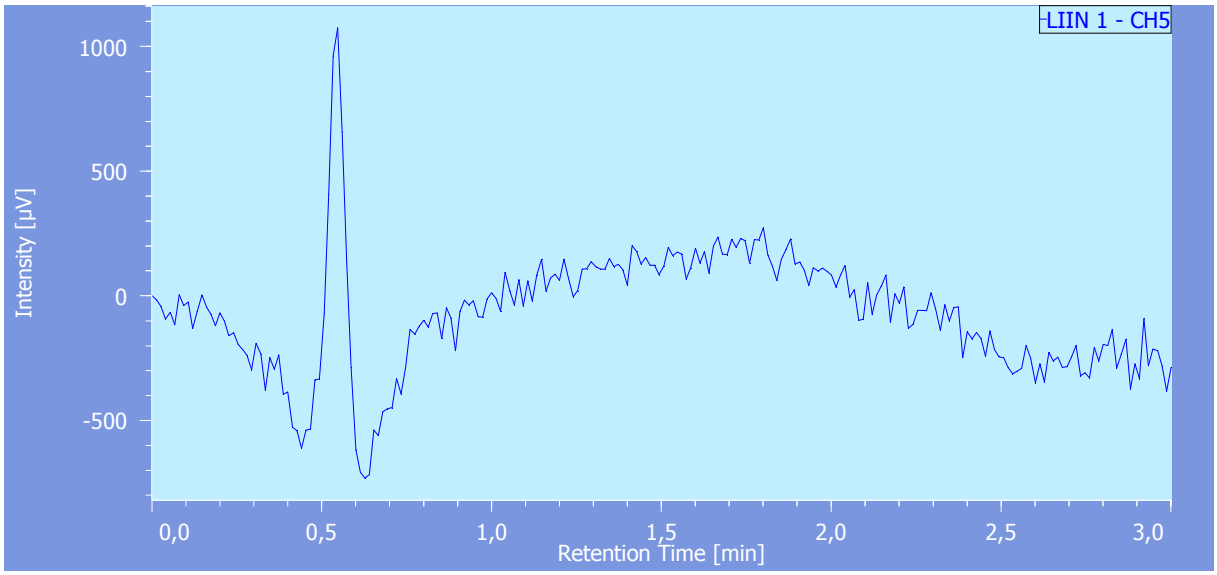


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 13:16:29
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:56:18
Volume	0,10 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 1-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

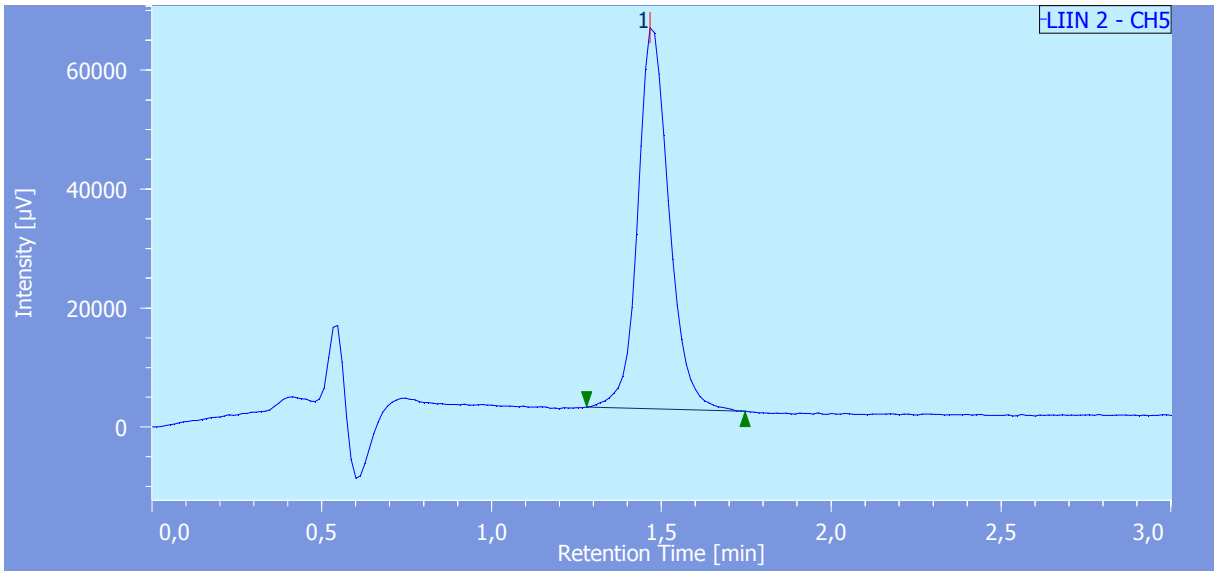


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 13:16:30
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 12:59:53
Volume	5,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 2-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,467	412204	63988	100,000	100,000	N/A	1318	N/A	1,206	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

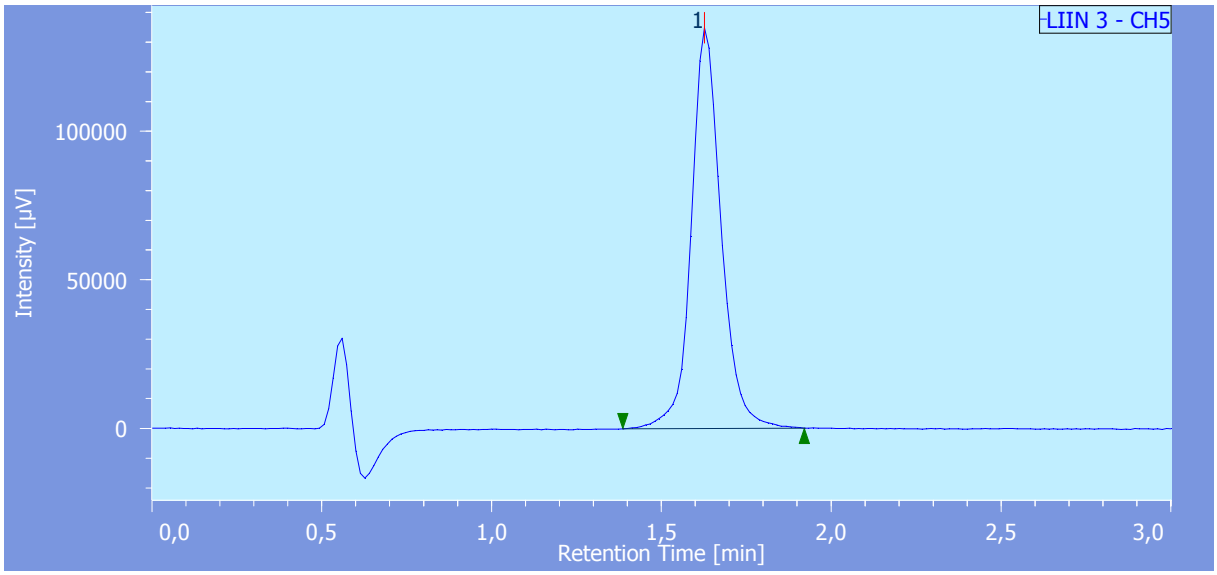


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 13:16:30
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 13:03:33
Volume	10,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 3-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,627	824361	134742	100,000	100,000	N/A	1854	N/A	1,114	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

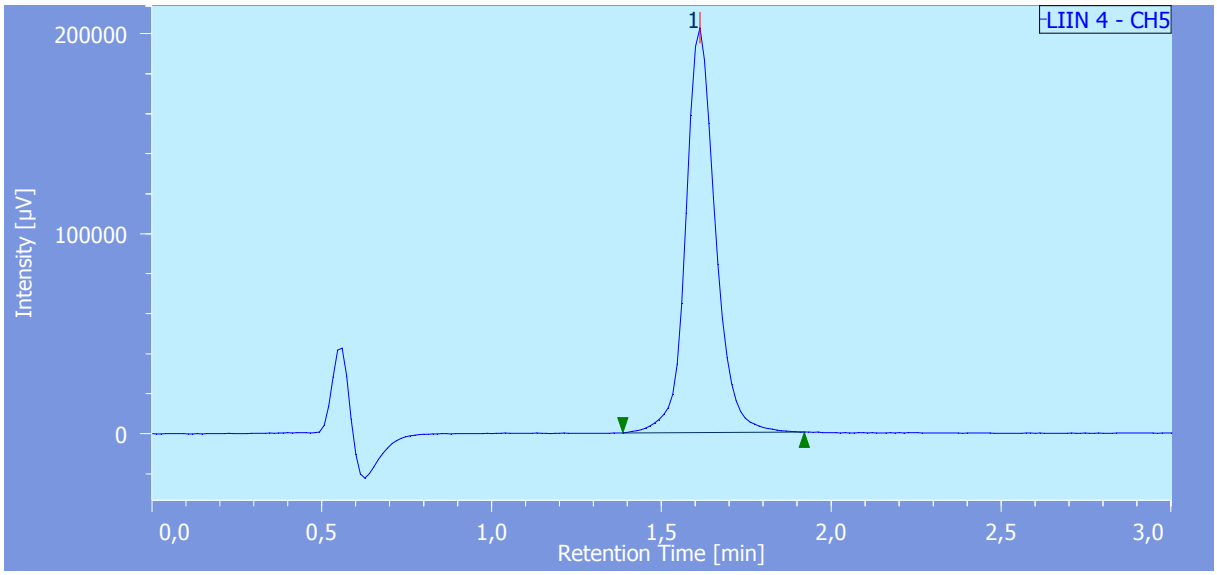


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 13:16:31
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 13:07:20
Volume	15,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 4-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,613	1231900	202192	100,000	100,000	N/A	1816	N/A	1,091	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

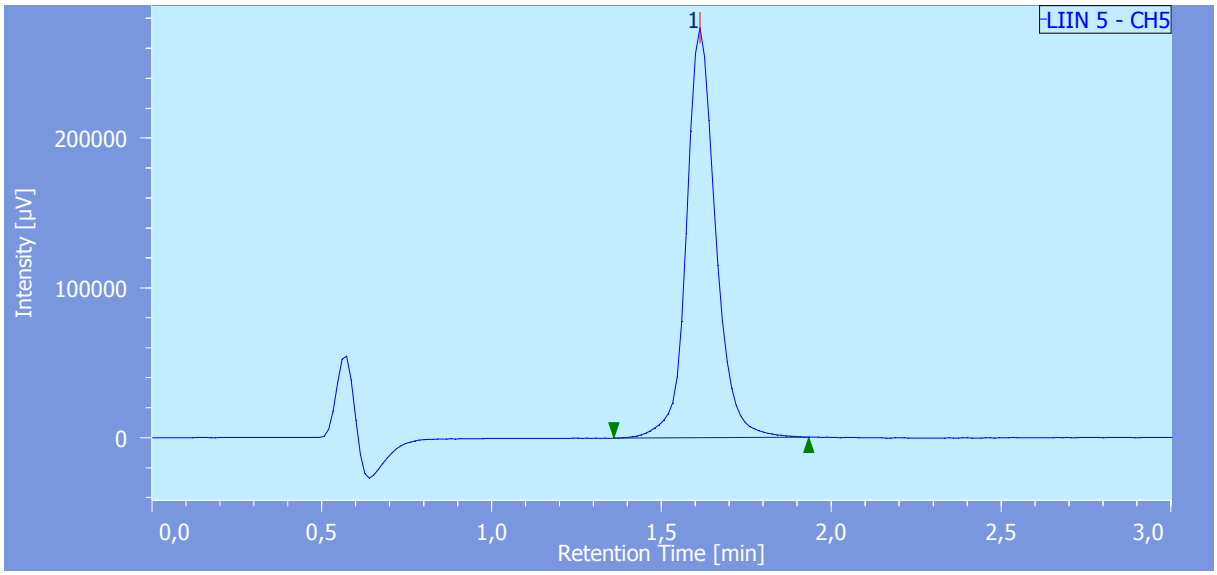


Chromatogram Information	
User Name	Administrator
Date Modified	12/12/2016 13:16:31
Description	
HPLC System Name	01-HP-01
Injection Date	12/12/2016 13:11:11
Volume	20,00 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	LIIN
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	LIIN 5-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Qualificação
Formula	
Decision	

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	5	1,613	1640685	273349	100,000	100,000	N/A	1901	N/A	1,109	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

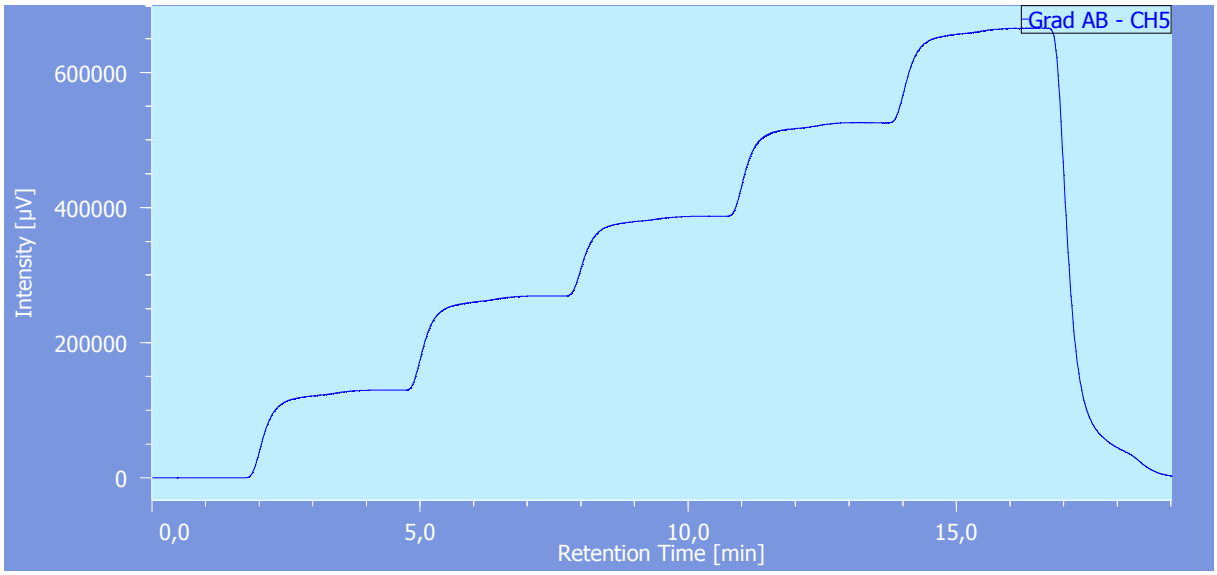


Chromatogram Information	
User Name	Administrator
Date Modified	13/12/2016 11:09:28
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2016 10:48:03
Volume	0,10 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	GRAD AB
Control Method	Grad AB
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Grad AB-CH5
Sample Name	
Channel Name	265,0nm
Sampling Interval	800 [msec]
Peak Method	Gradiente
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	

Chromatogram

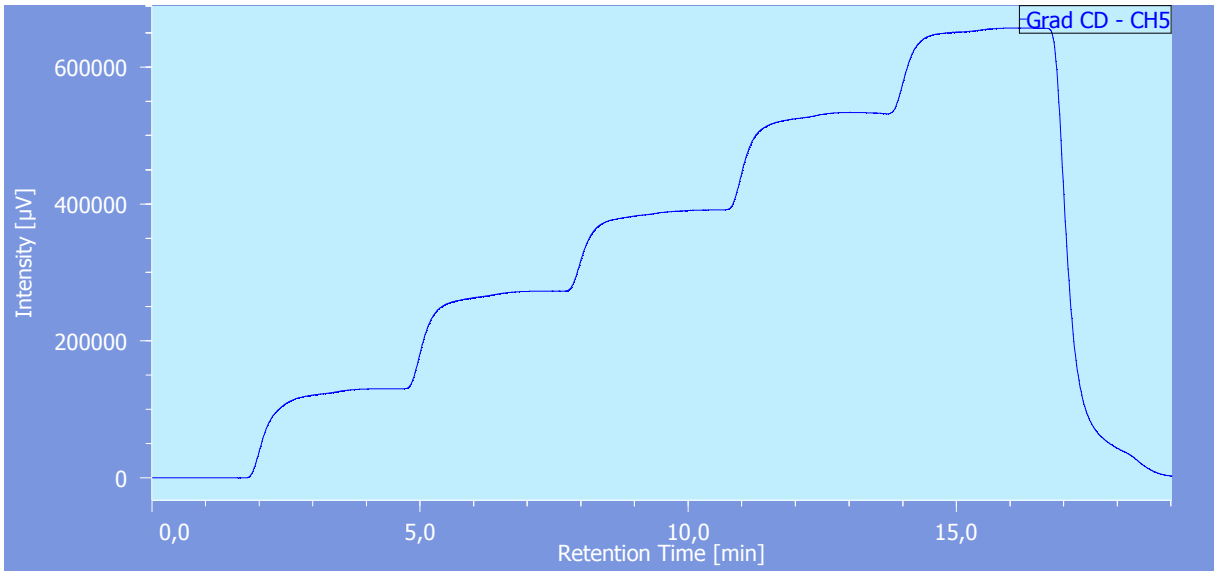

Chromatogram Information	
User Name	Administrator
Date Modified	13/12/2016 11:30:08
Description	
HPLC System Name	01-HP-01
Injection Date	13/12/2016 11:10:19
Volume	0,10 [µL]
Sample Number	1
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	GRAD CD
Control Method	Grad CD
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table	
Chromatogram Name	Grad CD-CH5
Sample Name	
Channel Name	265,0nm
Sampling Interval	800 [msec]
Peak Method	Gradiente
Formula	
Decision	

Creator	Administrator
Reviewer	
Approver	