
Peak Find - EDUV UV_tR1,28 D.jws

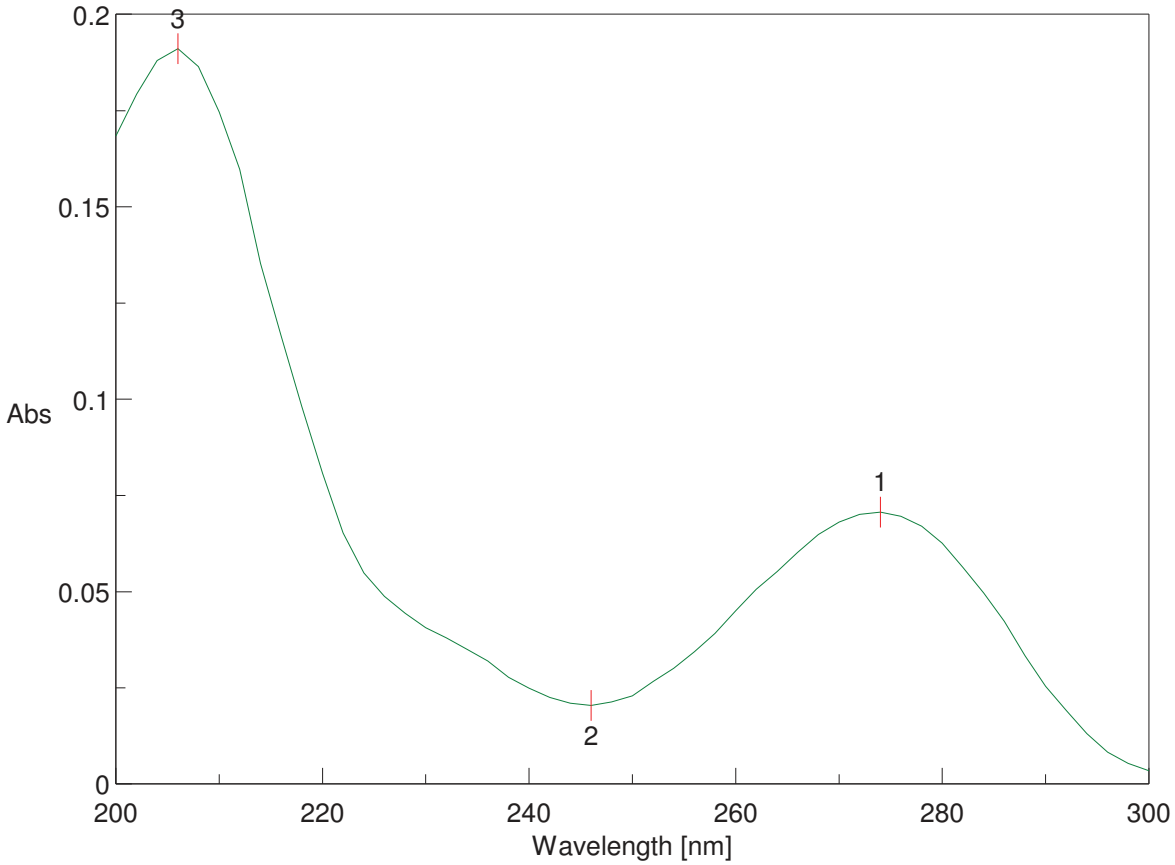

[Comments]

User	Administrator
Division	---
Company	HP Inc.
Creation date	22/08/2022 16:10

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	UV-2075
Model Name	UV-2075
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.070632	2	246	0.02036
3	206	0.190978			

Chromatogram

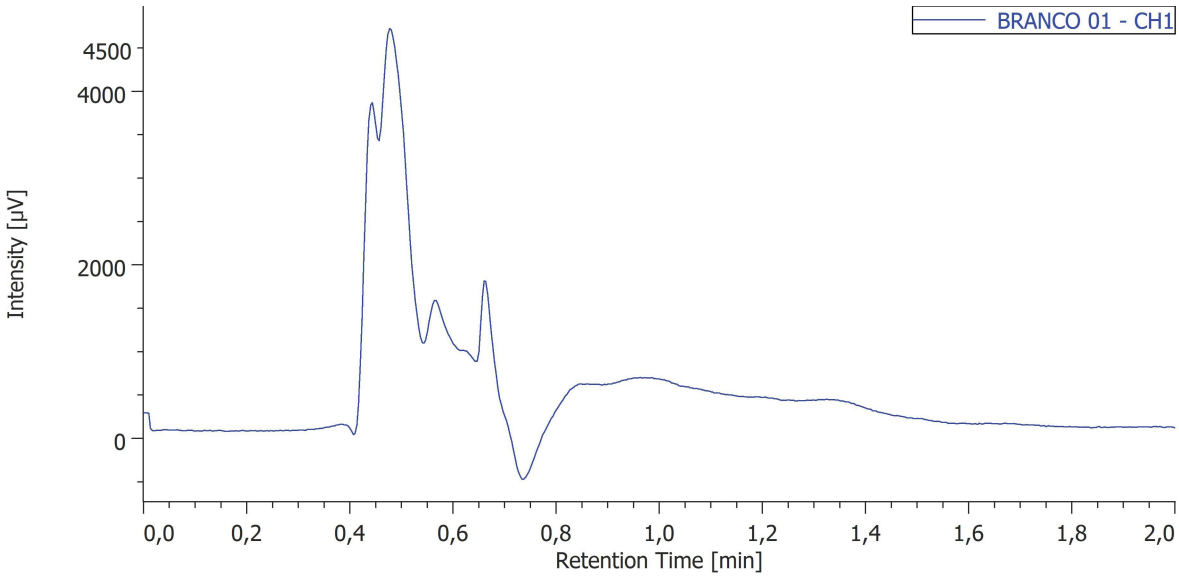


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:07:43
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:05:41
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

Chromatogram

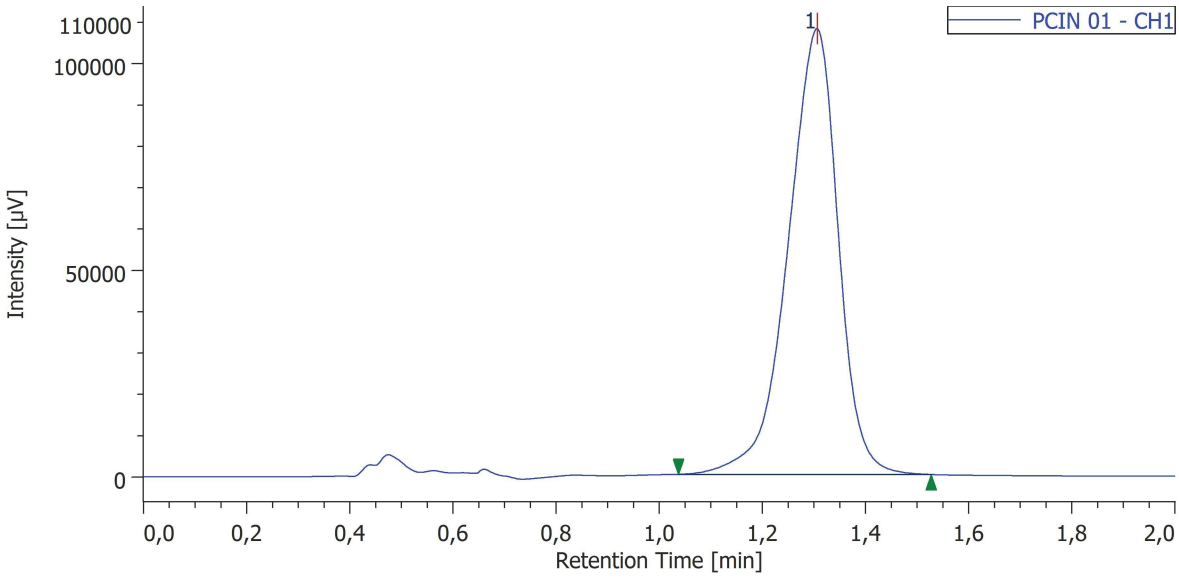


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:12:23
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:10:21
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	758079	107787	100,000	100,000	N/A	917	N/A	0,858	

Chromatogram

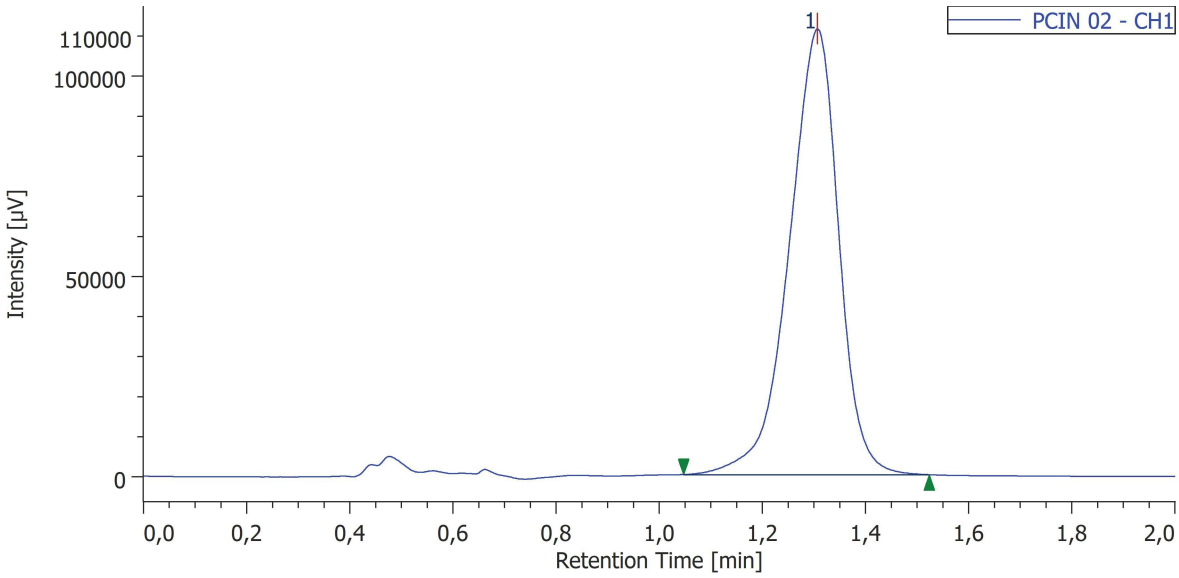


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:17:02
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:15:00
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	741316	111231	100,000	100,000	N/A	946	N/A	0,873	

Chromatogram

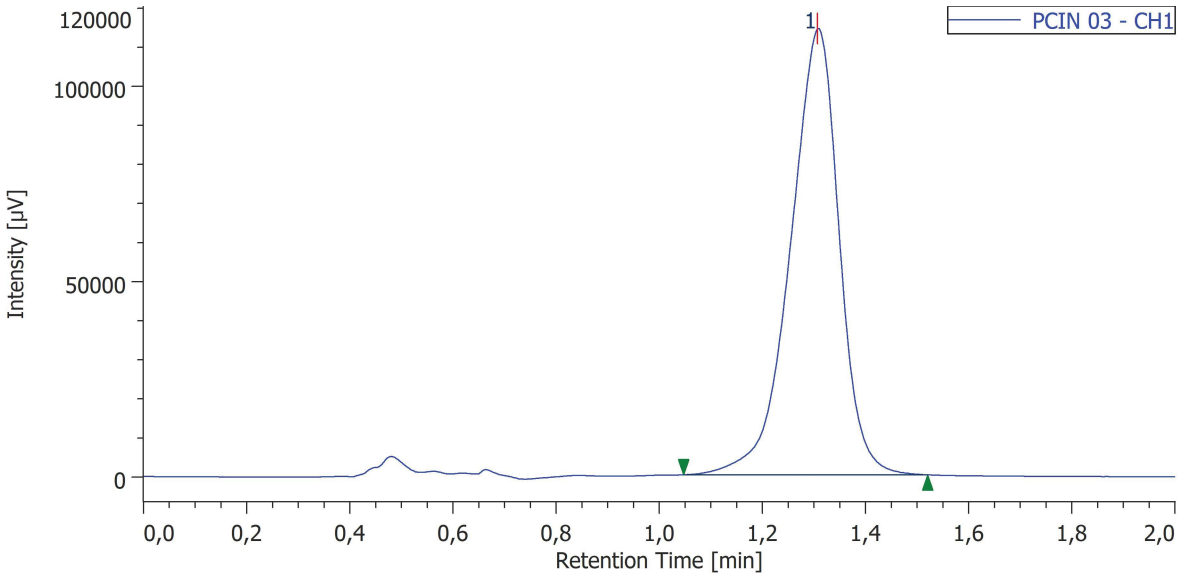


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:21:42
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:19:41
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	751044	114140	100,000	100,000	N/A	977	N/A	0,882	

Chromatogram

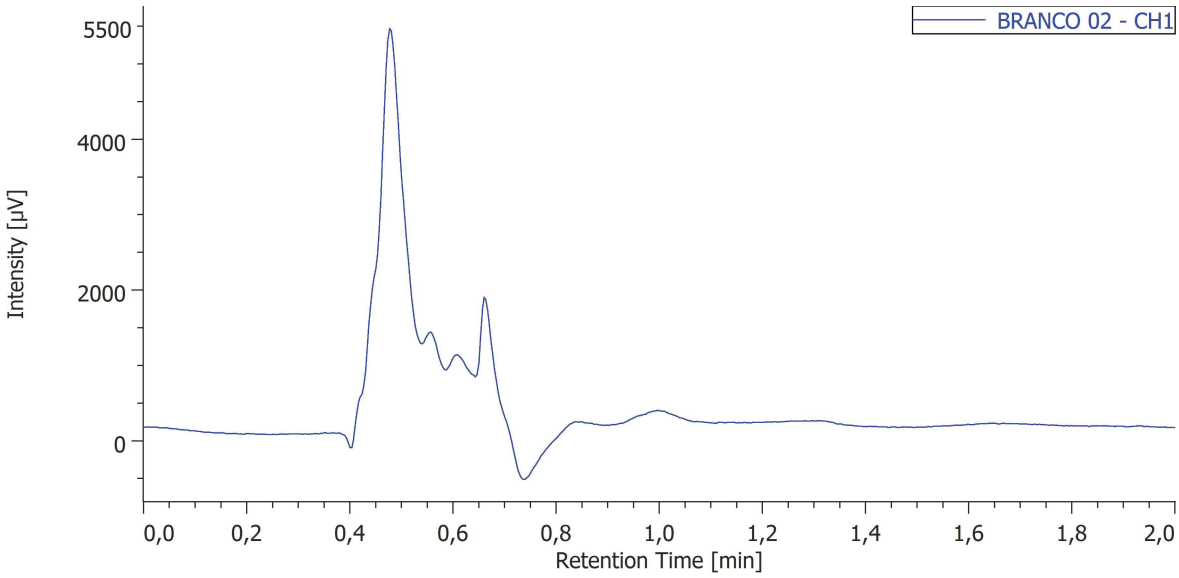


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:26:22
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:24:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

Chromatogram

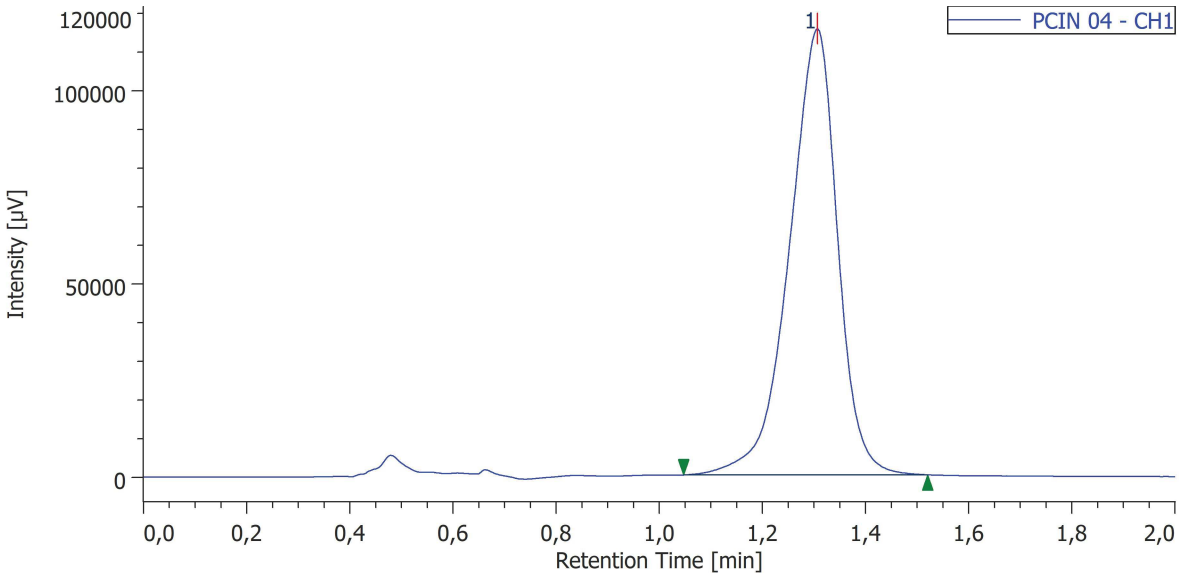


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:31:02
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:29:10
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	748841	115335	100,000	100,000	N/A	1011	N/A	0,866	

Chromatogram

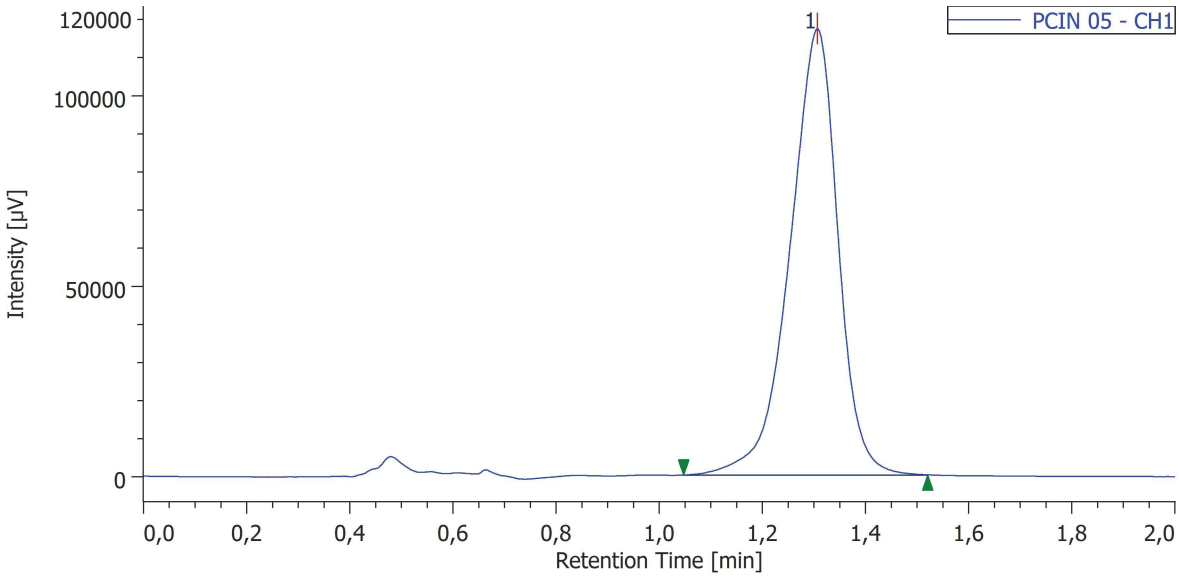


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:35:40
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:33:38
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	758241	117054	100,000	100,000	N/A	1017	N/A	0,872	

Chromatogram

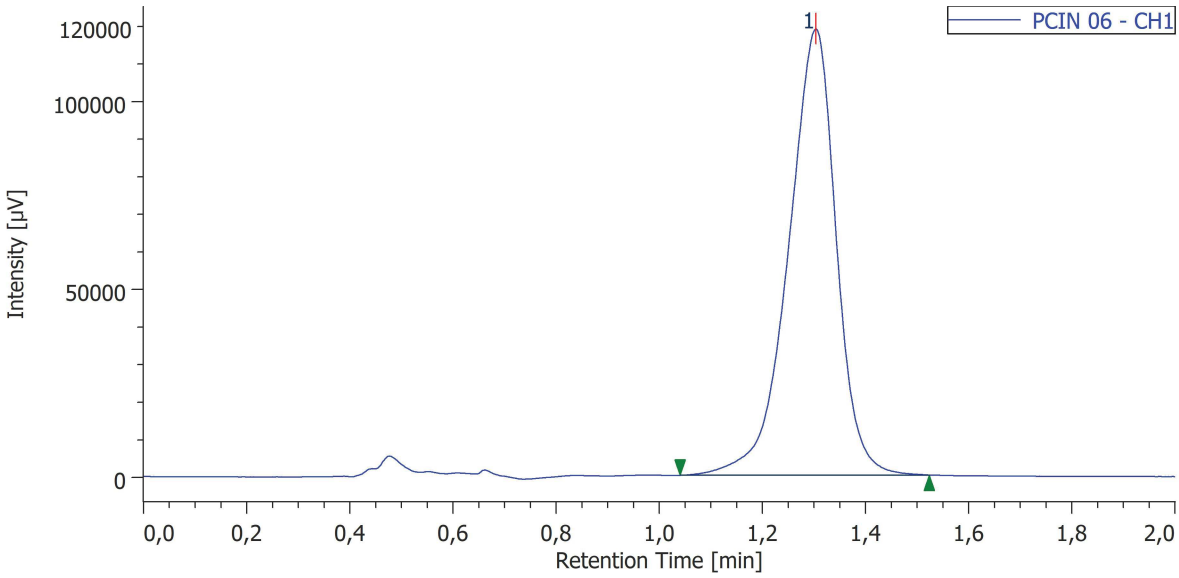


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:40:20
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:38:19
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,303	754280	118747	100,000	100,000	N/A	1031	N/A	0,875	

Chromatogram

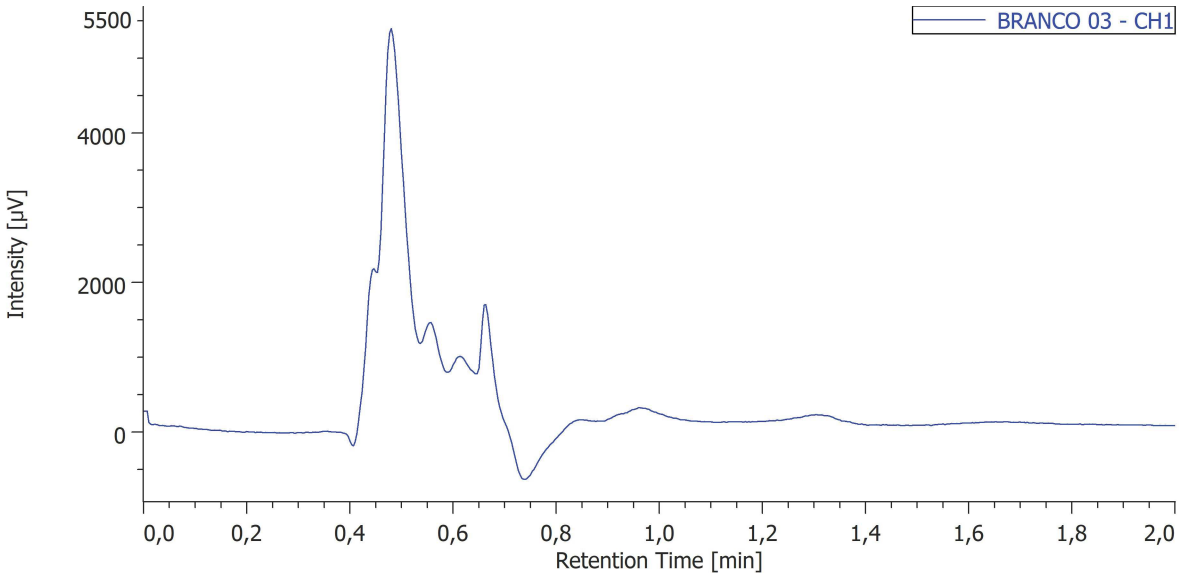


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:44:58
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:42:57
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	BRANCO 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

Chromatogram

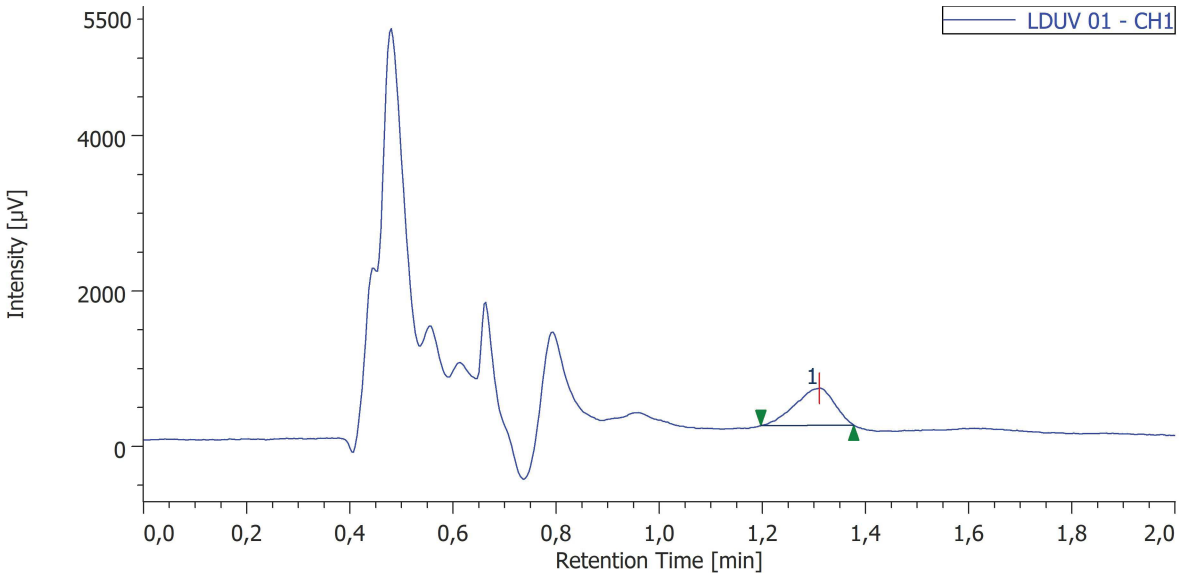


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:49:38
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:47:37
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,310	2523	477	100,000	100,000	N/A	1293	N/A	0,806	

Chromatogram

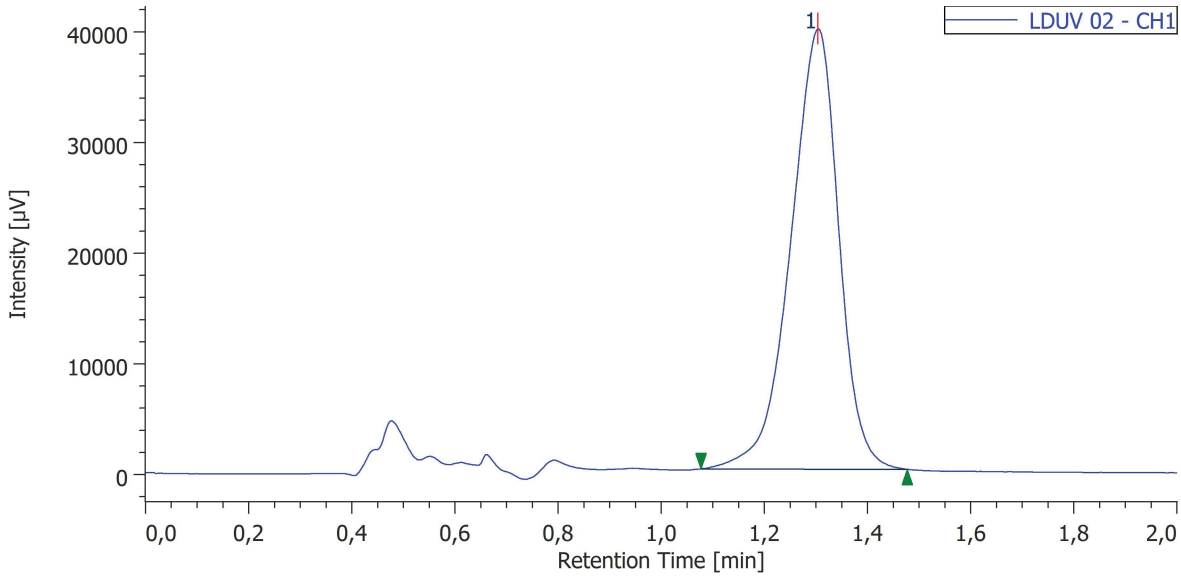


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:54:18
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:52:17
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,303	257135	39775	100,000	100,000	N/A	990	N/A	0,887	

Chromatogram

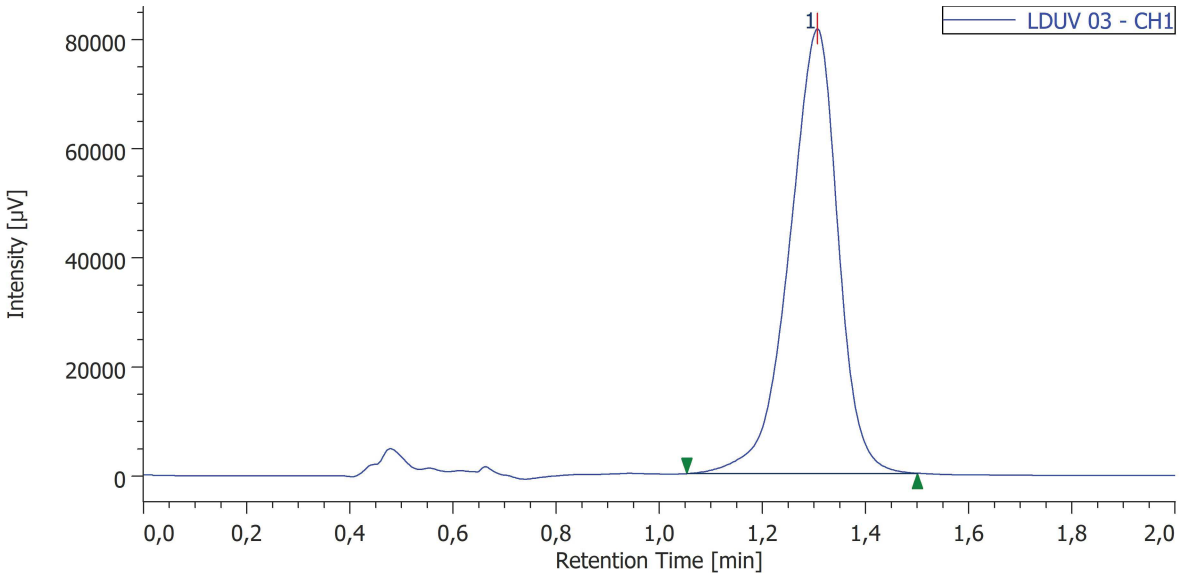


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 10:58:58
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 10:56:57
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	533811	81474	100,000	100,000	N/A	981	N/A	0,873	

Chromatogram

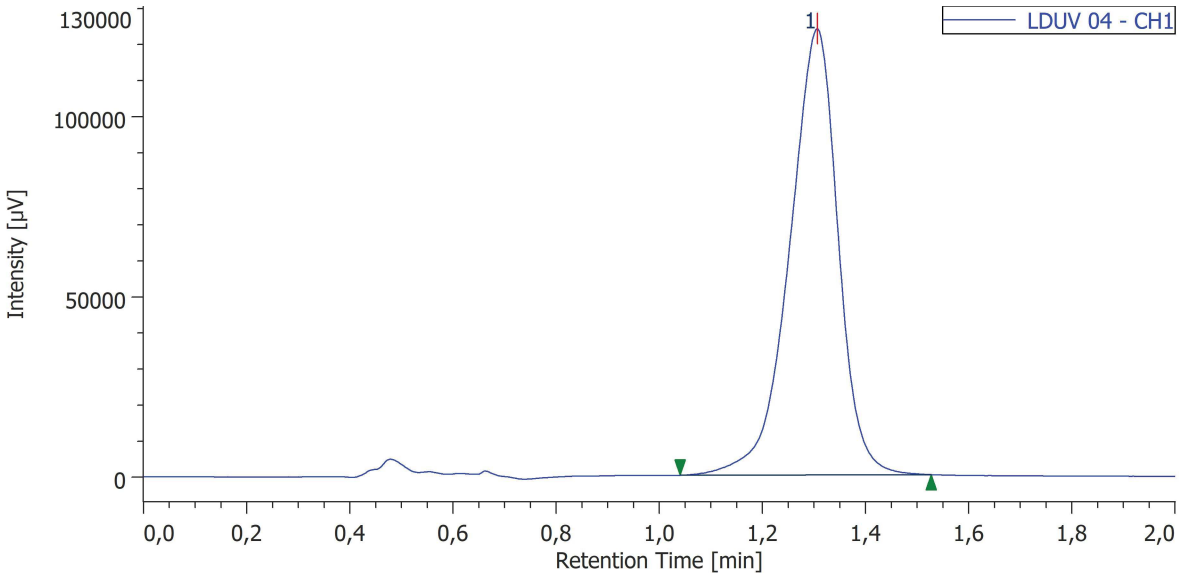


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 11:03:42
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 11:01:39
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	809749	123722	100,000	100,000	N/A	993	N/A	0,875	

Chromatogram

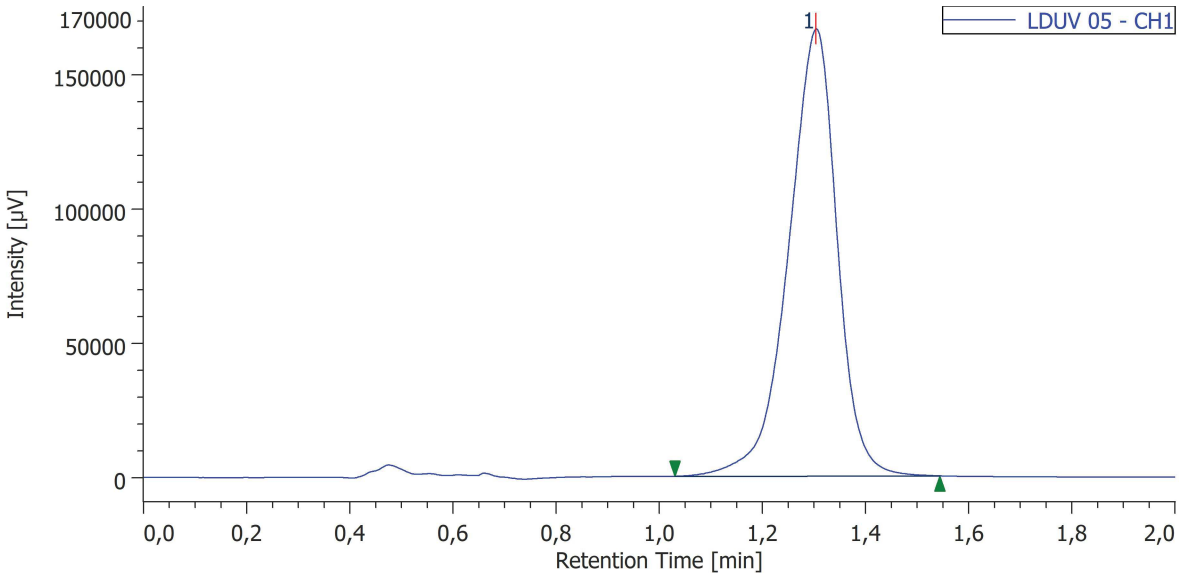


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 11:08:24
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 11:06:22
Volume	10,0 [µL]
Sample #	7
Project Name	Qualificação HPLC 1
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022_1
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,303	1089702	166471	100,000	100,000	N/A	993	N/A	0,885	

Chromatogram

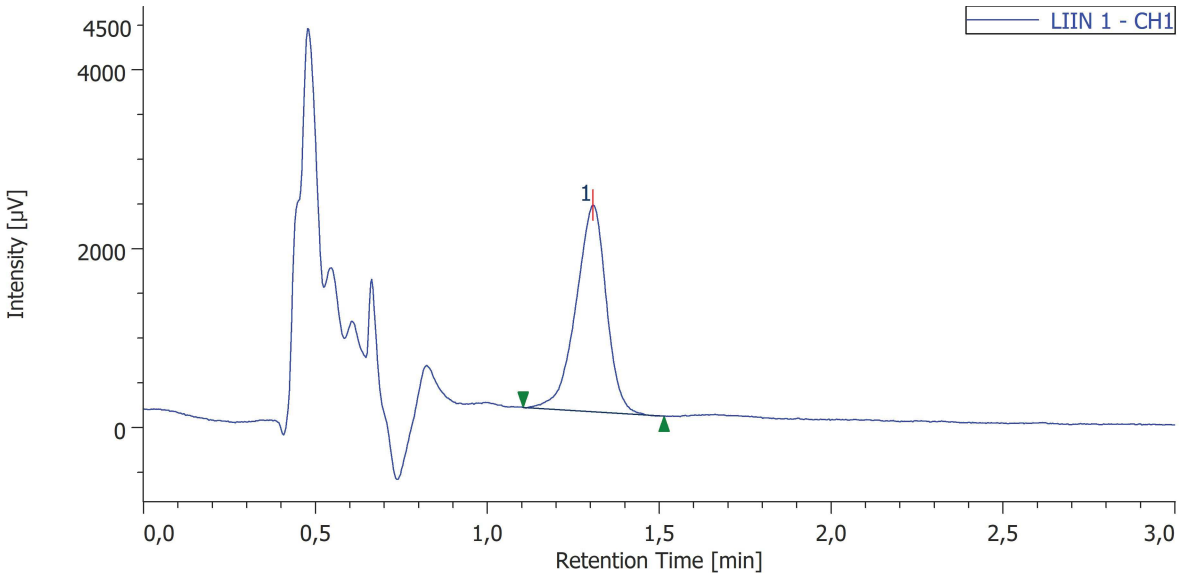


Chromatogram Information	
User Name	Administrator
Date Modified	22/08/2022 19:00:35
Description	
HPLC System Name	HPLC 0001
Injection Date	22/08/2022 18:57:33
Volume	0,1 [µL]
Sample #	8
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	14180	2310	100,000	100,000	N/A	1101	N/A	0,887	

Chromatogram

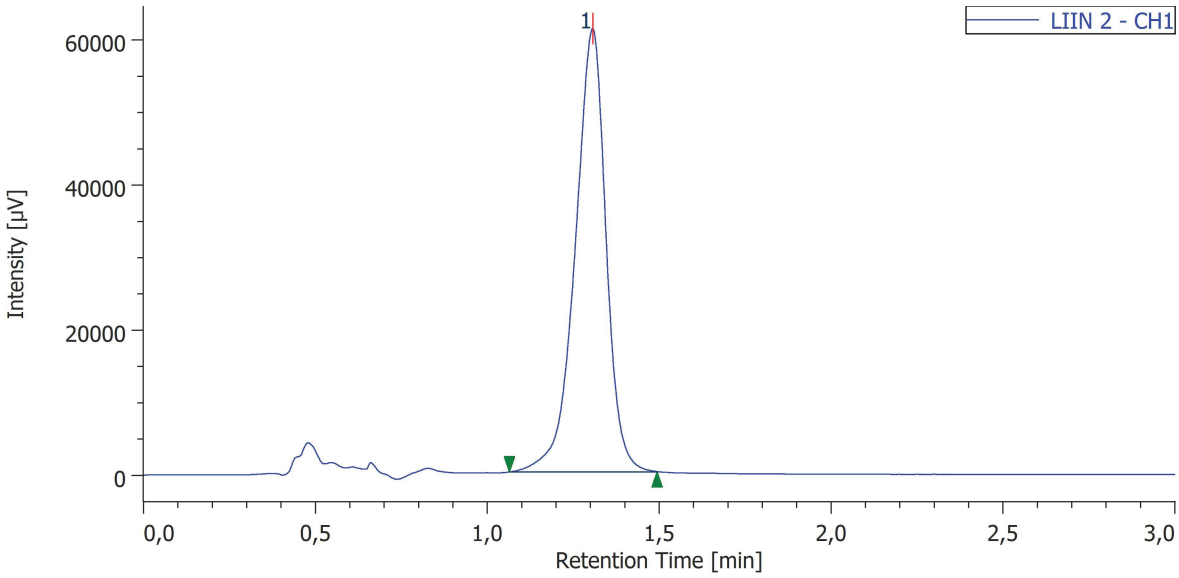


Chromatogram Information	
User Name	Administrator
Date Modified	22/08/2022 19:05:13
Description	
HPLC System Name	HPLC 0001
Injection Date	22/08/2022 19:02:11
Volume	5,0 [µL]
Sample #	8
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 2-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	380989	61048	100,000	100,000	N/A	1105	N/A	0,879	

Chromatogram

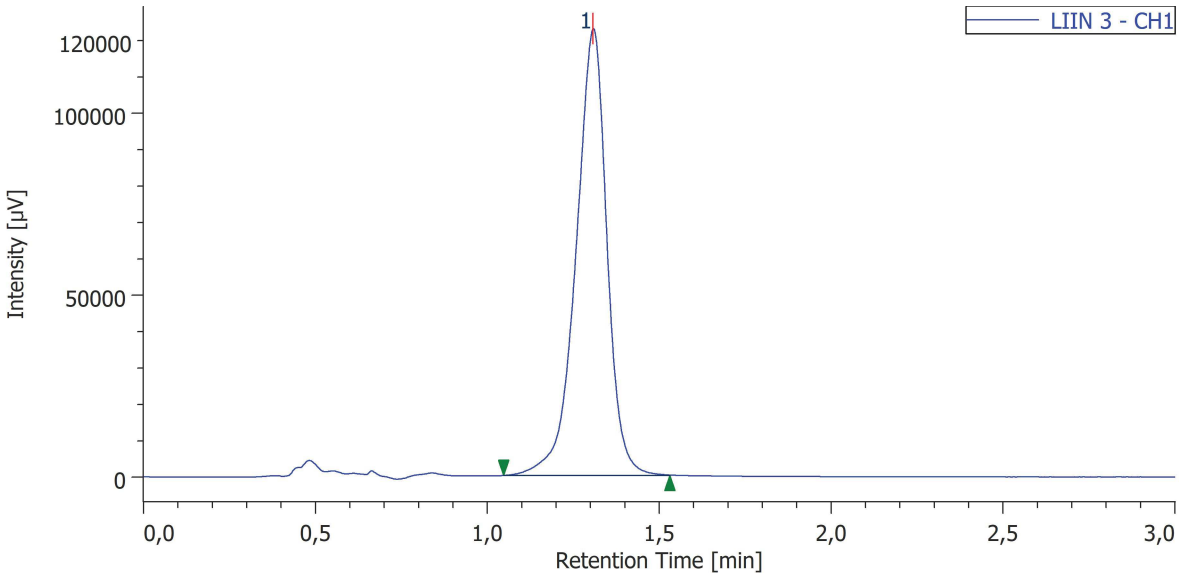


Chromatogram Information	
User Name	Administrator
Date Modified	22/08/2022 19:09:55
Description	
HPLC System Name	HPLC 0001
Injection Date	22/08/2022 19:06:54
Volume	10,0 [µL]
Sample #	8
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 3-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	766398	122660	100,000	100,000	N/A	1113	N/A	0,898	

Chromatogram

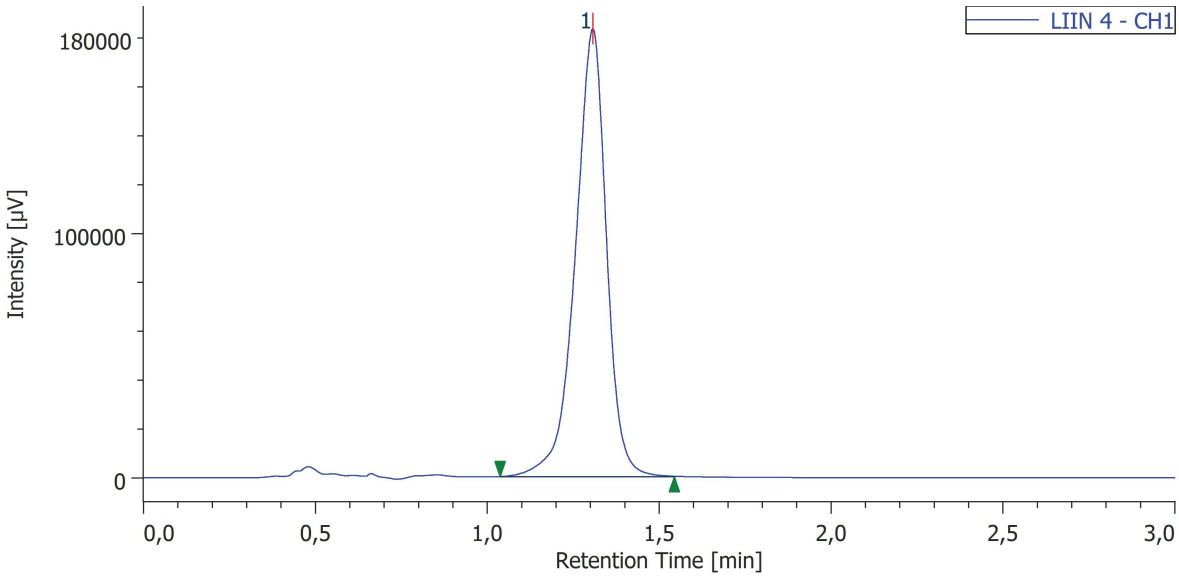


Chromatogram Information	
User Name	Administrator
Date Modified	22/08/2022 19:14:43
Description	
HPLC System Name	HPLC 0001
Injection Date	22/08/2022 19:11:41
Volume	15,0 [µL]
Sample #	8
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 4-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	1150999	183163	100,000	100,000	N/A	1098	N/A	0,888	

Chromatogram

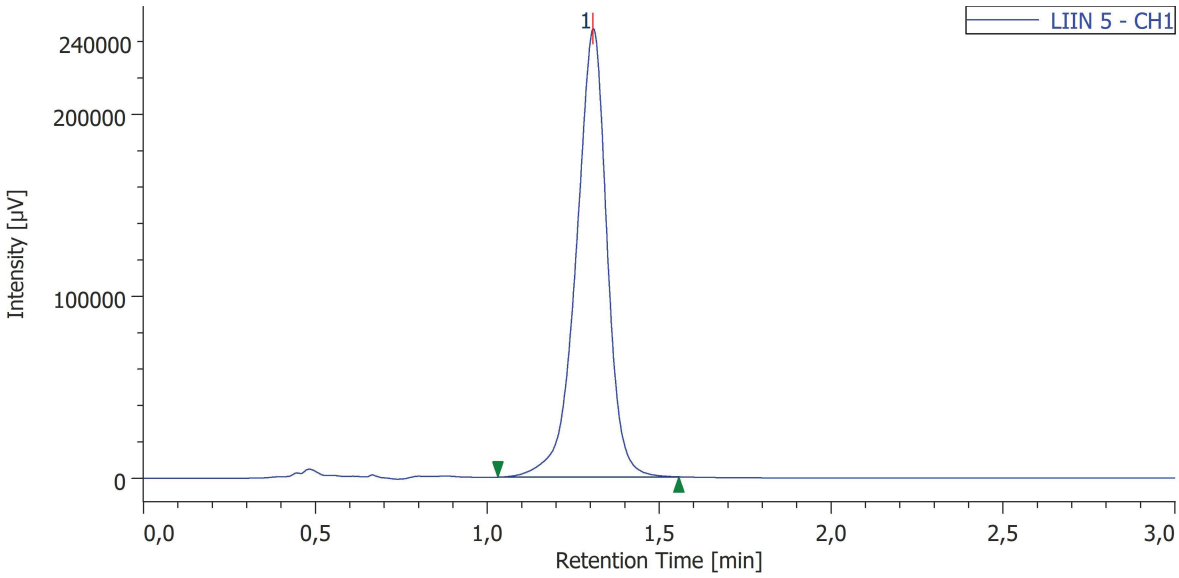


Chromatogram Information	
User Name	Administrator
Date Modified	22/08/2022 19:19:37
Description	
HPLC System Name	HPLC 0001
Injection Date	22/08/2022 19:16:35
Volume	20,0 [µL]
Sample #	8
Project Name	Qualificação HPLC 1
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HPLC 1_2022
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 5-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Qualificação Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,307	1535202	246292	100,000	100,000	N/A	1122	N/A	0,902	

Chromatogram

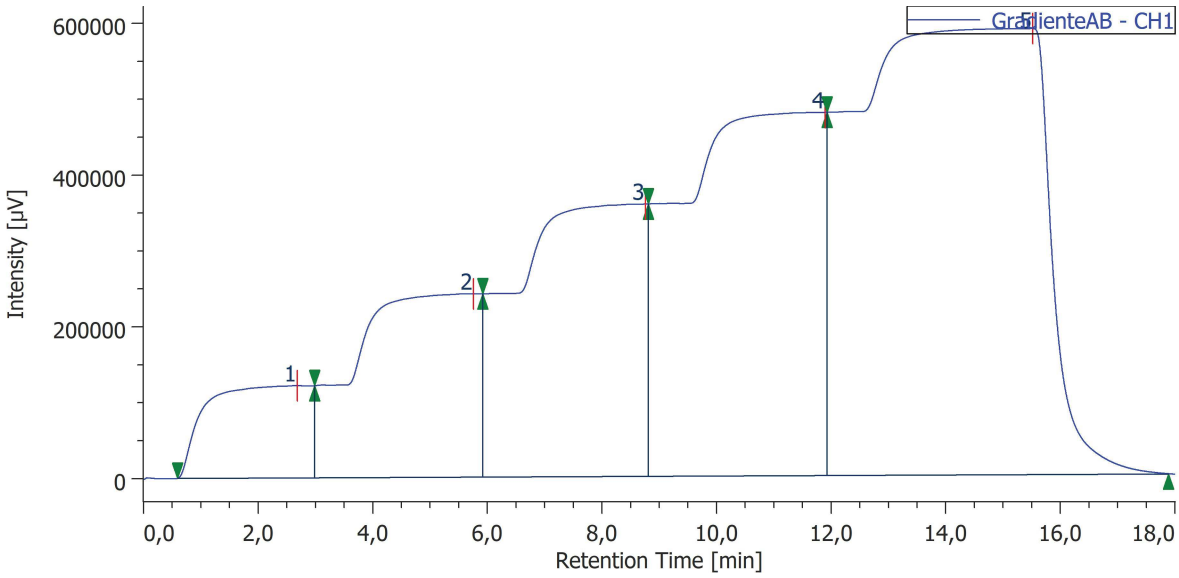


Chromatogram Information	
User Name	Administrator
Date Modified	23/08/2022 12:28:59
Description	
HPLC System Name	HPLC 0001
Injection Date	23/08/2022 12:10:57
Volume	0,1 [µL]
Sample #	1
Project Name	Qualificação HPLC 1
Acquisition Time	18,0 [min]
Acquisition Sequence	GRABO
Control Method	Teste de Gradiente AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GradienteAB-CH1
Sample Name	GradienteAB
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	2,680	14851183	121697	4,617	6,811	N/A	N/A	N/A	N/A	
2	Unknown	1	5,753	35707265	241266	11,101	13,503	N/A	N/A	N/A	N/A	
3	Unknown	1	8,757	55000215	358510	17,098	20,065	N/A	N/A	N/A	N/A	
4	Unknown	1	11,893	81520238	478103	25,343	26,758	N/A	N/A	N/A	N/A	
5	Unknown	1	15,513	134592886	587185	41,842	32,863	N/A	N/A	N/A	N/A	

Chromatogram

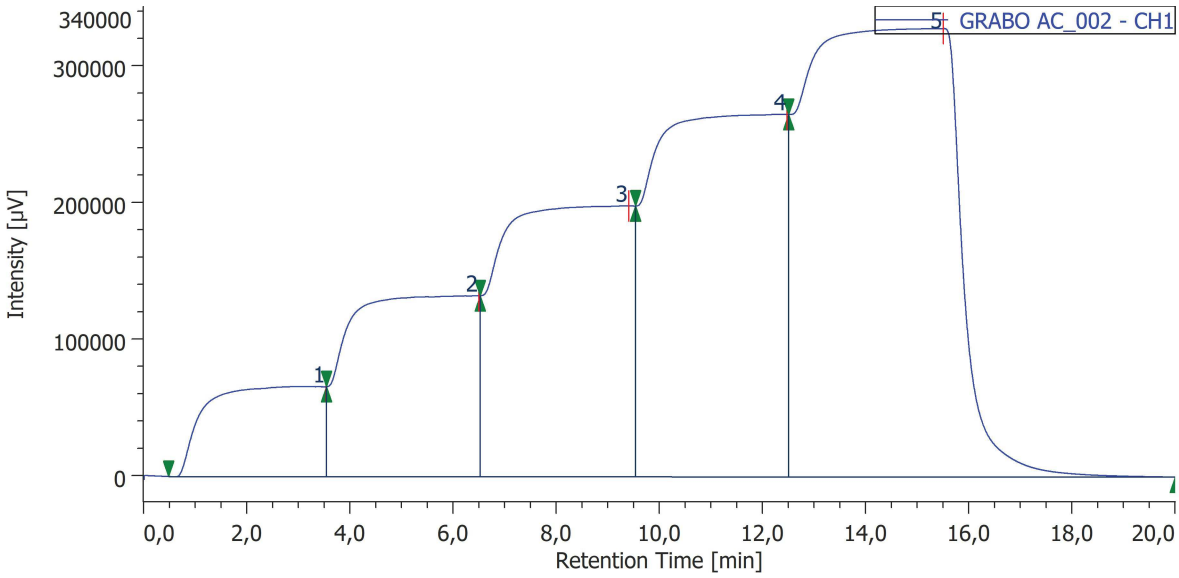

Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 11:39:32
Description	
HPLC System Name	HPLC 0001
Injection Date	25/08/2022 11:17:07
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 1
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Teste de Gradiente AC
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	GRABO AC_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3,540	9816514	65742	5,521	6,646	N/A	N/A	N/A	N/A	
2	40%	1	6,503	22006955	132389	12,378	13,383	N/A	N/A	N/A	N/A	
3	60%	1	9,407	34077385	198057	19,167	20,021	N/A	N/A	N/A	N/A	
4	80%	1	12,477	45398908	265129	25,535	26,801	N/A	N/A	N/A	N/A	
5	100%	1	15,503	66492356	327928	37,399	33,149	N/A	N/A	N/A	N/A	