
Chromatogram

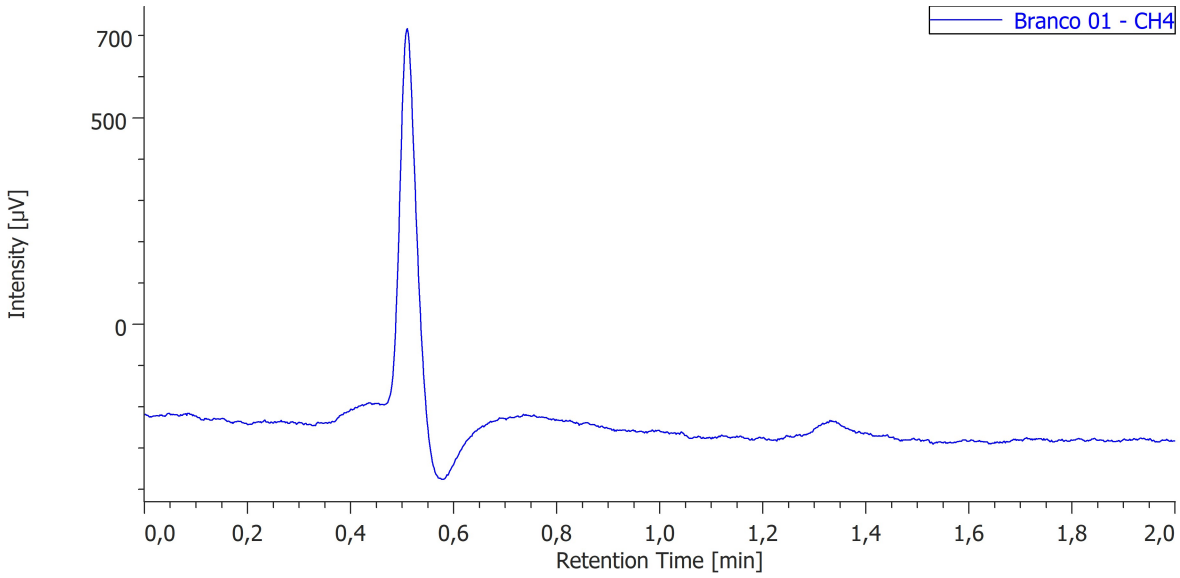


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:20:00
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:17:57
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

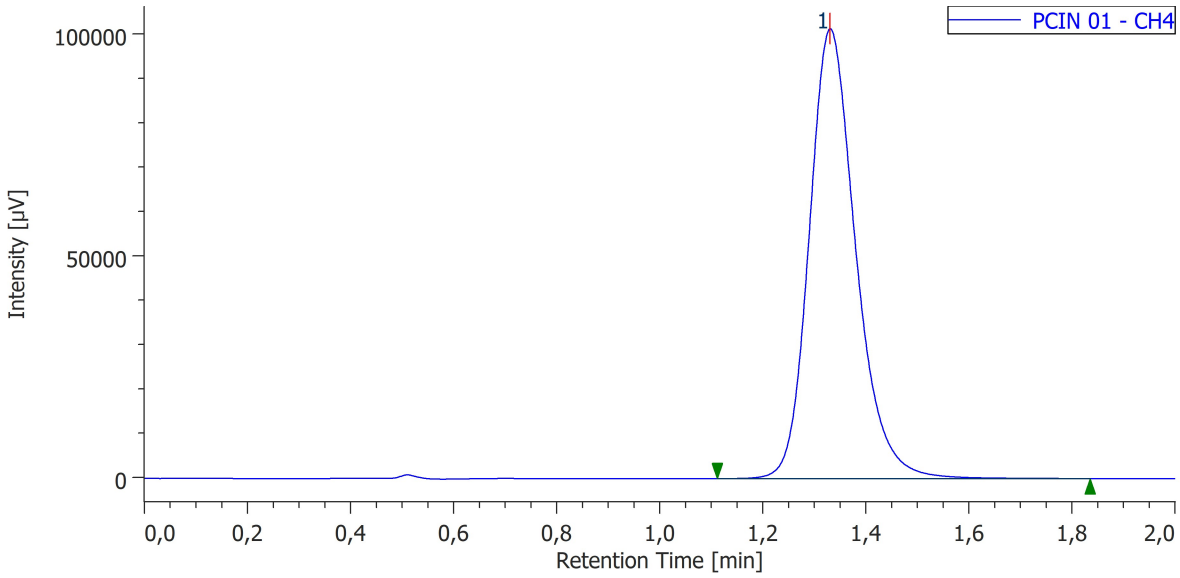


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:30:49
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:20:55
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,330	636465	101422	100,000	100,000	N/A	1110	N/A	1,226	

Chromatogram

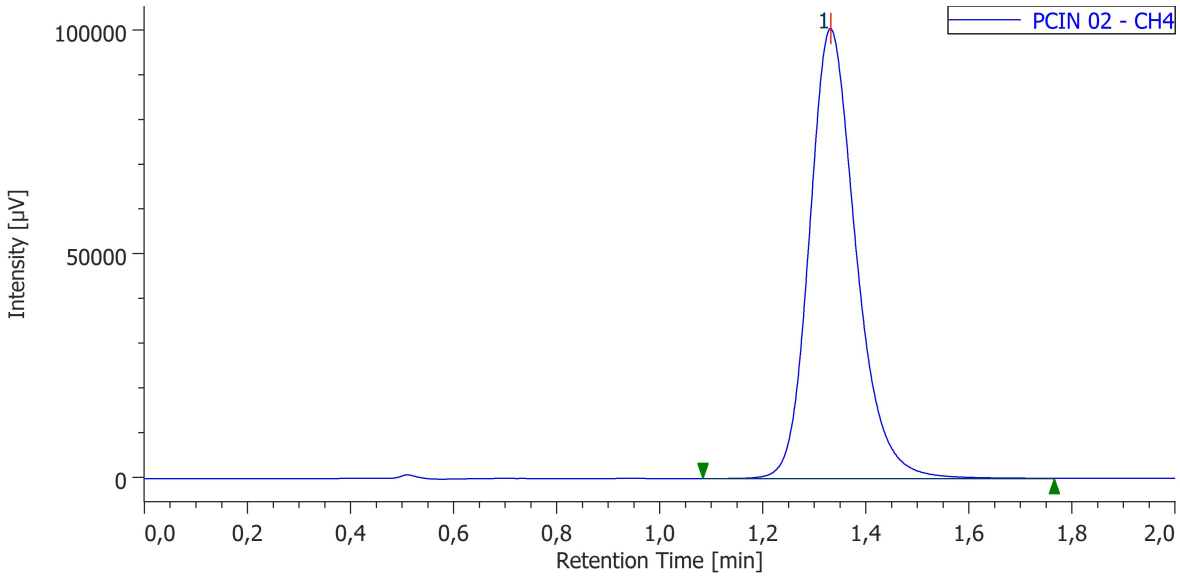


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:30:49
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:23:53
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,332	631073	100517	100,000	100,000	N/A	1109	N/A	1,209	

Chromatogram

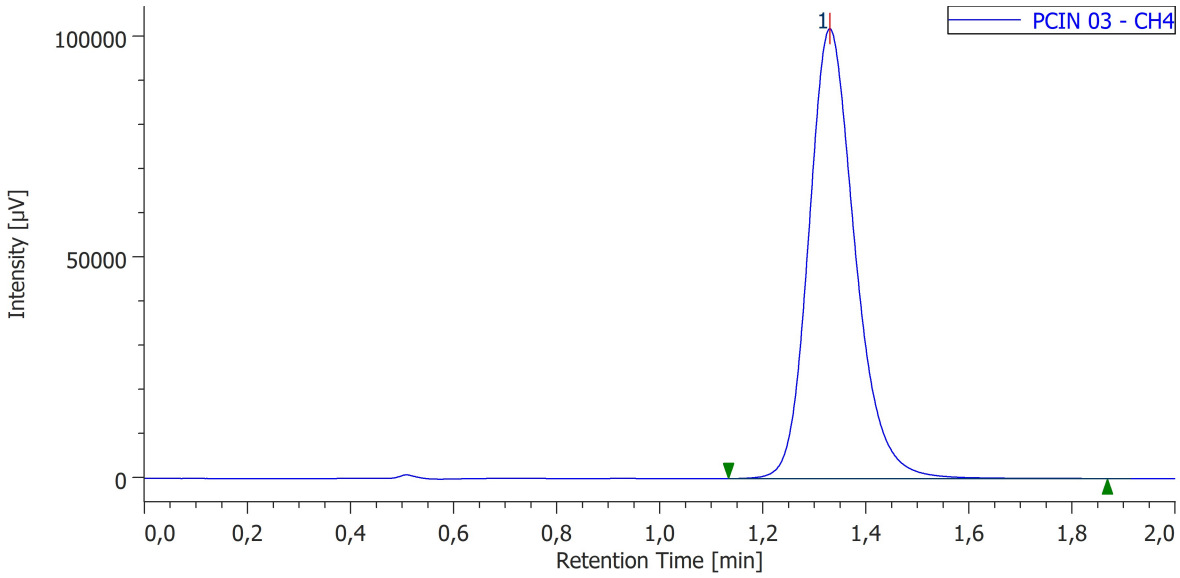


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:30:50
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:26:49
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,330	636714	101933	100,000	100,000	N/A	1115	N/A	1,206	

Chromatogram

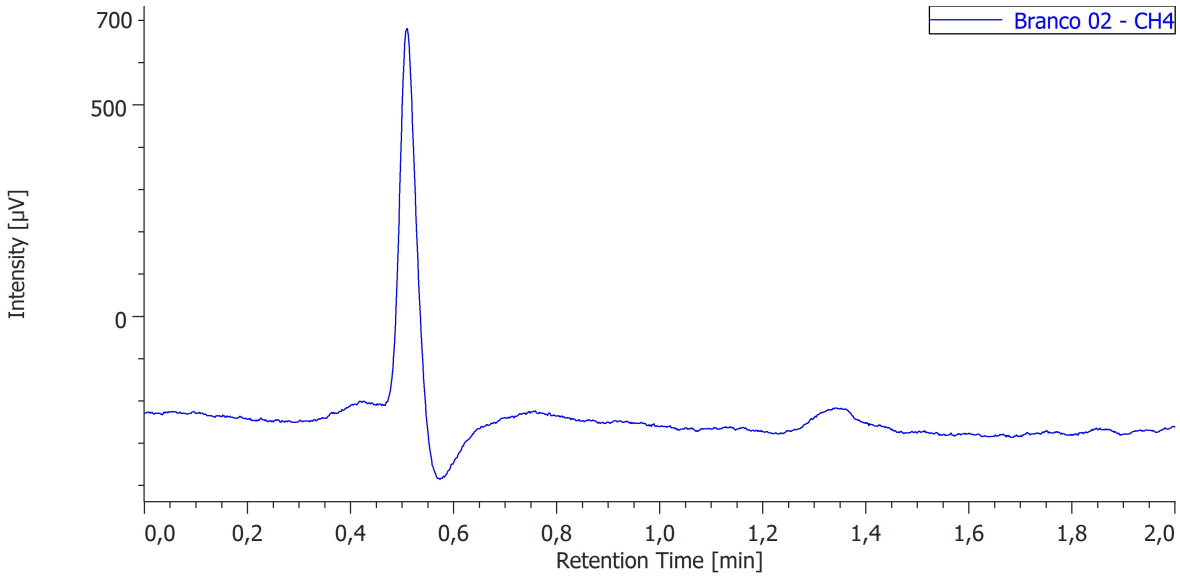


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:31:51
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:29:47
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

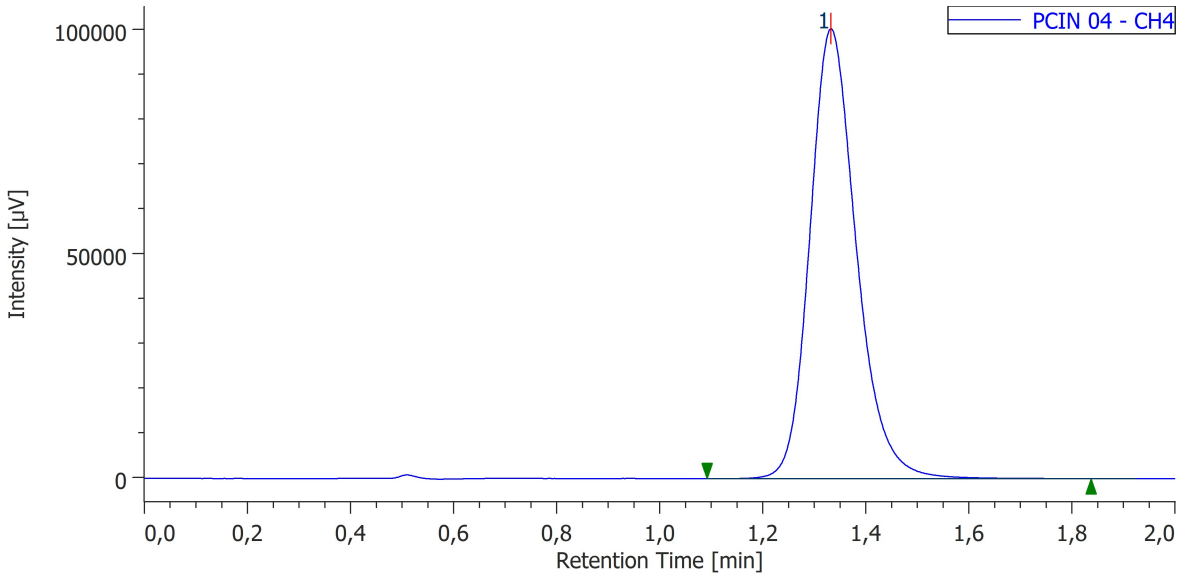


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:35:26
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:32:46
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,332	630870	100425	100,000	100,000	N/A	1107	N/A	1,216	

Chromatogram

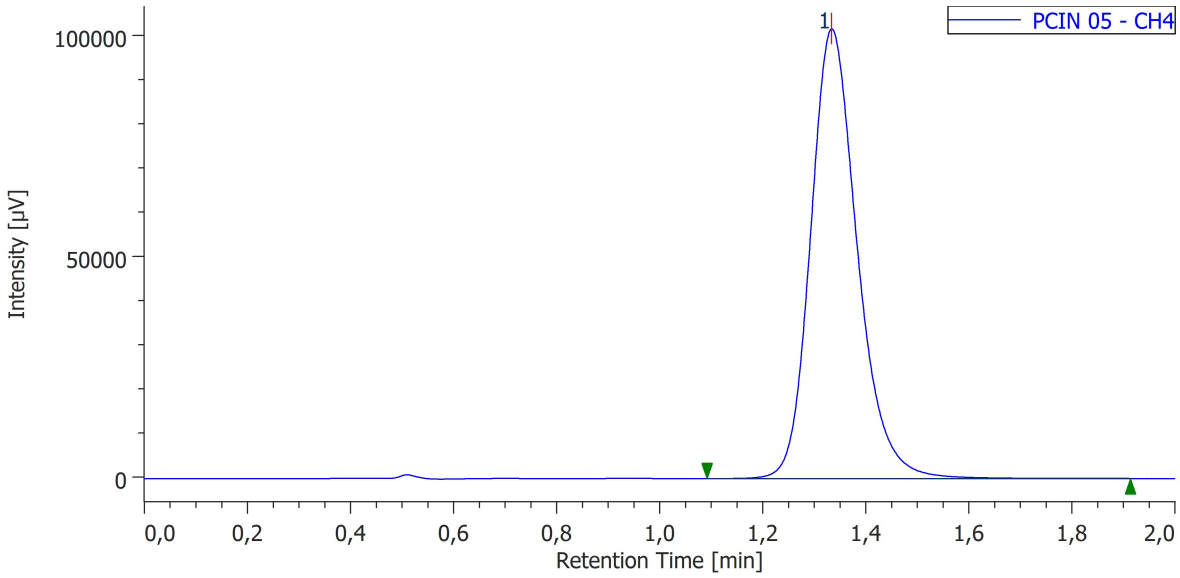


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:39:11
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:35:44
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,333	641529	101774	100,000	100,000	N/A	1103	N/A	1,216	

Chromatogram

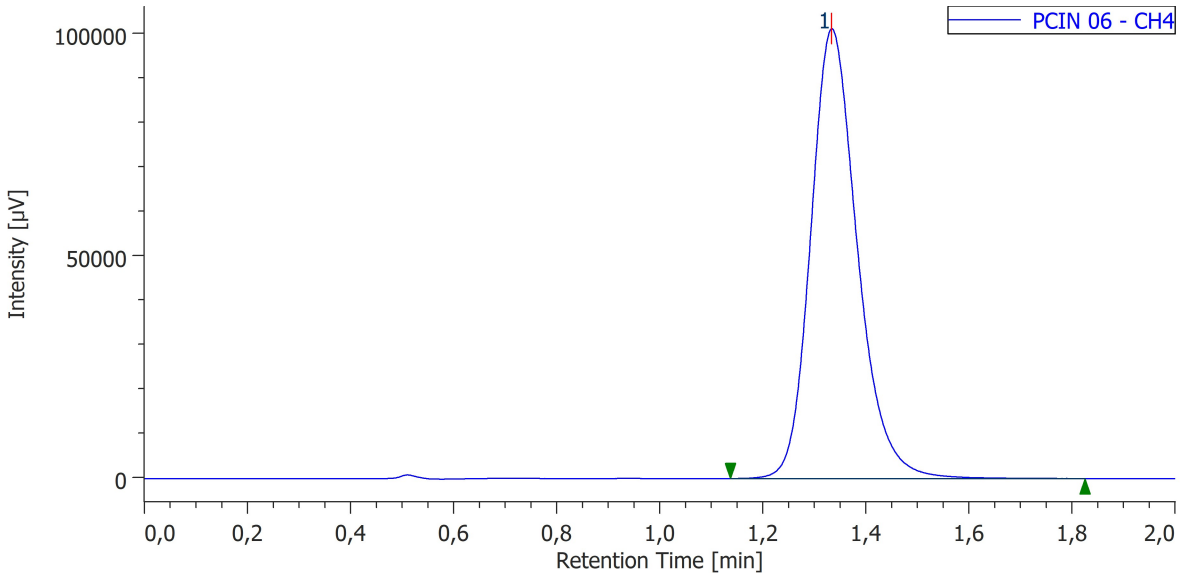


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:41:45
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:38:42
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,333	638026	101305	100,000	100,000	N/A	1103	N/A	1,221	

Chromatogram

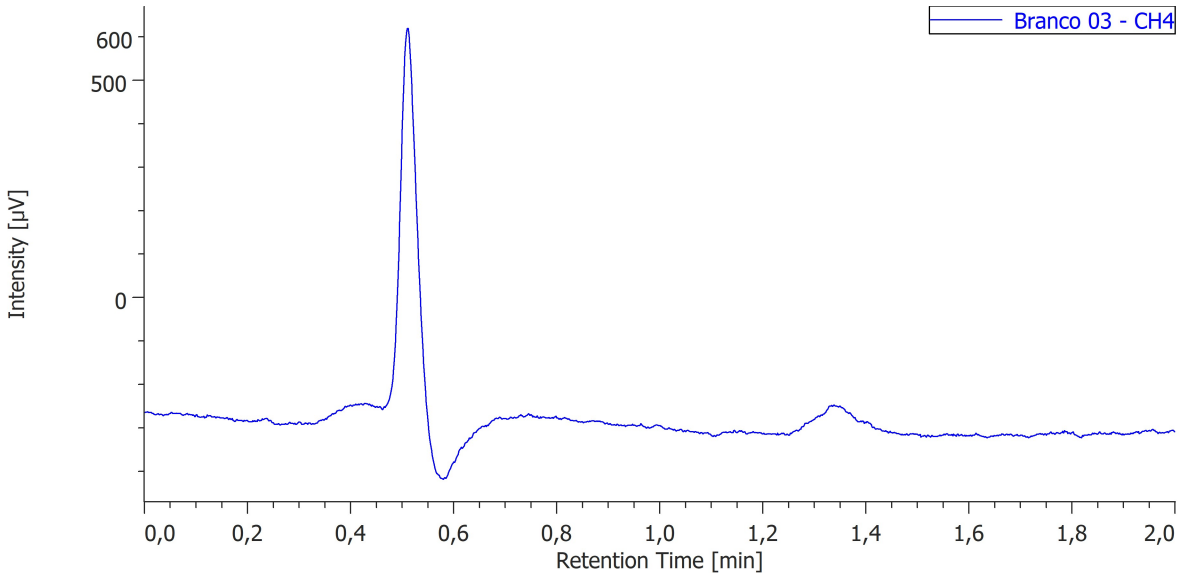


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:43:43
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 15:41:41
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	

Chromatogram

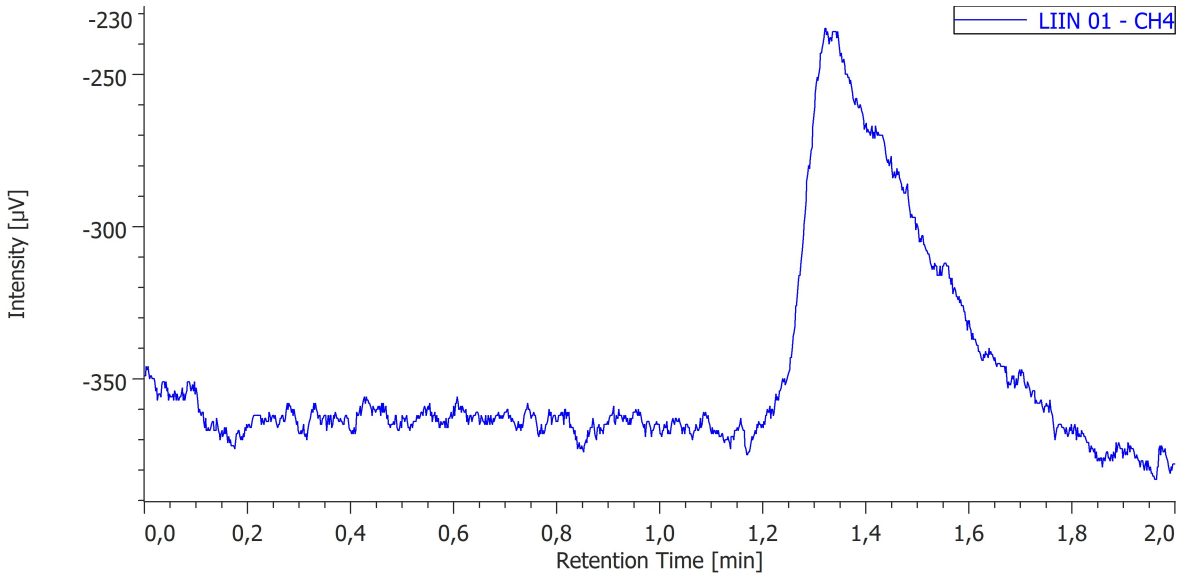


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 08:49:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 17:01:37
Volume	0,1 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

Chromatogram

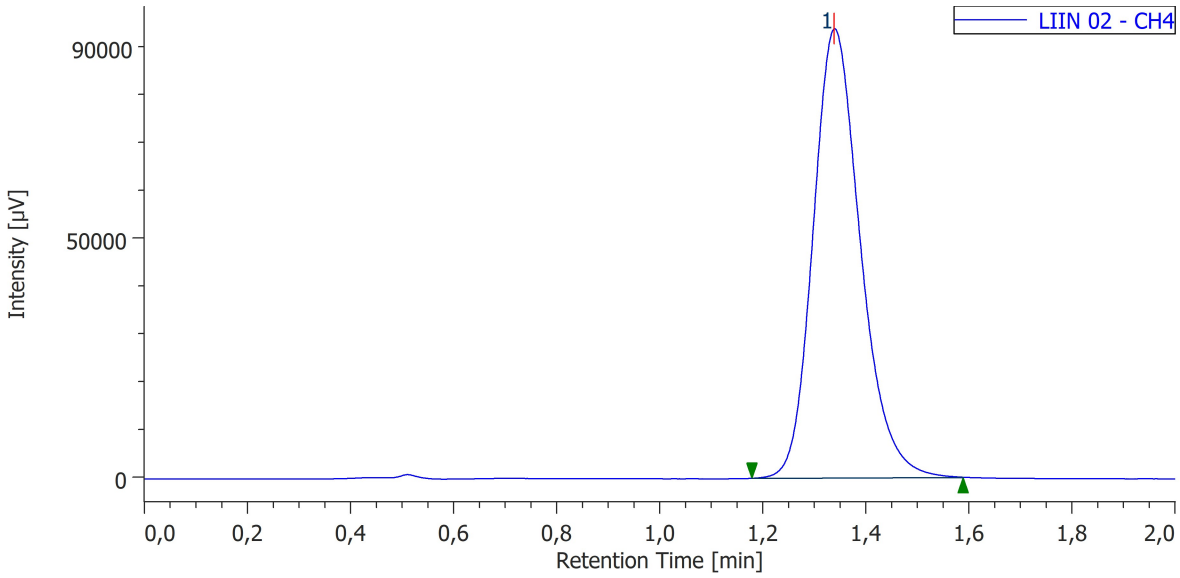


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 08:49:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 17:04:32
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,338	599427	93841	100,000	100,000	N/A	1060	N/A	1,223	

Chromatogram

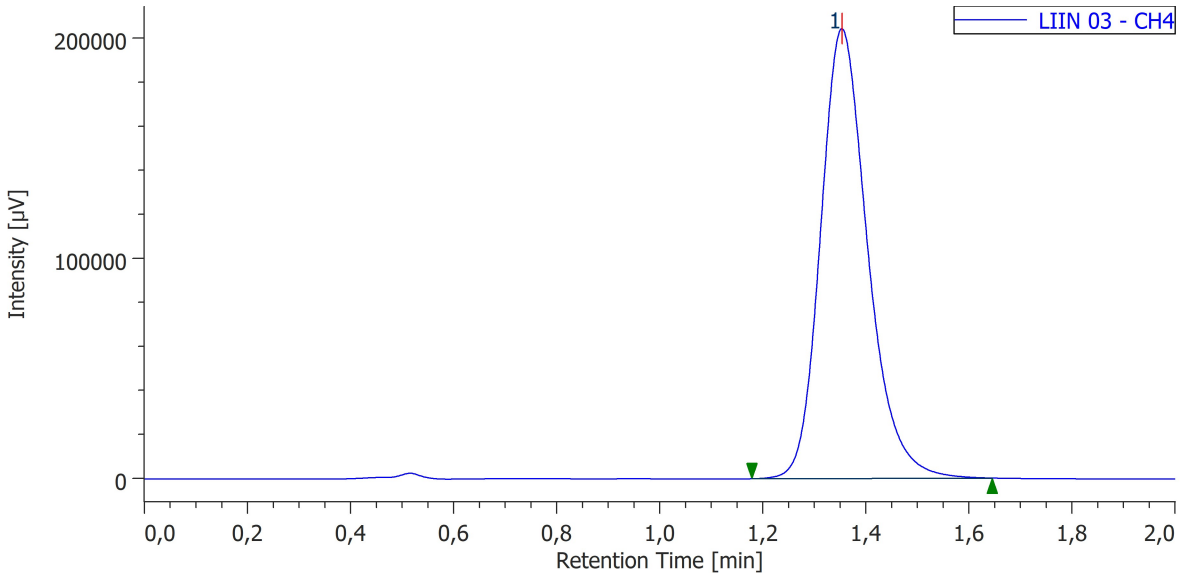


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 08:49:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 17:07:36
Volume	20,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,353	1299603	204337	100,000	100,000	N/A	1110	N/A	1,227	

Chromatogram

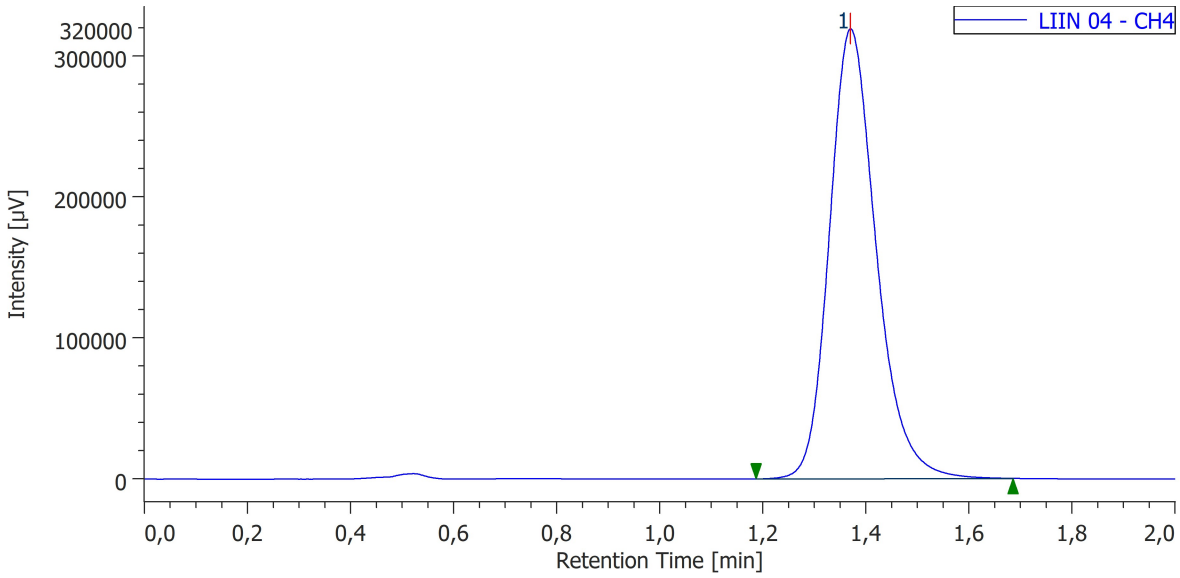


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 08:49:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 17:10:48
Volume	30,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,370	2015814	319211	100,000	100,000	N/A	1155	N/A	1,225	

Chromatogram

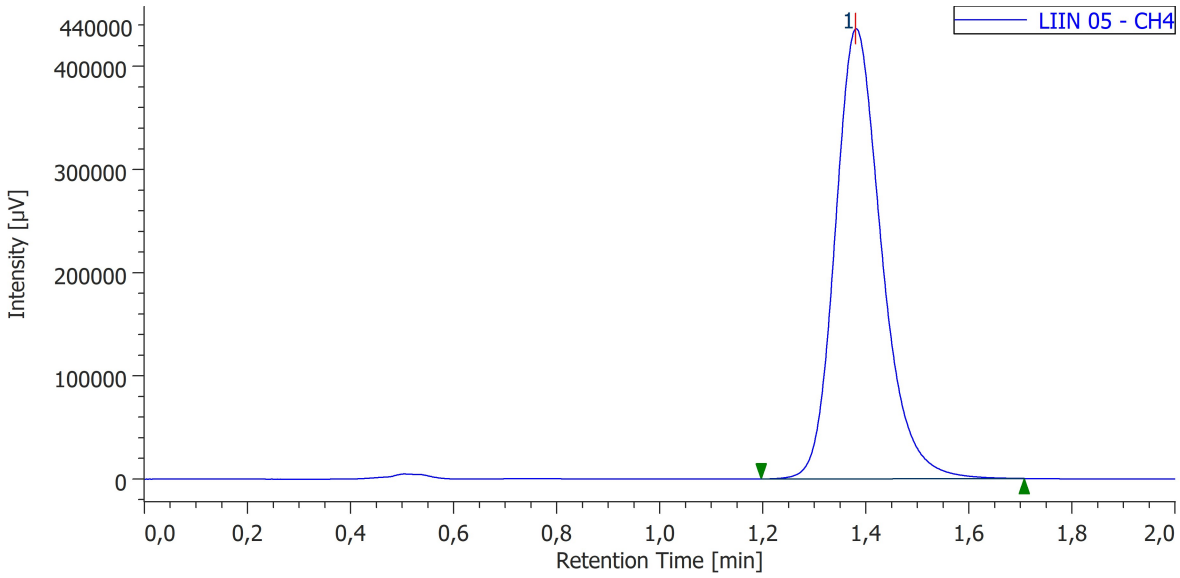


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 08:49:37
Description	
HPLC System Name	HPLC 002 RI
Injection Date	24/08/2022 17:14:13
Volume	40,0 [µL]
Sample #	2
Project Name	Qualificação HPLC 2
Acquisition Time	2,0 [min]
Acquisition Sequence	Qualificação HPLC 2
Control Method	Qualificação-RI
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	4	1,380	2728711	436294	100,000	100,000	N/A	1196	N/A	1,240	

Chromatogram

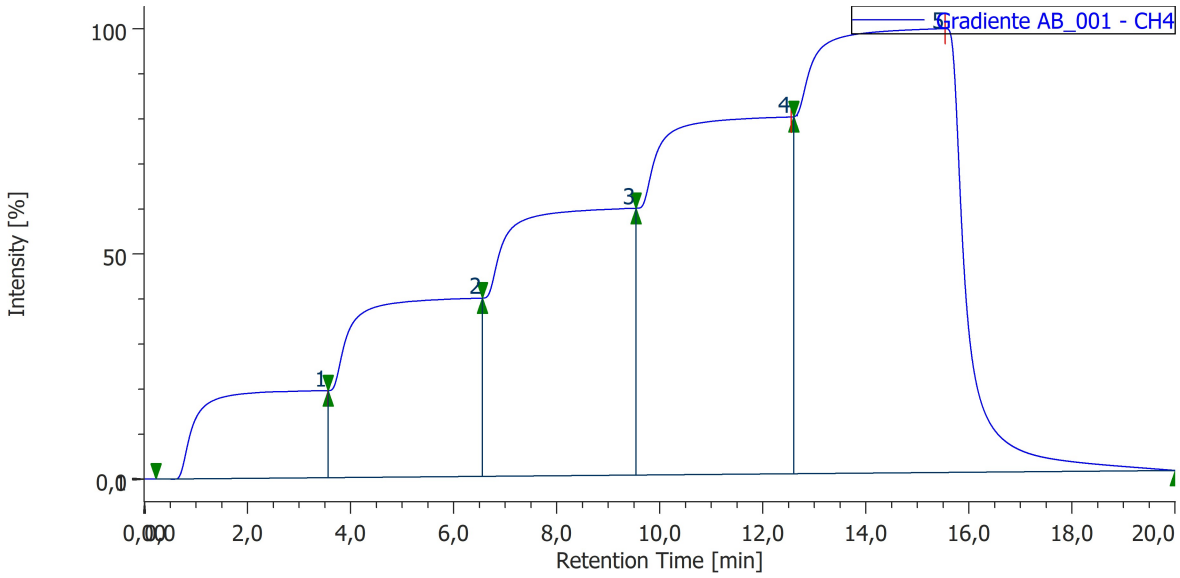


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 09:51:15
Description	
HPLC System Name	HPLC 002 RI
Injection Date	25/08/2022 09:25:40
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 2
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	4	3,560	9448273	61027	5,587	6,524	N/A	N/A	N/A	N/A	
2	40%	4	6,558	20815046	125077	12,308	13,371	N/A	N/A	N/A	N/A	
3	60%	4	9,538	31767169	187259	18,784	20,019	N/A	N/A	N/A	N/A	
4	80%	4	12,550	44156630	250420	26,109	26,771	N/A	N/A	N/A	N/A	
5	100%	4	15,537	62934847	311644	37,213	33,316	N/A	N/A	N/A	N/A	

Chromatogram

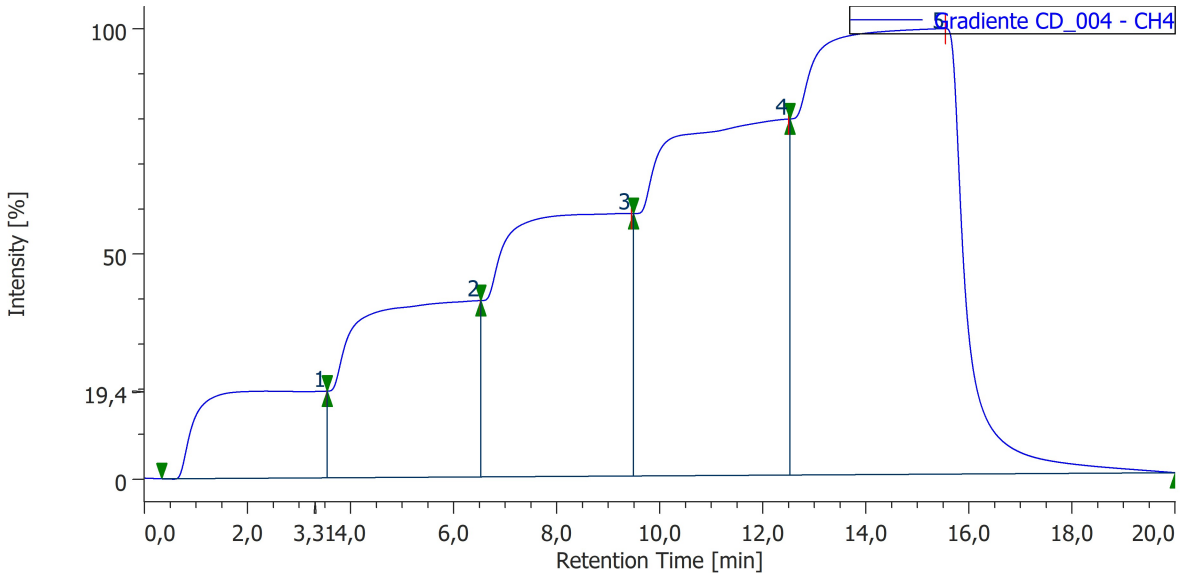


Chromatogram Information	
User Name	Administrator
Date Modified	25/08/2022 10:54:46
Description	
HPLC System Name	HPLC 002 RI
Injection Date	25/08/2022 10:31:36
Volume	0,0 [µL]
Sample #	–
Project Name	Qualificação HPLC 2
Acquisition Time	20,0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_004-CH4
Sample Name	
Channel Name	
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	4	3,540	9490260	60550	5,684	6,532	N/A	N/A	N/A	N/A	
2	40%	4	6,522	20061612	123155	12,015	13,287	N/A	N/A	N/A	N/A	
3	60%	4	9,448	30904954	183257	18,508	19,771	N/A	N/A	N/A	N/A	
4	80%	4	12,502	42744044	248714	25,599	26,833	N/A	N/A	N/A	N/A	
5	100%	4	15,540	63776245	311224	38,195	33,577	N/A	N/A	N/A	N/A	

Chromatogram

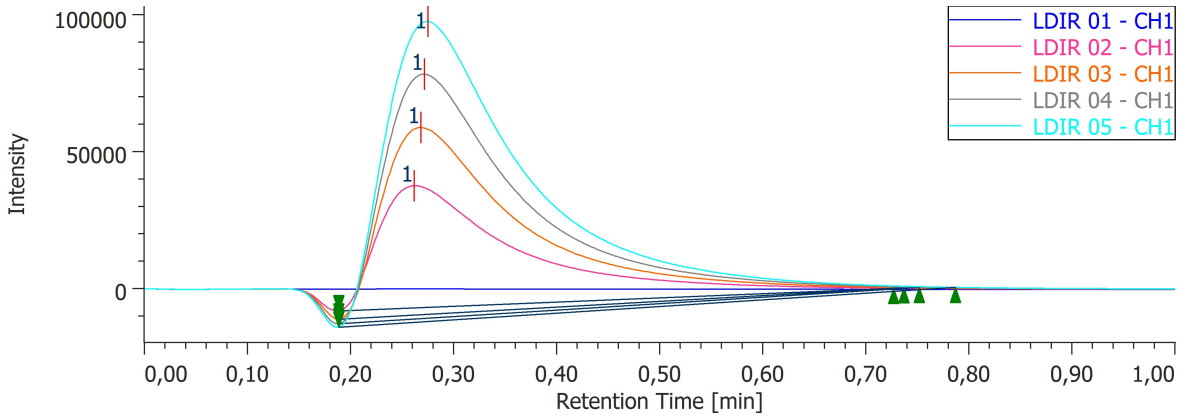

Channel & Peak Information Table

Chromatogram Name LDIR 01-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,262	435248	44548	100,000	100,000	N/A	23	N/A	3,352	

Chromatogram Name LDIR 03-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,268	677030	68250	100,000	100,000	N/A	23	N/A	3,111	


Chromatogram Name LDIR 04-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,272	892183	89022	100,000	100,000	N/A	23	N/A	2,993	

Chromatogram Name LDIR 05-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,275	1120205	109402	100,000	100,000	N/A	22	N/A	2,940	

Chromatogram

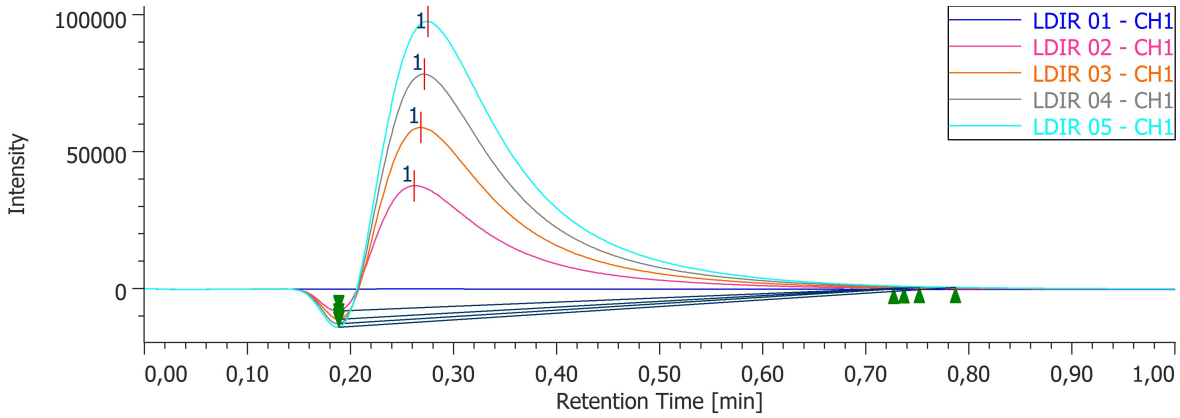

Channel & Peak Information Table

Chromatogram Name LDIR 01-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,262	435248	44548	100,000	100,000	N/A	23	N/A	3,352	

Chromatogram Name LDIR 03-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,268	677030	68250	100,000	100,000	N/A	23	N/A	3,111	


Chromatogram Name LDIR 04-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,272	892183	89022	100,000	100,000	N/A	23	N/A	2,993	

Chromatogram Name LDIR 05-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,275	1120205	109402	100,000	100,000	N/A	22	N/A	2,940	

Chromatogram

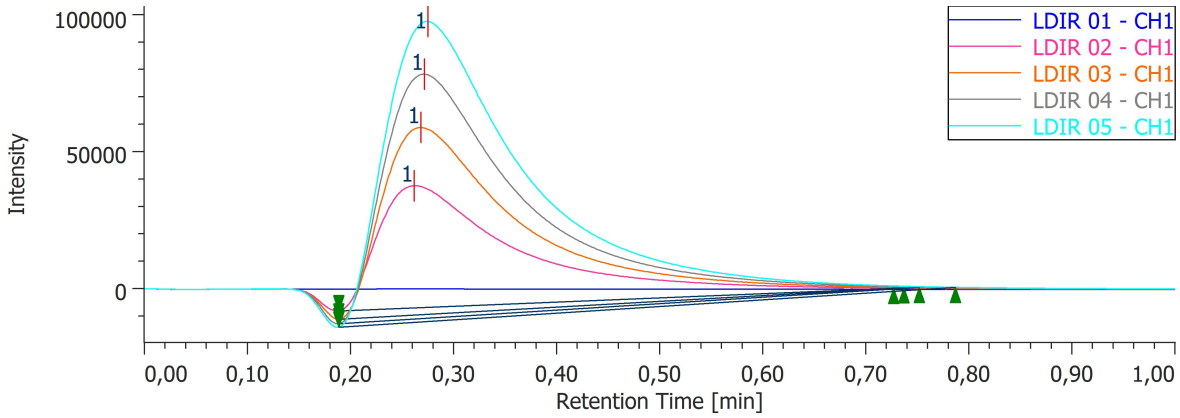

Channel & Peak Information Table

Chromatogram Name LDIR 01-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,262	435248	44548	100,000	100,000	N/A	23	N/A	3,352	

Chromatogram Name LDIR 03-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,268	677030	68250	100,000	100,000	N/A	23	N/A	3,111	


Chromatogram Name LDIR 04-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,272	892183	89022	100,000	100,000	N/A	23	N/A	2,993	

Chromatogram Name LDIR 05-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,275	1120205	109402	100,000	100,000	N/A	22	N/A	2,940	

Chromatogram

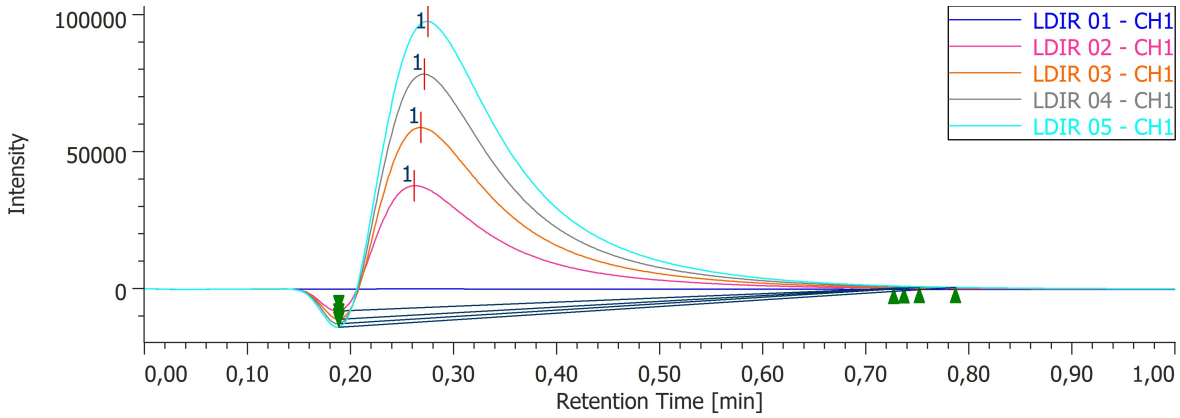

Channel & Peak Information Table

Chromatogram Name LDIR 01-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,262	435248	44548	100,000	100,000	N/A	23	N/A	3,352	

Chromatogram Name LDIR 03-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,268	677030	68250	100,000	100,000	N/A	23	N/A	3,111	


Chromatogram Name LDIR 04-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,272	892183	89022	100,000	100,000	N/A	23	N/A	2,993	

Chromatogram Name LDIR 05-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,275	1120205	109402	100,000	100,000	N/A	22	N/A	2,940	

Chromatogram

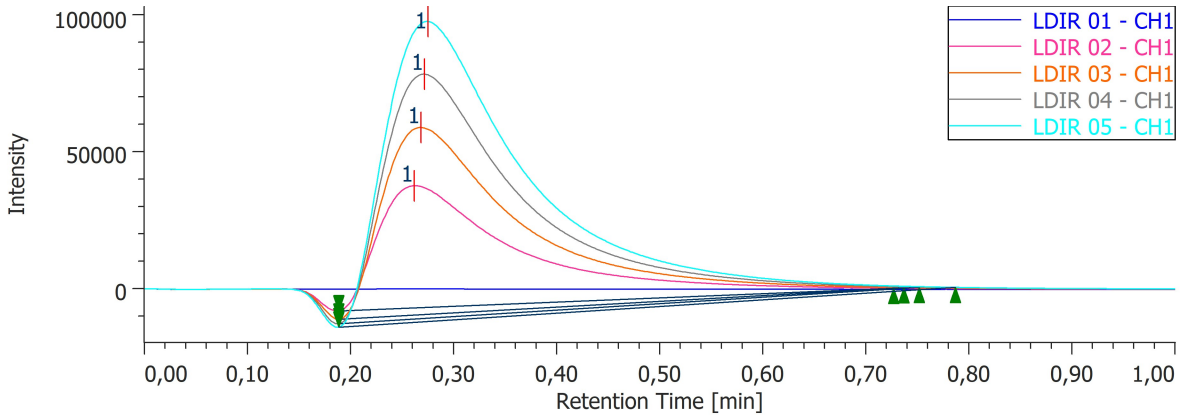

Channel & Peak Information Table

Chromatogram Name LDIR 01-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,262	435248	44548	100,000	100,000	N/A	23	N/A	3,352	

Chromatogram Name LDIR 03-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,268	677030	68250	100,000	100,000	N/A	23	N/A	3,111	

Chromatogram Name LDIR 04-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,272	892183	89022	100,000	100,000	N/A	23	N/A	2,993	

Chromatogram Name LDIR 05-CH1
Sample Name
Channel Name RI

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	RI	1	0,275	1120205	109402	100,000	100,000	N/A	22	N/A	2,940	