
Peak Find - EDUV

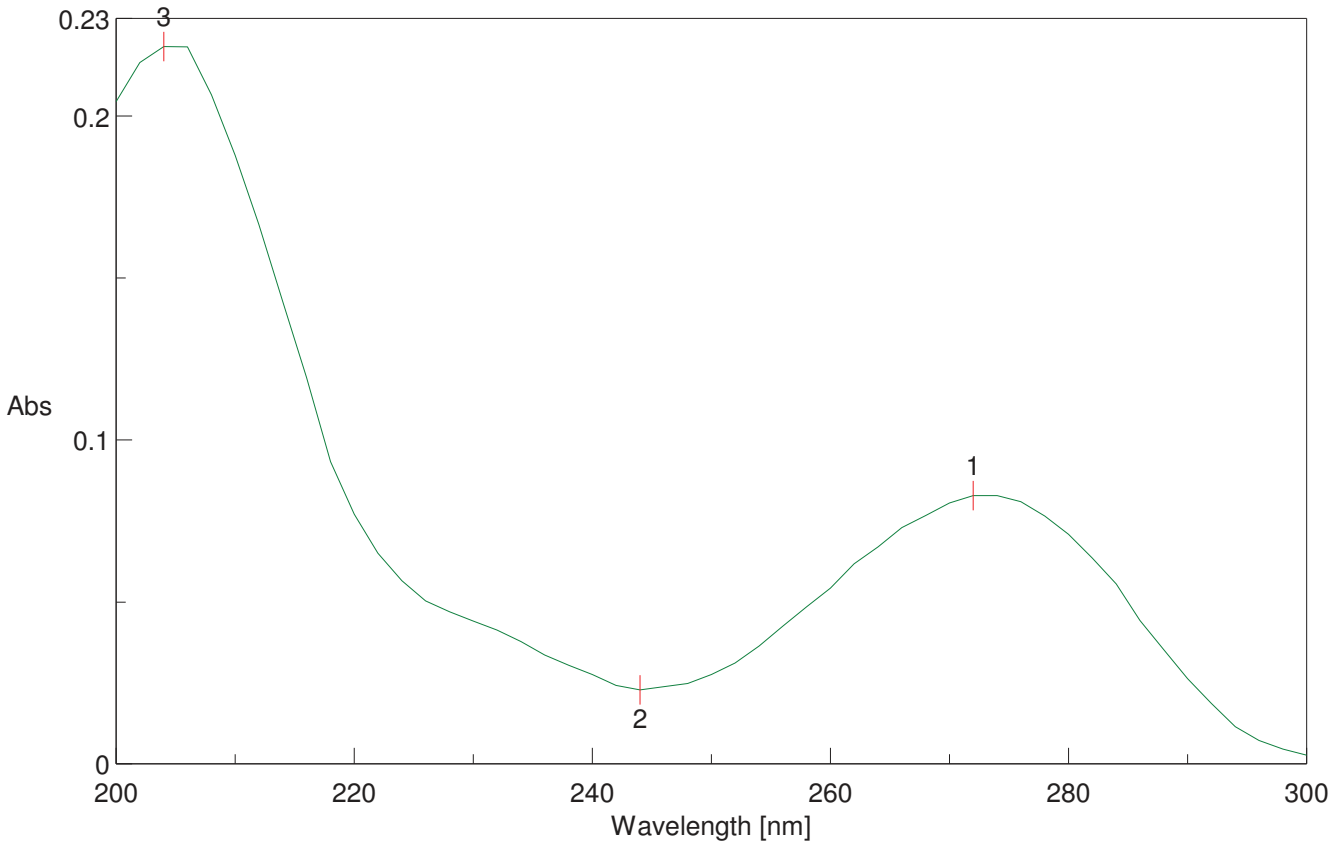

[Comments]

User	Administrator
Division	---
Company	JP
Creation date	24/08/2022 12:02

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	900 nm
Data interval	2 nm
Data points	351


[Measurement Information]

Instrument Name	UV-4070
Model Name	UV-4070
Serial No.	A010760888
ROM version	1.00.18

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity	No.	Position	Intensity
1	272	0.082751	2	244	0.0228499	3	204	0.221341

Chromatogram

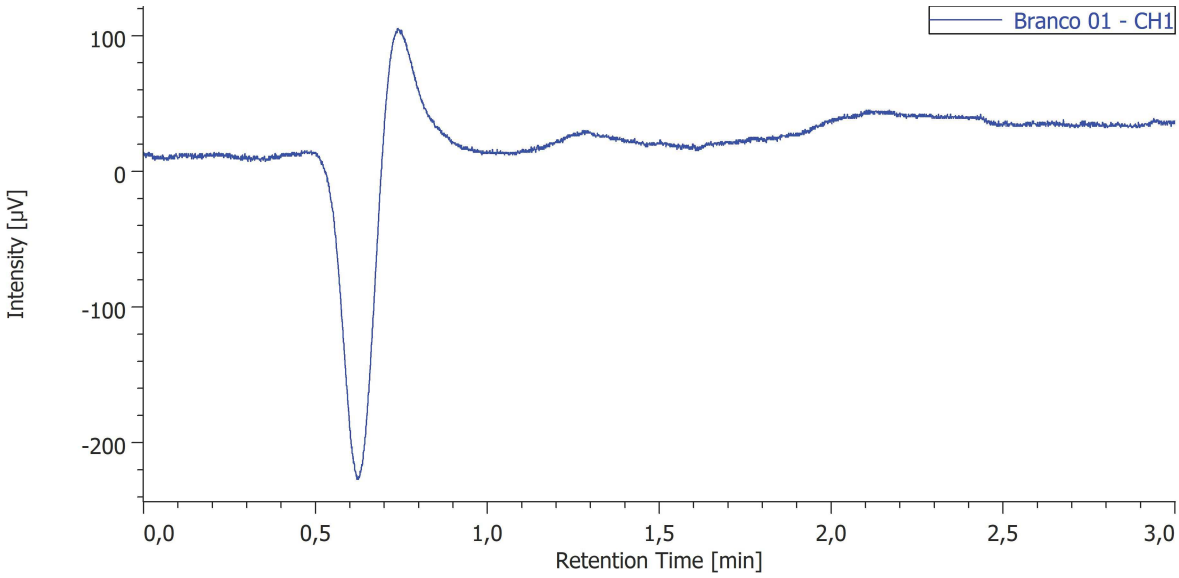


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:40
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:09:28
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

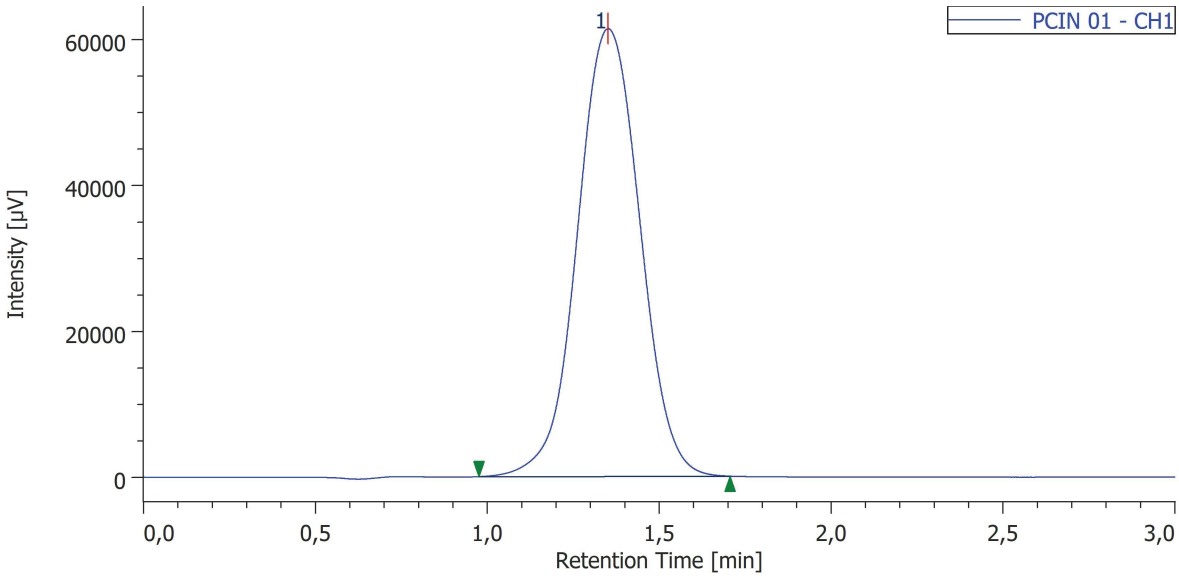


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:12:40
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,351	776349	61339	100,000	100,000	N/A	261	N/A	1,012	
Total				776349	61339			0,00000				

Chromatogram

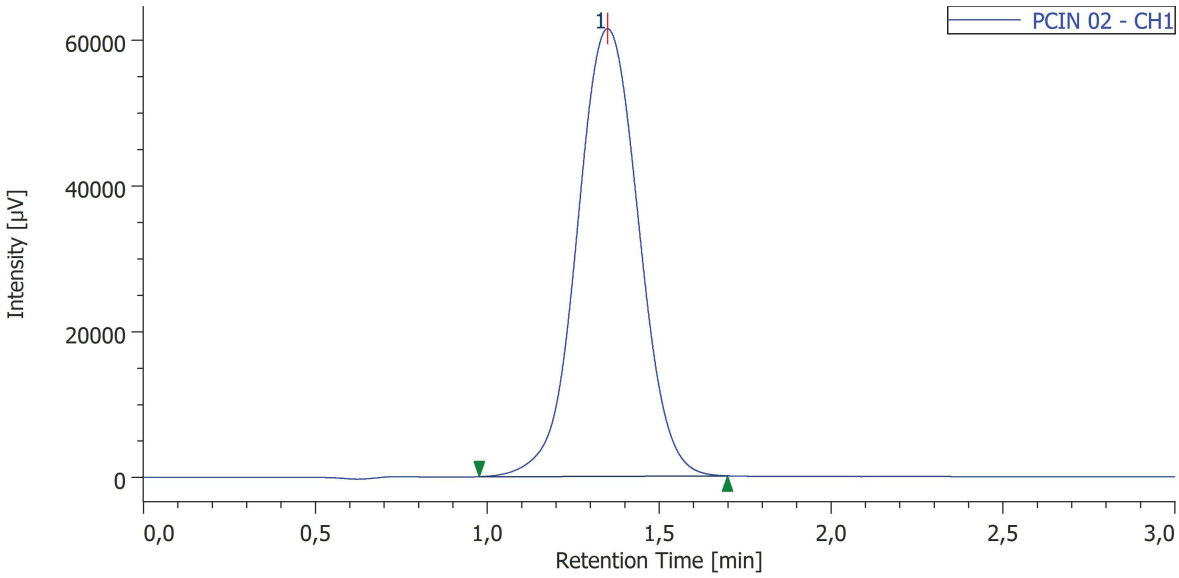


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:15:52
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,349	766007	61407	100,000	100,000	N/A	269	N/A	1,008	
Total				766007	61407			0,00000				

Chromatogram

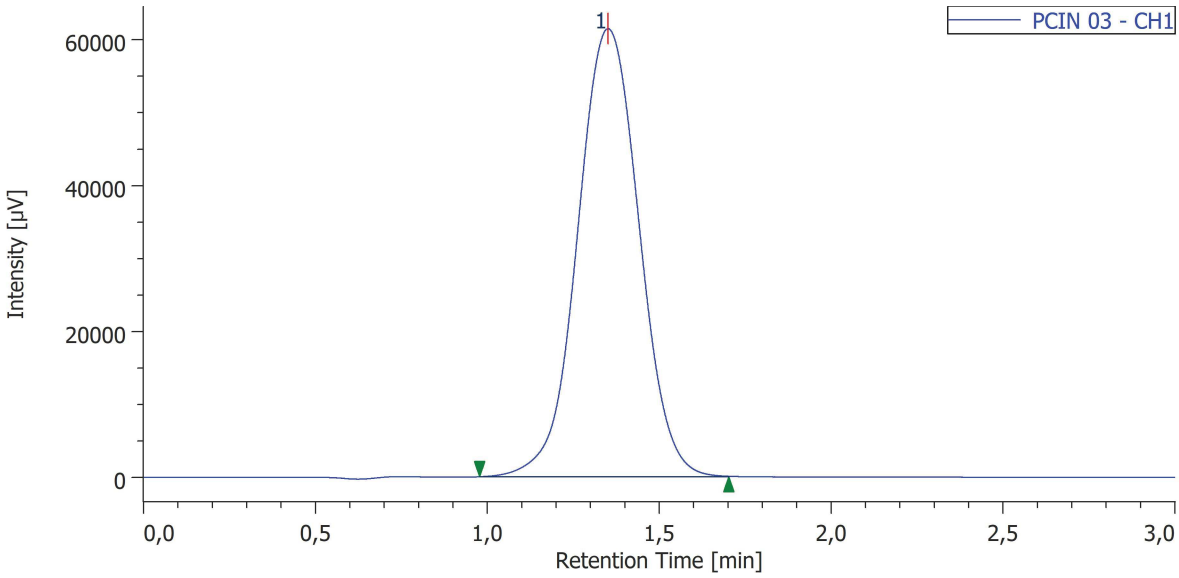


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:19:05
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,351	763084	61366	100,000	100,000	N/A	271	N/A	1,008	
Total				763084	61366			0,00000				

Chromatogram

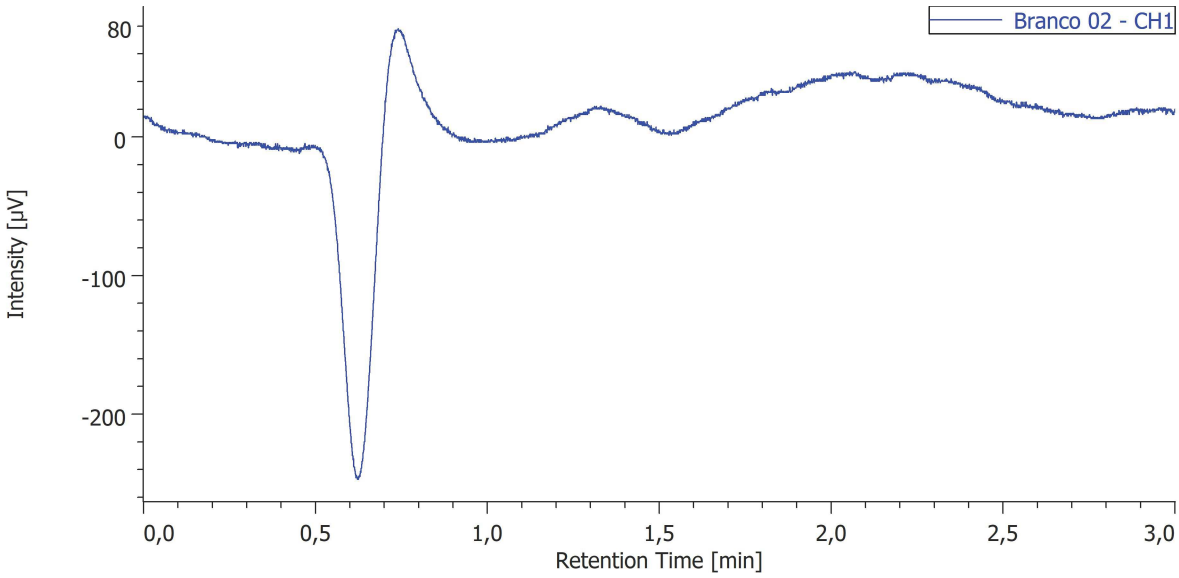


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:22:17
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

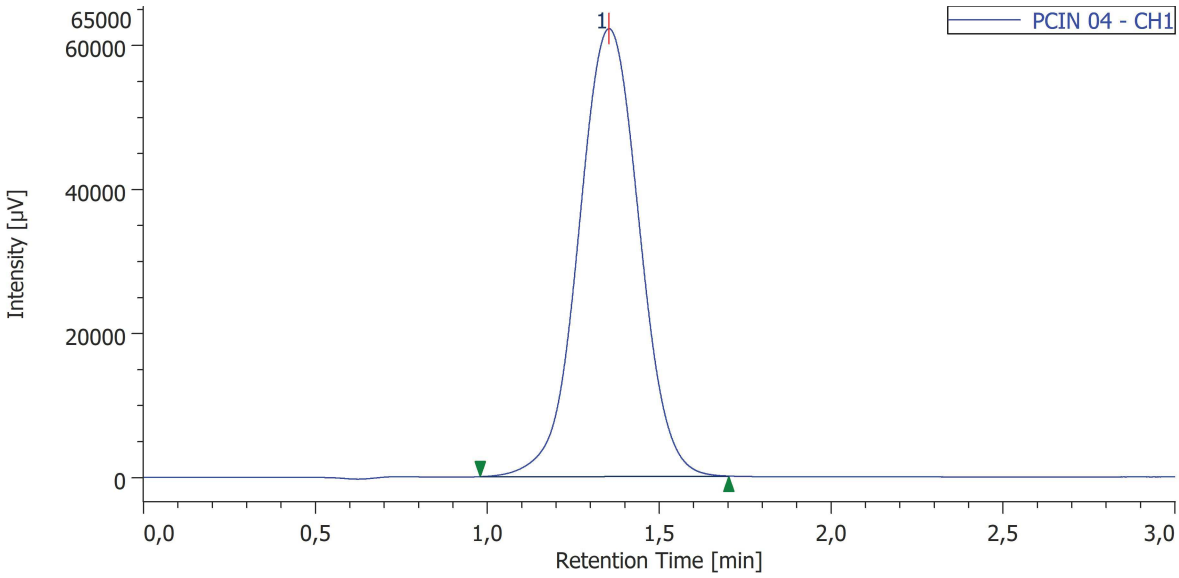


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:25:29
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,353	762198	62145	100,000	100,000	N/A	281	N/A	1,002	
Total				762198	62145			0,00000				

Chromatogram

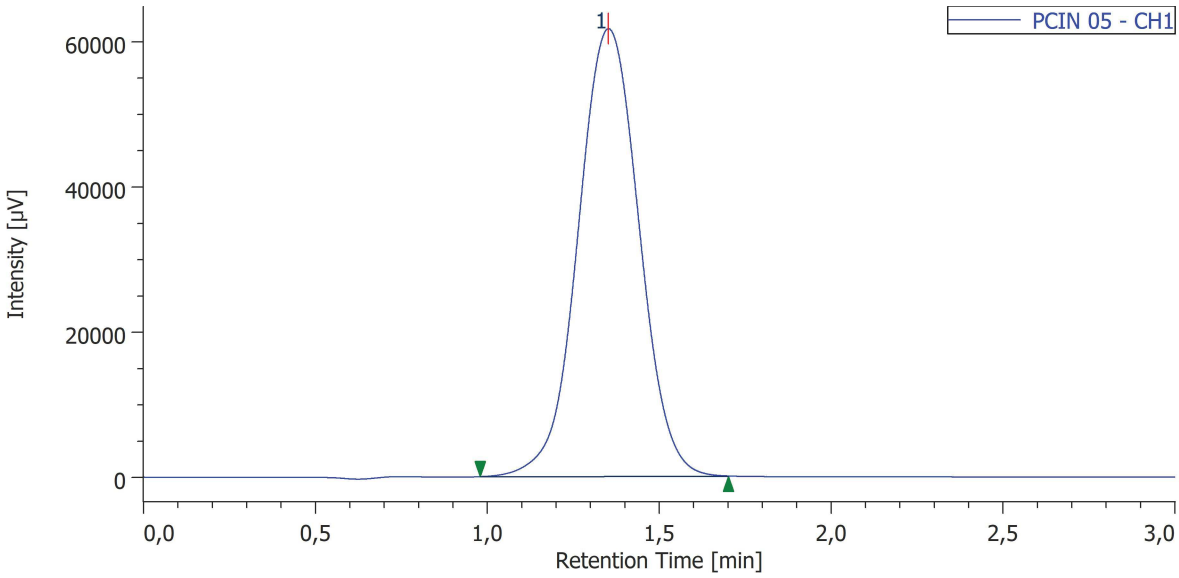


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:28:41
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,351	760857	61621	100,000	100,000	N/A	276	N/A	1,008	
Total				760857	61621			0,00000				

Chromatogram

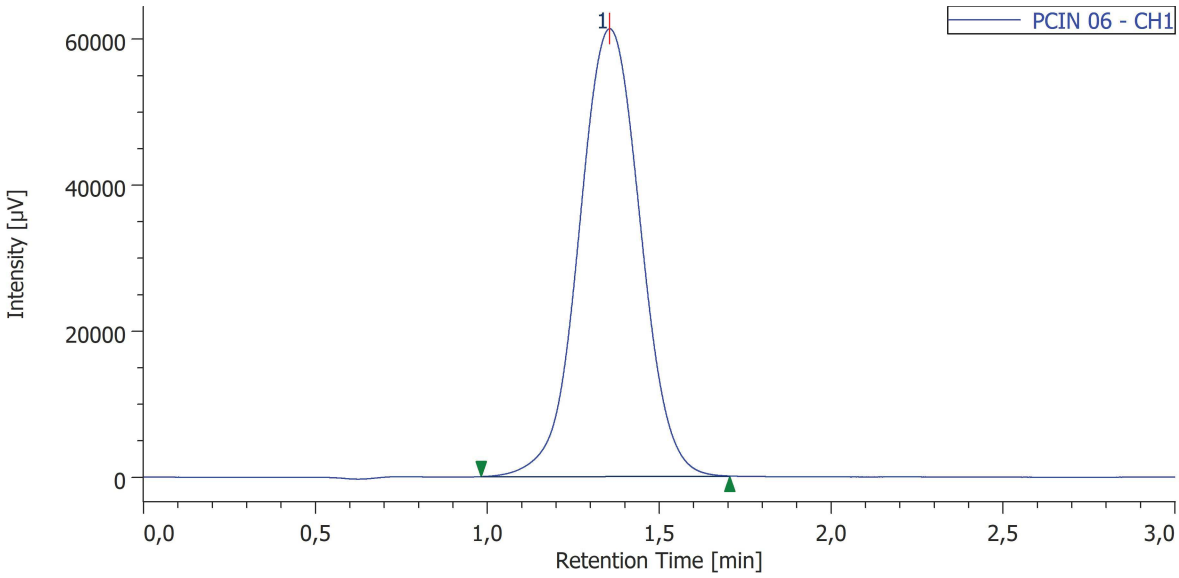


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:41
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:31:53
Volume	10,0 [µL]
Sample #	2
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,355	760695	61277	100,000	100,000	N/A	274	N/A	1,004	
Total				760695	61277			0,00000				

Chromatogram

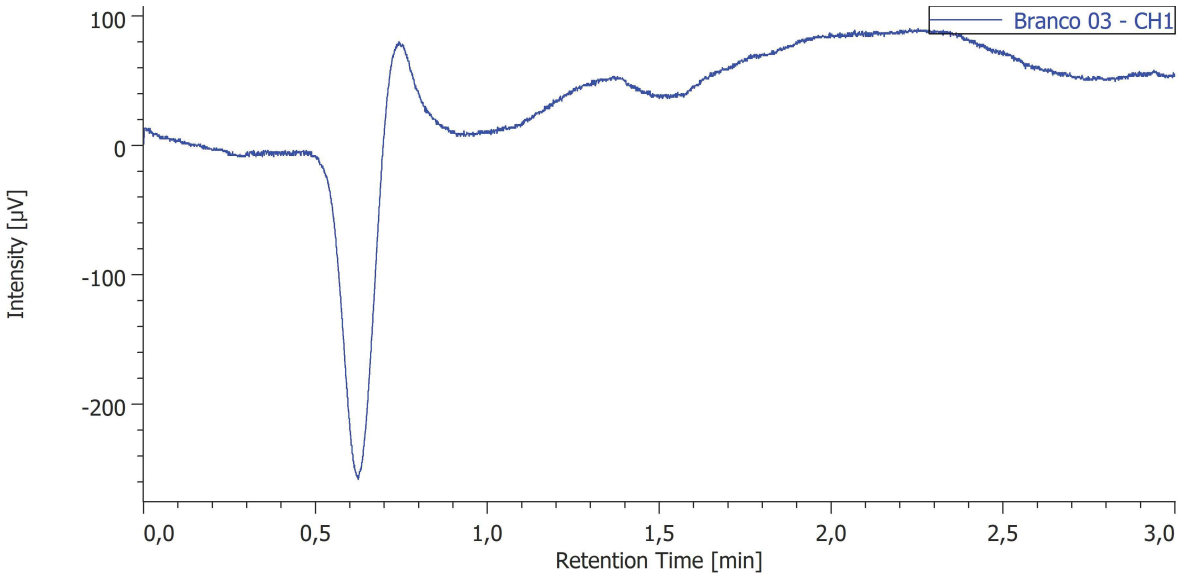


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:08:42
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:35:05
Volume	10,0 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

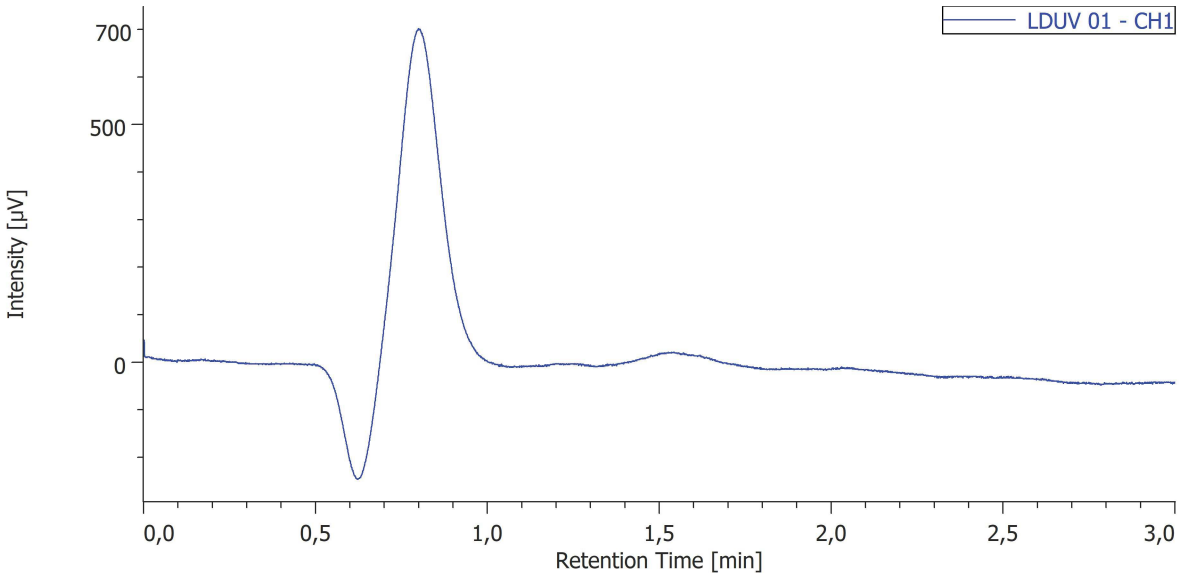


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:16:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:38:18
Volume	10,0 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

Chromatogram

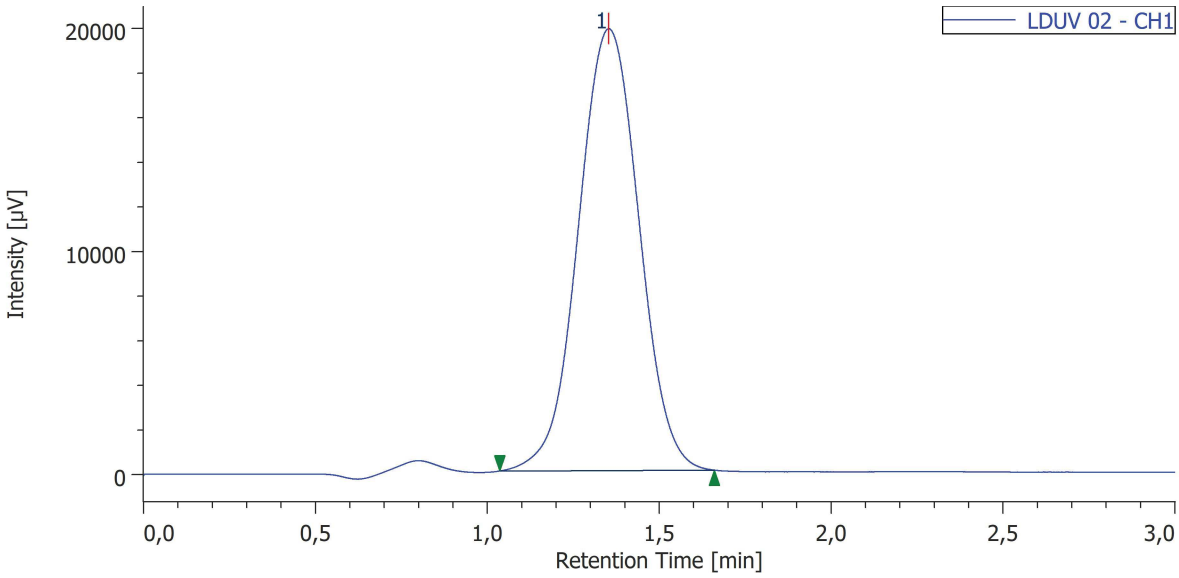


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:16:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:41:30
Volume	10,0 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,353	243238	19808	100,000	100,000	N/A	276	N/A	1,007	
Total				243238	19808			0,00000				

Chromatogram

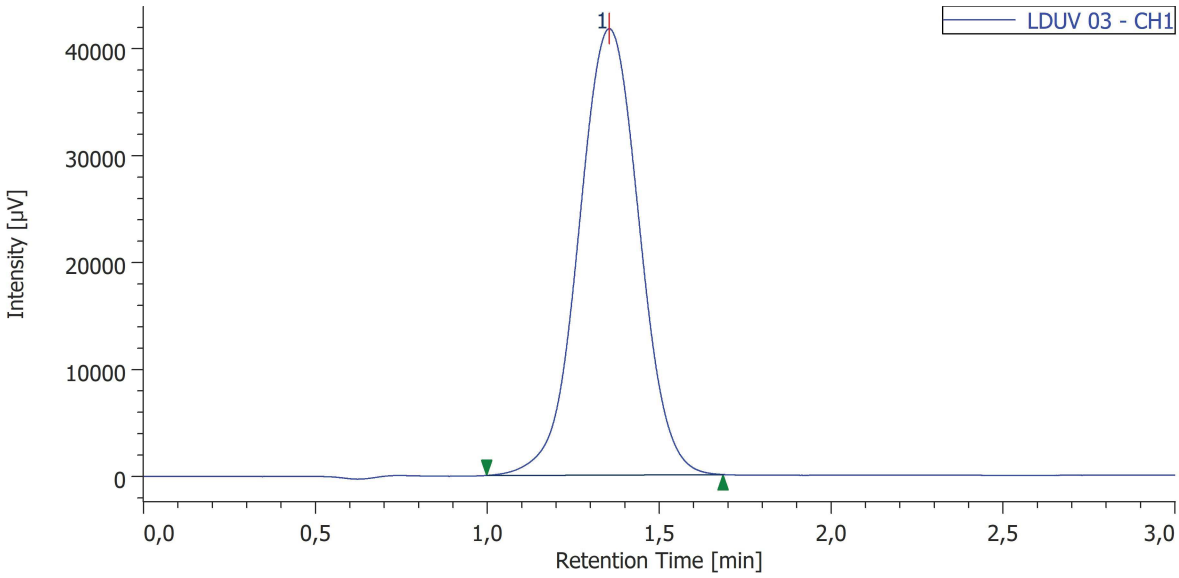


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:16:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:44:42
Volume	10,0 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,354	510887	41721	100,000	100,000	N/A	281	N/A	0,999	
Total				510887	41721			0,00000				

Chromatogram

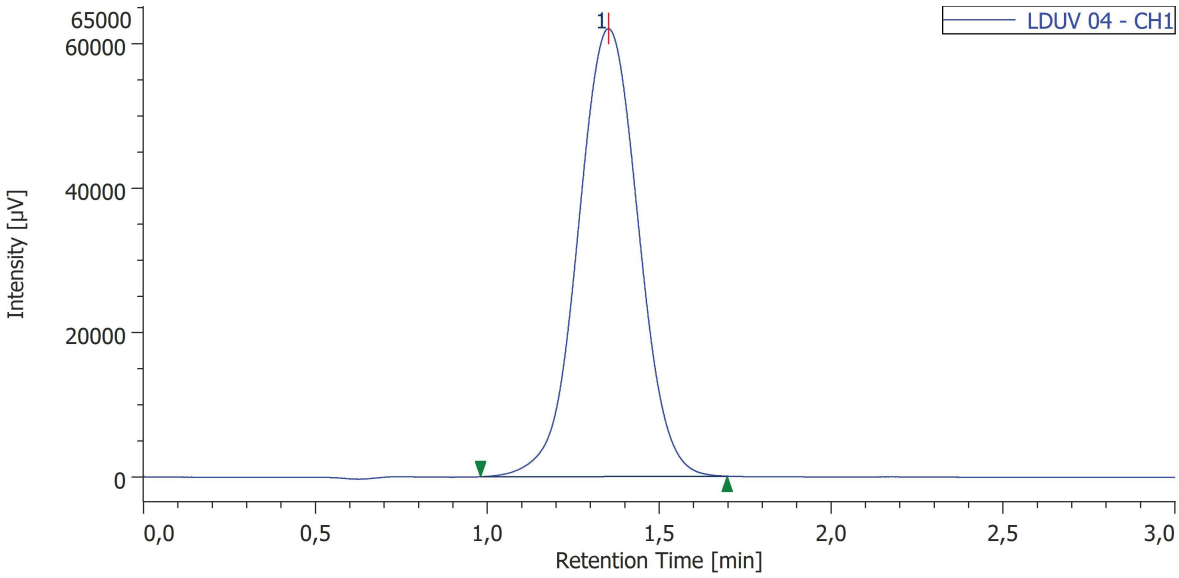


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:16:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:47:54
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,352	757275	61947	100,000	100,000	N/A	282	N/A	0,996	
Total				757275	61947			0,00000				

Chromatogram

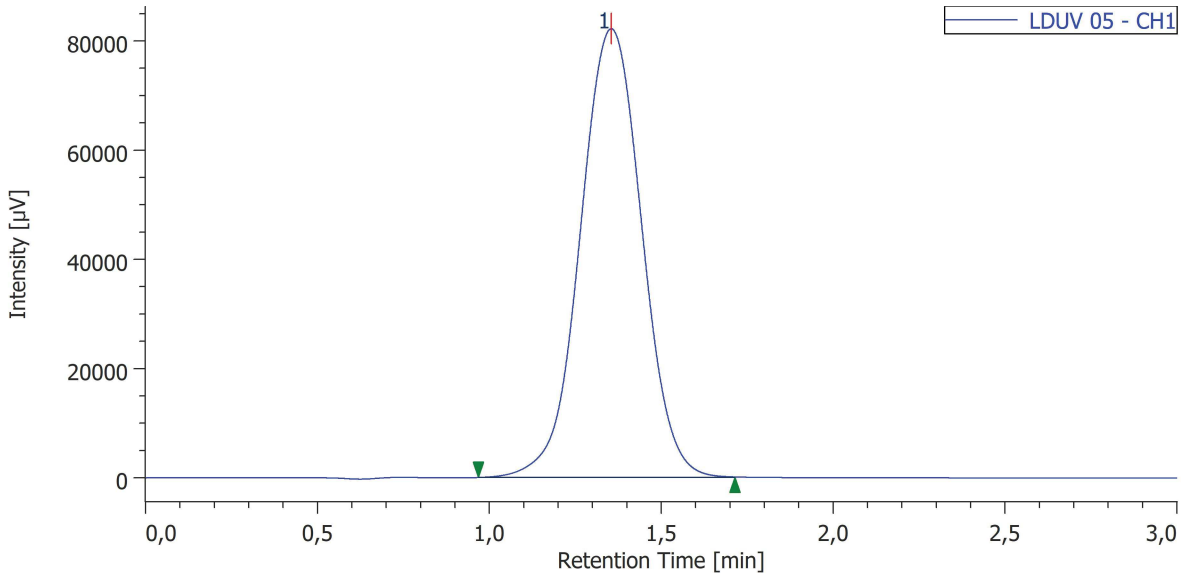


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:16:58
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:51:06
Volume	10,0 [µL]
Sample #	7
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	1	1,354	1020237	82106	100,000	100,000	N/A	273	N/A	0,998	
Total				1020237	82106			0,00000				

Chromatogram

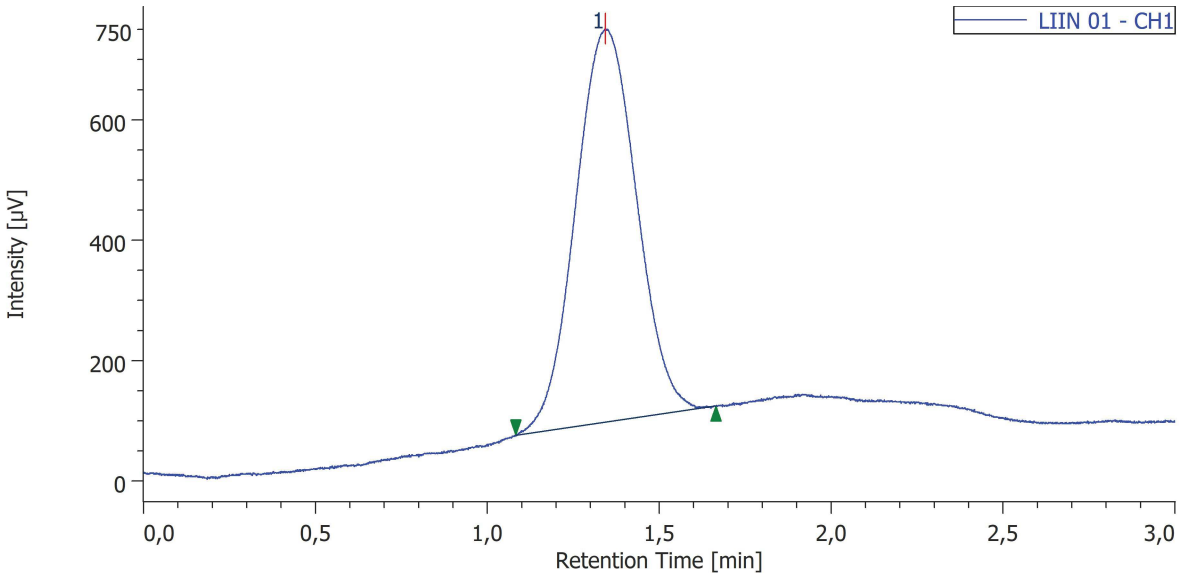


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:26:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:54:18
Volume	0,1 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,343	8045	653	100,000	100,000	N/A	265	N/A	1,037	
Total				8045	653			0,00000				

Chromatogram

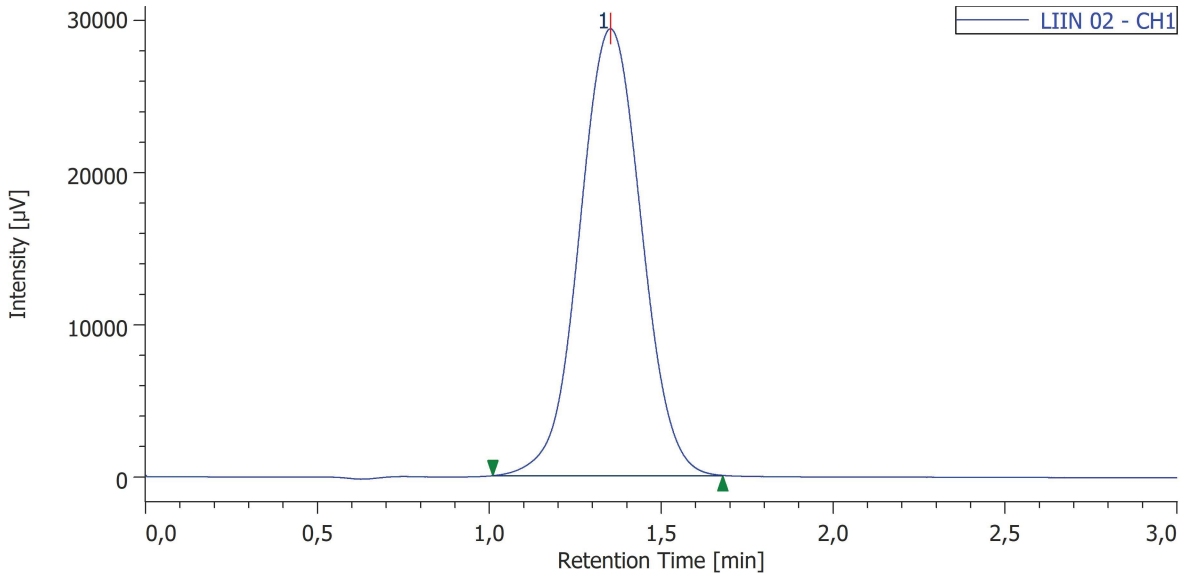


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:26:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 12:57:31
Volume	5,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,352	368149	29356	100,000	100,000	N/A	266	N/A	1,011	
Total				368149	29356			0,00000				

Chromatogram

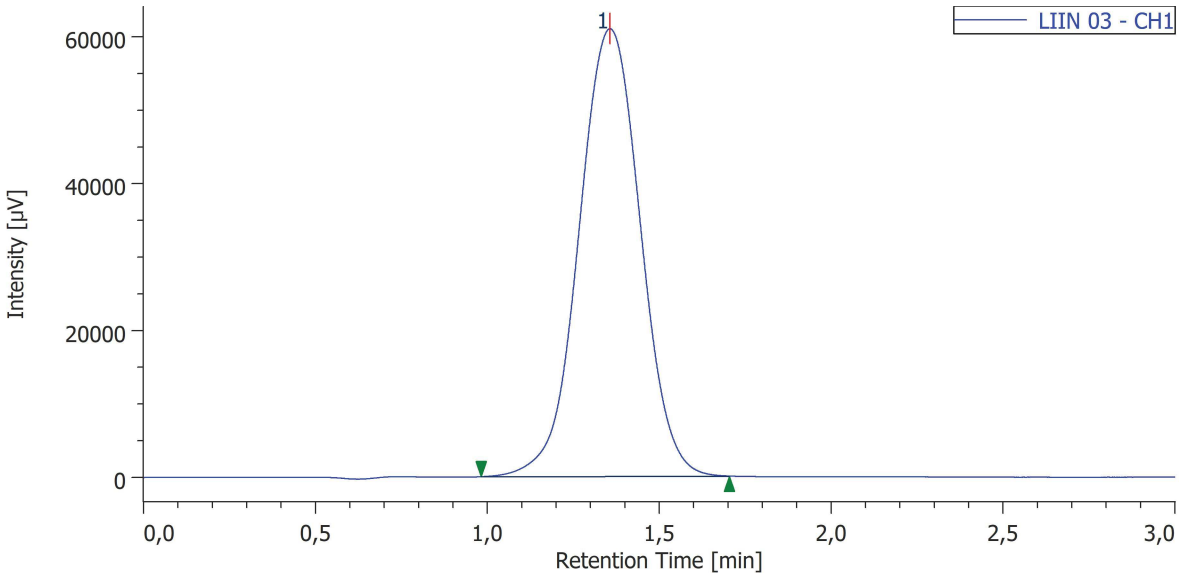


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:26:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 13:00:43
Volume	10,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,356	756962	60942	100,000	100,000	N/A	273	N/A	0,997	
Total				756962	60942			0,00000				

Chromatogram

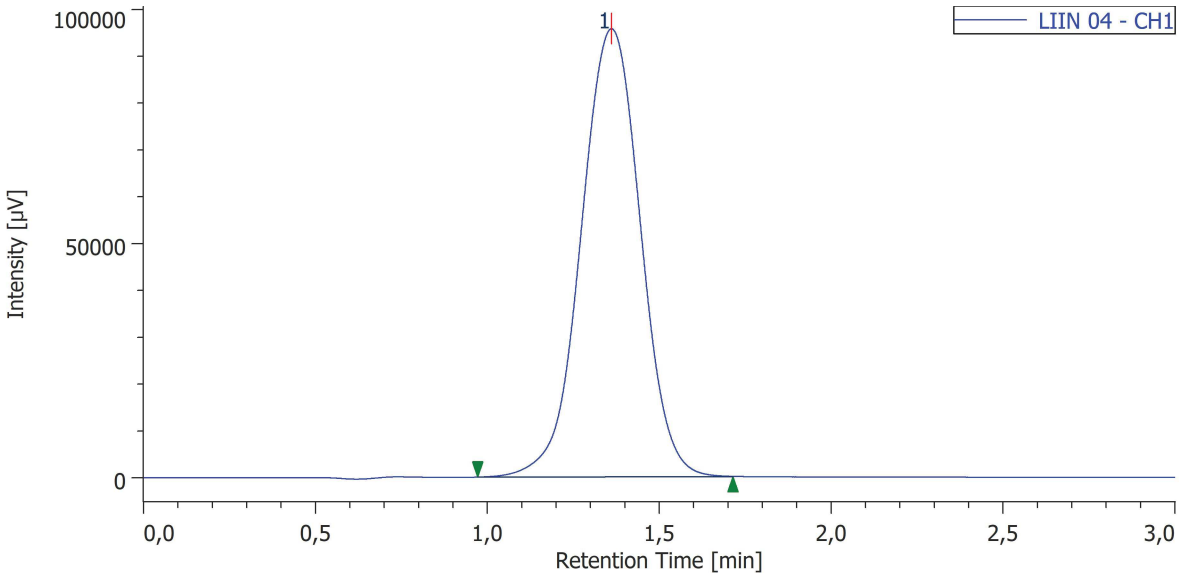


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:26:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 13:03:55
Volume	15,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,361	1147295	95640	100,000	100,000	N/A	296	N/A	0,981	
Total				1147295	95640			0,00000				

Chromatogram

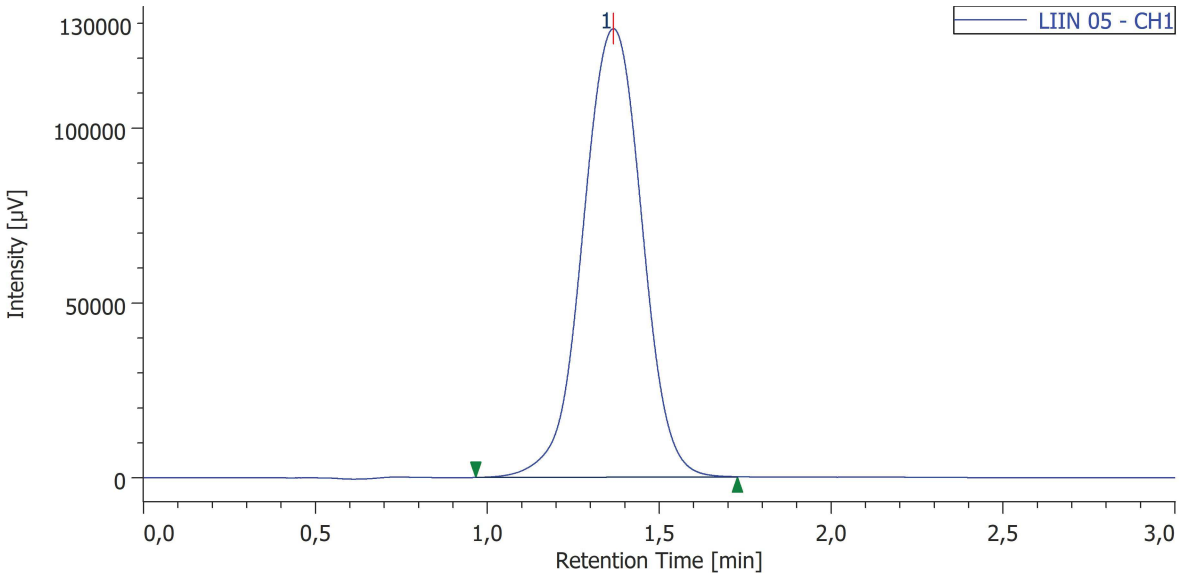


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 13:26:52
Description	
HPLC System Name	HPLC-0003 UV
Injection Date	24/08/2022 13:07:07
Volume	20,0 [µL]
Sample #	8
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 UV4070
Control Method	Qualificação UV4070
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1,366	1535290	128161	100,000	100,000	N/A	298	N/A	0,971	
Total				1535290	128161			0,00000				

Chromatogram

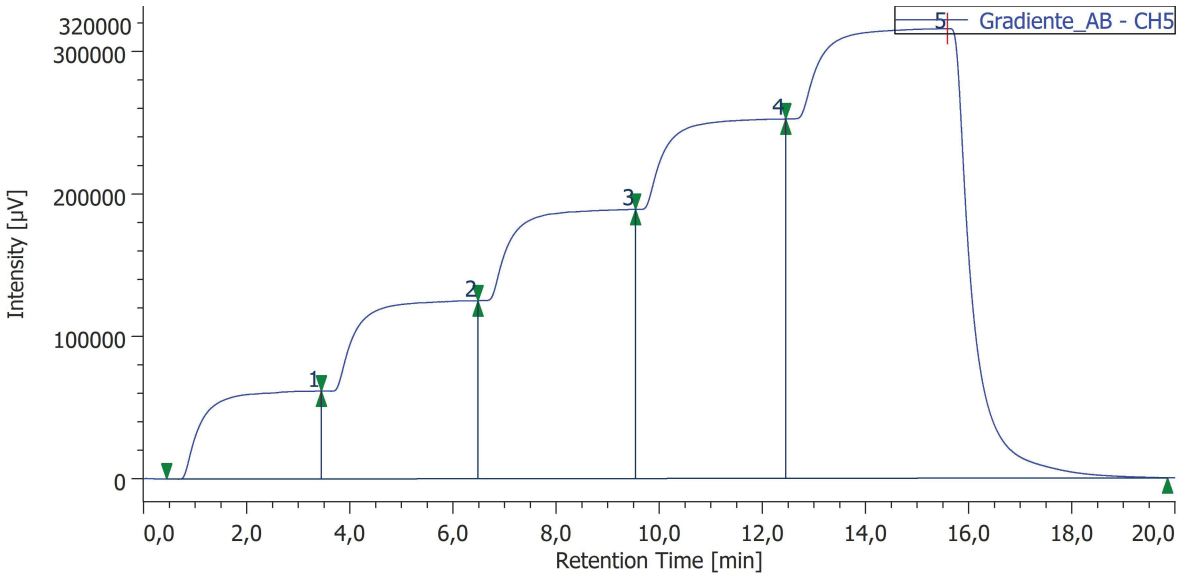


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 15:54:12
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 15:32:20
Volume	0,1 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente_AB
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente_AB-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,440	8570293	61580	5,044	6,532	N/A	N/A	N/A	N/A	
2	Unknown	5	6,483	20234764	124825	11,909	13,241	N/A	N/A	N/A	N/A	
3	Unknown	5	9,537	32196851	188793	18,949	20,027	N/A	N/A	N/A	N/A	
4	Unknown	5	12,445	41807685	252116	24,605	26,744	N/A	N/A	N/A	N/A	
5	Unknown	5	15,583	67103359	315369	39,493	33,454	N/A	N/A	N/A	N/A	
Total				169912952	942683			0,00000				

Chromatogram

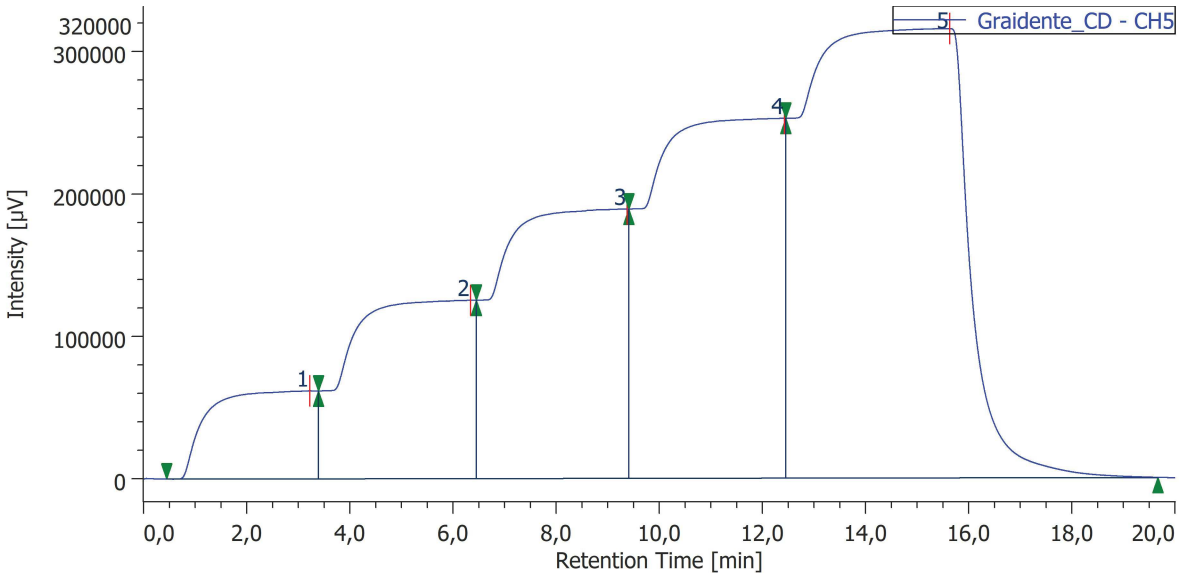


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 16:12:34
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 15:52:32
Volume	0,1 [µL]
Sample #	1
Project Name	JASCO
Acquisition Time	20,0 [min]
Acquisition Sequence	Gradiente
Control Method	Gradiente_CD
Peak ID Table	
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Graidente_CD-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	3,223	8393629	61748	4,933	6,545	N/A	N/A	N/A	N/A	
2	Unknown	5	6,340	20230201	125155	11,890	13,265	N/A	N/A	N/A	N/A	
3	Unknown	5	9,375	31034701	188964	18,240	20,028	N/A	N/A	N/A	N/A	
4	Unknown	5	12,422	43332752	252445	25,468	26,756	N/A	N/A	N/A	N/A	
5	Unknown	5	15,628	67156301	315179	39,469	33,406	N/A	N/A	N/A	N/A	
Total				170147584	943491			0,00000				

Peak Find - EDUVMD-2018

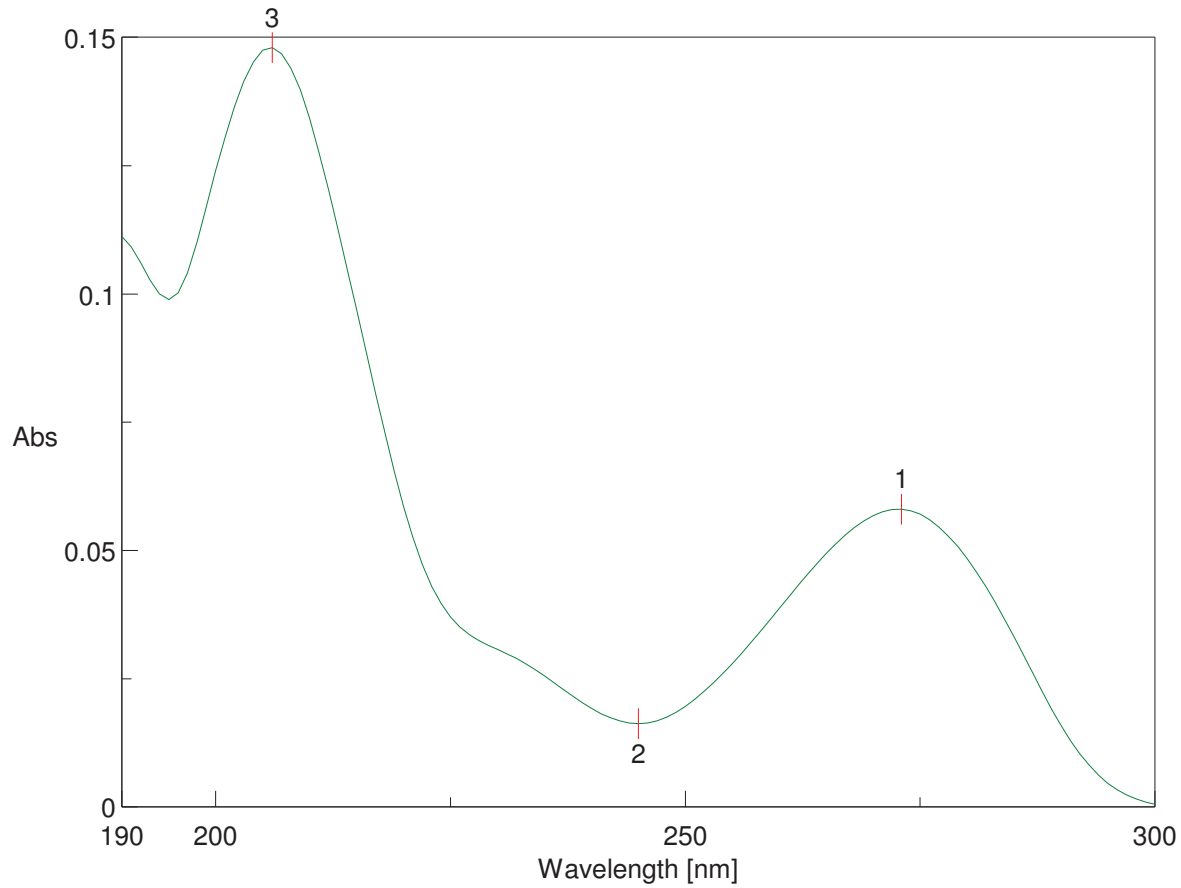

[Comments]

User	Administrator
Division	---
Company	JP
Creation date	24/08/2022 14:09

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	190 nm
End	300 nm
Data interval	1 nm
Data points	111


[Measurement Information]

Instrument Name	MD-2018
Model Name	MD-2018
Serial No.	A023761331
ROM version	V1.05.01

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	273	0.057997	2	245	0.016228
3	206	0.147923			

Chromatogram

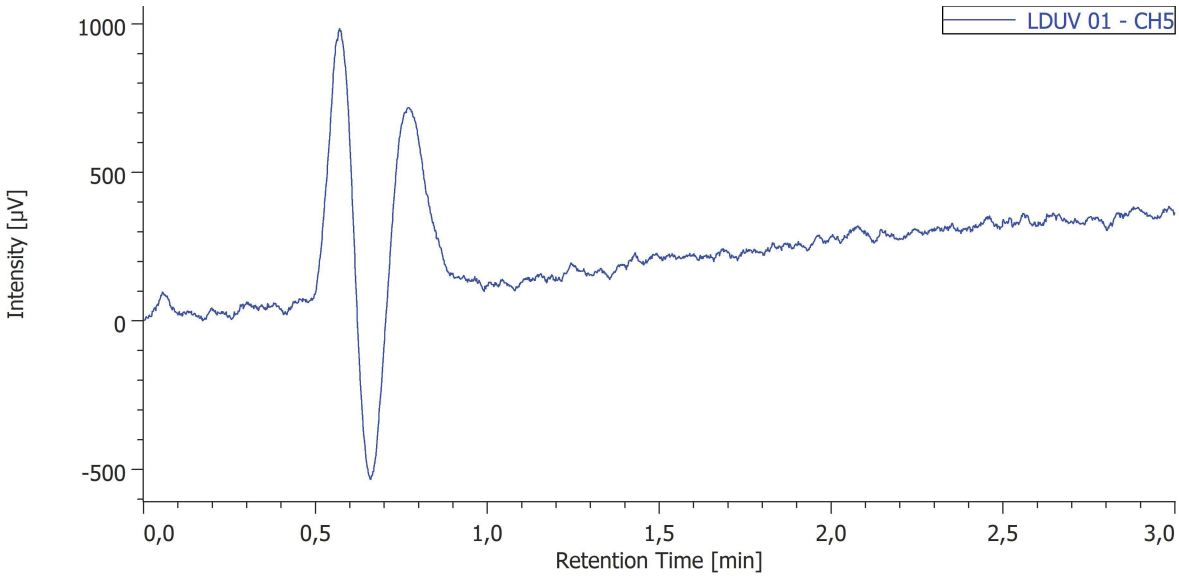


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 14:27:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 14:06:26
Volume	10,0 [µL]
Sample #	3
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 MD-2018
Control Method	Qualificação MD-2018
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

Chromatogram

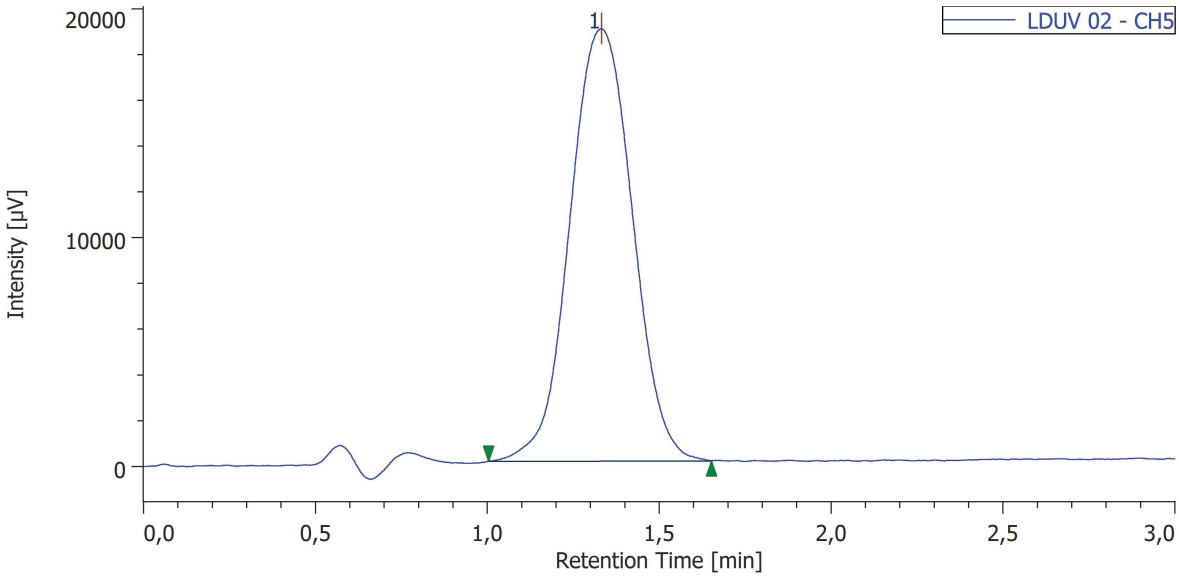


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 14:27:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 14:09:38
Volume	10,0 [µL]
Sample #	4
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 MD-2018
Control Method	Qualificação MD-2018
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,332	239100	18891	100,000	100,000	N/A	248	N/A	1,007	
Total				239100	18891			0,00000				

Chromatogram

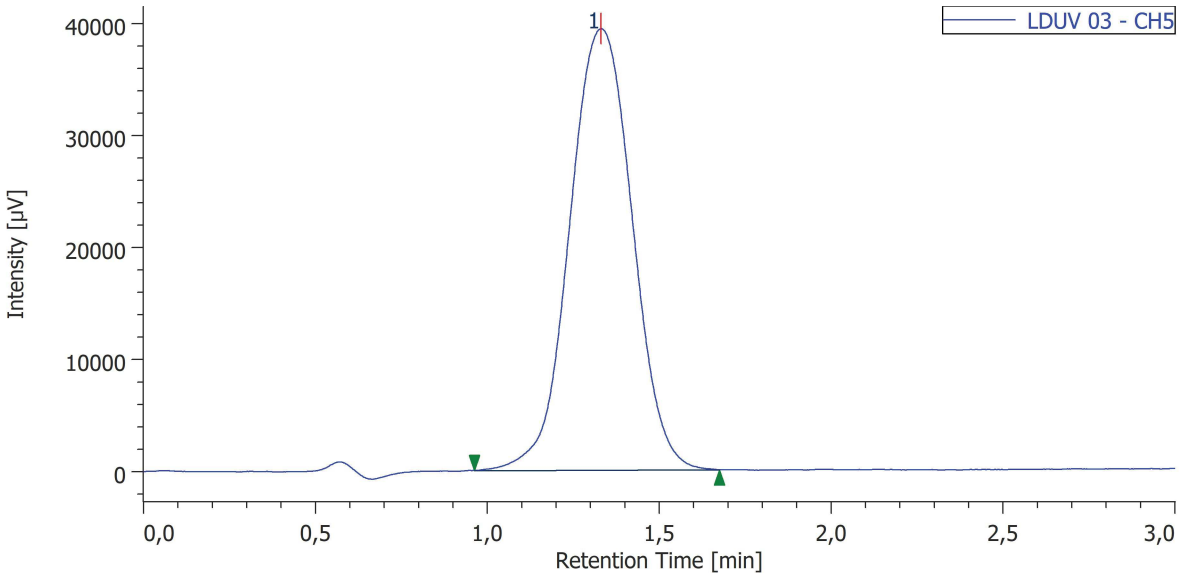


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 14:27:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 14:12:50
Volume	10,0 [µL]
Sample #	5
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 MD-2018
Control Method	Qualificação MD-2018
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,330	500174	39406	100,000	100,000	N/A	248	N/A	1,002	
Total				500174	39406			0,00000				

Chromatogram

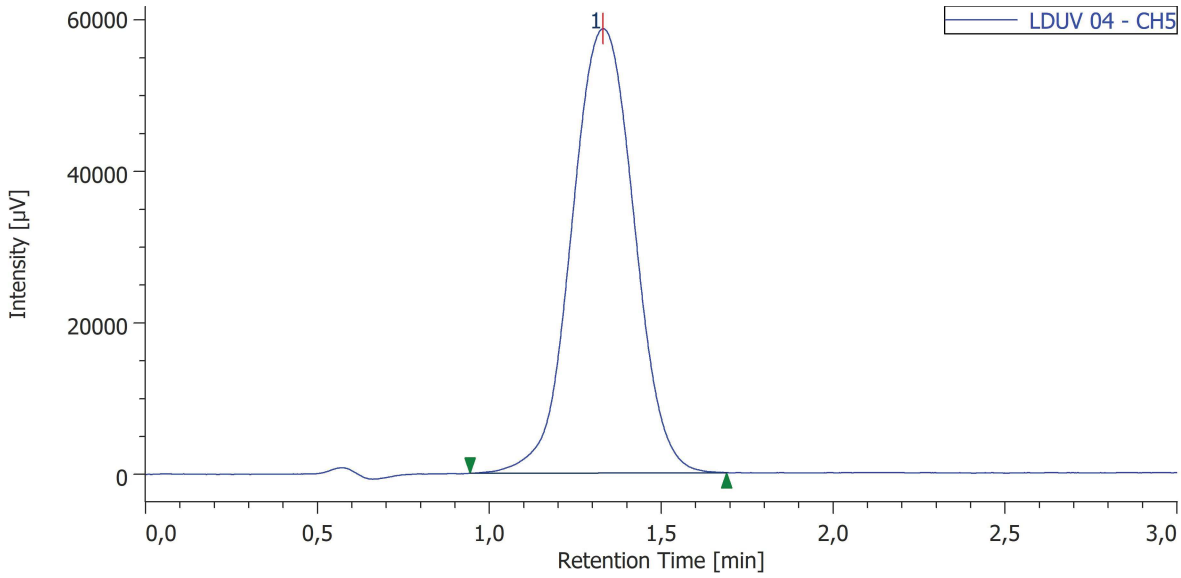


Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 14:27:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 14:16:03
Volume	10,0 [µL]
Sample #	6
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 MD-2018
Control Method	Qualificação MD-2018
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,330	740806	58646	100,000	100,000	N/A	251	N/A	1,002	
Total				740806	58646			0,00000				

Chromatogram

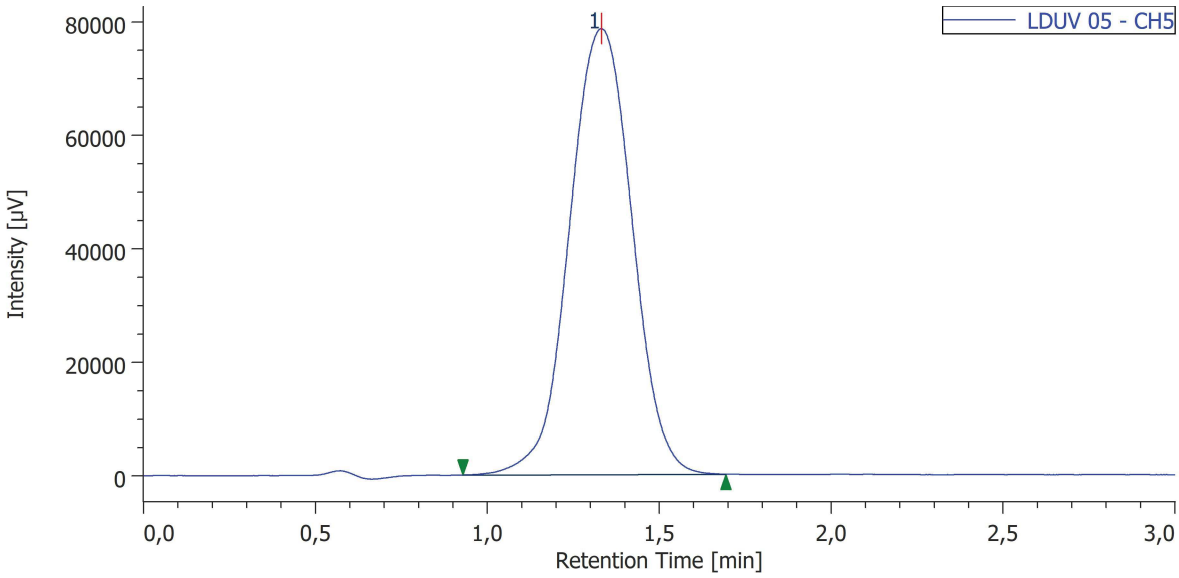

Chromatogram Information	
User Name	Administrator
Date Modified	24/08/2022 14:27:40
Description	
HPLC System Name	HPLC-0003 PDA
Injection Date	24/08/2022 14:19:15
Volume	10,0 [µL]
Sample #	7
Project Name	JASCO
Acquisition Time	3,0 [min]
Acquisition Sequence	OQ HPLC-0003 2022 MD-2018
Control Method	Qualificação MD-2018
Peak ID Table	Cafeina2022
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	100 [msec]
Peak Method	Cafeína

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Unknown	5	1,332	997662	78551	100,000	100,000	N/A	249	N/A	0,991	
Total				997662	78551			0,00000				