HPLC 1260 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1260
- Service & Diagnostics
- Instrument Control
- EMFs
- System Report


Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — HPLC 1260 » HPLC 1260 » G1314F:DEABB11232

Spectral Scan - 1260 VWD [DEABB11232]

UV Lamp On | Blank Scan

Sample Scan | from 190 | to 400 | step 1 | Export Data

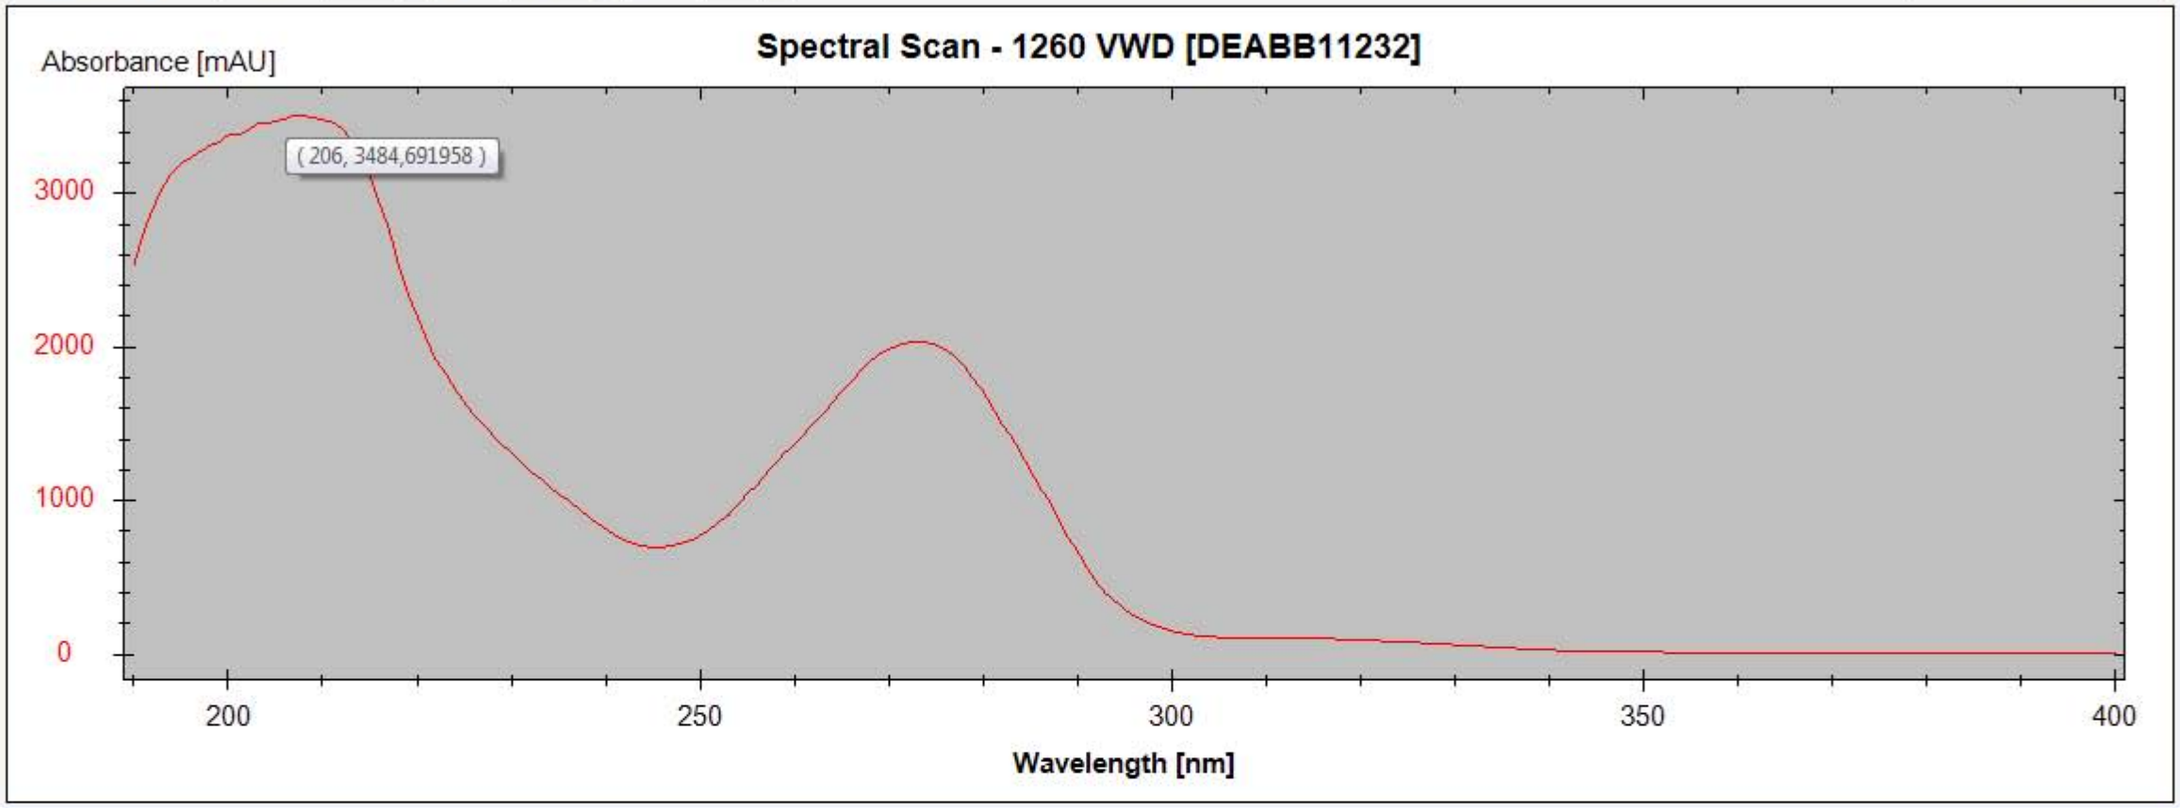

more... | Print Result | Back

Connection Address: 192.168.254.11

Version B.02.05 [114] - Basic | Licenses 4/10

PT 09:29 18/12/2019

HPLC 1260 - Agilent Lab Advisor

Agilent Lab Advisor

Service & Diagnostics

Basic Version

Tasks

Spectral Scan

HPLC 1260 » HPLC 1260 » G1314F:DEABB11232

Lab Advisor

- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1260

- Service & Diagnostics
- Instrument Control
- EMFs
- System Report


Help

- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan - 1260 VWD [DEABB11232]

UV Lamp On | Blank Scan

Sample Scan | from 190 | to 400 | step 1 | Export Data

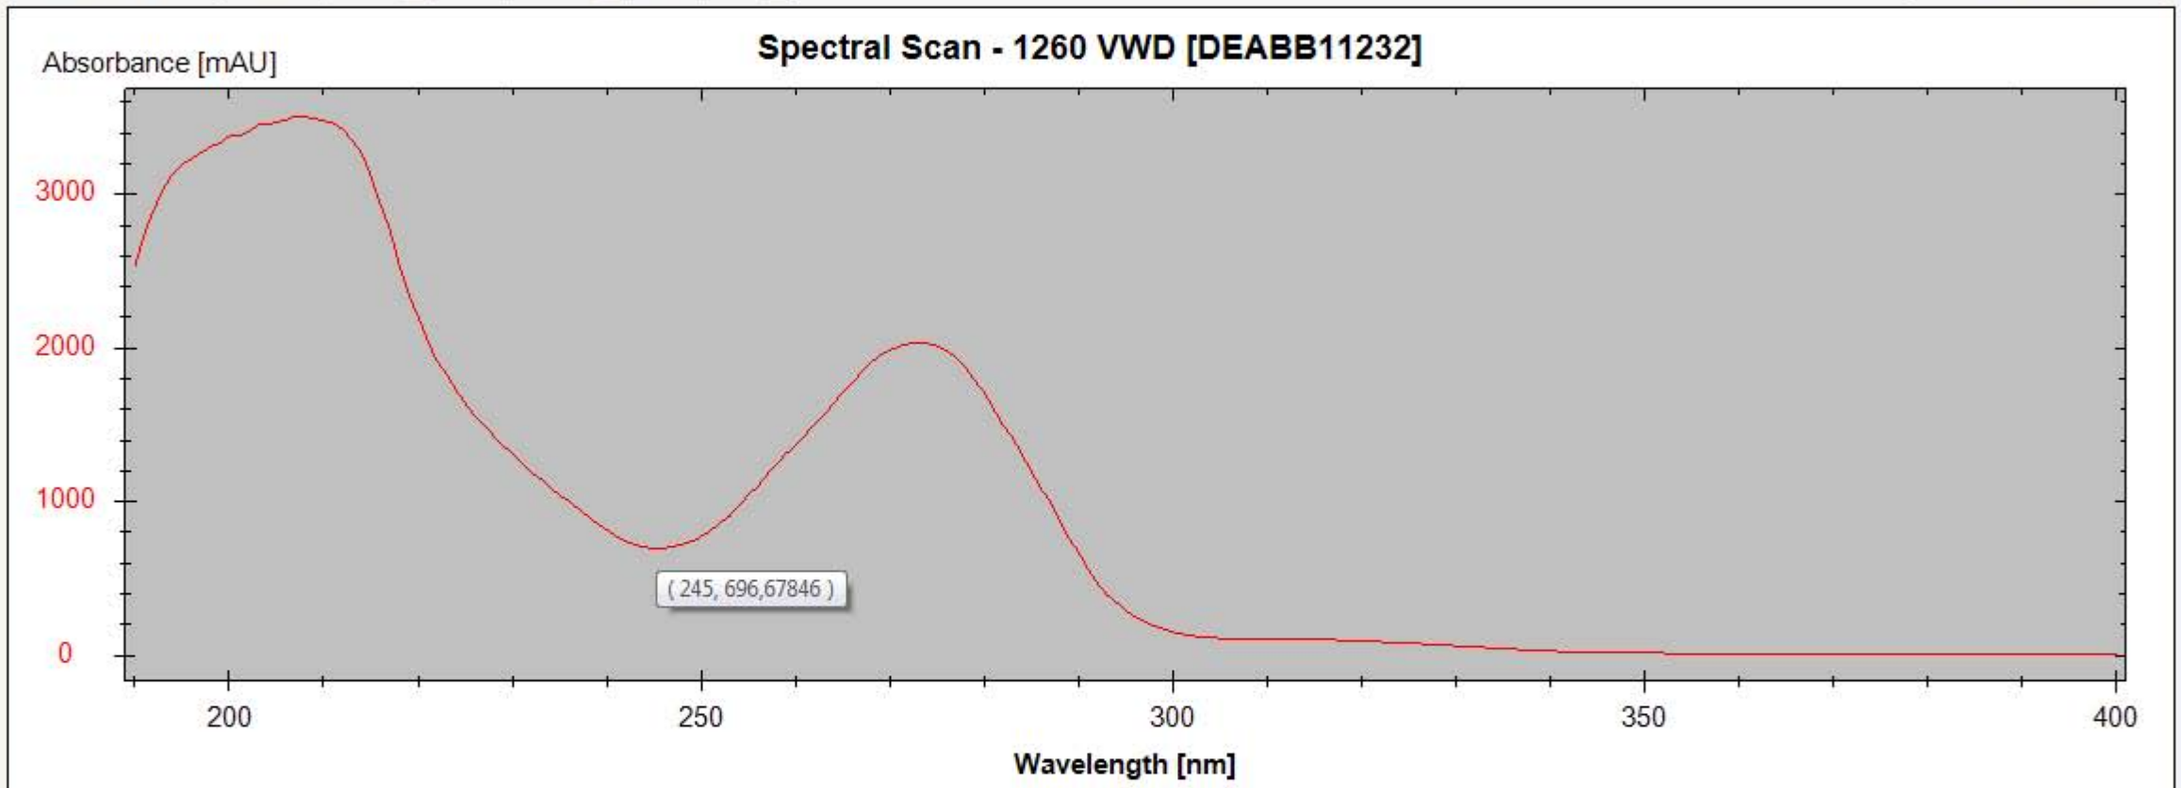

more... | Print Result | Back

Connection Address: 192.168.254.11

Version B.02.05 [114] - Basic | Licenses 4/10

PT 09:30 18/12/2019

HPLC 1260 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results

HPLC 1260
- Service & Diagnostics
- Instrument Control
- EMFs
- System Report


Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — HPLC 1260 » HPLC 1260 » G1314F:DEABB11232

Spectral Scan - 1260 VWD [DEABB11232]

UV Lamp On | Blank Scan

Sample Scan | from 190 | to 400 | step 1 | Export Data

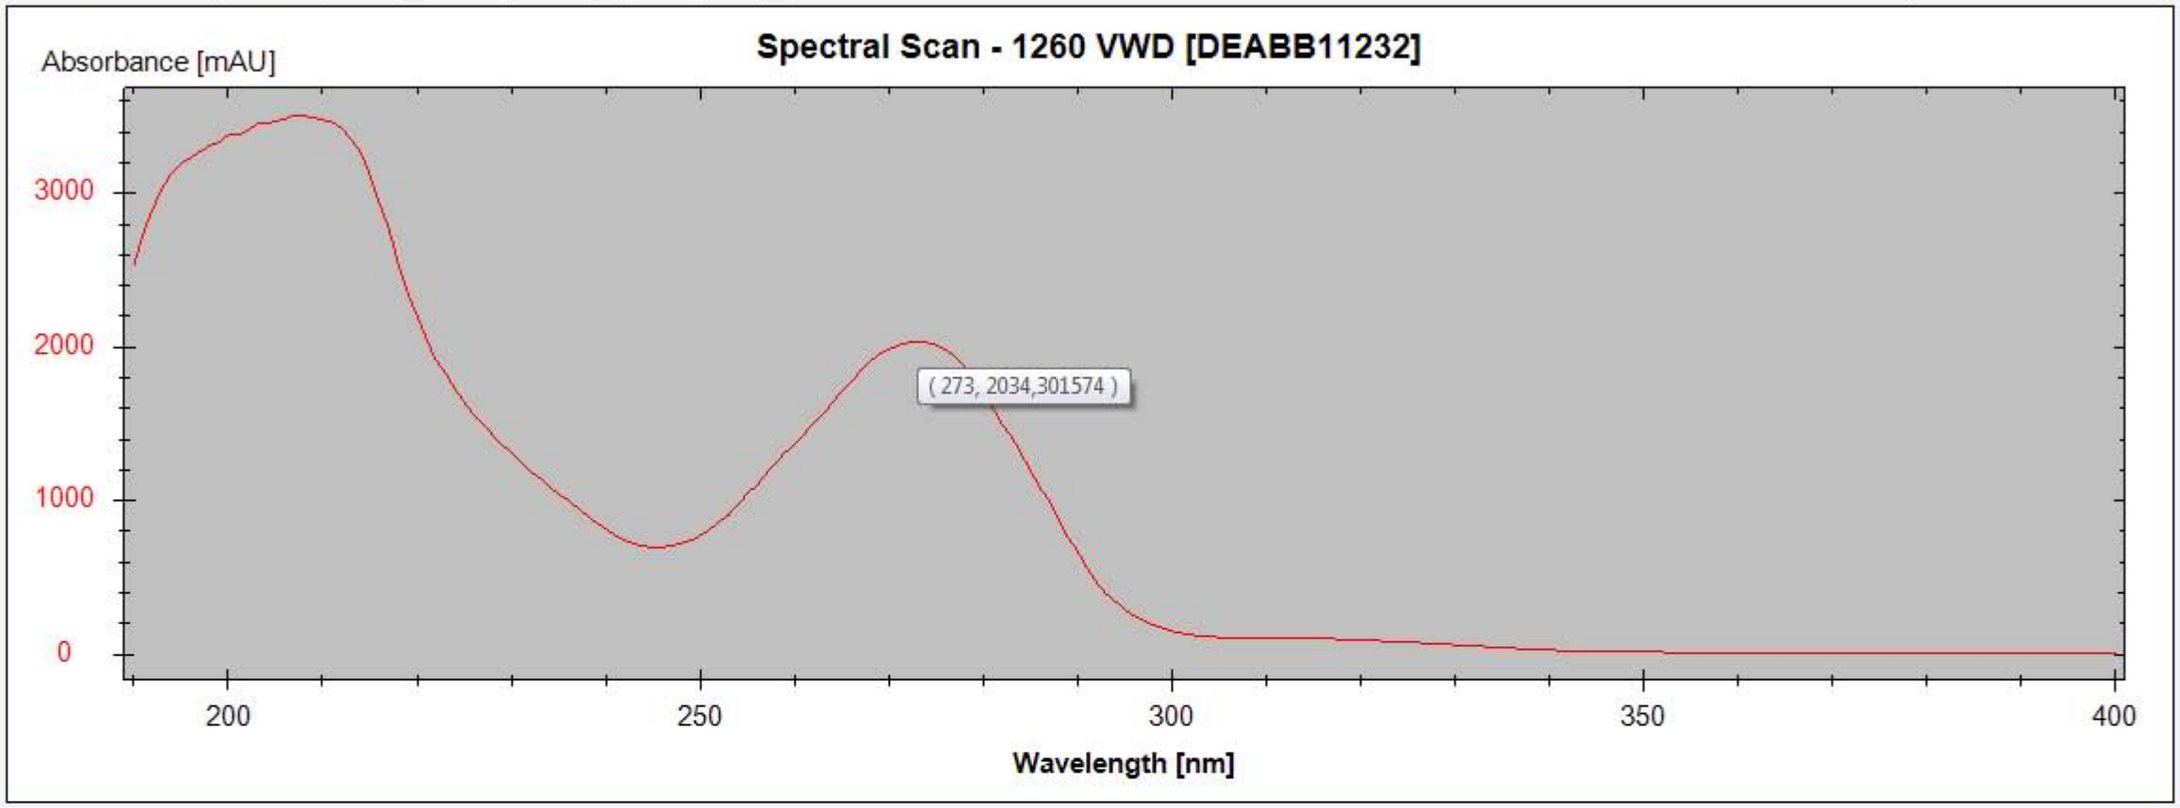

more... | Print Result | Back

Connection Address: 192.168.254.11


Version B.02.05 [114] - Basic | Licenses 4/10

PT 09:30 18/12/2019

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Branco 01.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:06:51 (GMT -03:00)
Printed: 18/12/2019 12:40:33 (GMT -03:00)

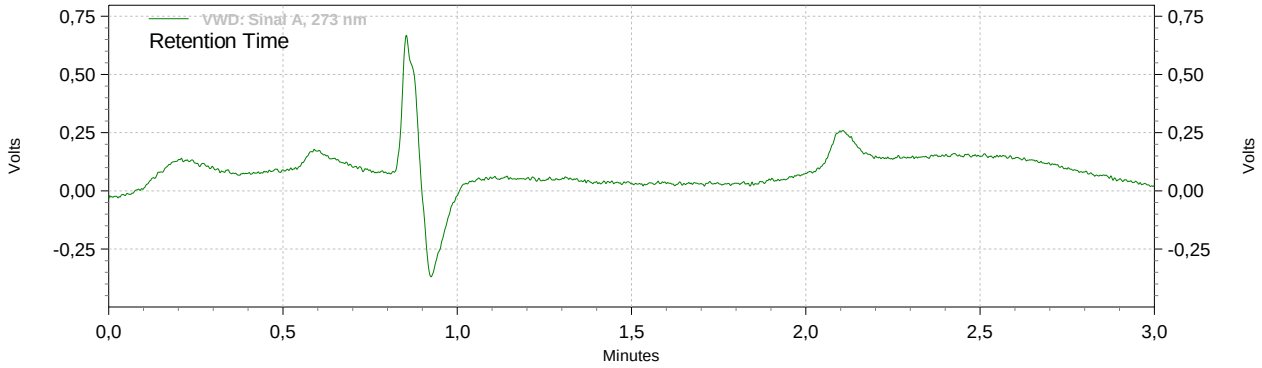


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Branco 02
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:22:35 (GMT -03:00)
Printed: 18/12/2019 12:49:30 (GMT -03:00)

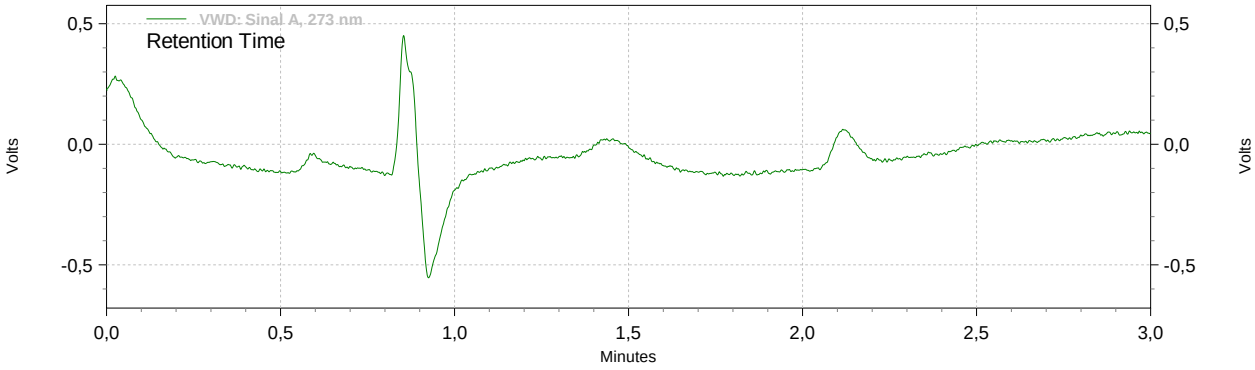


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Branco 03
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:38:22 (GMT -03:00)
Printed: 18/12/2019 12:51:03 (GMT -03:00)

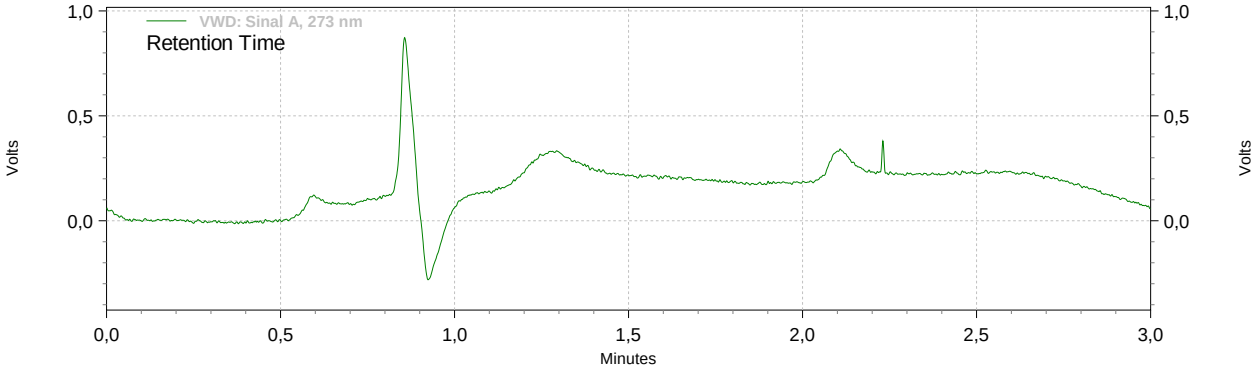


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\GRADIENTE AC.rslt\GRADIENTE AC.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Method\Gradiente AC013.met
Acquired: 18/12/2019 15:42:47 (GMT -03:00)
Printed: 18/12/2019 15:56:47 (GMT -03:00)

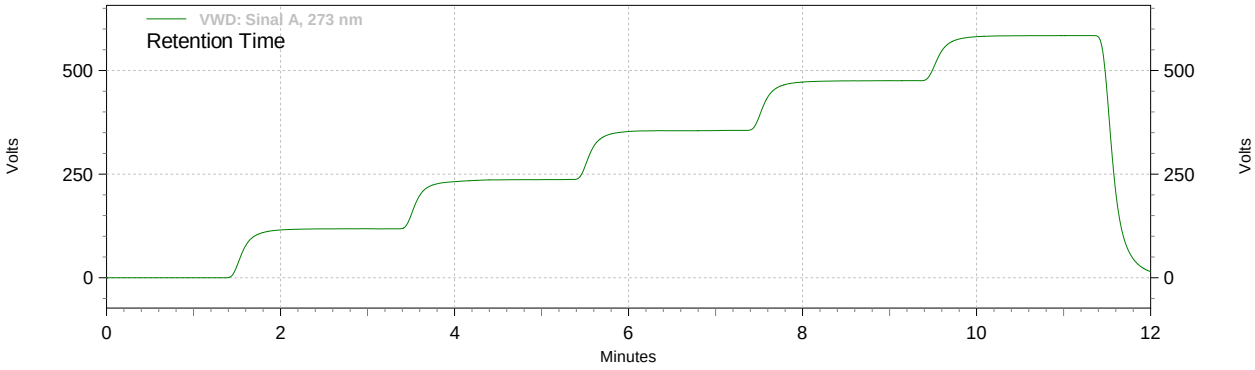


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\LDUV 01.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:11:49 (GMT -03:00)
Printed: 18/12/2019 14:52:17 (GMT -03:00)

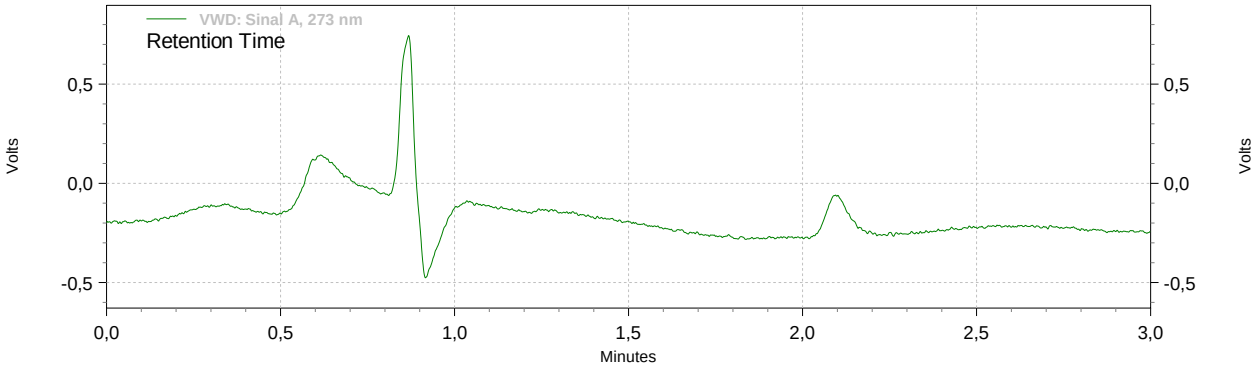


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\LDUV 02.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:15:49 (GMT -03:00)
Printed: 18/12/2019 14:52:41 (GMT -03:00)

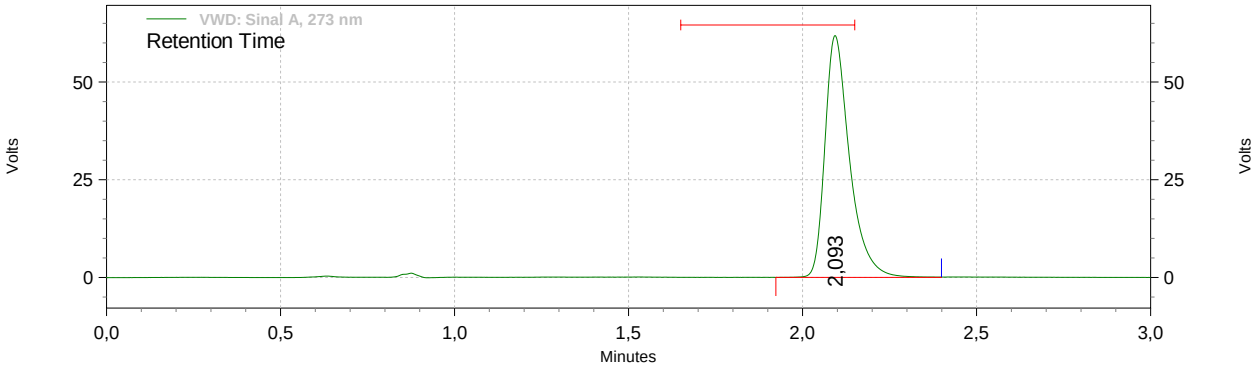

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,093	5115148	100,00	1037737	100,00

Totals	5115148	100,00	1037737	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\LDUV 03.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:19:46 (GMT -03:00)
Printed: 18/12/2019 14:53:07 (GMT -03:00)

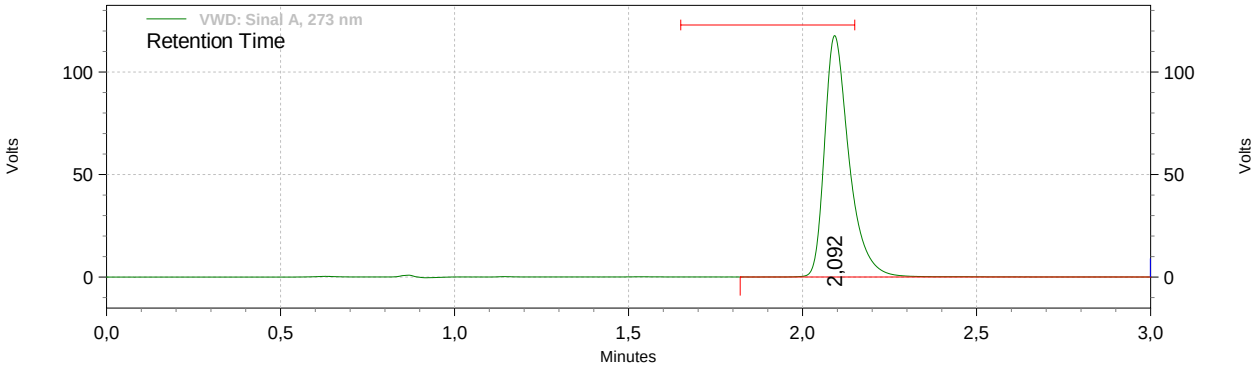

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,092	9714779	100,00	1974686	100,00

Totals	9714779	100,00	1974686	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\LDUV 04.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:23:46 (GMT -03:00)
Printed: 18/12/2019 14:53:27 (GMT -03:00)

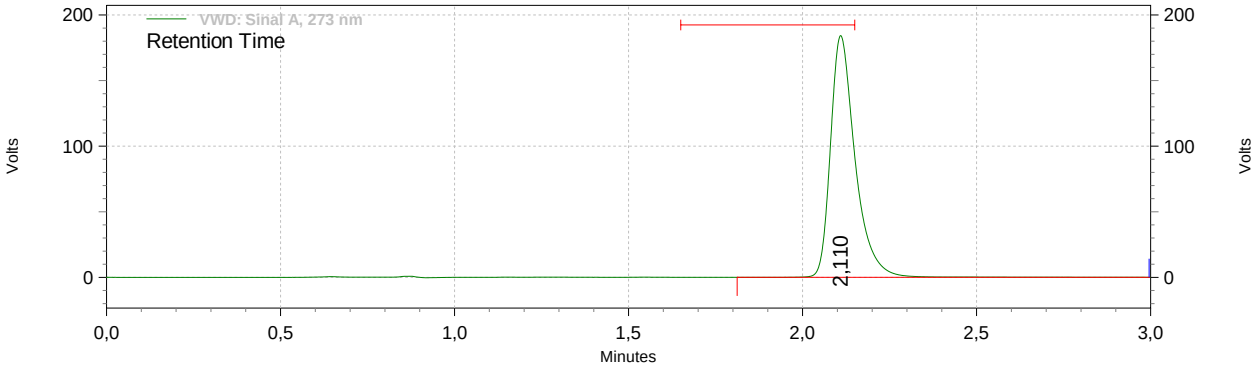

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,110	15210743	100,00	3090849	100,00

Totals	15210743	100,00	3090849	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\LDUV 05.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LVUV_LIIN002.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:27:45 (GMT -03:00)
Printed: 18/12/2019 14:53:42 (GMT -03:00)

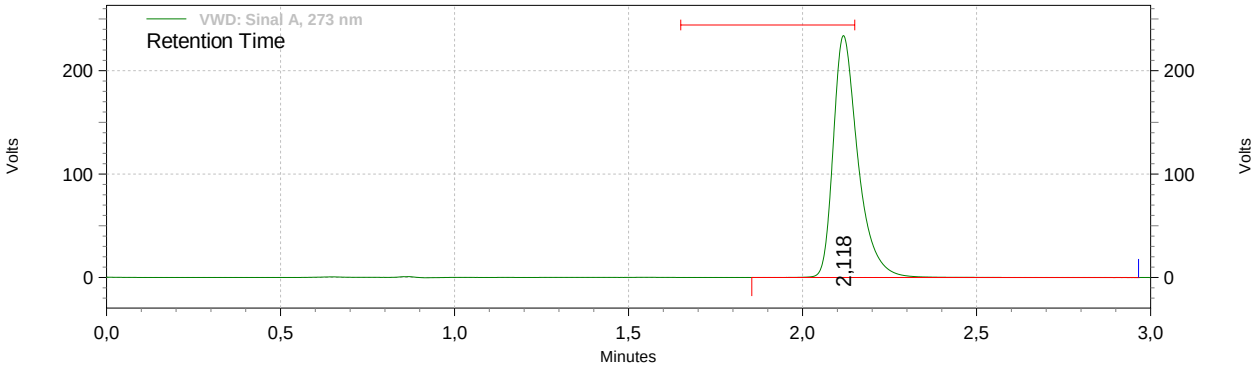

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,118	19402176	100,00	3925533	100,00

Totals	19402176	100,00	3925533	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\LIIN 001.dat
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:55:34 (GMT -03:00)
Printed: 18/12/2019 15:31:43 (GMT -03:00)

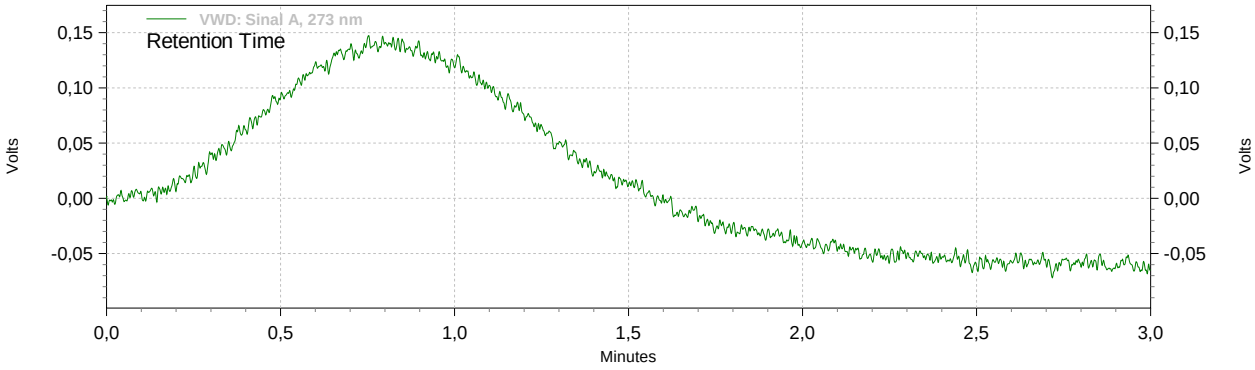


VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\LIIN 002
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\Qualificação 2019.met
Acquired: 18/12/2019 14:59:33 (GMT -03:00)
Printed: 18/12/2019 15:32:11 (GMT -03:00)

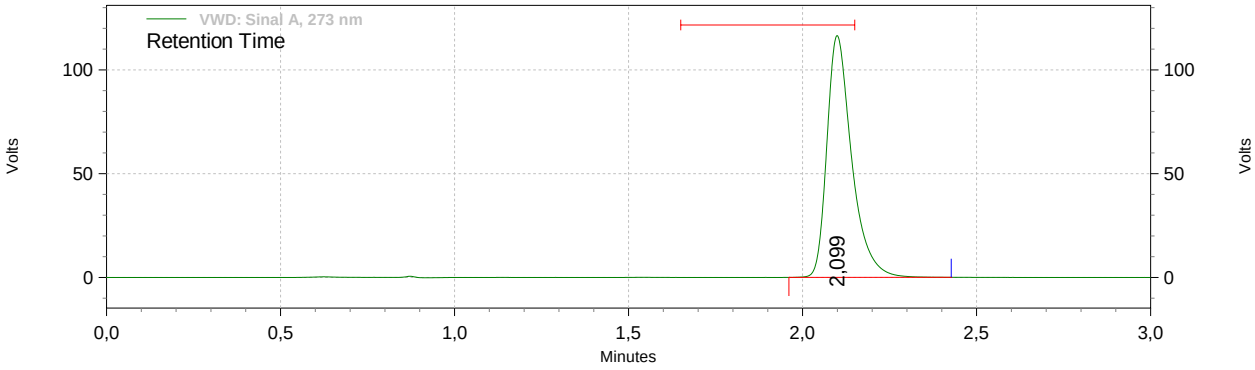

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,099	9680803	100,00	1954216	100,00

Totals	9680803	100,00	1954216	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\LIIN 003
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\Qualificação 2019.met
Acquired: 18/12/2019 15:03:30 (GMT -03:00)
Printed: 18/12/2019 15:32:45 (GMT -03:00)

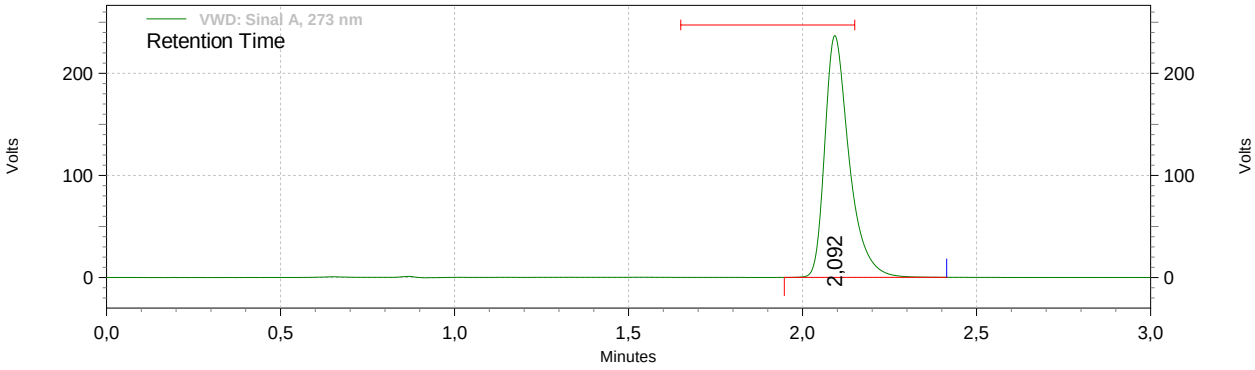

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,092	19339706	100,00	3973272	100,00

Totals	19339706	100,00	3973272	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\LIIN 004
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\Qualificação 2019.met
Acquired: 18/12/2019 15:07:31 (GMT -03:00)
Printed: 18/12/2019 15:33:05 (GMT -03:00)

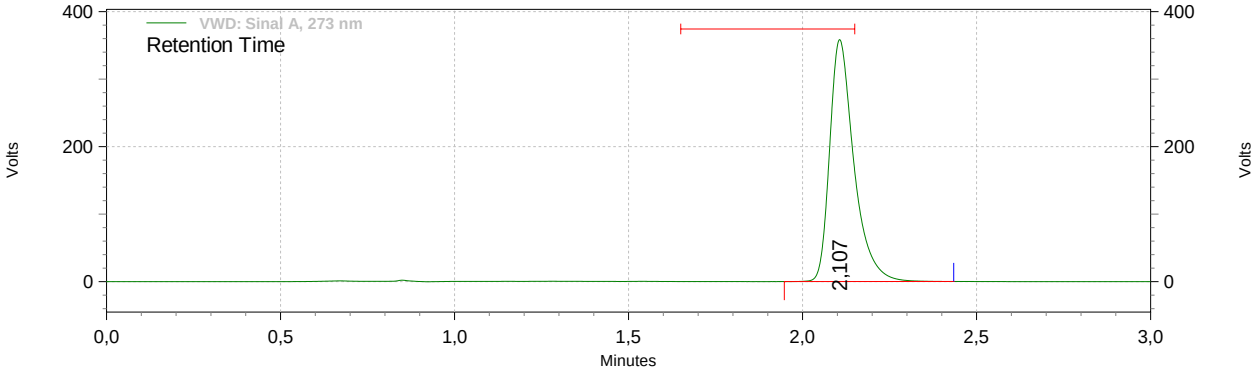

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,107	29104594	100,00	6013565	100,00

Totals	29104594	100,00	6013565	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\LIIN 005
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\LIIN005.rslt\Qualificação 2019.met
Acquired: 18/12/2019 15:11:34 (GMT -03:00)
Printed: 18/12/2019 15:33:18 (GMT -03:00)

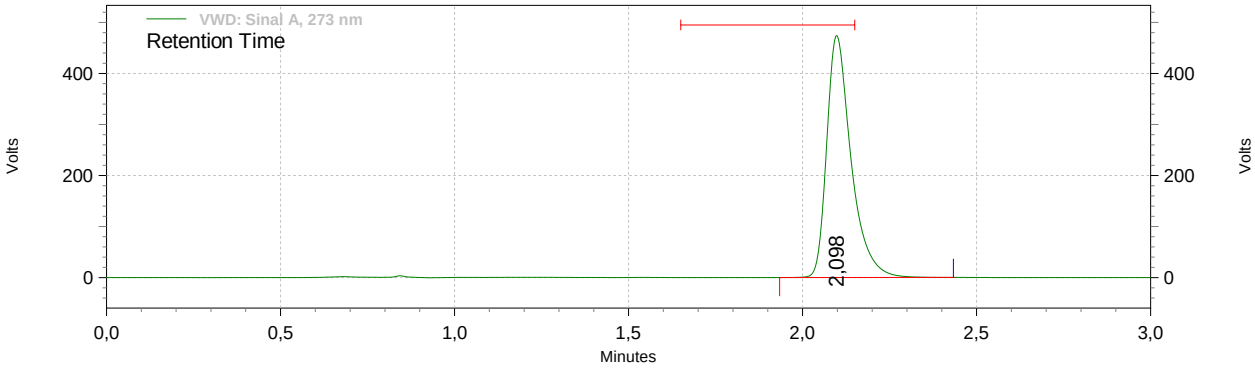

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,098	38666574	100,00	7951928	100,00

Totals	38666574	100,00	7951928	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 01
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:10:47 (GMT -03:00)
Printed: 18/12/2019 12:48:15 (GMT -03:00)

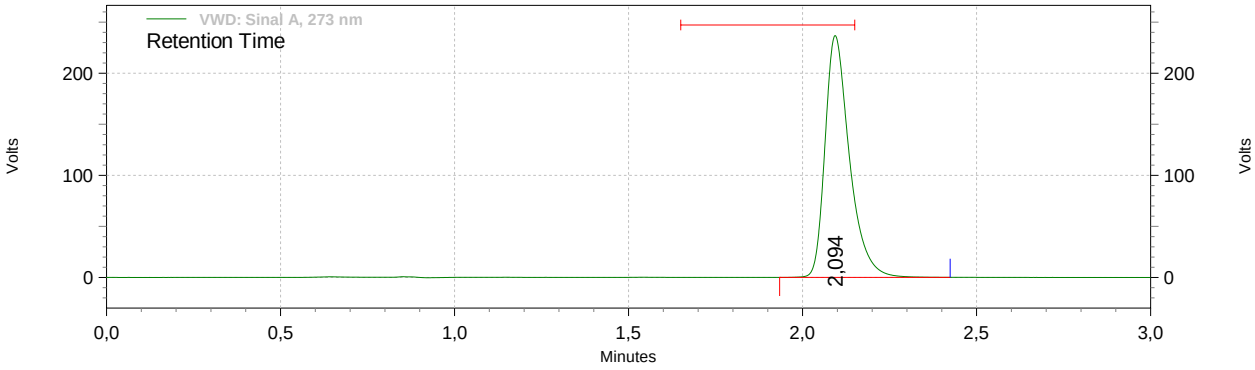

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,094	19394980	100,00	3972378	100,00

Totals	19394980	100,00	3972378	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 02
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:14:41 (GMT -03:00)
Printed: 18/12/2019 12:48:52 (GMT -03:00)

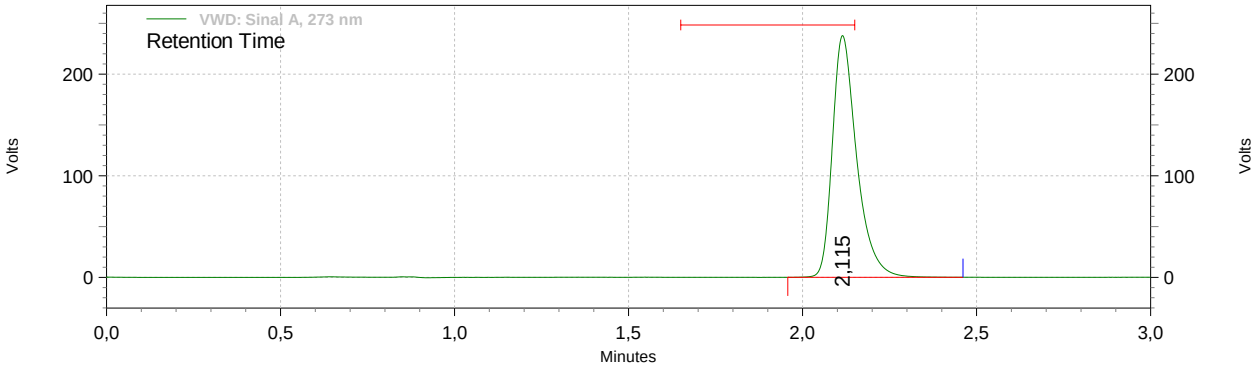

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,115	19402422	100,00	3990443	100,00

Totals	19402422	100,00	3990443	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 03
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:18:37 (GMT -03:00)
Printed: 18/12/2019 12:49:12 (GMT -03:00)

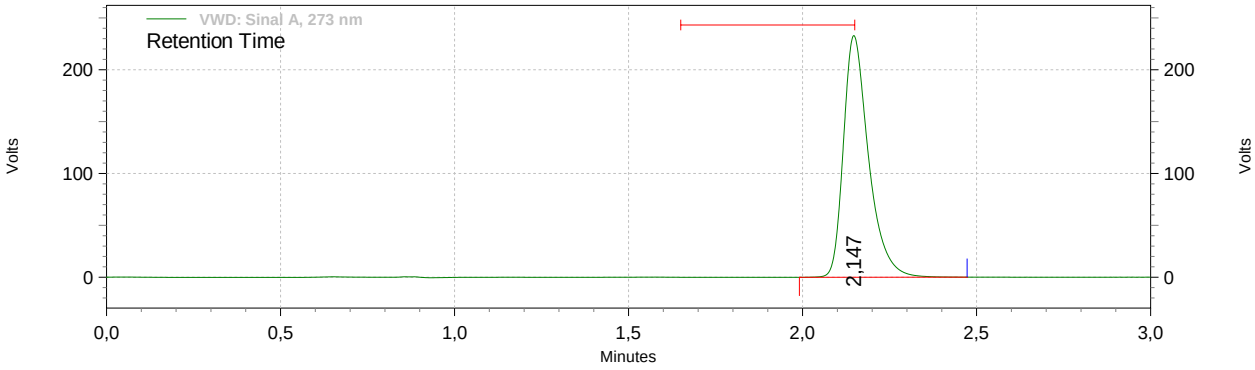

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,147	19636062	100,00	3908777	100,00

Totals	19636062	100,00	3908777	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 04
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:26:29 (GMT -03:00)
Printed: 18/12/2019 12:49:42 (GMT -03:00)

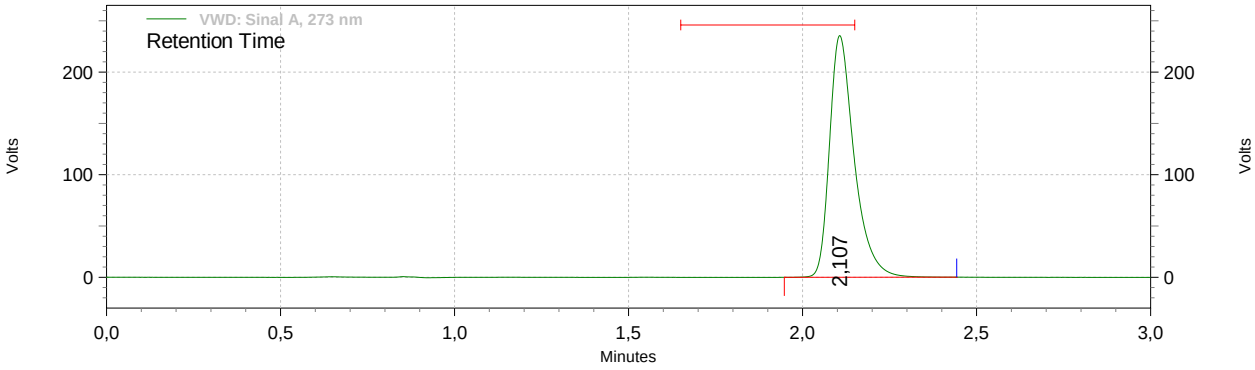

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,107	19482959	100,00	3952248	100,00

Totals	19482959	100,00	3952248	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 05
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:30:26 (GMT -03:00)
Printed: 18/12/2019 12:50:01 (GMT -03:00)

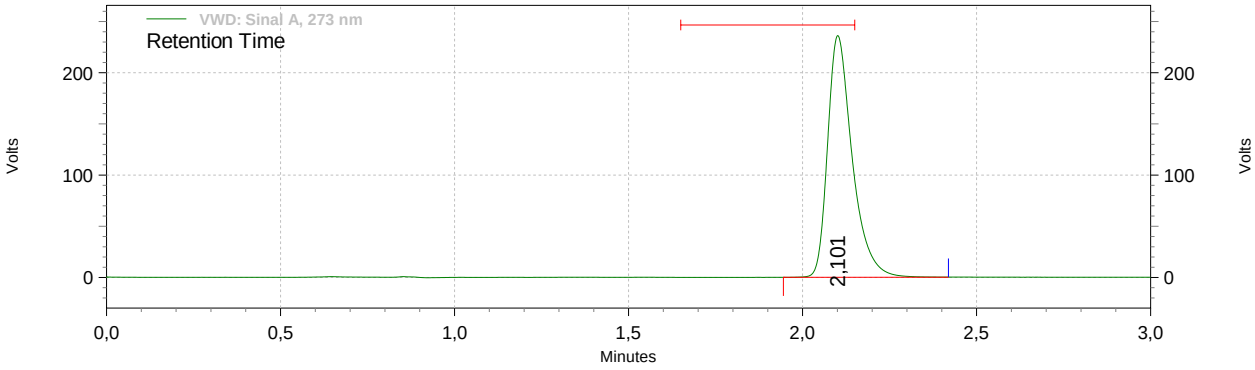

VWD: Sinal A, 273 nm Results


Retention Time	Area	Area %	Height	Height %
2,101	19481441	100,00	3960898	100,00

Totals	19481441	100,00	3960898	100,00

PDF-XChange
Click to buy NOW!
www.tracker-software.com

Area % Report

Data File: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\PCIN 06
Method: C:\Enterprise\Projects\Qualificação HPLC\Result\PCIN03.rslt\Qualificação 2019.met
Acquired: 18/12/2019 12:34:23 (GMT -03:00)
Printed: 18/12/2019 12:50:20 (GMT -03:00)

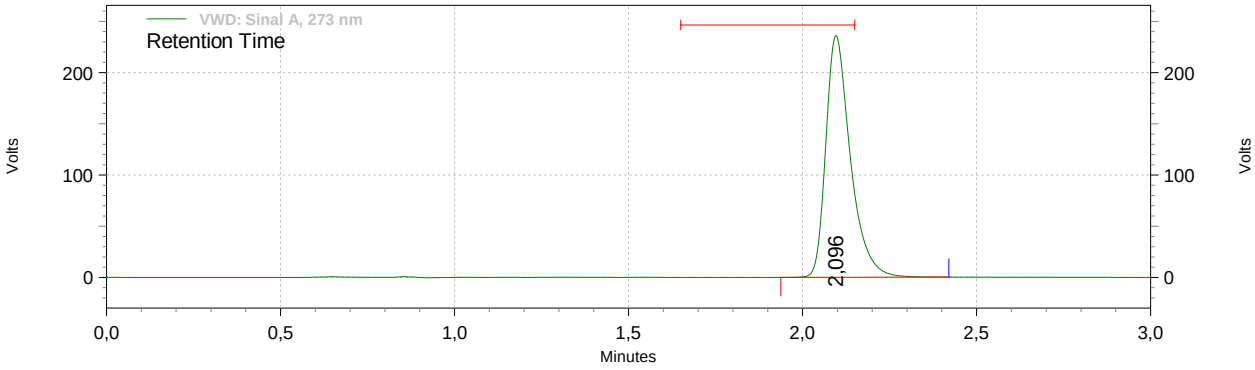

VWD: Sinal A, 273 nm Results

Retention Time	Area	Area %	Height	Height %
2,096	19440976	100,00	3959354	100,00

Totals	19440976	100,00	3959354	100,00