
Peak Find - Exatidão Do Comprimento De Onda.jws

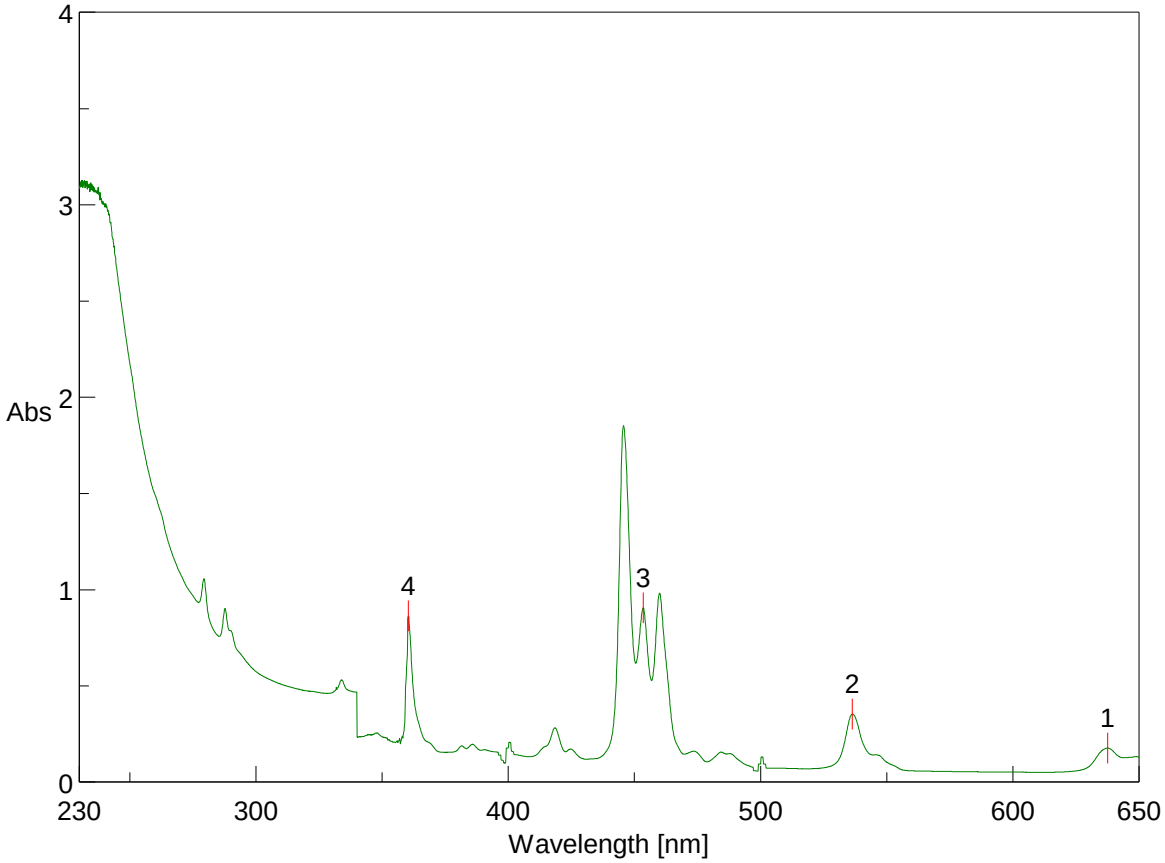

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 08:59
Date modified	7/7/2023 08:59
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	650 nm
End	230 nm
Data interval	0.1 nm
Data points	4201


[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Exatidão Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	650 - 230 nm
Data pitch	0.1 nm
Band width(UV/Vis)	1.5 nm
Response	Fast
Scanning speed	40 nm/min
Source change	340 nm
Light source	D2/WI

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	637.6	0.175886	2	536.4	0.352772
3	453.5	0.904533	4	360.4	0.86296

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 1.jws

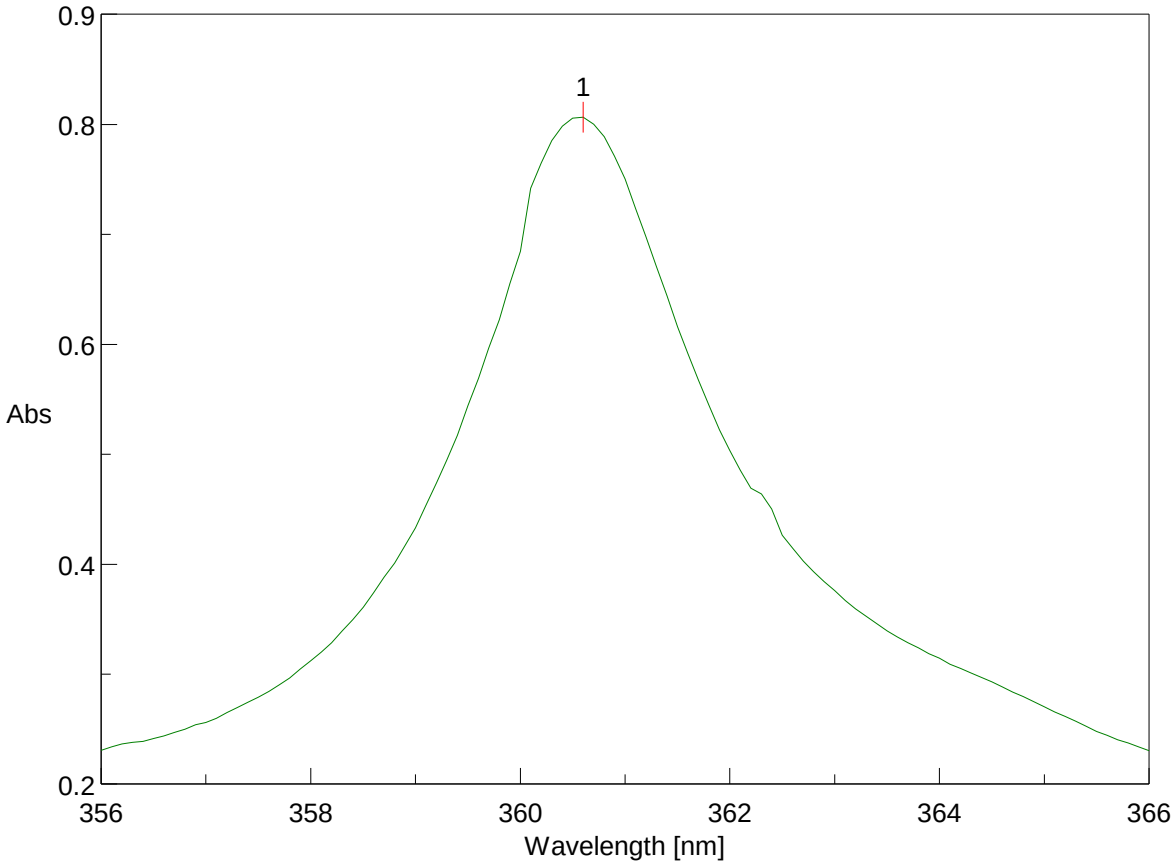

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 09:05
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101


[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data pitch	0.1 nm
Band width(UV/Vis)	1.5 nm
Response	Fast
Scanning speed	40 nm/min
Source change	340 nm
Light source	D2/WI

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.6	0.806209			

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 2.jws

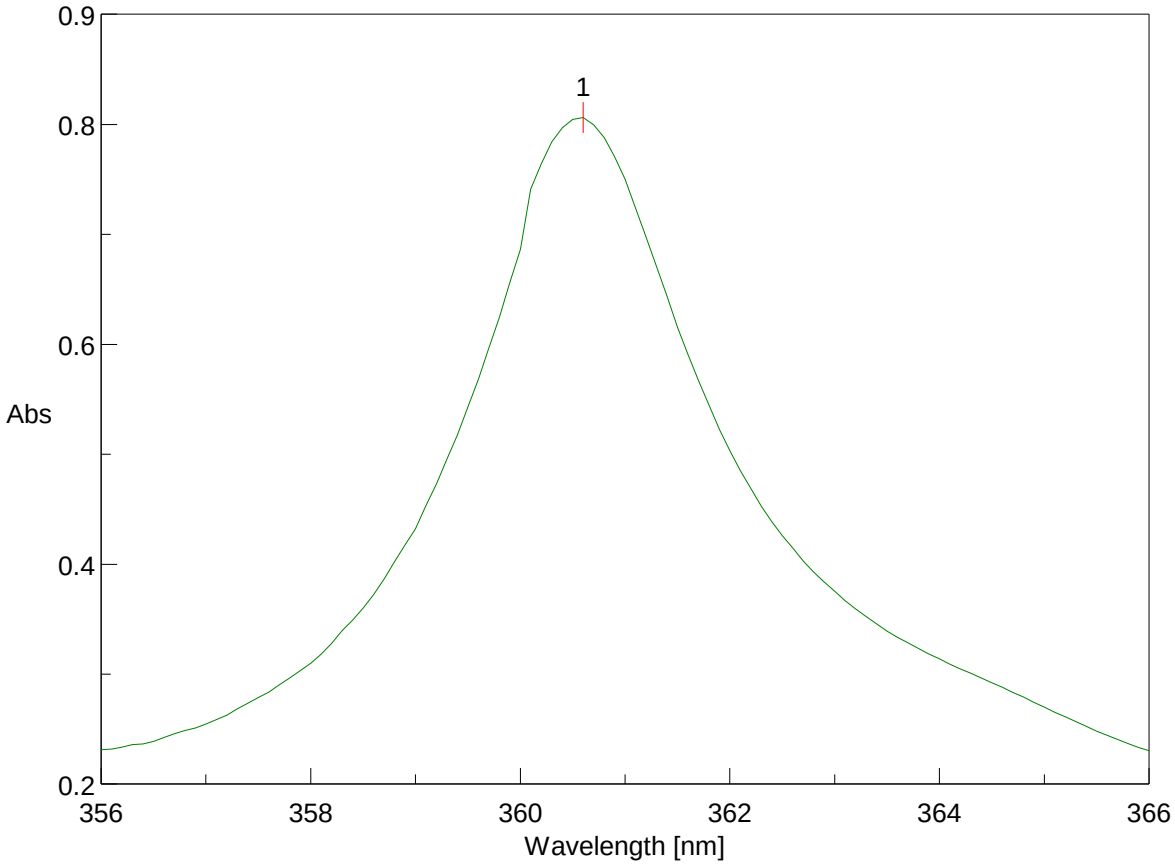

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 09:05
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101


[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data pitch	0.1 nm
Band width(UV/Vis)	1.5 nm
Response	Fast
Scanning speed	40 nm/min
Source change	340 nm
Light source	D2/WI

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.6	0.806022			

Peak Find - Repetibilidade Do Comprimento De Onda - Rep. 3.jws

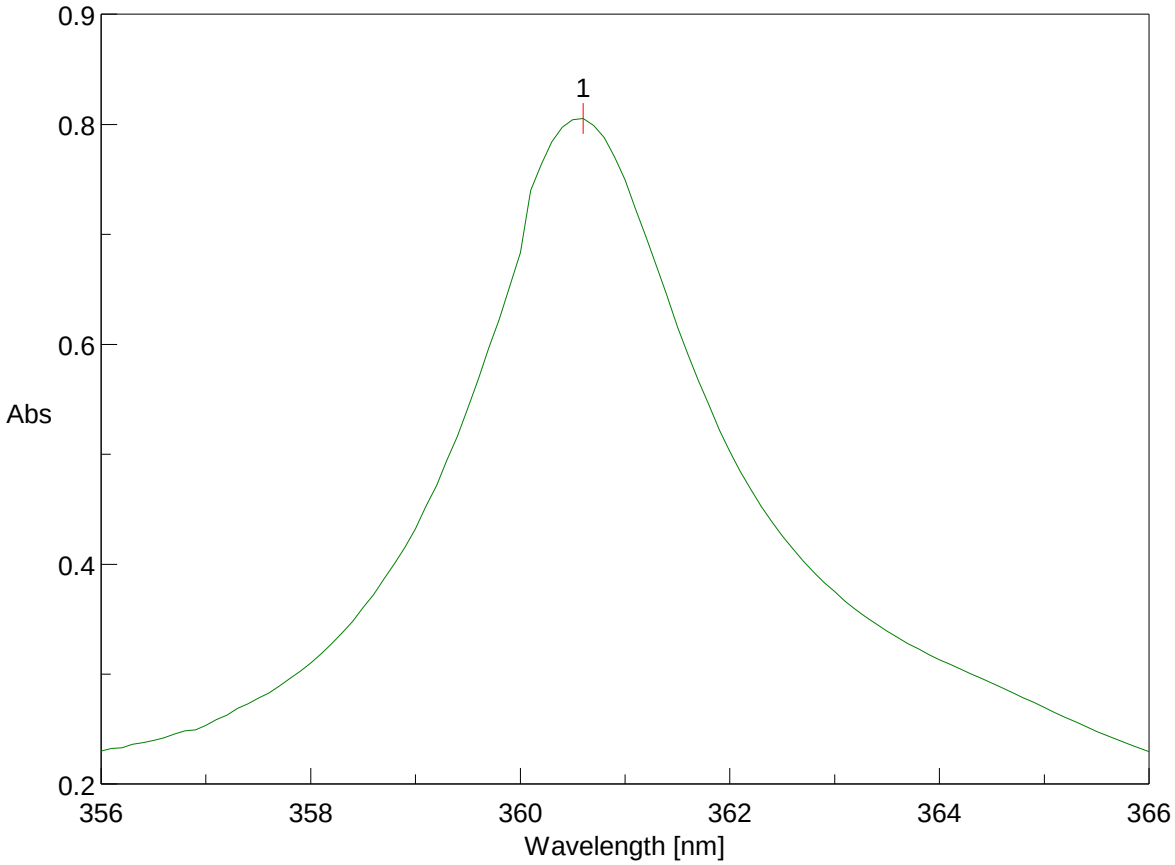

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 09:05
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	366 nm
End	356 nm
Data interval	0.1 nm
Data points	101


[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Repetibilidade Do Comprimento De Onda.uvsp
Photometric mode	Abs
Measurement range	366 - 356 nm
Data pitch	0.1 nm
Band width(UV/Vis)	1.5 nm
Response	Fast
Scanning speed	40 nm/min
Source change	340 nm
Light source	D2/WI

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	360.6	0.804979			

Full Width at Half Maximum - Resolução.jws

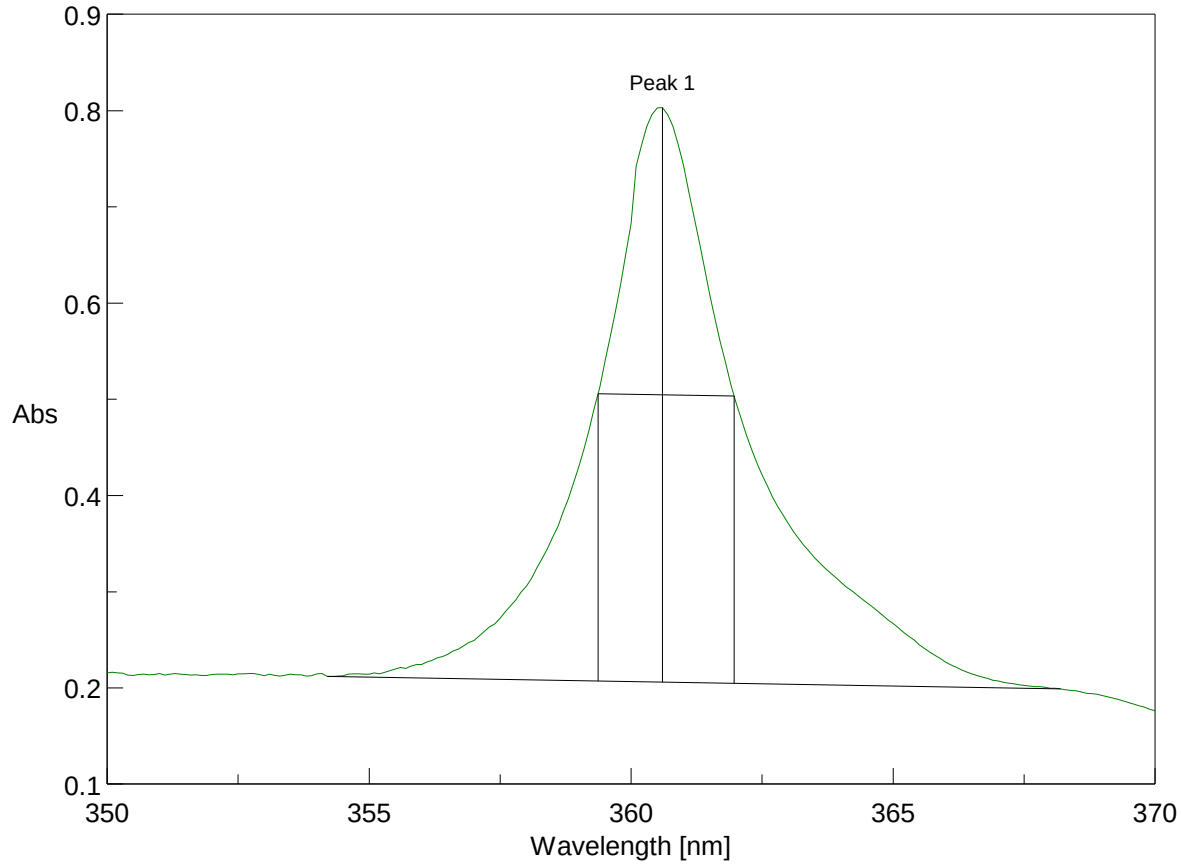

[Result of FWHM Calculation]

Base 1	Base 2	Peak	Height	FWHM
368.2	354.2	360.6	0.596836	2.59759

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 09:10
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	370 nm
End	350 nm
Data interval	0.1 nm
Data points	201

[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Resolução.uvsp
Photometric mode	Abs
Measurement range	370 - 350 nm
Data pitch	0.1 nm
Band width(UV/Vis)	1.5 nm
Response	Fast
Scanning speed	40 nm/min
Source change	340 nm
Light source	D2/WI
Filter exchange	Step

Exatidão Fotométrica.ufwd

Sheet Name
Comment

User
Division
Company IBERO MAGISTRAL

Creation date 7/7/2023 09:14

Instrument name V-630
Model name V-630
Serial No. A061661148
ROM version 1.40.01

Accessory USE-753
Accessory S/N A061661148
Cell length 10 mm

Parameter file C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Abs3\Exatidão Fotométrica.uvfw
Photometric mode
Band width(UV/Vis) 1.5 nm
Response Medium
Wavelength-1 440.0 nm
Source change 340 nm
Light source D2/WI
Dark correction Off

No.	Mode	Sample Name	Comment	440.0 nm
1	Sample-1	F2	F2	0.2673
2	Sample-2	F3	F3	0.5240
3	Sample-3	F4	F4	1.0975

Repetibilidade Fotométrica.ufwd

Sheet Name
Comment

User
Division
Company IBERO MAGISTRAL

Creation date 7/7/2023 09:18


Instrument name V-630
Model name V-630
Serial No. A061661148
ROM version 1.40.01

Accessory USE-753
Accessory S/N A061661148
Cell length 10 mm

Parameter file C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Abs3\Repetibilidade Fotométrica.uvfw
Photometric mode
Band width(UV/Vis) 1.5 nm
Response Medium
Wavelength-1 361.0 nm
Source change 340 nm
Light source D2/WI
Dark correction Off

No.	Mode	Sample Name	Comment	361.0 nm
1	Sample-1	Rep. 1	Rep. 1	0.6622
2	Sample-2	Rep. 2	Rep. 2	0.6622
3	Sample-3	Rep. 3	Rep. 3	0.6620

Peak Find - Estabilidade Da Linha De Base.jws

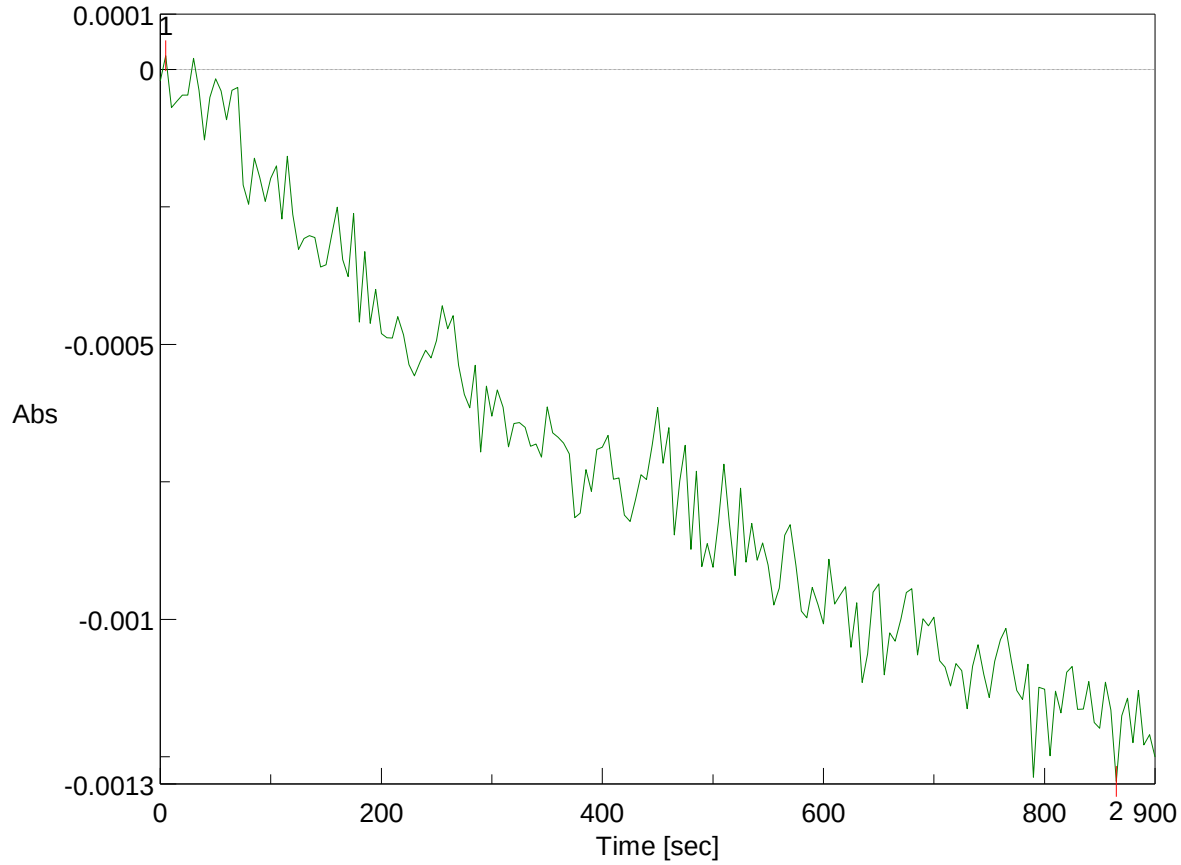

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 09:39
Data array type	Linear data array
Horizontal axis	Time [sec]
Vertical axis	Abs
Start	0 sec
End	900 sec
Data interval	5 sec
Data points	181


[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Estabilidade Da Linha De Base.uvtm
Photometric mode	Abs
Measurement range	0 - 900 sec
Data pitch	5 sec
Band width(UV/Vis)	1.5 nm
Response	Slow
Monitor wavelength	250 nm
Source change	340 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	5	2.43807E-005	2	865	-0.0012951

Peak Find - Uniformidade Da Linha De Base.jws

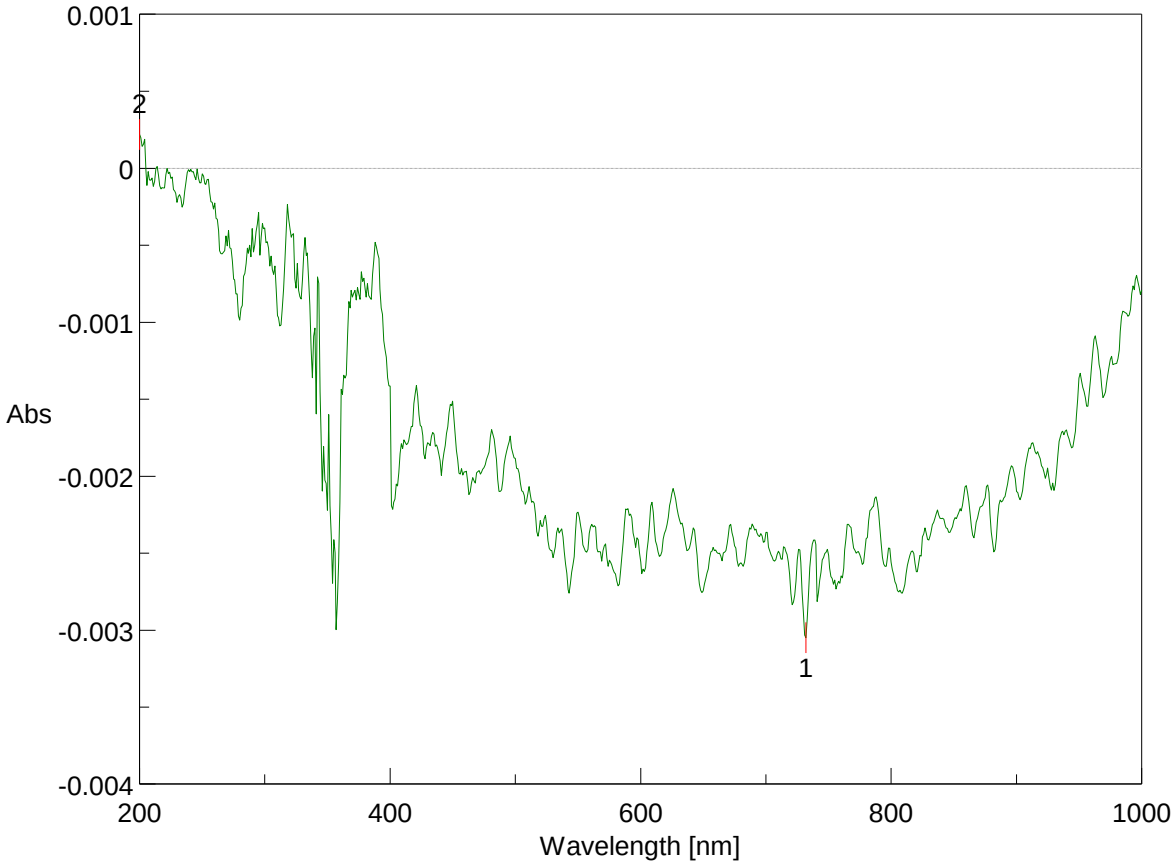

[Comments]
Sample name
Comment
User
Division
Company IBERO MAGISTRAL

[Detailed Information]

Creation date	7/7/2023 10:03
Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	1000 nm
End	200 nm
Data interval	1 nm
Data points	801

[Measurement Information]

Instrument name	V-630
Model name	V-630
Serial No.	A061661148
Accessory	USE-753
Accessory S/N	A061661148
Cell length	10 mm
Parameter file	C:\Documents and Settings\larissa.ferreira.IBEROMAGISTRAL\Desktop\01-09-0029 - Qualificação - 07.07.2023\Uniformidade Da Linha De Base.uvsp
Photometric mode	Abs
Measurement range	1000 - 200 nm
Data pitch	1 nm
Band width(UV/Vis)	1.5 nm
Response	Medium
Scanning speed	400 nm/min
Source change	340 nm
Light source	D2/WI

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	732	-0.00305053	2	200	0.0002182