SAL-0166 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results


SAL-0166
- Service & Diagnostics
- Instrument Control
- EMFs
- Firmware Update Report
- System Report

Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — SAL-0166 » SAL-0166 » G1365D:DEAAZ01095

Spectral Scan - 1260 MWD VL [DEAAZ01095]

UV Lamp On | Sample Scan | from 200 | to 300 | step 1.0 | Export Data

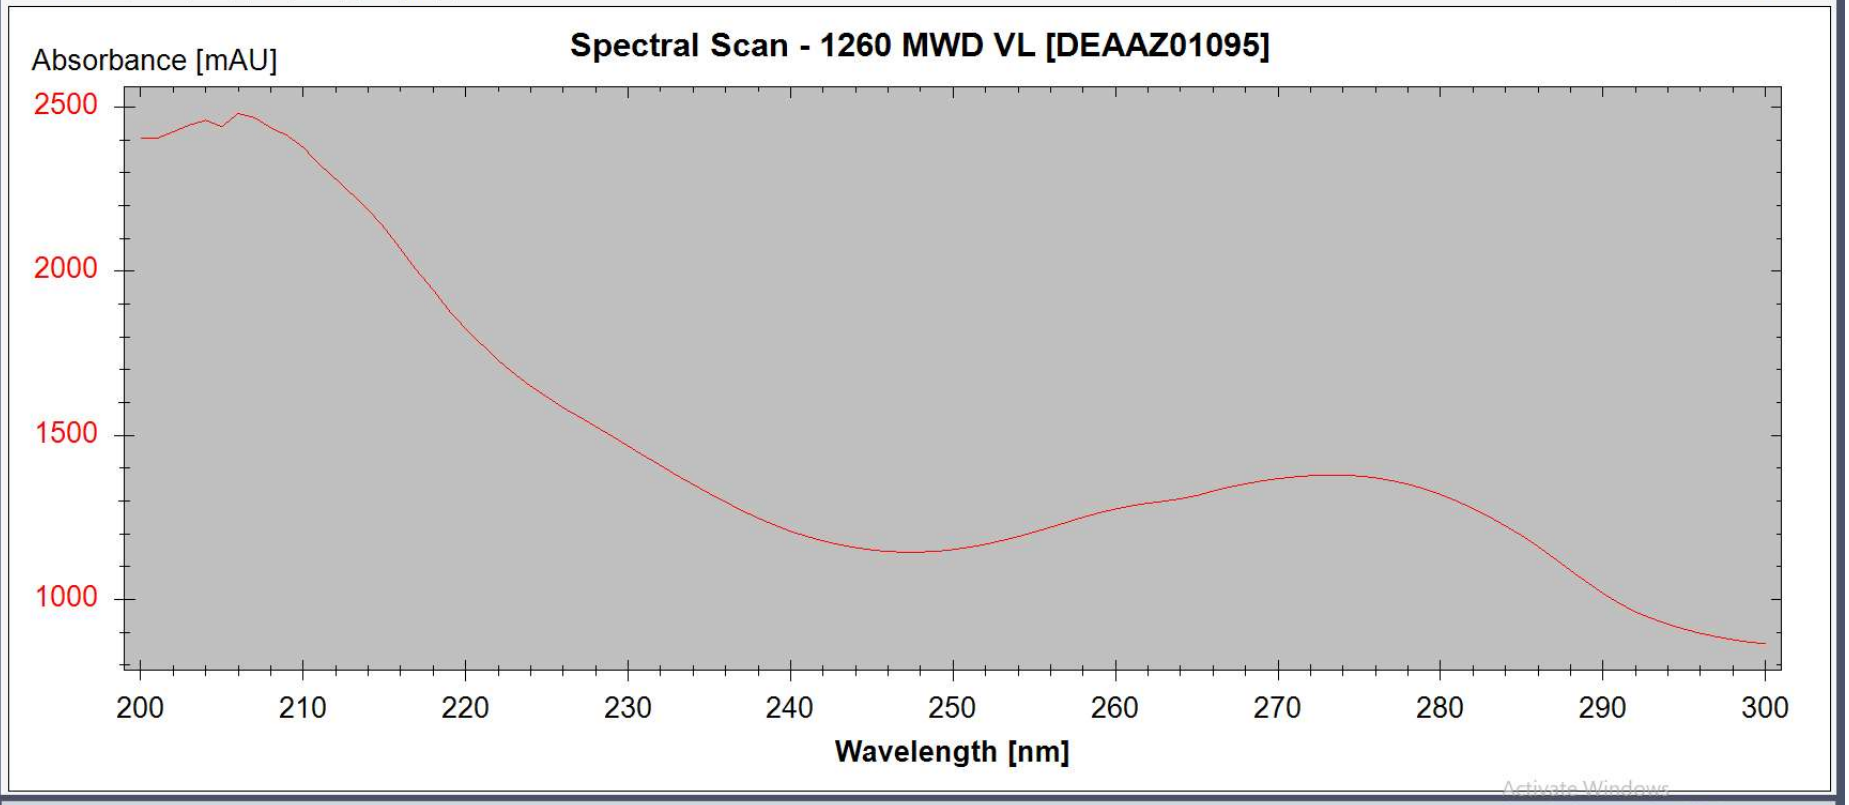

Activate Windows
Go to Settings to activate Windows.

more... | Print Result | Back

Connection Address: 192.168.0.253

Version 2.18.479 - Basic | Licenses 8/20

Type here to search
SAL-0315 - Acquisit...
SAL-0166 - Agilent ...
64°F Windy
POR PTB2 10:29 AM 7/19/2023

SAL-0166 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results


SAL-0166
- Service & Diagnostics
- Instrument Control
- EMFs
- Firmware Update Report
- System Report

Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — SAL-0166 » SAL-0166 » G1365D:DEAAZ01095

Spectral Scan - 1260 MWD VL [DEAAZ01095]

UV Lamp On | Sample Scan | from 200 | to 300 | step 1.0 | Export Data

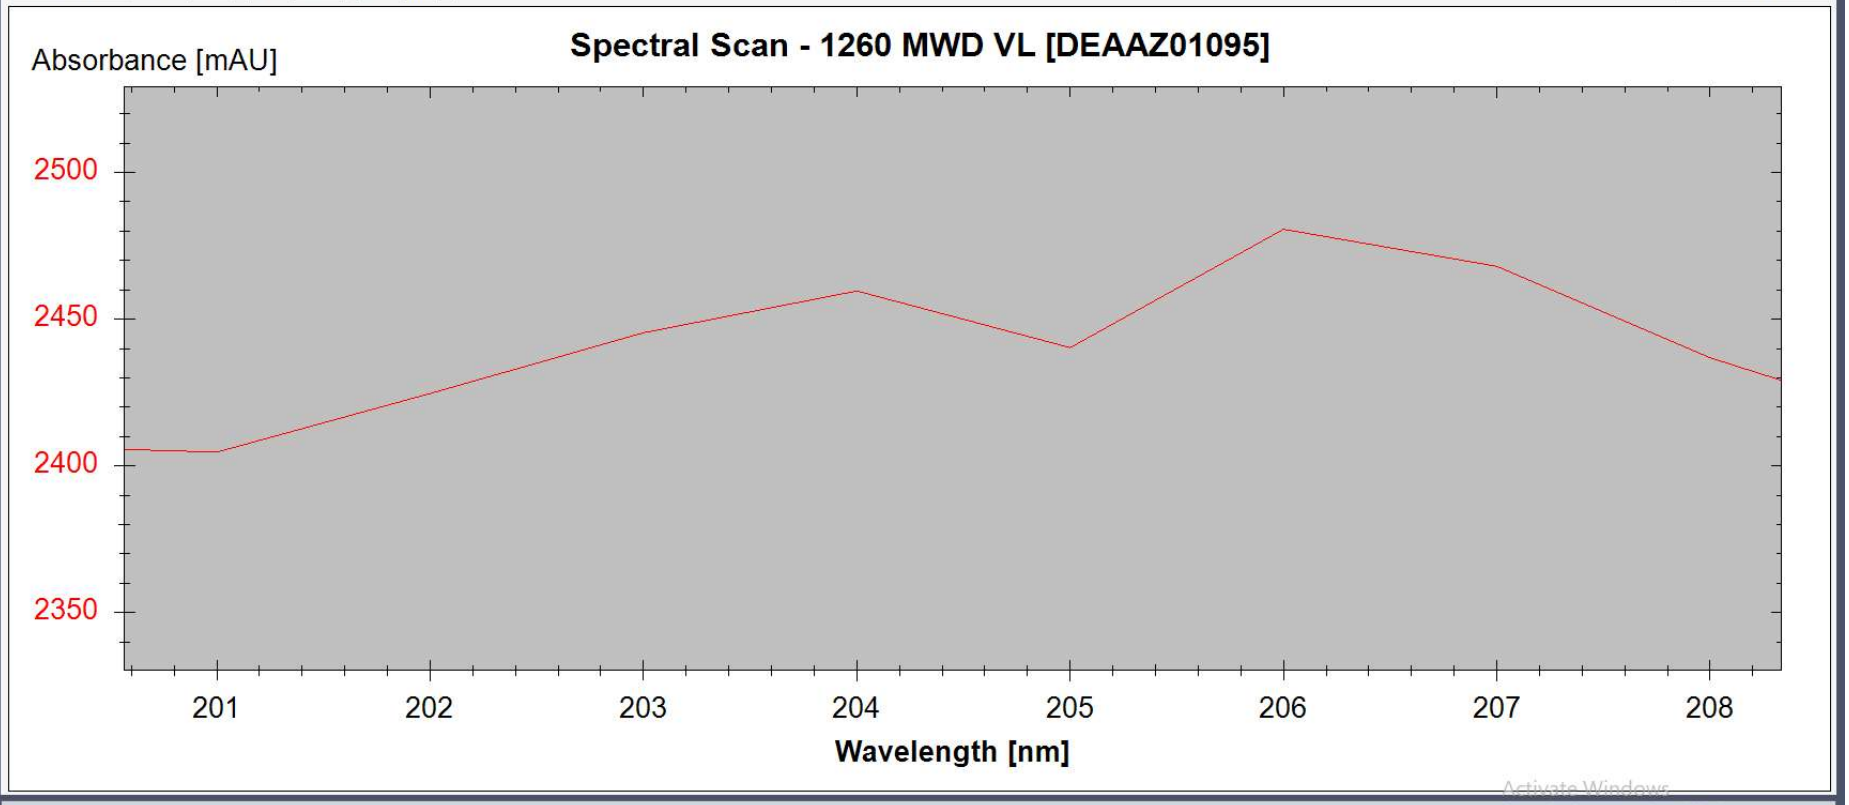

more... | Print Result | Back

Activate Windows
Go to Settings to activate Windows.

Connection Address: 192.168.0.253

Version 2.18.479 - Basic | Licenses 8/20

Type here to search
SAL-0315 - Acquisit...
SAL-0166 - Agilent ...
Untitled - Paint
64°F Windy
POR PTB2 10:31 AM 7/19/2023

SAL-0166 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results


SAL-0166
- Service & Diagnostics
- Instrument Control
- EMFs
- Firmware Update Report
- System Report

Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — SAL-0166 » SAL-0166 » G1365D:DEAAZ01095

Spectral Scan - 1260 MWD VL [DEAAZ01095]

UV Lamp On | Sample Scan | from 200 | to 300 | step 1.0 | Export Data

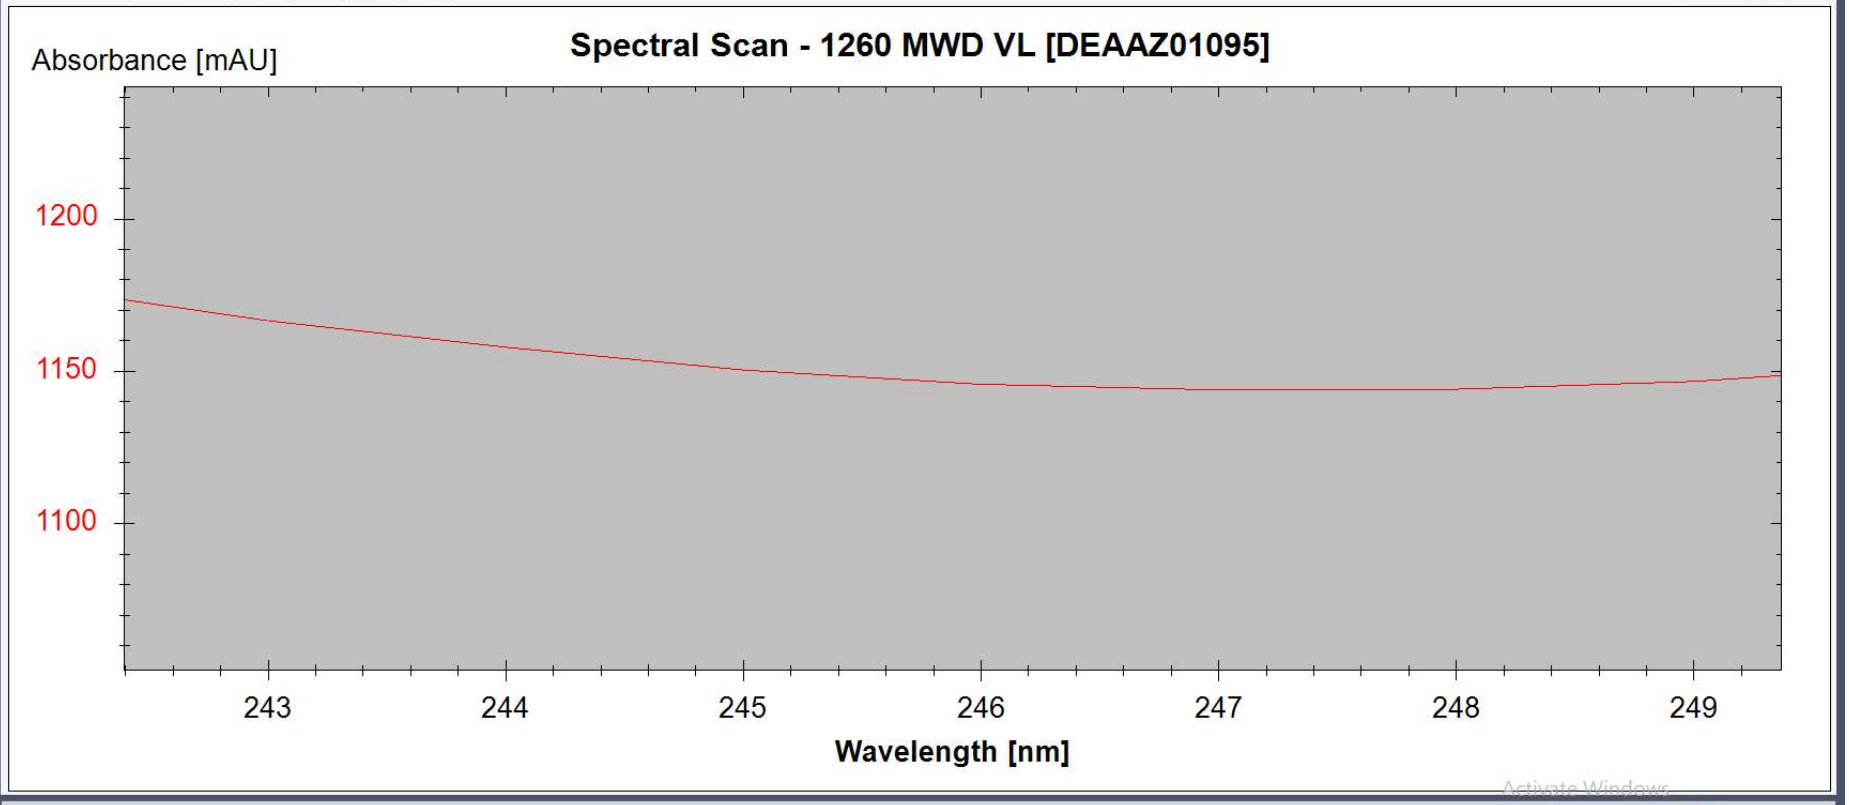

Activate Windows
Go to Settings to activate Windows.

more... | Print Result | Back

Connection Address: 192.168.0.253

Version 2.18.479 - Basic | Licenses 8/20

Type here to search
SAL-0315 - Acquisit...
SAL-0166 - Agilent ...
Untitled - Paint
64°F Windy
POR PTB2 10:32 AM 7/19/2023

SAL-0166 - Agilent Lab Advisor

Agilent Lab Advisor — Service & Diagnostics — Basic Version

Tasks

Lab Advisor
- System Overview
- Configuration
- Apps
- Firmware Update
- Logs & Results


SAL-0166
- Service & Diagnostics
- Instrument Control
- EMFs
- Firmware Update Report
- System Report

Help
- Context Help (F1)
- Help Topics
- What's New?

Spectral Scan — SAL-0166 » SAL-0166 » G1365D:DEAAZ01095

Spectral Scan - 1260 MWD VL [DEAAZ01095]

UV Lamp On | Sample Scan | from 200 | to 300 | step 1.0 | Export Data

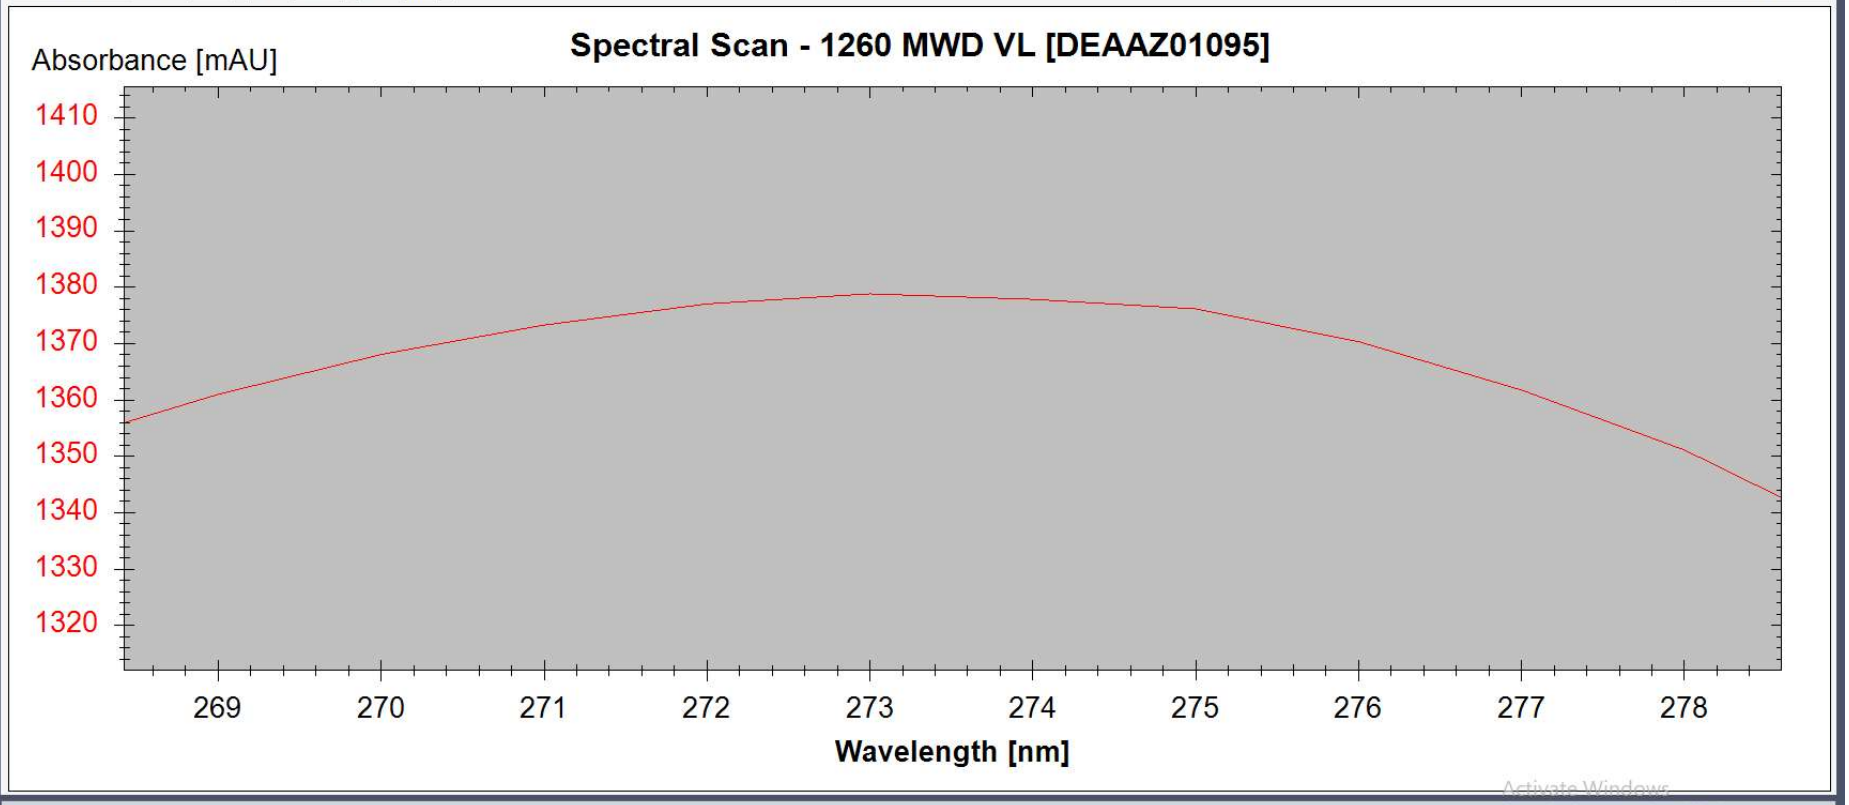

Activate Windows
Go to Settings to activate Windows.

more... | Print Result | Back


Connection Address: 192.168.0.253

Version 2.18.479 - Basic | Licenses 8/20

Type here to search
SAL-0315 - Acquisit... | SAL-0166 - Agilent ... | Untitled - Paint
64°F Windy
POR PTB2 10:32 AM 7/19/2023

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\Branco PCIN 01.dx		
Sample name:	Branco PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 11:03:44-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

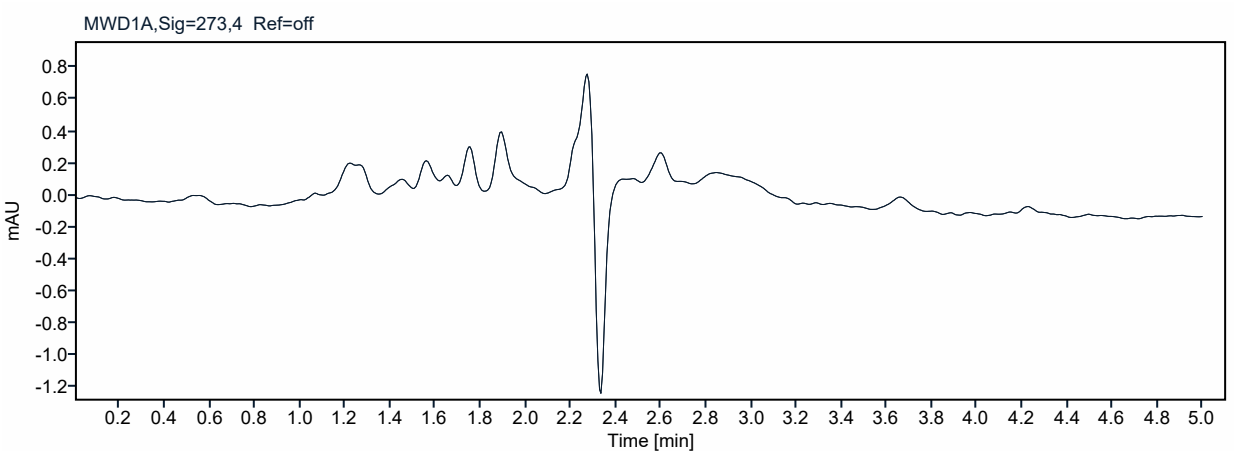

Name	RT [min]	Area	RF	Amount []	Concentration []

Single Injection Report

Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 01.dx		
Sample name:	PCIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:09:48-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

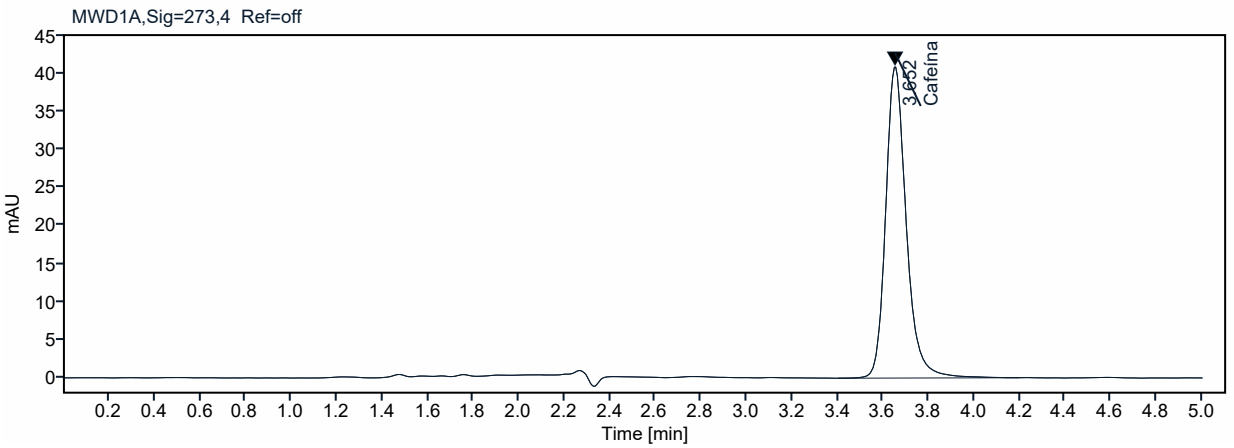


Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.652	257.4748			

Single Injection Report

Agilent


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 02.dx		
Sample name:	PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:15:49-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

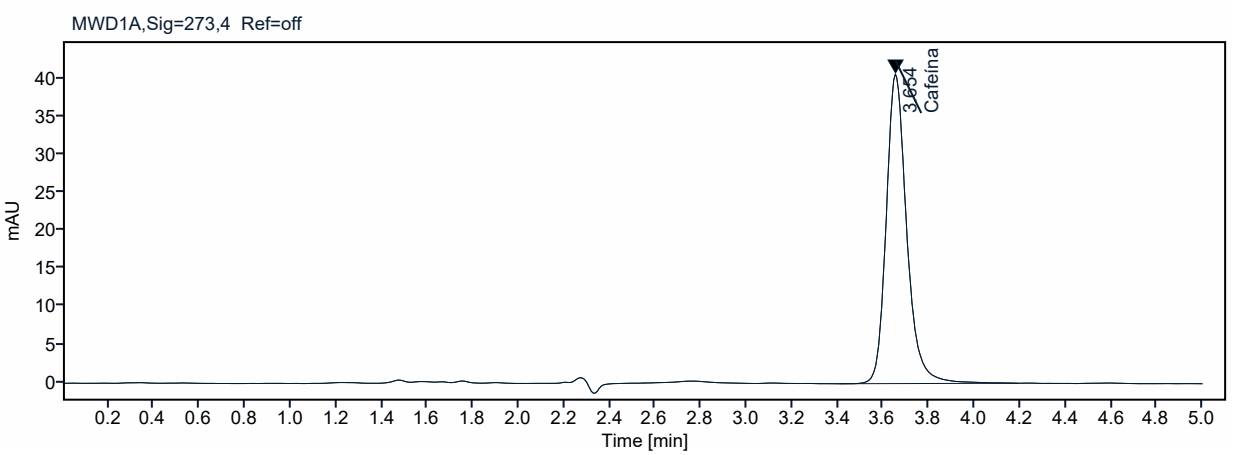

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.654	256.8148			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 03.dx		
Sample name:	PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:21:51-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

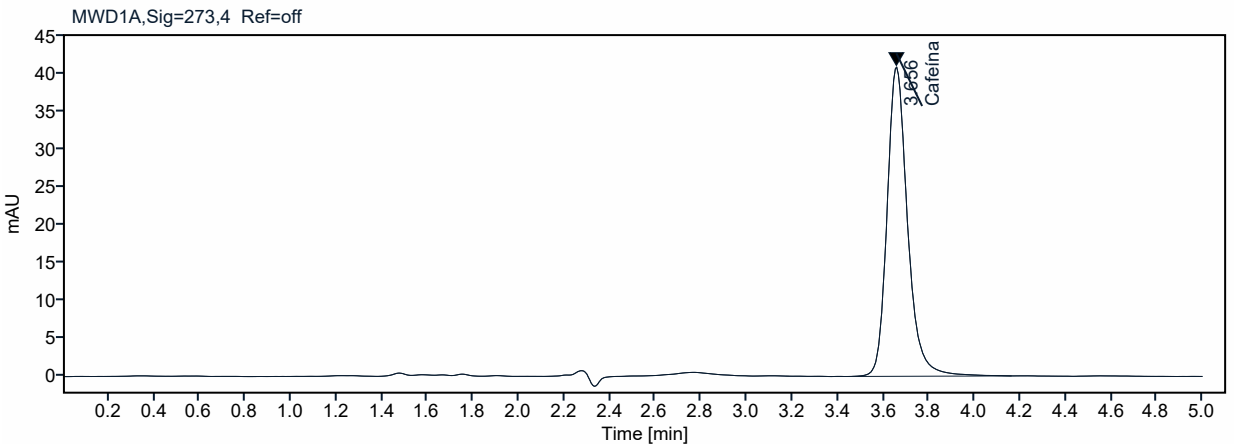

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.656	257.2481			

Single Injection Report

Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\Branco PCIN 02.dx		
Sample name:	Branco PCIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 11:27:51-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

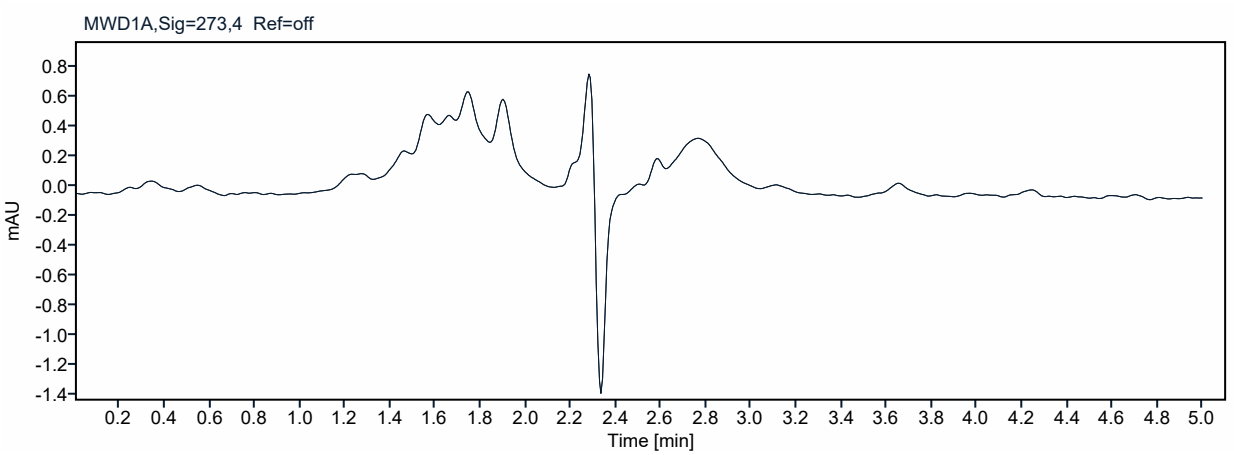


Name	RT [min]	Area	RF	Amount []	Concentration []

Single Injection Report

Agilent

Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 04.dx		
Sample name:	PCIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:33:53-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

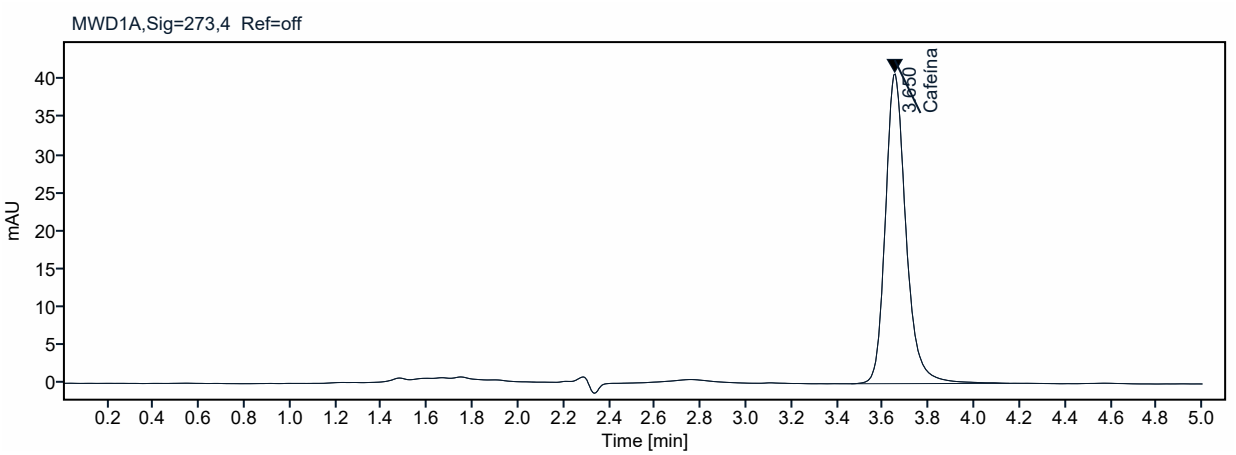


Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.650	256.8878			

Single Injection Report

Agilent


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 05.dx		
Sample name:	PCIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:39:55-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

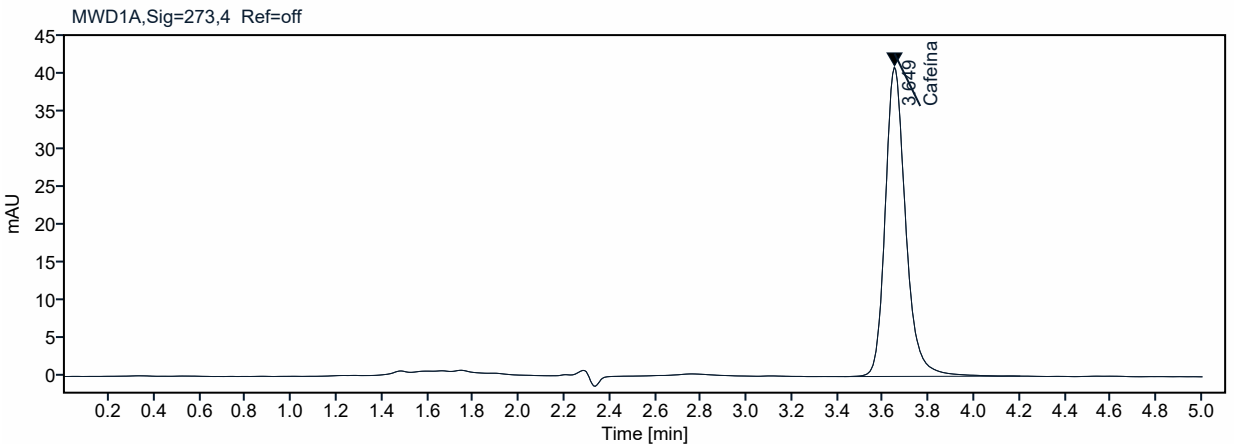

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.649	257.0107			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\PCIN 06.dx		
Sample name:	PCIN 06		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 11:45:56-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

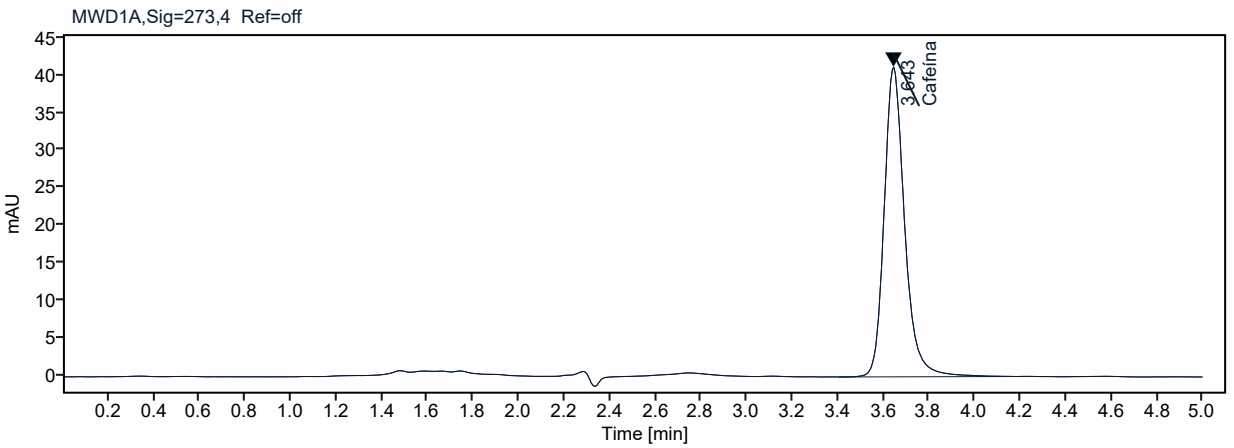

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.643	257.3600			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/PCIN 001.rslt\Branco PCIN 03.dx		
Sample name:	Branco PCIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 11:51:57-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

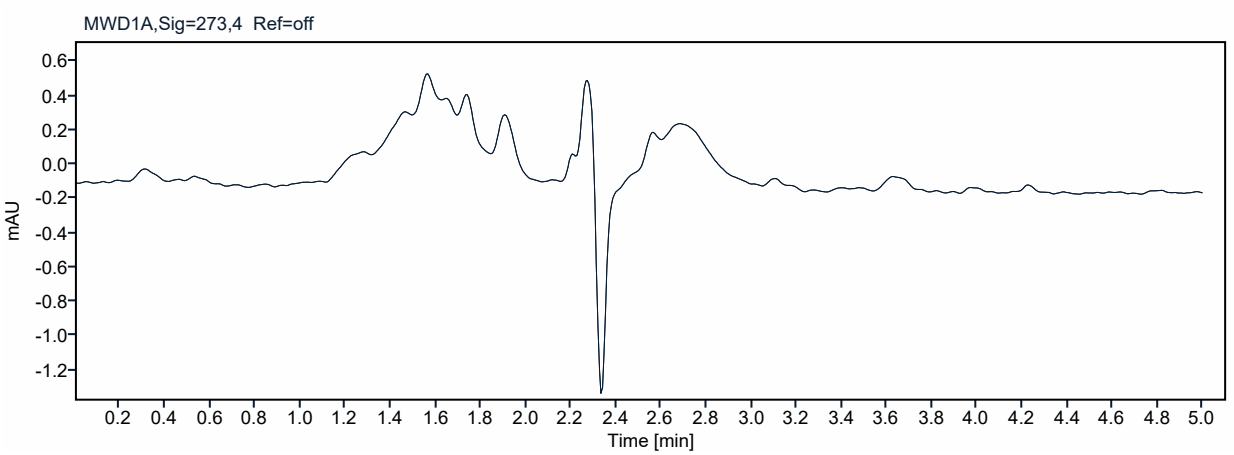

Name	RT [min]	Area	RF	Amount []	Concentration []

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LDUV 002.rslt\LDUV 01.dx		
Sample name:	LDUV 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 12:54:51-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

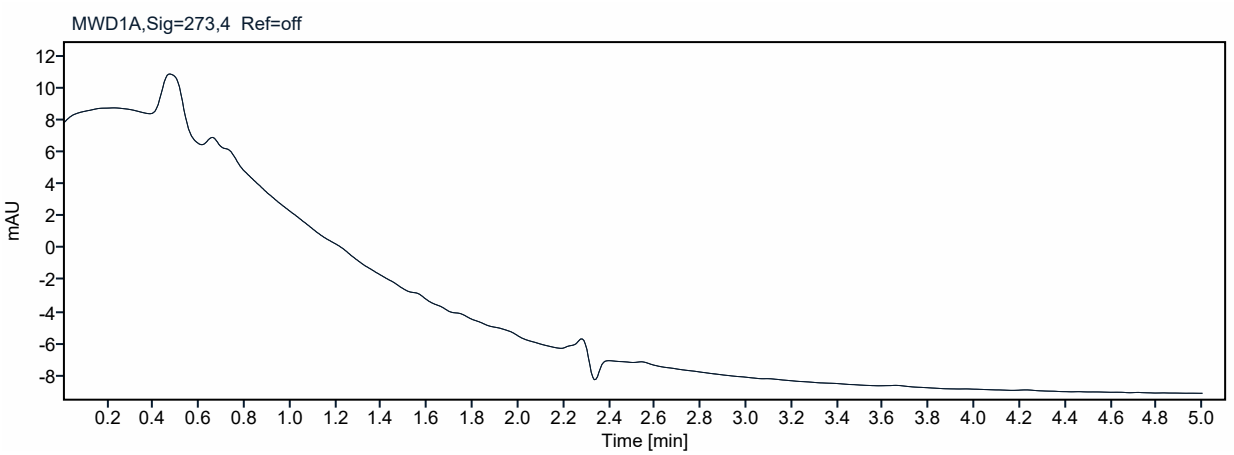

Name	RT [min]	Area	RF	Amount []	Concentration []

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LDUV 002.rslt\LDUV 02.dx		
Sample name:	LDUV 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	43
Injection date:	2023-07-19 13:00:52-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

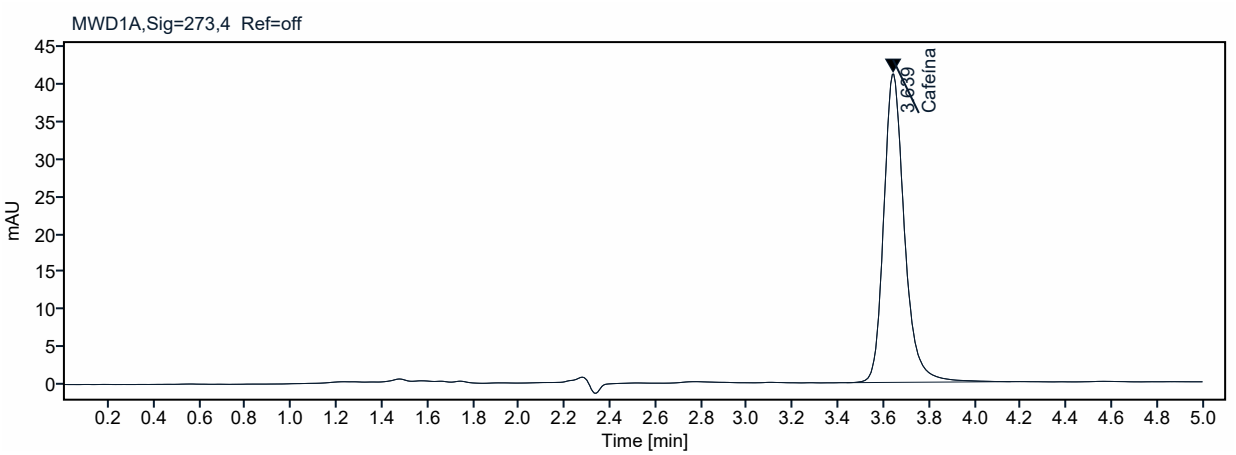

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.639	260.7999			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LDUV 002.rslt\LDUV 03.dx		
Sample name:	LDUV 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	44
Injection date:	2023-07-19 13:06:51-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

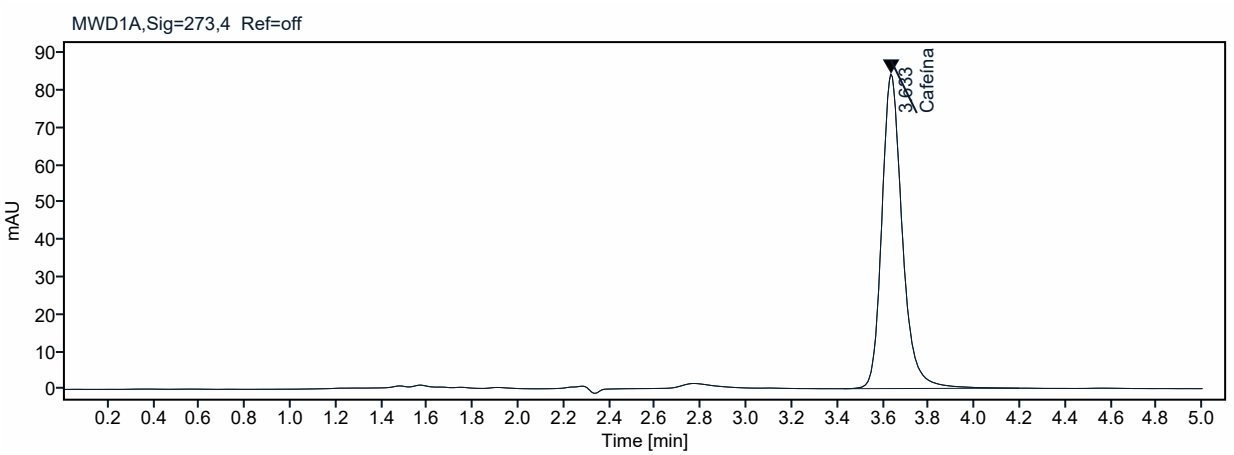

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.633	525.2275			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LDUV 002.rslt\LDUV 04.dx		
Sample name:	LDUV 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	45
Injection date:	2023-07-19 13:12:53-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

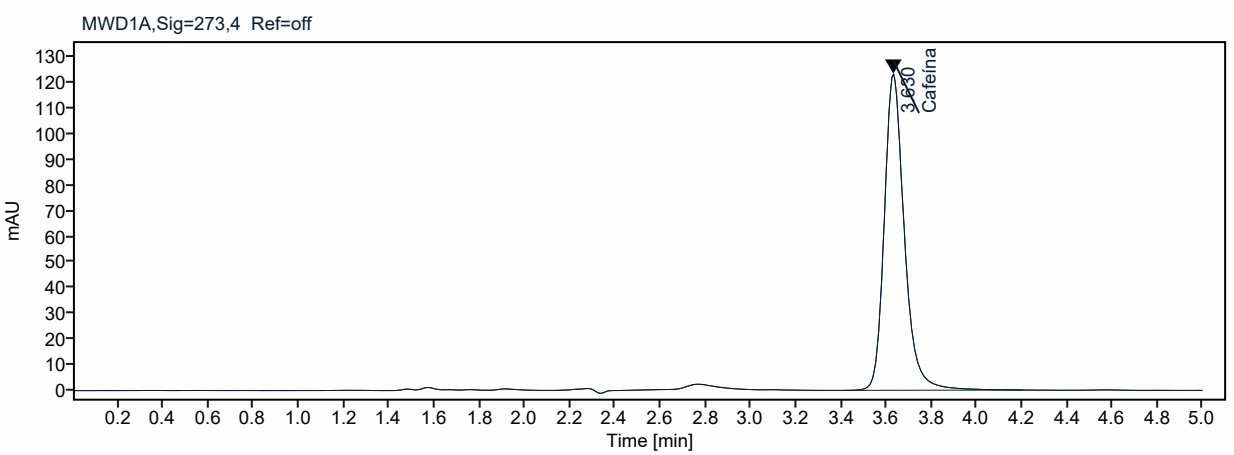

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.630	765.1500			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LDUV 002.rslt\LDUV 05.dx		
Sample name:	LDUV 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	46
Injection date:	2023-07-19 13:18:58-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

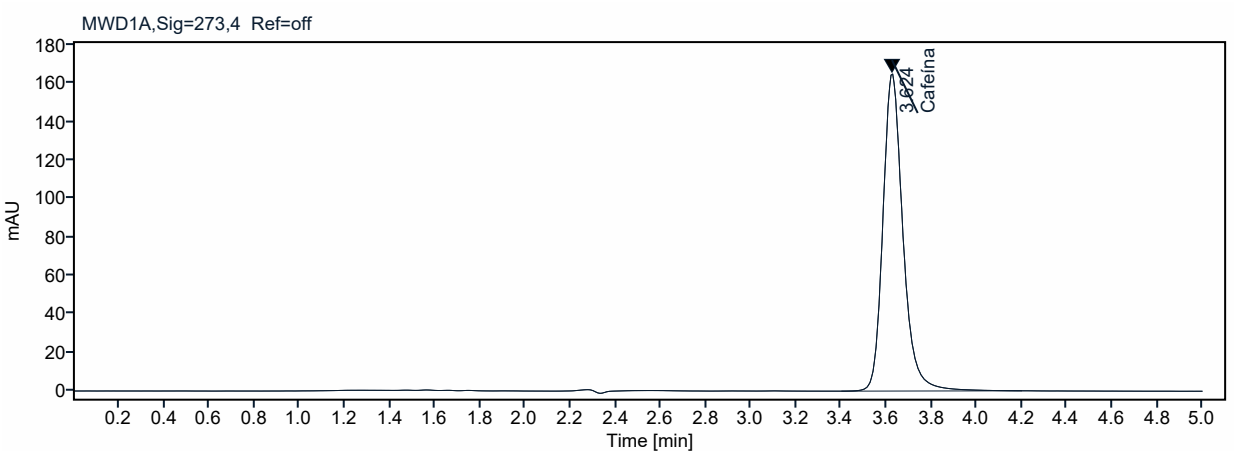

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.624	1020.8302			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LIIN 001.rslt\LIIN 01.dx		
Sample name:	LIIN 01		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	41
Injection date:	2023-07-19 13:34:02-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	0.100 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

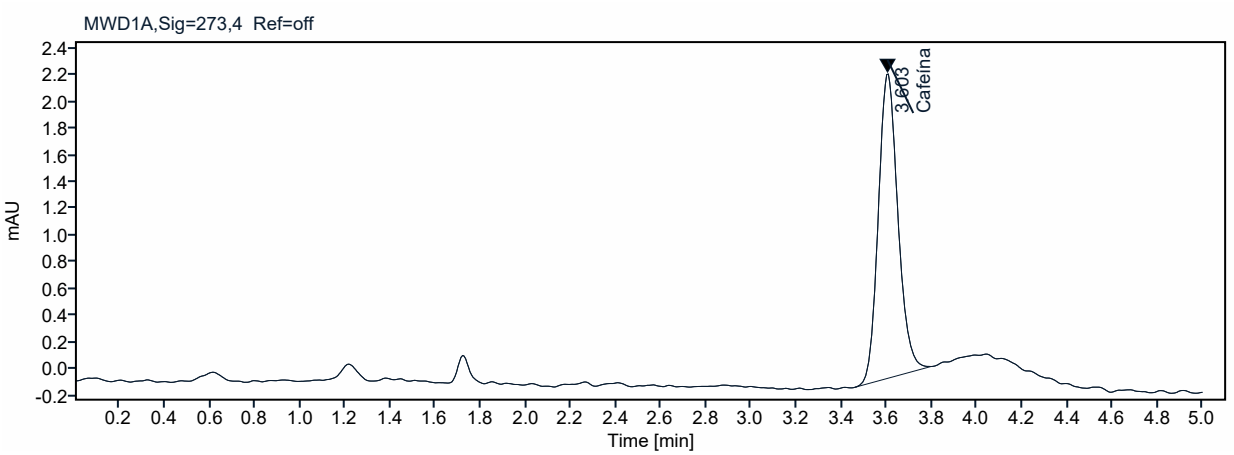

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.603	13.7037			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/LIIN 001.rslt\LIIN 02.dx		
Sample name:	LIIN 02		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	41
Injection date:	2023-07-19 13:39:57-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	5.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

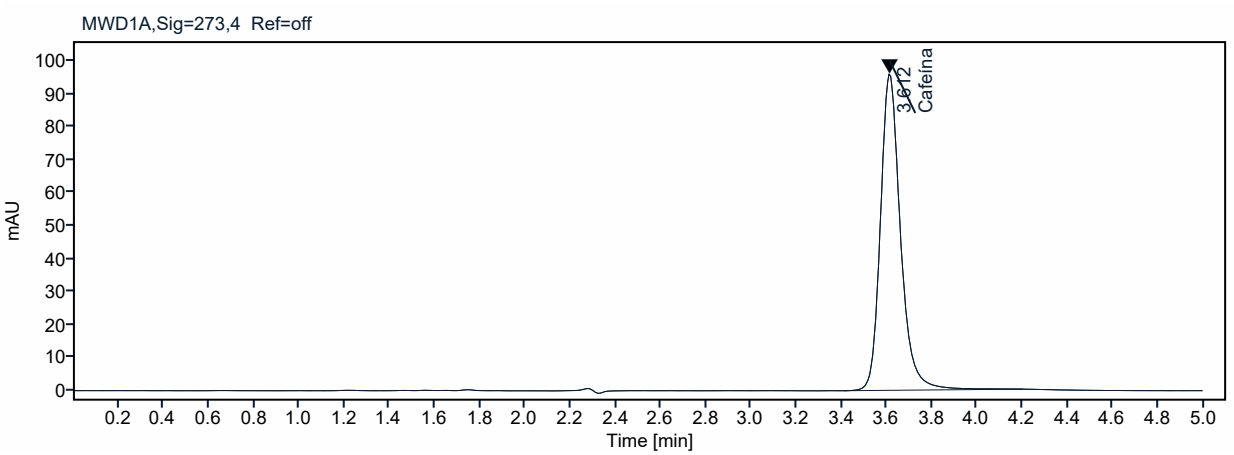

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.612	594.1769			

Single Injection Report

Data file:	/Agilent/Results/Qualificação 2023/LIIN 001.rslt\LIIN 03.dx		
Sample name:	LIIN 03		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	41
Injection date:	2023-07-19 13:45:56-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	10.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

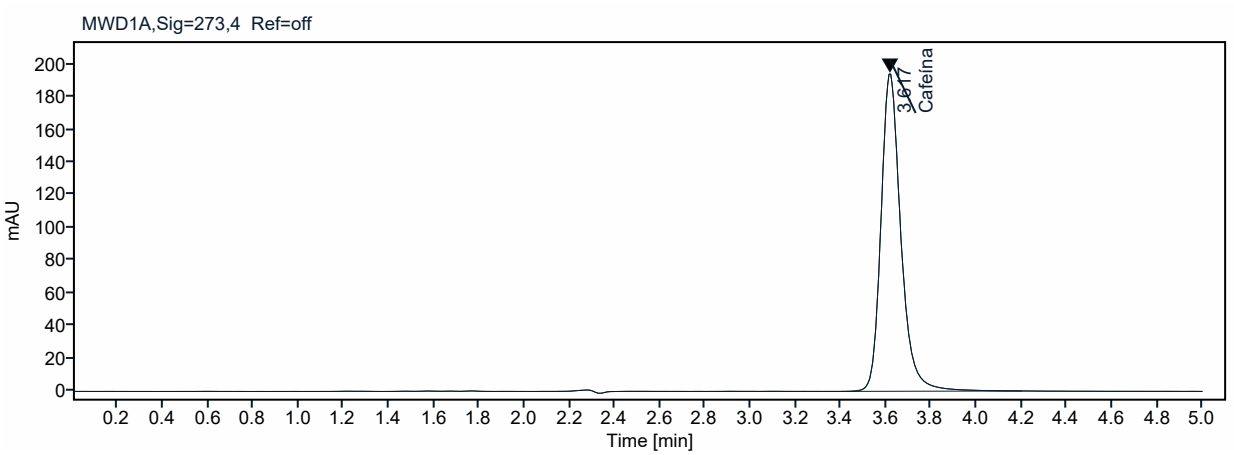


Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.617	1190.7667			

Single Injection Report

Agilent

Data file:	/Agilent/Results/Qualificação 2023/LIIN 001.rslt\LIIN 04.dx		
Sample name:	LIIN 04		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	41
Injection date:	2023-07-19 13:51:57-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	15.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

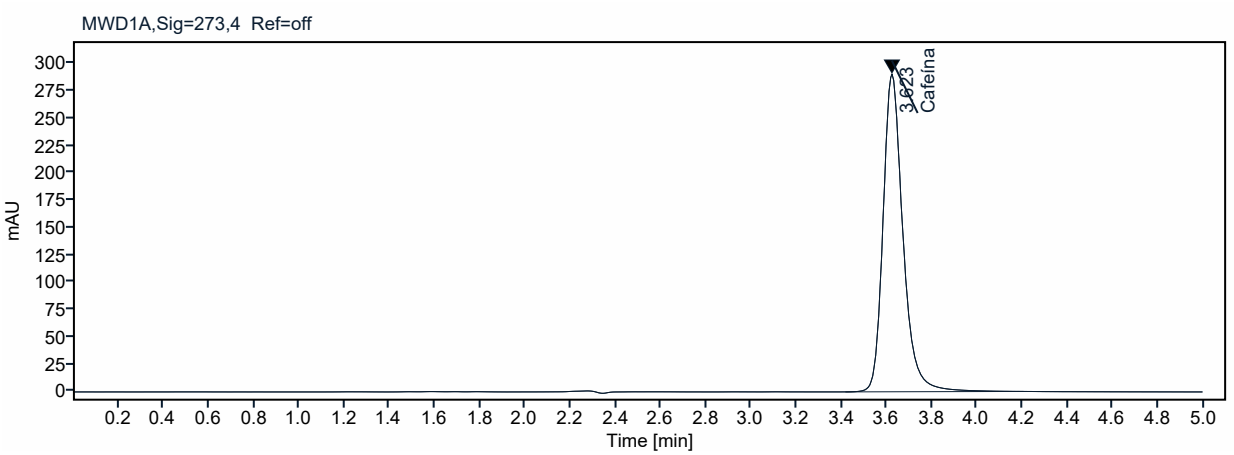


Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.623	1782.3999			

Single Injection Report

Agilent


Data file:	/Agilent/Results/Qualificação 2023/LIIN 001.rslt\LIIN 05.dx		
Sample name:	LIIN 05		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	41
Injection date:	2023-07-19 13:58:01-03:00	**Injection:**	1 of 1
Acq. method:	QPack.amx	**Injection volume:**	20.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

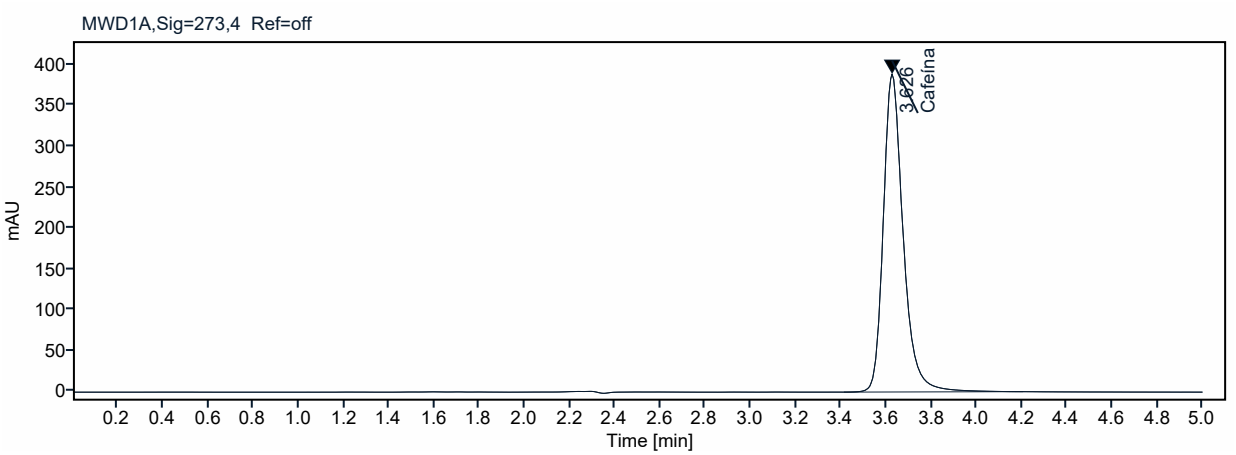

Name	RT [min]	Area	RF	Amount []	Concentration []
Cafeína	3.626	2376.3836			

Single Injection Report


Data file:	/Agilent/Results/Qualificação 2023/RELB 001.sirslt\RELB 001.dx		
Sample name:	RELB 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	46
Injection date:	2023-07-19 14:12:54-03:00	**Injection:**	1 of 1
Acq. method:	RELB.amx	**Injection volume:**	20.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

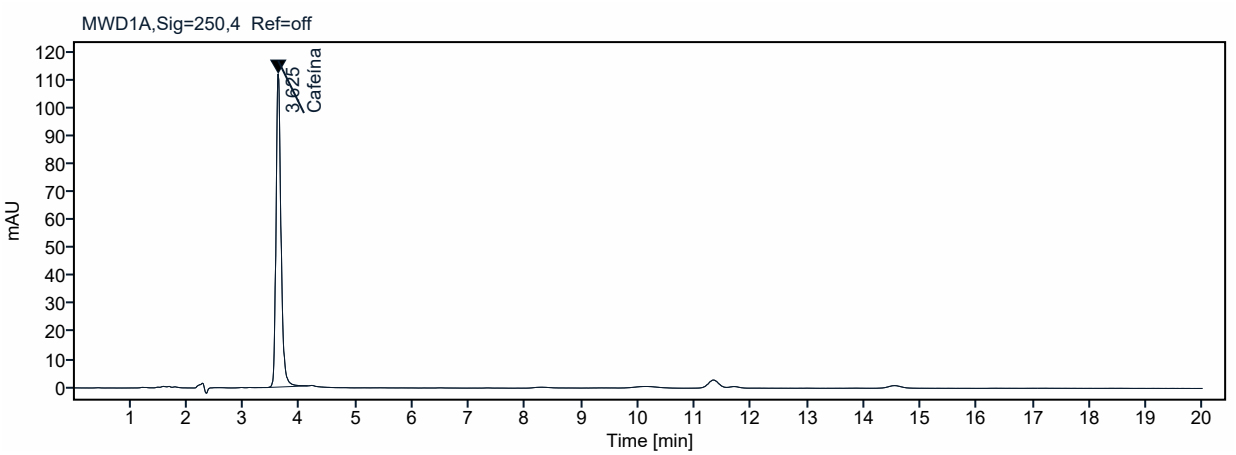

Name	RT [min]	Area	Concentration []	Peak Height
Cafeína	3.625	687.4170		112.275

Single Injection Report

Data file:	/Agilent/Results/Qualificação 2023/RELB 001.sirslt\RELB 001.dx		
Sample name:	RELB 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	46
Injection date:	2023-07-19 14:12:54-03:00	**Injection:**	1 of 1
Acq. method:	RELB.amx	**Injection volume:**	20.000 µL
Analysis method:	Cafeína.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:30-03:00		

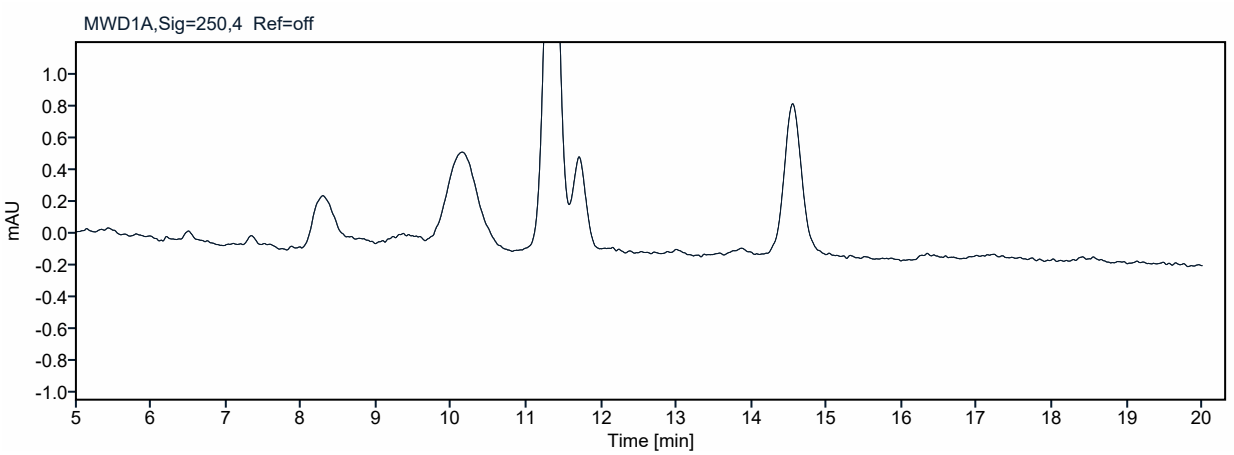


Name	RT [min]	Area	Concentration []	Peak Height
Cafeína	3.625	687.4170		112.275

Single Injection Report

Agilent


Data file:	/Agilent/Results/Qualificação 2023/GRAD AB 001.sirslt\GRAD AB 001.dx		
Sample name:	GRAD AB 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 15:09:16-03:00	**Injection:**	1 of 1
Acq. method:	GRAD AB.amx	**Injection volume:**	0.100 µL
Analysis method:	*GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 10:56:57-03:00		

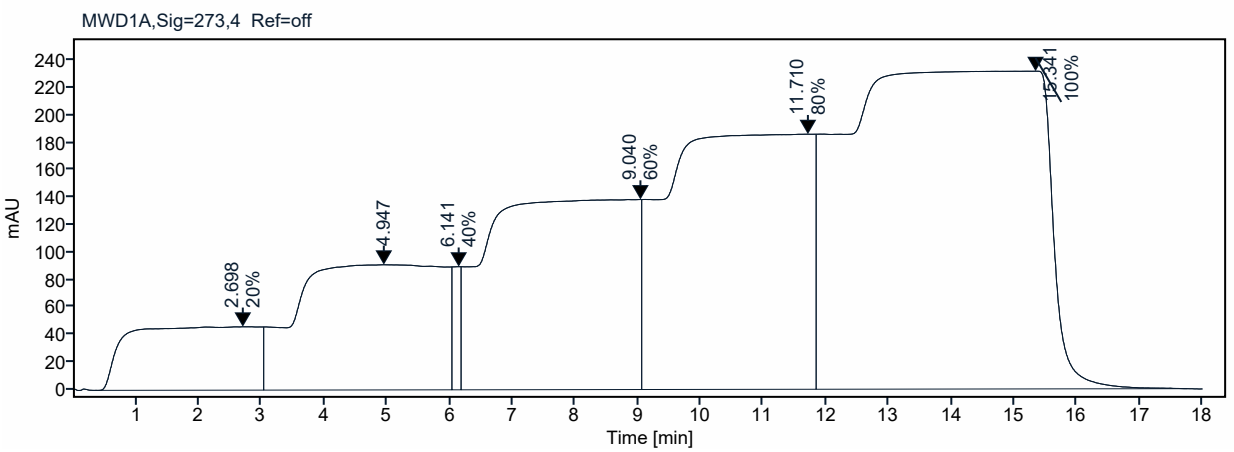

Name	RT [min]	Area	Concentration []	Peak Height
20%	2.698	6480.7334		46.185
40%	6.141	787.8177		89.731
60%	9.040	22330.9495		138.460
80%	11.710	29237.1832		185.886
100%	15.341	50873.9047		231.530

Single Injection Report

Data file:	/Agilent/Results/Qualificação 2023/GRAD CD 001.sirslt\GRAD CD 001.dx		
Sample name:	GRAD CD 001		
Description:			
Sample amount:	0.000	**Sample type:**	Sample
Instrument:	SAL-0166	**Location:**	42
Injection date:	2023-07-19 15:37:01-03:00	**Injection:**	1 of 1
Acq. method:	GRAD CD.amx	**Injection volume:**	0.100 µL
Analysis method:	GC_LC Area Percent_DefaultMethod.pmx	**Acq. operator:**	admin
Last changed:	2023-07-19 15:38:11-03:00		

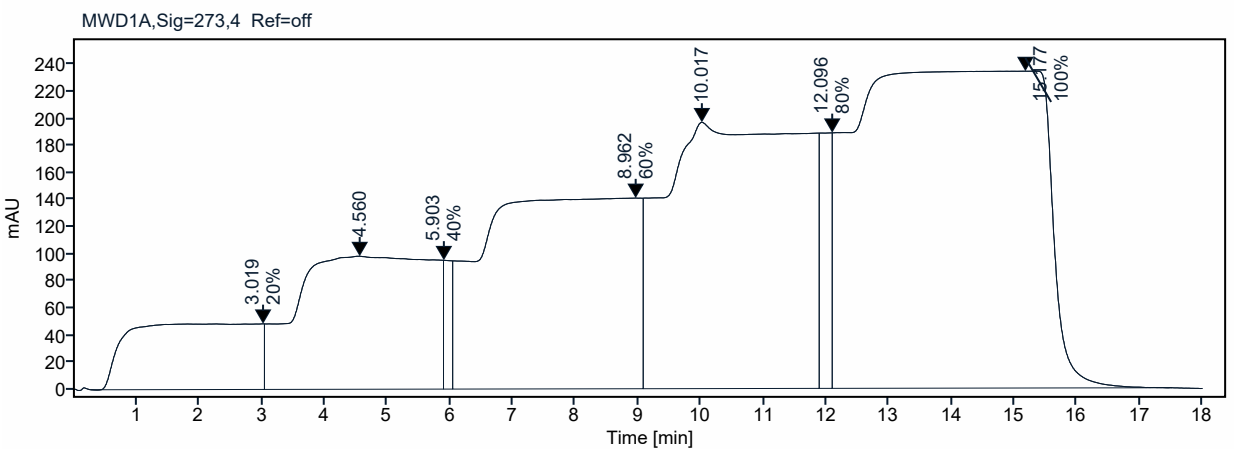

Name	RT [min]	Area	Concentration []	Peak Height
20%	3.019	6820.5822		48.386
40%	5.903	832.8521		94.987
60%	8.962	23790.3350		140.672
80%	12.096	2344.8568		188.505
100%	15.177	48510.6660		233.708