
Peak Find - Exploratória_007 UV_tR1,68.jws

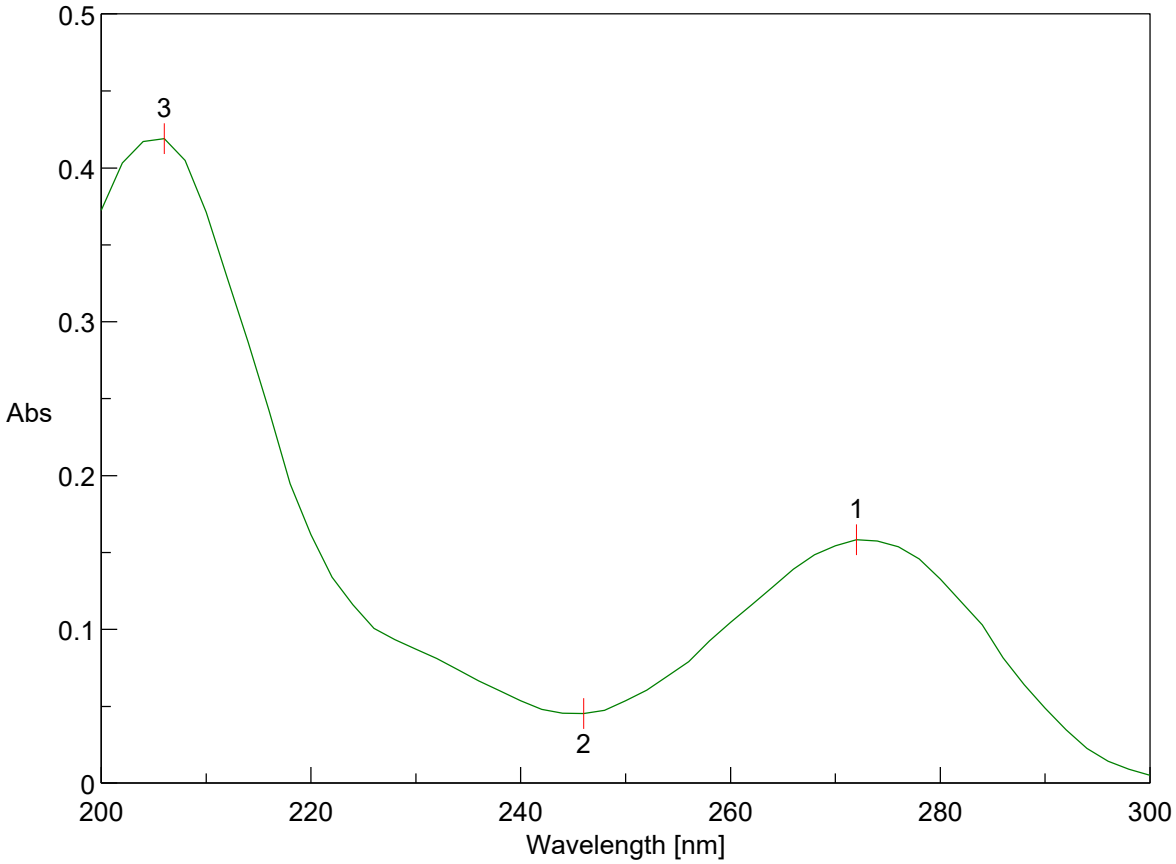

[Comments]


User	QPackSA
Division	
Company	QPack
Creation date	20/07/2023 16:11

[Detailed Information]		[Measurement Information]
Data array type	Linear data array	Model Name
Horizontal axis	Wavelength [nm]	Serial No.
Vertical axis	Abs	
Start	200 nm	
End	370 nm	
Data interval	2 nm	
Data points	85	

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	272	0.158141	2	246	0.045093
3	206	0.41875			

Chromatogram

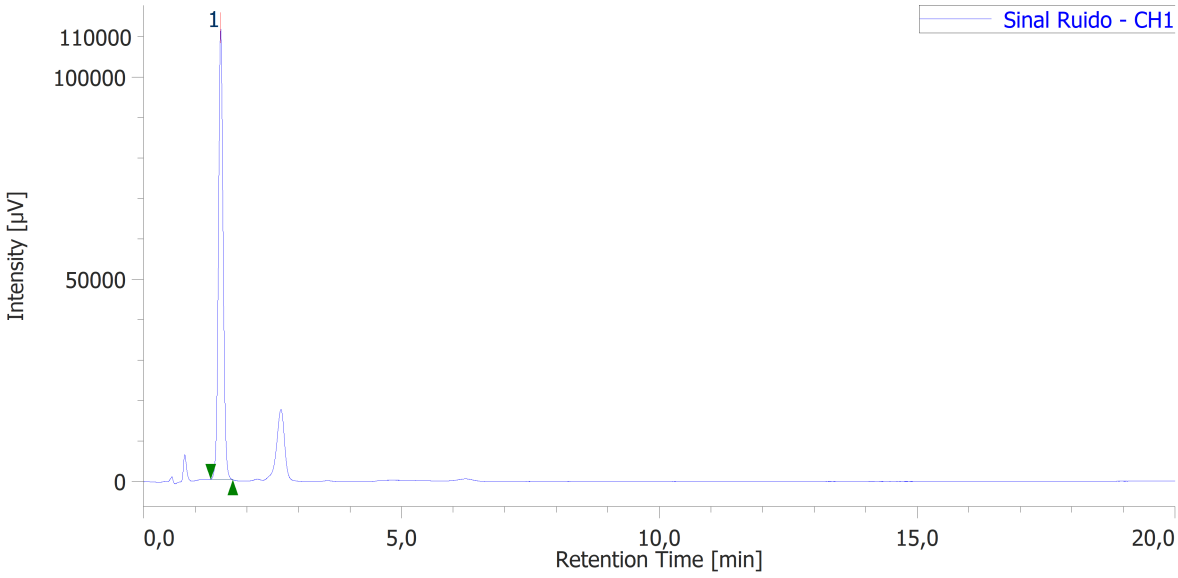


Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 11:51:29
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 17:33:23
Volume	20,0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	20,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Sinal Ruído
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table


Chromatogram Name	Sinal Ruido-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação
Formula1	{HEIGHT;Cafeína}/{SN;Cafeína}/1000

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,492	704360	111609	100,000	100,000	N/A	1368	N/A	1,063		10121,1	0,0110273

Creator QPackSA
Reviewer
Approver

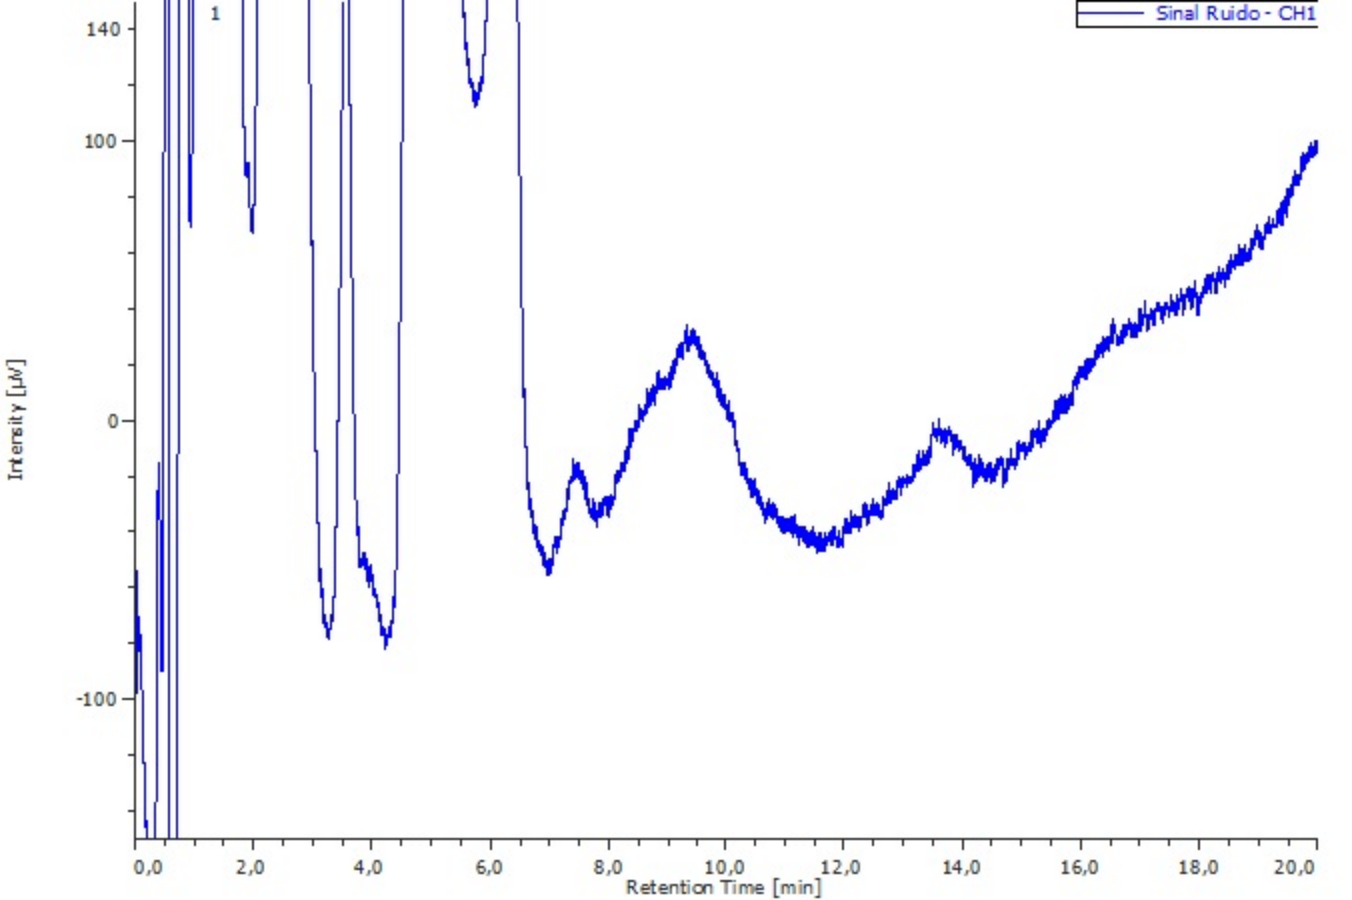
Sinal Ruido - CH1
1
140
100
0
-100
Intensity [µV]
0,0
2,0
4,0
6,0
8,0
10,0
12,0
14,0
16,0
18,0
20,0
Retention Time [min]

Chromatogram

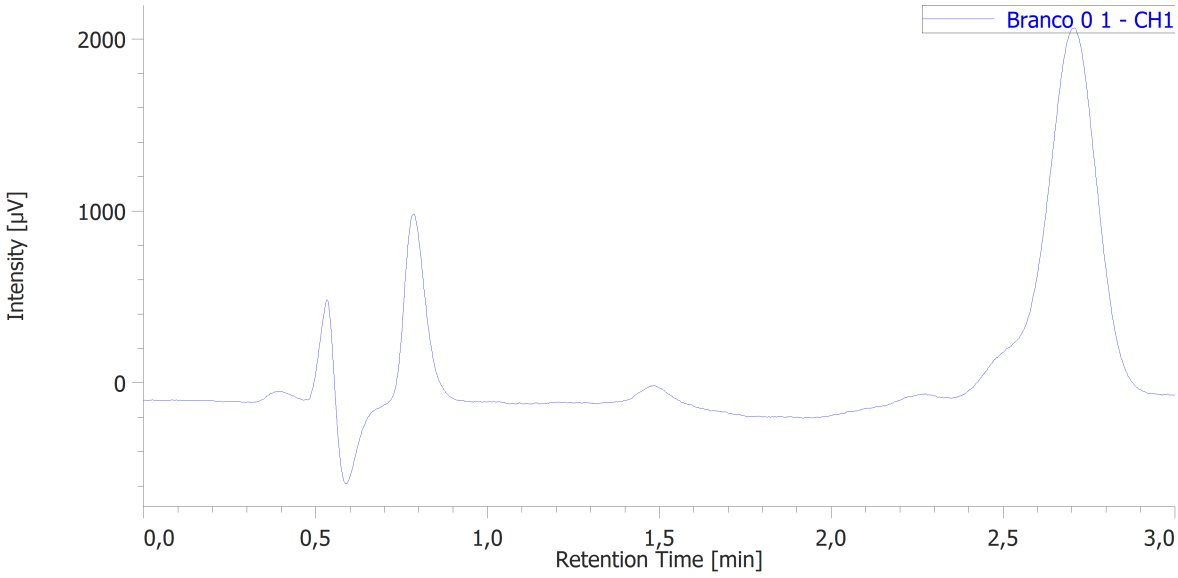


Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:46
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 17:53:43
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 0 1-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

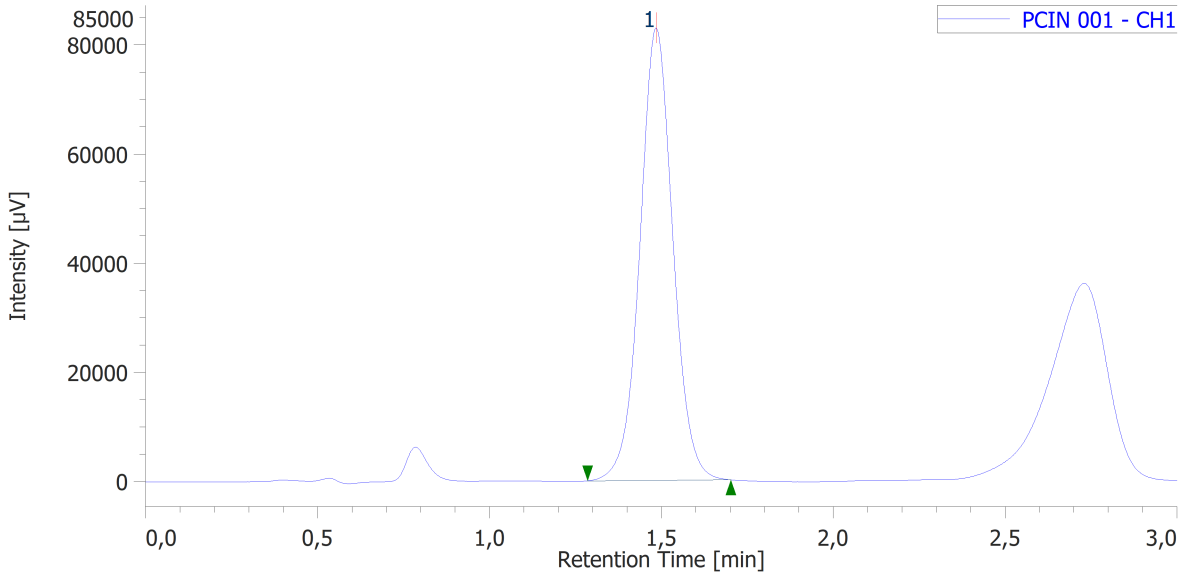

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:46
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 17:57:08
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,485	552519	82878	100,000	100,000	N/A	1209	N/A	1,027		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

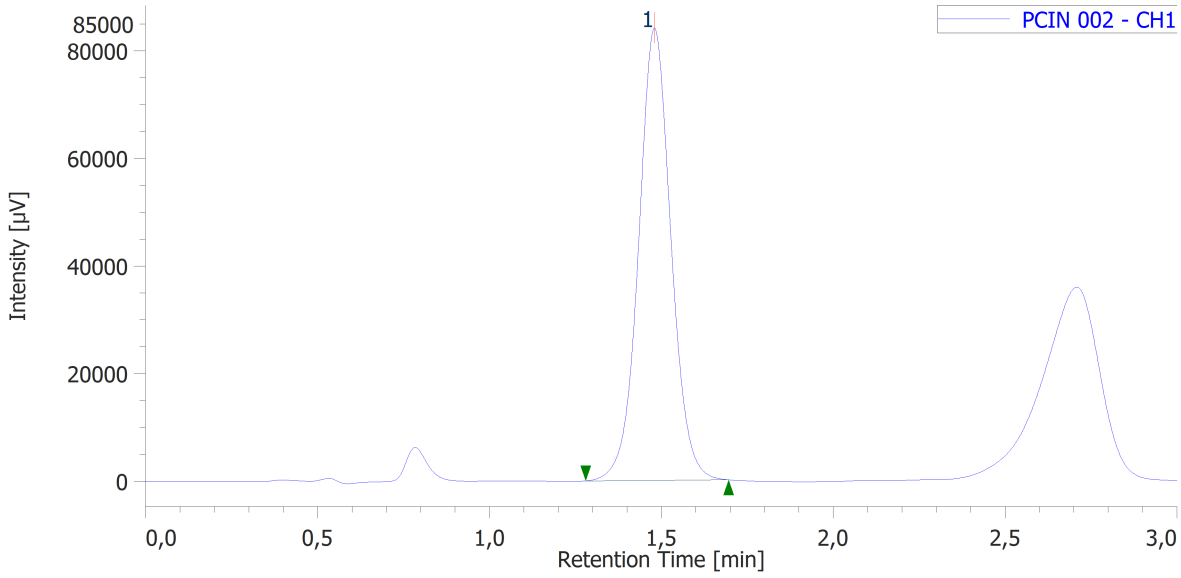

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:46
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:00:31
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,480	549975	84048	100,000	100,000	N/A	1249	N/A	1,029		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

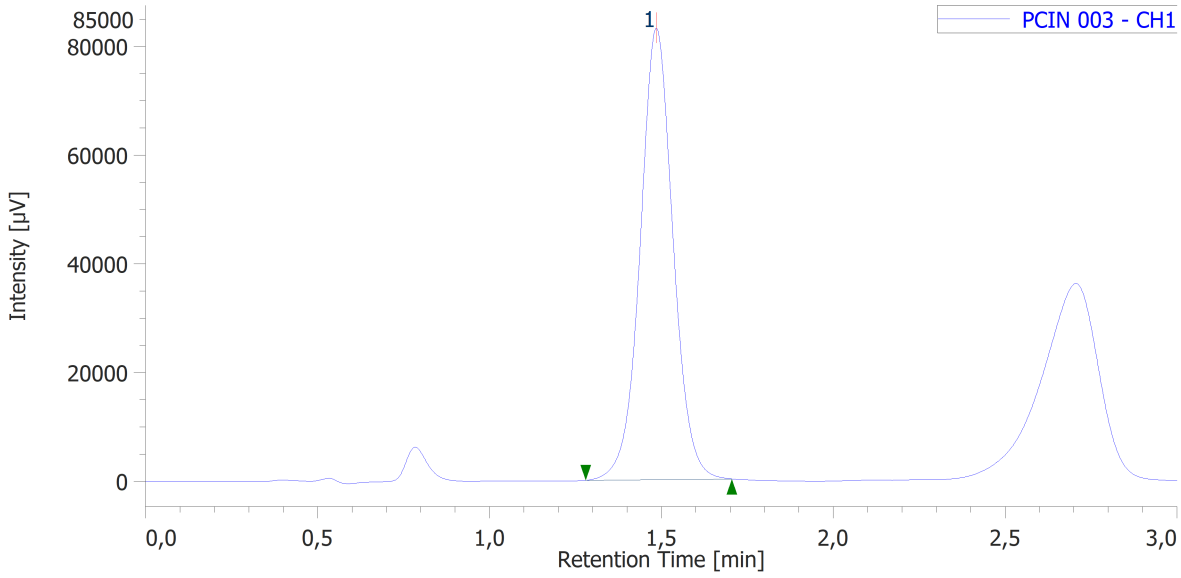

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:47
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:03:56
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,485	552395	83042	100,000	100,000	N/A	1222	N/A	1,027		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

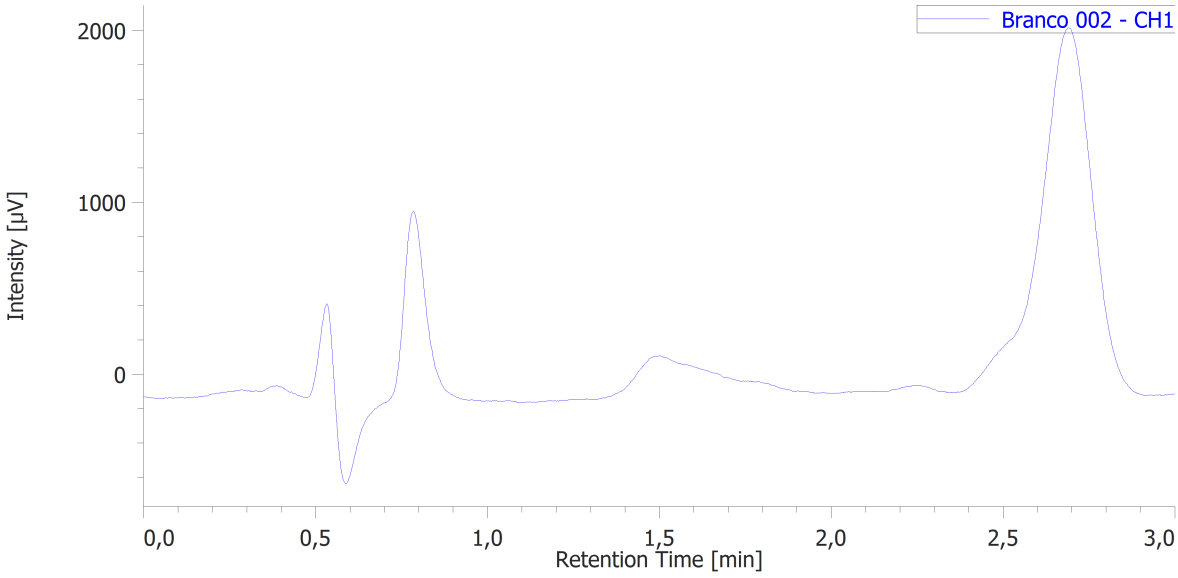


Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:47
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:07:16
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

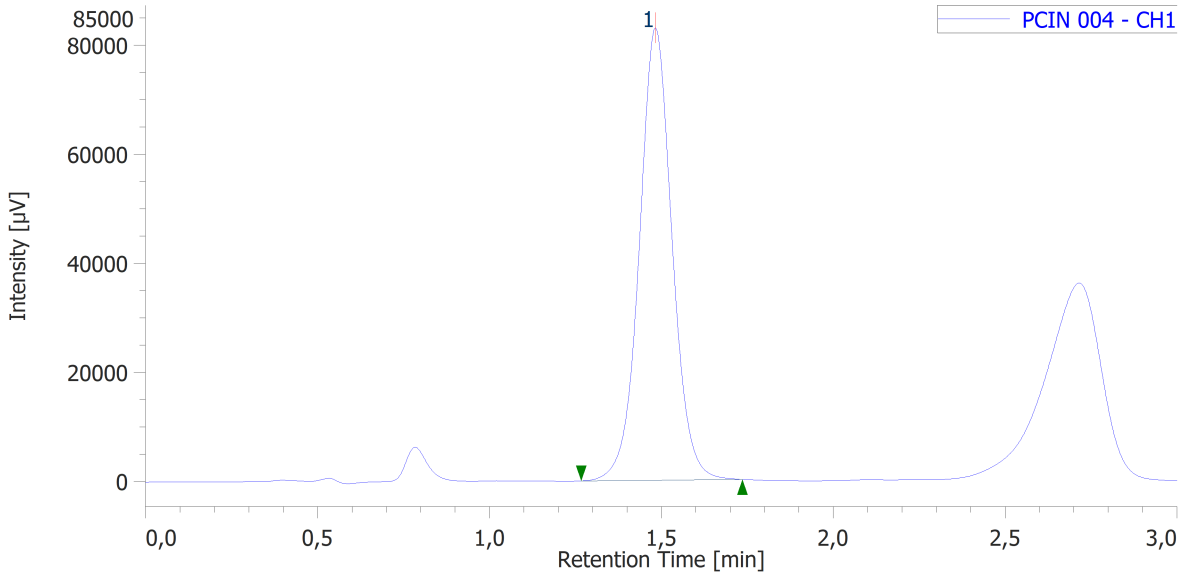

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:47
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:10:41
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,482	549634	82920	100,000	100,000	N/A	1232	N/A	1,037		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

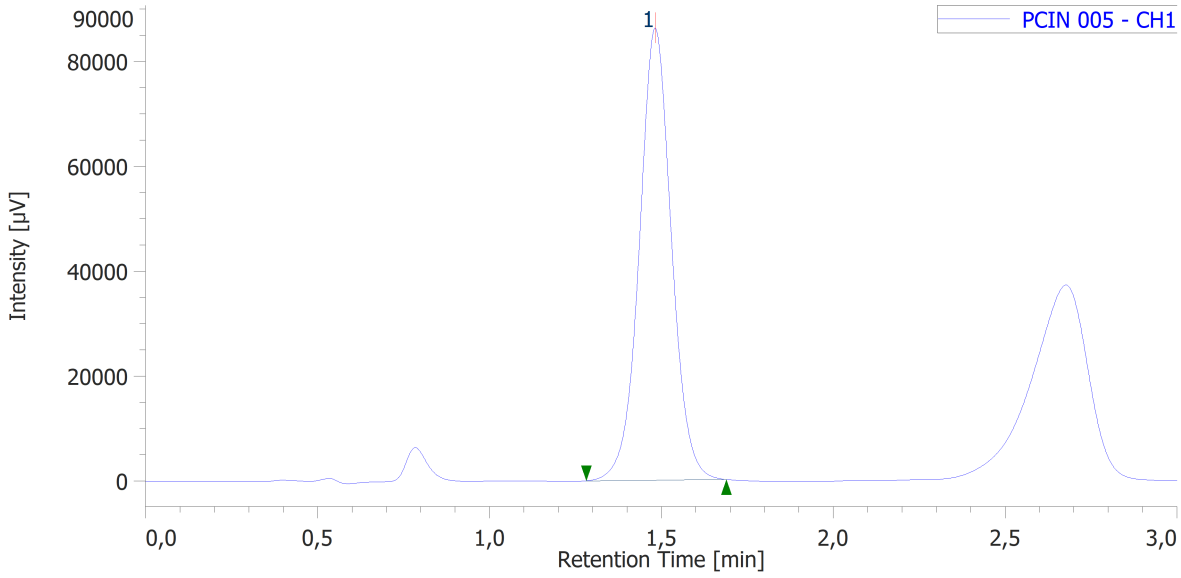

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:47
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:14:06
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,482	559271	86133	100,000	100,000	N/A	1274	N/A	1,024		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

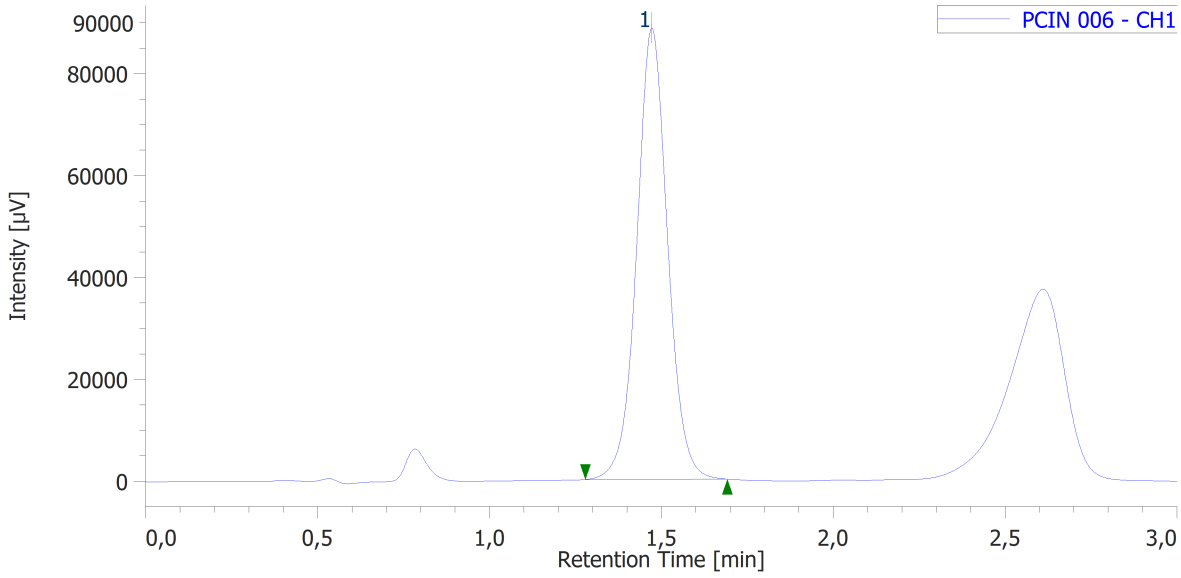

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:48
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:17:31
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,472	552451	88534	100,000	100,000	N/A	1370	N/A	1,038		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

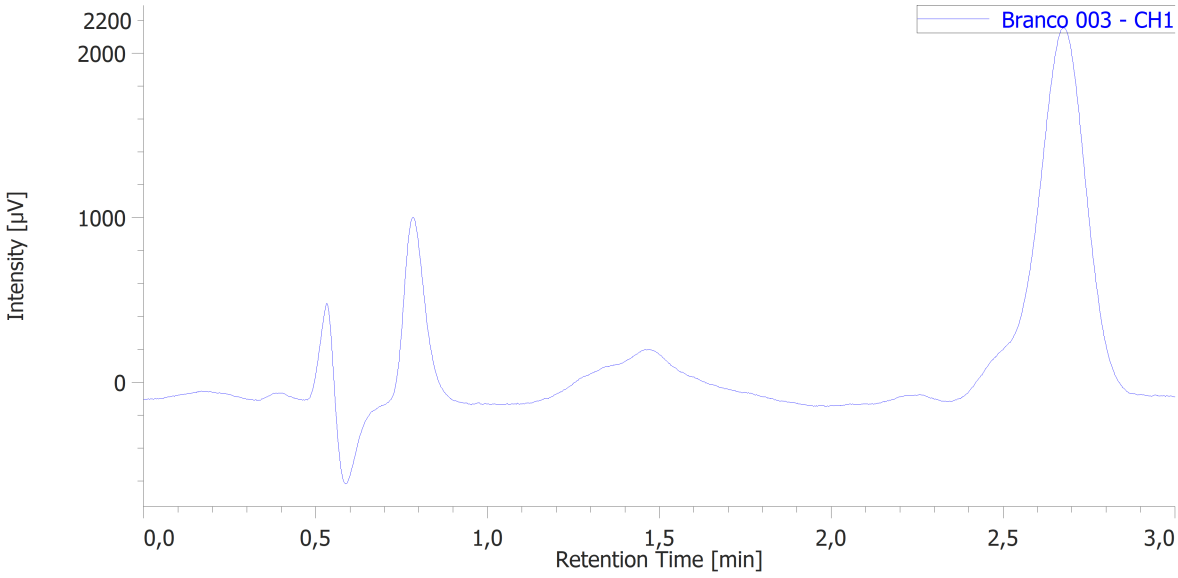


Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:48
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:20:51
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

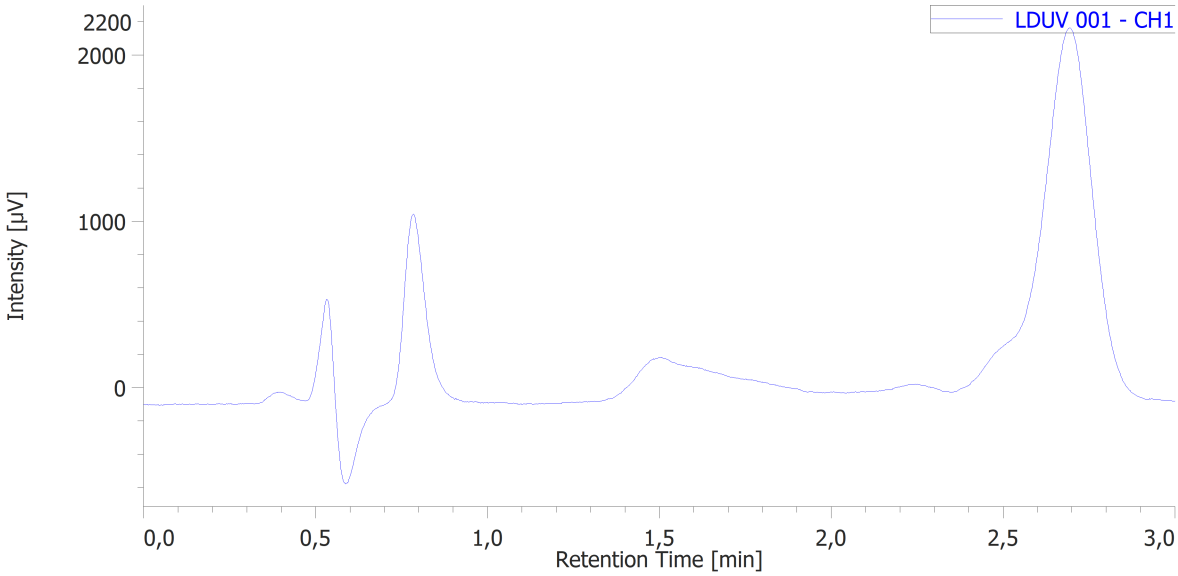


Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:48
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:24:11
Volume	10,0 [µL]
Sample #	11
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

Creator QPackSA
Reviewer
Approver

Chromatogram

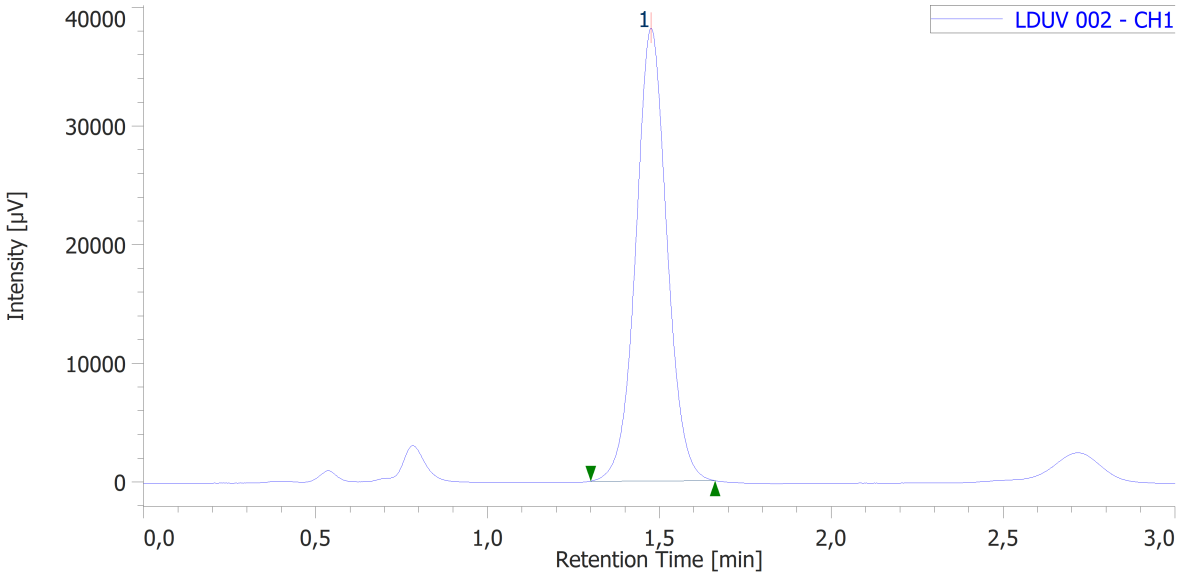

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:48
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:27:31
Volume	10,0 [µL]
Sample #	12
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,475	240322	38158	100,000	100,000	N/A	1334	N/A	1,045		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

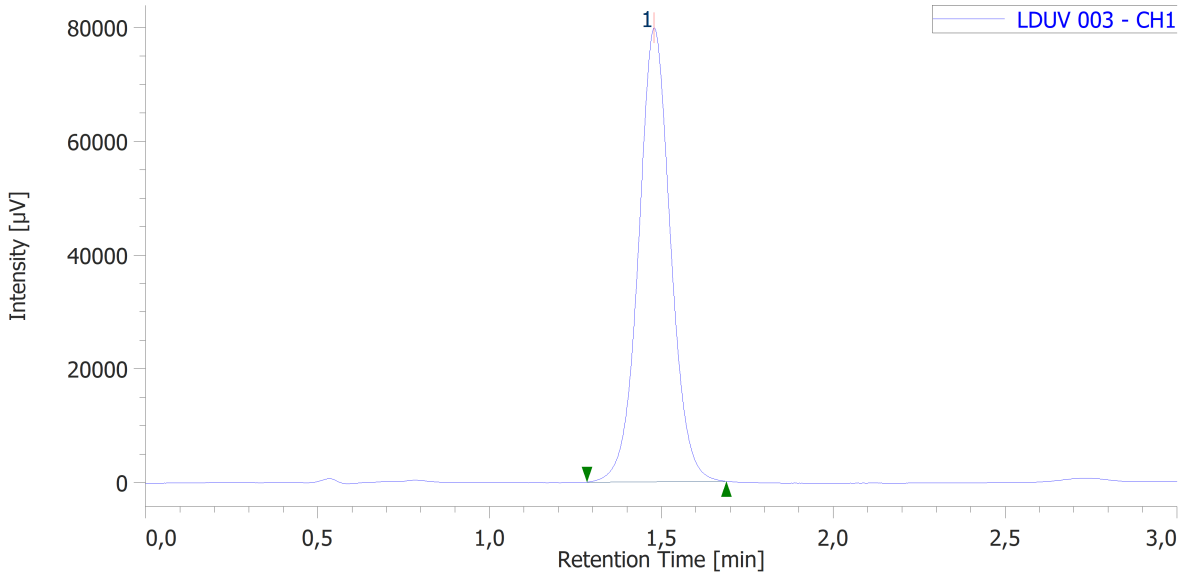

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:49
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:30:53
Volume	10,0 [µL]
Sample #	13
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,478	514812	79745	100,000	100,000	N/A	1284	N/A	1,043		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

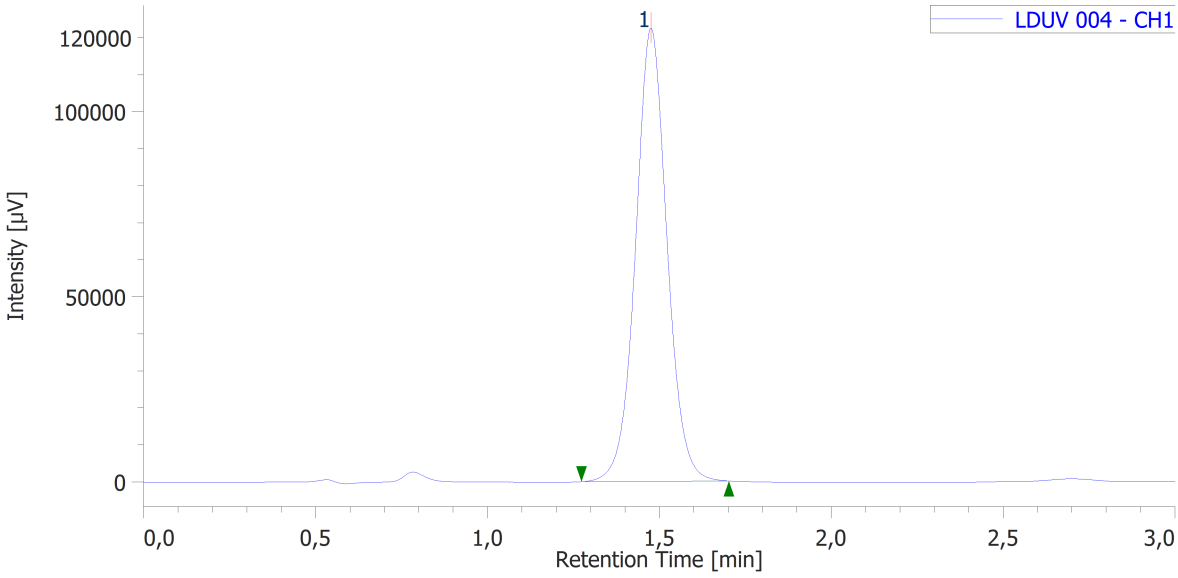

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:49
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:34:13
Volume	10,0 [µL]
Sample #	14
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,475	777673	122446	100,000	100,000	N/A	1324	N/A	1,041		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

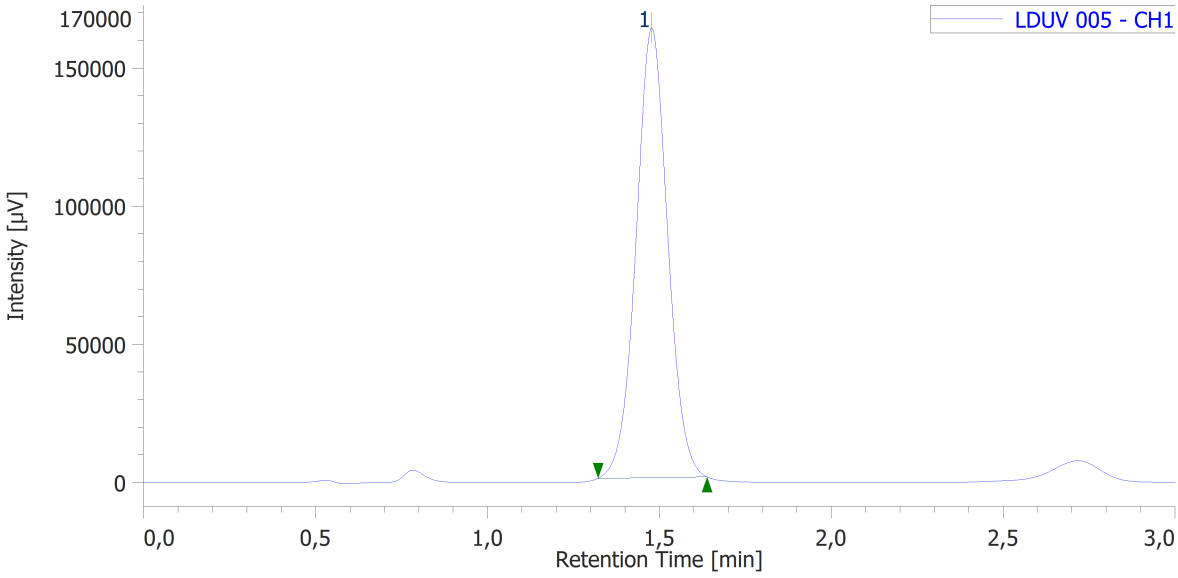

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:49
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:37:35
Volume	10,0 [µL]
Sample #	15
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,477	1038988	162679	100,000	100,000	N/A	1275	N/A	1,035		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

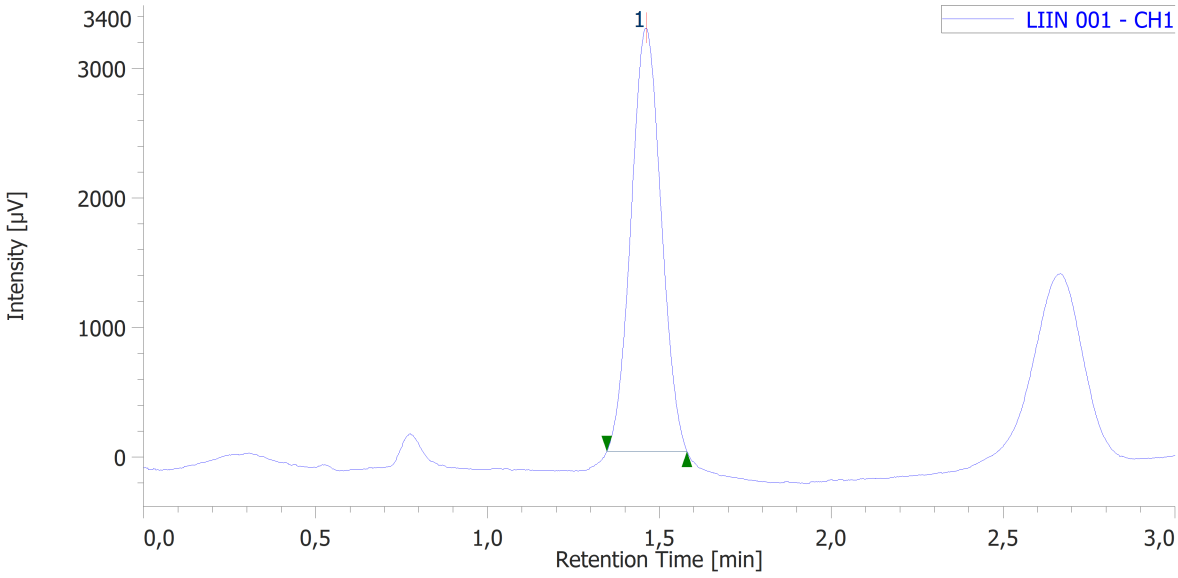

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:49
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:40:55
Volume	0,1 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,462	19884	3269	100,000	100,000	N/A	1289	N/A	1,021		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

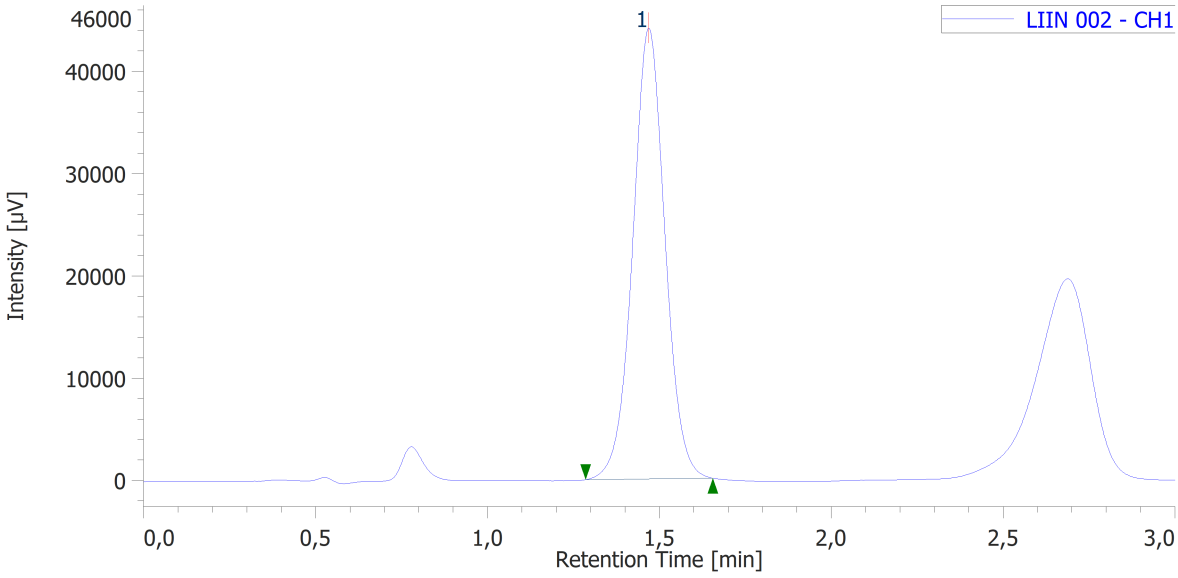

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:50
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:44:18
Volume	5,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,468	287307	44058	100,000	100,000	N/A	1226	N/A	1,024		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

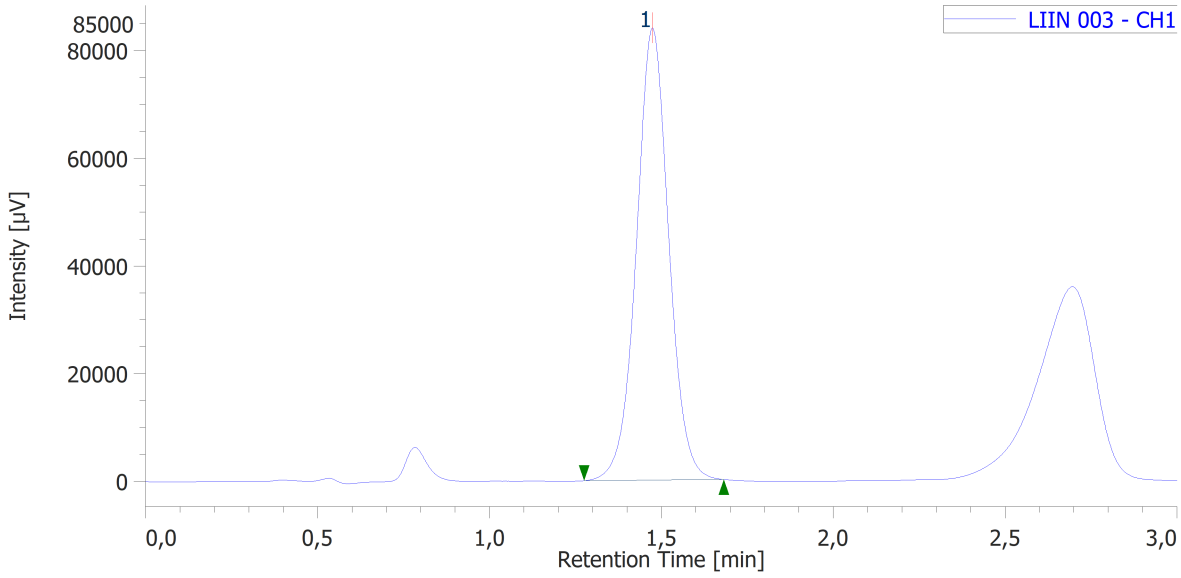

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:50
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:47:41
Volume	10,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,473	548964	83936	100,000	100,000	N/A	1240	N/A	1,025		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

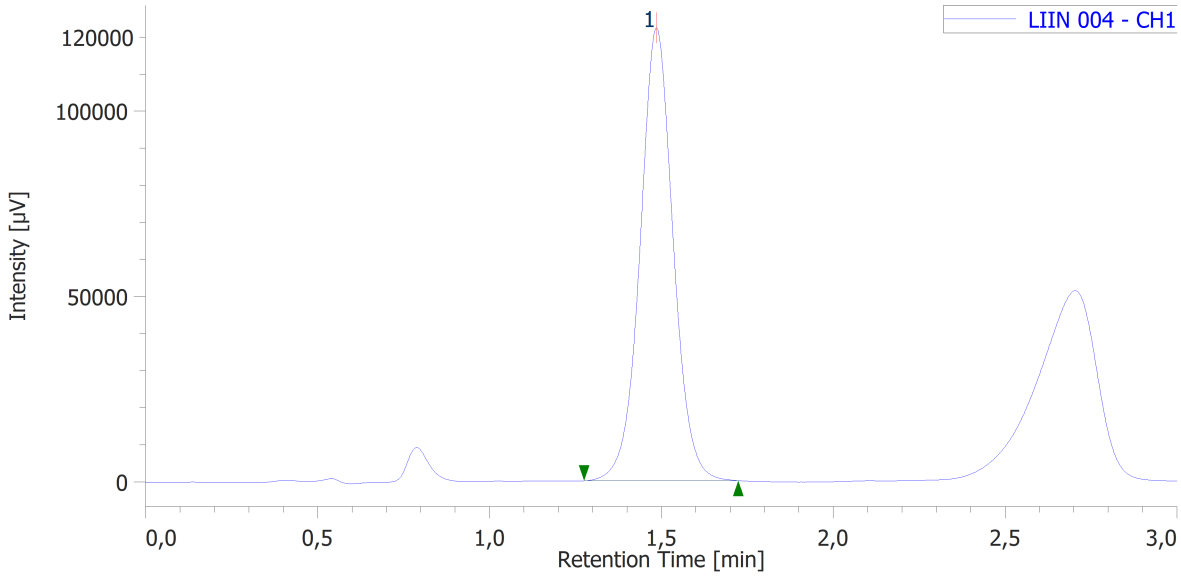

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:50
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:51:08
Volume	15,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 004-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,485	817646	122056	100,000	100,000	N/A	1210	N/A	1,028		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

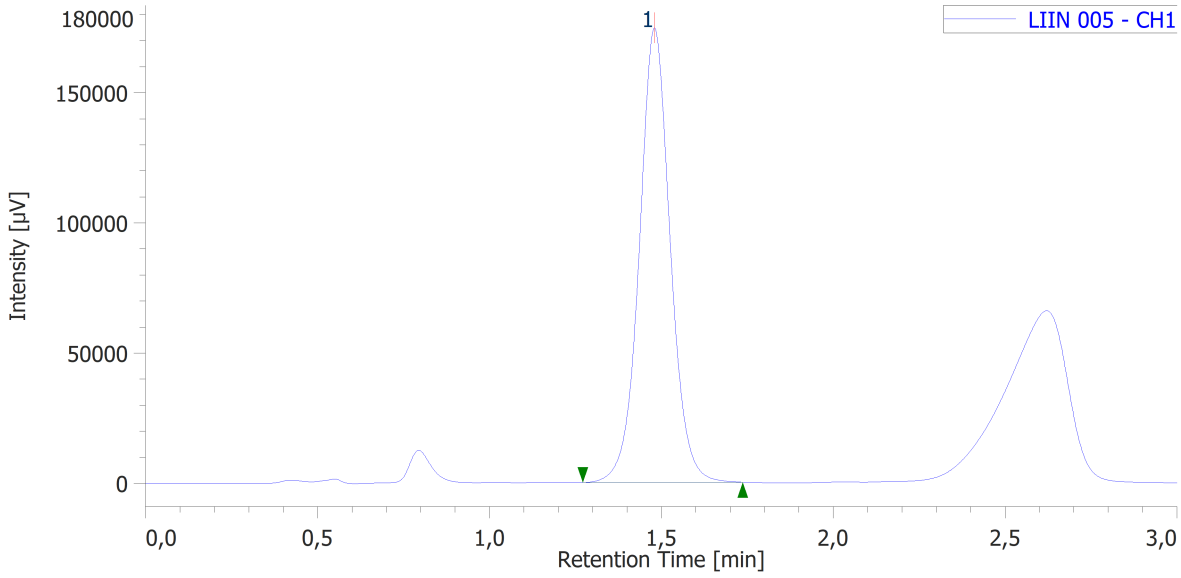

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 09:53:50
Description	
HPLC System Name	01-HP-02
Injection Date	20/07/2023 18:54:35
Volume	20,0 [µL]
Sample #	16
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação HP02
Control Method	Qualificação
Peak ID Table	Qualificação
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 005-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	Cafeína	1	1,480	1090913	174500	100,000	100,000	N/A	1396	N/A	1,030		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

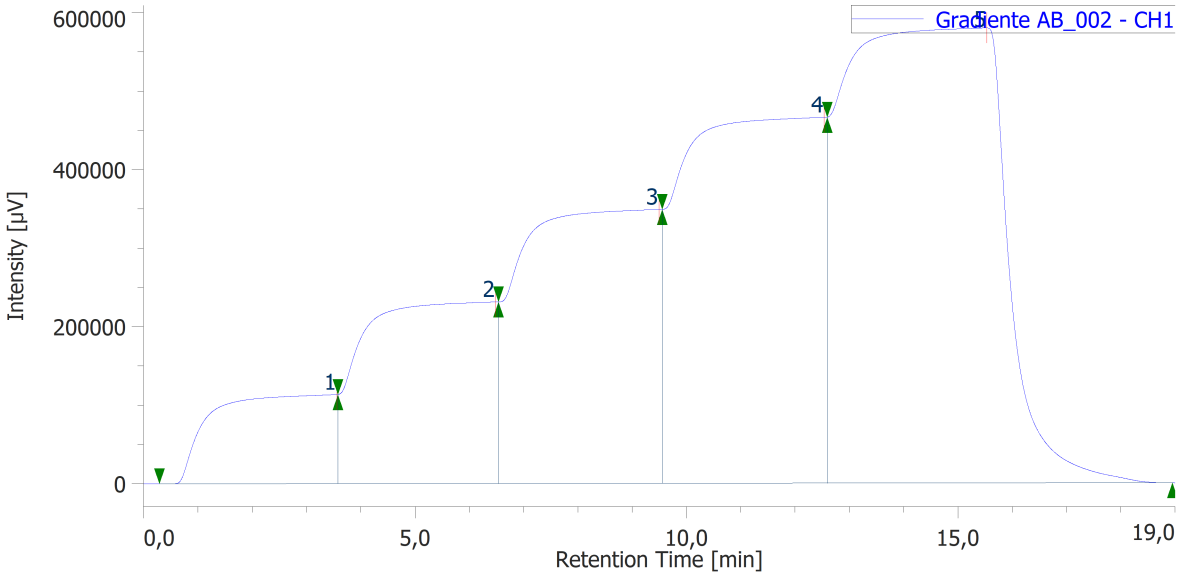

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 11:35:52
Description	
HPLC System Name	01-HP-02
Injection Date	21/07/2023 11:11:09
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	GradienteAB_ HPLC02
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	20%	1	3,560	16987754	113239	5,434	6,518	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,480	37655339	231005	12,046	13,296	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	9,493	59335550	348551	18,982	20,062	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	12,533	81351811	465387	26,025	26,787	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	15,528	117261003	579161	37,513	33,336	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver

Chromatogram

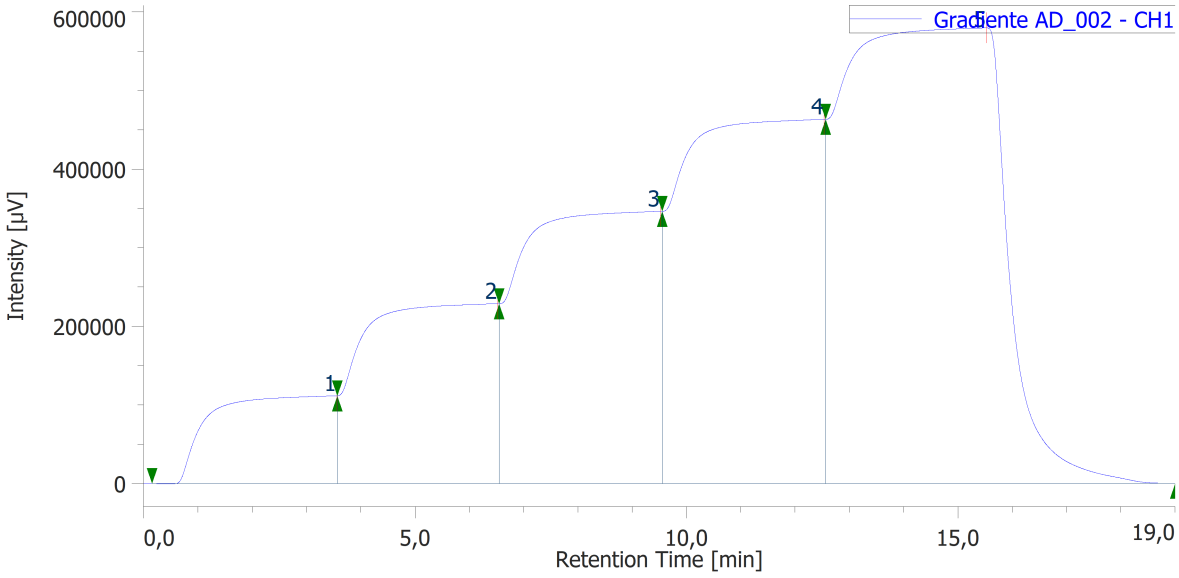

Chromatogram Information	
User Name	QPackSA
Date Modified	21/07/2023 11:53:32
Description	
HPLC System Name	01-HP-02
Injection Date	21/07/2023 11:31:05
Volume	0,0 [µL]
Sample #	-
Project Name	Qualificação
Acquisition Time	19,0 [min]
Acquisition Sequence	
Control Method	GradienteAD_ HPLC02
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente AD_002-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	100 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning	Sinal/Ruído	Ruído
1	20%	1	3,560	16747654	111562	5,387	6,458	N/A	N/A	N/A	N/A		N/A	N/A
2	40%	1	6,522	37557046	228566	12,081	13,231	N/A	N/A	N/A	N/A		N/A	N/A
3	60%	1	9,520	58717357	345828	18,887	20,019	N/A	N/A	N/A	N/A		N/A	N/A
4	80%	1	12,533	80153480	462675	25,782	26,782	N/A	N/A	N/A	N/A		N/A	N/A
5	100%	1	15,522	117712098	578908	37,863	33,511	N/A	N/A	N/A	N/A		N/A	N/A

Creator QPackSA
Reviewer
Approver