
SAMPLE INFORMATION

Sample Name:	FID MDL - 1	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 15:01:31 AMT		
Date Processed:	25/07/2024 07:53:13 AMT		

Auto-Scaled Chromatogram

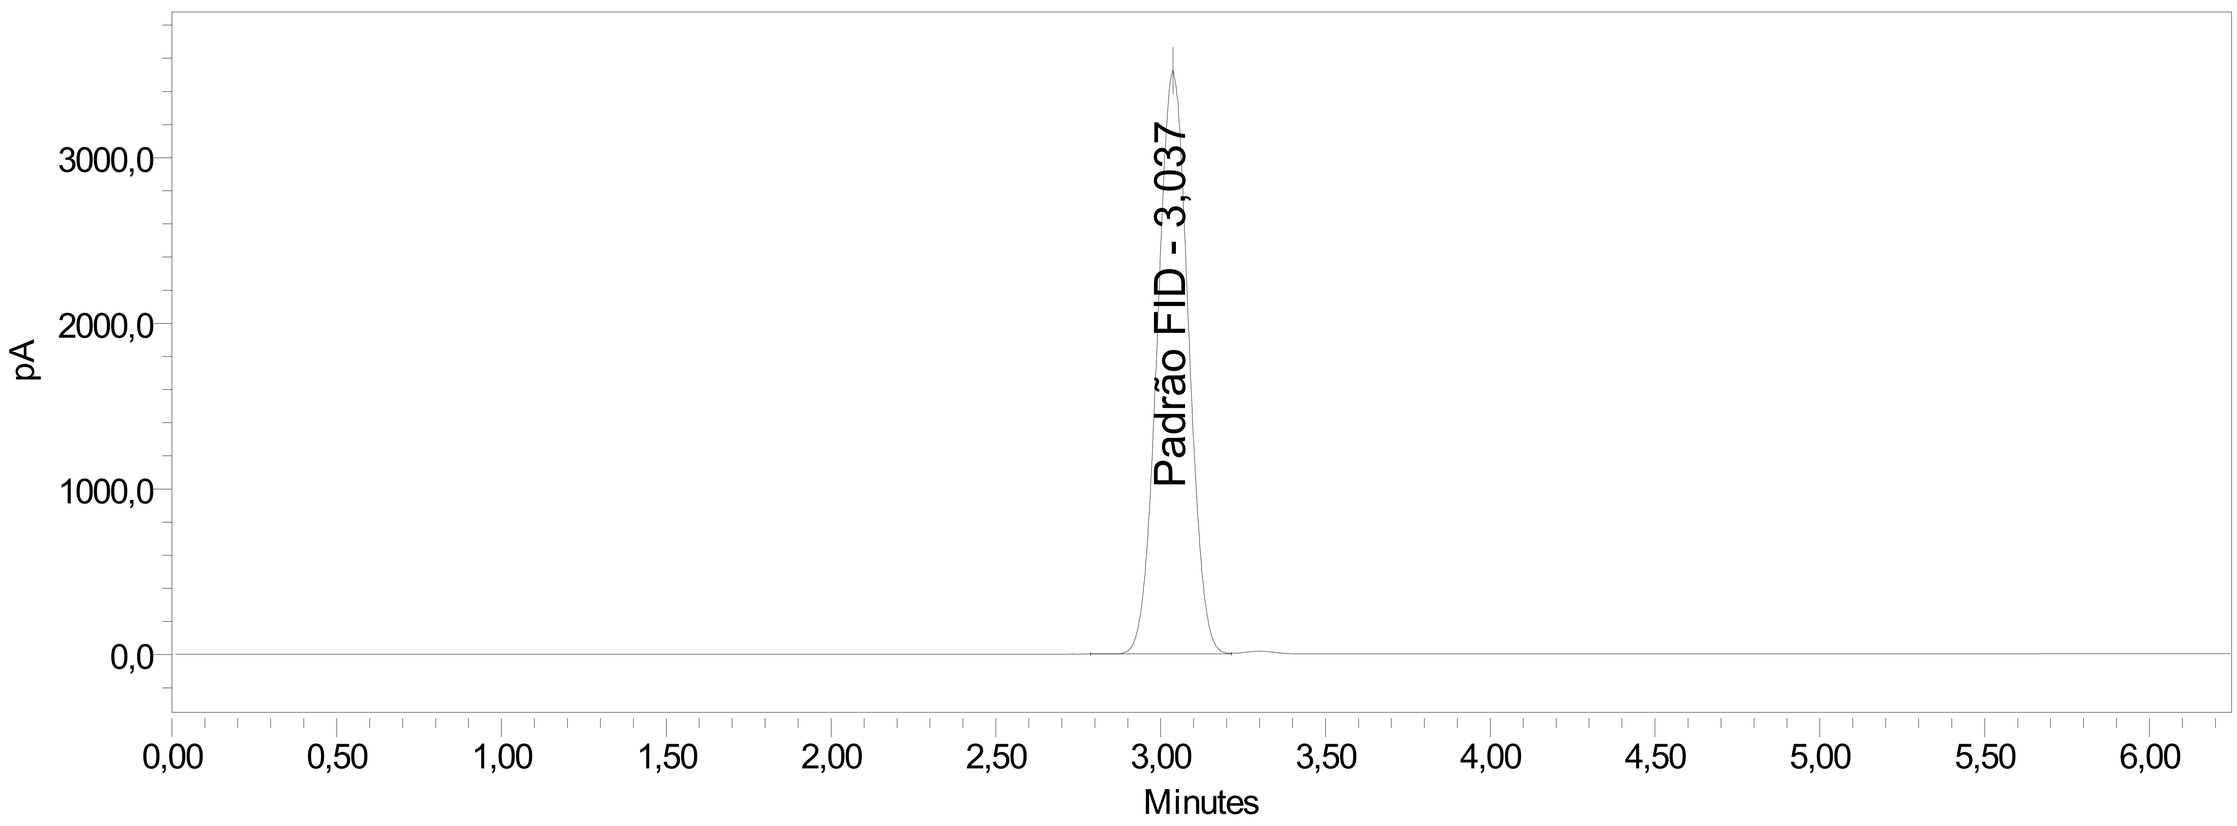

SampleName FID MDL - 1; Date Acquired 24/07/2024 15:01:31 AMT; Date Processed 25/07/2024 07:53:13 AMT


Peak Results

Padrão FID	3,037	23101,062296	1,0000	23101,0623		1,000000		1446

SAMPLE INFORMATION

Sample Name:	FID MDL - 2	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 15:11:42 AMT		
Date Processed:	25/07/2024 07:53:19 AMT		

Auto-Scaled Chromatogram

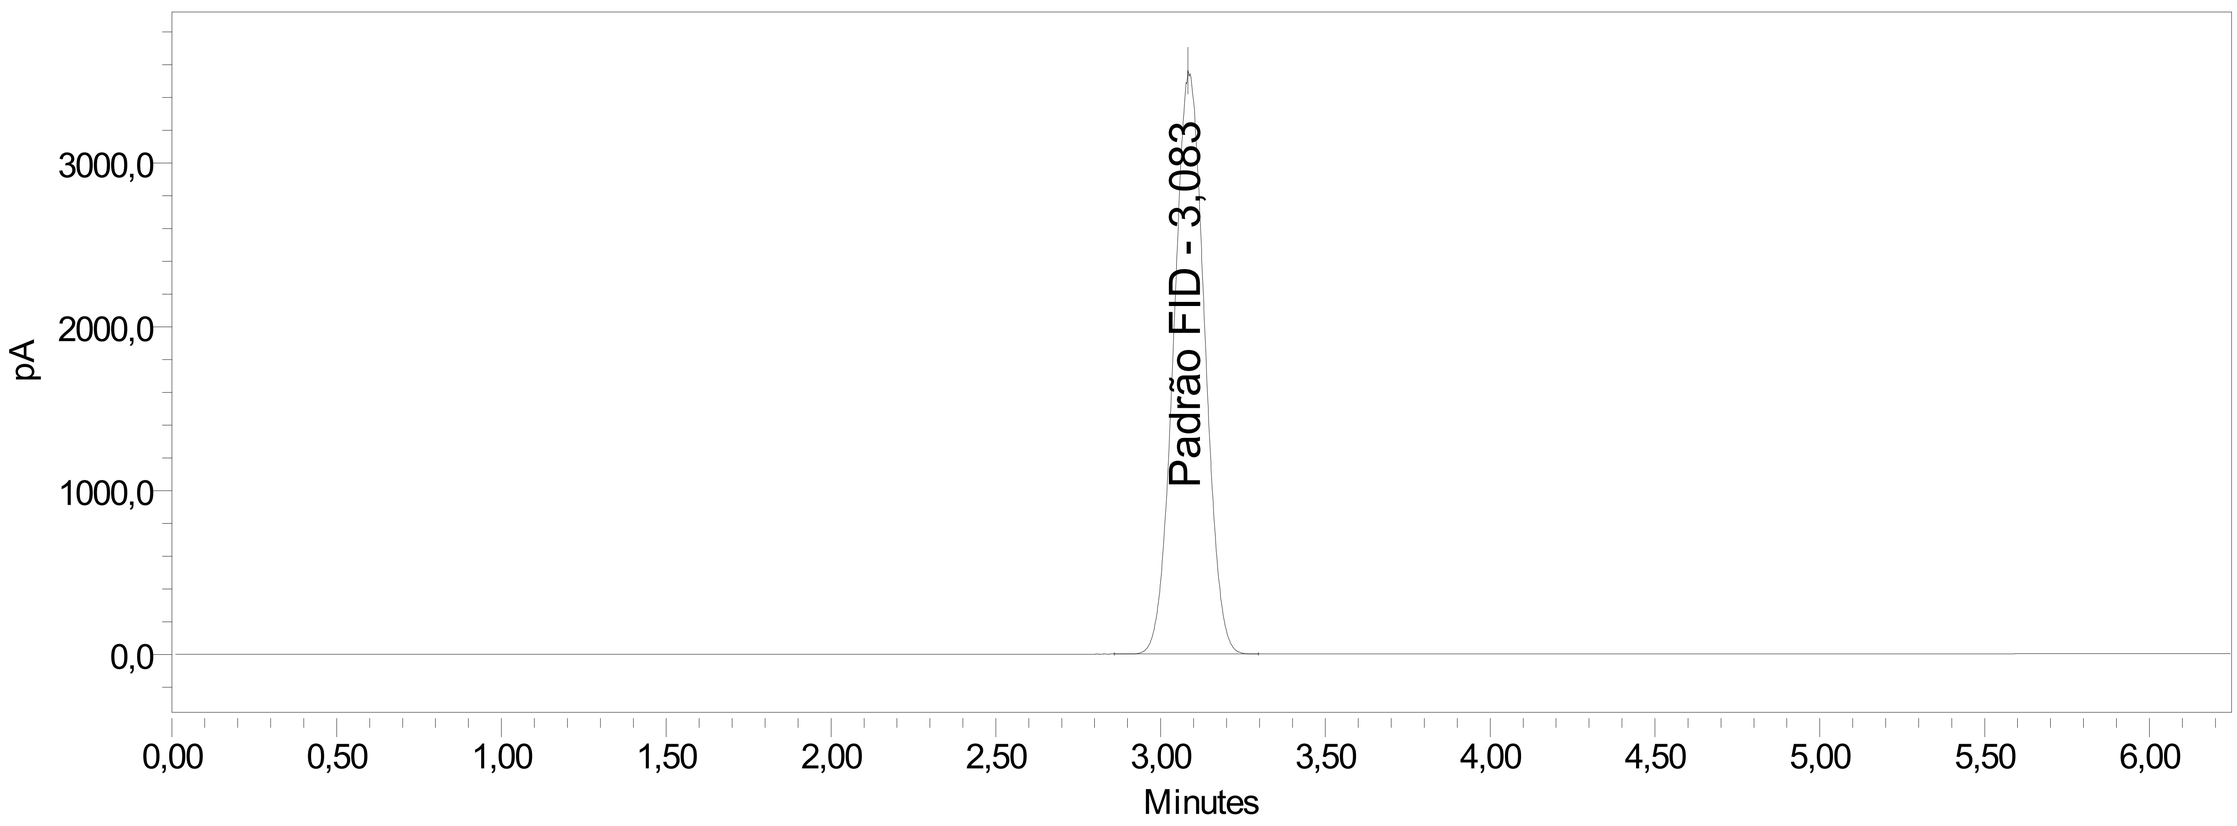

SampleName FID MDL - 2; Date Acquired 24/07/2024 15:11:42 AMT; Date Processed 25/07/2024 07:53:19 AMT


Peak Results

Padrão FID	3,083	23118,490956	1,0000	23118,4910		1,000000		1449

SAMPLE INFORMATION

Sample Name:	FID MDL - 3	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 15:22:03 AMT		
Date Processed:	25/07/2024 07:53:25 AMT		

Auto-Scaled Chromatogram

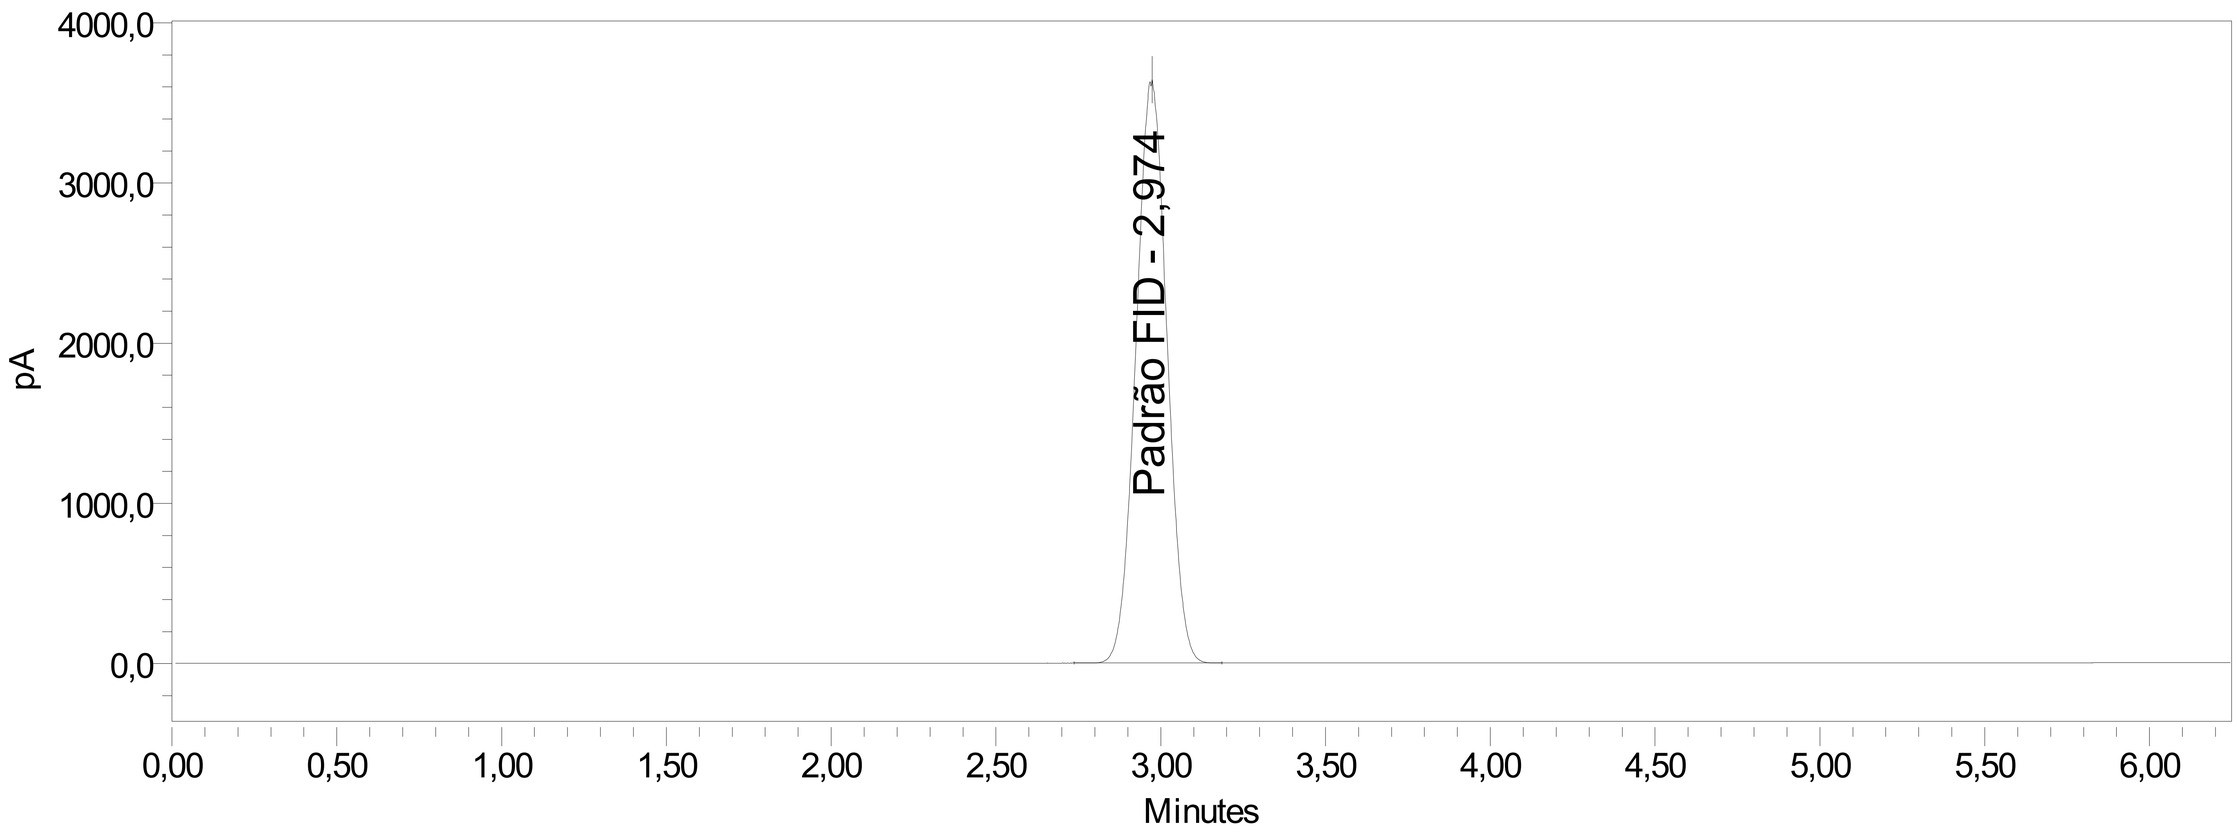


Peak Results

Padrão FID	2,974	23798,060082	1,0000	23798,0601		1,000000		1452

SAMPLE INFORMATION

Sample Name:	FID MDL - 4	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 15:42:40 AMT		
Date Processed:	25/07/2024 07:53:37 AMT		

Auto-Scaled Chromatogram

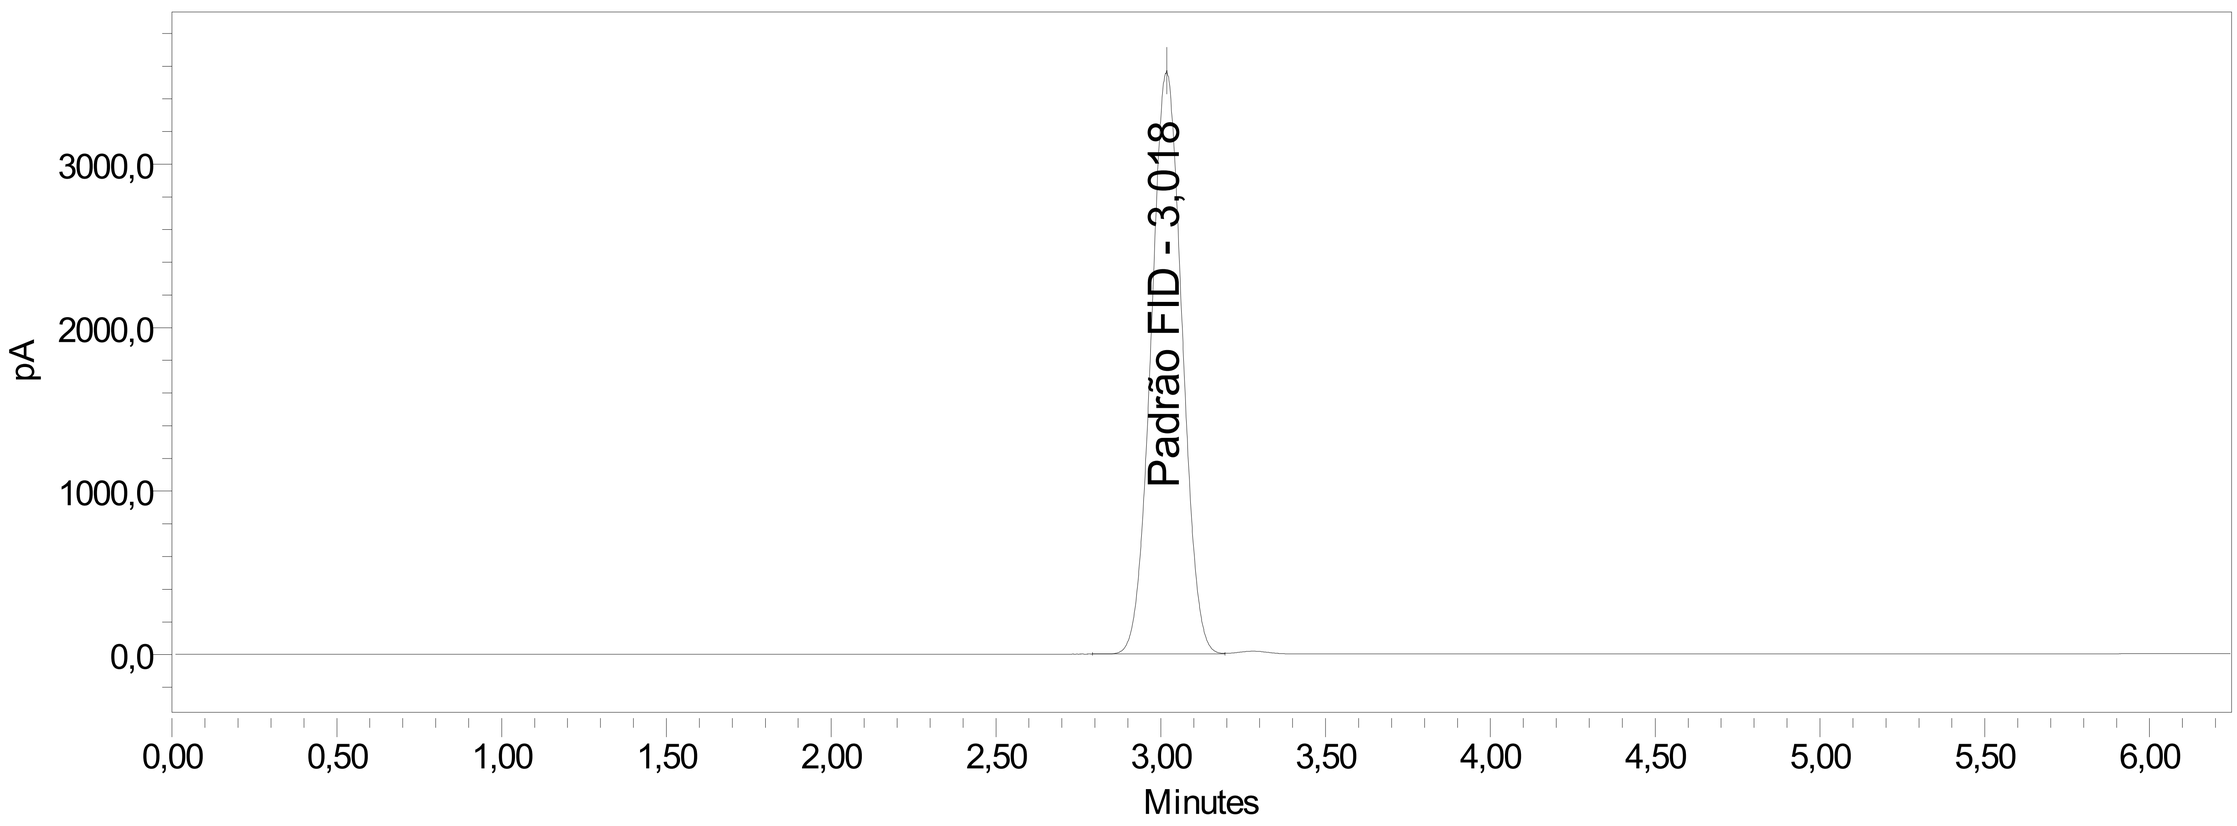

SampleName FID MDL - 4; Date Acquired 24/07/2024 15:42:40 AMT; Date Processed 25/07/2024 07:53:37 AMT


Peak Results

Padrão FID	3,018	23276,326797	1,0000	23276,3268		1,000000		1458

SAMPLE INFORMATION

Sample Name:	FID MDL - 5	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 15:53:05 AMT		
Date Processed:	25/07/2024 07:53:42 AMT		

Auto-Scaled Chromatogram

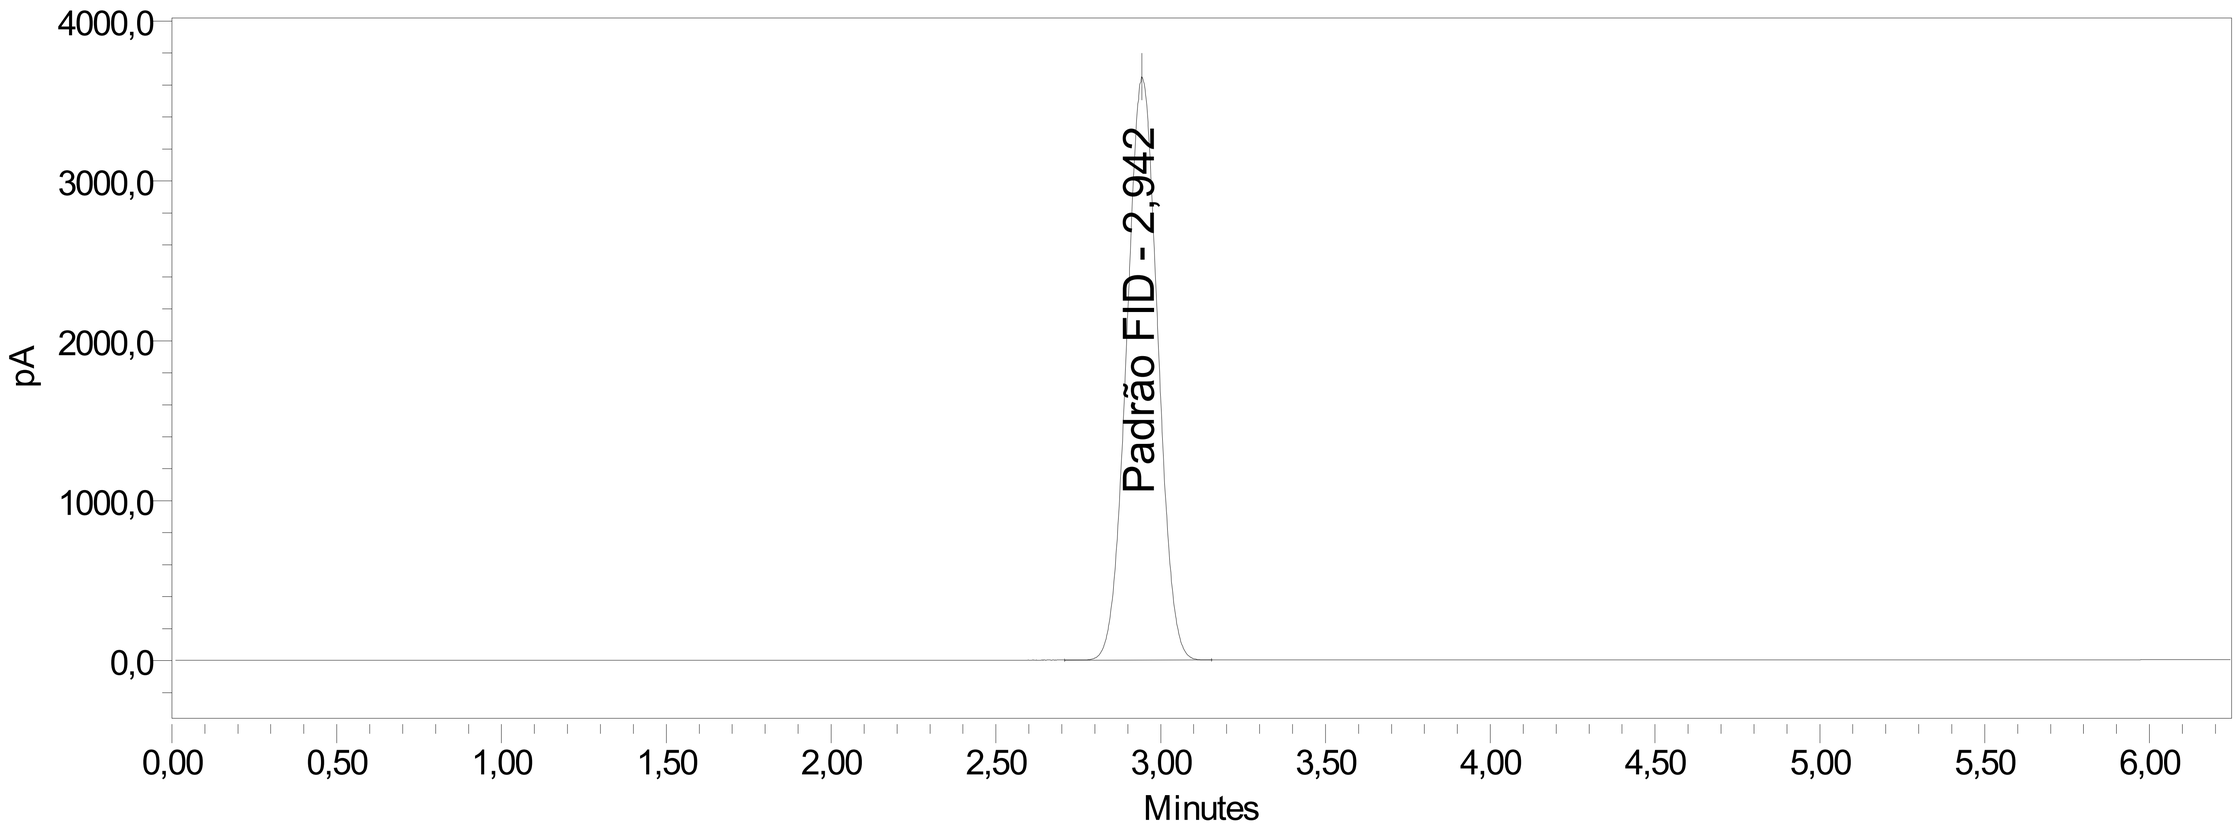

SampleName FID MDL - 5; Date Acquired 24/07/2024 15:53:05 AMT; Date Processed 25/07/2024 07:53:42 AMT


Peak Results

Padrão FID	2,942	23889,145732	1,0000	23889,1457		1,000000		1461

SAMPLE INFORMATION

Sample Name:	FID MDL - 6	Acquired By:	Analista
Sample Type:	Unknown	Sample Set Name:	QPACK QUAL FID MDL
Vial:	502	Acq. Method Set:	QPACK QUAL 6890 24072024
Injection #:	1	Processing Method	QPAC
Injection Volume:	1,00 ul	Channel Name:	GC.0.1
Run Time:	10,0 Minutes	Proc. Chnl. Descr.:	back detector
Date Acquired:	24/07/2024 16:03:26 AMT		
Date Processed:	25/07/2024 07:53:47 AMT		

Auto-Scaled Chromatogram

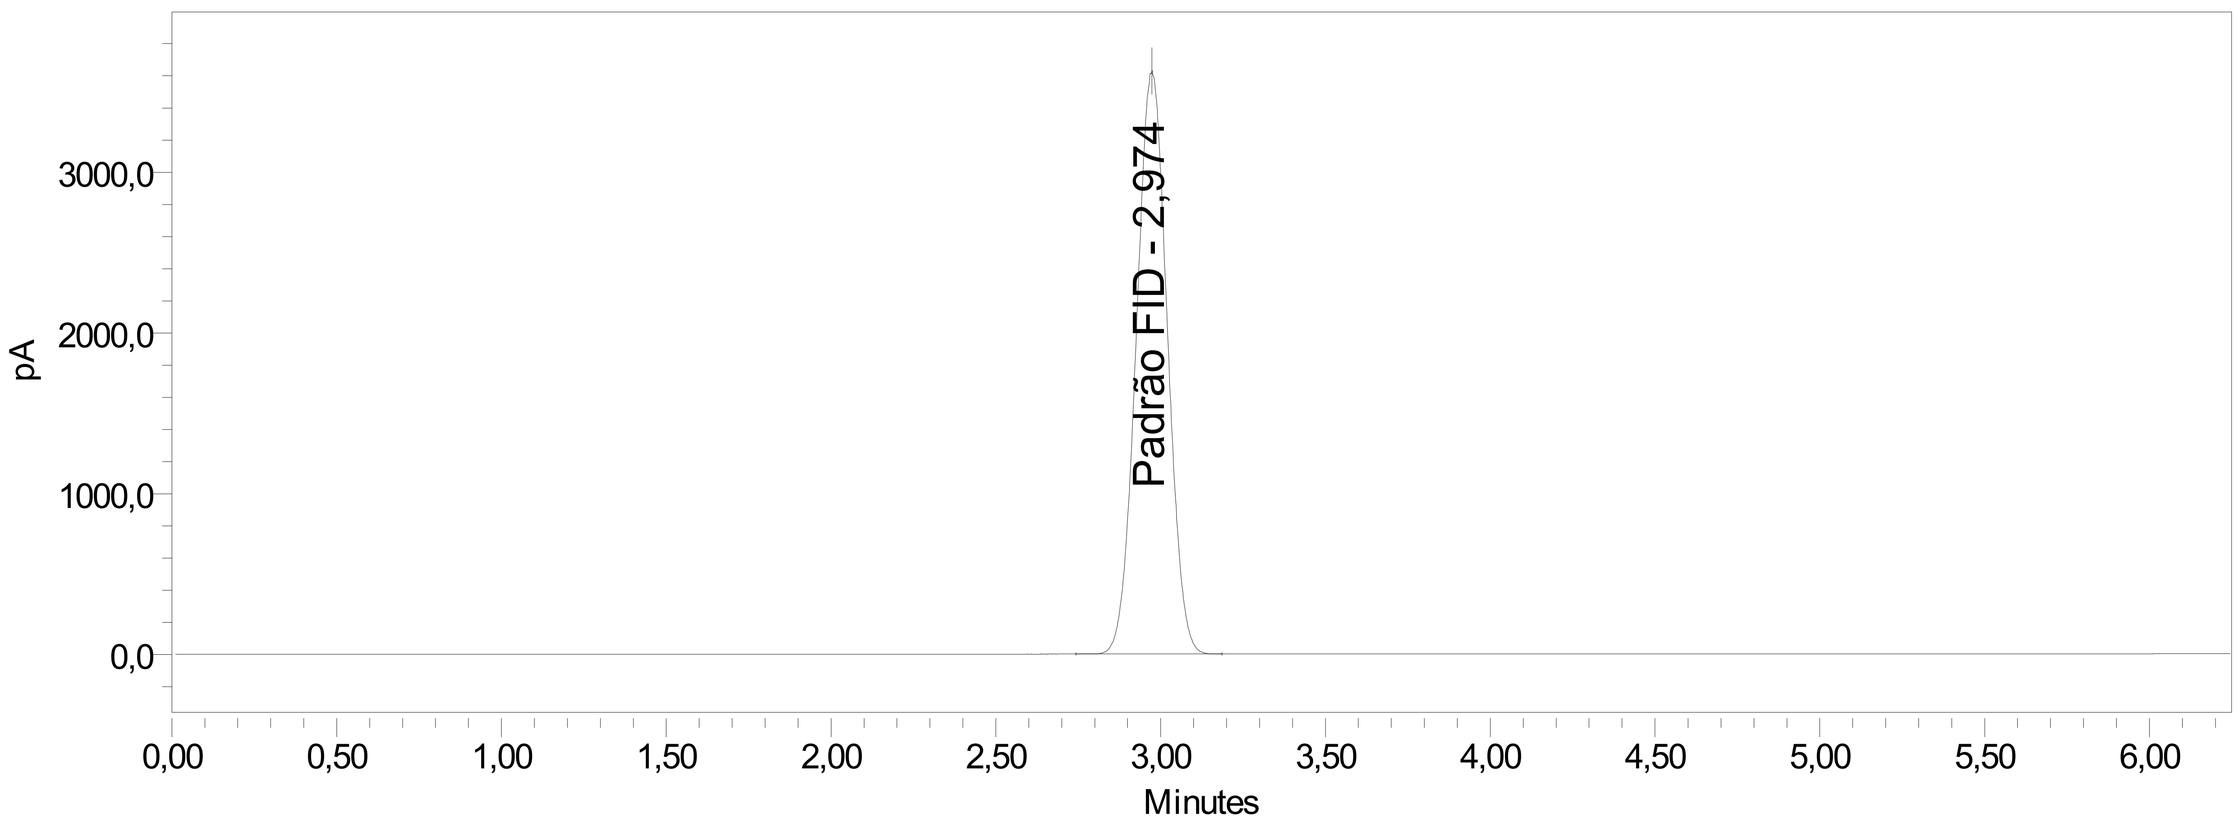

SampleName FID MDL - 6; Date Acquired 24/07/2024 16:03:26 AMT; Date Processed 25/07/2024 07:53:47 AMT

Peak Results

Padrão FID	2,974	23709,097685	1,0000	23709,0977		1,000000		1464