
Peak Find - EDUV_002 UV_tR1.20 D.jws

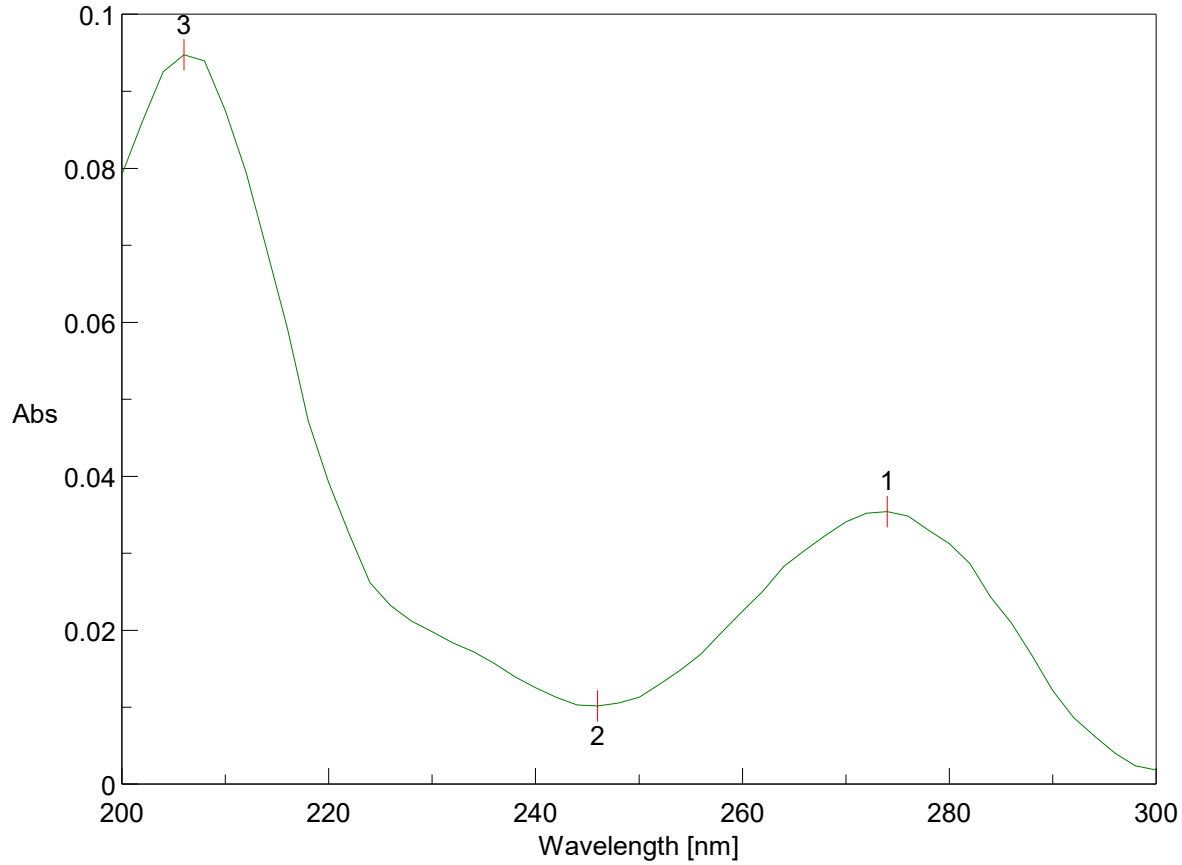

[Comments]

User	QPackSA
Division	---
Company	JP INDÚSTRIA FARMACÊUTICA S.A
Creation date	08-Jul-26 17:41
Date modified	08-Jul-26 17:42

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	600 nm
Data interval	2 nm
Data points	200


[Measurement Information]

Instrument Name	X-LC 3075UV
Model Name	X-LC 3075UV
Serial No.	0000000000
ROM version	V6.45

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.035401	2	246	0.010134
3	206	0.0947195			

Chromatogram

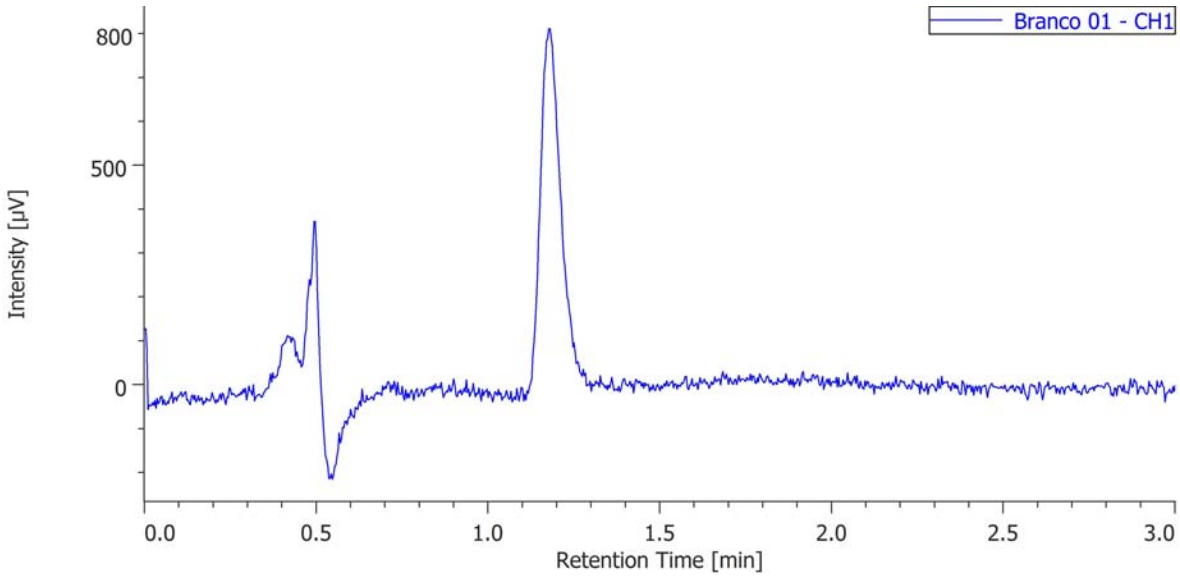


Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:27:48
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:24:47
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

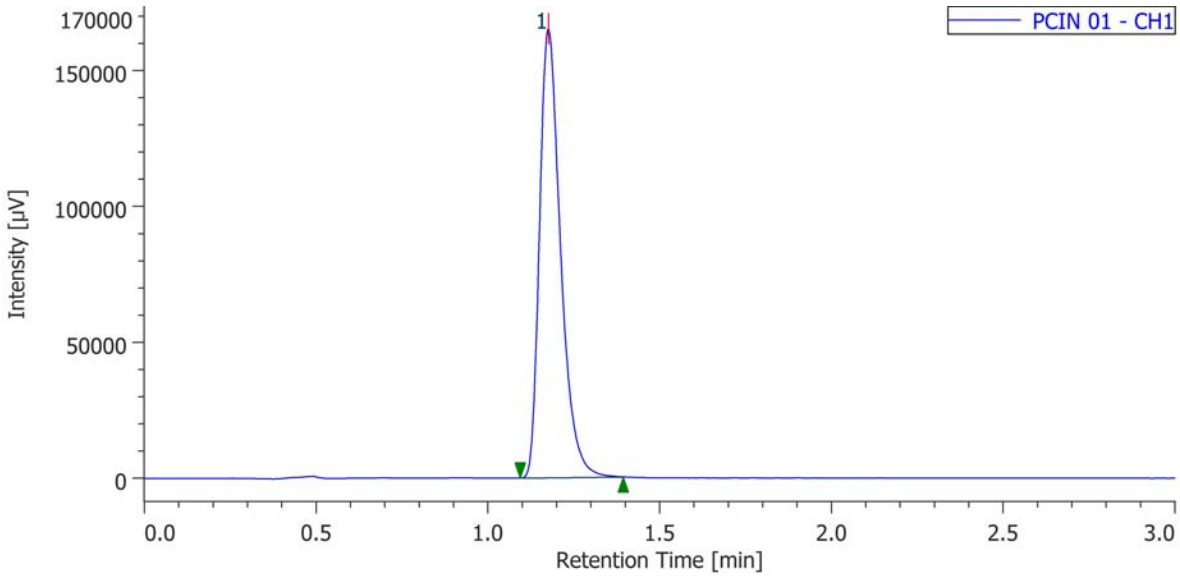

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:32:02
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:29:00
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	702462	165071	100	100.000	N/A	1872	N/A	1.373	

Creator QPackSA
Reviewer
Approver

Chromatogram

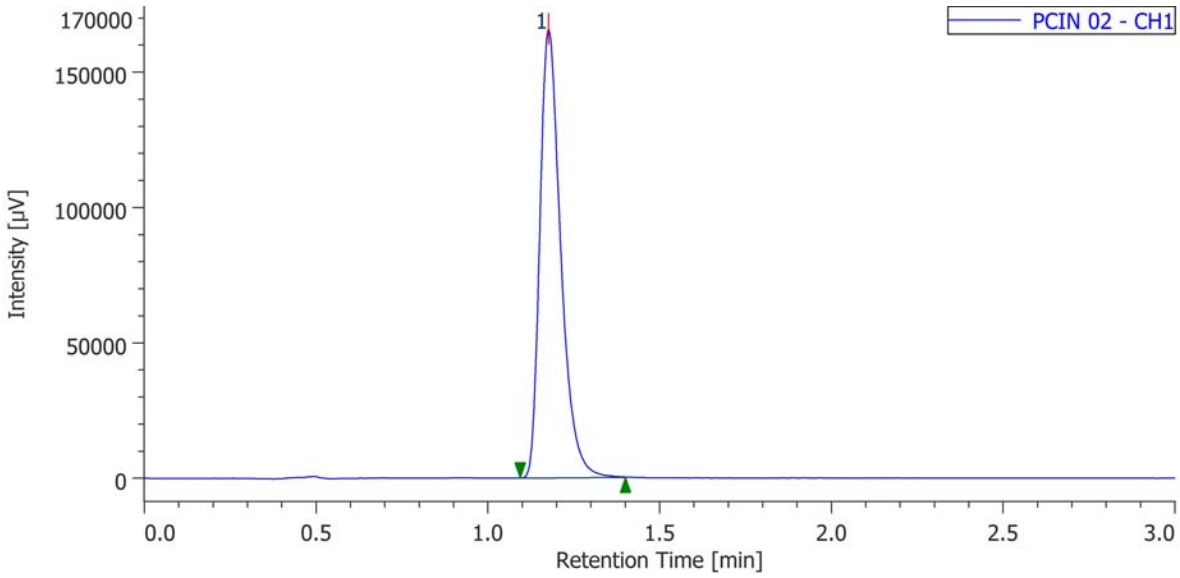

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:36:14
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:33:11
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	700237	165762	100	100.000	N/A	1899	N/A	1.389	

Creator QPackSA
Reviewer
Approver

Chromatogram

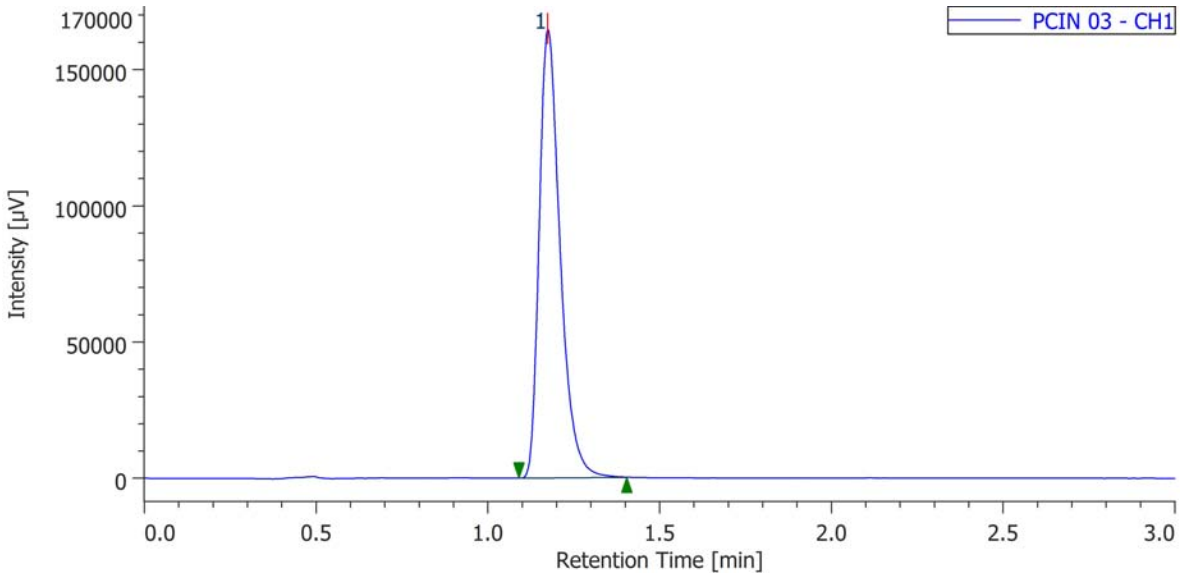

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:40:24
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:37:22
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.17	696698	164709	100	100.000	N/A	1886	N/A	1.429	

Creator QPackSA
Reviewer
Approver

Chromatogram

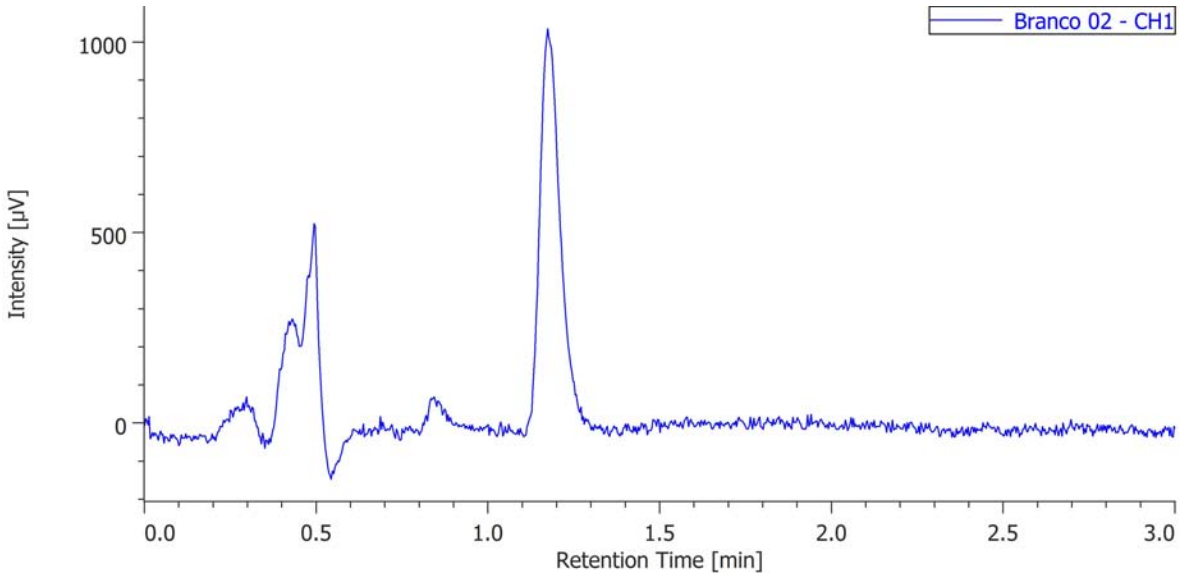


Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:44:36
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:41:33
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

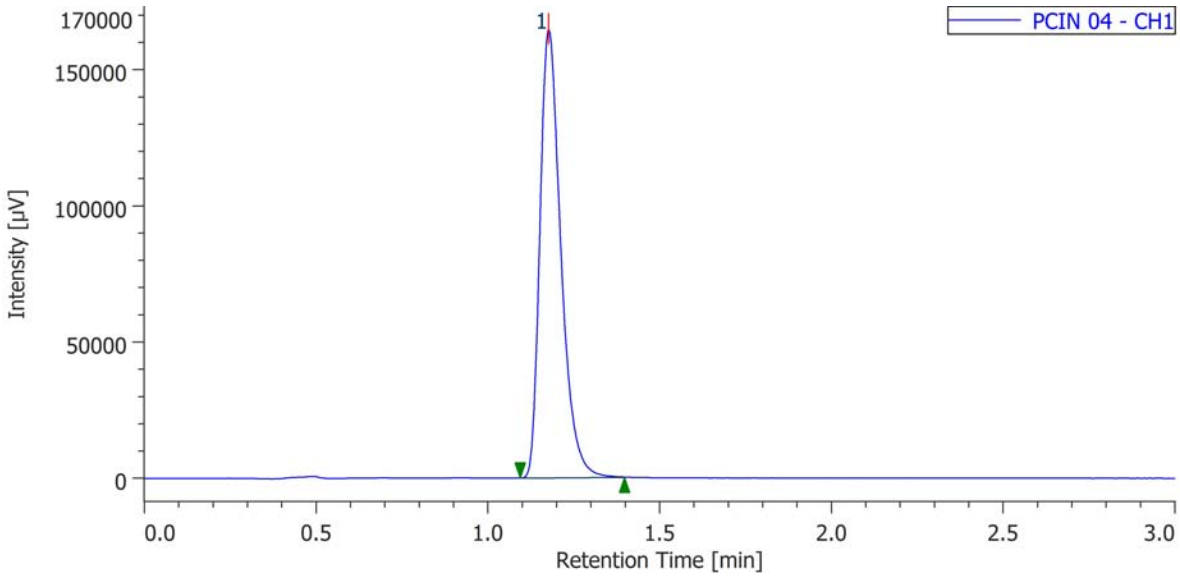

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:48:46
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:45:44
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	696059	164722	100	100.000	N/A	1889	N/A	1.391	

Creator QPackSA
Reviewer
Approver

Chromatogram

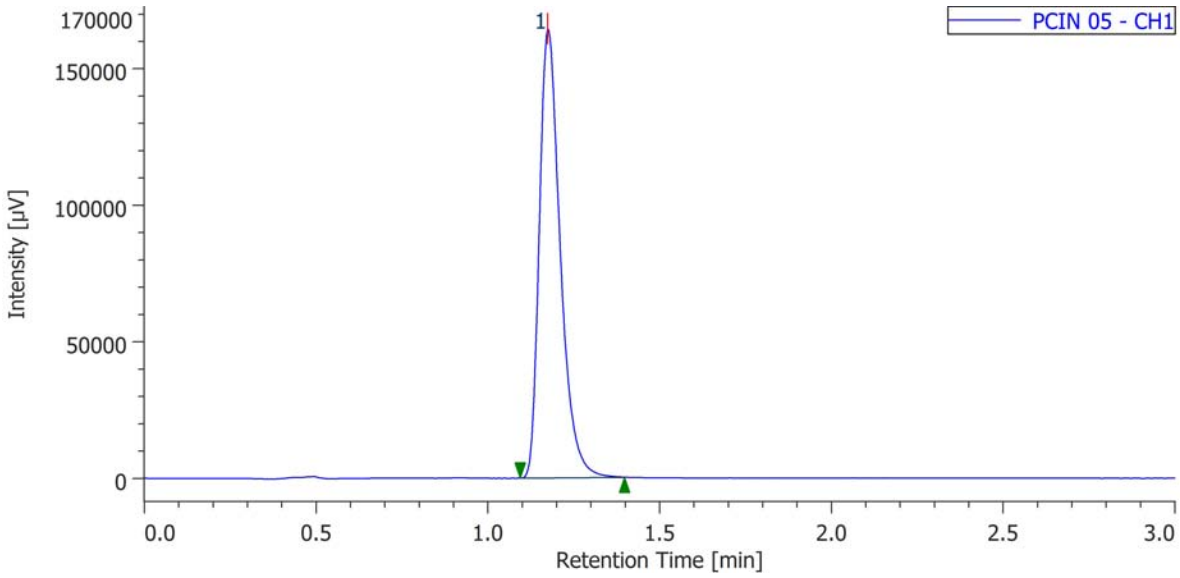

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:52:58
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:49:56
Volume	10.0 [µL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.17	695847	164375	100	100.000	N/A	1884	N/A	1.442	

Creator QPackSA
Reviewer
Approver

Chromatogram

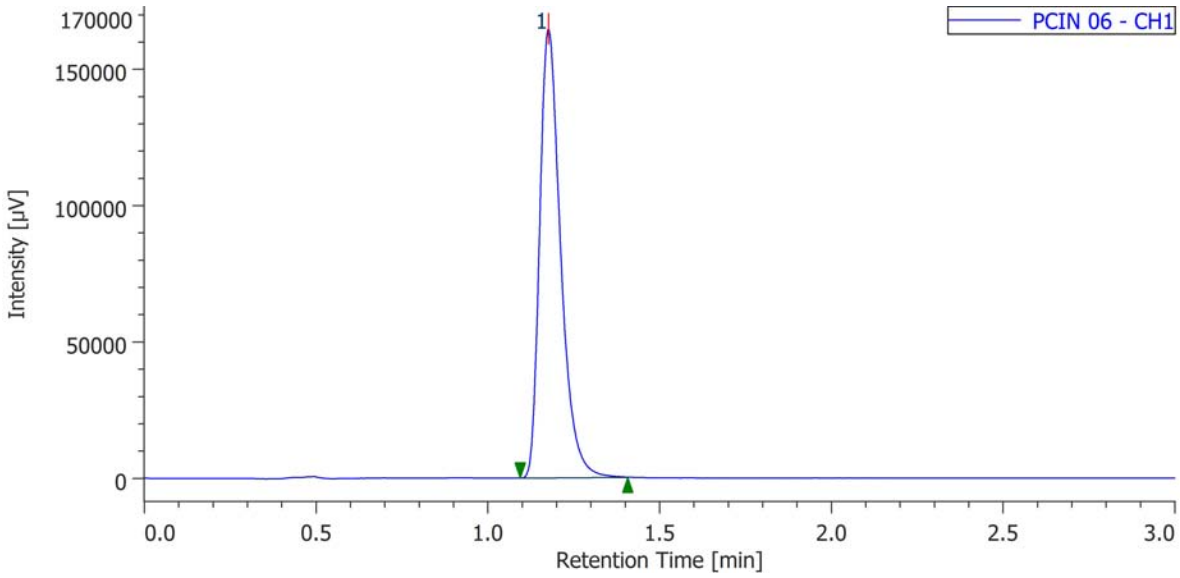

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 18:57:08
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:54:07
Volume	10.0 [μL]
Sample #	3
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 06-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	697794	164586	100	100.000	N/A	1888	N/A	1.380	

Creator QPackSA
Reviewer
Approver

Chromatogram

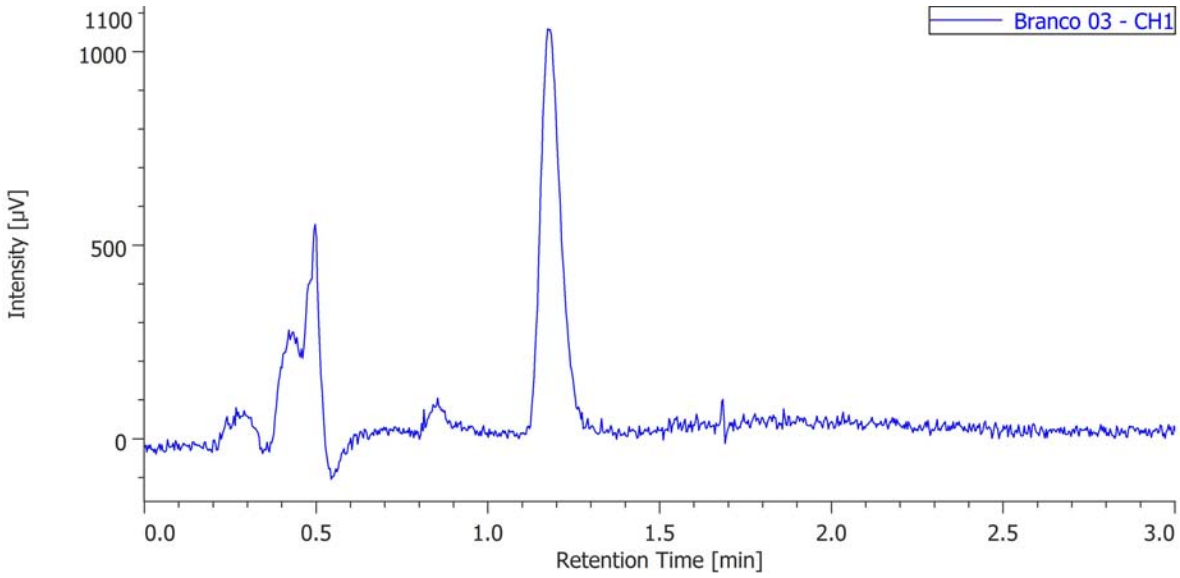


Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:01:20
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 18:58:18
Volume	10.0 [µL]
Sample #	2
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

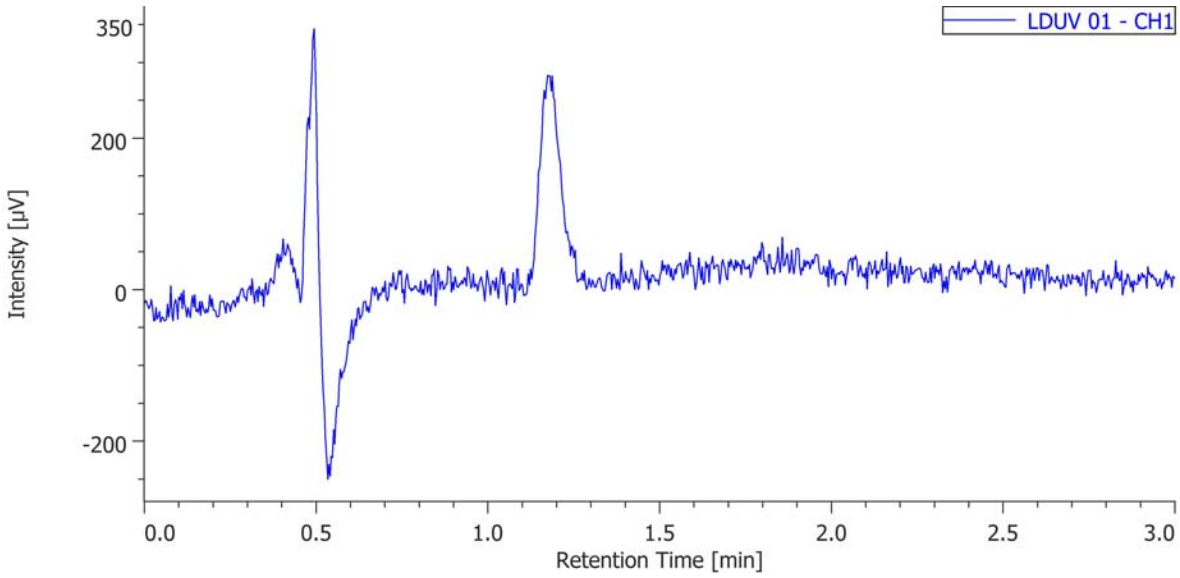


Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:05:34
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:02:31
Volume	10.0 [µL]
Sample #	4
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

Creator QPackSA
Reviewer
Approver

Chromatogram

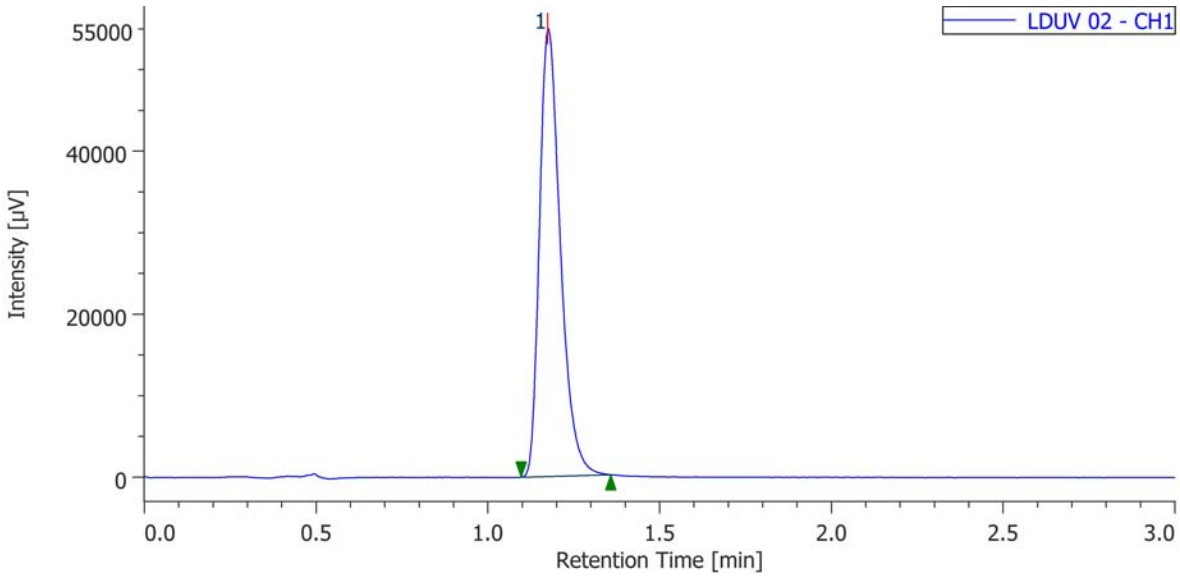

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:09:46
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:06:45
Volume	10.0 [µL]
Sample #	5
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.17	232260	54886	100	100.000	N/A	1858	N/A	1.438	

Creator QPackSA
Reviewer
Approver

Chromatogram

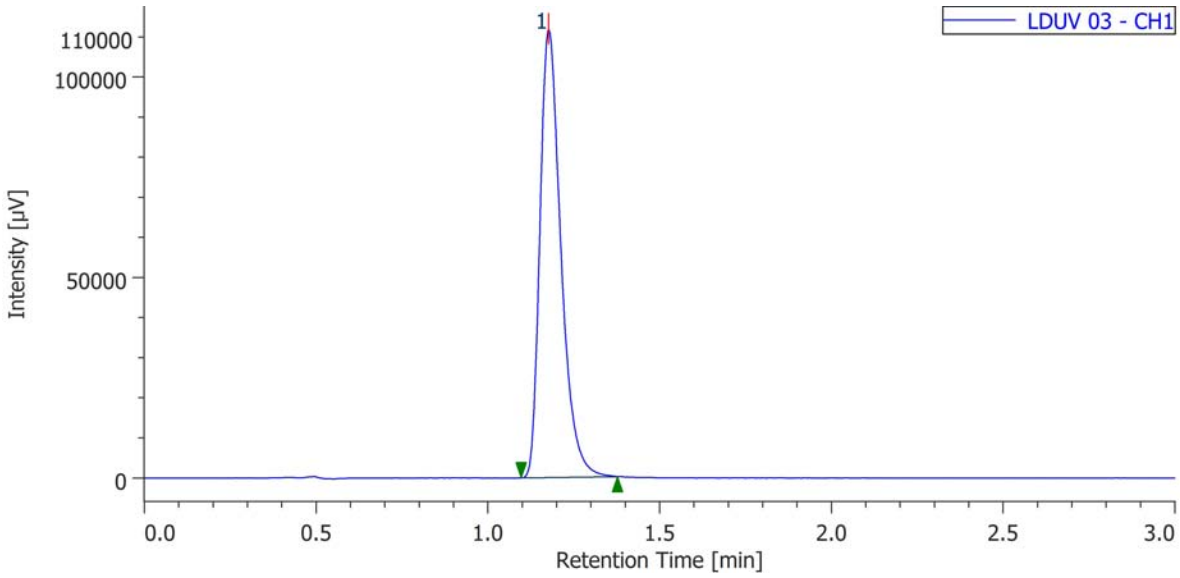

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:14:00
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:10:58
Volume	10.0 [µL]
Sample #	6
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	473366	111806	100	100.000	N/A	1884	N/A	1.398	

Creator QPackSA
Reviewer
Approver

Chromatogram

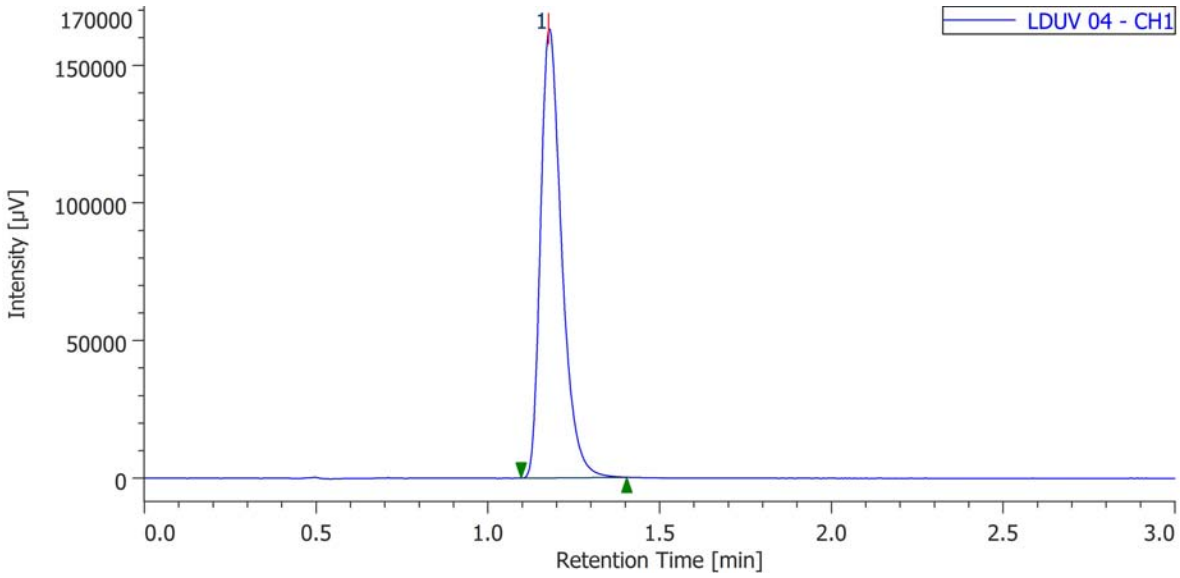

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:18:16
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:15:14
Volume	10.0 [µL]
Sample #	7
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	697158	163064	100	100.000	N/A	1848	N/A	1.449	

Creator QPackSA
Reviewer
Approver

Chromatogram

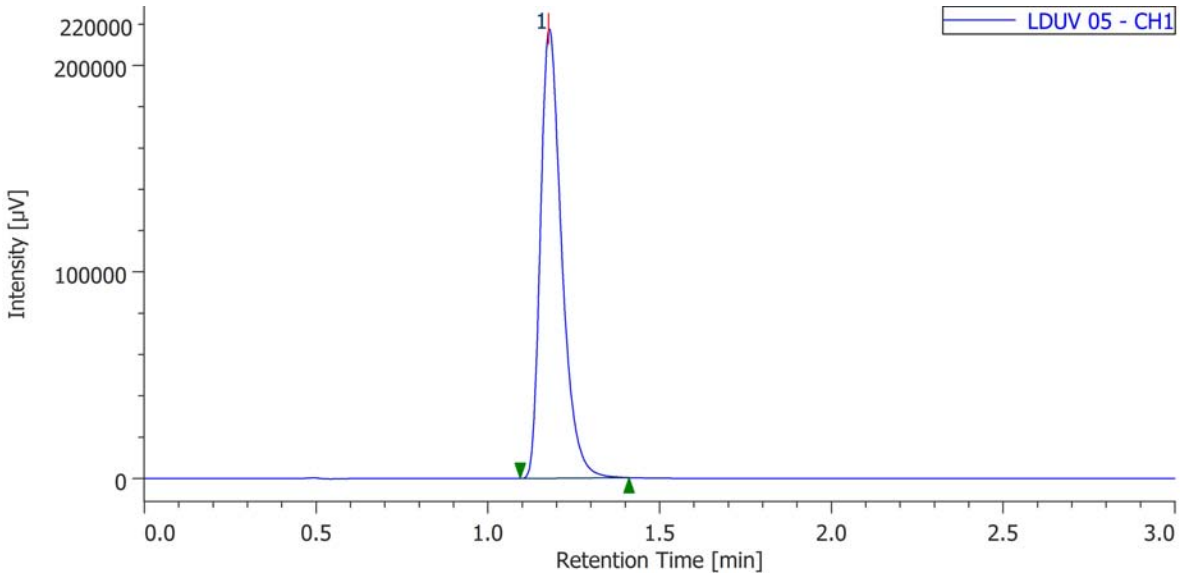

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:22:32
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:19:30
Volume	10.0 [µL]
Sample #	8
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	933145	217502	100	100.000	N/A	1839	N/A	1.449	

Creator QPackSA
Reviewer
Approver

Chromatogram

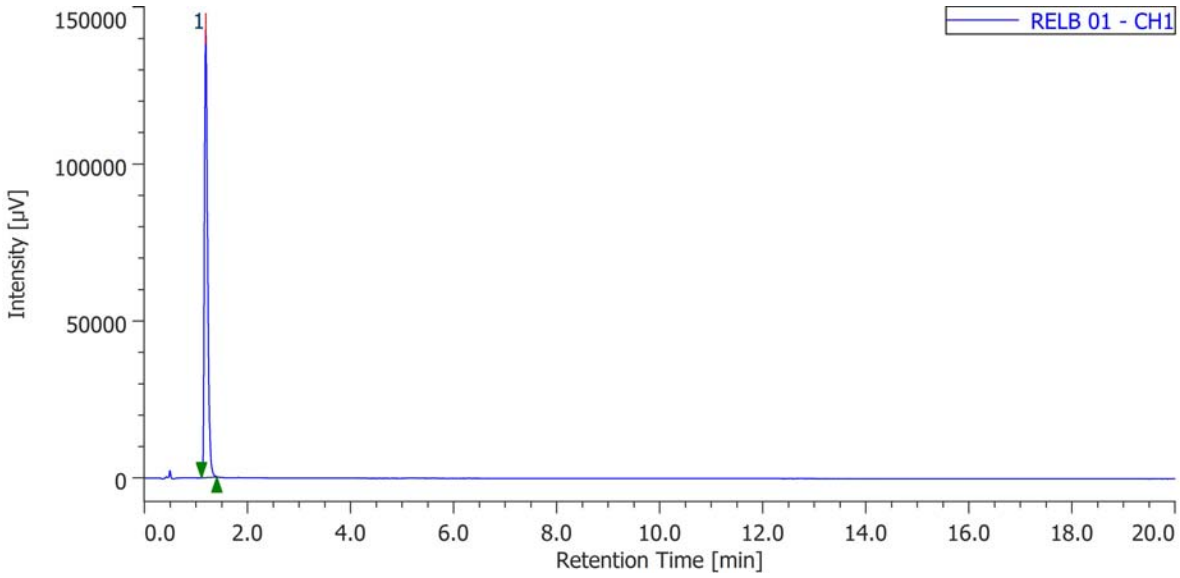

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:43:52
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:23:50
Volume	20.0 [µL]
Sample #	9
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	Qualificação
Control Method	RELB
Peak ID Table	Cafeina
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	RELB 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.19	612403	142861	100	100.000	N/A	1880	N/A	1.396	


Creator QPackSA
Reviewer
Approver

Certificado Nº: 340/26-RELB	Início da Qualificação: 08/07/2026	Página 1 de 3	

Resultado obtido na altura do pico

	ALTURA DO PICO (mAU)
Resultado:	142,861

Chromatogram

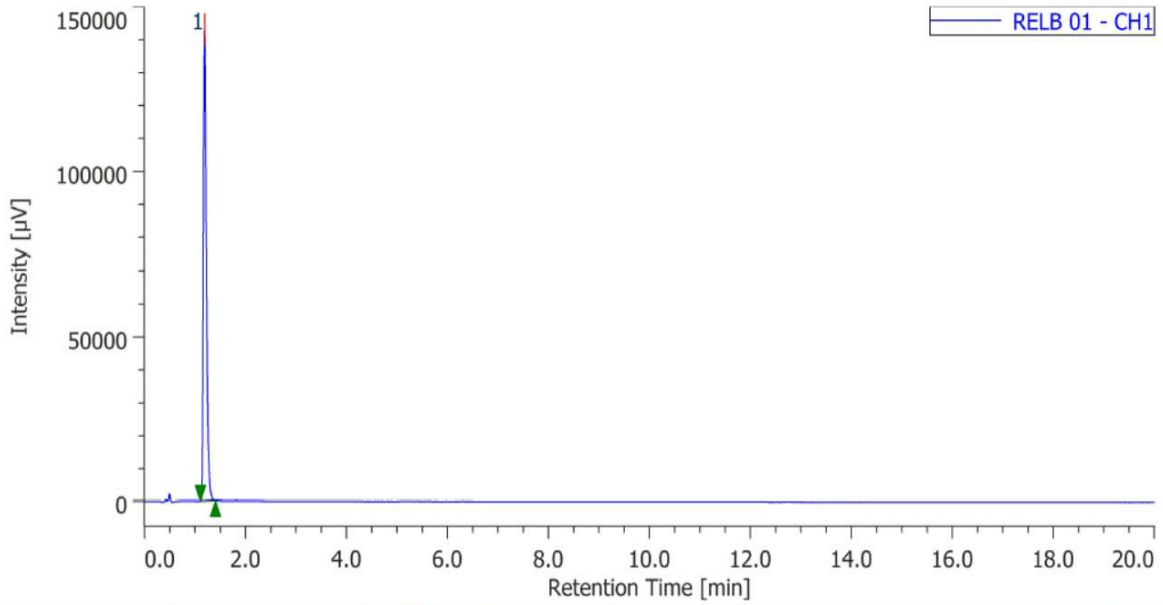


#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.19	612403	142861	100	100.000	N/A	1880	N/A	1.396	

Certificado Nº: 340/26-RELB	Início da Qualificação: 08/07/2026	Página 2 de 3

Resultado obtido no teste de sinal/ruído

Resultado:	Ruído (mAU)
VALOR MÁXIMO:	-0,0161
VALOR MÍNIMO:	-0,0179
	Ruído
	0,0018

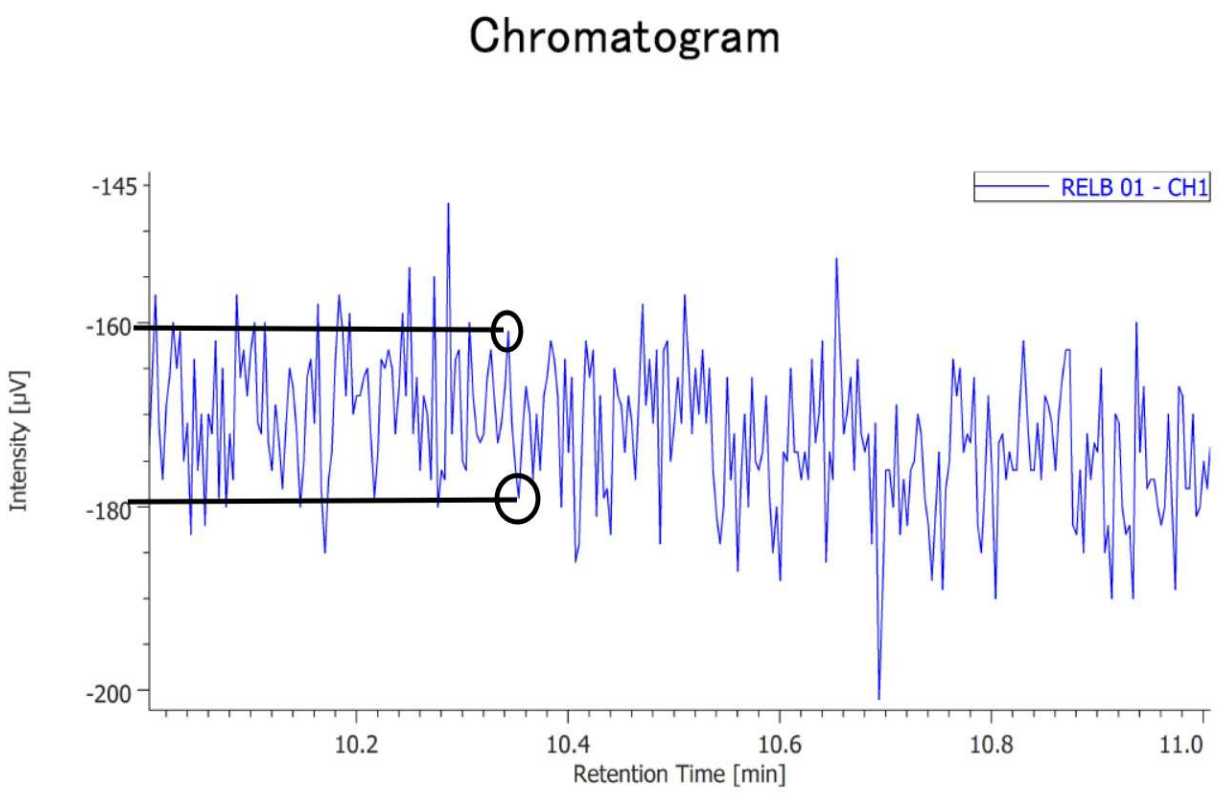


Certificado Nº: 340/26-RELB	Início da Qualificação: 08/07/2026	Página 3 de 3


Resultado obtido no teste estabilidade da linha de base

Estabilidade da Linha de Base	Diferença 20 min	Diferença 60 min
VALOR MÁXIMO:	-0,0150	0,0396
VALOR MÍNIMO:	-0,0282	
Resultado:	0,0132	

Chromatogram

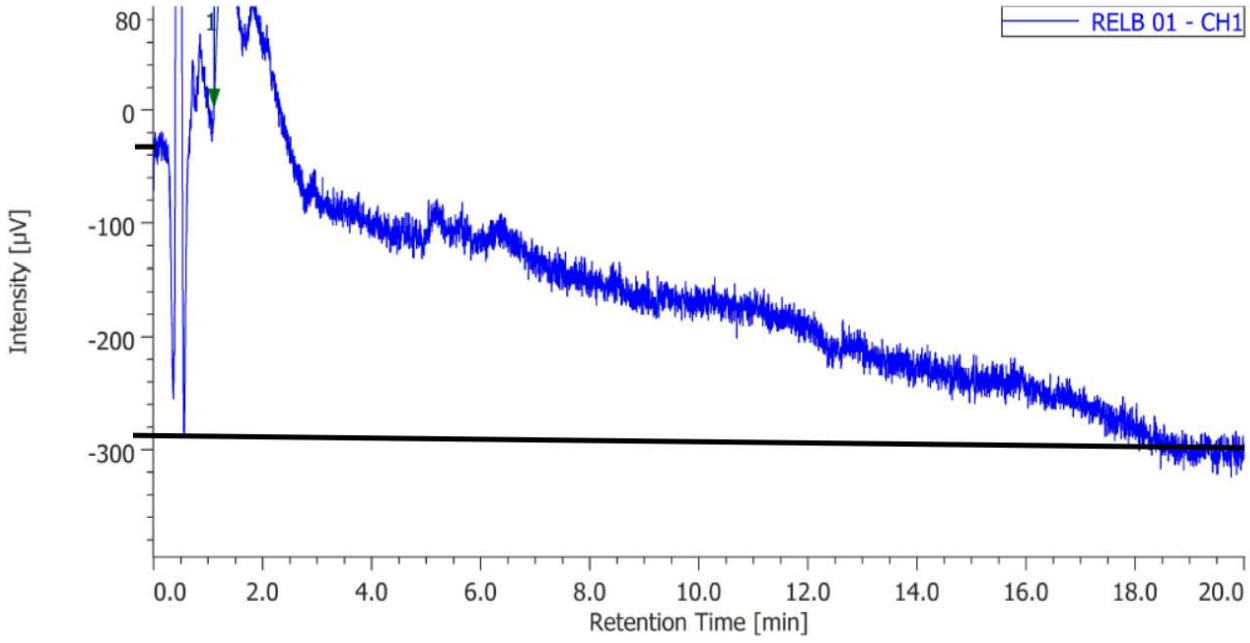

Chromatogram

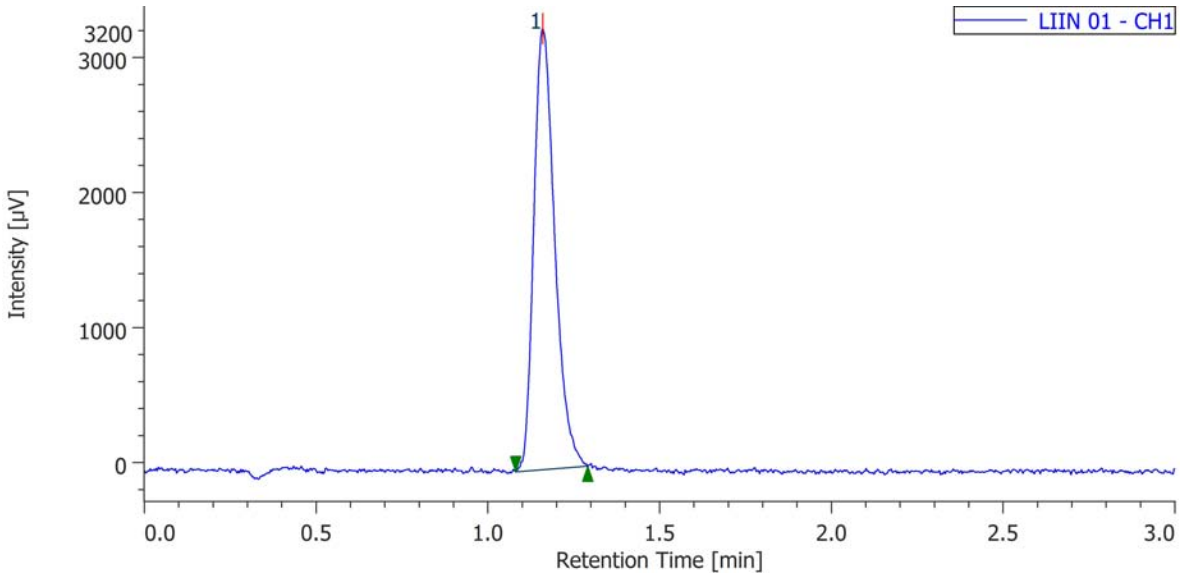

Chromatogram Information	
User Name	QPackSA
Date Modified	09-Jul-26 09:18:47
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:45:04
Volume	0.1 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 01-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina (Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.16	13854	3262	100	100.000	N/A	1782	N/A	1.326	

Creator QPackSA
Reviewer
Approver

Chromatogram

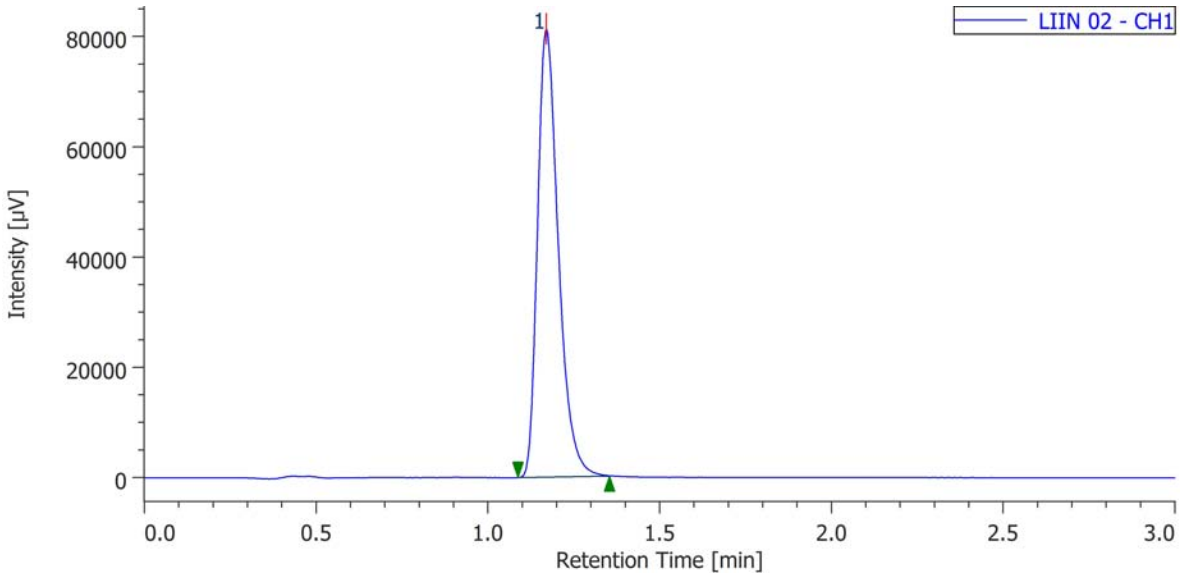

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:52:22
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:49:20
Volume	5.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 02-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.17	342022	81239	100	100.000	N/A	1868	N/A	1.367	

Creator QPackSA
Reviewer
Approver

Chromatogram

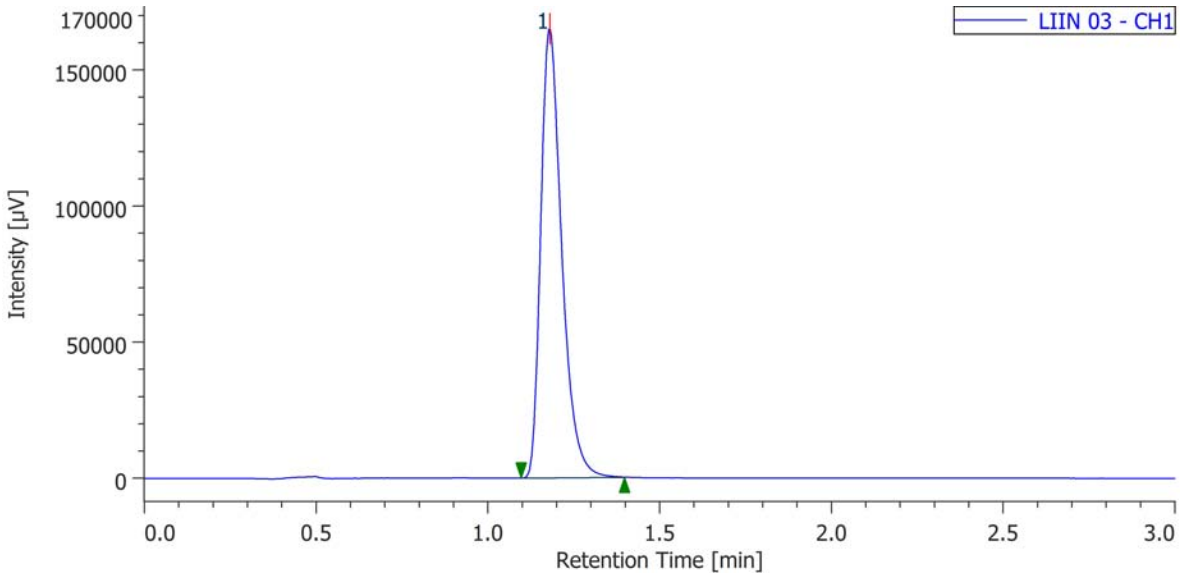

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 19:56:40
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:53:38
Volume	10.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 03-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	700629	164842	100	100.000	N/A	1884	N/A	1.376	

Creator QPackSA
Reviewer
Approver

Chromatogram

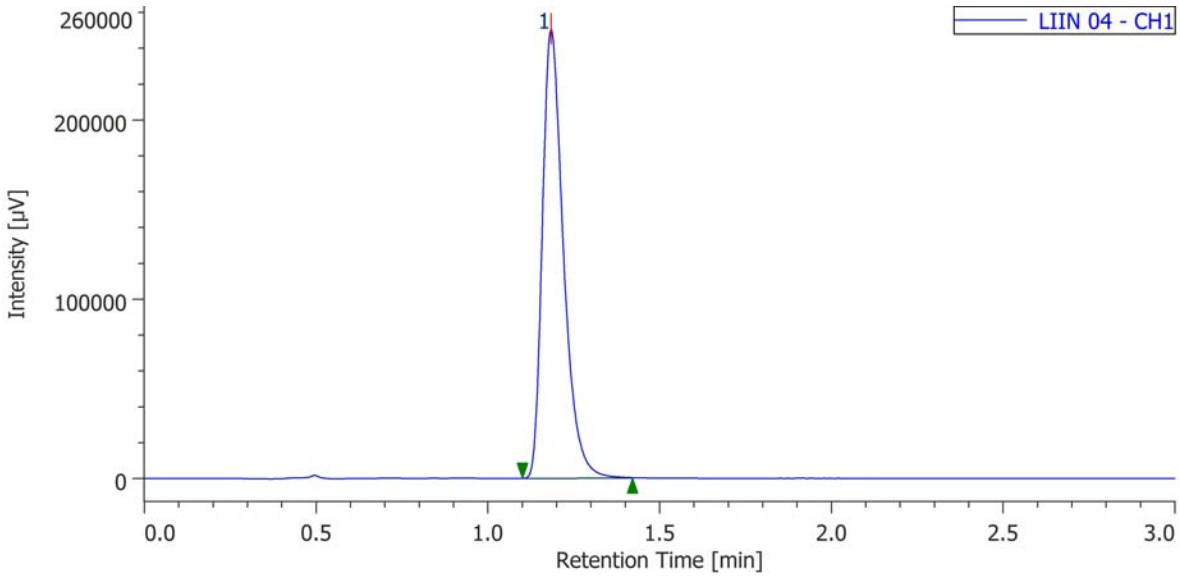

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 20:00:58
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 19:57:56
Volume	15.0 [µL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 04-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.18	1066501	250512	100	100.000	N/A	1894	N/A	1.419	

Creator QPackSA
Reviewer
Approver

Chromatogram

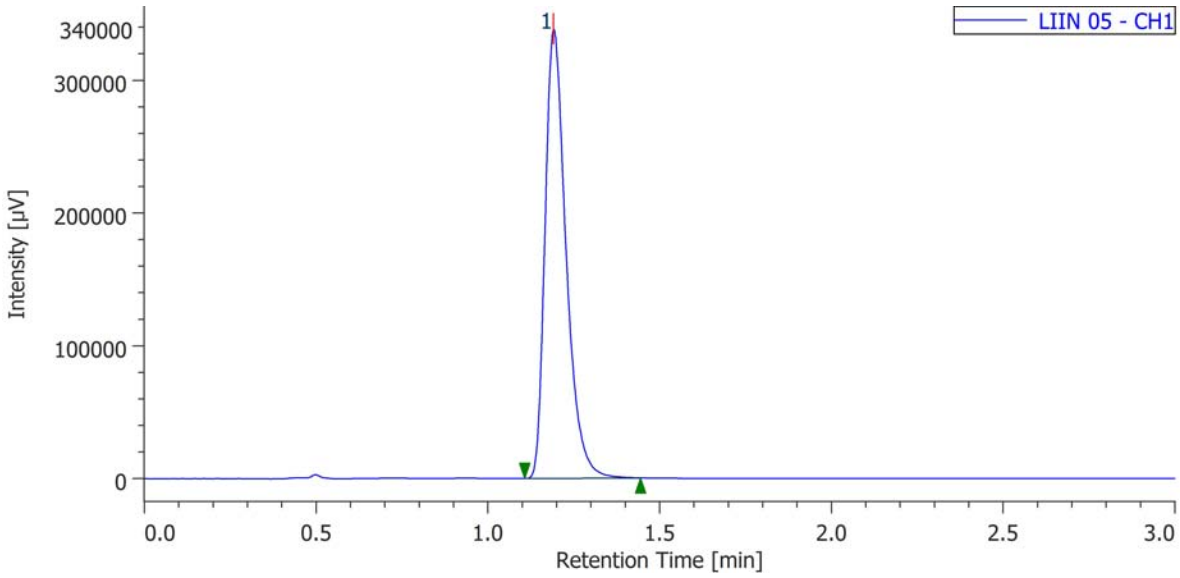

Chromatogram Information	
User Name	QPackSA
Date Modified	08-Jul-26 20:05:22
Description	
HPLC System Name	HPLC-0005
Injection Date	08-Jul-26 20:02:20
Volume	20.0 [μL]
Sample #	10
Project Name	QPACKSA
Acquisition Time	3.0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Cafeina
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN 05-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	Cafeina

#	Peak Name	CH	tR [min]	Area [μV·sec]	Height [μV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeina	1	1.19	1435814	338350	100	100.000	N/A	1932	N/A	1.453	

Creator QPackSA
Reviewer
Approver

Chromatogram

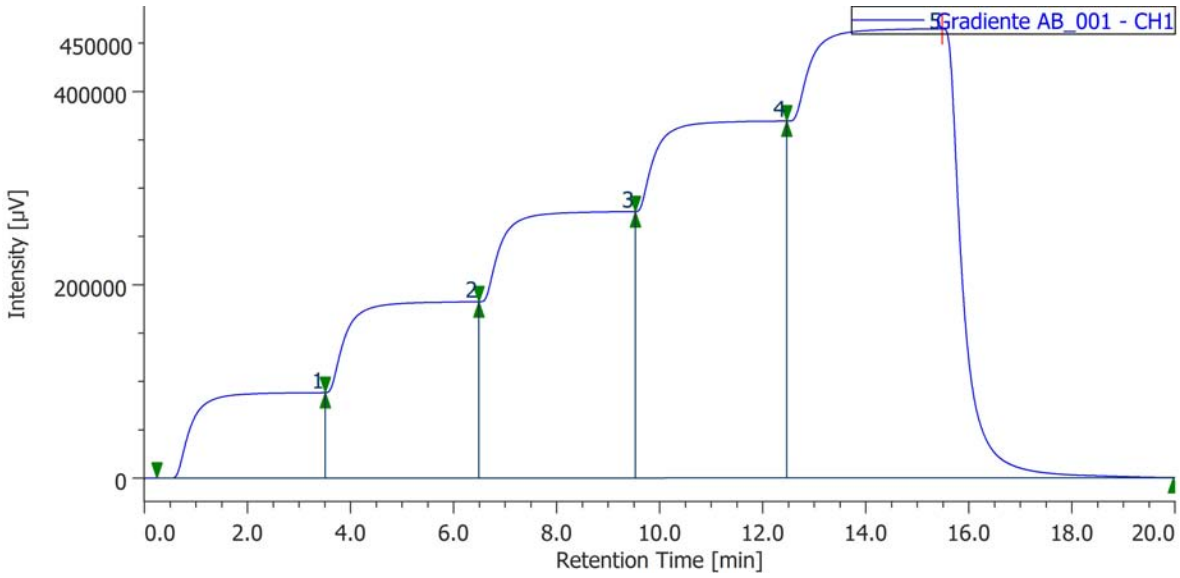

Chromatogram Information	
User Name	QPackSA
Date Modified	09-Jul-26 10:19:42
Description	
HPLC System Name	HPLC-0005
Injection Date	09-Jul-26 09:48:43
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente AB
Peak ID Table	Gradiente
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Gradiente AB_001-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.50	13704053	88431	5.51	6.412	N/A	N/A	N/A	N/A	
2	40%	1	6.48	30286910	182307	12.2	13.218	N/A	N/A	N/A	N/A	
3	60%	1	9.52	47723812	275349	19.2	19.964	N/A	N/A	N/A	N/A	
4	80%	1	12.5	62856214	368998	25.3	26.754	N/A	N/A	N/A	N/A	
5	100%	1	15.5	93973838	464145	37.8	33.652	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver

Chromatogram

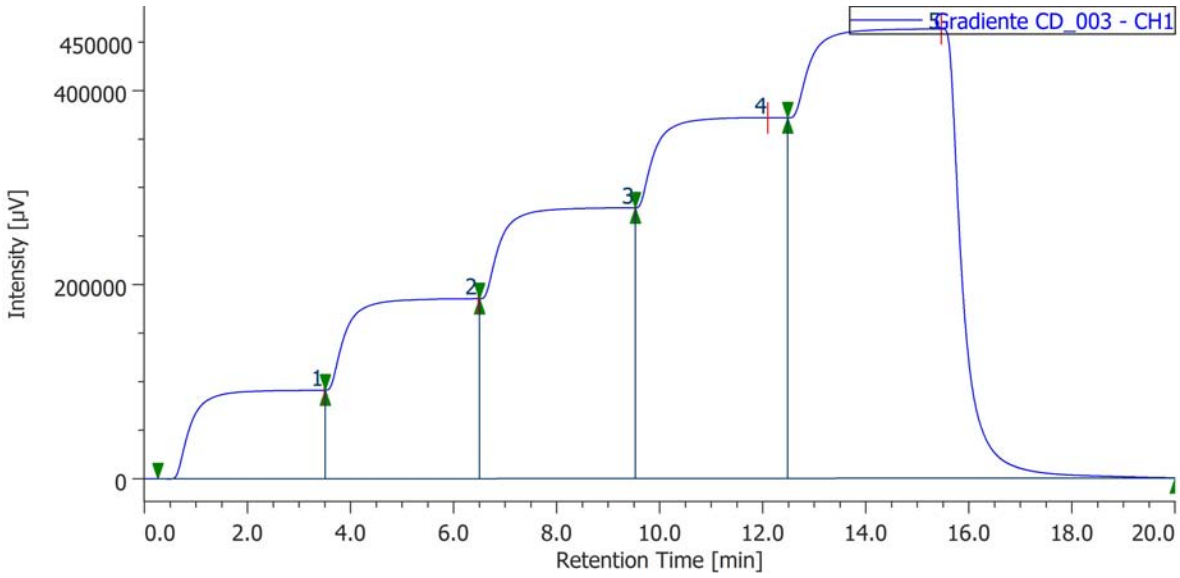

Chromatogram Information	
User Name	QPackSA
Date Modified	09-Jul-26 10:38:16
Description	
HPLC System Name	HPLC-0005
Injection Date	09-Jul-26 10:15:57
Volume	0.0 [µL]
Sample #	-
Project Name	QPACKSA
Acquisition Time	20.0 [min]
Acquisition Sequence	
Control Method	Gradiente CD
Peak ID Table	Gradiente
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Gradiente CD_003-CH1
Sample Name	
Channel Name	CH1
Sampling Interval	200 [msec]
Peak Method	(Manual)

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	20%	1	3.49	14155874	91225	5.65	6.570	N/A	N/A	N/A	N/A	
2	40%	1	6.47	30993659	185168	12.4	13.335	N/A	N/A	N/A	N/A	
3	60%	1	9.52	48147549	278442	19.2	20.053	N/A	N/A	N/A	N/A	
4	80%	1	12.1	63764801	371216	25.5	26.734	N/A	N/A	N/A	N/A	
5	100%	1	15.5	93269995	462505	37.3	33.308	N/A	N/A	N/A	N/A	

Creator QPackSA
Reviewer
Approver