
Peak Find - EDFL 1.jws

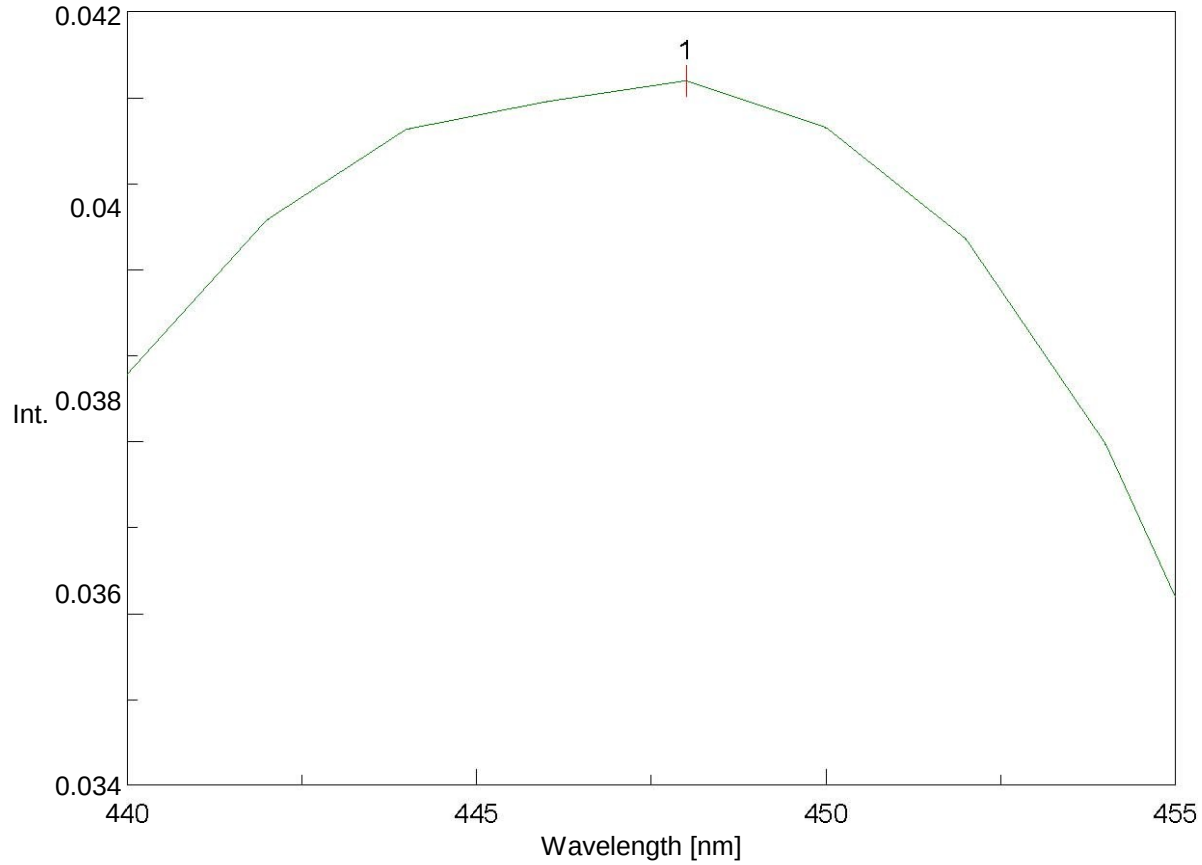

[Comments]

User	QPackSA
Division	---
Company	Valer Laboratórios
Creation date	06/09/2022 10:57
Date modified	06/09/2022 11:03

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Int.
Start	360 nm
End	700 nm
Data interval	4 nm
Data points	86


[Measurement Information]

Instrument Name	FP-4020
Model Name	FP-4020
Serial No.	A009561653
ROM version	1.01.05
Measurement mode	Emission
Ex Wavelength	350 nm

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	448	0.041938			

Chromatogram

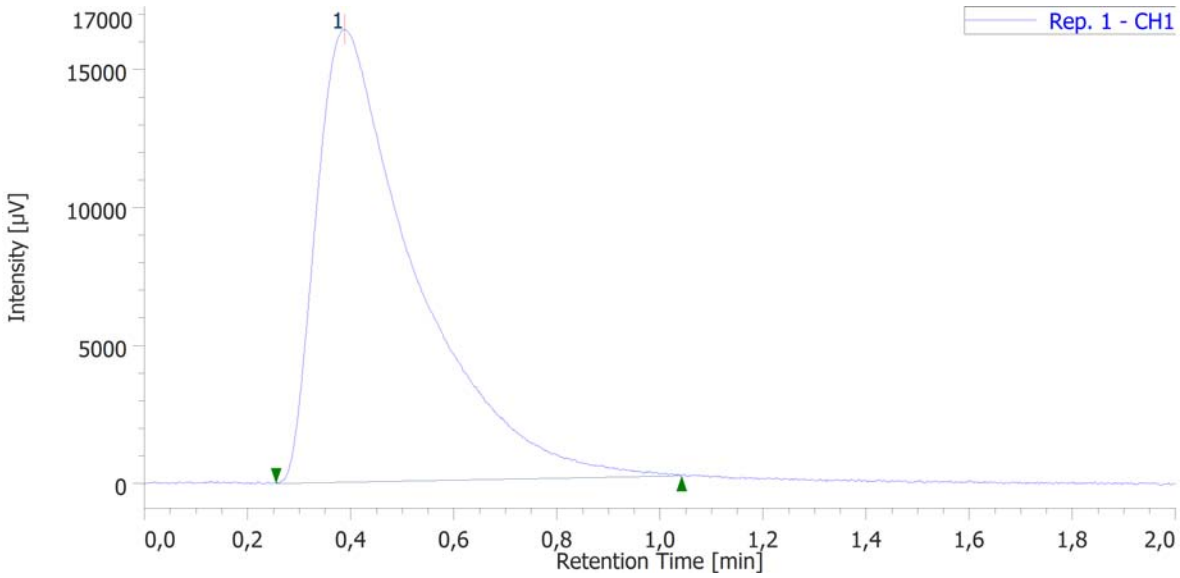

Chromatogram Information	
User Name	QPackSA
Date Modified	06/09/2022 12:39:36
Description	
HPLC System Name	HPL24UV_FL
Injection Date	06/09/2022 12:22:52
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Rep. FL
Control Method	Qualificação FL
Peak ID Table	FL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Rep. 1-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD FL	1	0,388	219116	16407	100,000	100,000	N/A	24	N/A	2,503	

Creator QPackSA
Reviewer
Approver

Chromatogram

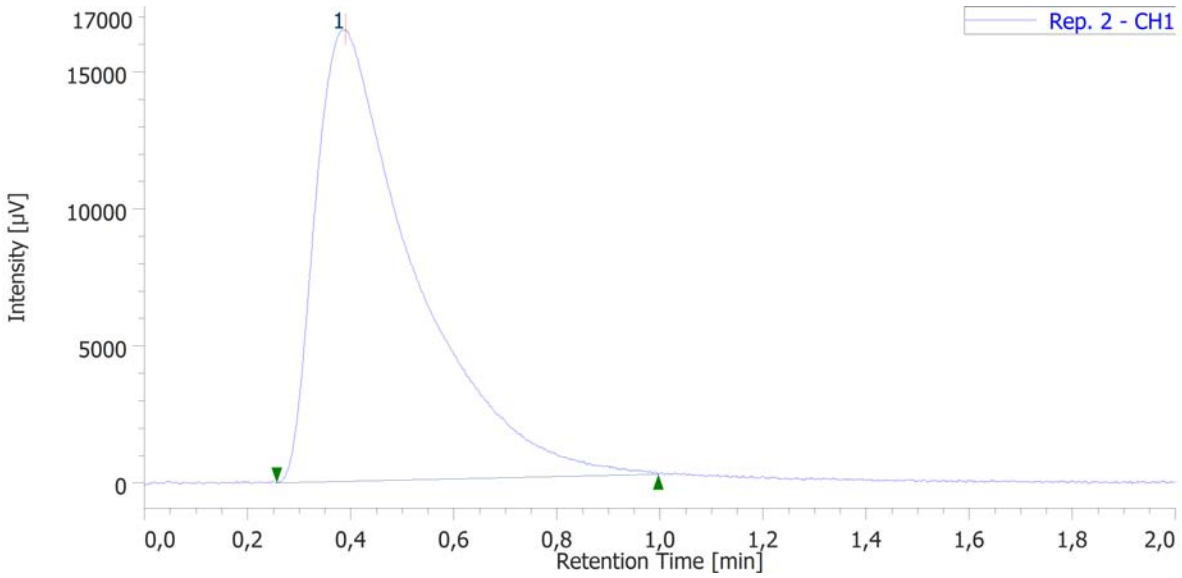

Chromatogram Information	
User Name	QPackSA
Date Modified	06/09/2022 12:39:37
Description	
HPLC System Name	HPL24UV_FL
Injection Date	06/09/2022 12:26:07
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Rep. FL
Control Method	Qualificação FL
Peak ID Table	FL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Rep. 2-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD FL	1	0,390	220048	16490	100,000	100,000	N/A	24	N/A	2,411	

Creator QPackSA
Reviewer
Approver

Chromatogram

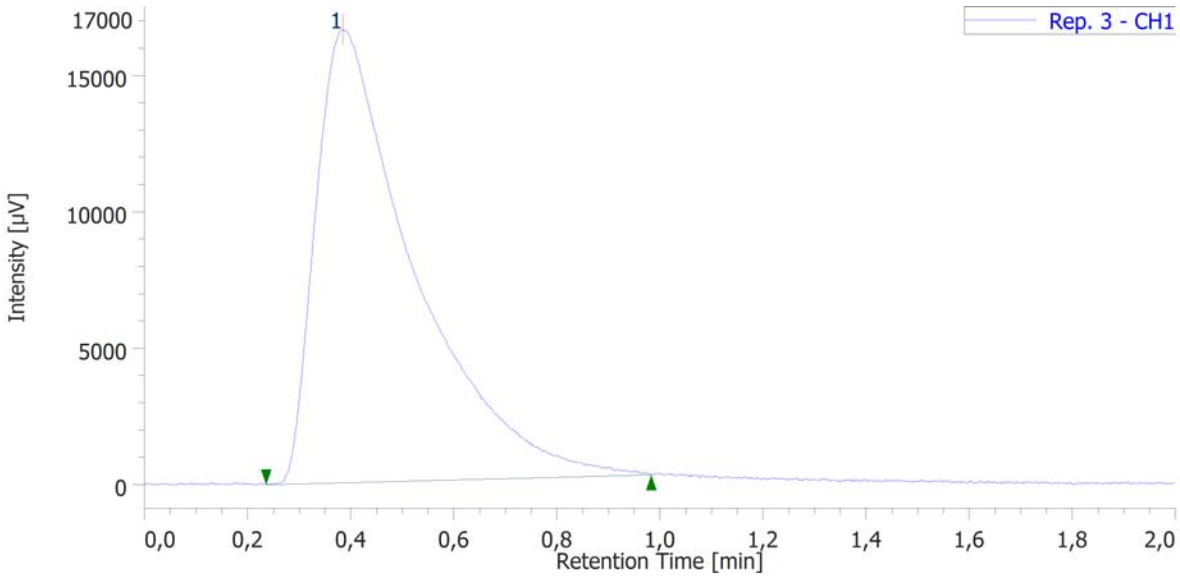

Chromatogram Information	
User Name	QPackSA
Date Modified	06/09/2022 12:39:37
Description	
HPLC System Name	HPL24UV_FL
Injection Date	06/09/2022 12:29:21
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Rep. FL
Control Method	Qualificação FL
Peak ID Table	FL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Rep. 3-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD FL	1	0,385	220481	16619	100,000	100,000	N/A	24	N/A	2,495	

Creator QPackSA
Reviewer
Approver

Chromatogram

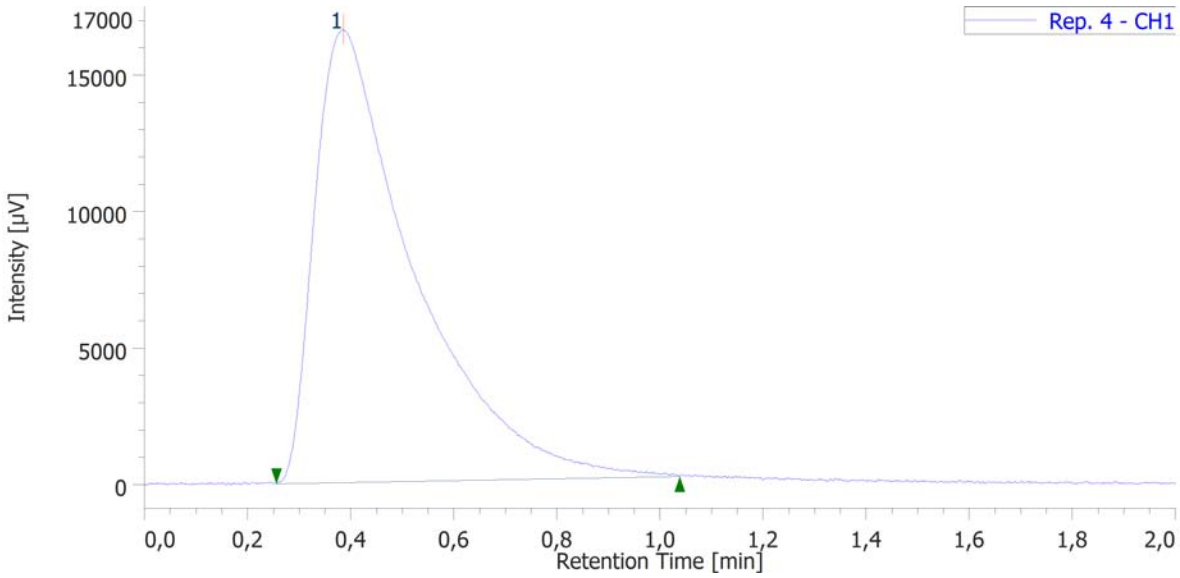

Chromatogram Information	
User Name	QPackSA
Date Modified	06/09/2022 12:39:37
Description	
HPLC System Name	HPL24UV_FL
Injection Date	06/09/2022 12:32:36
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Rep. FL
Control Method	Qualificação FL
Peak ID Table	FL
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	Rep. 4-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD FL	1	0,385	222423	16589	100,000	100,000	N/A	23	N/A	2,492	

Creator QPackSA
Reviewer
Approver

Chromatogram

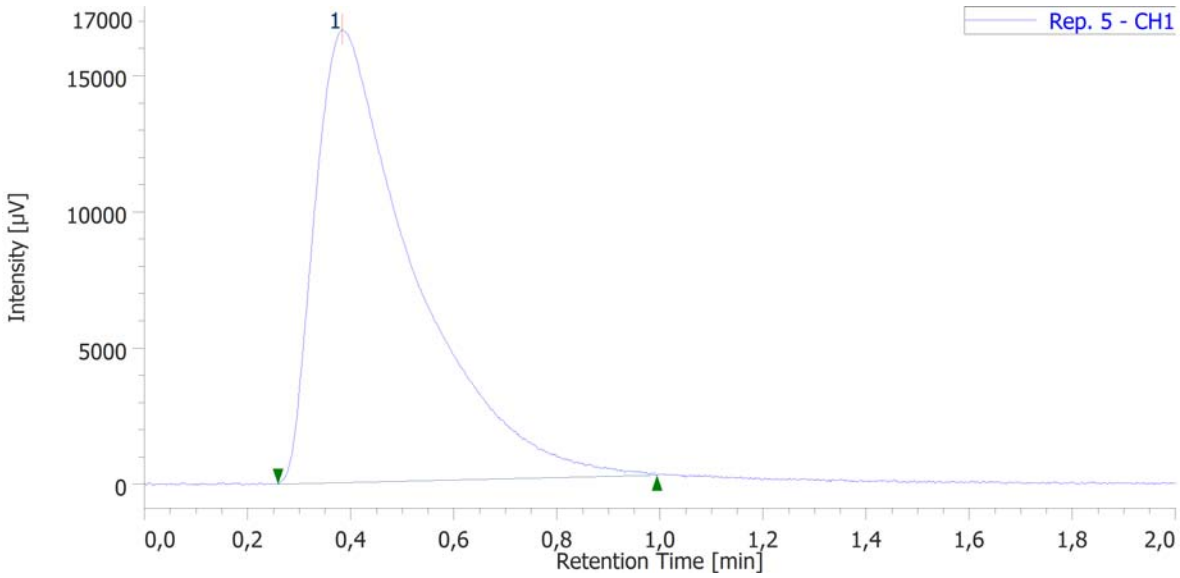

Chromatogram Information	
User Name	QPackSA
Date Modified	06/09/2022 12:39:38
Description	
HPLC System Name	HPL24UV_FL
Injection Date	06/09/2022 12:35:50
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	2,0 [min]
Acquisition Sequence	Rep. FL
Control Method	Qualificação FL
Peak ID Table	FL
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Rep. 5-CH1
Sample Name	
Channel Name	UV
Sampling Interval	40 [msec]
Peak Method	Qualificação

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	PD FL	1	0,383	221400	16636	100,000	100,000	N/A	23	N/A	2,559	

Creator QPackSA
Reviewer
Approver