
Peak Find - EDUV PDA_1,3733.JWS

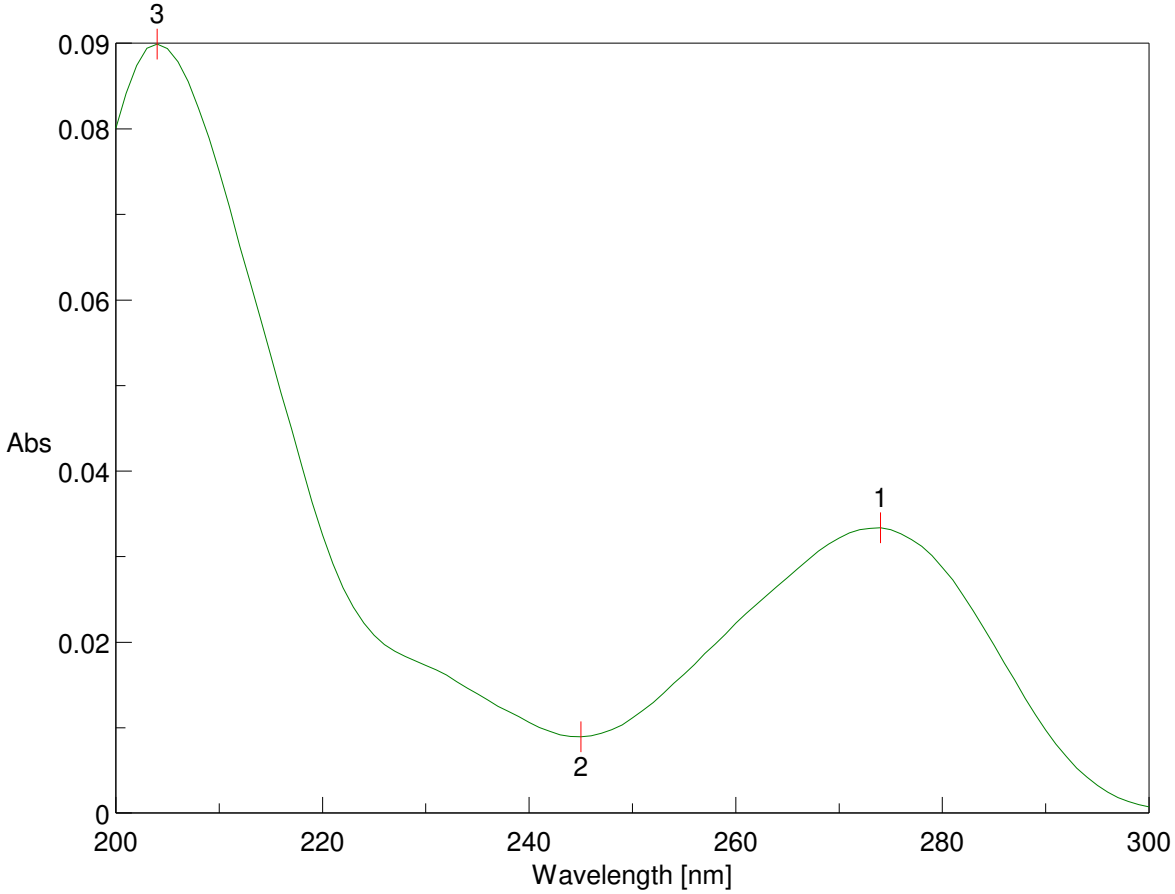

[Comments]

User	QPackSA
Division	---
Company	Valer
Creation date	13/10/2022 16:31

[Detailed Information]

Data array type	Linear data array
Horizontal axis	Wavelength [nm]
Vertical axis	Abs
Start	200 nm
End	300 nm
Data interval	1 nm
Data points	101


[Measurement Information]

Instrument Name	MD-2010
Model Name	MD-2010
Serial No.	072260870
ROM version	V2.36

[Result of Peak Picking]

No.	Position	Intensity	No.	Position	Intensity
1	274	0.033339	2	245	0.008895
3	204	0.089875			

Chromatogram

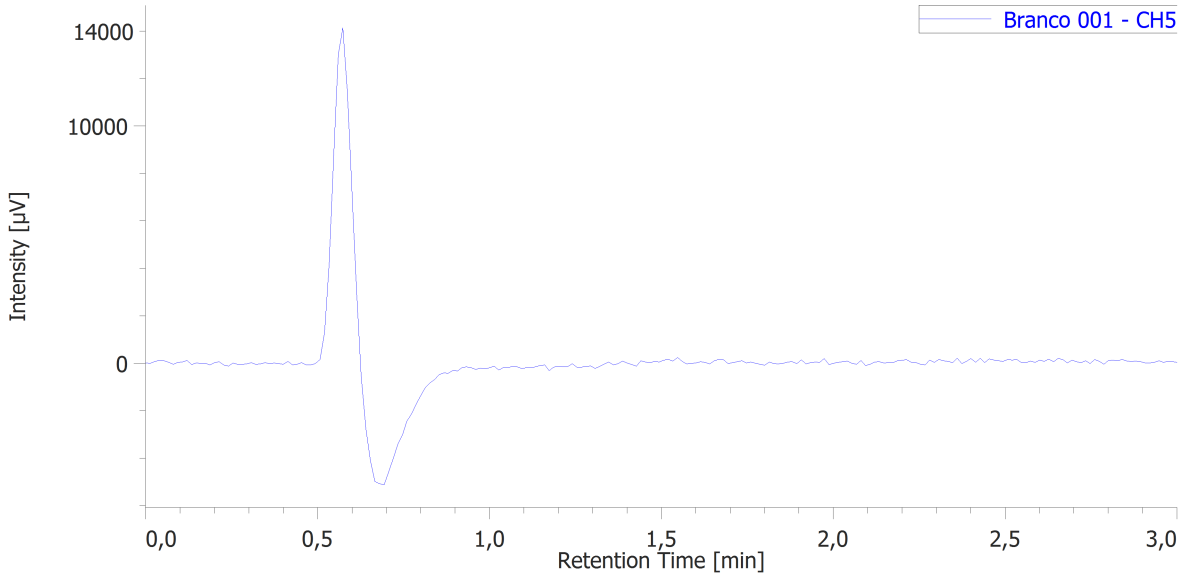


Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:12:33
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:09:31
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

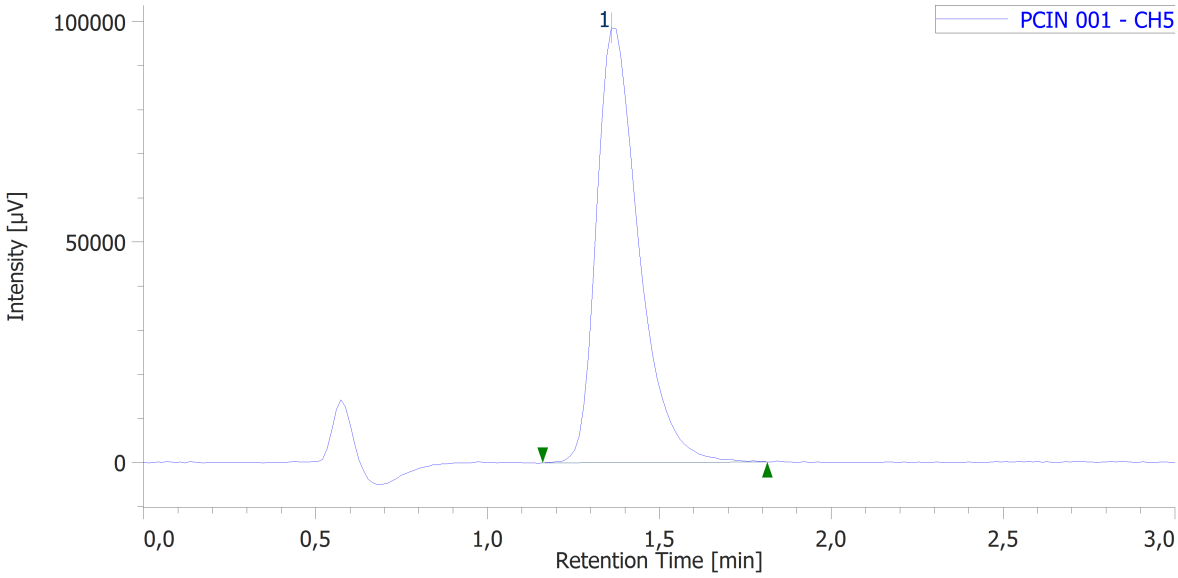

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:16:23
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:13:21
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 001-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,360	846906	98603	100,000	100,000	N/A	629	N/A	1,536	

Creator QPackSA
Reviewer
Approver

Chromatogram

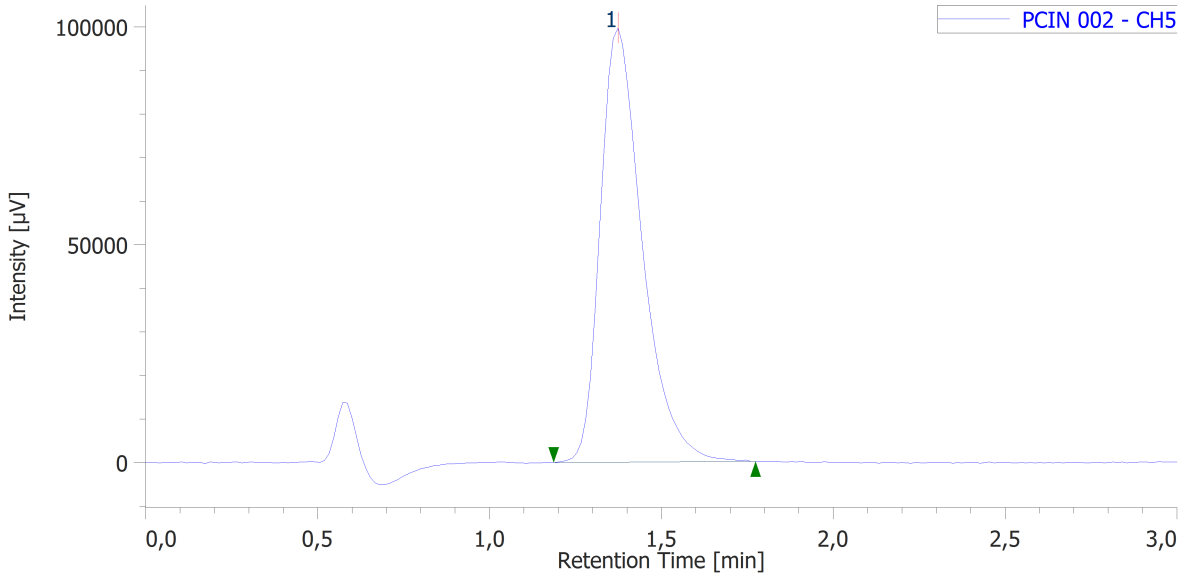

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:20:15
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:17:14
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	846832	99610	100,000	100,000	N/A	646	N/A	1,421	

Creator QPackSA
Reviewer
Approver

Chromatogram

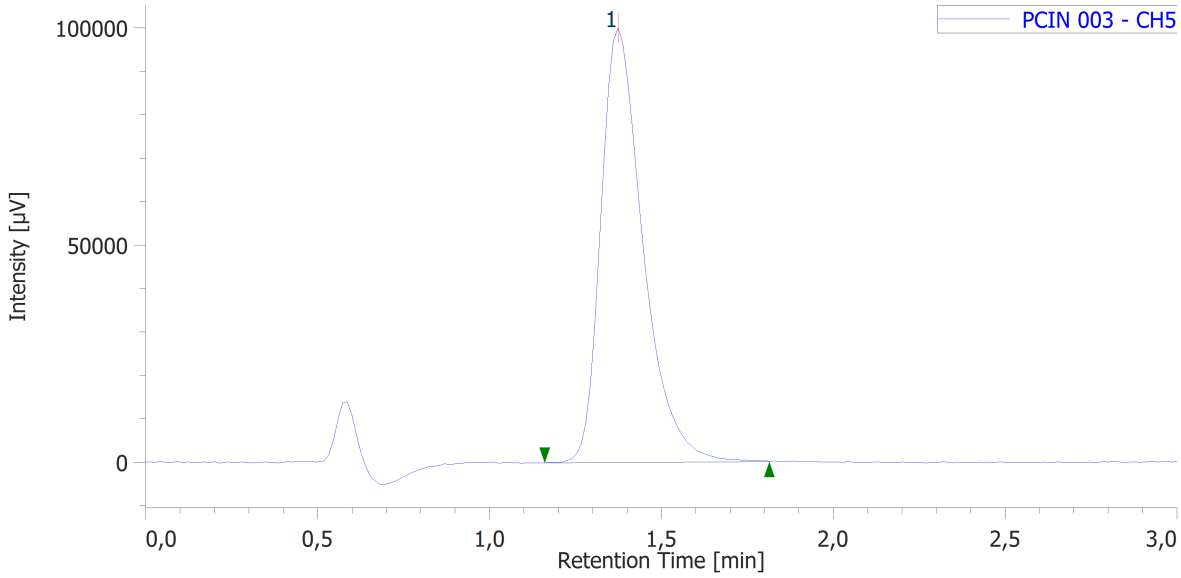

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:24:05
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:21:03
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	854399	100003	100,000	100,000	N/A	644	N/A	1,443	

Creator QPackSA
Reviewer
Approver

Chromatogram

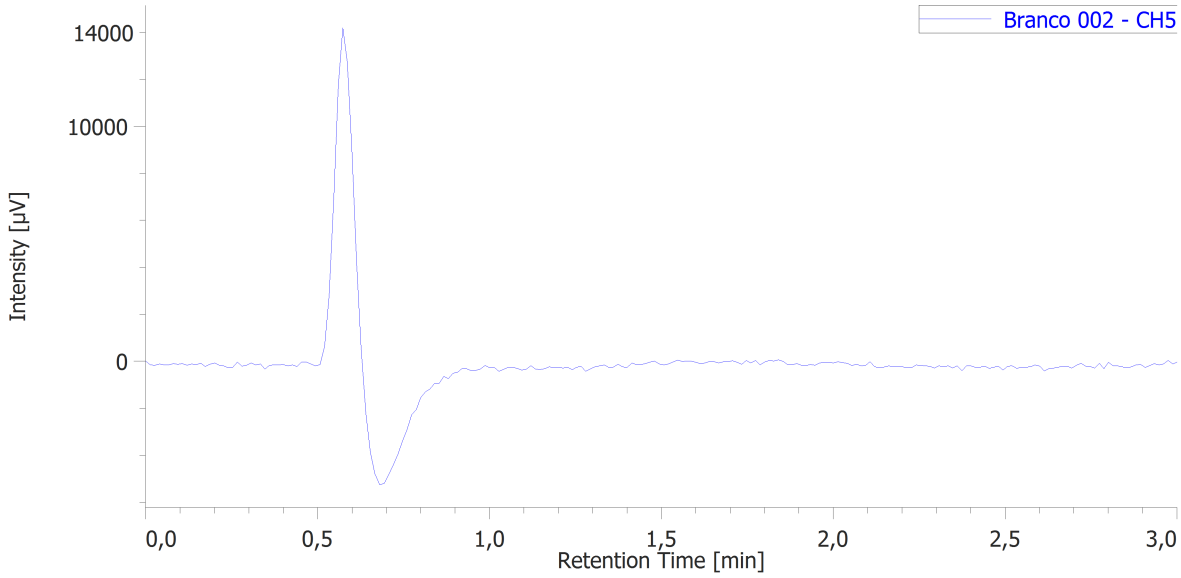


Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:27:53
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:24:51
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 002-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

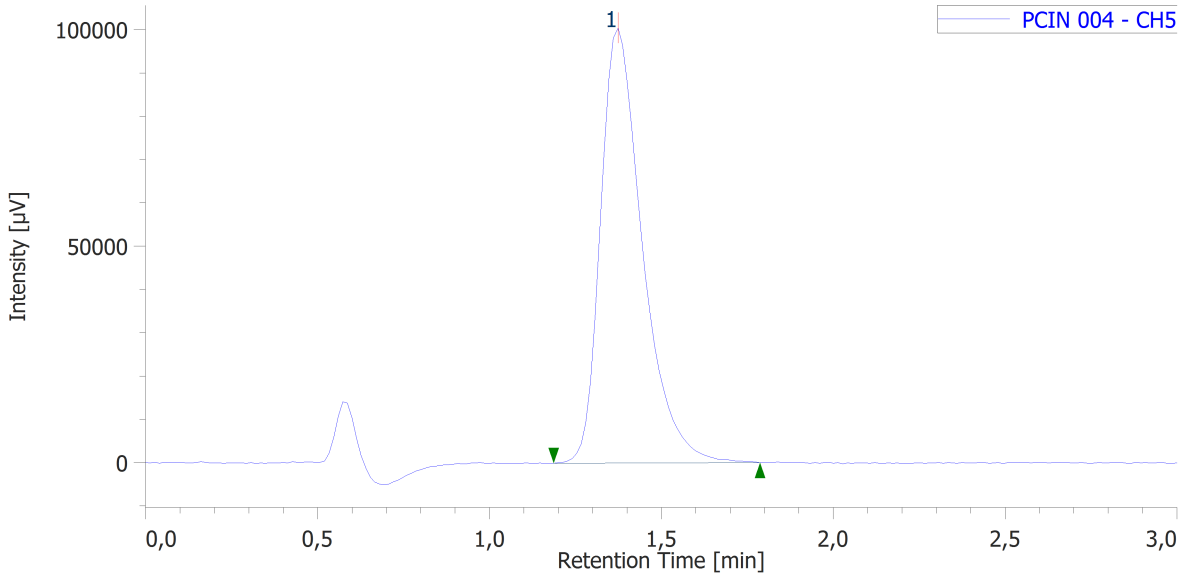

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:31:43
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:28:41
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 004-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	850549	100423	100,000	100,000	N/A	656	N/A	1,435	

Creator QPackSA
Reviewer
Approver

Chromatogram

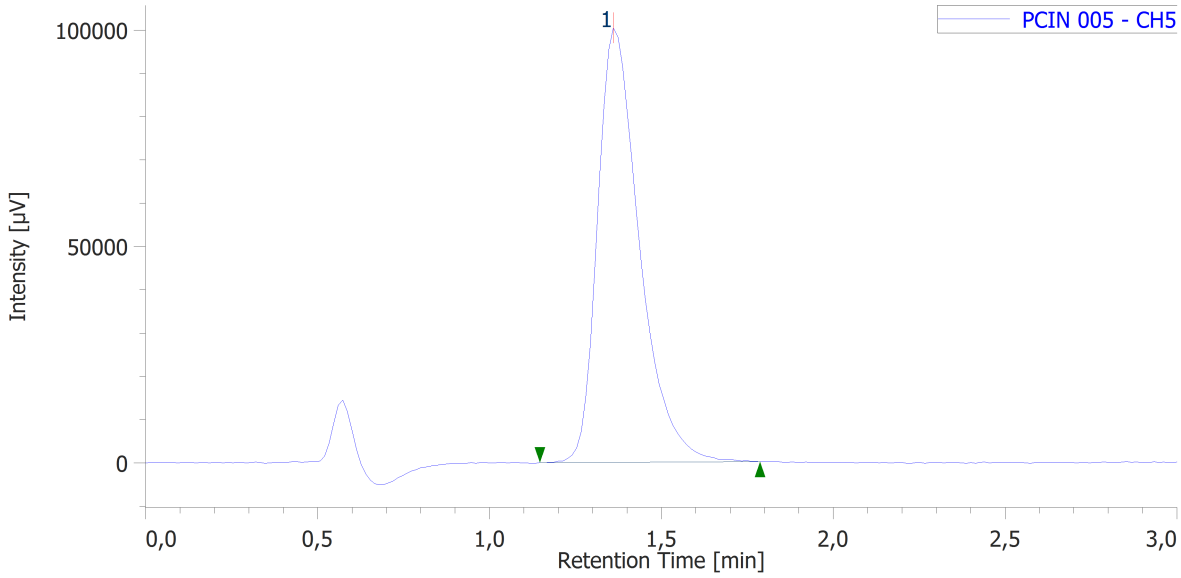

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:35:35
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:32:33
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 005-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,360	850731	100254	100,000	100,000	N/A	640	N/A	1,501	

Creator QPackSA
Reviewer
Approver

Chromatogram

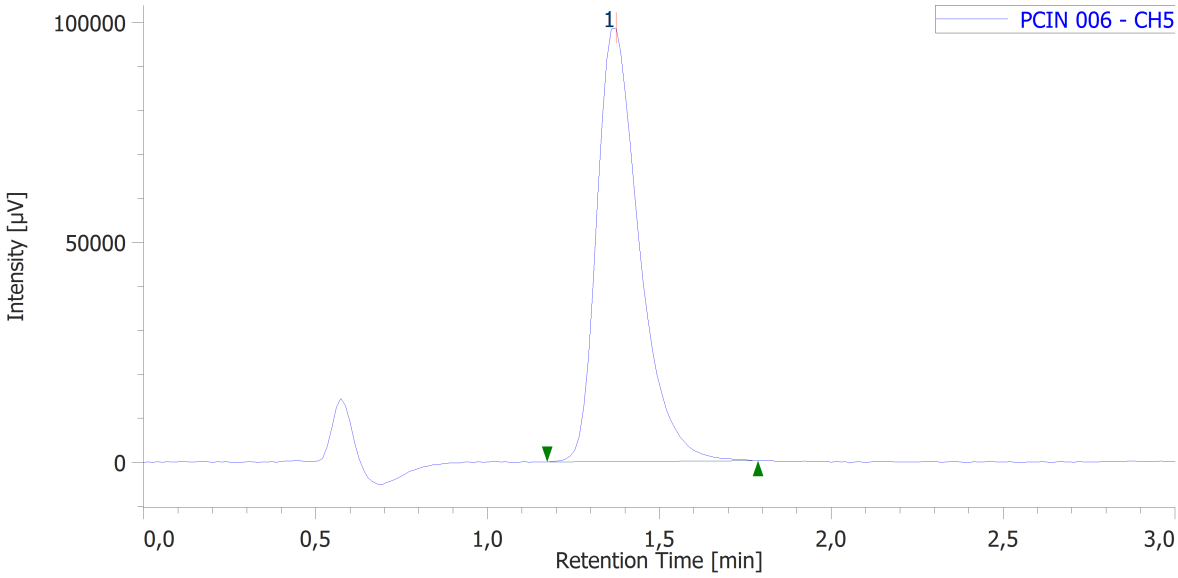

Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:39:27
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:36:25
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	PCIN 006-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	847286	98536	100,000	100,000	N/A	635	N/A	1,374	

Creator QPackSA
Reviewer
Approver

Chromatogram

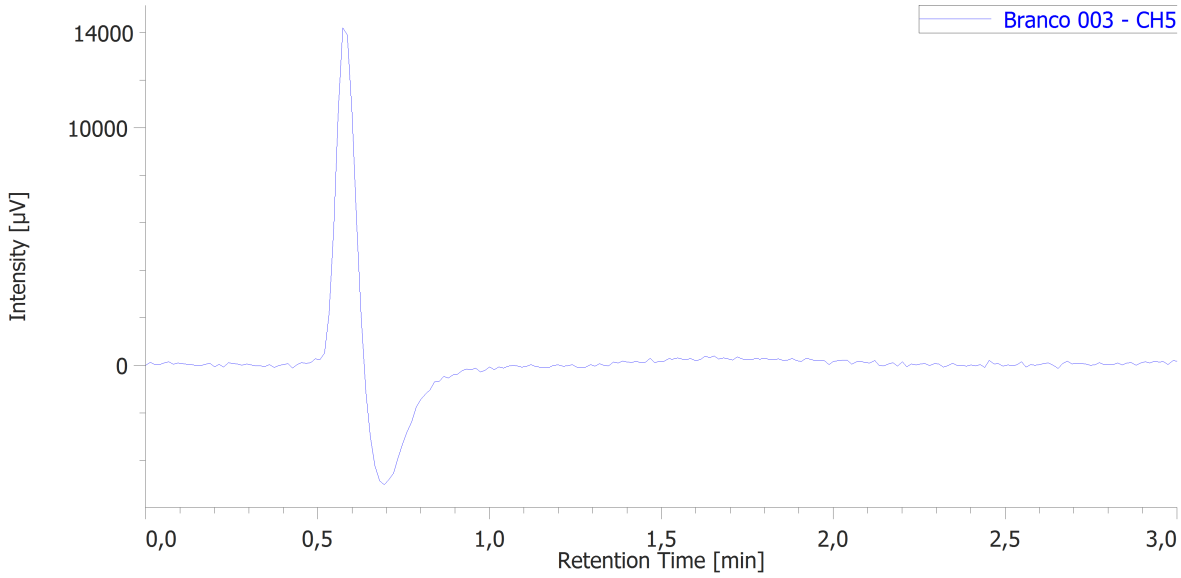


Chromatogram Information	
User Name	QPackSA
Date Modified	13/10/2022 17:43:13
Description	
HPLC System Name	HPL 25
Injection Date	13/10/2022 17:40:10
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	Branco 003-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

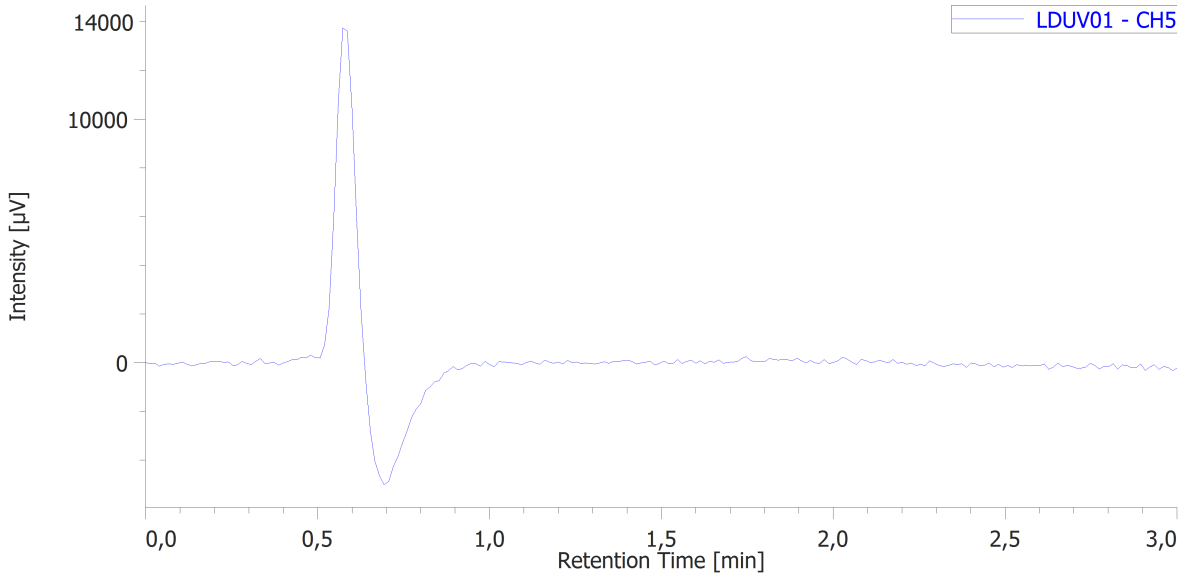


Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 08:59:51
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 08:56:49
Volume	10,0 [µL]
Sample #	1
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LDUV01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

Creator QPackSA
Reviewer
Approver

Chromatogram

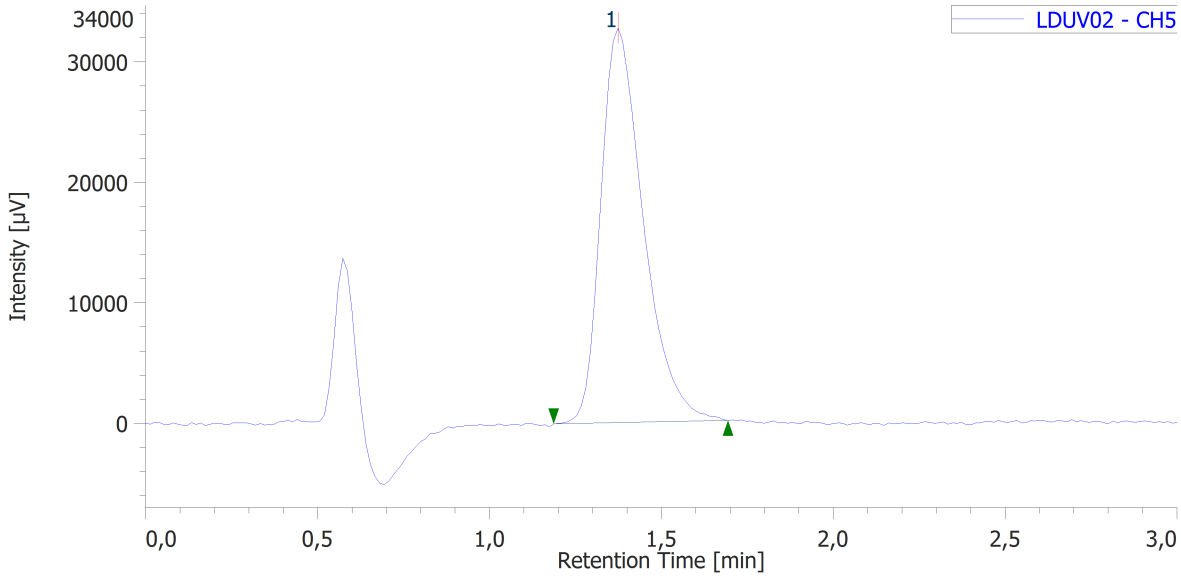

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:03:39
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:00:36
Volume	10,0 [µL]
Sample #	2
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	281254	32735	100,000	100,000	N/A	622	N/A	1,445	

Creator QPackSA
Reviewer
Approver

Chromatogram

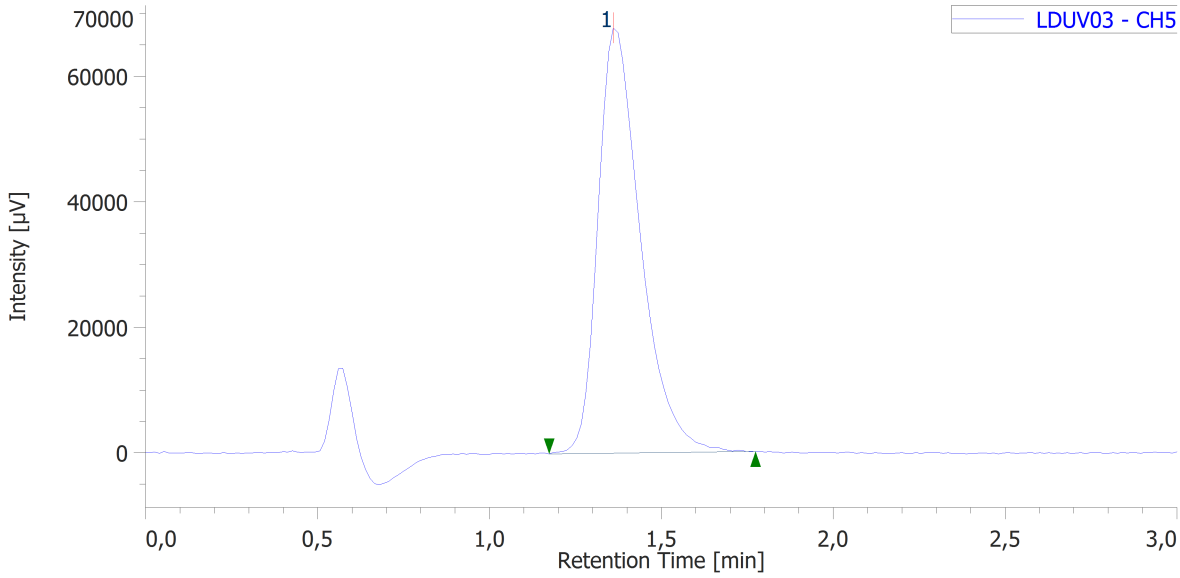

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:07:27
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:04:24
Volume	10,0 [µL]
Sample #	3
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,360	582622	67706	100,000	100,000	N/A	621	N/A	1,506	

Creator QPackSA
Reviewer
Approver

Chromatogram

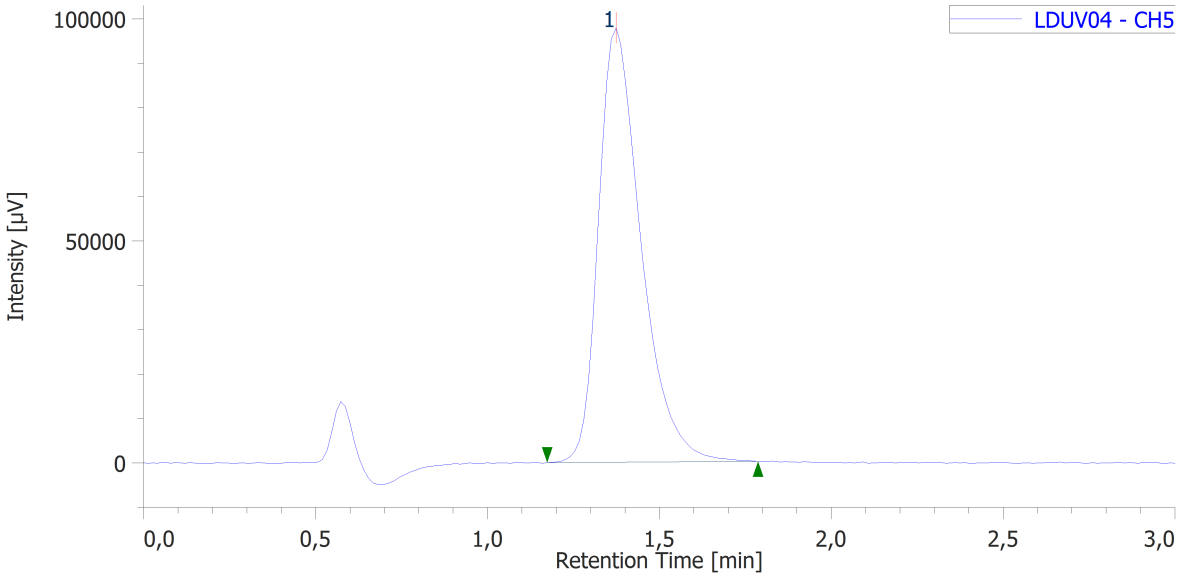

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:11:15
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:08:12
Volume	10,0 [µL]
Sample #	4
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	840011	97740	100,000	100,000	N/A	631	N/A	1,431	

Creator QPackSA
Reviewer
Approver

Chromatogram

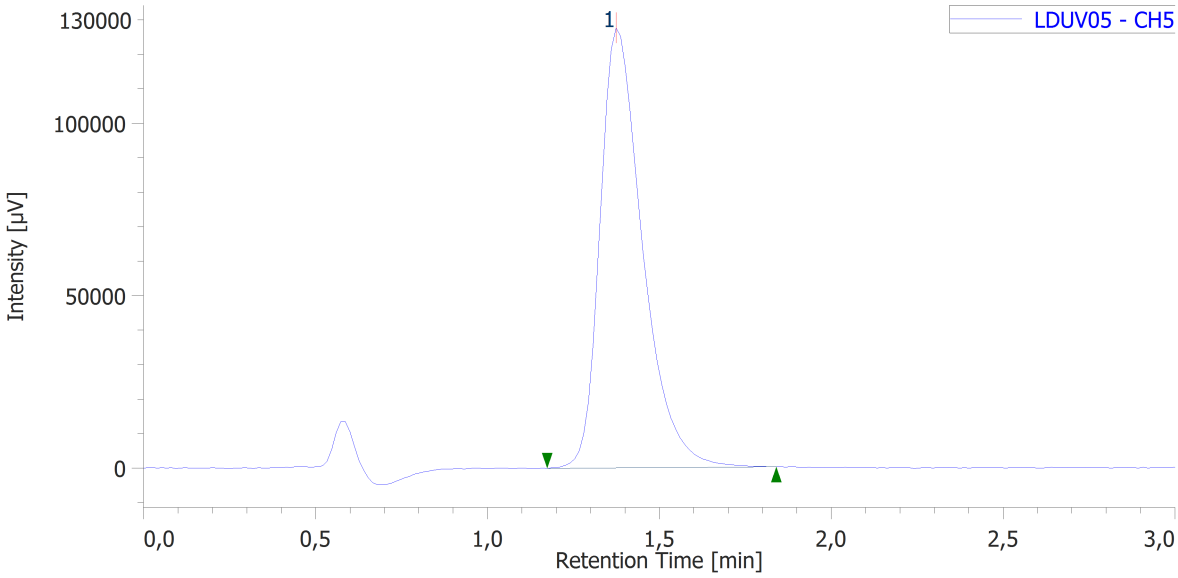

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:15:03
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:12:01
Volume	10,0 [µL]
Sample #	5
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LDUV05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	1097958	127526	100,000	100,000	N/A	634	N/A	1,486	

Creator QPackSA
Reviewer
Approver

Chromatogram

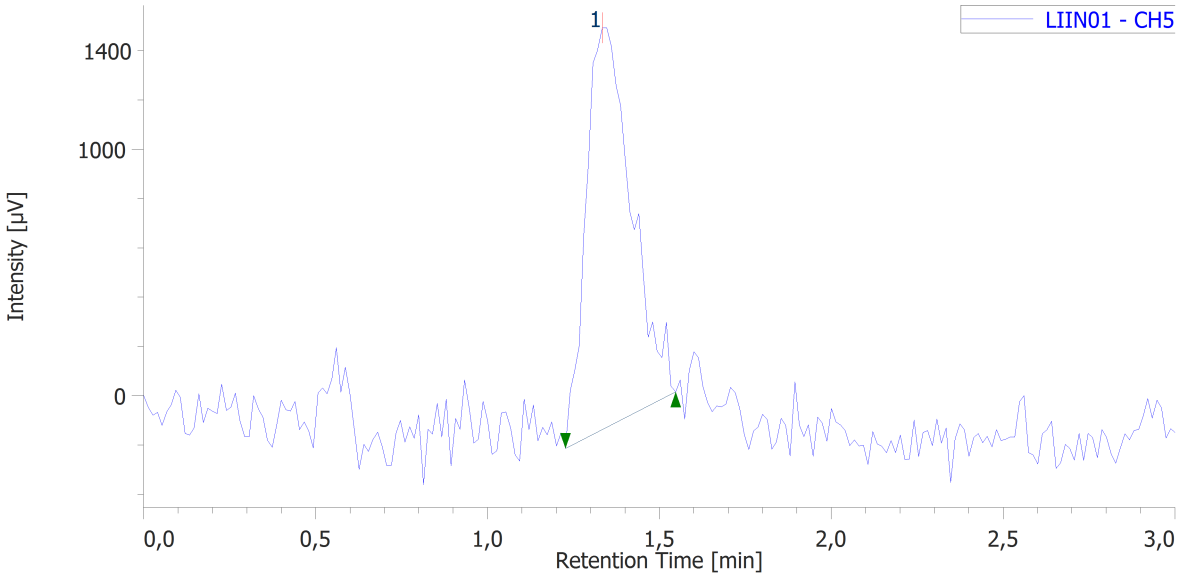

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:18:51
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:15:49
Volume	0,1 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN01-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,333	14886	1628	100,000	100,000	N/A	538	N/A	1,470	

Creator QPackSA
Reviewer
Approver

Chromatogram

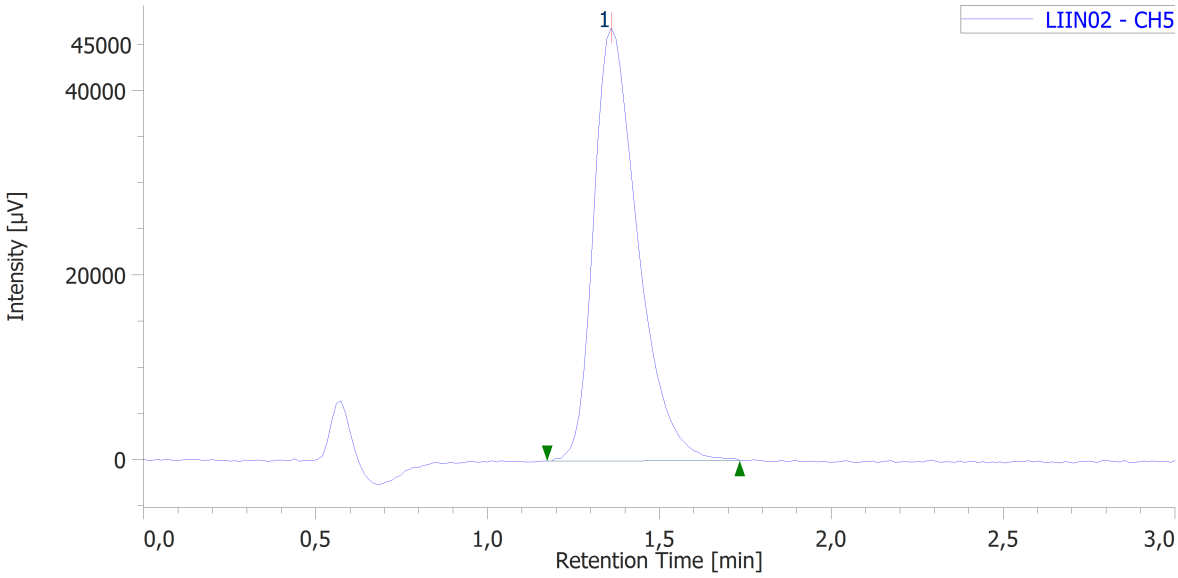

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:22:41
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:19:39
Volume	5,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN02-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,360	420414	46947	100,000	100,000	N/A	567	N/A	1,424	

Creator QPackSA
Reviewer
Approver

Chromatogram

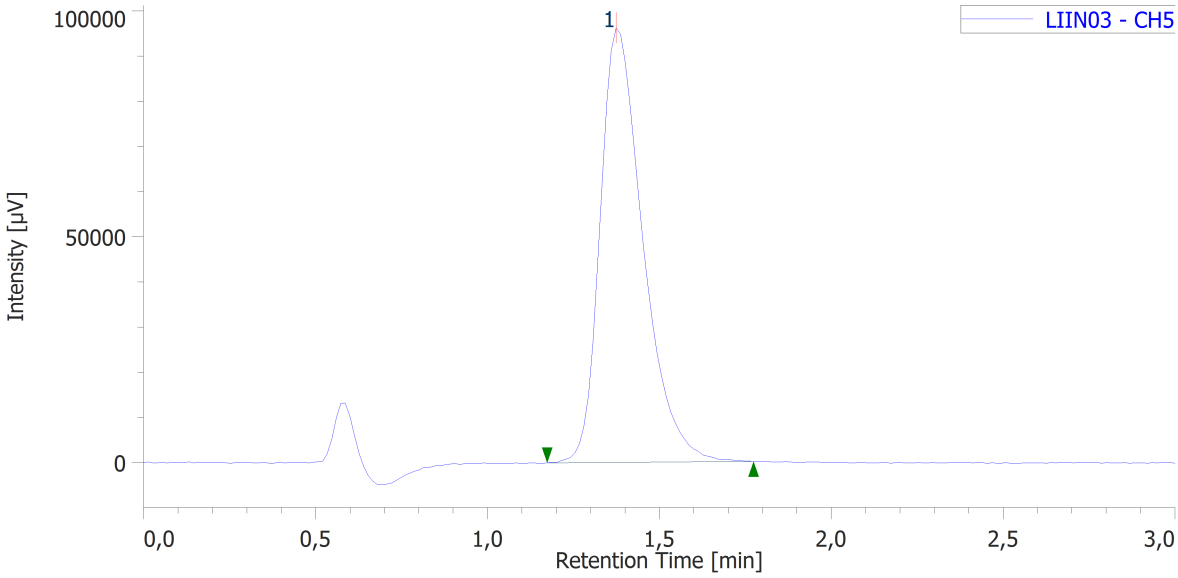

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:26:30
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:23:29
Volume	10,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN03-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,373	833558	96109	100,000	100,000	N/A	618	N/A	1,472	

Creator QPackSA
Reviewer
Approver

Chromatogram

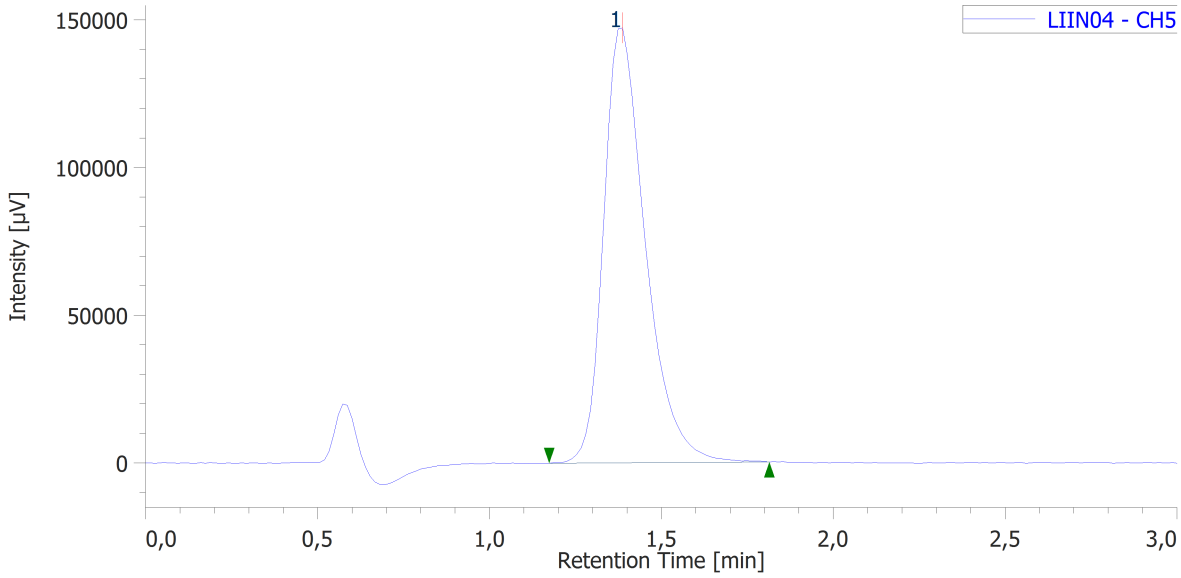

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:30:23
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:27:21
Volume	15,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	


Channel & Peak Information Table

Chromatogram Name	LIIN04-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,387	1243851	147151	100,000	100,000	N/A	672	N/A	1,318	

Creator QPackSA
Reviewer
Approver

Chromatogram

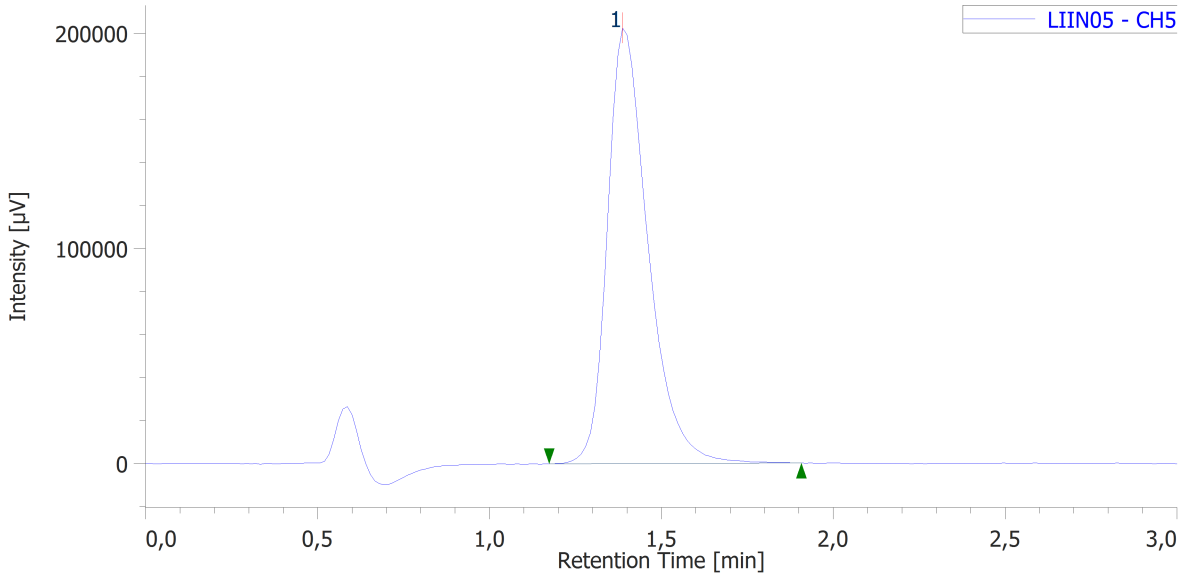

Chromatogram Information	
User Name	QPackSA
Date Modified	14/10/2022 09:34:18
Description	
HPLC System Name	HPL 25
Injection Date	14/10/2022 09:31:15
Volume	20,0 [µL]
Sample #	6
Project Name	Qualificação
Acquisition Time	3,0 [min]
Acquisition Sequence	Qualificação
Control Method	Qualificação
Peak ID Table	Peak
Calibration Method	
Additional Information	

Channel & Peak Information Table

Chromatogram Name	LIIN05-CH5
Sample Name	
Channel Name	273,0nm
Sampling Interval	800 [msec]
Peak Method	Peak

#	Peak Name	CH	tR [min]	Area [µV·sec]	Height [µV]	Area%	Height%	Quantity	NTP	Resolution	Symmetry Factor	Warning
1	Cafeína	5	1,387	1666382	202476	100,000	100,000	N/A	714	N/A	1,434	

Creator QPackSA
Reviewer
Approver