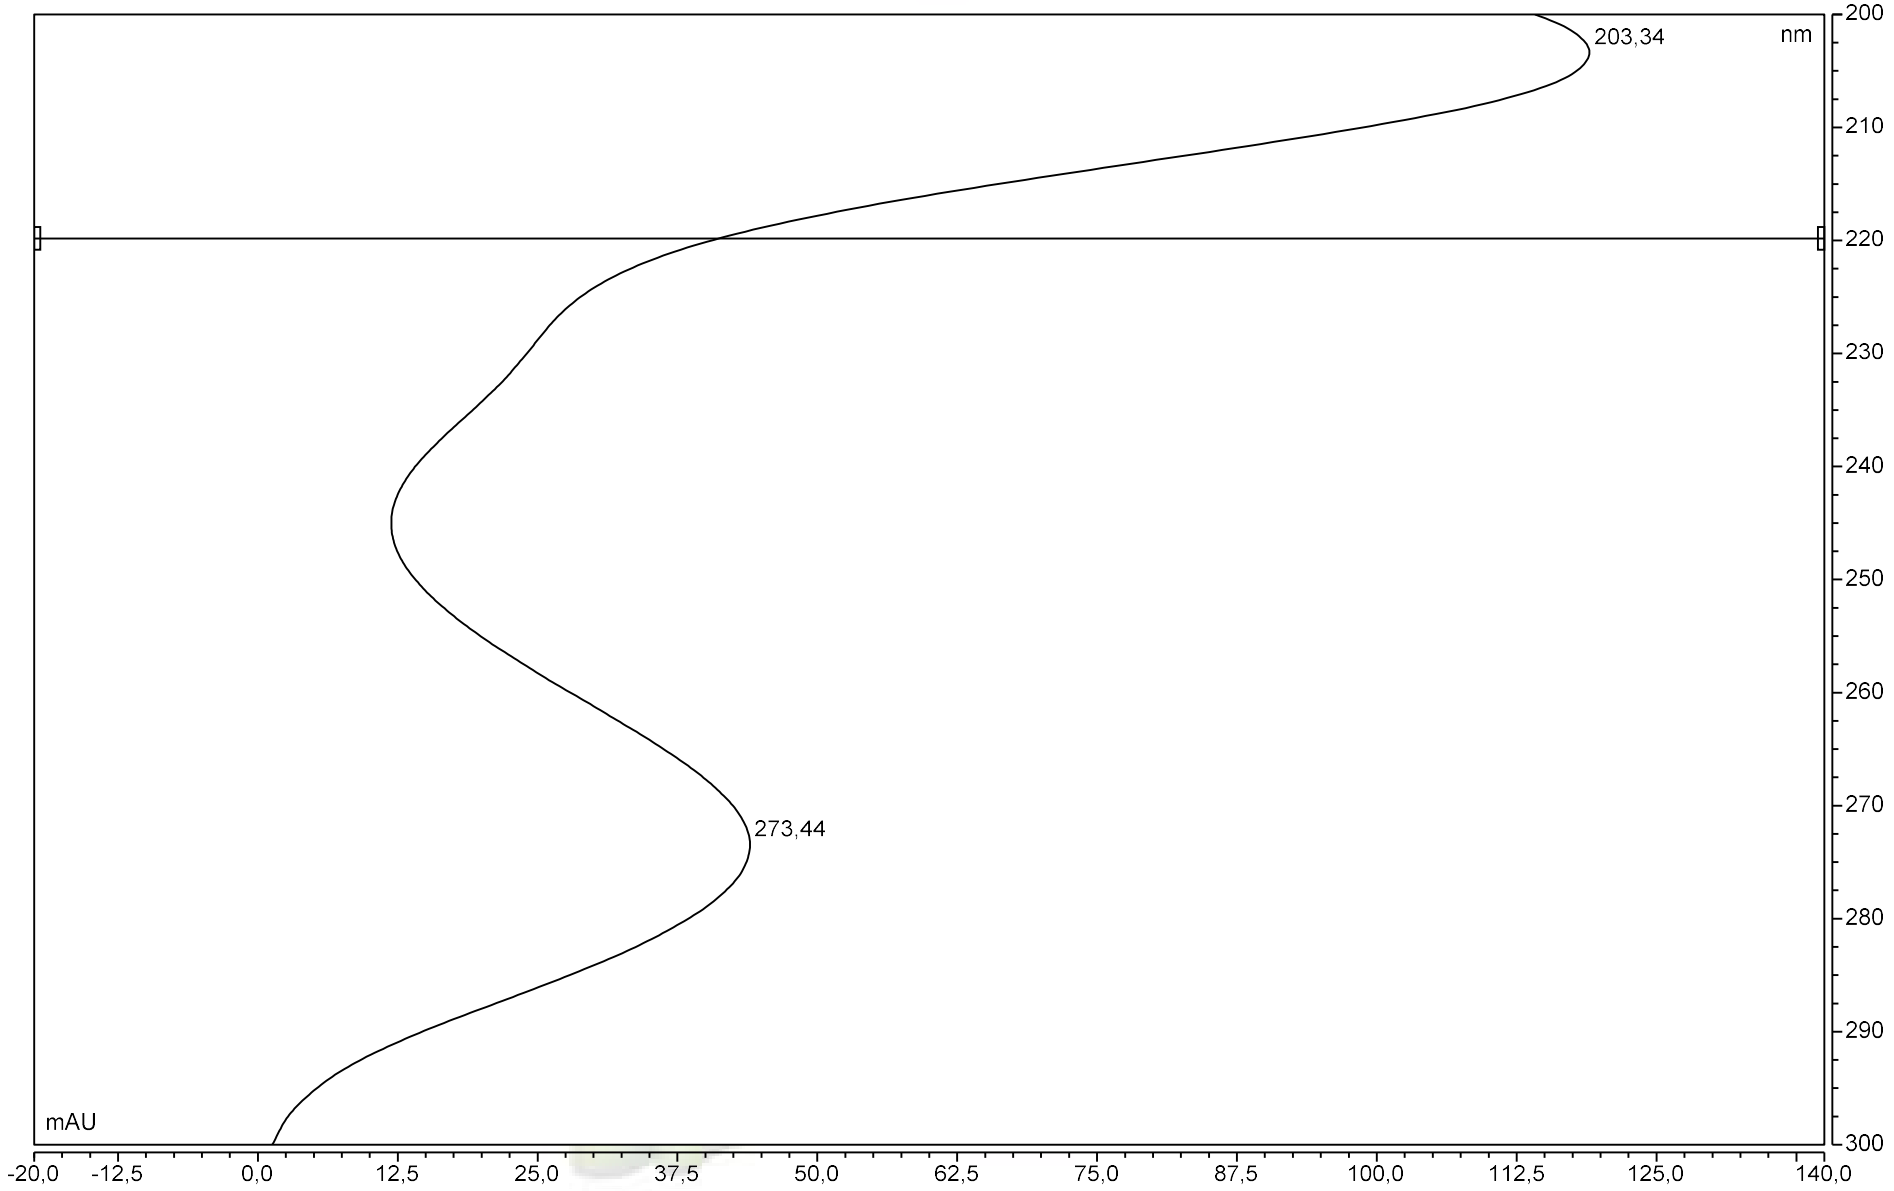
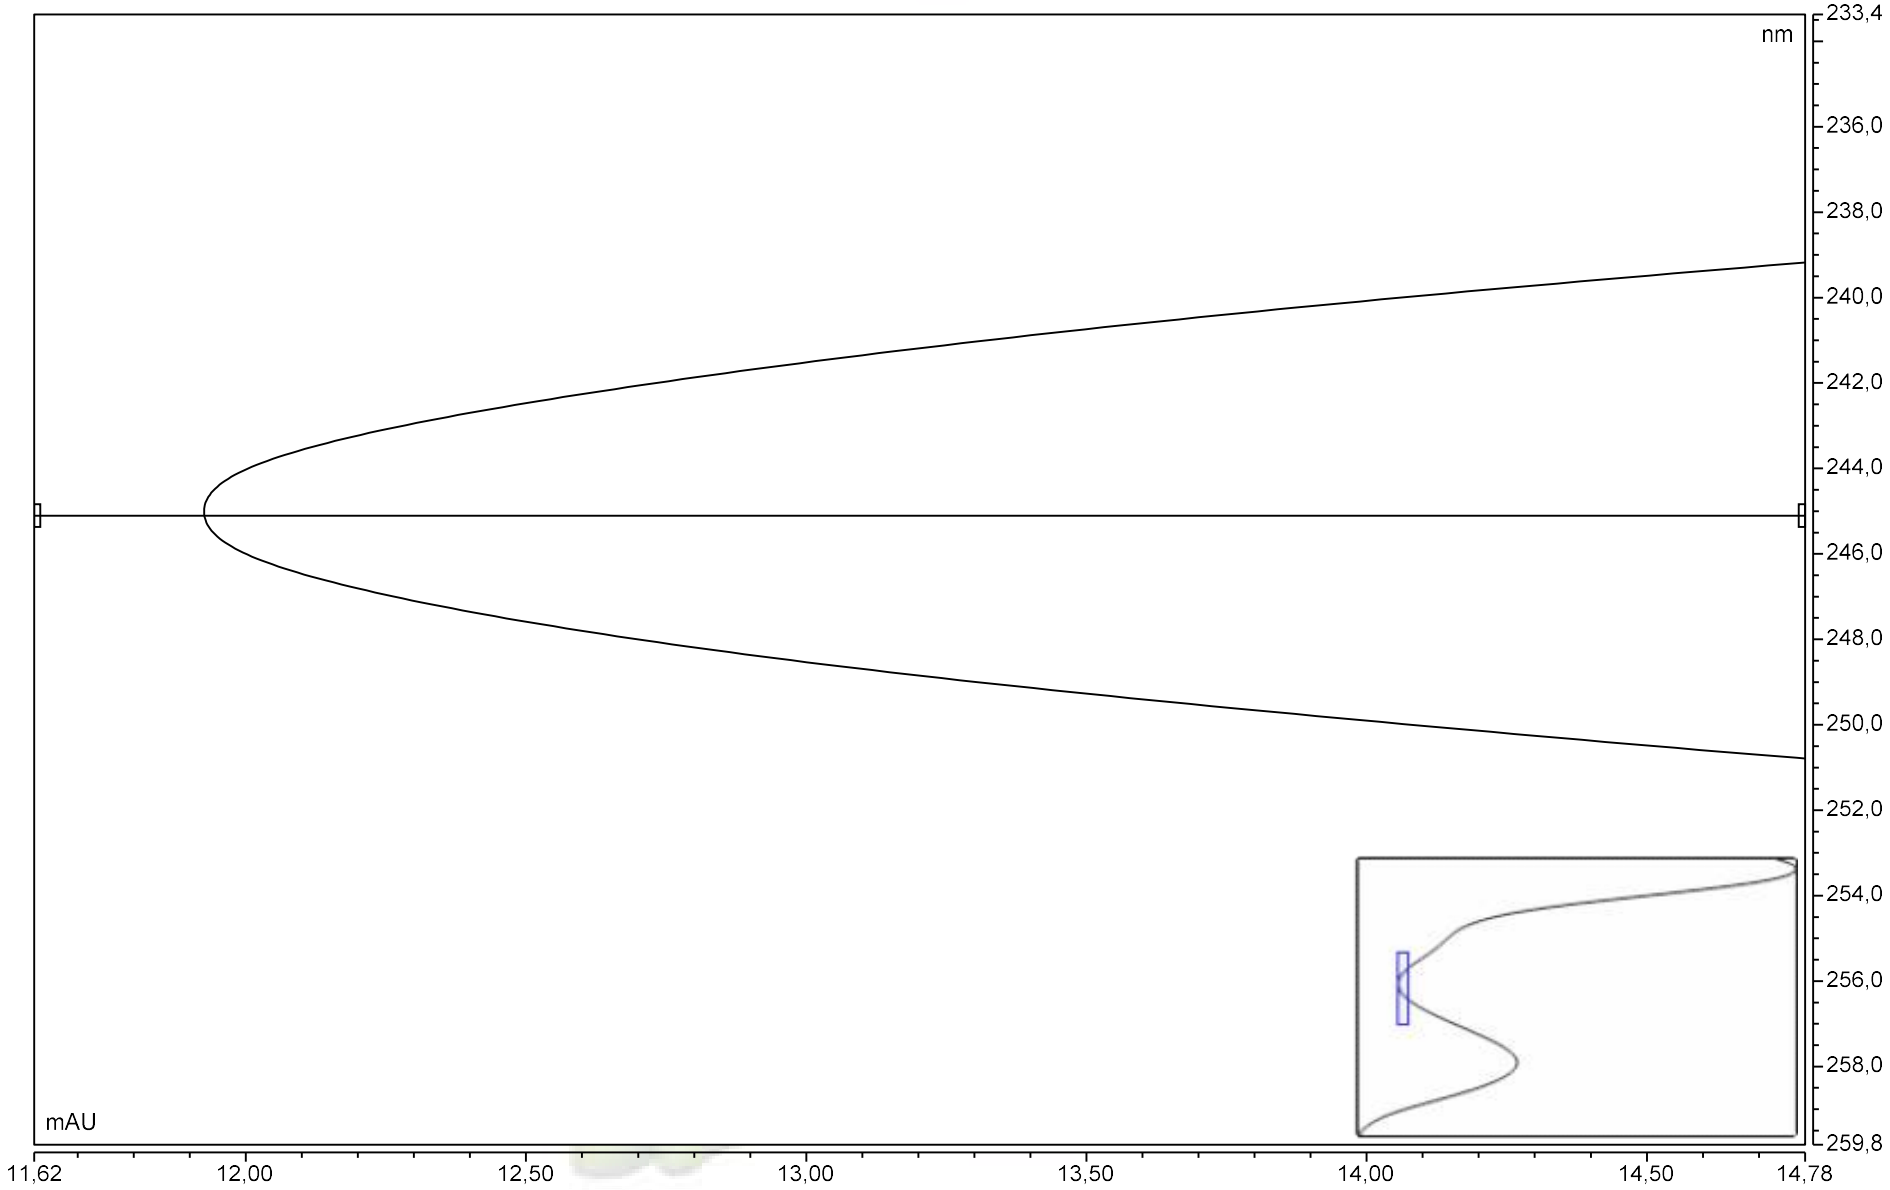

203,34
nm
273,44
mAU
200
210
220
230
240
250
260
270
280
290
300
-20,0
-12,5
0,0
12,5
25,0
37,5
50,0
62,5
75,0
87,5
100,0
112,5
125,0
140,0



nm
233,4
236,0
238,0
240,0
242,0
244,0
246,0
248,0
250,0
252,0
254,0
256,0
258,0
259,8
mAU
11,62
12,00
12,50
13,00
13,50
14,00
14,50
14,78

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:06**	*Sample Weight:*	**1,0000**

Chromatogram

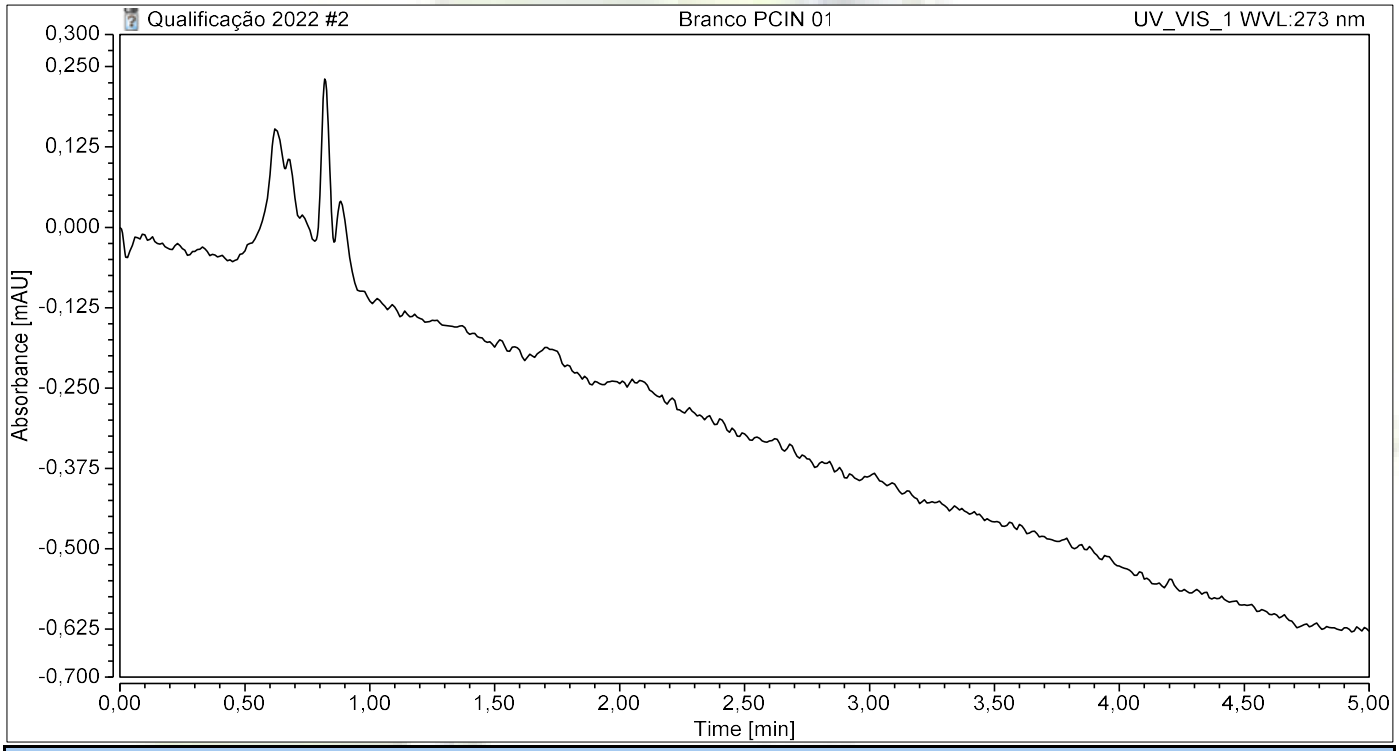

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:12**	*Sample Weight:*	**1,0000**

Chromatogram

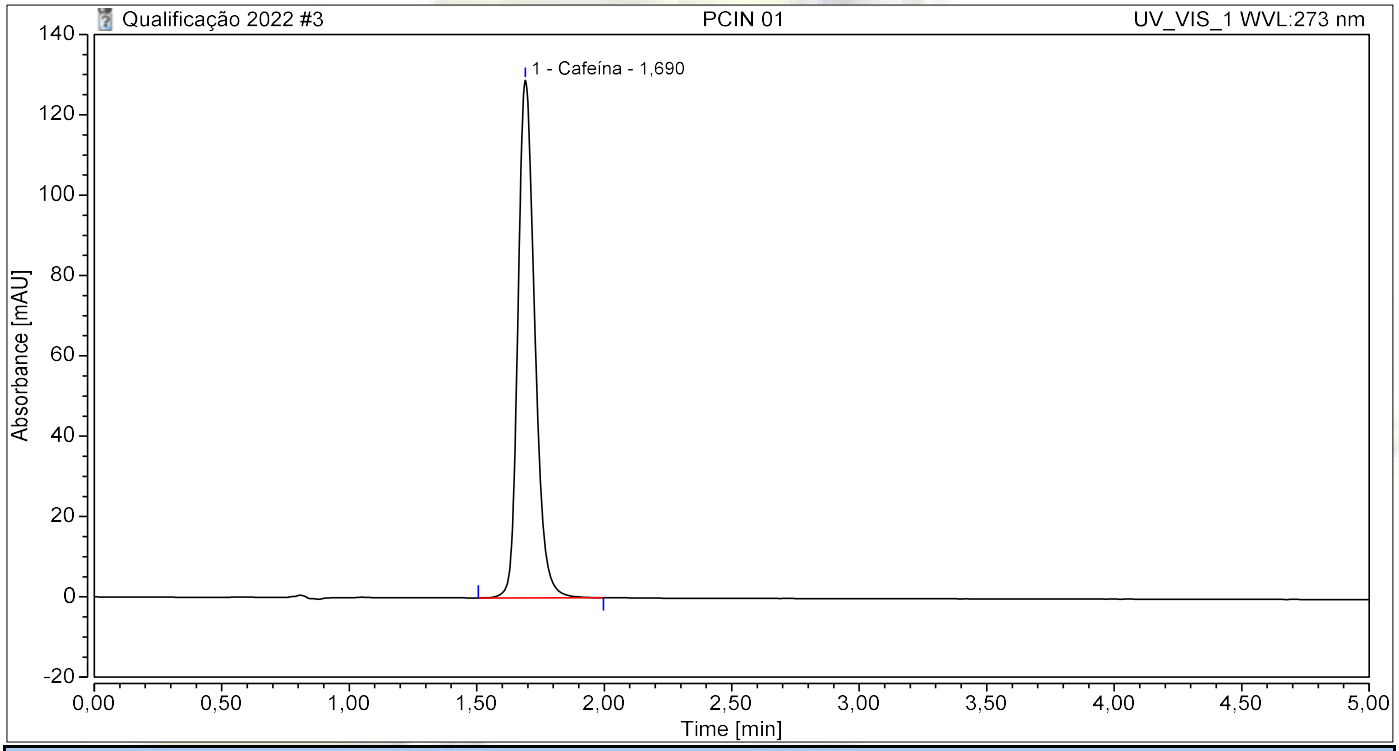

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,690	9,946	128,854	100,00	100,00	n.a.
Total:			**9,946**	**128,854**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:18**	*Sample Weight:*	**1,0000**

Chromatogram

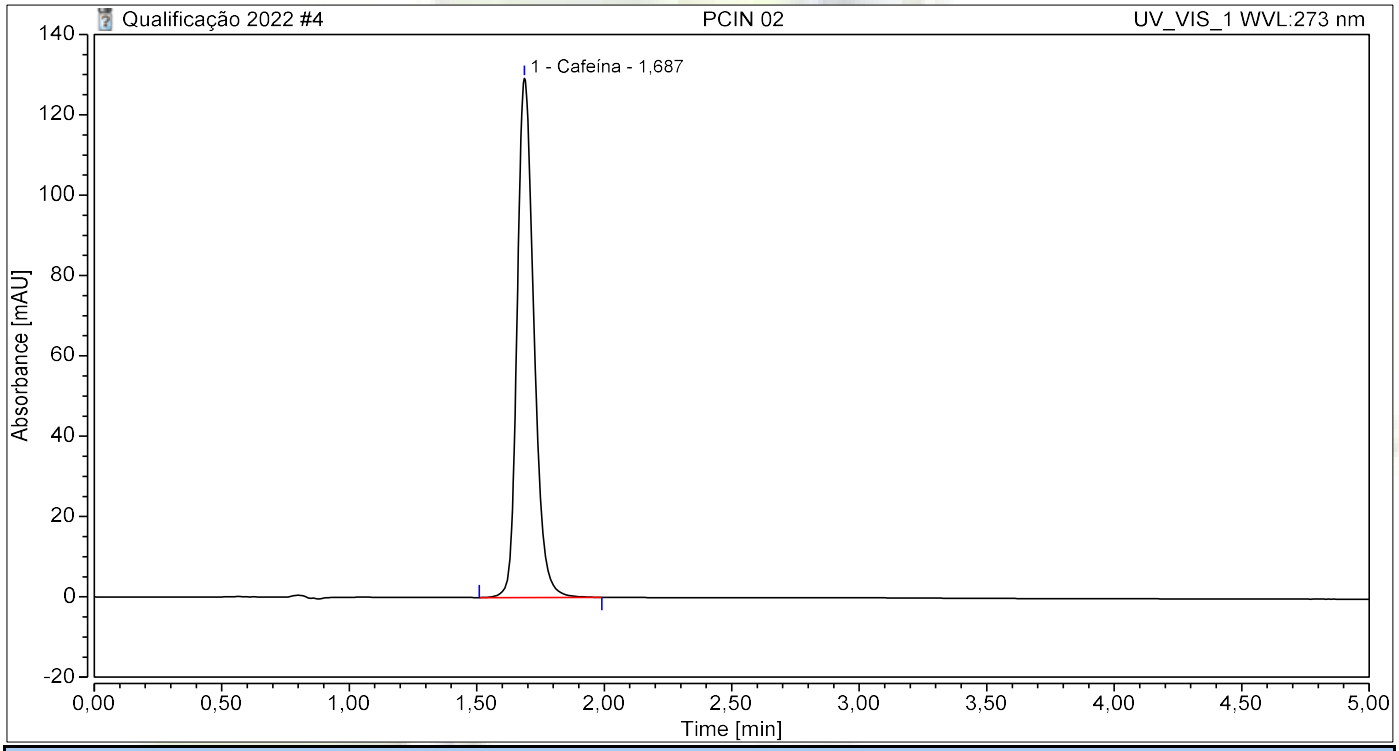

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,687	9,914	129,257	100,00	100,00	n.a.
Total:			**9,914**	**129,257**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:24**	*Sample Weight:*	**1,0000**

Chromatogram

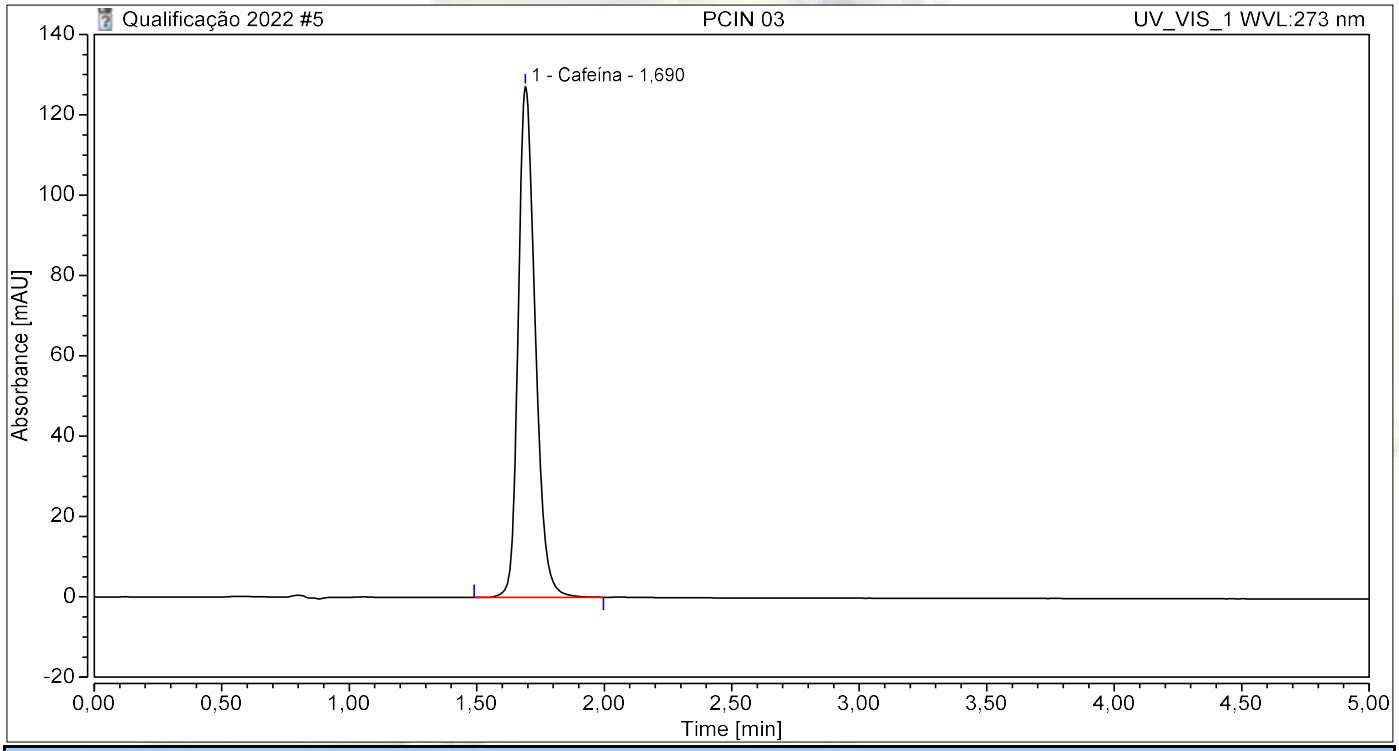

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,690	9,946	127,122	100,00	100,00	n.a.
Total:			**9,946**	**127,122**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:30**	*Sample Weight:*	**1,0000**

Chromatogram

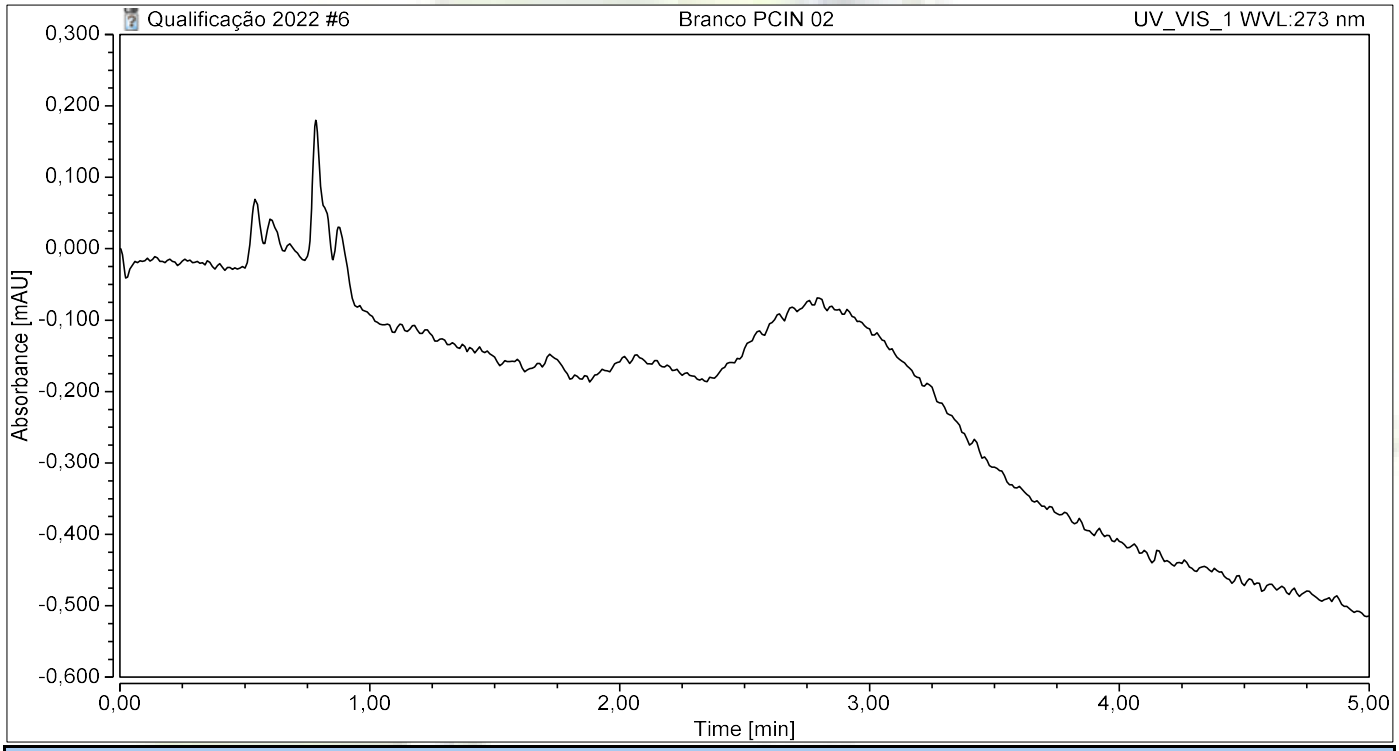

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 04**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:36**	*Sample Weight:*	**1,0000**

Chromatogram

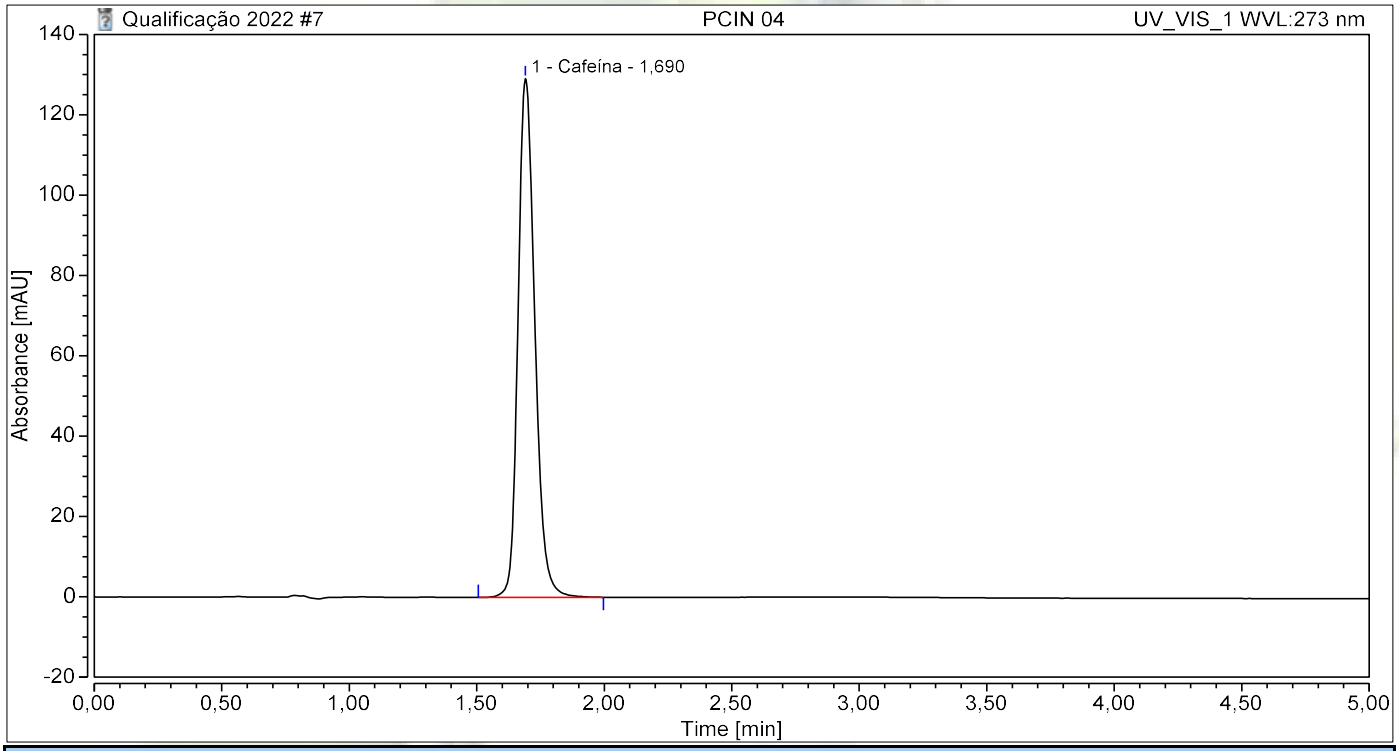

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,690	9,933	129,111	100,00	100,00	n.a.
Total:			**9,933**	**129,111**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 05**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:41**	*Sample Weight:*	**1,0000**

Chromatogram

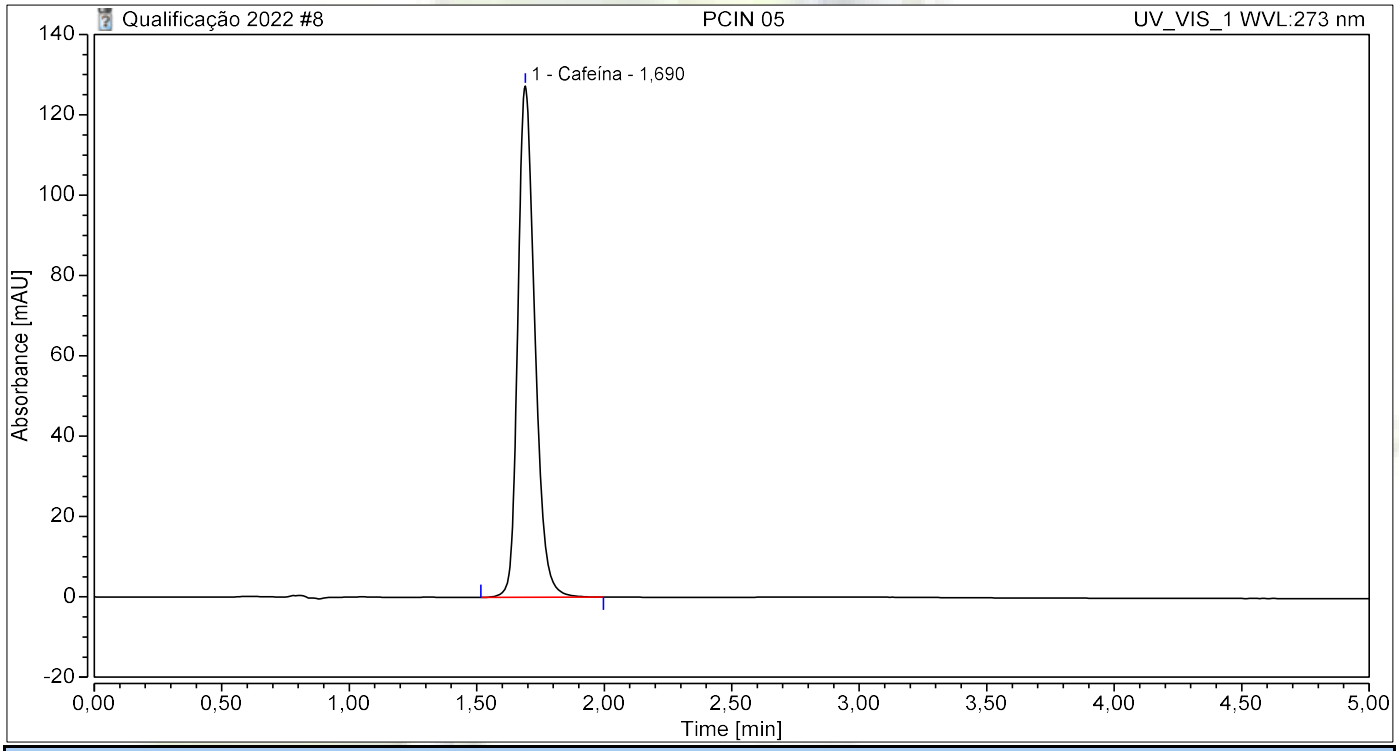

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,690	9,923	127,304	100,00	100,00	n.a.
Total:			**9,923**	**127,304**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN 06**	*Run Time (min):*	**5,00**
Vial Number:	**RA3**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:47**	*Sample Weight:*	**1,0000**

Chromatogram

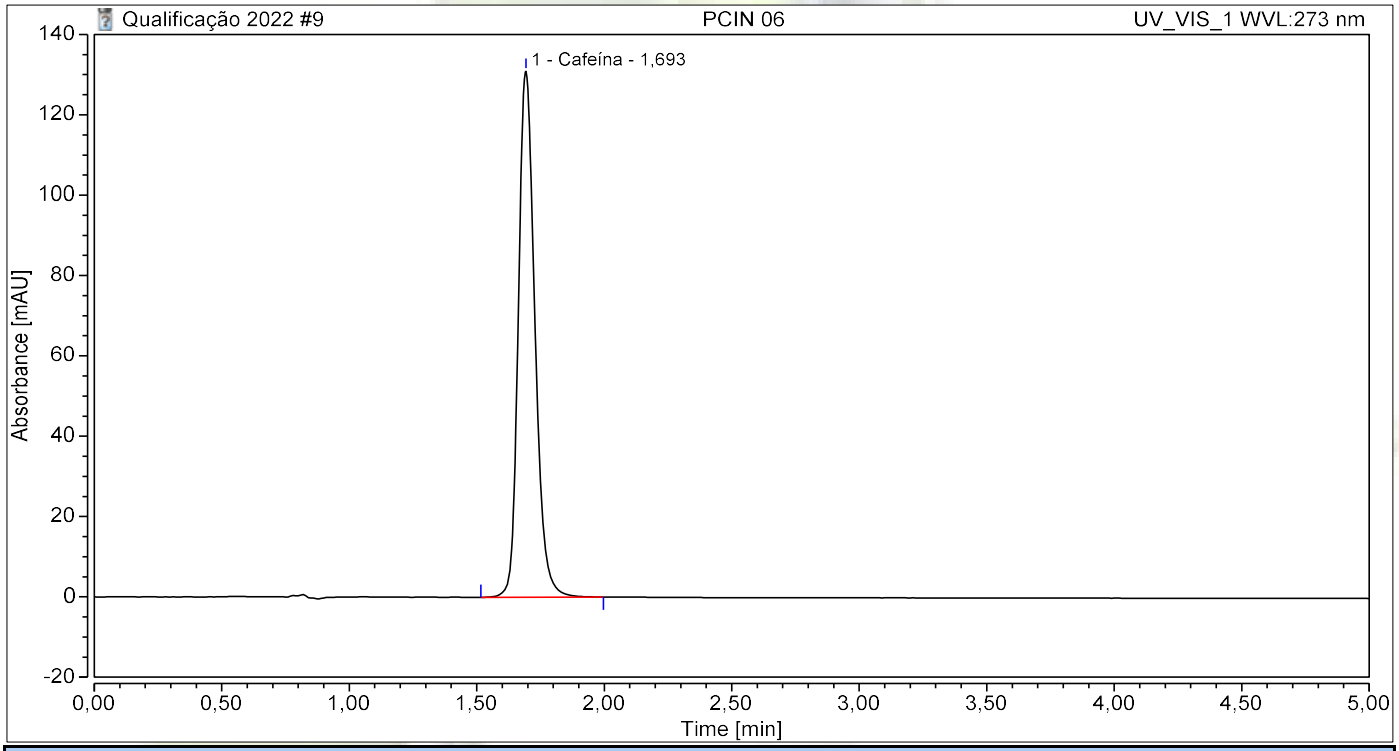

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,693	9,921	130,895	100,00	100,00	n.a.
Total:			**9,921**	**130,895**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**Branco PCIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA2**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:53**	*Sample Weight:*	**1,0000**

Chromatogram

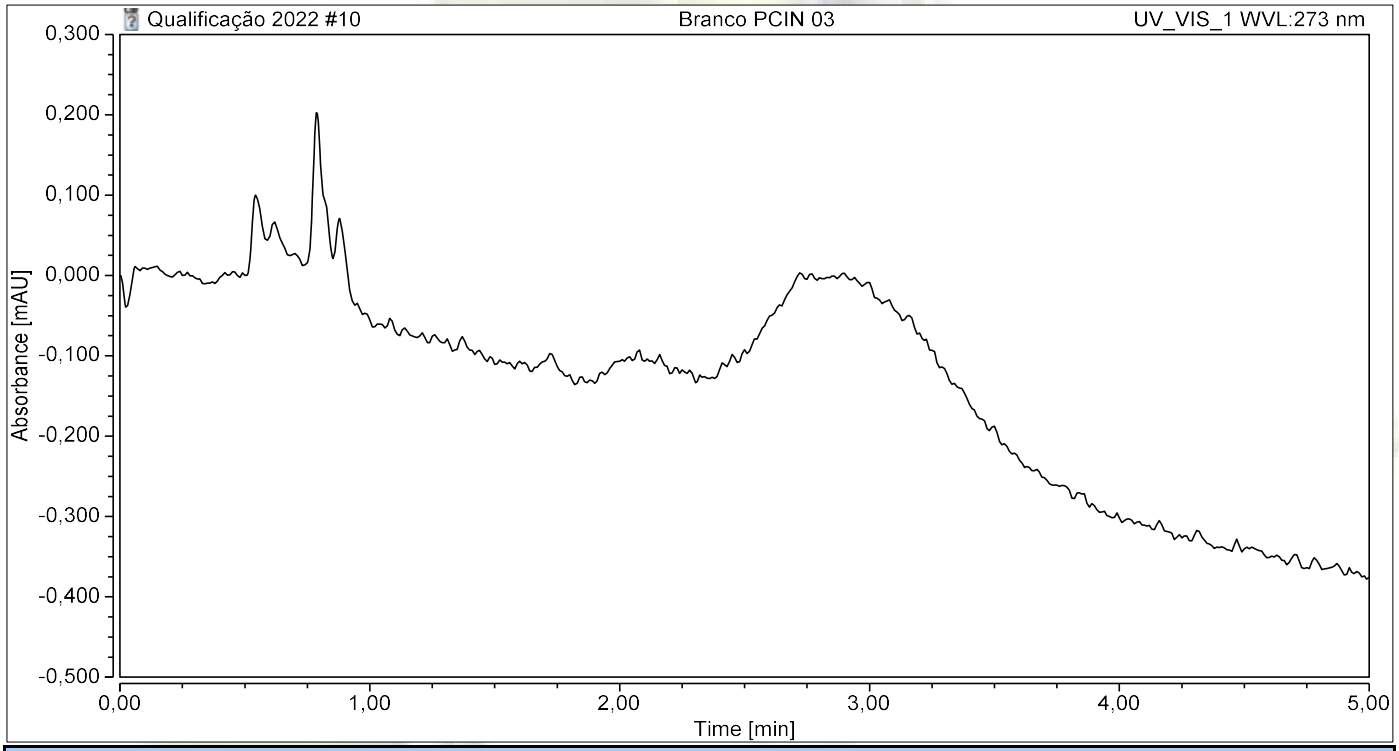

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**0,000**	**0,000**	**0,00**	**0,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 01**	*Run Time (min):*	**5,00**
Vial Number:	**RA4**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 17:59**	*Sample Weight:*	**1,0000**

Chromatogram

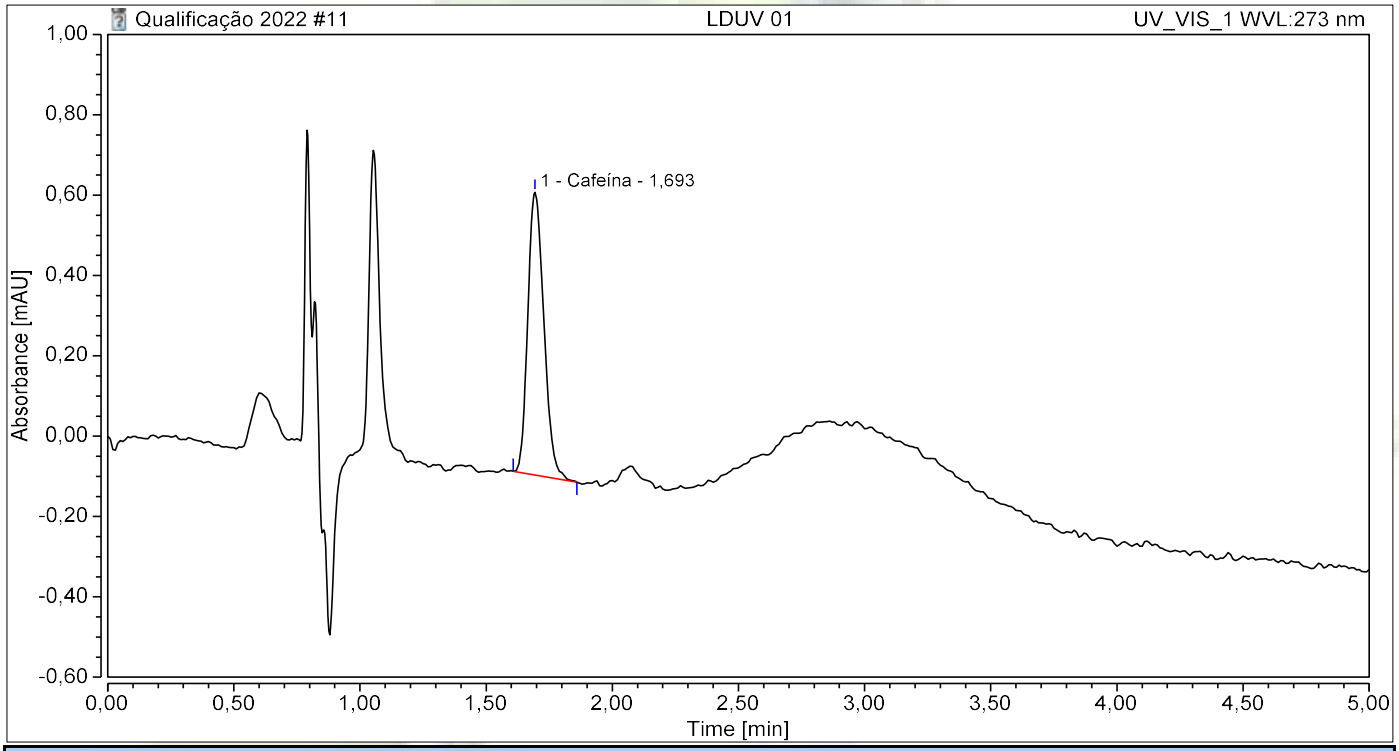

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,693	0,052	0,704	100,00	100,00	n.a.
Total:			**0,052**	**0,704**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 02**	*Run Time (min):*	**5,00**
Vial Number:	**RA5**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:05**	*Sample Weight:*	**1,0000**

Chromatogram

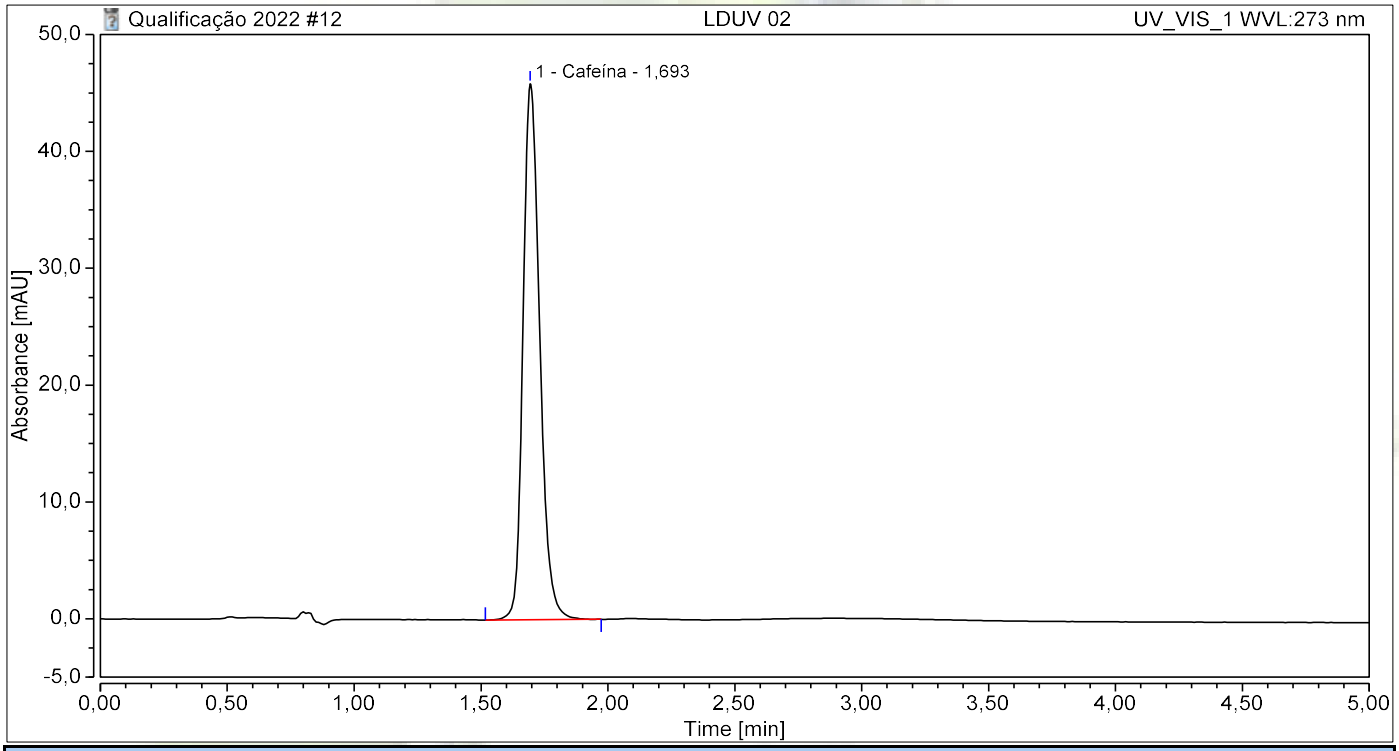

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,693	3,500	45,859	100,00	100,00	n.a.
Total:			**3,500**	**45,859**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 03**	*Run Time (min):*	**5,00**
Vial Number:	**RA6**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:11**	*Sample Weight:*	**1,0000**

Chromatogram

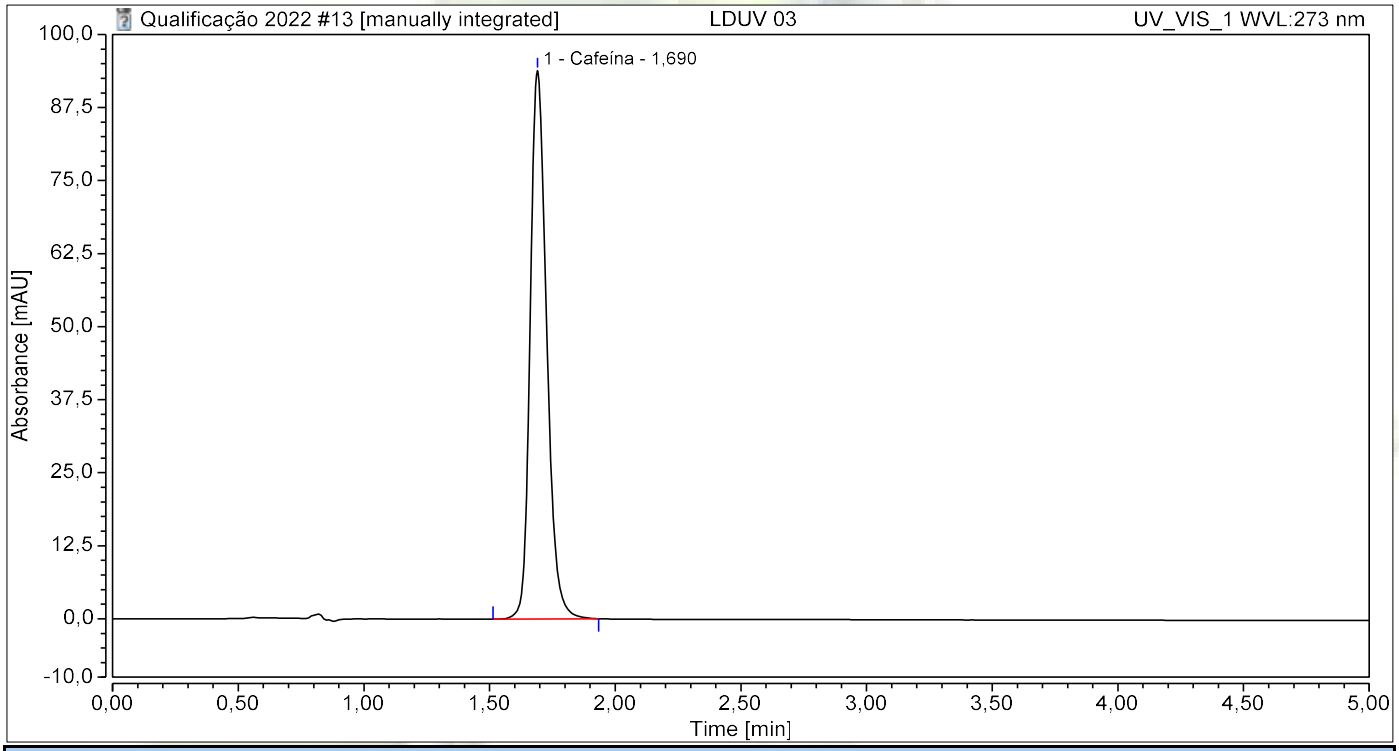

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,690	7,149	93,857	100,00	100,00	n.a.
Total:			**7,149**	**93,857**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 04**	*Run Time (min):*	**5,00**
Vial Number:	**RA7**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:17**	*Sample Weight:*	**1,0000**

Chromatogram

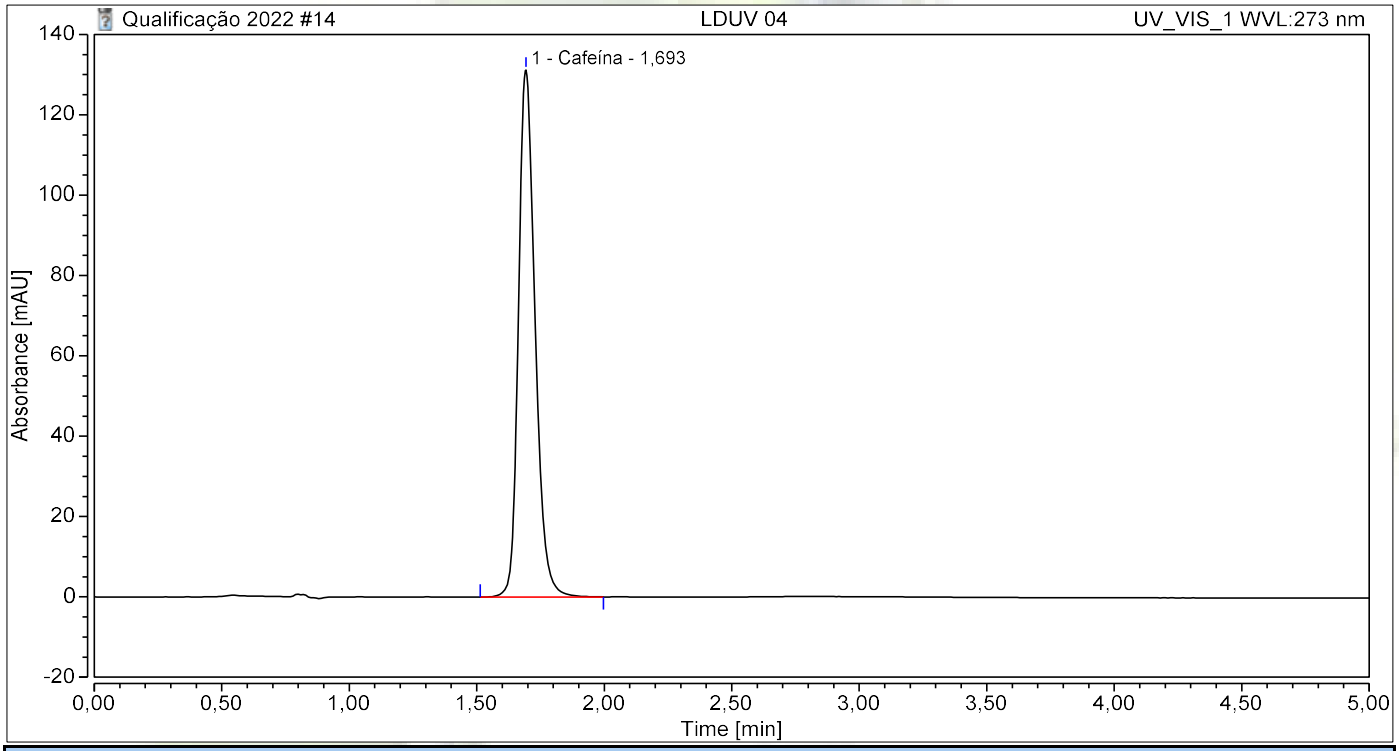

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,693	10,008	131,195	100,00	100,00	n.a.
Total:			**10,008**	**131,195**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LDUV 005**	*Run Time (min):*	**3,50**
Vial Number:	**RD8**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação2**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**10/set/21 12:51**	*Sample Weight:*	**1,0000**

Chromatogram

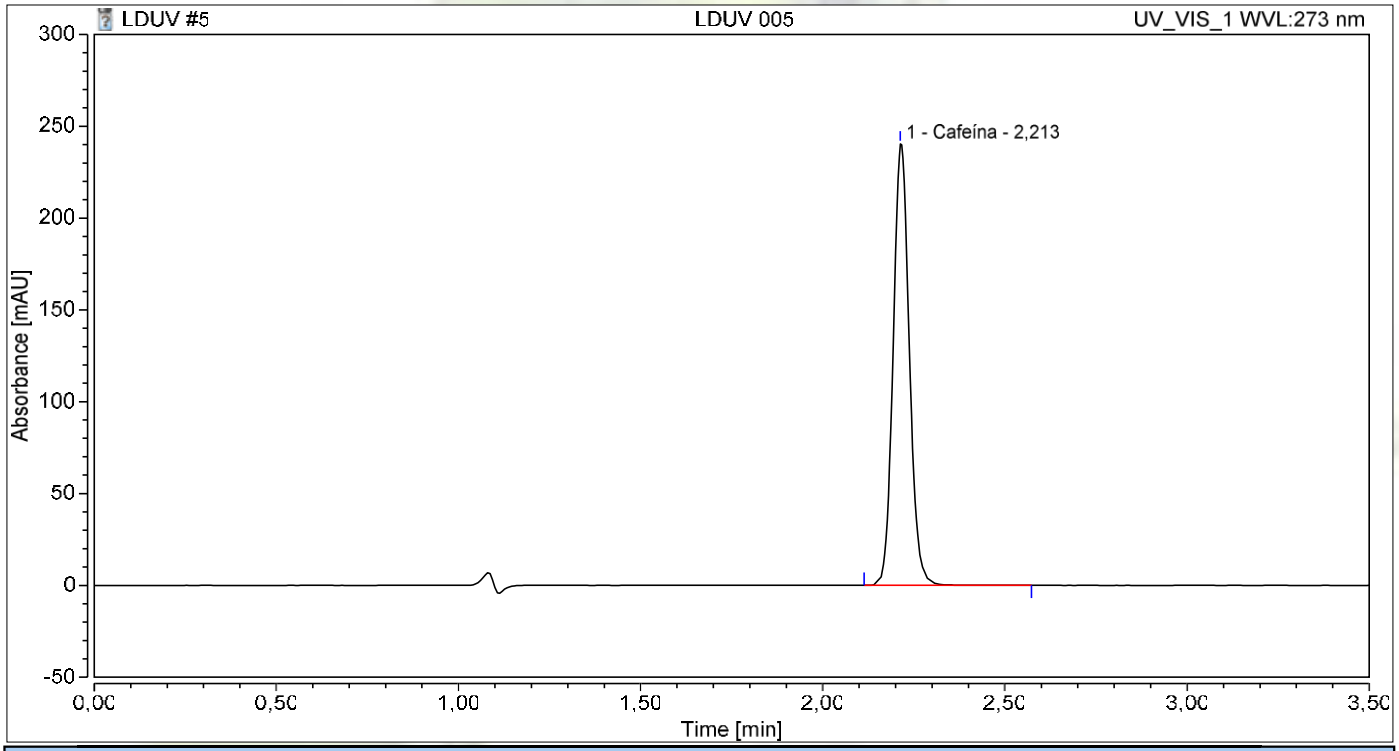

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	2,213	13,751	240,372	100,00	100,00	n.a.
Total:			**13,751**	**240,372**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 01**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**0,10**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:28**	*Sample Weight:*	**1,0000**

Chromatogram

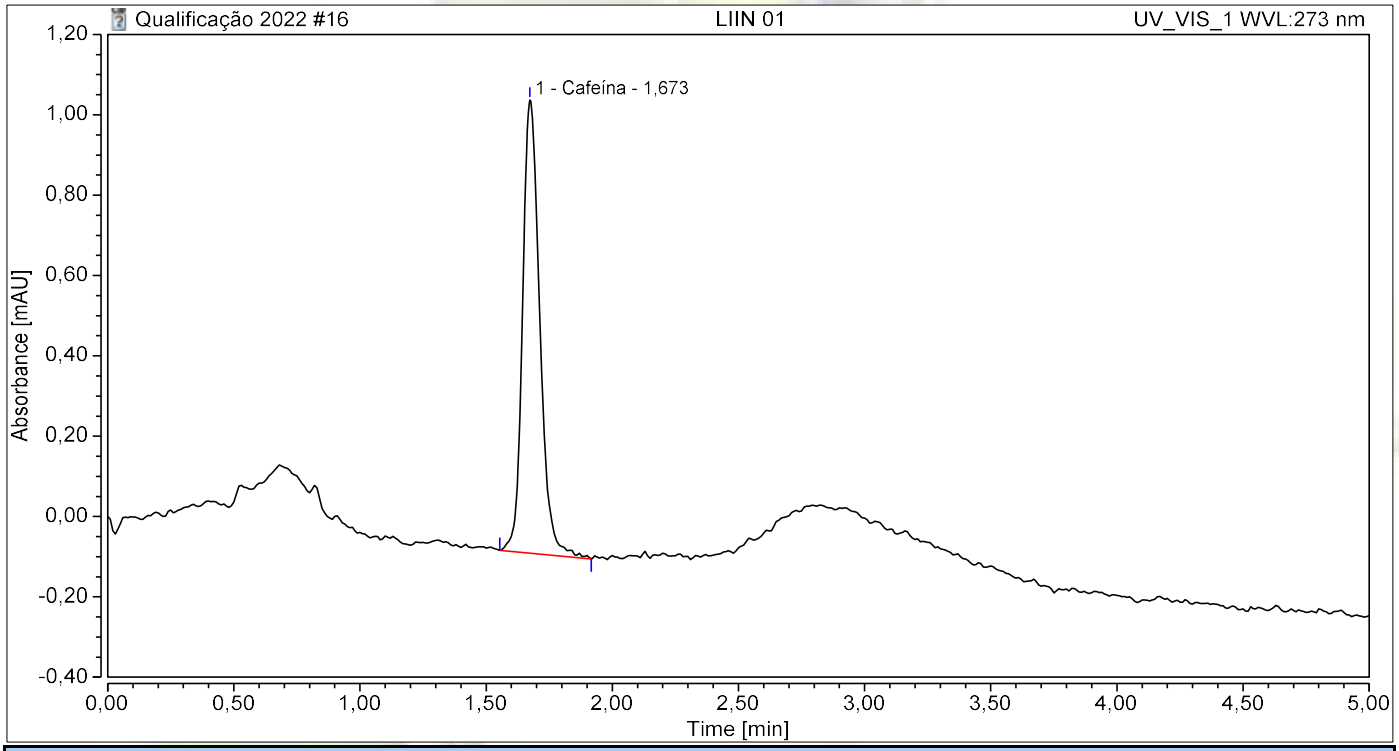

Integration Results


No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,673	0,089	1,128	100,00	100,00	n.a.
Total:			**0,089**	**1,128**	**100,00**	**100,00**	

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 02**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:34**	*Sample Weight:*	**1,0000**

Chromatogram

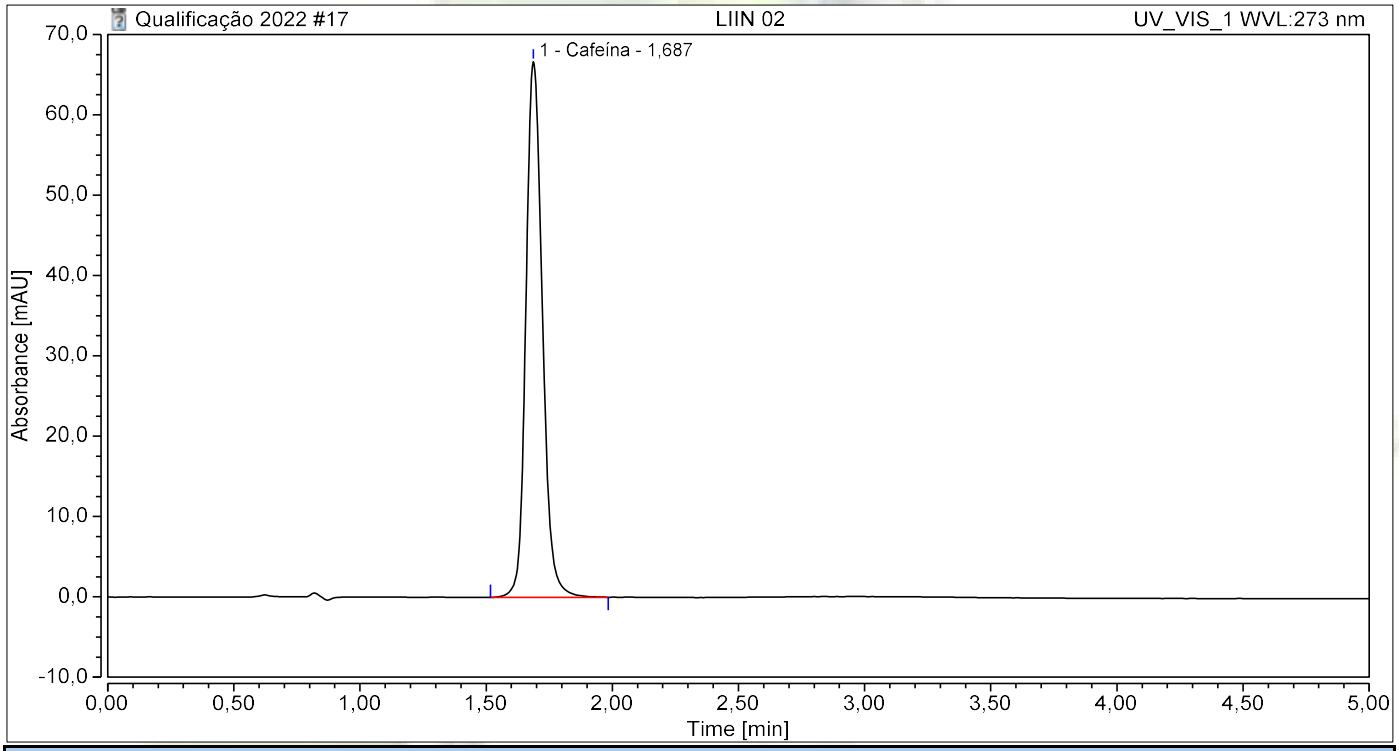

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,687	5,050	66,649	100,00	100,00	n.a.
Total:			**5,050**	**66,649**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 03**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**10,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:40**	*Sample Weight:*	**1,0000**

Chromatogram

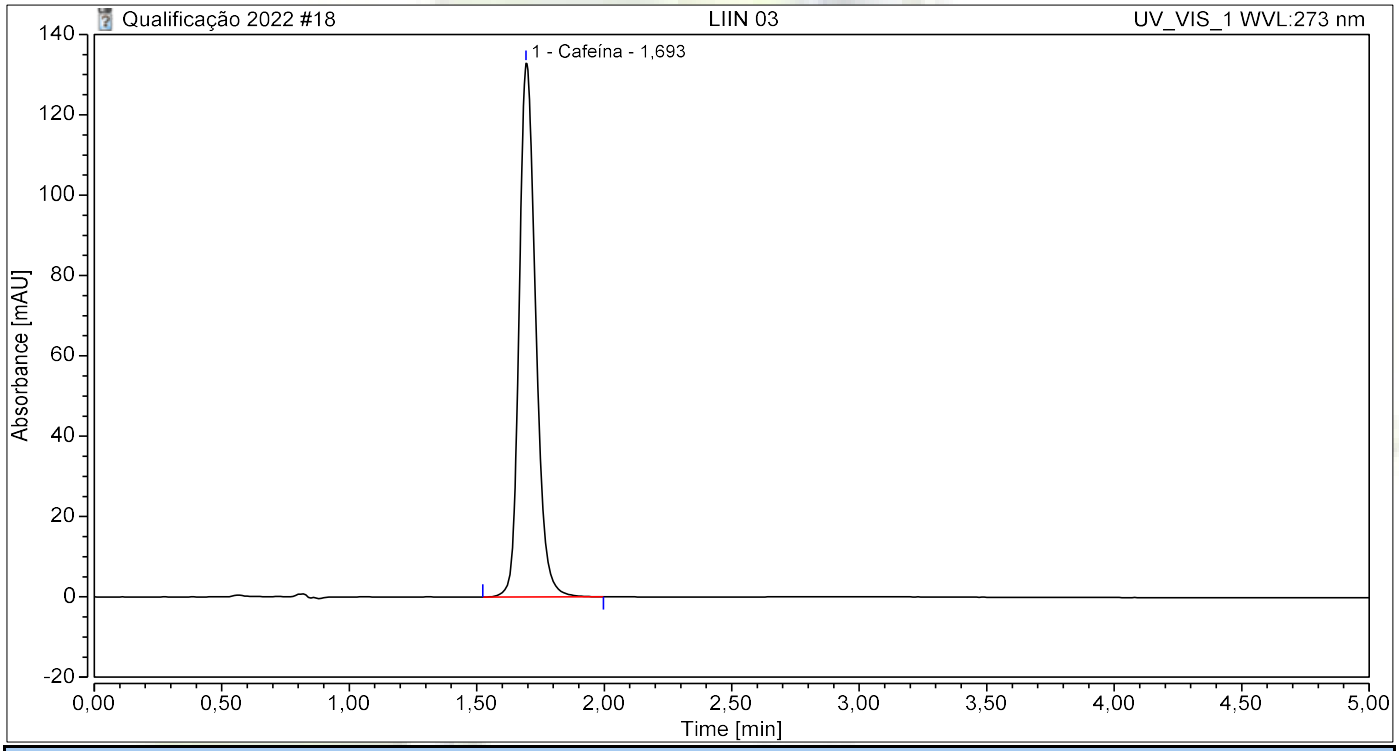

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,693	10,104	132,838	100,00	100,00	n.a.
Total:			**10,104**	**132,838**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 04**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**15,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:46**	*Sample Weight:*	**1,0000**

Chromatogram

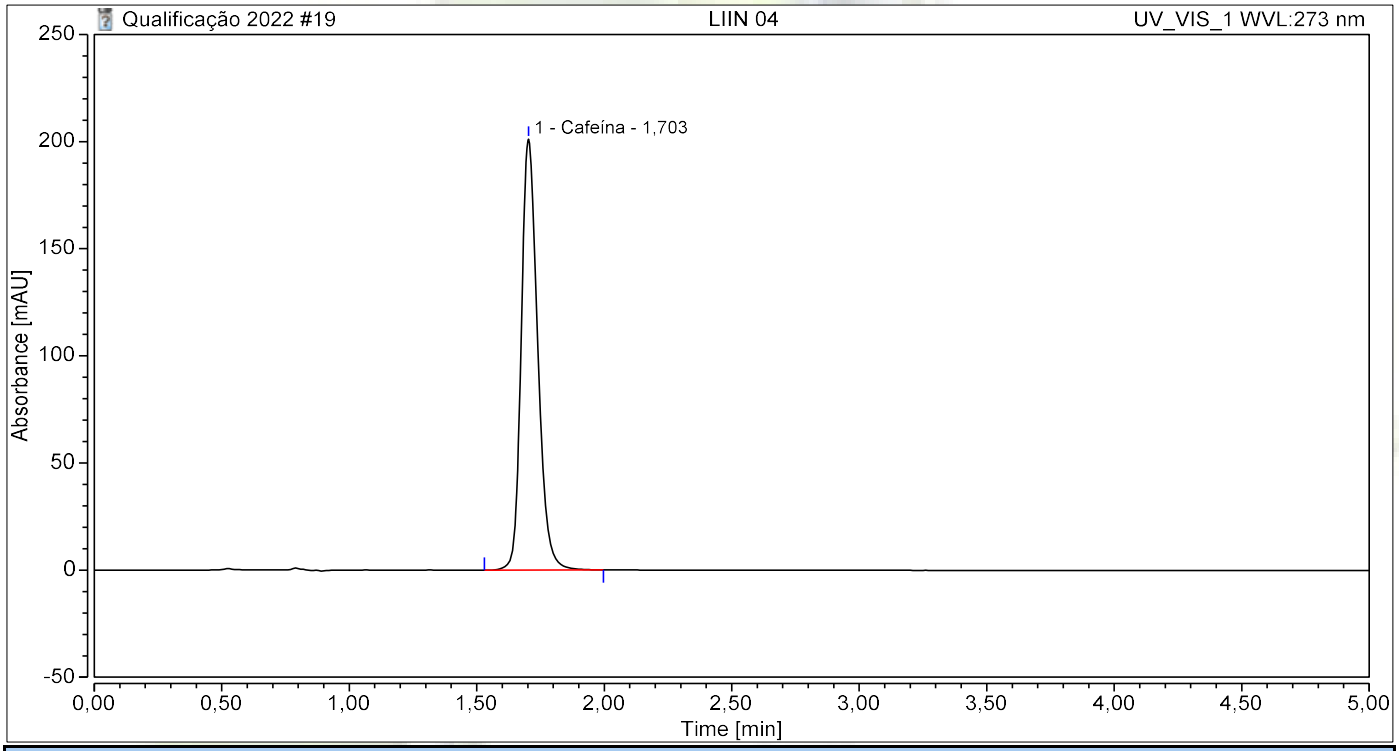

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,703	15,152	201,098	100,00	100,00	n.a.
Total:			**15,152**	**201,098**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**LIIN 05**	*Run Time (min):*	**5,00**
Vial Number:	**RB1**	*Injection Volume:*	**20,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**Qualificação 2022**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**13/set/22 18:52**	*Sample Weight:*	**1,0000**

Chromatogram

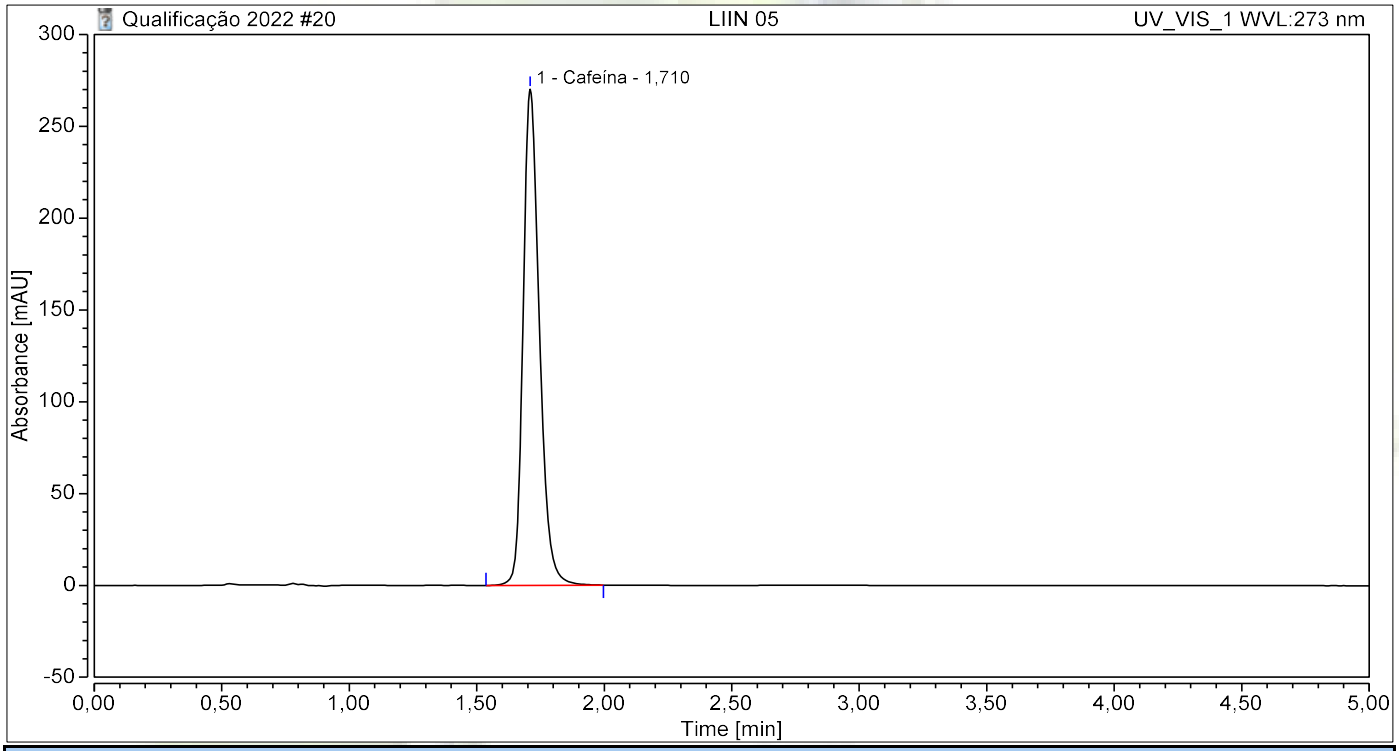

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	Cafeína	1,710	20,193	270,139	100,00	100,00	n.a.
Total:			**20,193**	**270,139**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**GRAD AB**	*Run Time (min):*	**18,00**
Vial Number:	**RA2**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD AB**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 09:17**	*Sample Weight:*	**1,0000**

Chromatogram

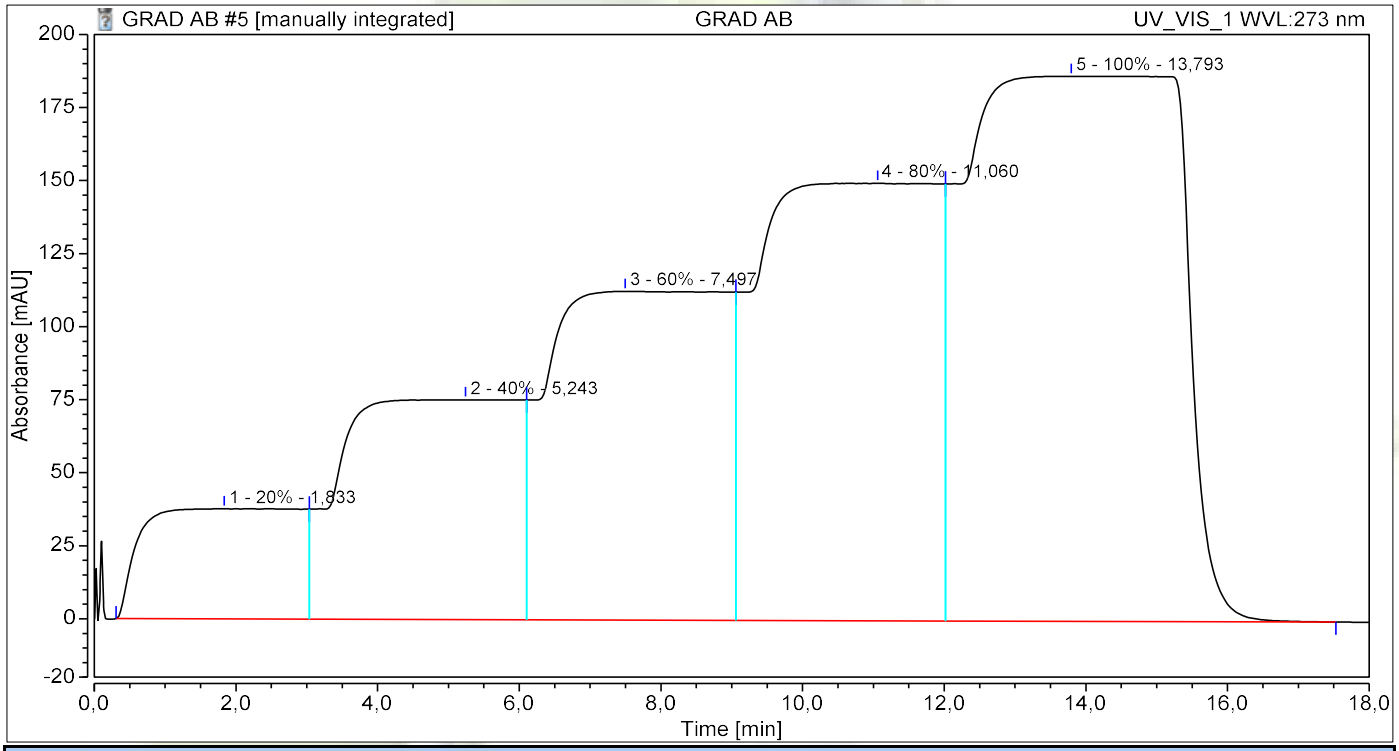

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	20%	1,833	93,422	37,702	5,54	6,71	n.a.
2	40%	5,243	211,451	75,259	12,55	13,40	n.a.
3	60%	7,497	315,817	112,494	18,74	20,03	n.a.
4	80%	11,060	425,675	149,746	25,26	26,66	n.a.
5	100%	13,793	638,830	186,555	37,91	33,21	n.a.
Total:			**1685,196**	**561,756**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**GRAD CD**	*Run Time (min):*	**18,00**
Vial Number:	**RA2**	*Injection Volume:*	**0,00**
Injection Type:	**Unknown**	*Channel:*	**UV_VIS_1**
Calibration Level:		*Wavelength:*	**273**
Instrument Method:	**GRAD CD**	*Bandwidth:*	**5**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 09:44**	*Sample Weight:*	**1,0000**

Chromatogram

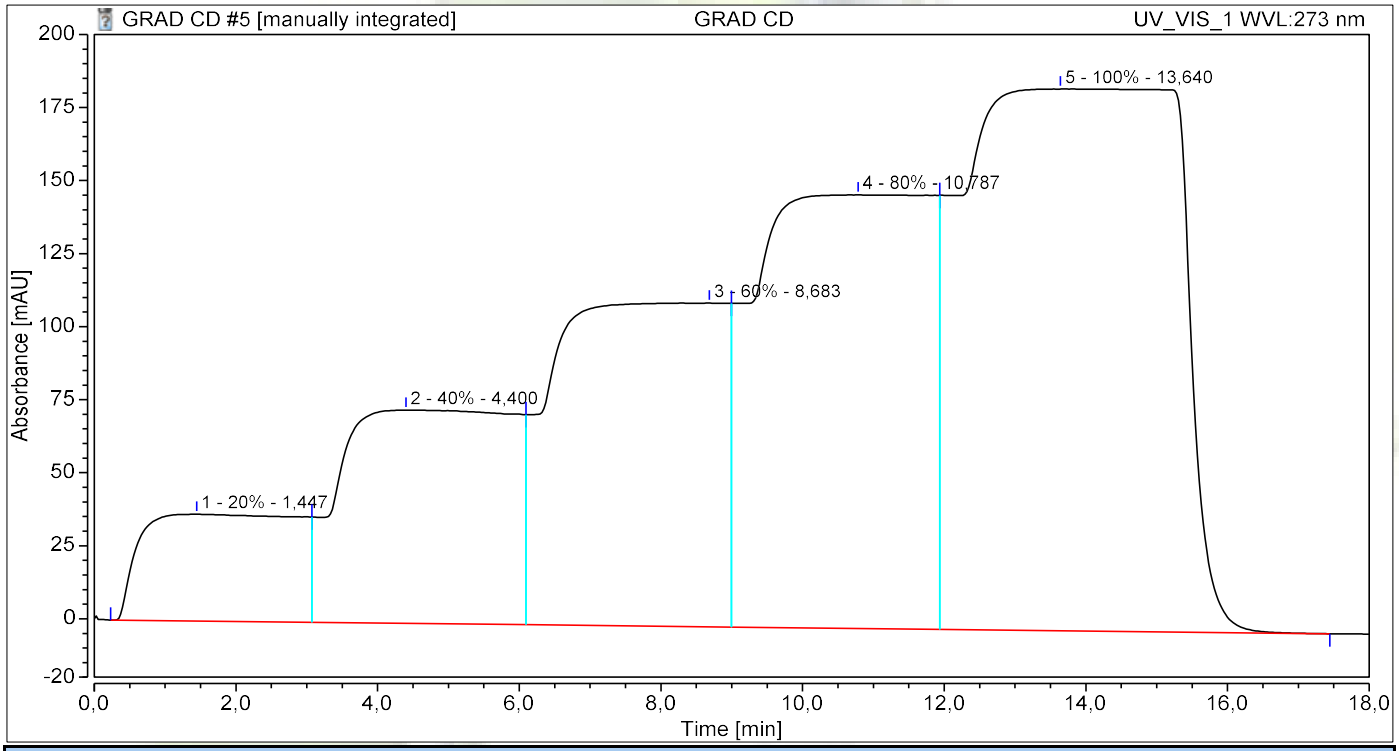

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount
1	20%	1,447	91,437	36,553	5,51	6,60	n.a.
2	40%	4,400	202,468	73,007	12,20	13,17	n.a.
3	60%	8,683	302,241	110,774	18,21	19,99	n.a.
4	80%	10,787	416,273	148,407	25,09	26,78	n.a.
5	100%	13,640	647,025	185,410	38,99	33,46	n.a.
Total:			**1659,442**	**554,151**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 1**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:12**	*Sample Weight:*	**1,0000**

Chromatogram

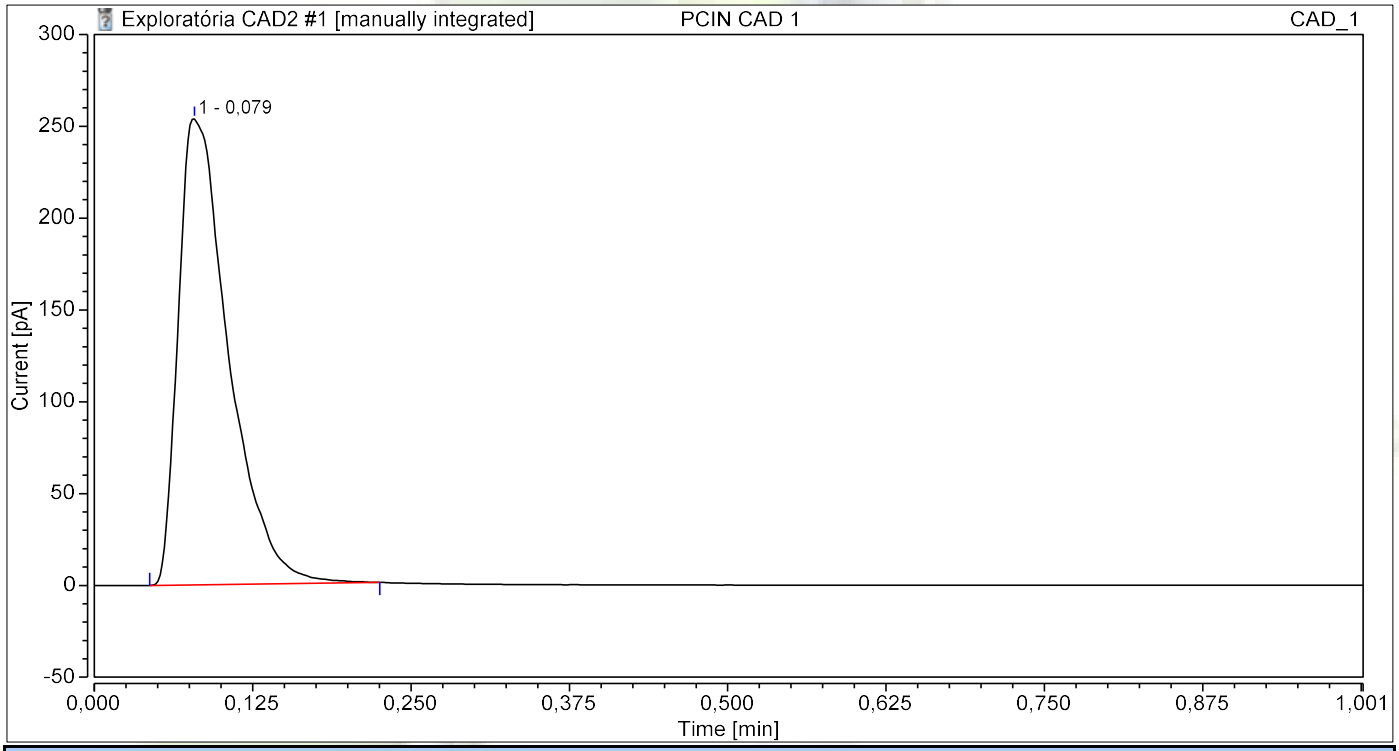

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,079	11,676	253,581	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,676**	**253,581**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 2**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:13**	*Sample Weight:*	**1,0000**

Chromatogram

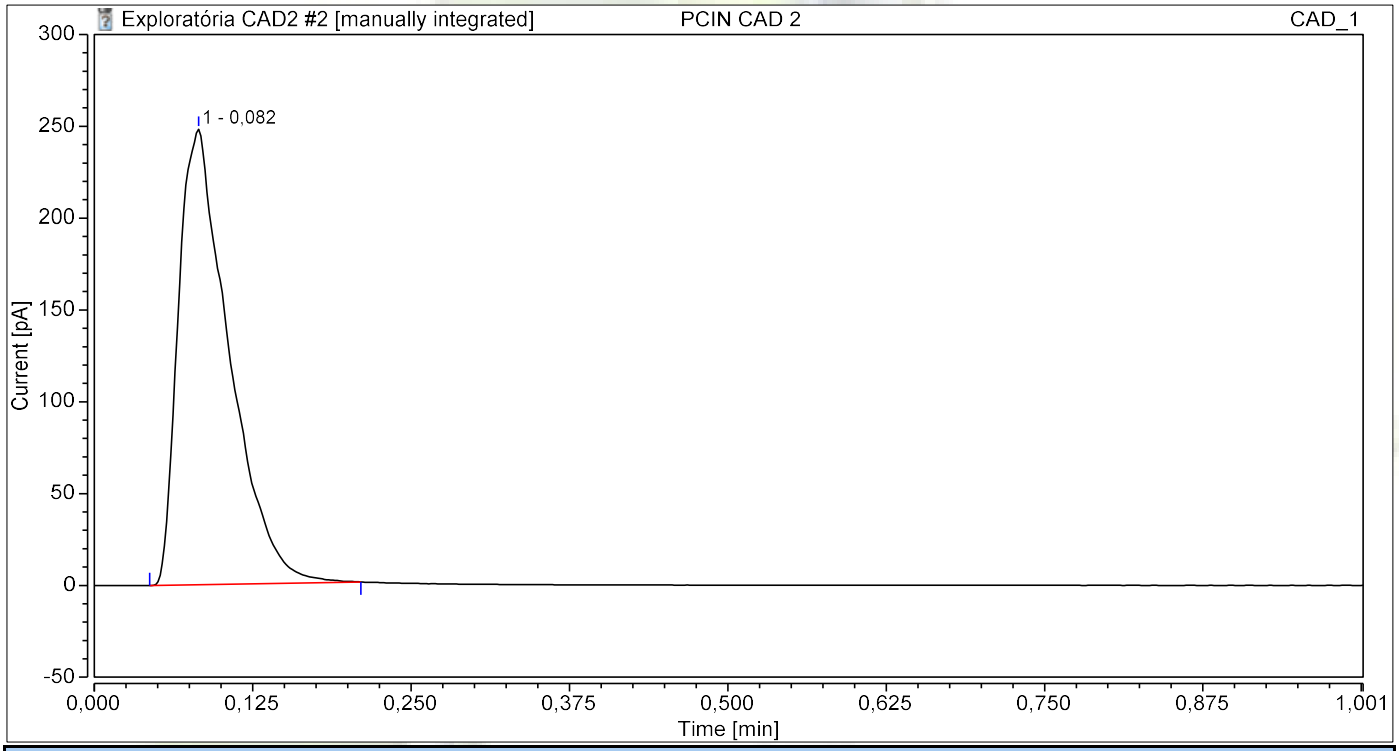

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,082	11,500	248,010	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,500**	**248,010**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 3**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:15**	*Sample Weight:*	**1,0000**

Chromatogram

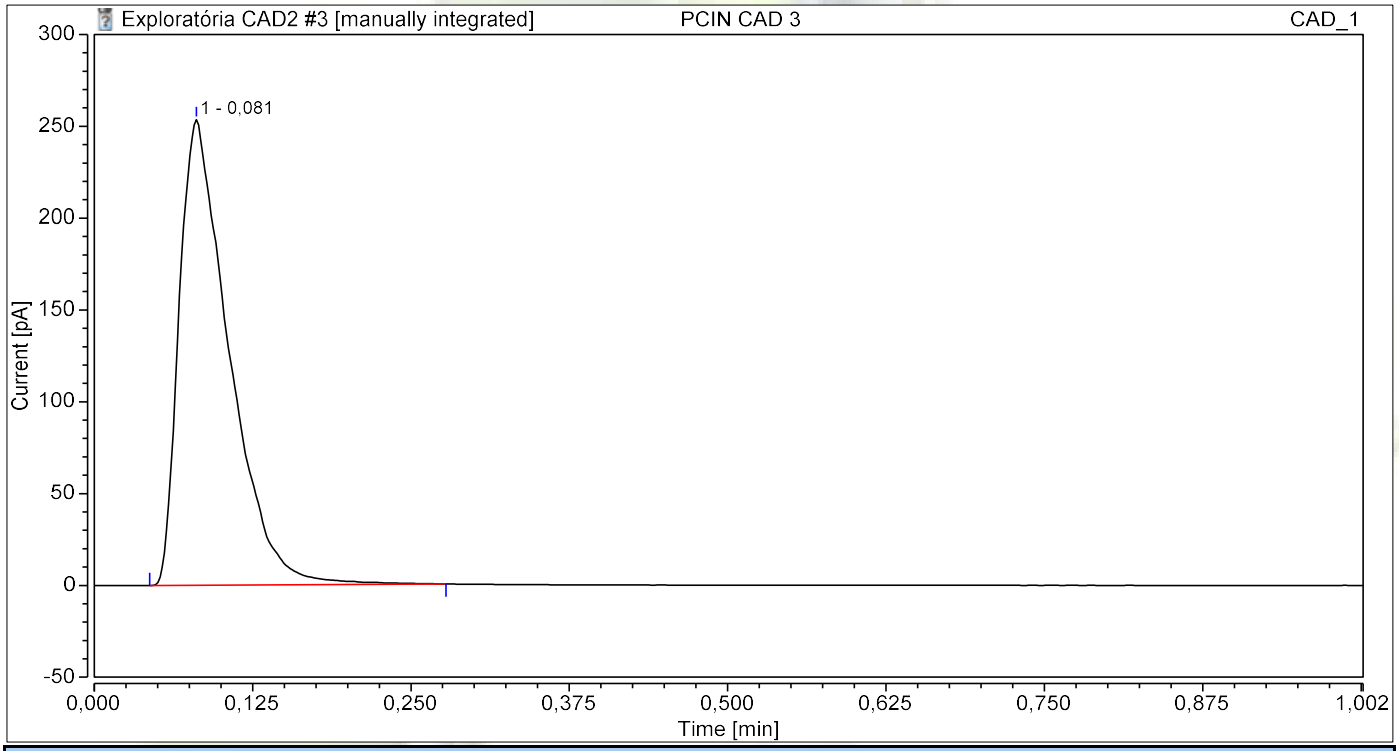

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,081	11,536	253,594	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,536**	**253,594**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 4**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:17**	*Sample Weight:*	**1,0000**

Chromatogram

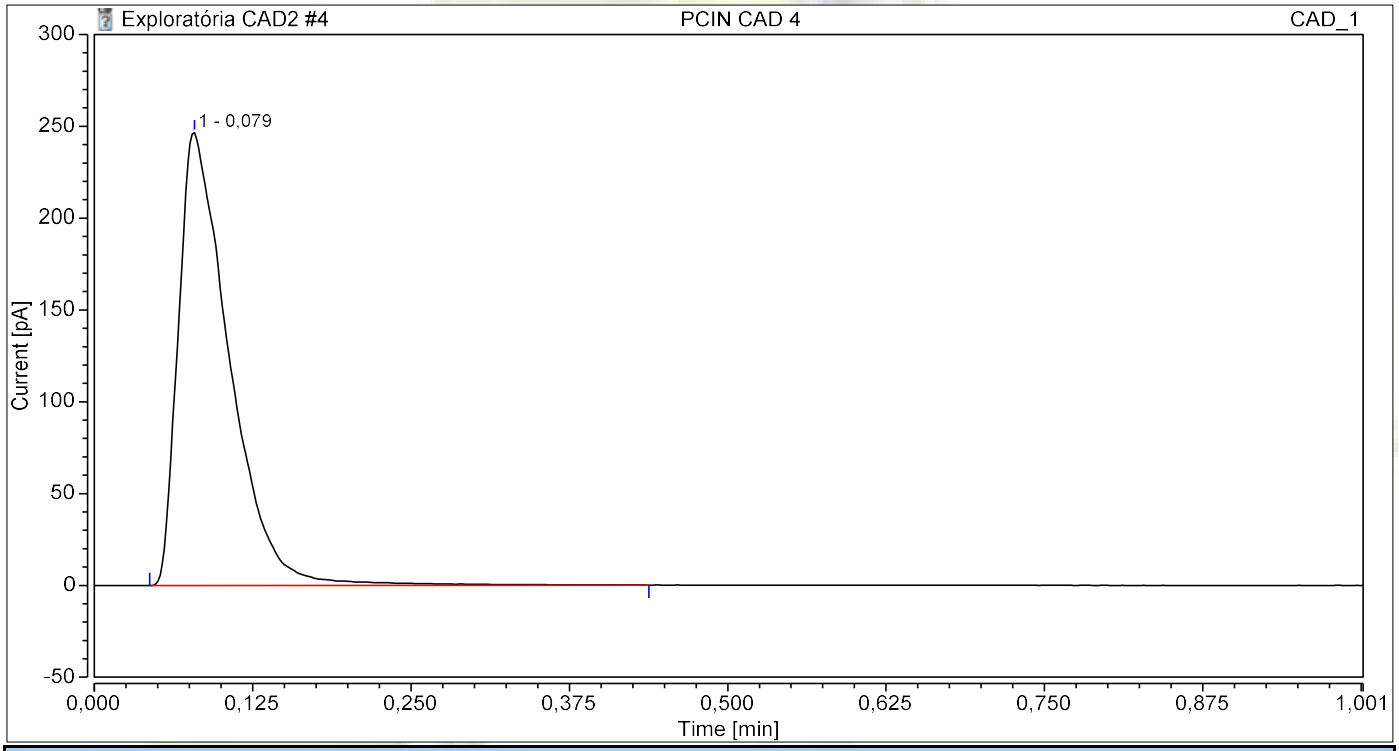

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,079	11,500	246,533	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,500**	**246,533**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 5**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:19**	*Sample Weight:*	**1,0000**

Chromatogram

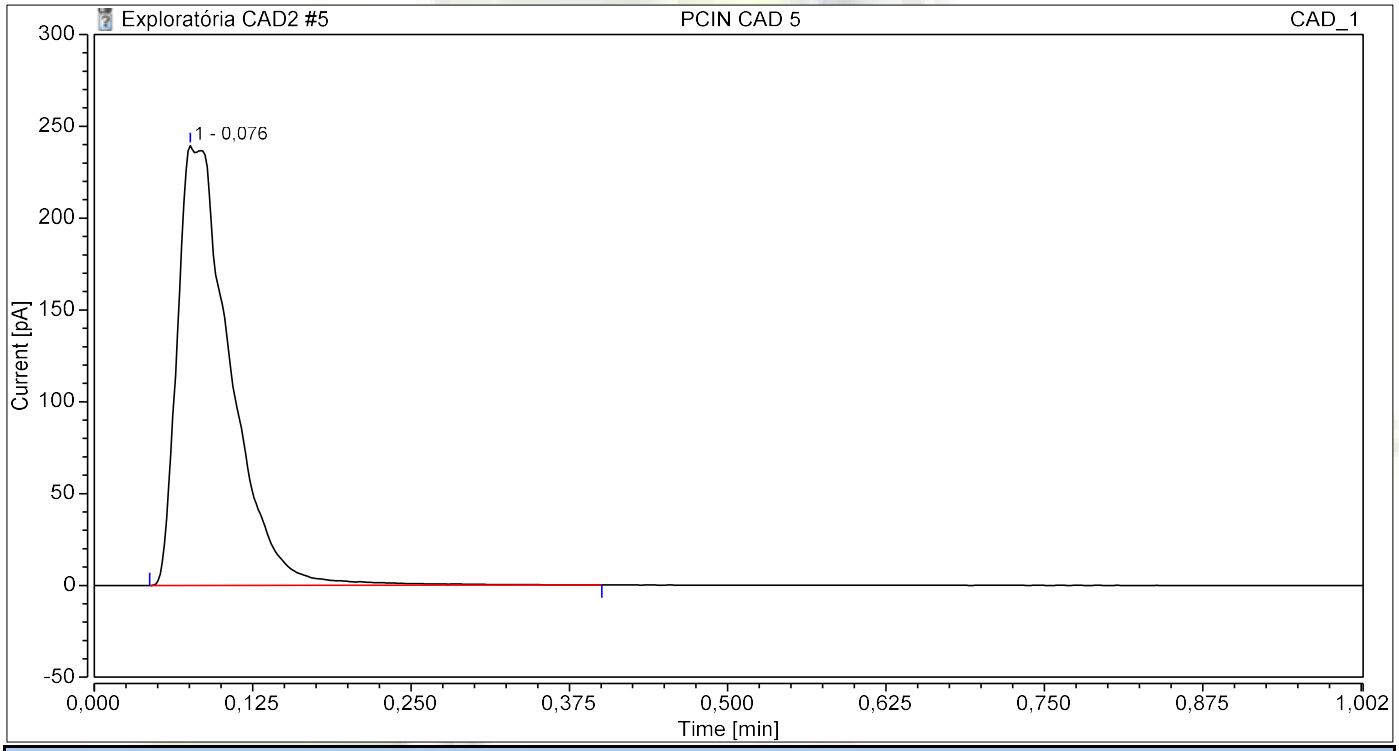

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,076	11,585	239,606	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,585**	**239,606**	**100,00**	**100,00**	


Chromeleon (c) Dionex
Version 7.2.10.23925

Chromatogram and Results

Injection Details

Injection Name:	**PCIN CAD 6**	*Run Time (min):*	**1,00**
Vial Number:	**RB2**	*Injection Volume:*	**5,00**
Injection Type:	**Unknown**	*Channel:*	**CAD_1**
Calibration Level:		*Wavelength:*	**n.a.**
Instrument Method:	**Qualificação_CAD**	*Bandwidth:*	**n.a.**
Processing Method:	**Cafeína**	*Dilution Factor:*	**1,0000**
Injection Date/Time:	**14/set/22 15:20**	*Sample Weight:*	**1,0000**

Chromatogram

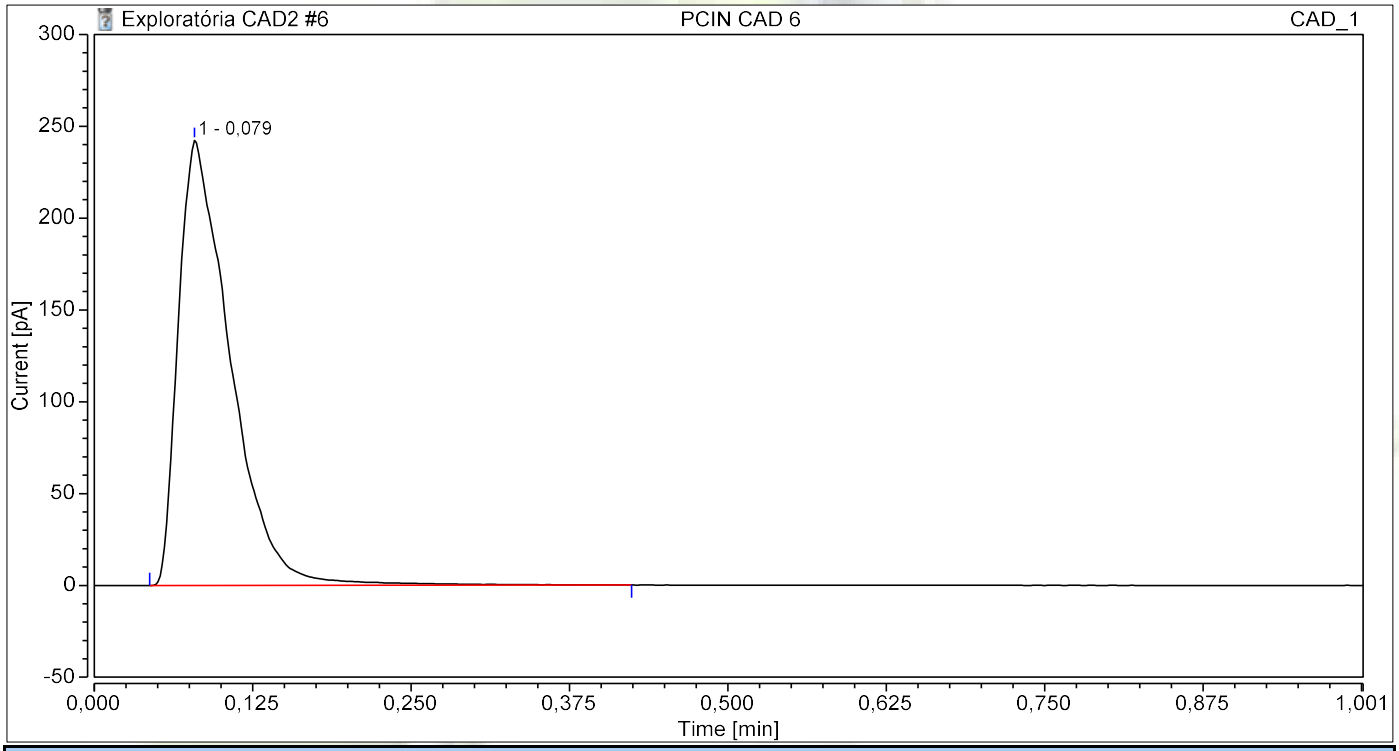

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount
1		0,079	11,502	242,357	100,00	100,00	n.a.
n.a.	Cafeína	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			**11,502**	**242,357**	**100,00**	**100,00**	

Chromeleon (c) Dionex
Version 7.2.10.23925